
Chromatogram

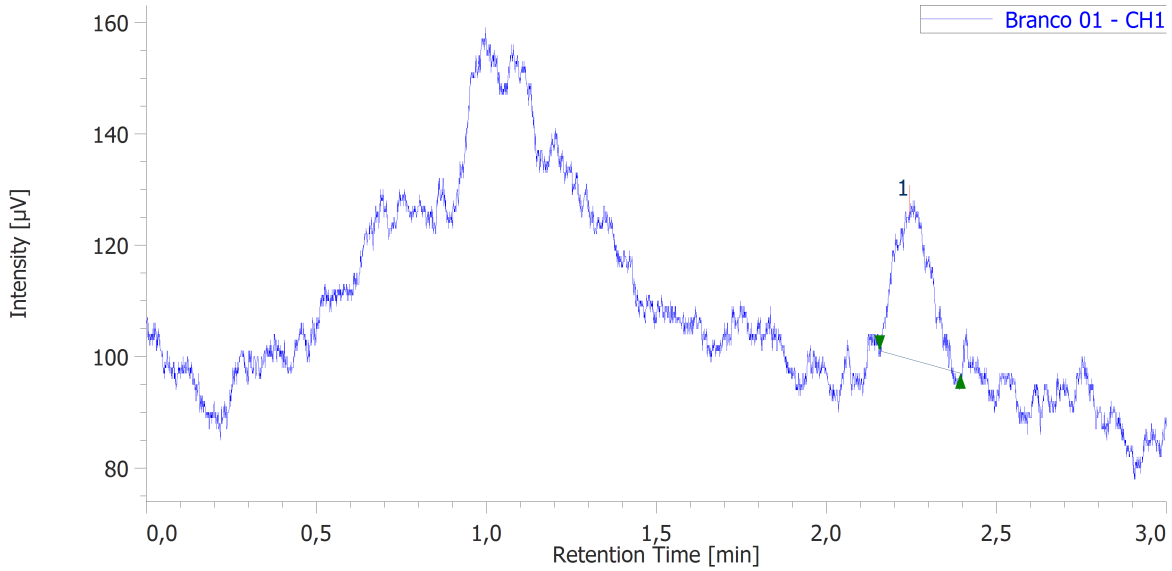

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:05:09
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:02:05
Volume	10,00 [µL]
Sample #	1
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,245	197	28	100,000	100,000	N/A	1694	N/A	1,225	

Creator
Reviewer
Approver

Chromatogram

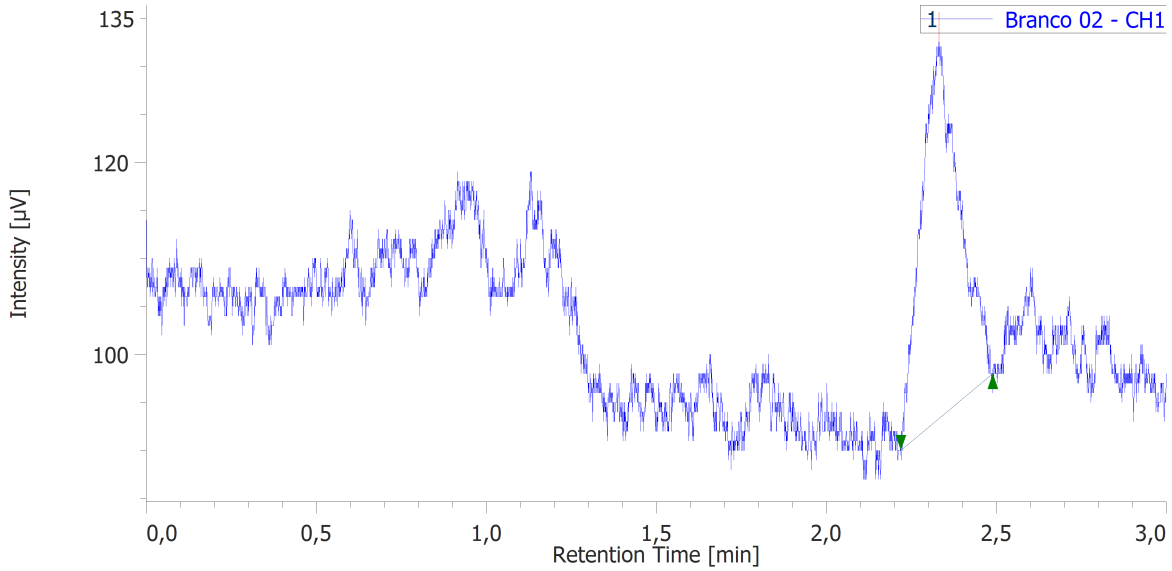

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 11:02:59
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:17:17
Volume	10,00 [µL]
Sample #	1
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,331	304	41	100,000	100,000	N/A	1754	N/A	1,211	

Creator Administrator
Reviewer
Approver

Chromatogram

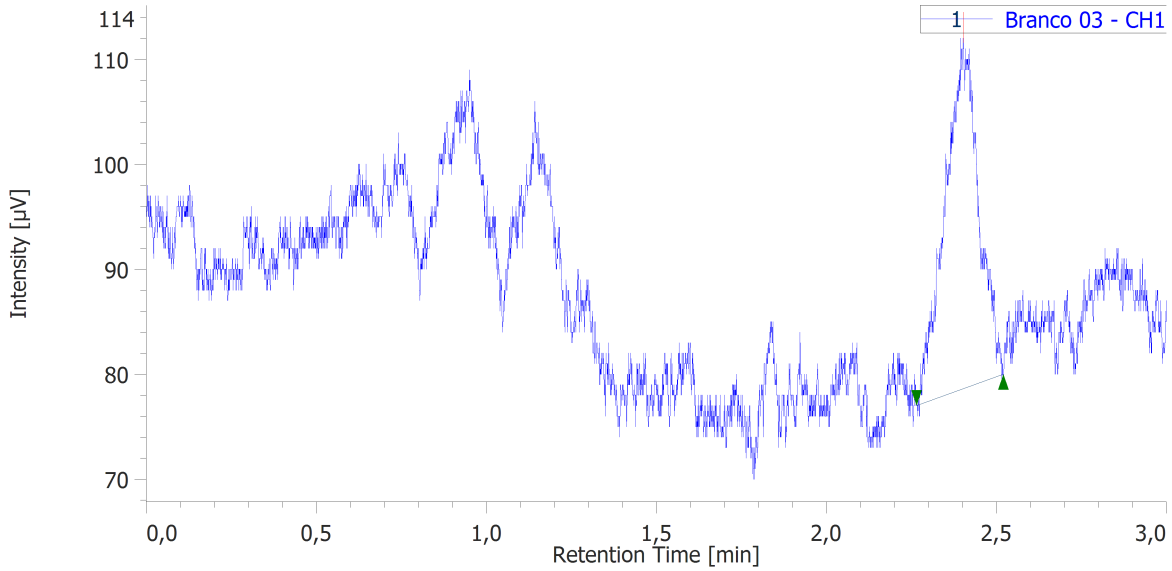

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:35:35
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:32:31
Volume	10,00 [µL]
Sample #	1
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,402	227	34	100,000	100,000	N/A	3062	N/A	0,943	

Creator
Reviewer
Approver

Chromatogram

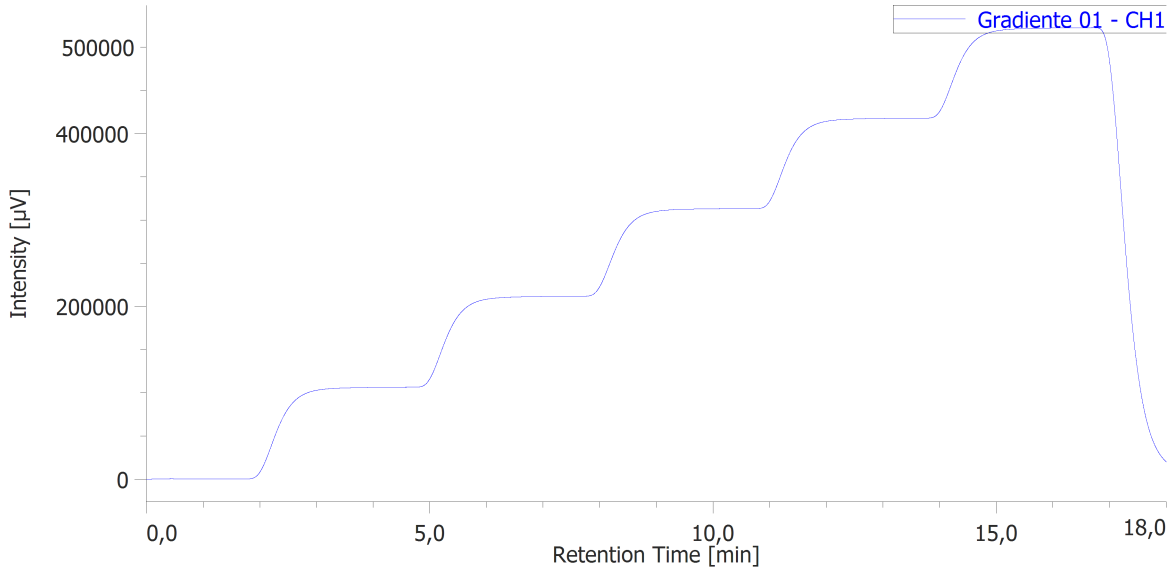


Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 12:33:46
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 12:15:44
Volume	0,10 [µL]
Sample #	1
Project Name	Treinamento QPack
Acquisition Time	18,0 [min]
Acquisition Sequence	GRBO
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

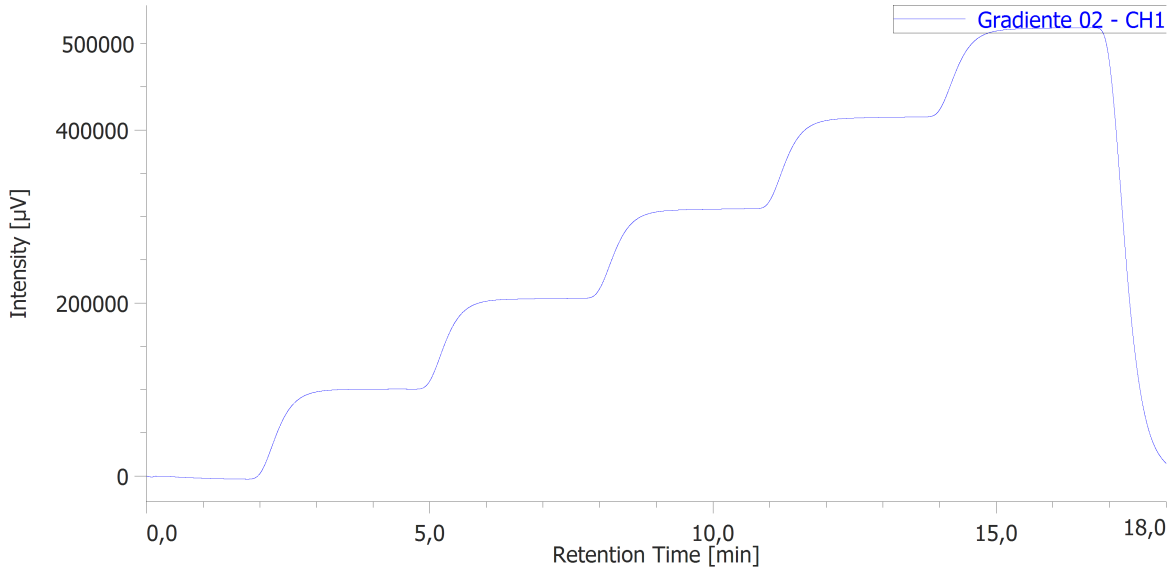


Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 12:52:28
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 12:34:24
Volume	0,10 [µL]
Sample #	1
Project Name	Treinamento QPack
Acquisition Time	18,0 [min]
Acquisition Sequence	GRBO
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

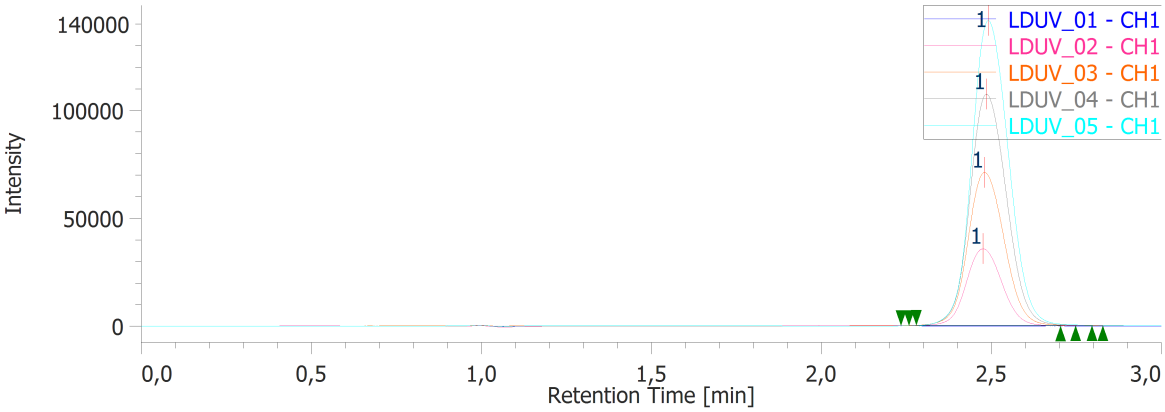

Channel & Peak Information Table

Chromatogram Name LDUV_01-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,475	260233	35568	100,000	100,000	N/A	2621	N/A	1,074	

Chromatogram Name LDUV_03-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,479	529227	70878	100,000	100,000	N/A	2548	N/A	1,092	


Chromatogram Name LDUV_04-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,485	808083	107170	100,000	100,000	N/A	2502	N/A	1,105	

Chromatogram Name LDUV_05-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,490	1067164	141295	100,000	100,000	N/A	2495	N/A	1,119	

Chromatogram

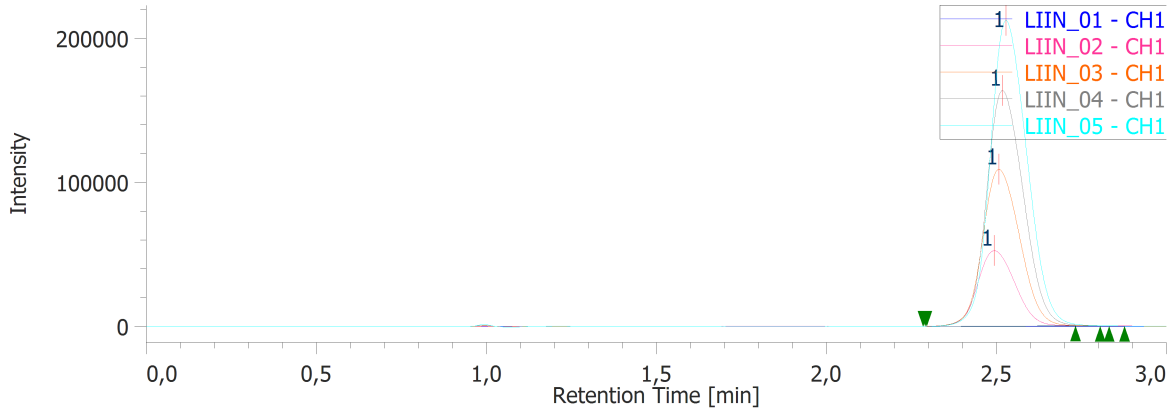

Channel & Peak Information Table

Chromatogram Name LIIN_01-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,493	400799	52225	100,000	100,000	N/A	2383	N/A	1,123	

Chromatogram Name LIIN_03-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,507	830871	108818	100,000	100,000	N/A	2452	N/A	1,140	


Chromatogram Name LIIN_04-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,517	1239655	163421	100,000	100,000	N/A	2510	N/A	1,160	

Chromatogram Name LIIN_05-CH1
Sample Name
Channel Name CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,528	1601700	212054	100,000	100,000	N/A	2558	N/A	1,168	

Chromatogram

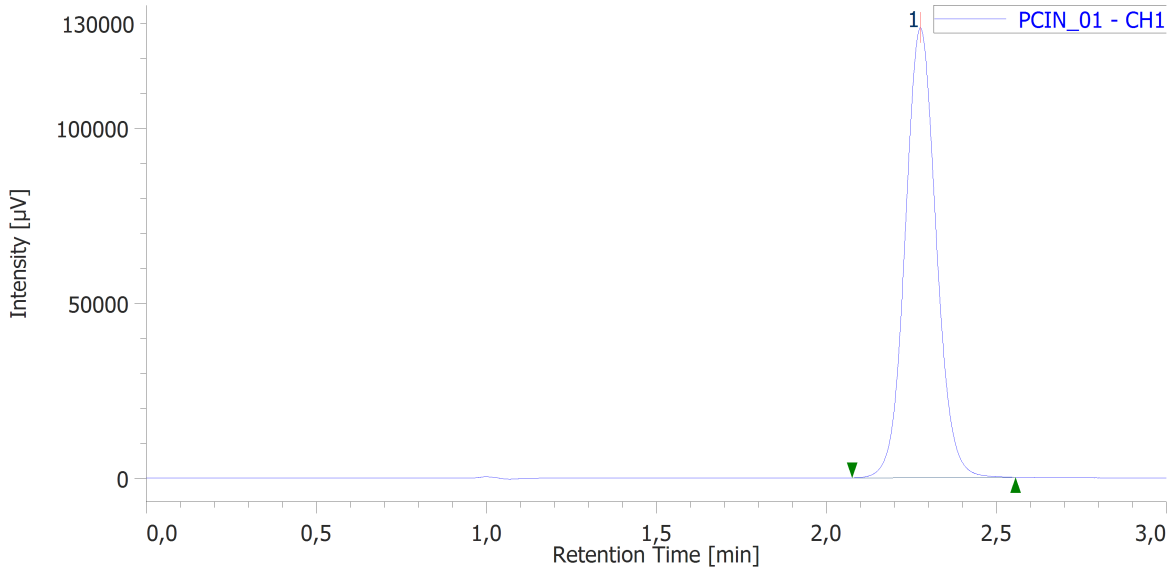

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:08:57
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:05:53
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,276	813050	128511	100,000	100,000	N/A	3064	N/A	1,064	

Creator Administrator
Reviewer
Approver

Chromatogram

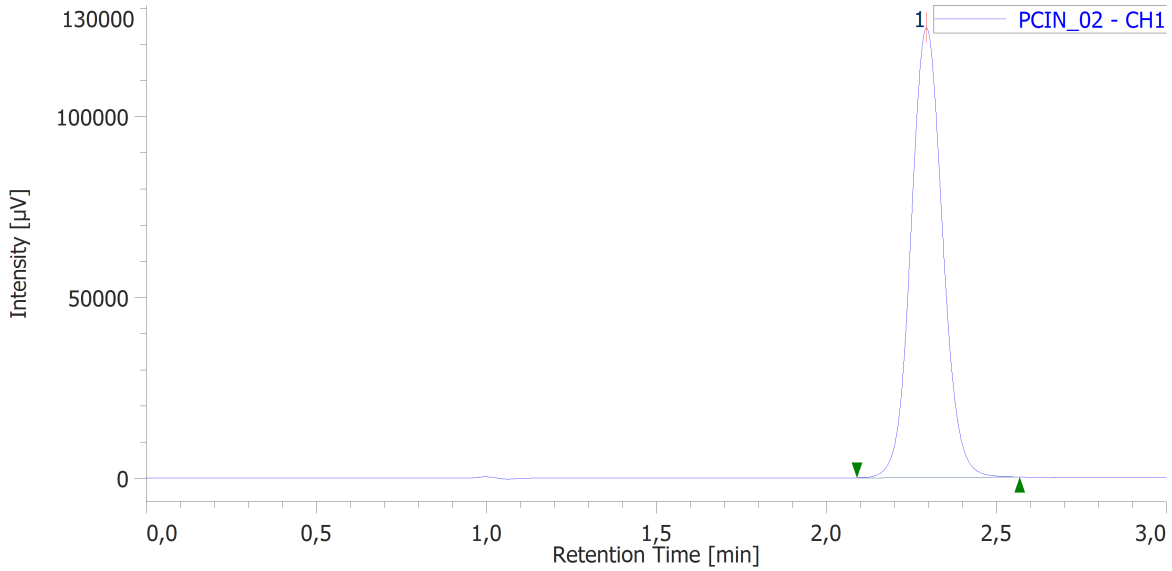

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:12:45
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:09:42
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,294	803898	124303	100,000	100,000	N/A	2957	N/A	1,066	

Creator Administrator
Reviewer
Approver

Chromatogram

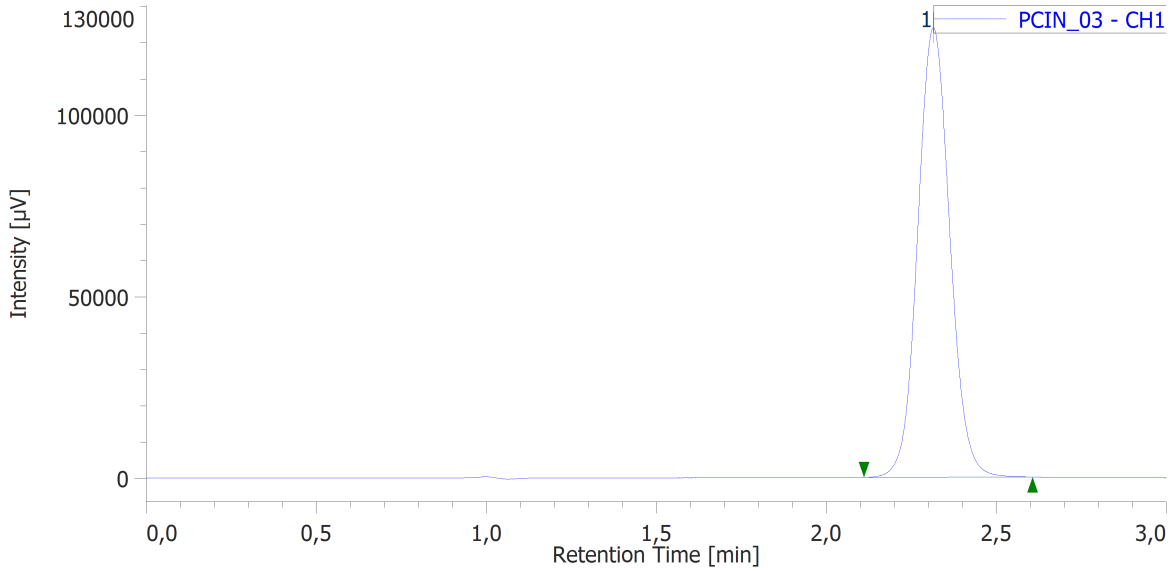

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:16:31
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:13:28
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,314	813176	123737	100,000	100,000	N/A	2905	N/A	1,072	

Creator Administrator
Reviewer
Approver

Chromatogram

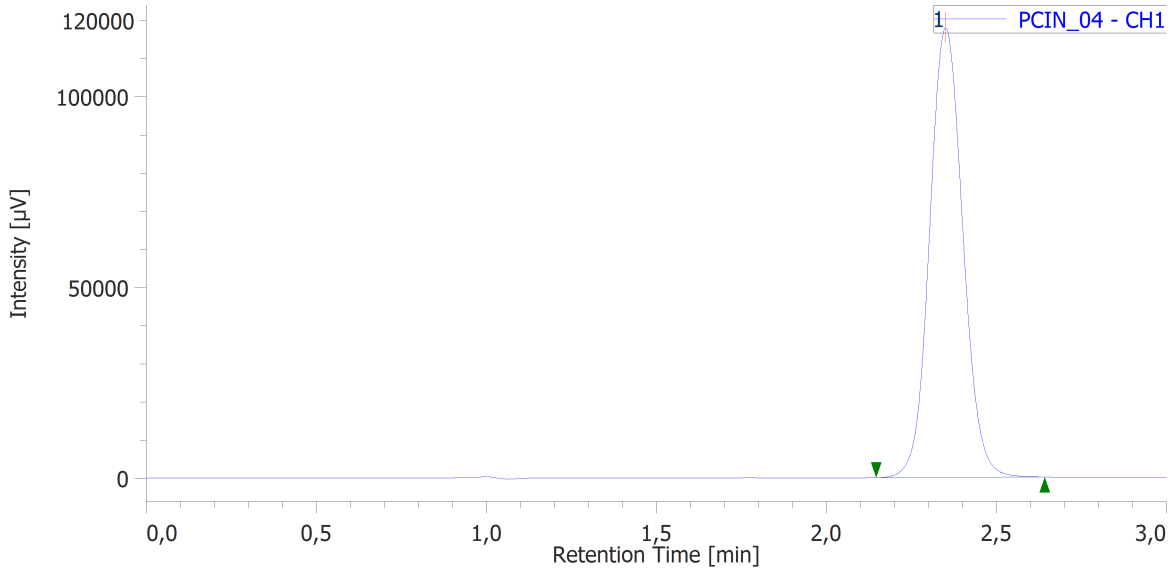

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:24:09
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:21:05
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,350	800420	117819	100,000	100,000	N/A	2782	N/A	1,083	

Creator Administrator
Reviewer
Approver

Chromatogram

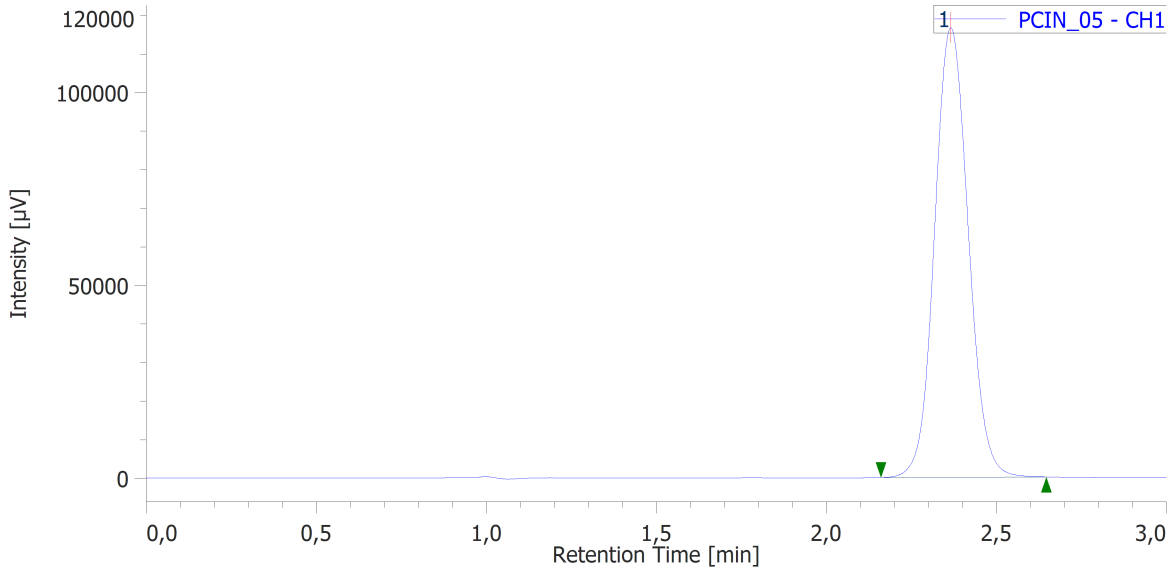

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:27:57
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:24:54
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,366	802361	116508	100,000	100,000	N/A	2735	N/A	1,074	

Creator Administrator
Reviewer
Approver

Chromatogram

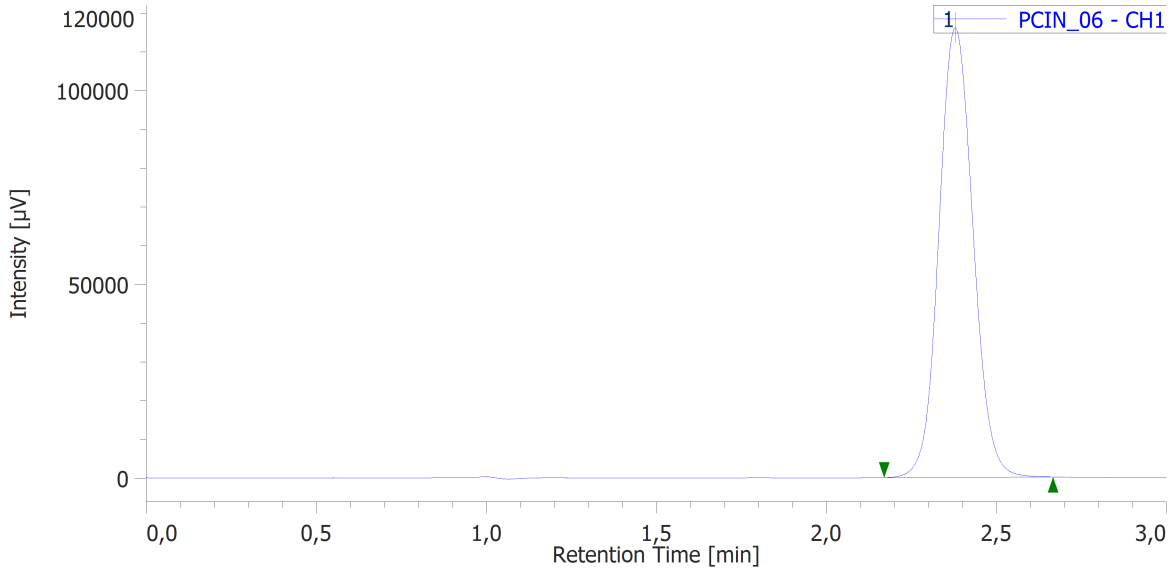

Chromatogram Information	
User Name	Administrator
Date Modified	23/02/2018 10:31:45
Description	
HPLC System Name	HPL 09
Injection Date	23/02/2018 10:28:42
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Treinamento
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	2,379	807998	115928	100,000	100,000	N/A	2694	N/A	1,082	

Creator Administrator
Reviewer
Approver

Peak Find - PD Cafeina_004 UV_tR1,77 D.jws

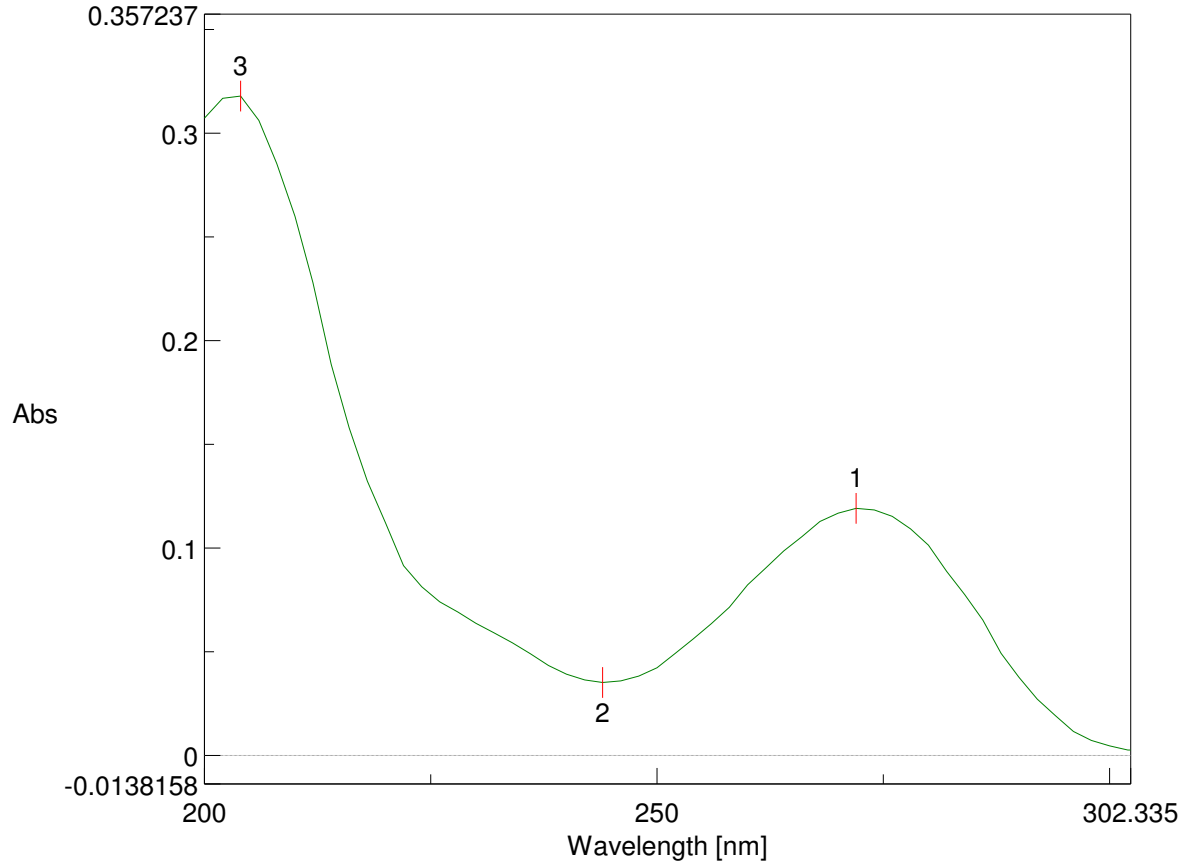

[Comments]

User	Administrator
Division	---
Company	Jasco do Brasil
Creation date	23/02/2018 07:42
Date modified	23/02/2018 07:47

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200

[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.118968	2	244	0.0351115
3	204	0.317784			