


Spectral Scan - VWD [DECAD00126]
Absorbance [mAU]
2500
2000
1500
1000
500
0
200
220
240
260
280
300
Wavelength [nm]

[nm],[mAU]	[nm],[mAU]	[nm],[mAU]	[nm],[mAU]
190.00,219.379	217.00,1069.247	244.00,300.426	271.00,647.093
191.00,328.430	218.00,984.908	245.00,296.956	272.00,652.870
192.00,531.981	219.00,924.873	246.00,295.125	273.00,655.745
193.00,754.634	220.00,850.648	247.00,296.432	274.00,655.116
194.00,924.295	221.00,789.565	248.00,299.461	275.00,652.228
195.00,1150.628	222.00,749.225	249.00,305.414	276.00,644.612
196.00,1339.684	223.00,701.643	250.00,313.895	277.00,633.051
197.00,1471.112	224.00,662.169	251.00,320.868	278.00,619.465
198.00,1623.795	225.00,638.915	252.00,332.522	279.00,598.182
199.00,1735.719	226.00,611.306	253.00,346.614	280.00,574.565
200.00,1804.270	227.00,585.589	254.00,362.913	281.00,543.685
201.00,1874.129	228.00,562.236	255.00,375.771	282.00,518.067
202.00,1920.389	229.00,544.282	256.00,395.414	283.00,486.324
203.00,1945.995	230.00,522.070	257.00,415.488	284.00,452.742
204.00,1959.405	231.00,498.988	258.00,431.681	285.00,428.347
205.00,1950.915	232.00,482.119	259.00,452.859	286.00,394.262
206.00,1928.297	233.00,459.099	260.00,473.497	287.00,363.124
207.00,1885.990	234.00,437.981	261.00,488.692	288.00,328.246
208.00,1810.717	235.00,422.650	262.00,508.709	289.00,304.789
209.00,1728.572	236.00,402.719	263.00,528.366	290.00,271.786
210.00,1658.060	237.00,385.212	264.00,547.453	291.00,239.334
211.00,1567.374	238.00,372.033	265.00,562.081	292.00,216.608
212.00,1477.569	239.00,356.868	266.00,581.418	293.00,189.123
213.00,1408.209	240.00,341.921	267.00,599.863	294.00,165.652
214.00,1316.505	241.00,328.057	268.00,612.390	295.00,145.943
215.00,1223.339	242.00,318.794	269.00,627.686	296.00,134.575
216.00,1161.471	243.00,308.393	270.00,639.644	297.00,122.429

Data File C:\CHEM32\2\DATA\BRANCO 1.D
Sample Name: Branco 1

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   1
Acq. Instrument : HPLC                            Location : Vial 1
Injection Date  : 1/26/2017 6:00:34 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

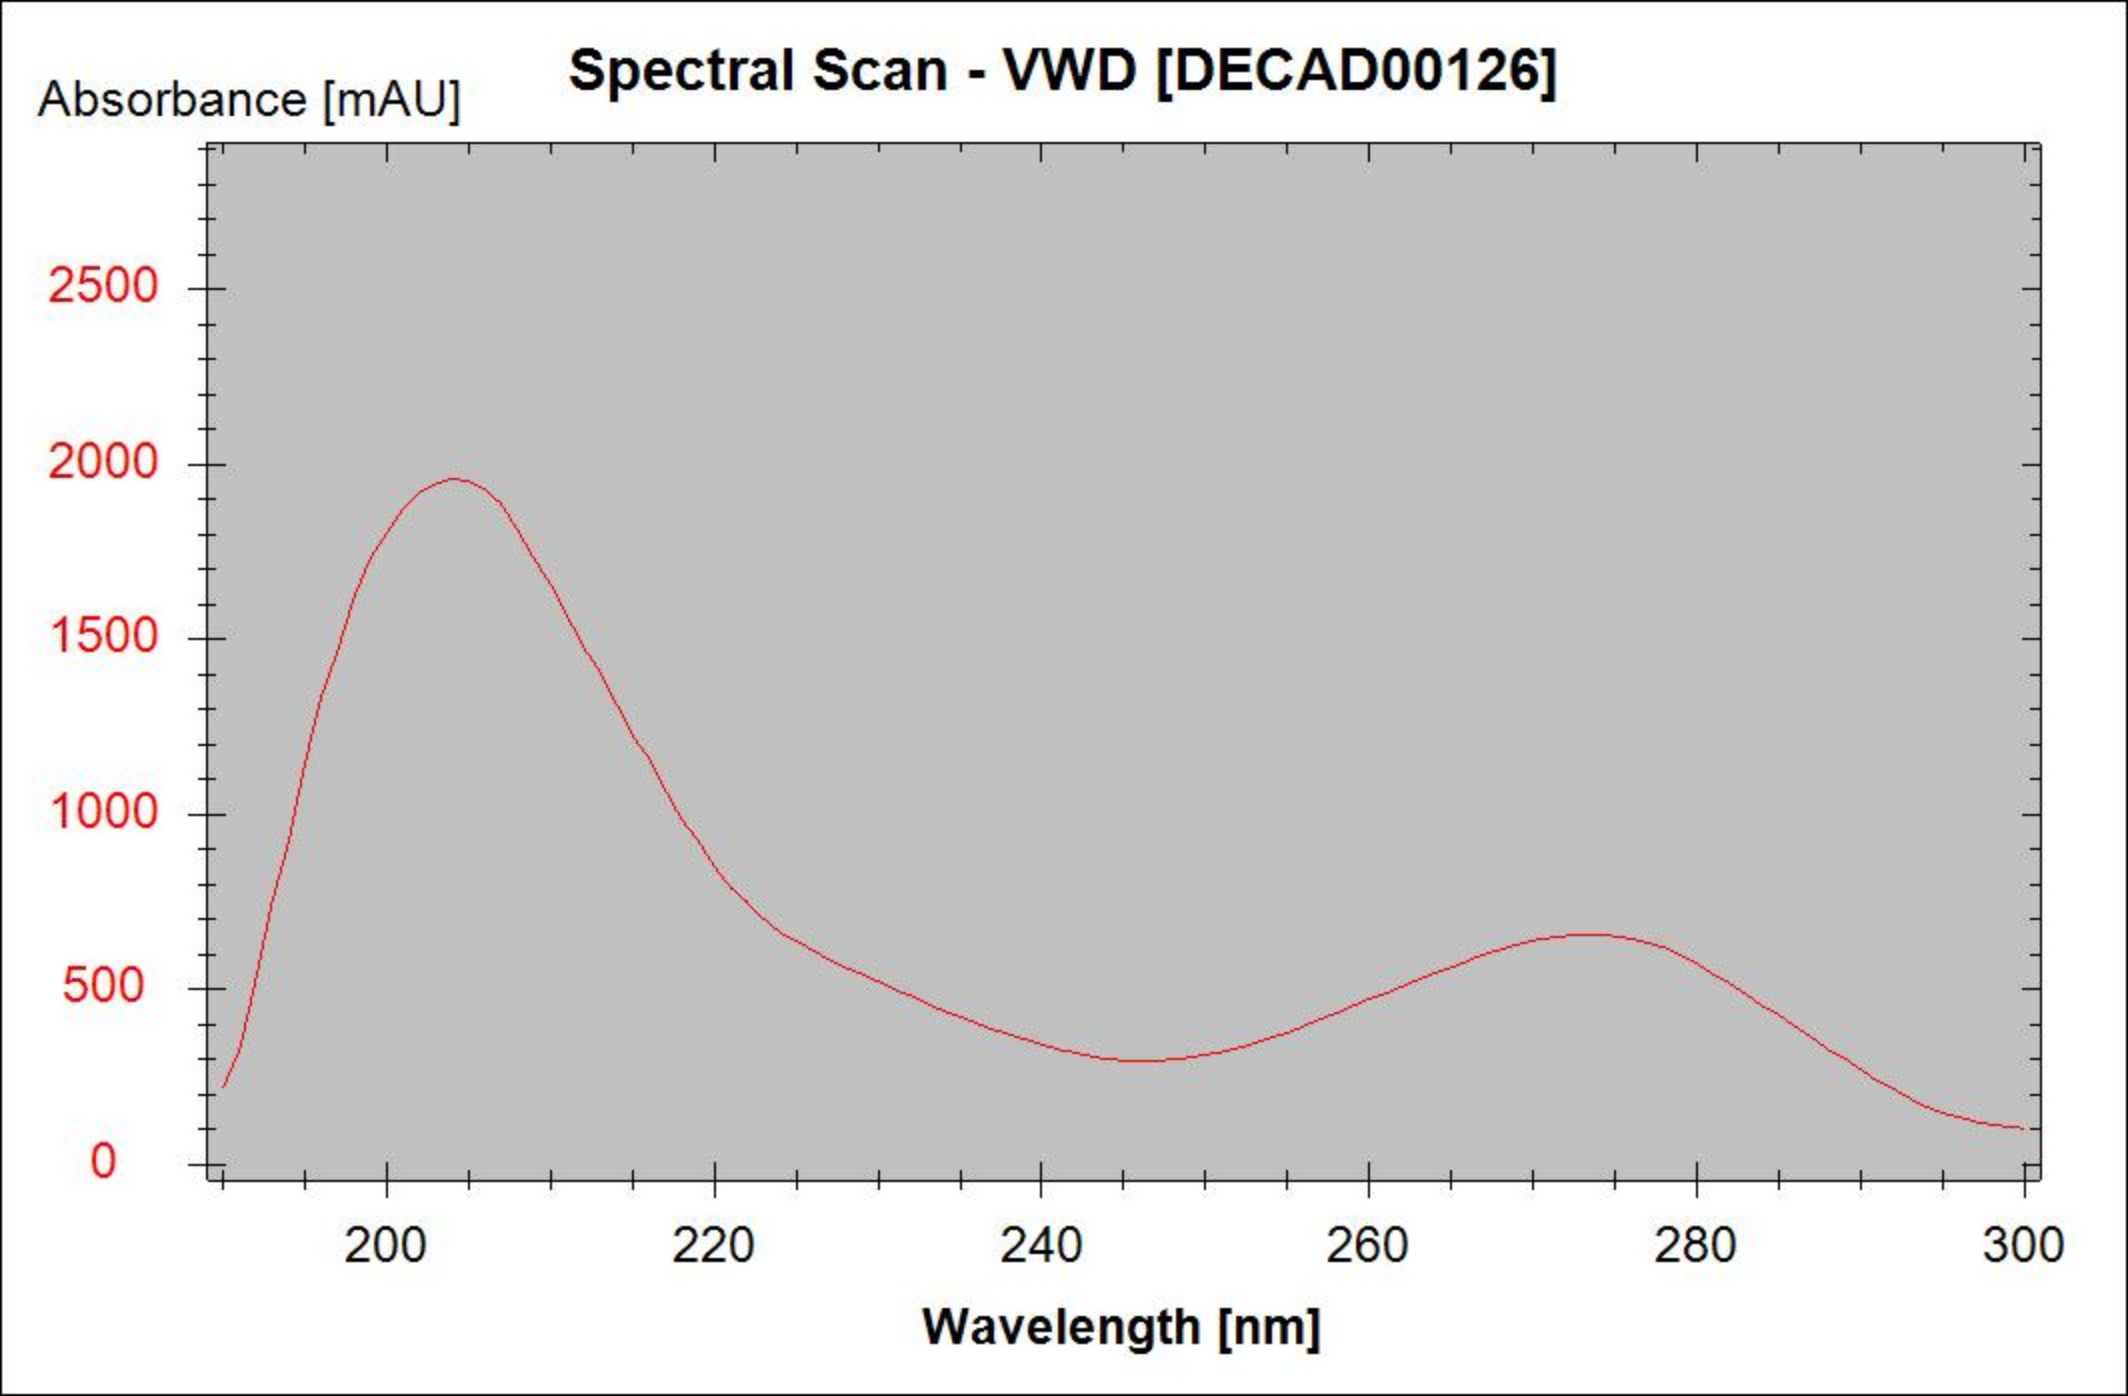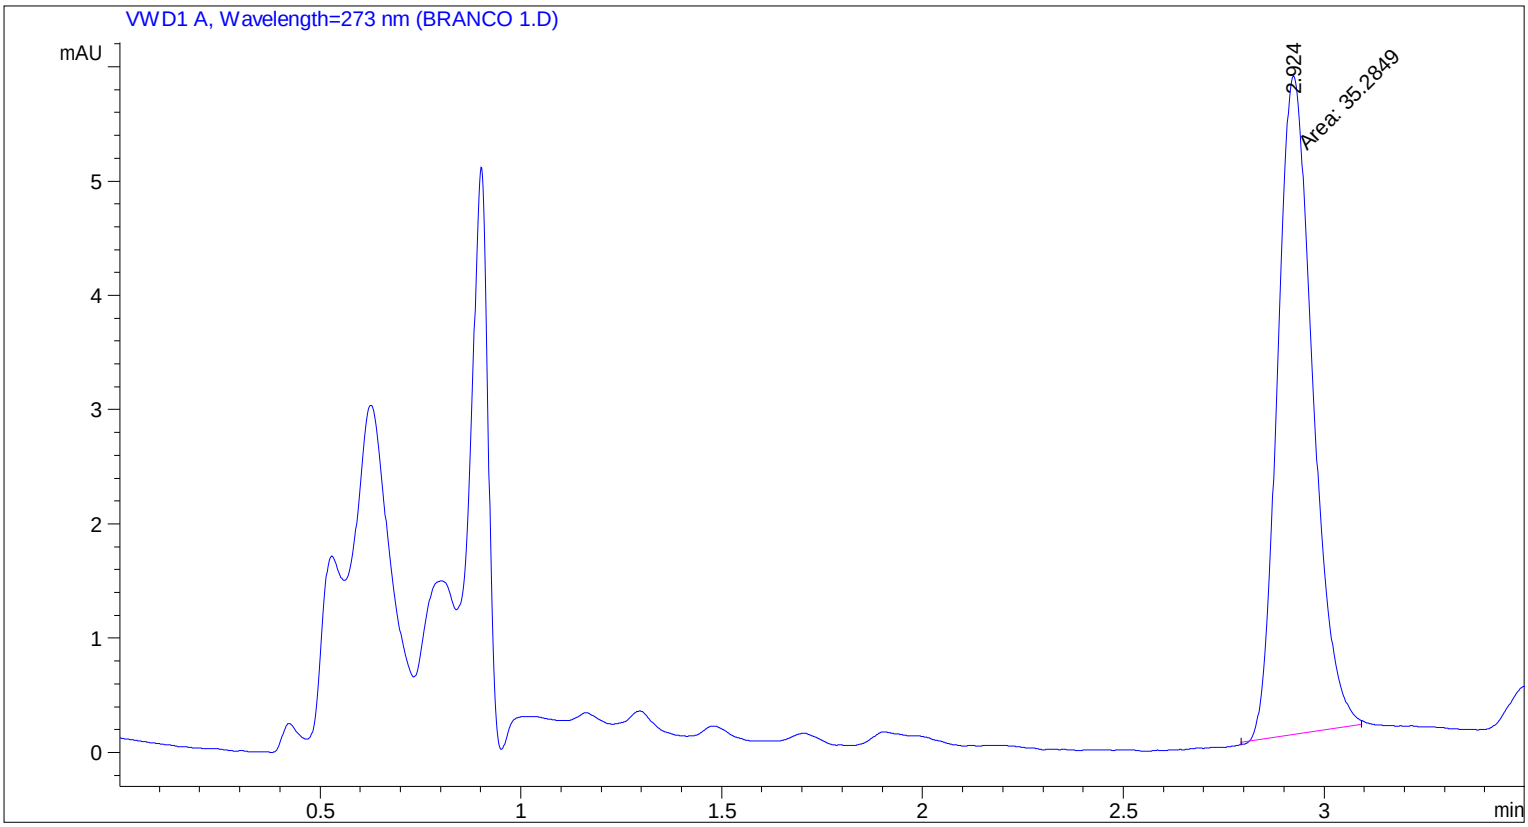


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.924 MM T    0.1020   35.28487 100.0000 Cafeina

Totals :                     35.28487


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 1.D
Sample Name: PCIN 1

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   2
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:04:54 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

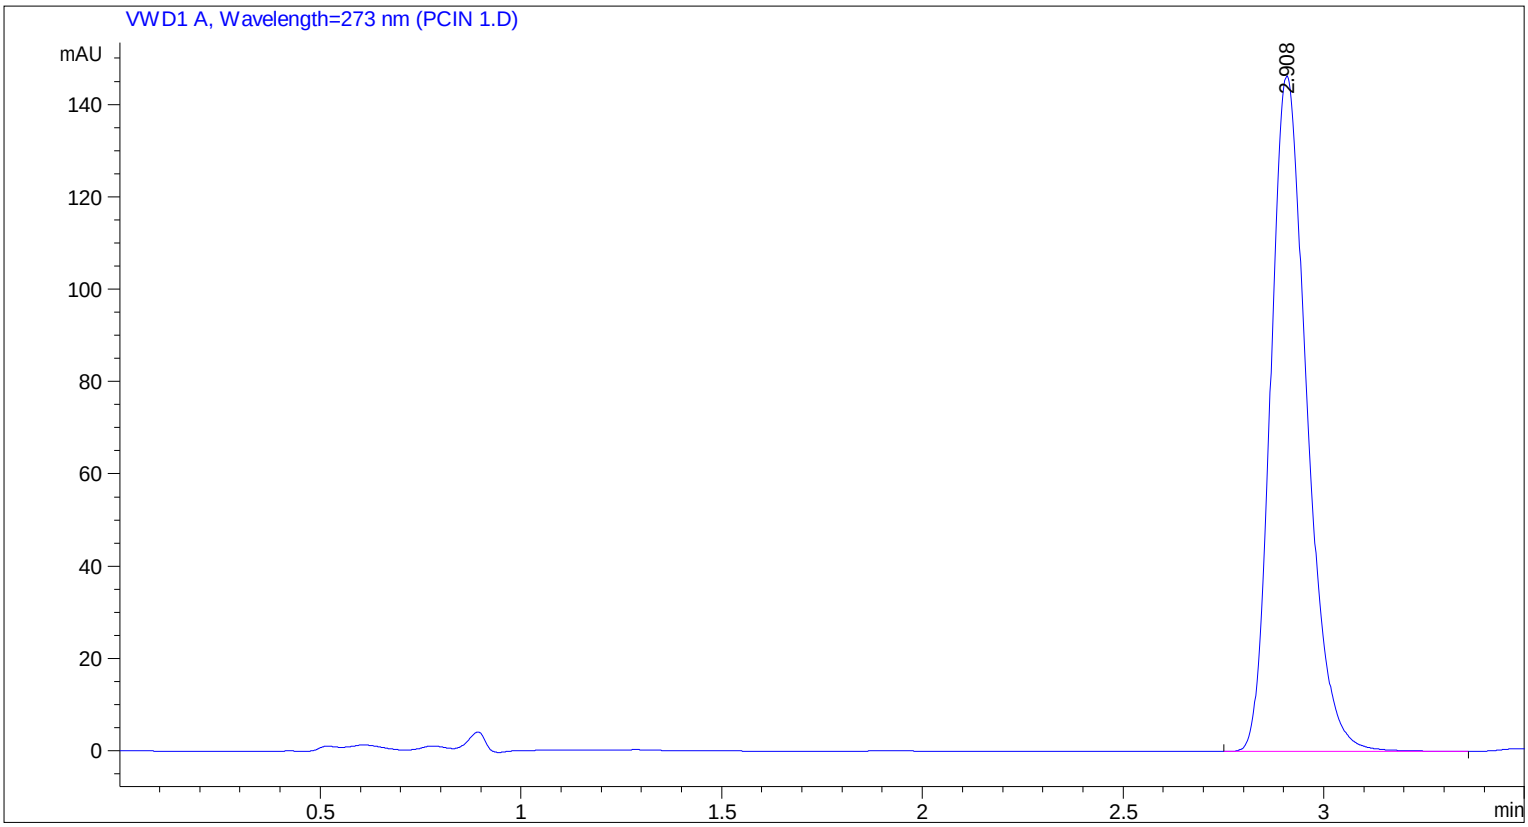


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.908 BB      0.0959  913.79596 100.0000 Cafeina

Totals :                     913.79596


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 2.D
Sample Name: PCIN 2

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   3
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:09:15 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

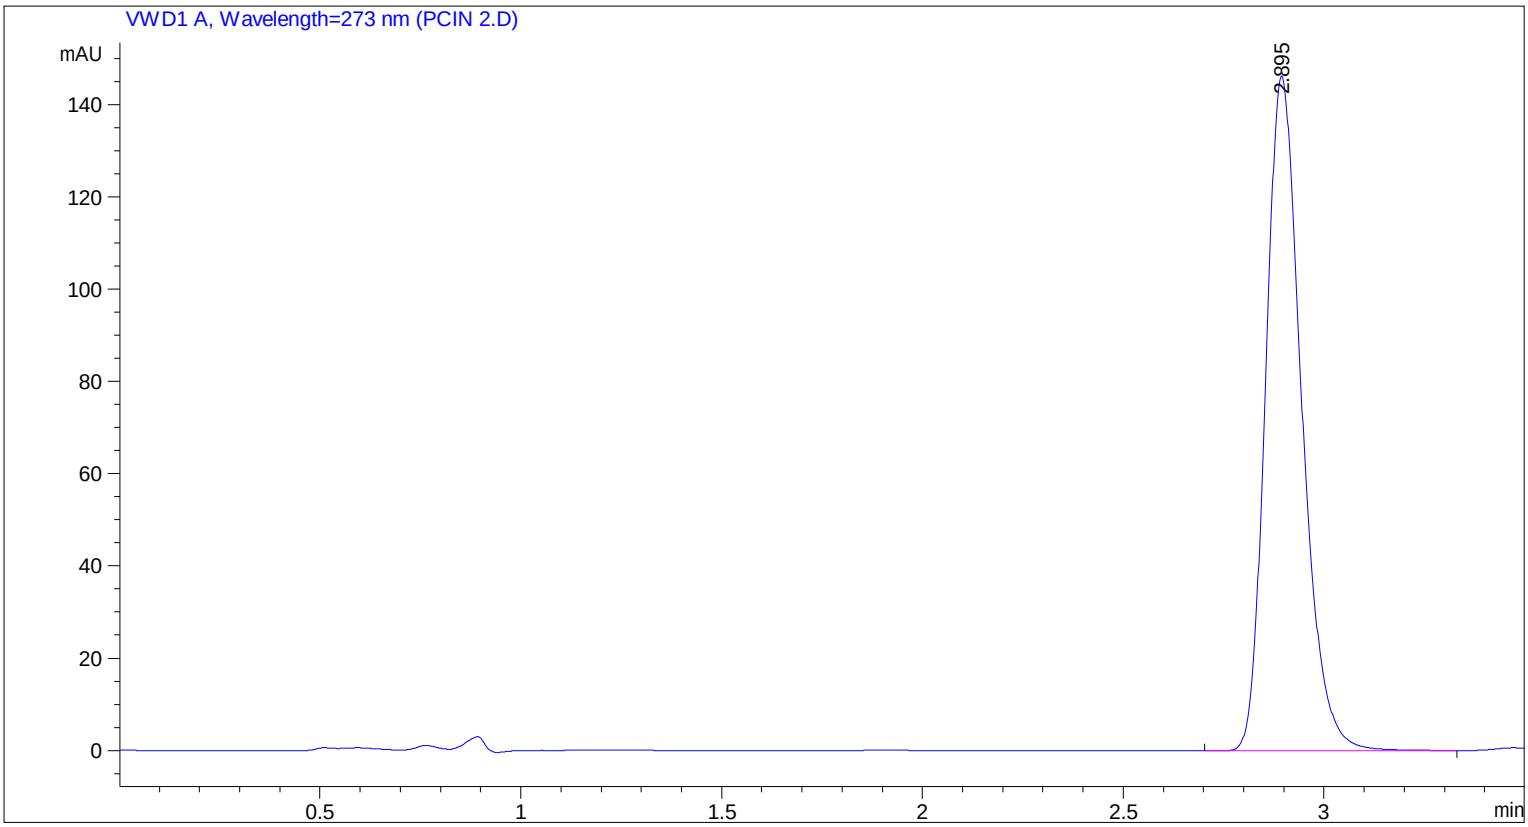


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.895 BB      0.0951  910.24609 100.0000 Cafeina

Totals :                     910.24609


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 3.D
Sample Name: PCIN 3

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   4
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:13:35 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

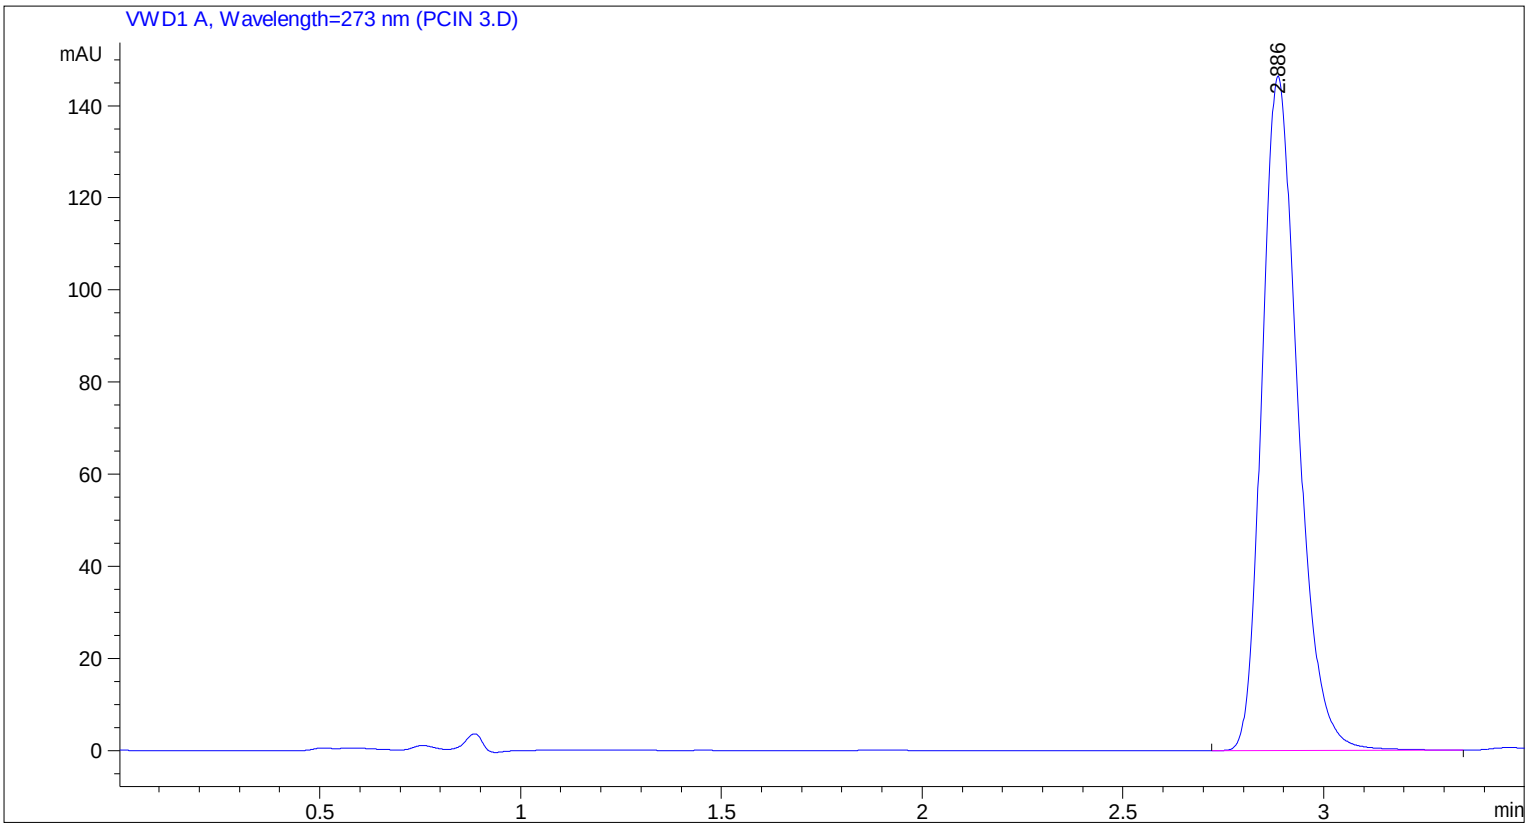


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.886 BB      0.0956  910.91803 100.0000 Cafeina

Totals :                     910.91803


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\BRANCO 2.D
Sample Name: Branco 2

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   5
Acq. Instrument : HPLC                            Location : Vial 1
Injection Date  : 1/26/2017 6:17:55 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

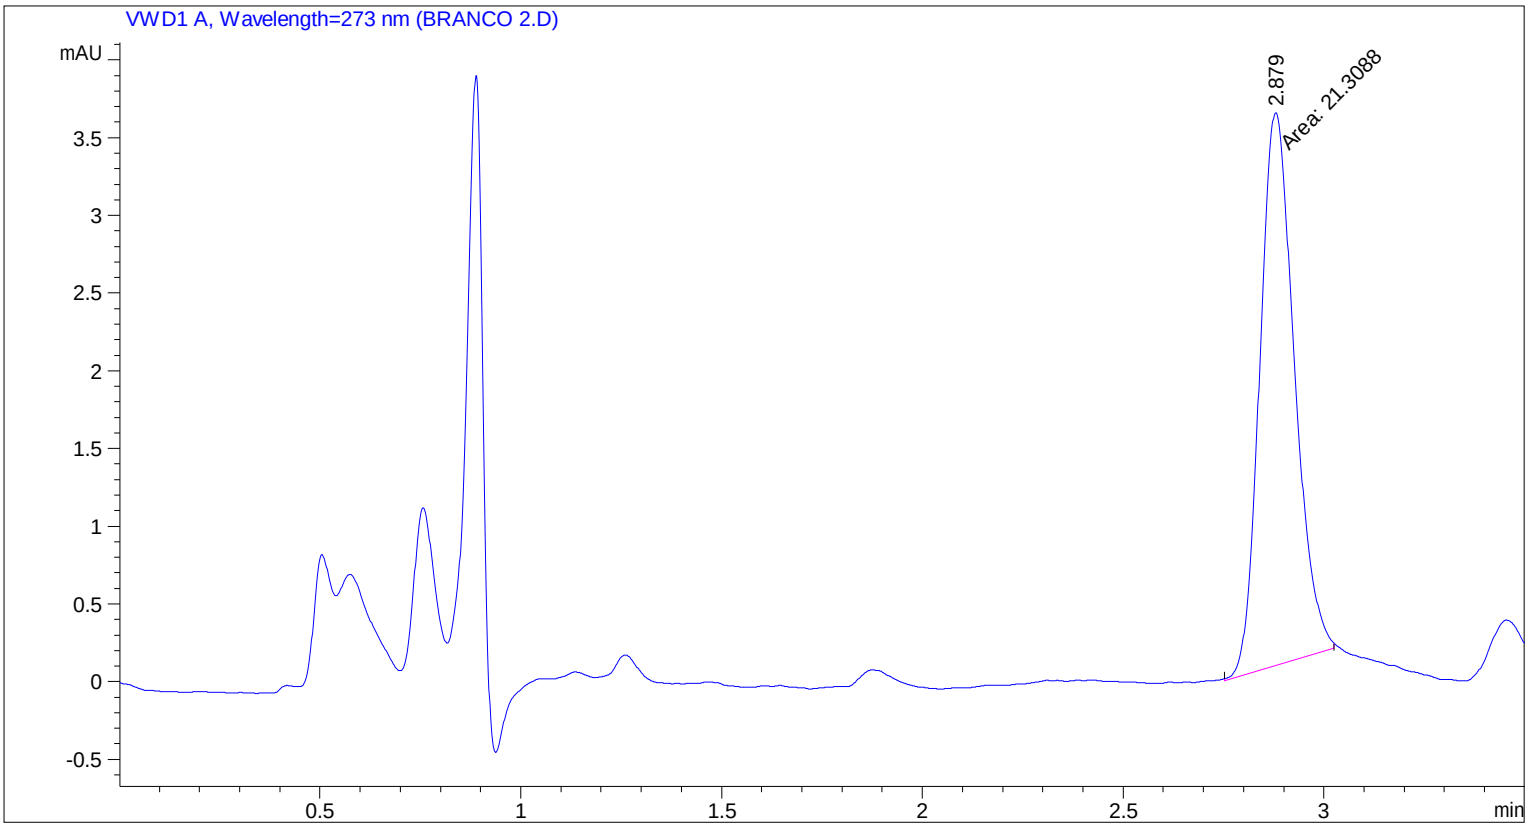


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.879 MM T    0.0998   21.30883 100.0000 Cafeina

Totals :                      21.30883


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 4.D
Sample Name: PCIN 4

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   6
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:22:16 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

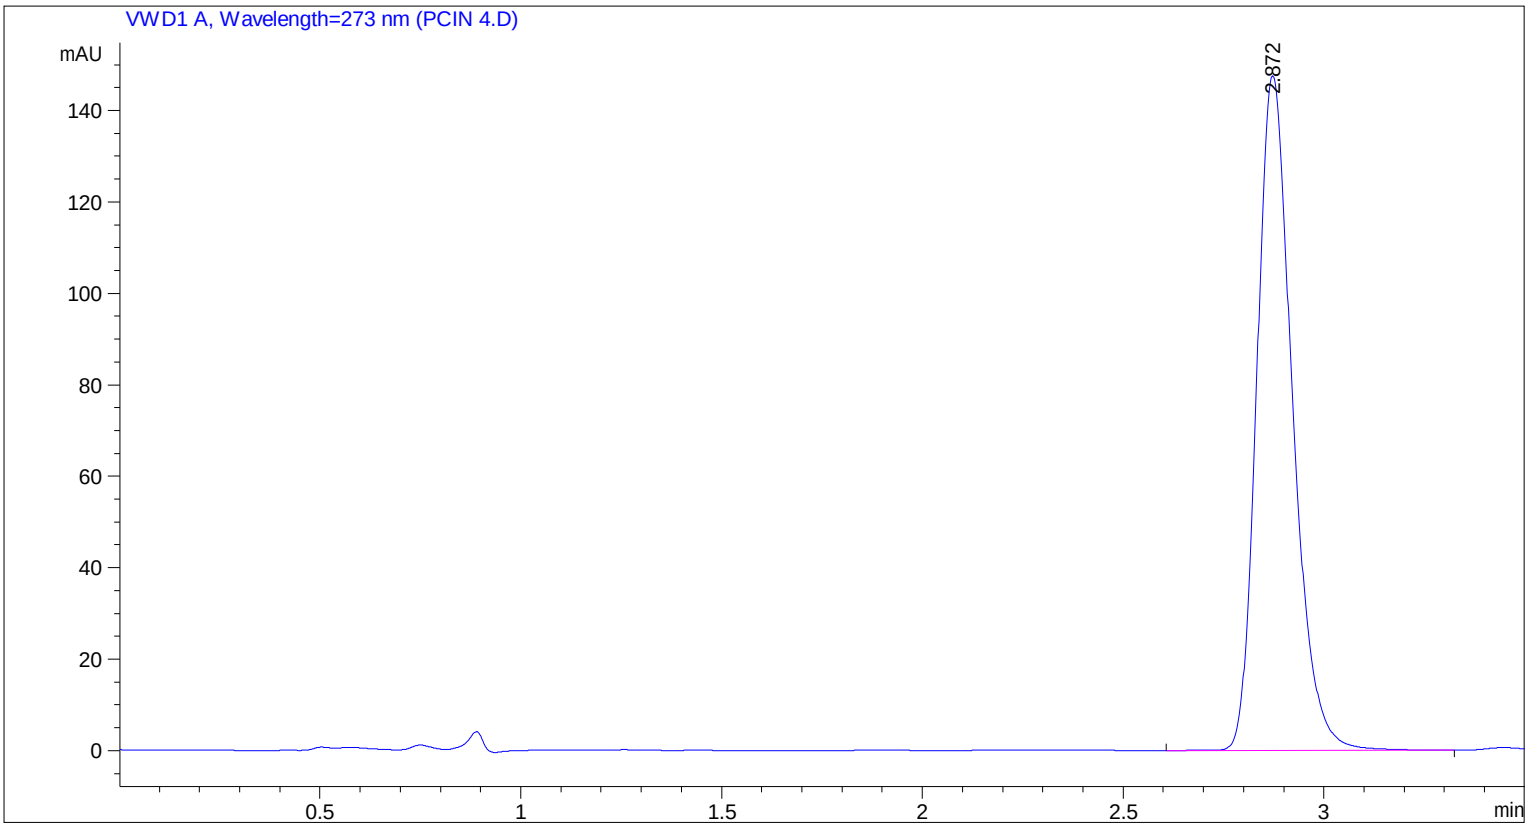


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.872 BB      0.0951  911.29193 100.0000 Cafeina

Totals :                     911.29193


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 5.D
Sample Name: PCIN 5

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   7
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:26:36 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

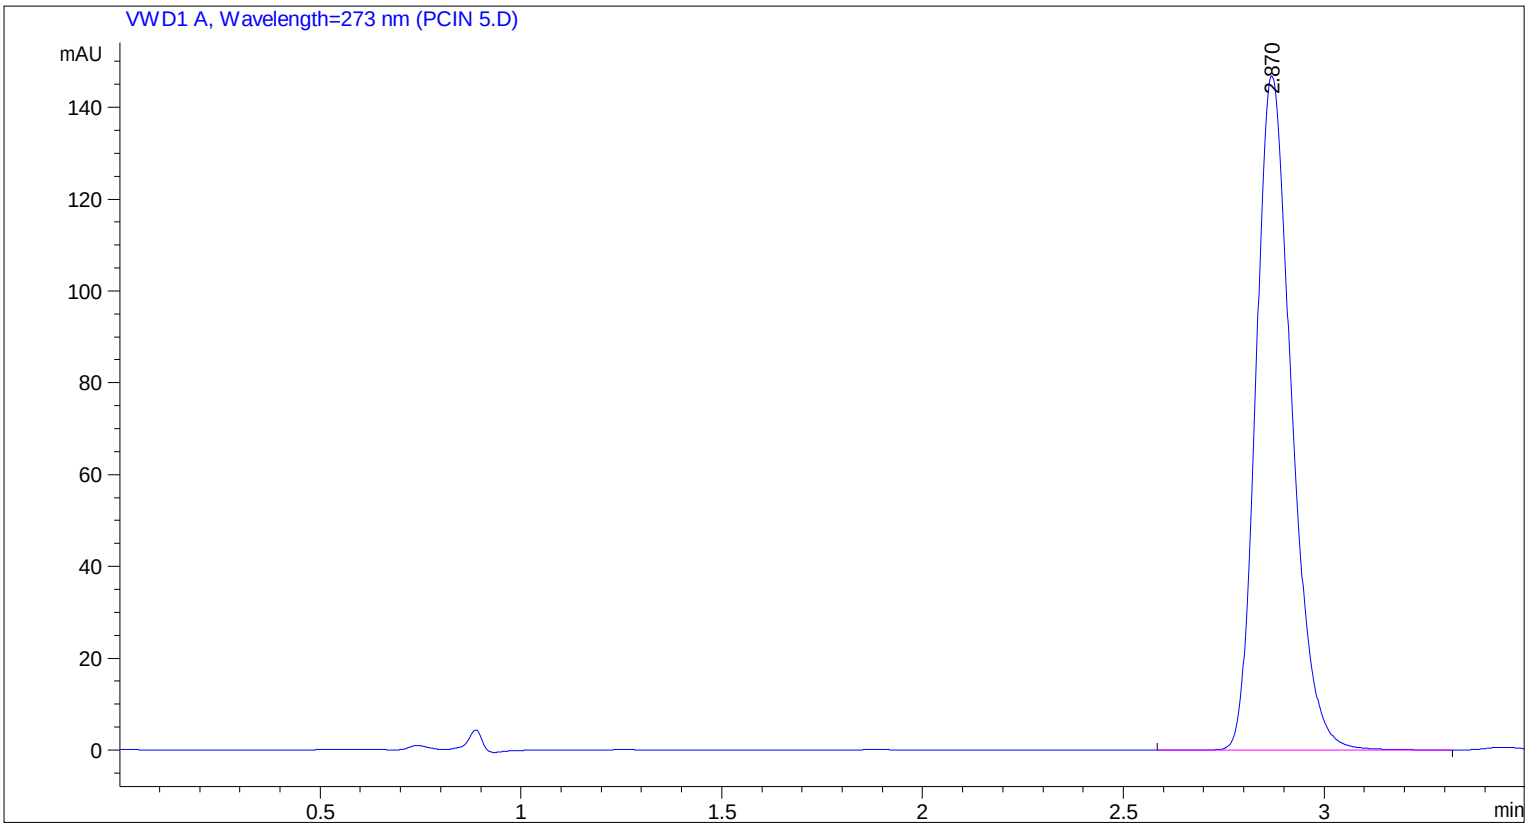


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.870 BB      0.0944  904.79053 100.0000 Cafeina

Totals :                     904.79053


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\PCIN 6.D
Sample Name: PCIN 6

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   8
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/26/2017 6:30:57 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

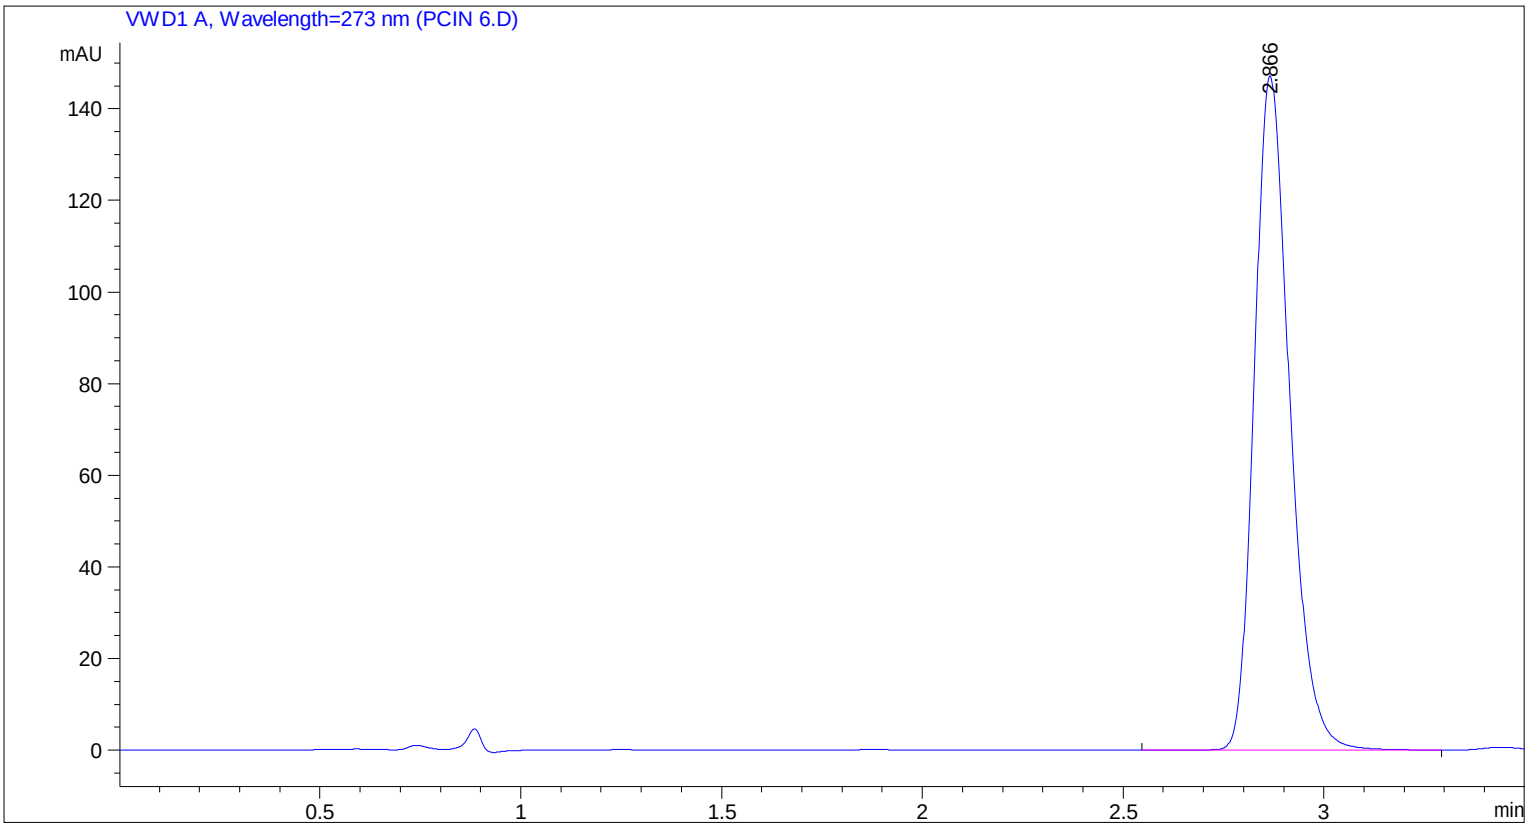


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.866 BB      0.0943  905.79810 100.0000 Cafeina

Totals :                     905.79810


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\BRANCO 3.D
Sample Name: Branco 3

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :   9
Acq. Instrument : HPLC                            Location : Vial 1
Injection Date  : 1/26/2017 6:35:17 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

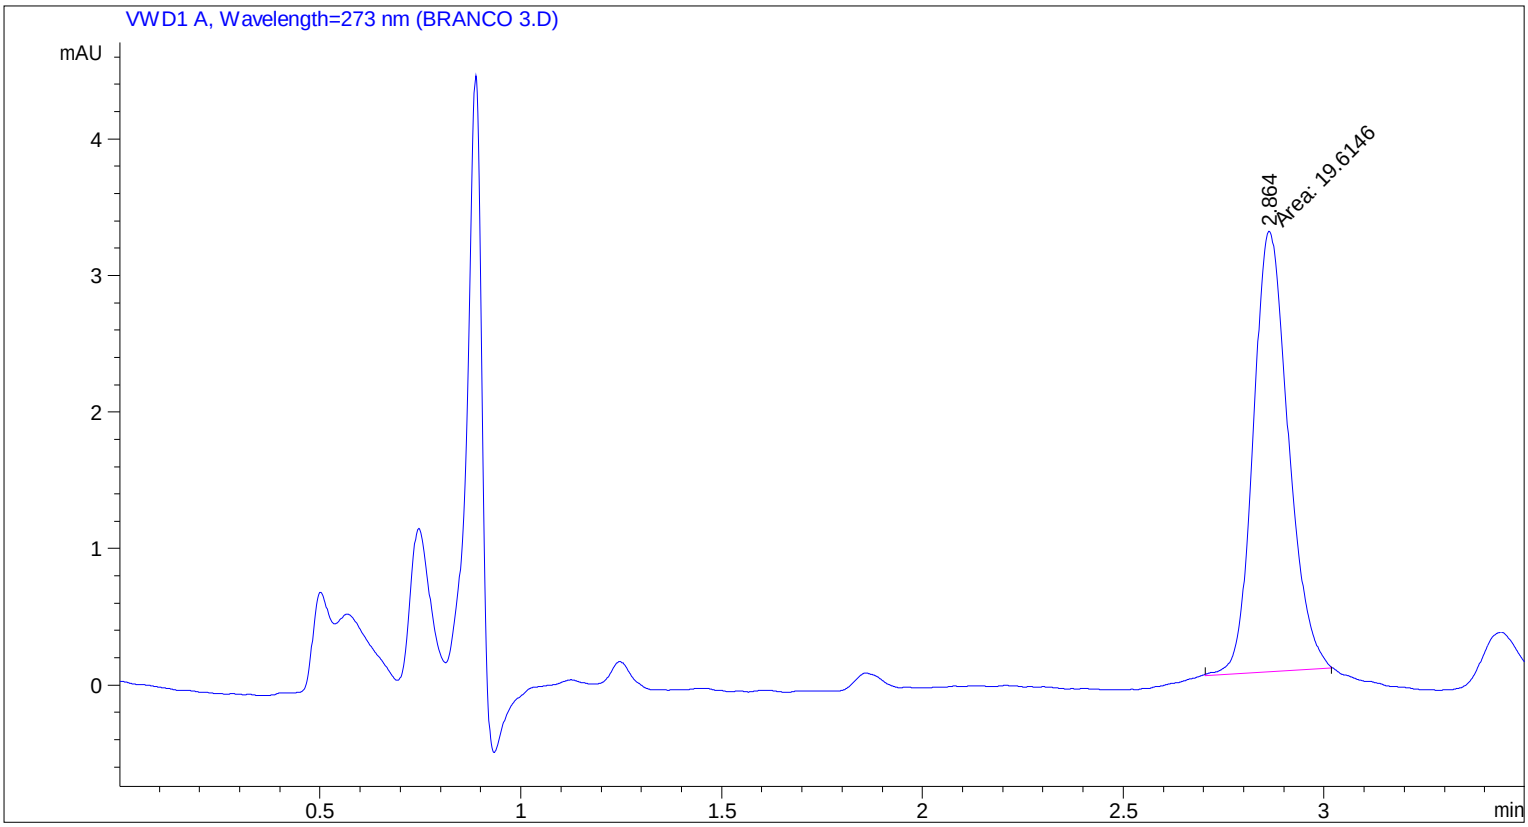


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.864 MM T    0.1014   19.61465 100.0000 Cafeina

Totals :                      19.61465


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LDUV 1.D
Sample Name: LDUV 1

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  10
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 1/26/2017 6:39:40 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

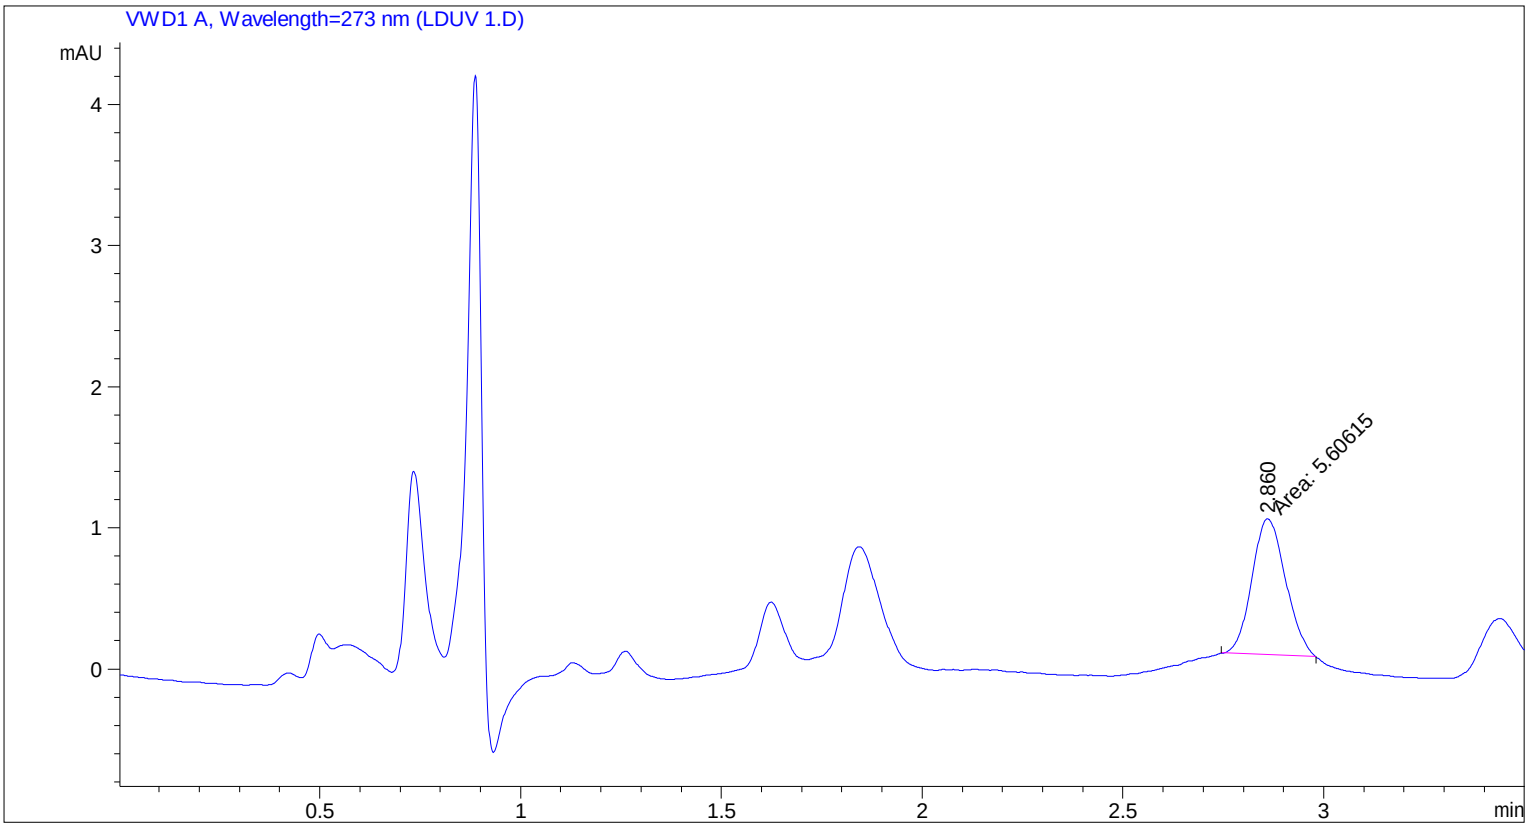


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.860 MM T    0.0972    5.60615 100.0000 Cafeina

Totals :                       5.60615


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LDUV 2.D
Sample Name: LDUV 2

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  11
Acq. Instrument : HPLC                            Location : Vial 4
Injection Date  : 1/26/2017 6:44:03 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

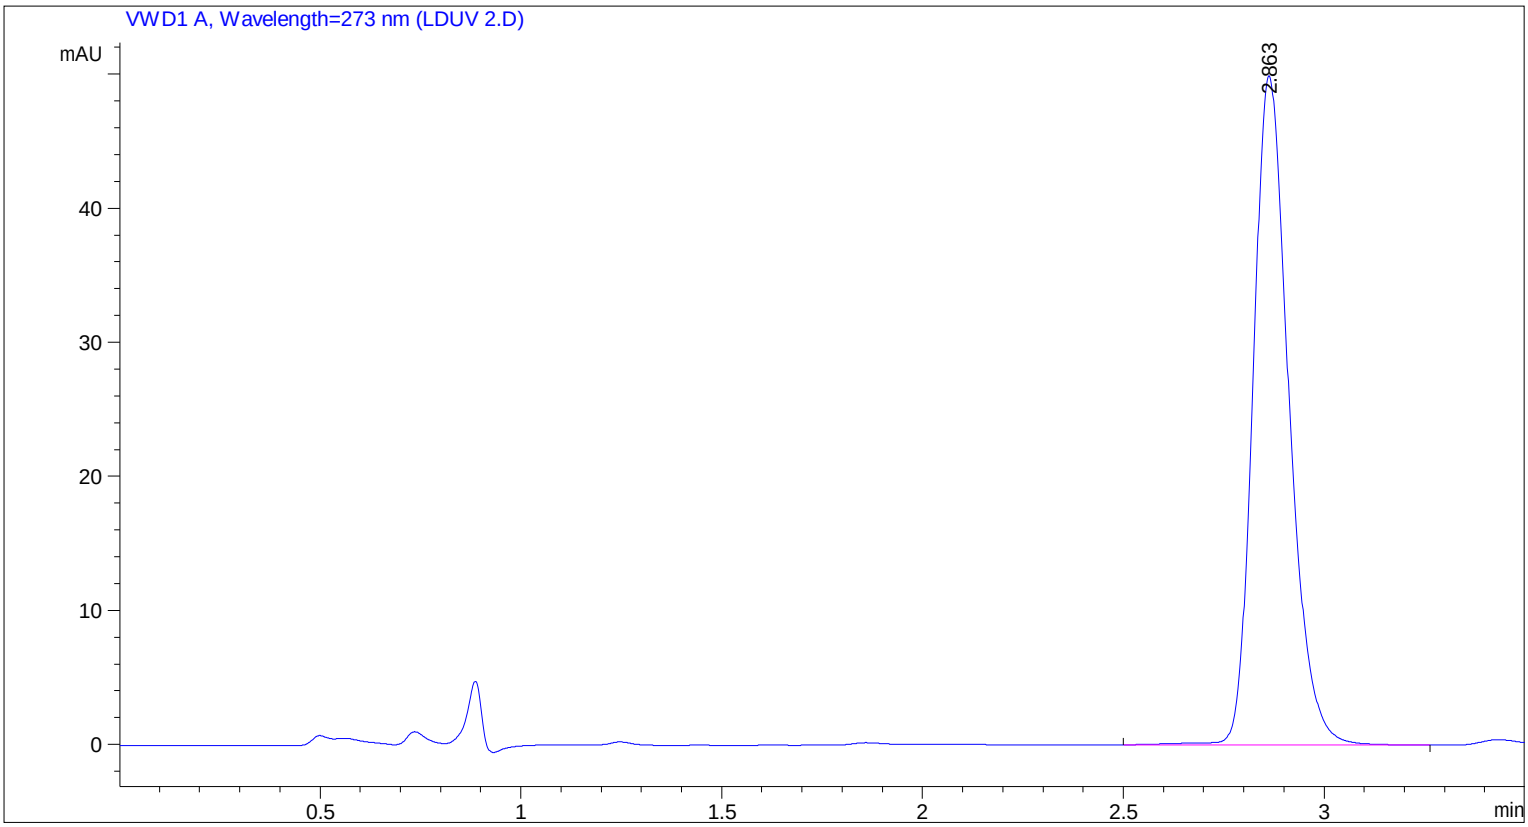


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.863 BB      0.0949  309.69348 100.0000 Cafeina

Totals :                     309.69348


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LDUV 3.D
Sample Name: LDUV 3

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  12
Acq. Instrument : HPLC                            Location : Vial 5
Injection Date  : 1/26/2017 6:48:21 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

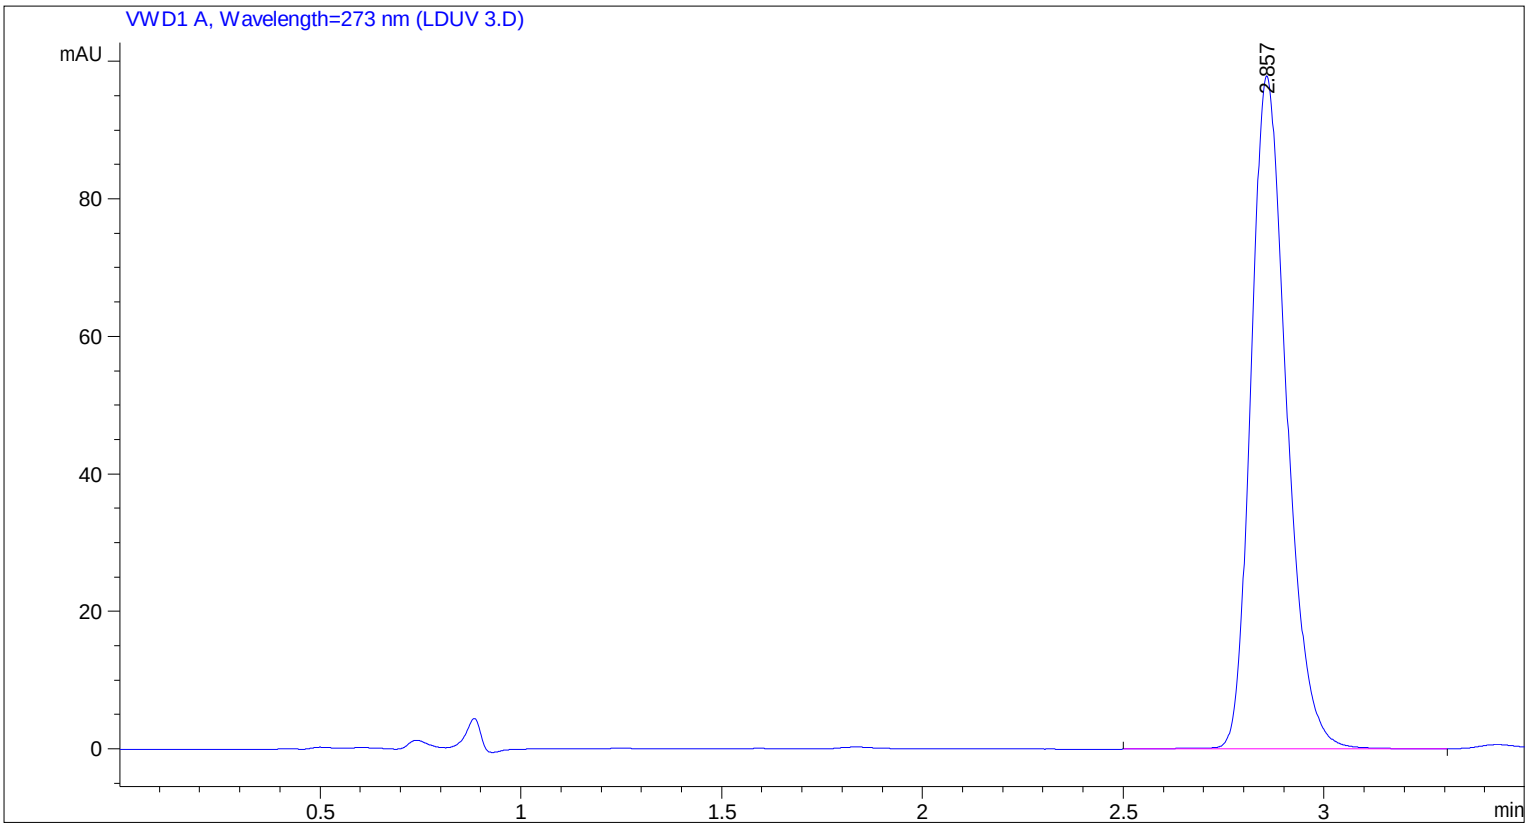


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.857 BB      0.0944  603.06848 100.0000 Cafeina

Totals :                     603.06848


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LDUV 4.D
Sample Name: LDUV 4

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  13
Acq. Instrument : HPLC                            Location : Vial 6
Injection Date  : 1/26/2017 6:52:44 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

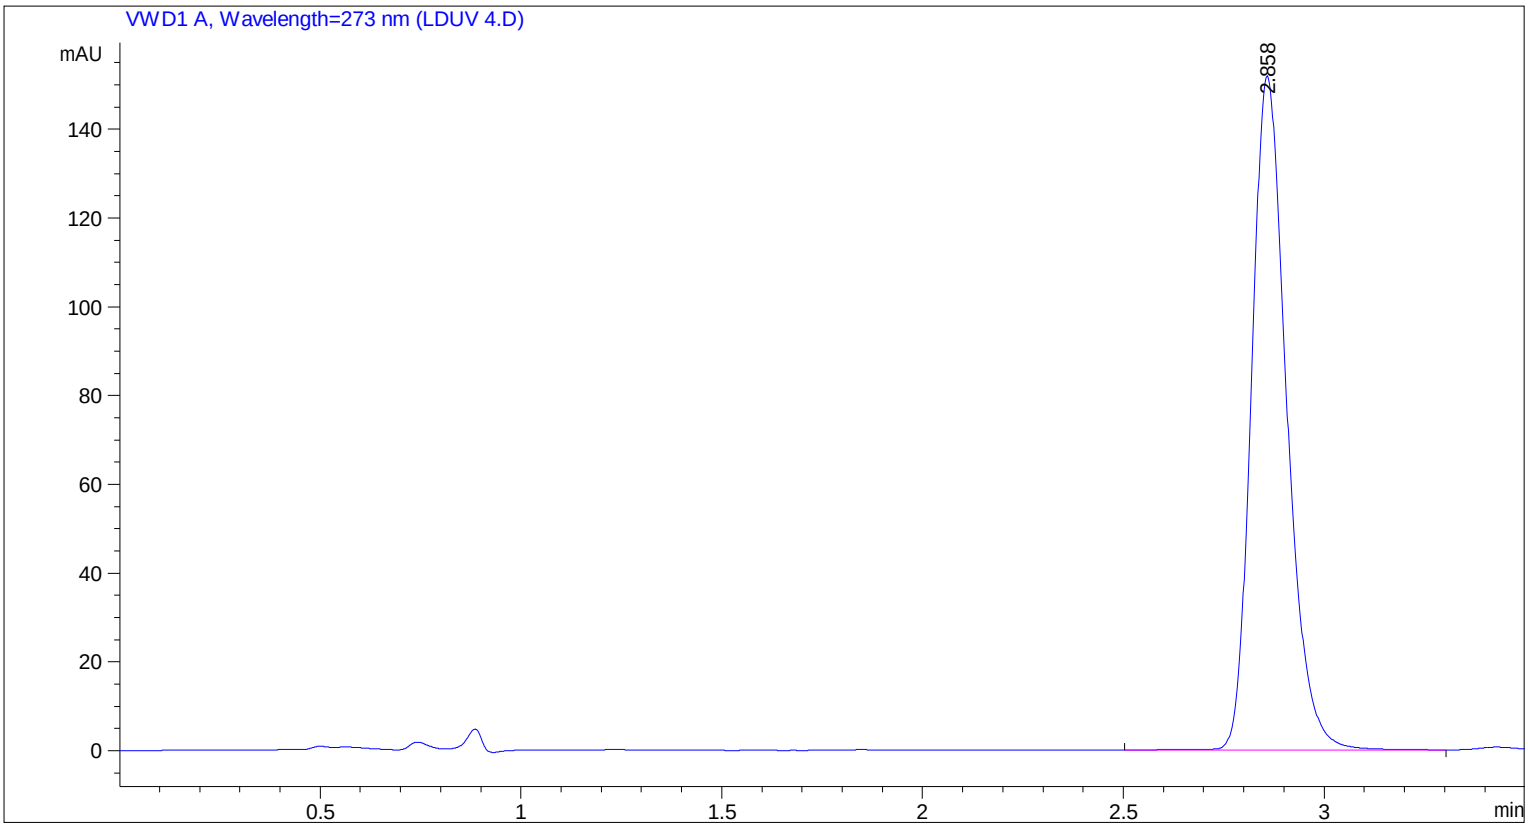


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.858 BB      0.0929  922.58392 100.0000 Cafeina

Totals :                     922.58392


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LDUV 5.D
Sample Name: LDUV 5

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  14
Acq. Instrument : HPLC                            Location : Vial 7
Injection Date  : 1/26/2017 6:57:04 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

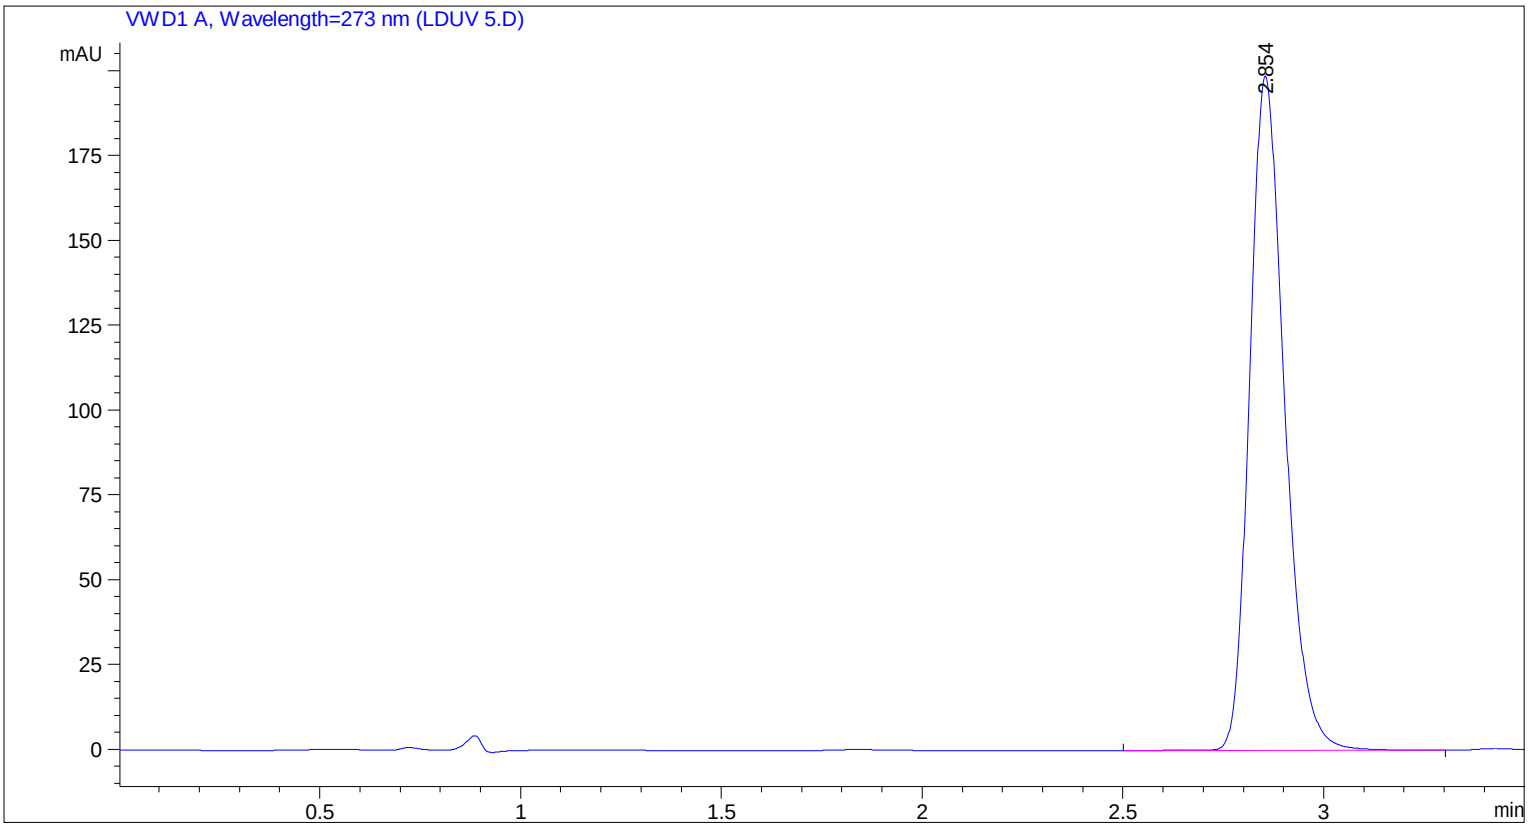


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.854 BB      0.0927 1204.71594 100.0000 Cafeina

Totals :                    1204.71594


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LIIN 1.D
Sample Name: LIIN 1

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  15
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/26/2017 7:00:43 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 0.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

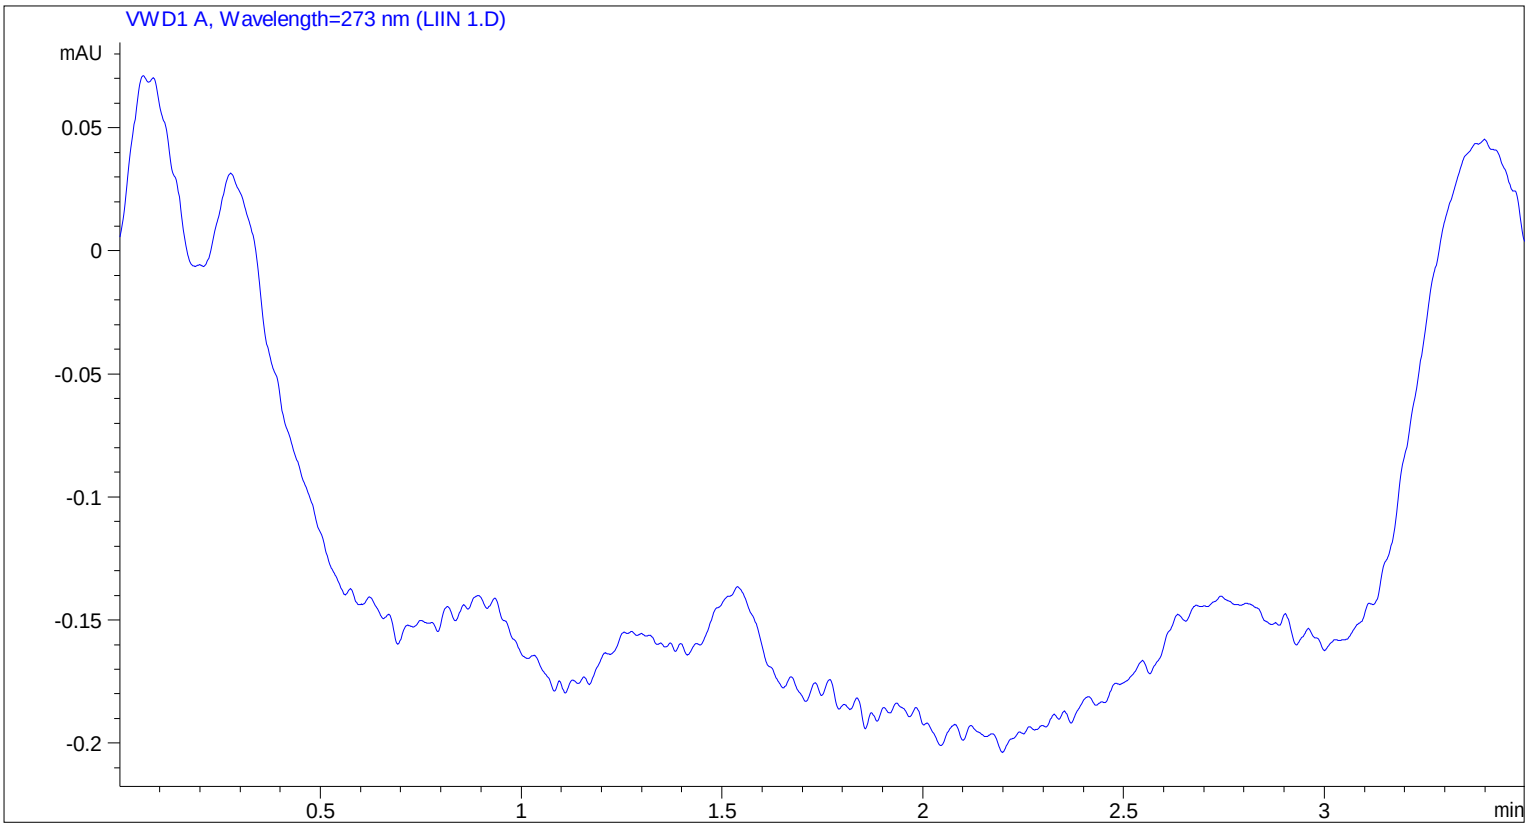


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.908         0.0000    0.00000   0.0000 Cafeina

Totals :                      0.00000


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LIIN 2.D
Sample Name: LIIN 2

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  16
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/26/2017 7:05:01 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 5.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

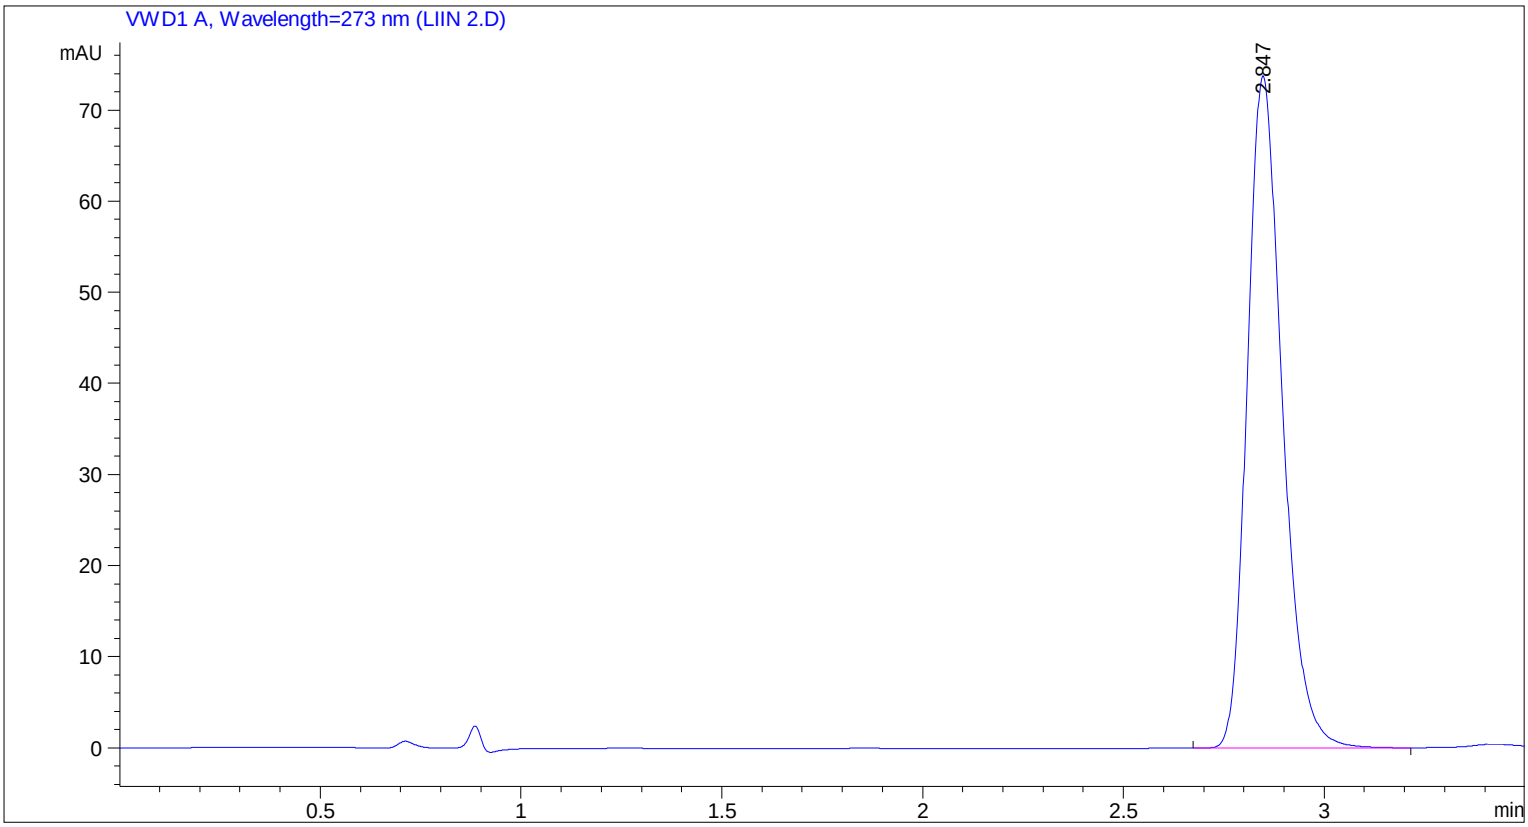


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.847 BB      0.0935  448.83920 100.0000 Cafeina

Totals :                    448.83920


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LIIN 3.D
Sample Name: LIIN 3

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  17
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/26/2017 7:09:22 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

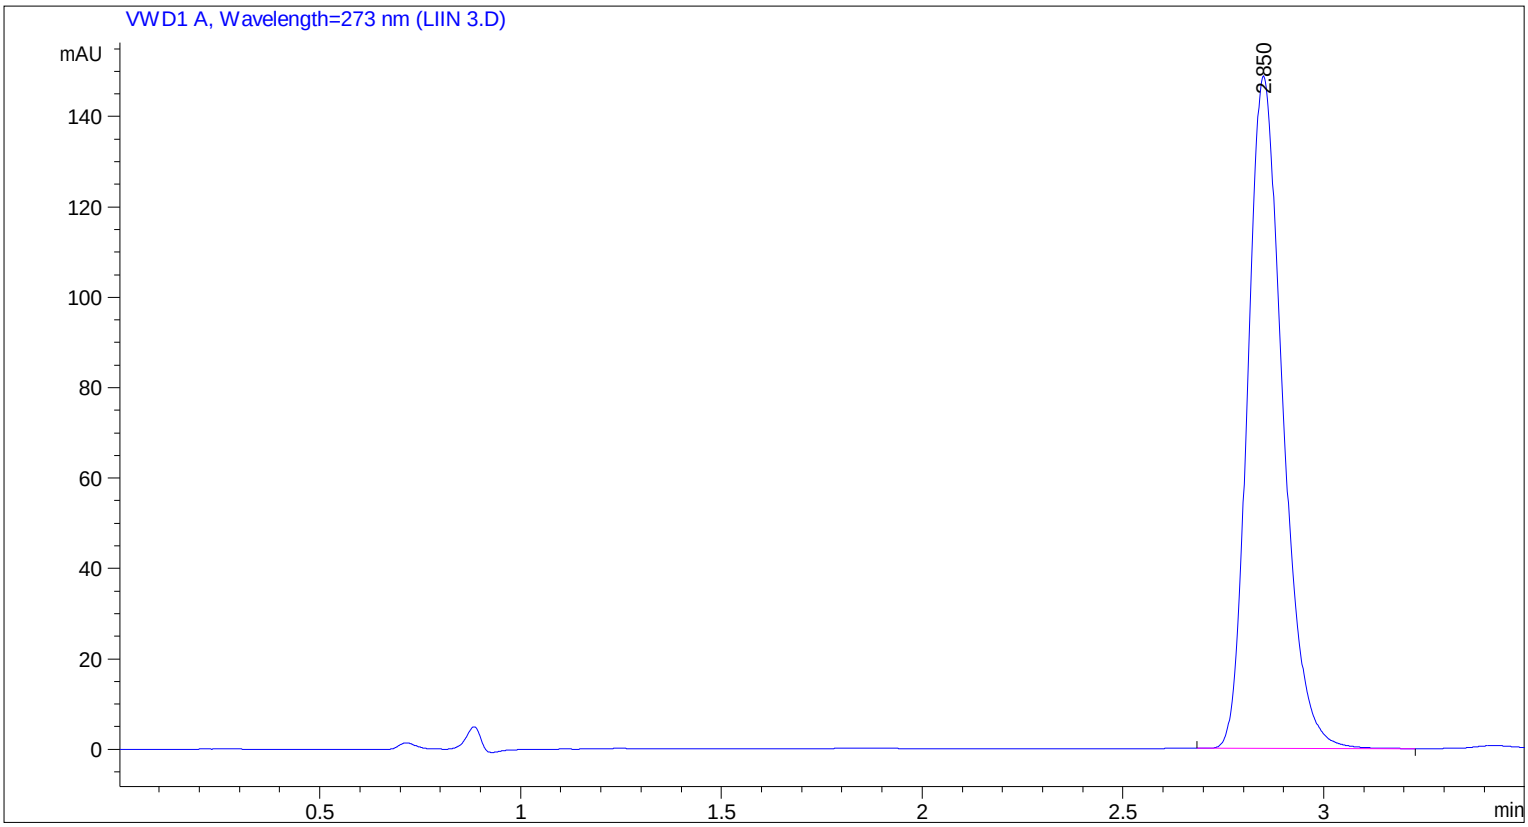


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.850 BB      0.0925  898.92114 100.0000 Cafeina

Totals :                     898.92114


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LIIN 4.D
Sample Name: LIIN 4

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  18
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/26/2017 7:13:43 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 15.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

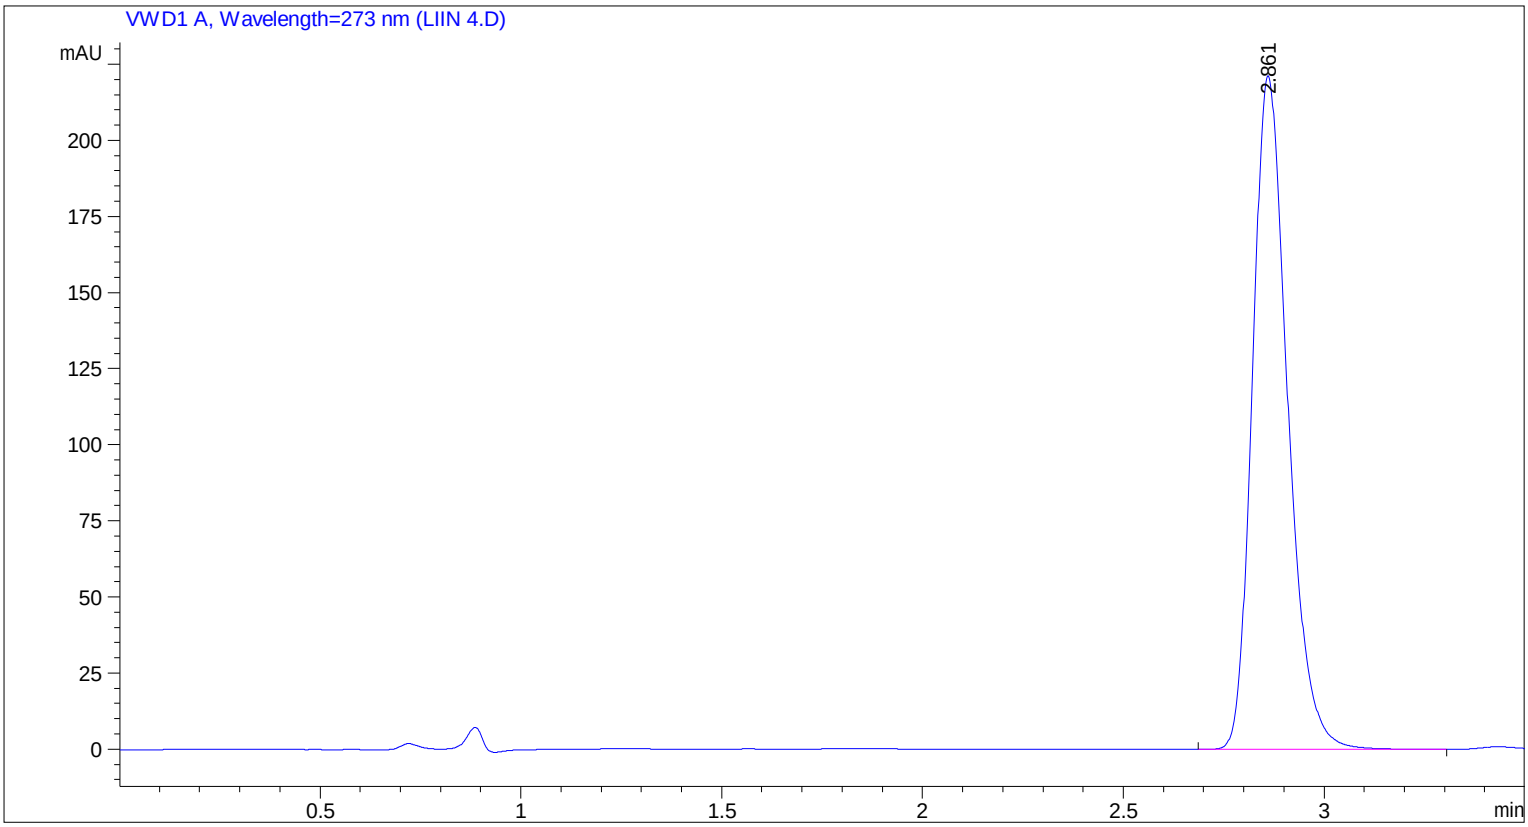


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.861 BB      0.0937 1349.85449 100.0000 Cafeina

Totals :                   1349.85449


1 Warnings or Errors :
```

Data File C:\CHEM32\2\DATA\LIIN 5.D
Sample Name: LIIN 5

```
==========================================================================
Acq. Operator   : WELLINGTON                      Seq. Line :  19
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/26/2017 7:18:08 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 20.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 5:53:42 PM by WELLINGTON
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/26/2017 6:24:41 PM by WELLINGTON
                  (modified after loading)
```

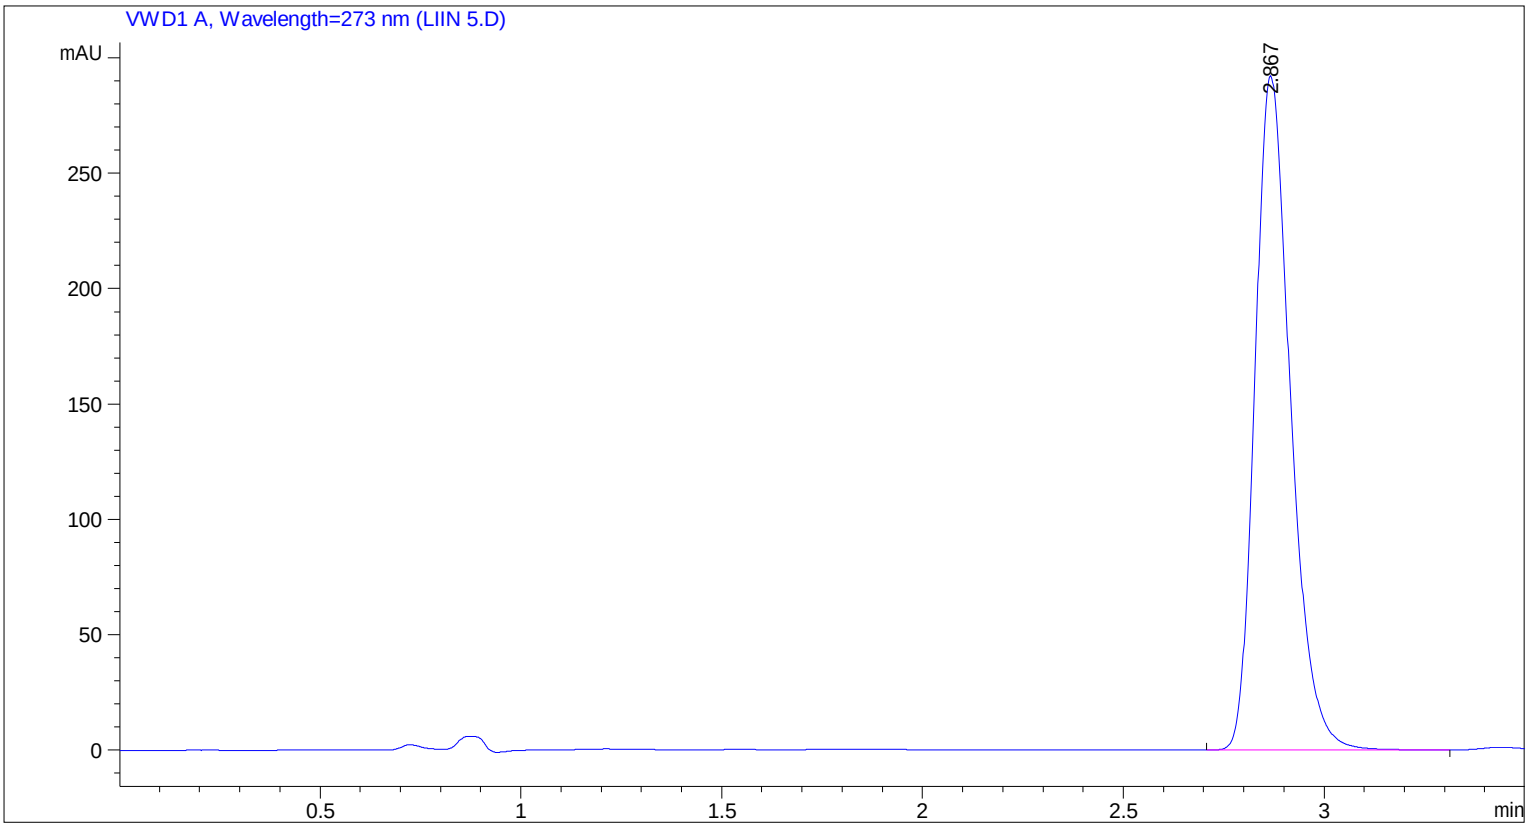


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      1/26/2017 6:24:41 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   2.867 BB      0.0944 1801.40356 100.0000 Cafeina

Totals :                    1801.40356


1 Warnings or Errors :
```