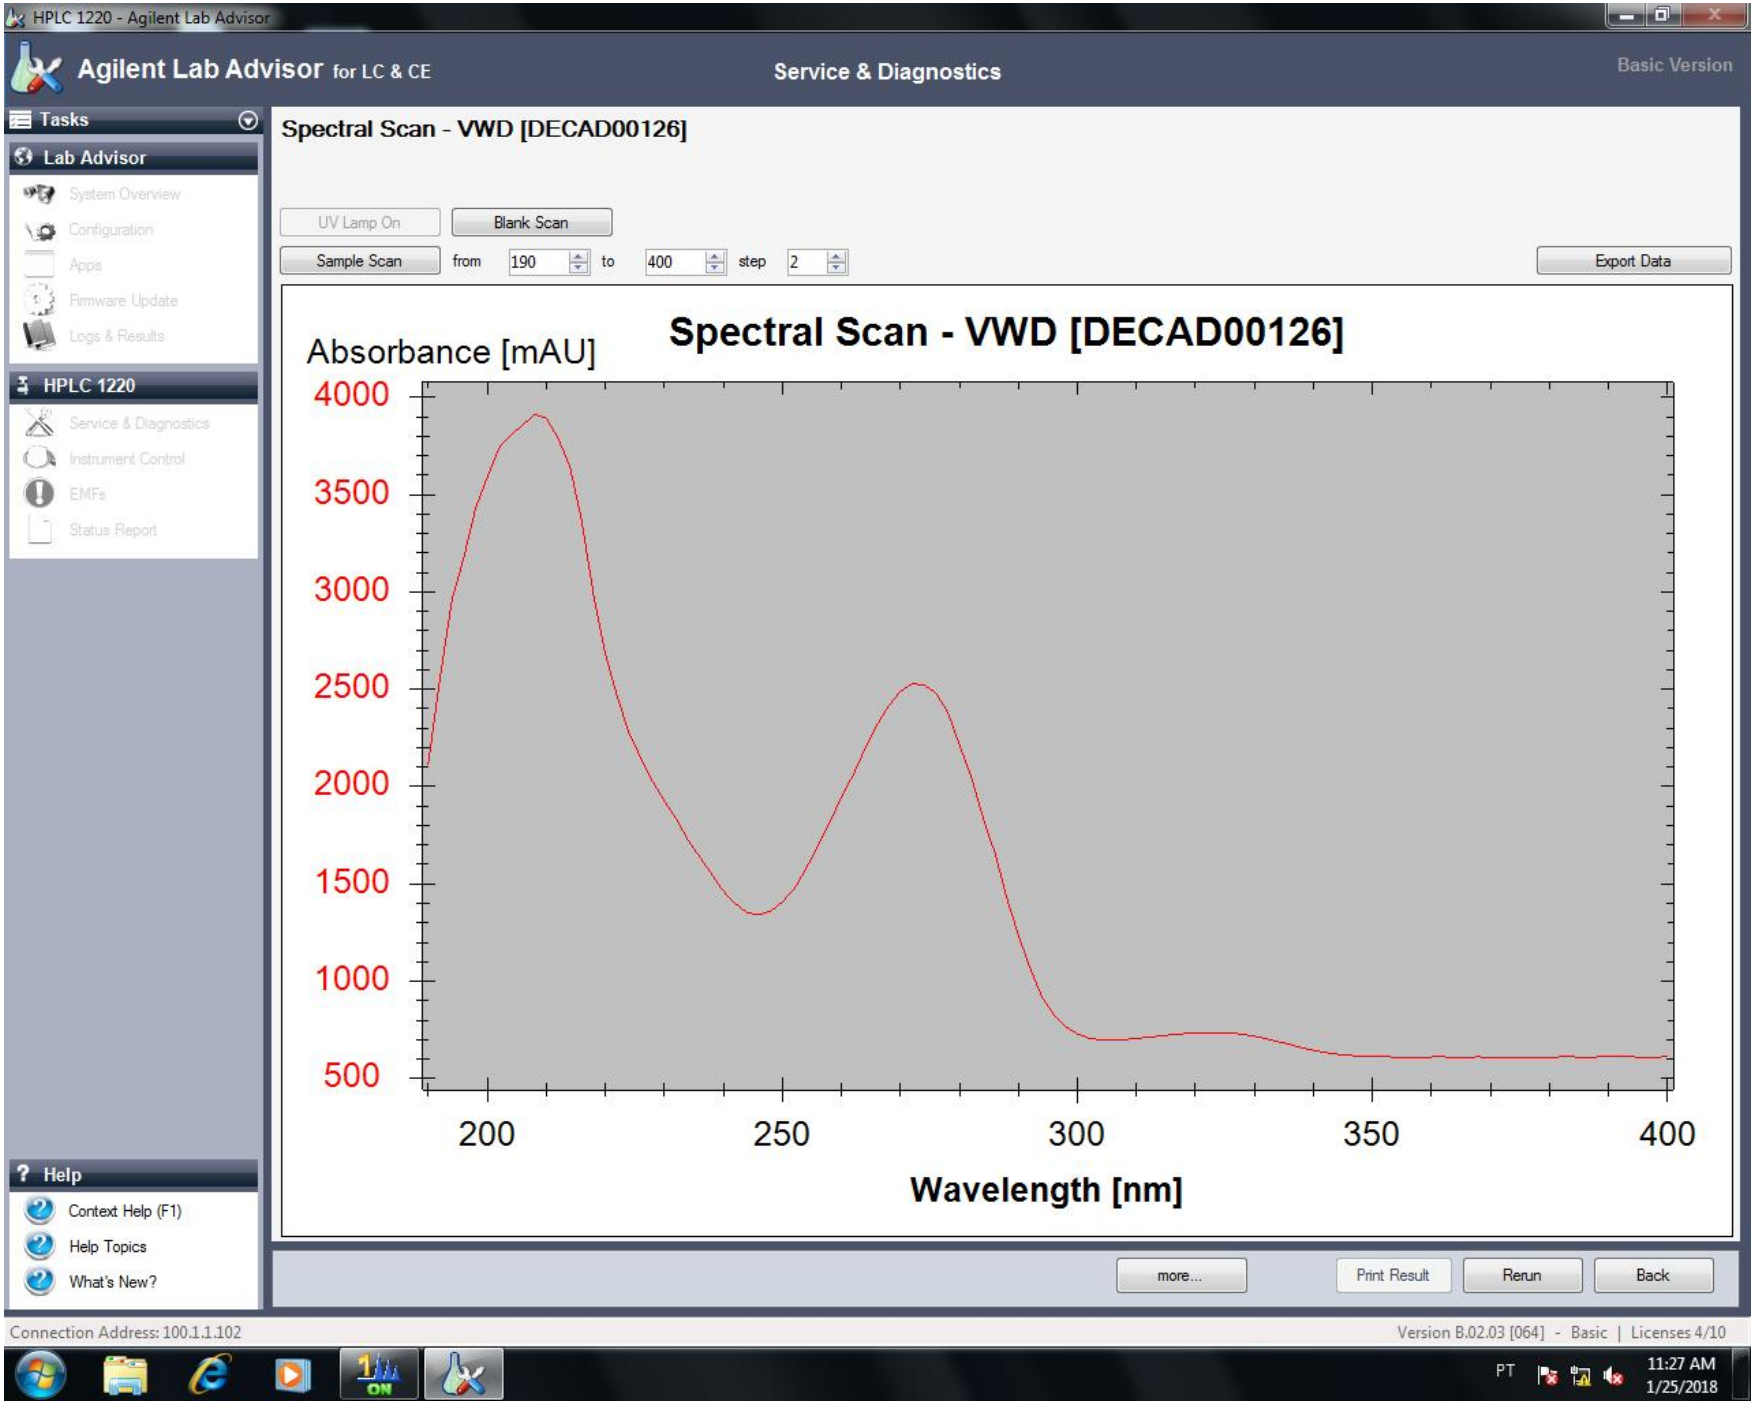
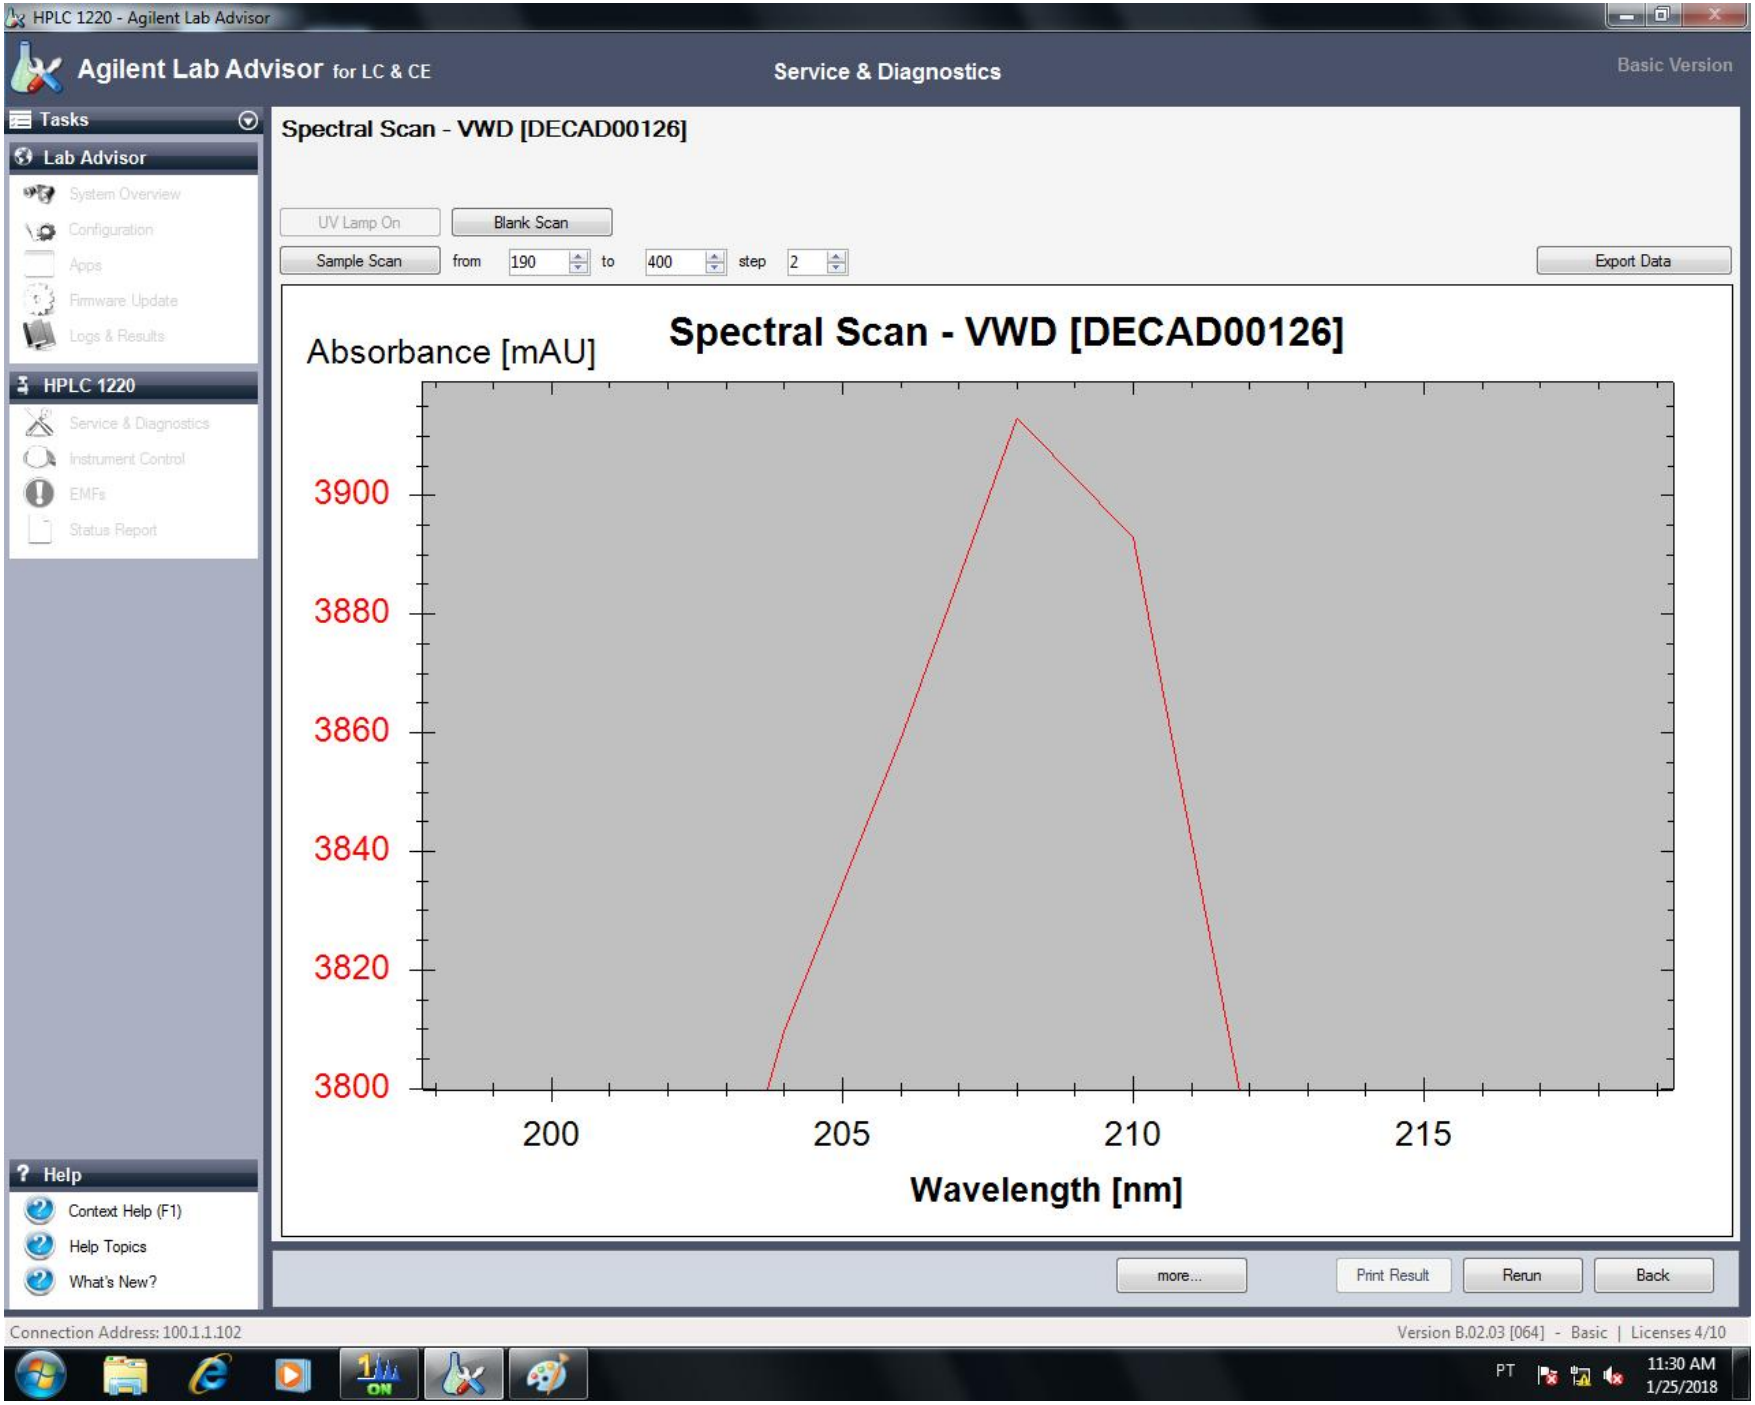
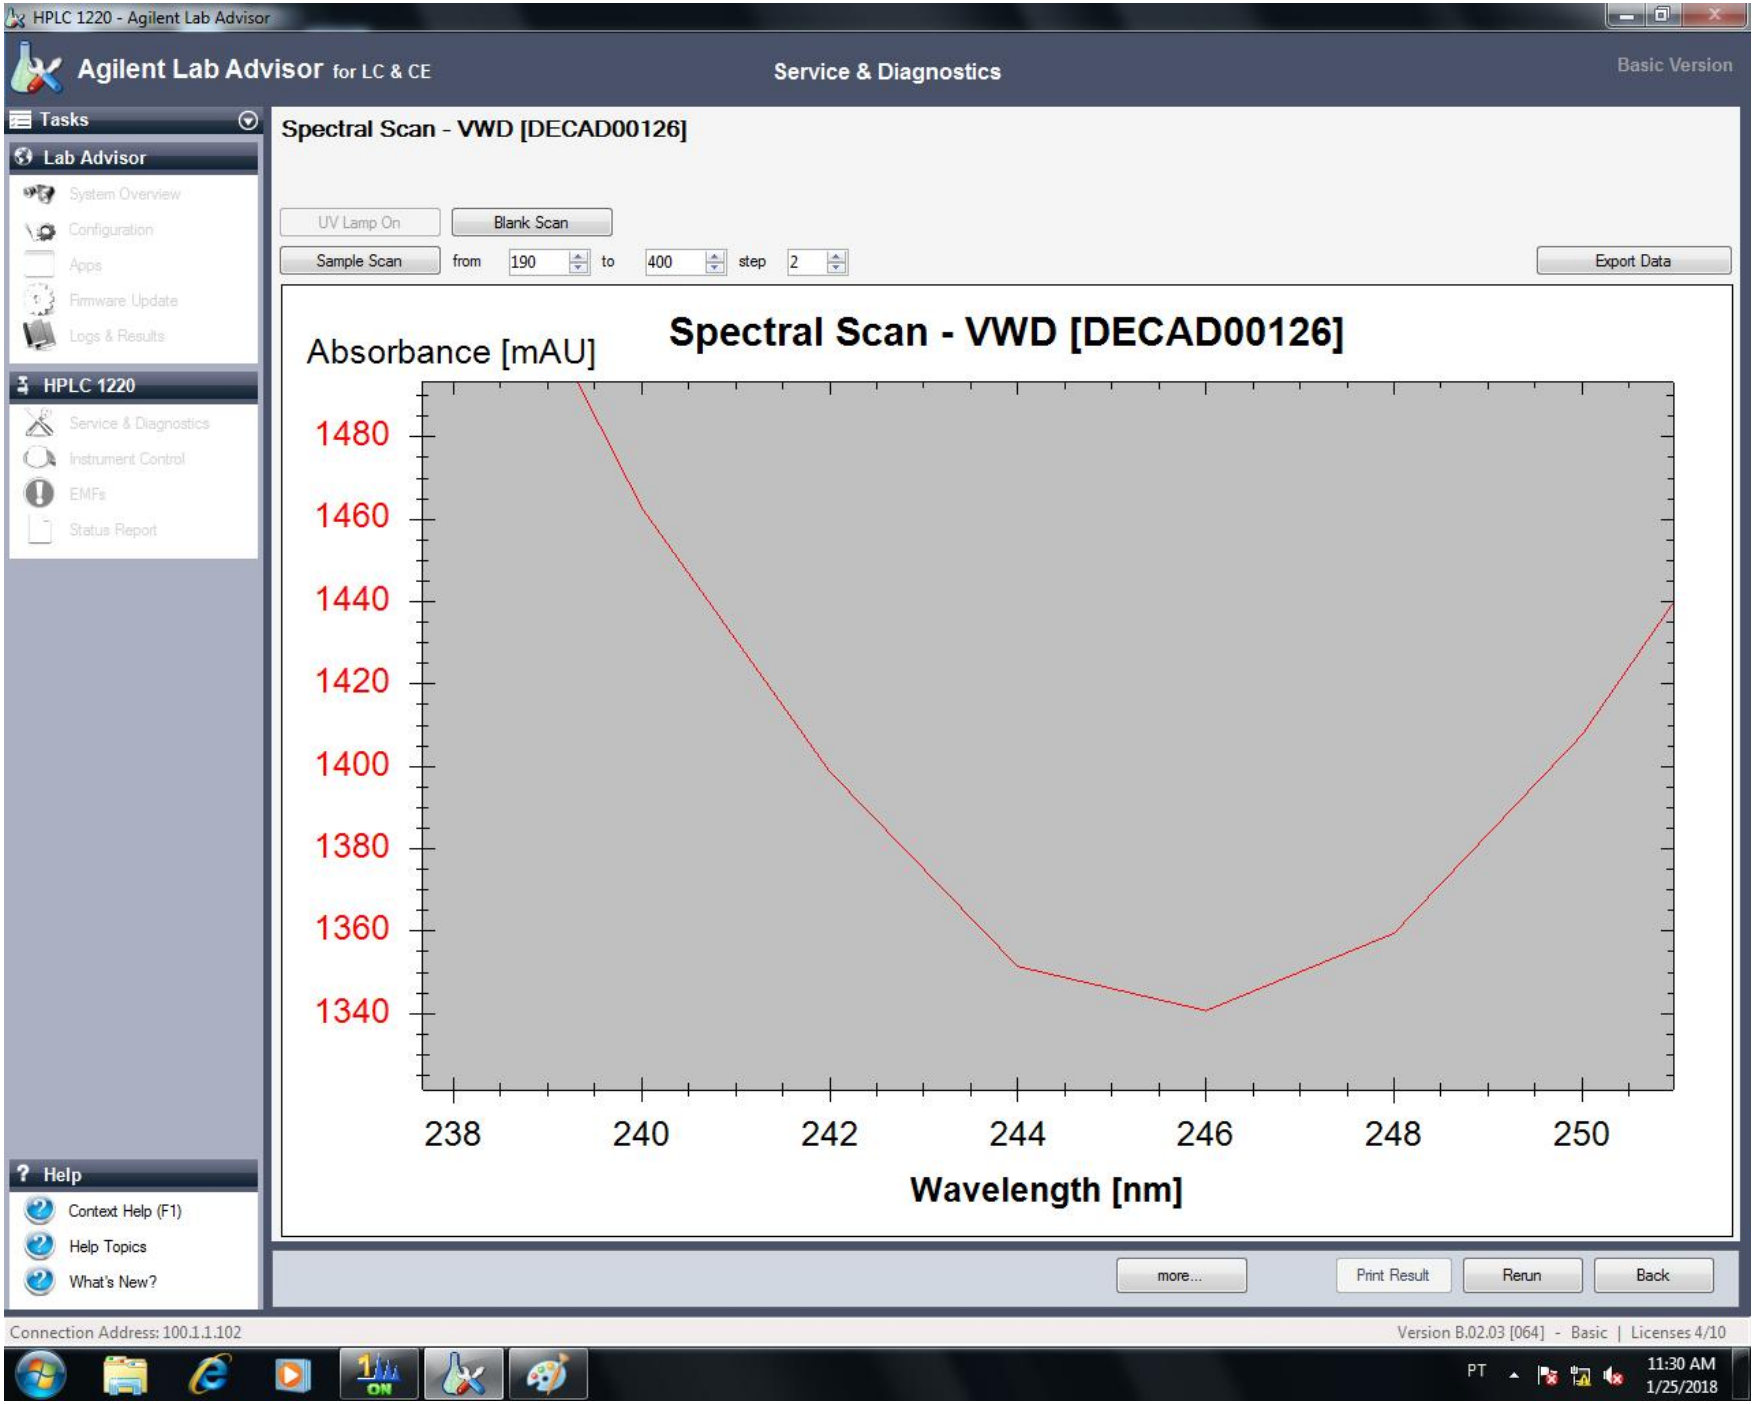
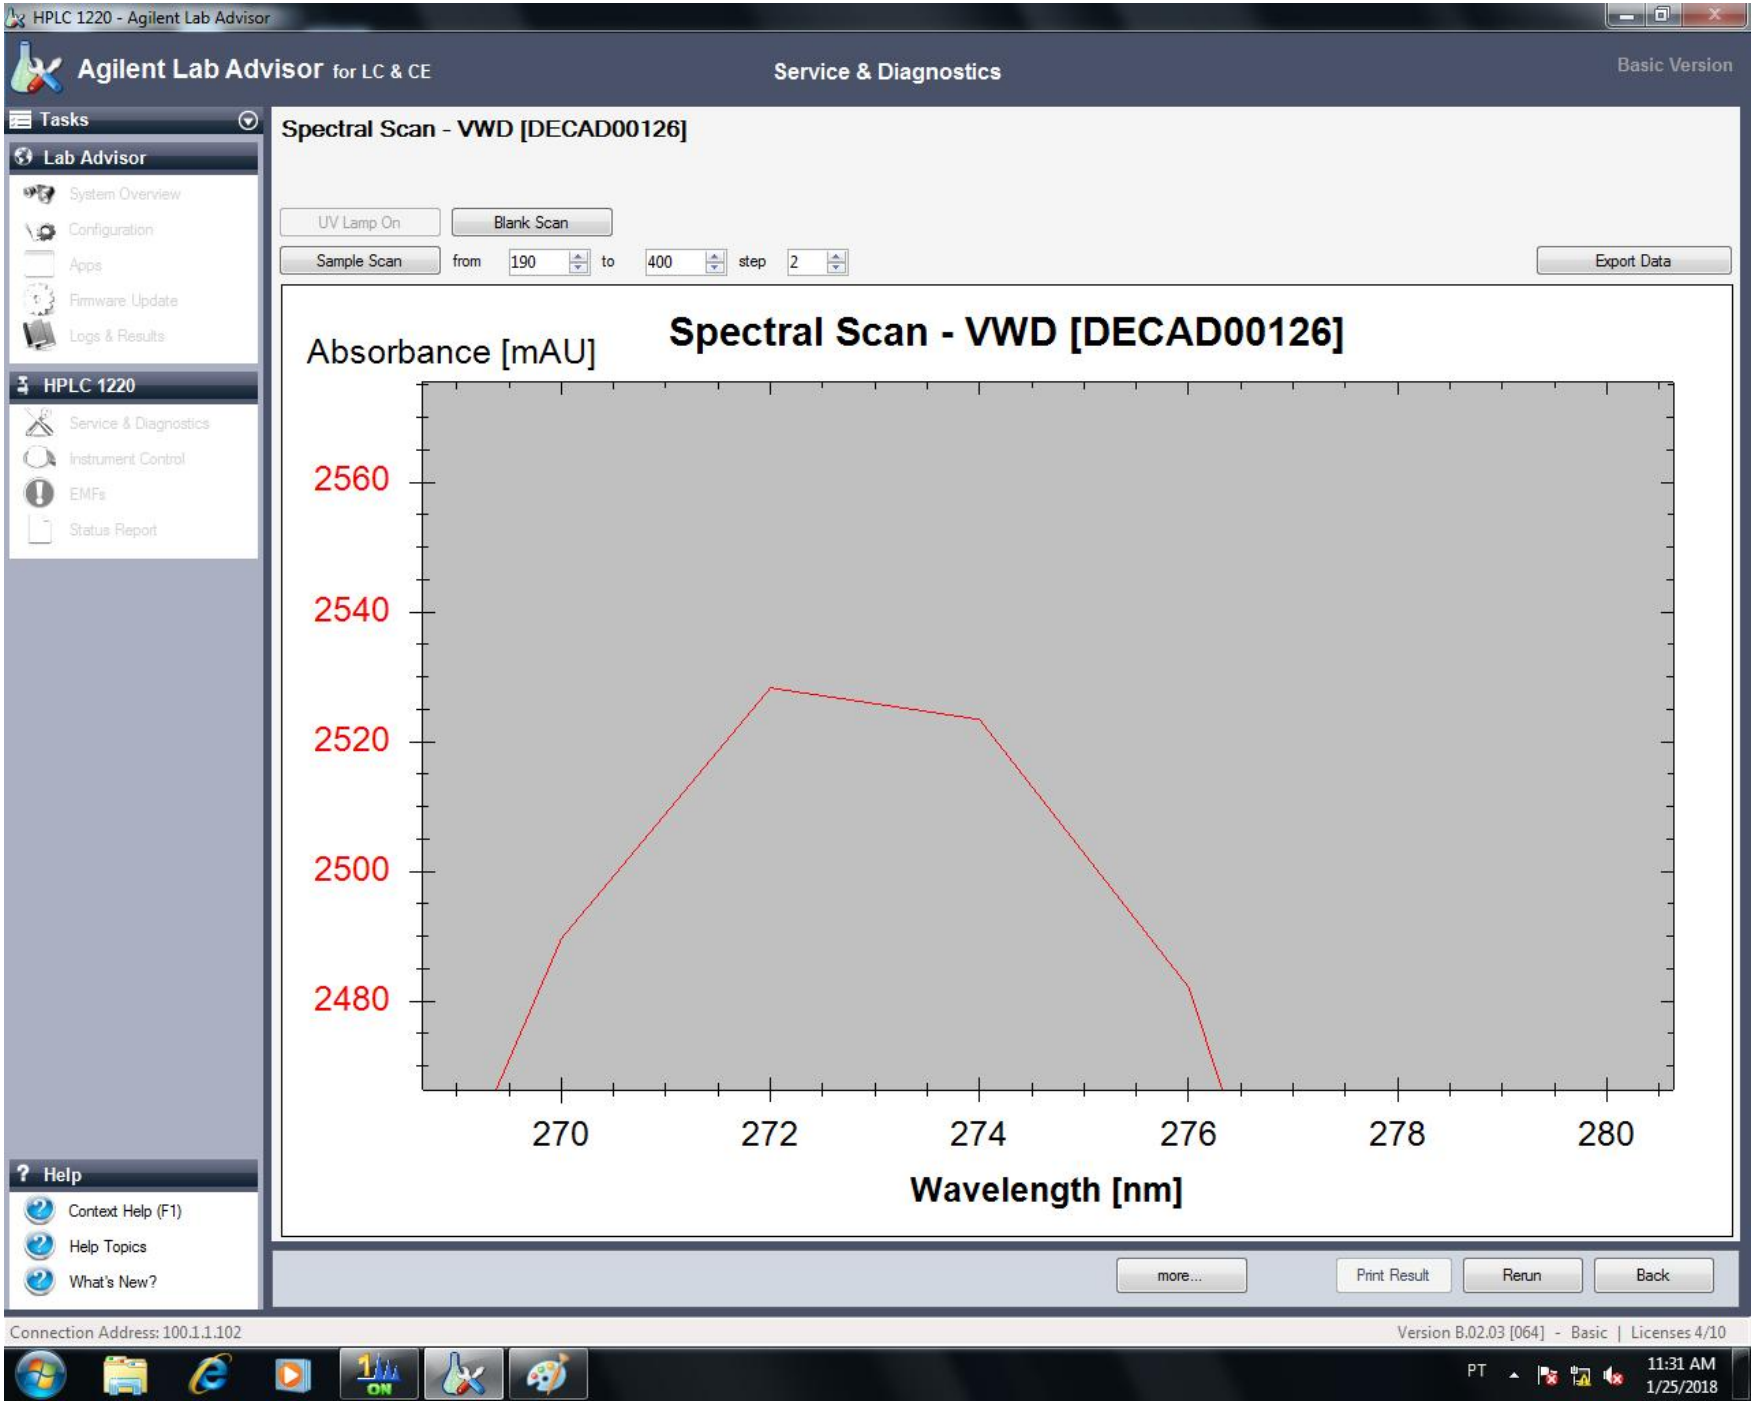

HPLC 1220 - Agilent Lab Advisor
Agilent Lab Advisor for LC & CE
Service & Diagnostics
Basic Version
Tasks
Lab Advisor
System Overview
Configuration
Apps
Firmware Update
Logs & Results
HPLC 1220
Service & Diagnostics
Instrument Control
EMFs
Status Report
Help
Context Help (F1)
Help Topics
What's New?
Spectral Scan - VWD [DECAD00126]
UV Lamp On
Blank Scan
Sample Scan
from 190
to 400
step 2
Export Data
Spectral Scan - VWD [DECAD00126]
Absorbance [mAU]
4000
3500
3000
2500
2000
1500
1000
500
200
250
300
350
400
Wavelength [nm]
more...
Print Result
Rerun
Back
Connection Address: 100.1.1.102
Version B.02.03 [064] - Basic | Licenses 4/10
PT
11:27 AM
1/25/2018



HPLC 1220 - Agilent Lab Advisor
Agilent Lab Advisor for LC & CE
Service & Diagnostics
Basic Version
Tasks
Lab Advisor
System Overview
Configuration
Apps
Firmware Update
Logs & Results
HPLC 1220
Service & Diagnostics
Instrument Control
EMFs
Status Report
Help
Context Help (F1)
Help Topics
What's New?
Spectral Scan - VWD [DECAD00126]
UV Lamp On
Blank Scan
Sample Scan
from 190
to 400
step 2
Export Data
Absorbance [mAU]
Spectral Scan - VWD [DECAD00126]
3900
3880
3860
3840
3820
3800
200
205
210
215
Wavelength [nm]
more...
Print Result
Rerun
Back
Connection Address: 100.1.1.102
Version B.02.03 [064] - Basic | Licenses 4/10
PT
11:30 AM
1/25/2018


HPLC 1220 - Agilent Lab Advisor
Agilent Lab Advisor for LC & CE
Service & Diagnostics
Basic Version
Tasks
Lab Advisor
System Overview
Configuration
Apps
Firmware Update
Logs & Results
HPLC 1220
Service & Diagnostics
Instrument Control
EMFs
Status Report
Help
Context Help (F1)
Help Topics
What's New?
Spectral Scan - VWD [DECAD00126]
UV Lamp On
Blank Scan
Sample Scan
from 190
to 400
step 2
Export Data
Spectral Scan - VWD [DECAD00126]
Absorbance [mAU]
1480
1460
1440
1420
1400
1380
1360
1340
238
240
242
244
246
248
250
Wavelength [nm]
more...
Print Result
Rerun
Back
Connection Address: 100.1.1.102
Version B.02.03 [064] - Basic | Licenses 4/10
PT
11:30 AM
1/25/2018


HPLC 1220 - Agilent Lab Advisor
Agilent Lab Advisor for LC & CE
Service & Diagnostics
Basic Version
Tasks
Lab Advisor
System Overview
Configuration
Apps
Firmware Update
Logs & Results
HPLC 1220
Service & Diagnostics
Instrument Control
EMFs
Status Report
Help
Context Help (F1)
Help Topics
What's New?
Spectral Scan - VWD [DECAD00126]
UV Lamp On
Blank Scan
Sample Scan
from 190
to 400
step 2
Export Data
Absorbance [mAU]
Spectral Scan - VWD [DECAD00126]
2560
2540
2520
2500
2480
270
272
274
276
278
280
Wavelength [nm]
more...
Print Result
Rerun
Back
Connection Address: 100.1.1.102
Version B.02.03 [064] - Basic | Licenses 4/10
PT
11:31 AM
1/25/2018

Data File C:\CHEM32\2\DATA\2018-01-25\001-0101.D
Sample Name: Branco 01

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   1
Acq. Instrument : HPLC                            Location : Vial 1
Injection Date  : 1/25/2018 1:07:57 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

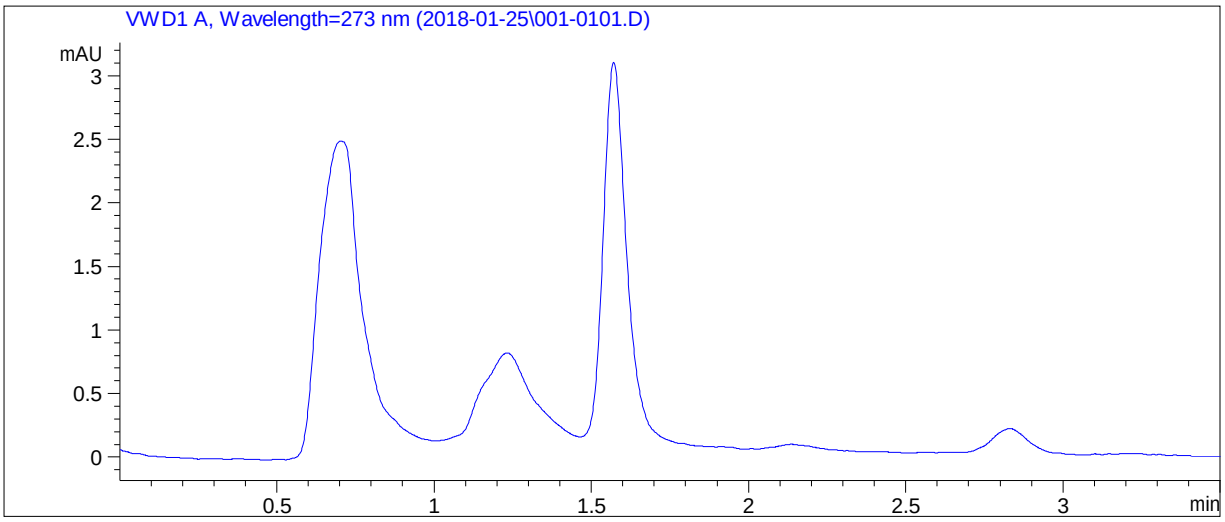


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                         *** End of Report ***
```

Data File C:\CHEM32\2\DATA\2018-01-25\002-0201.D
Sample Name: PCIN 01

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   2
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/25/2018 1:12:20 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

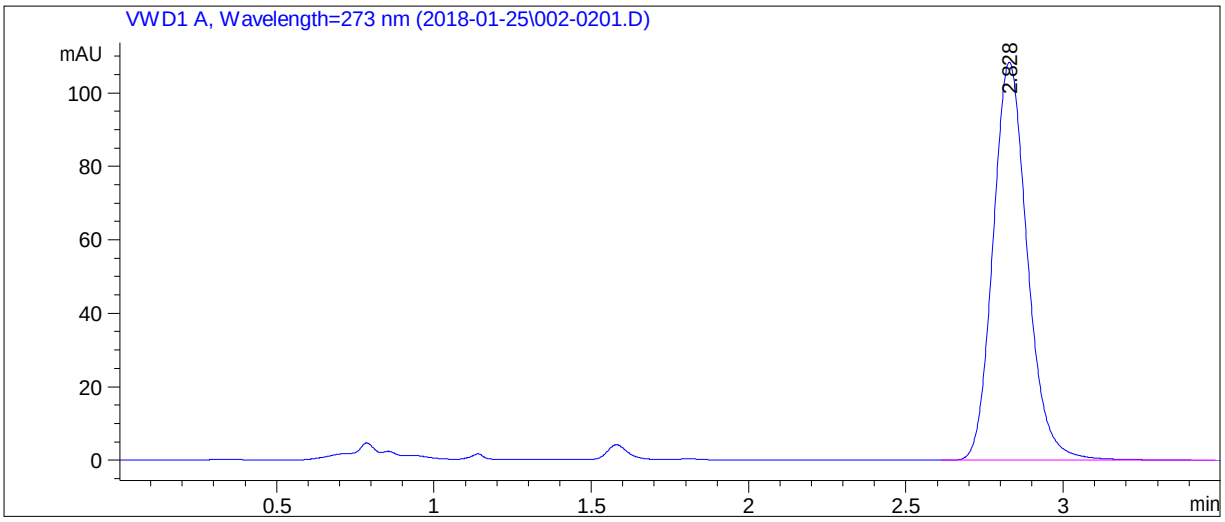


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.828 BB    0.1171  823.39331  108.43031 100.0000


Totals :                   823.39331  108.43031
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\002-0301.D
Sample Name: PCIN 02

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   3
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/25/2018 1:16:43 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

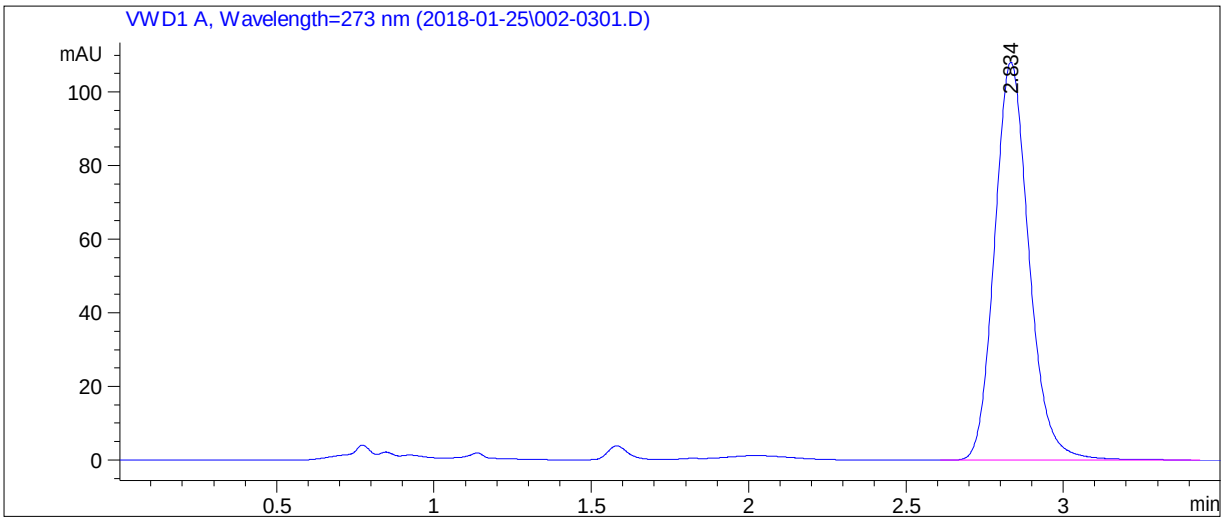


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.834 BB    0.1172  821.65210  108.11284 100.0000


Totals :                   821.65210  108.11284
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\002-0401.D
Sample Name: PCIN 03

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   4
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/25/2018 1:21:06 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

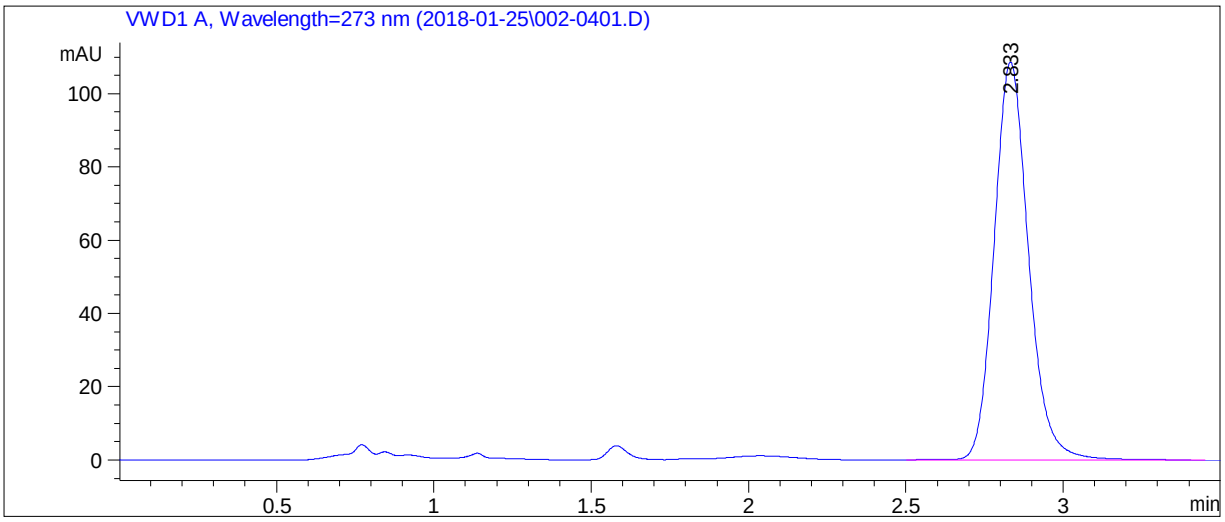


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.833 BB    0.1172  825.02411  108.55399 100.0000


Totals :                   825.02411  108.55399
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\001-0501.D
Sample Name: Branco 02

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   5
Acq. Instrument : HPLC                            Location : Vial 1
Injection Date  : 1/25/2018 1:25:27 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

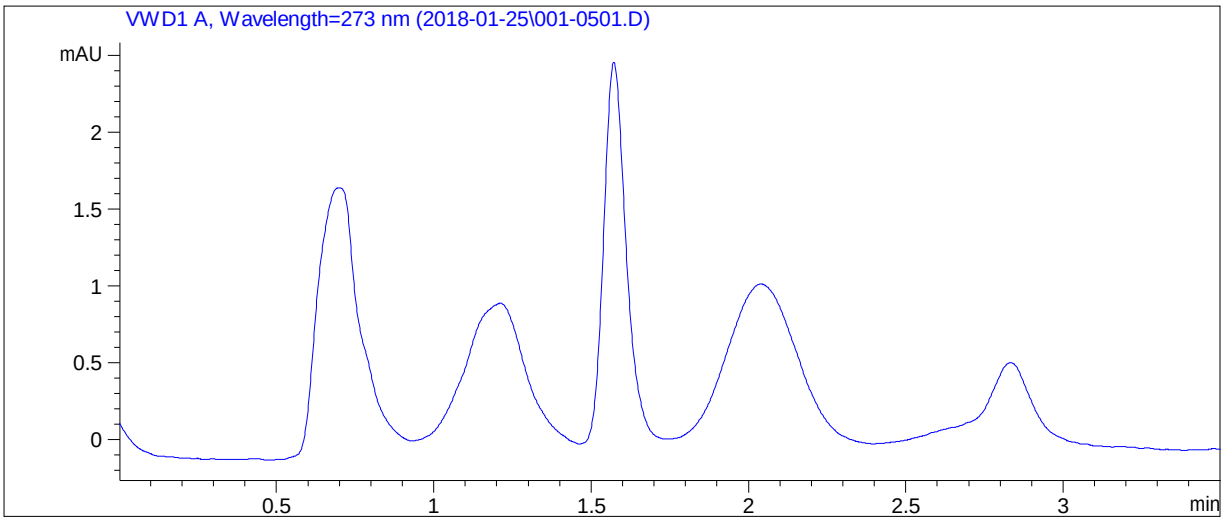


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                         *** End of Report ***
```

Data File C:\CHEM32\2\DATA\2018-01-25\002-0601.D
Sample Name: PCIN 04

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   6
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 1/25/2018 1:29:53 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

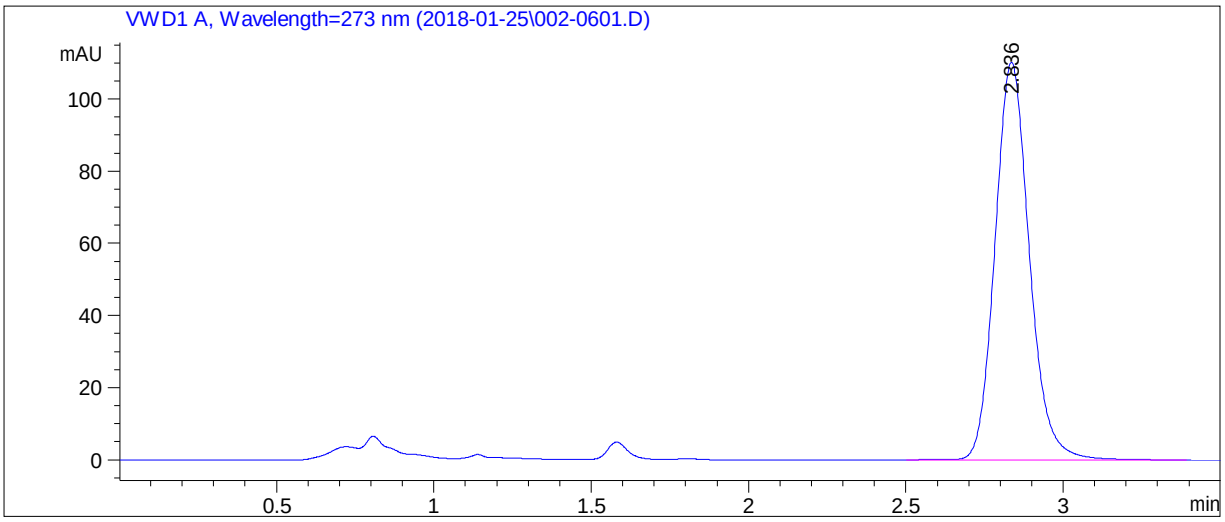


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.836 BB    0.1170  836.39215  110.23160 100.0000


Totals :                   836.39215  110.23160
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\002-0701.D
Sample Name: PCIN 05

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)              Seq. Line :   7
Acq. Instrument : HPLC                         Location : Vial 2
Injection Date  : 1/25/2018 1:34:17 PM              Inj :   1
                                              Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

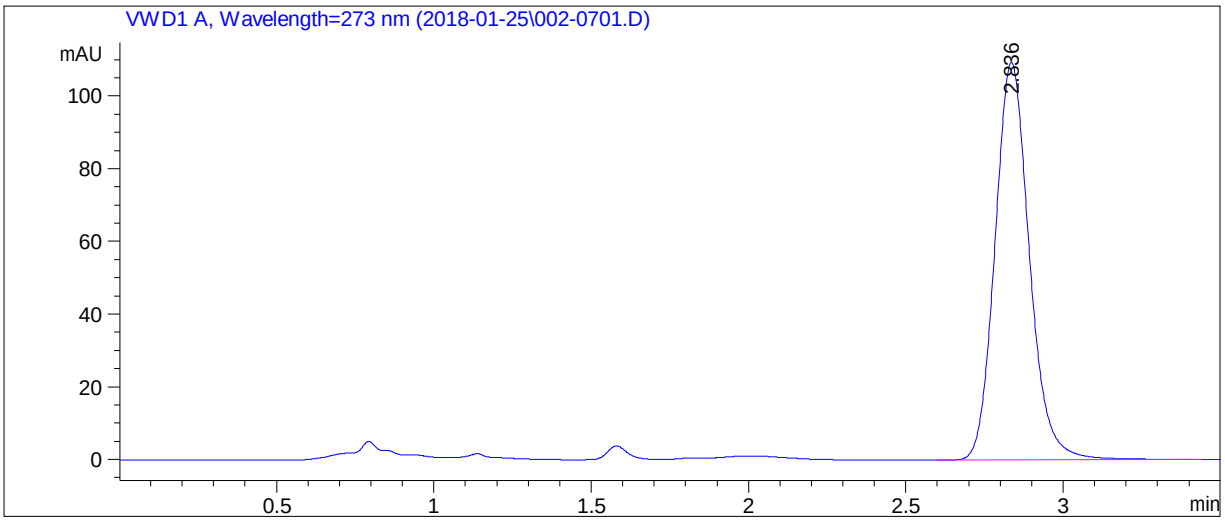


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.836 BB    0.1171  830.45911  109.41052 100.0000


Totals :                   830.45911  109.41052
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\002-0801.D
Sample Name: PCIN 06

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :   8
Acq. Instrument : HPLC                           Location : Vial 2
Injection Date  : 1/25/2018 1:38:40 PM                Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

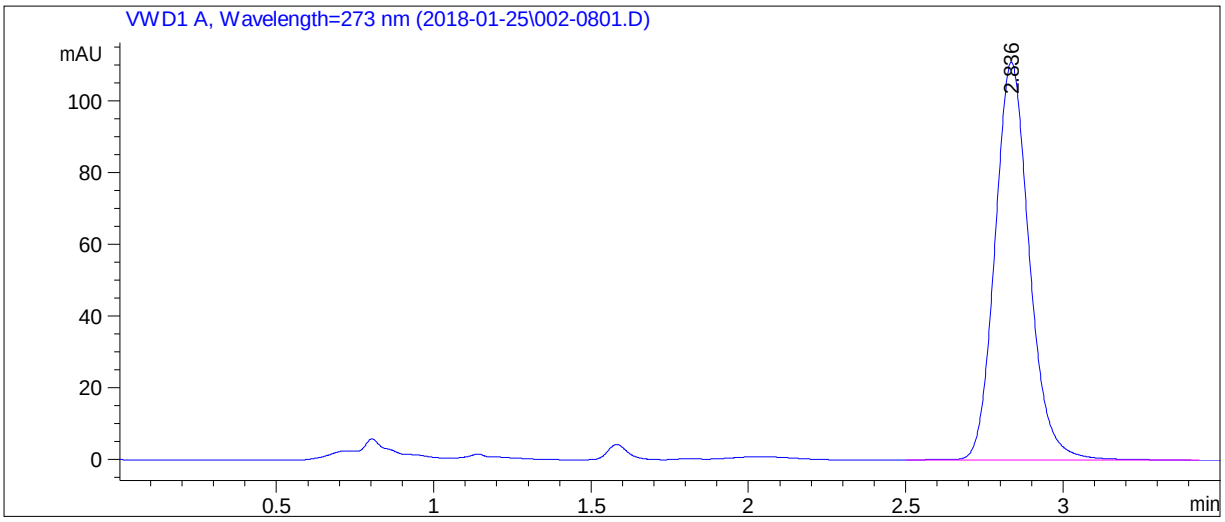


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.836 BB    0.1170  841.76813  110.95871 100.0000


Totals :                   841.76813  110.95871
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\001-0901.D
Sample Name: Branco 03

Acq. Operator	: Rodolfo (Verde)	Seq. Line	: 9
Acq. Instrument	: HPLC	Location	: Vial 1
Injection Date	: 1/25/2018 1:43:03 PM	Inj	: 1
		Inj Volume	: 10.000 µl
Acq. Method	: C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M		
Last changed	: 1/25/2018 11:16:44 AM by JOSÉ CARLOS		
Analysis Method	: C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M		
Last changed	: 1/25/2018 1:18:27 PM by Rodolfo (Verde) (modified after loading)		

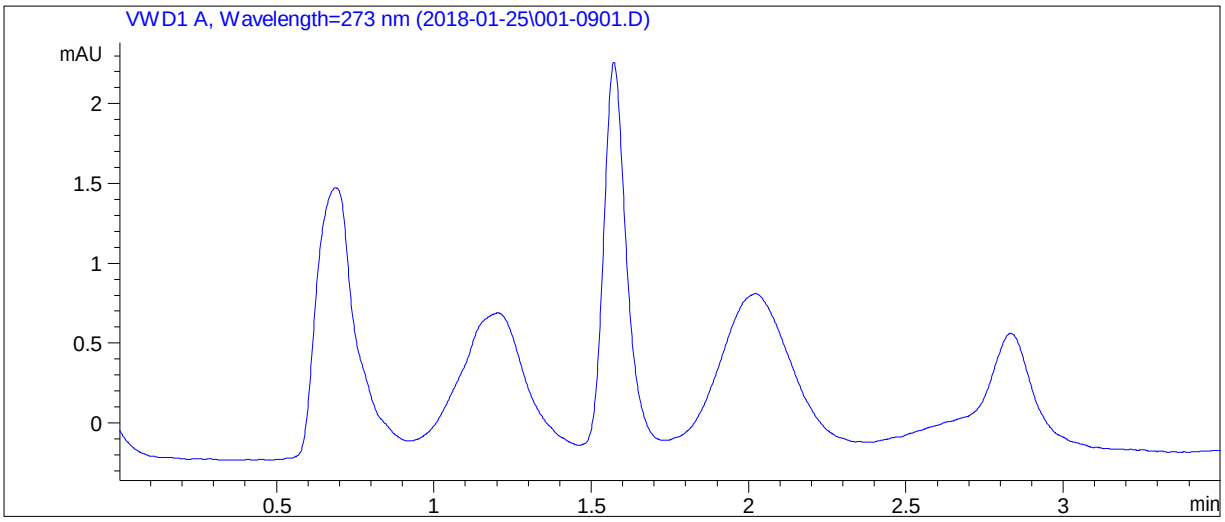

External Standard Report

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

Area Percent Report


Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\003-1001.D
Sample Name: LDUV 01

Acq. Operator	: Rodolfo (Verde)	Seq. Line	: 10
Acq. Instrument	: HPLC	Location	: Vial 3
Injection Date	: 1/25/2018 1:47:23 PM	Inj	: 1
		Inj Volume	: 10.000 µl
Acq. Method	: C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M		
Last changed	: 1/25/2018 11:16:44 AM by JOSÉ CARLOS		
Analysis Method	: C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M		
Last changed	: 1/25/2018 1:18:27 PM by Rodolfo (Verde) (modified after loading)		

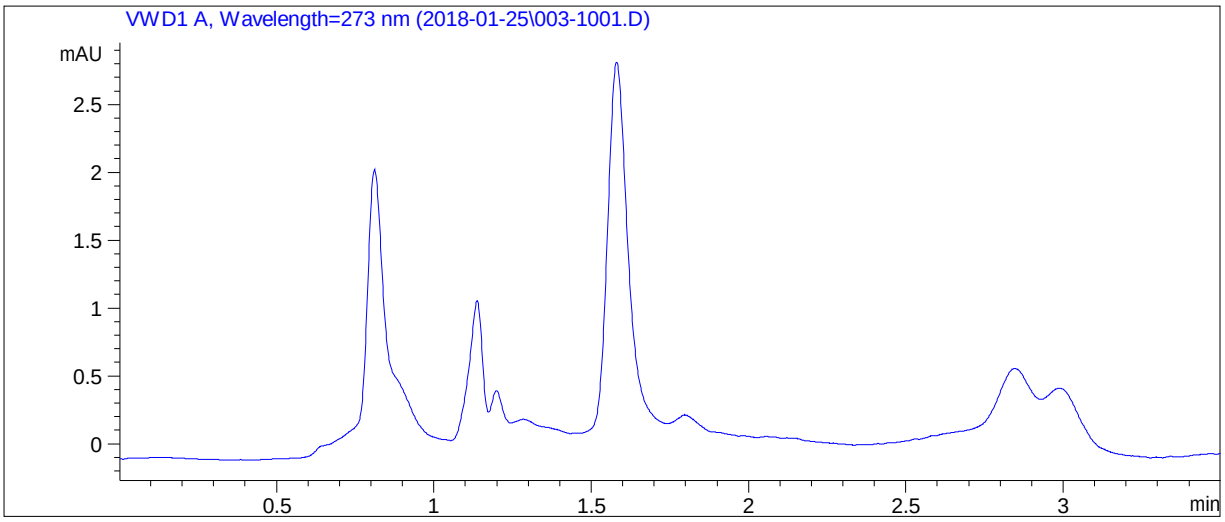

External Standard Report

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

Area Percent Report


Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\004-1101.D
Sample Name: LDUV 02

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :  11
Acq. Instrument : HPLC                            Location : Vial 4
Injection Date  : 1/25/2018 1:51:48 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

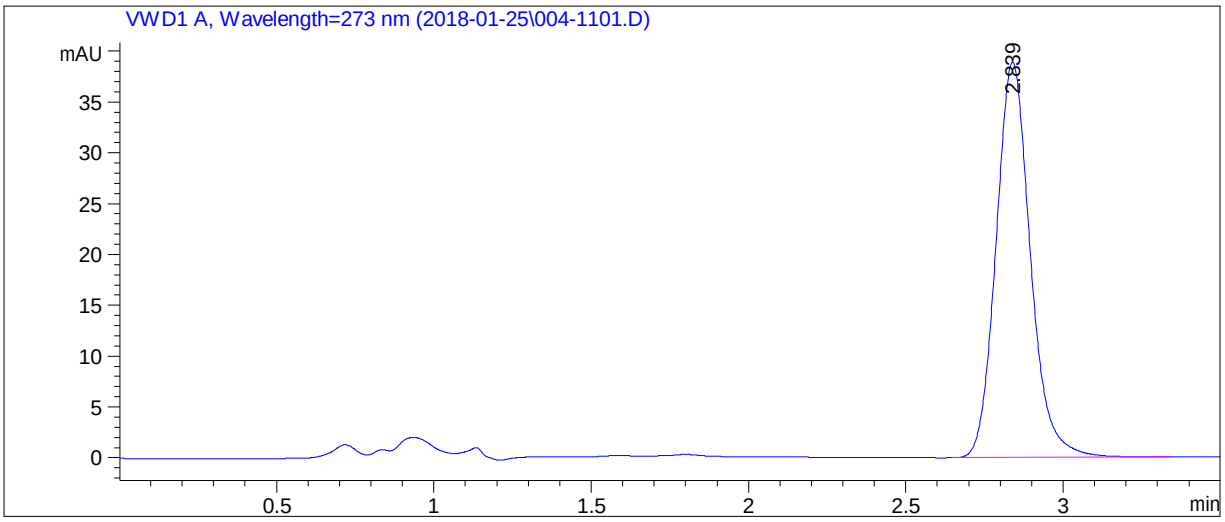


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.839 BB    0.1166  295.44595   38.90517 100.0000


Totals :                   295.44595   38.90517
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\005-1201.D
Sample Name: LDUV 03

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :  12
Acq. Instrument : HPLC                            Location : Vial 5
Injection Date  : 1/25/2018 1:56:10 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

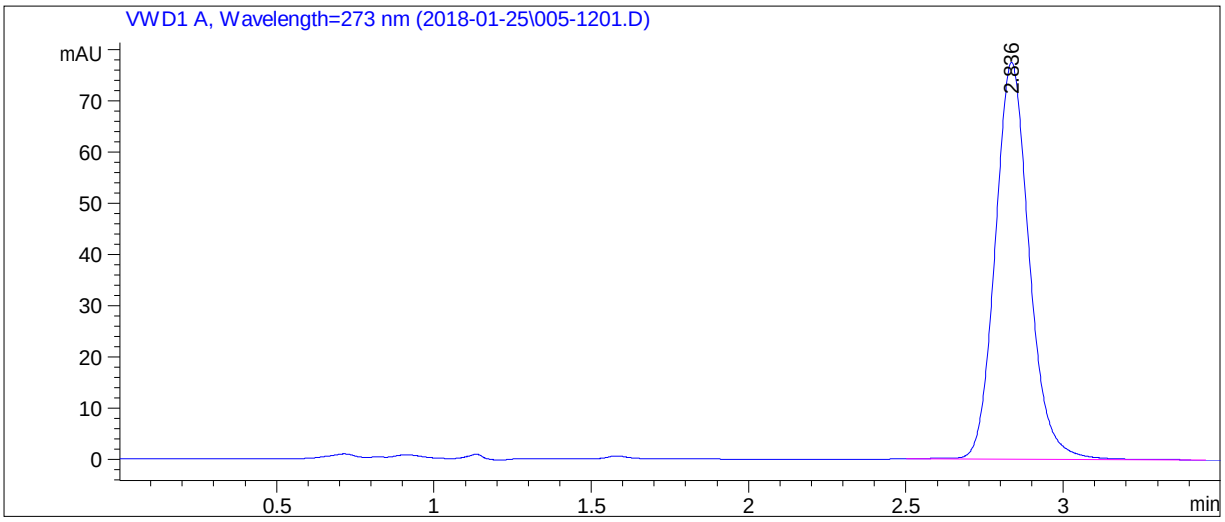


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.836 BBA   0.1157  582.85669   77.55527 100.0000


Totals :                   582.85669   77.55527
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\006-1301.D
Sample Name: LDUV 04

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :  13
Acq. Instrument : HPLC                            Location : Vial 6
Injection Date  : 1/25/2018 2:00:33 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

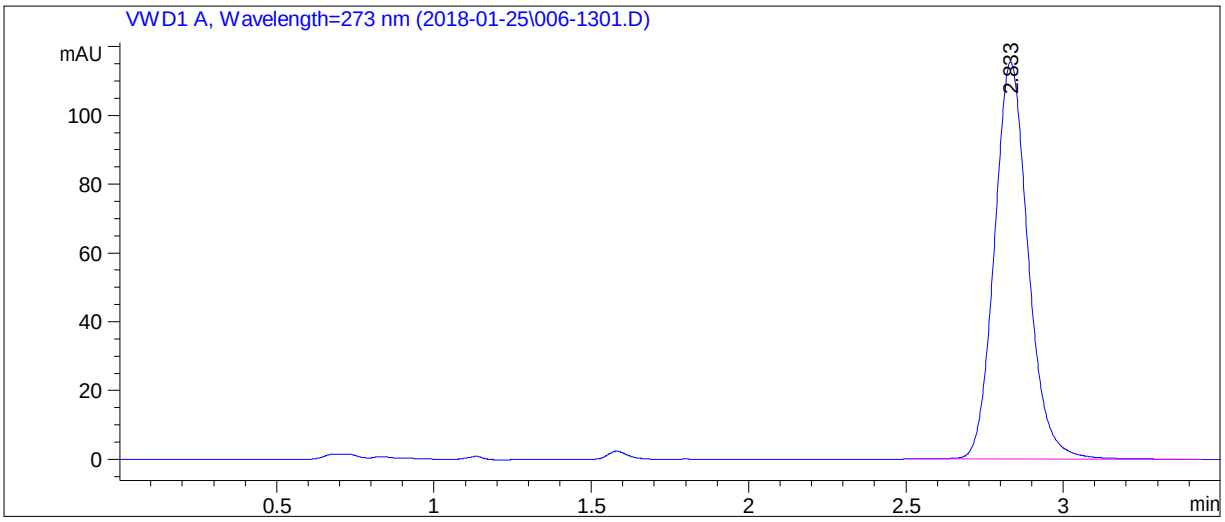


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.833 BB    0.1147  862.43195  115.41978 100.0000


Totals :                   862.43195  115.41978
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\007-1401.D
Sample Name: LDUV 05

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)               Seq. Line :  14
Acq. Instrument : HPLC                          Location : Vial 7
Injection Date  : 1/25/2018 2:04:55 PM               Inj :   1
                                               Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

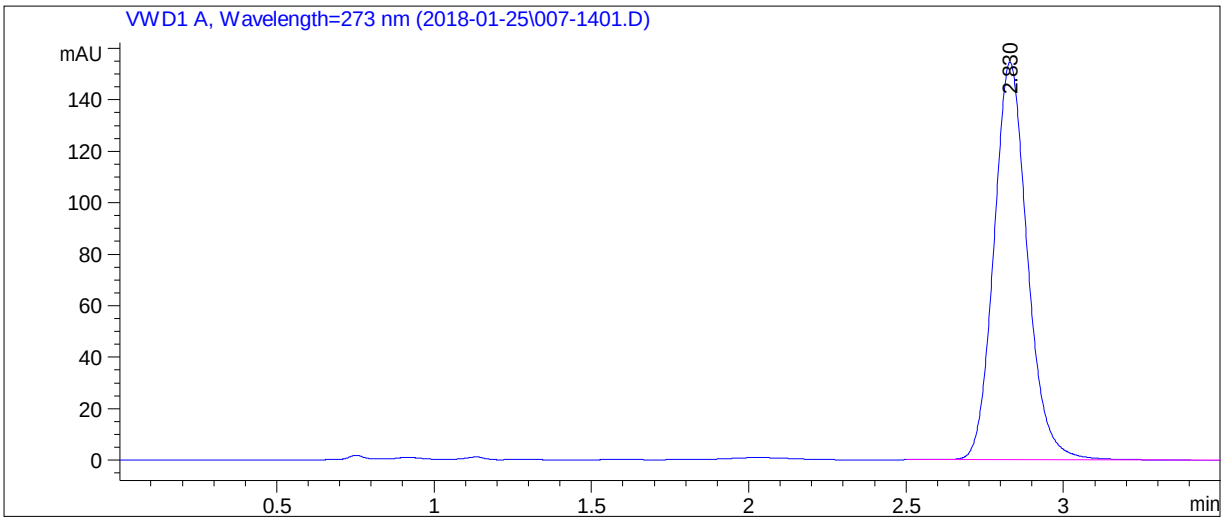


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.830 BBA   0.1135 1145.44885  154.50868 100.0000


Totals :                  1145.44885  154.50868
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\008-1501.D
Sample Name: LIIN 01

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :  15
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/25/2018 2:08:34 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 0.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

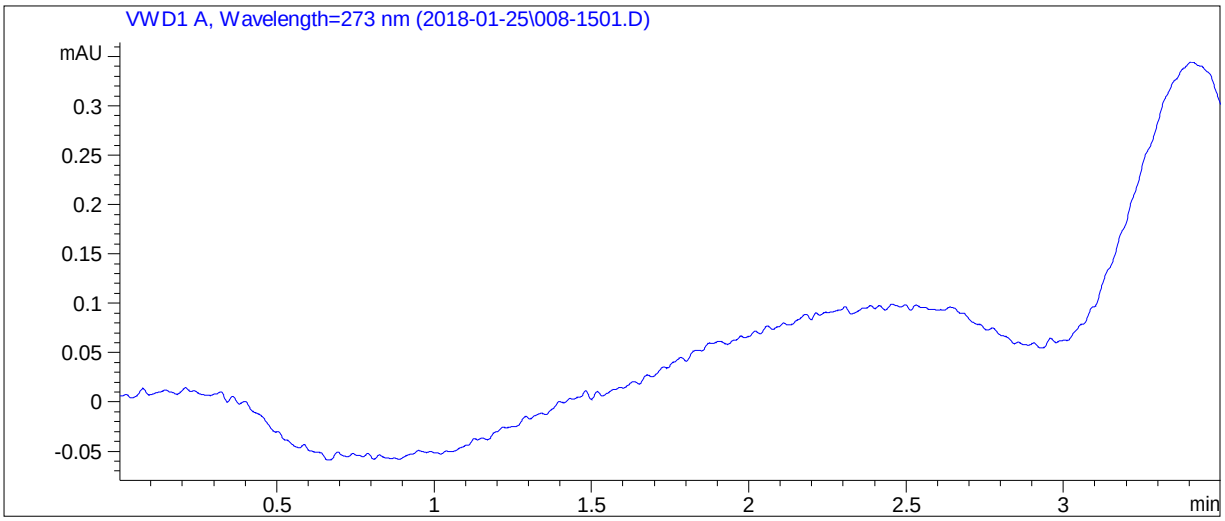


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\2018-01-25\008-1601.D
Sample Name: LIIN 02

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)               Seq. Line :  16
Acq. Instrument : HPLC                          Location : Vial 8
Injection Date  : 1/25/2018 2:12:54 PM               Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 5.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

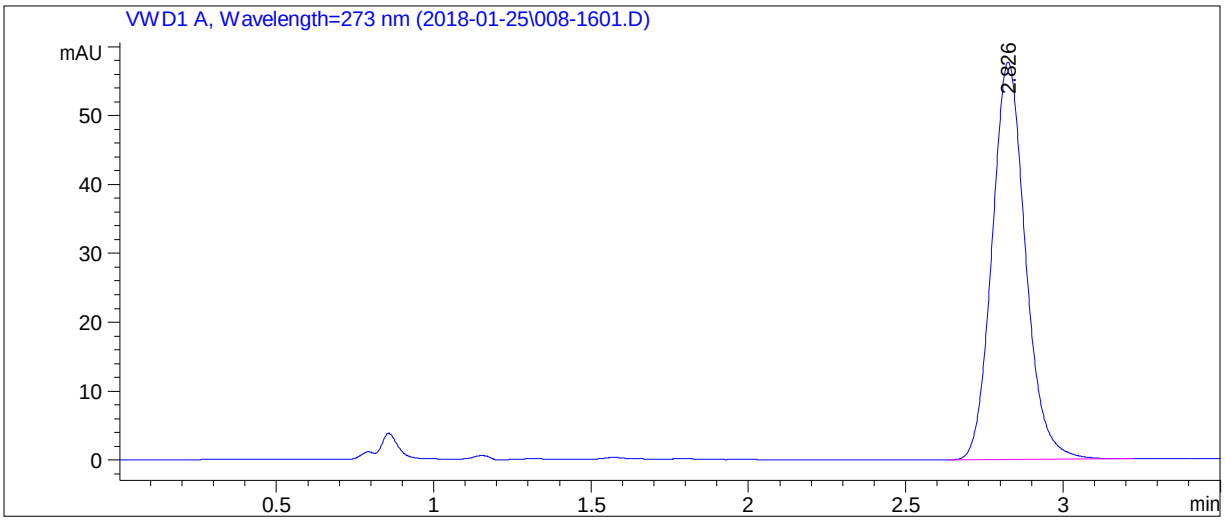


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.826 BB    0.1136  425.95404   57.71646 100.0000


Totals :                   425.95404   57.71646
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\008-1701.D
Sample Name: LIIN 03

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)                Seq. Line :  17
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 1/25/2018 2:17:14 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

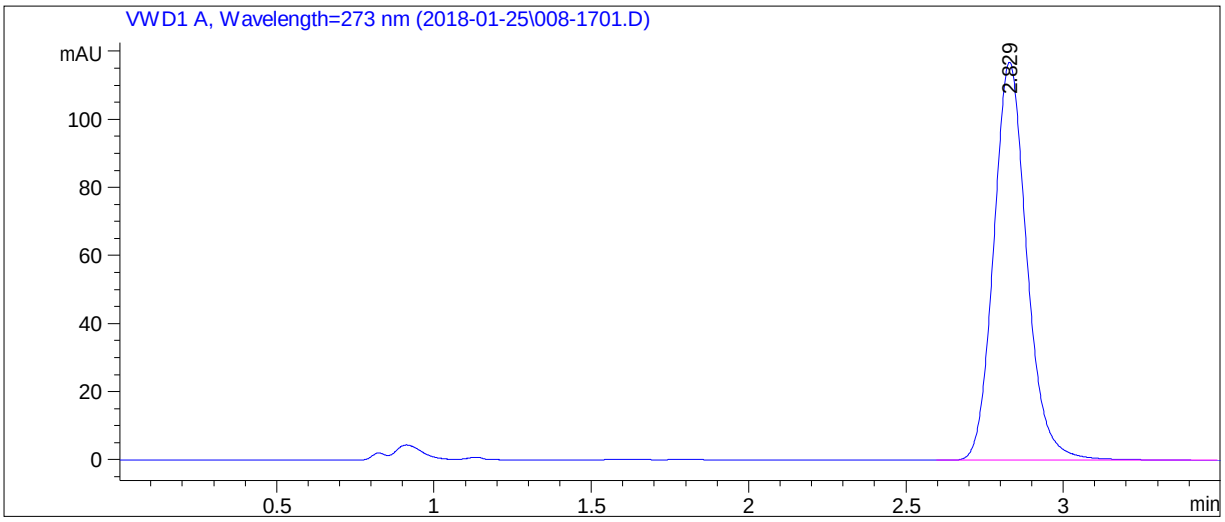


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.829 BBA   0.1125  856.99799  116.94487 100.0000


Totals :                   856.99799  116.94487
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\008-1801.D
Sample Name: LIIN 04

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)               Seq. Line :  18
Acq. Instrument : HPLC                          Location : Vial 8
Injection Date  : 1/25/2018 2:21:36 PM               Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 15.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

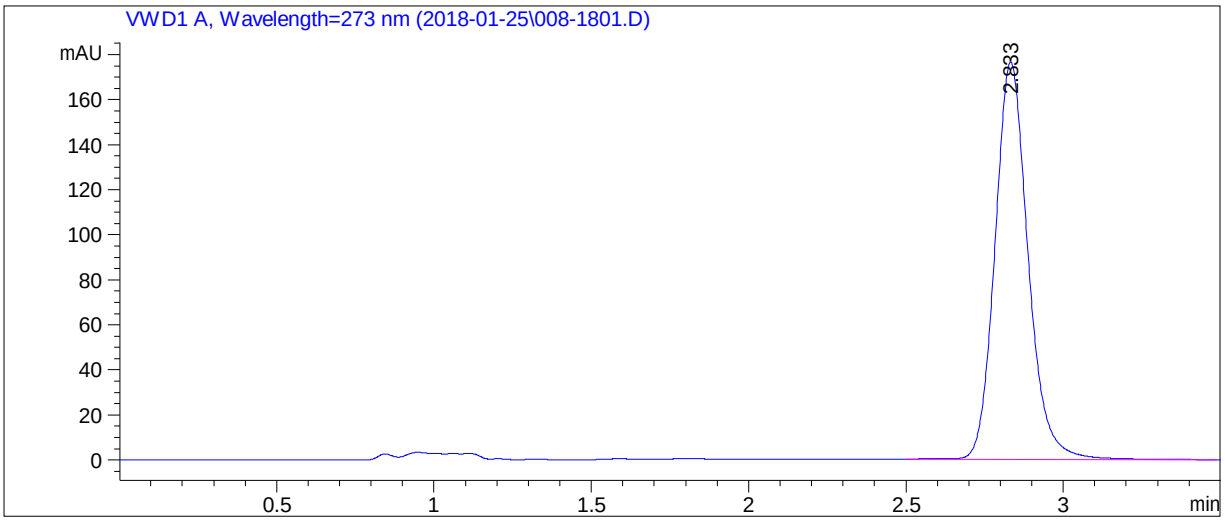


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.833 BBA   0.1117 1288.88745  176.39021 100.0000


Totals :                  1288.88745  176.39021
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\008-1901.D
Sample Name: LIIN 05

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)               Seq. Line :  19
Acq. Instrument : HPLC                          Location : Vial 8
Injection Date  : 1/25/2018 2:26:01 PM               Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 20.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 11:16:44 AM by JOSÉ CARLOS
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
```

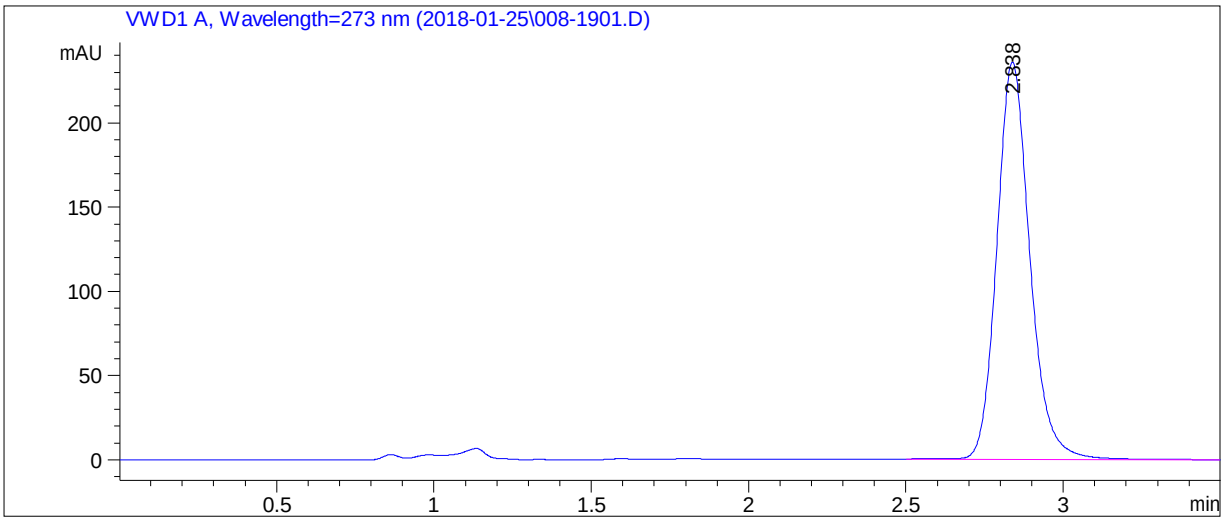


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.838 BBA   0.1115 1717.18481  235.68071 100.0000


Totals :                  1717.18481  235.68071
```

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\2018-01-25\DEFAULT1.D
Sample Name: GRBO-A

```
==========================================================================
Acq. Operator   : Rodolfo (Verde)
Acq. Instrument : HPLC                          Location : Vial 1
Injection Date  : 1/25/2018 2:59:15 PM
                                                Inj Volume : 0.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\GRAD AB.M
Last changed    : 1/25/2018 2:54:07 PM by Rodolfo (Verde)
                  (modified after loading)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 1/25/2018 1:18:27 PM by Rodolfo (Verde)
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

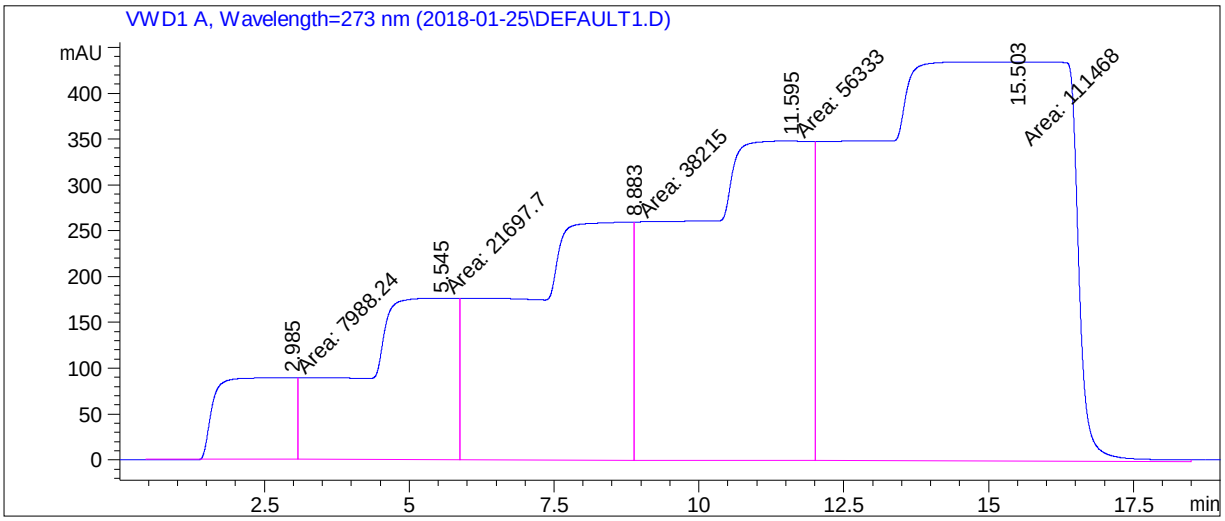


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.985 MF    1.4968 7988.24121   88.94534   3.3891
   2   5.545 FM    2.0517 2.16977e4   176.25827   9.2055
```

Data File C:\CHEM32\2\DATA\2018-01-25\DEFAULT1.D
Sample Name: GRBO-A

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
3	8.883	FM	2.4517	3.82150e4	259.78720	16.2132
4	11.595	FM	2.6939	5.63330e4	348.51578	23.9001
5	15.503	FM	4.2658	1.11468e5	435.51663	47.2920
Totals :				2.35702e5	1309.02322	

==========

*** End of Report ***