
EDUV_001 PDA_0.0933.JWS

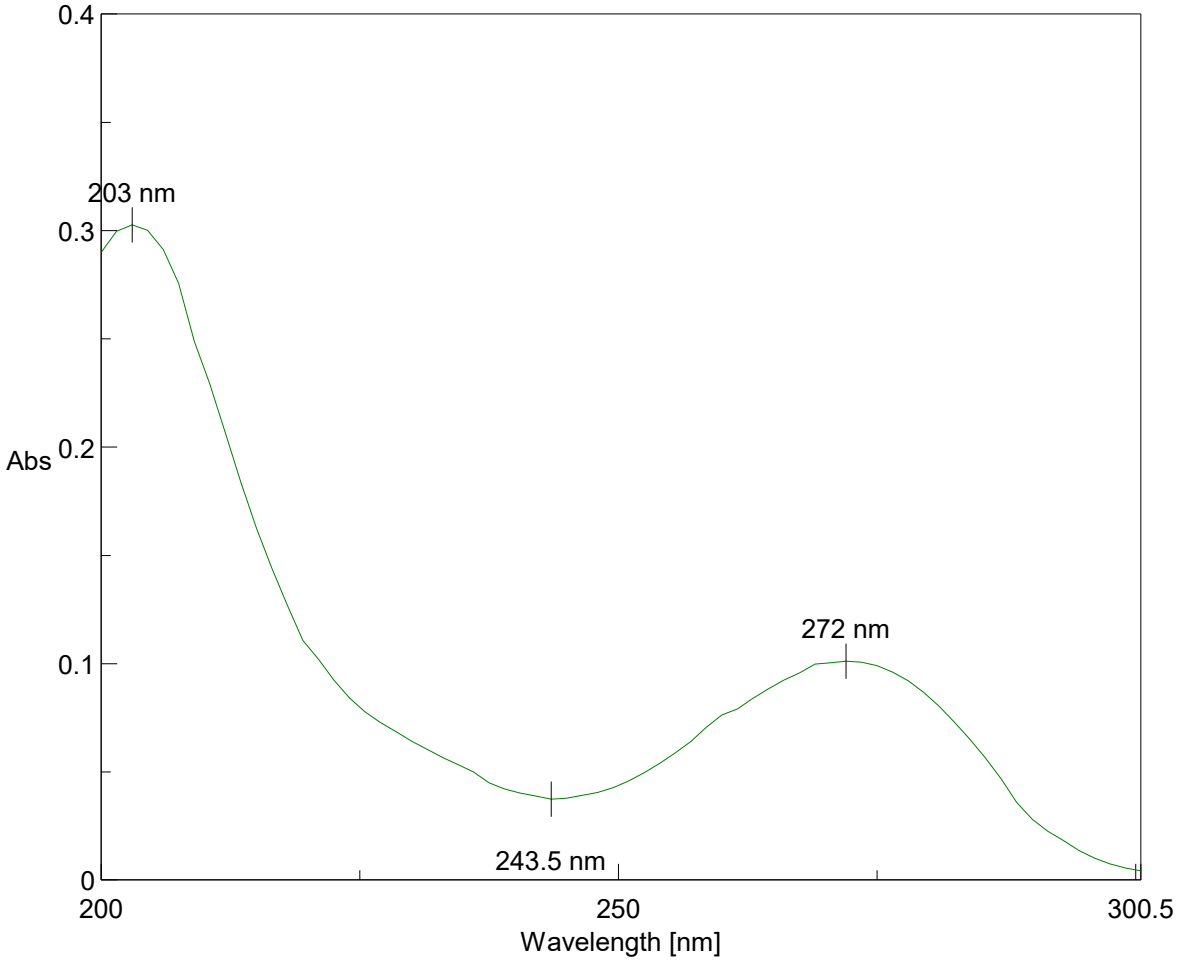

[Comments]

User	Administrator
Division	---
Company	QPack
Creation date	18/01/2021 15:16
Date modified	19/01/2021 13:44

EDUV_001 PDA_0.0933.JWS


[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300.5 nm
Data interval	1.5 nm
Data points	68

[Measurement Information]

Instrument Name	MD-2015
Model Name	MD-2015
Serial No.	0000000000
ROM version	V2.36

Chromatogram

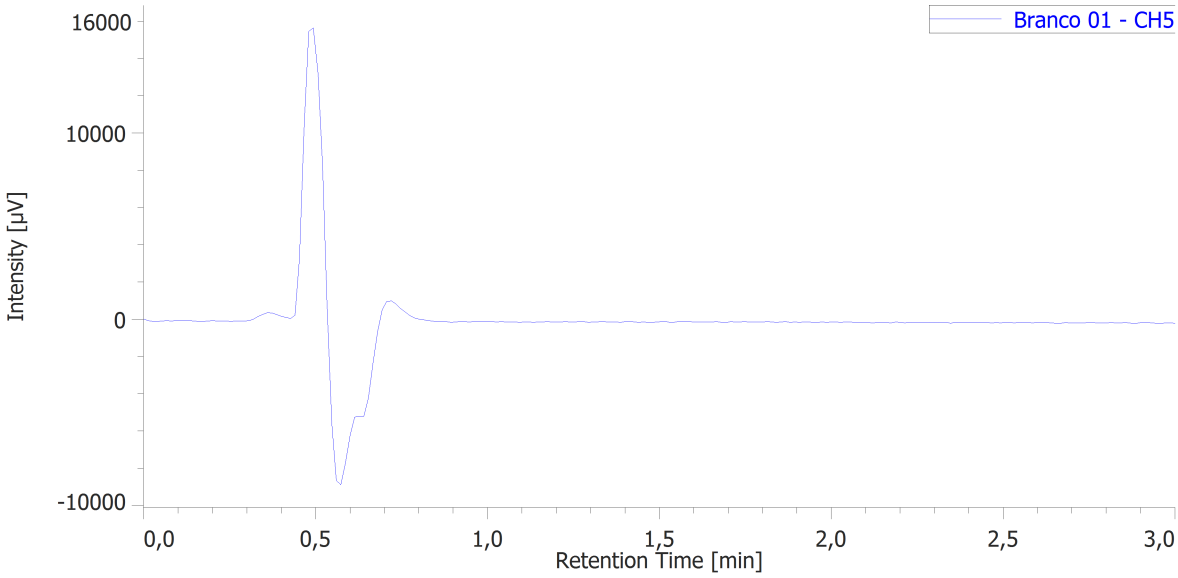


Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 15:51:08
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 15:48:05
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

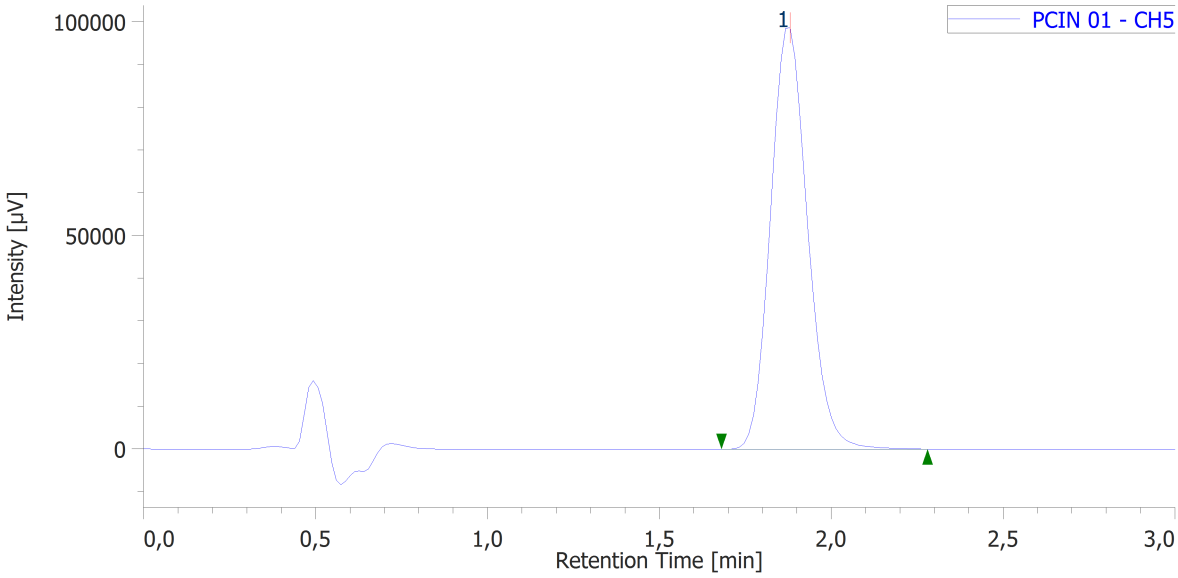

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 15:55:08
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 15:52:05
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	740630	98537	100,000	100,000	N/A	1467	N/A	1,072	

Creator Administrator
Reviewer
Approver

Chromatogram

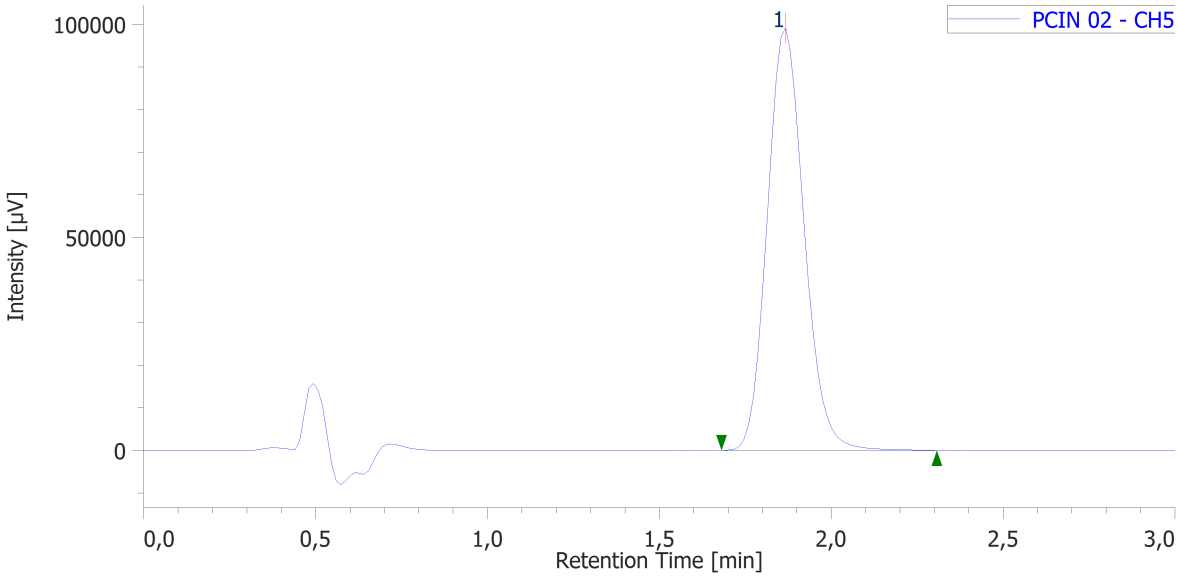

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 15:59:05
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 15:56:02
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,867	736645	99121	100,000	100,000	N/A	1472	N/A	1,108	

Creator Administrator
Reviewer
Approver

Chromatogram

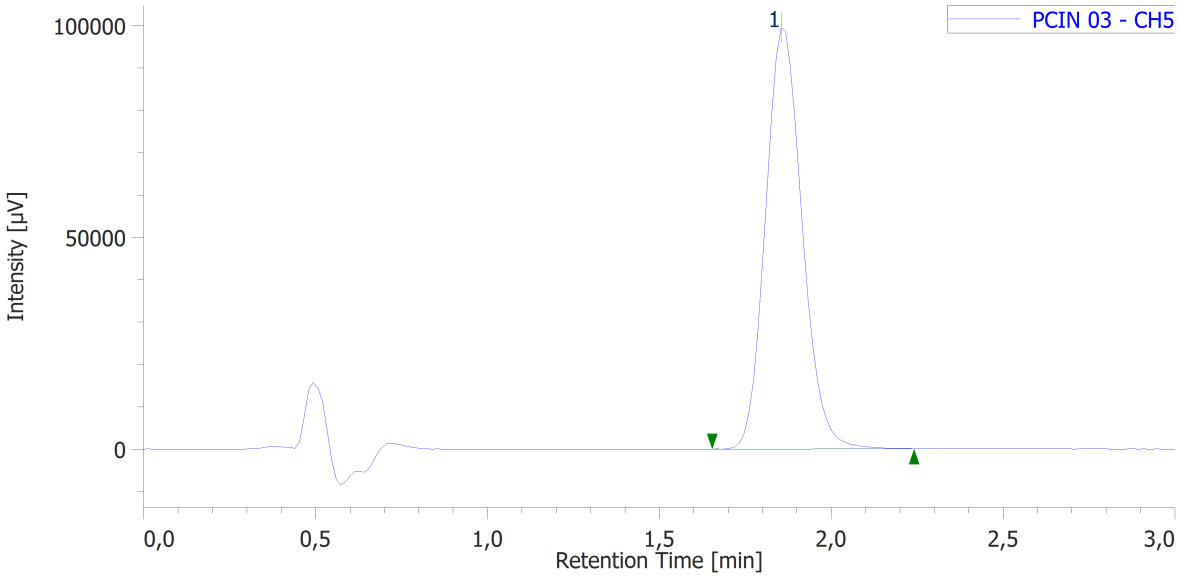

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:03:05
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:00:02
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,853	738051	99381	100,000	100,000	N/A	1459	N/A	1,194	

Creator Administrator
Reviewer
Approver

Chromatogram

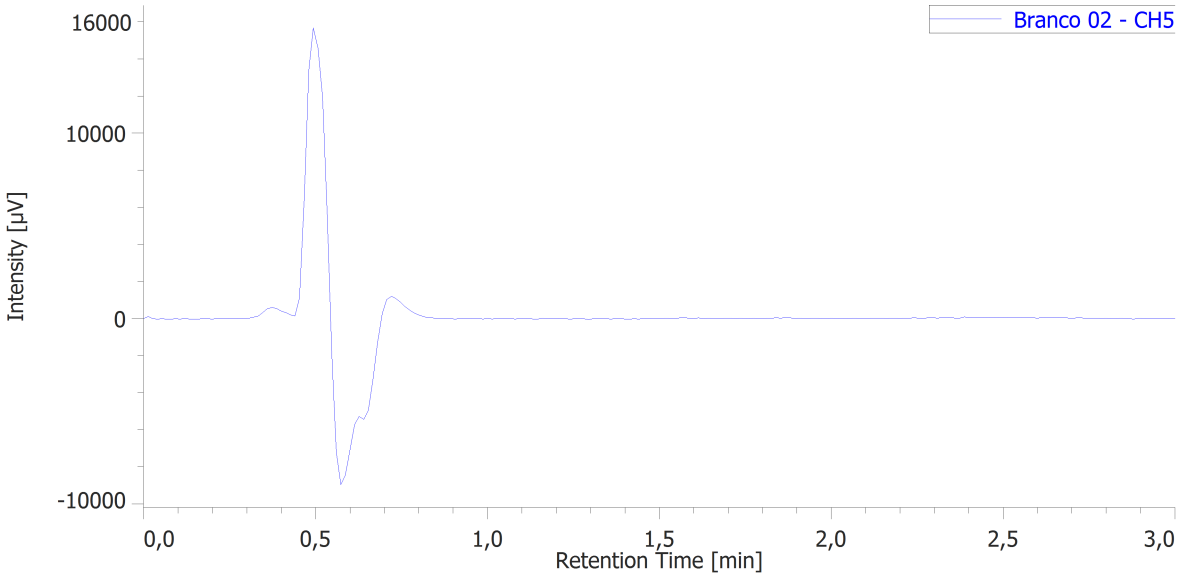


Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:06:59
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:03:58
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

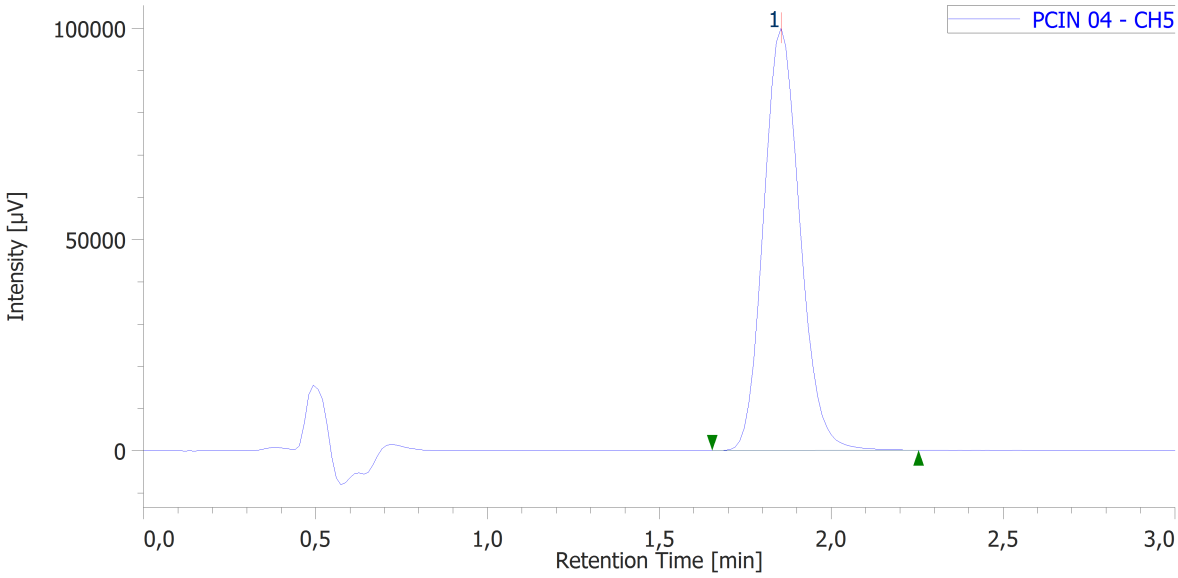

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:10:57
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:07:55
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,853	732885	99944	100,000	100,000	N/A	1488	N/A	1,131	

Creator Administrator
Reviewer
Approver

Chromatogram

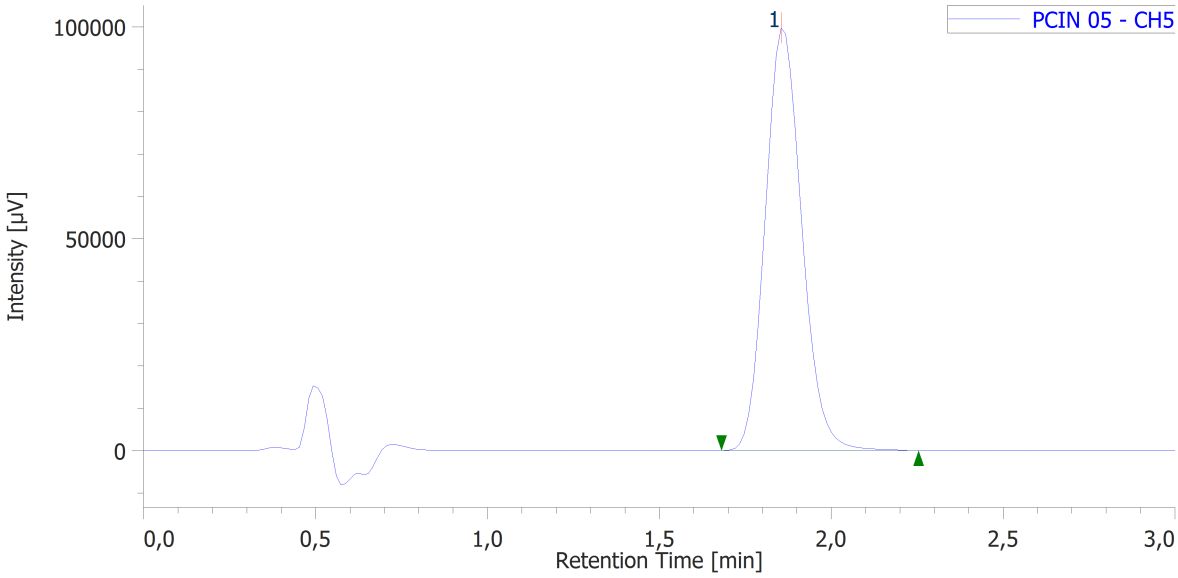

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:14:57
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:11:55
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,853	735496	99611	100,000	100,000	N/A	1472	N/A	1,184	

Creator Administrator
Reviewer
Approver

Chromatogram

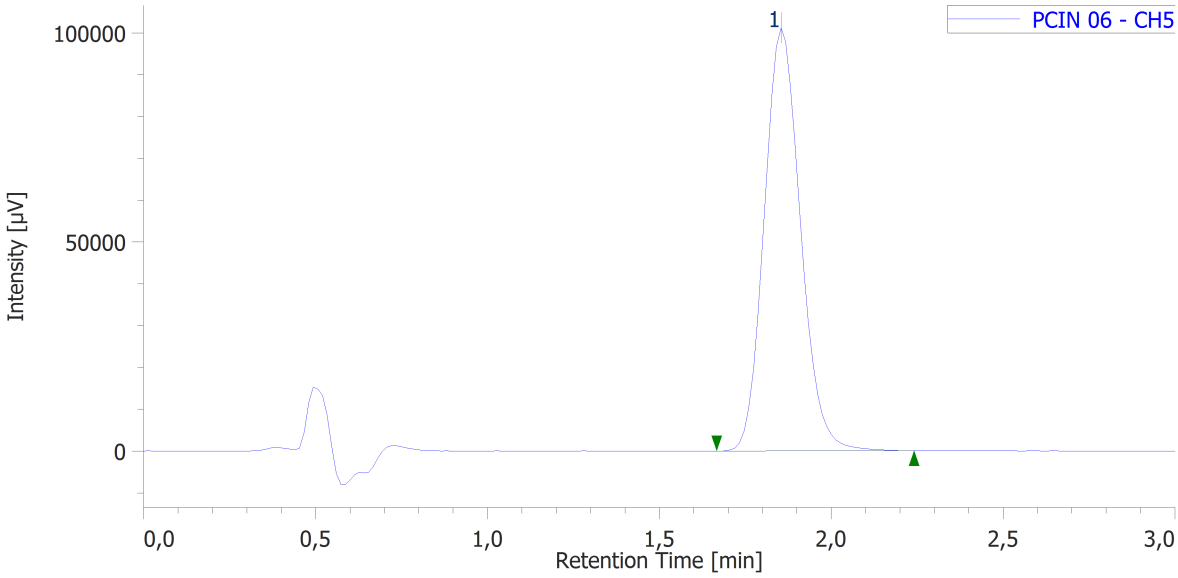

Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:18:55
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:15:53
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,853	740286	101064	100,000	100,000	N/A	1493	N/A	1,149	

Creator Administrator
Reviewer
Approver

Chromatogram

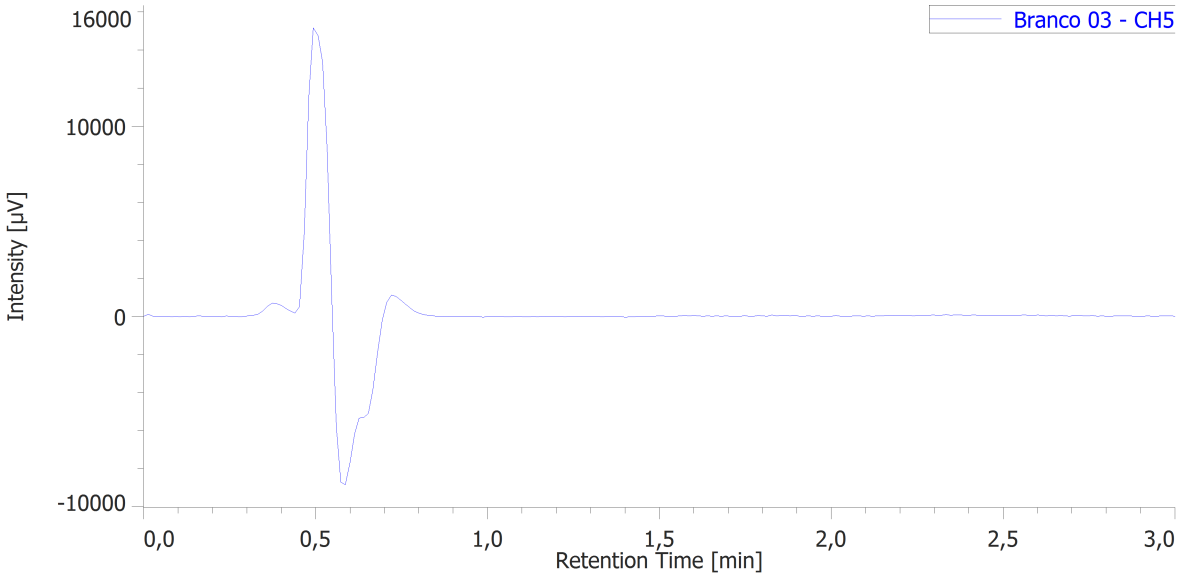


Chromatogram Information	
User Name	Administrator
Date Modified	18/01/2021 16:22:53
Description	
HPLC System Name	HPL18
Injection Date	18/01/2021 16:19:51
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

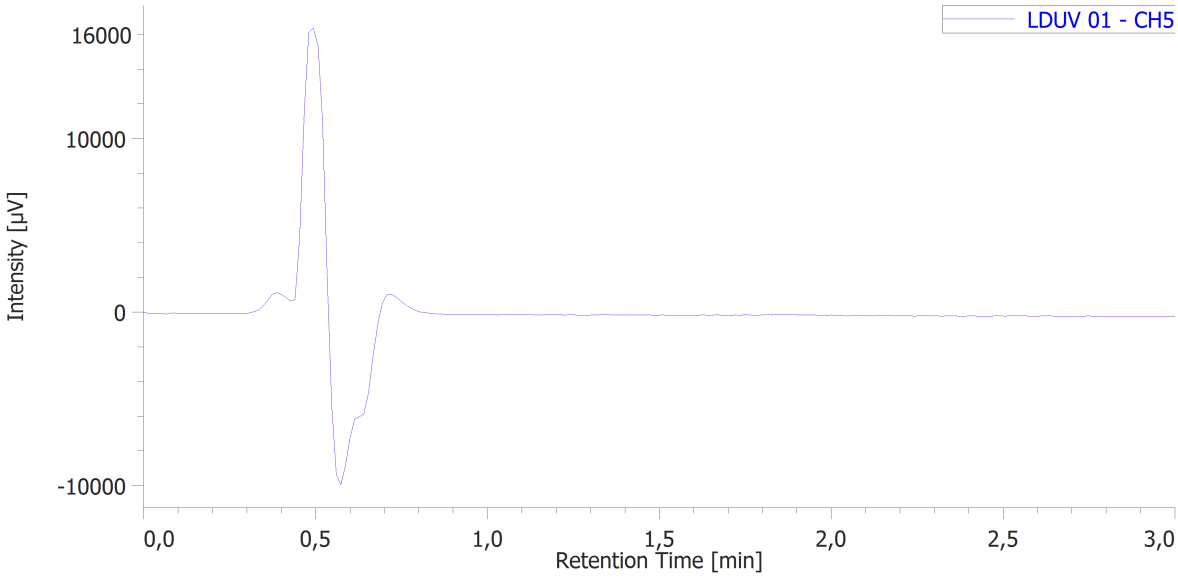


Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 08:57:11
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 08:54:08
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator Administrator
Reviewer
Approver

Chromatogram

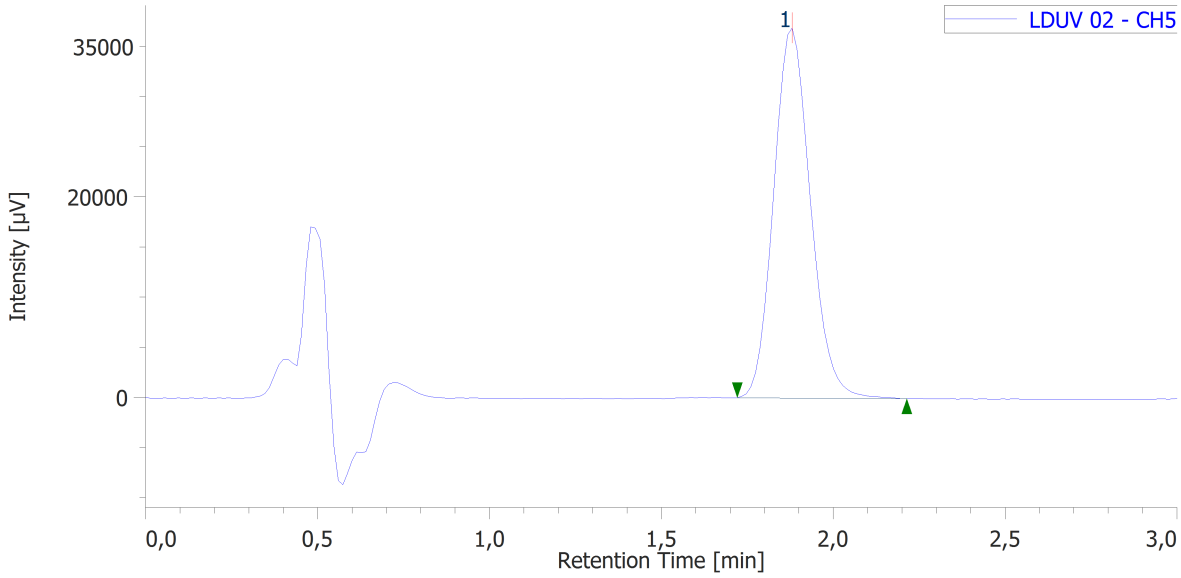

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:01:07
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 08:58:04
Volume	10,0 [µL]
Sample #	32
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	274123	36900	100,000	100,000	N/A	1493	N/A	1,100	

Creator Administrator
Reviewer
Approver

Chromatogram

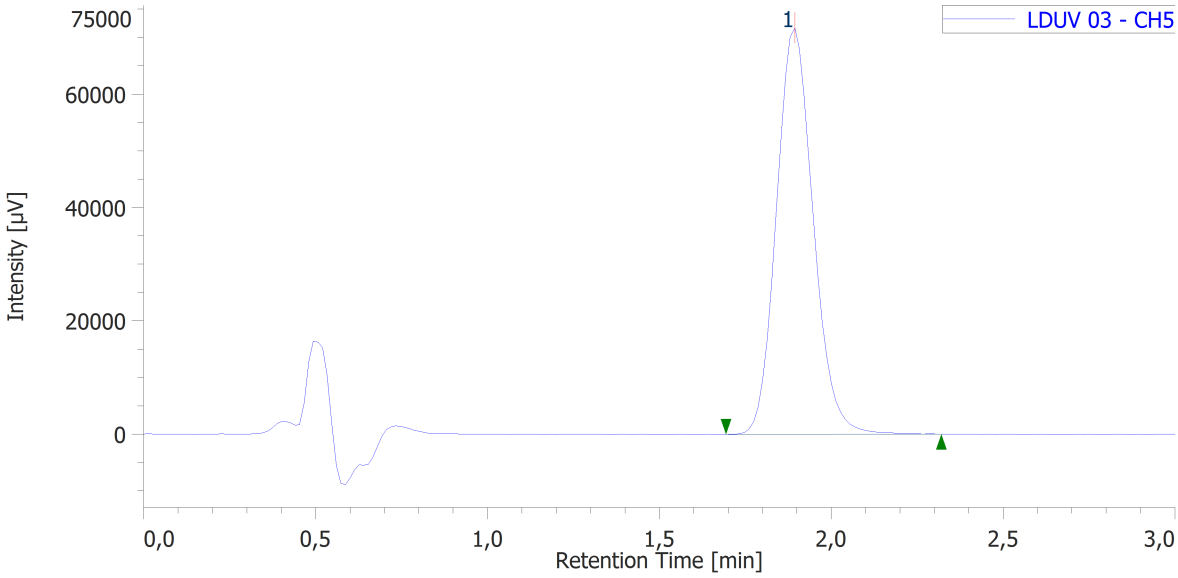

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:05:01
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:01:59
Volume	10,0 [µL]
Sample #	33
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	532730	71623	100,000	100,000	N/A	1520	N/A	1,104	

Creator Administrator
Reviewer
Approver

Chromatogram

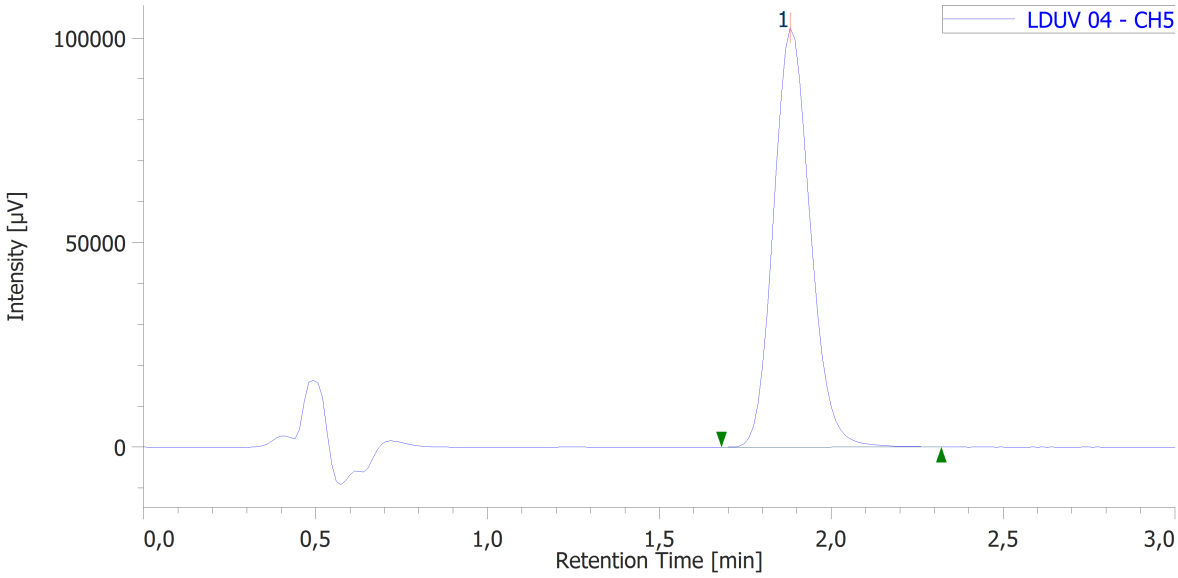

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:08:59
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:05:56
Volume	10,0 [µL]
Sample #	34
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	760883	102452	100,000	100,000	N/A	1503	N/A	1,159	

Creator Administrator
Reviewer
Approver

Chromatogram

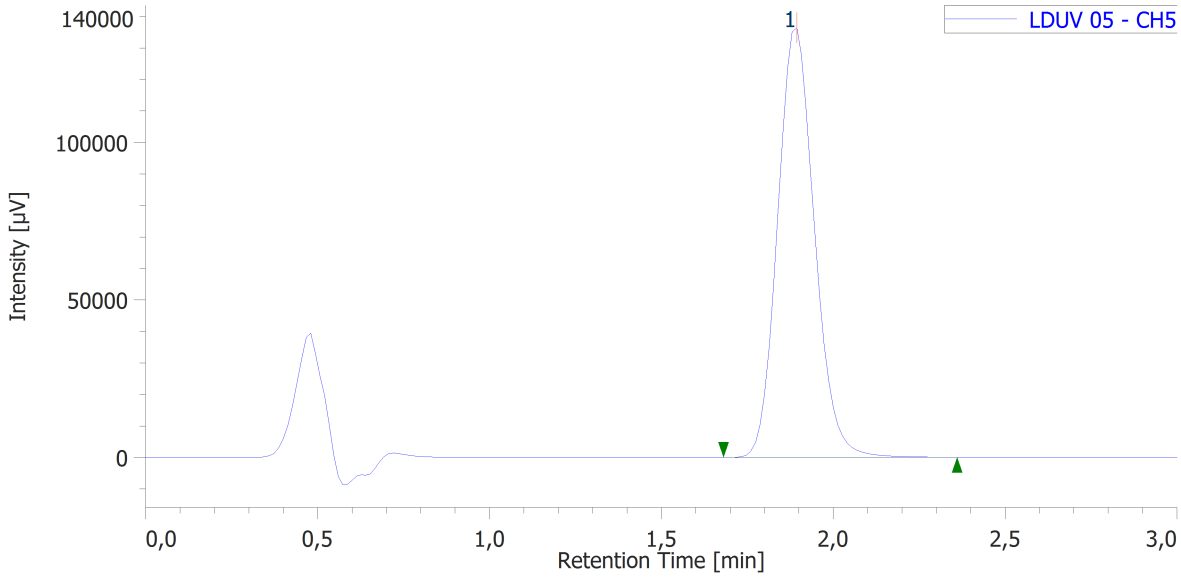

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:12:57
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:09:54
Volume	10,0 [µL]
Sample #	35
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	1016733	136240	100,000	100,000	N/A	1512	N/A	1,077	

Creator Administrator
Reviewer
Approver

Chromatogram

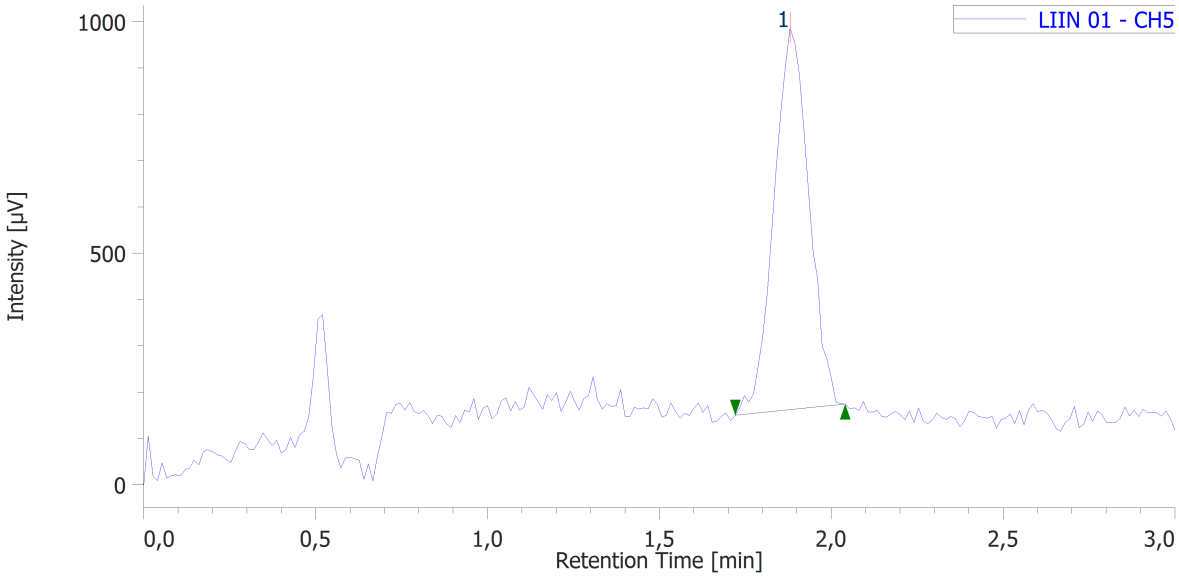

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:25:30
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:15:59
Volume	0,1 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak.

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	5820	824	100,000	100,000	N/A	1603	N/A	1,079	

Creator Administrator
Reviewer
Approver

Chromatogram

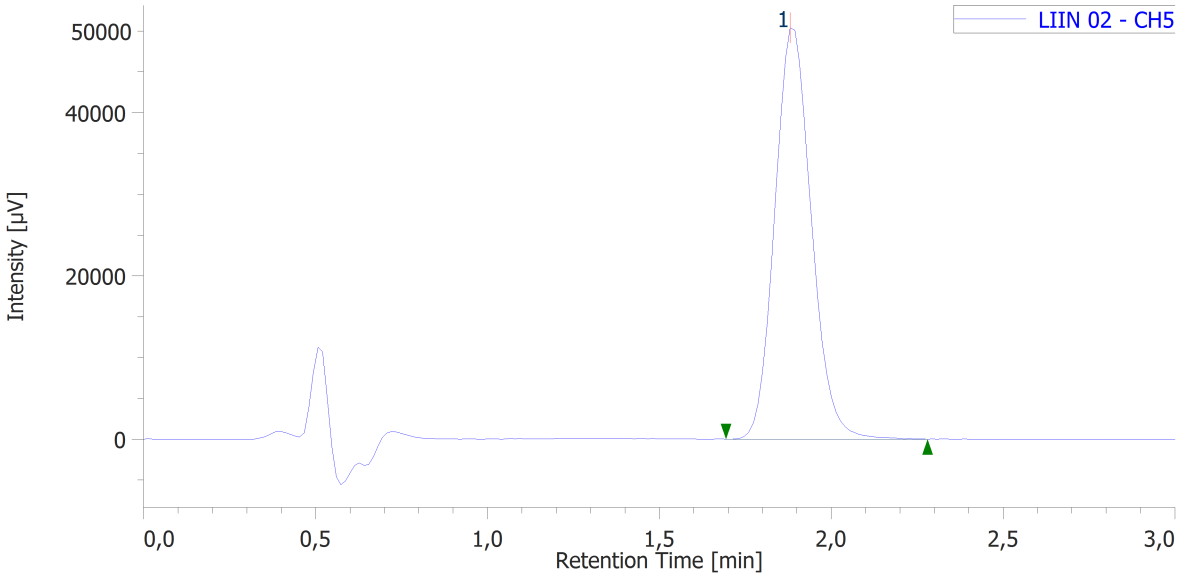

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:22:57
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:19:54
Volume	5,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	373395	50326	100,000	100,000	N/A	1509	N/A	1,187	

Creator Administrator
Reviewer
Approver

Chromatogram

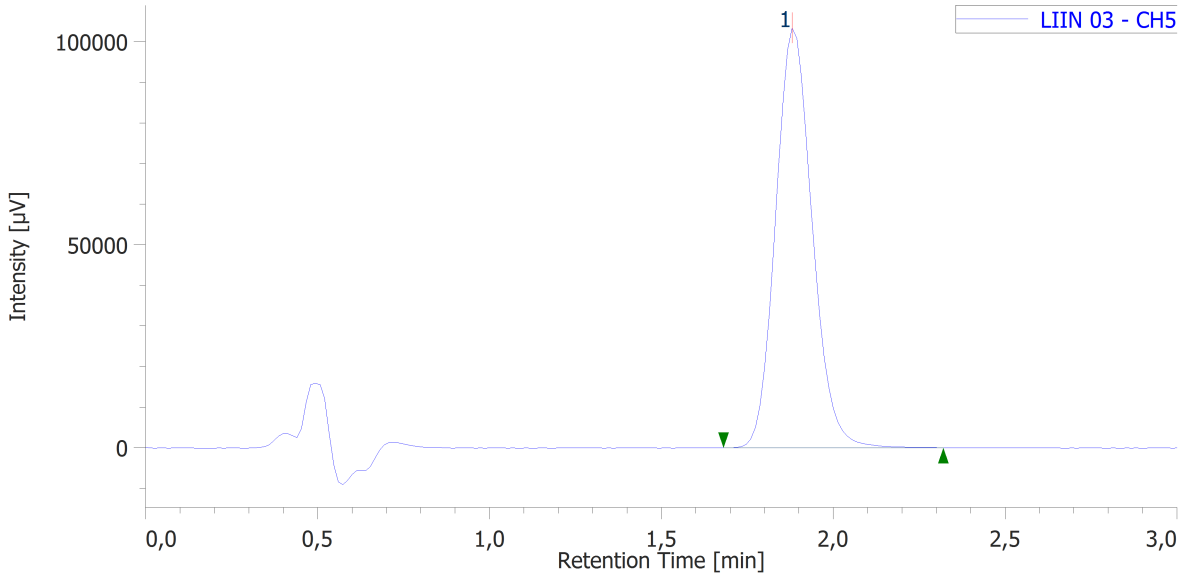

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:26:57
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:23:54
Volume	10,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,880	765066	103384	100,000	100,000	N/A	1514	N/A	1,159	

Creator Administrator
Reviewer
Approver

Chromatogram

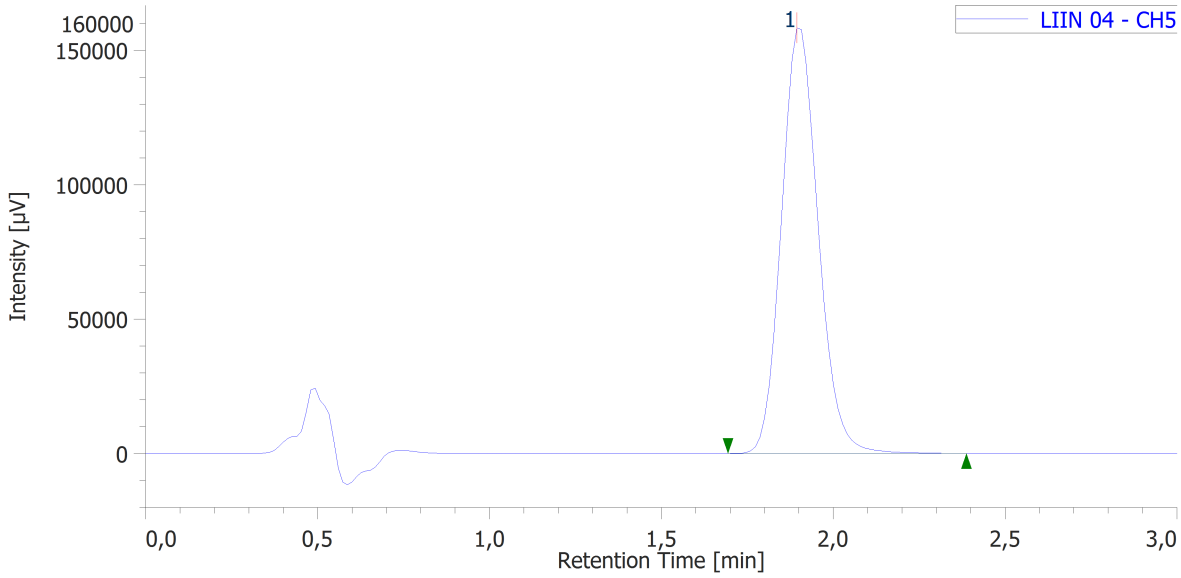

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:30:59
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:27:57
Volume	15,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	1176219	158150	100,000	100,000	N/A	1530	N/A	1,197	

Creator Administrator
Reviewer
Approver

Chromatogram

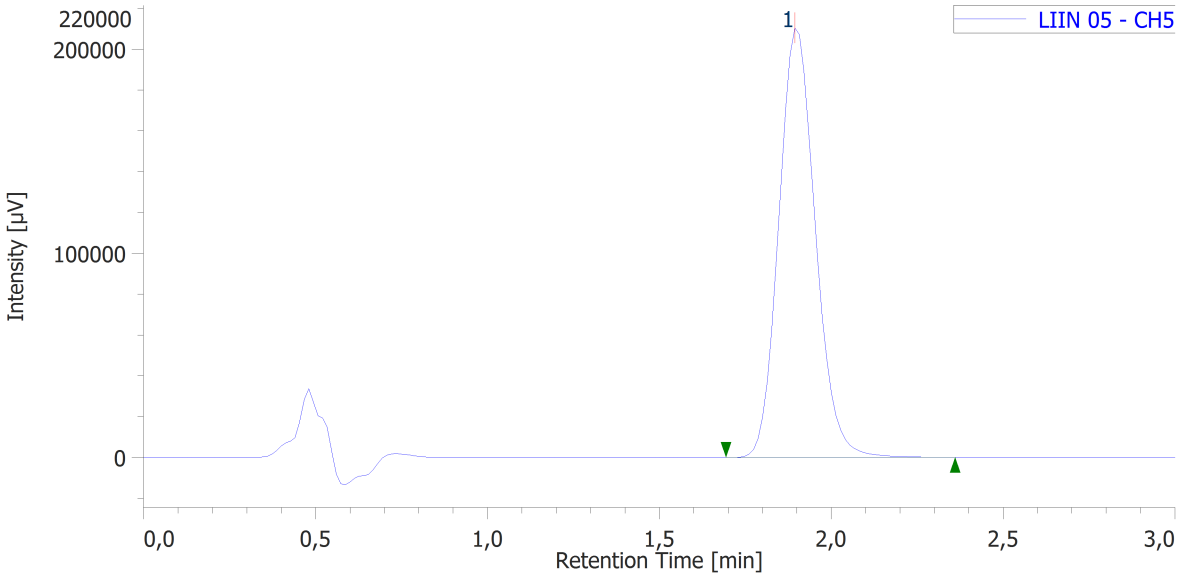

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 09:35:04
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 09:32:02
Volume	20,0 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	1556444	210256	100,000	100,000	N/A	1537	N/A	1,175	

Creator Administrator
Reviewer
Approver

Chromatogram

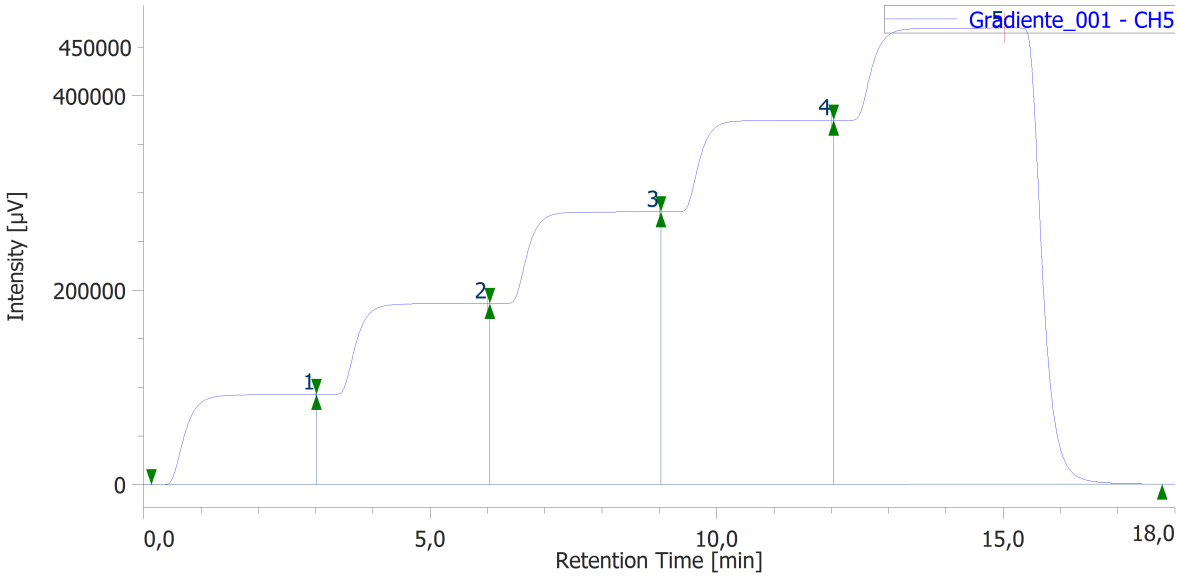

Chromatogram Information	
User Name	Administrator
Date Modified	19/01/2021 10:23:46
Description	
HPLC System Name	HPL18
Injection Date	19/01/2021 10:05:44
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,000	12671904	92640	5,025	6,605	N/A	N/A	N/A	N/A	
2	40%	5	6,000	29840356	186151	11,834	13,273	N/A	N/A	N/A	N/A	
3	60%	5	9,000	46419021	280301	18,409	19,986	N/A	N/A	N/A	N/A	
4	80%	5	12,000	63822327	374347	25,310	26,691	N/A	N/A	N/A	N/A	
5	100%	5	15,013	99405277	469061	39,422	33,445	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver