
Peak Find - EDUV_001 PDA_2,9467.JWS

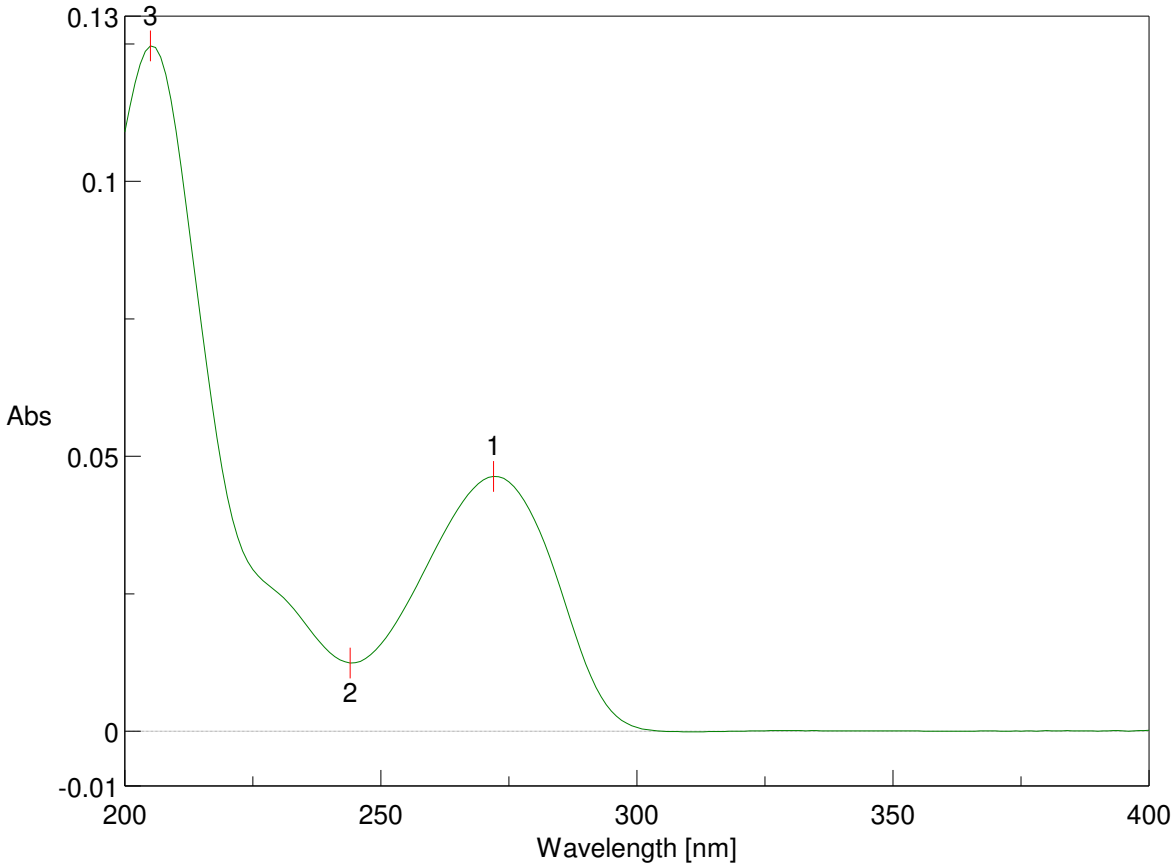

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	07/02/2023 18:21

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	400 nm
Data interval	1 nm
Data points	201


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.04631	2	244	0.012372
3	205	0.124614			

Chromatogram

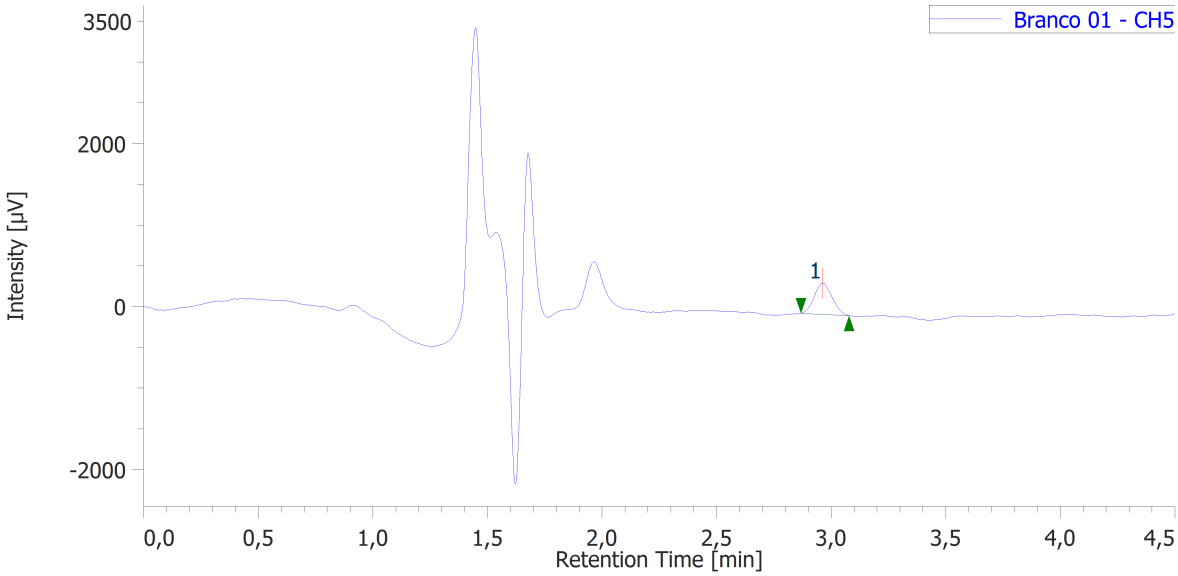

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:08
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:09:25
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,960	2075	382	100,000	100,000	N/A	6592	N/A	1,120	

Creator QPackSA
Reviewer
Approver

Chromatogram

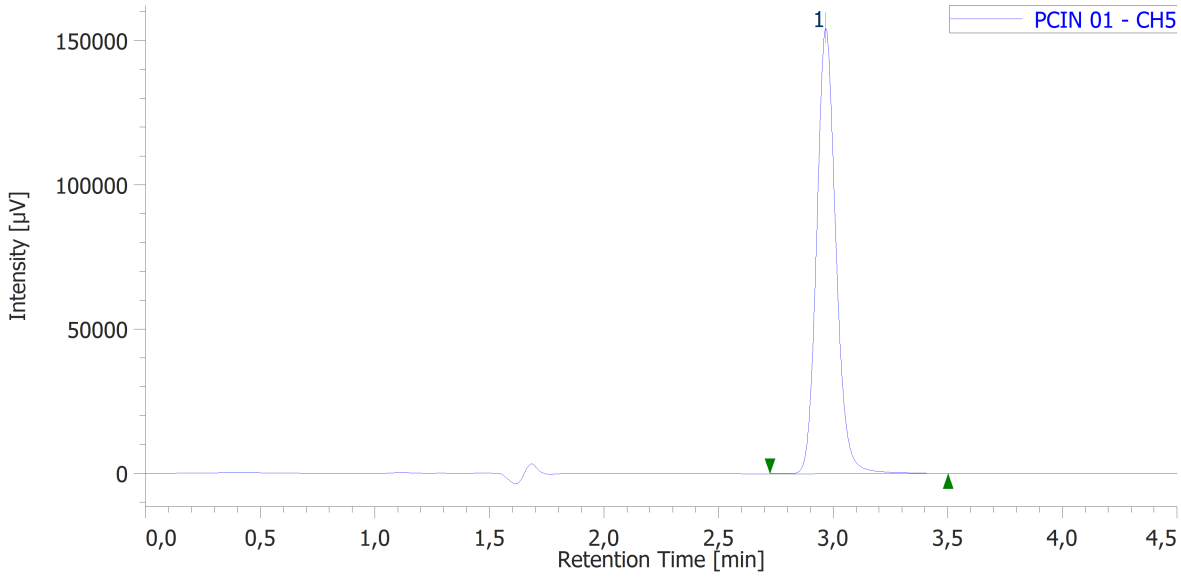

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:11
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:14:08
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,967	894087	154361	100,000	100,000	N/A	6394	N/A	1,134	

Creator QPackSA
Reviewer
Approver

Chromatogram

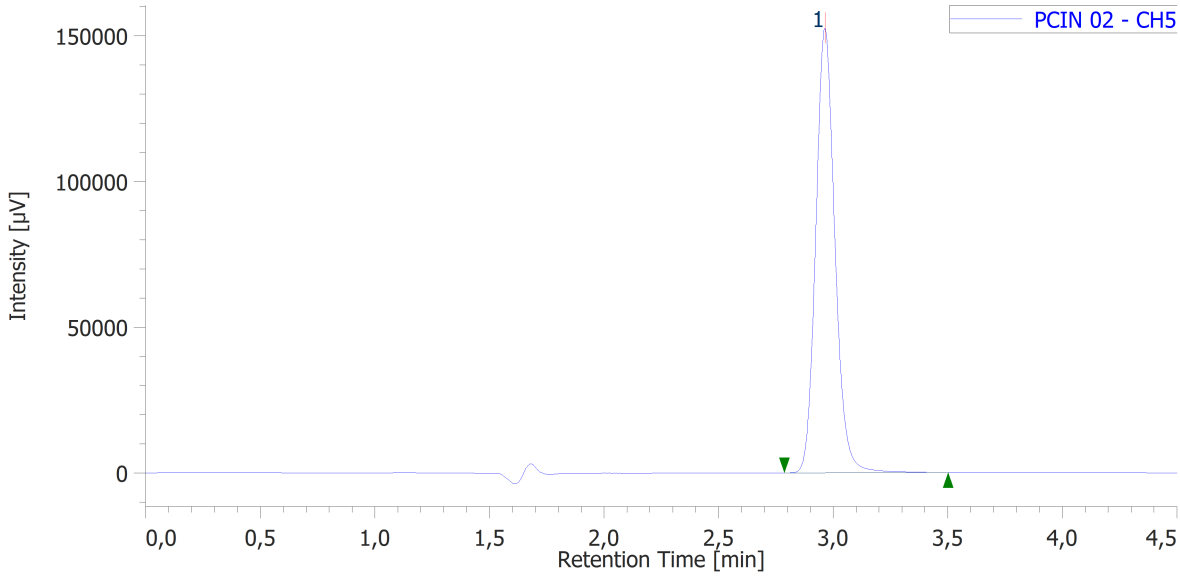

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:11
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:18:50
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,963	886119	152599	100,000	100,000	N/A	6349	N/A	1,125	

Creator QPackSA
Reviewer
Approver

Chromatogram

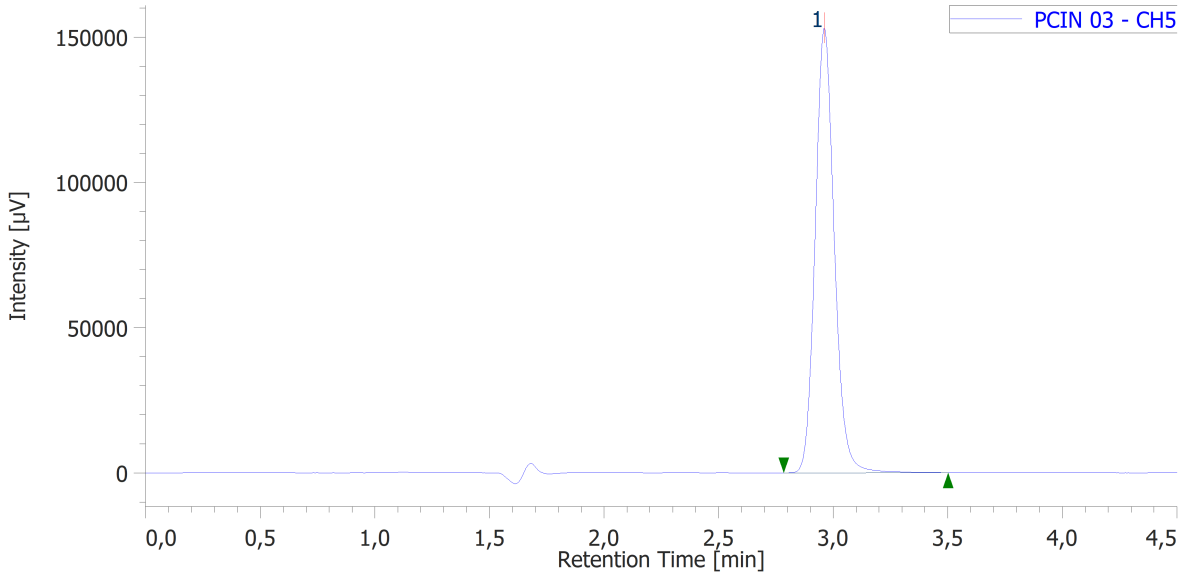

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:11
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:23:32
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,960	887547	153041	100,000	100,000	N/A	6340	N/A	1,132	

Creator QPackSA
Reviewer
Approver

Chromatogram

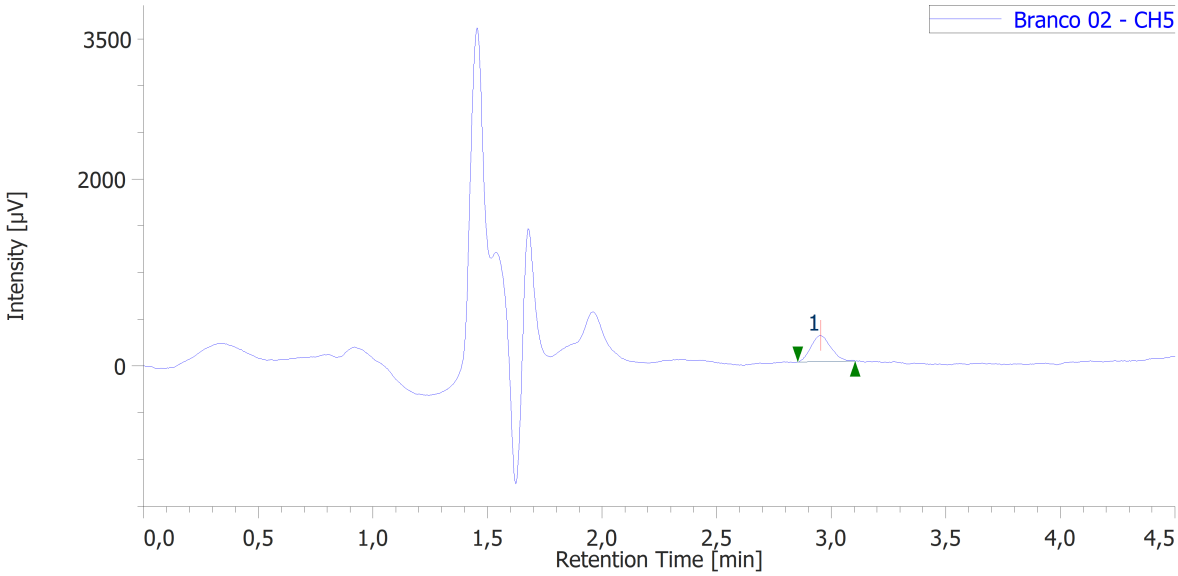

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:12
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:28:14
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,953	1679	279	100,000	100,000	N/A	5389	N/A	1,112	

Creator QPackSA
Reviewer
Approver

Chromatogram

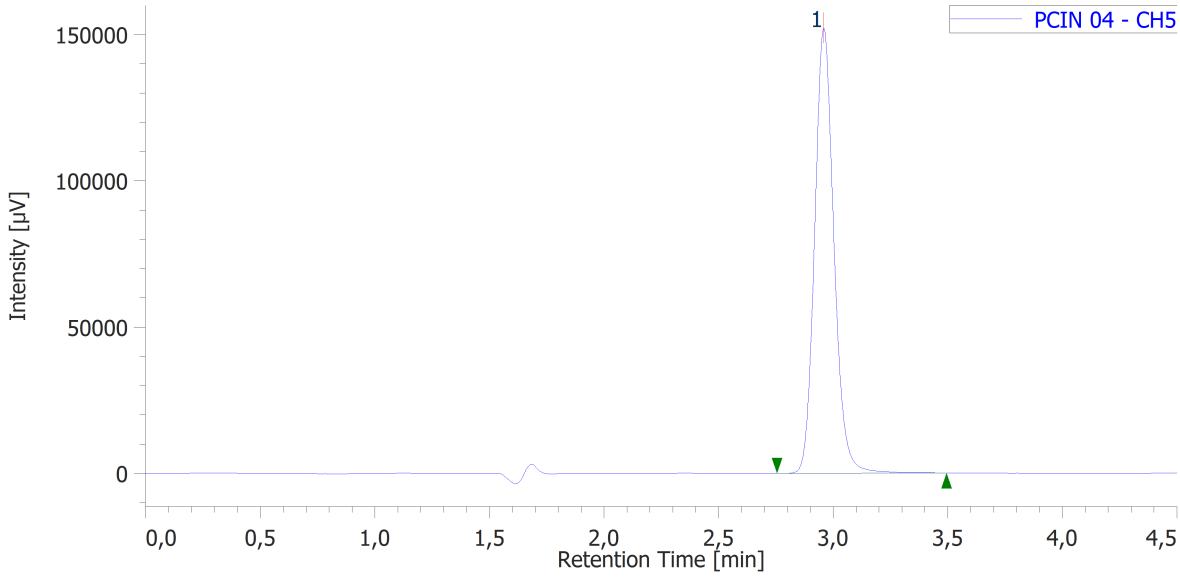

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:12
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:32:57
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,957	888436	152114	100,000	100,000	N/A	6240	N/A	1,155	

Creator QPackSA
Reviewer
Approver

Chromatogram

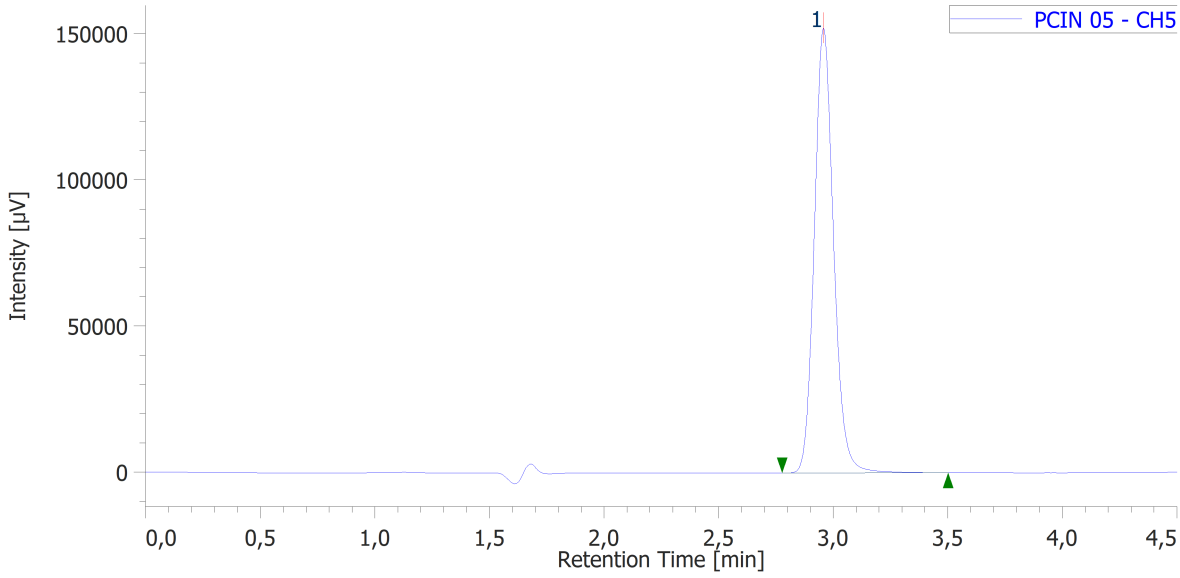

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:12
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:37:39
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,957	888795	152194	100,000	100,000	N/A	6235	N/A	1,134	

Creator QPackSA
Reviewer
Approver

Chromatogram

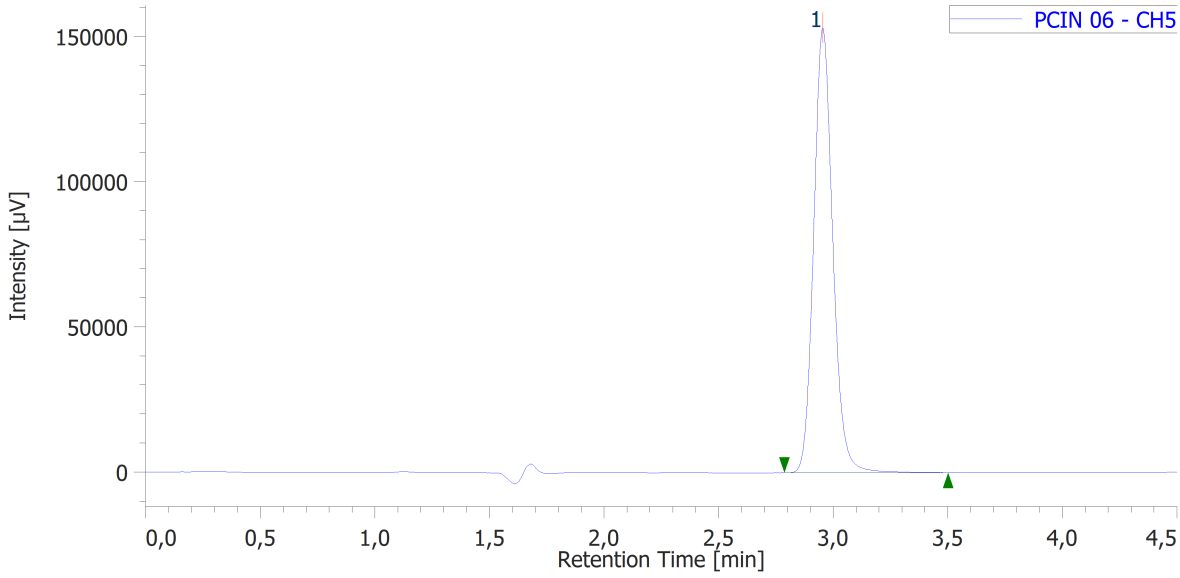

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:12
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:42:21
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,953	885951	153138	100,000	100,000	N/A	6338	N/A	1,137	

Creator QPackSA
Reviewer
Approver

Chromatogram

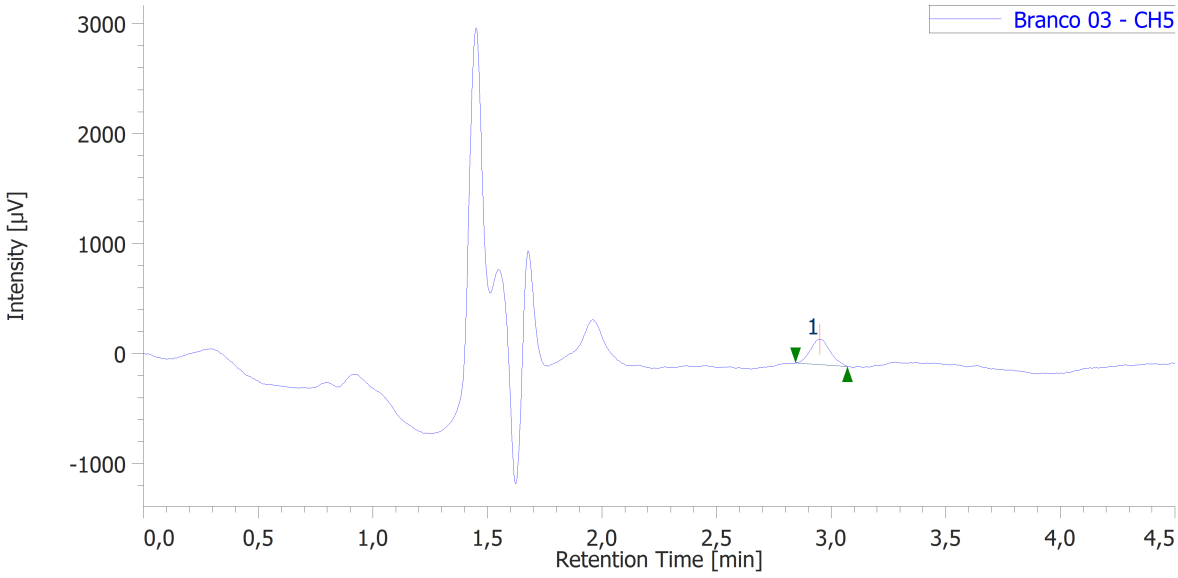

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 09:53:13
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 09:47:03
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,950	1388	231	100,000	100,000	N/A	5589	N/A	1,081	

Creator QPackSA
Reviewer
Approver

Chromatogram

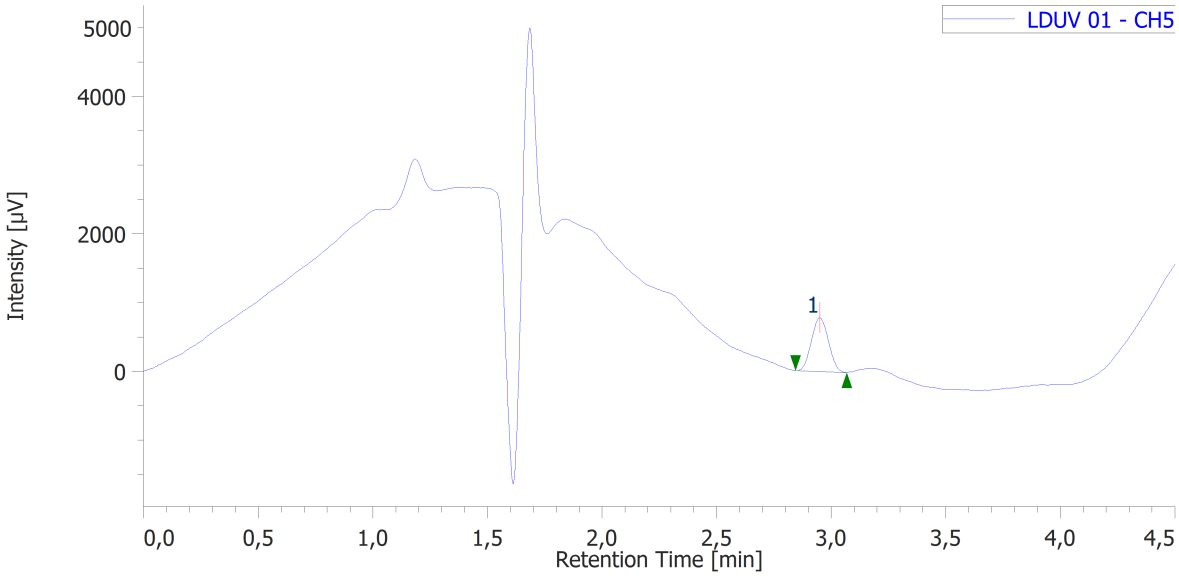

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:02:37
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 10:38:33
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,950	4038	784	100,000	100,000	N/A	7109	N/A	1,034	

Creator QPackSA
Reviewer
Approver

Chromatogram

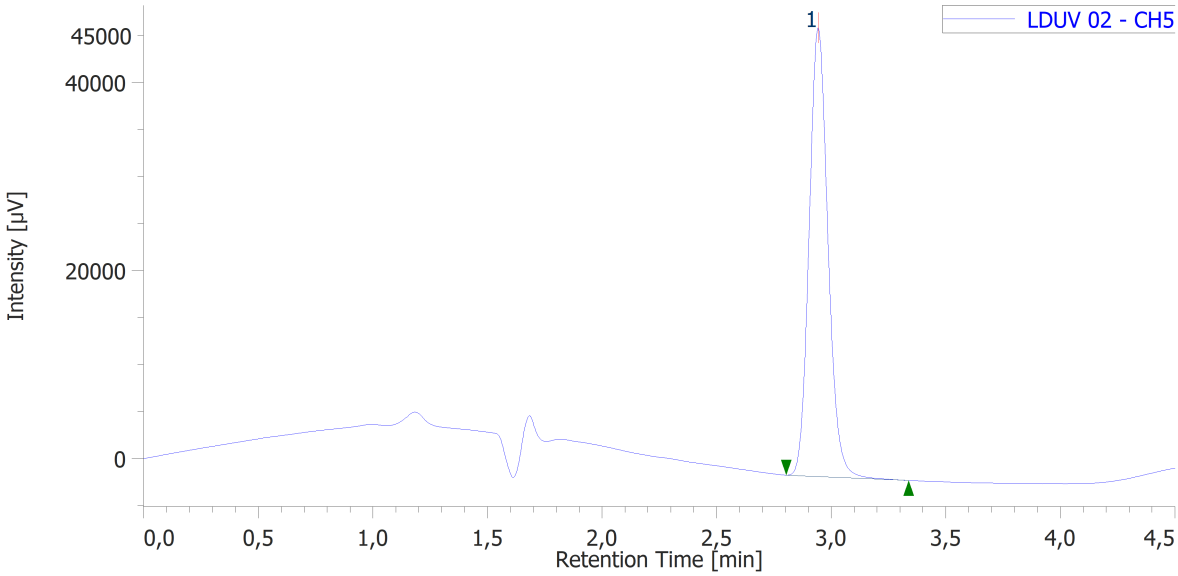

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:02:39
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 10:43:16
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,943	272536	47686	100,000	100,000	N/A	6317	N/A	1,111	

Creator QPackSA
Reviewer
Approver

Chromatogram

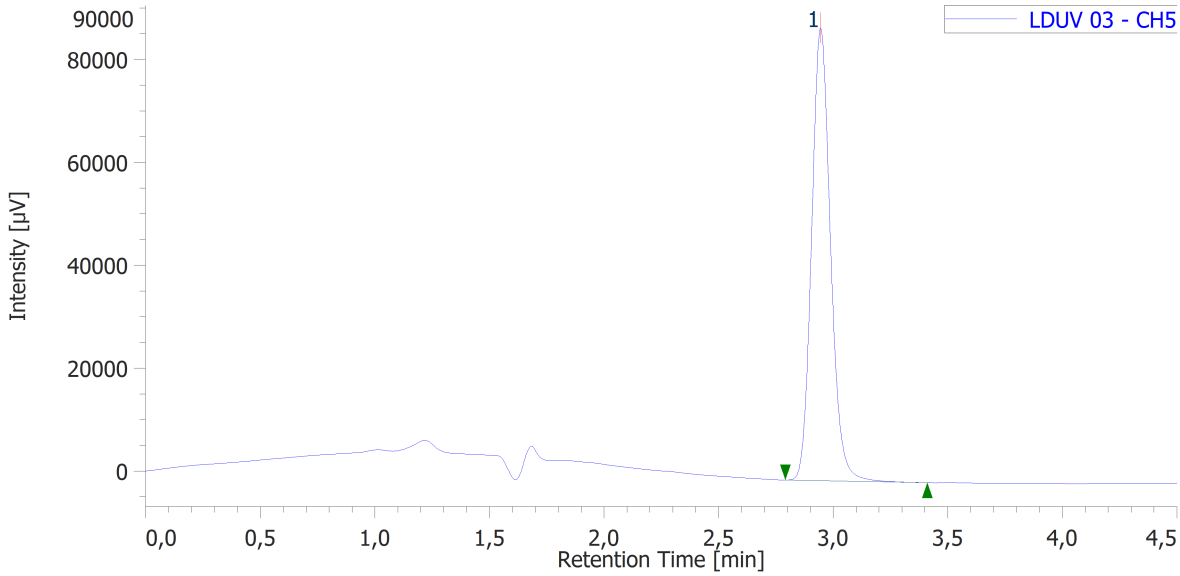

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:02:39
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 10:47:58
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,943	504347	87943	100,000	100,000	N/A	6349	N/A	1,147	

Creator QPackSA
Reviewer
Approver

Chromatogram

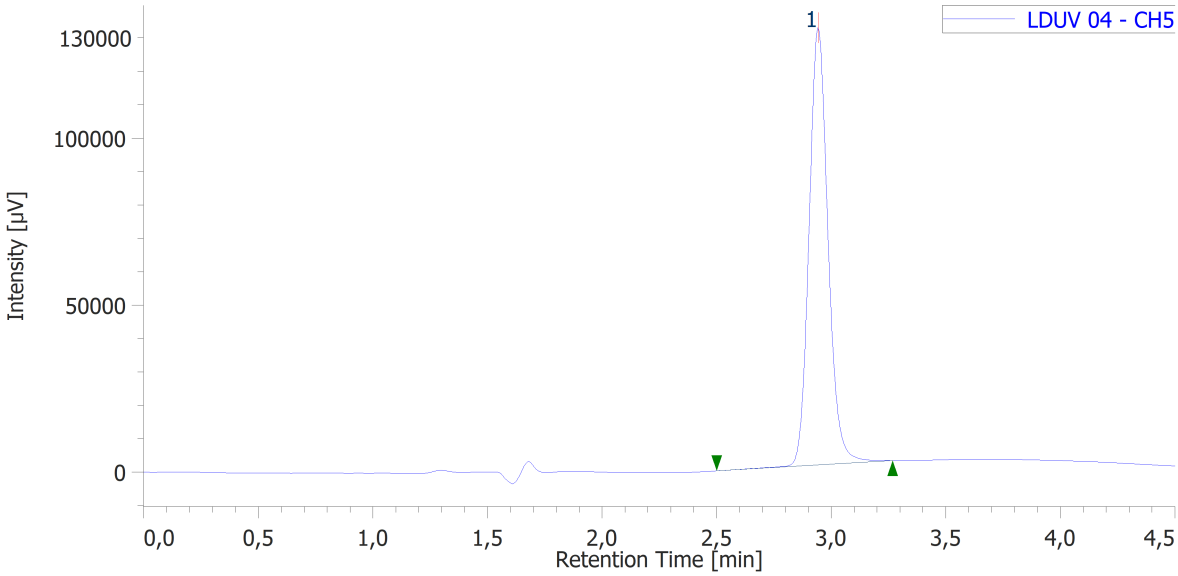

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:02:39
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 10:52:40
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,943	752531	130719	100,000	100,000	N/A	6370	N/A	1,118	

Creator QPackSA
Reviewer
Approver

Chromatogram

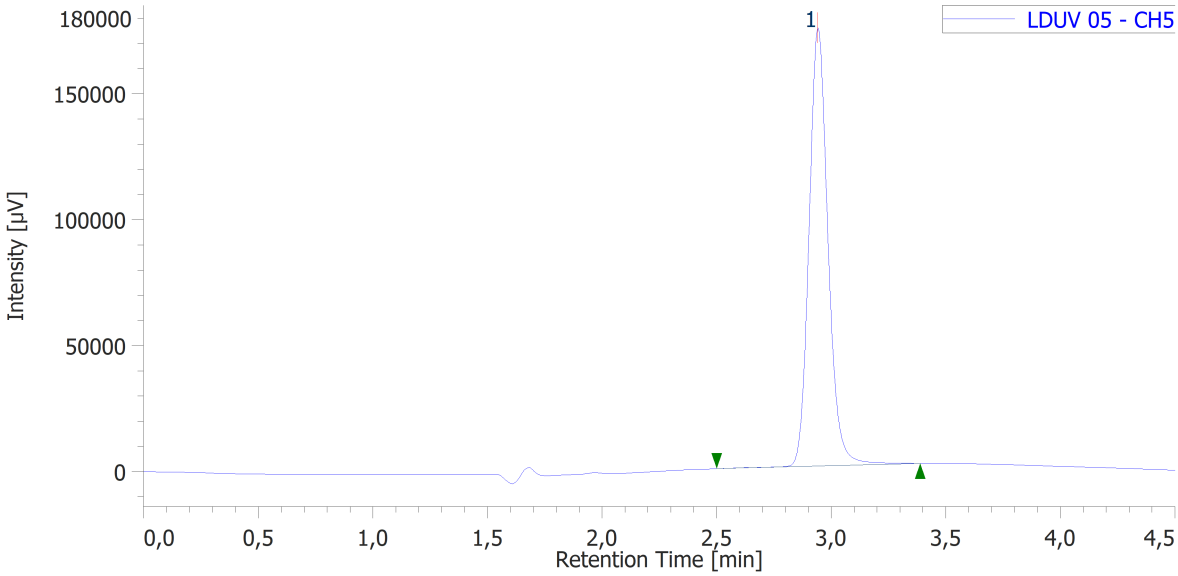

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:02:39
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 10:57:22
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,940	999995	173807	100,000	100,000	N/A	6428	N/A	1,166	

Creator QPackSA
Reviewer
Approver

Chromatogram

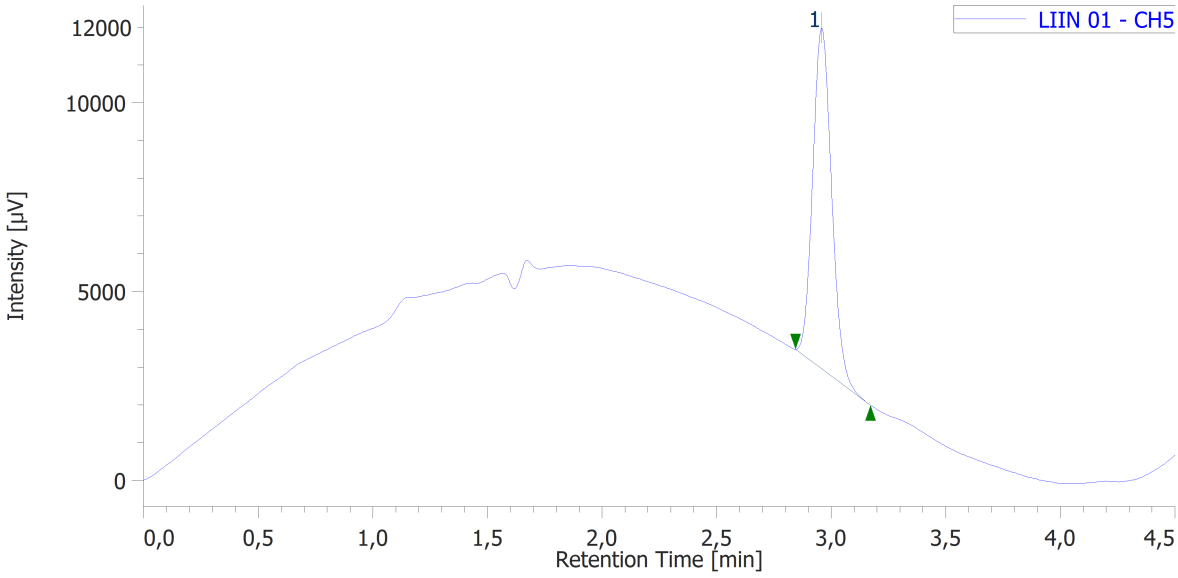

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:16:52
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 11:12:10
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,957	51779	9024	100,000	100,000	N/A	6154	N/A	1,140	

Creator QPackSA
Reviewer
Approver

Chromatogram

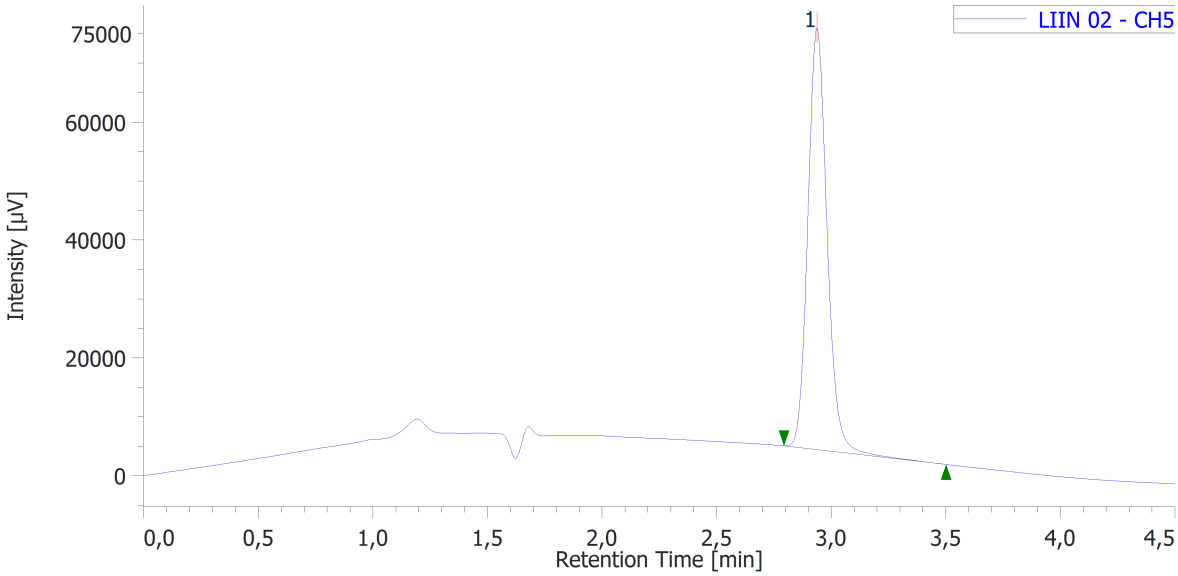

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:21:35
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 11:16:53
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,937	417090	71492	100,000	100,000	N/A	6146	N/A	1,143	

Creator QPackSA
Reviewer
Approver

Chromatogram

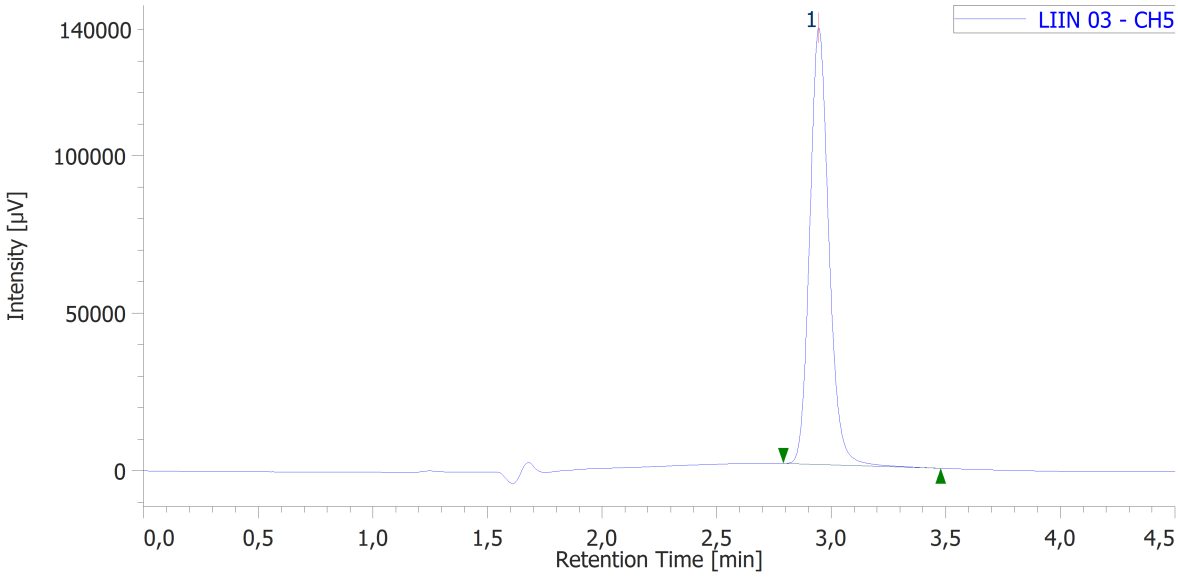

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:26:17
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 11:21:35
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,943	801349	138385	100,000	100,000	N/A	6318	N/A	1,167	

Creator QPackSA
Reviewer
Approver

Chromatogram

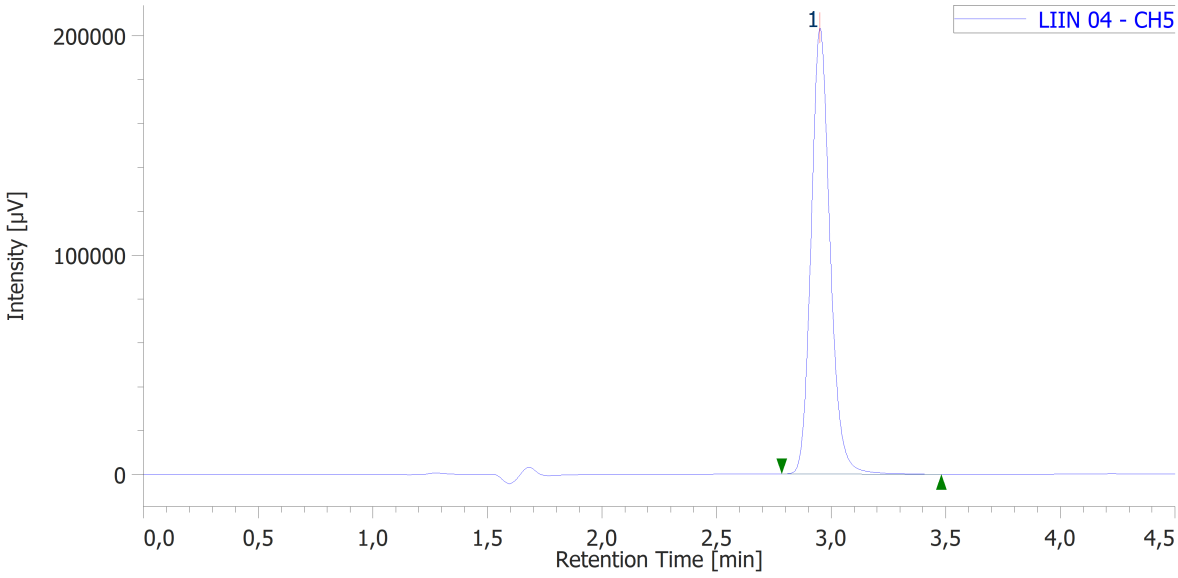

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:30:59
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 11:26:17
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,950	1165278	203210	100,000	100,000	N/A	6488	N/A	1,161	

Creator QPackSA
Reviewer
Approver

Chromatogram

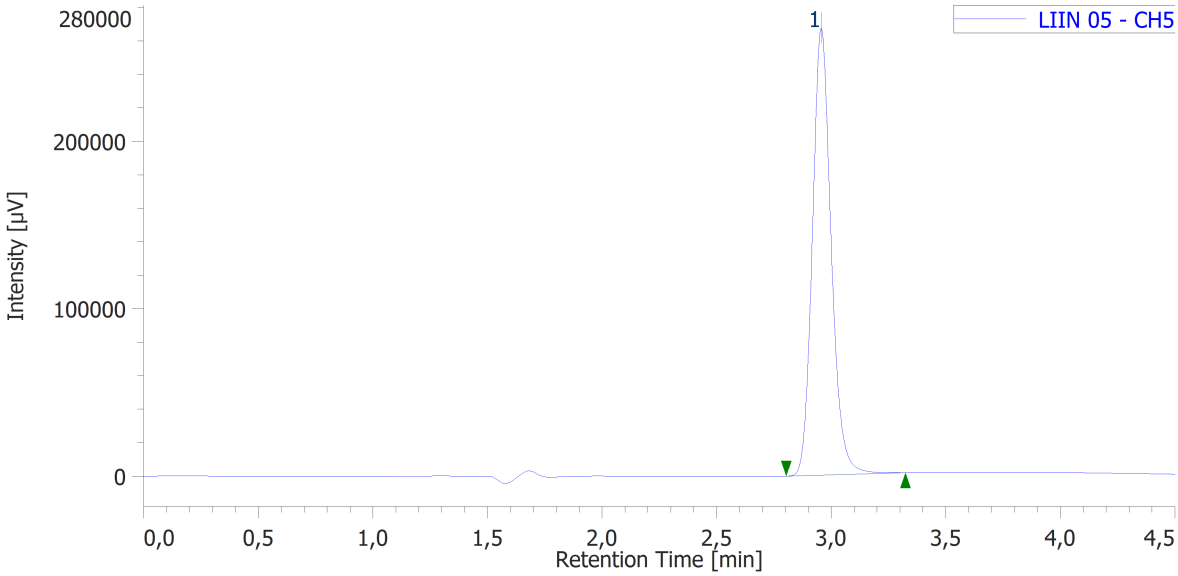

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 11:35:41
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 11:30:59
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP06
Control Method	Qualificação HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,957	1519591	267095	100,000	100,000	N/A	6624	N/A	1,143	

Creator QPackSA
Reviewer
Approver

Chromatogram

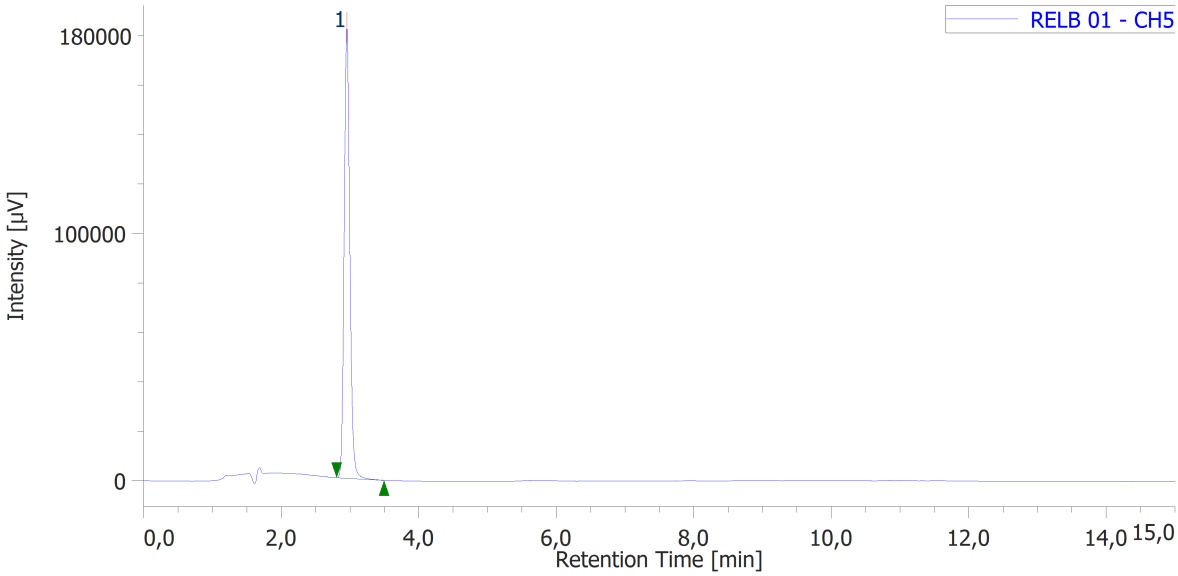

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 14:12:49
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 13:57:37
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação QPack
Acquisition Time	15,0 [min]
Acquisition Sequence	RELB HP06
Control Method	Sinal Ruído HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,953	1035710	182067	100,000	100,000	N/A	6564	N/A	1,146	

Creator
Reviewer
Approver

Chromatogram

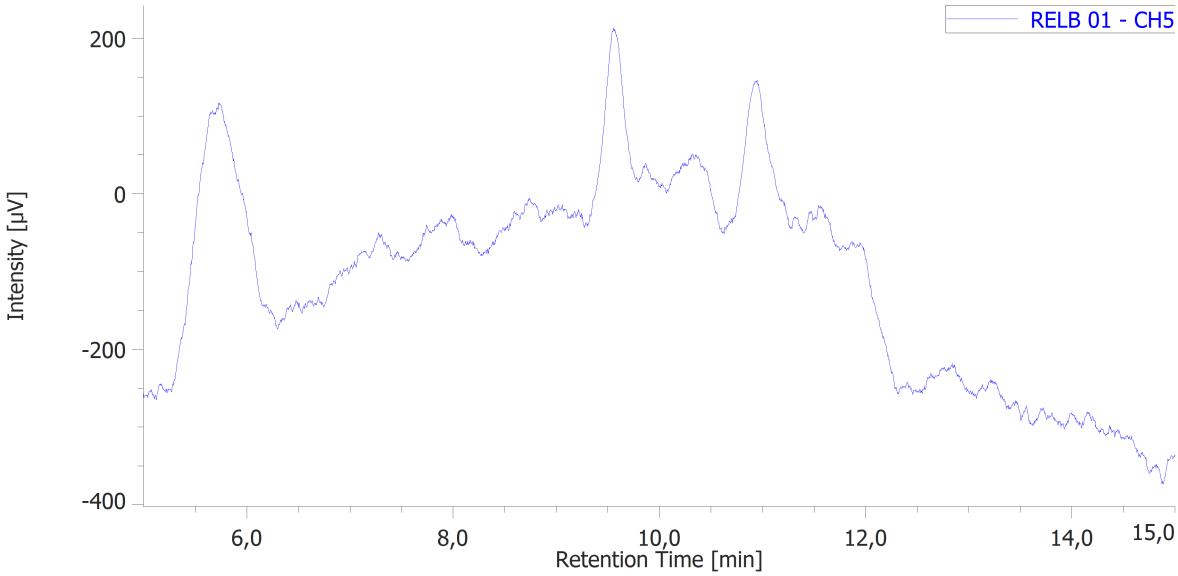

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 14:14:35
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 13:57:37
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação QPack
Acquisition Time	15,0 [min]
Acquisition Sequence	RELB HP06
Control Method	Sinal Ruído HP06
Peak ID Table	Identificação HP06
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração HP06

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,953	1035710	182067	100,000	100,000	N/A	6564	N/A	1,146	

Creator QPackSA
Reviewer
Approver

Chromatogram

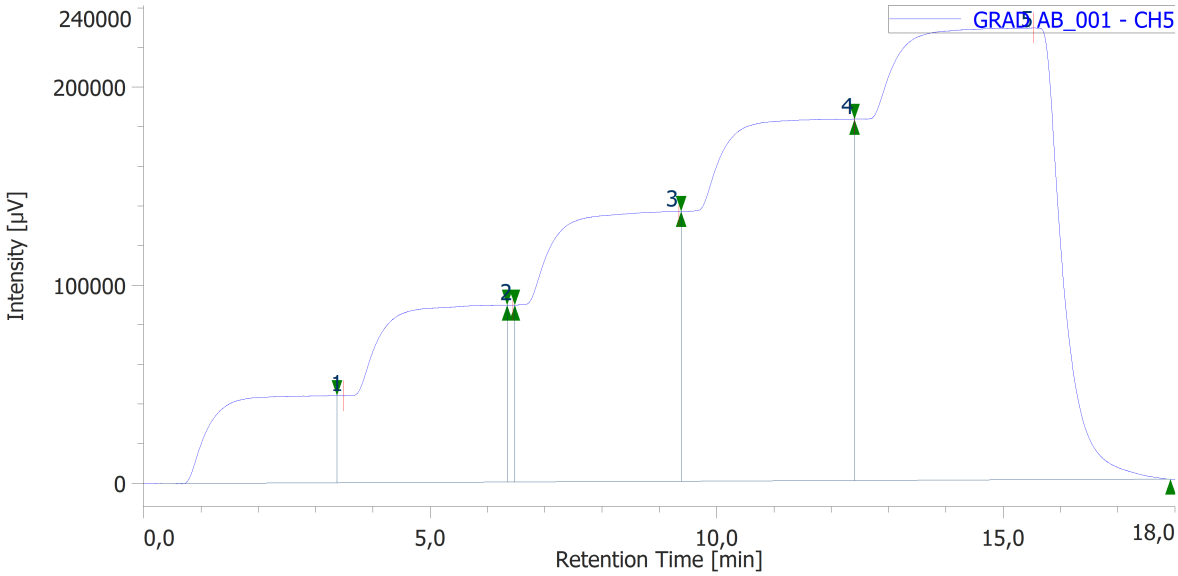

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 14:59:15
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 14:41:03
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação QPack
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	GRAD AB HP06
Peak ID Table	Identificação GRBO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,490	13933197	43822	11,985	6,447	N/A	N/A	N/A	N/A	
2	40%	5	6,440	714198	89301	0,614	13,138	N/A	N/A	N/A	N/A	
3	60%	5	9,340	21920002	136208	18,855	20,040	N/A	N/A	N/A	N/A	
4	80%	5	12,397	31101983	182371	26,753	26,831	N/A	N/A	N/A	N/A	
5	100%	5	15,530	48585927	227993	41,792	33,543	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

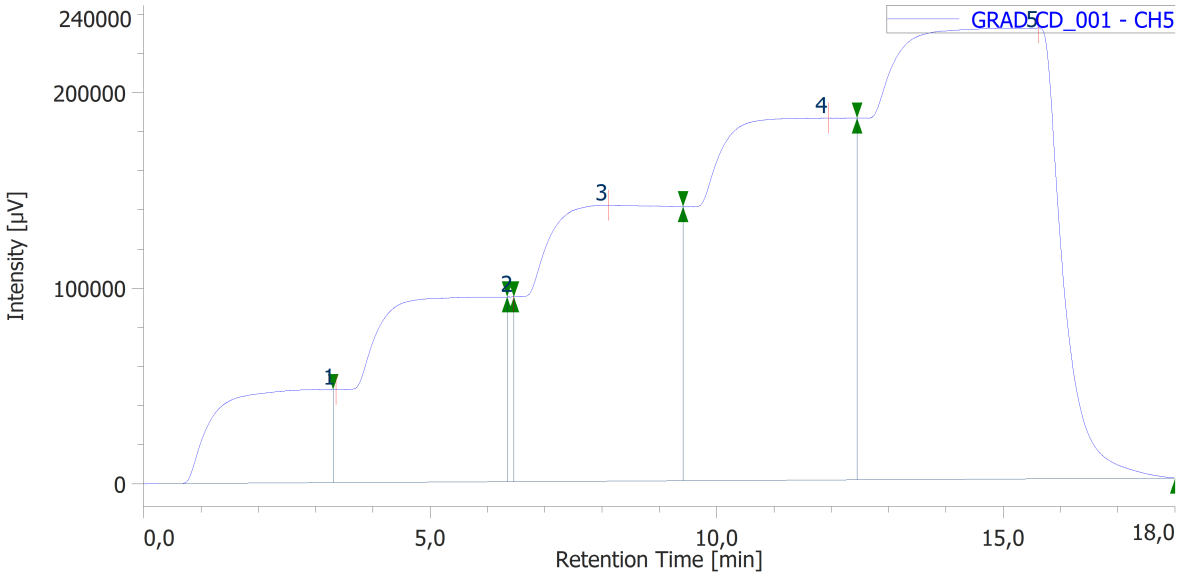

Chromatogram Information	
User Name	QPackSA
Date Modified	08/02/2023 15:44:59
Description	
HPLC System Name	HP06
Injection Date	08/02/2023 15:26:47
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação QPack
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	GRAD CD HP06
Peak ID Table	Identificação GRBO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,357	15091311	47504	12,607	6,803	N/A	N/A	N/A	N/A	
2	40%	5	6,453	660883	94458	0,552	13,528	N/A	N/A	N/A	N/A	
3	60%	5	8,107	23318356	140944	19,480	20,185	N/A	N/A	N/A	N/A	
4	80%	5	11,943	31968742	184957	26,707	26,488	N/A	N/A	N/A	N/A	
5	100%	5	15,617	48664641	230404	40,654	32,997	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Peak Find - EDFL_004 FPEm_tR0,30 D.jws

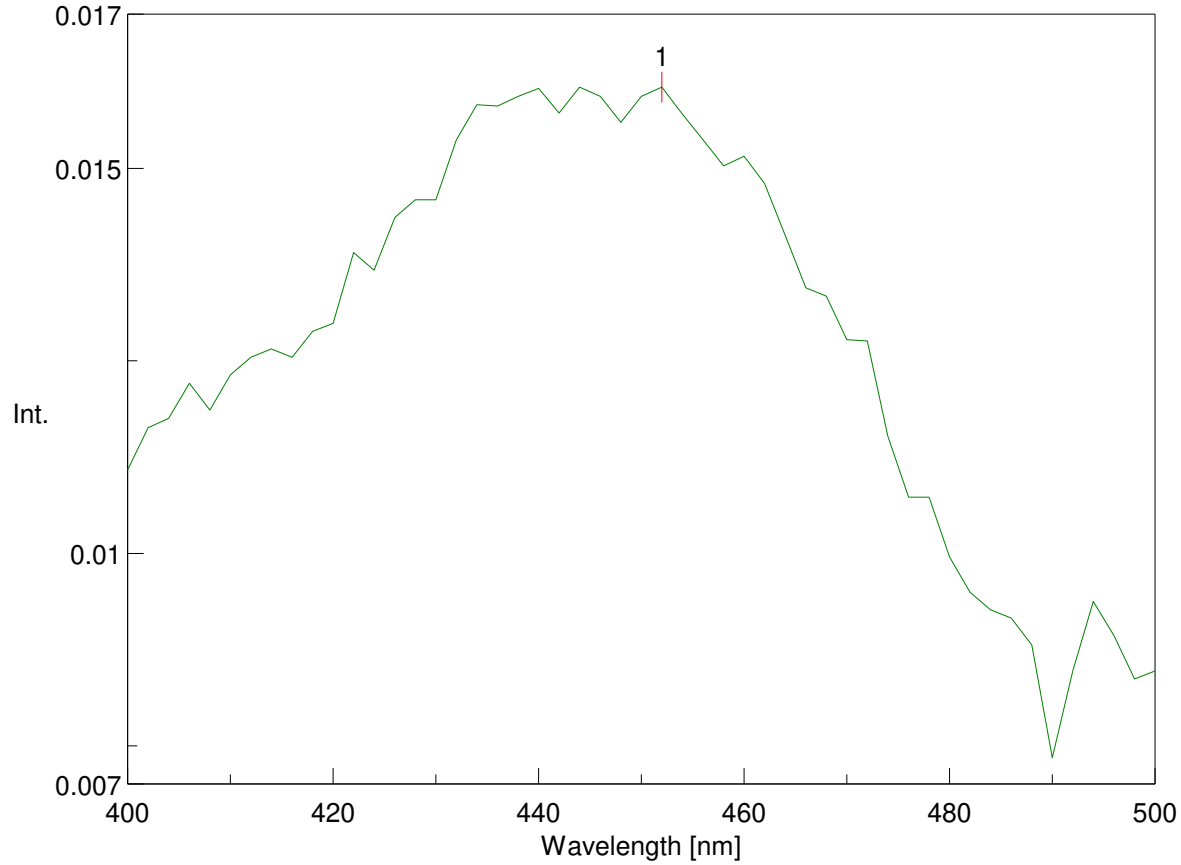

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	08/02/2023 16:09

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	452	0.0160522			

Chromatogram

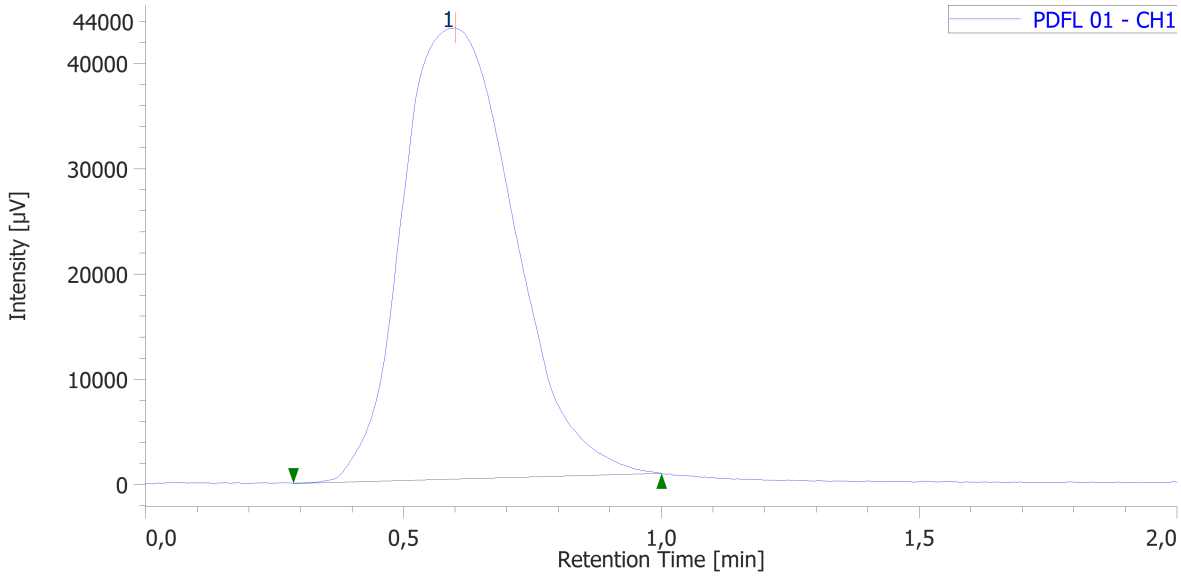

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:47:58
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:45:56
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,600	645746	42820	100,000	100,000	N/A	35	N/A	1,189	

Creator
Reviewer
Approver

Chromatogram

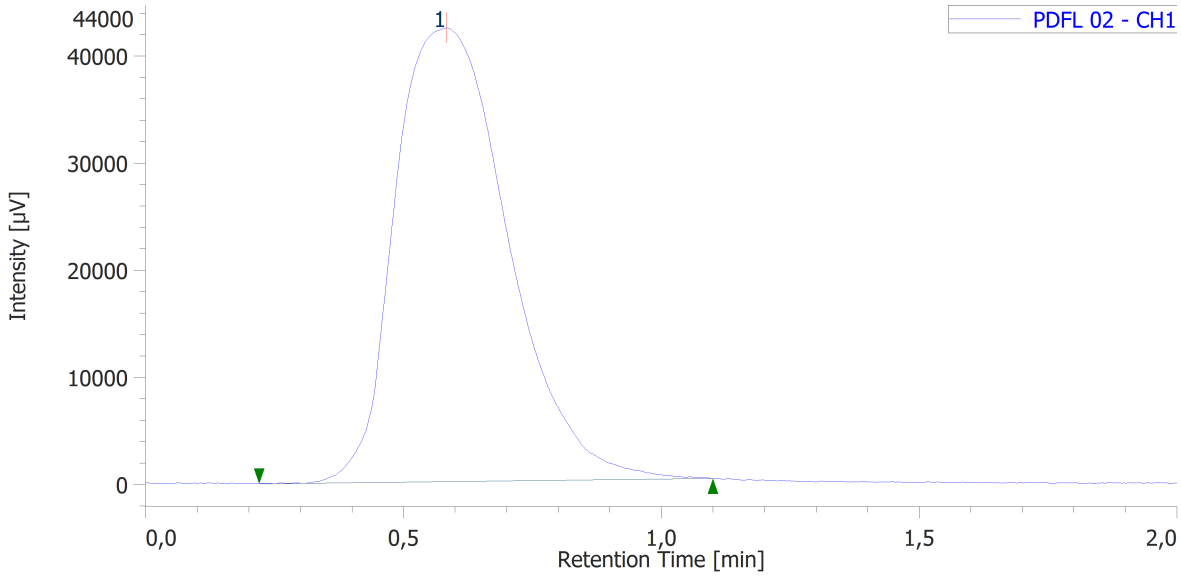

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:50:16
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:48:14
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,583	645974	42335	100,000	100,000	N/A	34	N/A	1,285	

Creator
Reviewer
Approver

Chromatogram

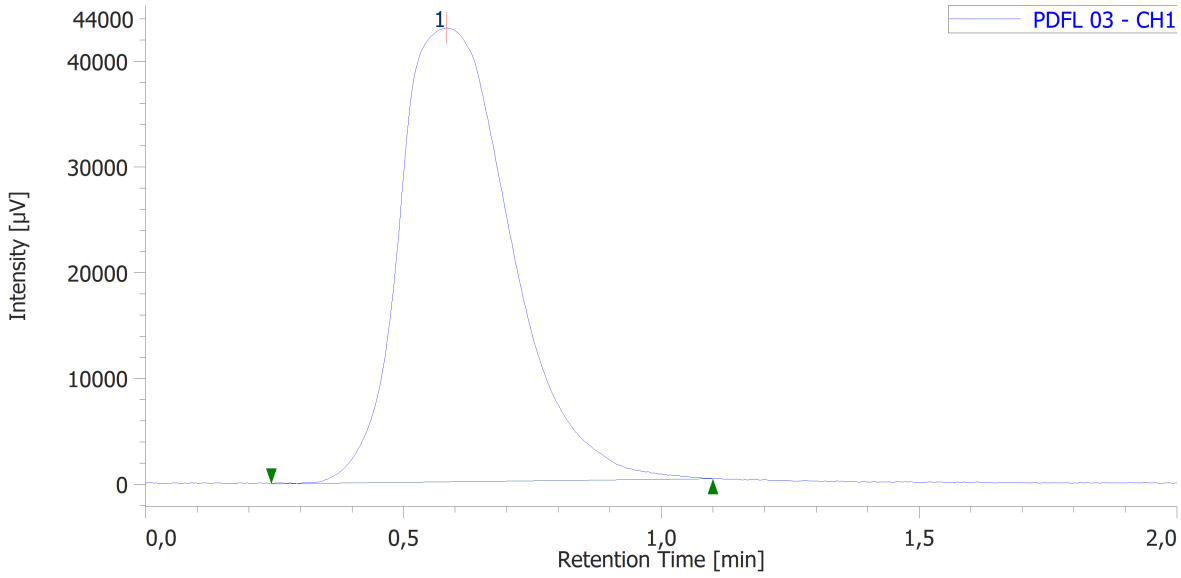

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:52:34
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:50:31
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,583	644522	42890	100,000	100,000	N/A	37	N/A	1,333	

Creator
Reviewer
Approver

Chromatogram

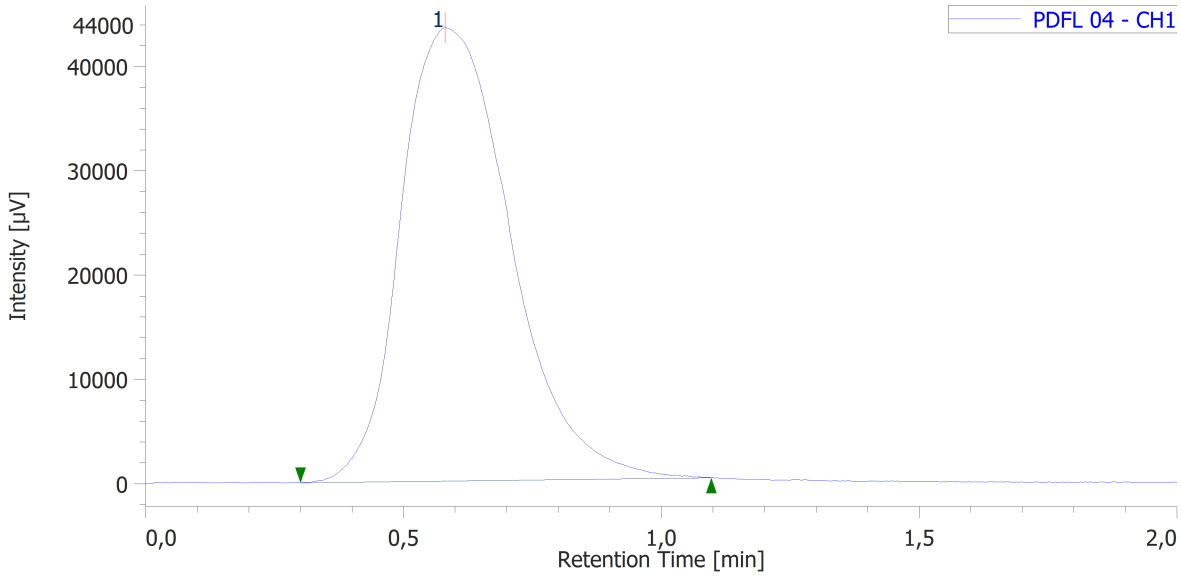

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:54:52
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:52:49
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,580	642997	43423	100,000	100,000	N/A	36	N/A	1,340	

Creator
Reviewer
Approver

Chromatogram

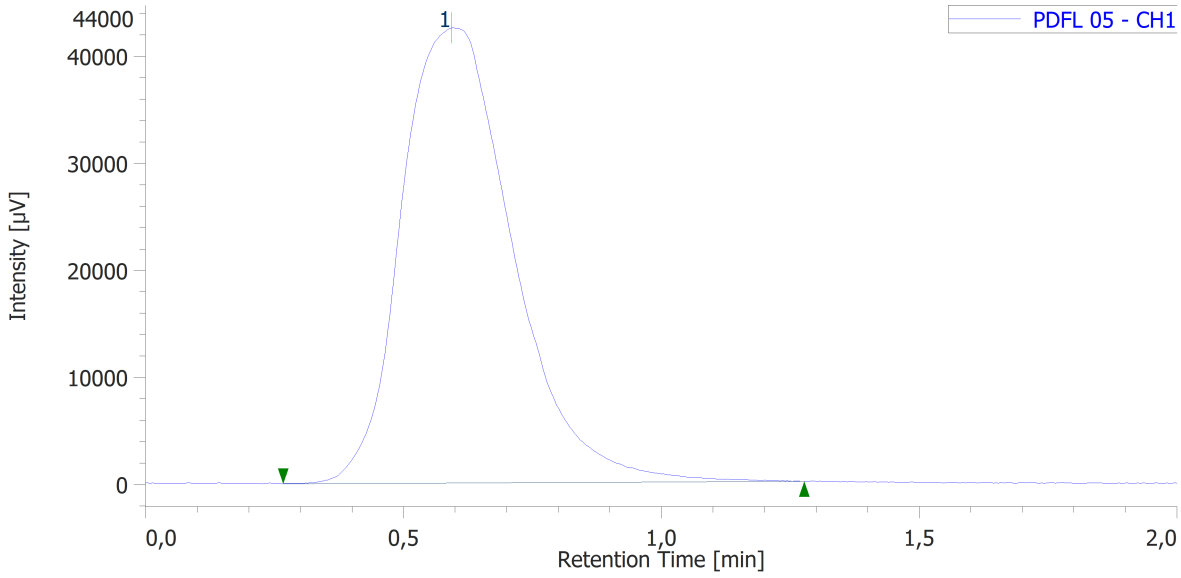

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:57:10
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:55:07
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,593	639026	42492	100,000	100,000	N/A	37	N/A	1,281	

Creator
Reviewer
Approver

Chromatogram

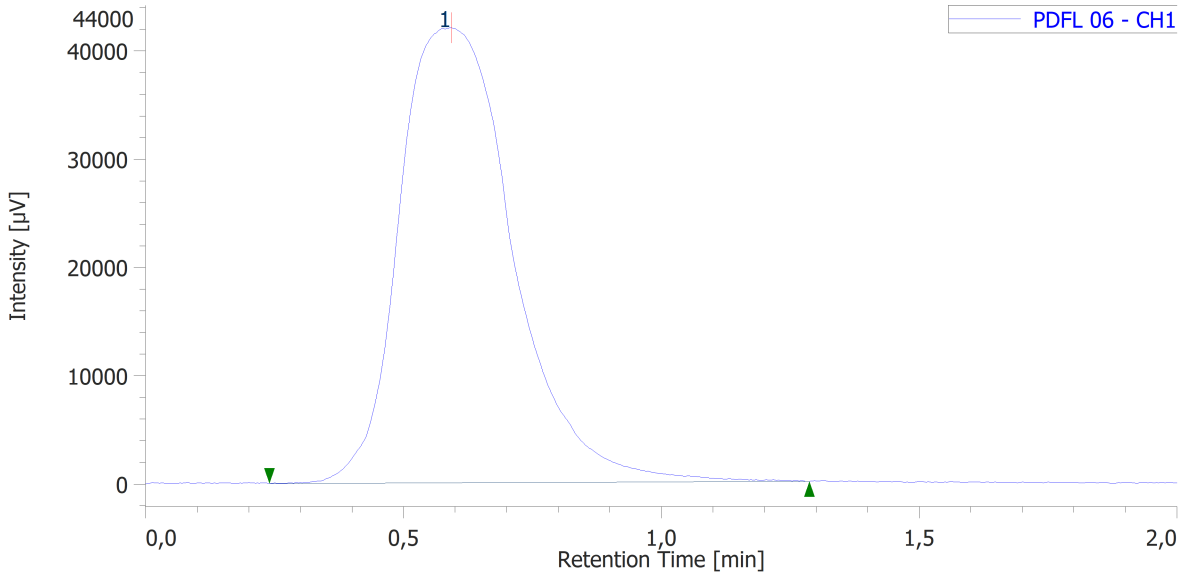

Chromatogram Information	
User Name	QPackSA
Date Modified	09/02/2023 10:59:28
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/02/2023 10:57:25
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP06
Control Method	Qualificação 3120FP HP06
Peak ID Table	Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PDFL 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,593	644111	41983	100,000	100,000	N/A	37	N/A	1,270	

Creator
Reviewer
Approver