
Peak Find - EDUV_001 UV_tR1.42 D.jws

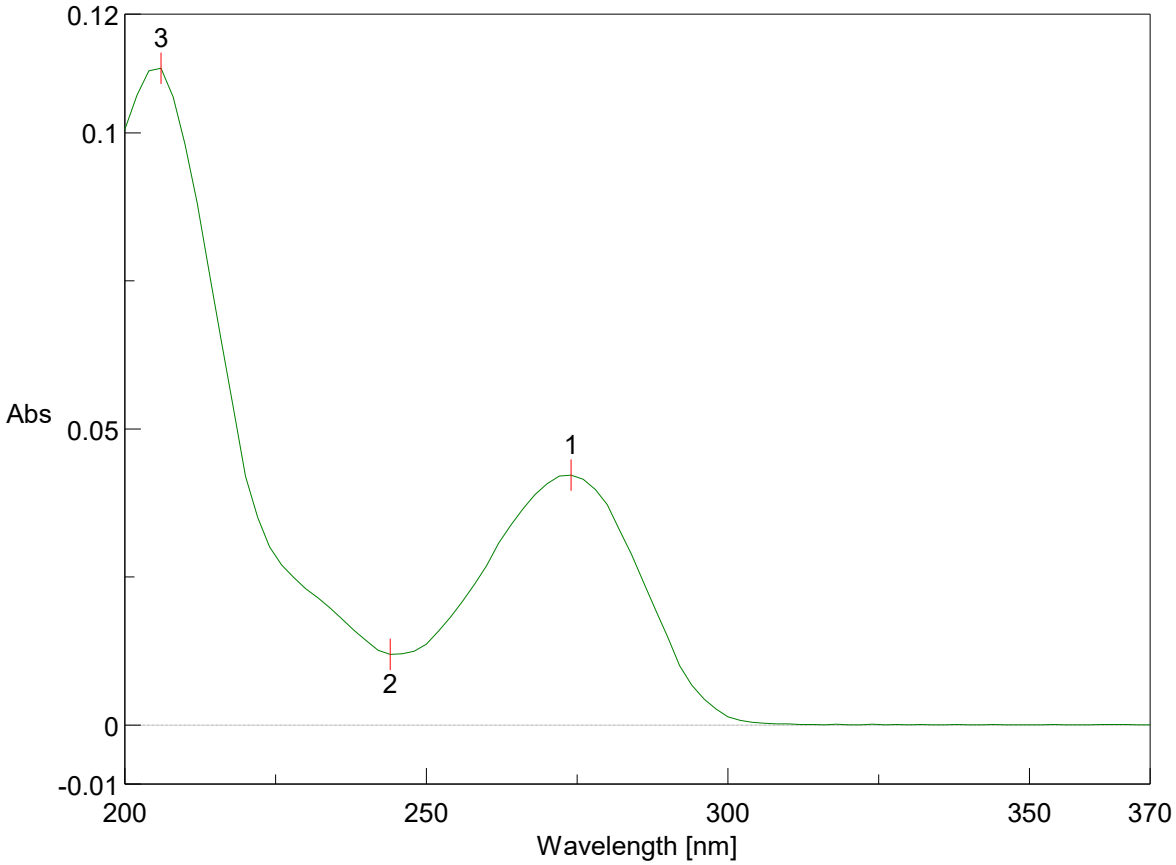

[Comments]

User	QPackSA
Division	---
Company	BBA
Creation date	05/02/2026 11:18
Date modified	05/02/2026 11:19

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	86


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	C044061657
ROM version	1.01.16

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0421824	2	244	0.0118846
3	206	0.110849			

Chromatogram

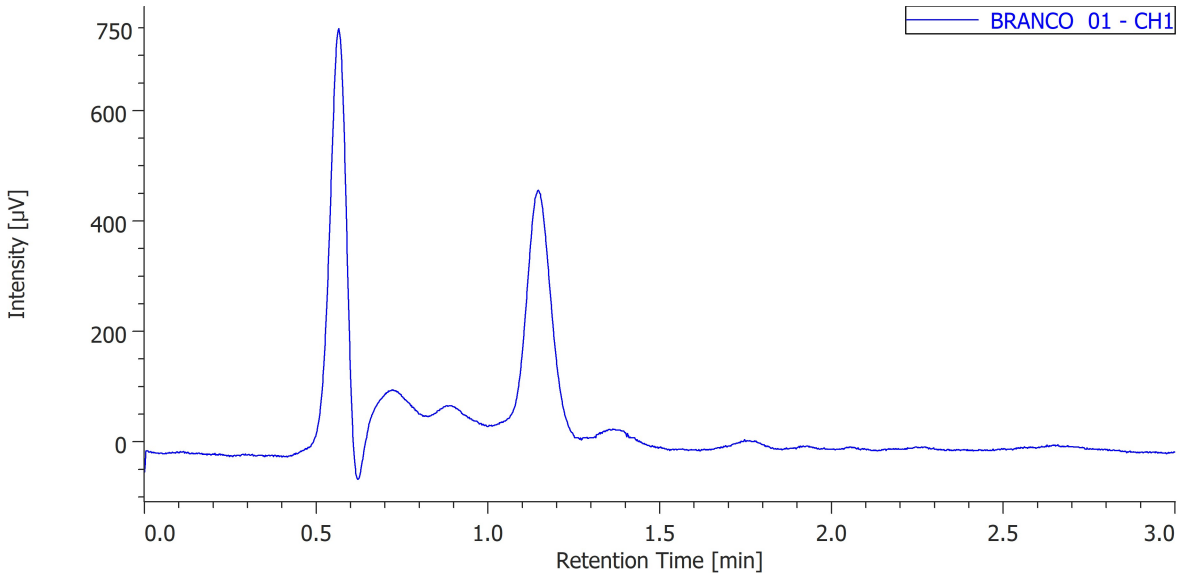


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 11:49:31
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 11:46:31
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

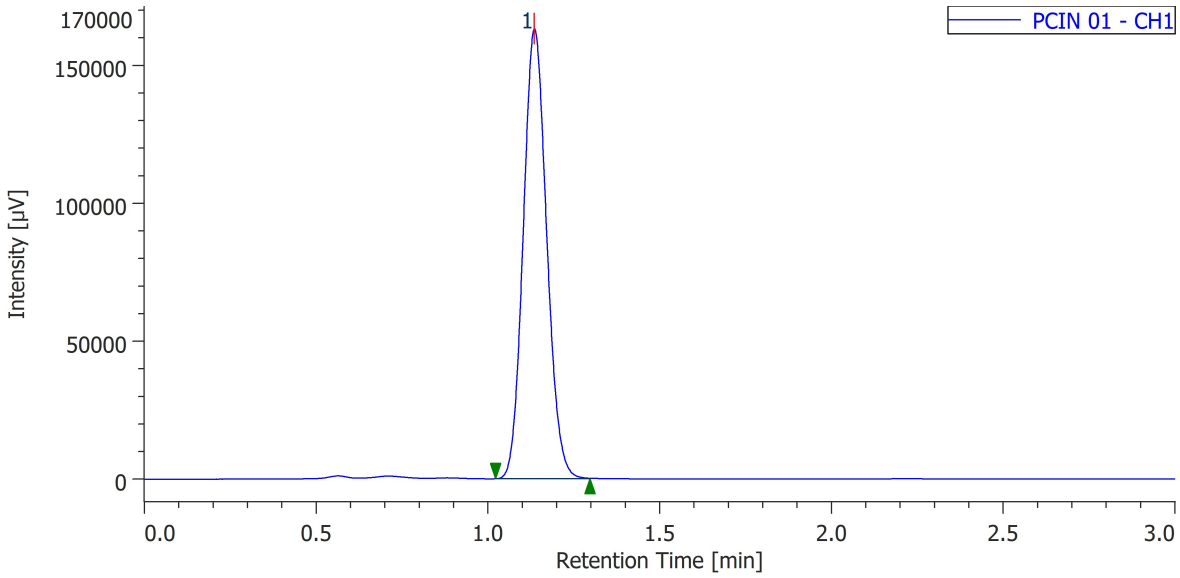

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 11:54:31
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 11:51:30
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.135	772265	163060	100.000	100.000	N/A	1325	N/A	1.105	

Creator QPackSA
Reviewer
Approver

Chromatogram

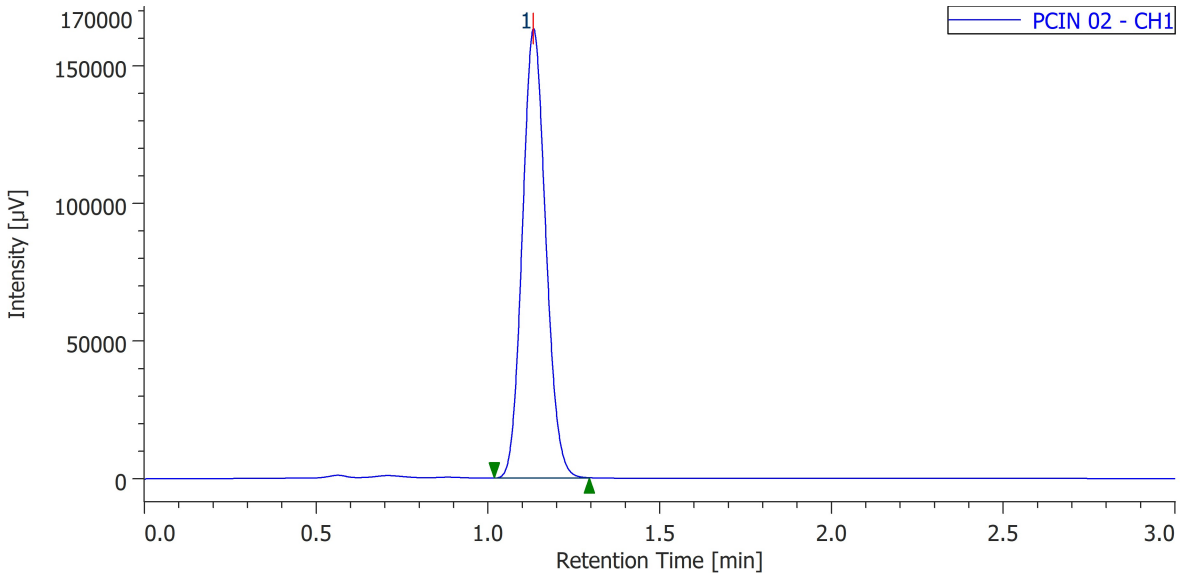

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 11:59:29
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 11:56:28
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.132	772044	163288	100.000	100.000	N/A	1323	N/A	1.113	

Creator QPackSA
Reviewer
Approver

Chromatogram

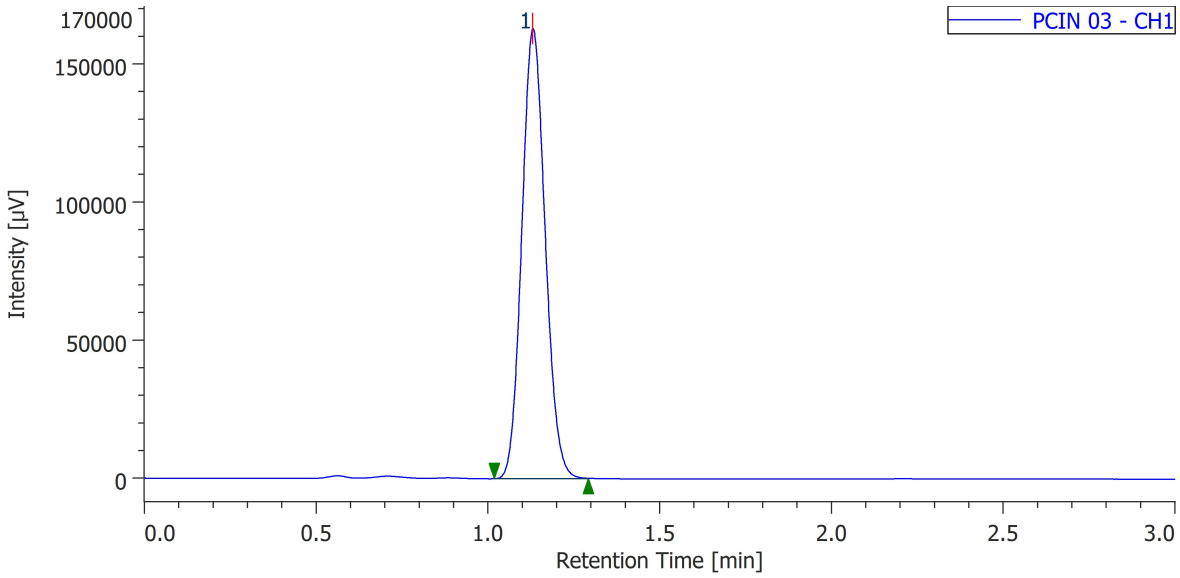

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:04:29
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:01:27
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.130	768821	162823	100.000	100.000	N/A	1322	N/A	1.114	

Creator QPackSA
Reviewer
Approver

Chromatogram

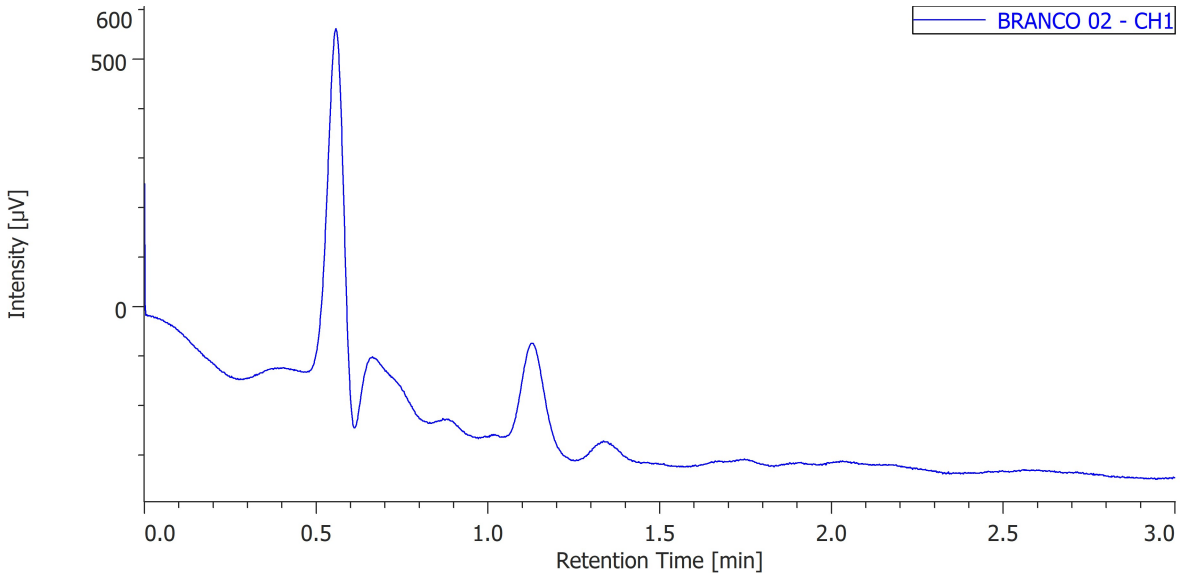


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:09:27
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:06:26
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

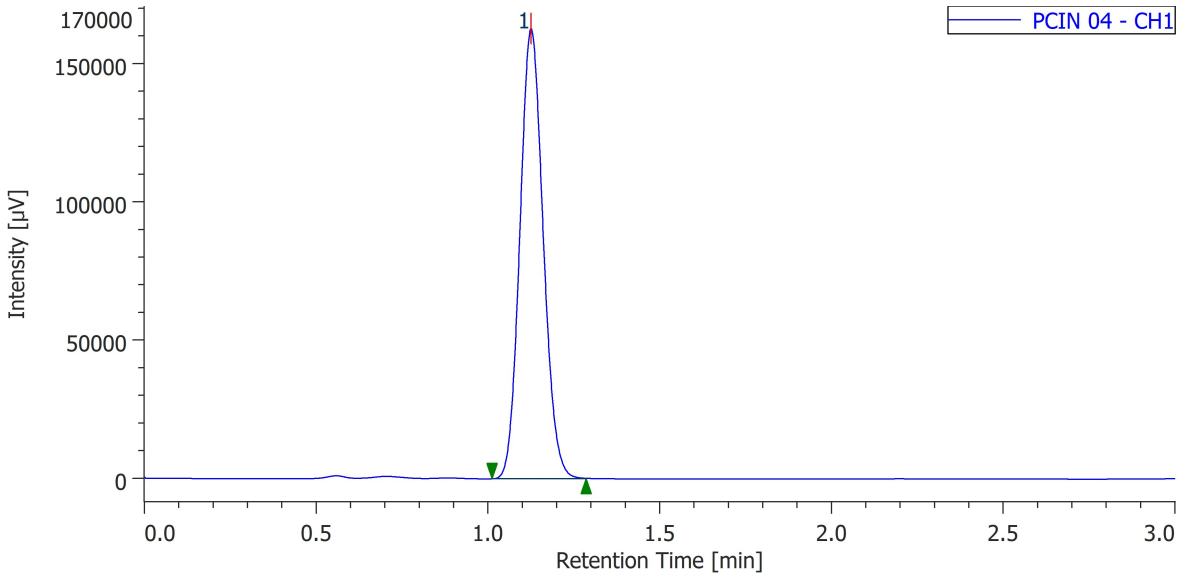

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:14:25
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:11:24
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.125	765793	162668	100.000	100.000	N/A	1318	N/A	1.102	

Creator QPackSA
Reviewer
Approver

Chromatogram

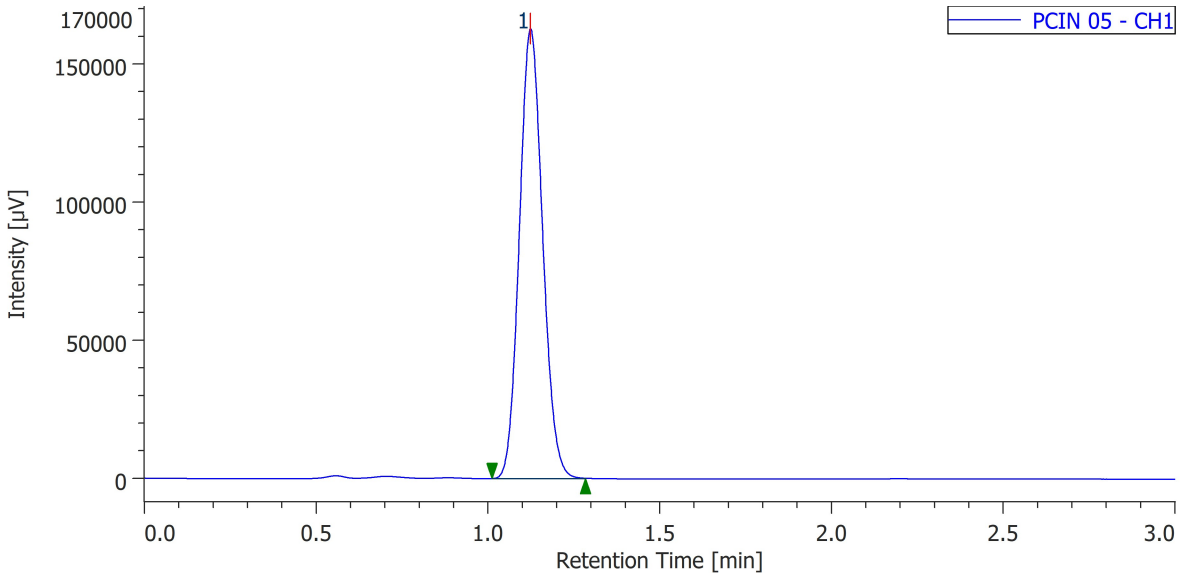

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:19:25
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:16:23
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.123	765110	162780	100.000	100.000	N/A	1318	N/A	1.102	

Creator QPackSA
Reviewer
Approver

Chromatogram

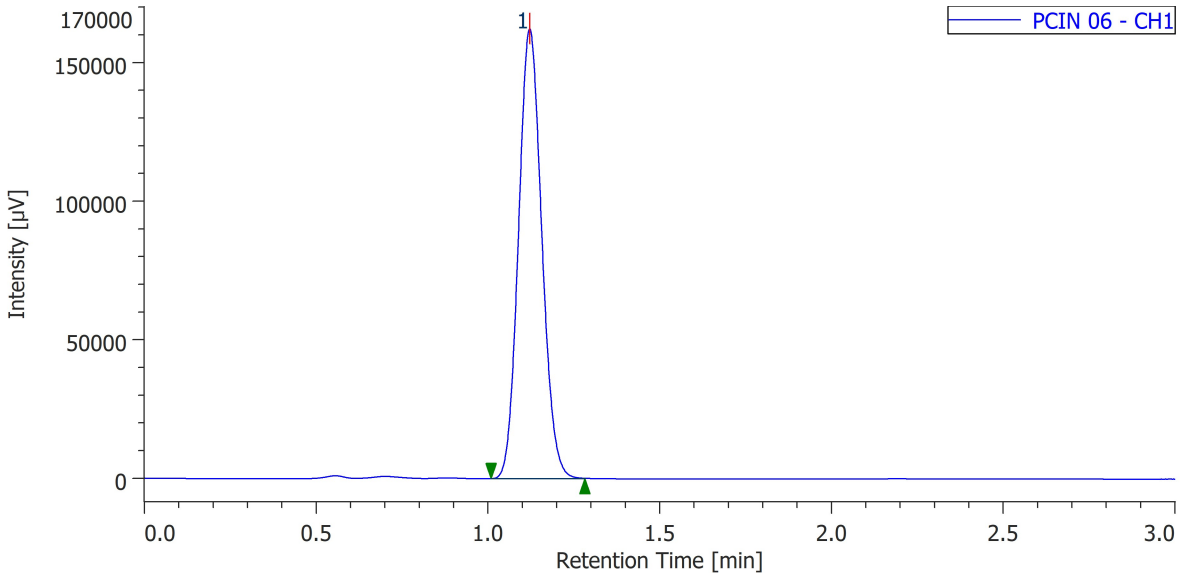

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:24:23
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:21:21
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.122	762079	162269	100.000	100.000	N/A	1316	N/A	1.090	

Creator QPackSA
Reviewer
Approver

Chromatogram

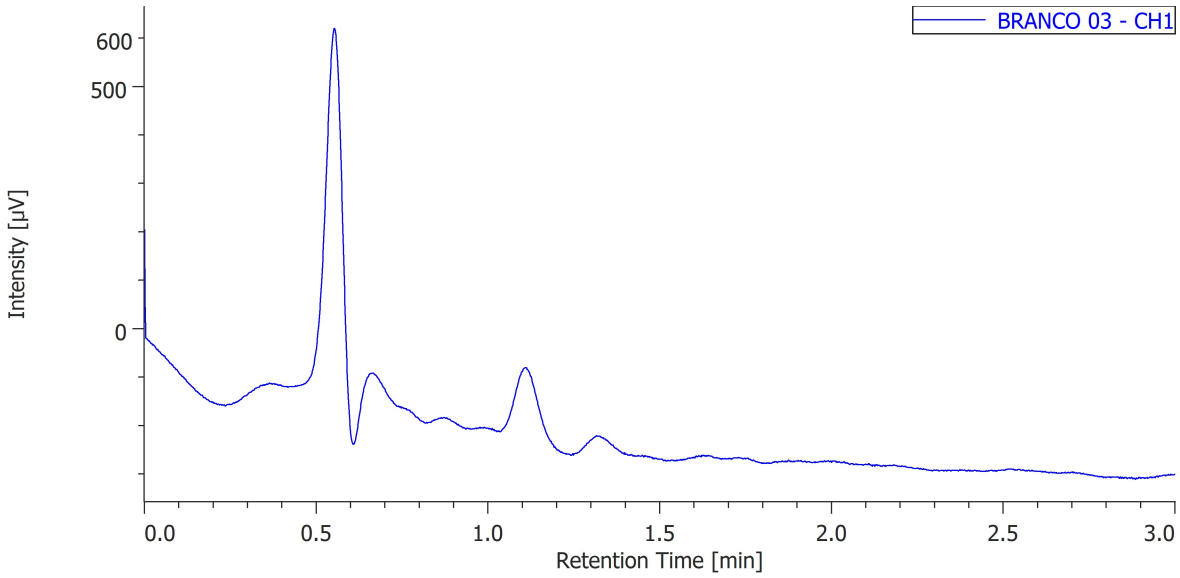


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:29:21
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:26:20
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

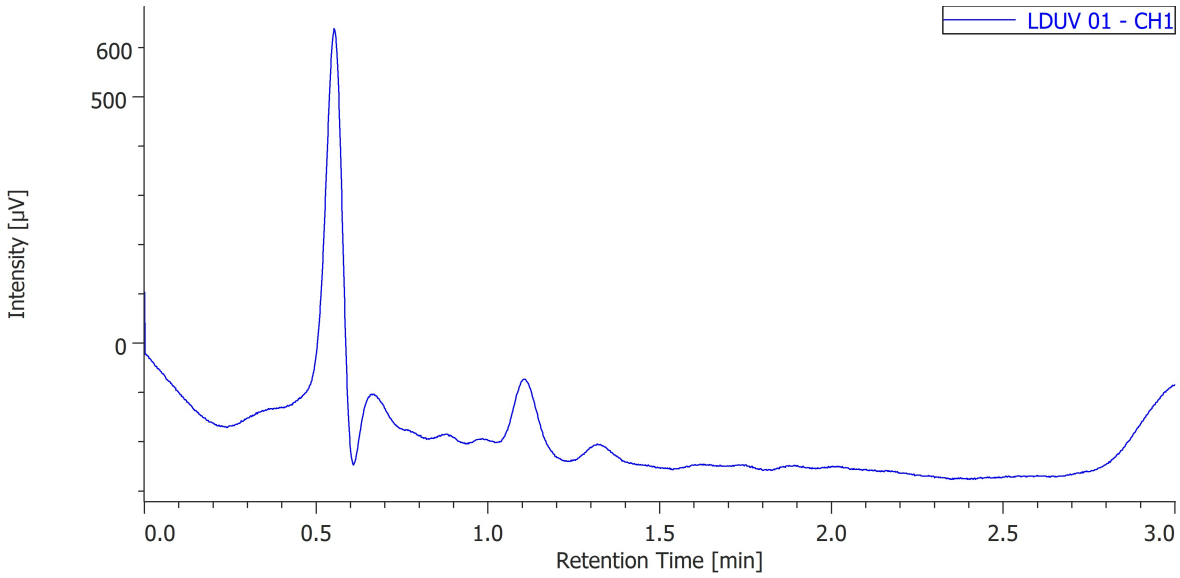


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:34:19
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:31:19
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

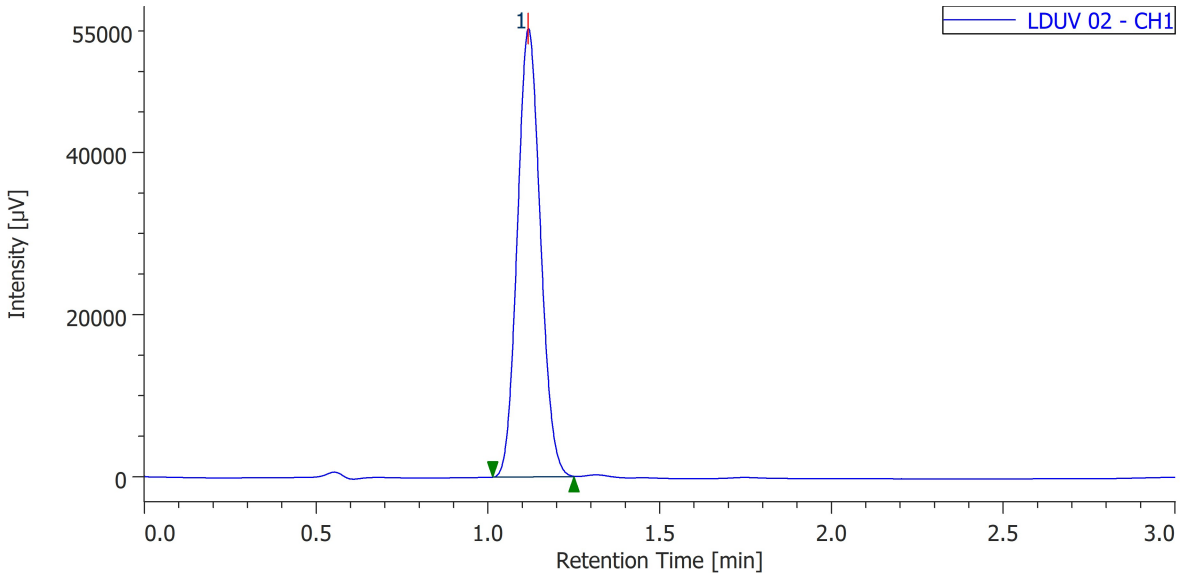

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:39:19
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:36:17
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.117	257808	55268	100.000	100.000	N/A	1313	N/A	1.109	

Creator QPackSA
Reviewer
Approver

Chromatogram

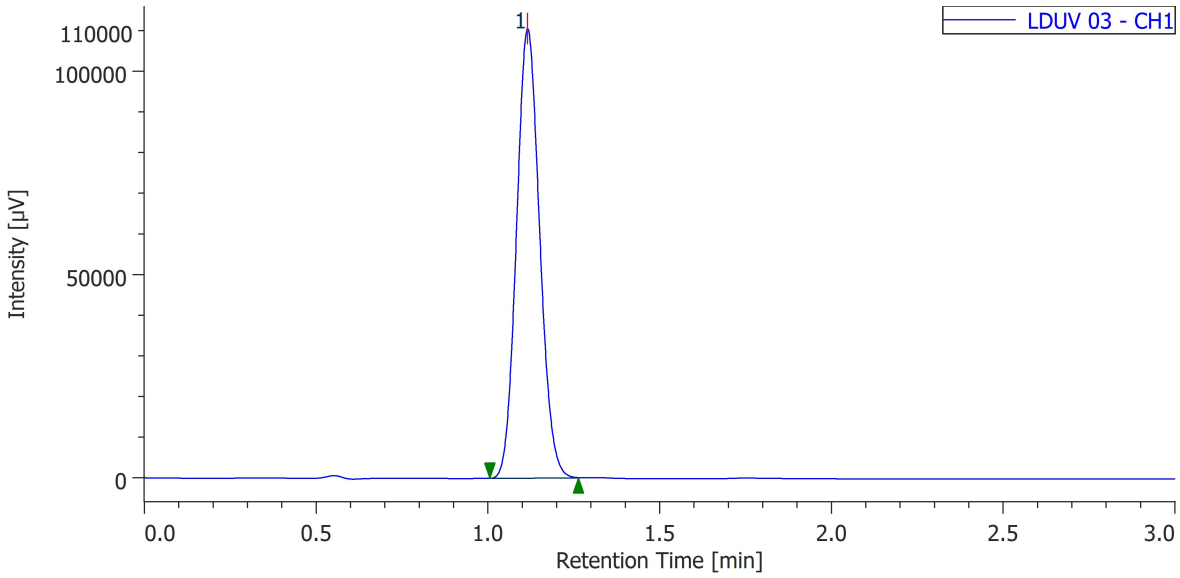

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:44:17
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:41:16
Volume	10.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.115	517300	110500	100.000	100.000	N/A	1306	N/A	1.100	

Creator QPackSA
Reviewer
Approver

Chromatogram

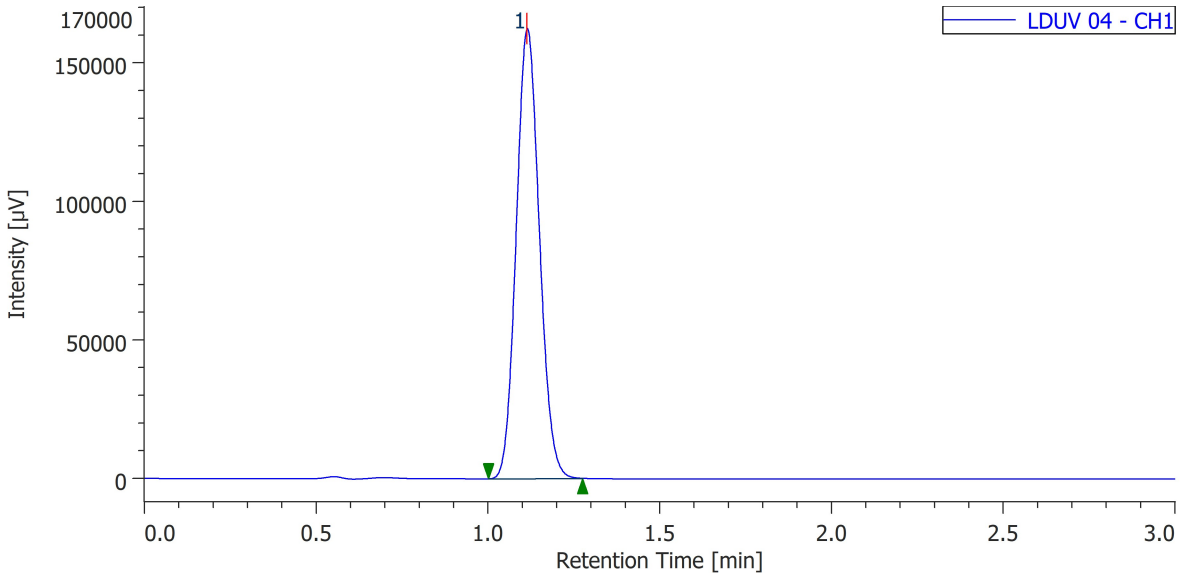

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:49:17
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:46:15
Volume	10.0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.113	761038	162325	100.000	100.000	N/A	1301	N/A	1.115	

Creator QPackSA
Reviewer
Approver

Chromatogram

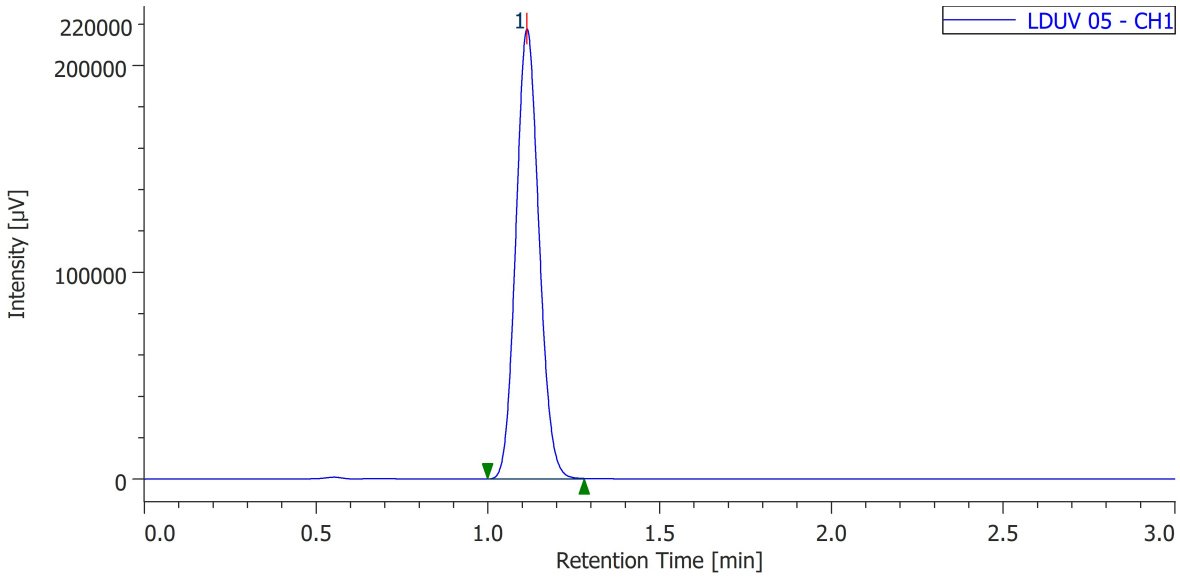

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 12:54:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:51:11
Volume	10.0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.113	1017941	217606	100.000	100.000	N/A	1307	N/A	1.100	

Creator QPackSA
Reviewer
Approver

Chromatogram

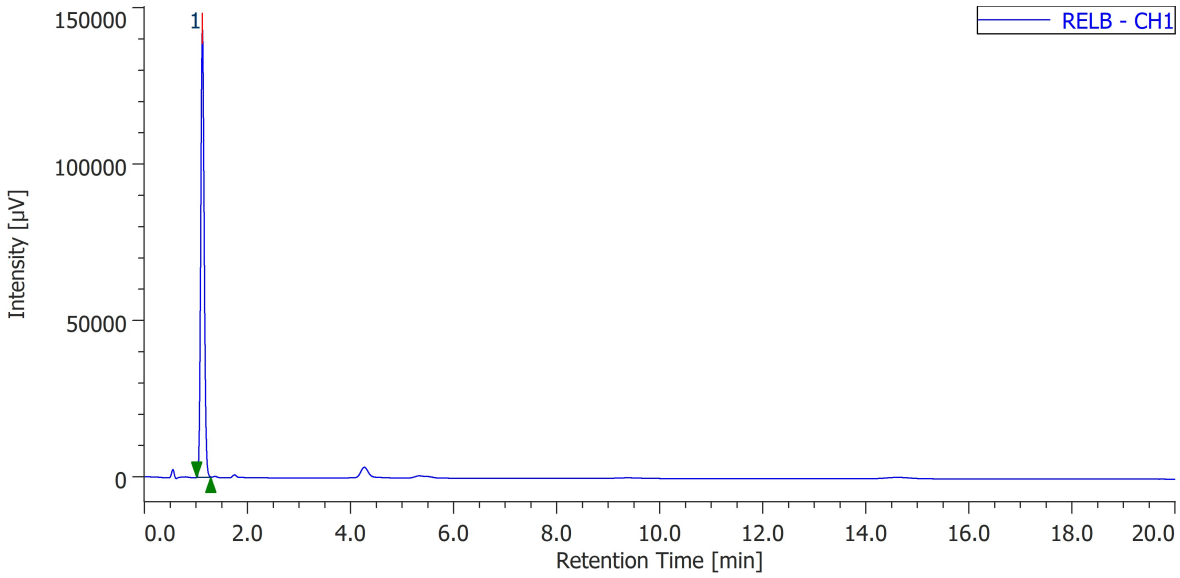

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:23:56
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:56:28
Volume	20.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.125	666538	143396	100.000	100.000	N/A	1358	N/A	1.099	

Creator QPackSA
Reviewer
Approver

Chromatogram

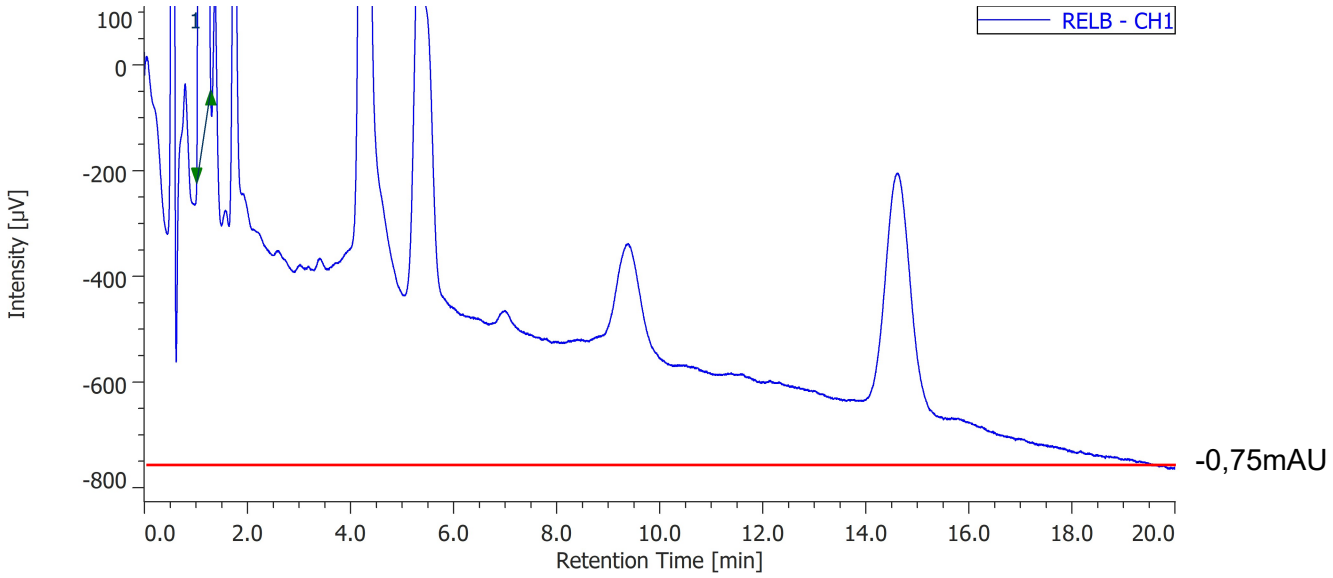

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:23:56
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:56:28
Volume	20.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.125	666538	143396	100.000	100.000	N/A	1358	N/A	1.099	

Creator QPackSA
Reviewer
Approver

Chromatogram

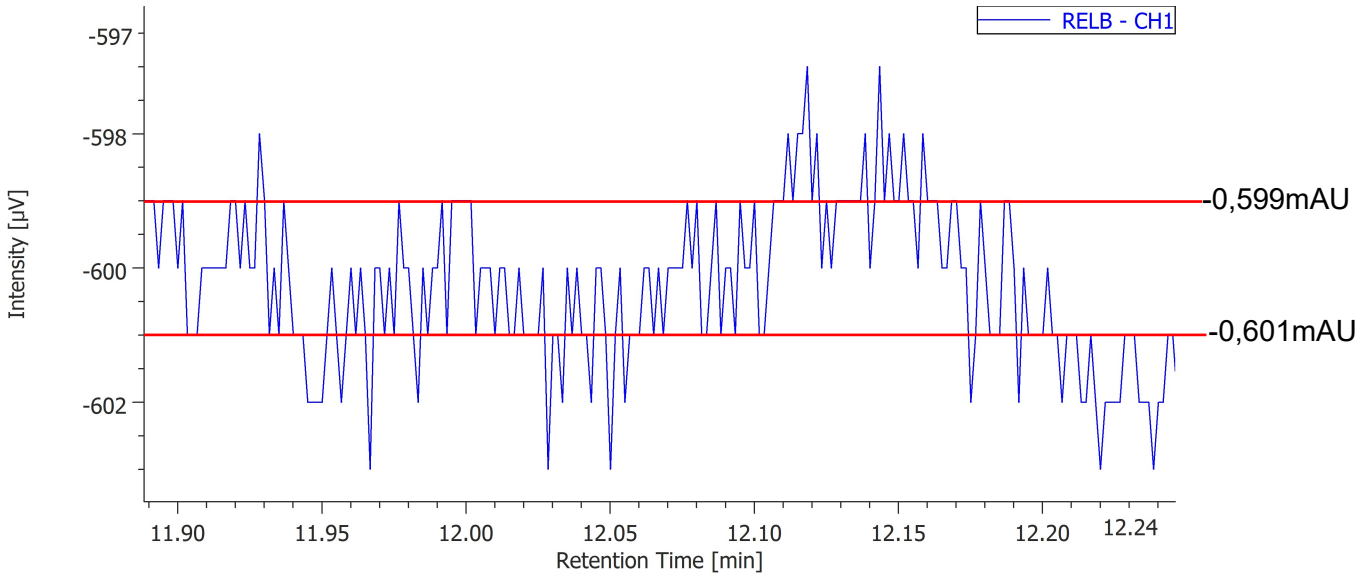

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:23:56
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 12:56:28
Volume	20.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.125	666538	143396	100.000	100.000	N/A	1358	N/A	1.099	

Creator QPackSA
Reviewer
Approver

Chromatogram

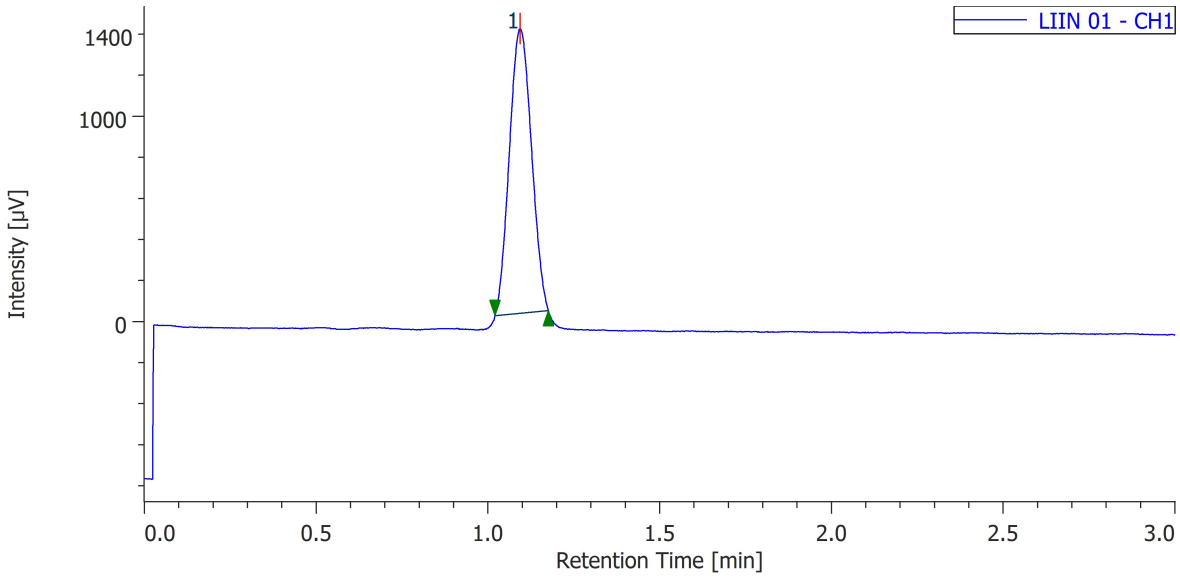

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 13:19:41
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 13:16:40
Volume	0.1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.093	6178	1386	100.000	100.000	N/A	1282	N/A	1.058	

Creator QPackSA
Reviewer
Approver

Chromatogram

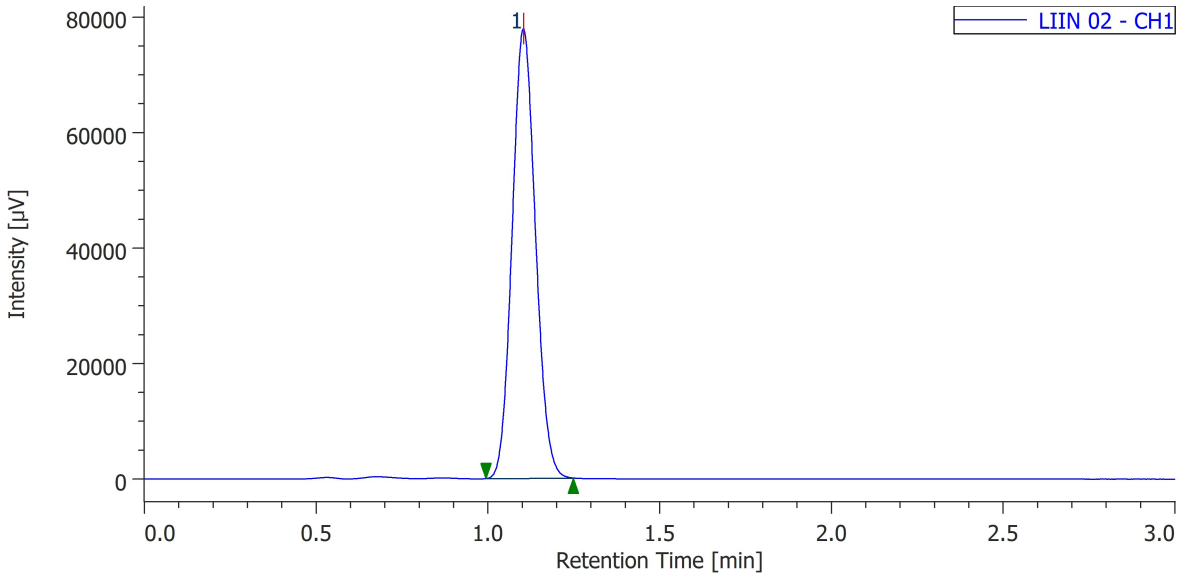

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 13:24:29
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 13:21:28
Volume	5.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.103	366905	77857	100.000	100.000	N/A	1259	N/A	1.082	

Creator QPackSA
Reviewer
Approver

Chromatogram

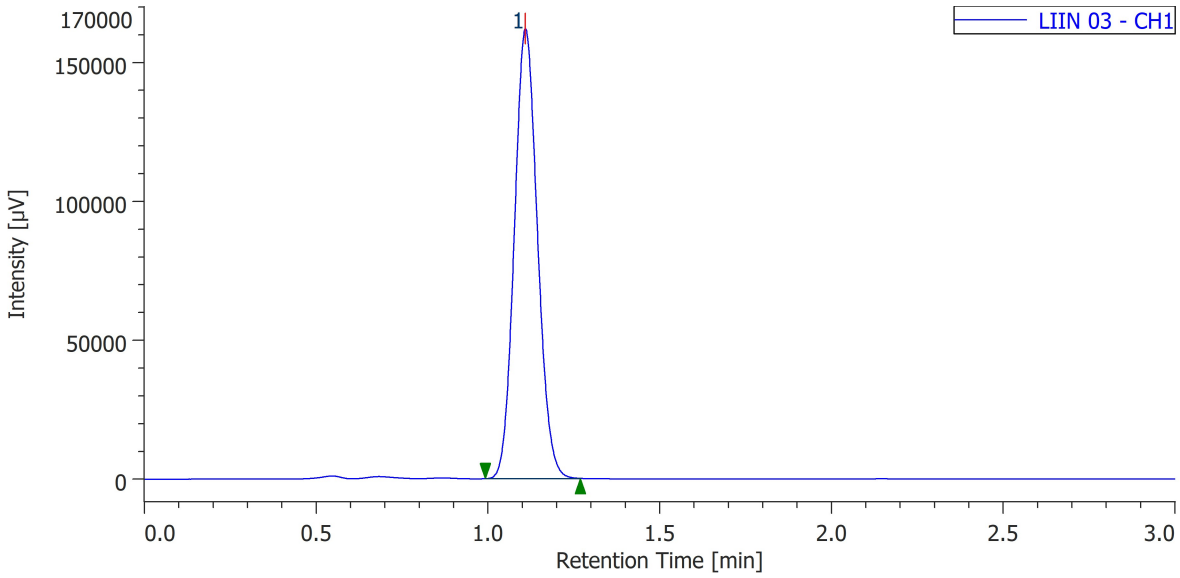

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 13:29:25
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 13:26:24
Volume	10.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.108	756419	161923	100.000	100.000	N/A	1300	N/A	1.101	

Creator QPackSA
Reviewer
Approver

Chromatogram

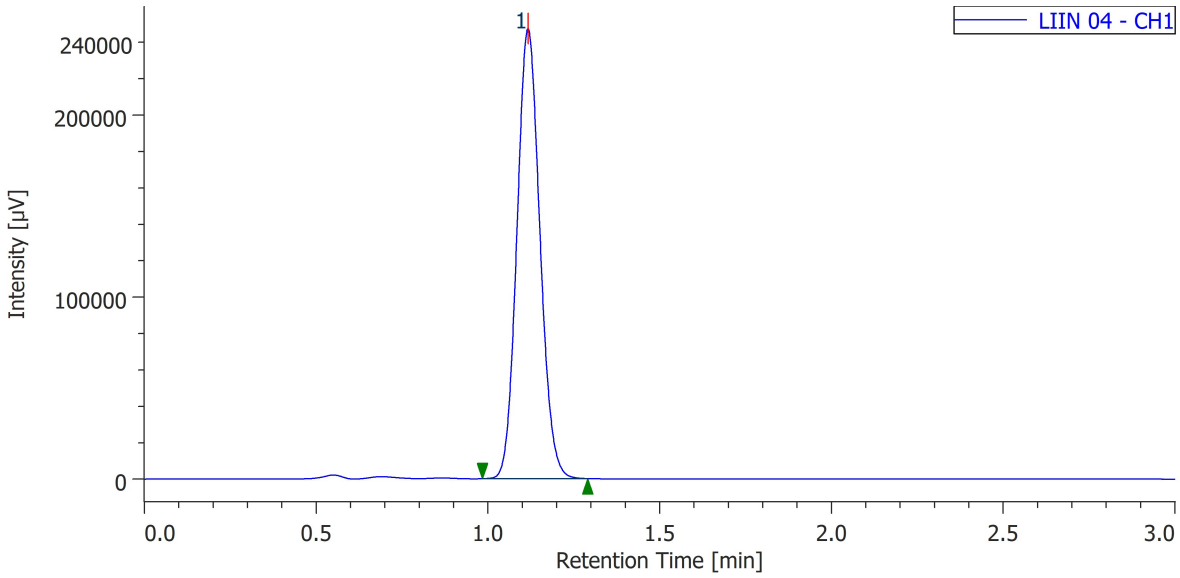

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 13:34:33
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 13:31:31
Volume	15.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.117	1149764	247148	100.000	100.000	N/A	1337	N/A	1.090	

Creator QPackSA
Reviewer
Approver

Chromatogram

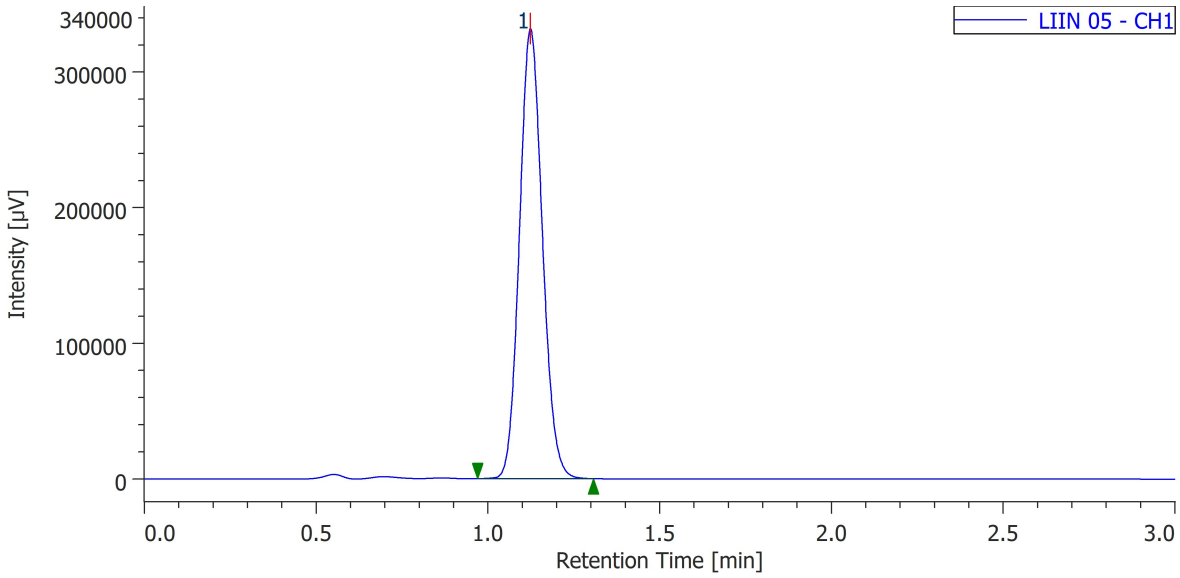

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 13:39:51
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 13:36:49
Volume	20.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.123	1540519	331722	100.000	100.000	N/A	1362	N/A	1.107	

Creator QPackSA
Reviewer
Approver

Chromatogram

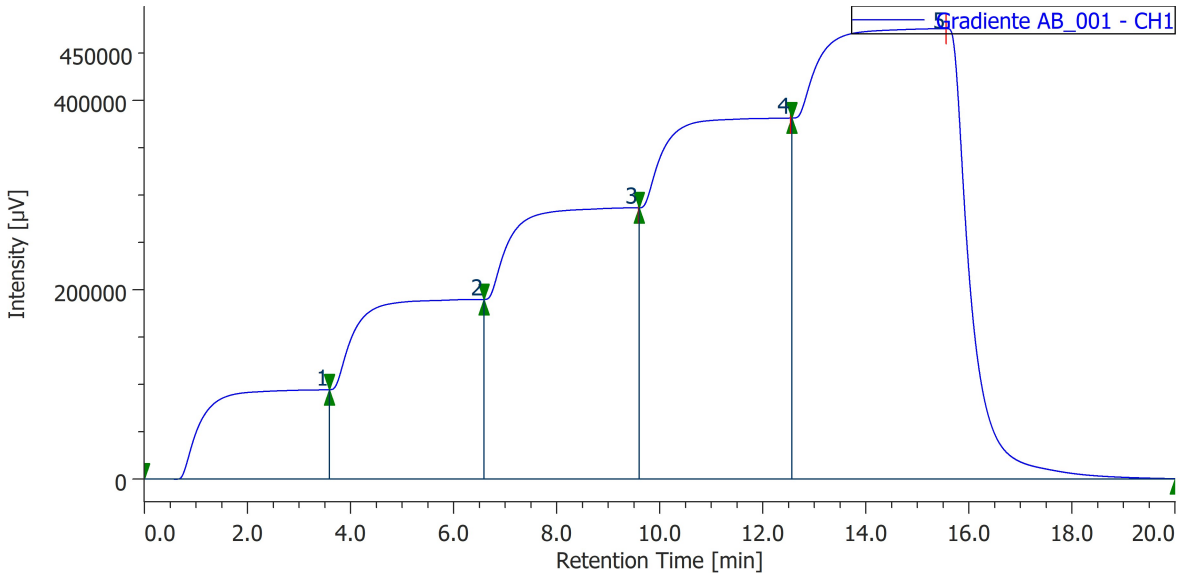

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:30:39
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 14:17:30
Volume	0.0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.588	14125601	94149	5.494	6.603	N/A	N/A	N/A	N/A	
2	40%	1	6.587	31359371	189394	12.198	13.283	N/A	N/A	N/A	N/A	
3	60%	1	9.587	48814497	286070	18.987	20.064	N/A	N/A	N/A	N/A	
4	80%	1	12.535	65058483	380851	25.306	26.711	N/A	N/A	N/A	N/A	
5	100%	1	15.557	97732058	475337	38.015	33.338	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

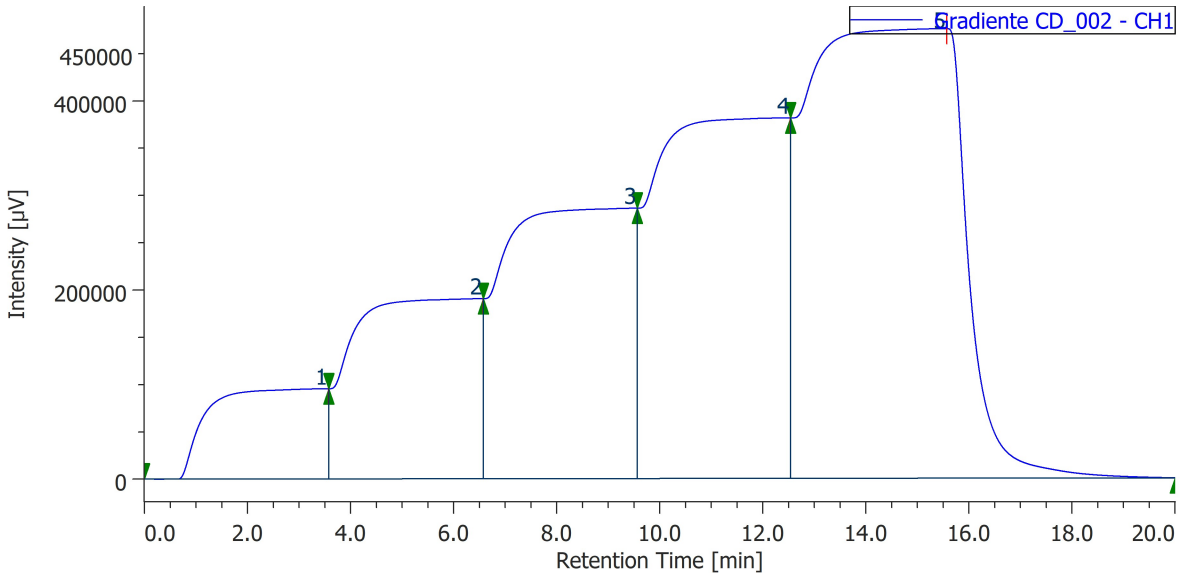

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:30:39
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	05/02/2026 14:40:08
Volume	0.0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.570	14199716	95237	5.518	6.672	N/A	N/A	N/A	N/A	
2	40%	1	6.570	31434844	190265	12.216	13.330	N/A	N/A	N/A	N/A	
3	60%	1	9.560	48327826	285775	18.781	20.021	N/A	N/A	N/A	N/A	
4	80%	1	12.533	65078503	380960	25.291	26.690	N/A	N/A	N/A	N/A	
5	100%	1	15.567	98277197	475123	38.193	33.287	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

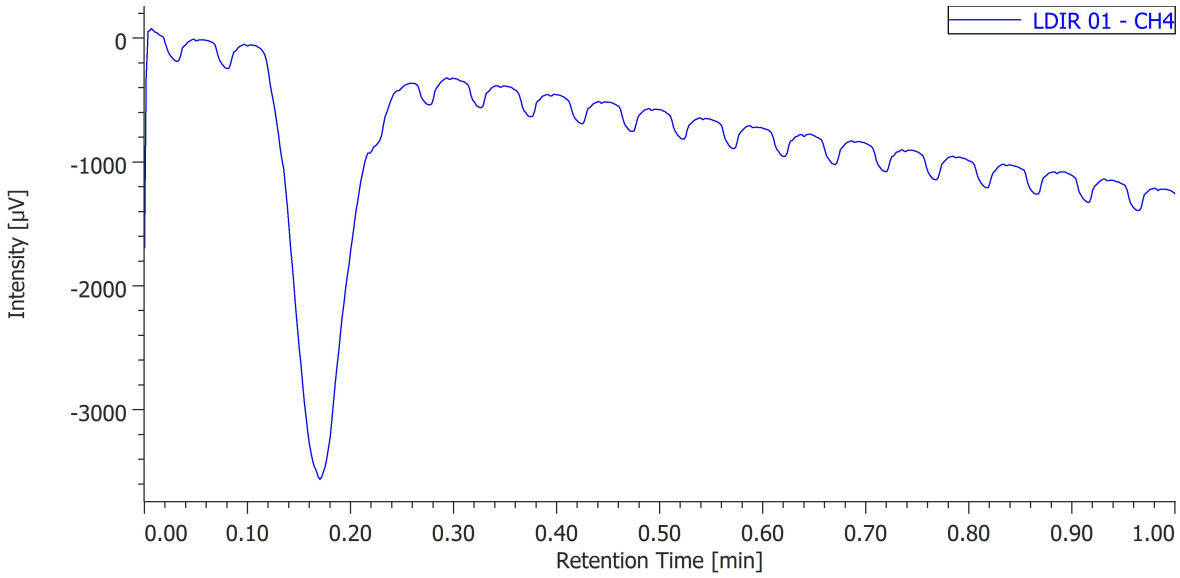


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:11:55
Description	
HPLC System Name	BBA HPLC 03 RI
Injection Date	05/02/2026 16:53:11
Volume	10.0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	OQ_IR
Control Method	OQ RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	100 [msec]
Peak Method	IR

Creator QPackSA
Reviewer
Approver

Chromatogram

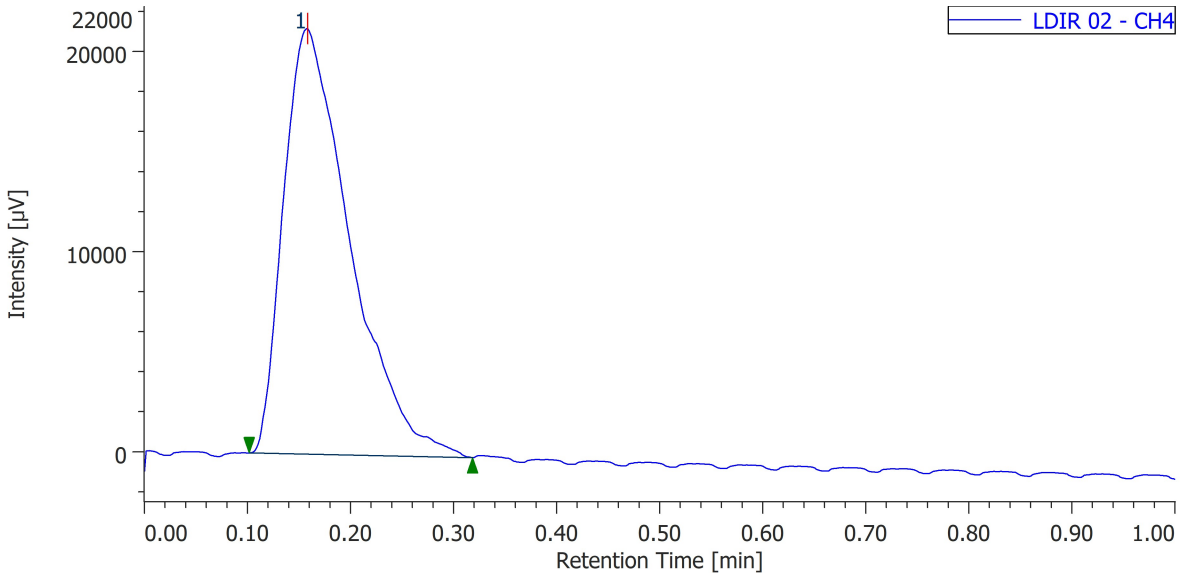

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:11:55
Description	
HPLC System Name	BBA HPLC 03 RI
Injection Date	05/02/2026 16:57:19
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	OQ_IR
Control Method	OQ RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	100 [msec]
Peak Method	IR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.158	95154	21253	100.000	100.000	N/A	30	N/A	1.694	

Creator QPackSA
Reviewer
Approver

Chromatogram

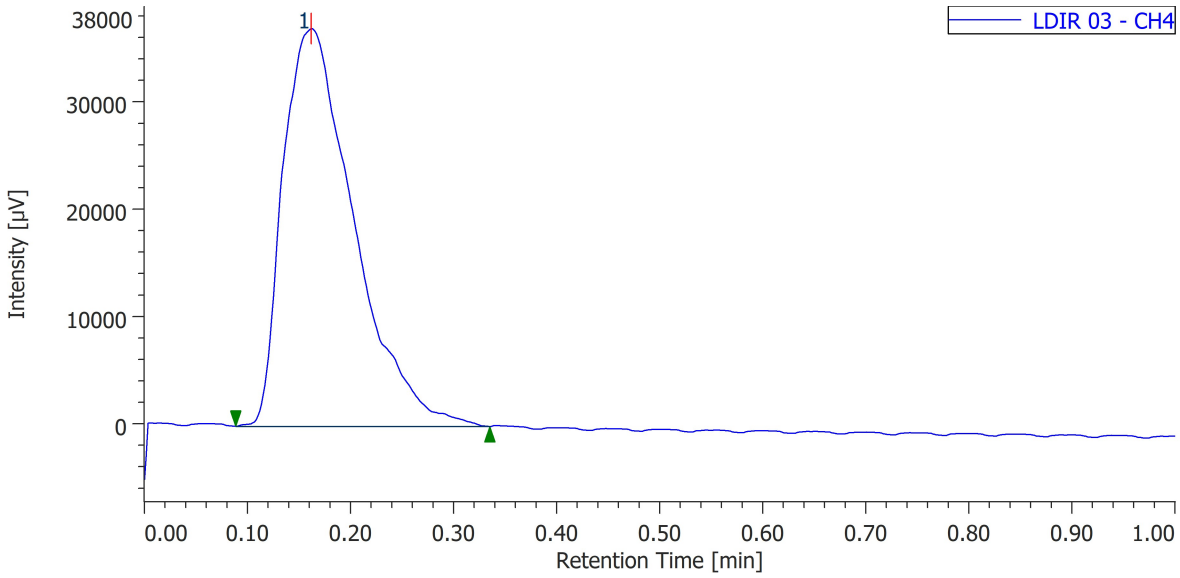

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:11:55
Description	
HPLC System Name	BBA HPLC 03 RI
Injection Date	05/02/2026 17:01:25
Volume	10.0 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	OQ_IR
Control Method	OQ RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	100 [msec]
Peak Method	IR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.162	177297	37034	100.000	100.000	N/A	26	N/A	1.640	

Creator QPackSA
Reviewer
Approver

Chromatogram

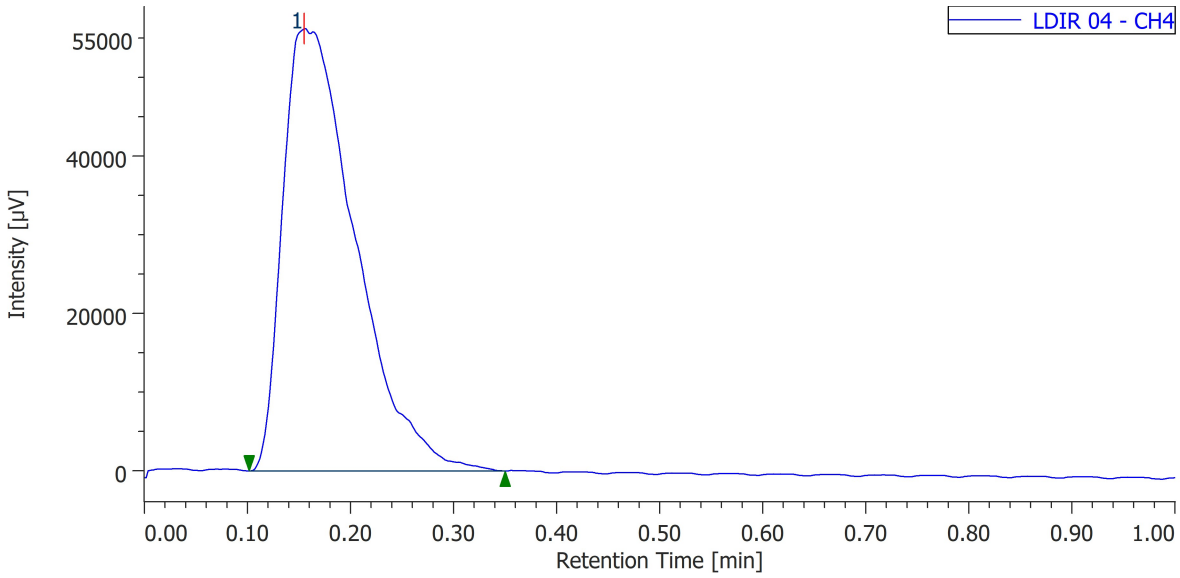

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:11:56
Description	
HPLC System Name	BBA HPLC 03 RI
Injection Date	05/02/2026 17:05:32
Volume	10.0 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	OQ_IR
Control Method	OQ RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	100 [msec]
Peak Method	IR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.155	275587	56217	100.000	100.000	N/A	23	N/A	2.004	

Creator QPackSA
Reviewer
Approver

Chromatogram

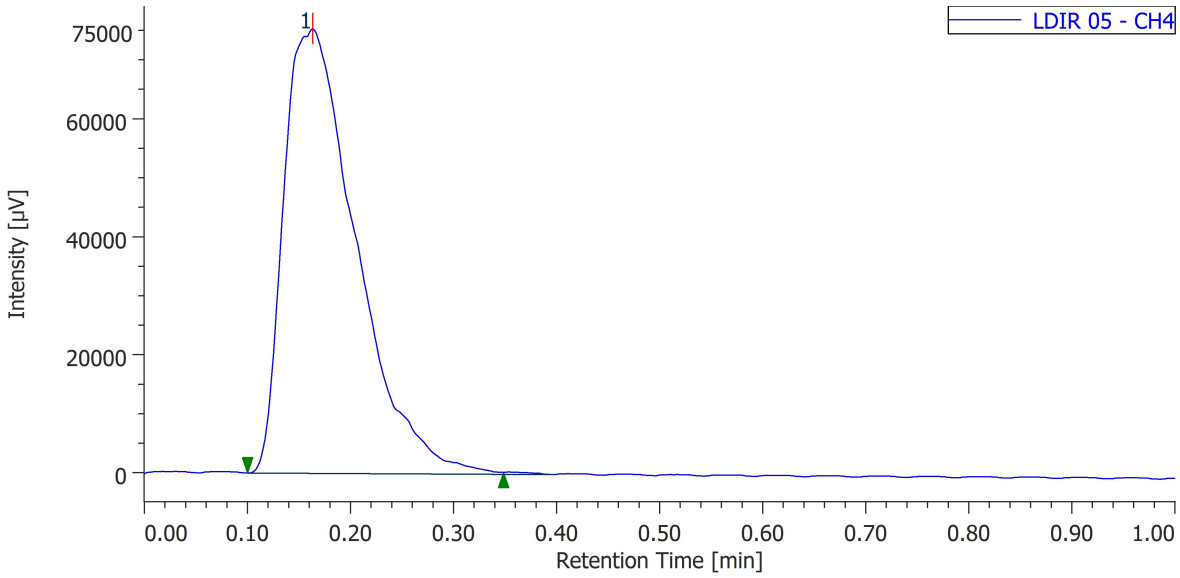

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 17:11:56
Description	
HPLC System Name	BBA HPLC 03 RI
Injection Date	05/02/2026 17:09:39
Volume	10.0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	OQ_IR
Control Method	OQ RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	100 [msec]
Peak Method	IR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.163	368602	75365	100.000	100.000	N/A	25	N/A	1.687	

Creator QPackSA
Reviewer
Approver