
Peak Find - EDUV_003 PDA_tR1,80 D.jws

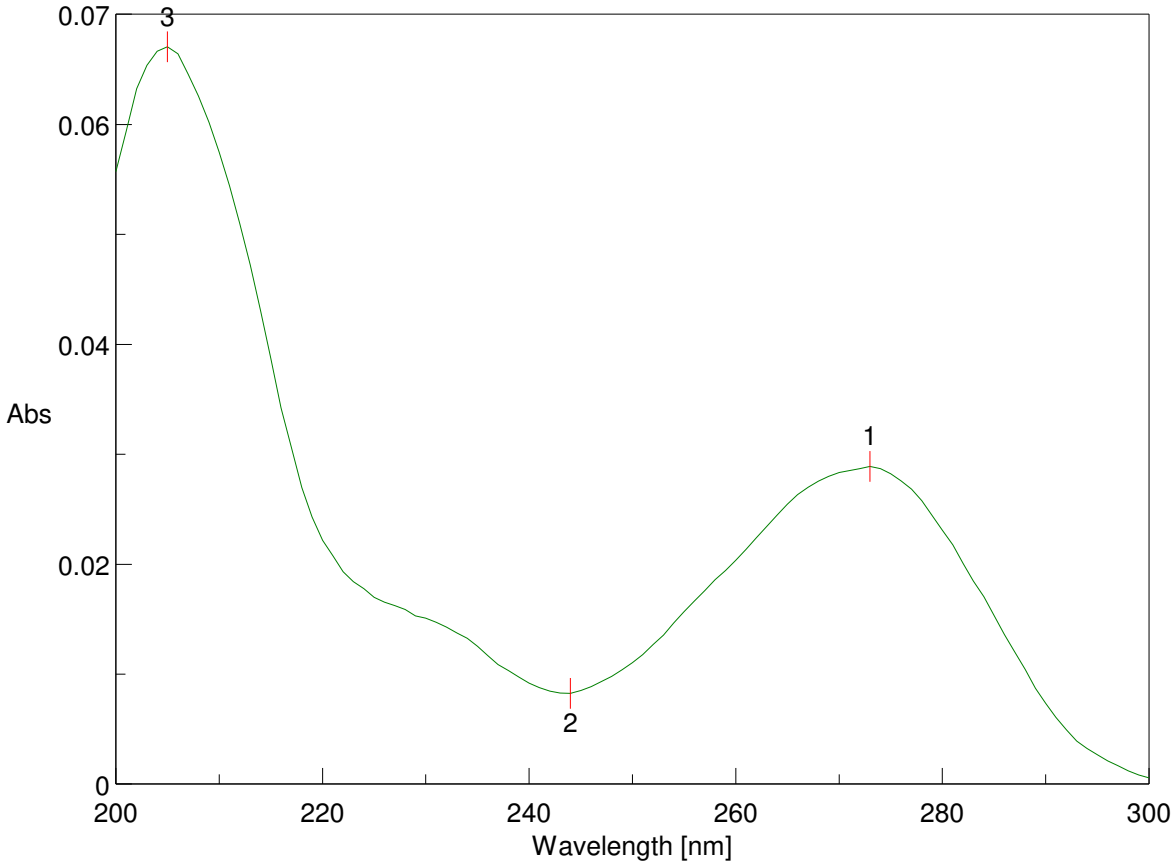

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	22/02/2021 16:12

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.028875	2	244	0.008234
3	205	0.067037			

Chromatogram

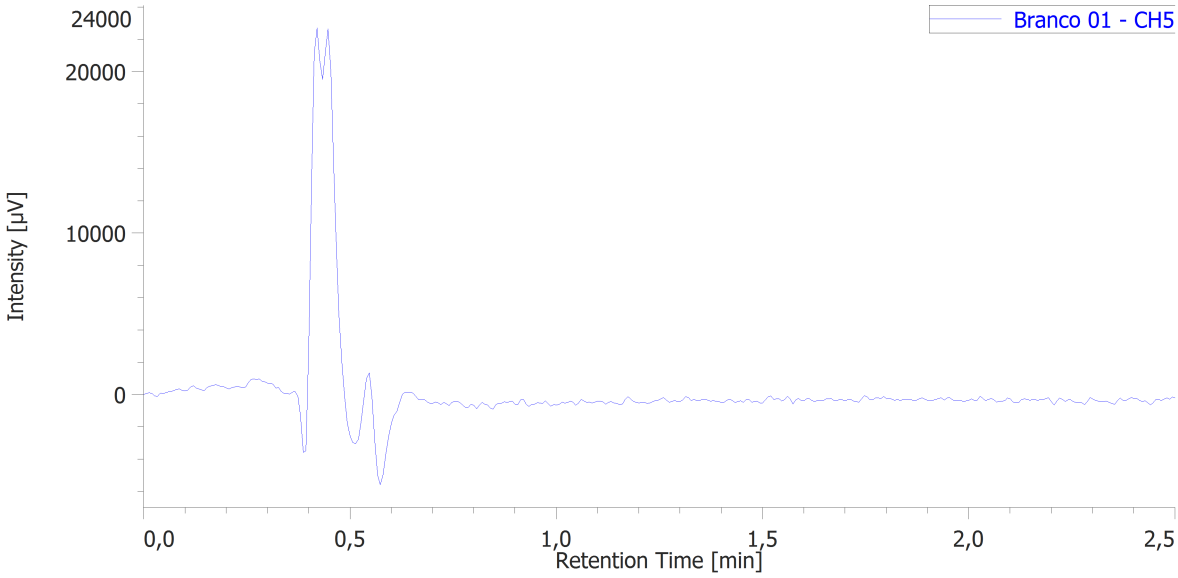


Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:55:53
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 16:57:55
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

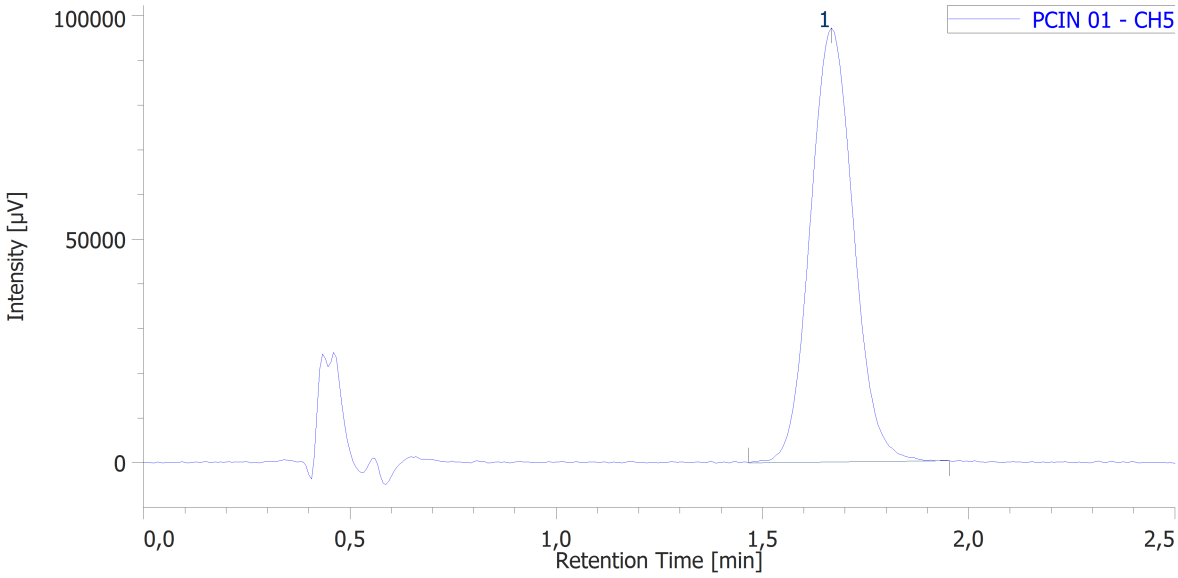

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:55:55
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:02:11
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,667	705740	97039	100,000	100,000	N/A	1211	N/A	1,081	

Creator QPackSA
Reviewer
Approver

Chromatogram

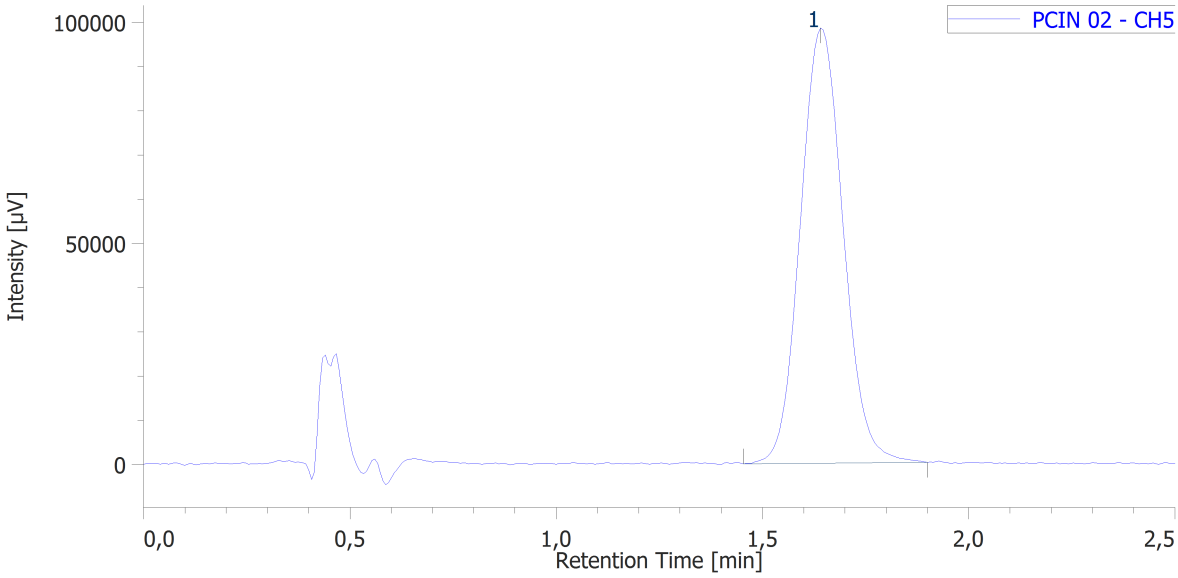

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:55:57
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:06:28
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,640	708666	98367	100,000	100,000	N/A	1199	N/A	1,103	

Creator QPackSA
Reviewer
Approver

Chromatogram

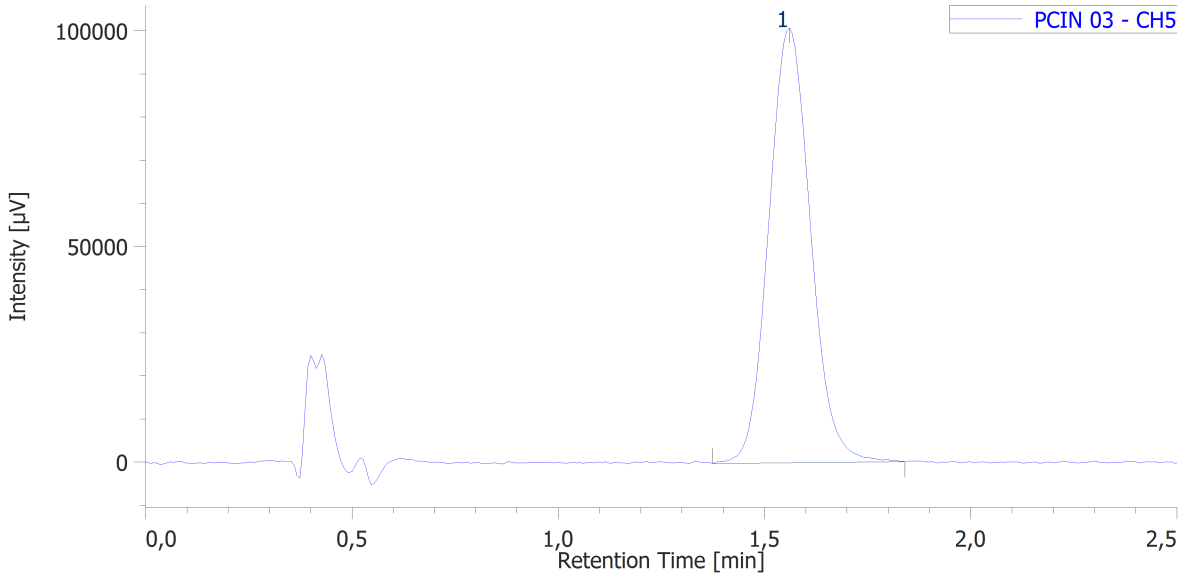

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:55:58
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:10:43
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,560	709482	100754	100,000	100,000	N/A	1141	N/A	1,090	

Creator QPackSA
Reviewer
Approver

Chromatogram

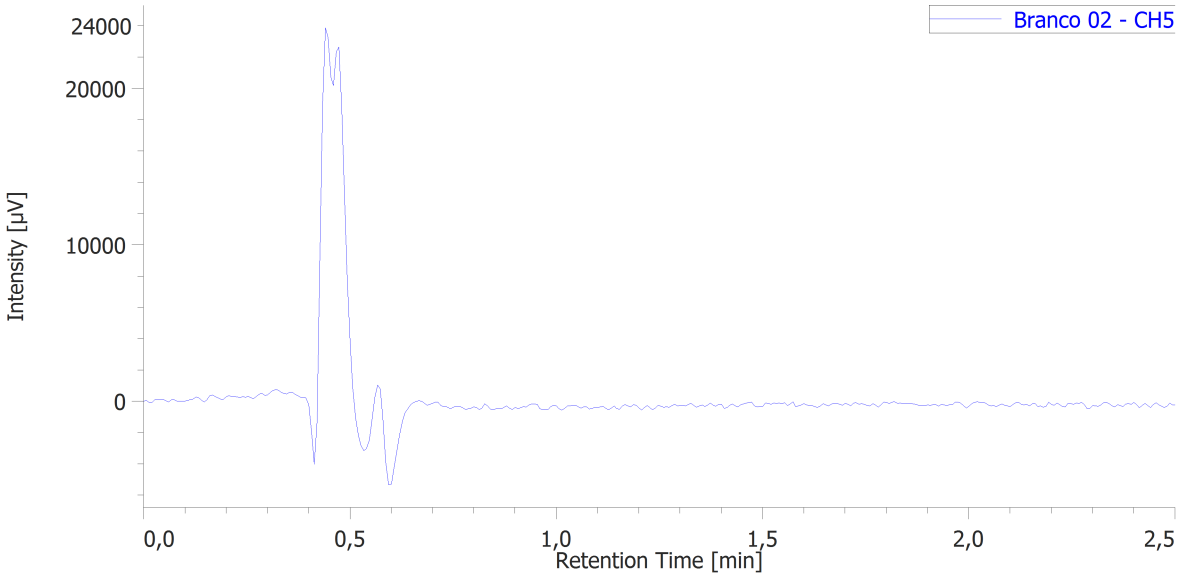


Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:55:59
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:14:54
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

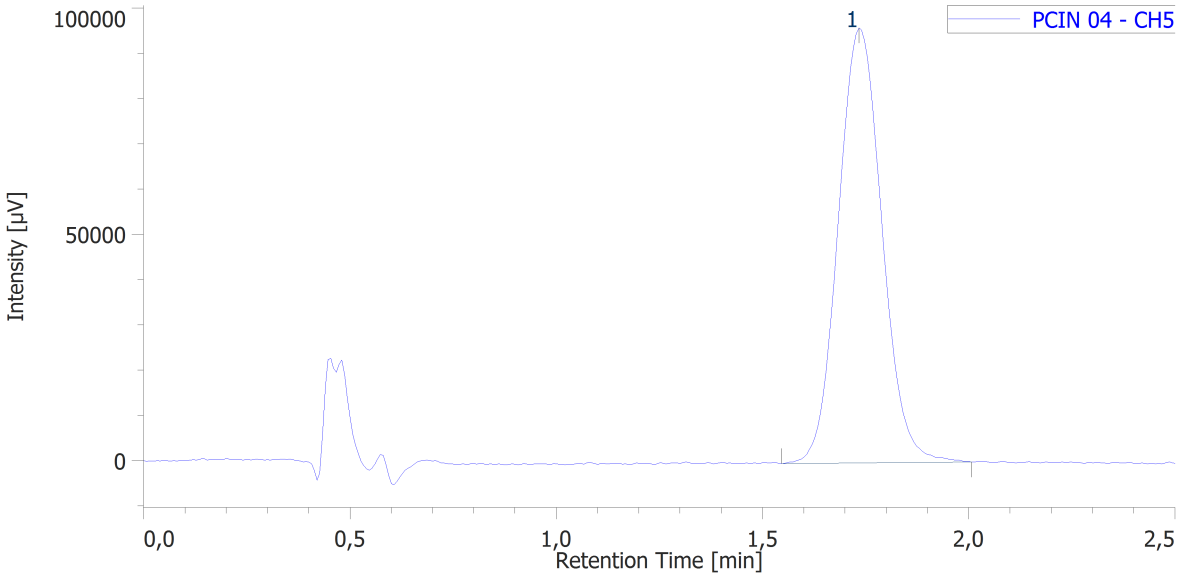

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:01
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:19:09
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,733	707654	96052	100,000	100,000	N/A	1286	N/A	1,093	

Creator QPackSA
Reviewer
Approver

Chromatogram

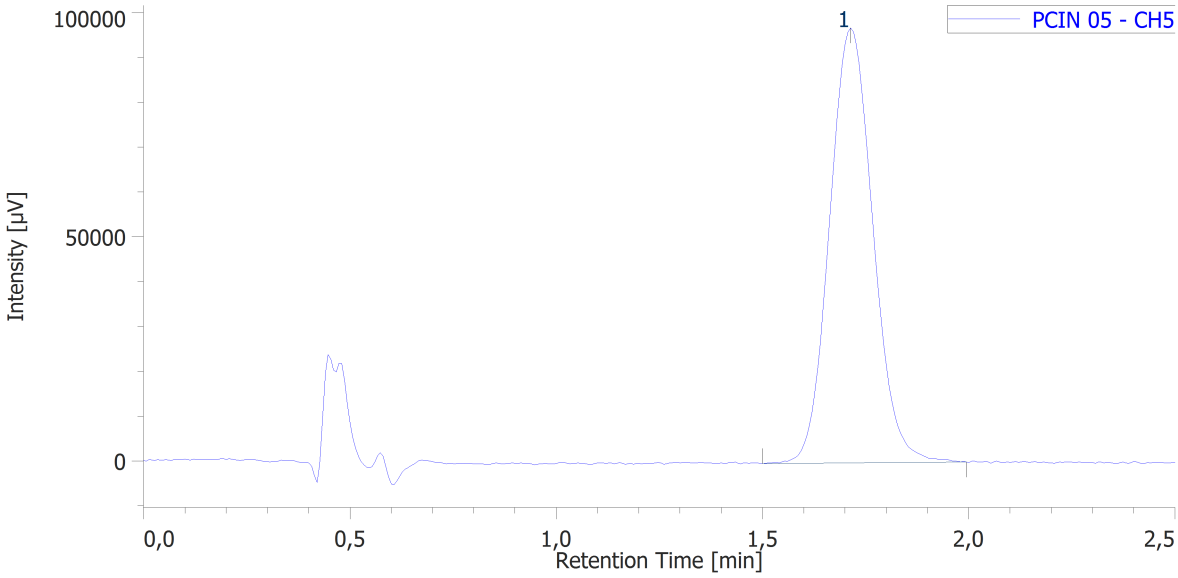

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:02
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:23:26
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,713	708755	96962	100,000	100,000	N/A	1269	N/A	1,088	

Creator QPackSA
Reviewer
Approver

Chromatogram

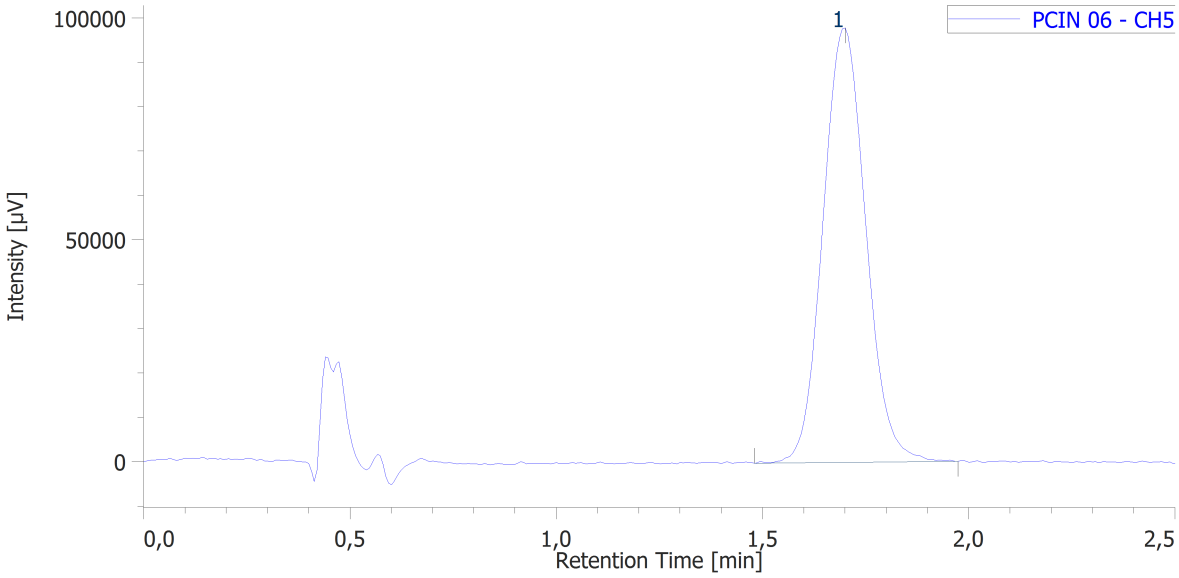

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:03
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:27:44
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,700	707166	97815	100,000	100,000	N/A	1285	N/A	1,059	

Creator QPackSA
Reviewer
Approver

Chromatogram

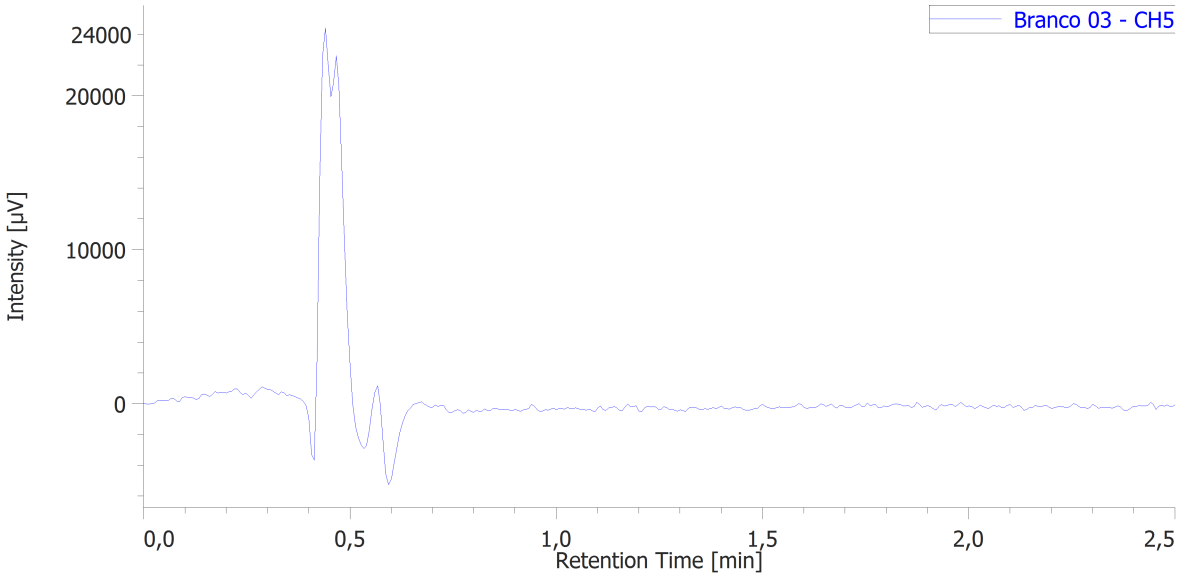


Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:05
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 17:31:56
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

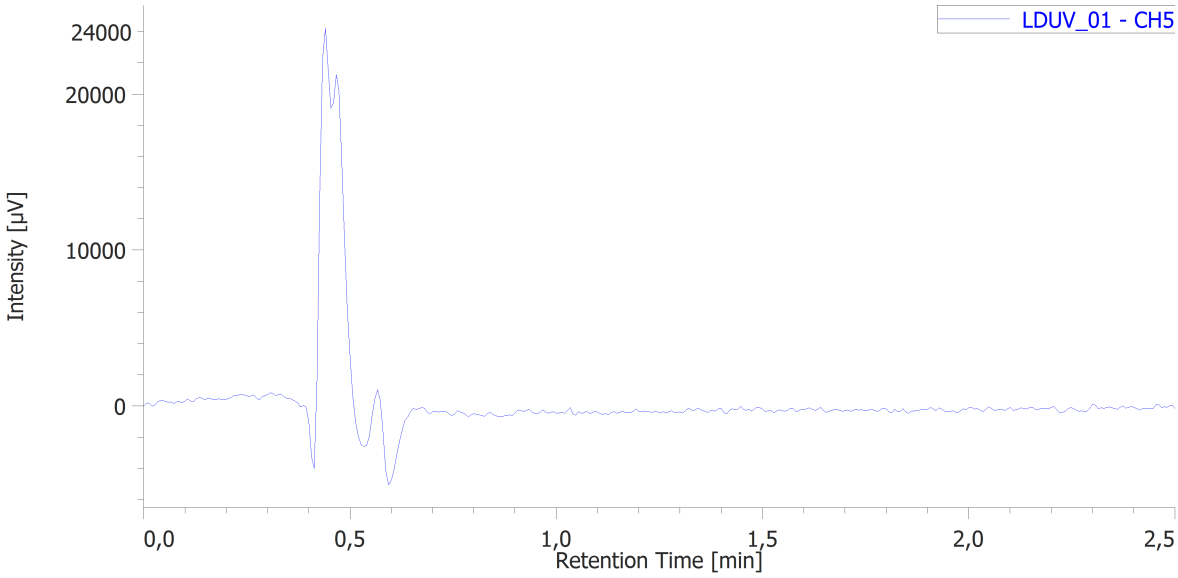


Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:06
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:14:24
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

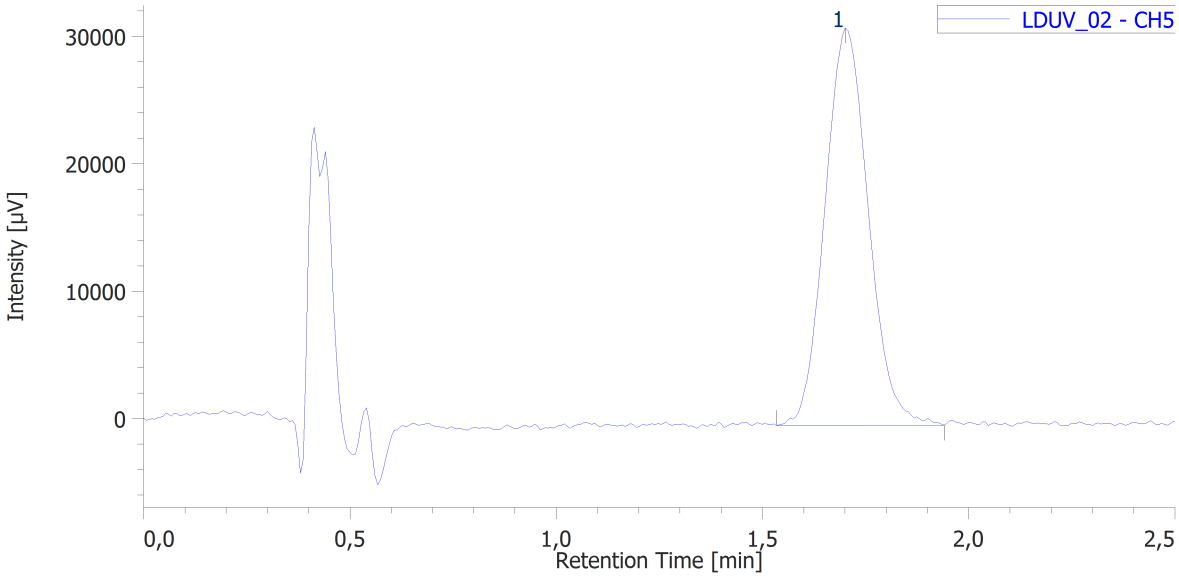

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:07
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:18:37
Volume	10,00 [µL]
Sample #	32
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,700	227226	31170	100,000	100,000	N/A	1261	N/A	1,123	

Creator QPackSA
Reviewer
Approver

Chromatogram

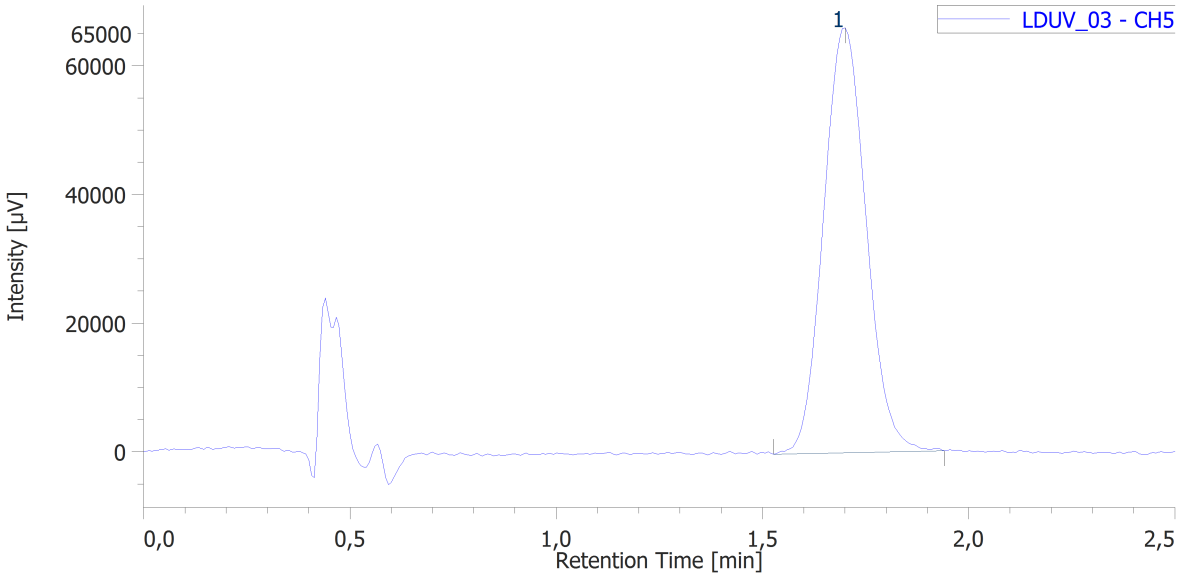

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:09
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:22:52
Volume	10,00 [µL]
Sample #	33
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,700	474127	65980	100,000	100,000	N/A	1285	N/A	1,071	

Creator QPackSA
Reviewer
Approver

Chromatogram

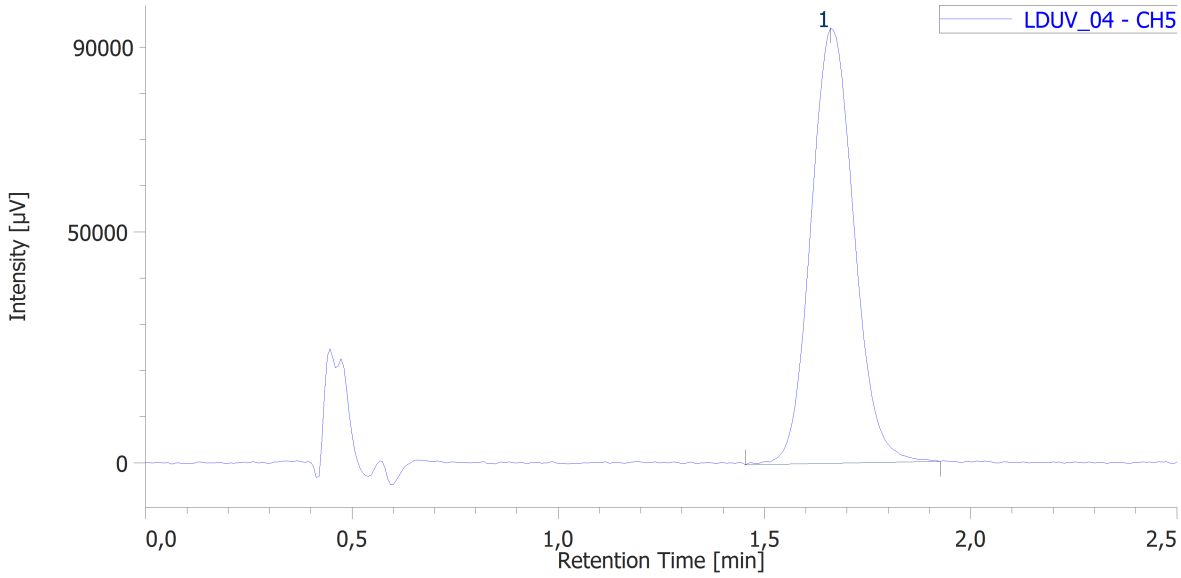

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:10
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:27:05
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,660	682846	94199	100,000	100,000	N/A	1221	N/A	1,126	

Creator QPackSA
Reviewer
Approver

Chromatogram

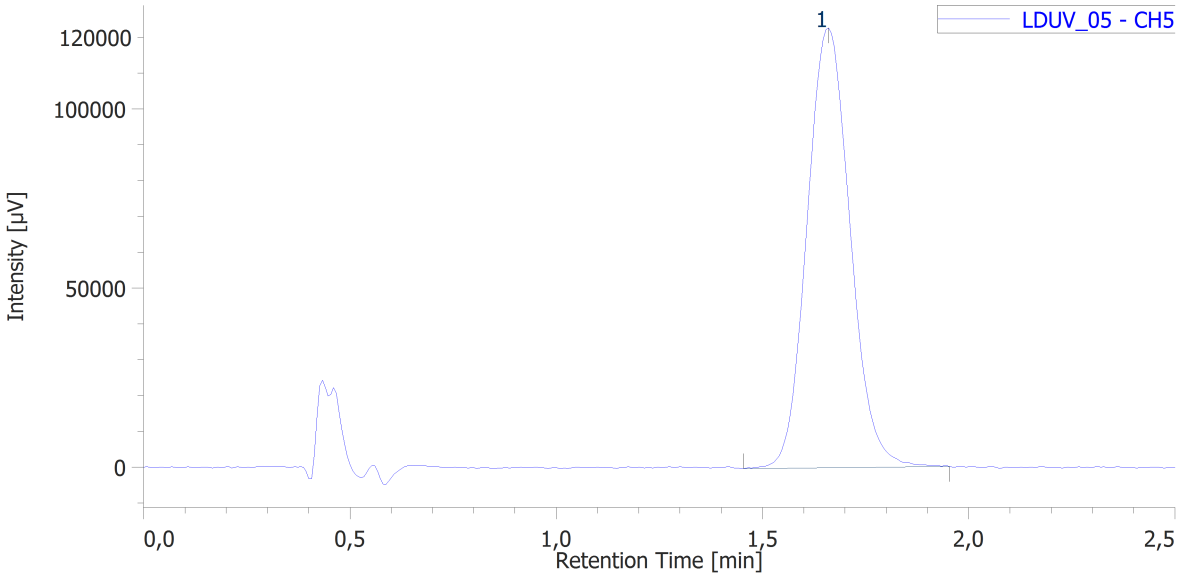

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:12
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:31:20
Volume	10,00 [µL]
Sample #	35
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,660	892609	122718	100,000	100,000	N/A	1203	N/A	1,083	

Creator QPackSA
Reviewer
Approver

Chromatogram

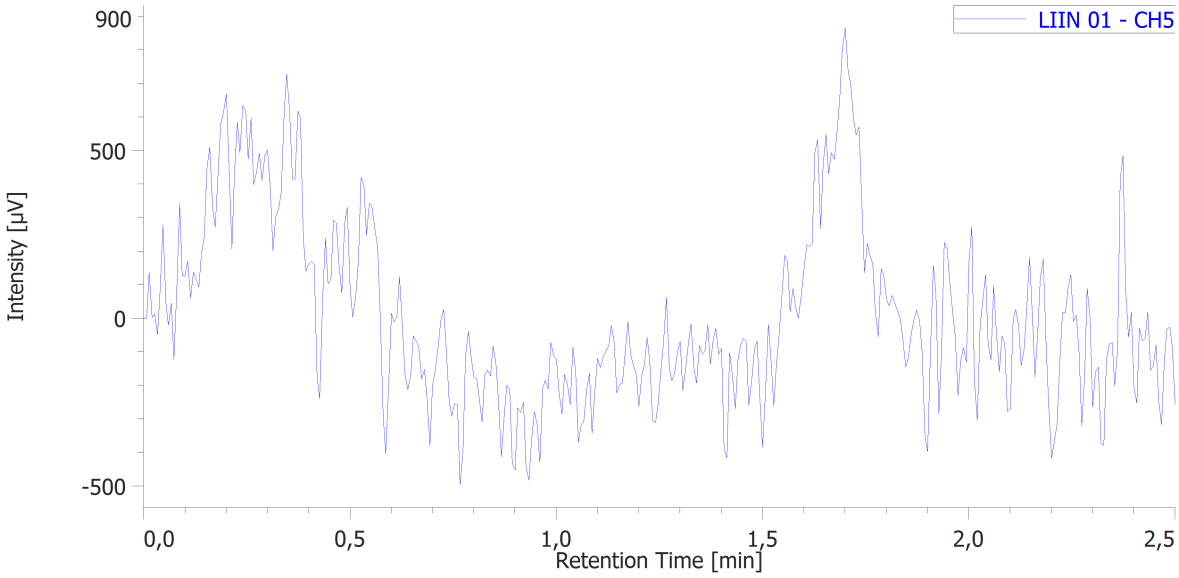


Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:13
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 18:56:38
Volume	0,10 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

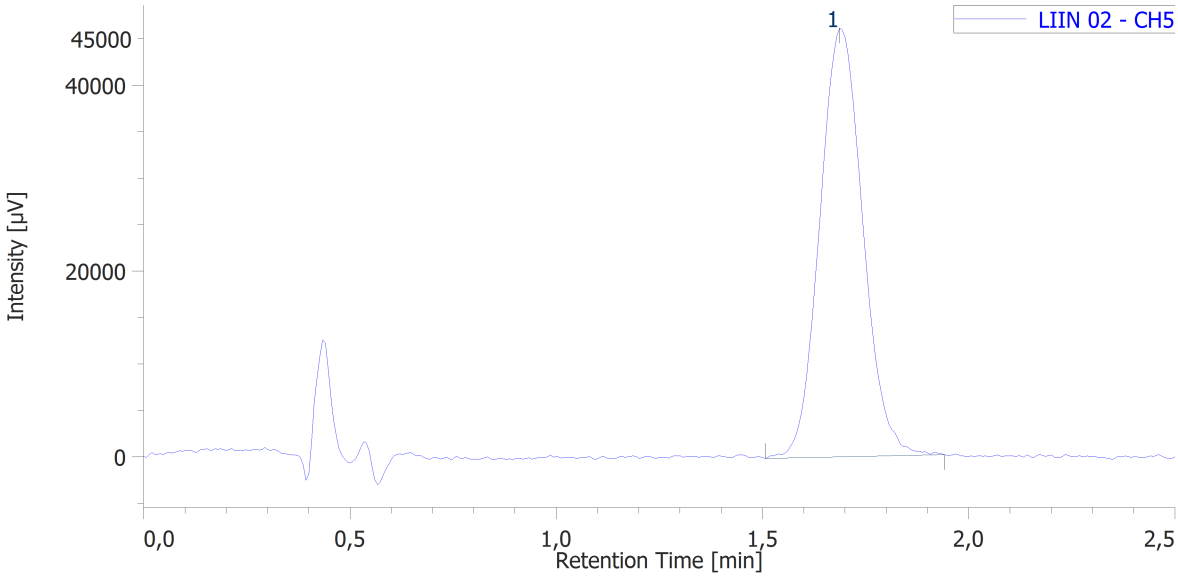

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:14
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 19:00:51
Volume	5,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,687	334568	46121	100,000	100,000	N/A	1253	N/A	1,135	

Creator QPackSA
Reviewer
Approver

Chromatogram

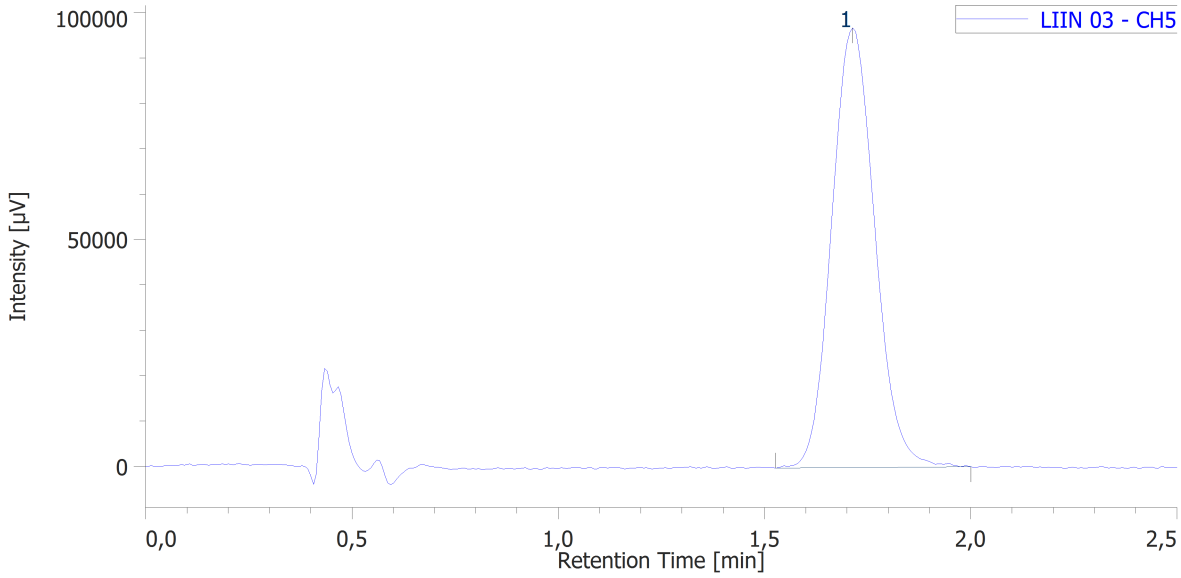

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:16
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 19:05:06
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,713	703798	96766	100,000	100,000	N/A	1279	N/A	1,102	

Creator QPackSA
Reviewer
Approver

Chromatogram

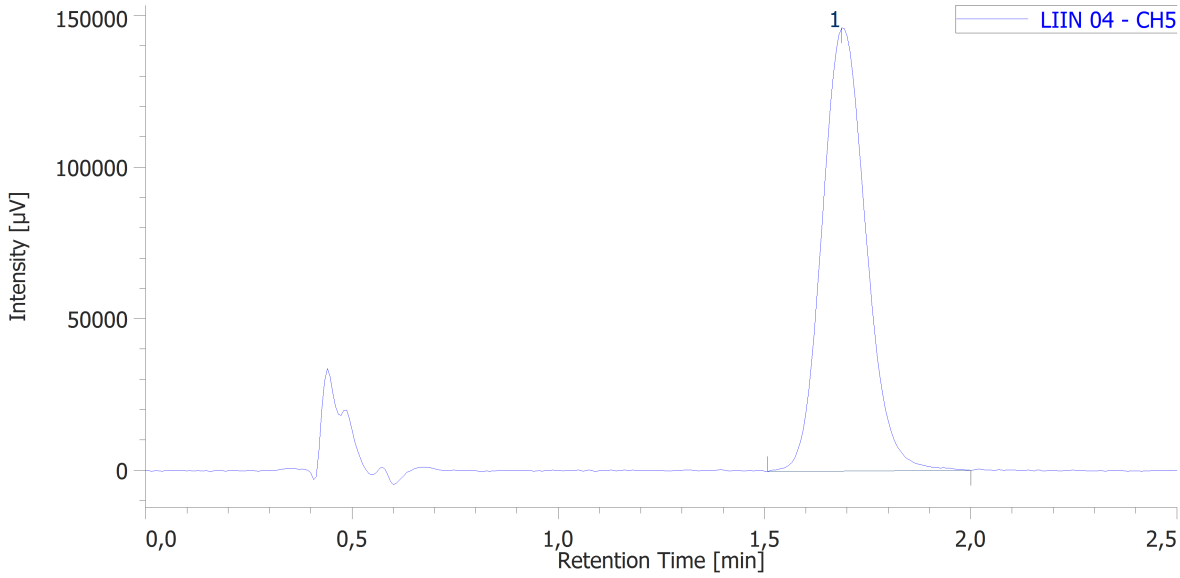

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:17
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 19:09:26
Volume	15,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,687	1077827	146103	100,000	100,000	N/A	1216	N/A	1,154	

Creator QPackSA
Reviewer
Approver

Chromatogram

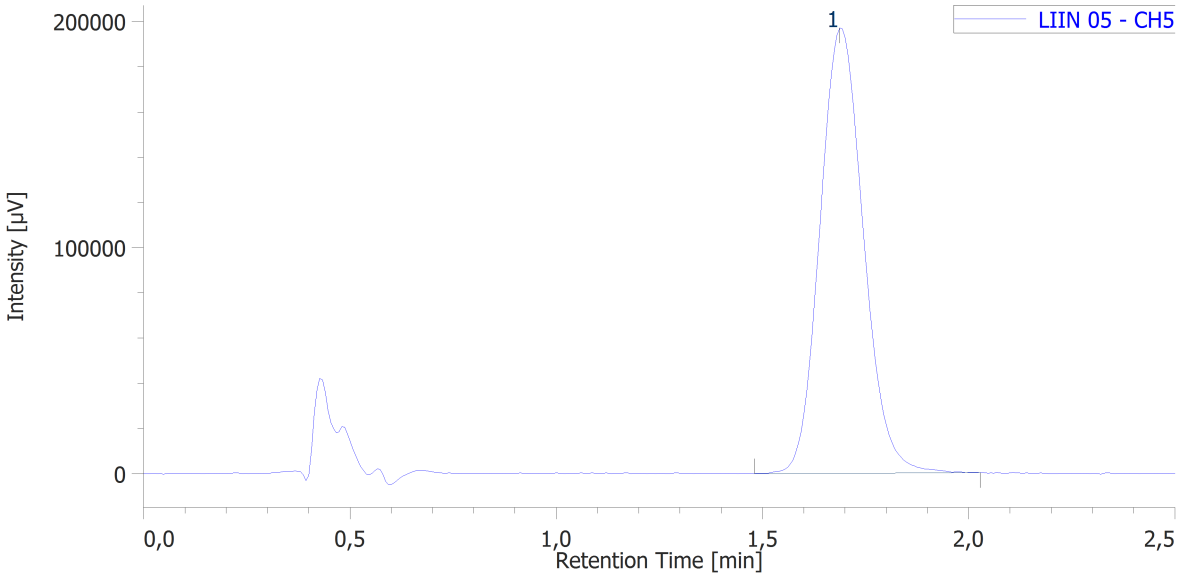

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 08:56:18
Description	
HPLC System Name	HPL 08_PDA
Injection Date	22/02/2021 19:13:50
Volume	20,00 [µL]
Sample #	36
Project Name	Qualificação HPL 08
Acquisition Time	2,5 [min]
Acquisition Sequence	QPack
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,687	1444131	196838	100,000	100,000	N/A	1231	N/A	1,149	

Creator QPackSA
Reviewer
Approver

Chromatogram

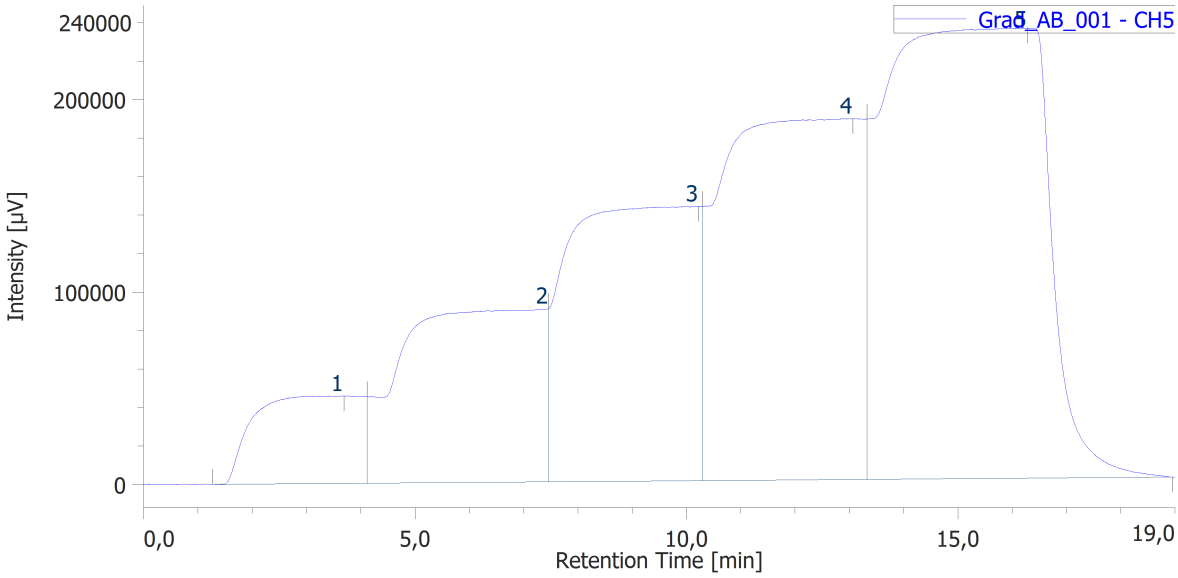

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 11:50:57
Description	
HPLC System Name	HPL 08_PDA
Injection Date	23/02/2021 10:12:05
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação HPL 08
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Grad_AB
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad_AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,687	6087758	45417	4,846	6,497	N/A	N/A	N/A	N/A	
2	40%	5	7,460	16040438	90055	12,770	12,883	N/A	N/A	N/A	N/A	
3	60%	5	10,223	23065224	142437	18,362	20,376	N/A	N/A	N/A	N/A	
4	80%	5	13,063	32616677	187363	25,966	26,803	N/A	N/A	N/A	N/A	
5	100%	5	16,273	47803780	233770	38,056	33,441	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

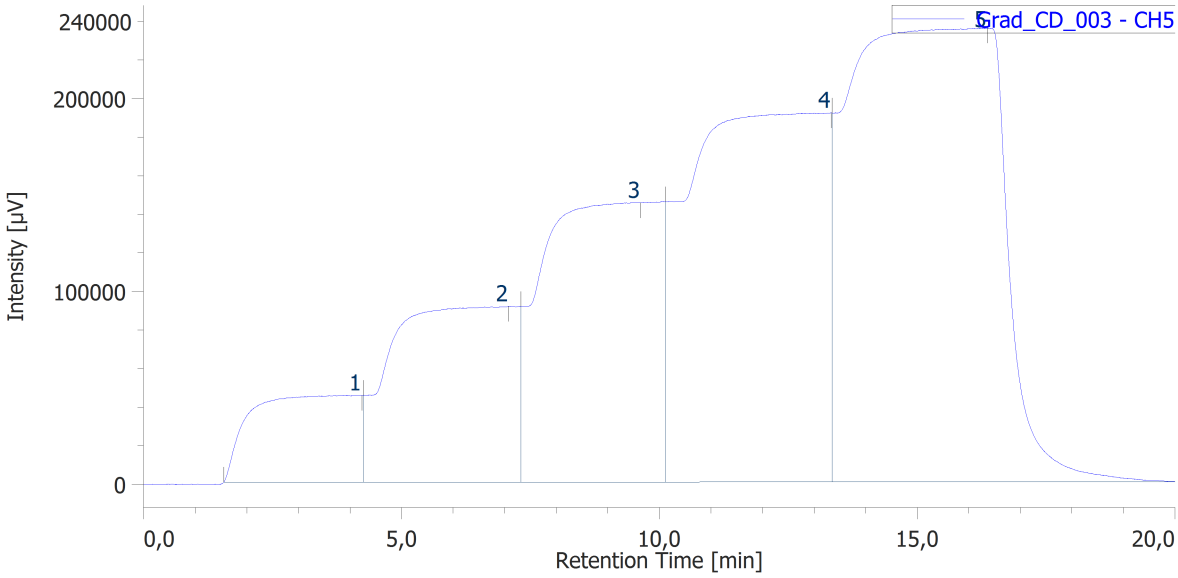

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2021 11:47:39
Description	
HPLC System Name	HPL 08_PDA
Injection Date	23/02/2021 11:10:02
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação HPL 08
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Grad_AB
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad_CD_003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,230	6346860	45005	4,985	6,364	N/A	N/A	N/A	N/A	
2	40%	5	7,077	14987070	91045	11,771	12,874	N/A	N/A	N/A	N/A	
3	60%	5	9,637	22694772	144637	17,825	20,452	N/A	N/A	N/A	N/A	
4	80%	5	13,330	34897127	191311	27,409	27,052	N/A	N/A	N/A	N/A	
5	100%	5	16,353	48394839	235187	38,010	33,257	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver