
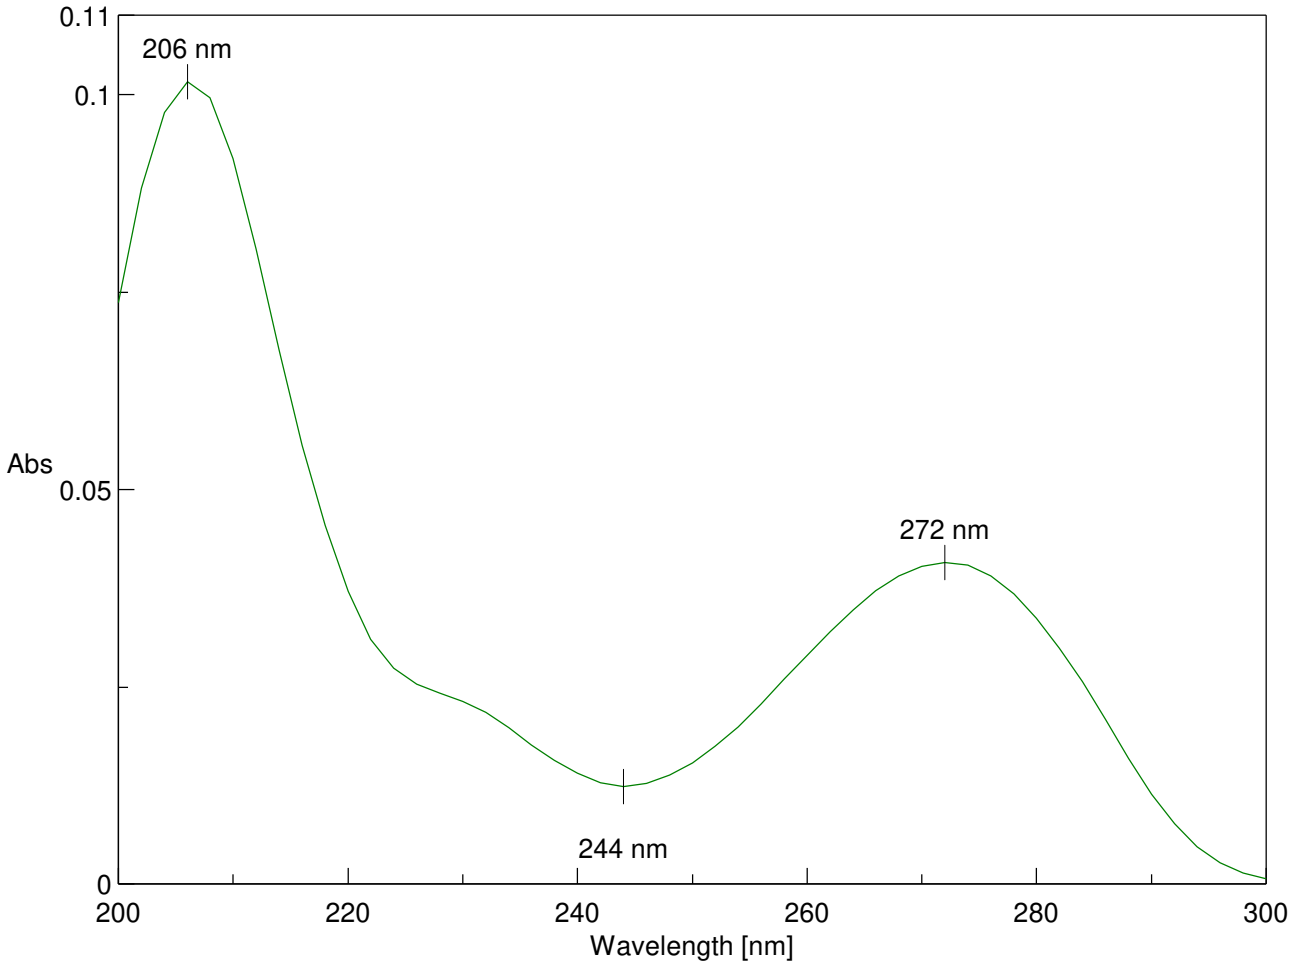


[Comments]	
User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	06/02/2023 13:29

[Measurement Information]	
Model Name	X-LC 3110MD
Serial No.	A002661329
ROM version	V1.05.01

[Detailed Information]	
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	2 nm
Data points	51

Chromatogram

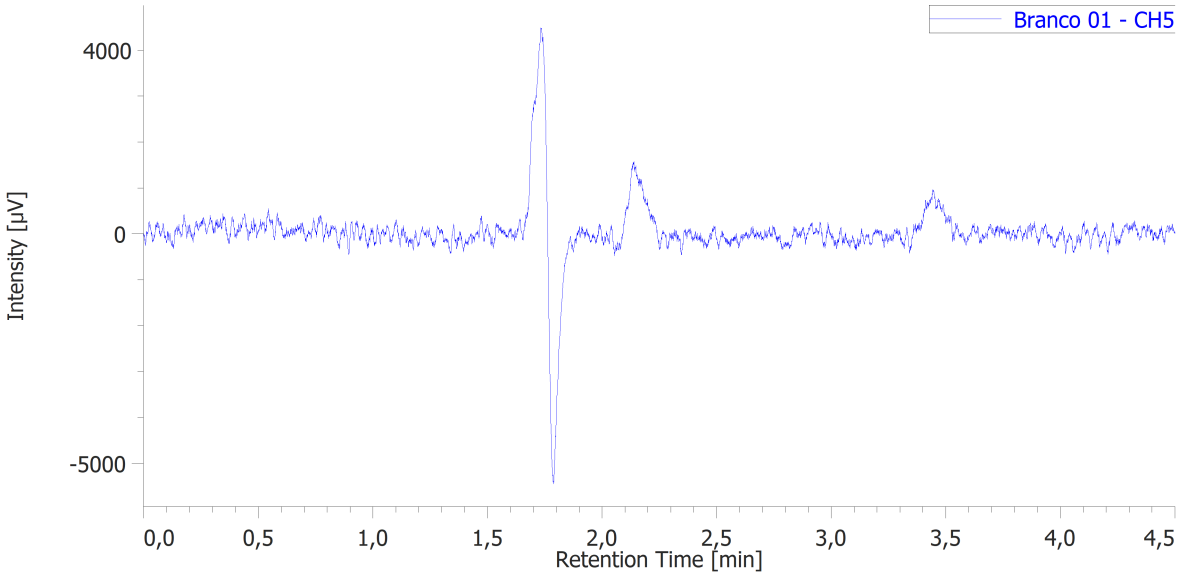


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:37
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:26:59
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

Creator QPackSA
Reviewer
Approver

Chromatogram

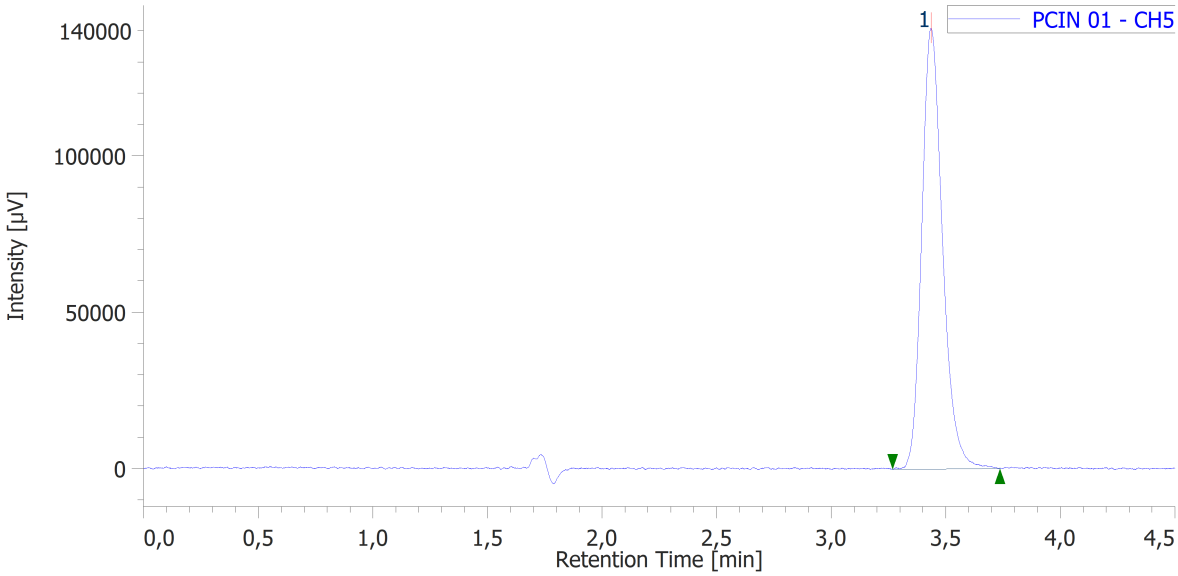

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:41
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:32:11
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,434	888588	140956	100,000	100,000	N/A	7281	N/A	1,245	

Creator QPackSA
Reviewer
Approver

Chromatogram

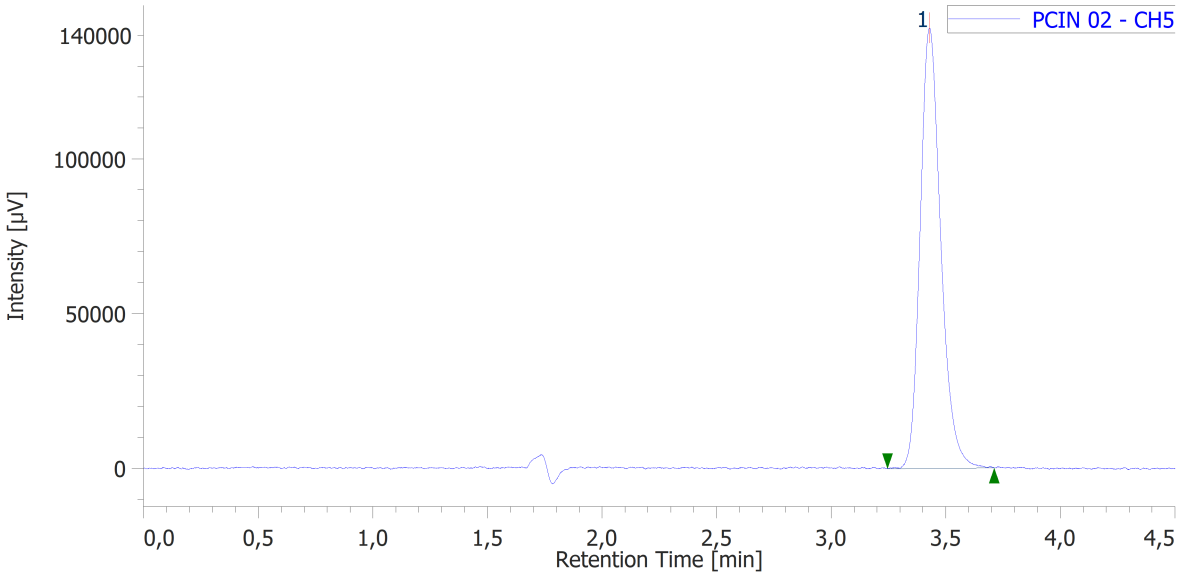

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:41
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:37:24
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,428	891180	142347	100,000	100,000	N/A	7296	N/A	1,226	

Creator QPackSA
Reviewer
Approver

Chromatogram

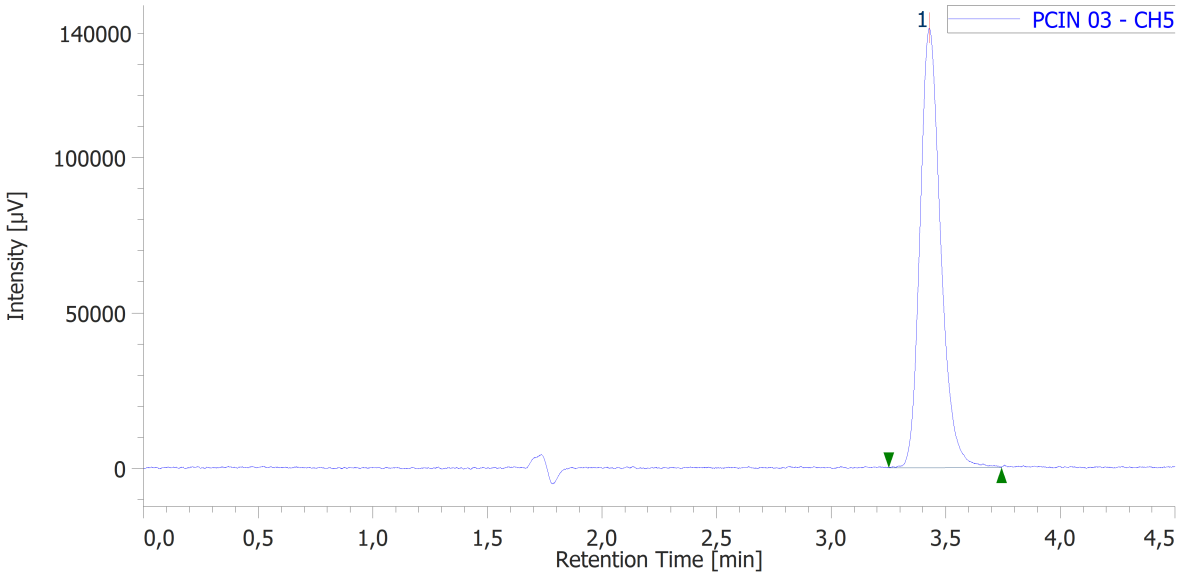

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:41
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:42:36
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,427	887398	141438	100,000	100,000	N/A	7319	N/A	1,239	

Creator QPackSA
Reviewer
Approver

Chromatogram

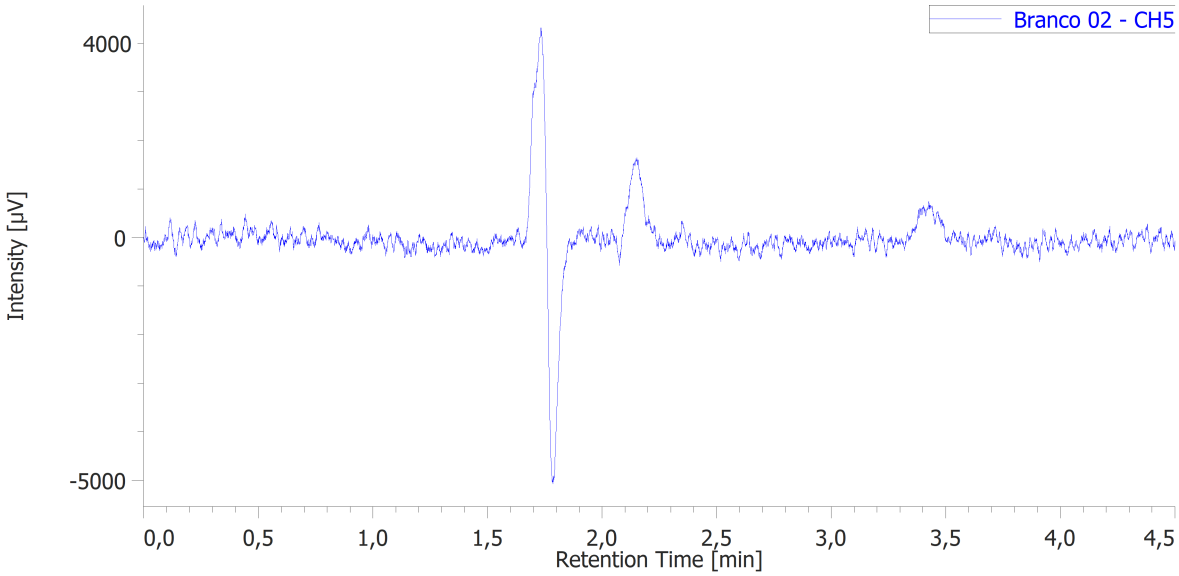


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:47:46
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

Creator QPackSA
Reviewer
Approver

Chromatogram

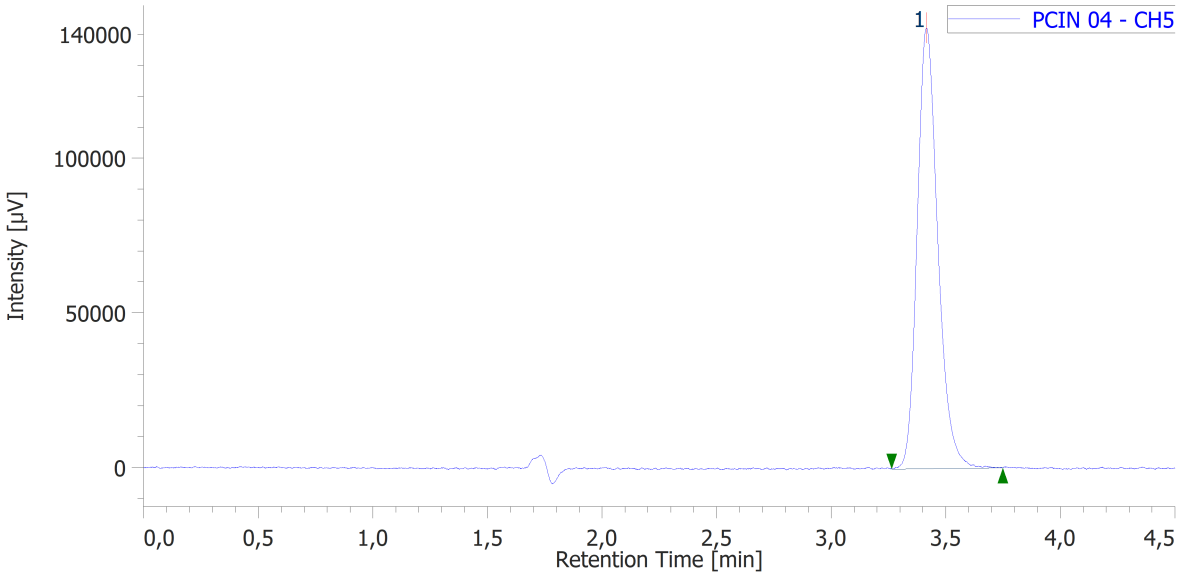

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:52:59
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,414	891380	142318	100,000	100,000	N/A	7263	N/A	1,246	

Creator QPackSA
Reviewer
Approver

Chromatogram

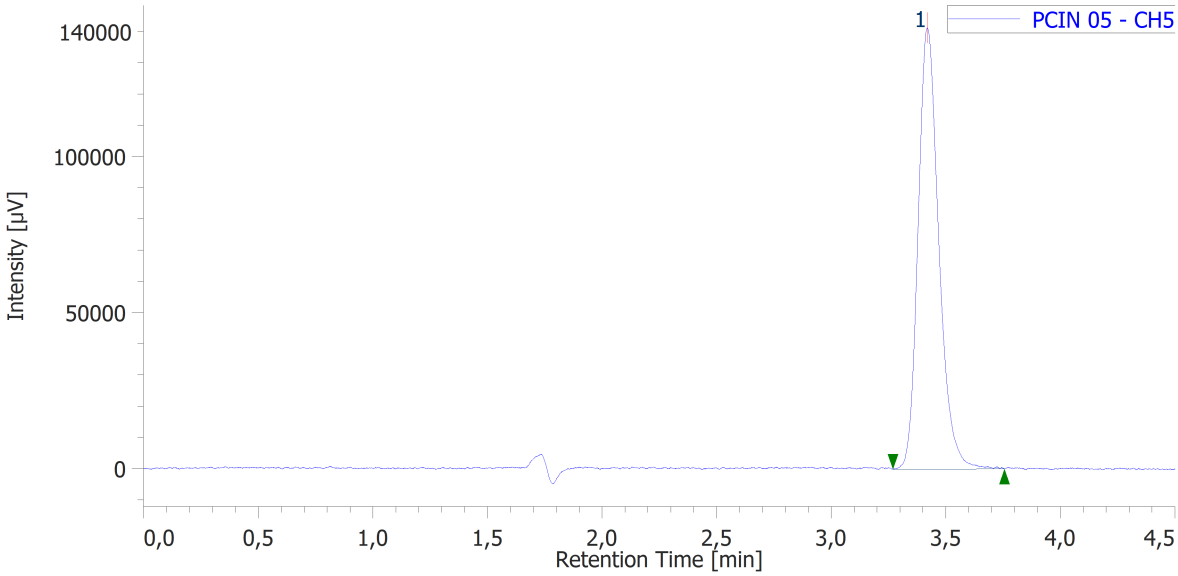

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 14:58:10
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,418	888697	141286	100,000	100,000	N/A	7269	N/A	1,245	

Creator QPackSA
Reviewer
Approver

Chromatogram

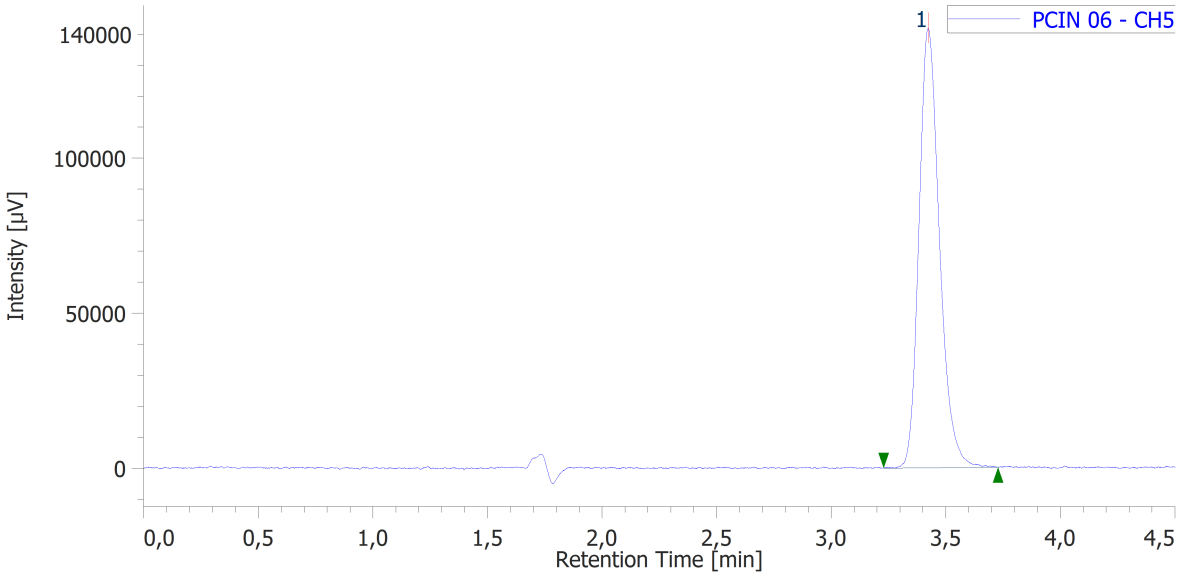

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:03:22
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,422	884456	141843	100,000	100,000	N/A	7384	N/A	1,235	

Creator QPackSA
Reviewer
Approver

Chromatogram

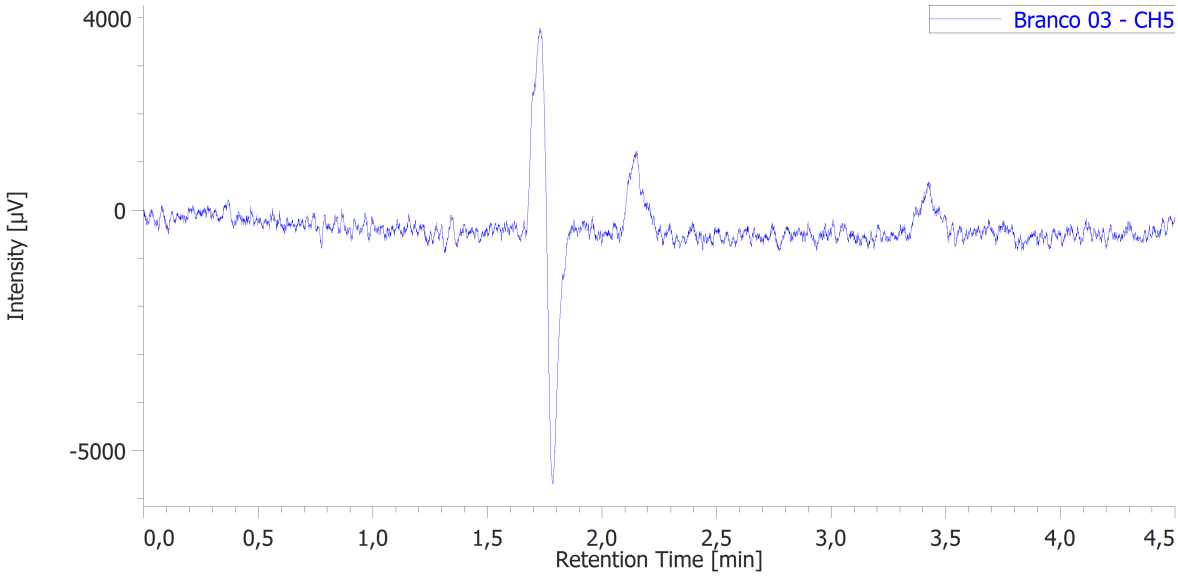


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:24:43
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:08:32
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	PCIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

Creator QPackSA
Reviewer
Approver

Chromatogram

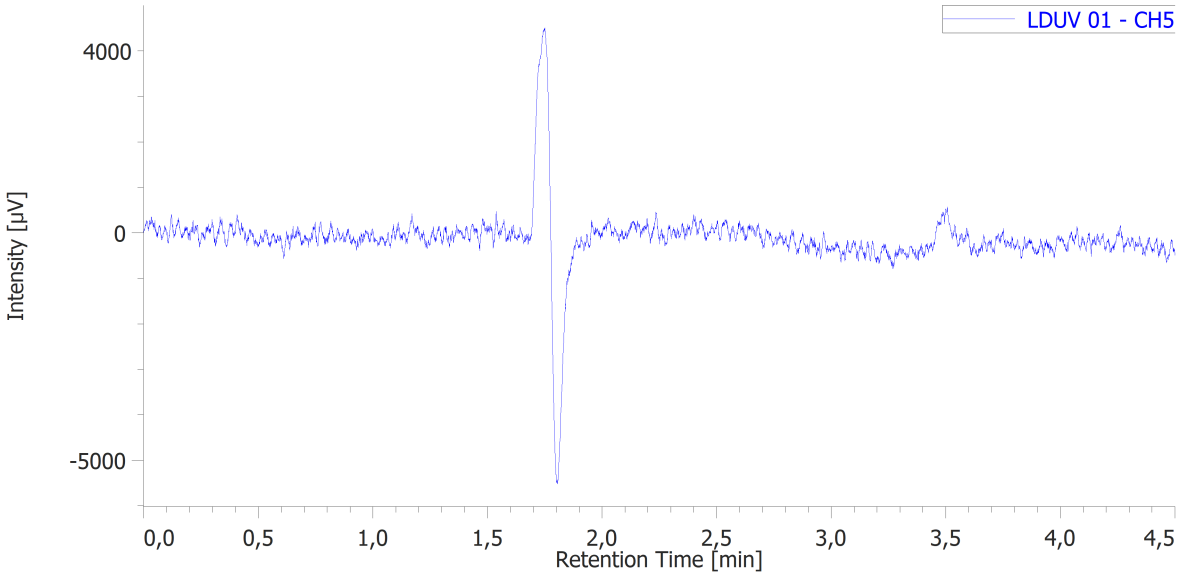


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:45:28
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:40:57
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

Creator
Reviewer
Approver

Chromatogram

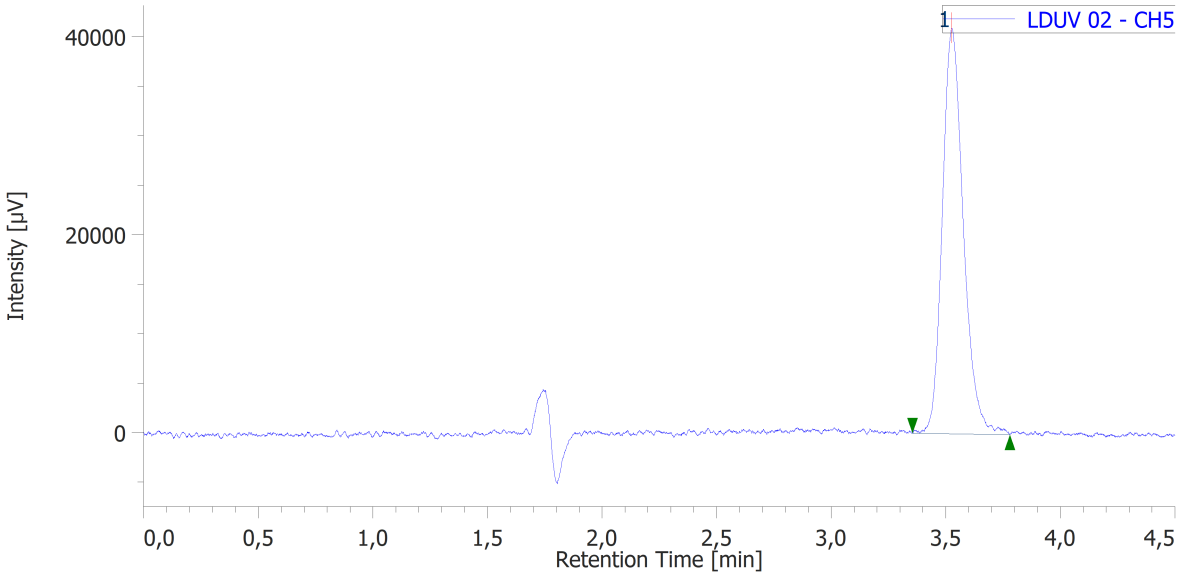

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:50:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:46:09
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,523	262194	41018	100,000	100,000	N/A	7521	N/A	1,250	

Creator QPackSA
Reviewer
Approver

Chromatogram

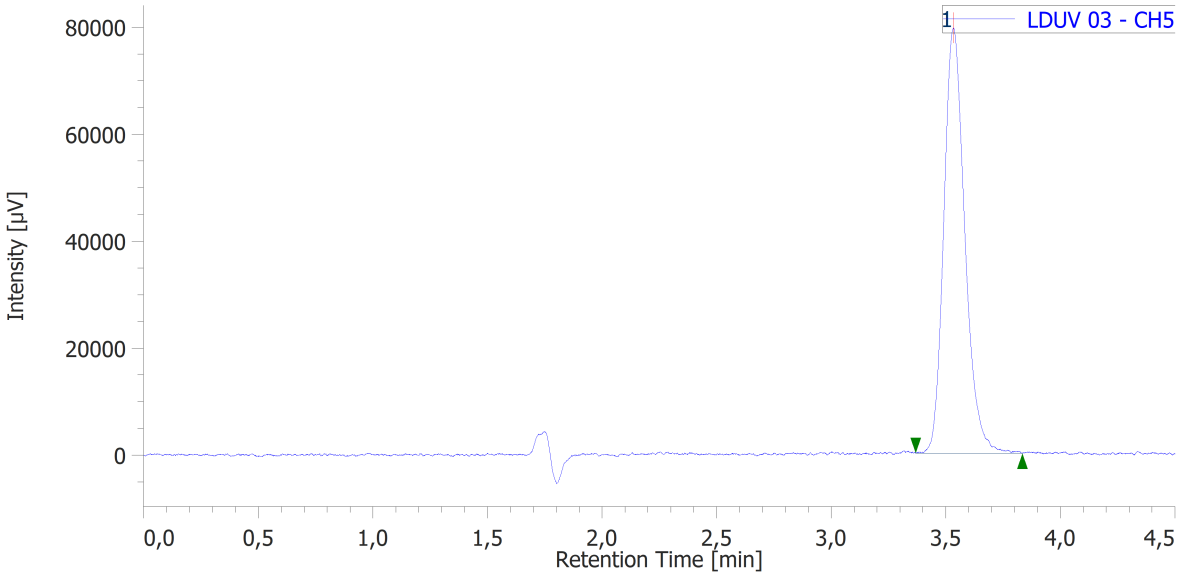

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 15:55:54
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:51:22
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,533	508734	79451	100,000	100,000	N/A	7437	N/A	1,213	

Creator QPackSA
Reviewer
Approver

Chromatogram

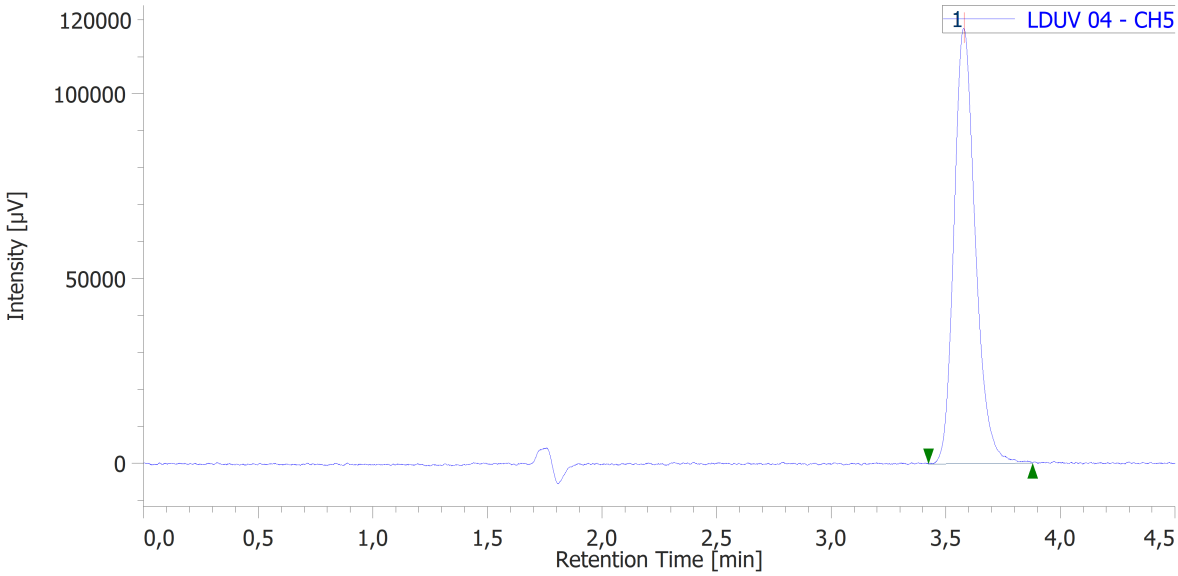

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:01:10
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 15:56:37
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,578	764386	117923	100,000	100,000	N/A	7442	N/A	1,210	

Creator QPackSA
Reviewer
Approver

Chromatogram

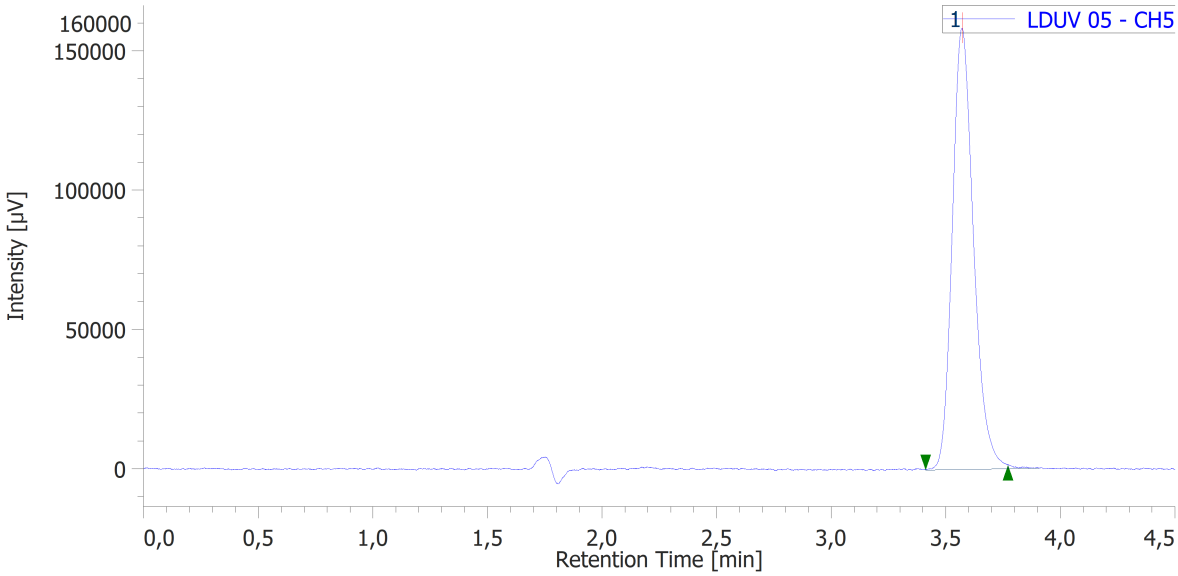

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:06:24
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:01:52
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LDUV HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,571	1020599	158335	100,000	100,000	N/A	7450	N/A	1,209	

Creator
Reviewer
Approver

Chromatogram

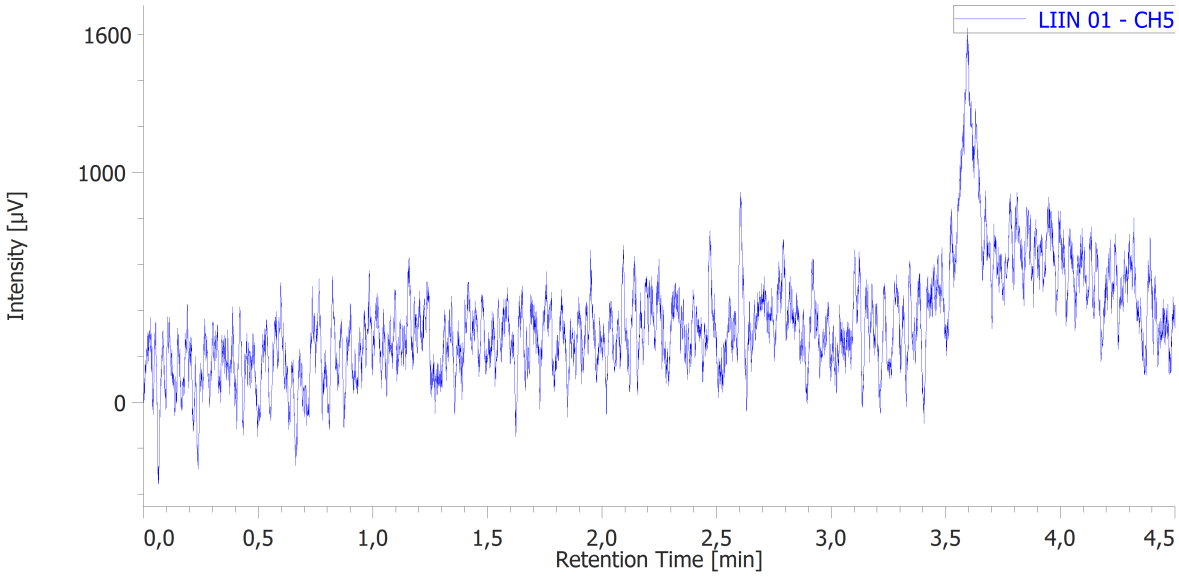


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:24:18
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:19:46
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração2

Creator
Reviewer
Approver

Chromatogram

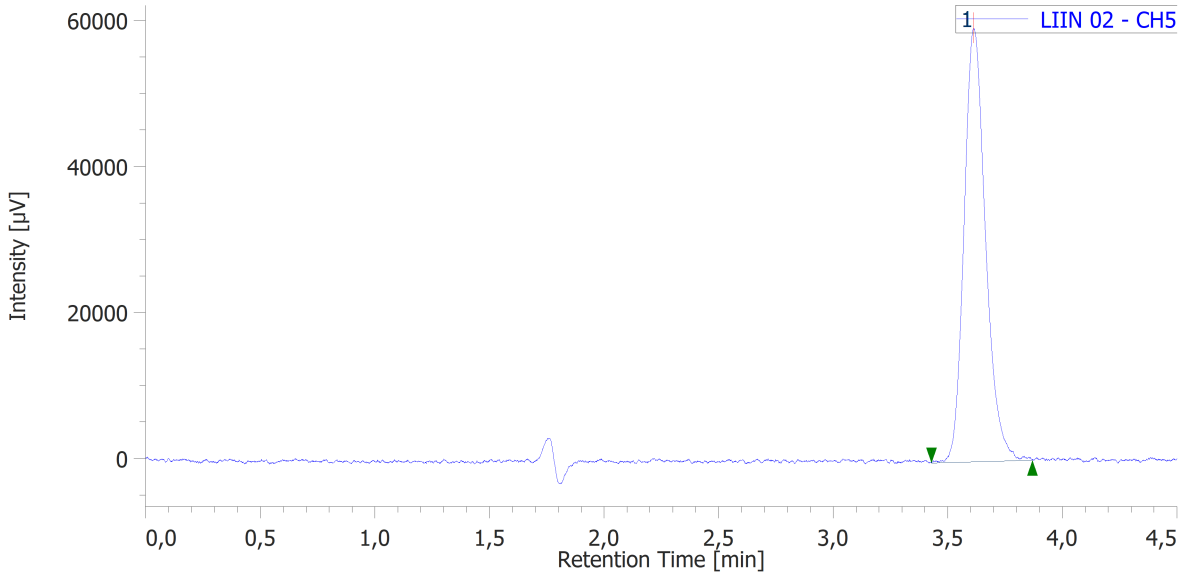

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:29:26
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:24:54
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,612	388765	59411	100,000	100,000	N/A	7442	N/A	1,226	

Creator QPackSA
Reviewer
Approver

Chromatogram

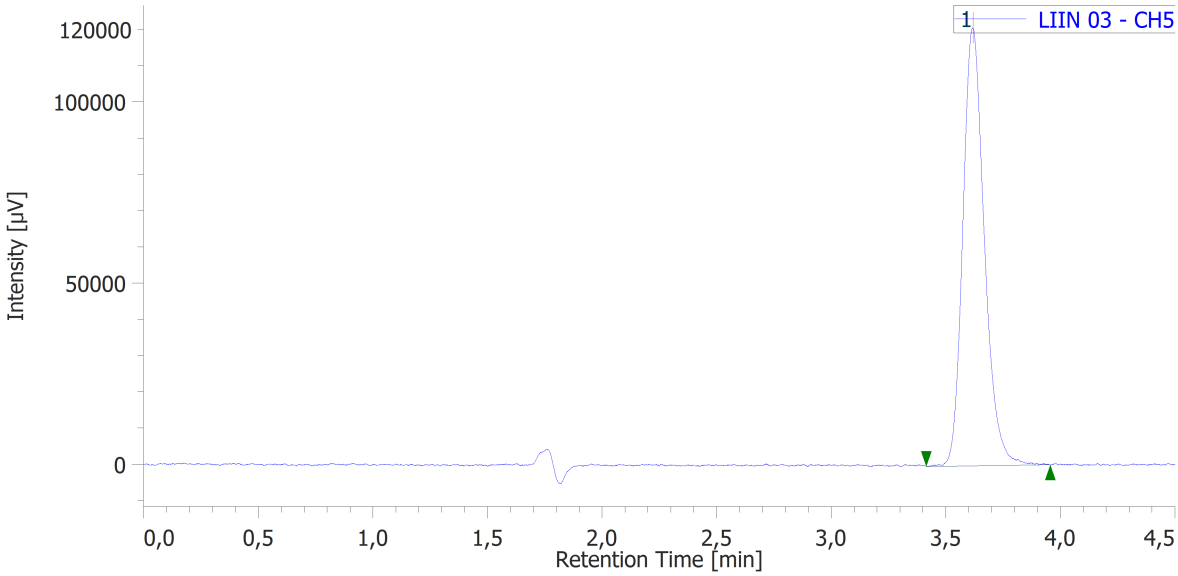

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:34:42
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:30:09
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,618	791617	120821	100,000	100,000	N/A	7428	N/A	1,201	

Creator QPackSA
Reviewer
Approver

Chromatogram

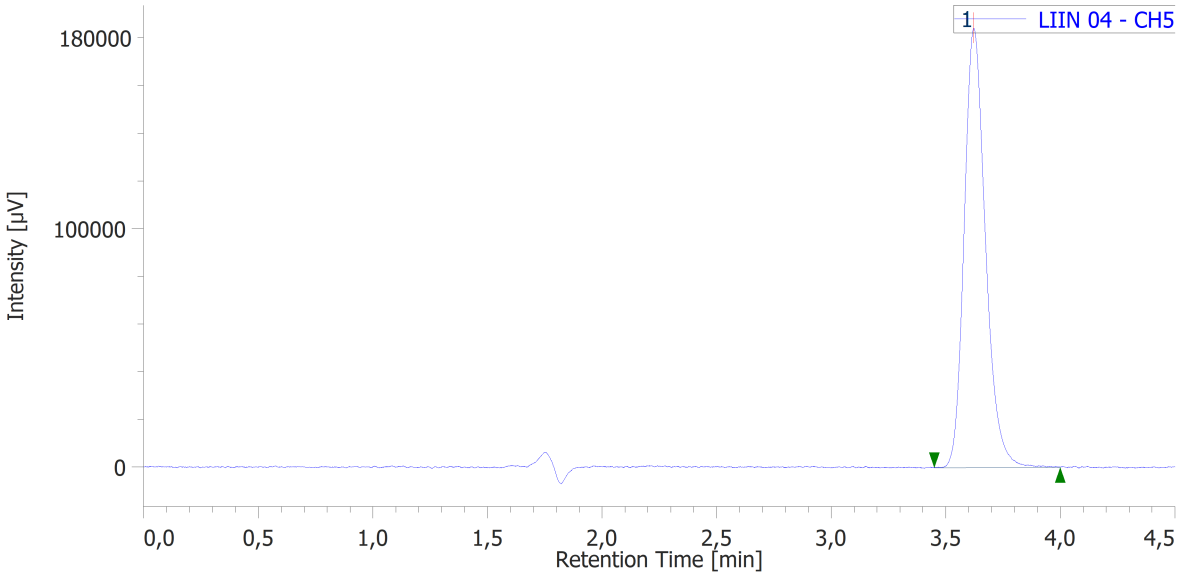

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:39:58
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:35:27
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,621	1192928	184330	100,000	100,000	N/A	7622	N/A	1,233	

Creator QPackSA
Reviewer
Approver

Chromatogram

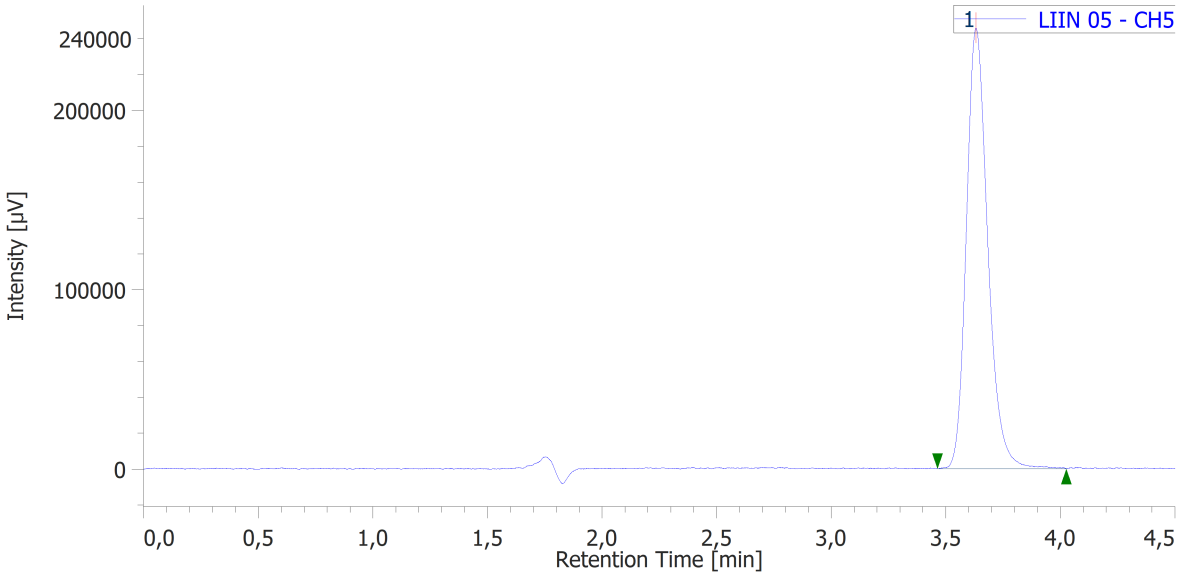

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 16:45:24
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:40:52
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação QPack
Acquisition Time	4,5 [min]
Acquisition Sequence	LIIN HP03
Control Method	QUALIFICAÇÃO
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,630	1598466	245787	100,000	100,000	N/A	7689	N/A	1,241	

Creator QPackSA
Reviewer
Approver

Chromatogram

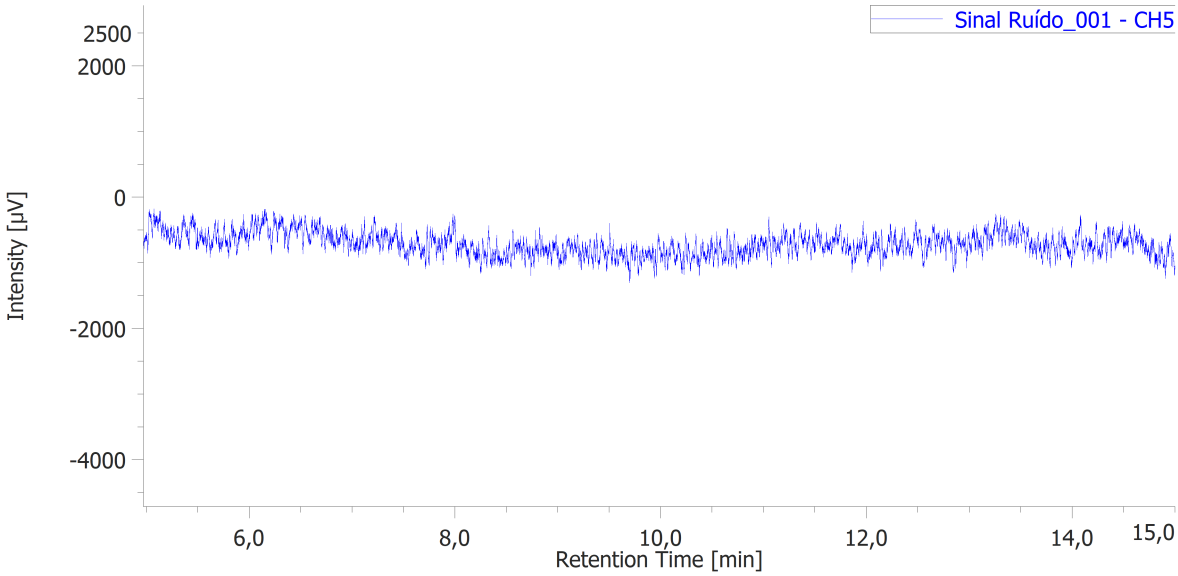

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 17:12:50
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:57:47
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação QPack
Acquisition Time	15,0 [min]
Acquisition Sequence	
Control Method	Sinal Ruído
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal Ruído_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,598	1043675	161001	100,000	100,000	N/A	7531	N/A	1,217	

Creator QPackSA
Reviewer
Approver

Chromatogram

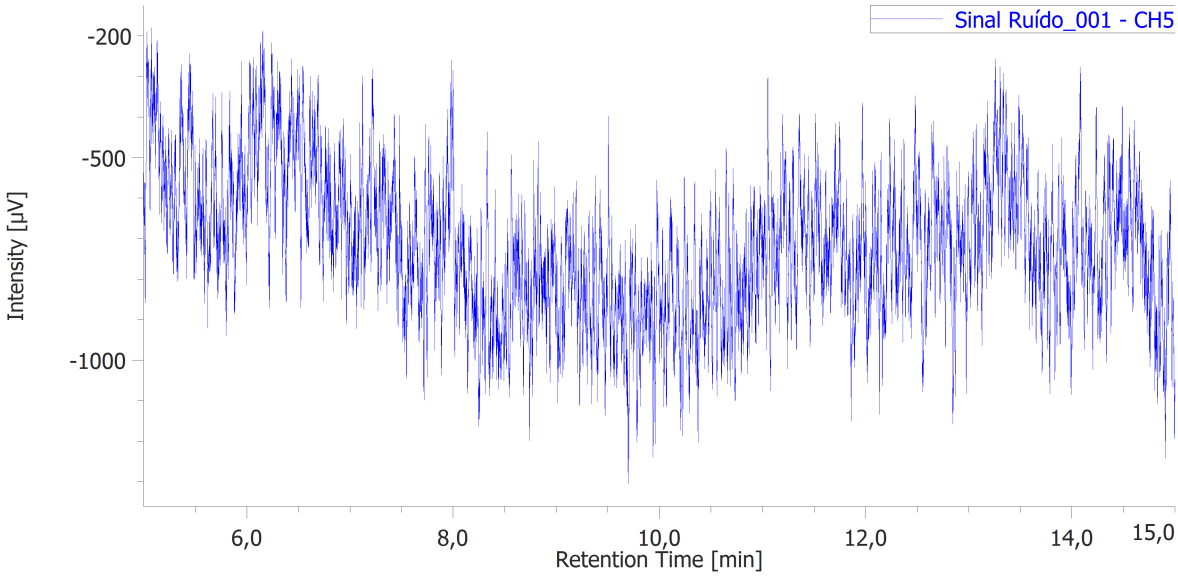

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 17:12:50
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 16:57:47
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação QPack
Acquisition Time	15,0 [min]
Acquisition Sequence	
Control Method	Sinal Ruído
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal Ruído_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,598	1043675	161001	100,000	100,000	N/A	7531	N/A	1,217	

Creator QPackSA
Reviewer
Approver

Chromatogram

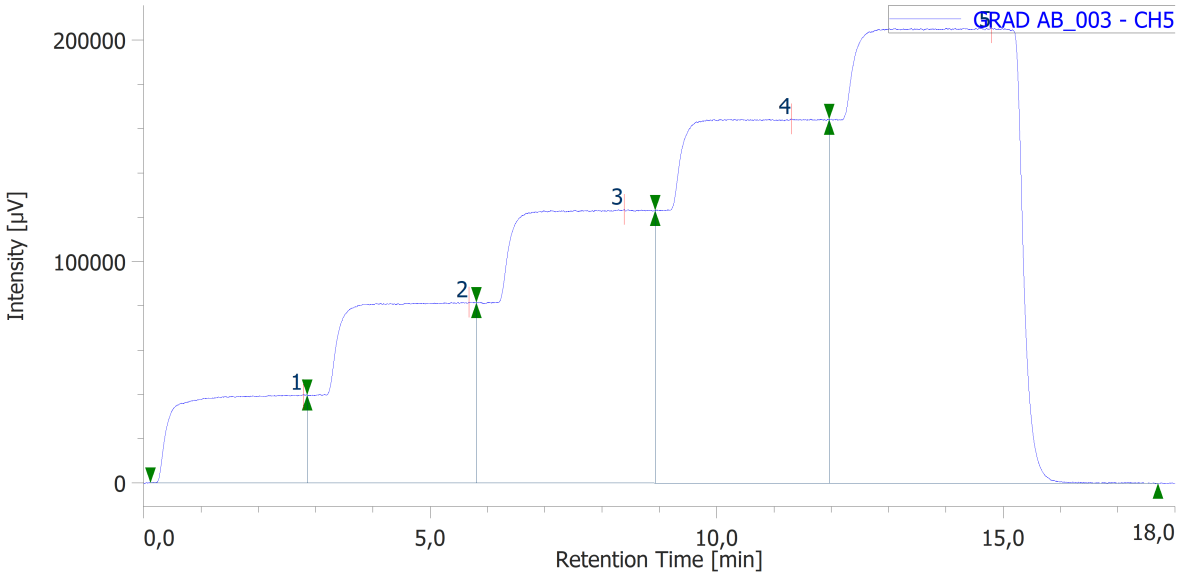

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2023 18:02:20
Description	
HPLC System Name	X-LC
Injection Date	06/02/2023 17:44:18
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação QPack
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	QUALIFICAÇÃO GRD A_B
Peak ID Table	Identificação GRBO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB_003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	2,787	5701505	39807	5,185	6,480	N/A	N/A	N/A	N/A	
2	40%	5	5,677	13021798	81550	11,843	13,274	N/A	N/A	N/A	N/A	
3	60%	5	8,383	21561037	123413	19,609	20,088	N/A	N/A	N/A	N/A	
4	80%	5	11,308	28749099	164241	26,146	26,734	N/A	N/A	N/A	N/A	
5	100%	5	14,798	40921468	205336	37,217	33,423	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Peak Find - EDFL_003 FPEm_tR0,58 D.jws

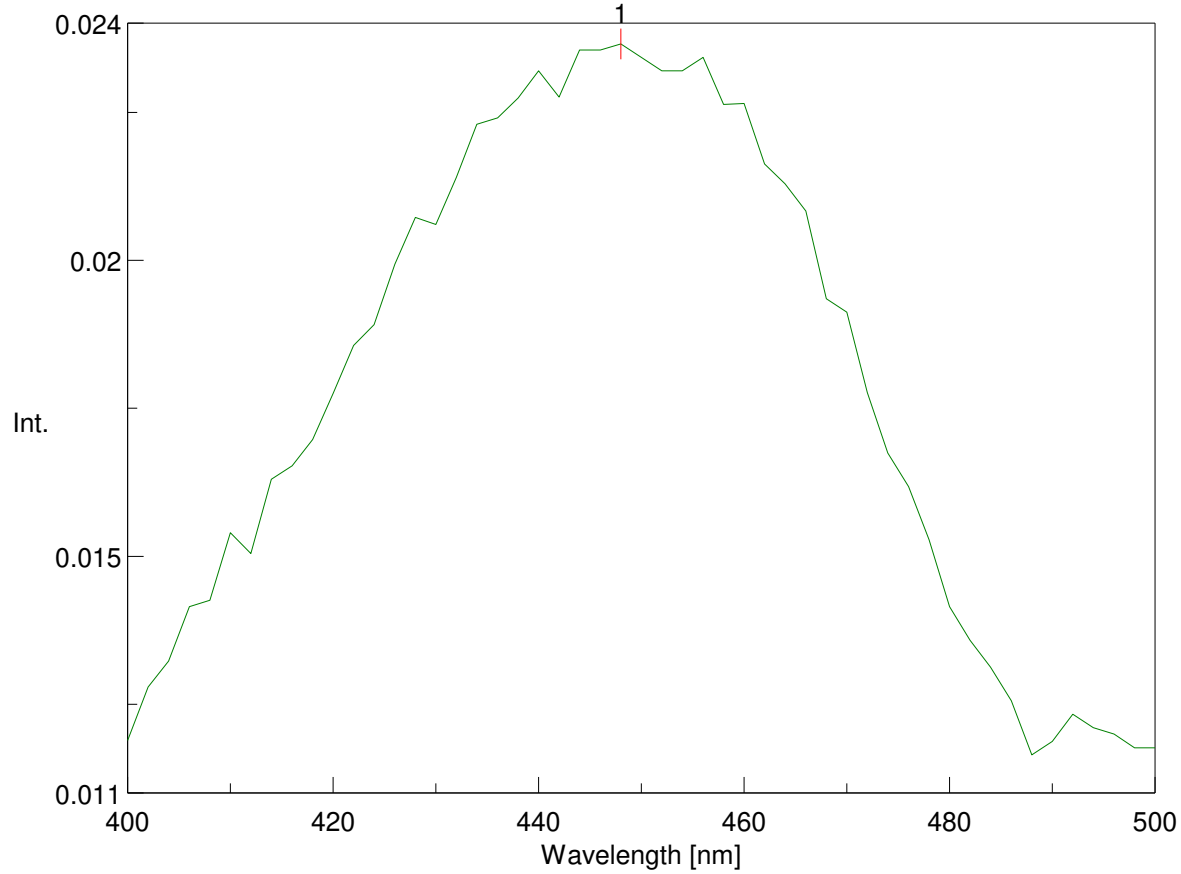

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	07/02/2023 10:02
Date modified	07/02/2023 10:08

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	448	0.0236511			

Chromatogram

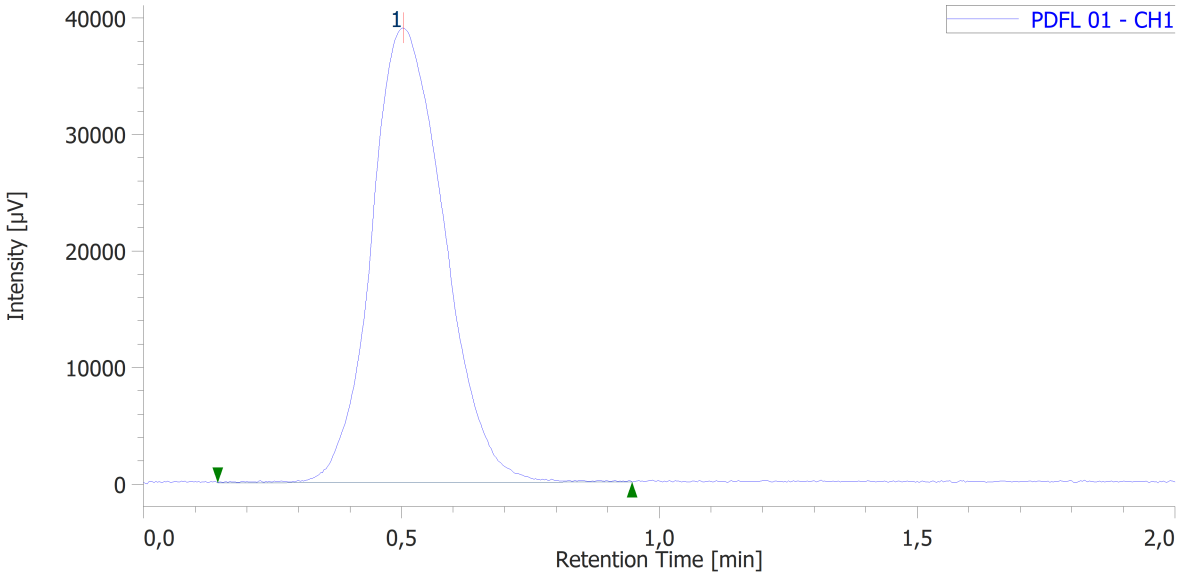

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:43
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 10:43:50
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,503	383431	38982	100,000	100,000	N/A	61	N/A	1,153	

Creator QPackSA
Reviewer
Approver

Chromatogram

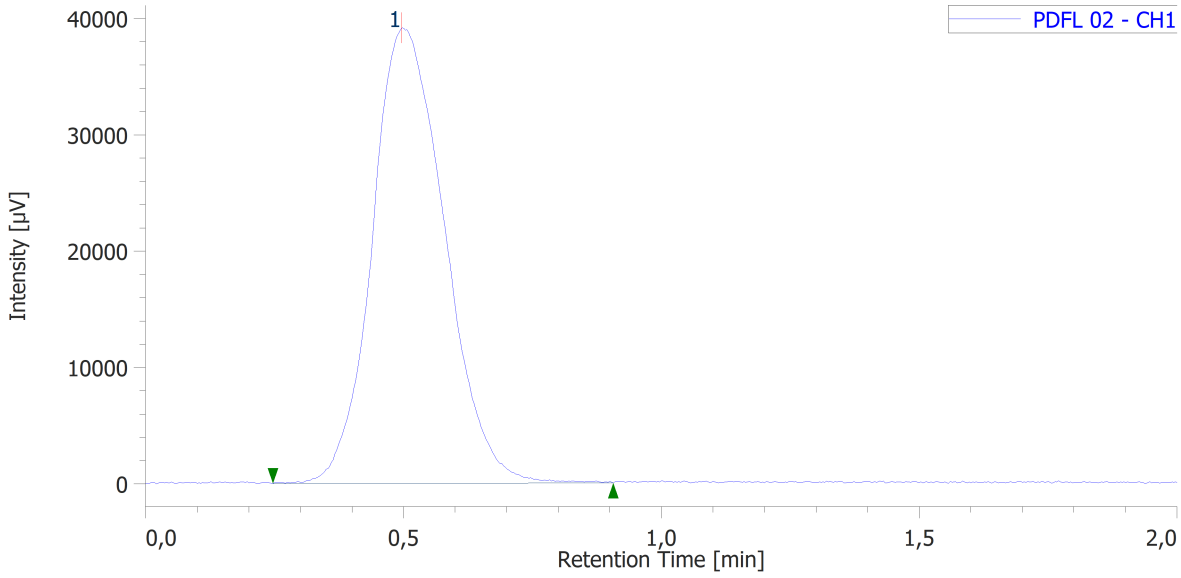

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:46
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 10:47:51
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,497	382507	39113	100,000	100,000	N/A	60	N/A	1,188	

Creator QPackSA
Reviewer
Approver

Chromatogram

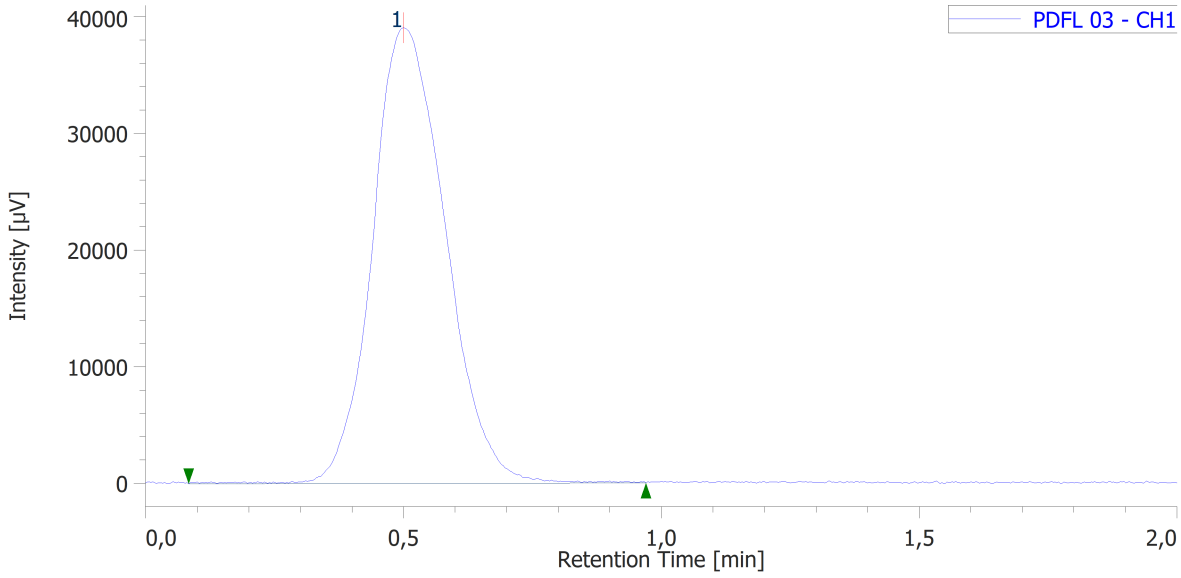

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:46
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 10:51:51
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,500	383505	39011	100,000	100,000	N/A	61	N/A	1,171	

Creator QPackSA
Reviewer
Approver

Chromatogram

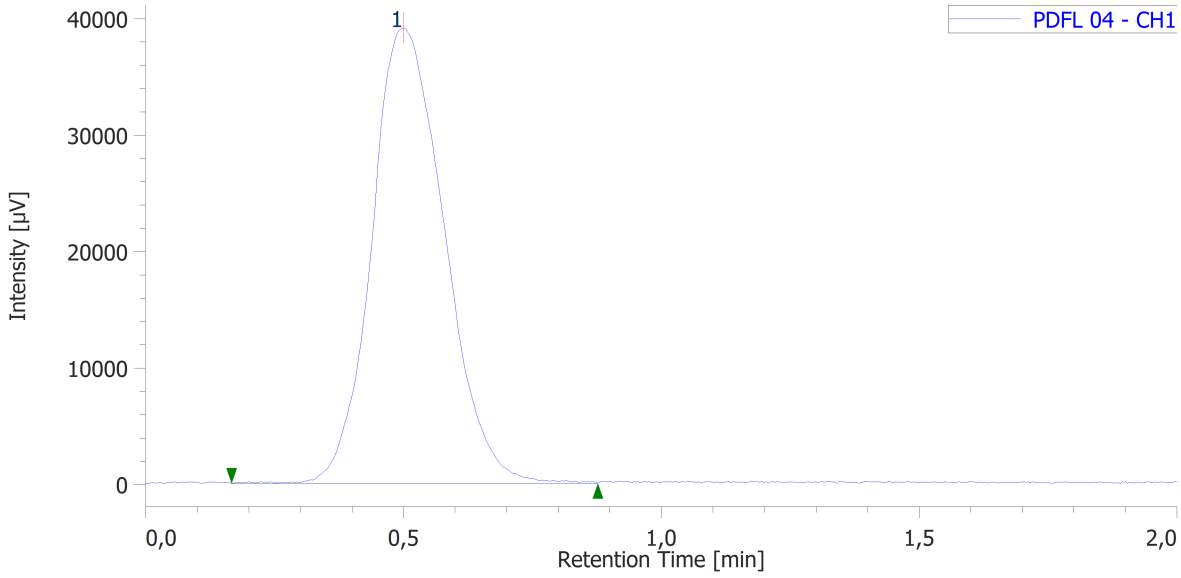

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:46
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 10:55:52
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,500	383023	39082	100,000	100,000	N/A	61	N/A	1,160	

Creator QPackSA
Reviewer
Approver

Chromatogram

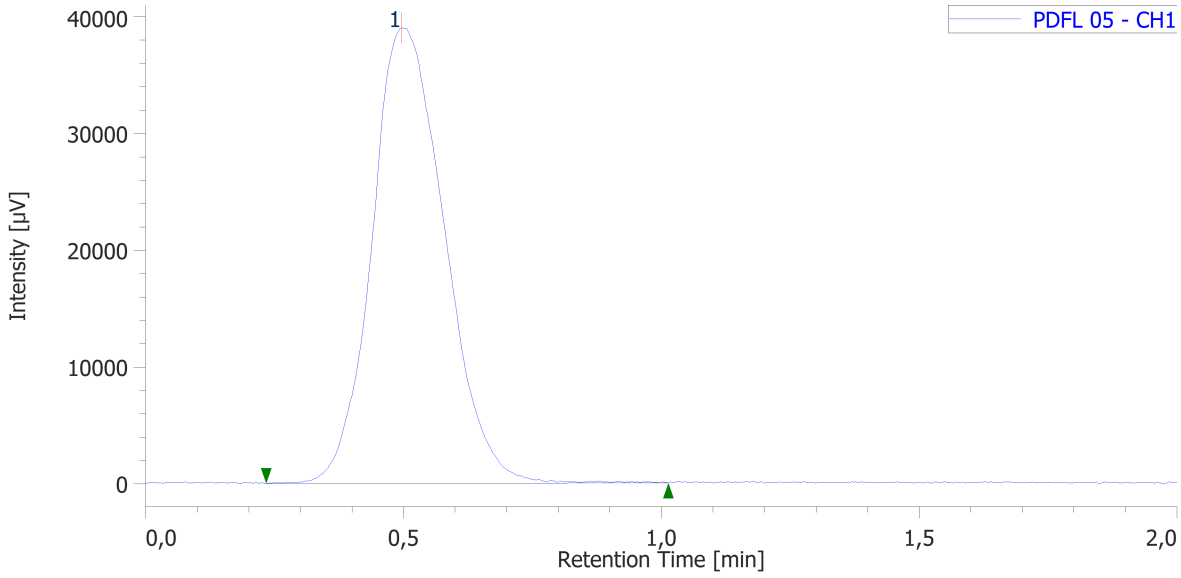

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:46
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 10:59:53
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,497	381977	38975	100,000	100,000	N/A	60	N/A	1,195	

Creator QPackSA
Reviewer
Approver

Chromatogram

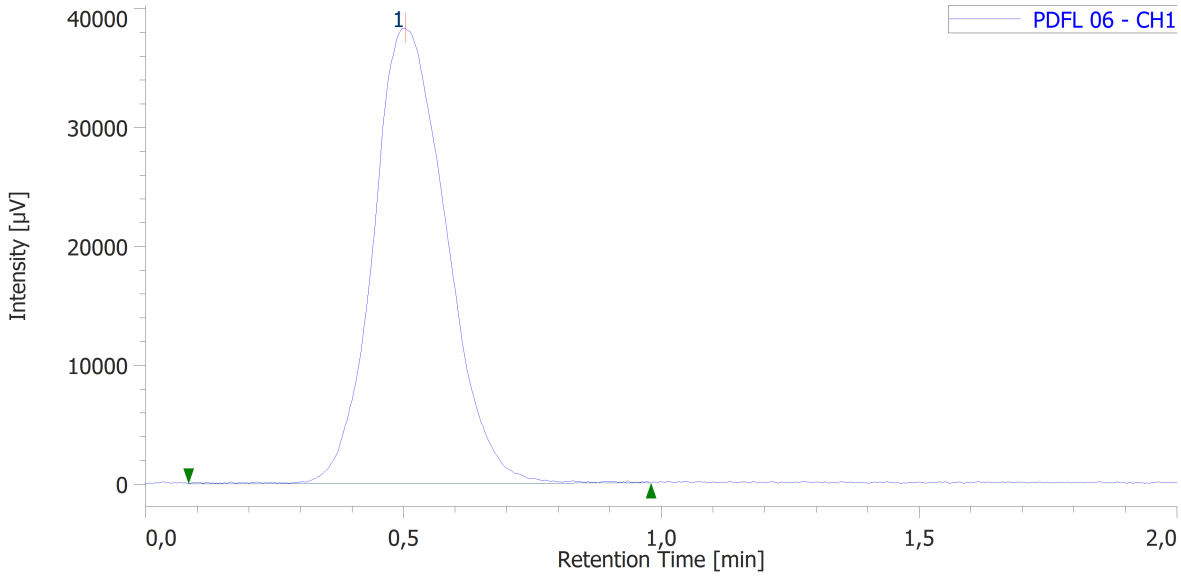

Chromatogram Information	
User Name	QPackSA
Date Modified	07/02/2023 11:07:46
Description	
HPLC System Name	X-LC - Det FL
Injection Date	07/02/2023 11:03:54
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	PDFL HP03
Control Method	Qualificação 3120FP
Peak ID Table	Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PDFL 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração2

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	0,503	378138	38295	100,000	100,000	N/A	61	N/A	1,157	

Creator QPackSA
Reviewer
Approver