
Peak Find - EDUV.jws

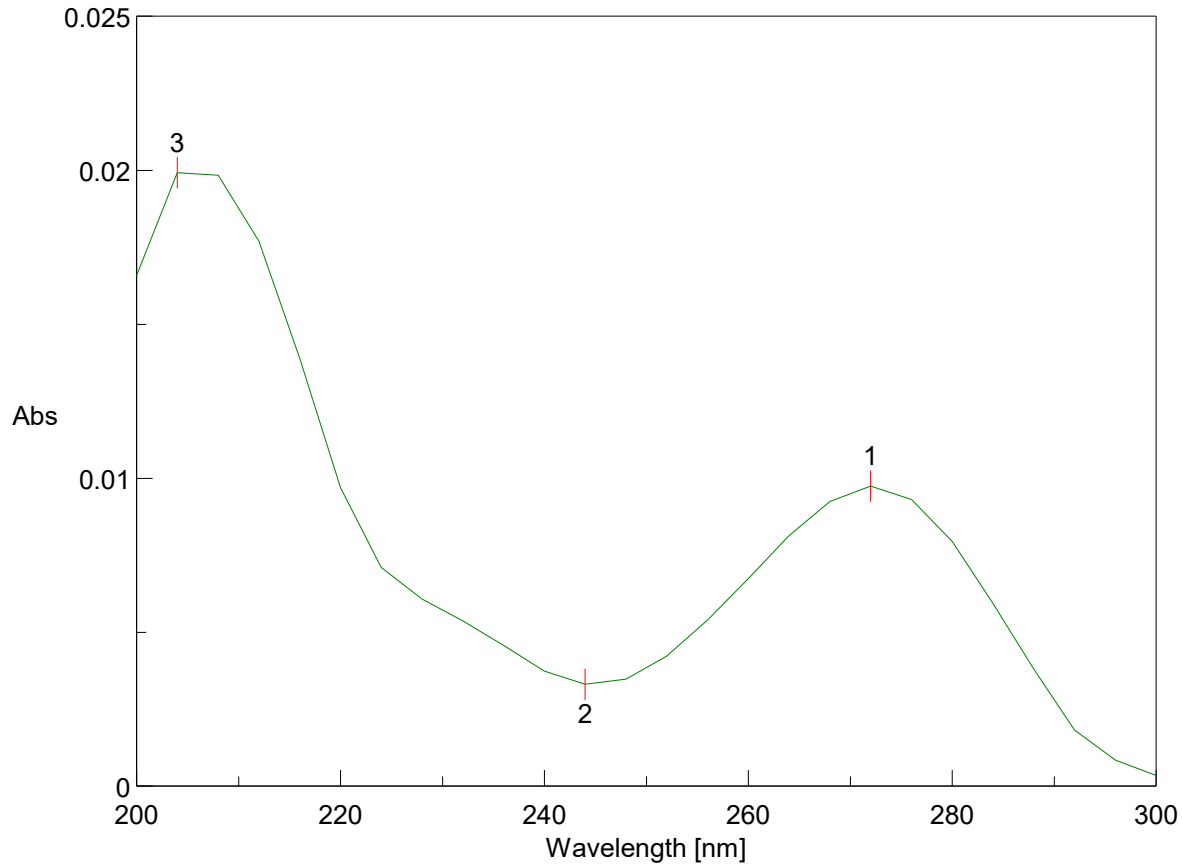

[Comments]

User	QPackSA
Division	---
Company	TRB Pharma
Creation date	05/02/2026 14:25

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	4 nm
Data points	26


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A015061665
ROM version	V1.02.03

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.009737	2	244	0.003309
3	204	0.019922			

Chromatogram

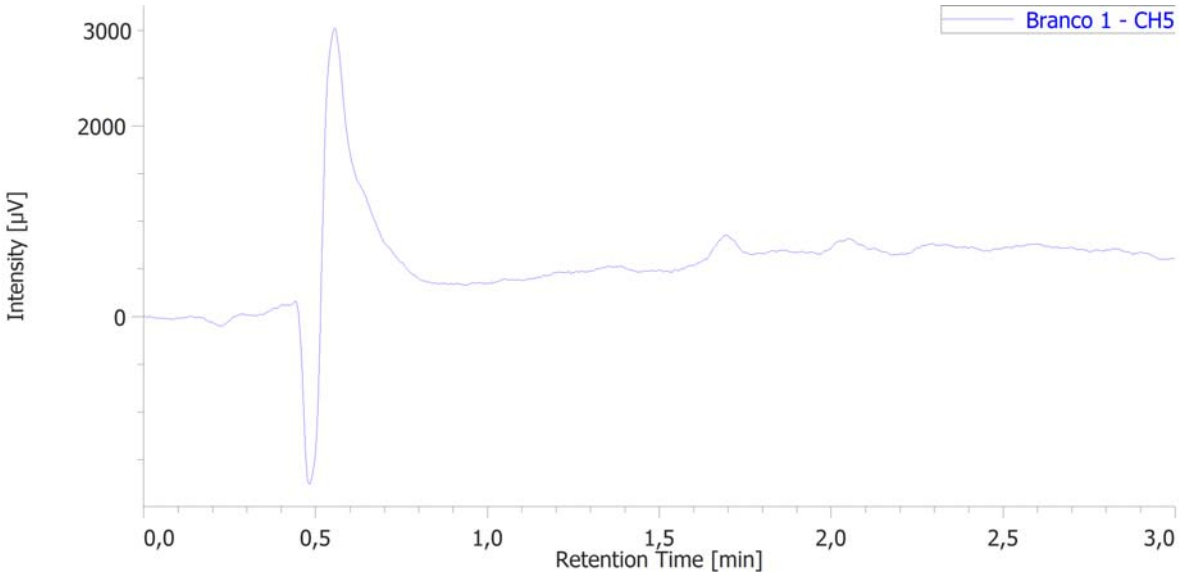


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:25
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:15:32
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

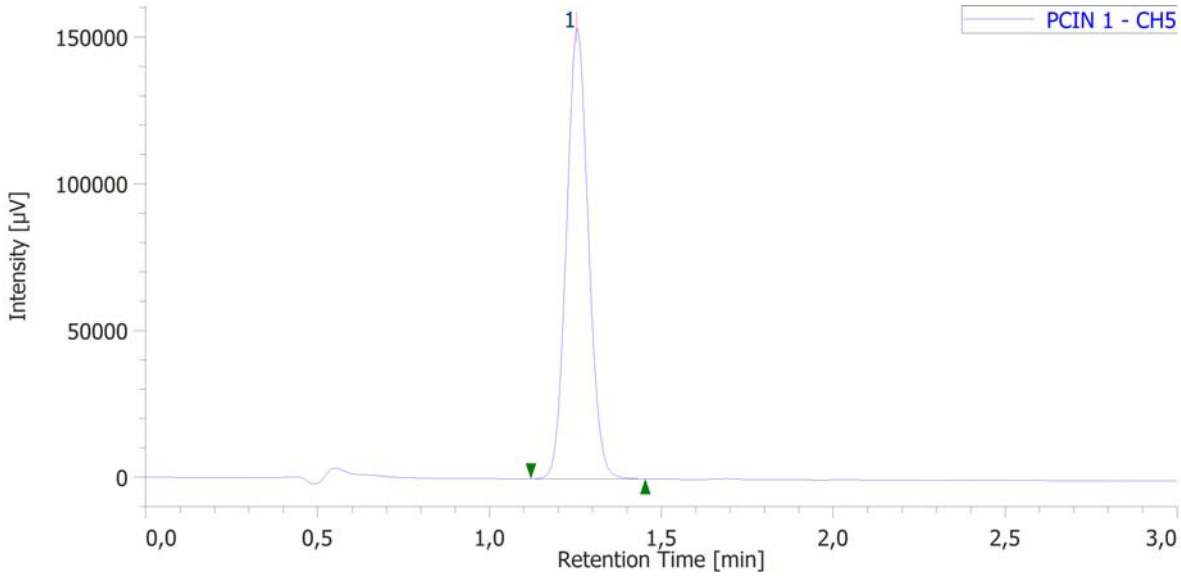

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:25
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:18:44
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,253	682663	153478	100,000	100,000	N/A	1848	N/A	1,096		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

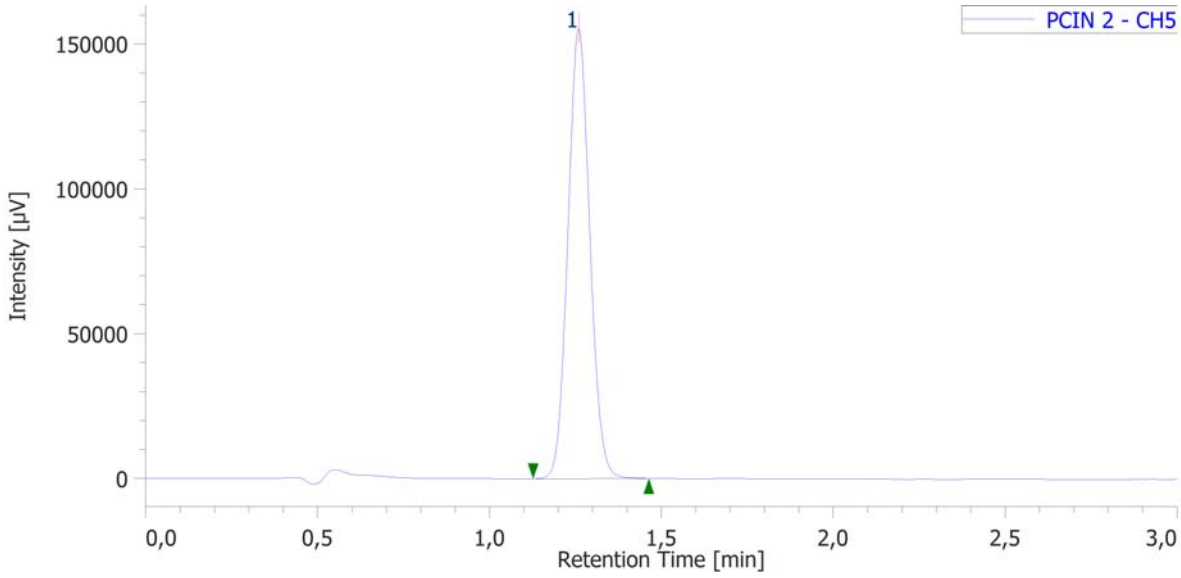

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:25
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:21:56
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,260	688464	155369	100,000	100,000	N/A	1882	N/A	1,061		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

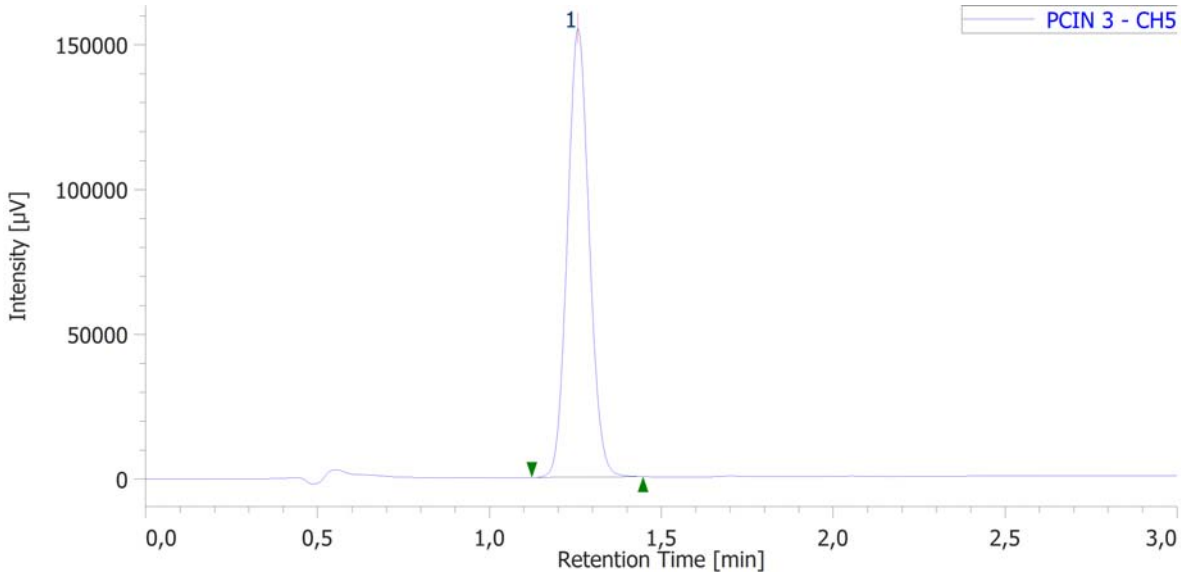

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:25:08
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,257	683726	154968	100,000	100,000	N/A	1885	N/A	1,087		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

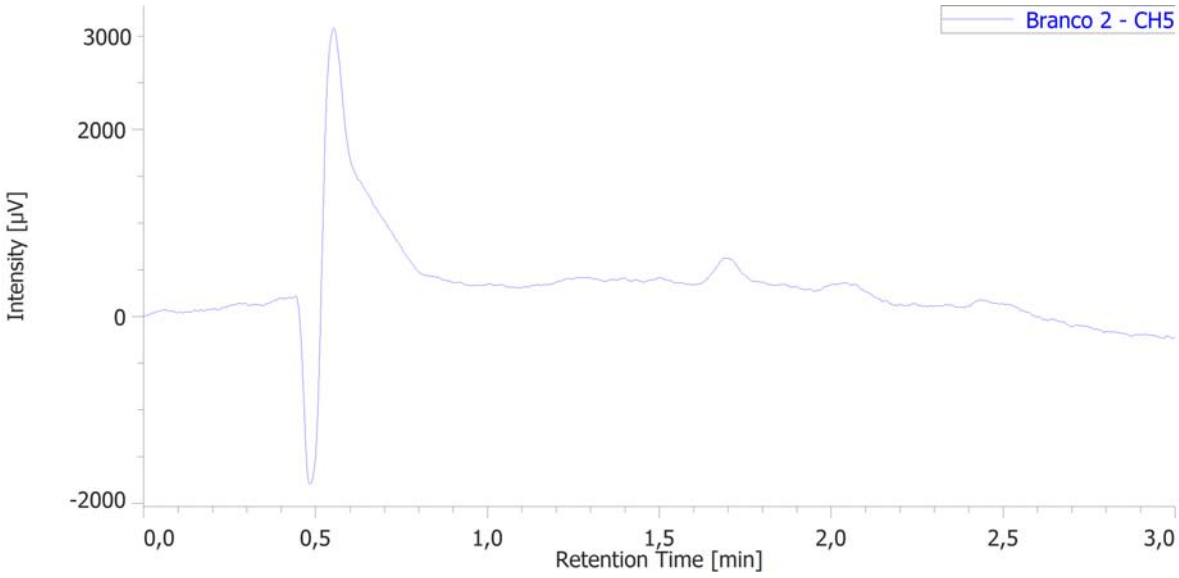


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:28:20
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

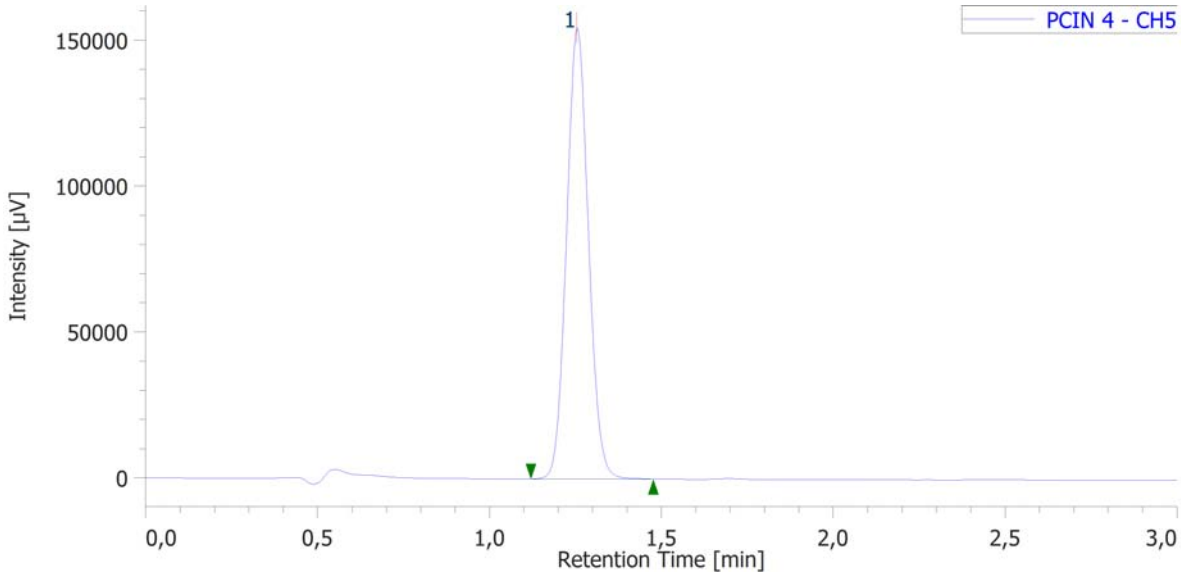

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:31:32
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,253	683439	154402	100,000	100,000	N/A	1869	N/A	1,104		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

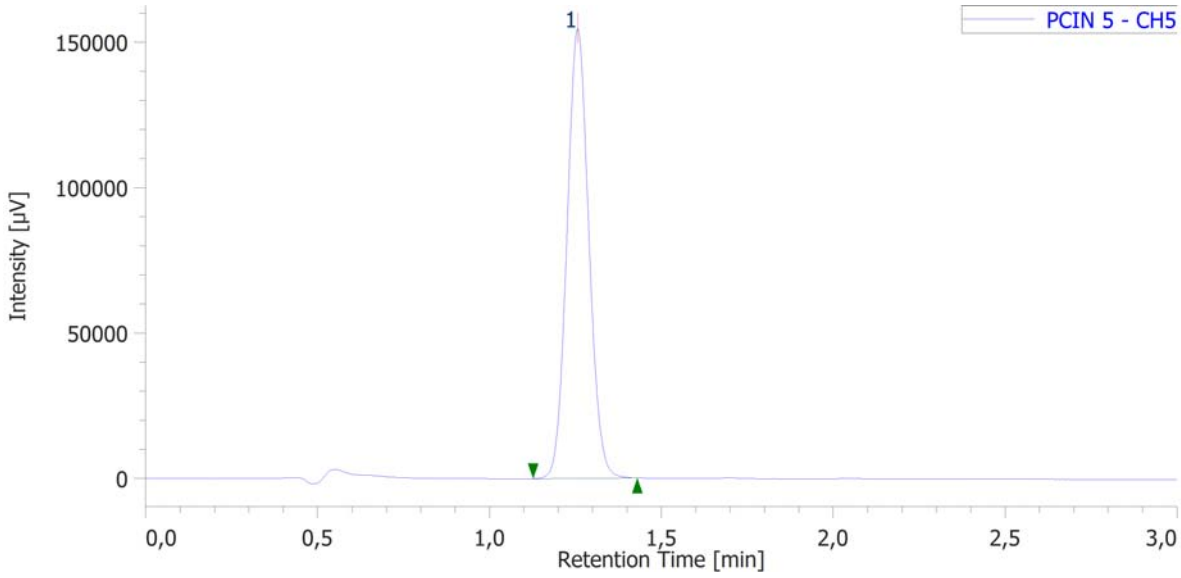

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:34:44
Volume	10,0 [μL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,257	682885	154678	100,000	100,000	N/A	1881	N/A	1,067		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

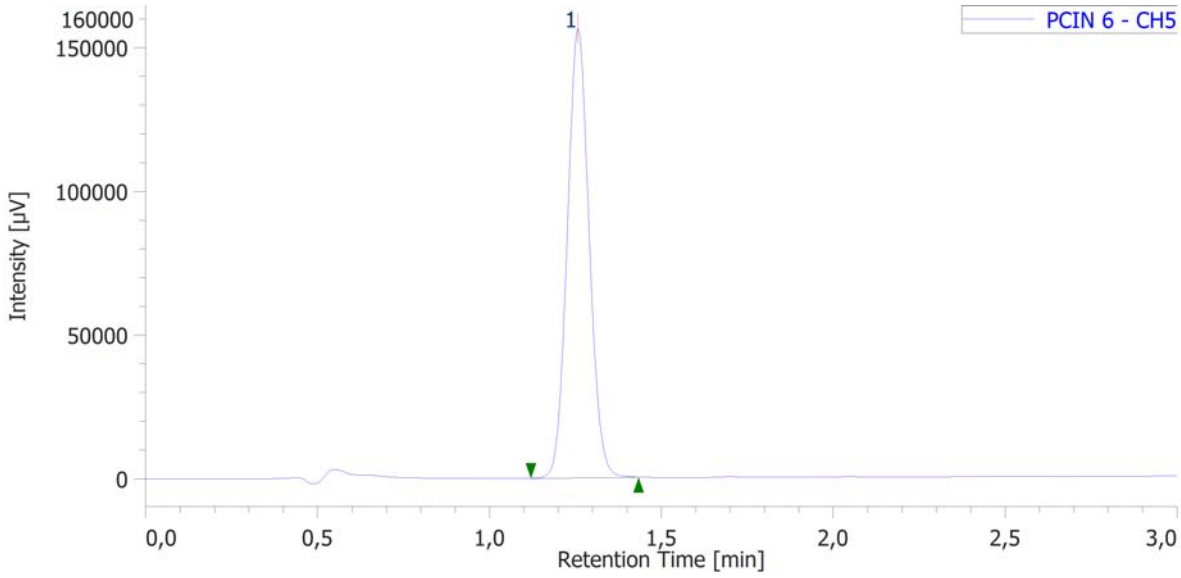

Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:37:56
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,257	690566	156359	100,000	100,000	N/A	1882	N/A	1,081		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

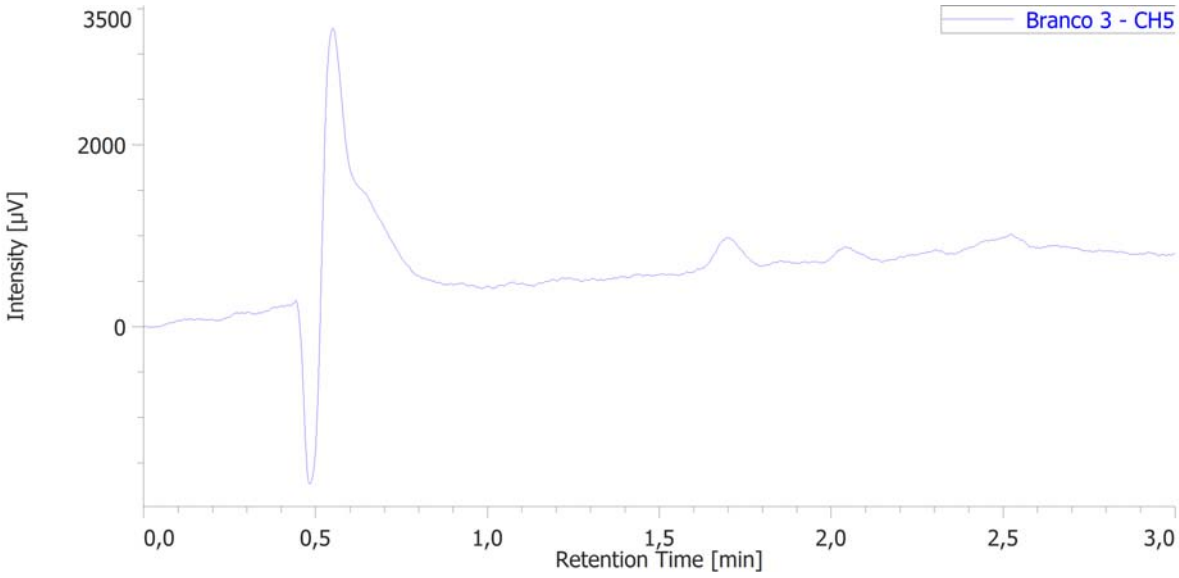


Chromatogram Information	
User Name	QPackSA
Date Modified	05/02/2026 15:45:26
Description	
HPLC System Name	01-HP-03
Injection Date	05/02/2026 15:41:08
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

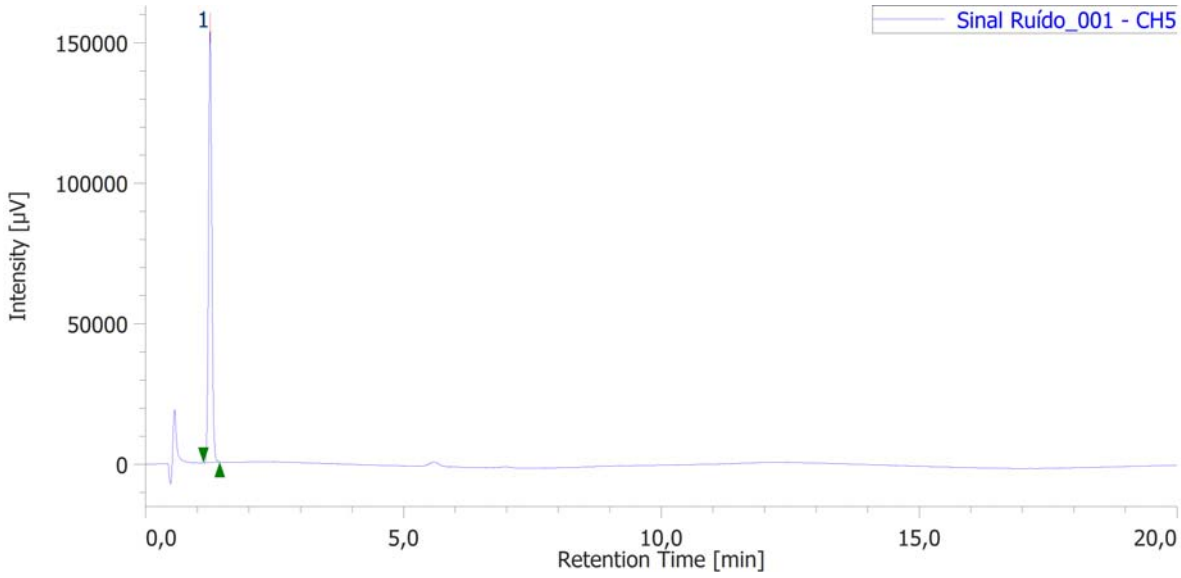

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 12:27:10
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:58:18
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Sinal Ruído
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Sinal Ruído_001-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,250	685191	154414	100,000	100,000	N/A	1849	N/A	1,079		N/A	N/A

Creator QPackSA
Reviewer
Approver

Certificado Nº: 062/26 - RELB	Início da Qualificação: 05/02/2026	Página 1 de 3	

Resultado obtido na altura do pico


	ALTURA DO PICO (mAU)
Resultado:	154,4140

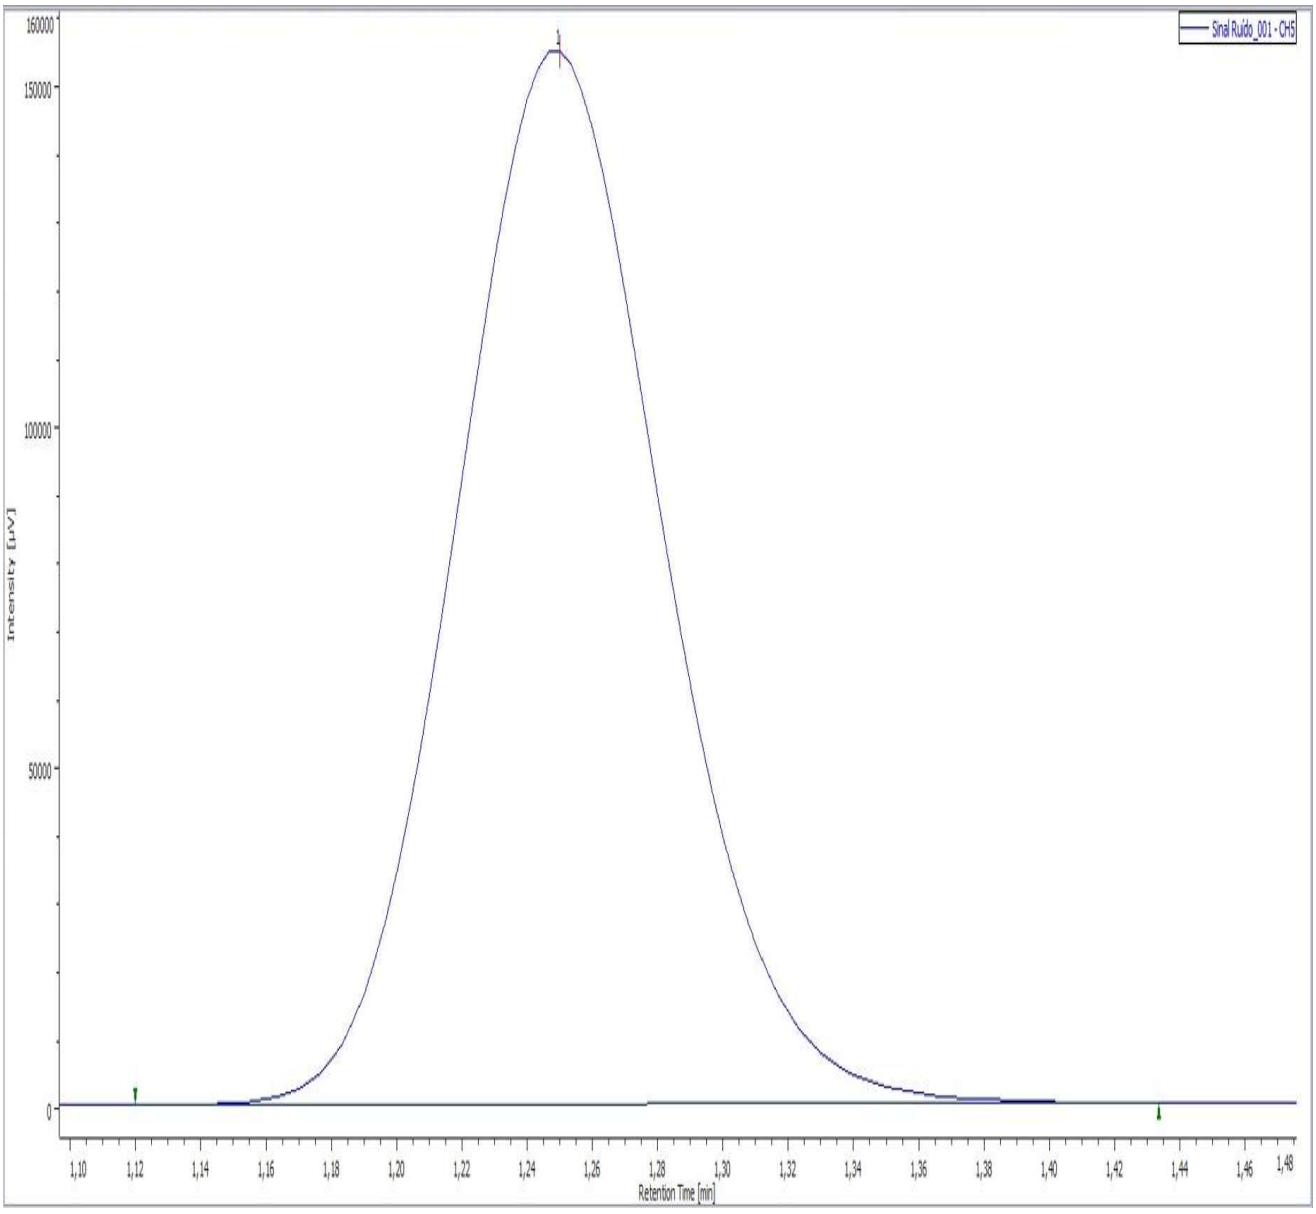


Certificado Nº: 062/26 - RELB	Início da Qualificação: 05/02/2026	Página 2 de 3

Resultado obtido no teste de sinal/ruído

Resultado:	Ruído (mAU)
VALOR MÁXIMO:	1,2706
VALOR MÍNIMO:	1,2635
	Ruído
	0,0071

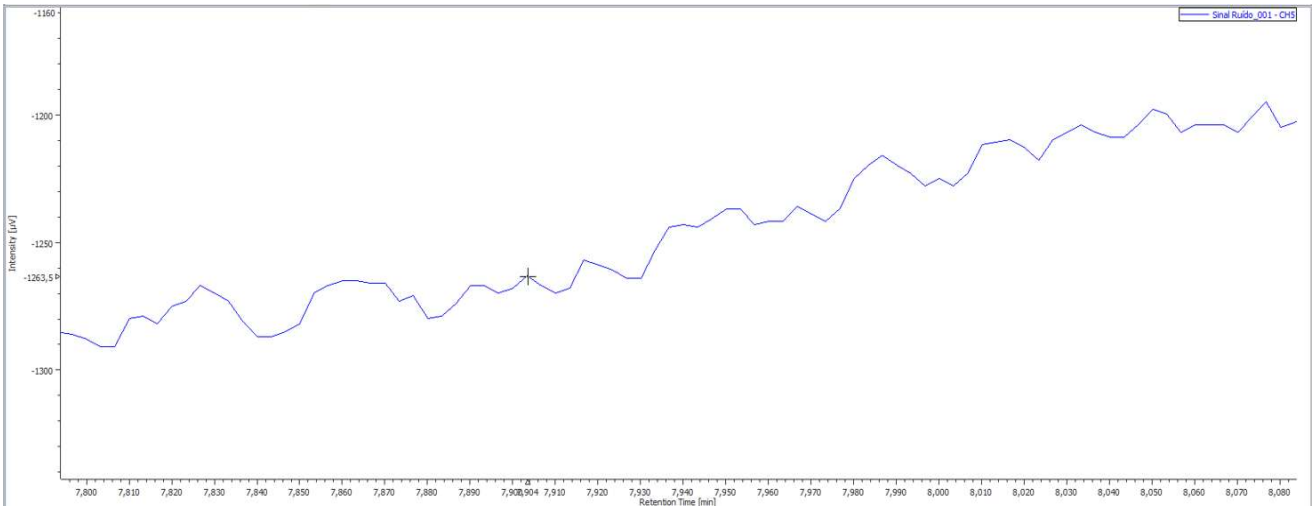


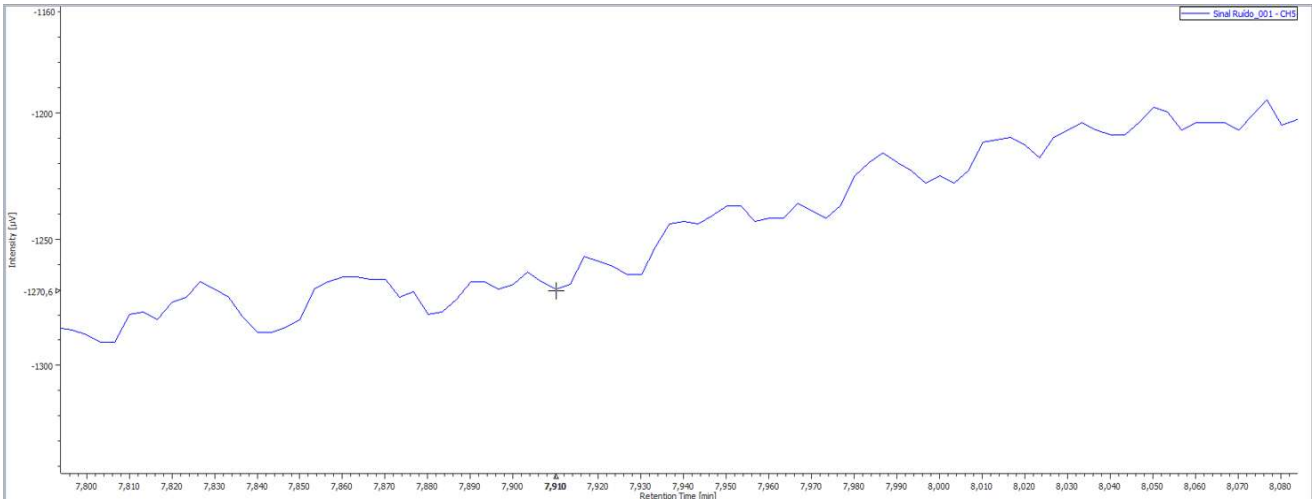


Certificado Nº: 062/26 - RELB	Início da Qualificação: 05/02/2026	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	0,3251	0,8391
VALOR MÍNIMO:	0,0454	
Resultado:	0,2797	

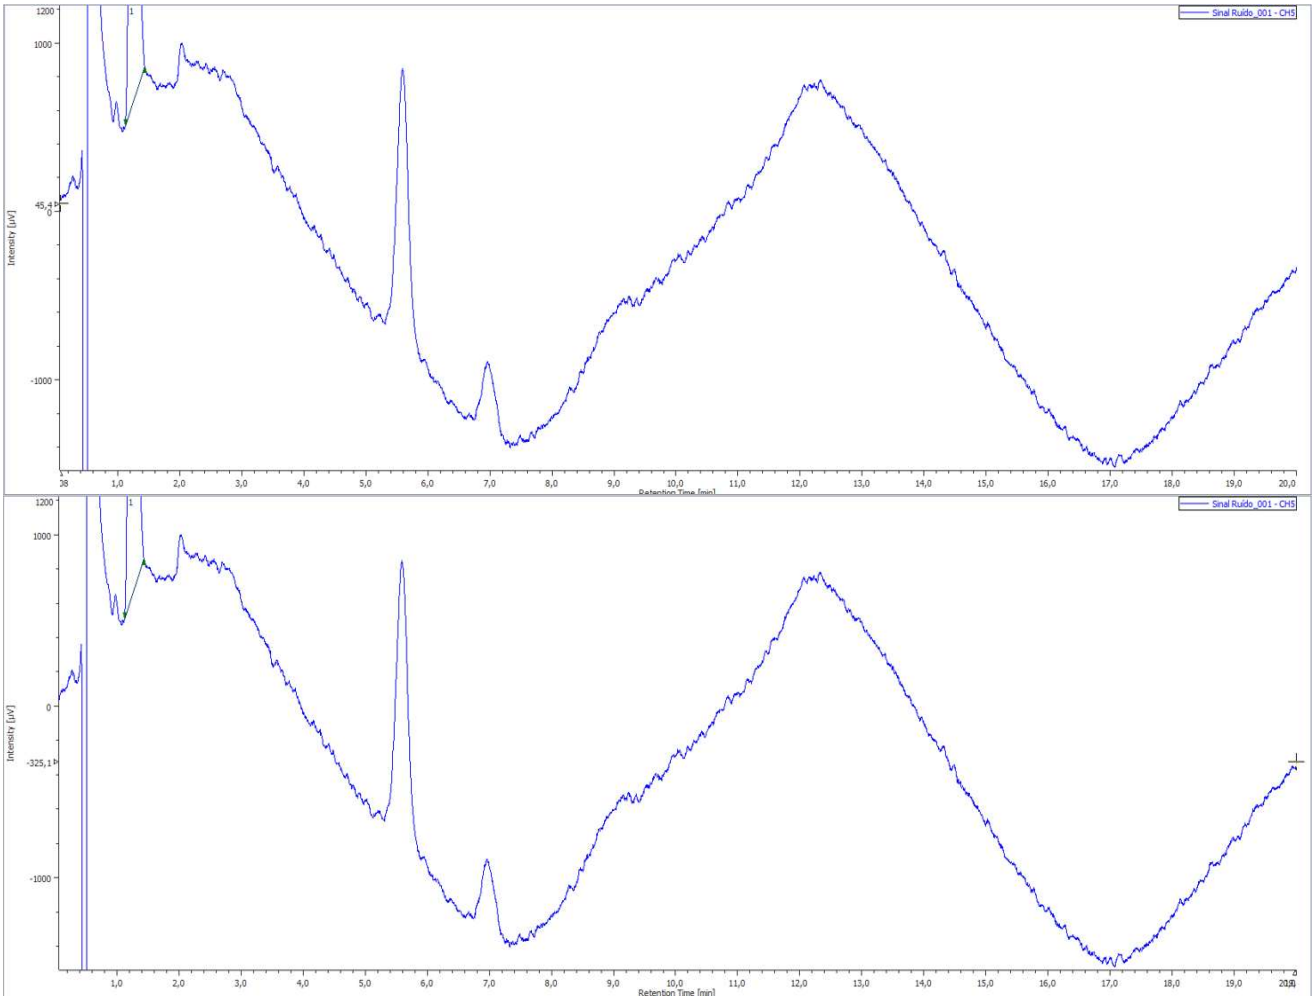

Chromatogram

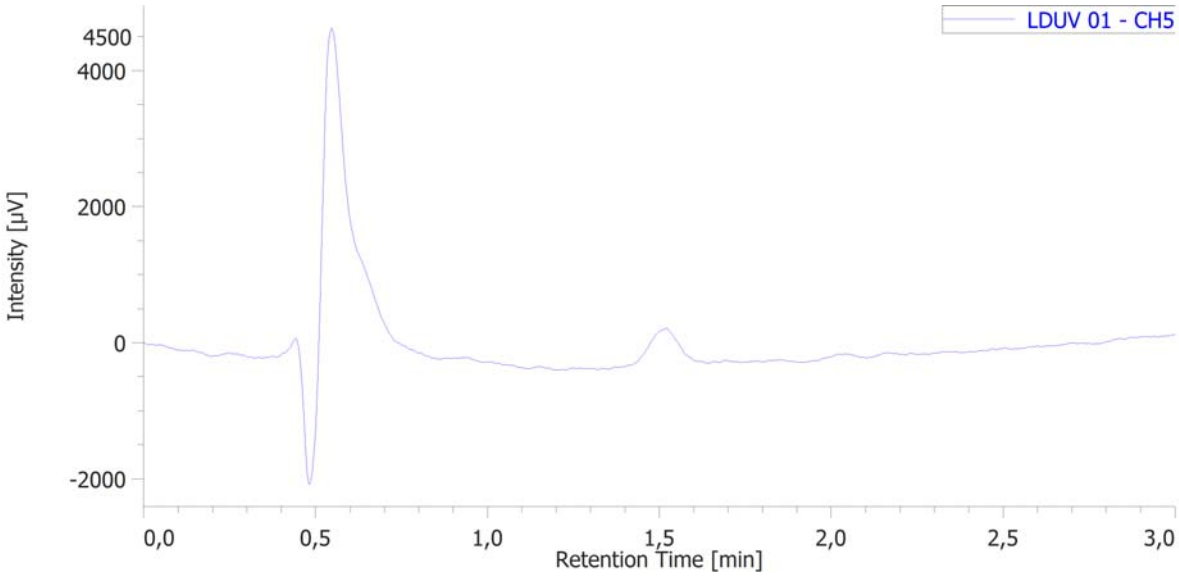


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:16:18
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 10:58:45
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

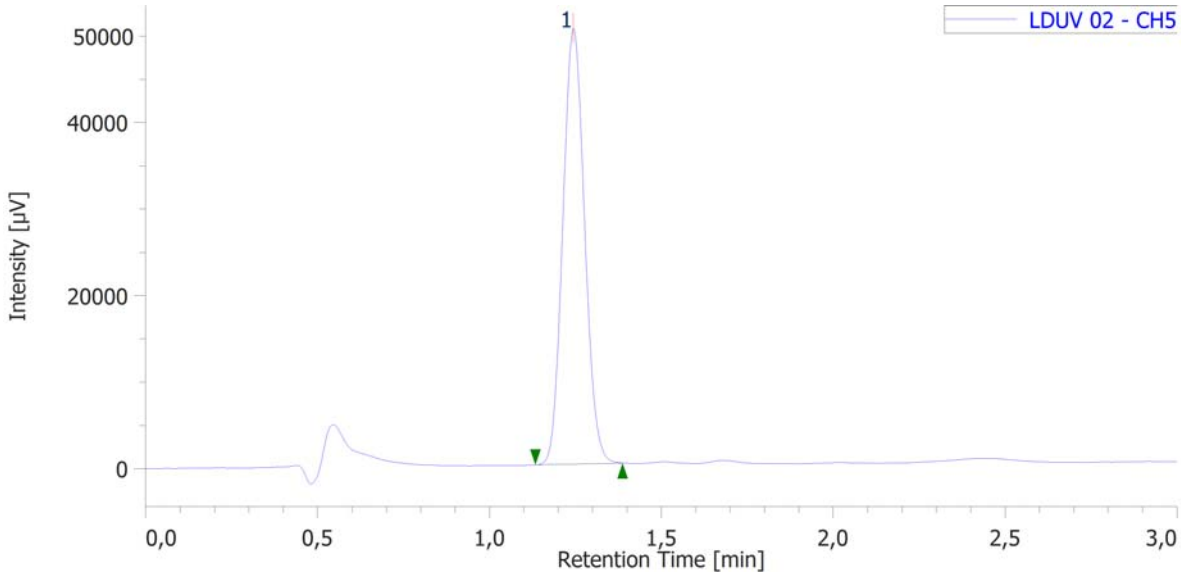

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:16:18
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:01:57
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,243	221272	50335	100,000	100,000	N/A	1819	N/A	1,095		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

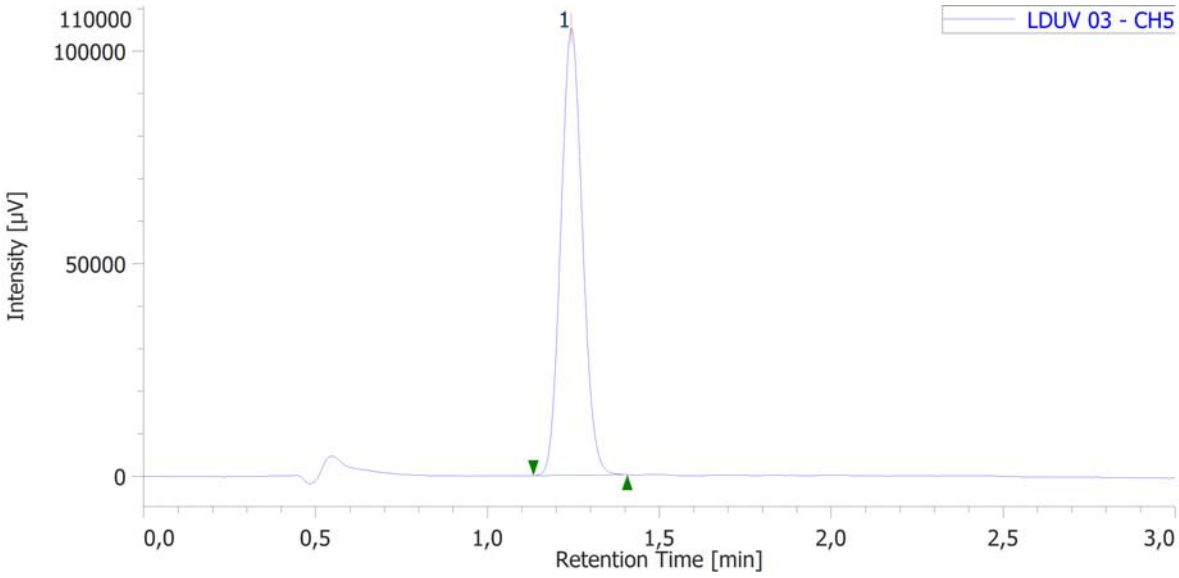

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:16:18
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:05:09
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,243	459123	105084	100,000	100,000	N/A	1857	N/A	1,095		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

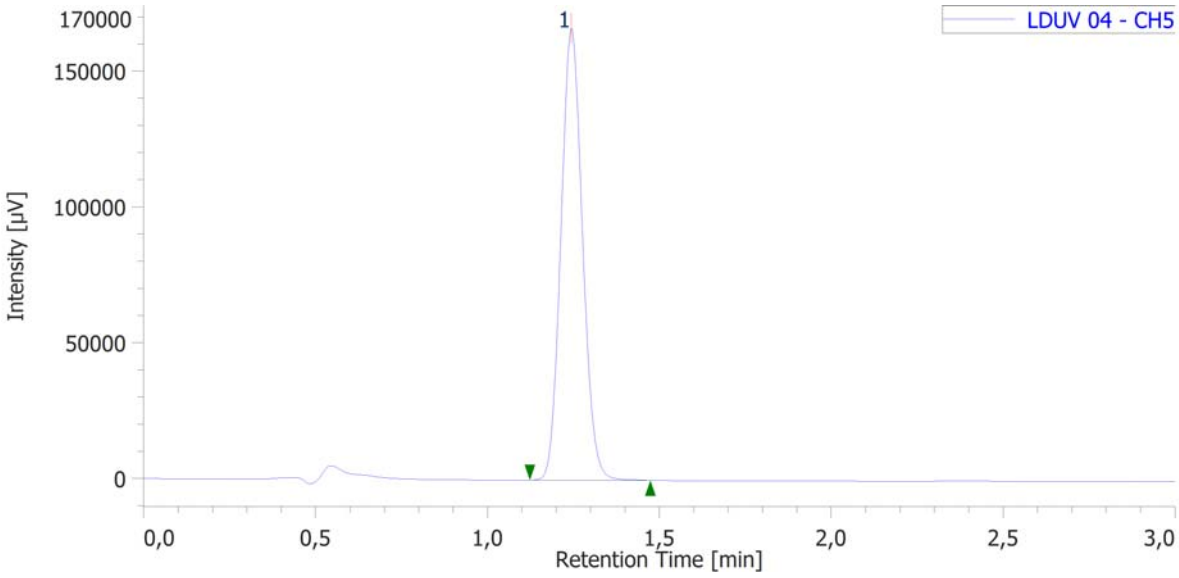

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:16:18
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:08:21
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,243	724465	166285	100,000	100,000	N/A	1890	N/A	1,100		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

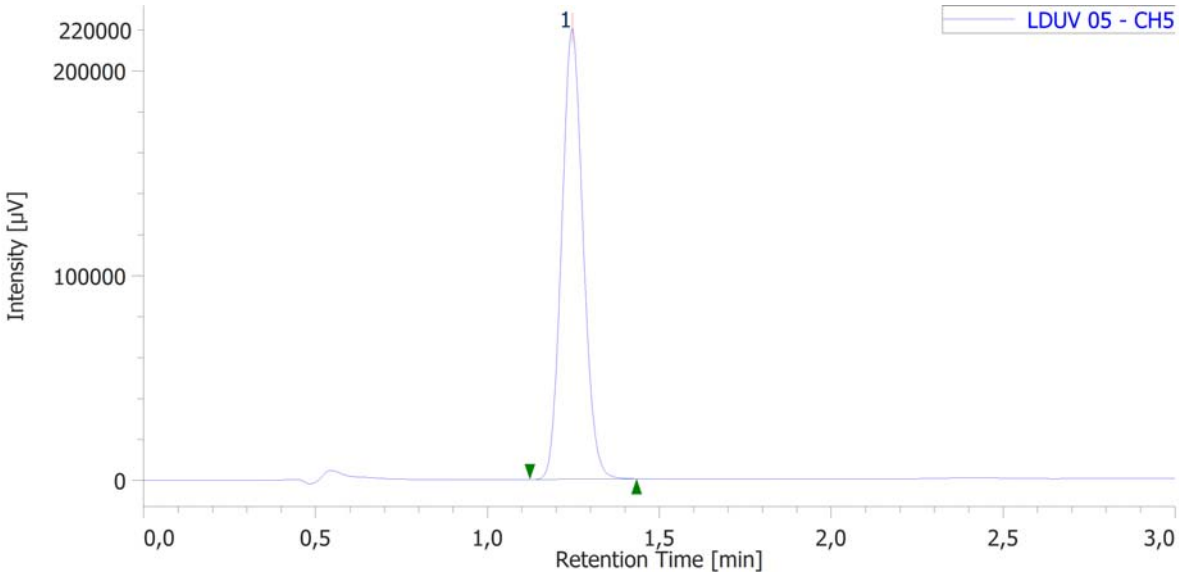

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:16:18
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:11:33
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,247	952591	220142	100,000	100,000	N/A	1936	N/A	1,077		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

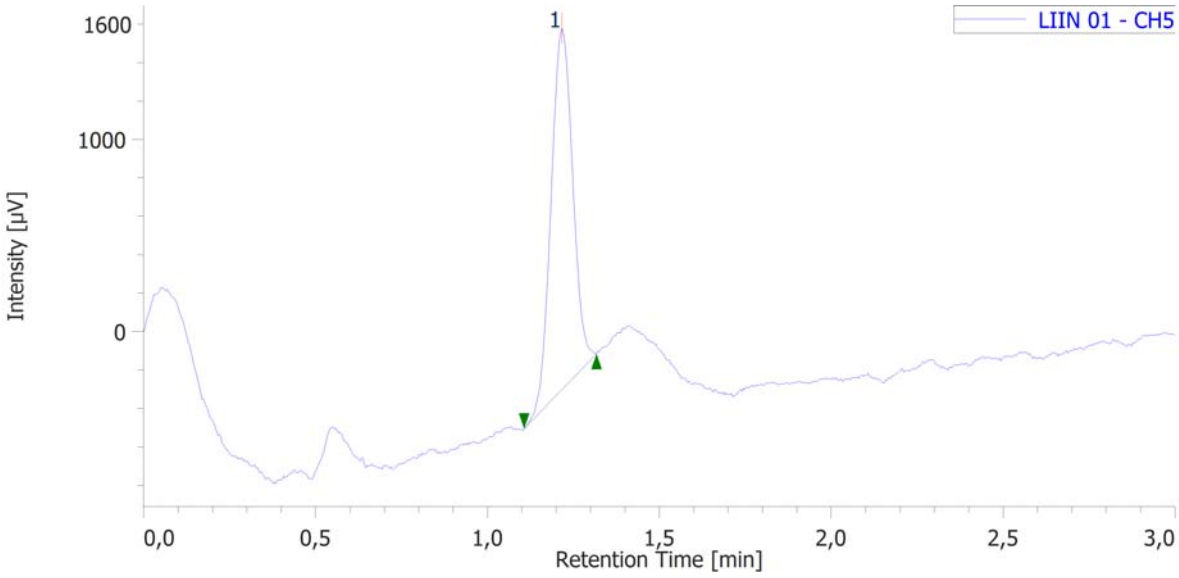

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:43:14
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:35:48
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,217	8220	1879	100,000	100,000	N/A	1756	N/A	1,027		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

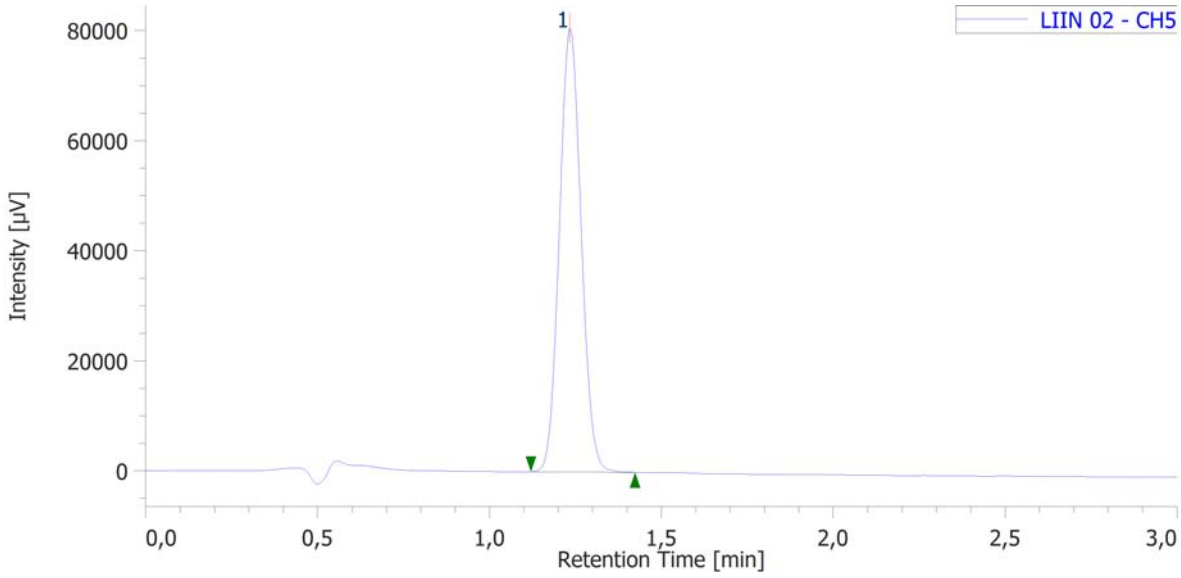

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:44:30
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:39:00
Volume	5,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,233	354044	80574	100,000	100,000	N/A	1804	N/A	1,084		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

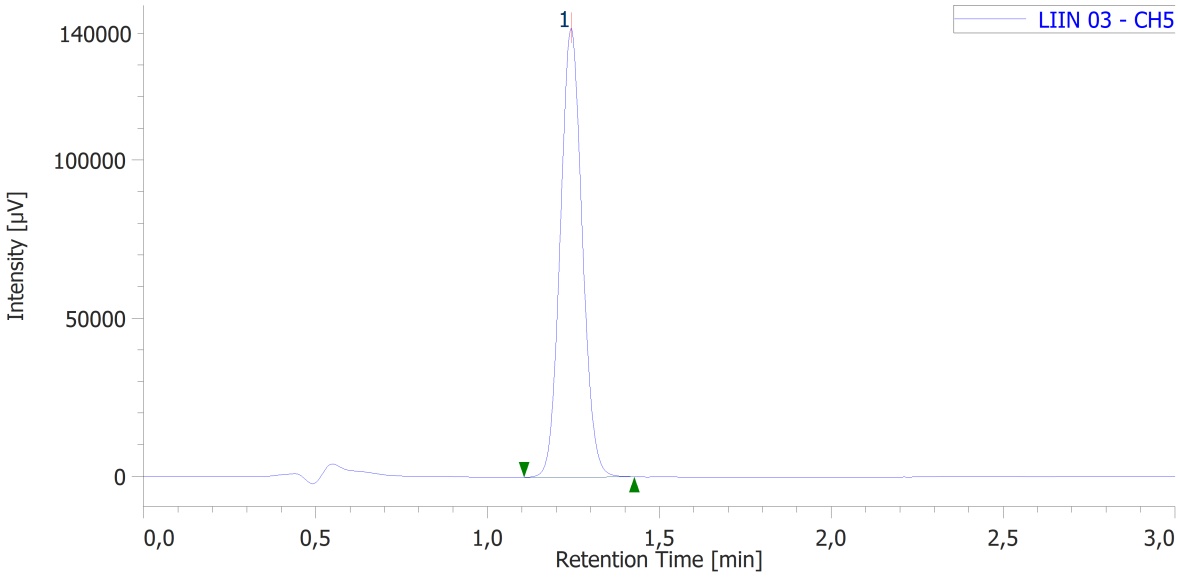

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:45:52
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:42:12
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,243	728907	141908	100,000	100,000	N/A	1831	N/A	1,064		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

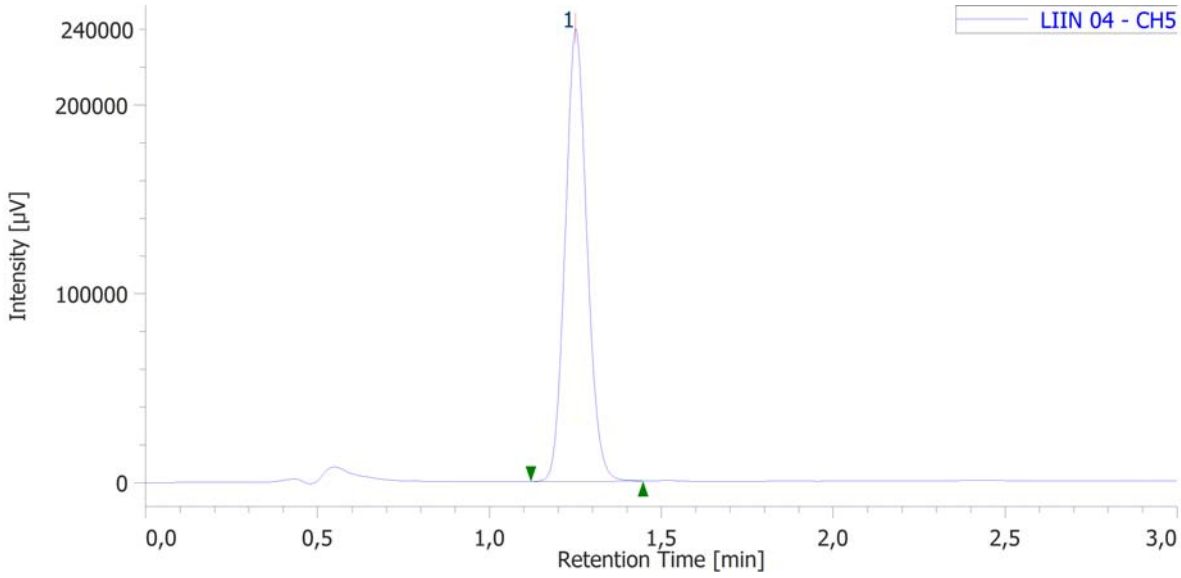

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:51:27
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:45:24
Volume	15,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,250	1053826	239909	100,000	100,000	N/A	1910	N/A	1,108		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

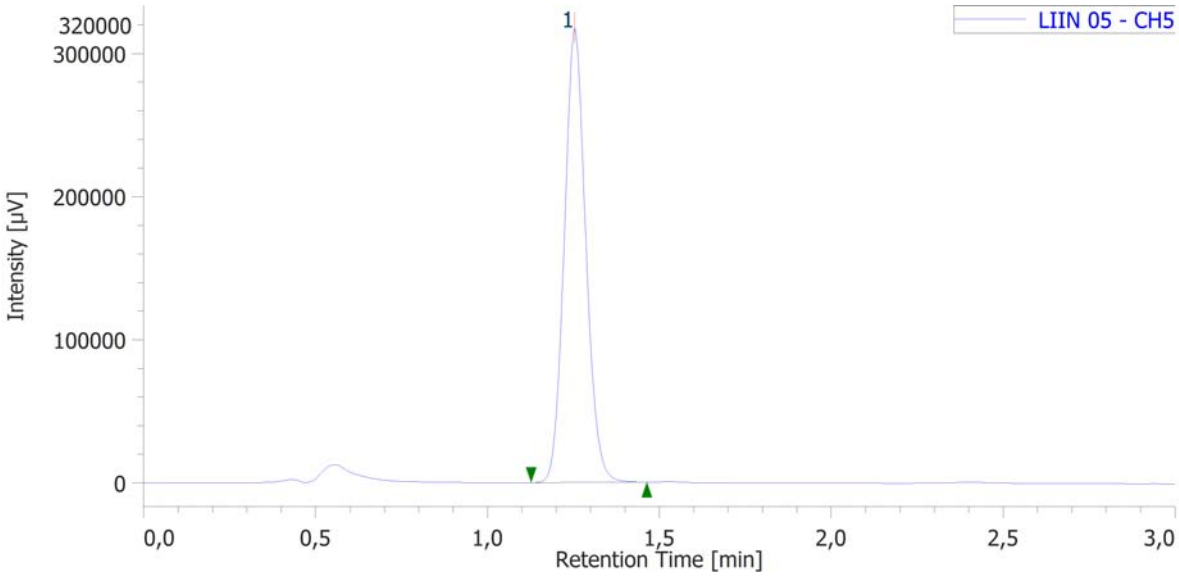

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 11:53:23
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 11:48:36
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	5	1,253	1377410	317214	100,000	100,000	N/A	1983	N/A	1,102		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

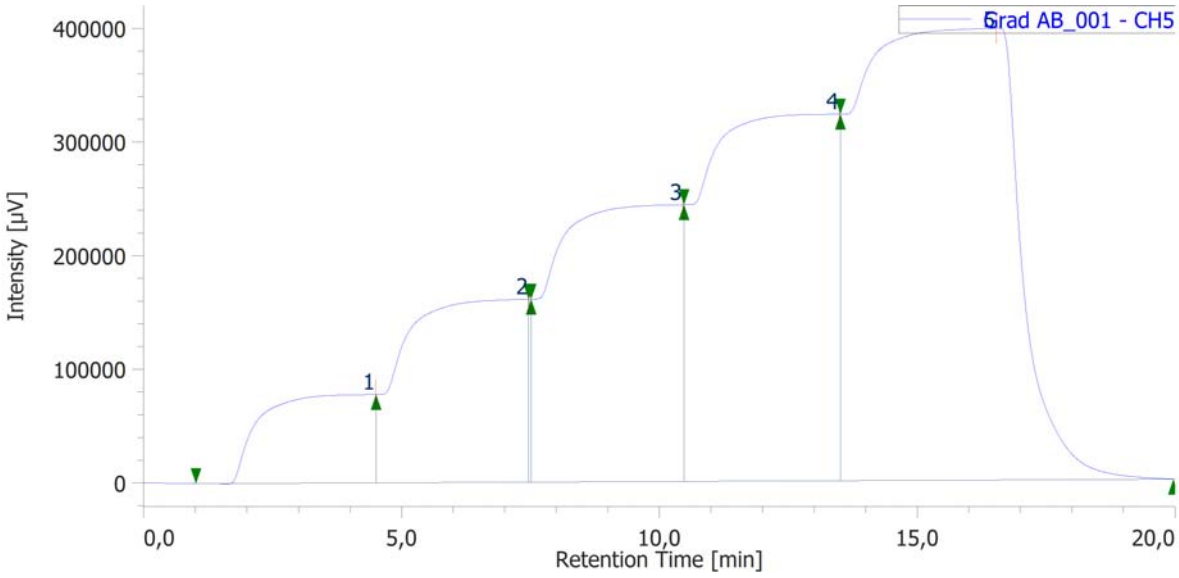

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 13:20:17
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 12:55:38
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	20%	5	4,500	10996301	77756	5,754	6,473	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	5	7,467	482212	160691	0,252	13,377	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	5	10,450	40178441	243209	21,024	20,247	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	5	13,483	55631188	322339	29,110	26,834	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	5	16,527	83820949	397219	43,860	33,068	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

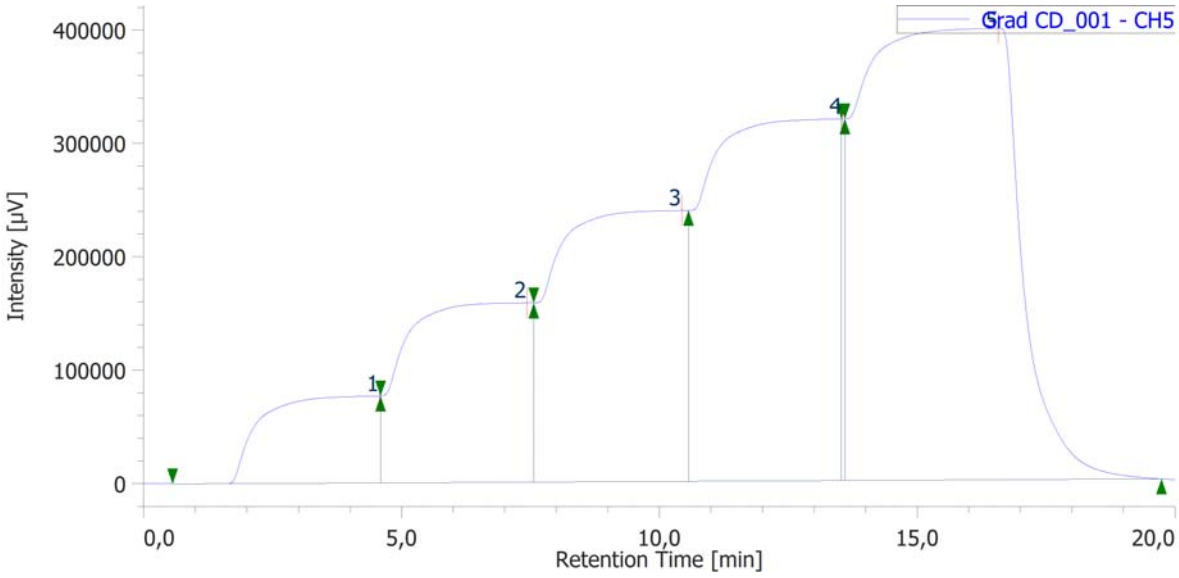

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 13:47:37
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 13:22:17
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	20%	5	4,570	11193790	76550	6,969	6,435	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	5	7,433	25633956	157942	15,959	13,277	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	5	10,433	40215245	238680	25,037	20,064	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	5	13,547	1401984	318601	0,873	26,782	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	5	16,573	82177806	397844	51,162	33,443	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

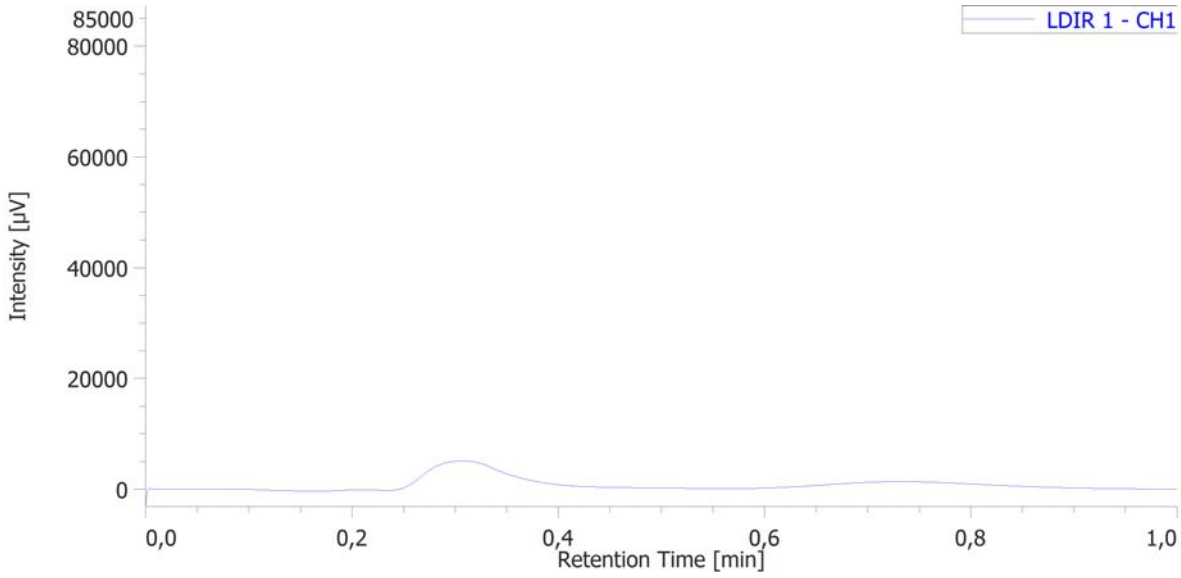


Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 14:55:36
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 14:40:53
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Qualificação RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação RI (Manual)

Creator
Reviewer
Approver

Chromatogram

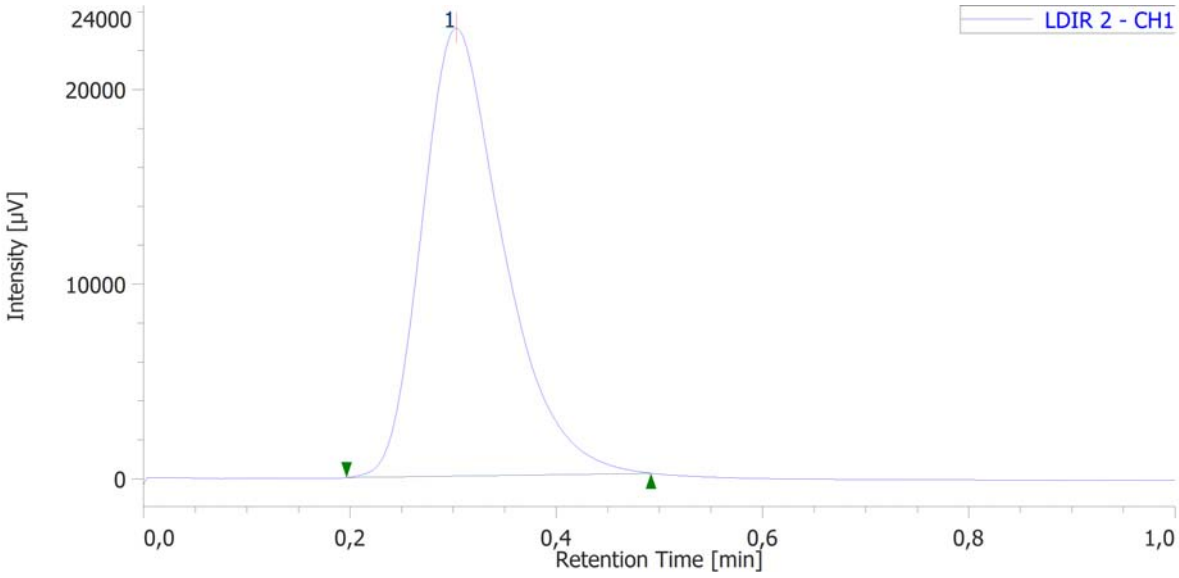

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 15:11:31
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 14:59:55
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Qualificação RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	LDRI	1	0,303	126422	22992	100,000	100,000	N/A	74	N/A	1,374		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

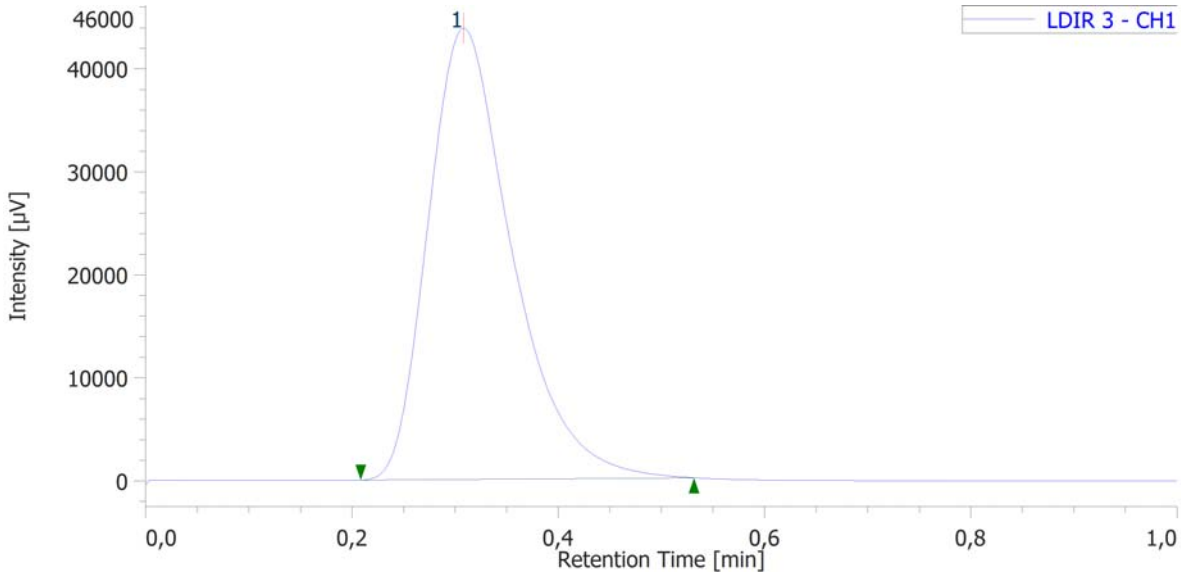

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 15:11:31
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 15:02:32
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Qualificação RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	LDRI	1	0,308	247462	43770	100,000	100,000	N/A	72	N/A	1,409		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

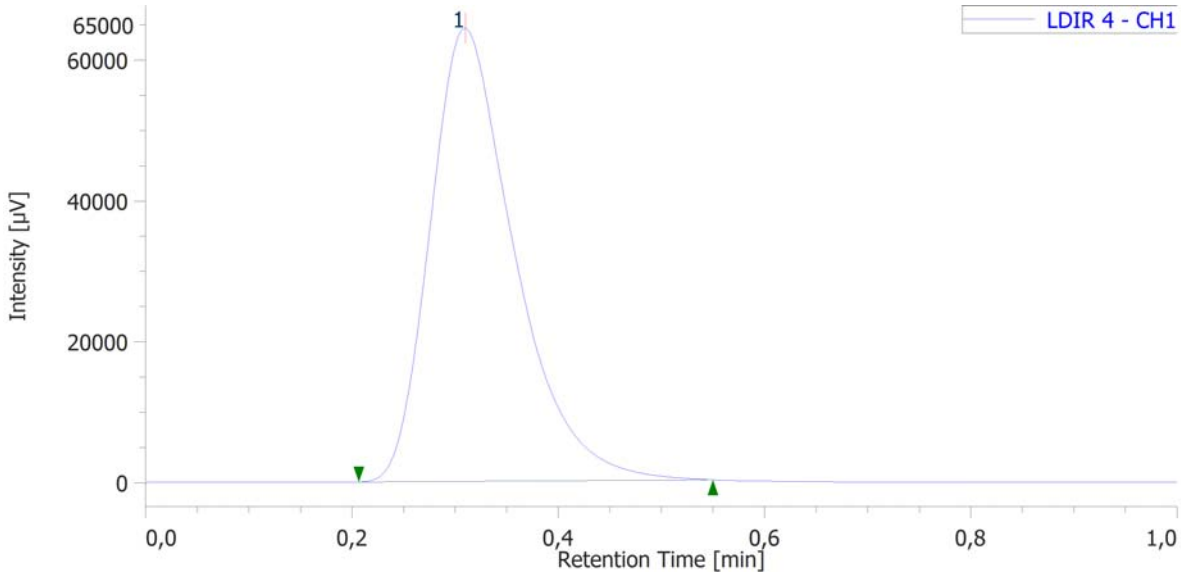

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 15:11:32
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 15:05:18
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Qualificação RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	LDRI	1	0,310	365730	64302	100,000	100,000	N/A	73	N/A	1,410		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

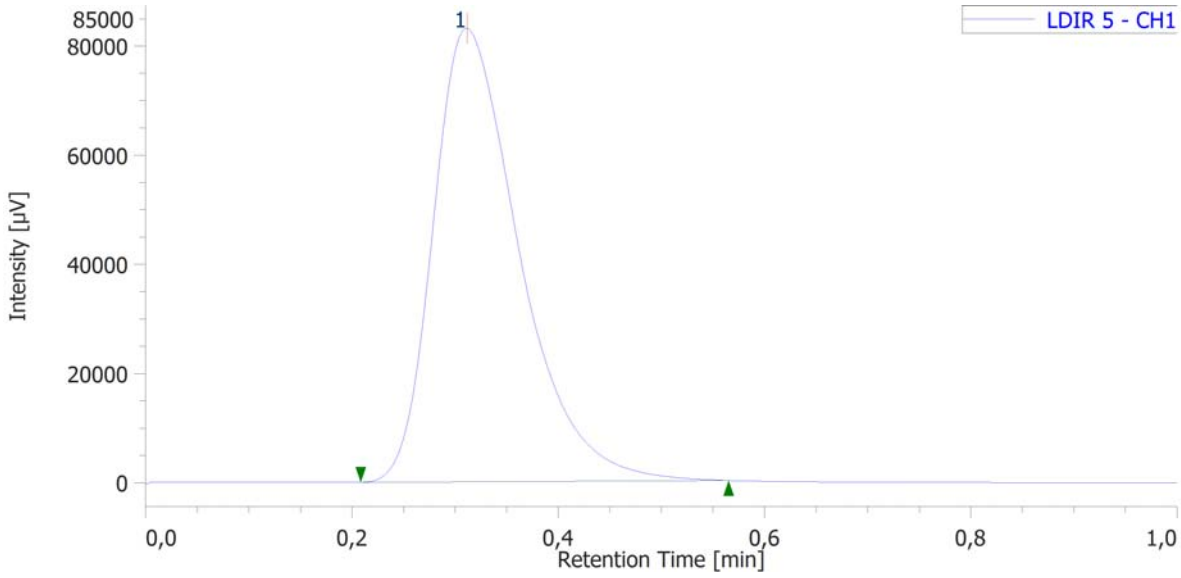

Chromatogram Information	
User Name	QPackSA
Date Modified	06/02/2026 15:11:32
Description	
HPLC System Name	01-HP-03
Injection Date	06/02/2026 15:08:15
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Qualificação RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	LDRI	1	0,312	481370	83029	100,000	100,000	N/A	71	N/A	1,465		N/A	N/A

Creator QPackSA
Reviewer
Approver