
Peak Find - EDUV PDA_1.7600.JWS

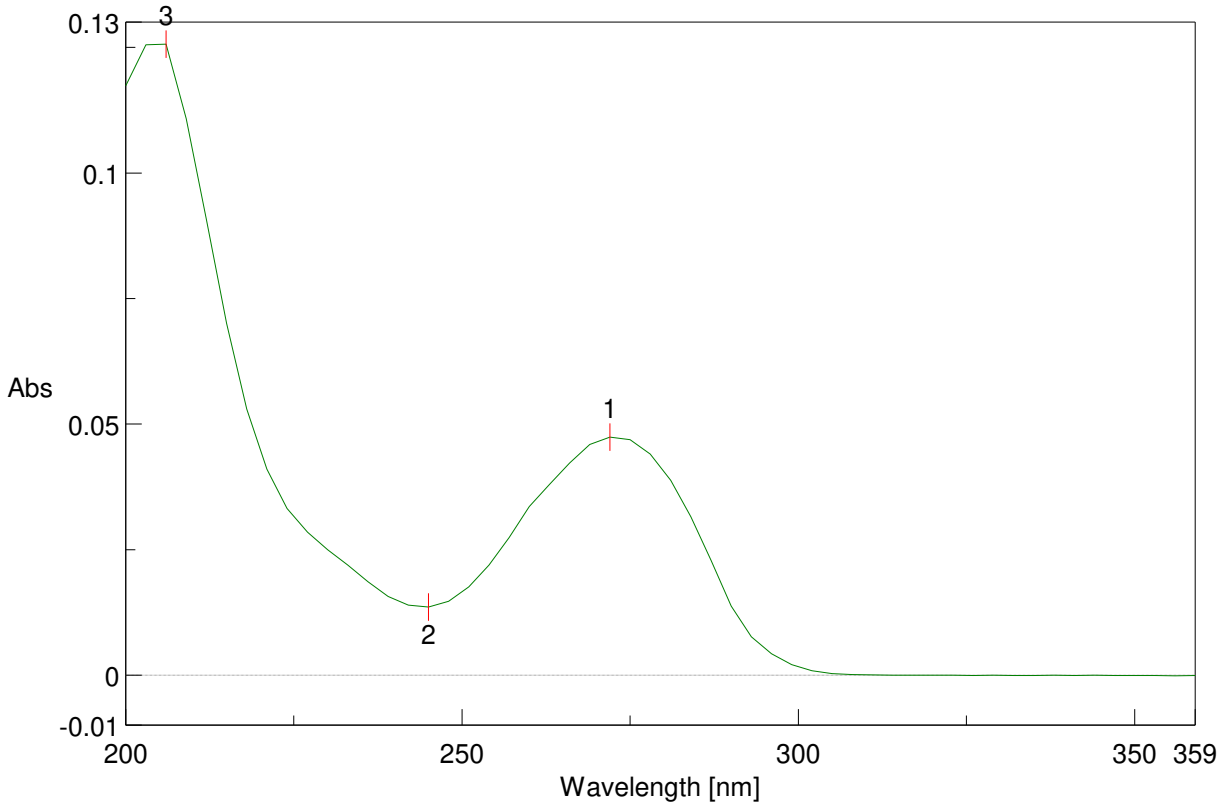

[Comments]

User	Administrator
Division	---
Company	Valer Laboratorios
Creation date	12/17/2019 2:55 PM

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	359 nm
Data interval	3 nm
Data points	54


[Measurement Information]

Instrument Name	MD-2015
Model Name	MD-2015
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.047358	2	245	0.013521
3	206	0.125596			

Chromatogram

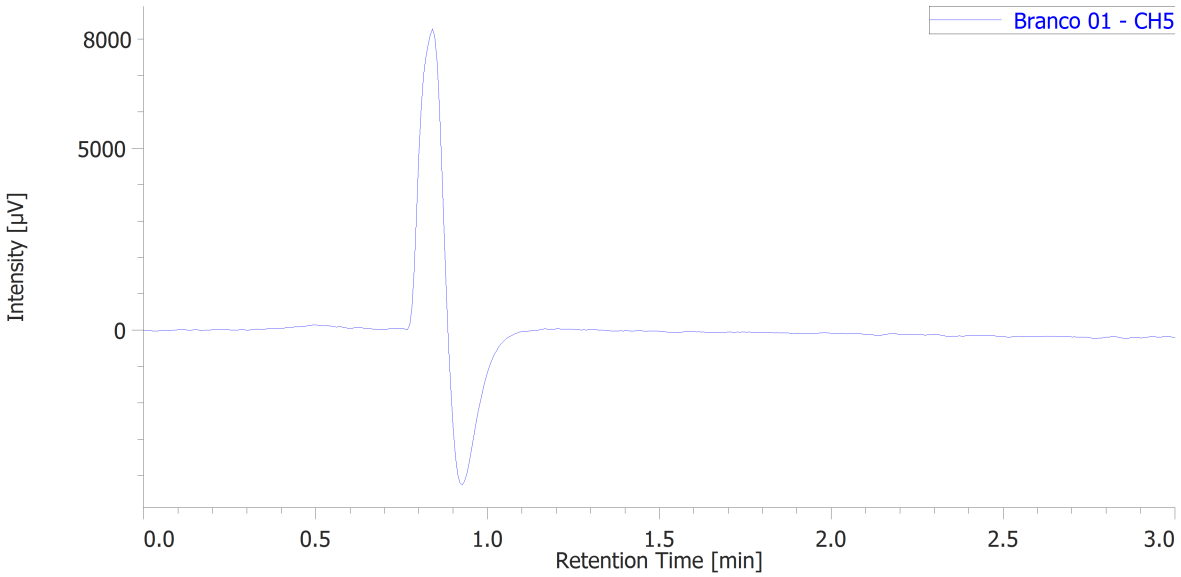


Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:33:20 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:30:20 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

Creator Administrator

Chromatogram

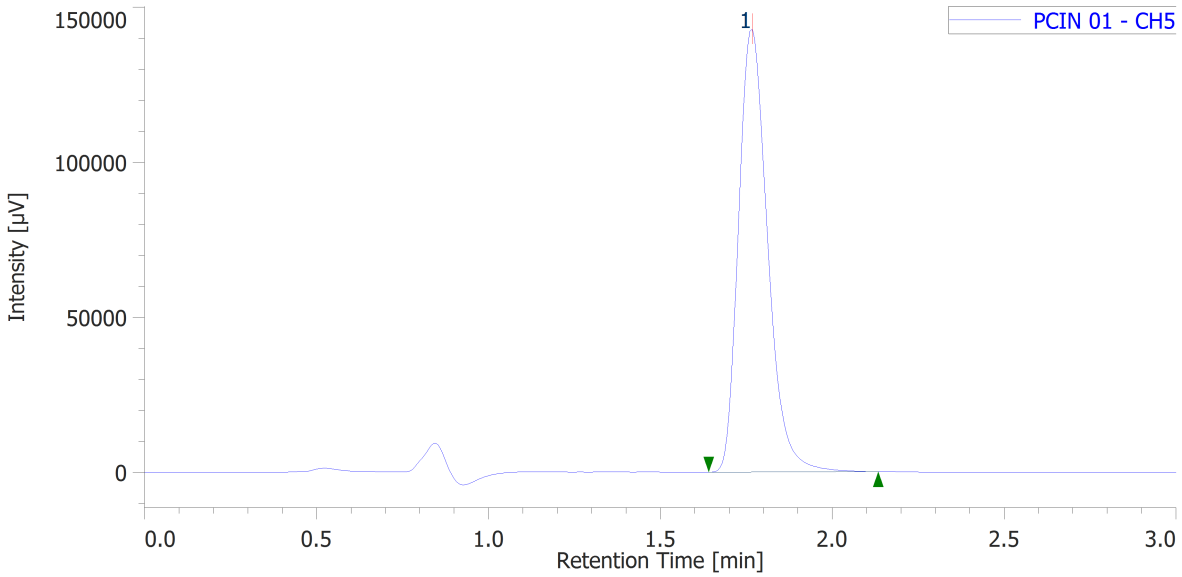

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:37:41 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:34:41 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	838997	142849	100.000	100.000	N/A	2148	N/A	1.246	

Creator Administrator

Chromatogram

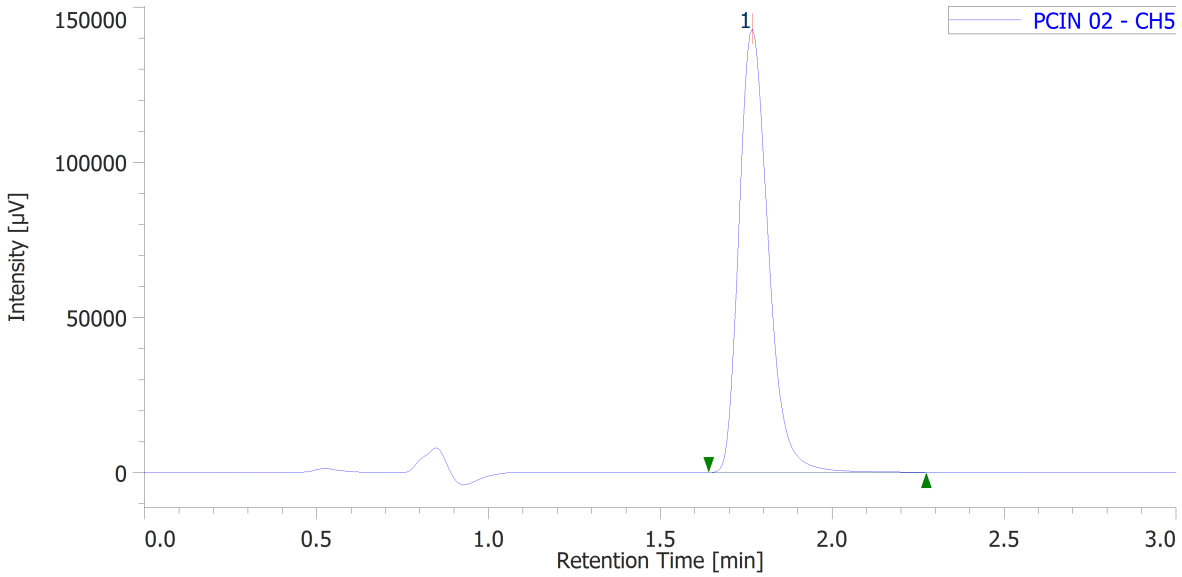

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:41:52 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:38:53 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	841132	142746	100.000	100.000	N/A	2145	N/A	1.270	

Creator Administrator

Chromatogram

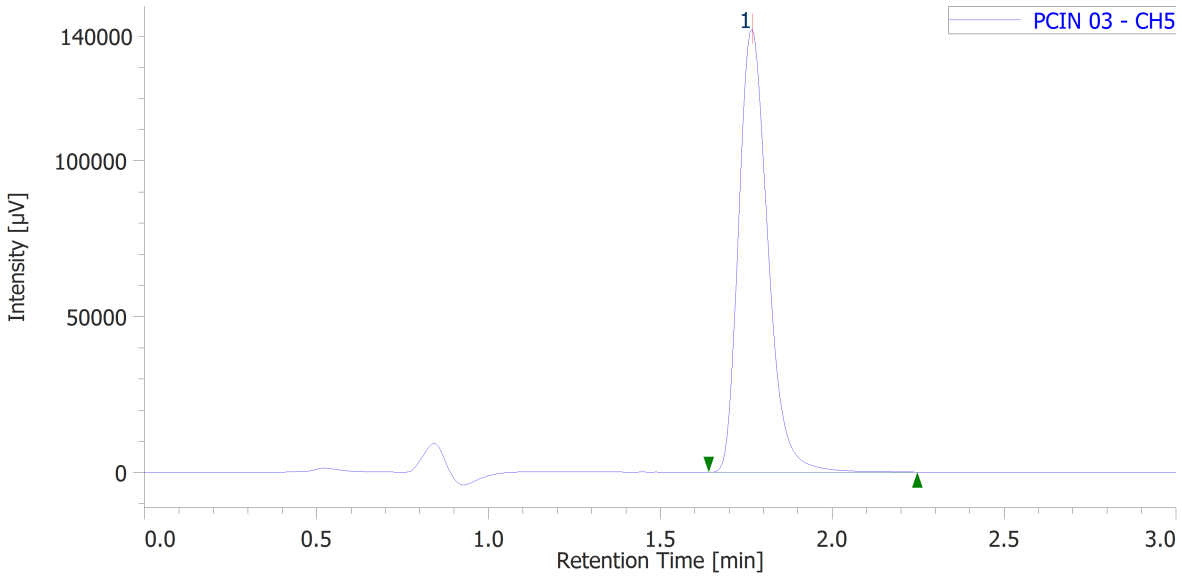

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:46:00 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:43:00 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	838178	142114	100.000	100.000	N/A	2140	N/A	1.254	

Creator Administrator

Chromatogram

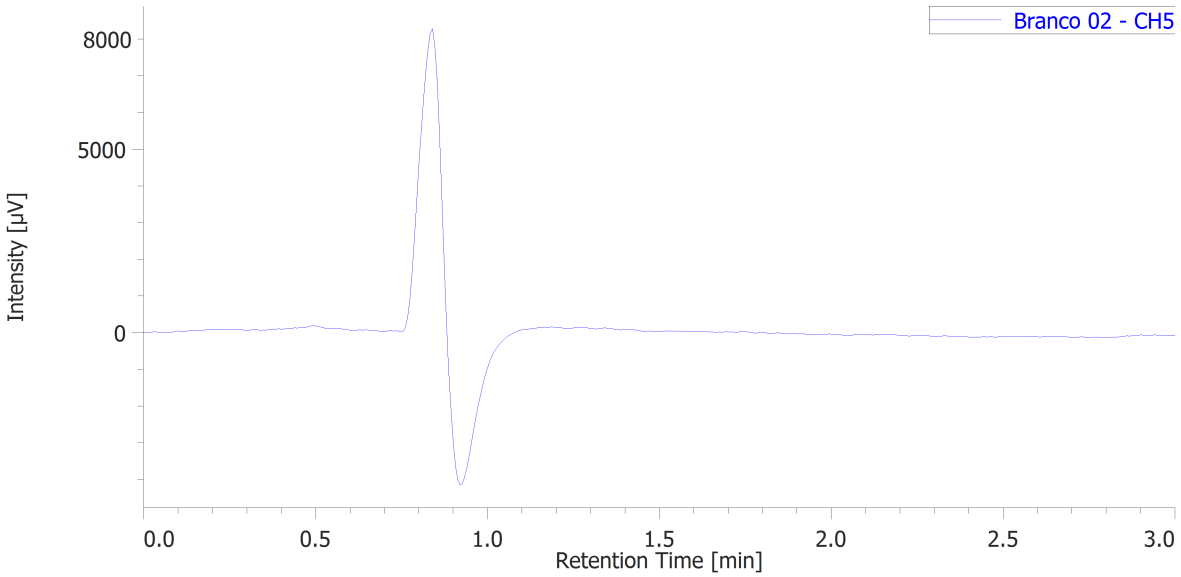


Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:50:14 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:47:15 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

Creator Administrator

Chromatogram

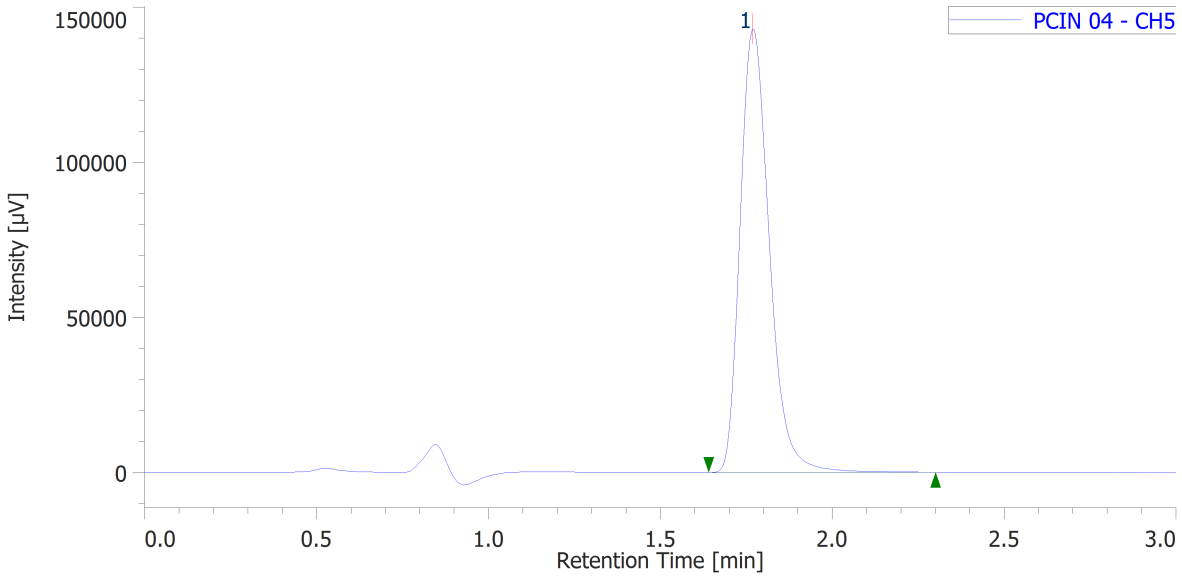

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:54:25 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:51:25 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	843176	142809	100.000	100.000	N/A	2149	N/A	1.328	

Creator Administrator

Chromatogram

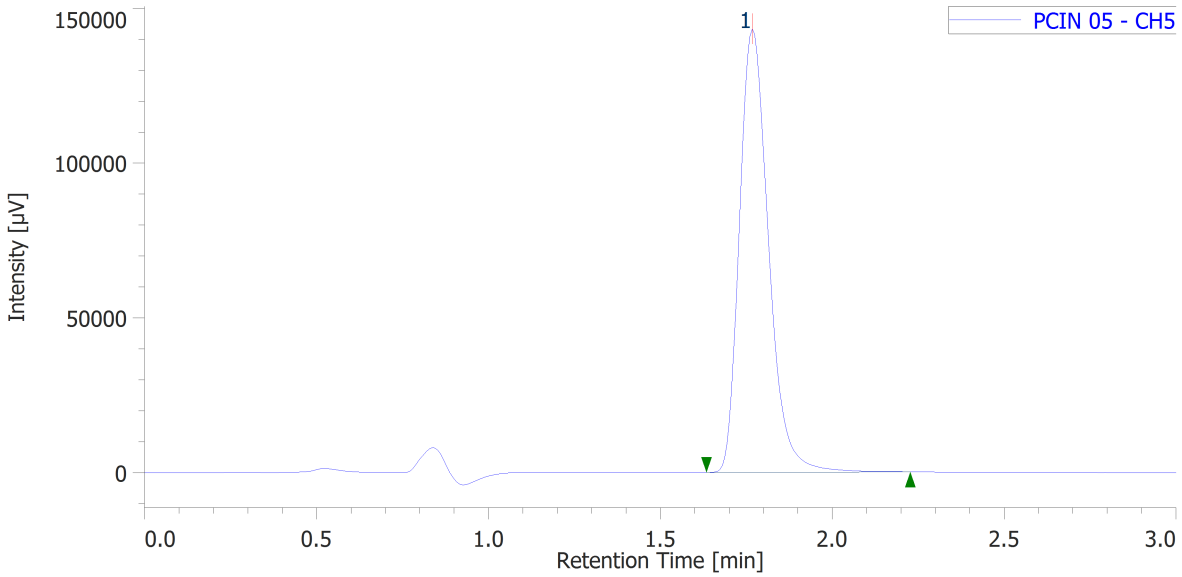

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 3:59:03 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:55:37 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	840572	143070	100.000	100.000	N/A	2161	N/A	1.287	

Creator Administrator

Chromatogram

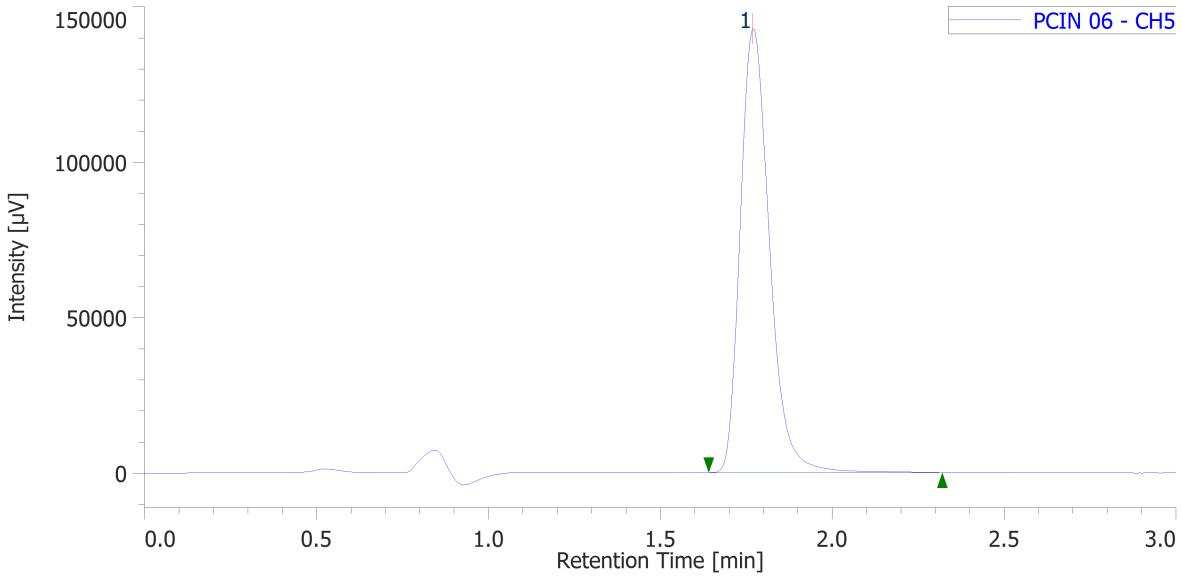

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:02:47 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 3:59:47 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	844066	142646	100.000	100.000	N/A	2146	N/A	1.336	

Creator Administrator

Chromatogram

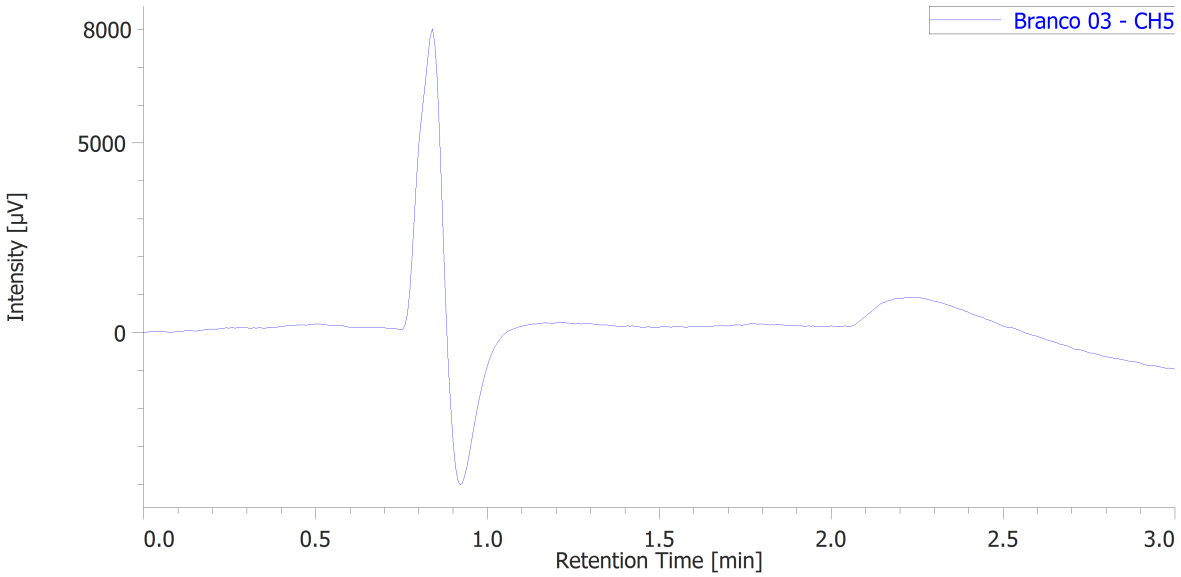


Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:07:10 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:04:01 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

Creator Administrator

Chromatogram

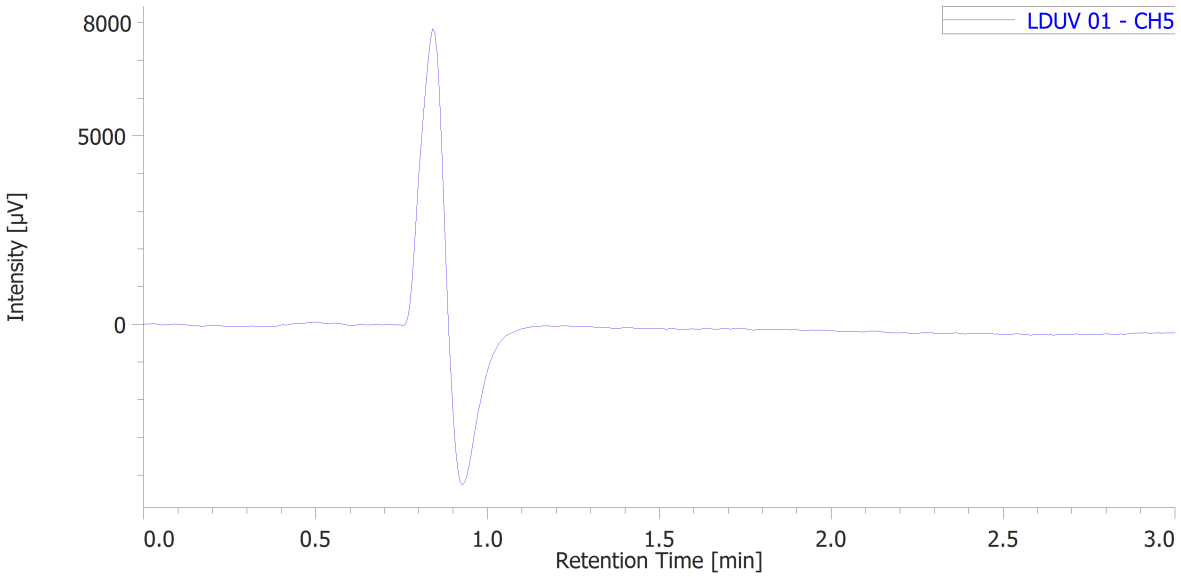


Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:29:04 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:26:05 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

Creator Administrator

Chromatogram

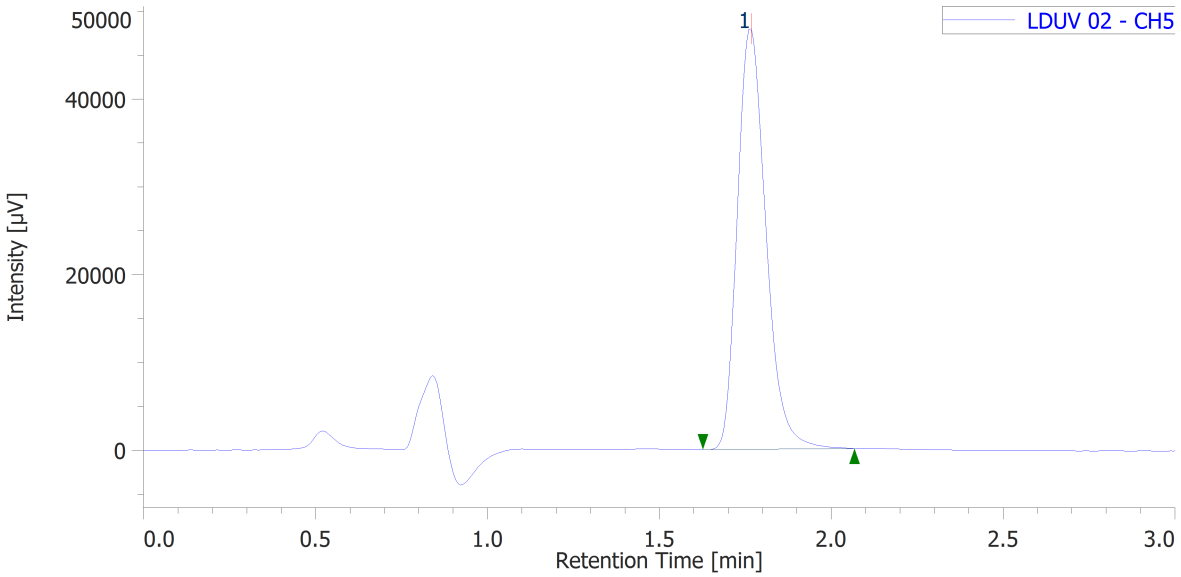

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:33:14 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:30:14 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	276900	47839	100.000	100.000	N/A	2209	N/A	1.213	

Creator Administrator

Chromatogram

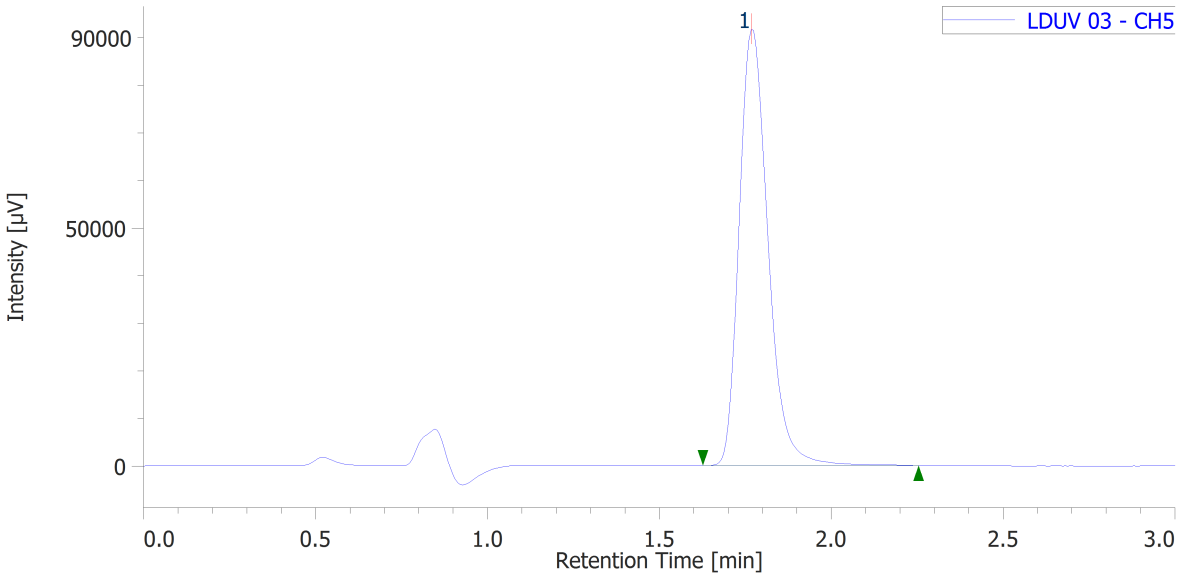

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:37:26 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:34:25 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	533506	91690	100.000	100.000	N/A	2219	N/A	1.308	

Creator Administrator

Chromatogram

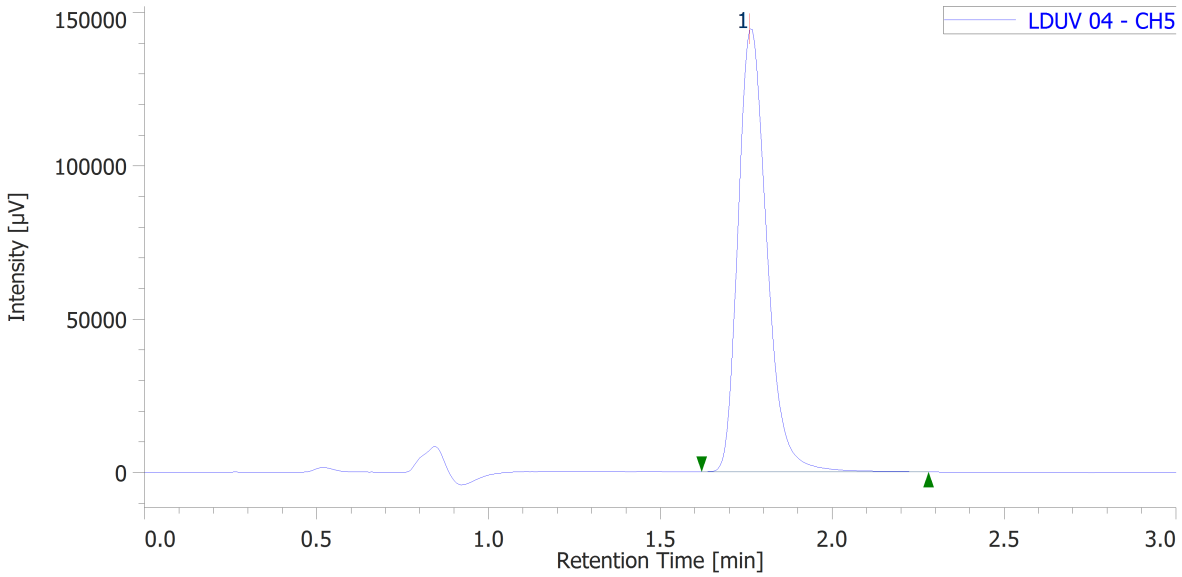

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:41:42 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:38:41 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.760	840105	144406	100.000	100.000	N/A	2209	N/A	1.319	

Creator Administrator

Chromatogram

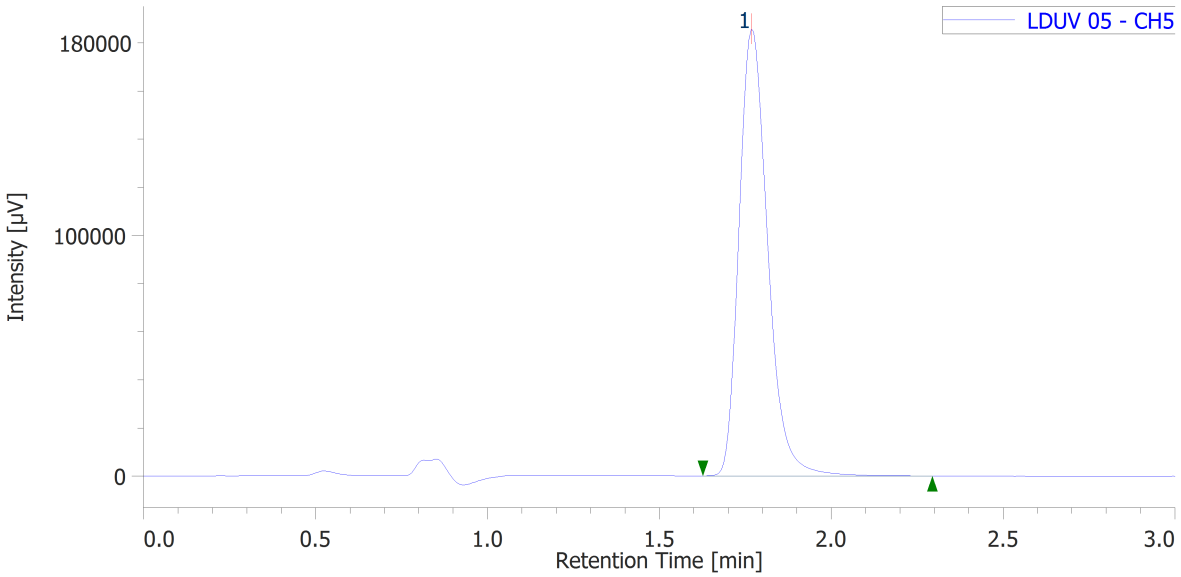

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:45:48 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:42:49 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	1075286	185596	100.000	100.000	N/A	2236	N/A	1.299	

Creator Administrator

Chromatogram

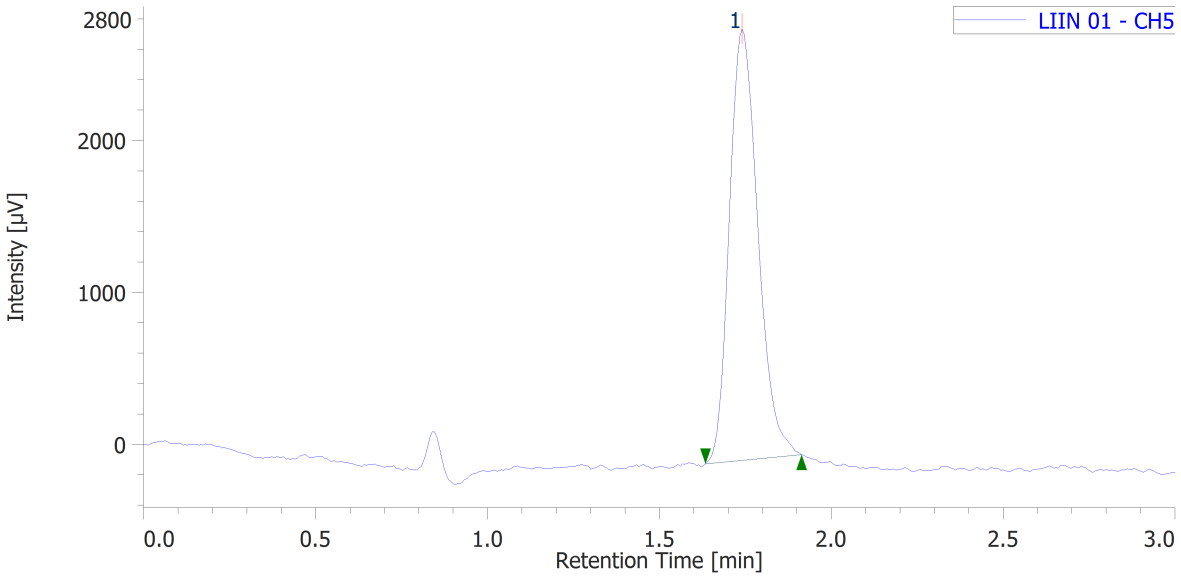

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:51:14 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:48:13 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.740	16388	2838	100.000	100.000	N/A	2104	N/A	1.259	

Creator Administrator

Chromatogram

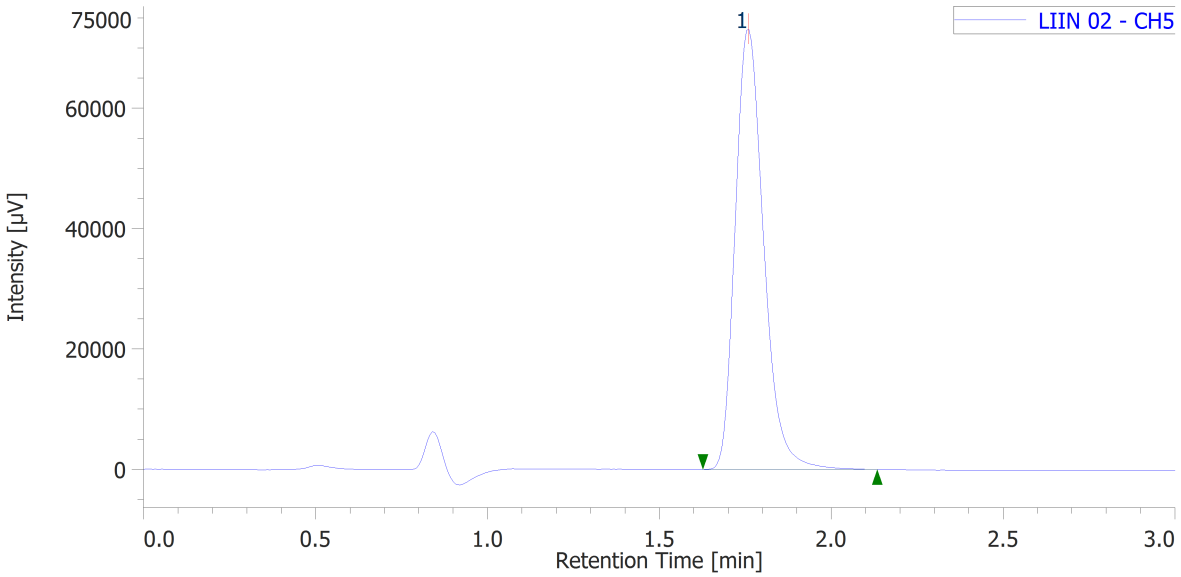

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:55:18 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:52:18 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.760	420770	73166	100.000	100.000	N/A	2240	N/A	1.220	

Creator Administrator

Chromatogram

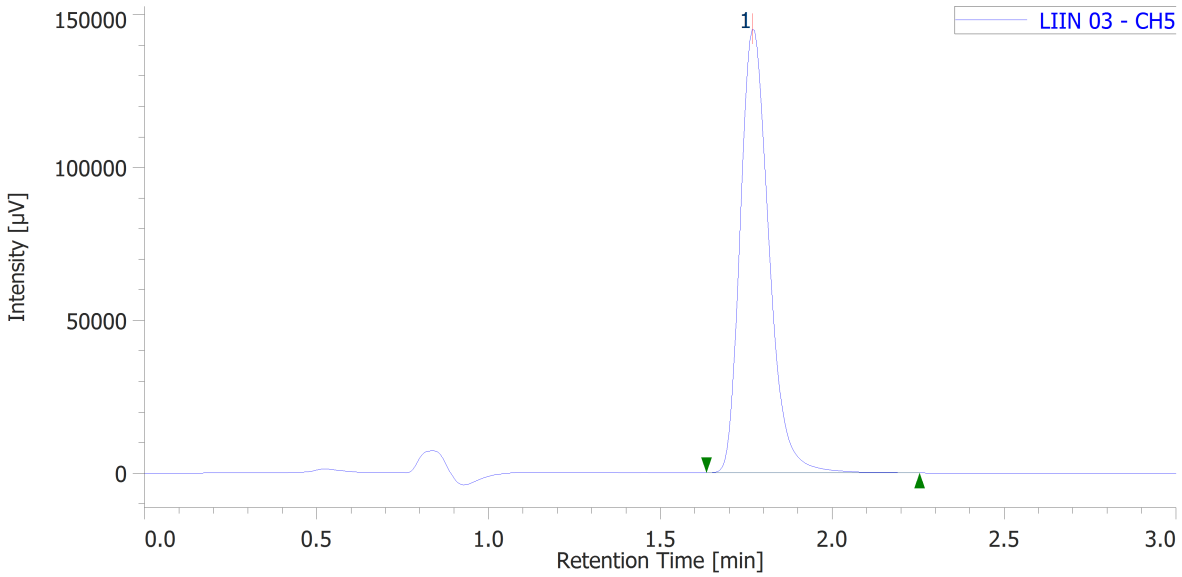

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 4:59:31 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 4:56:31 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.767	841981	145171	100.000	100.000	N/A	2229	N/A	1.310	

Creator Administrator

Chromatogram

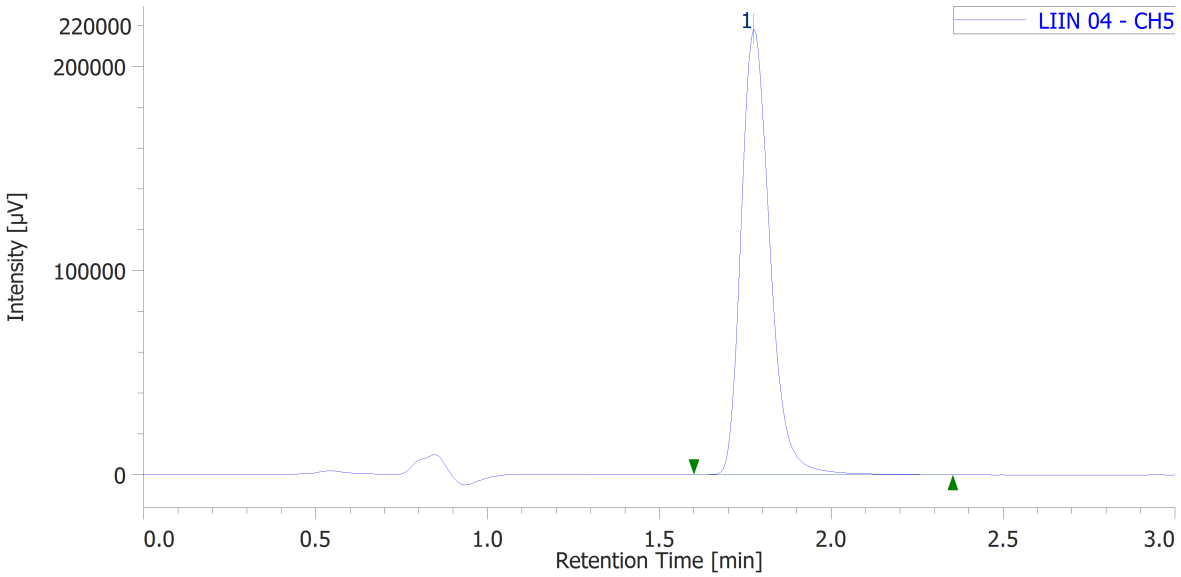

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 5:03:46 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 5:00:47 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.773	1267278	218329	100.000	100.000	N/A	2244	N/A	1.288	

Creator Administrator

Chromatogram

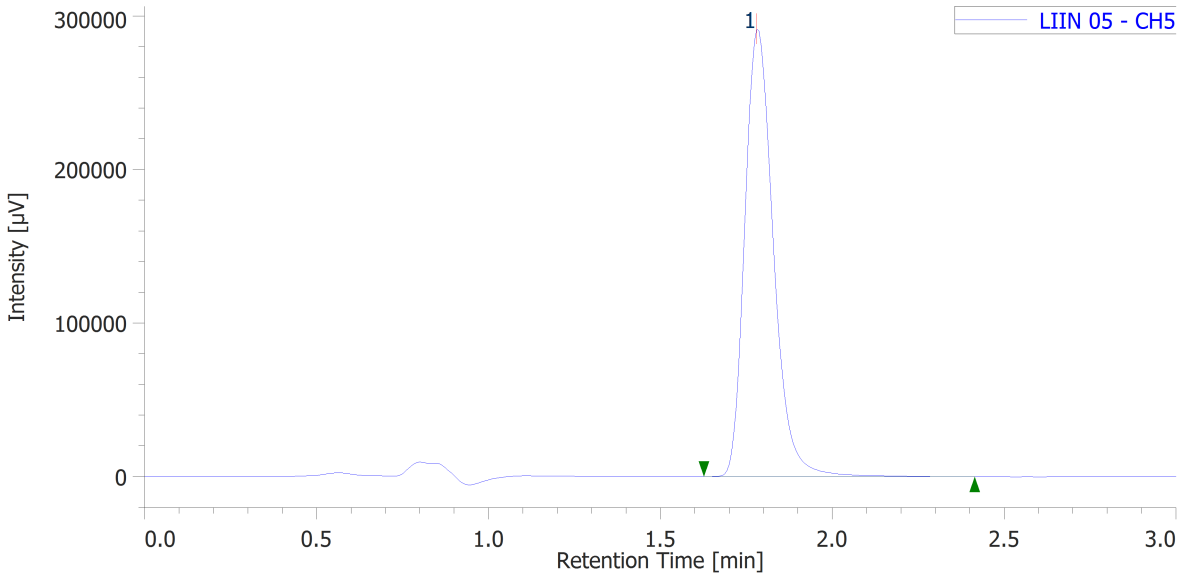

Chromatogram Information	
User Name	Administrator
Date Modified	12/17/2019 5:08:04 PM
Description	
HPLC System Name	HPL 02
Injection Date	12/17/2019 5:05:04 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação1
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.780	1688914	291397	100.000	100.000	N/A	2274	N/A	1.303	

Creator Administrator

Chromatogram

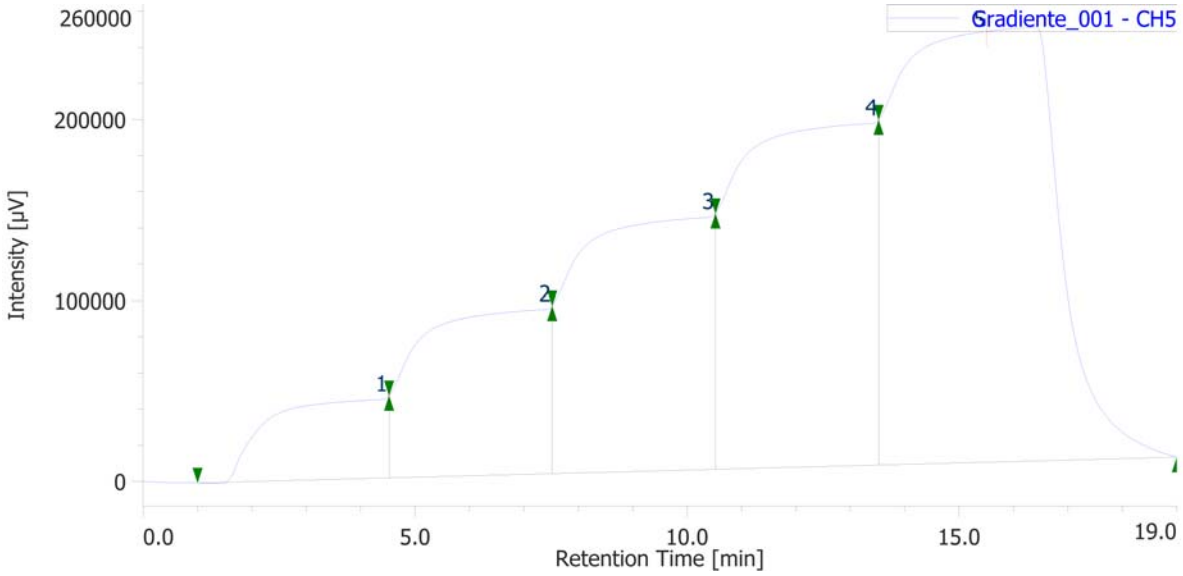

Chromatogram Information	
User Name	Administrator
Date Modified	30/03/2020 10:11:06
Description	
HPLC System Name	HPL 02
Injection Date	17/12/2019 18:26:31
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	19.0 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4.513	6390301	45213	5.071	6.392	N/A	N/A	N/A	N/A	
2	40%	5	7.513	14893326	92508	11.819	13.078	N/A	N/A	N/A	N/A	
3	60%	5	10.513	23523055	141030	18.668	19.938	N/A	N/A	N/A	N/A	
4	80%	5	13.513	32432741	190488	25.739	26.931	N/A	N/A	N/A	N/A	
5	100%	5	15.500	48769119	238094	38.703	33.661	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver