
Peak Find - Memory-1

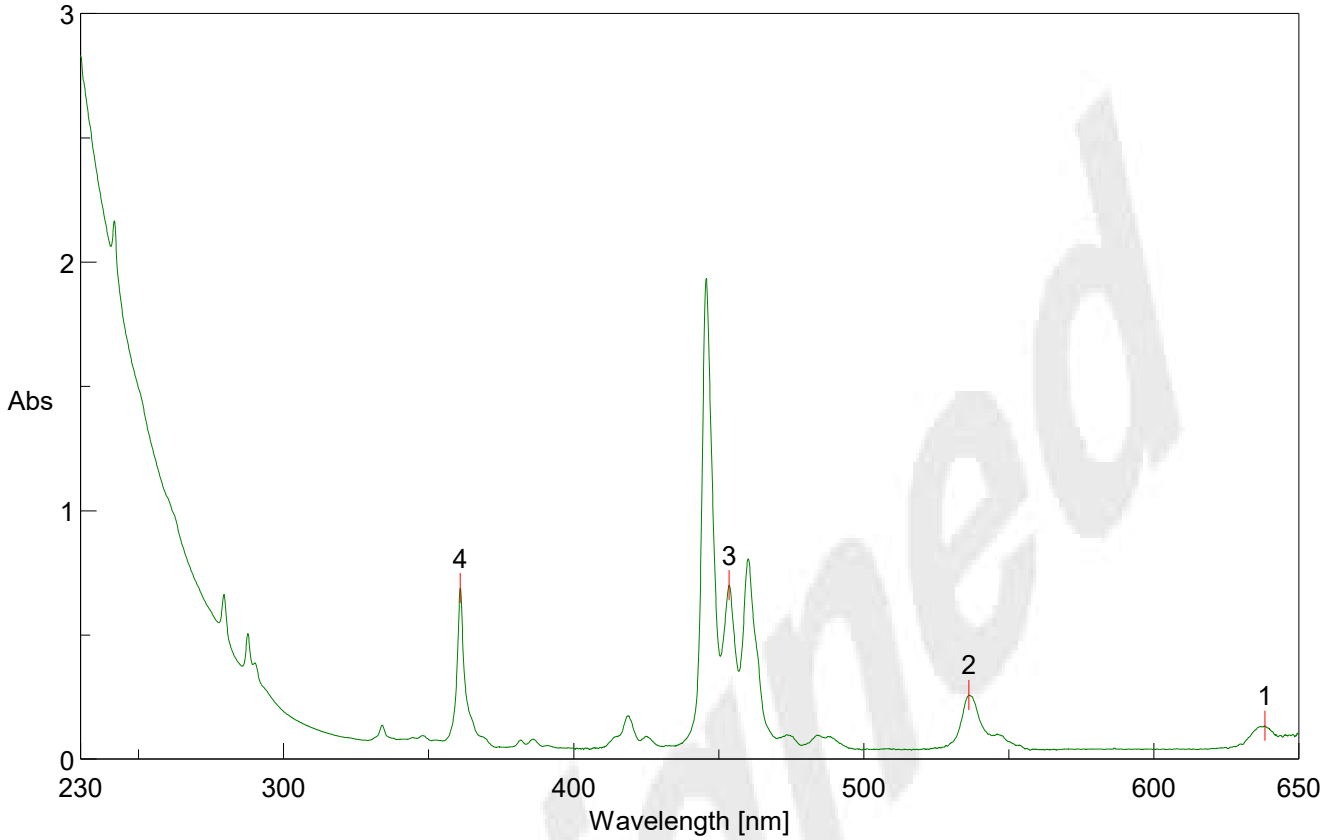

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Workgroup001
Division	Suporte Técnico
Company	FAGRON

[Detailed Information]

Creation date	31/01/2024 17:09
Date modified	31/01/2024 17:11
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201

[Measurement Information]

Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Measurement date	31/01/2024 17:09
Parameter file	C:\Workgroup001\QPack\01 - Exatidão do Comprimento de Onda.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.96 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation
Review
Approval

Unsigned


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity	No.	Position	Intensity
1	638.3	0.133937	2	536.2	0.257472	3	453.6	0.699051
4	360.9	0.68819						

Unsigned

Creation
Review
Approval

Peak Find - Memory-2

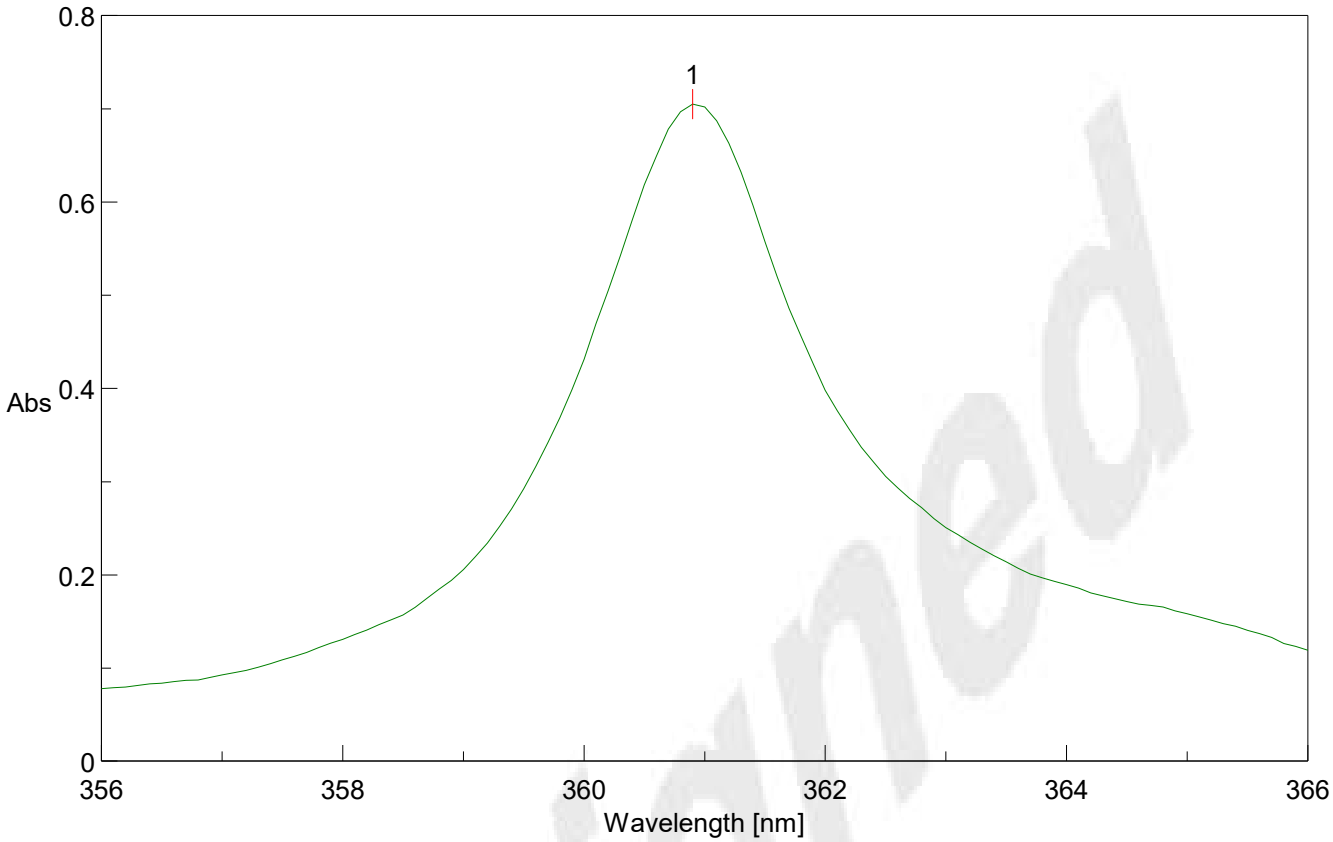

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Workgroup001
Division	Suporte Técnico
Company	FAGRON

[Detailed Information]

Creation date	31/01/2024 17:16
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Measurement date	31/01/2024 17:16
Parameter file	C:\Workgroup001\QPack\02 - Repetibilidade do Comprimento de Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation
Review
Approval

Unsigned


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.704998						

Unsigned

Creation
Review
Approval

Peak Find - Memory-3

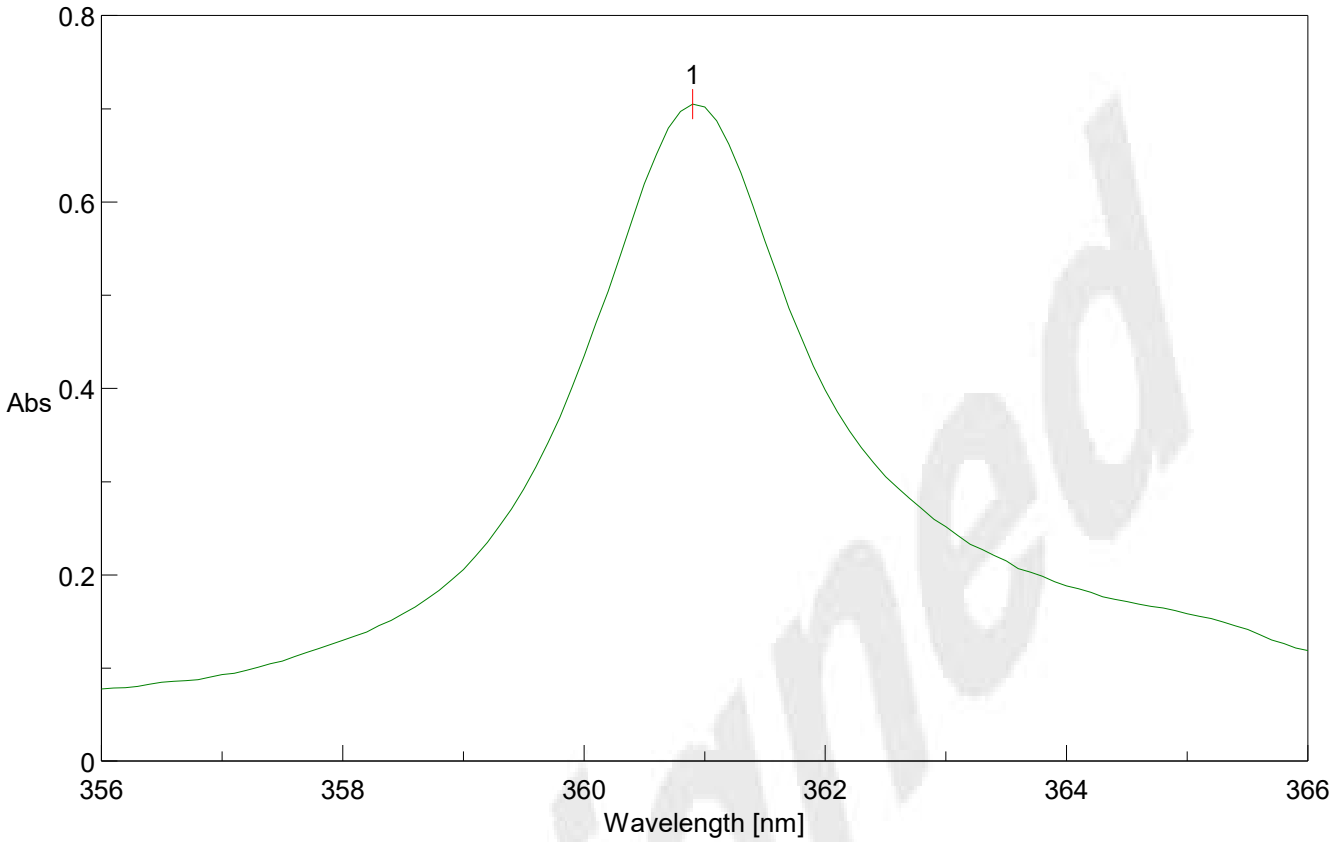

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Workgroup001
Division	Suporte Técnico
Company	FAGRON

[Detailed Information]

Creation date	31/01/2024 17:17
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Measurement date	31/01/2024 17:17
Parameter file	C:\Workgroup001\QPack\02 - Repetibilidade do Comprimento de Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation
Review
Approval

Unsigned


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.704901						

Unsigned

Creation
Review
Approval

Peak Find - Memory-4

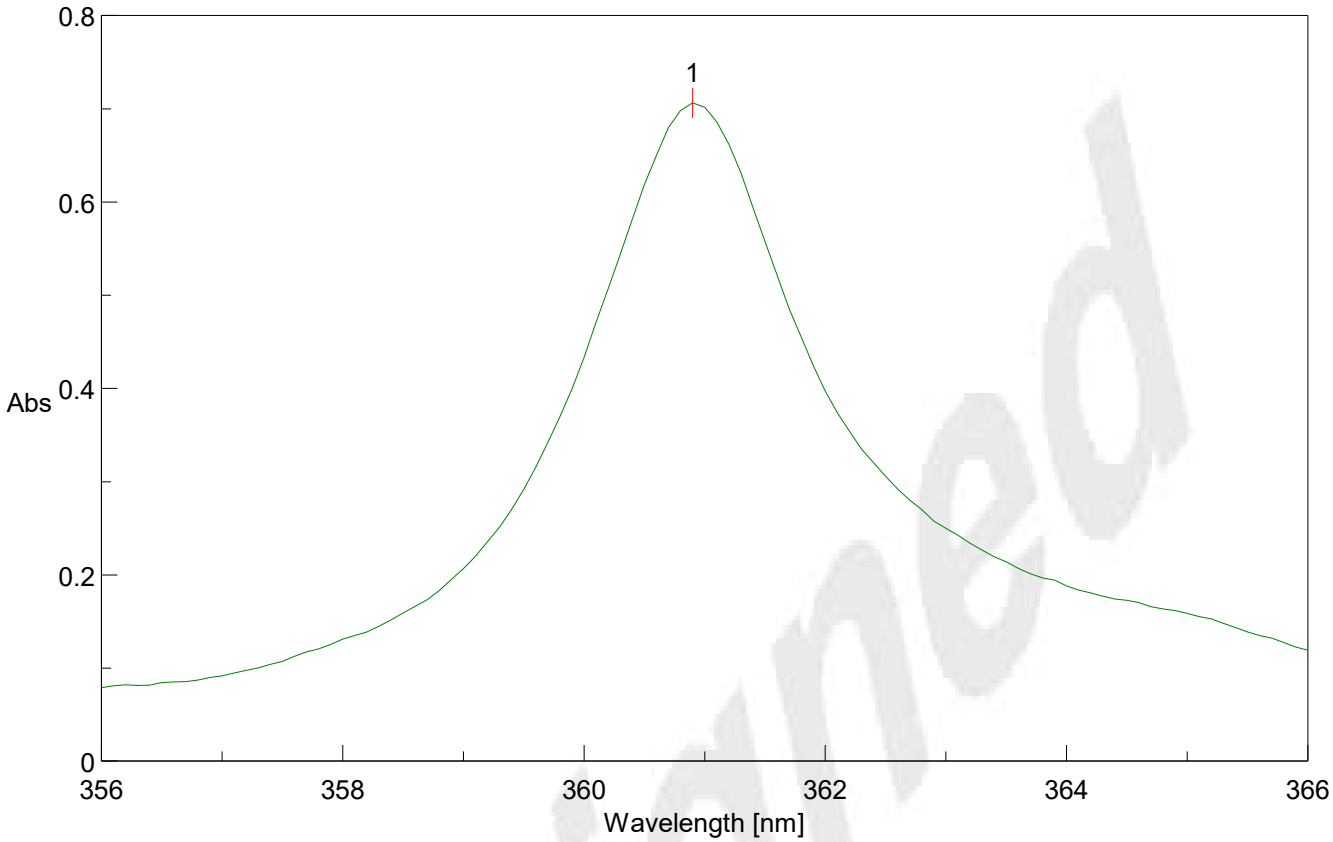

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Workgroup001
Division	Suporte Técnico
Company	FAGRON

[Detailed Information]

Creation date	31/01/2024 17:19
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Measurement date	31/01/2024 17:19
Parameter file	C:\Workgroup001\QPack\02 - Repetibilidade do Comprimento de Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation
Review
Approval

Unsigned


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.706354						

Unsigned

Creation
Review
Approval

Full Width at Half Maximum - Memory-5

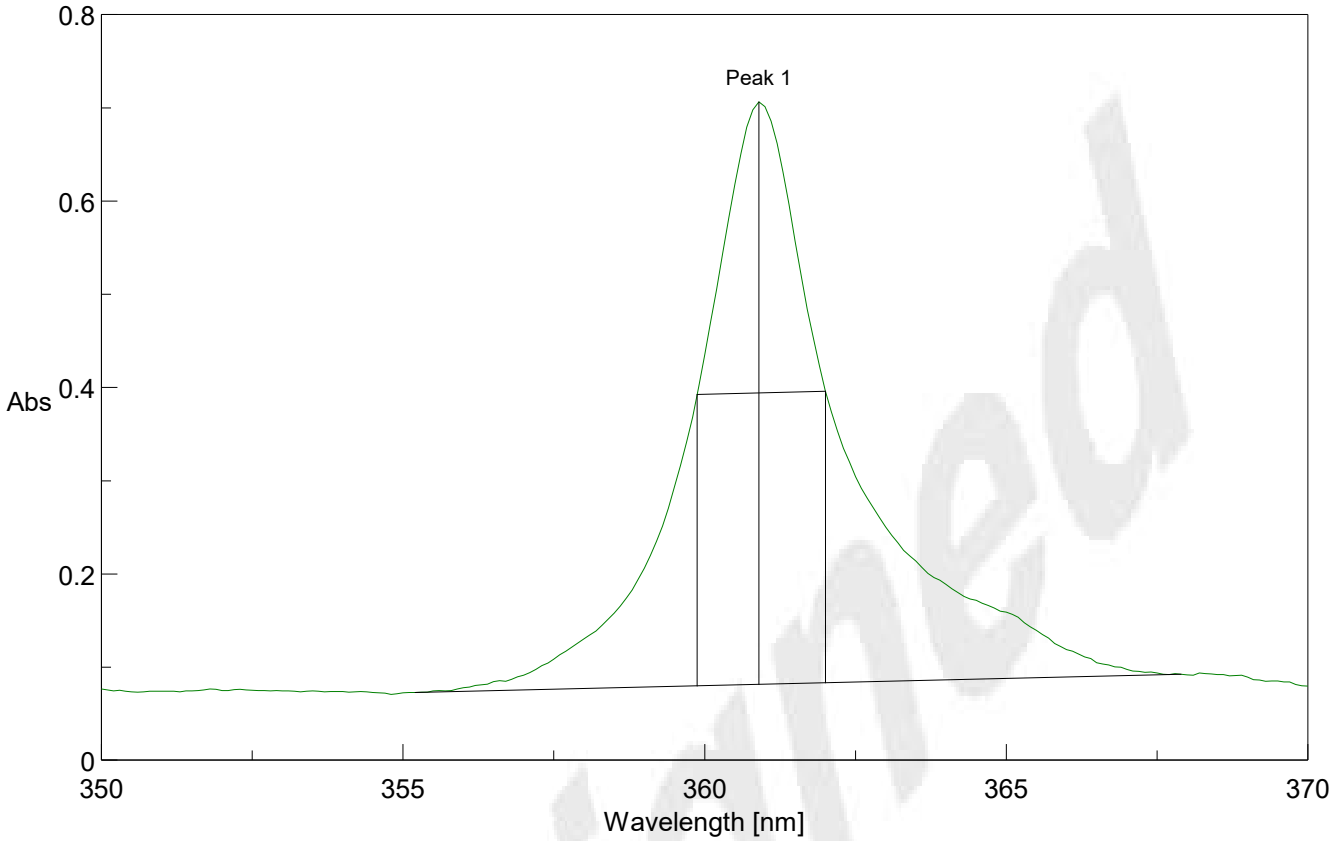

[Result of FWHM Calculation]

Base 1	Base 2	Peak	Height	FWHM
355.2	367.9	360.9	0.625017	2.13124

[Comments]
Sample name
Comment
User QPackSA
Workgroup Workgroup001
Division Suporte Técnico
Company FAGRON

[Detailed Information]
Creation date 31/01/2024 17:22
Date modified 31/01/2024 17:23

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 370 nm
End 350 nm
Data interval 0.1 nm
Data points 201

[Measurement Information]
Instrument name EQUIP-UV5
Model name V-730
Serial No. D334361798

Accessory USE-753
Accessory S/N D334361798
Cell
Ref. beam

Measurement date 31/01/2024 17:21

Parameter file C:\Workgroup001\QPack\03 - Resolução .uvsp
Photometric mode Abs
Measurement range 370 - 350 nm
Data interval 0.1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 40 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction Baseline
No. of cycles 1

Creation
Review
Approval

Unsigned

Exatidão Fotométrica

Sample name	
Comment	
User	QPackSA
Division	Suporte Técnico
Company	FAGRON
Creation date	31/01/2024 17:25
Last update	31/01/2024 17:30
Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Parameter file	C:\Workgroup001\QPack\04 Exatidão Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.96 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	On/Not measured
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Sample-1	Filtro 0		0.0380
Sample-2	Filtro 3		0.5137
Sample-3	Filtro 4		0.9904

Unsigned

Creation
Review
Approval

Sample name	
Comment	
User	QPackSA
Division	Suporte Técnico
Company	FAGRON
Creation date	31/01/2024 17:34
Last update	31/01/2024 17:35
Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Parameter file	C:\Workgroup001\QPack\05 REP Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.96 sec
Wavelength-1	361.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	On/Measured
No. of cycles	3
Cycle interval	1 sec


Mode	Sample Name	Comment	361.0 nm
Blank-1			-0.0002
ample-1-			0.7064
ample-1-2			0.7068
ample-1-3			0.7069
mple-1-Av			0.7067
mple-1-S.			0.0003
mple-1-C			0.0394

Unsigned

Creation
Review
Approval

Estabilidade da Linha de Base.jws

Date	quinta-feira, 1 de fevereiro de 2024
Model name	EQUIP-UV5
Serial No.	D334361798

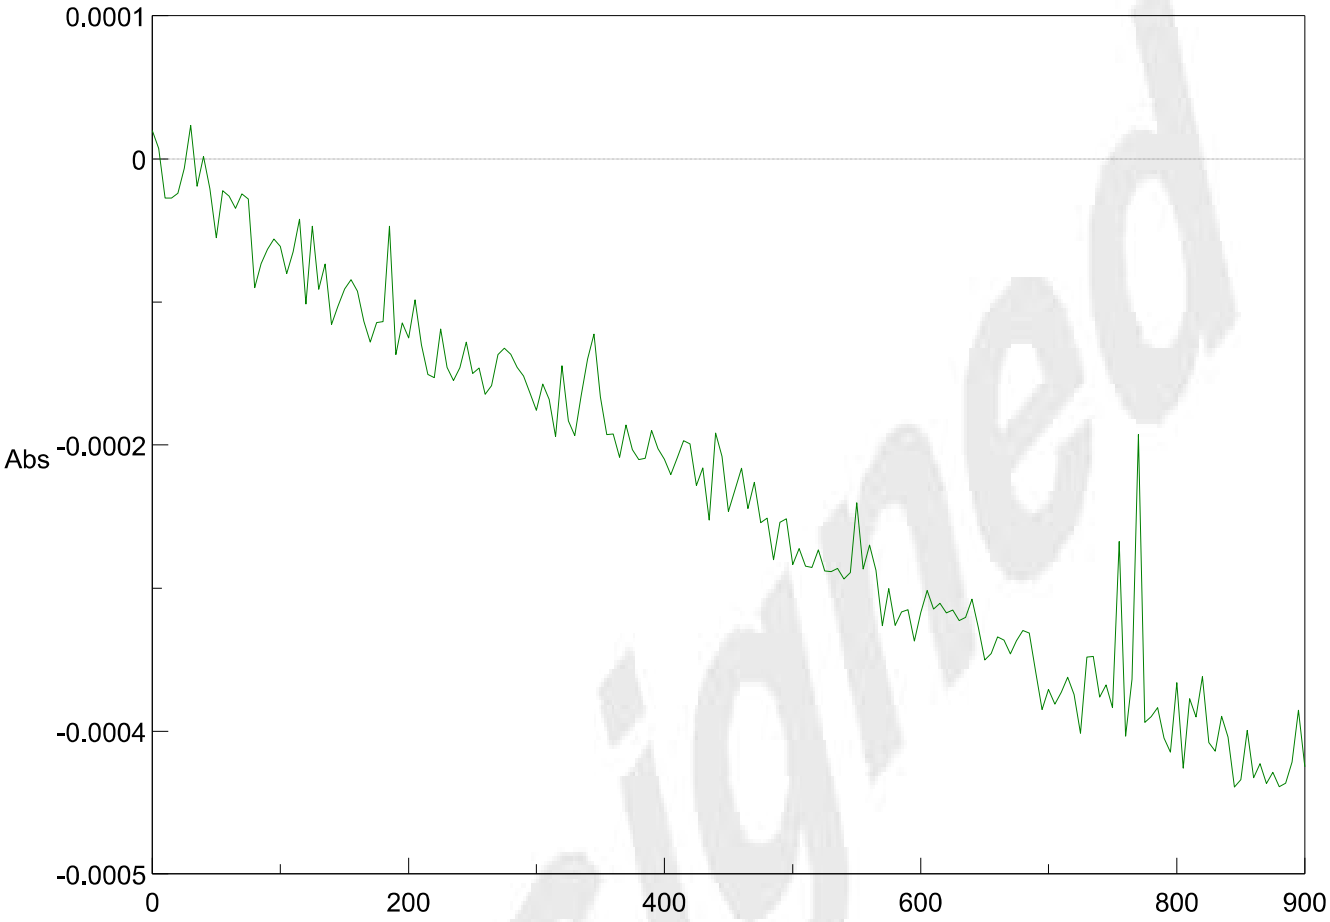


Baseline Flatness

Criteria: <= 0.00050 Abs
Minimum: -0.01332 Abs, Maximum: 0.00105 Abs, (Max.-Min.)/2: 0.00719 Abs, Fail

Unsigned

Creation
Review
Approval

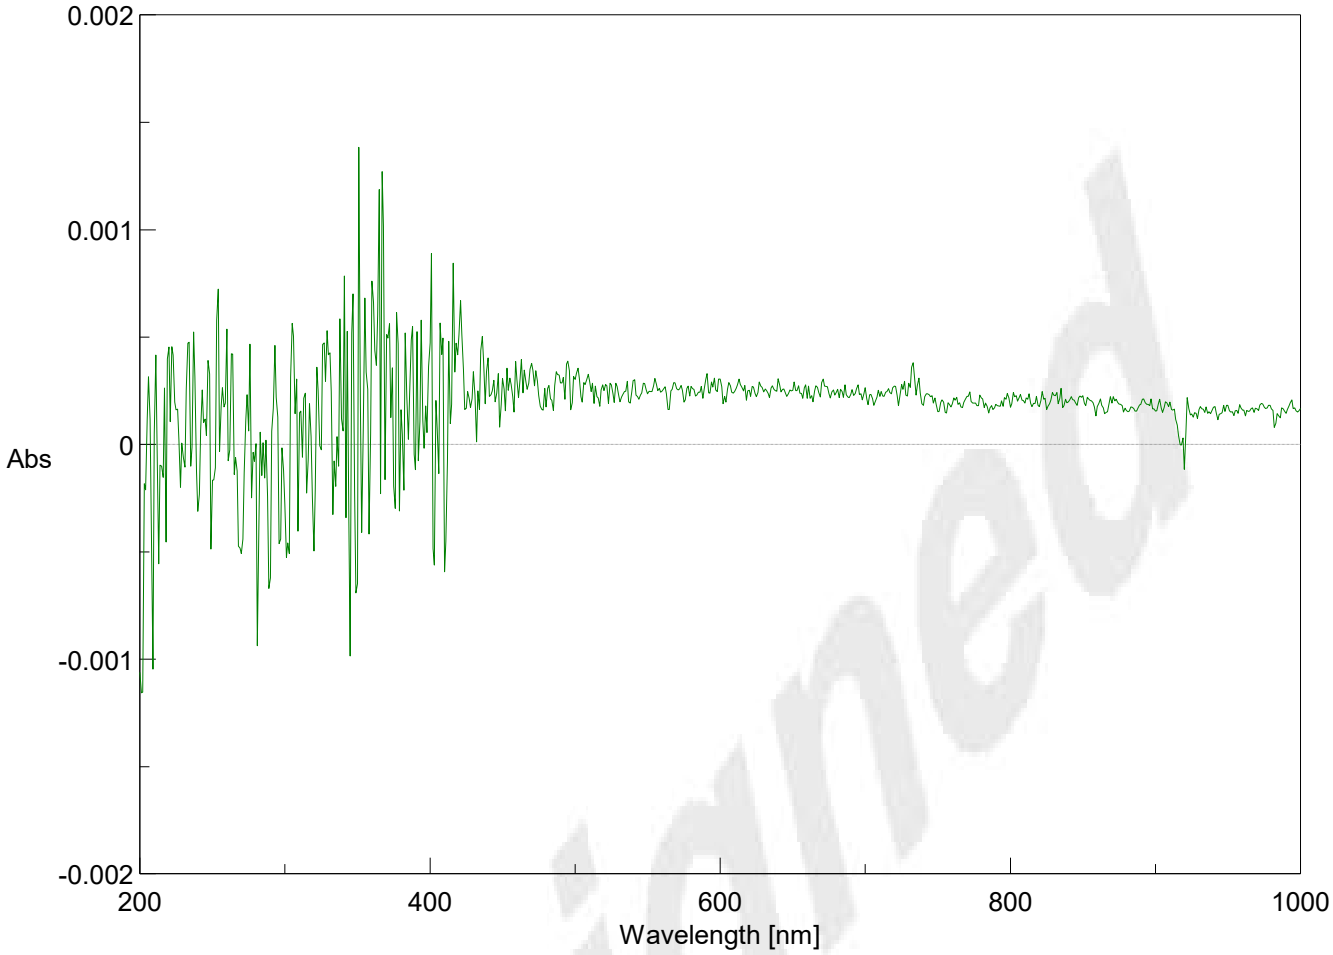

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Workgroup001
Division	Suporte Técnico
Company	FAGRON

Memory-1

[Detailed Information]

Creation date	01/02/2024 07:59
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	1000 nm
End	200 nm
Data interval	1 nm
Data points	801

[Measurement Information]

Instrument name	EQUIP-UV5
Model name	V-730
Serial No.	D334361798
Accessory	USE-753
Accessory S/N	D334361798
Cell	
Ref. beam	
Measurement date	01/02/2024 07:58
Parameter file	C:\Workgroup001\QPack\07 - Uniformidade da Linha de Base.uvsp
Photometric mode	Abs
Measurement range	1000 - 200 nm
Data interval	1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	400 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline

Creation
Review
Approval

Unsigned

No. of cycles 1

Unsigned

Creation
Review
Approval