
# Peak Find - Memory-1

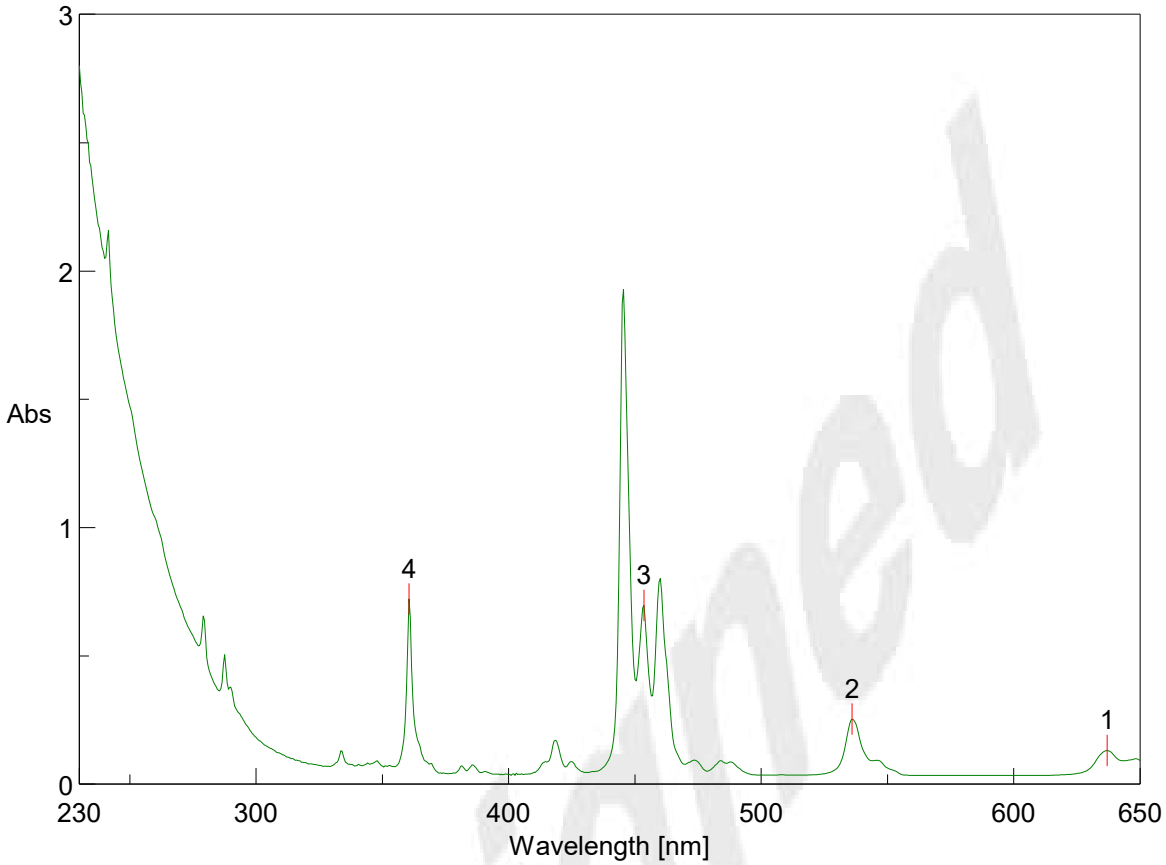


[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:07 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 650 nm |
| End | 230 nm |
| Data interval | 0.5 nm |
| Data points | 841 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:07 |
| Parameter file | C:\Workgroups\QPack\EXATIDÃO COMP ONDA.uvsp |
| Photometric mode | Abs |
| Measurement range | 650 - 230 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |
| No. of cycles | 1 |

Creation
Review
Approval

Unsigned


[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 637 | 0.130619 | 2 | 536 | 0.253251 |
| 3 | 453.5 | 0.69596 | 4 | 360.5 | 0.72077 |

Unsigned

Creation
Review
Approval

# Peak Find - Memory-2

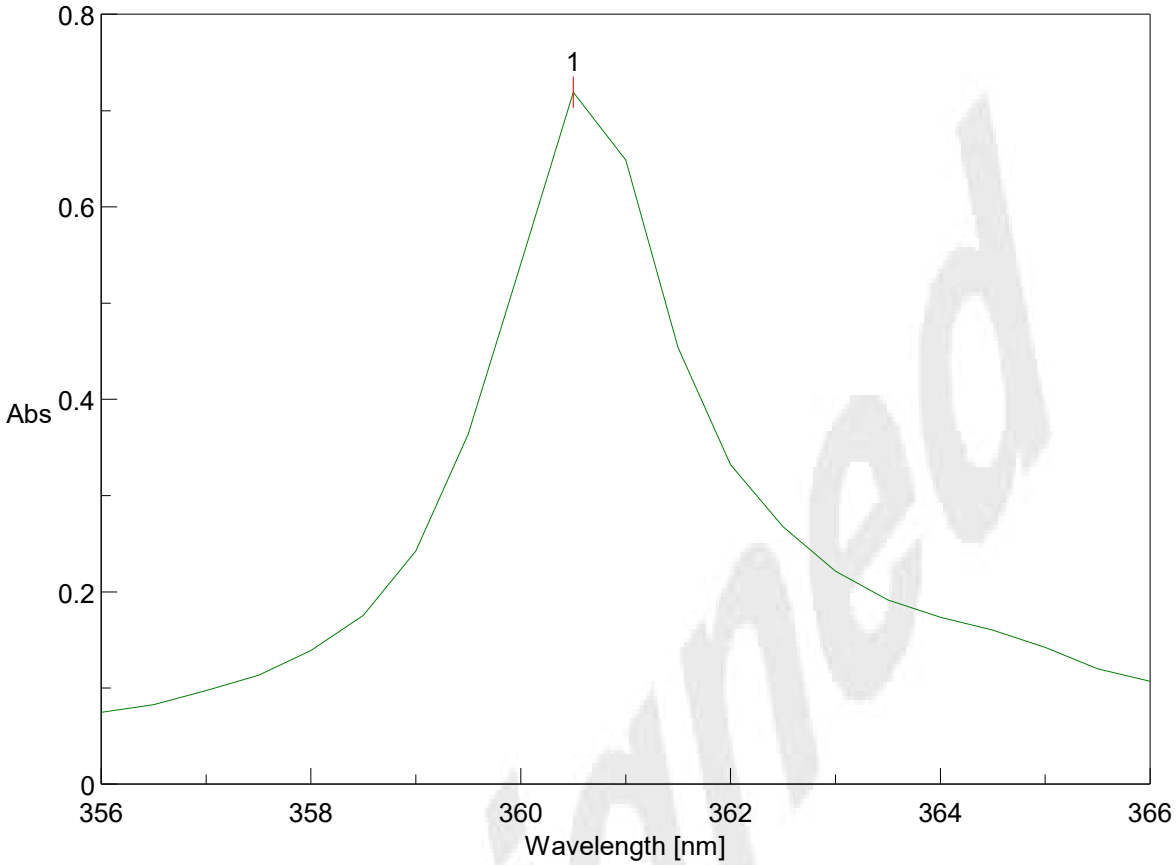


[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:11 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 366 nm |
| End | 356 nm |
| Data interval | 0.5 nm |
| Data points | 21 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:11 |
| Parameter file | C:\Workgroups\QPack\Repetibilidade do Comprimento de Onda.uvsp |
| Photometric mode | Abs |
| Measurement range | 366 - 356 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |
| No. of cycles | 1 |

Creation
Review
Approval

Unsigned


[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 360.5 | 0.718817 | | | |

Unsigned

Creation
Review
Approval

# Peak Find - Memory-3

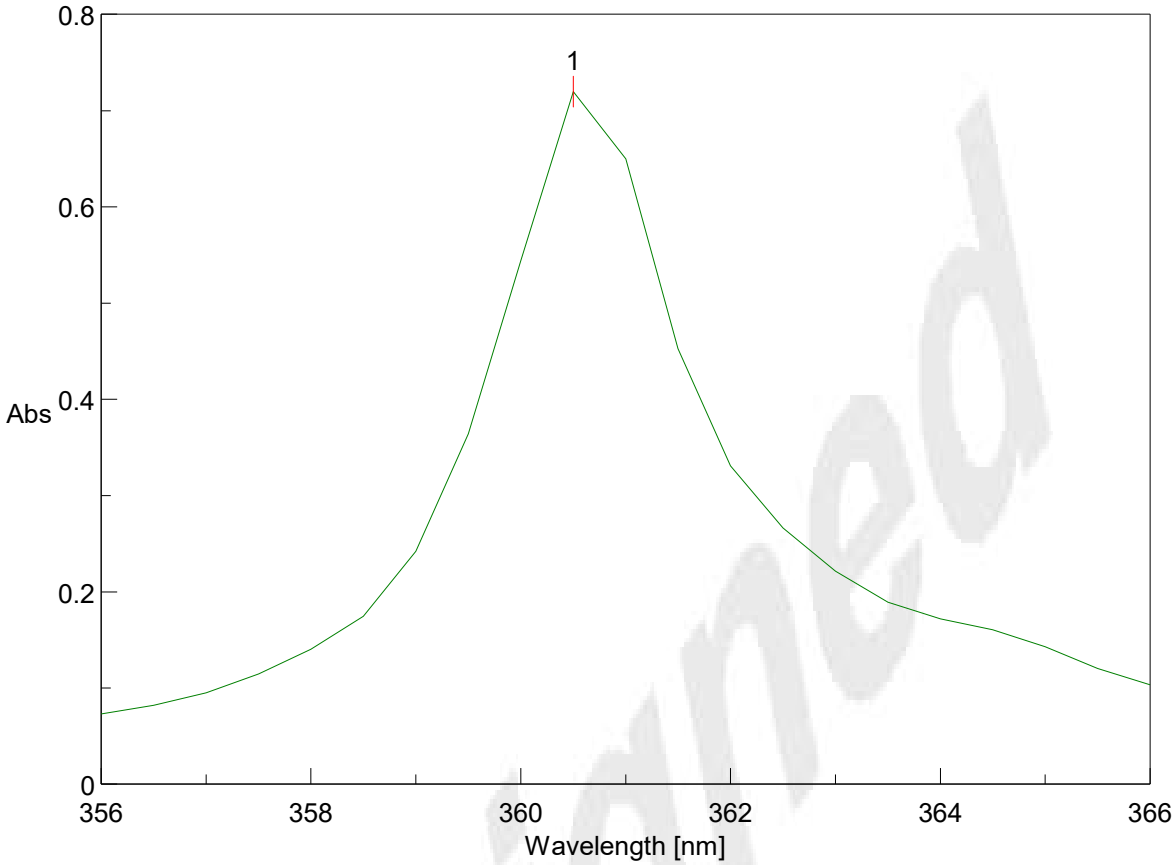


[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:13 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 366 nm |
| End | 356 nm |
| Data interval | 0.5 nm |
| Data points | 21 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:12 |

Parameter file
C:\Workgroups\QPack\Repetibilidade do Comprimento de Onda.uvsp

| | |
|---|---|
| Photometric mode | Abs |
| Measurement range | 366 - 356 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |

Creation
Review
Approval

Unsigned


[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 360.5 | 0.71957 | | | |

Unsigned

Creation
Review
Approval

# Peak Find - Memory-4

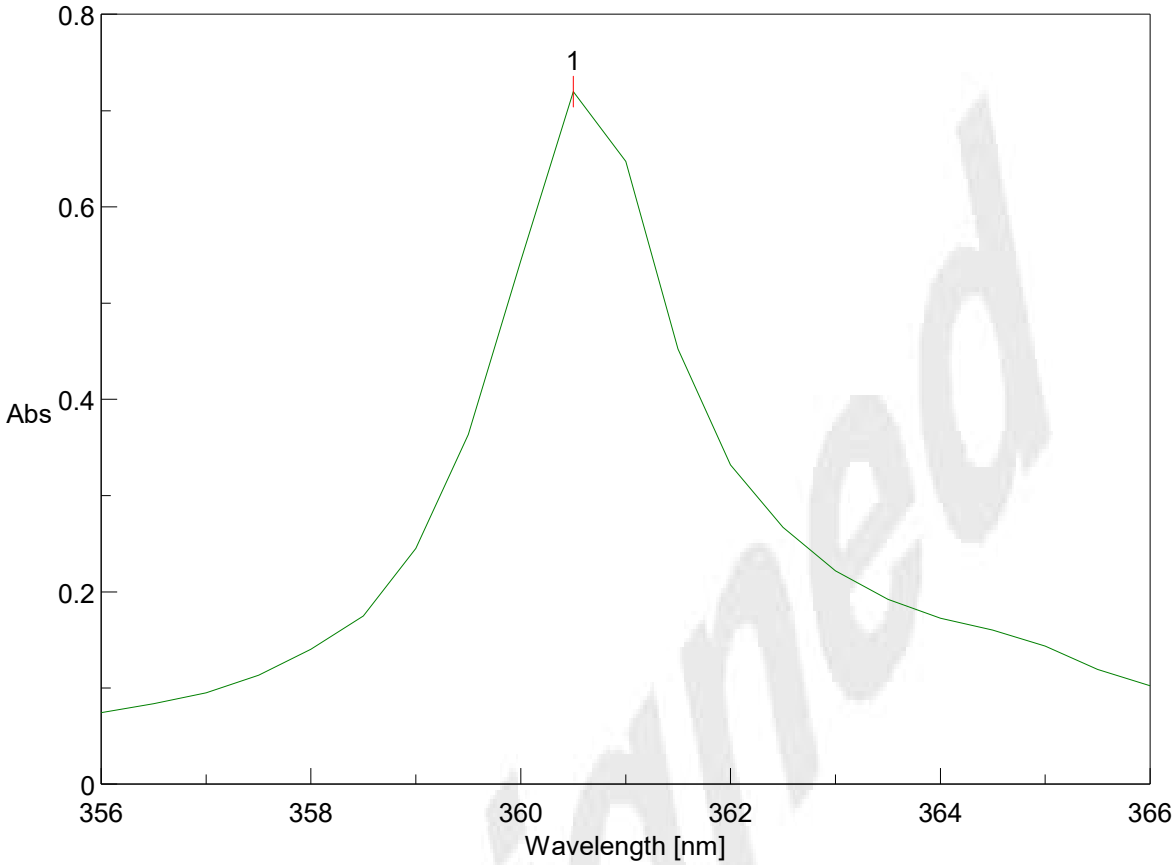


[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:14 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 366 nm |
| End | 356 nm |
| Data interval | 0.5 nm |
| Data points | 21 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:14 |

Parameter file
C:\Workgroups\QPack\Repetibilidade do Comprimento de Onda.uvsp

| | |
|---|---|
| Photometric mode | Abs |
| Measurement range | 366 - 356 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |

Creation
Review
Approval

Unsigned


[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 360.5 | 0.719481 | | | |

Unsigned

Creation
Review
Approval

## Full Width at Half Maximum - Memory-5

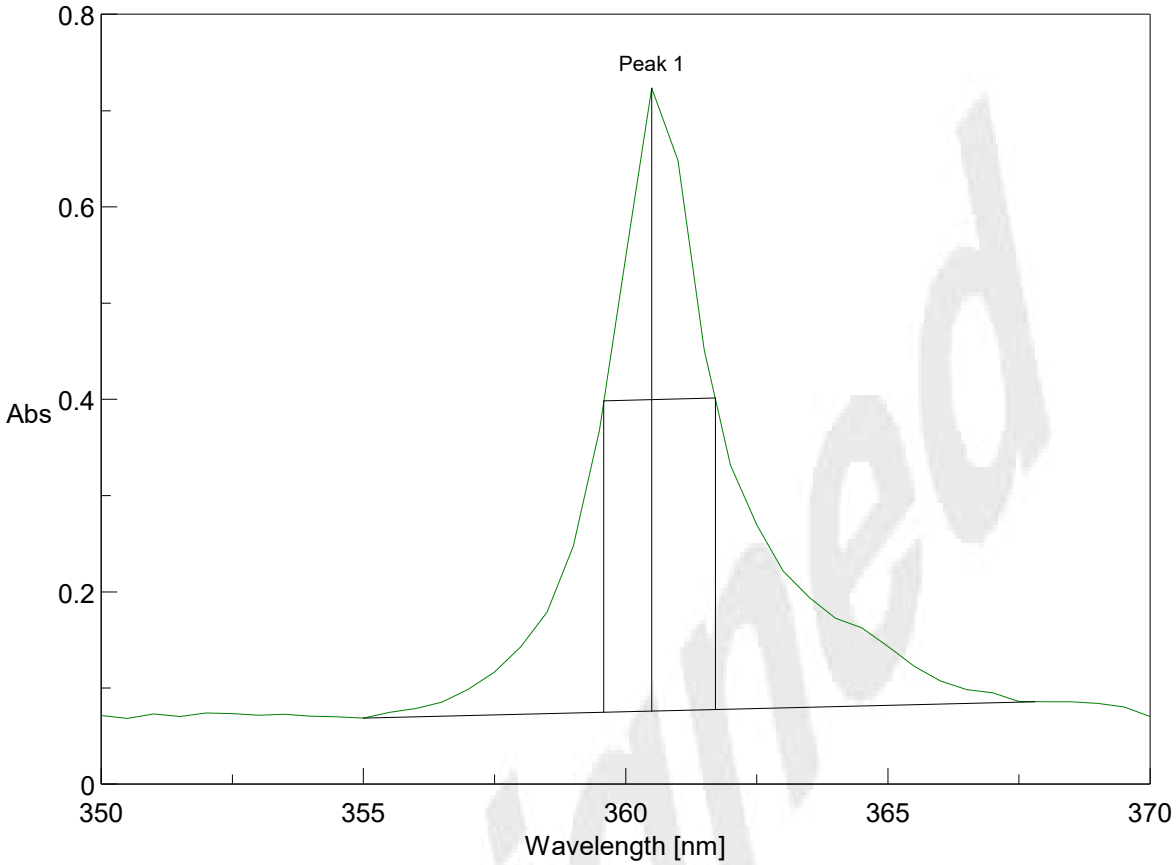


[ Result of FWHM Calculation ]

| Base 1 | Base 2 | Peak | Height | FWHM |
|---|---|---|---|---|
| 355 | 367.8 | 360.5 | 0.647466 | 2.12559 |

[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:17 |
| Date modified | 01/02/2024 12:17 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 370 nm |
| End | 350 nm |
| Data interval | 0.5 nm |
| Data points | 41 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:16 |

Parameter file
C:\Workgroups\QPack\Resolução.uvsp

| | |
|---|---|
| Photometric mode | Abs |
| Measurement range | 370 - 350 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |

Creation
Review
Approval

Unsigned

# Exatidão Fotométrica

| | |
|---|---|
| Sample name | |
| Comment | |
| User | QPackSA |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |
| | |
| Creation date | 01/02/2024 12:19 |
| Last update | 01/02/2024 12:22 |
| | |
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| ROM version | 1.02.01 |
| | |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| | |
| Parameter file | C:\Workgroups\QPack\Exatidão Fotométrica.uvfw |
| Photometric mode | Abs |
| Bandwidth | 1.0 nm |
| Response | 0.96 sec |
| Wavelength-1 | 440.0 nm |
| Change source at | 340 nm |
| Light source | D2/WI |
| Dark correction | Off |
| Blank correction | On/Measured |
| No. of cycles | 1 |

| Mode | Sample Name | Comment | 440.0 nm |
|---|---|---|---|
| Blank-1 | | | -0.0001 |
| Sample-1 | Filtro 0 | | 0.0382 |
| Sample-2 | Filtro 3 | | 0.5144 |
| Sample-3 | Fitro 4 | | 0.9844 |

Unsigned

Creation
Review
Approval

Repetibilidade Fotométrica


| | |
|---|---|
| Sample name | |
| Comment | |
| User | QPackSA |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |
| | |
| Creation date | 01/02/2024 12:24 |
| Last update | 01/02/2024 12:27 |
| | |
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| ROM version | 1.02.01 |
| | |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| | |
| Parameter file | C:\Workgroups\QPack\Repetibilidade Fotométrica.uvfw |
| Photometric mode | Abs |
| Bandwidth | 1.0 nm |
| Response | 0.96 sec |
| Wavelength-1 | 361.0 nm |
| Change source at | 340 nm |
| Light source | D2/WI |
| Dark correction | Off |
| Blank correction | On/Measured |
| No. of cycles | 1 |

| Mode | Sample Name | Comment | 361.0 nm |
|---|---|---|---|
| Blank-1 | | | 0.0001 |
| Sample-1 | Repetibilidade Fotométrica_01 | | 0.7163 |
| Sample-2 | Repetibilidade Fotométrica_02 | | 0.7167 |
| Sample-3 | Repetibilidade Fotométrica_03 | | 0.7166 |

Unsigned

Creation
Review
Approval

## Peak Find - Memory-2

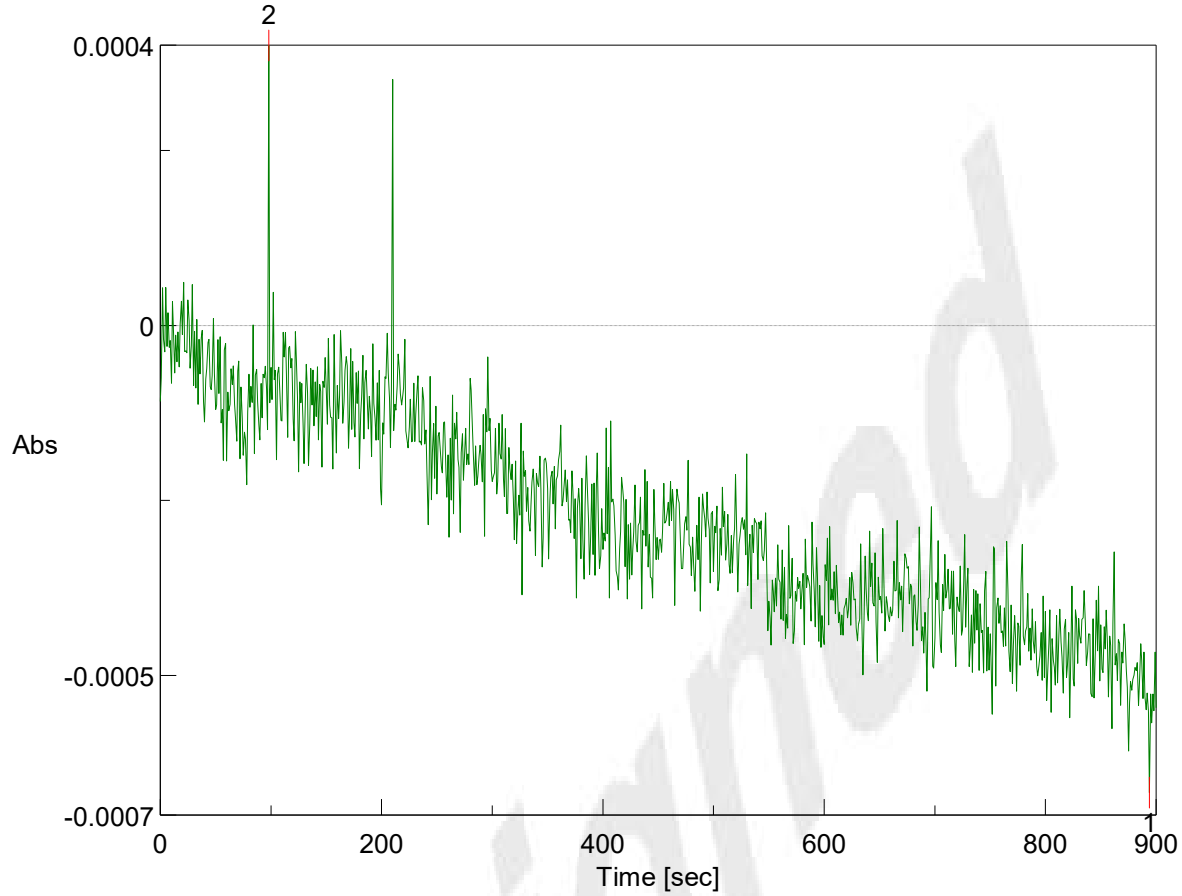


[Comments]
Sample name
Comment
User QPackSA
Workgroup QPack
Division Assistência Técnica
Company Ortofarma Laboratório de Controle de Qualidade

[Detailed Information]
Creation date 01/02/2024 12:46

Data array type Linear data array
Horizontal axis Time [sec]
Vertical axis Abs
Start 0 sec
End 900 sec
Data interval 1 sec
Data points 901

[Measurement Information]
Instrument name UV-07
Model name V-730
Serial No. D362561798

Accessory USE-753
Accessory S/N D362561798
Cell
Ref. beam

Measurement date 01/02/2024 12:45

Parameter file C:\Workgroups\QPack\Estabilidade de Linha de Base.uvtm
Photometric mode Abs
Measurement range 0 - 900 sec
Data interval 1 sec
UV/Vis bandwidth 1.0 nm
Response 0.96 sec
Monitor wavelength 250 nm
Change source at 340 nm
Light source D2/WI
Correction Blank

Creation
Review
Approval

Unsigned


[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 894 | -0.000668143 | 2 | 98 | 0.000399604 |

Unsigned

Creation
Review
Approval

# Peak Find - Memory-3

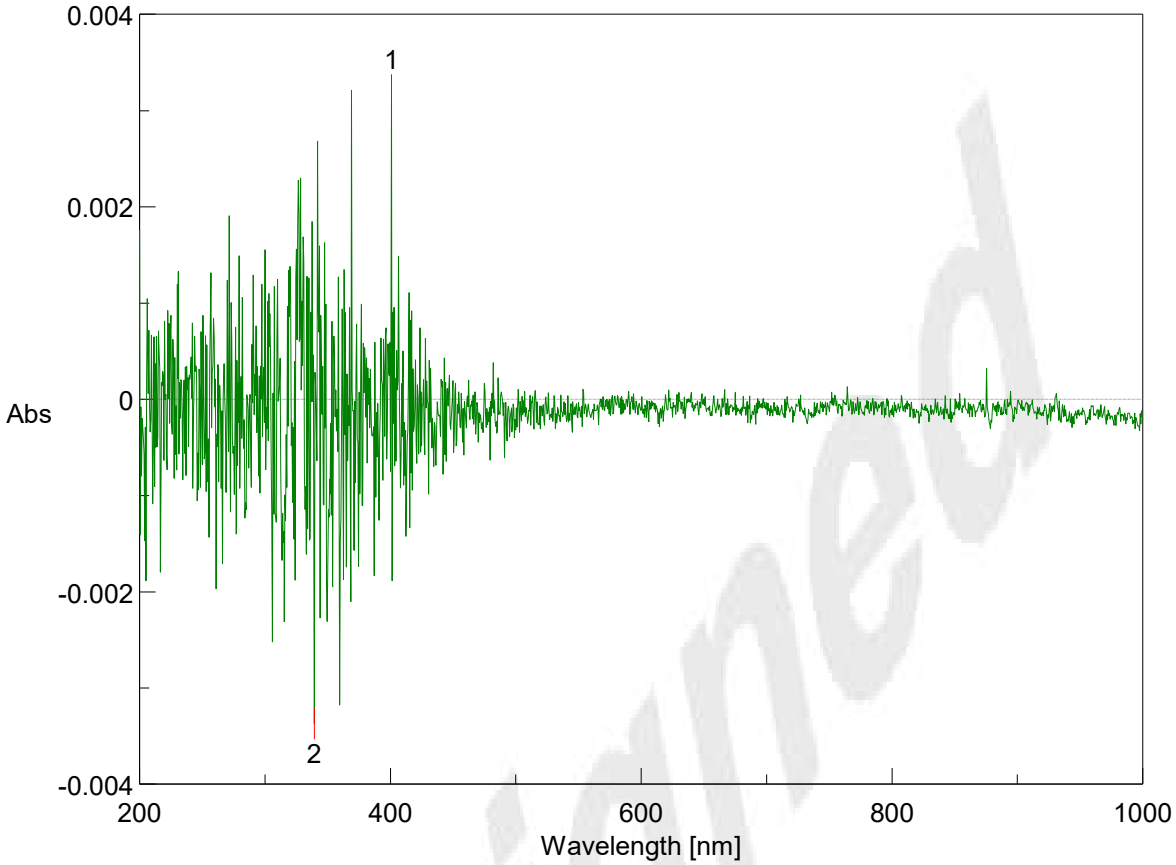


[Comments]
Sample name
Comment

| | |
|---|---|
| User | QPackSA |
| Workgroup | QPack |
| Division | Assistência Técnica |
| Company | Ortofarma Laboratório de Controle de Qualidade |

[Detailed Information]

| | |
|---|---|
| Creation date | 01/02/2024 12:55 |
| Data array type | Linear data array |
| Horizontal axis | Wavelength [nm] |
| Vertical axis | Abs |
| Start | 1000 nm |
| End | 200 nm |
| Data interval | 0.5 nm |
| Data points | 1601 |

[Measurement Information]

| | |
|---|---|
| Instrument name | UV-07 |
| Model name | V-730 |
| Serial No. | D362561798 |
| Accessory | USE-753 |
| Accessory S/N | D362561798 |
| Cell | |
| Ref. beam | |
| Measurement date | 01/02/2024 12:54 |

Parameter file
C:\Workgroups\QPack\Uniformidadae da Linha de Base.uvsp

| | |
|---|---|
| Photometric mode | Abs |
| Measurement range | 1000 - 200 nm |
| Data interval | 0.5 nm |
| Bandwidth | 1.0 nm |
| Response | 0.015 sec |
| Scan mode | Continuous |
| Scan speed | 1000 nm/min |
| Change source at | 340 nm |
| Light source | D2/WI |
| Filter exchange | Step |
| Correction | Baseline |

Creation
Review
Approval

Unsigned

[ Result of Peak Picking ]

| No. | Position | Intensity | No. | Position | Intensity |
|---|---|---|---|---|---|
| 1 | 401 | 0.00321023 | 2 | 339.5 | -0.00336967 |

Unsigned

Creation
Review
Approval