
Peak Find - EDUV_002 UV_tR1.77 D.jws

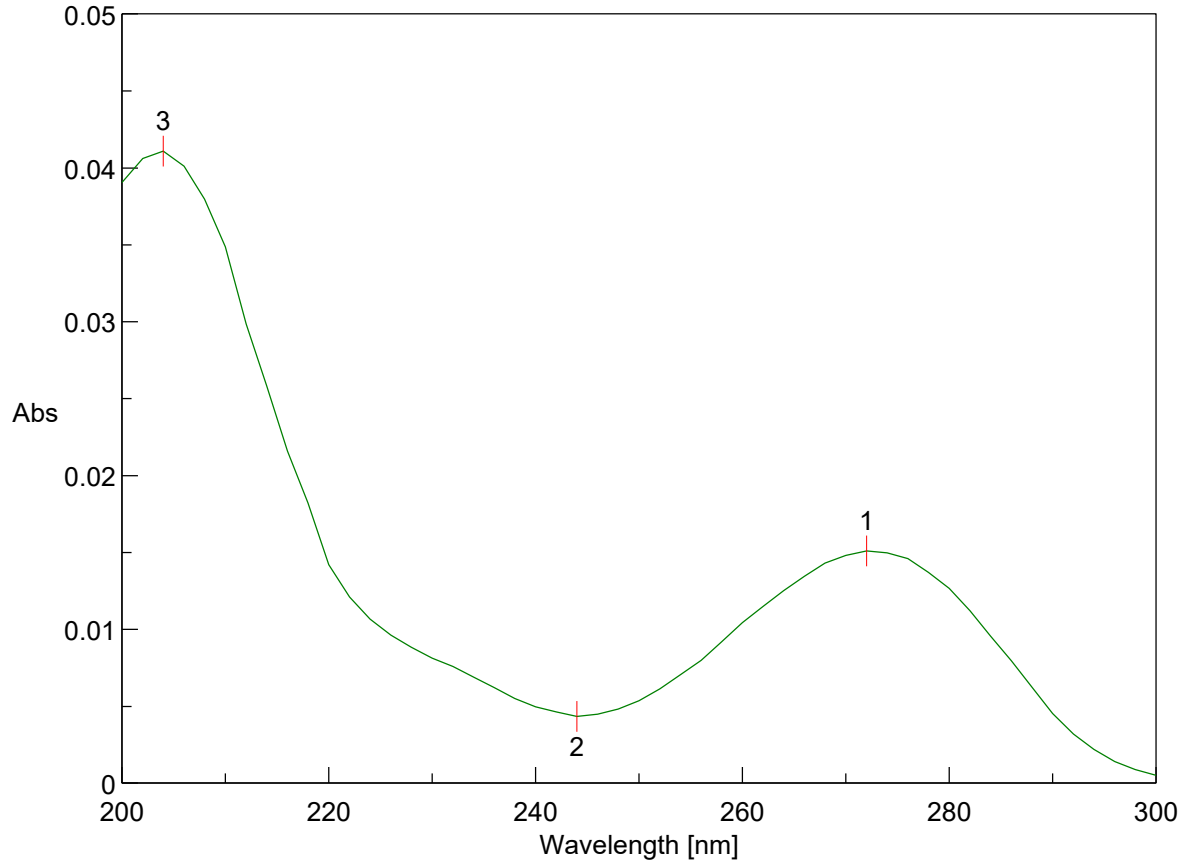

[Comments]

User	Administrator
Division	---
Company	Qpack
Creation date	06/04/2020 14:56

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.015086	2	244	0.00431997
3	204	0.041073			

Chromatogram

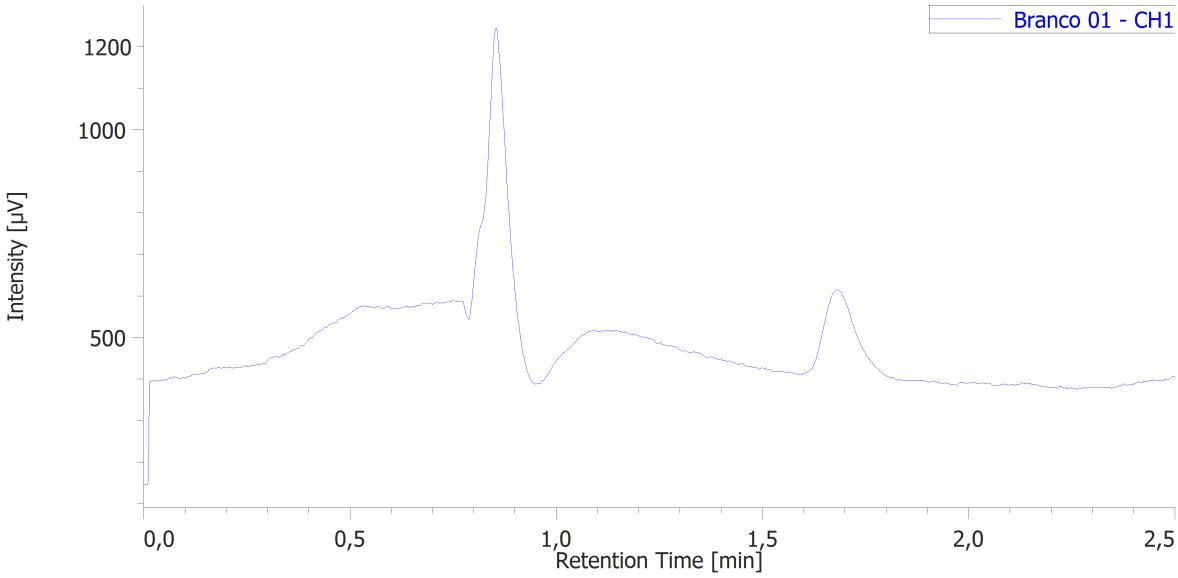


Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:00
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 11:43:01
Volume	10,00 [µL]
Sample #	35
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

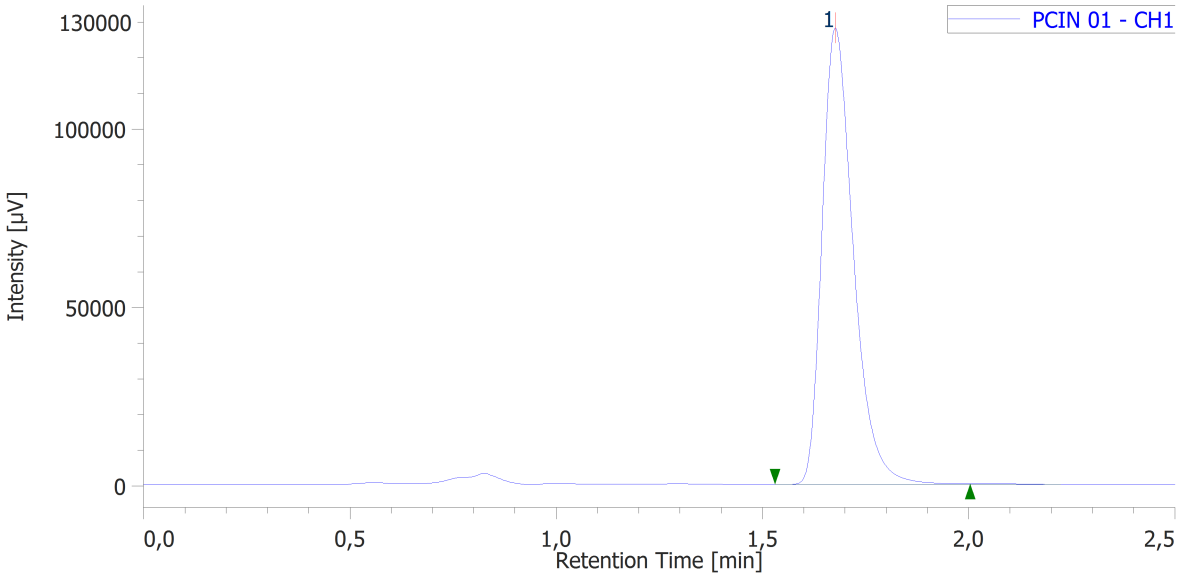

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:01
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 11:46:56
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	673700	127853	100,000	100,000	N/A	2472	N/A	1,368	

Creator Administrator
Reviewer
Approver

Chromatogram

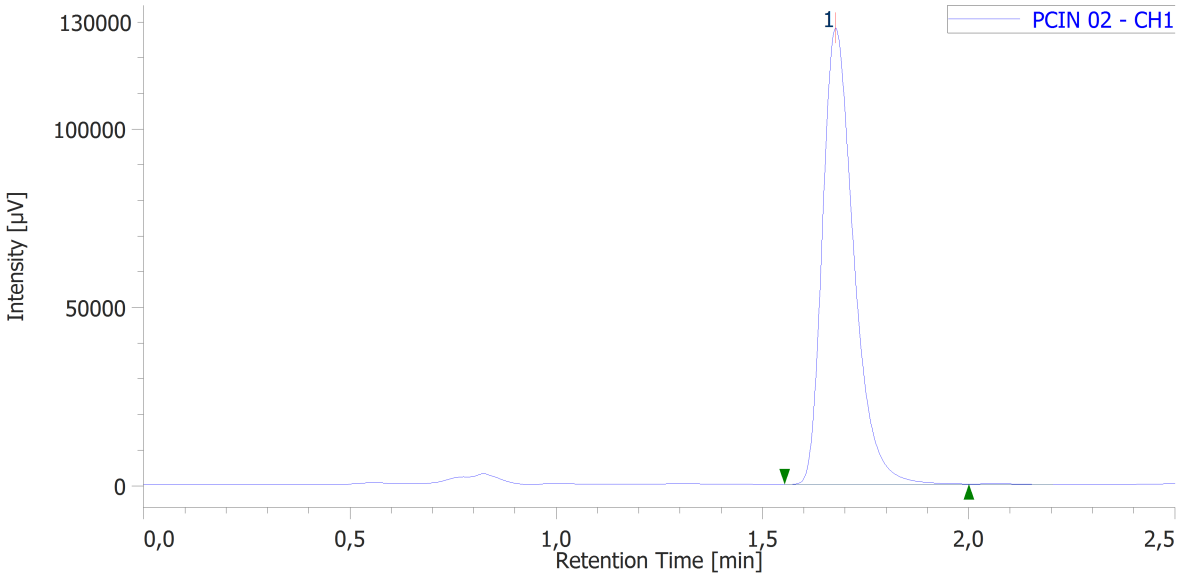

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:01
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 11:50:53
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	671973	127811	100,000	100,000	N/A	2483	N/A	1,387	

Creator Administrator
Reviewer
Approver

Chromatogram

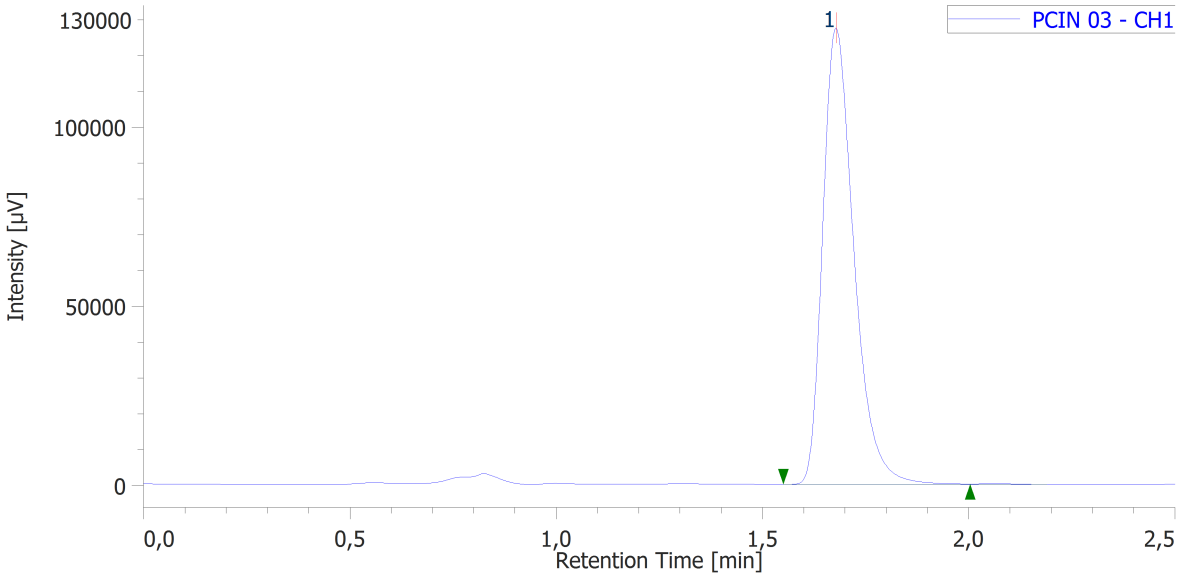

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:02
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 11:54:49
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,678	668343	127295	100,000	100,000	N/A	2491	N/A	1,363	

Creator Administrator
Reviewer
Approver

Chromatogram

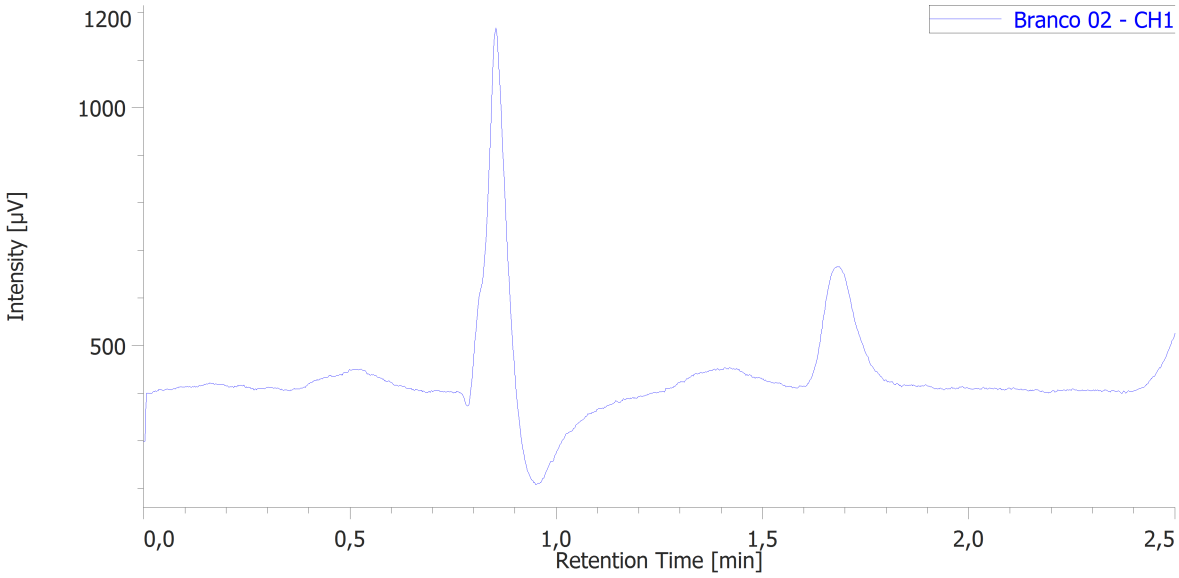


Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:03
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 11:58:46
Volume	10,00 [µL]
Sample #	35
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

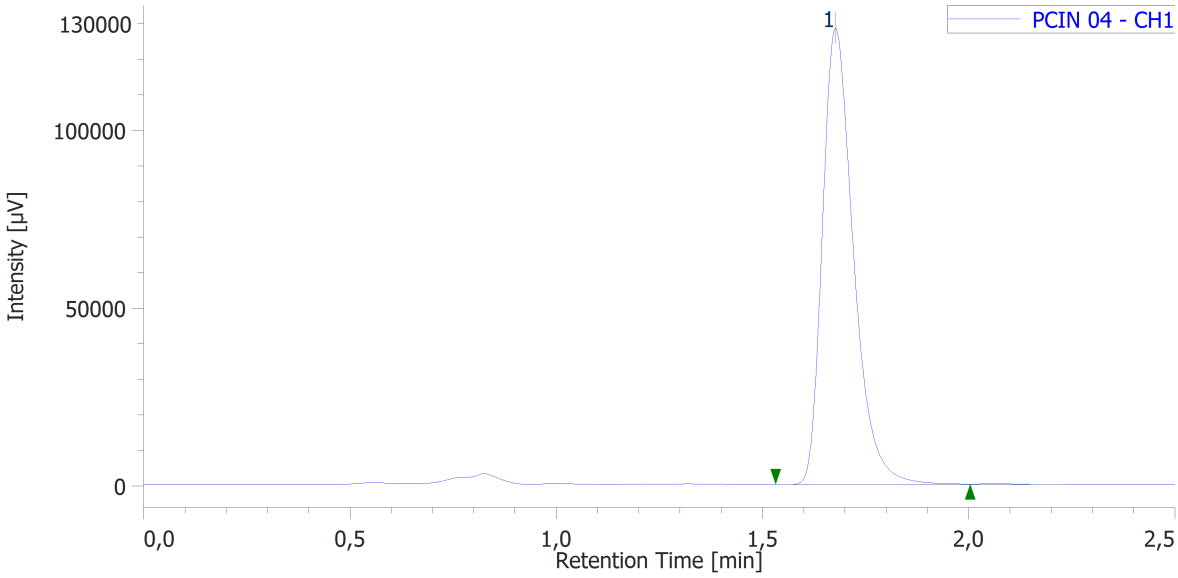

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:03
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 12:02:42
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	671516	128337	100,000	100,000	N/A	2513	N/A	1,379	

Creator Administrator
Reviewer
Approver

Chromatogram

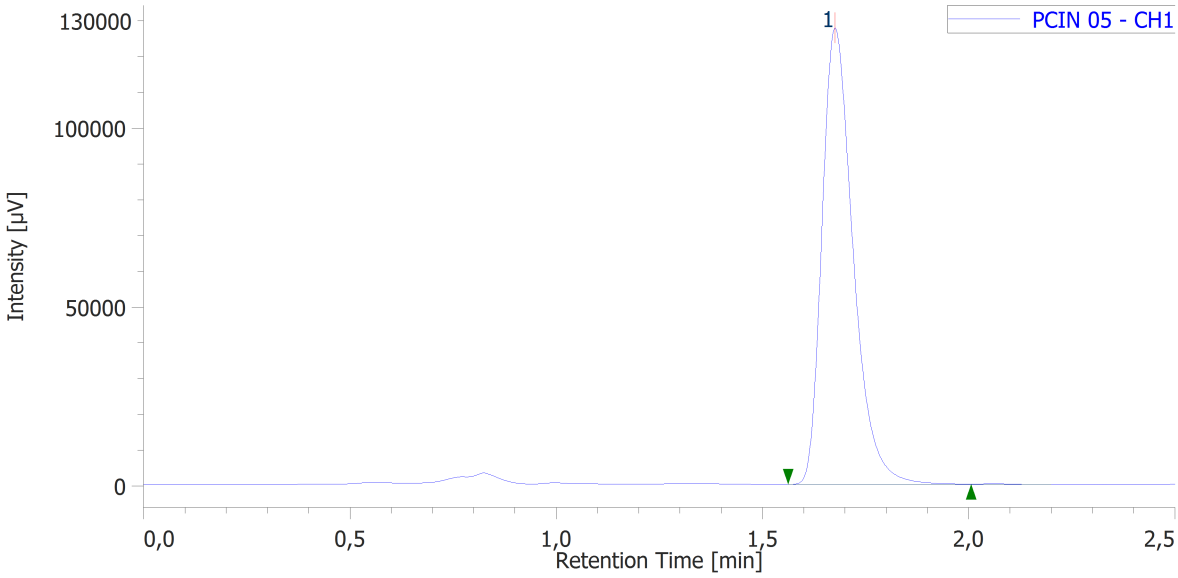

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:04
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 12:06:39
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,675	669891	127462	100,000	100,000	N/A	2479	N/A	1,396	

Creator Administrator
Reviewer
Approver

Chromatogram

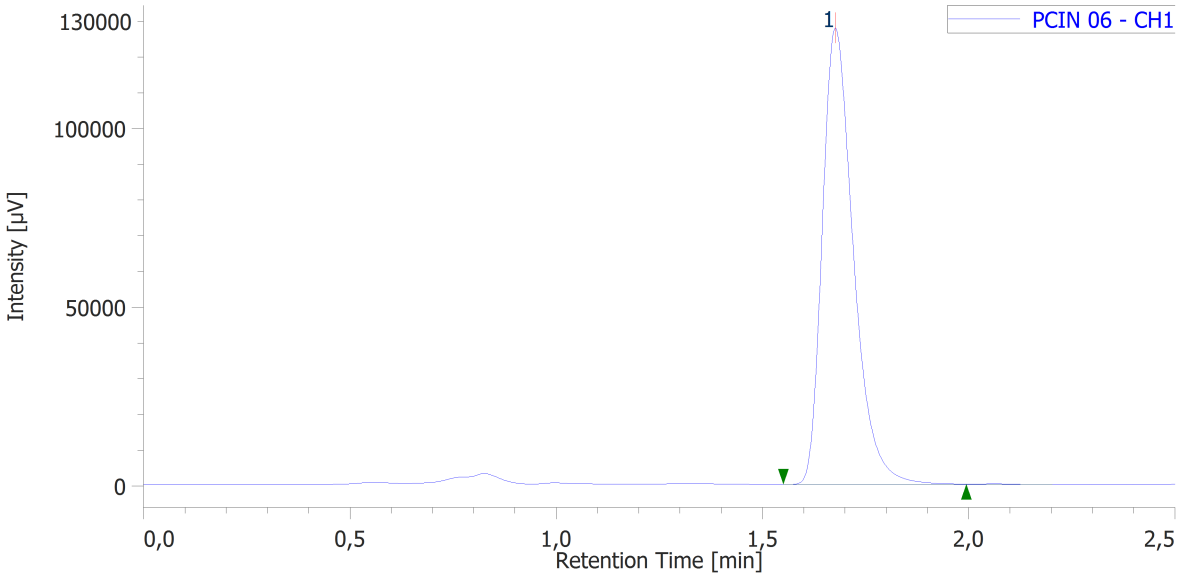

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:05
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 12:10:35
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	668553	127575	100,000	100,000	N/A	2503	N/A	1,377	

Creator Administrator
Reviewer
Approver

Chromatogram

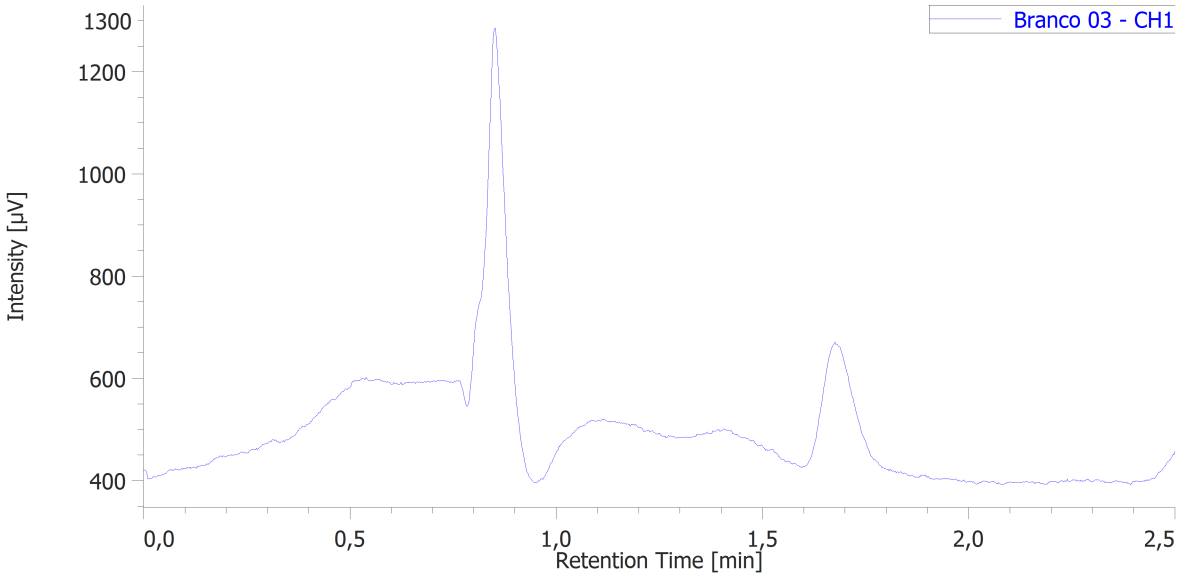


Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:13:05
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 12:14:30
Volume	10,00 [µL]
Sample #	35
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

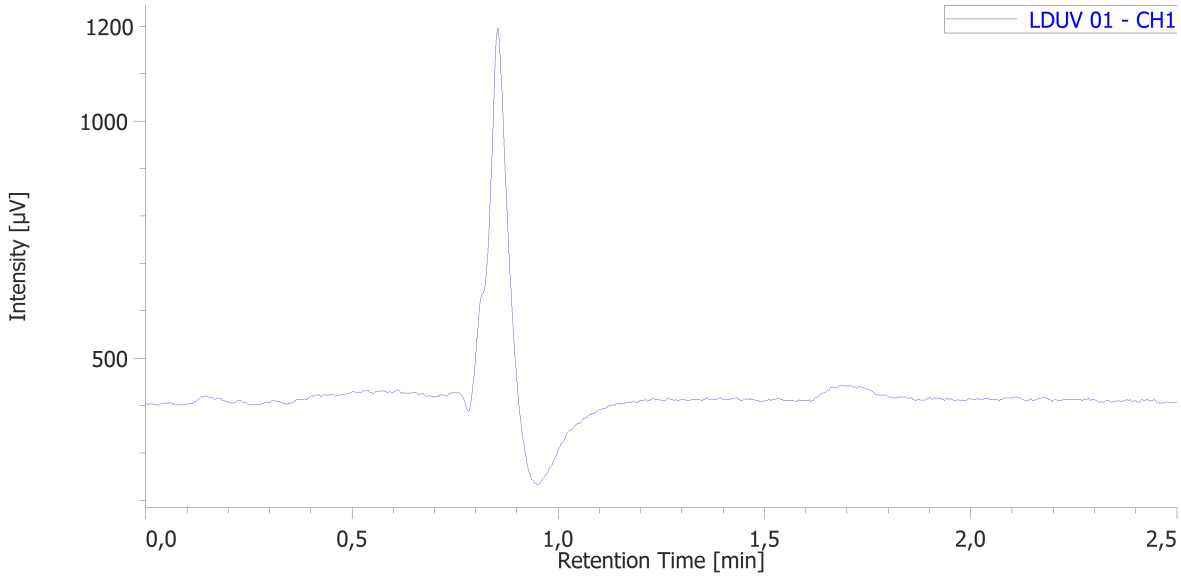


Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:21:35
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:19:03
Volume	10,00 [µL]
Sample #	25
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

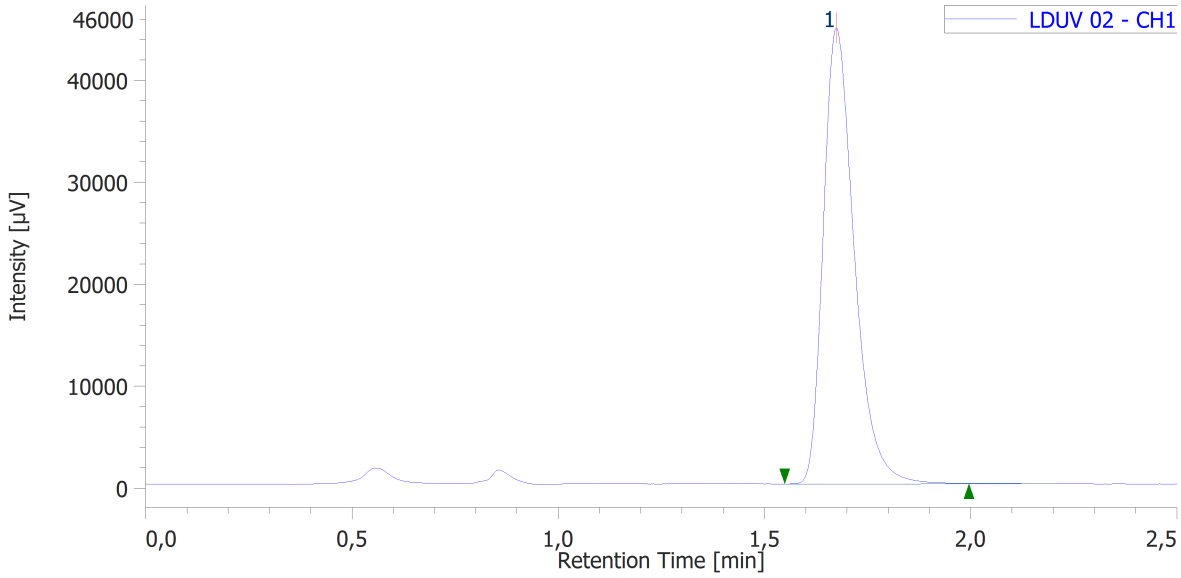

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:25:31
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:23:00
Volume	10,00 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,673	233620	44693	100,000	100,000	N/A	2516	N/A	1,393	

Creator Administrator
Reviewer
Approver

Chromatogram

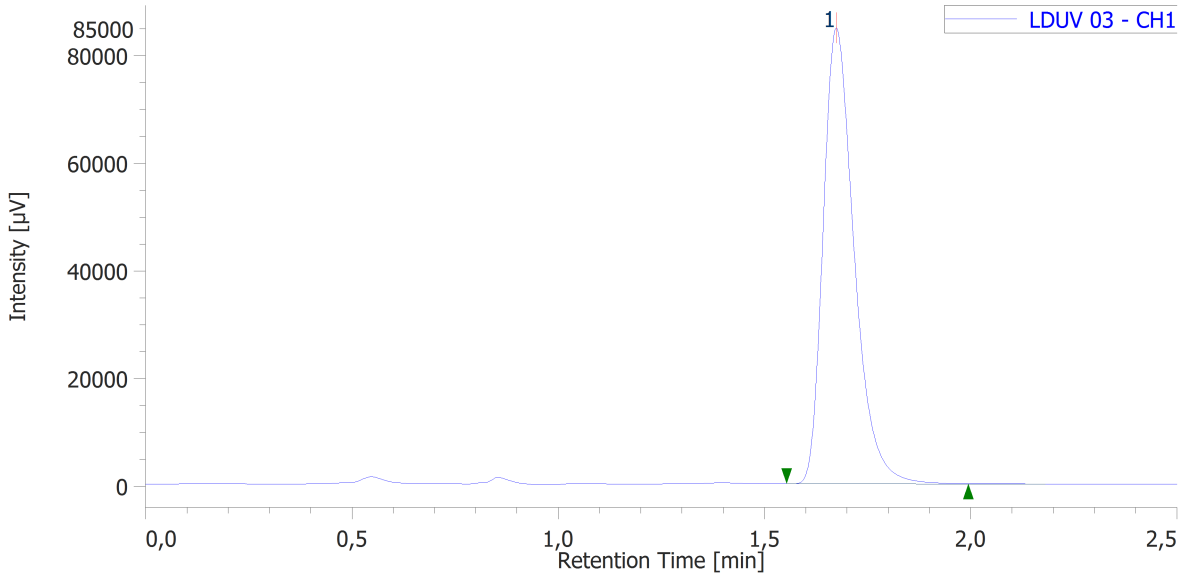

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:29:29
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:27:30
Volume	10,00 [µL]
Sample #	27
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,673	443121	84704	100,000	100,000	N/A	2499	N/A	1,379	

Creator Administrator
Reviewer
Approver

Chromatogram

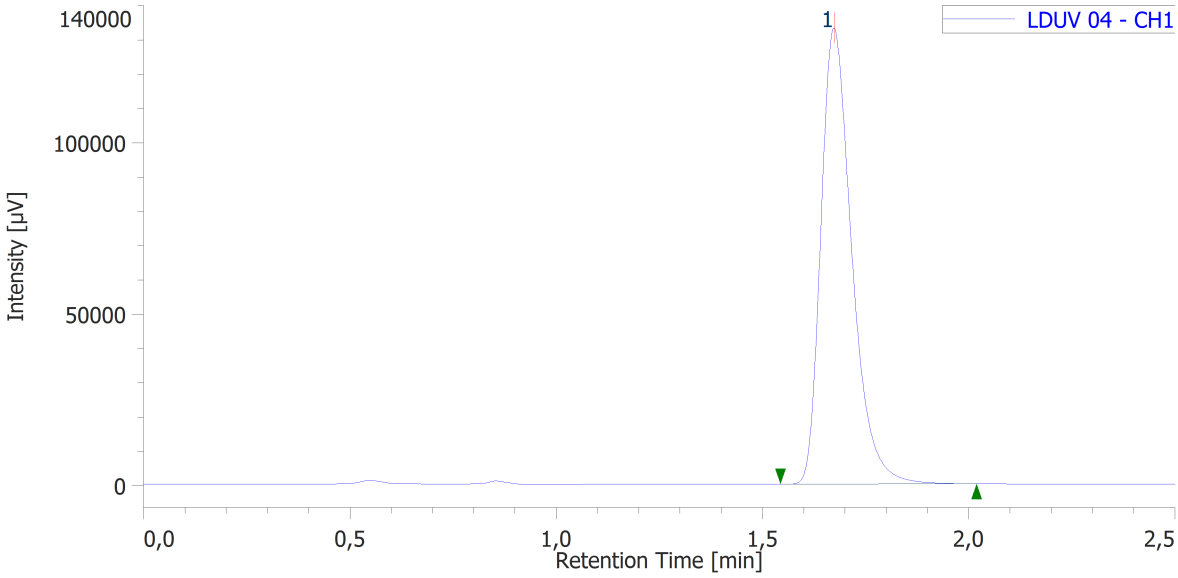

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:33:25
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:30:53
Volume	10,00 [µL]
Sample #	28
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,673	693620	133057	100,000	100,000	N/A	2519	N/A	1,367	

Creator Administrator
Reviewer
Approver

Chromatogram

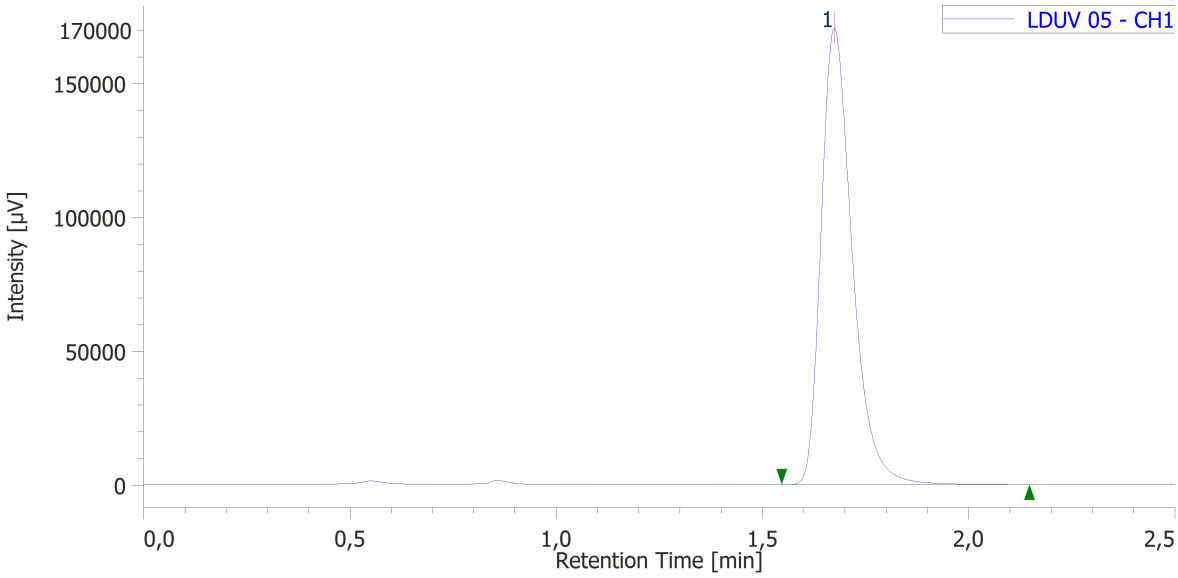

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 13:37:32
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:34:53
Volume	10,00 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,673	892183	170346	100,000	100,000	N/A	2506	N/A	1,384	

Creator Administrator
Reviewer
Approver

Chromatogram

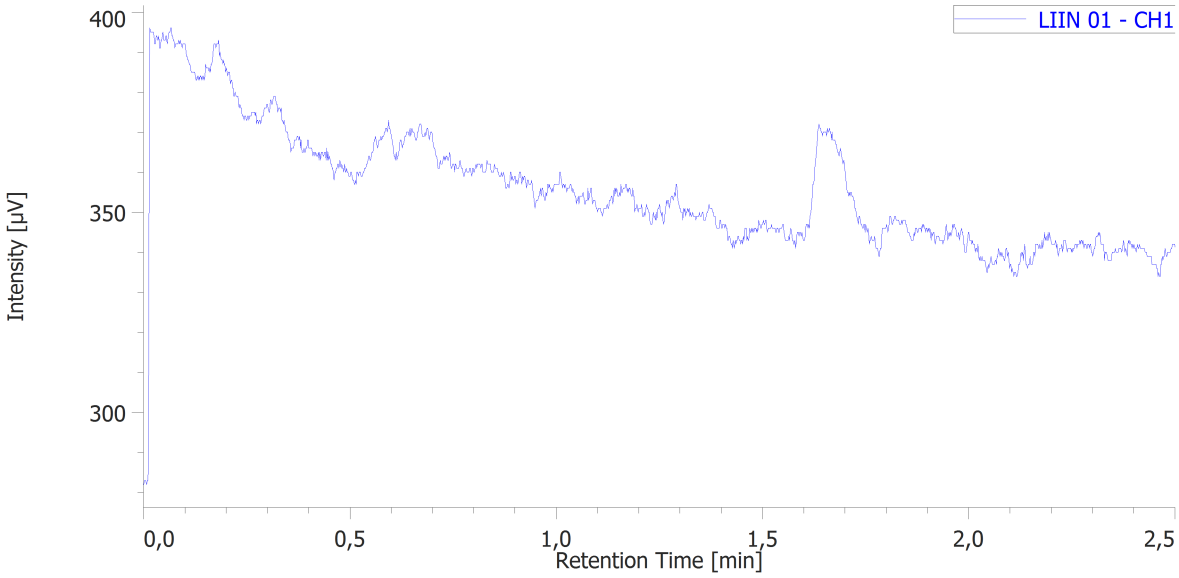


Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 14:07:11
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:55:32
Volume	0,10 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

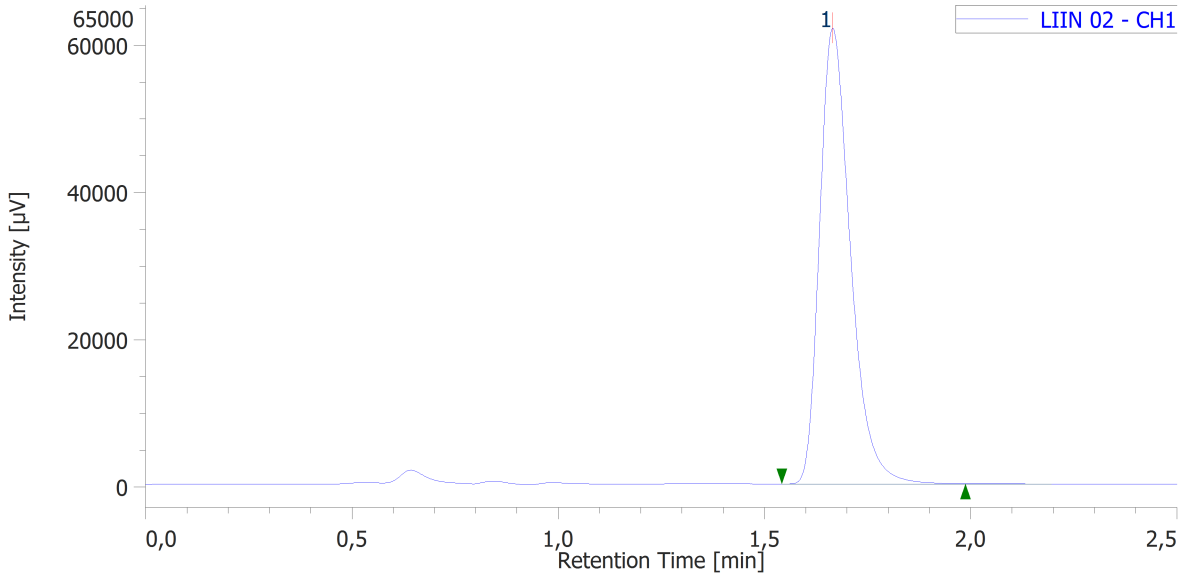

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 14:07:13
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 13:59:24
Volume	5,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,665	321938	61915	100,000	100,000	N/A	2504	N/A	1,362	

Creator Administrator
Reviewer
Approver

Chromatogram

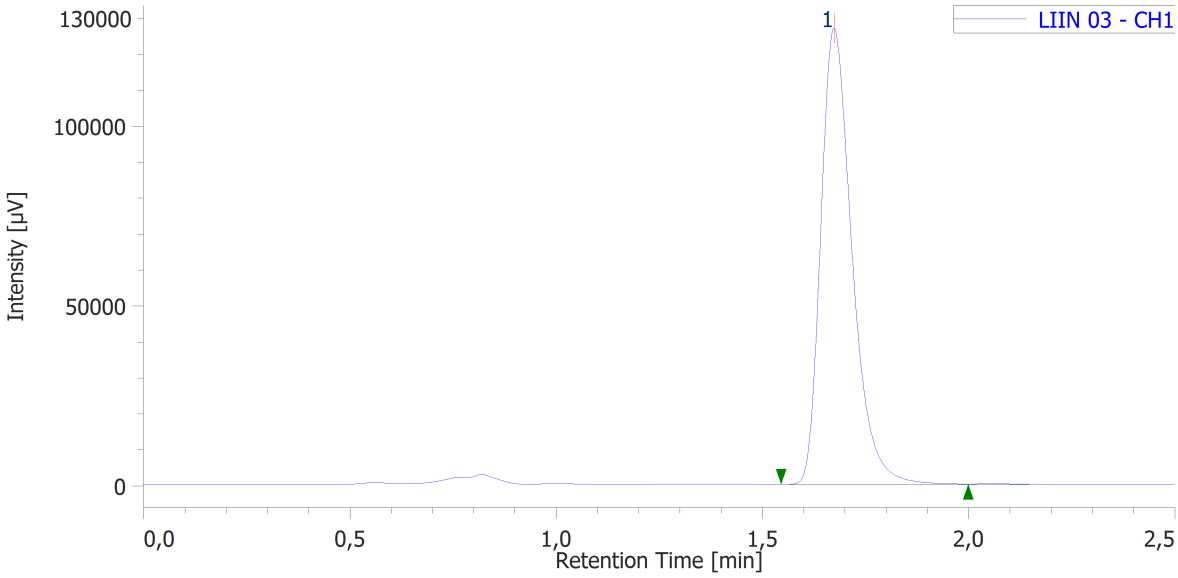

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 14:07:14
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 14:03:21
Volume	10,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,673	666806	126791	100,000	100,000	N/A	2476	N/A	1,363	

Creator Administrator
Reviewer
Approver

Chromatogram

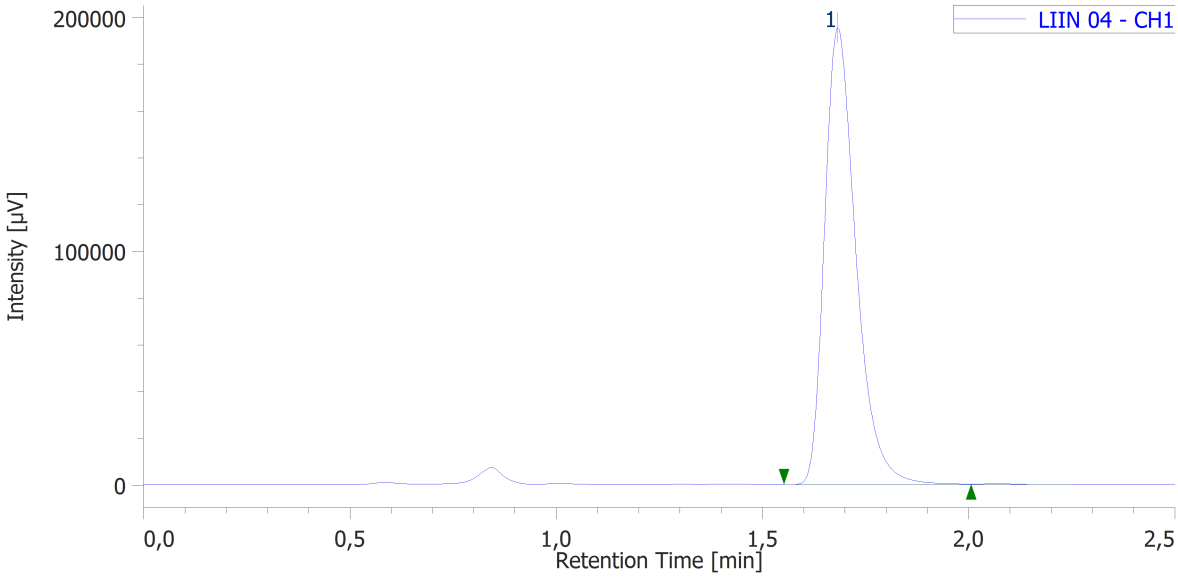

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 14:21:00
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 14:13:24
Volume	15,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,682	1031252	194923	100,000	100,000	N/A	2476	N/A	1,394	

Creator Administrator
Reviewer
Approver

Chromatogram

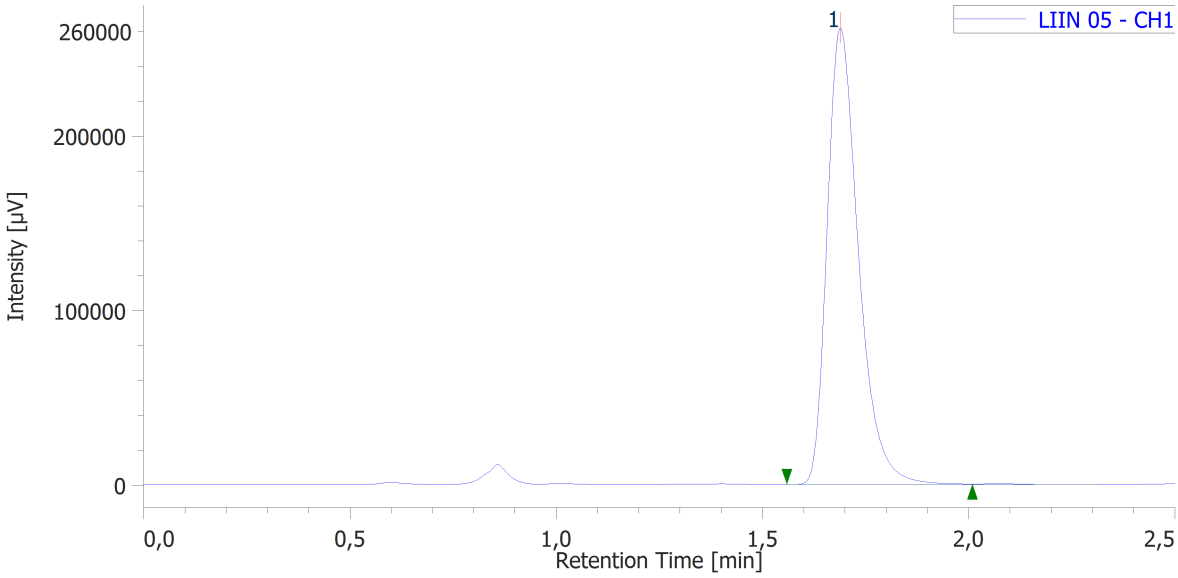

Chromatogram Information	
User Name	Administrator
Date Modified	08/04/2020 14:21:02
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 14:17:24
Volume	20,00 [µL]
Sample #	36
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,688	1380370	261362	100,000	100,000	N/A	2507	N/A	1,386	

Creator Administrator
Reviewer
Approver

Chromatogram

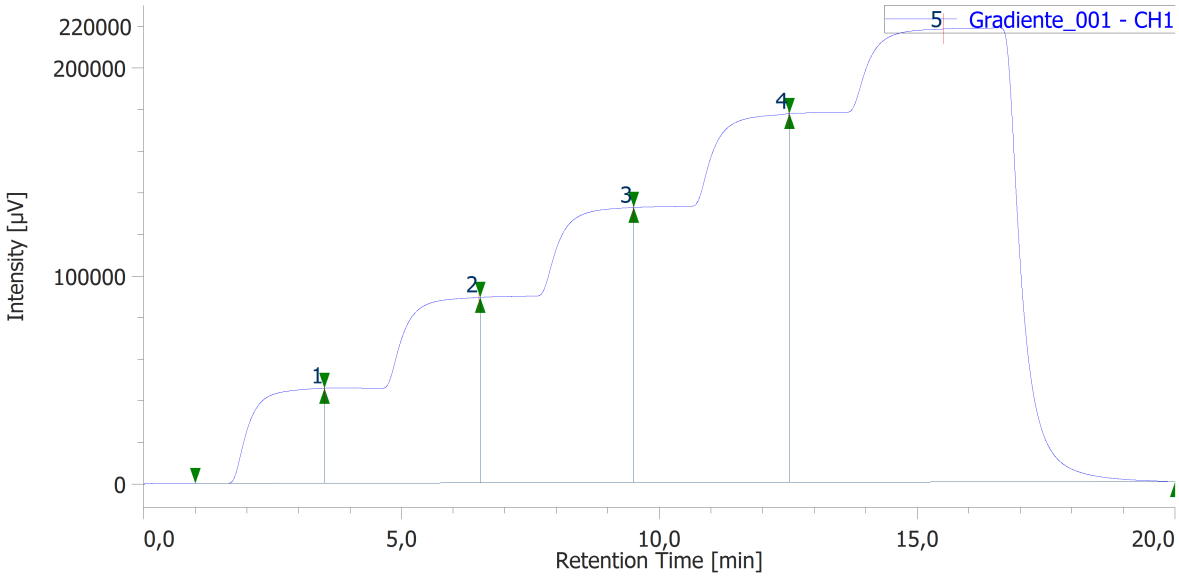

Chromatogram Information

User Name	Administrator
Date Modified	08/04/2020 15:13:51
Description	
HPLC System Name	HPL10
Injection Date	08/04/2020 14:46:56
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,500	4007232	45604	3,354	6,896	N/A	N/A	N/A	N/A	
2	40%	1	6,500	12097435	89030	10,125	13,463	N/A	N/A	N/A	N/A	
3	60%	1	9,490	19673356	132105	16,465	19,977	N/A	N/A	N/A	N/A	
4	80%	1	12,500	27872954	177020	23,328	26,769	N/A	N/A	N/A	N/A	
5	100%	1	15,500	55832468	217521	46,728	32,894	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver