
Peak Find - EDUV.jws

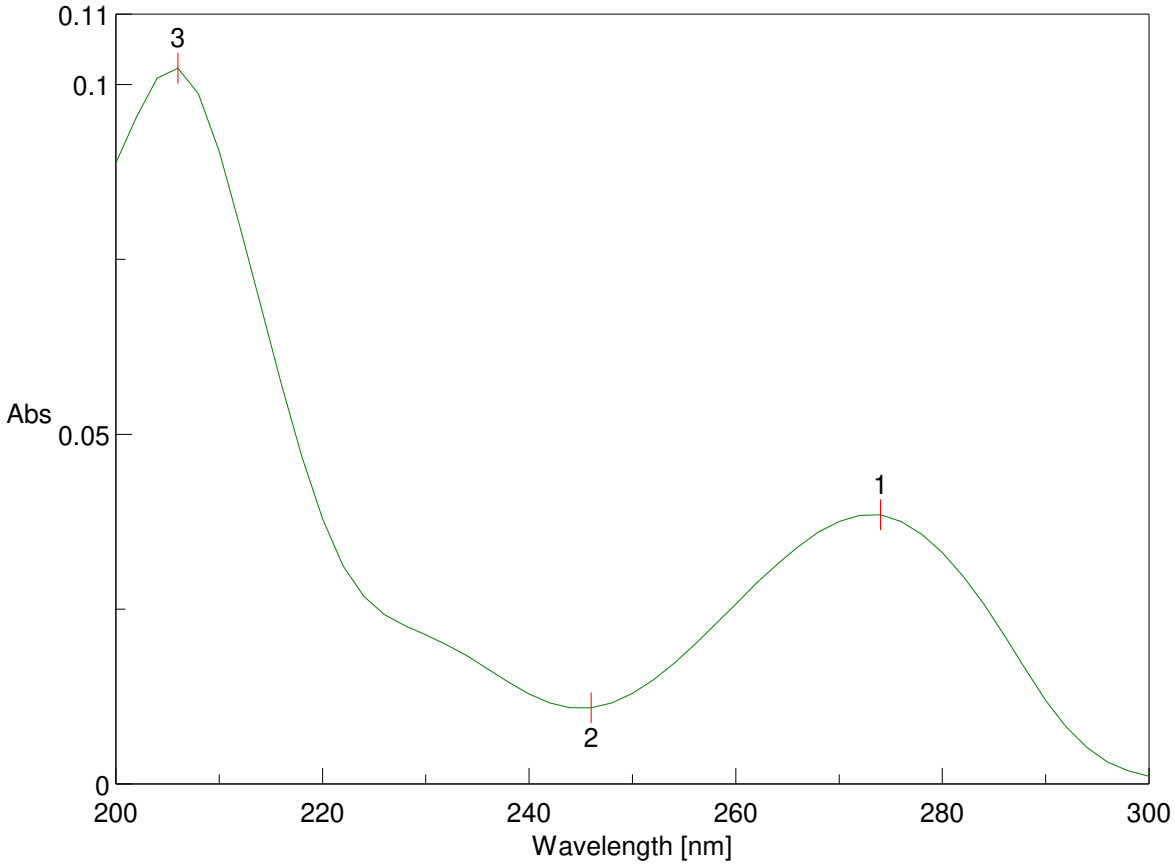

[Comments]

User	Administrator
Division	---
Company	Valer Laboratórios
Creation date	13/04/2020 09:17

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	2 nm
Data points	51


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A011361665
ROM version	1.01.22

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.038443	2	246	0.010891
3	206	0.102276			

Chromatogram

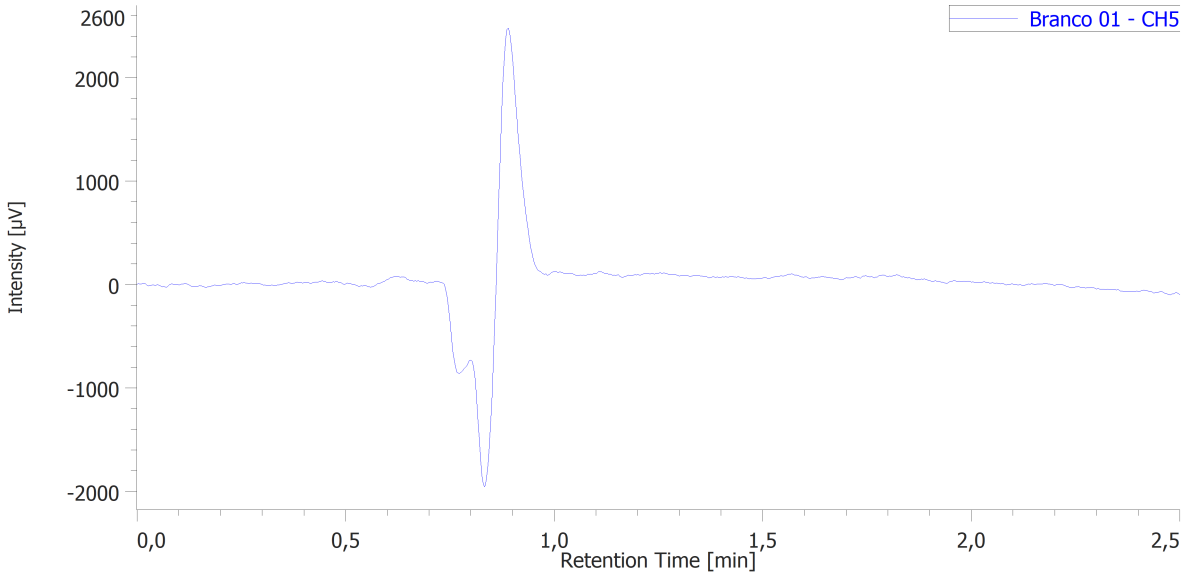


Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:36:43
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:21:52
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

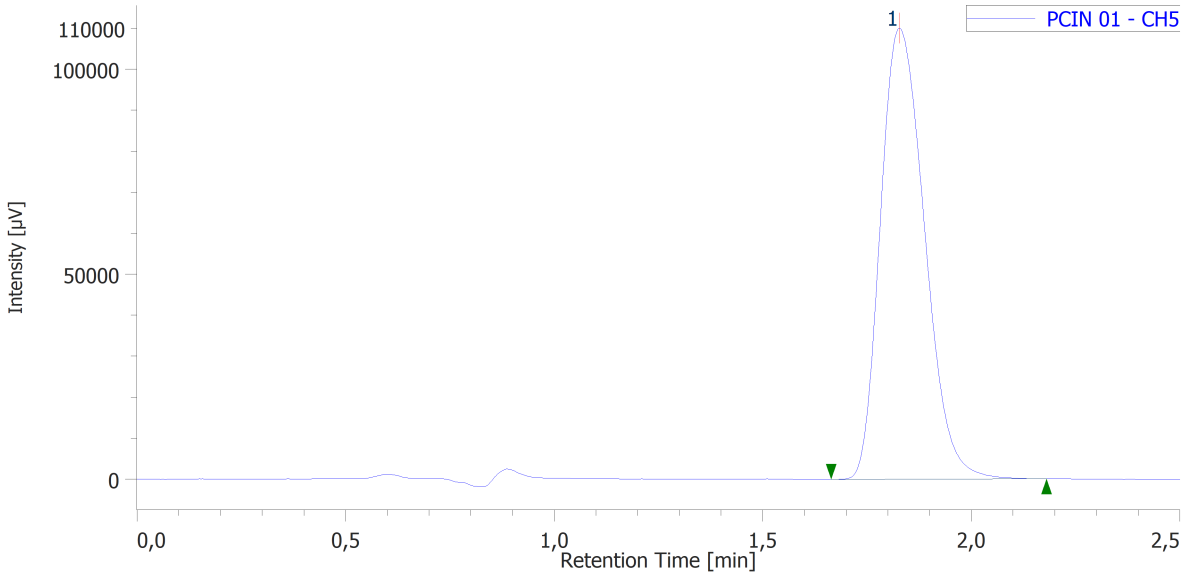

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:36:44
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:25:06
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	809437	110003	100,000	100,000	N/A	1373	N/A	1,272	

Creator Administrator
Reviewer
Approver

Chromatogram

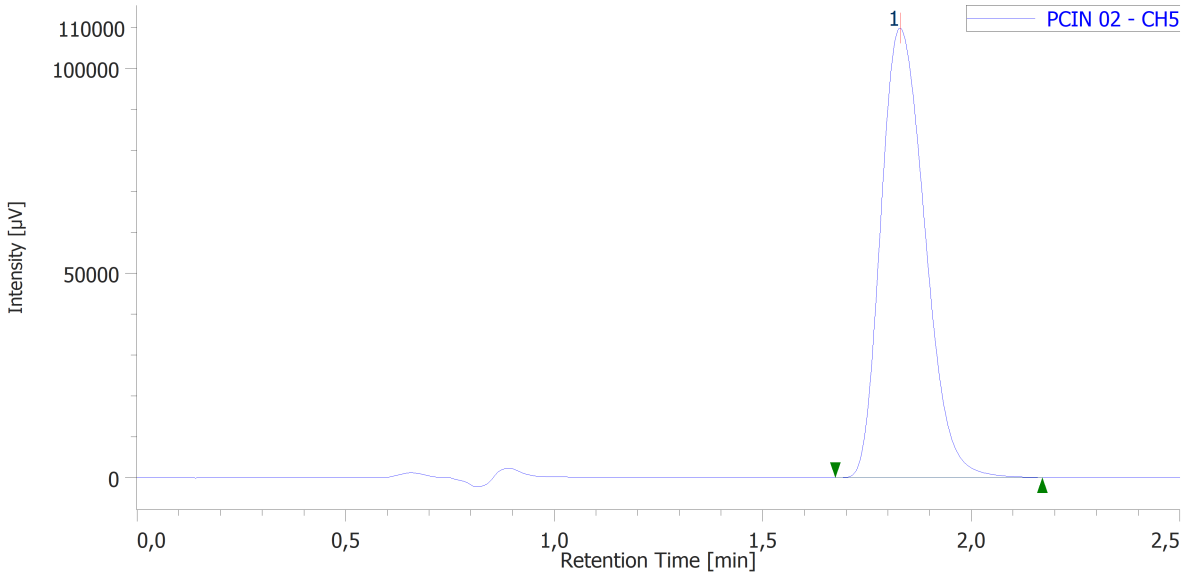

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:36:44
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:28:19
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,830	806351	109763	100,000	100,000	N/A	1387	N/A	1,237	

Creator Administrator
Reviewer
Approver

Chromatogram

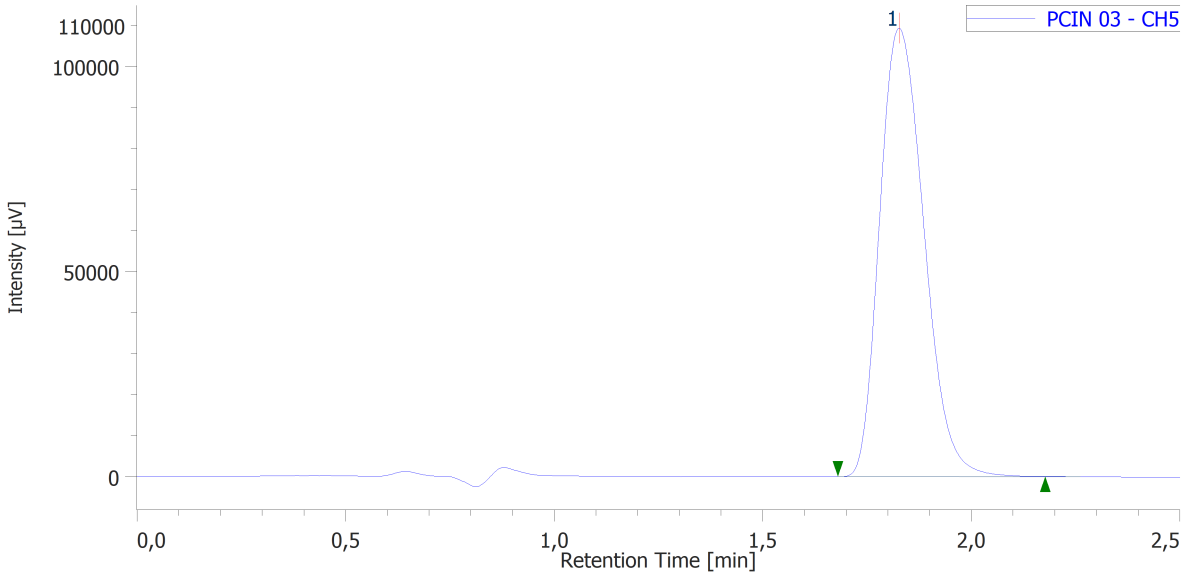

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:36:45
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:31:33
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	808085	109288	100,000	100,000	N/A	1365	N/A	1,249	

Creator Administrator
Reviewer
Approver

Chromatogram

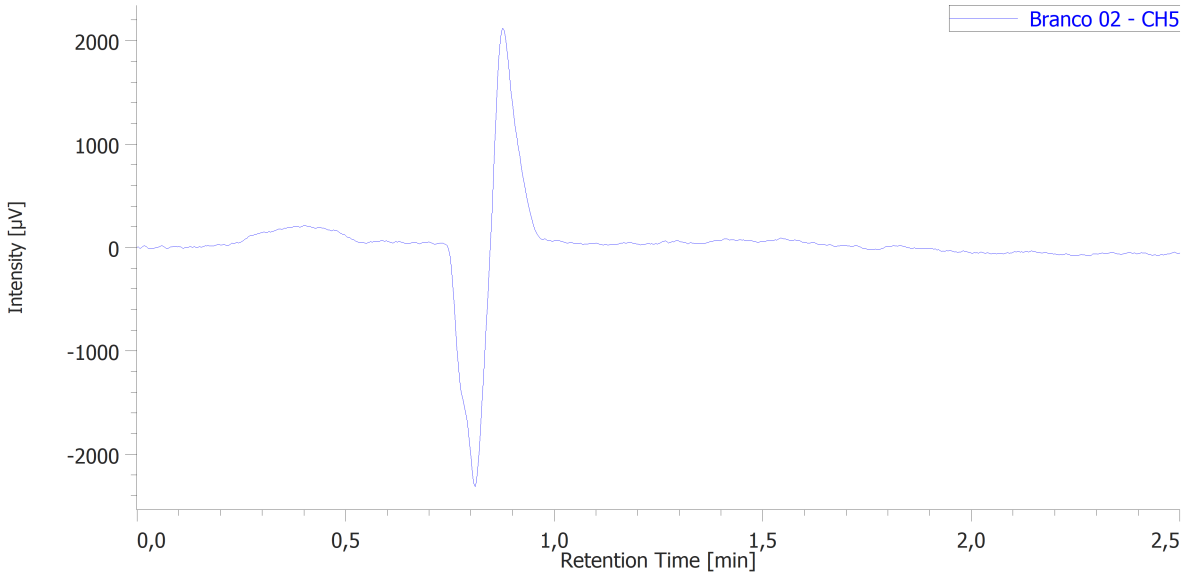


Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:38:20
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:34:48
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

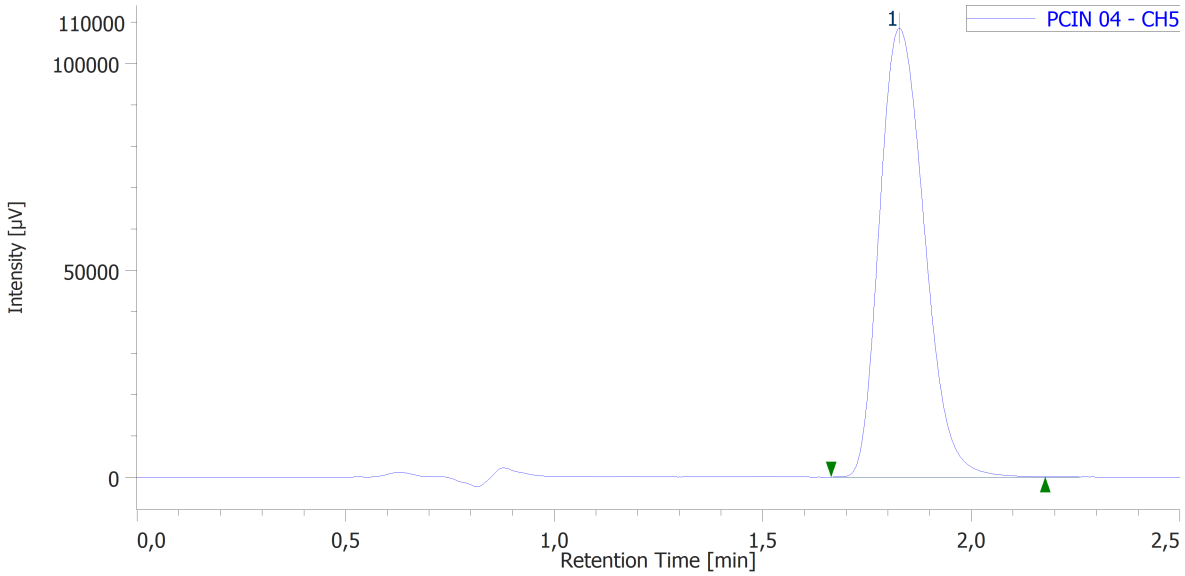

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:41:24
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:38:01
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	810428	108371	100,000	100,000	N/A	1336	N/A	1,251	

Creator Administrator
Reviewer
Approver

Chromatogram

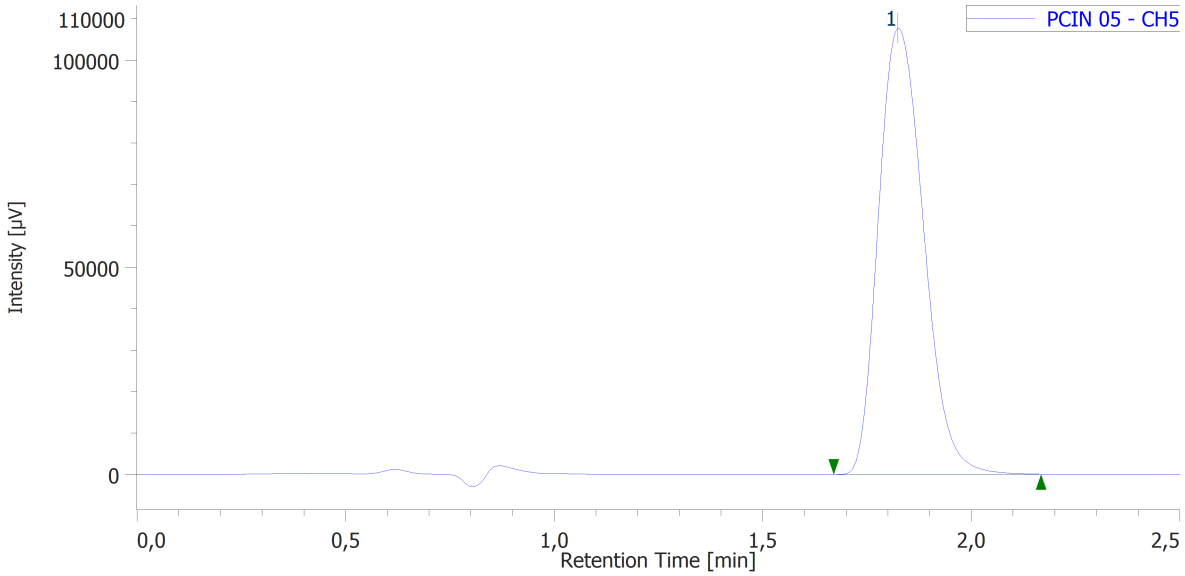

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:45:31
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:41:15
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,823	809083	107639	100,000	100,000	N/A	1313	N/A	1,261	

Creator Administrator
Reviewer
Approver

Chromatogram

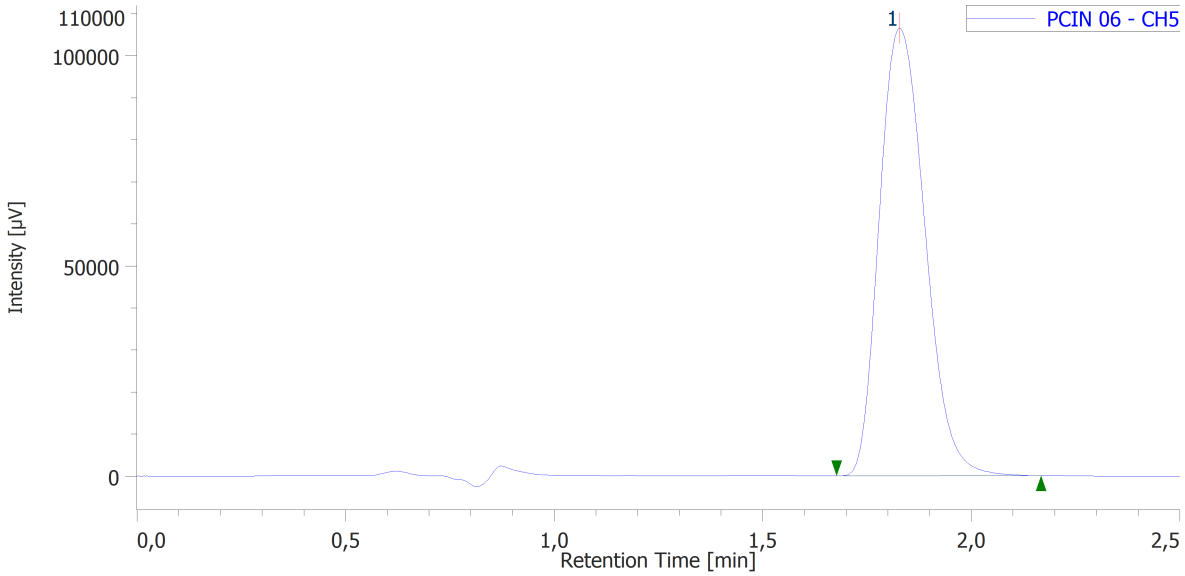

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:49:26
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:44:28
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	809558	106467	100,000	100,000	N/A	1284	N/A	1,250	

Creator Administrator
Reviewer
Approver

Chromatogram

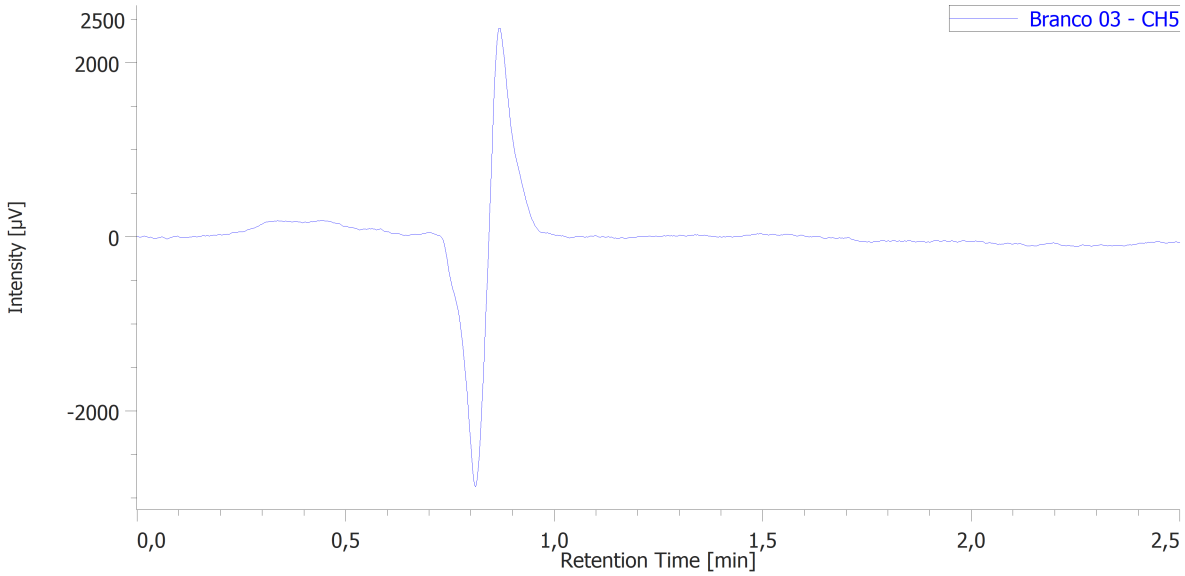


Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:51:02
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:47:42
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

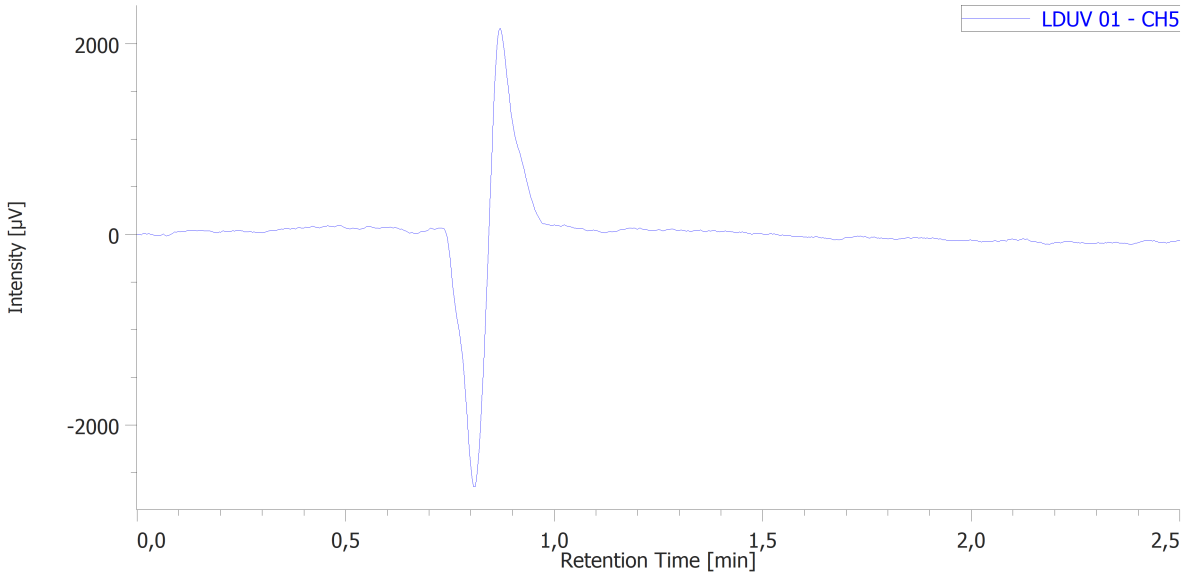


Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:59:43
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:53:29
Volume	10,00 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

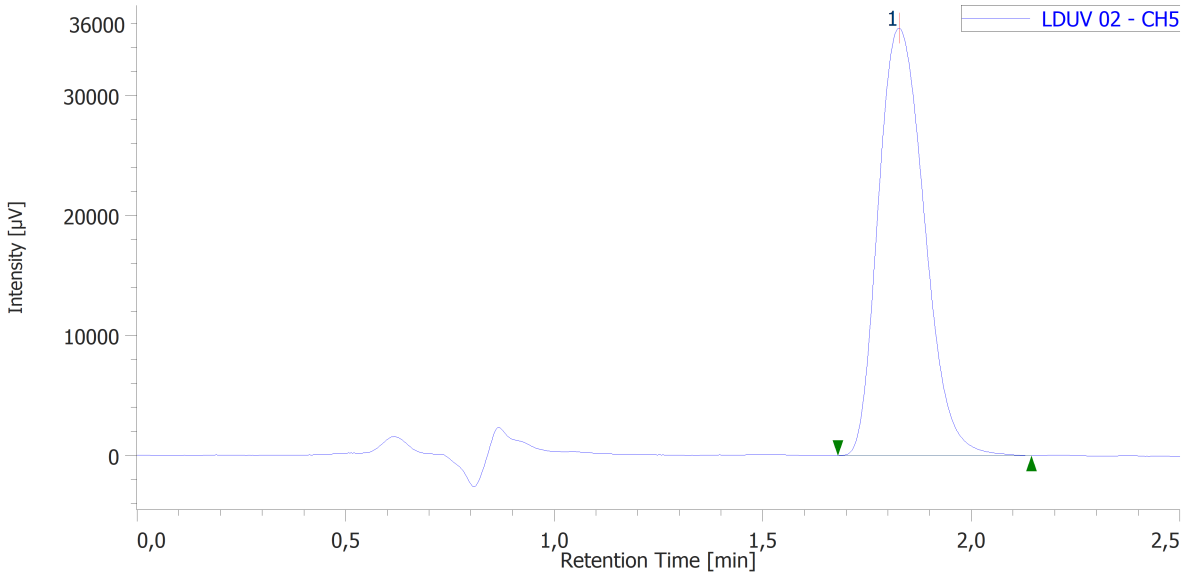

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 09:59:44
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:56:42
Volume	10,00 [µL]
Sample #	32
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	274224	35607	100,000	100,000	N/A	1248	N/A	1,224	

Creator Administrator
Reviewer
Approver

Chromatogram

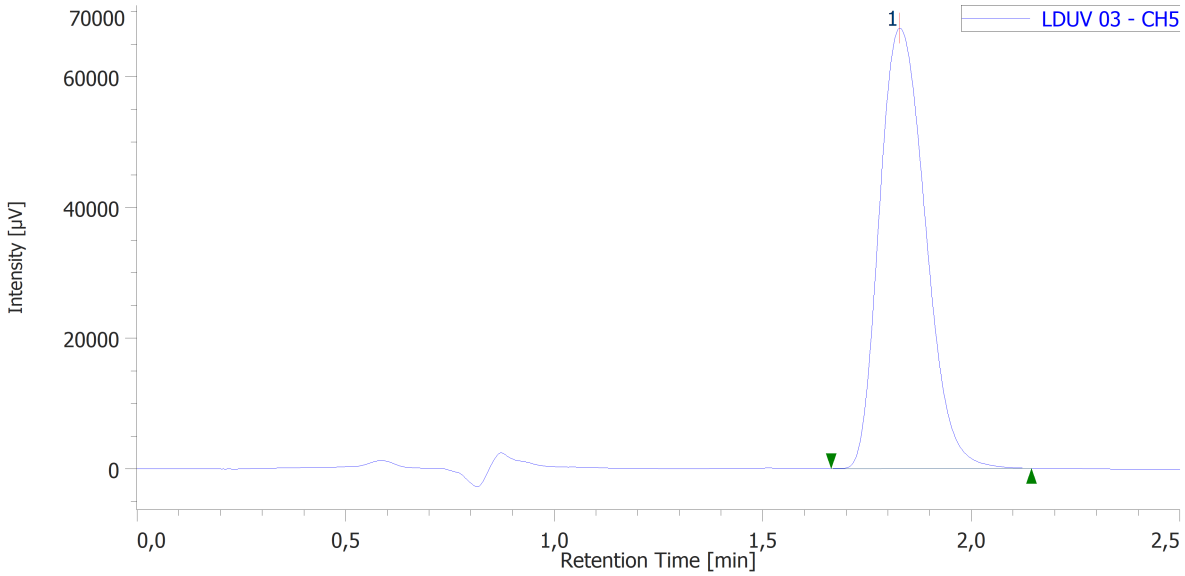

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:03:56
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 09:59:56
Volume	10,00 [µL]
Sample #	33
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	517479	67368	100,000	100,000	N/A	1252	N/A	1,255	

Creator Administrator
Reviewer
Approver

Chromatogram

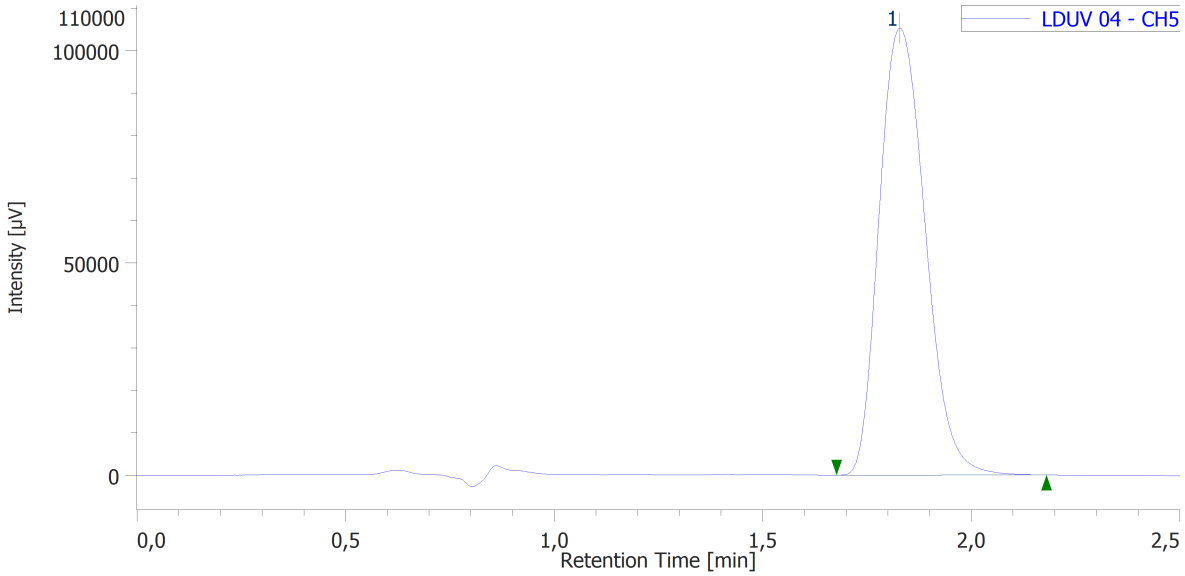

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:06:30
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:03:10
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	808840	105249	100,000	100,000	N/A	1257	N/A	1,247	

Creator Administrator
Reviewer
Approver

Chromatogram

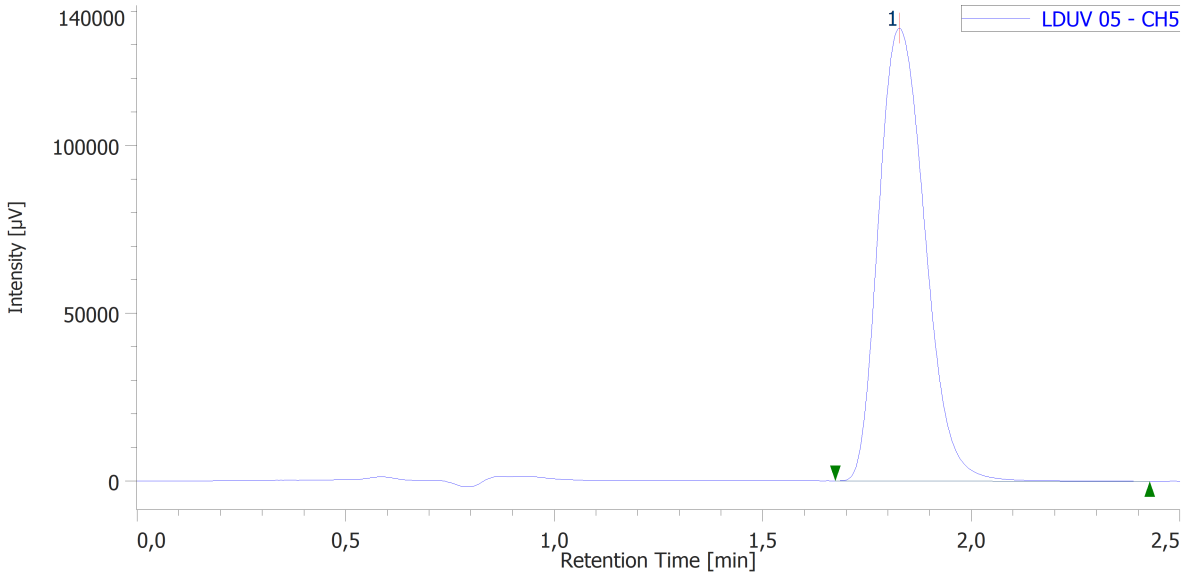

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:11:25
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:06:23
Volume	10,00 [µL]
Sample #	35
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	1041471	134954	100,000	100,000	N/A	1253	N/A	1,241	

Creator Administrator
Reviewer
Approver

Chromatogram

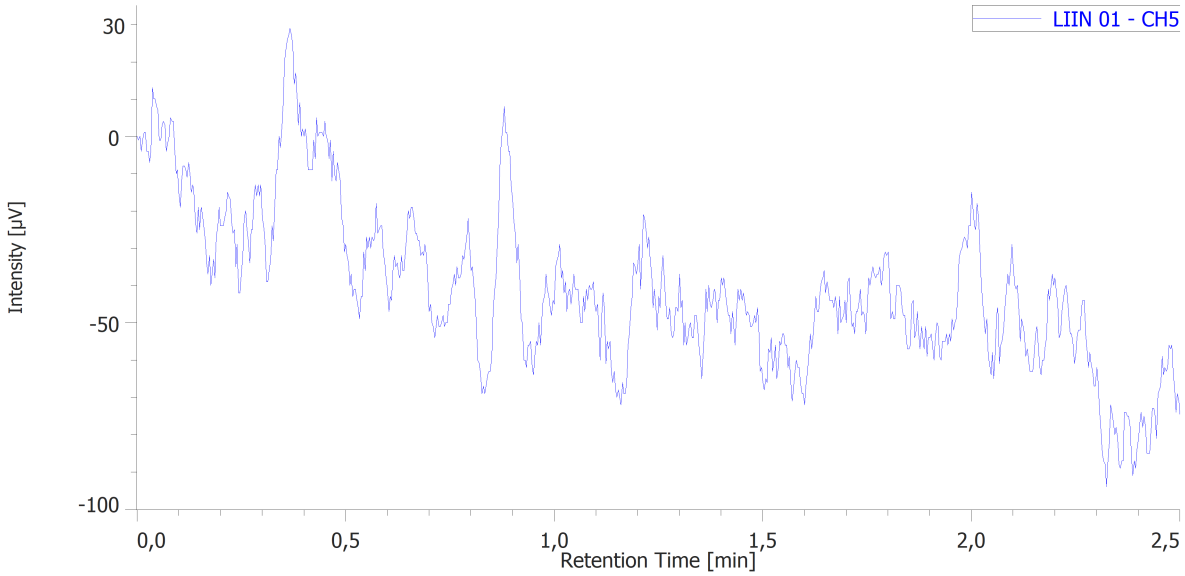


Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:28:39
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:21:41
Volume	0,10 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

Creator Administrator
Reviewer
Approver

Chromatogram

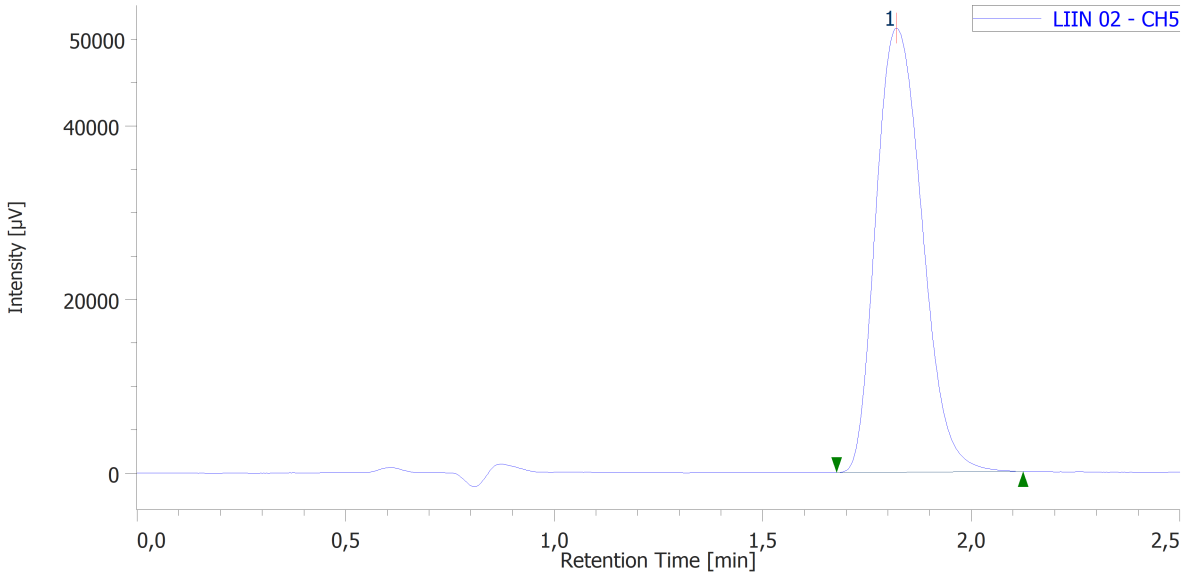

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:28:39
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:24:39
Volume	5,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,820	395324	51157	100,000	100,000	N/A	1225	N/A	1,240	

Creator Administrator
Reviewer
Approver

Chromatogram

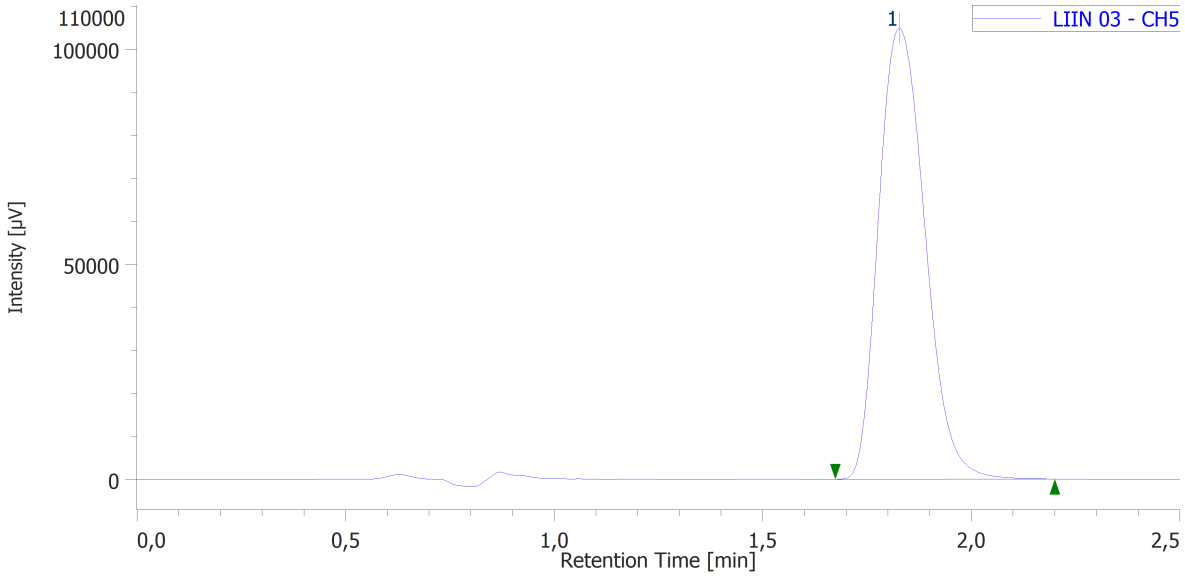

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:33:25
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:27:51
Volume	10,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,827	809149	104757	100,000	100,000	N/A	1242	N/A	1,238	

Creator Administrator
Reviewer
Approver

Chromatogram

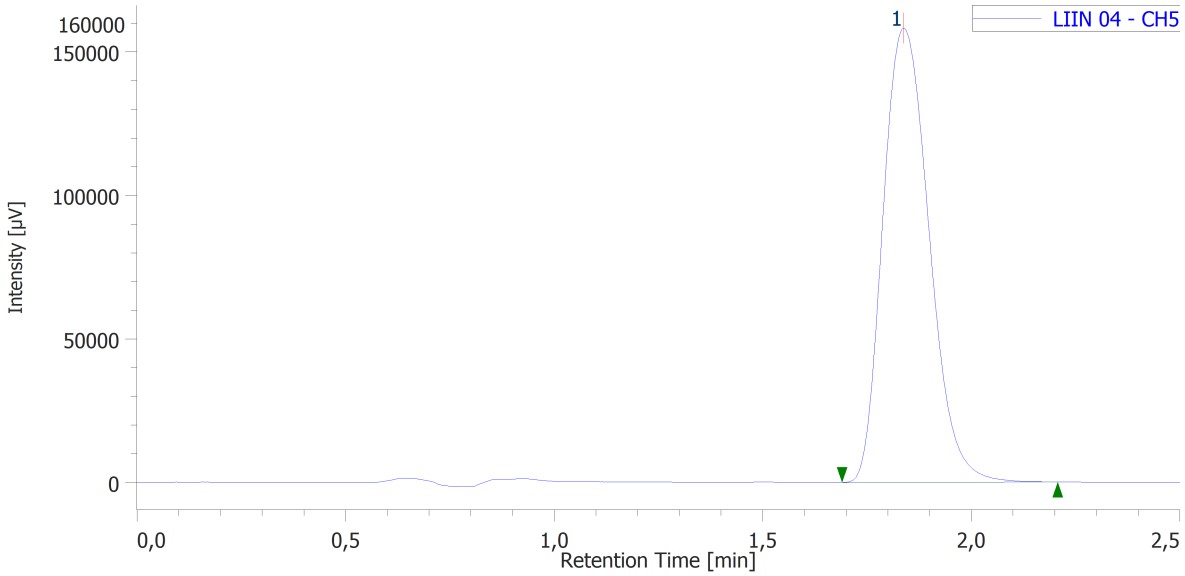

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:34:17
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:31:20
Volume	15,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,837	1219206	158168	100,000	100,000	N/A	1272	N/A	1,245	

Creator Administrator
Reviewer
Approver

Chromatogram

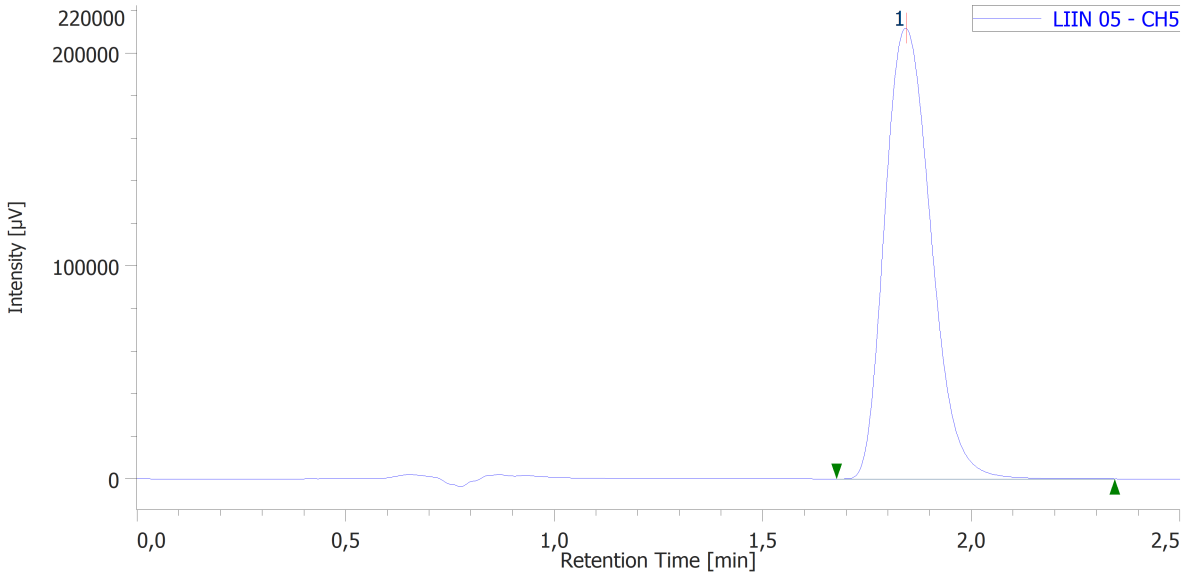

Chromatogram Information	
User Name	Administrator
Date Modified	13/04/2020 10:39:00
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 10:35:03
Volume	20,00 [µL]
Sample #	34
Project Name	Qualificação Operacional
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	OQ
Peak ID Table	Int
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,843	1634329	211682	100,000	100,000	N/A	1288	N/A	1,219	

Creator Administrator
Reviewer
Approver

Chromatogram

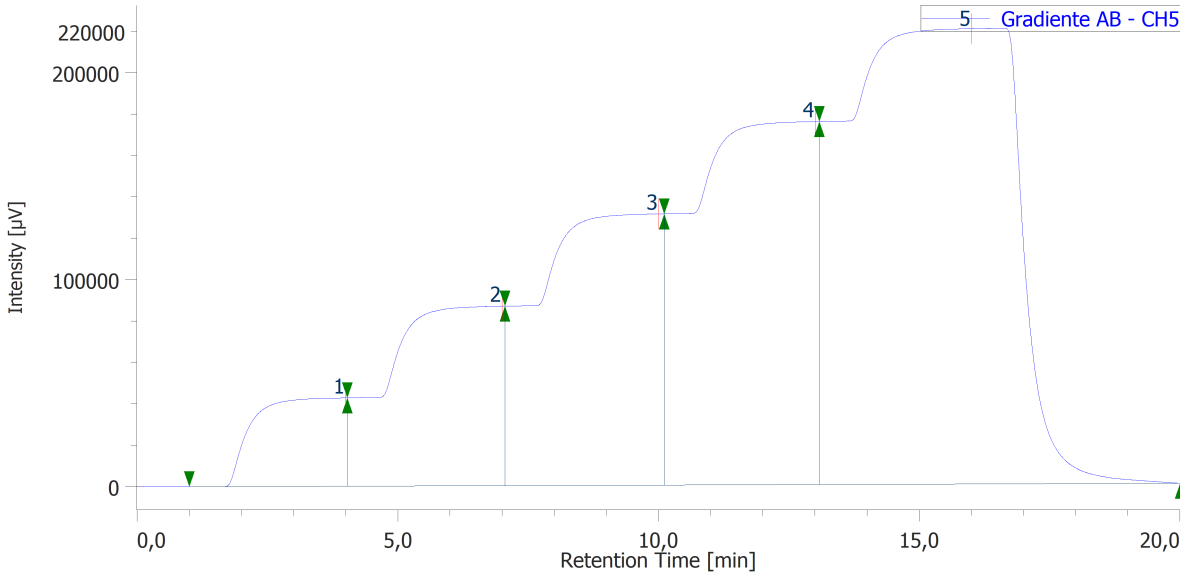

Chromatogram Information

User Name	Administrator
Date Modified	13/04/2020 12:17:39
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 11:57:38
Volume	0,10 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,000	4932892	42628	4,167	6,503	N/A	N/A	N/A	N/A	
2	40%	5	7,000	12953498	86704	10,943	13,227	N/A	N/A	N/A	N/A	
3	60%	5	10,000	21267440	130983	17,967	19,982	N/A	N/A	N/A	N/A	
4	80%	5	13,000	28687119	175300	24,235	26,743	N/A	N/A	N/A	N/A	
5	100%	5	16,000	50528204	219874	42,687	33,544	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

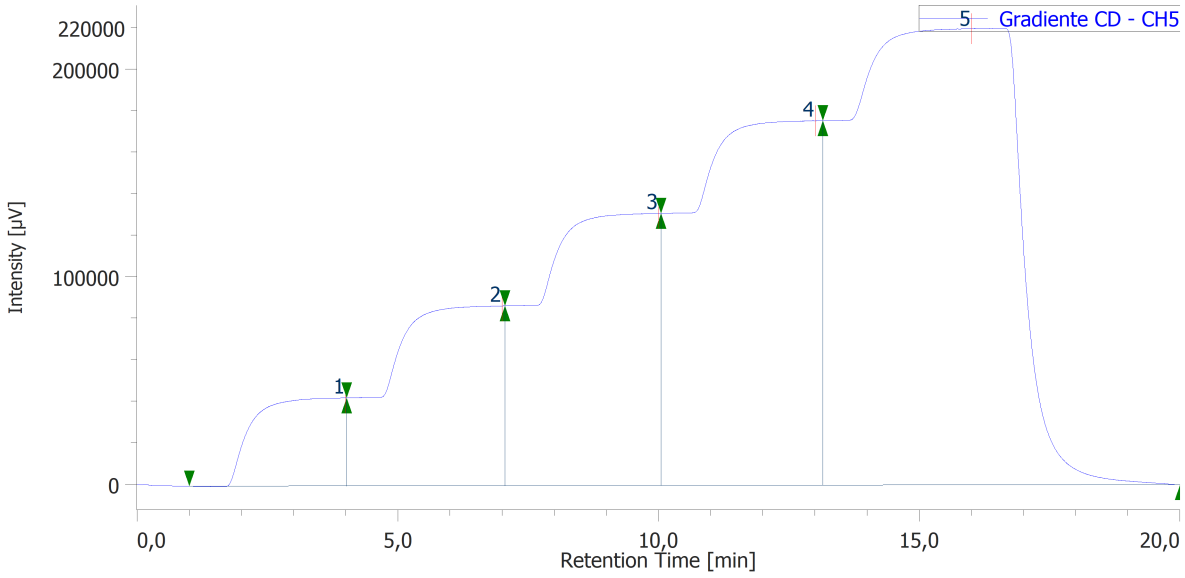

Chromatogram Information

User Name	Administrator
Date Modified	13/04/2020 12:37:51
Description	
HPLC System Name	HPL19
Injection Date	13/04/2020 12:17:50
Volume	0,10 [µL]
Sample #	31
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,000	4833592	42423	4,092	6,475	N/A	N/A	N/A	N/A	
2	40%	5	7,000	12942729	86572	10,956	13,214	N/A	N/A	N/A	N/A	
3	60%	5	10,000	20749296	130992	17,565	19,994	N/A	N/A	N/A	N/A	
4	80%	5	13,000	29860852	175463	25,278	26,782	N/A	N/A	N/A	N/A	
5	100%	5	16,000	49743973	219709	42,109	33,535	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver