HPLC - Agilent Lab Advisor

visor

Service & Diagnostics


Spectral Scan

HPLC

Spectral Scan - 1260 VWD [DEACX00141]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1

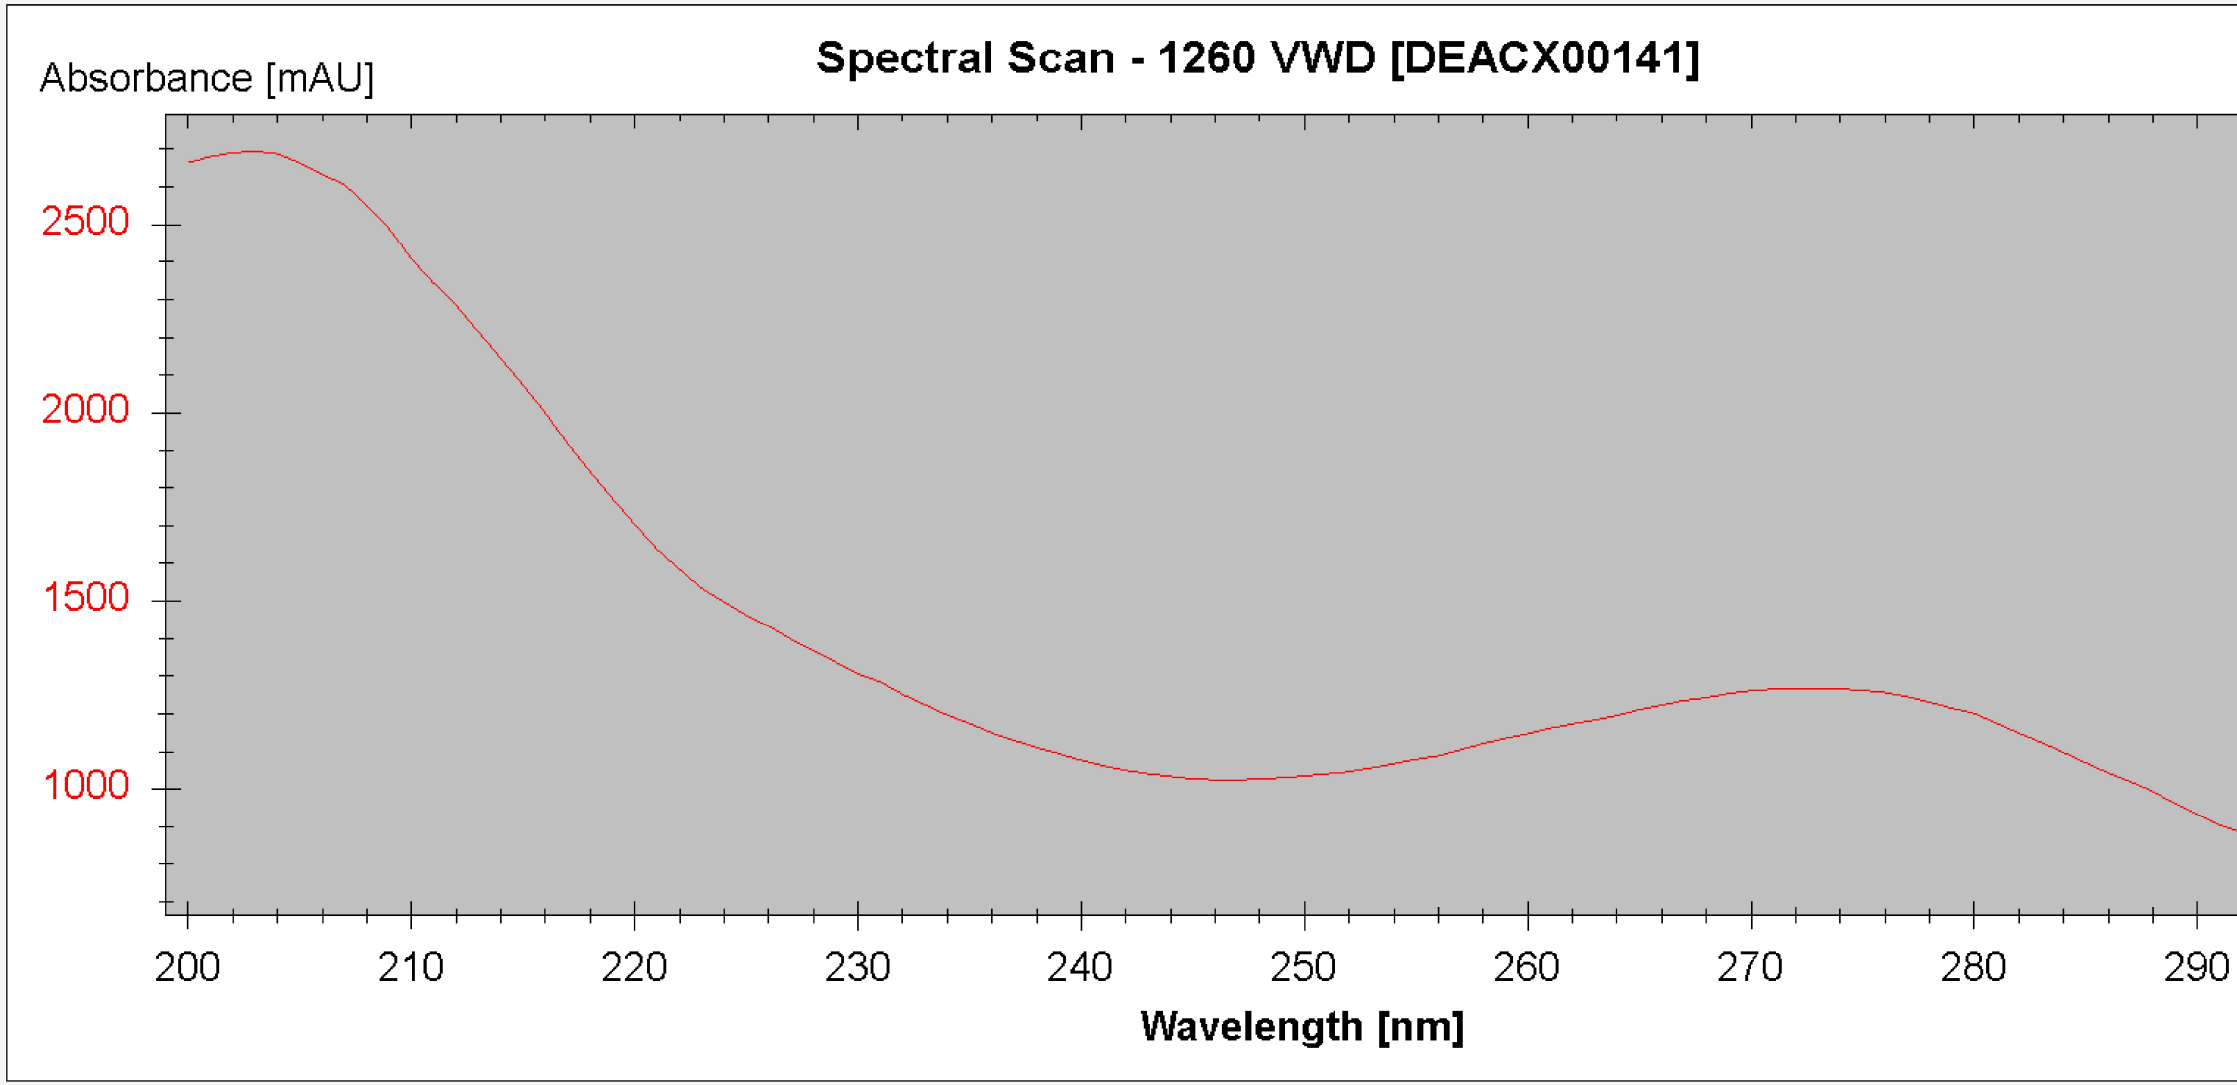


more...

Version B.02

Spectral Scan - 1260 VWD [DEACX00141]

UV Lamp On | Blank Scan


Sample Scan | from 200 | to 300 | step 1

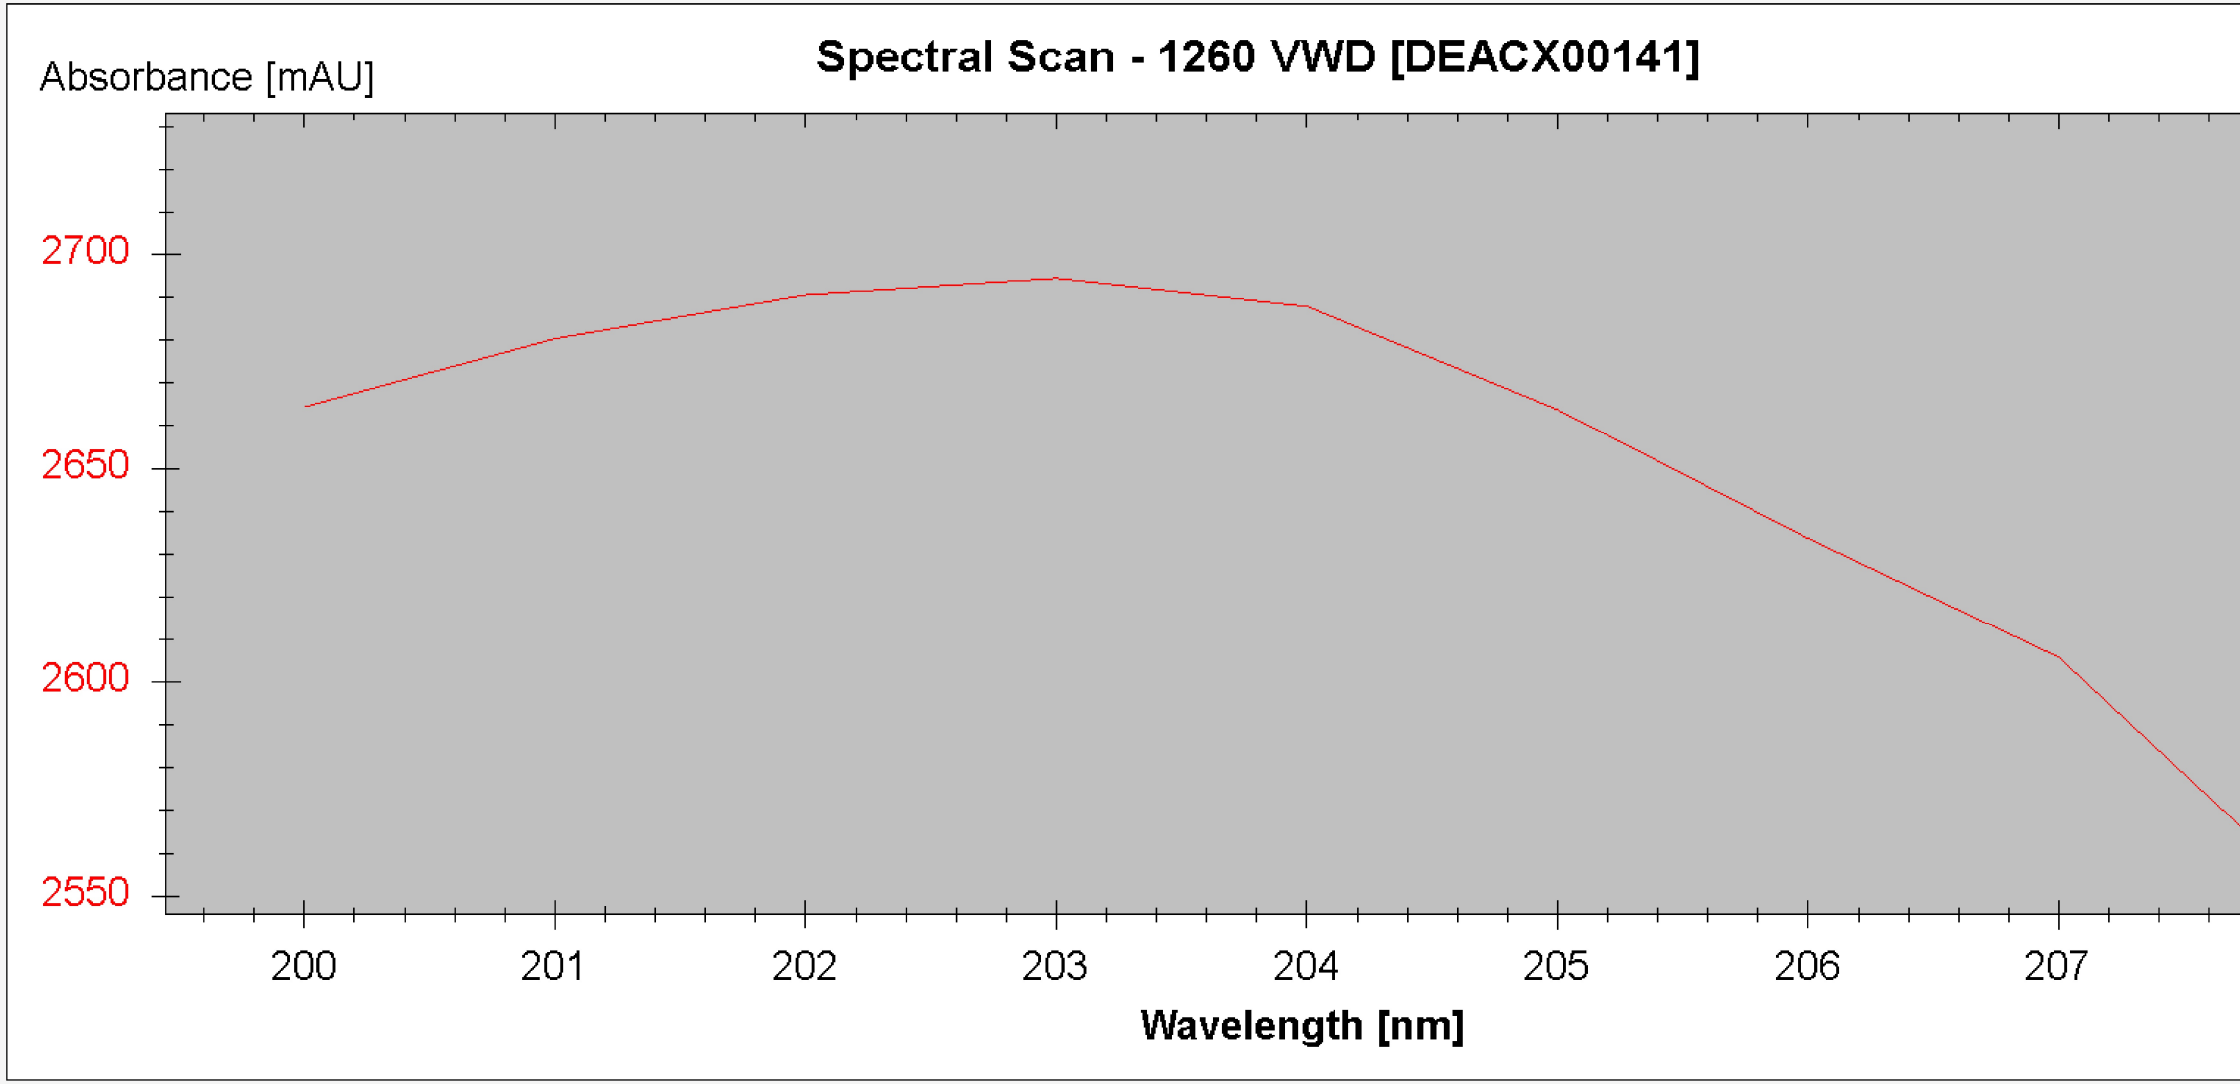

Spectral Scan - 1260 VWD [DEACX00141]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1

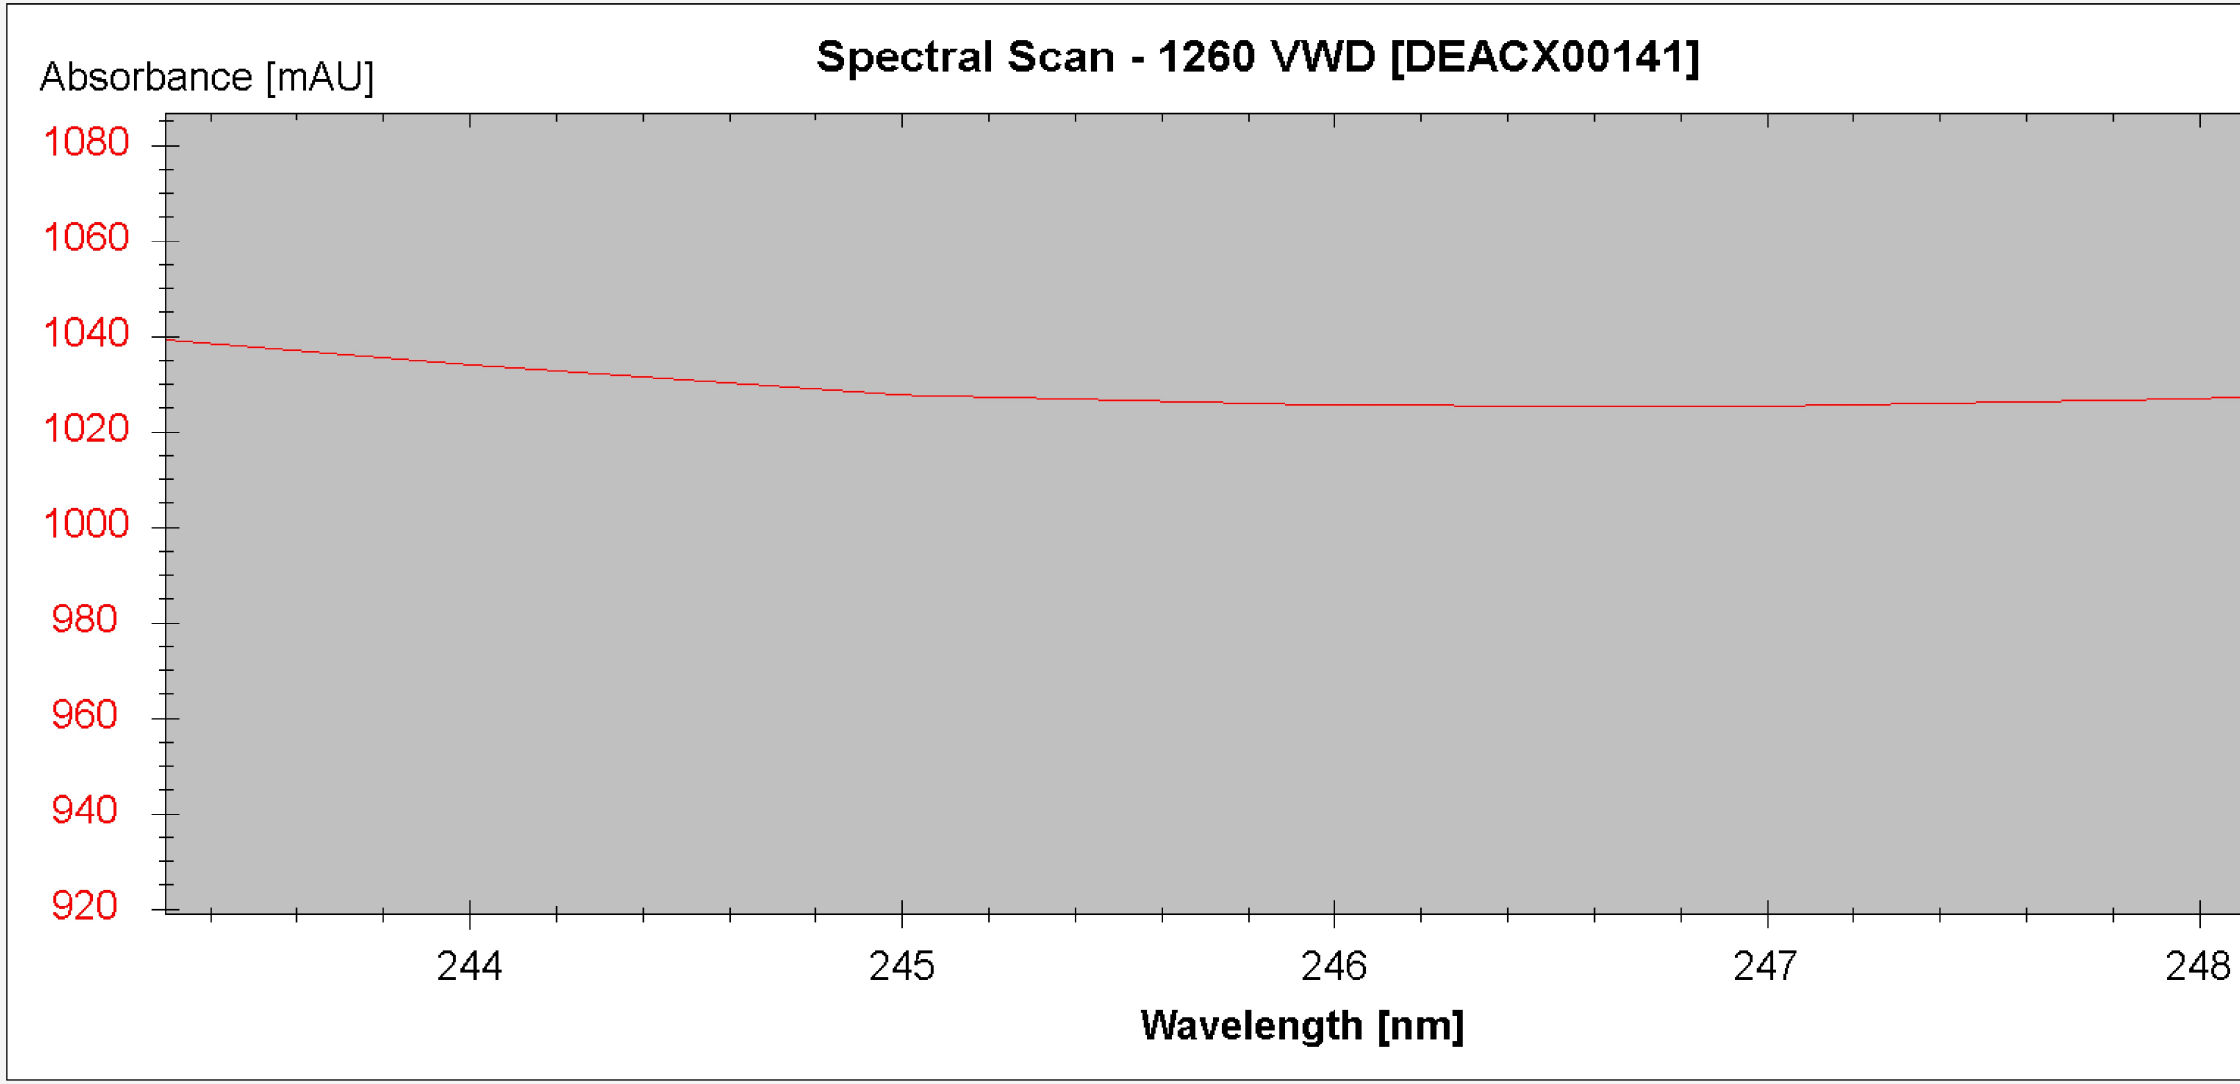

HPLC - Agilent Lab Advisor

visor

Service & Diagnostics


Spectral Scan

HPLC

Spectral Scan - 1260 VWD [DEACX00141]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1

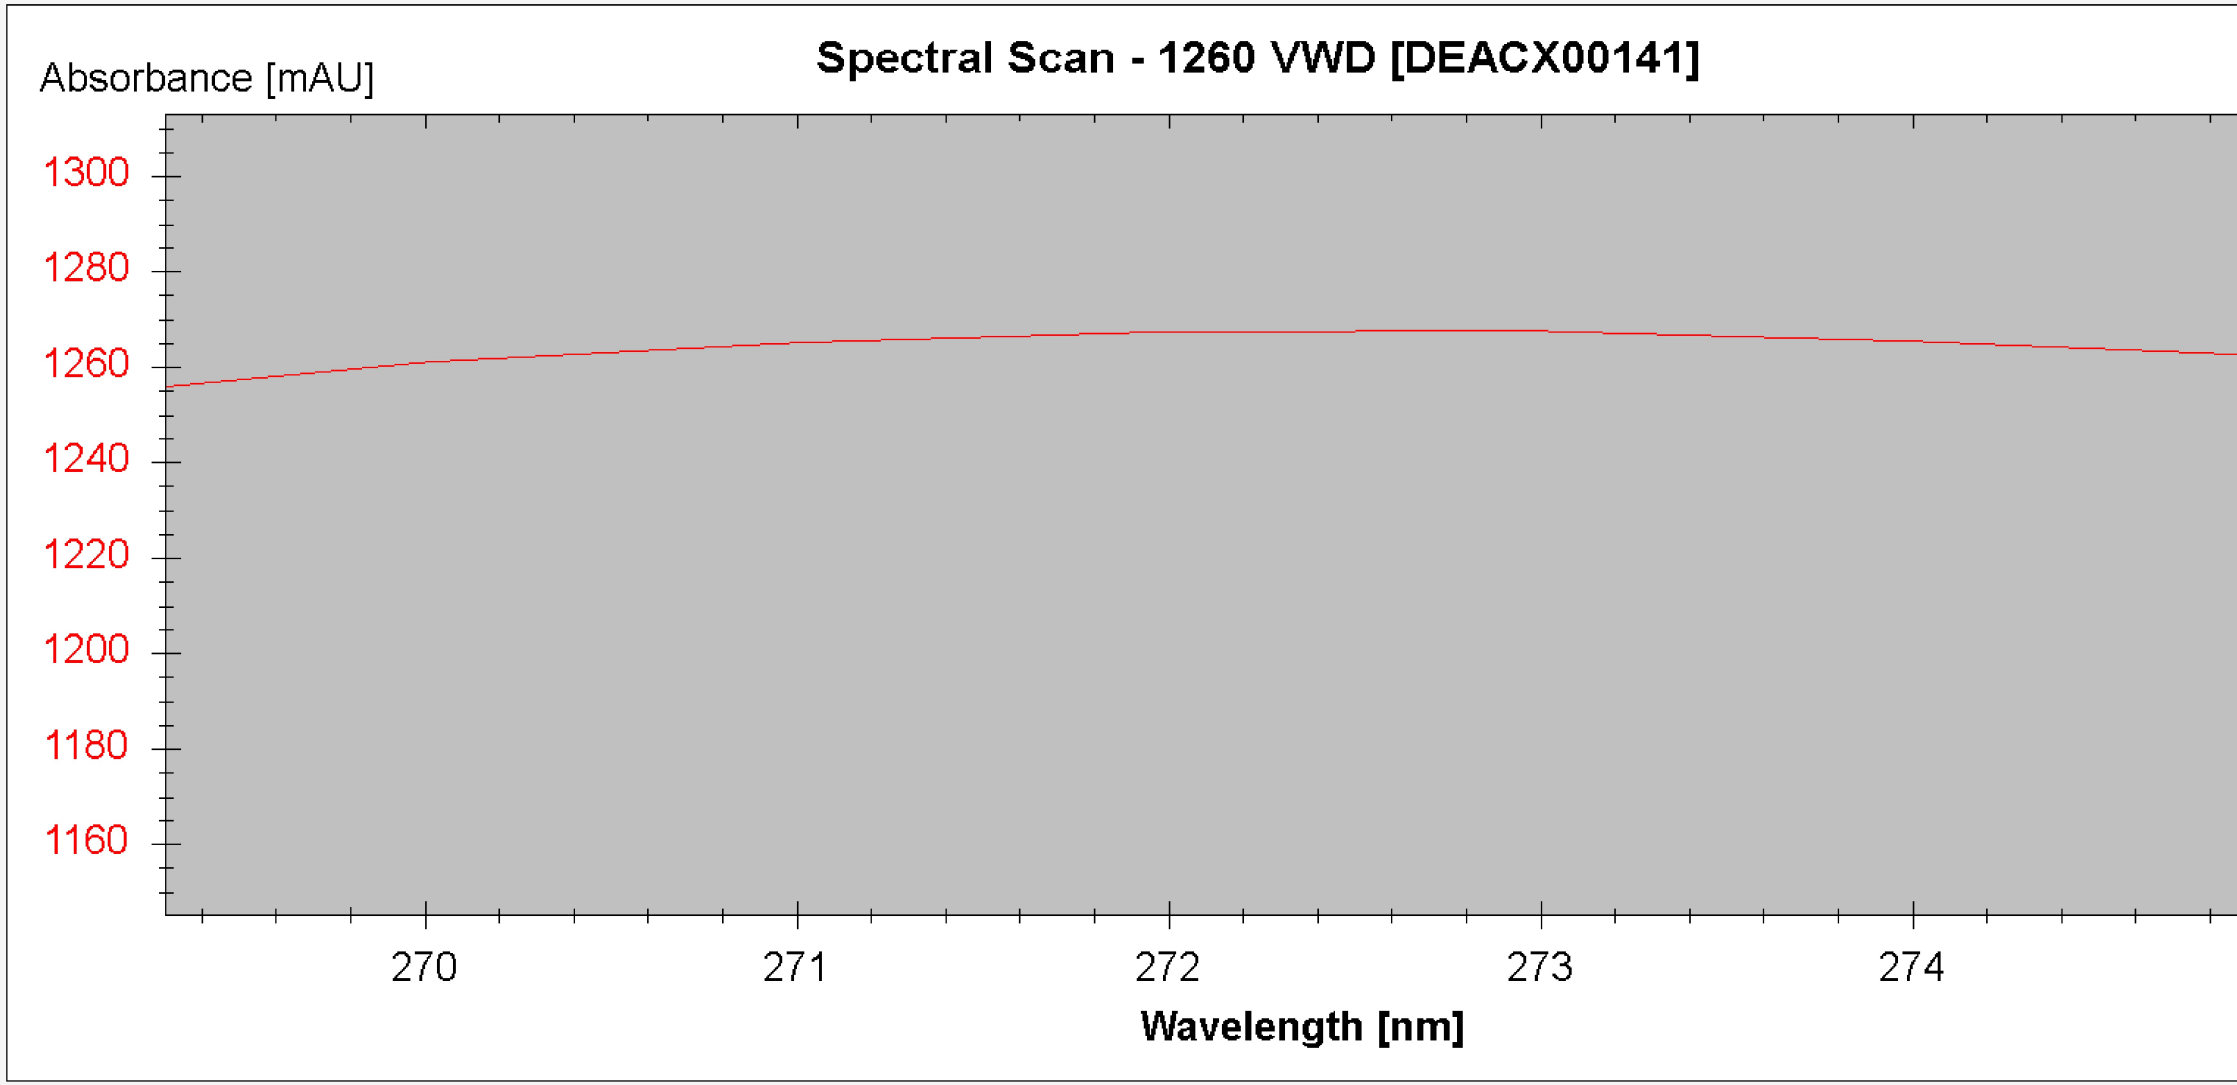


more...

Version B.02

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\001-P2-A1-Branco PCIN 001.D
Sample Name: Branco PCIN 001

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Acq. Instrument : HPLC 2                         Location :   P2-A1
Injection Date  : 3/24/2022 12:33:56 PM               Inj :   1
                                                Inj Volume : 10.000 µl
Method          : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Method Info     : Qualificacao
```

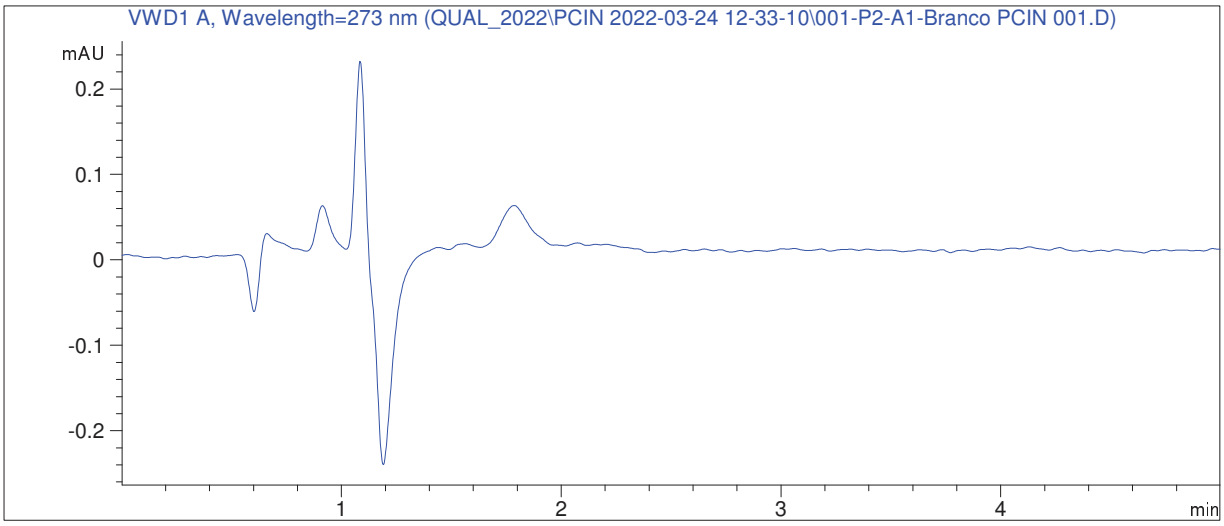


```
==========================================================================
                          Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\002-P2-A2-PCIN 001.D
Sample Name: PCIN 001

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   2
Acq. Instrument : HPLC 2                           Location :   P2-A2
Injection Date  : 3/24/2022 12:40:00 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

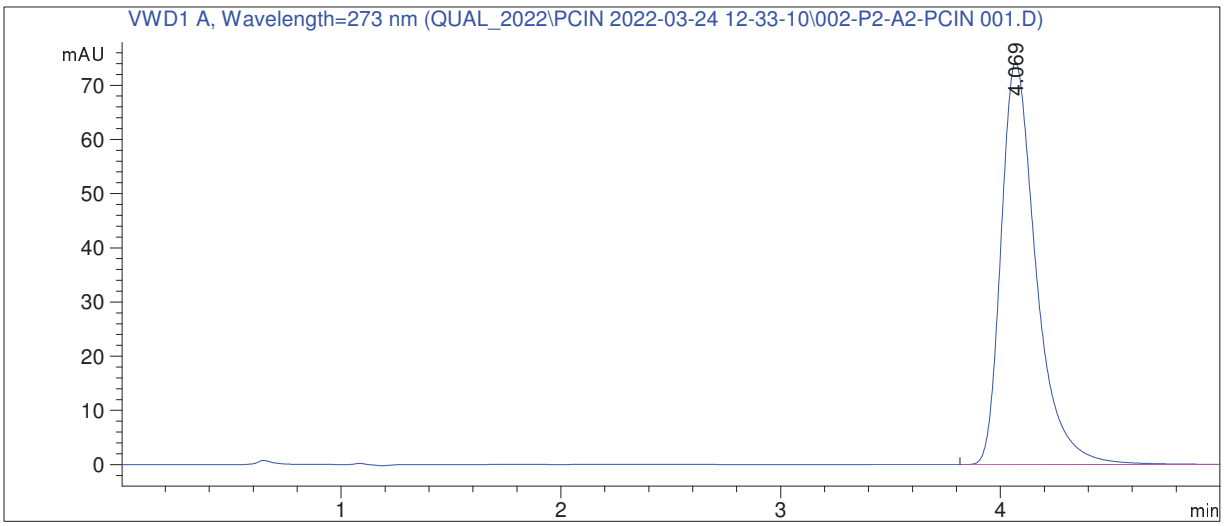


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.069 BBA     0.1682  821.88025 100.0000 Cafeina

Totals :                     821.88025


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\003-P2-A2-PCIN 002.D
Sample Name: PCIN 002

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Acq. Instrument : HPLC 2                           Location :   P2-A2
Injection Date  : 3/24/2022 12:46:06 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

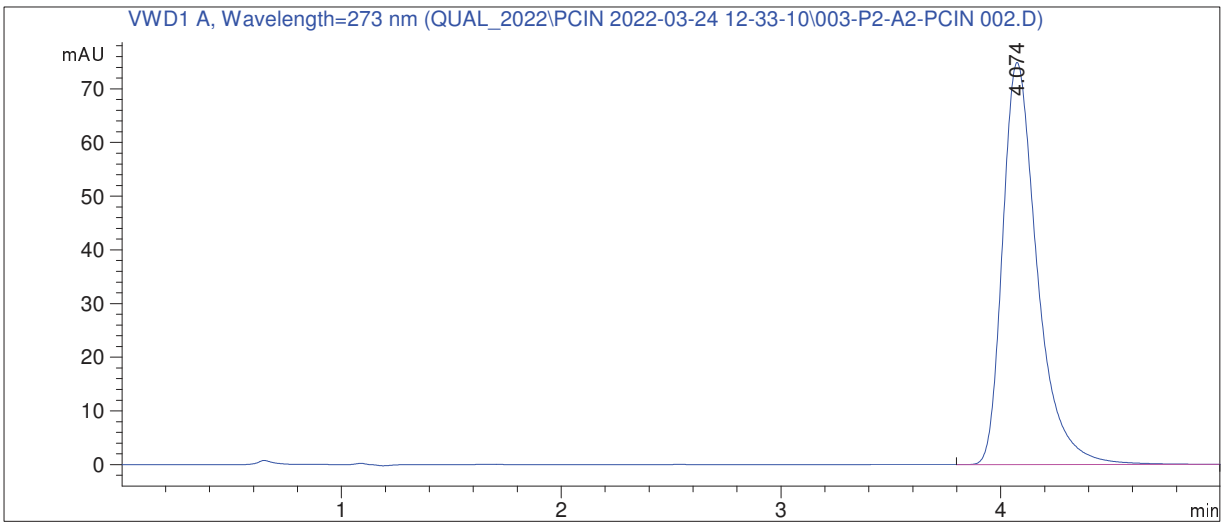


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.074 BBA     0.1668  820.34015 100.0000 Cafeina

Totals :                    820.34015


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\004-P2-A2-PCIN 003.D
Sample Name: PCIN 003

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Acq. Instrument : HPLC 2                           Location :   P2-A2
Injection Date  : 3/24/2022 12:52:09 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

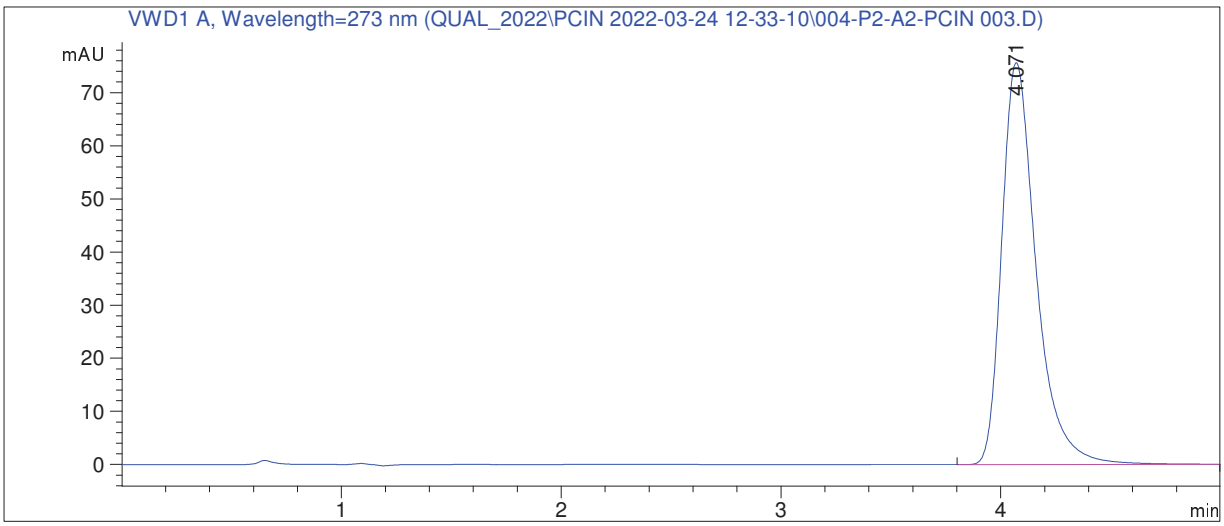


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.071 BBA     0.1647  822.25781 100.0000 Cafeina

Totals :                     822.25781


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\005-P2-A1-Branco PCIN 002.D
Sample Name: Branco PCIN 002

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   5
Acq. Instrument : HPLC 2                           Location :   P2-A1
Injection Date  : 3/24/2022 12:58:05 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method      : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed     : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed     : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info      : Qualificacao
```

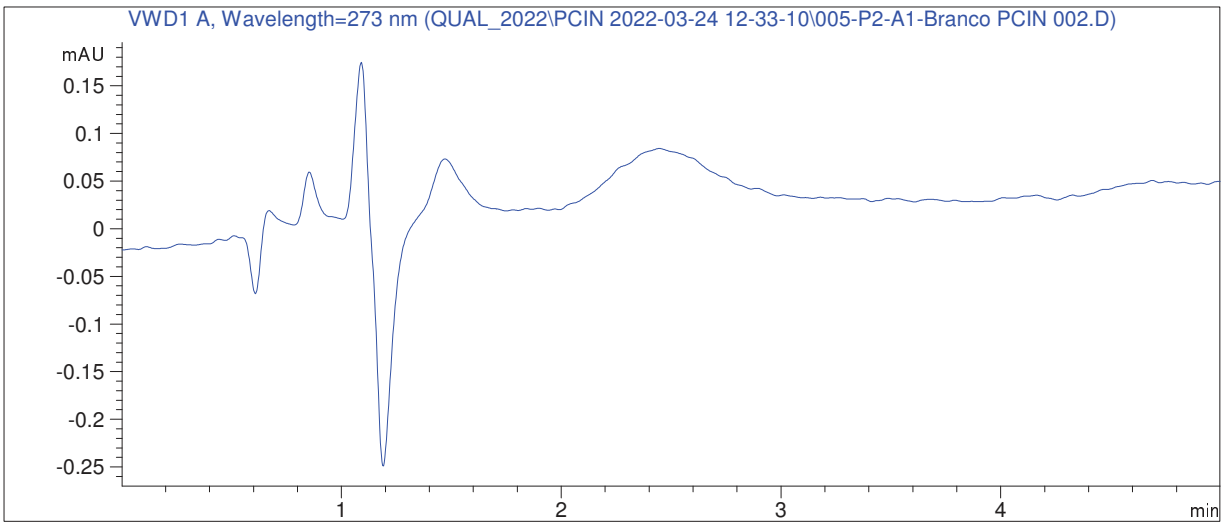


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.069         0.0000    0.00000   0.0000 Cafeina

Totals :                       0.00000



1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\006-P2-A2-PCIN 004.D
Sample Name: PCIN 004

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   6
Acq. Instrument : HPLC 2                           Location :   P2-A2
Injection Date  : 3/24/2022 1:04:03 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

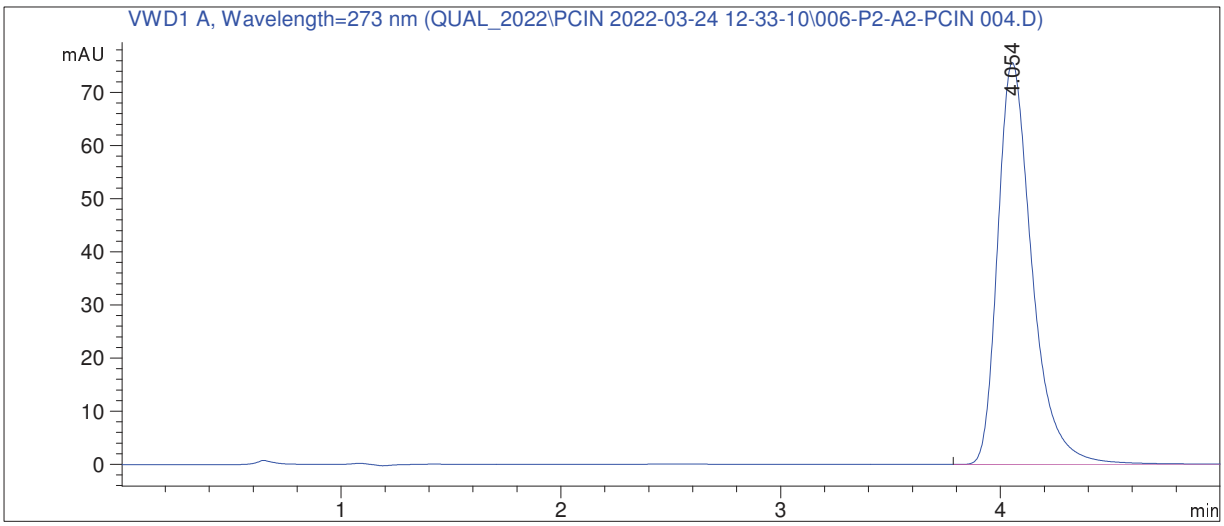


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.054 BBA     0.1656  820.87335 100.0000 Cafeina

Totals :                     820.87335


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\007-P2-A2-PCIN 005.D
Sample Name: PCIN 005

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   7
Acq. Instrument : HPLC 2                           Location :   P2-A2
Injection Date  : 3/24/2022 1:09:59 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:23:20 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

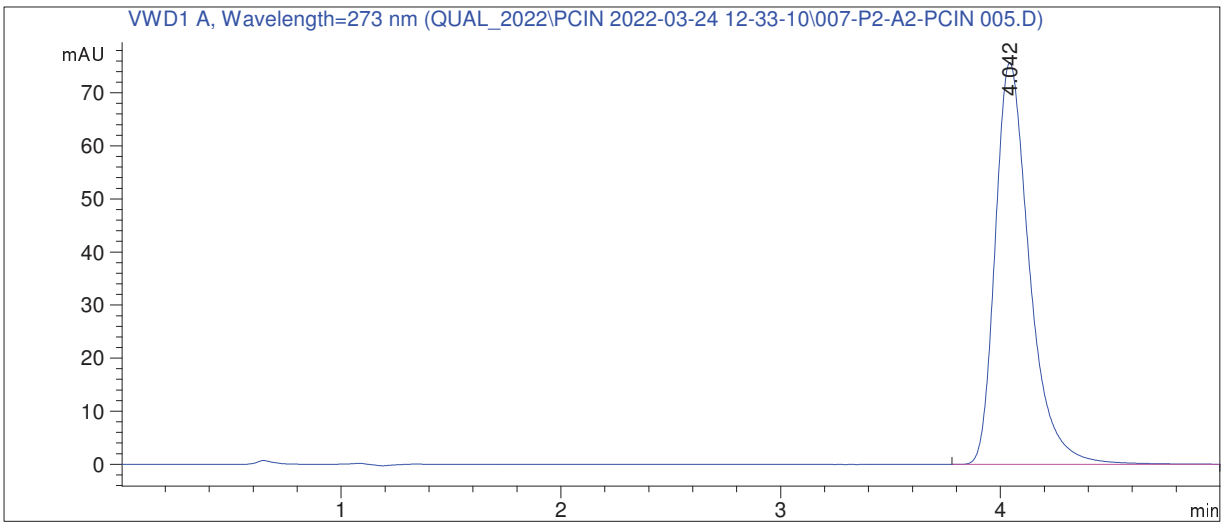


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.042 BBA     0.1653  819.89502 100.0000 Cafeina

Totals :                     819.89502


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\008-P2-A2-PCIN 006.D
Sample Name: PCIN 006

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   8
Acq. Instrument  : HPLC 2                           Location :   P2-A2
Injection Date   : 3/24/2022 1:16:02 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method      : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M
Last changed     : 3/24/2022 12:33:10 PM by SYSTEM
Analysis Method  : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                   Sequence Method)
Last changed     : 3/24/2022 1:23:20 PM by SYSTEM
                   (modified after loading)
Method Info      : Qualificacao
```

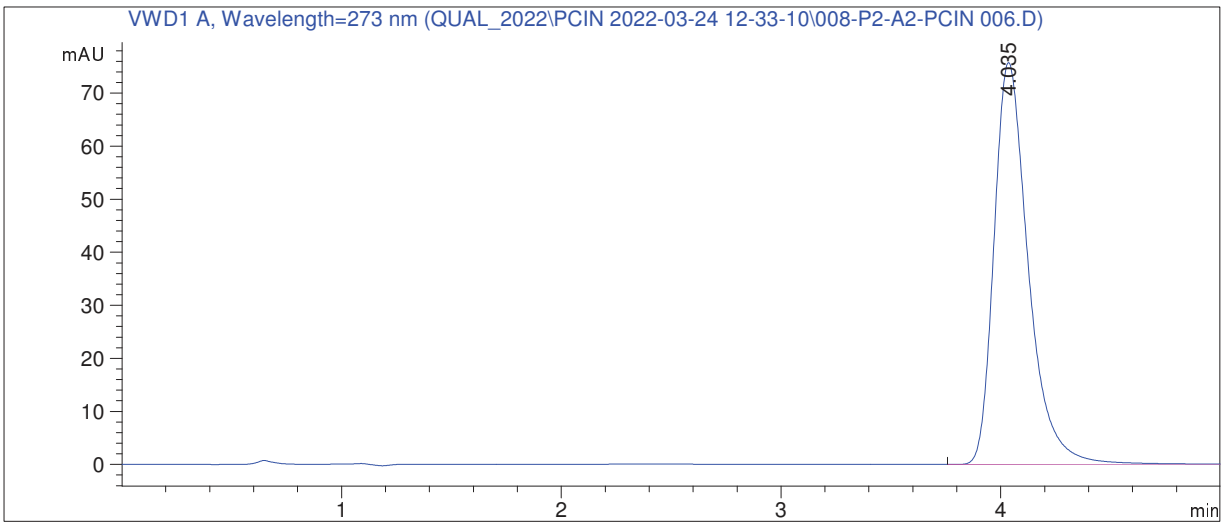


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Thursday, March 24, 2022 1:23:05 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   4.035 BBA     0.1654  821.08984 100.0000 Cafeina

Totals :                     821.08984


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\009-P2-A1-Branco PCIN 003.D
Sample Name: Branco PCIN 003

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   9
Acq. Instrument : HPLC 2                         Location :   P2-A1
Injection Date  : 3/24/2022 1:22:00 PM                Inj :   1
                                                Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\PCIN.S
Method          : C:\Chem32\3\Data\QUAL_2022\PCIN 2022-03-24 12-33-10\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 12:33:10 PM by SYSTEM
Method Info     : Qualificacao
```

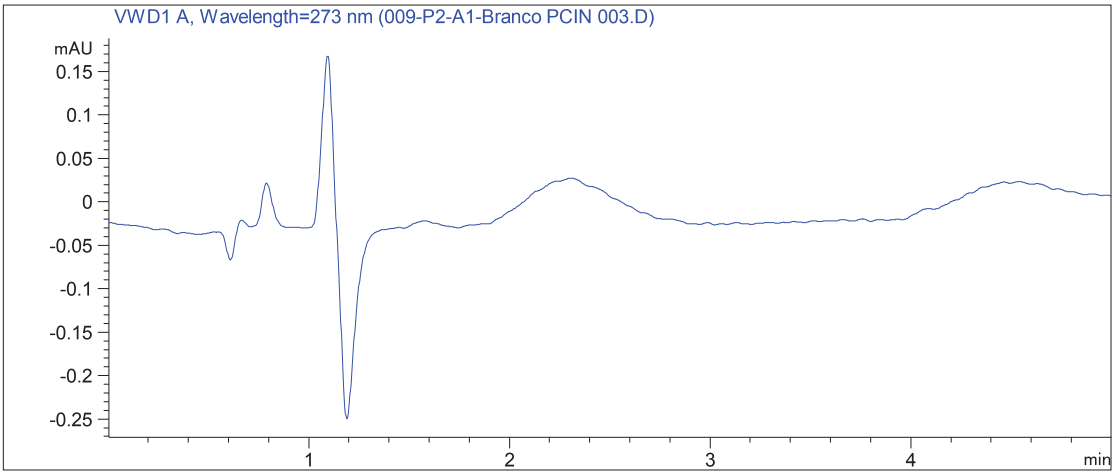


```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

=====================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\001-P2-A3-LDUV 001.D
Sample Name: LDUV 001

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   1
Acq. Instrument : HPLC 2                          Location :   P2-A3
Injection Date  : 3/24/2022 1:30:58 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\LDUV.S
Method          : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:30:13 PM by SYSTEM
Method Info     : Qualificacao
```

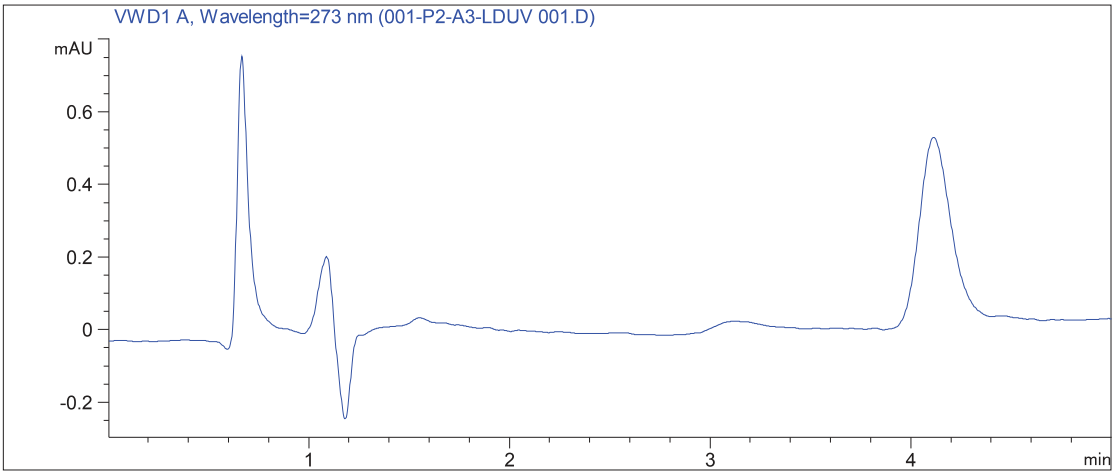


```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

=====================================================================
                         *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\002-P2-A4-LDUV 002.D
Sample Name: LDUV 002

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   2
Acq. Instrument : HPLC 2                           Location :   P2-A4
Injection Date  : 3/24/2022 1:37:16 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\LDUV.S
Method          : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:30:13 PM by SYSTEM
Method Info     : Qualificacao
```

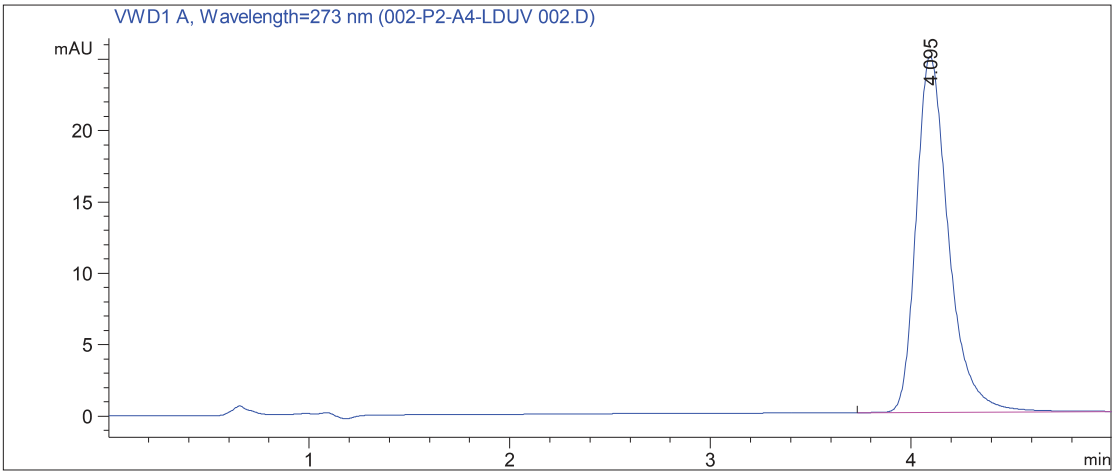


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.095 BBA   0.1695  279.09070   24.94384 100.0000

Totals :                   279.09070   24.94384


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\003-P2-A5-LDUV 003.D
Sample Name: LDUV 003

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Acq. Instrument : HPLC 2                           Location :   P2-A5
Injection Date  : 3/24/2022 1:43:18 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M
Last changed    : 3/24/2022 1:30:13 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 1:50:53 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

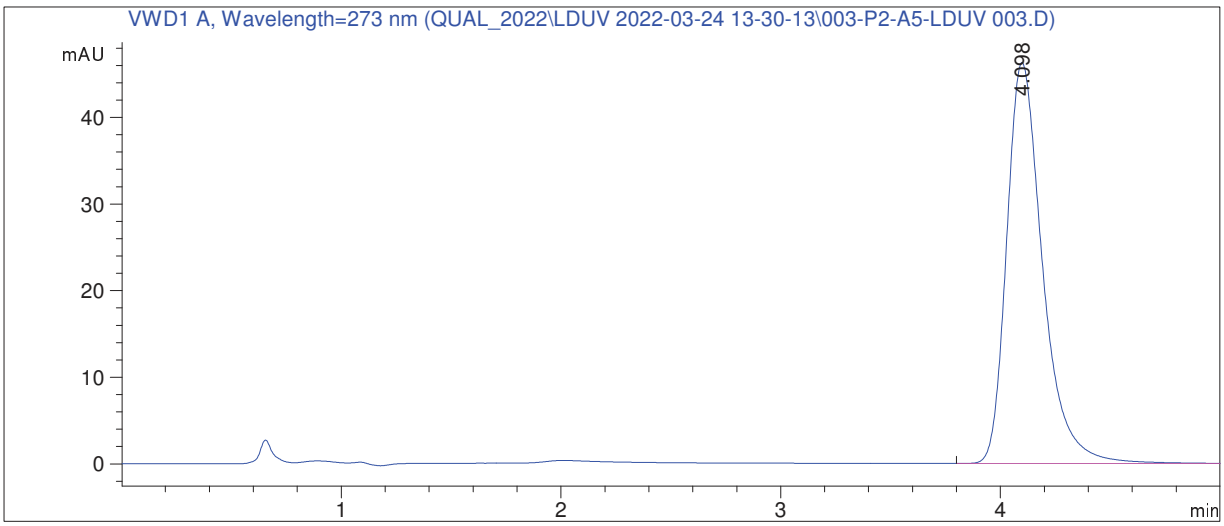


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.098 BBA   0.1724  525.46216   46.29479 100.0000

Totals :                   525.46216   46.29479


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\004-P2-A6-LDUV 004.D
Sample Name: LDUV 004

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Acq. Instrument : HPLC 2                           Location :   P2-A6
Injection Date  : 3/24/2022 1:49:15 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method      : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M
Last changed     : 3/24/2022 1:30:13 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M (
                  Sequence Method)
Last changed     : 3/24/2022 2:04:41 PM by SYSTEM
                  (modified after loading)
Method Info      : Qualificacao
```

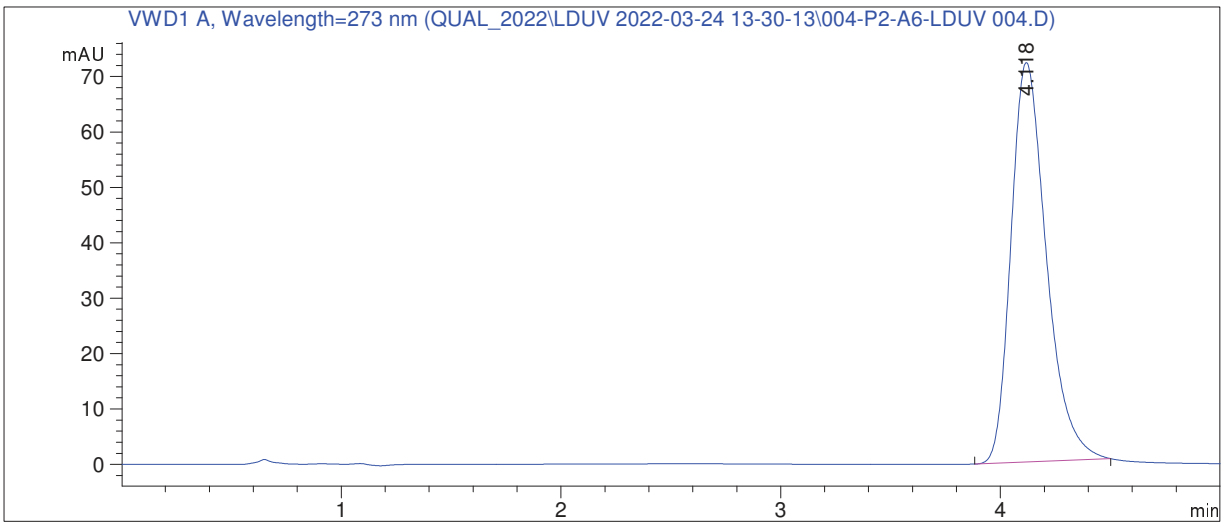


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.118 BBA   0.1724  806.35992   72.12197 100.0000

Totals :                   806.35992   72.12197


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\005-P2-A7-LDUV 005.D
Sample Name: LDUV 005

```
======================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   5
Acq. Instrument : HPLC 2                           Location :   P2-A7
Injection Date  : 3/24/2022 1:55:14 PM                  Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M
Last changed    : 3/24/2022 1:30:13 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\LDUV 2022-03-24 13-30-13\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:04:41 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

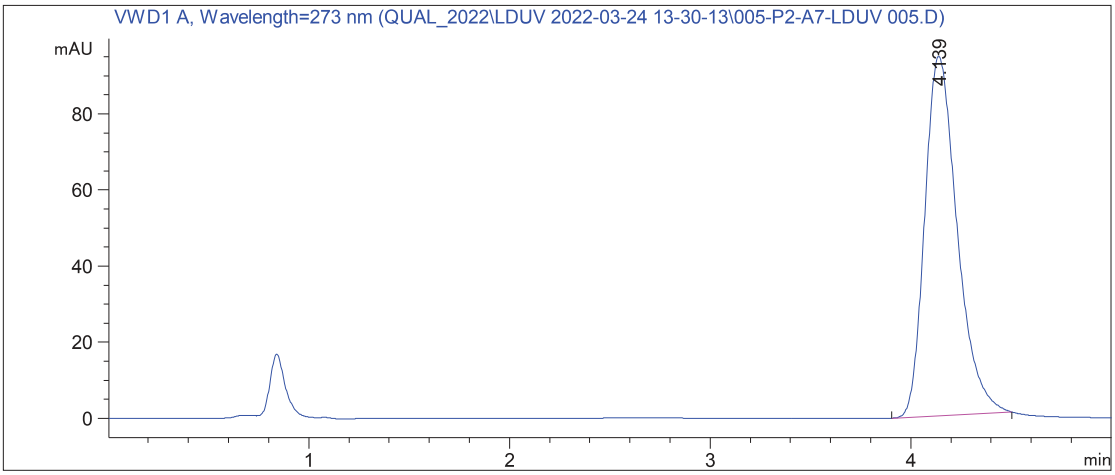


```
======================================================================
                        Area Percent Report
======================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.139 BBA   0.1720 1060.11975   94.37908 100.0000

Totals :                  1060.11975   94.37908


======================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\001-P2-A8-LIIN 001.D
Sample Name: LIIN 001

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   1
Acq. Instrument : HPLC 2                          Location :   P2-A8
Injection Date  : 3/24/2022 2:32:51 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\LIIN.S
Method          : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:32:07 PM by SYSTEM
Method Info     : Qualificacao
```

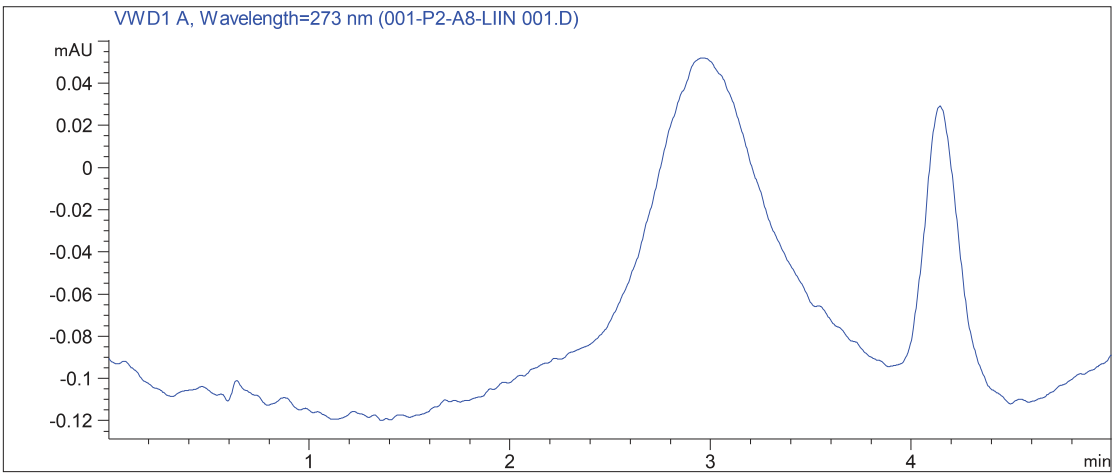


```
=====================================================================
                        Area Percent Report
=====================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

=====================================================================
                         *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\002-P2-A8-LIIN 002.D
Sample Name: LIIN 002

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   2
Acq. Instrument : HPLC 2                          Location :   P2-A8
Injection Date  : 3/24/2022 2:38:51 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 5.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\LIIN.S
Method          : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:32:07 PM by SYSTEM
Method Info     : Qualificacao
```

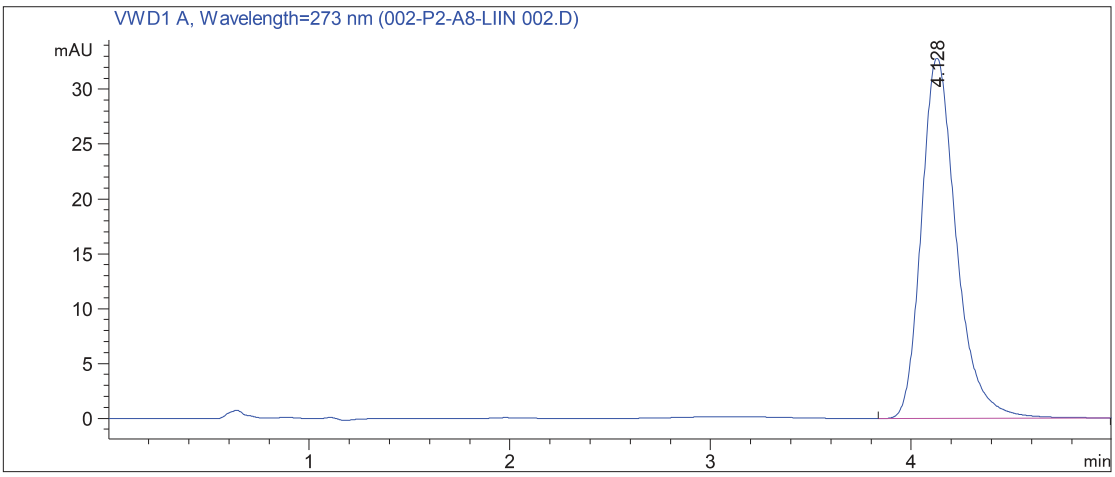


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.128 BBA   0.1839  397.11404   32.87136 100.0000

Totals :                   397.11404   32.87136


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\003-P2-A8-LIIN 003.D
Sample Name: LIIN 003

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   3
Acq. Instrument : HPLC 2                         Location :   P2-A8
Injection Date  : 3/24/2022 2:44:46 PM                Inj :   1
                                               Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\LIIN.S
Method          : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:32:07 PM by SYSTEM
Method Info     : Qualificacao
```

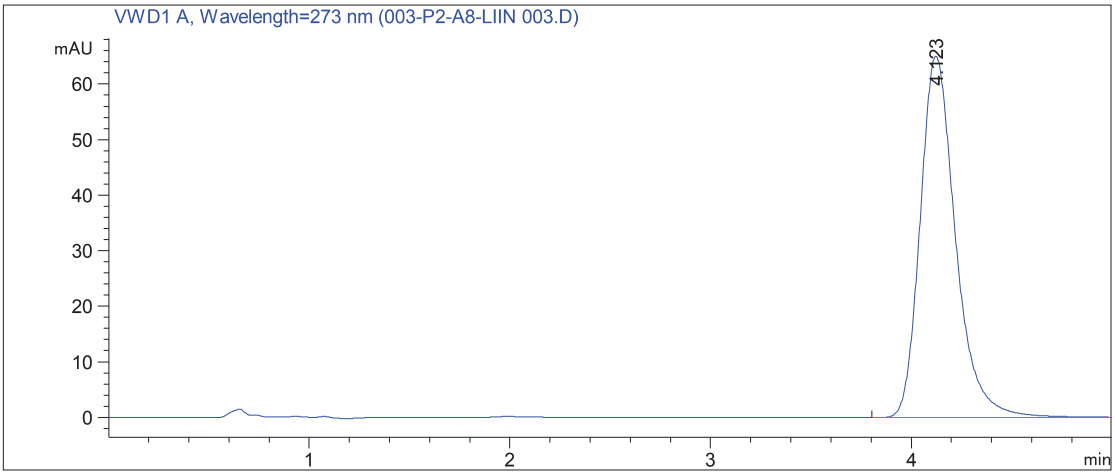


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.123 BBA   0.1869  796.69141   65.05025 100.0000

Totals :                   796.69141   65.05025


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\004-P2-A8-LIIN 004.D
Sample Name: LIIN 004

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Acq. Instrument : HPLC 2                           Location :   P2-A8
Injection Date  : 3/24/2022 2:50:52 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M
Last changed    : 3/24/2022 2:32:07 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:59:29 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

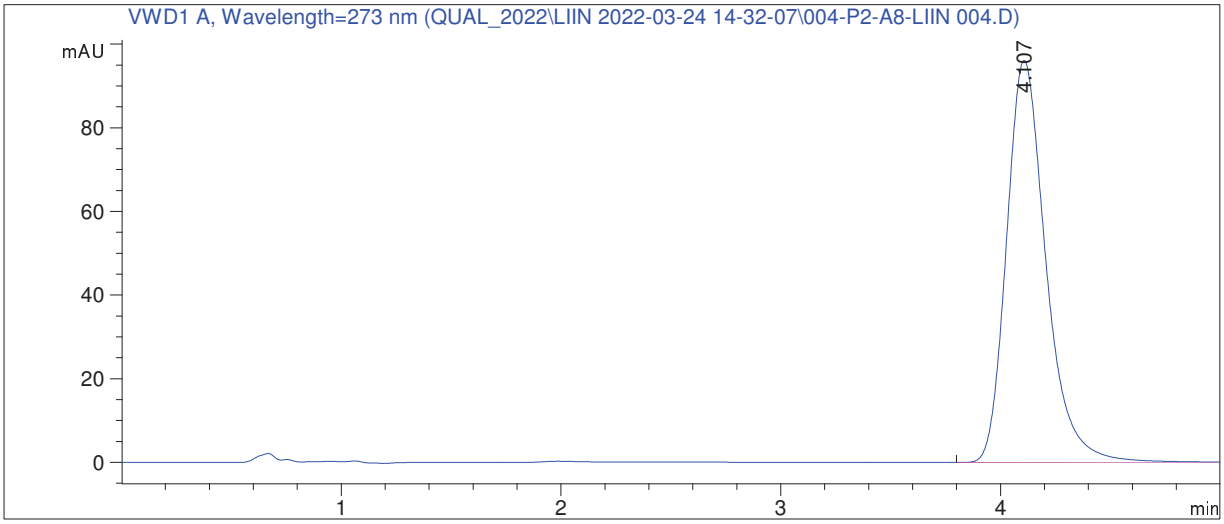


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.107 BBA   0.1901 1196.52783   96.17297 100.0000

Totals :                  1196.52783   96.17297


==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\005-P2-A8-LIIN 005.D
Sample Name: LIIN 005

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   5
Acq. Instrument : HPLC 2                           Location :   P2-A8
Injection Date  : 3/24/2022 2:56:58 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M
Last changed    : 3/24/2022 2:32:07 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2022\LIIN 2022-03-24 14-32-07\Qualificacao.M (
                  Sequence Method)
Last changed    : 3/24/2022 2:59:29 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

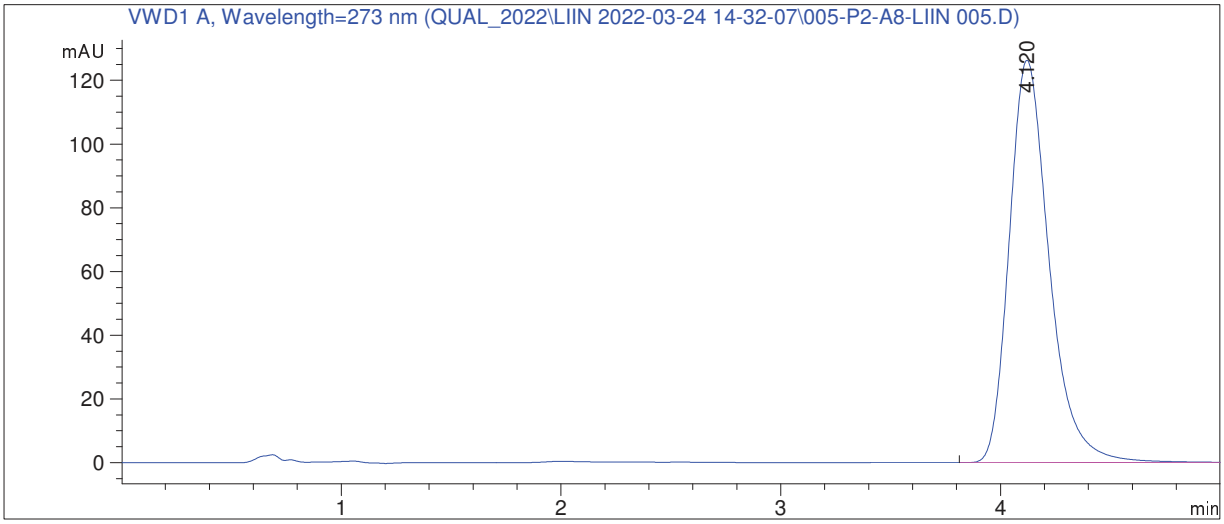


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   4.120 BBA   0.1934 1595.57544  126.31829 100.0000

Totals :                  1595.57544  126.31829



==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2022\GRAD 2022-03-24 15-26-30\001-P2-A1-GRAD AB.D
Sample Name: GRAD AB

==========

Acq. Operator : SYSTEM Seq. Line : 1
Acq. Instrument : HPLC 2 Location : P2-A1
Injection Date : 3/24/2022 3:27:17 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 0.000 µl
Method : C:\Chem32\3\Data\QUAL_2022\GRAD 2022-03-24 15-26-30\GRAD AB.M (Sequence Method)
Last changed : 3/24/2022 3:26:30 PM by SYSTEM
Method Info : Qualificacao Gradiente AB

Additional Info : Peak(s) manually integrated

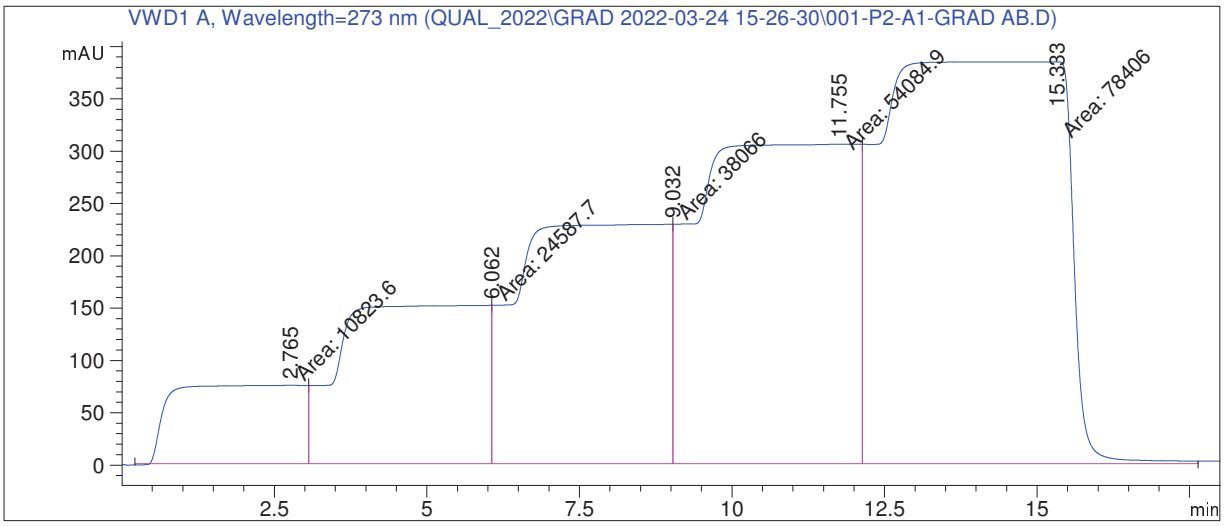

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.765	MF	2.4048	1.08236e4	75.01261	5.2550
2	6.062	FM	2.7070	2.45877e4	151.38564	11.9376
3	9.032	FM	2.7718	3.80660e4	228.88896	18.4815
4	11.755	FM	2.9532	5.40849e4	305.23376	26.2589
5	15.333	FM	3.4025	7.84060e4	384.05804	38.0670
Totals :				2.05968e5	1144.57902	

==========

*** End of Report ***


Data File C:\Chem32\3\Data\QUAL_2022\GRAD 2022-03-24 16-15-55\001-P2-A1-GRAD CD.D
Sample Name: GRAD CD

==========

Acq. Operator	: SYSTEM	Seq. Line	: 1
Acq. Instrument	: HPLC 2	Location	: P2-A1
Injection Date	: 3/24/2022 4:16:36 PM	Inj	: 1
		Inj Volume	: 10.000 µl

Different Inj Volume from Sample Entry! Actual Inj Volume : 0.000 µl
Method : C:\Chem32\3\Data\QUAL_2022\GRAD 2022-03-24 16-15-55\GRAD CD.M (Sequence Method)
Last changed : 3/24/2022 4:15:55 PM by SYSTEM
Method Info : Qualificacao Gradiente CD

Additional Info : Peak(s) manually integrated

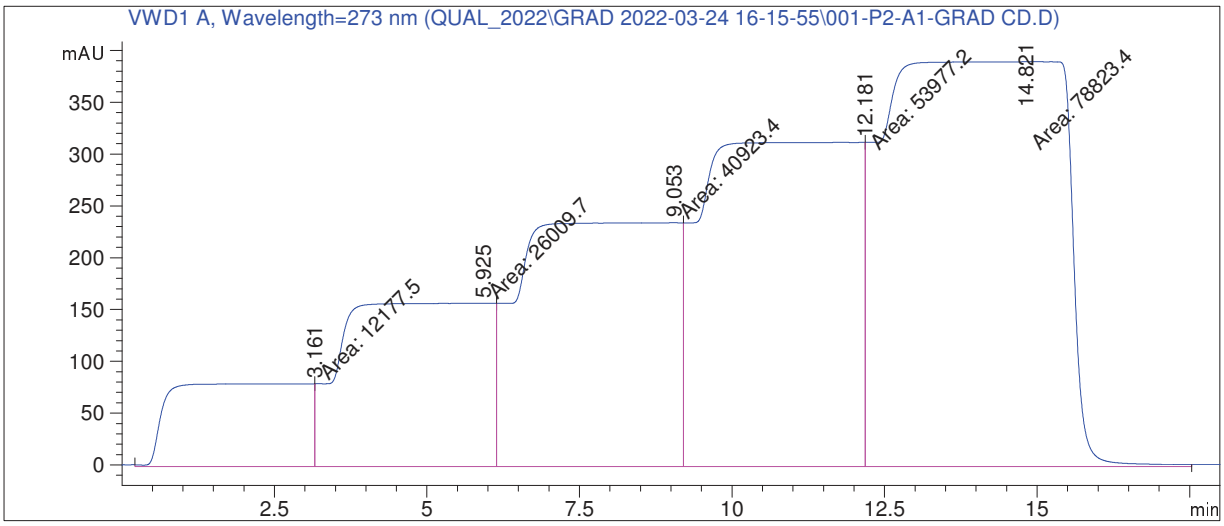

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.161	MF	2.5383	1.21775e4	79.95863	5.7465
2	5.925	FM	2.7504	2.60097e4	157.61426	12.2739
3	9.053	FM	2.8984	4.09234e4	235.32262	19.3116
4	12.181	FM	2.8754	5.39772e4	312.87094	25.4716
5	14.821	FM	3.3628	7.88234e4	390.66061	37.1964
Totals :				2.11911e5	1176.42706	

==========

*** End of Report ***