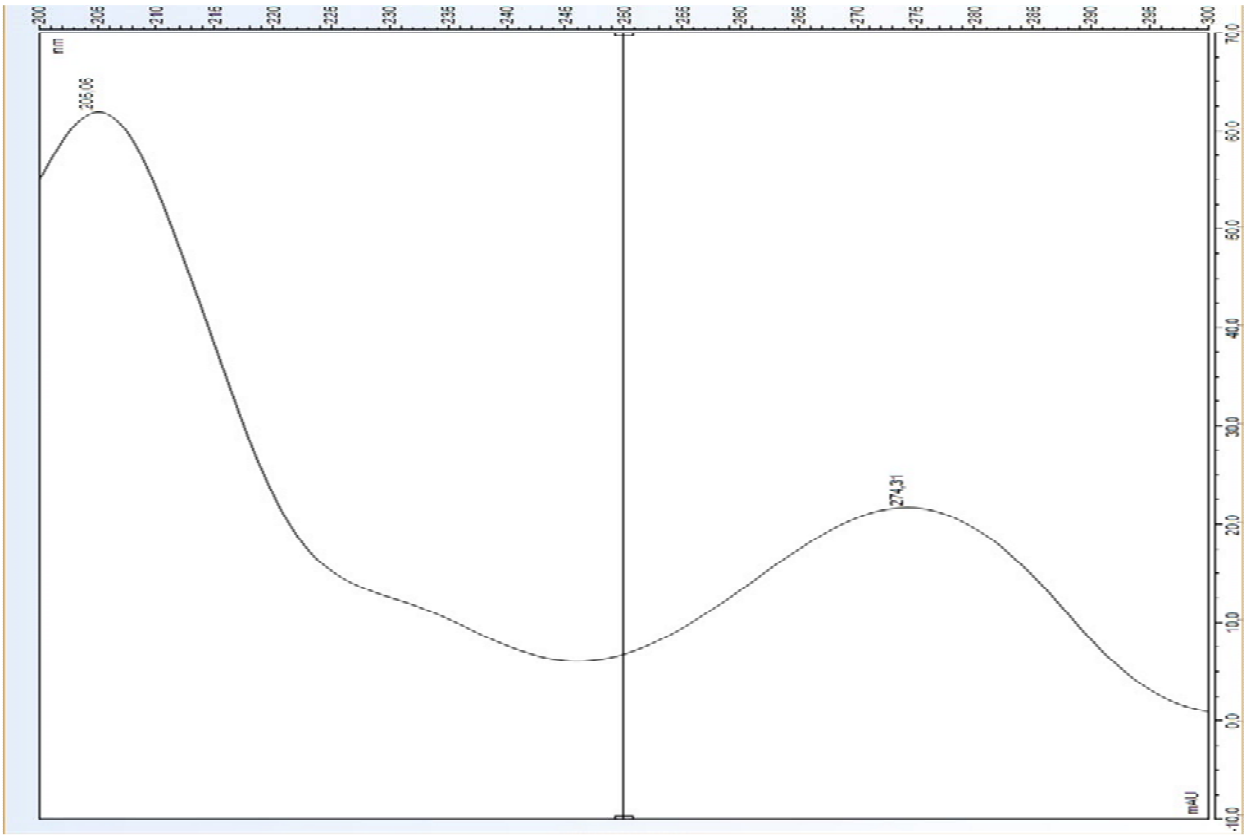



File Path chrom://clbap1357/ChromeleonLocal/Sequência/EDUV.seq/615.smp/3DFIELD.field
Channel UV_VIS_1

Injection Information:
Data Vault ChromeleonLocal
Injection EDUV
Injection Number 1
Position GA1
Comment
Processing Method Qualificação
Instrument Method Qualificação
Type Unknown
Status Finished
Injection Date 09/05/2018
Injection Time 10:39:49
Injection Volume (µl) 10,000
Dilution Factor 1,0000
Weight 1,0000

Raw Data Information:
Data Points 101
Wavelength Min. (nm) 200,000000
Wavelength Max. (nm) 300,000000
Retention Time (min) 1,780000

Raw Data:


| Wavelength (nm) | Value (mAU) |
|---|---|
| 200,0 | 55,030707 |
| 201,0 | 57,112936 |
| 202,0 | 59,018377 |
| 203,0 | 60,561422 |
| 204,0 | 61,520163 |
| 205,0 | 61,907712 |
| 206,0 | 61,589781 |
| 207,0 | 60,619715 |
| 208,0 | 59,013072 |
| 209,0 | 56,805018 |
| 210,0 | 54,154399 |
| 211,0 | 51,206592 |
| 212,0 | 48,030975 |
| 213,0 | 44,839266 |
| 214,0 | 41,569295 |
| 215,0 | 38,196566 |
| 216,0 | 34,877004 |
| 217,0 | 31,589152 |
| 218,0 | 28,399052 |
| 219,0 | 25,578441 |
| 220,0 | 23,001672 |
| 221,0 | 20,773054 |
| 222,0 | 18,898250 |
| 223,0 | 17,356516 |
| 224,0 | 16,154648 |
| 225,0 | 15,228630 |
| 226,0 | 14,460922 |
| 227,0 | 13,868929 |
| 228,0 | 13,365985 |
| 229,0 | 12,919844 |
| 230,0 | 12,531460 |
| 231,0 | 12,166799 |
| 232,0 | 11,776686 |
| 233,0 | 11,321307 |
| 234,0 | 10,841251 |
| 235,0 | 10,321141 |
| 236,0 | 9,786785 |
| 237,0 | 9,214521 |
| 238,0 | 8,651555 |
| 239,0 | 8,117378 |
| 240,0 | 7,639468 |
| 241,0 | 7,205427 |
| 242,0 | 6,828010 |
| 243,0 | 6,486476 |
| 244,0 | 6,257475 |
| 245,0 | 6,112516 |
| 246,0 | 6,048143 |
| 247,0 | 6,115258 |
| 248,0 | 6,244243 |
| 249,0 | 6,465674 |
| 250,0 | 6,772161 |
| 251,0 | 7,177651 |
| 252,0 | 7,639289 |
| 253,0 | 8,180619 |
| 254,0 | 8,773268 |
| 255,0 | 9,429277 |
| 256,0 | 10,135651 |
| 257,0 | 10,898770 |
| 258,0 | 11,683584 |
| 259,0 | 12,458921 |
| 260,0 | 13,310254 |
| 261,0 | 14,150501 |
| 262,0 | 15,014351 |
| 263,0 | 15,862108 |
| 264,0 | 16,691745 |
| 265,0 | 17,444135 |
| 266,0 | 18,231095 |
| 267,0 | 18,942298 |
| 268,0 | 19,586445 |
| 269,0 | 20,155610 |
| 270,0 | 20,650984 |
| 271,0 | 21,103503 |
| 272,0 | 21,402181 |
| 273,0 | 21,601499 |
| 274,0 | 21,683277 |
| 275,0 | 21,659852 |
| 276,0 | 21,498026 |
| 277,0 | 21,196188 |
| 278,0 | 20,771445 |
| 279,0 | 20,203472 |
| 280,0 | 19,570531 |
| 281,0 | 18,839658 |
| 282,0 | 17,968536 |
| 283,0 | 16,945065 |
| 284,0 | 15,860737 |
| 285,0 | 14,714838 |
| 286,0 | 13,505400 |
| 287,0 | 12,186886 |
| 288,0 | 10,849953 |
| 289,0 | 9,488822 |
| 290,0 | 8,220077 |
| 291,0 | 6,977499 |
| 292,0 | 5,883694 |
| 293,0 | 4,850149 |
| 294,0 | 3,935814 |
| 295,0 | 3,145874 |
| 296,0 | 2,486825 |
| 297,0 | 1,933396 |
| 298,0 | 1,496554 |
| 299,0 | 1,159906 |
| 300,0 | 0,908494 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *Branco 1* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 10:59* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

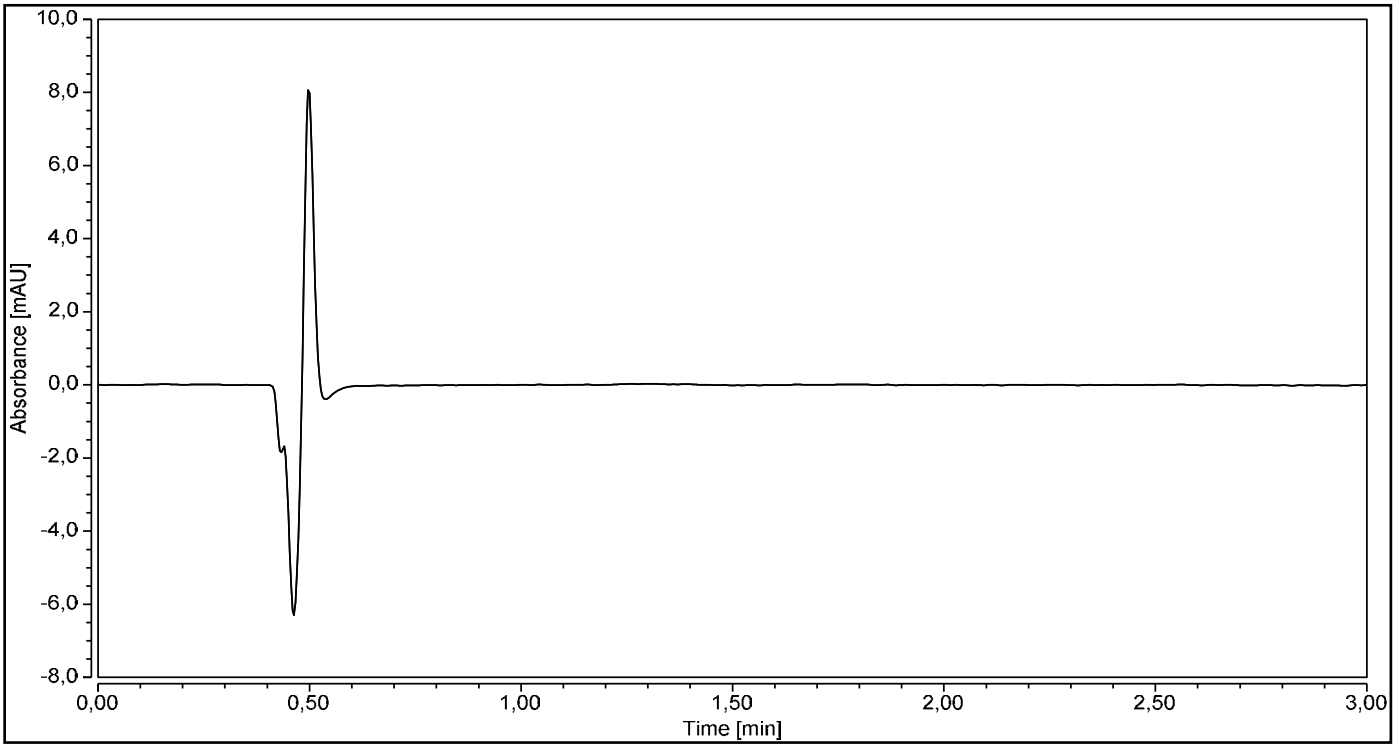


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 1* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:03* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

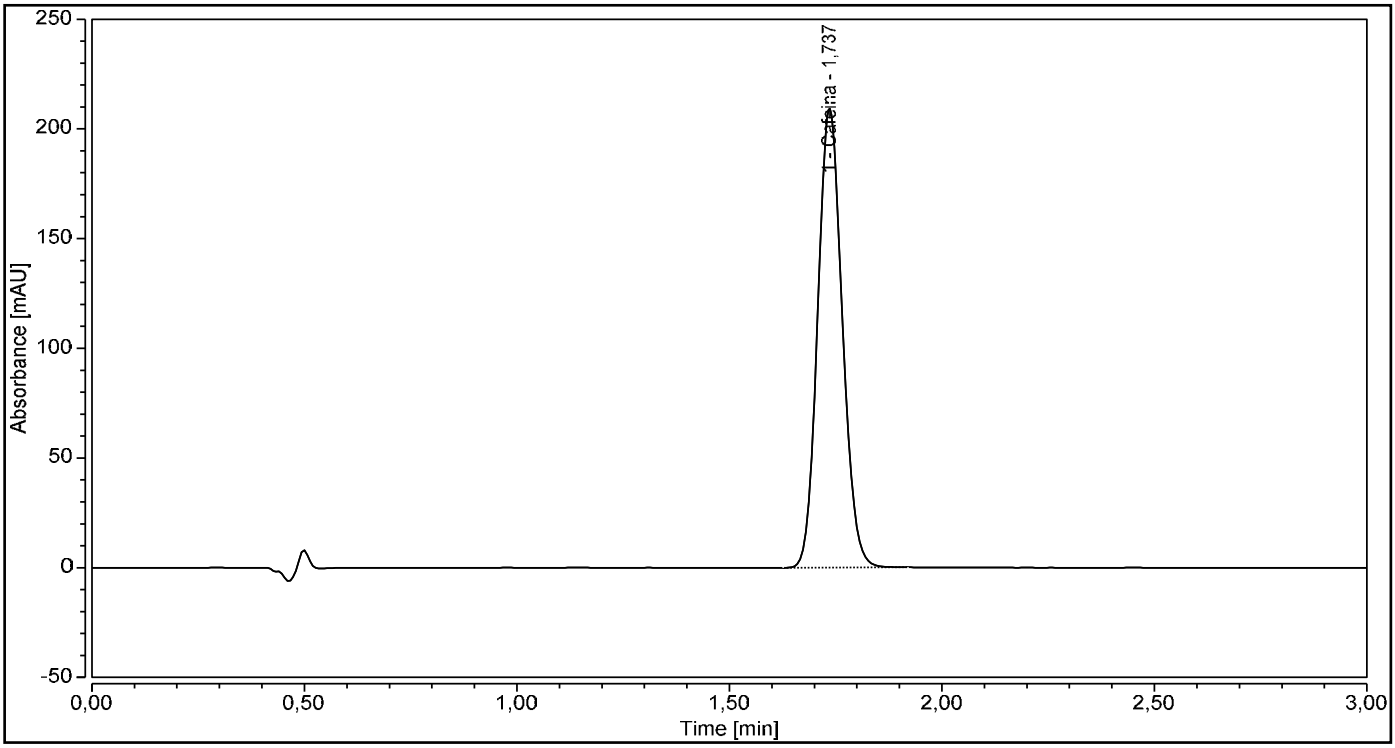


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,737 | 14,0123846 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 2* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:08* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

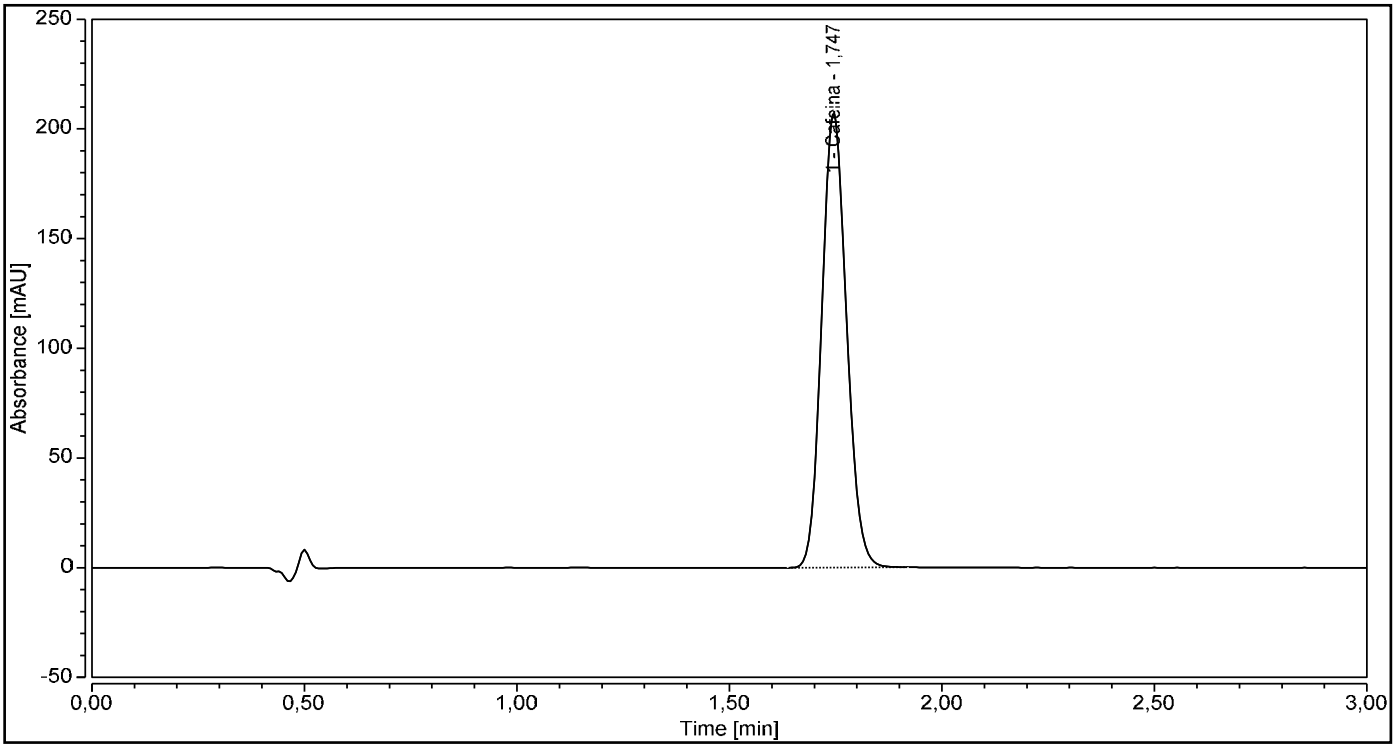


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,747 | 13,9925571 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 3* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:12* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

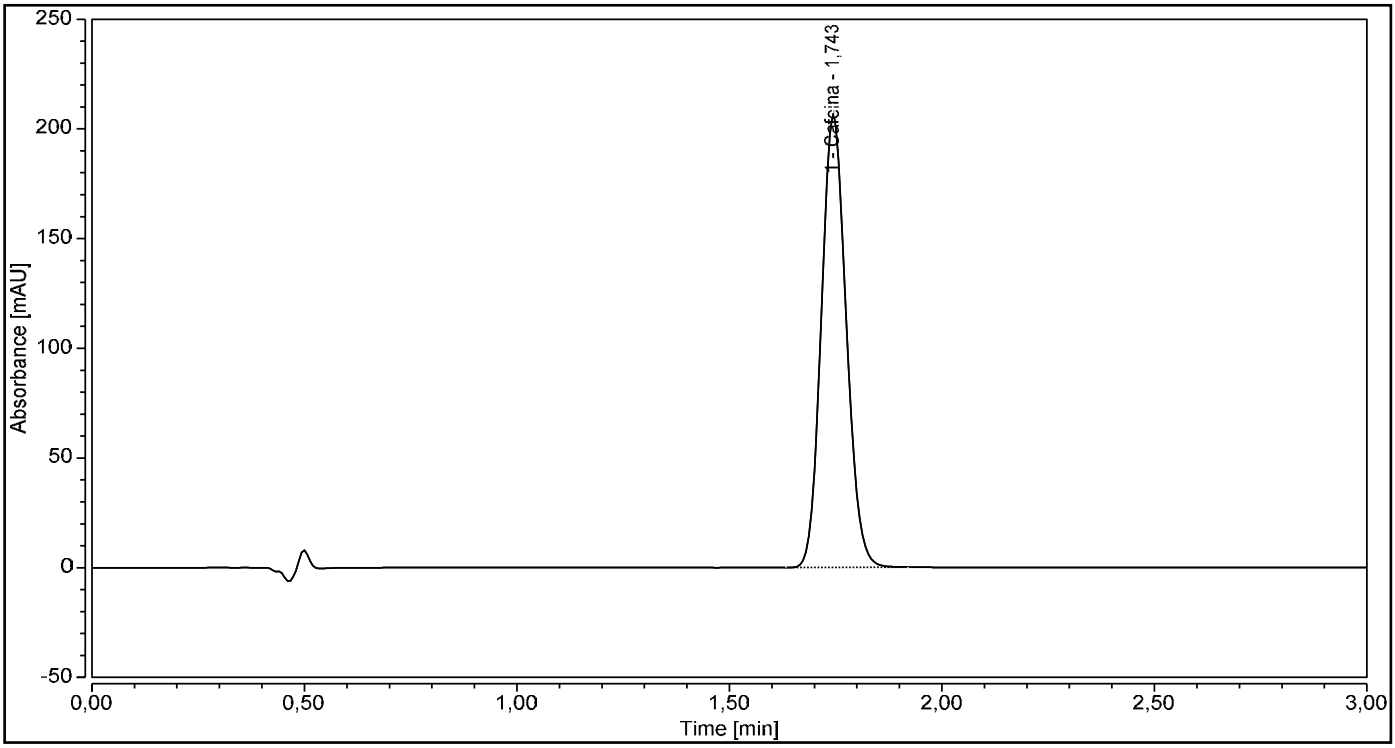


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,743 | 13,9830025 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *Branco 2* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:16* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

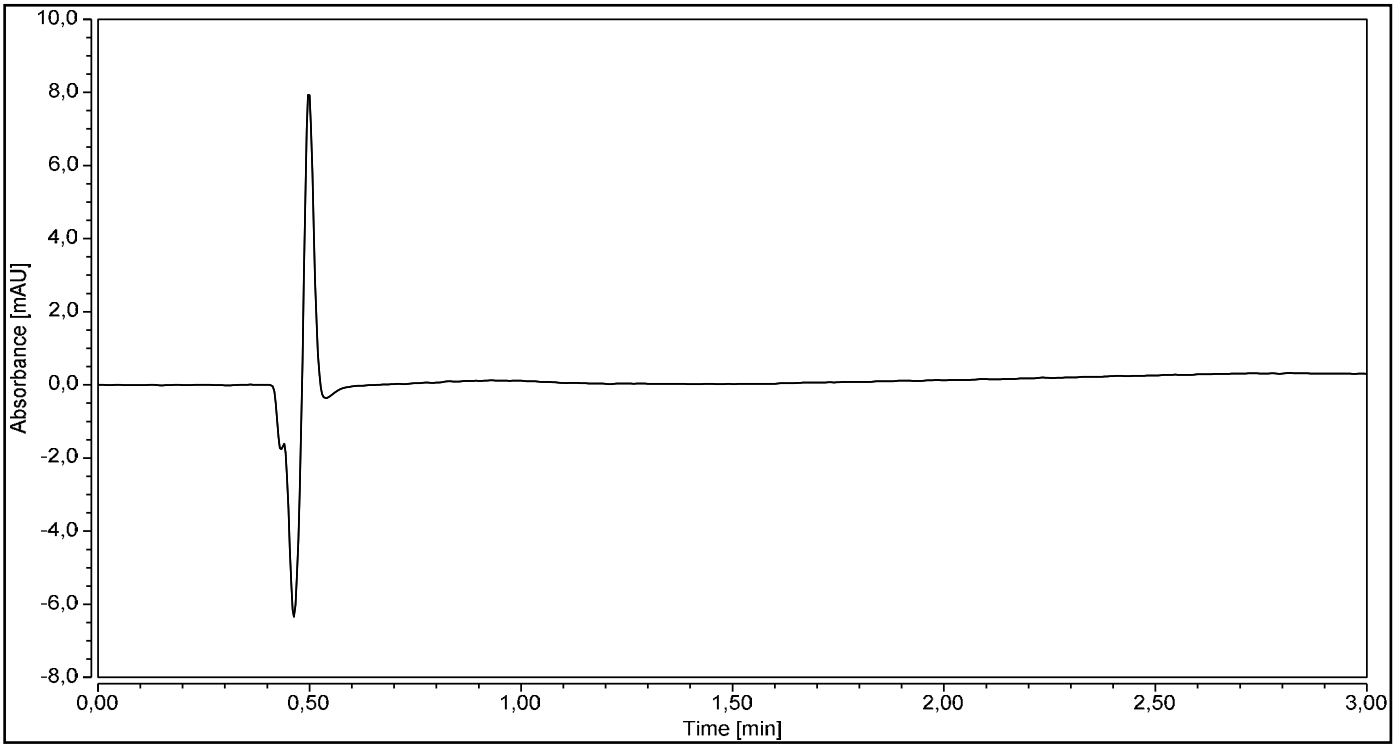


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 4* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:20* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

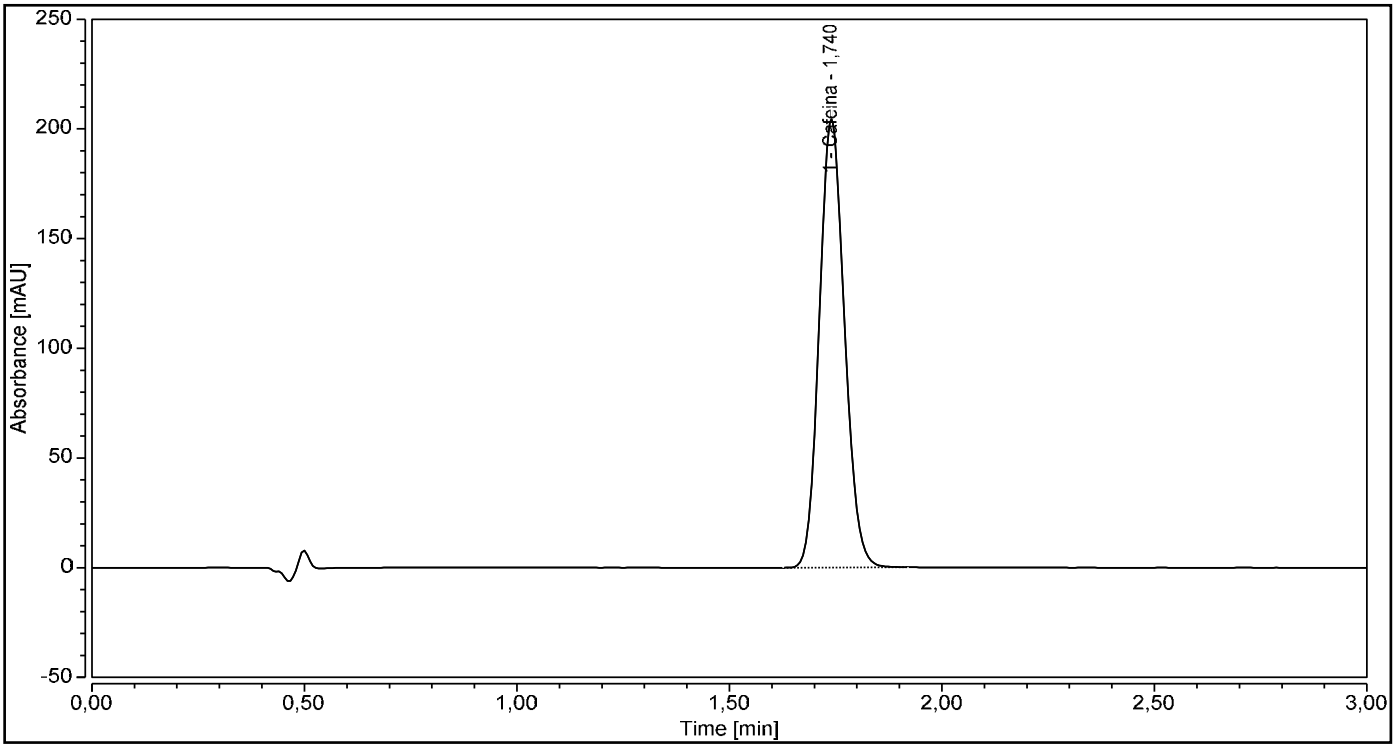


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,740 | 14,0111203 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 5* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:24* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

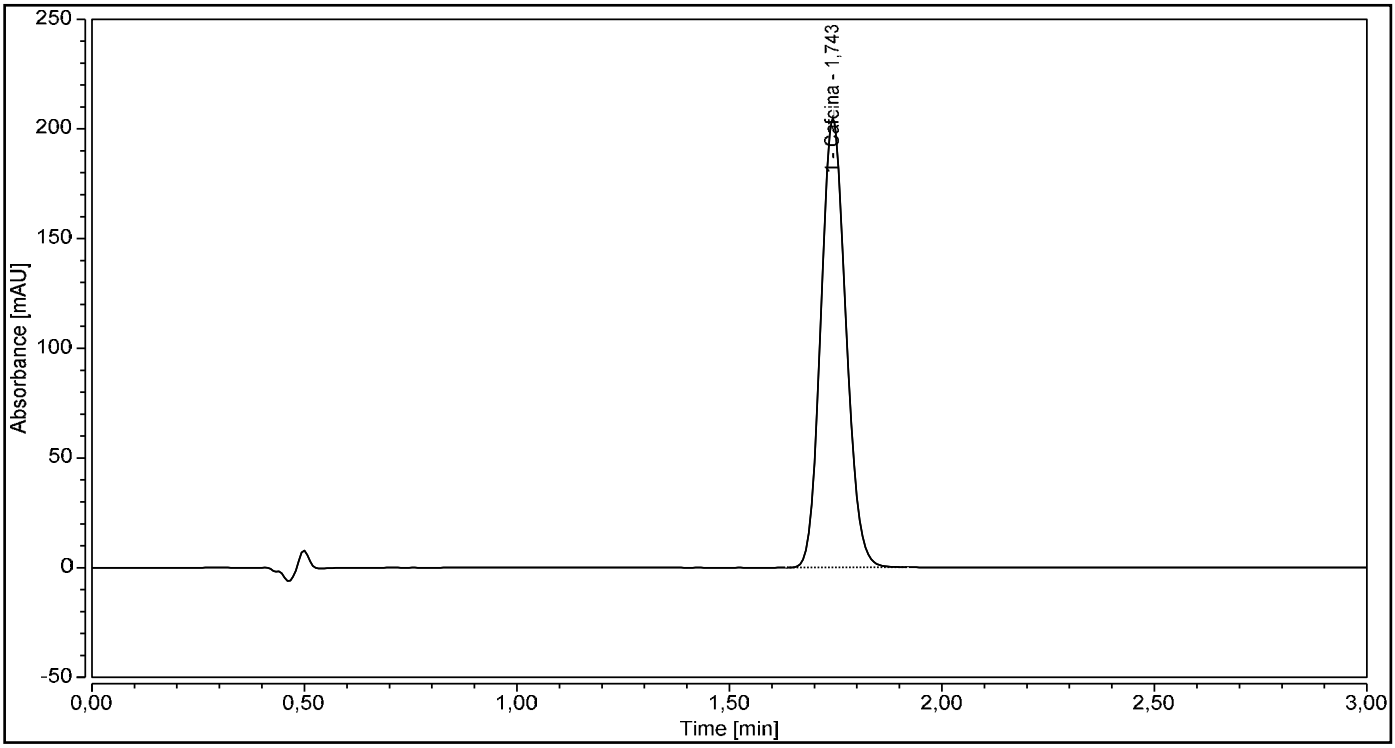


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,743 | 13,9880810 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *PCIN 6* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:29* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

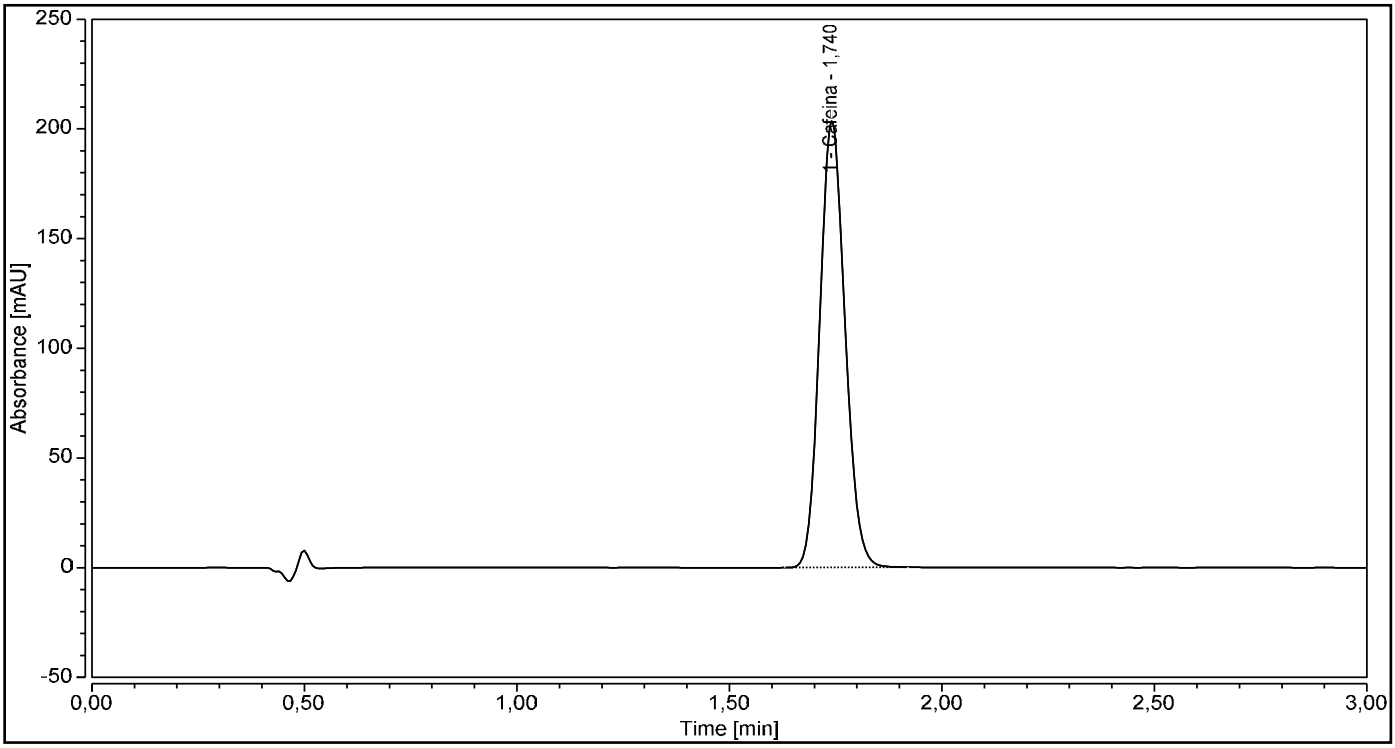


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,740 | 13,9941824 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *Branco 3* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:33* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

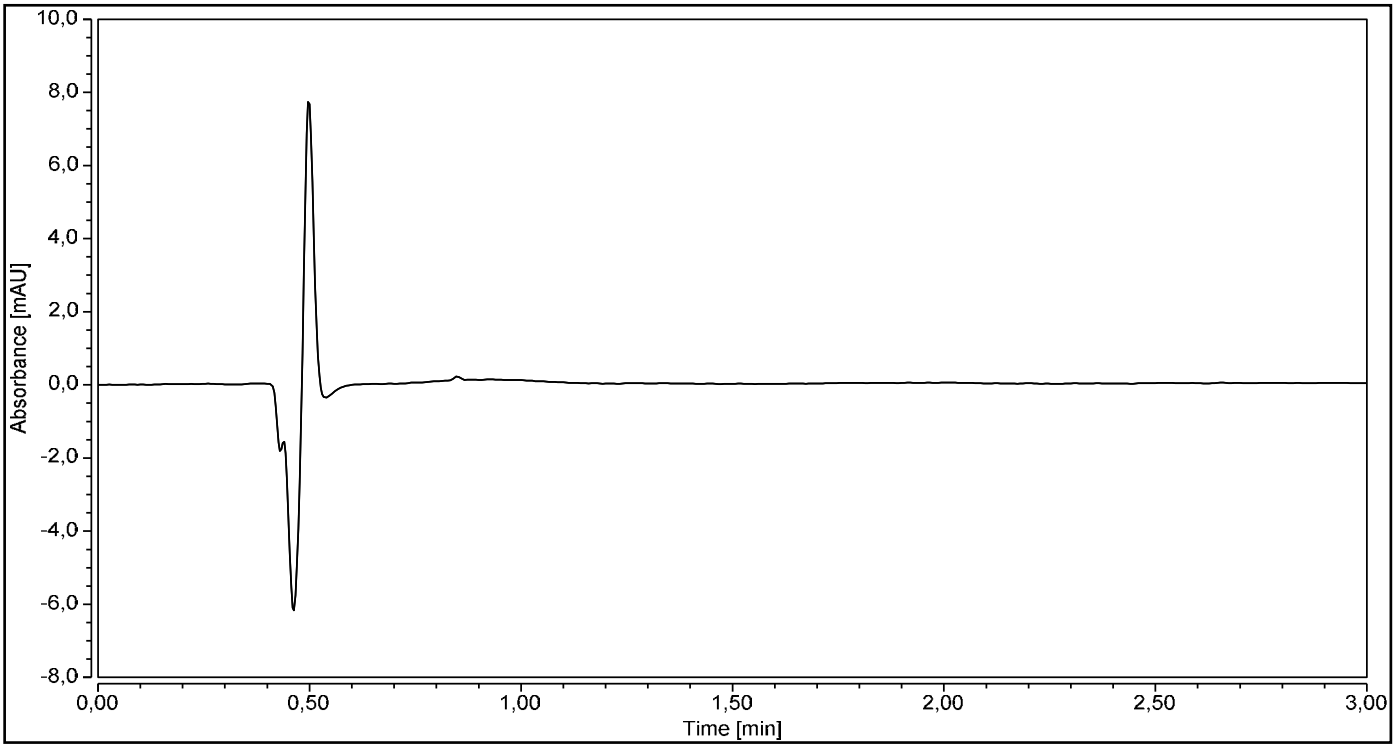


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LDUV 1* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:42* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

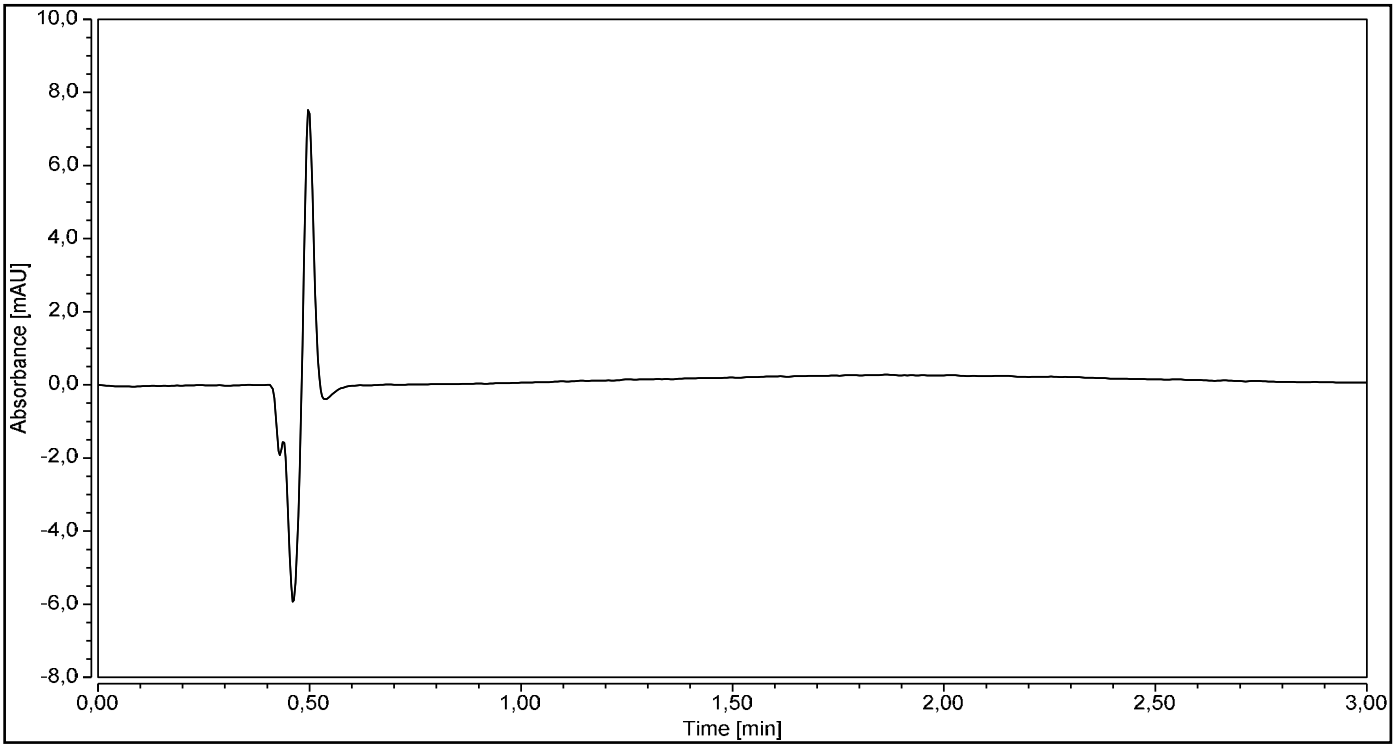


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LDUV 2* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:46* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

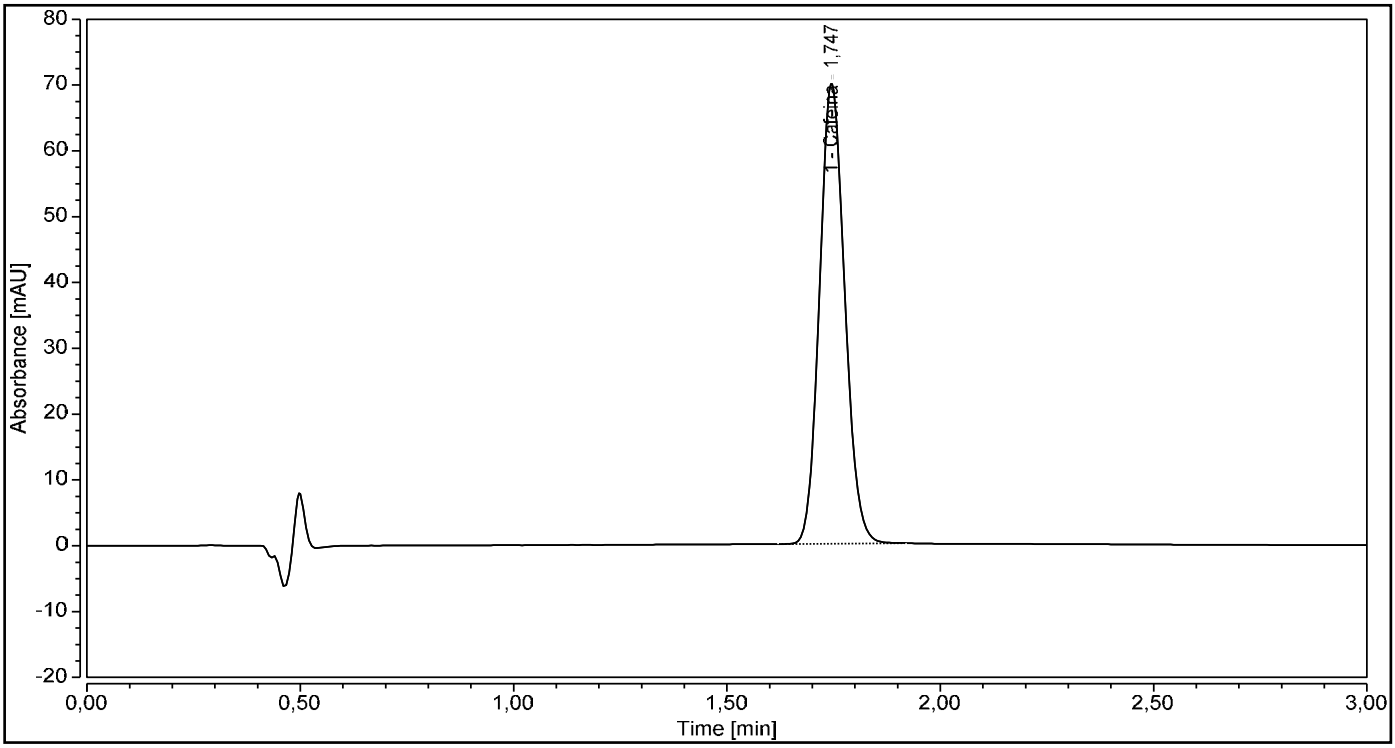


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,747 | 4,7864013 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LDUV 3* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:50* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

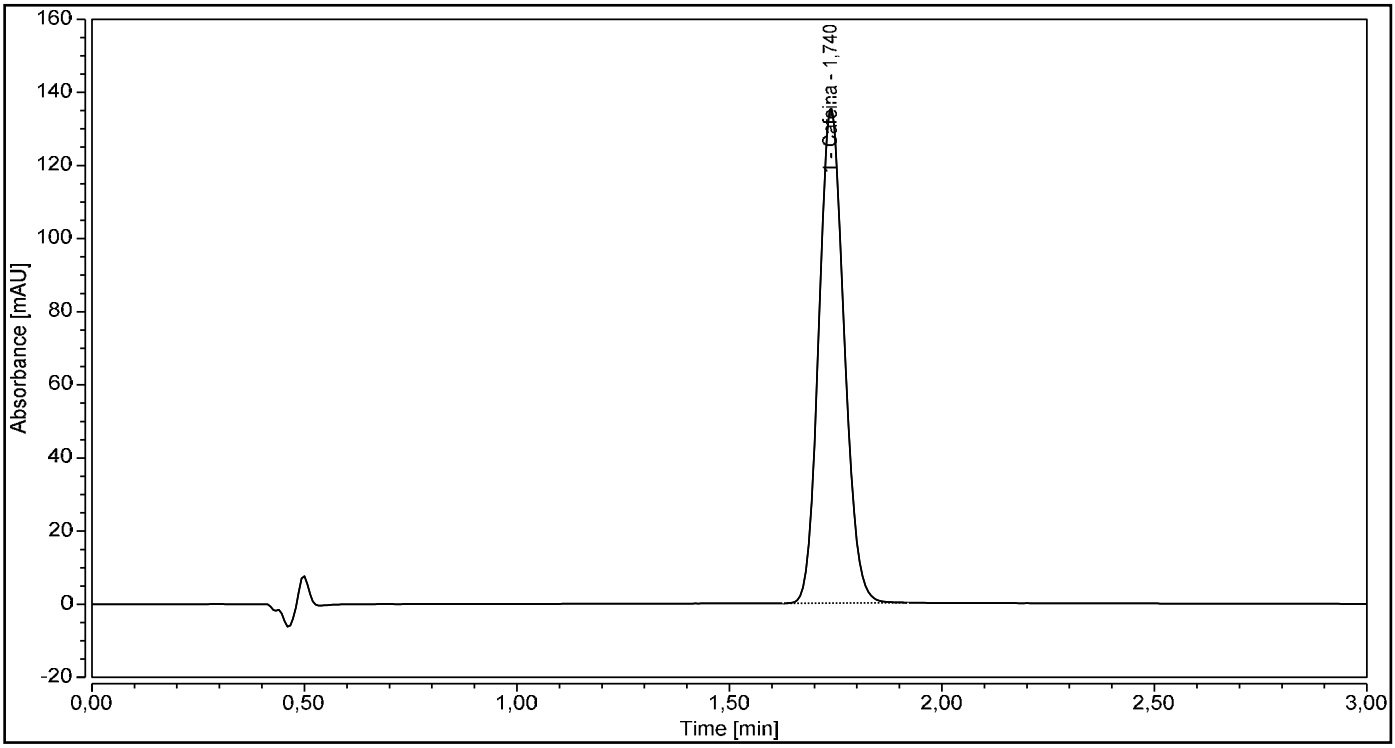


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,740 | 9,3290345 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LDUV 4* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:54* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

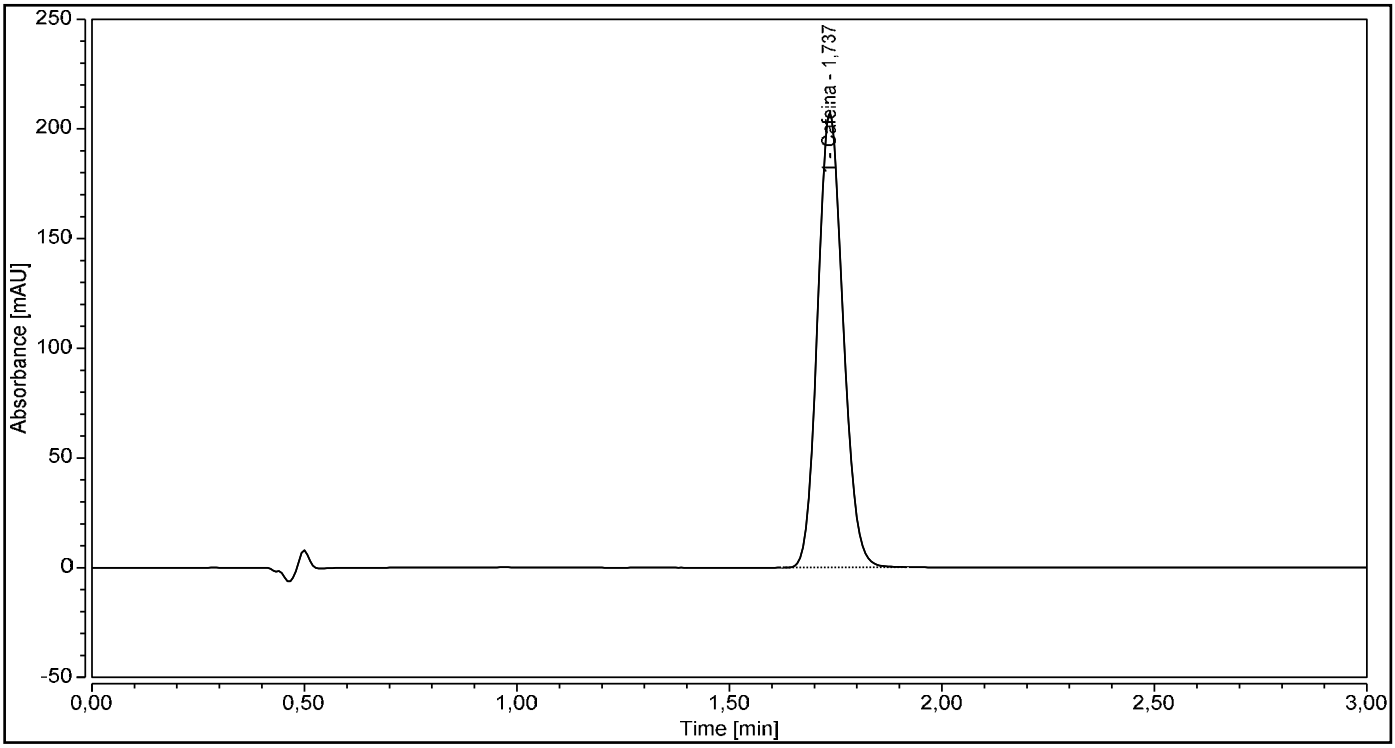


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,737 | 14,3809531 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LDUV 5* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 11:58* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

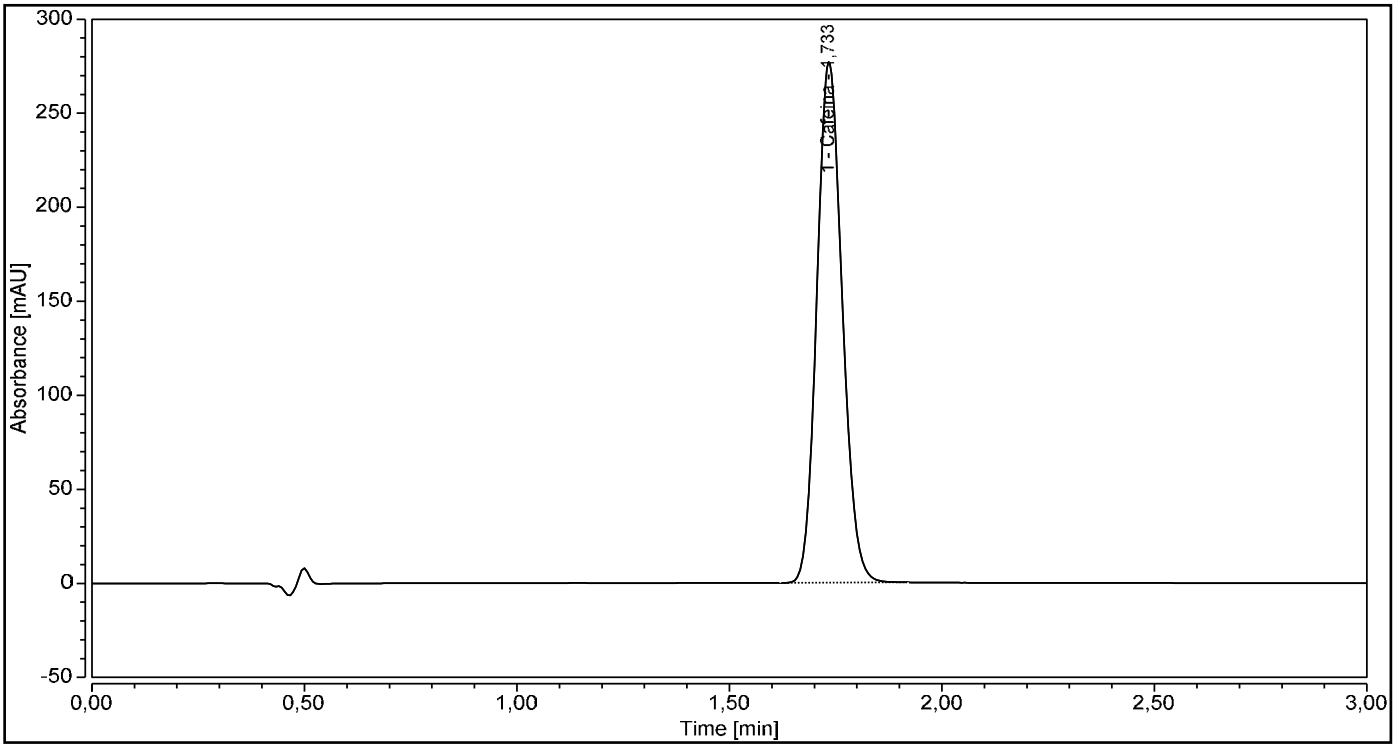


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,733 | 19,1217922 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LIIN 1* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *0,10* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 12:06* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

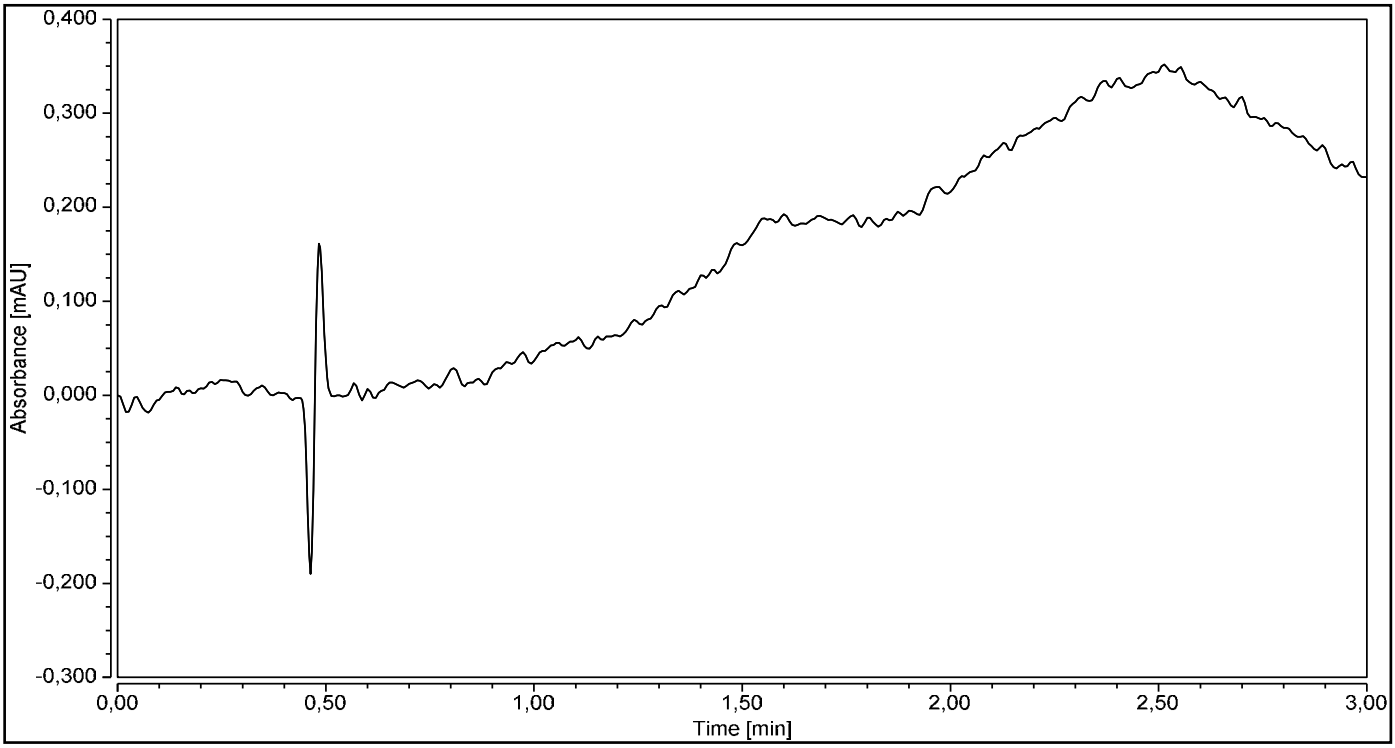


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LIIN 2* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *5,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 12:10* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

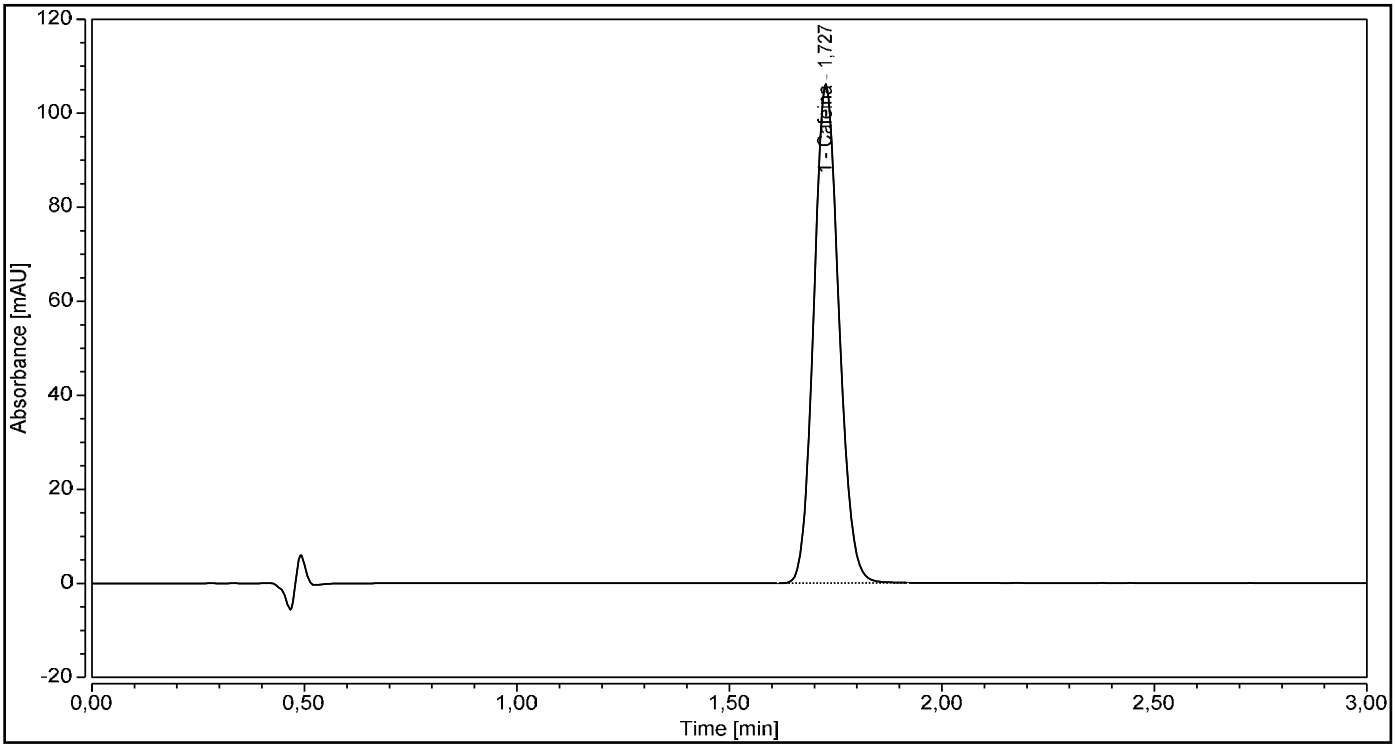


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,727 | 7,2750848 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LIIN 3* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *10,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 12:15* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

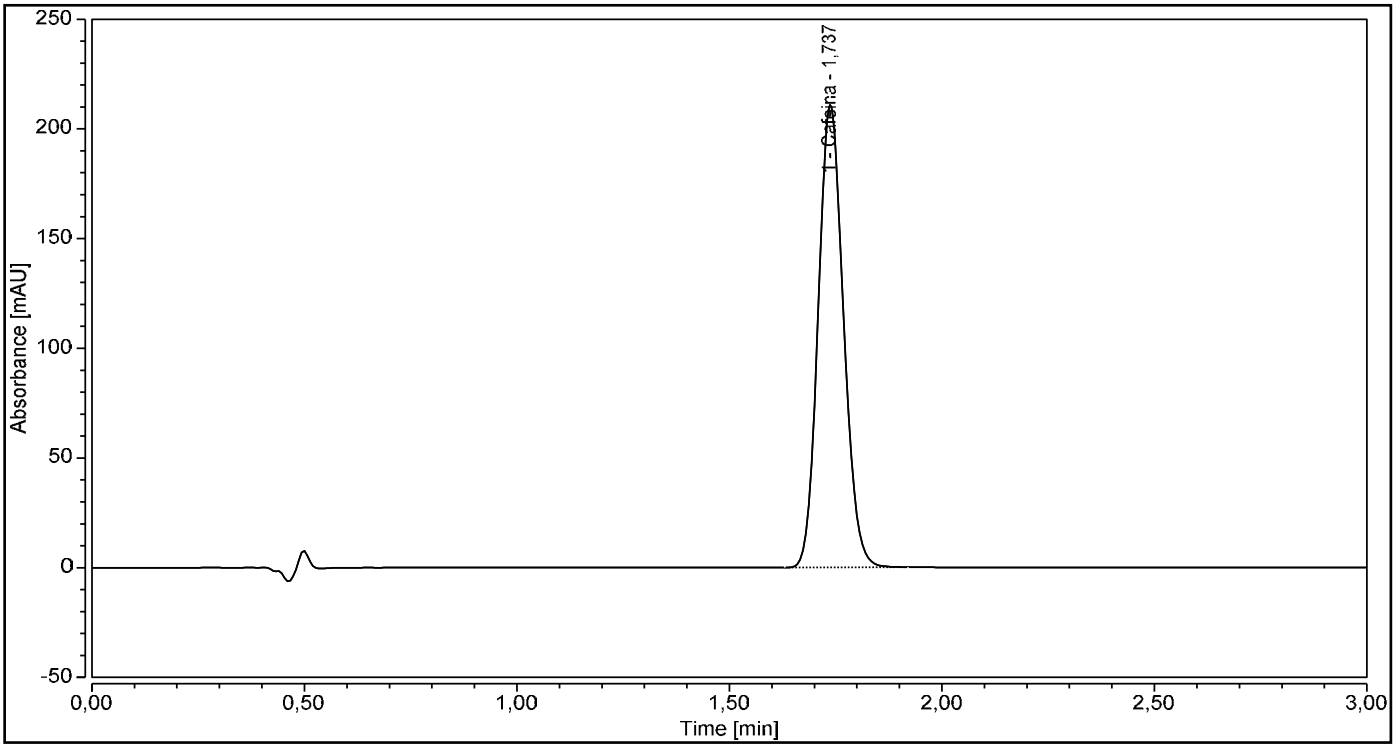


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,737 | 14,5209081 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LIIN 4* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *15,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 12:19* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

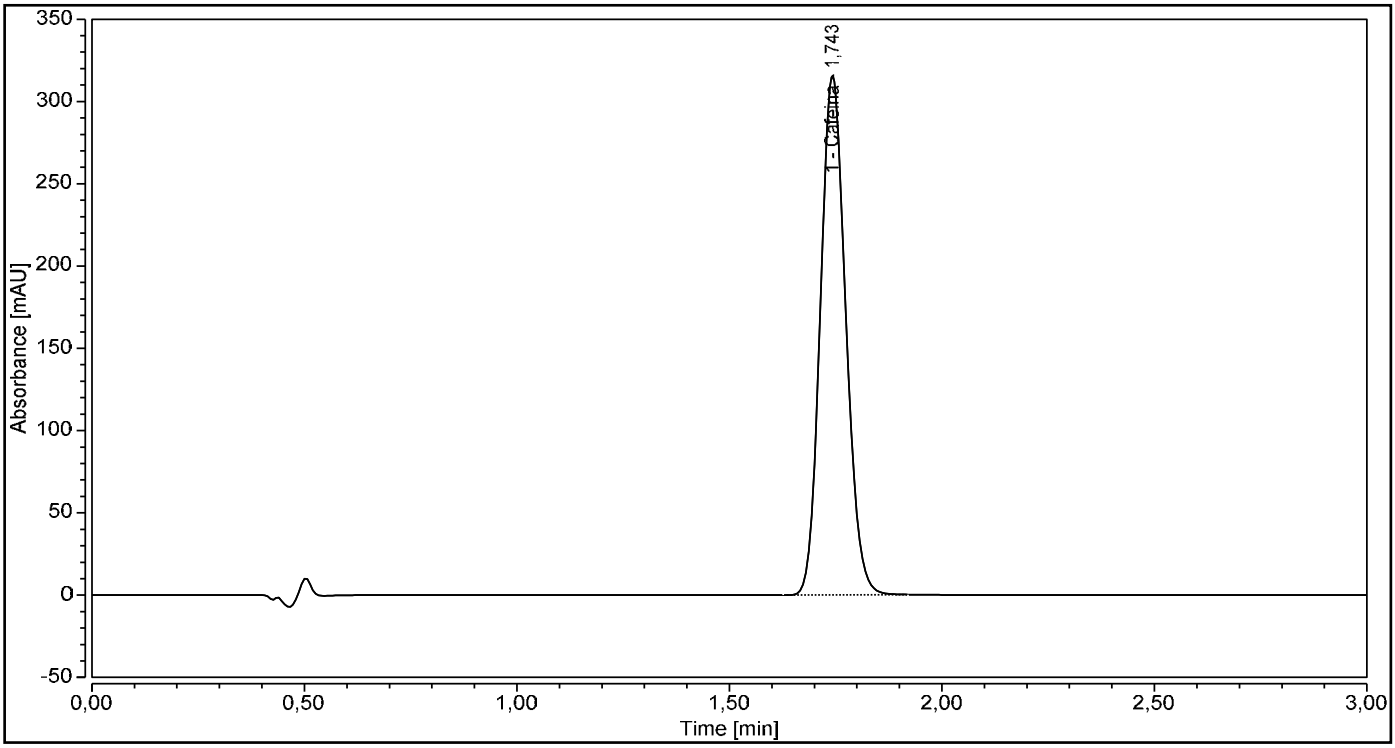


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,743 | 21,7617897 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *LIIN 5* |
| ***Run Time (min):*** | *3,00* |
| ***Injection Volume:*** | *20,00* |
| ***Instrument Method:*** | *Qualificação* |
| ***Processing Method:*** | *Qualificação* |
| ***Injection Date/Time:*** | *09/mai/18 12:23* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

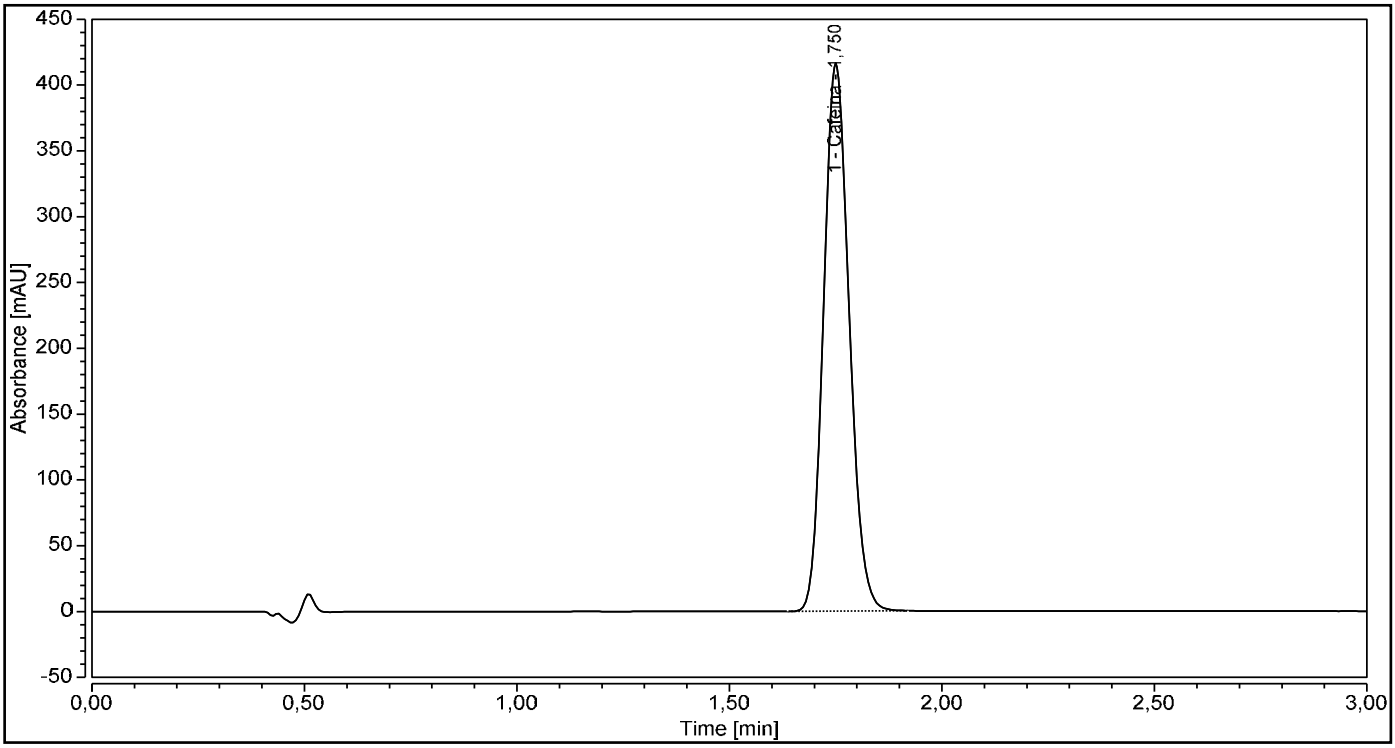


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|
| 1 | Cafeina | 1,750 | 28,9705232 |

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *Grad AB* |
| ***Run Time (min):*** | *19,00* |
| ***Injection Volume:*** | *0,10* |
| ***Instrument Method:*** | *Grad AB* |
| ***Processing Method:*** | |
| ***Injection Date/Time:*** | *09/mai/18 14:31* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

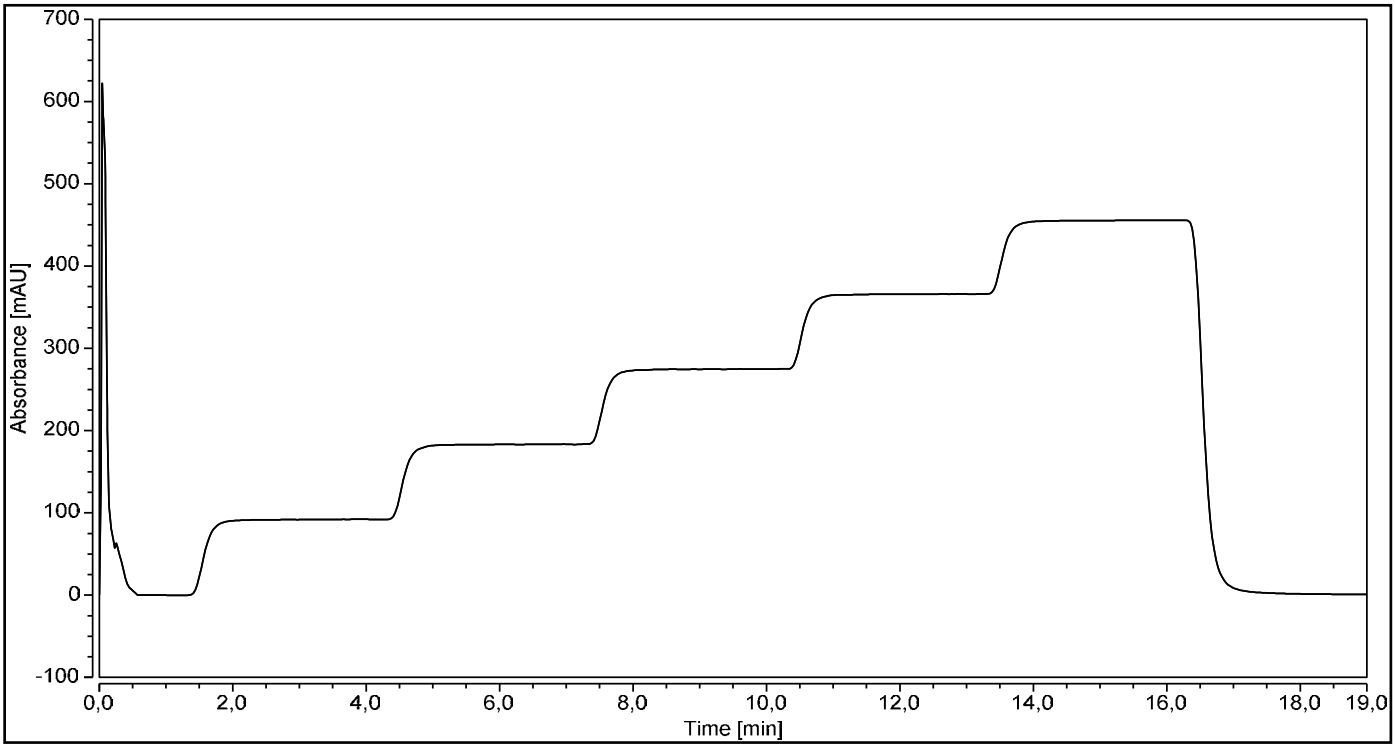


## Integration Results


| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

## Injection Details

| | |
|---|---|
| ***Injection Name:*** | *Grad CD* |
| ***Run Time (min):*** | *19,00* |
| ***Injection Volume:*** | *0,10* |
| ***Instrument Method:*** | *Grad CD* |
| ***Processing Method:*** | |
| ***Injection Date/Time:*** | *09/mai/18 14:54* |
| ***Created By:*** | *Michael Careli* |

## Chromatogram

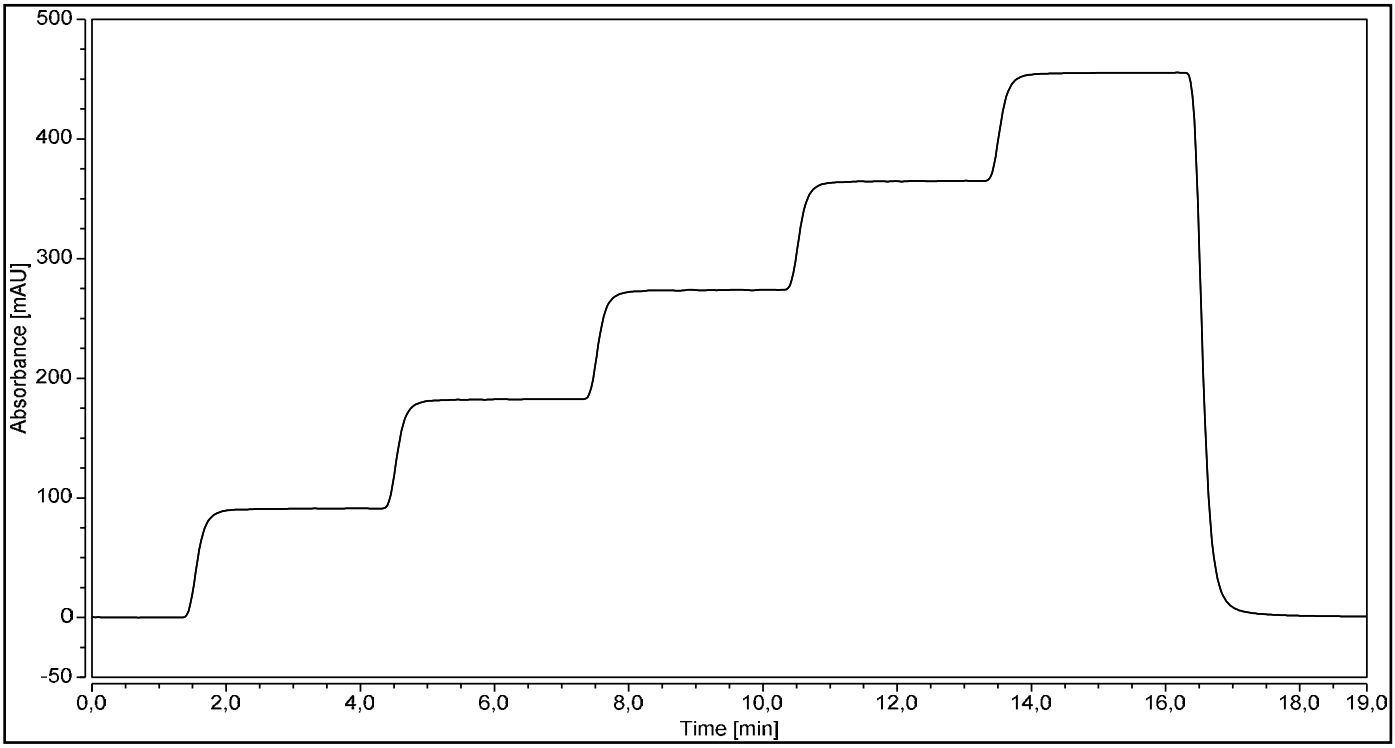


## Integration Results

| No. | Peak Name | Retention Time min | Area mAU*min |
|---|---|---|---|