
Peak Find - EDUV PDA_1,3033.JWS

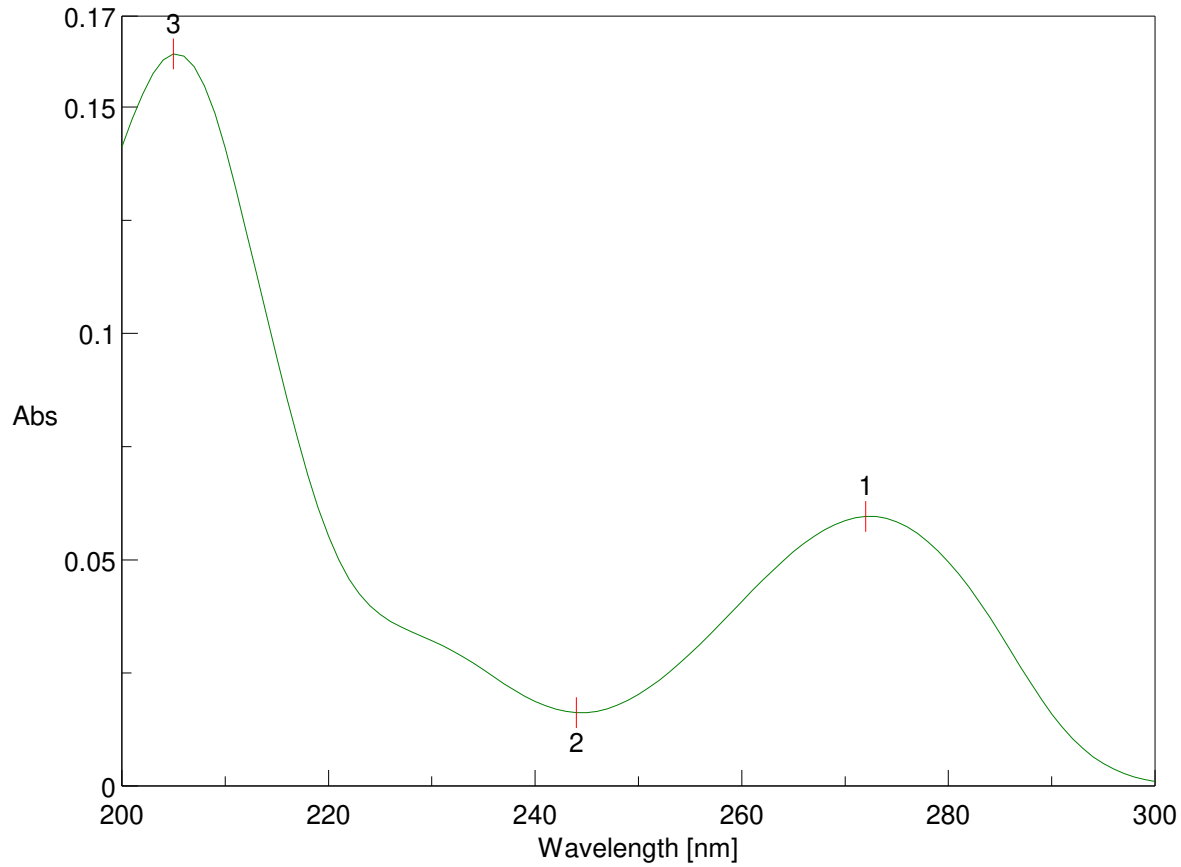

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	27/02/2024 14:20

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.05955	2	244	0.016193
3	205	0.161668			

Chromatogram

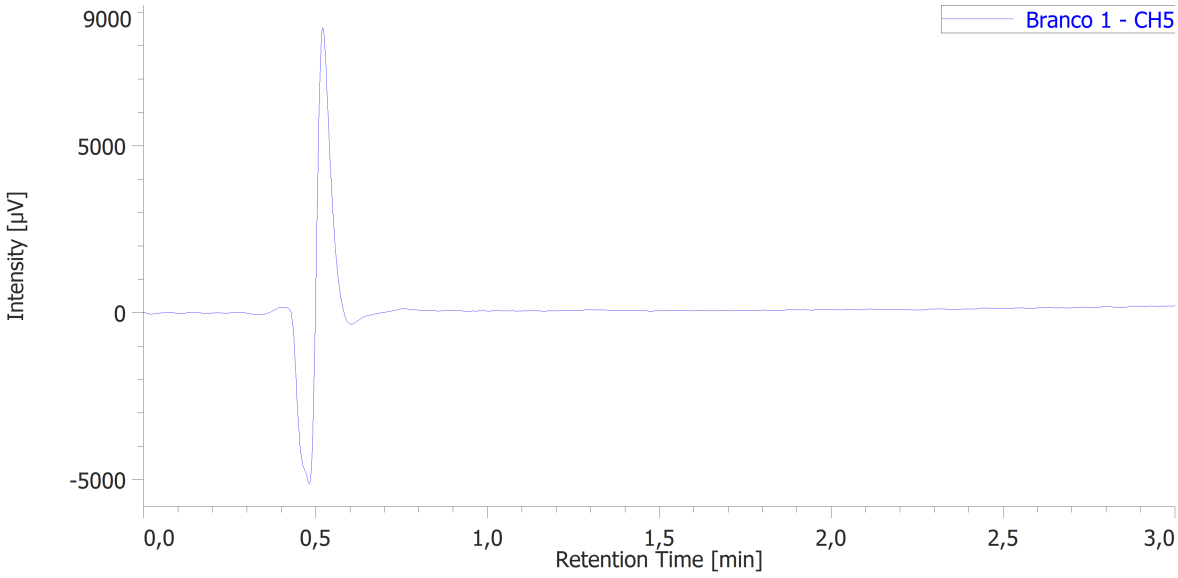


Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:44
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:23:38
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

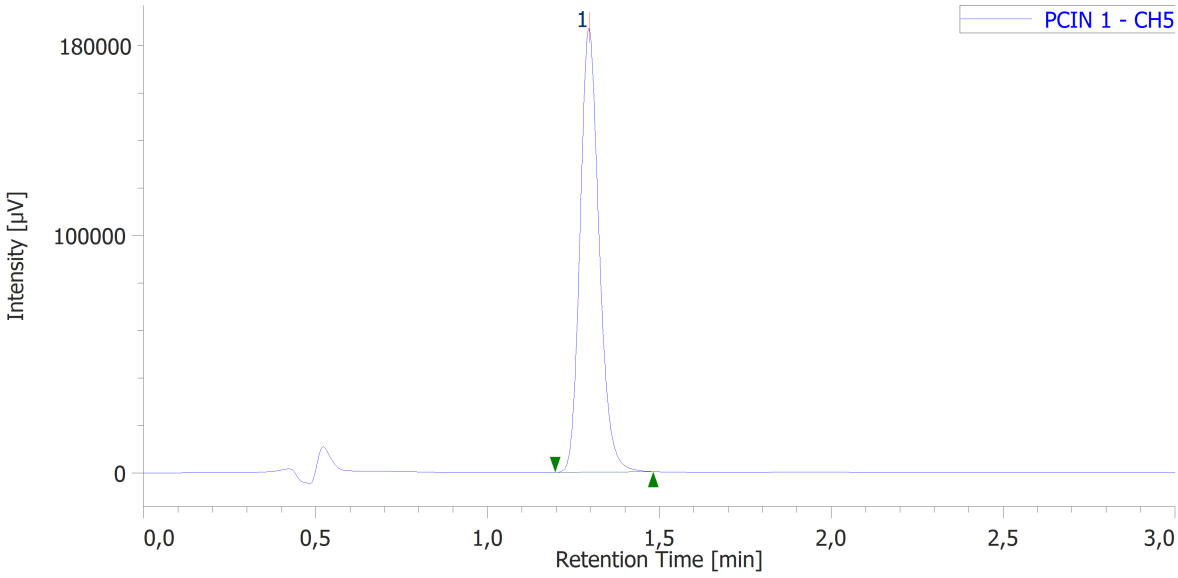

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:26:50
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,295	718898	187010	100,000	100,000	N/A	2743	N/A	1,181		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

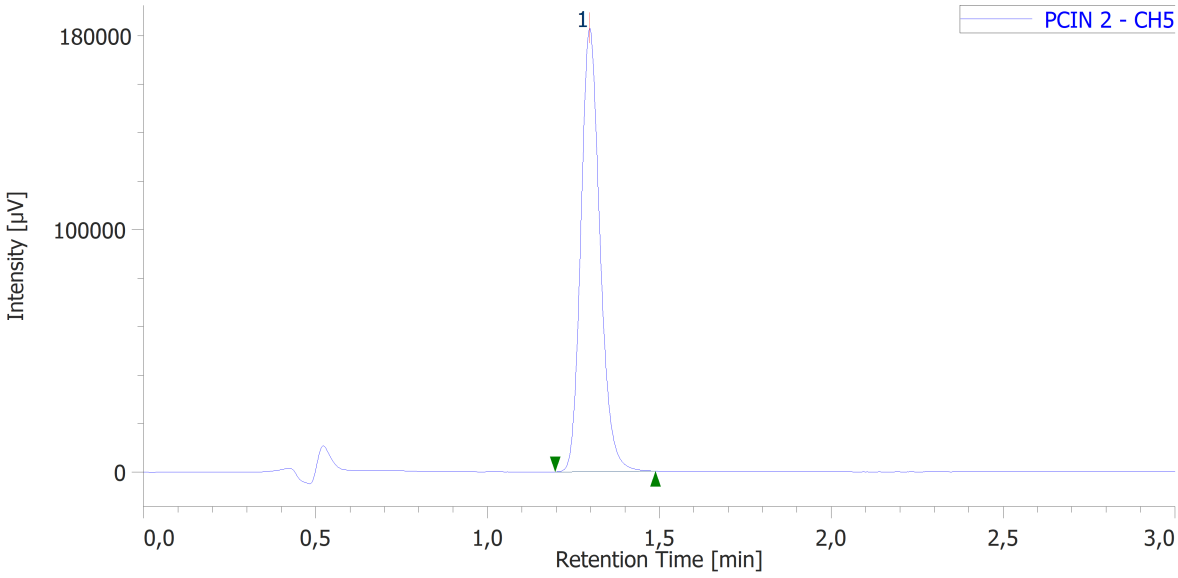

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:30:02
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,297	706325	182926	100,000	100,000	N/A	2729	N/A	1,195		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

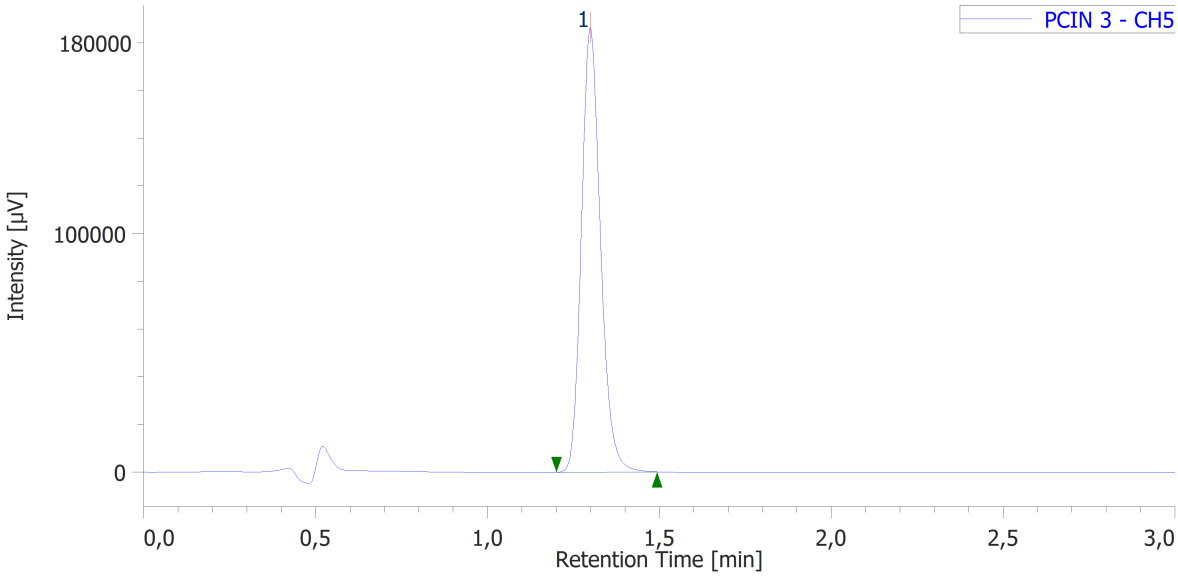

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:33:14
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,298	719458	186188	100,000	100,000	N/A	2732	N/A	1,192		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

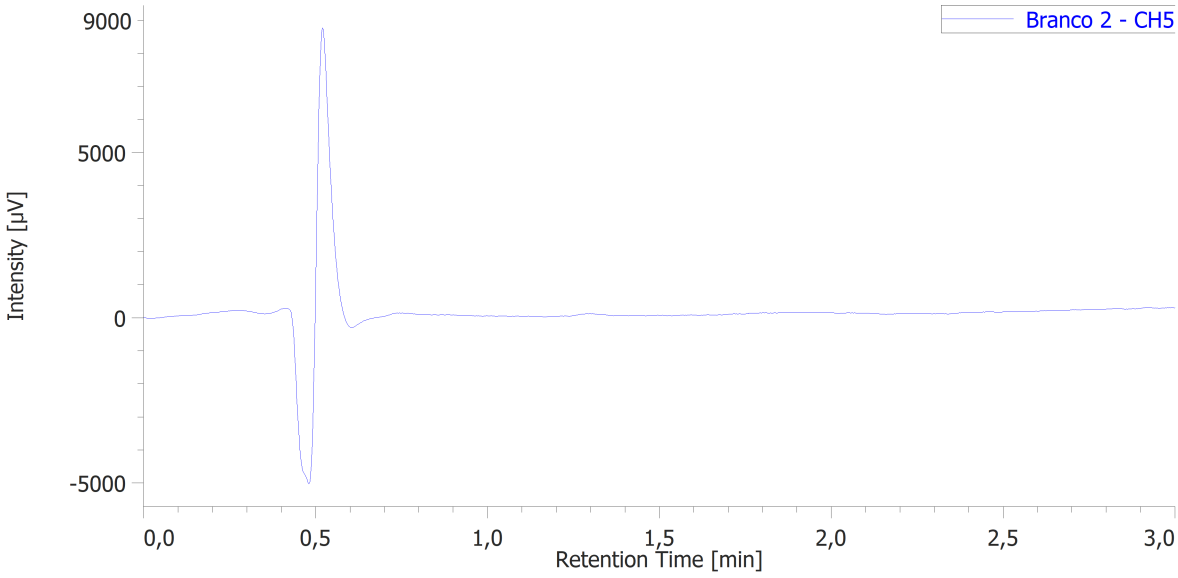


Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:36:27
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

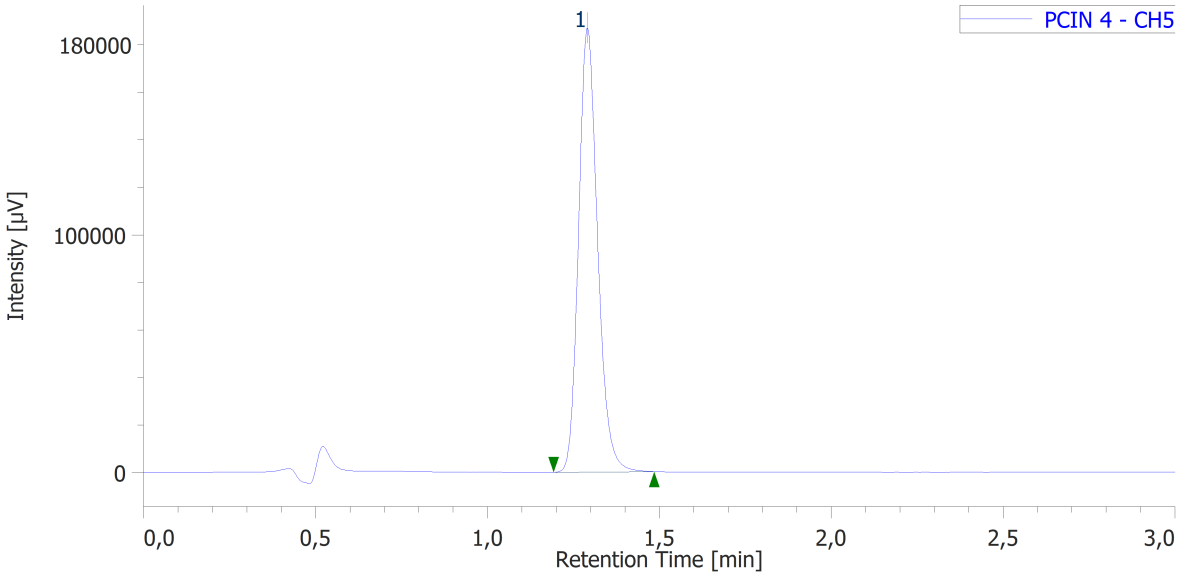

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:39:39
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,290	717521	186757	100,000	100,000	N/A	2727	N/A	1,194		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

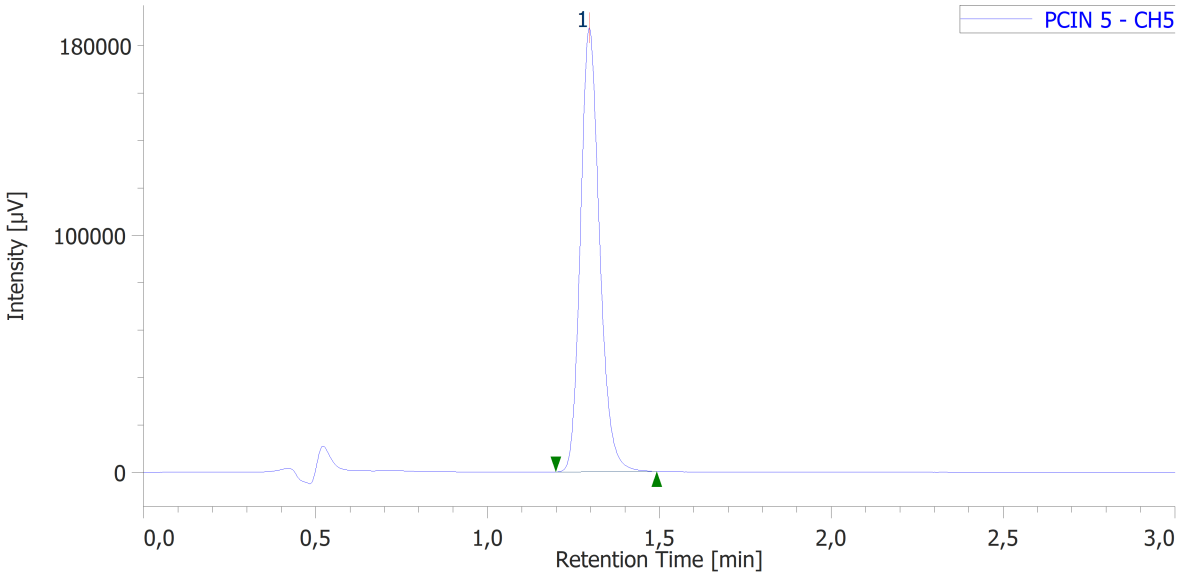

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:42:51
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,297	722949	187201	100,000	100,000	N/A	2733	N/A	1,172		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

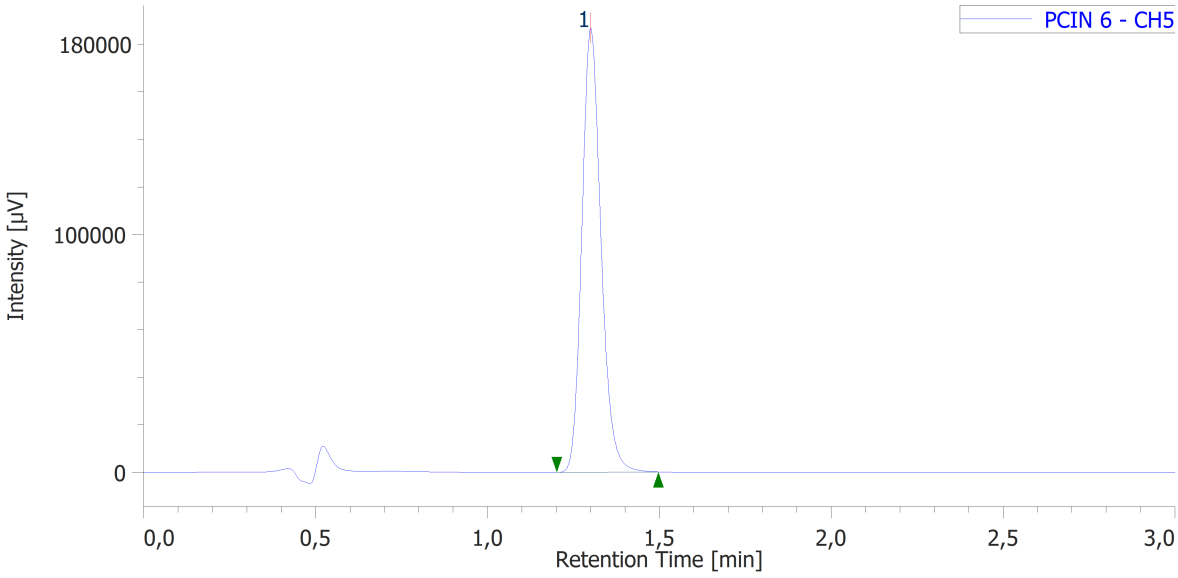

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:45
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:46:03
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,300	722082	186684	100,000	100,000	N/A	2734	N/A	1,188		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

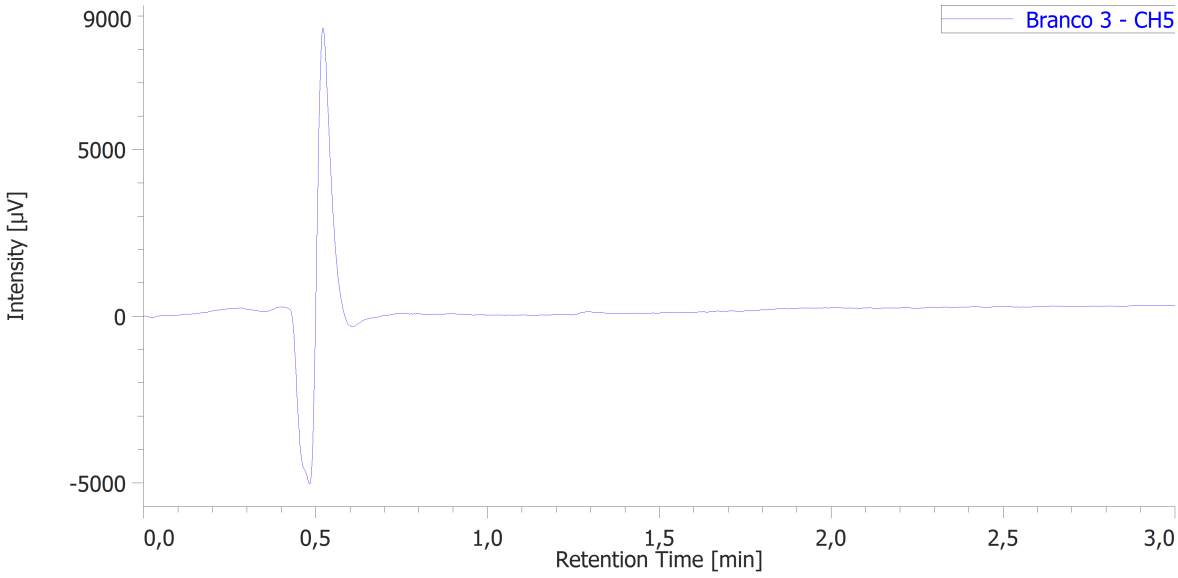


Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:49:15
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

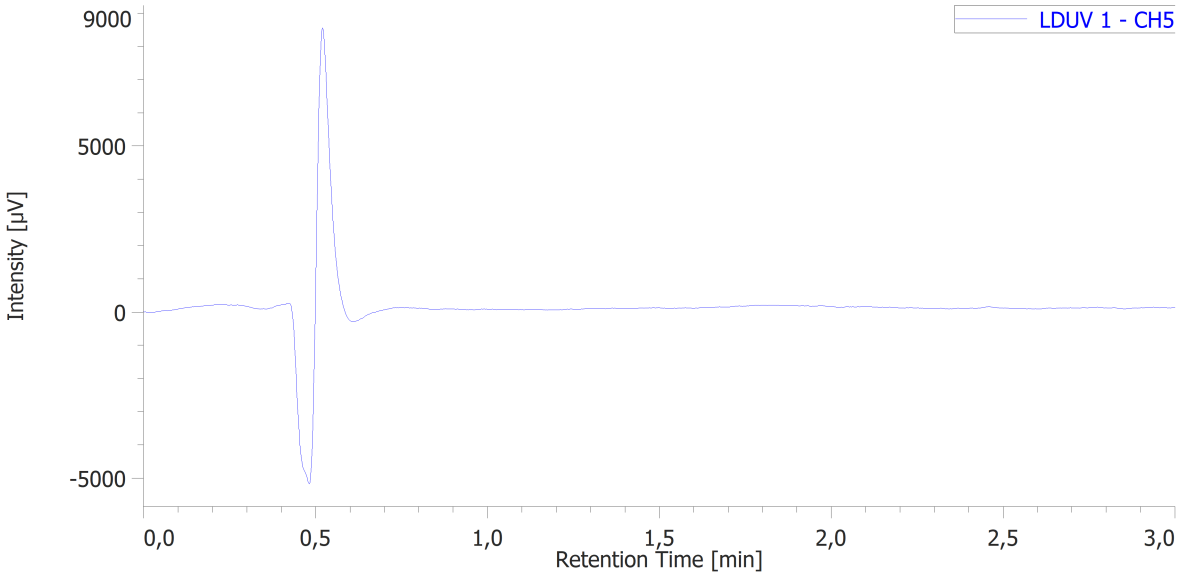


Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:52:27
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

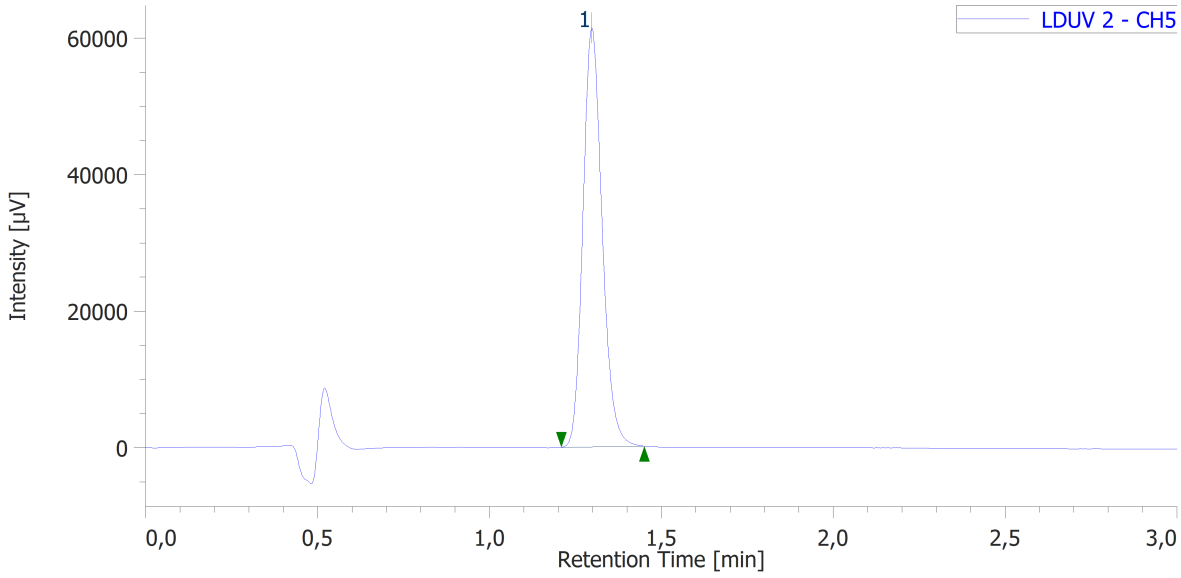

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:55:40
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,297	237624	61334	100,000	100,000	N/A	2677	N/A	1,199		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

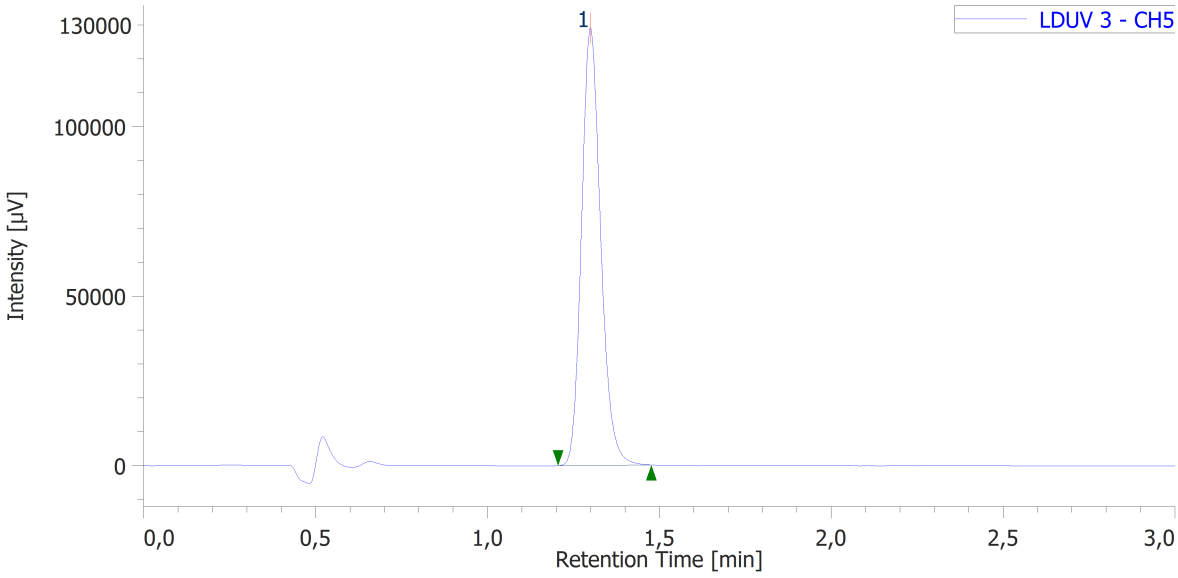

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 14:58:52
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,298	499804	128958	100,000	100,000	N/A	2703	N/A	1,202		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

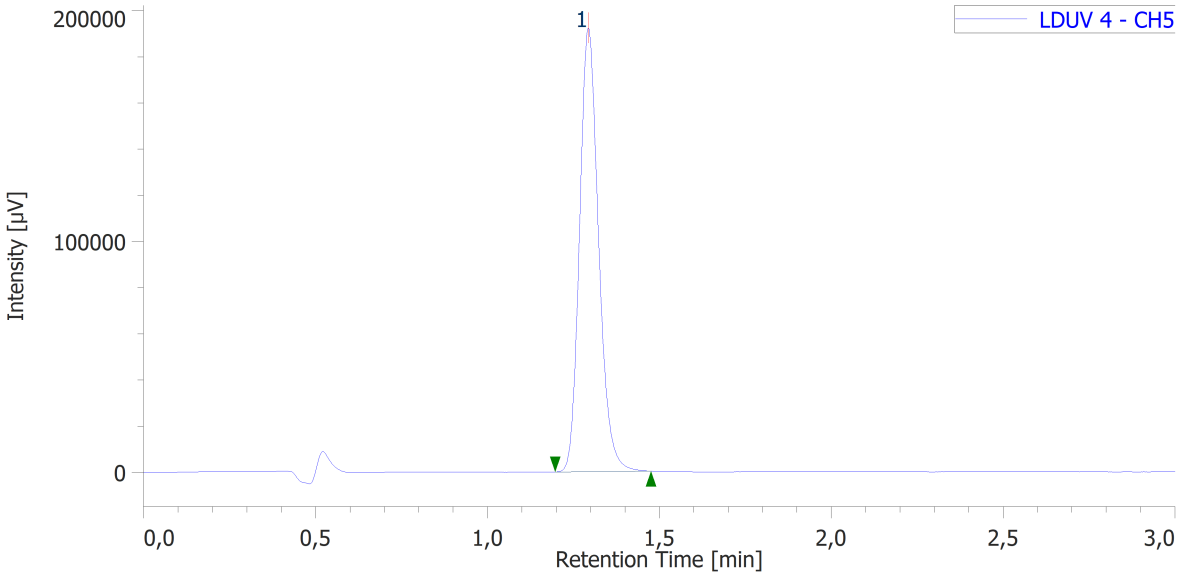

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:02:04
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,293	738879	192100	100,000	100,000	N/A	2732	N/A	1,183		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

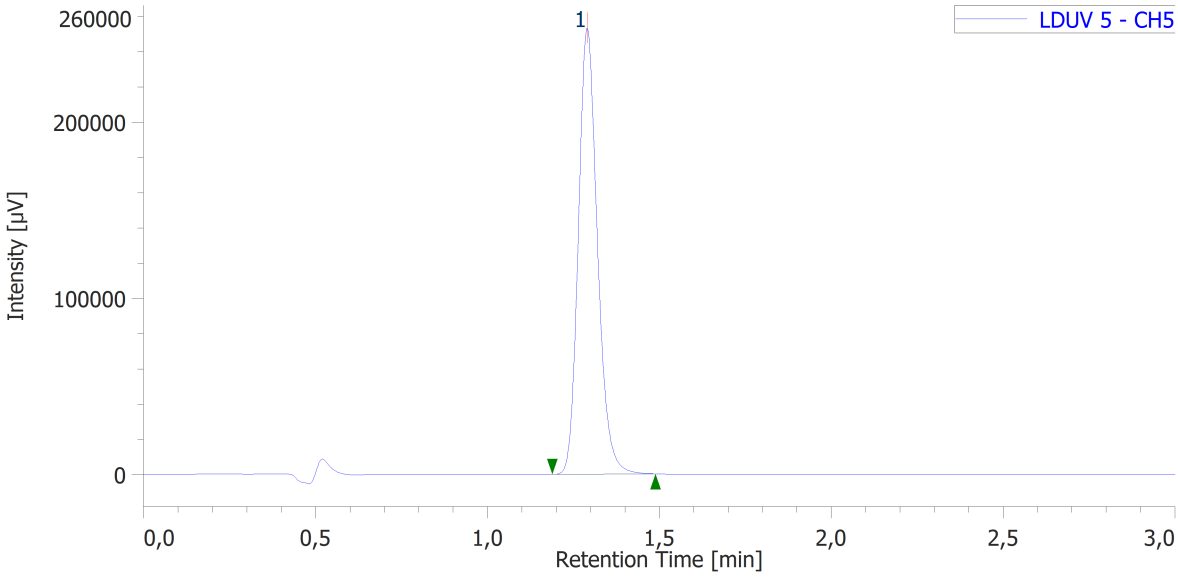

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:05:16
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,290	974221	253133	100,000	100,000	N/A	2729	N/A	1,182		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

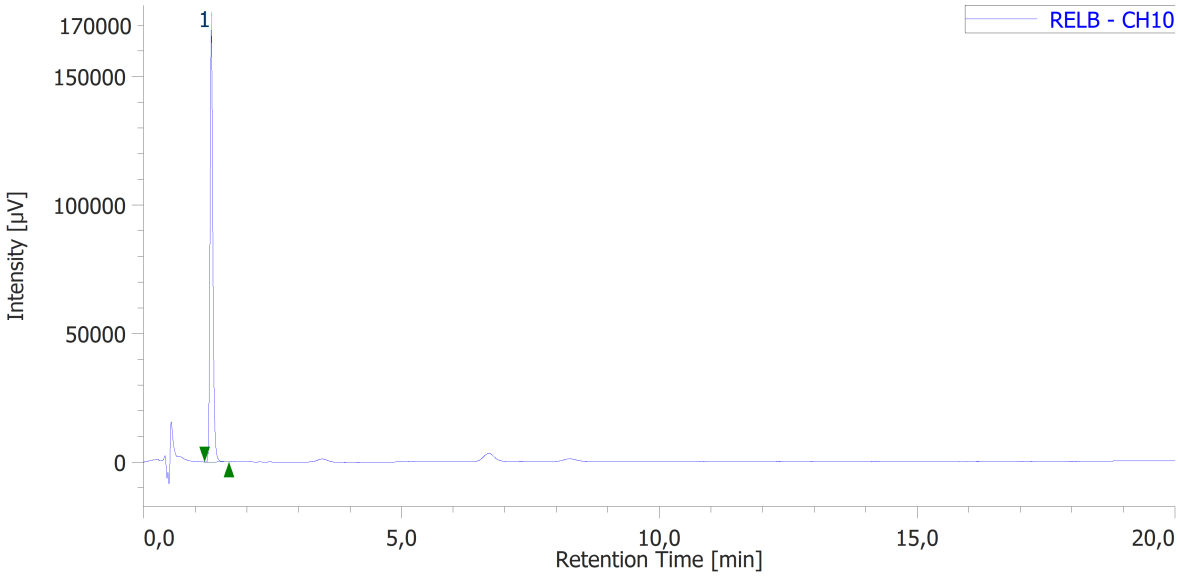

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:08:28
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH10
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	10	1,310	655602	168795	100,000	100,000	N/A	2800	N/A	1,217		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

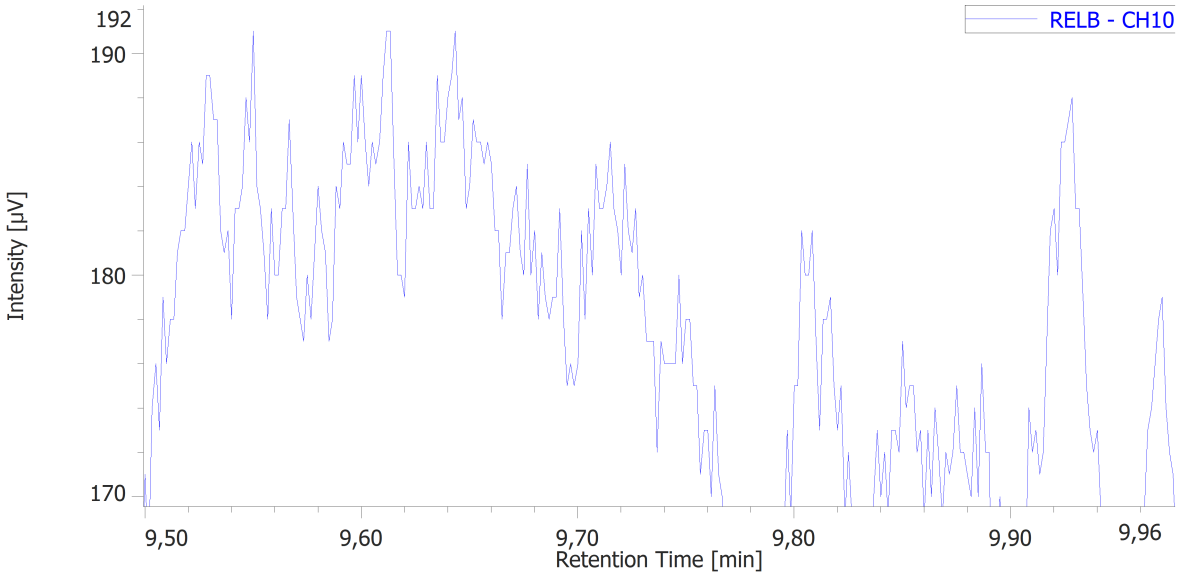

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:08:28
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH10
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	10	1,310	655602	168795	100,000	100,000	N/A	2800	N/A	1,217		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

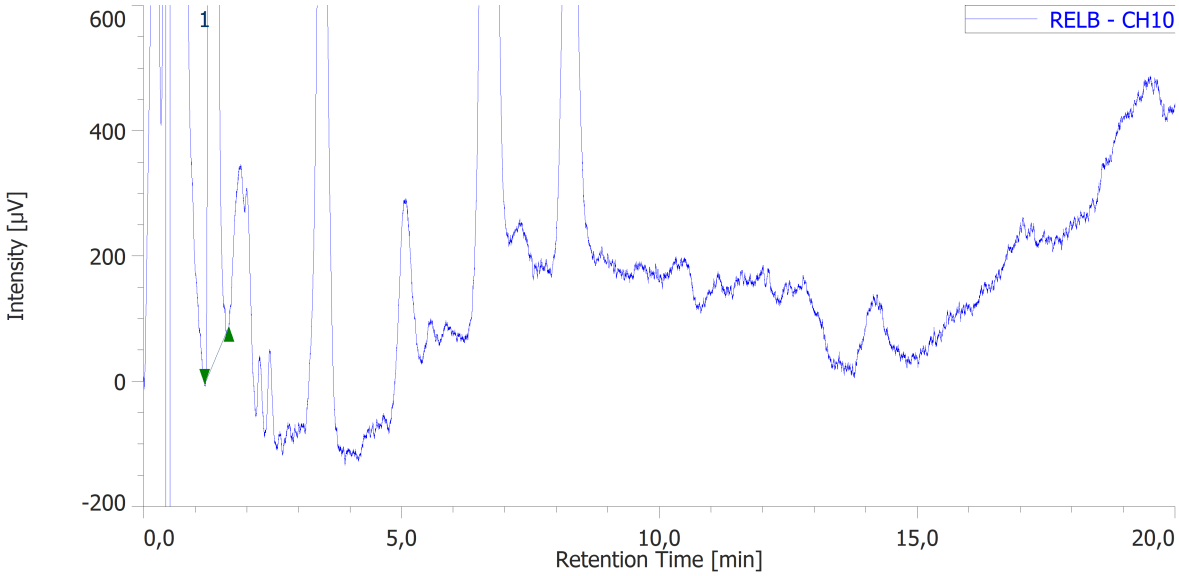

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:46
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:08:28
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH10
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	10	1,310	655602	168795	100,000	100,000	N/A	2800	N/A	1,217		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

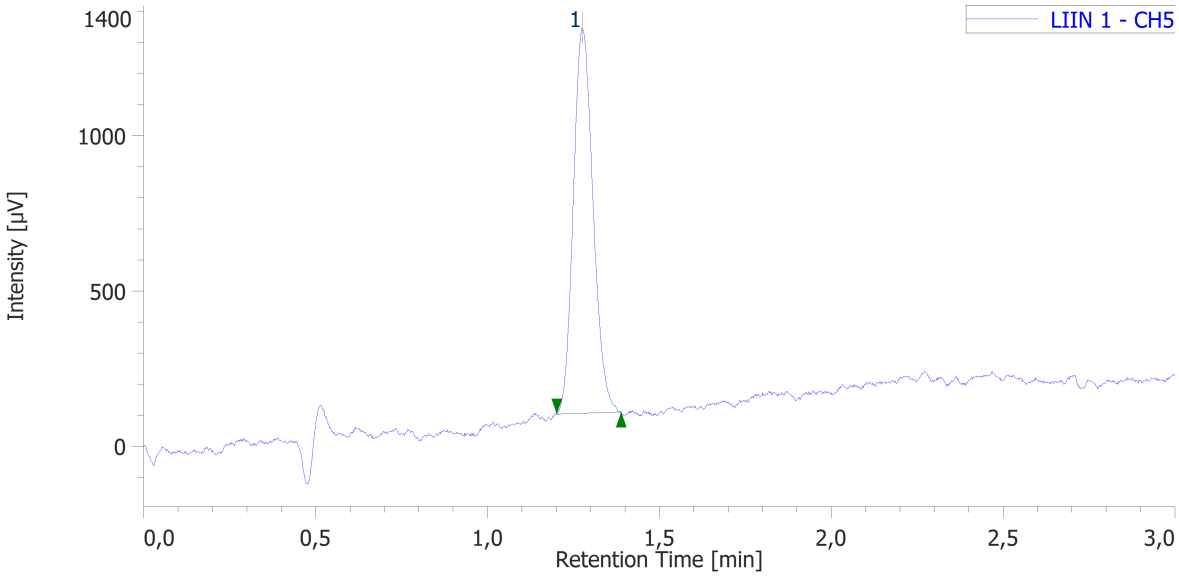

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:47
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:28:40
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,275	4938	1240	100,000	100,000	N/A	2376	N/A	1,192		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

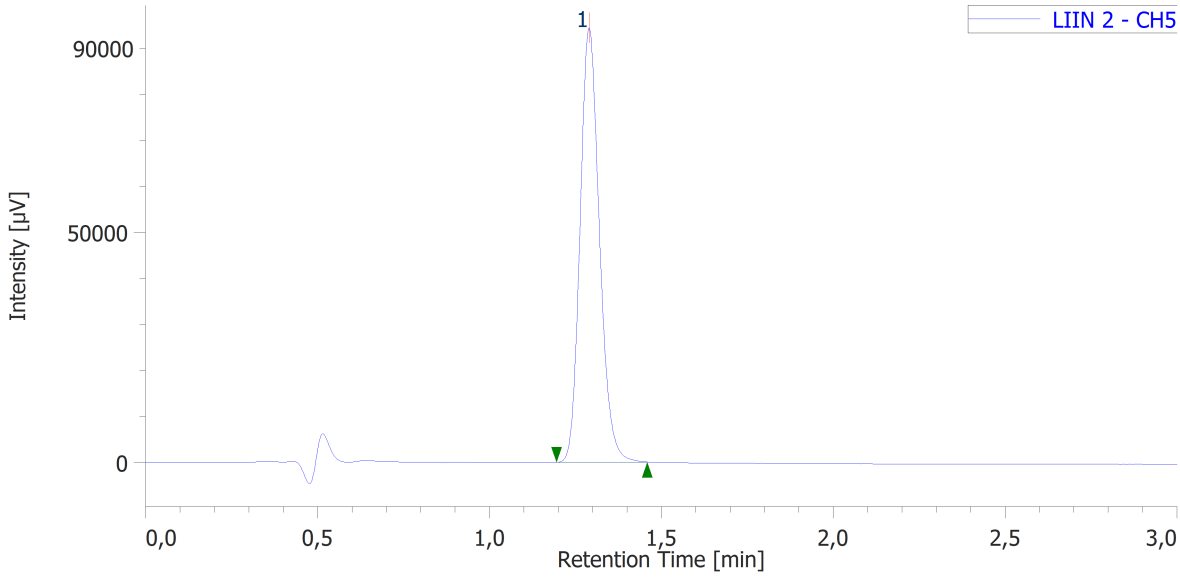

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:47
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:31:53
Volume	5,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,290	369295	94276	100,000	100,000	N/A	2589	N/A	1,159		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

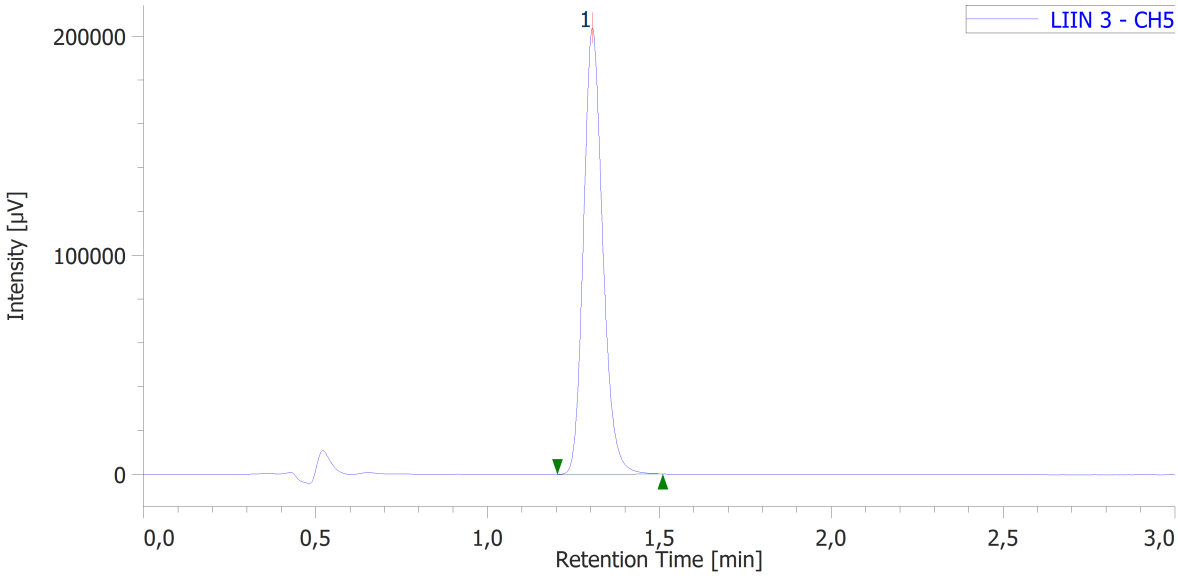

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:47
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:35:05
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,305	791190	203558	100,000	100,000	N/A	2730	N/A	1,185		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

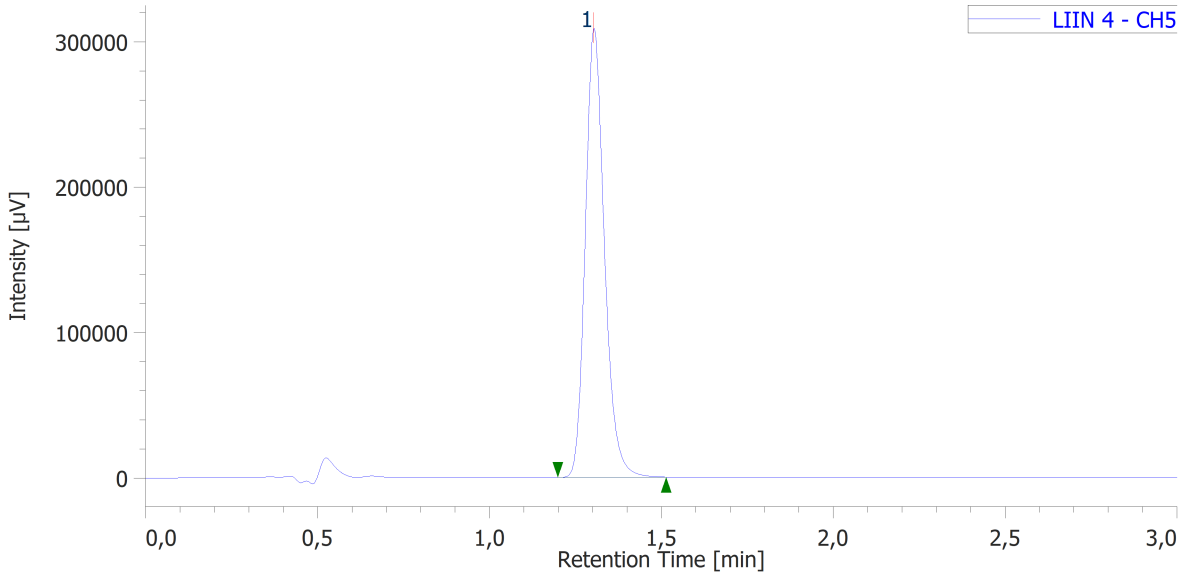

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:47
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:38:17
Volume	15,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,303	1192496	308924	100,000	100,000	N/A	2800	N/A	1,222		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

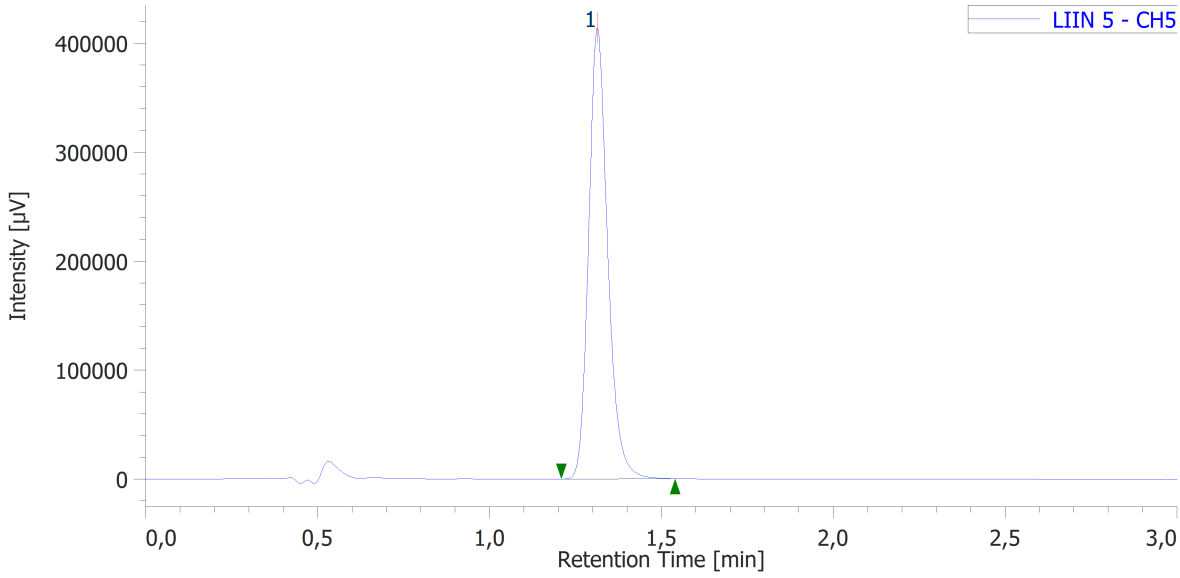

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:00:47
Description	
HPLC System Name	HP06
Injection Date	27/02/2024 15:41:29
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,313	1589463	413498	100,000	100,000	N/A	2897	N/A	1,218		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Peak Find - EDFL.jws

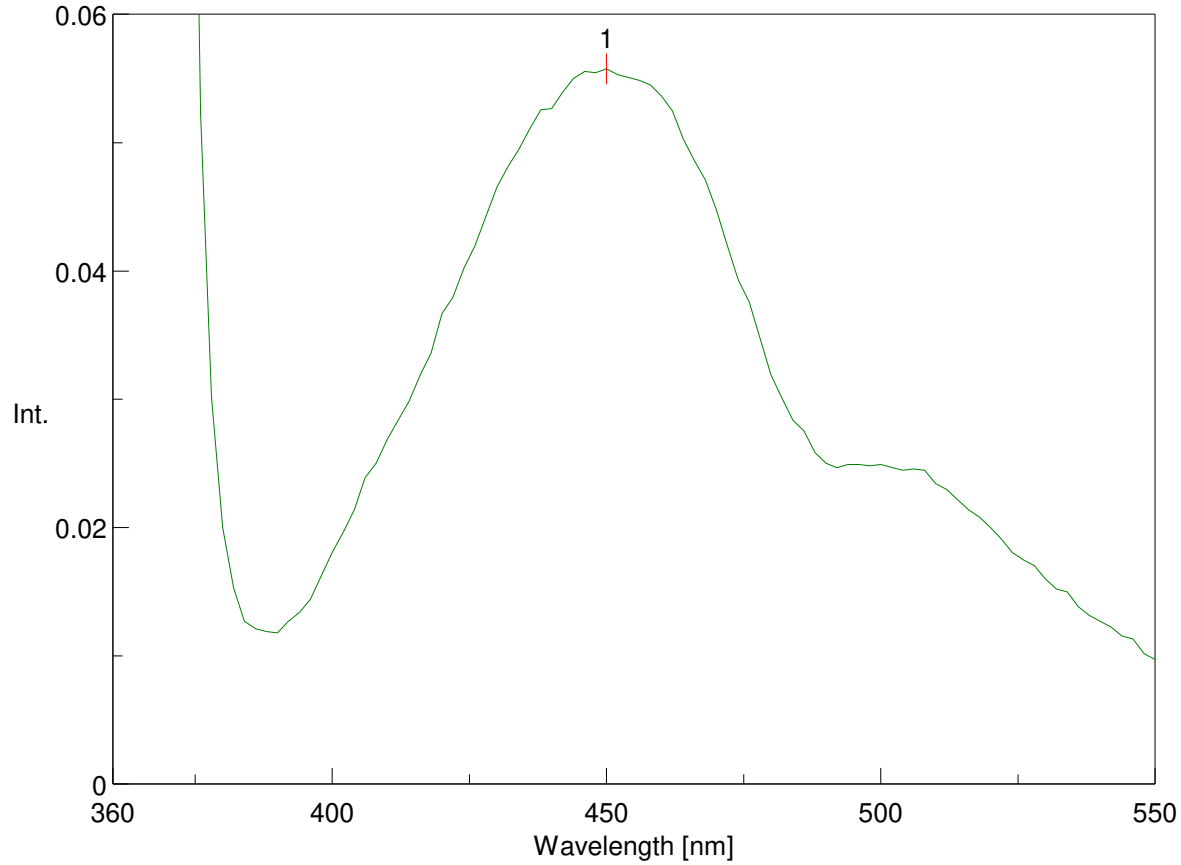

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	28/02/2024 09:29

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	0.0557404			

Chromatogram

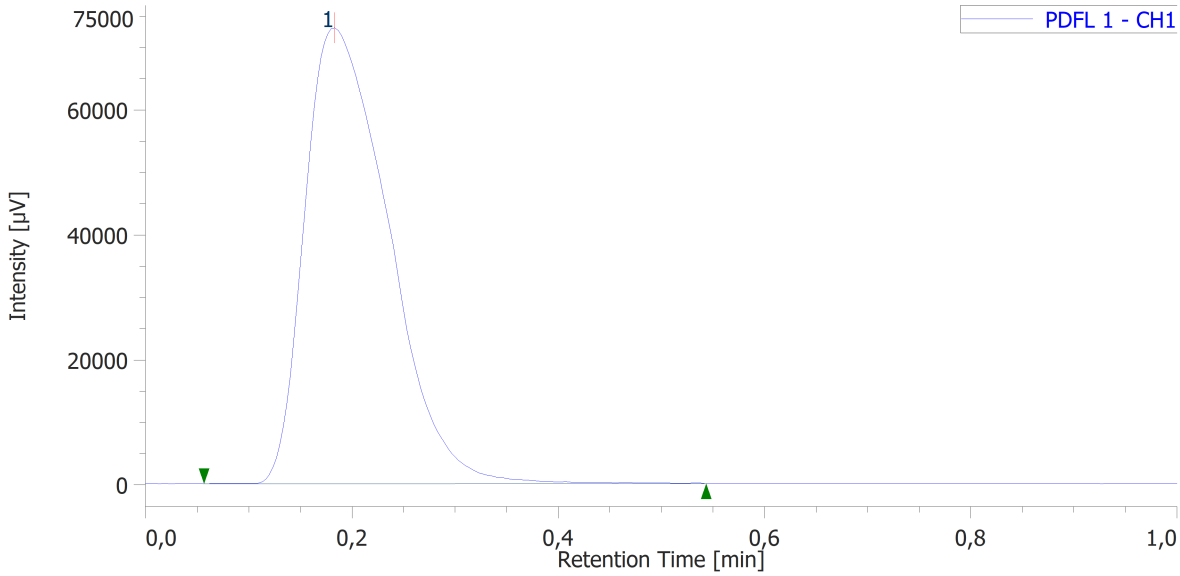

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:31
Description	
HPLC System Name	HP06 - Det FL
Injection Date	28/02/2024 09:41:39
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,183	412400	72898	100,000	100,000	N/A	22	N/A	1,542		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

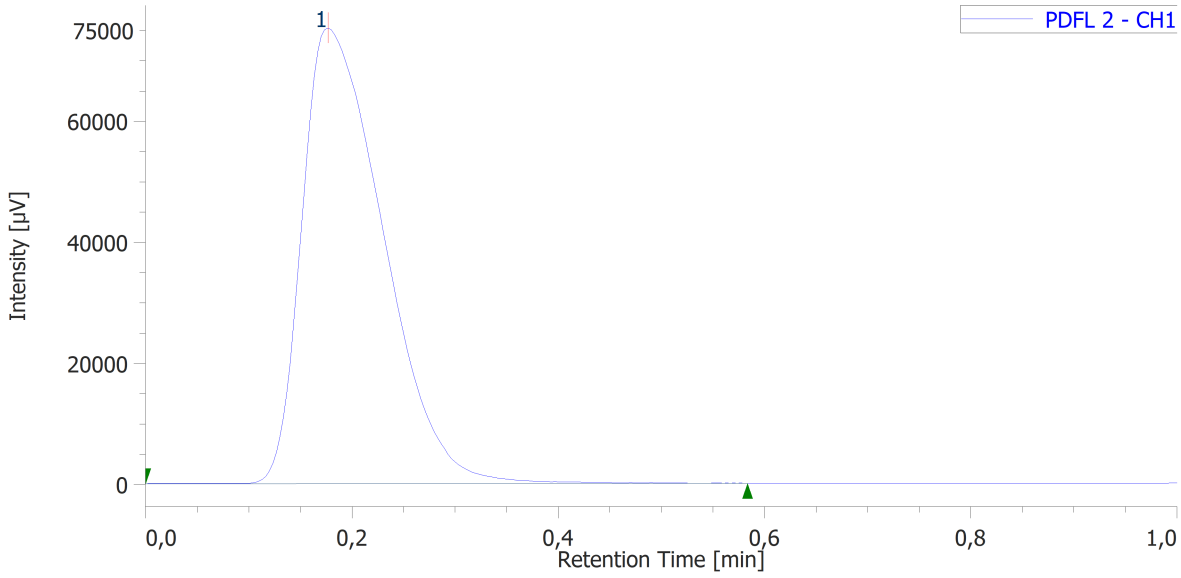

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:31
Description	
HPLC System Name	HP06 – Det FL
Injection Date	28/02/2024 09:43:57
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,177	412711	75232	100,000	100,000	N/A	23	N/A	1,657		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

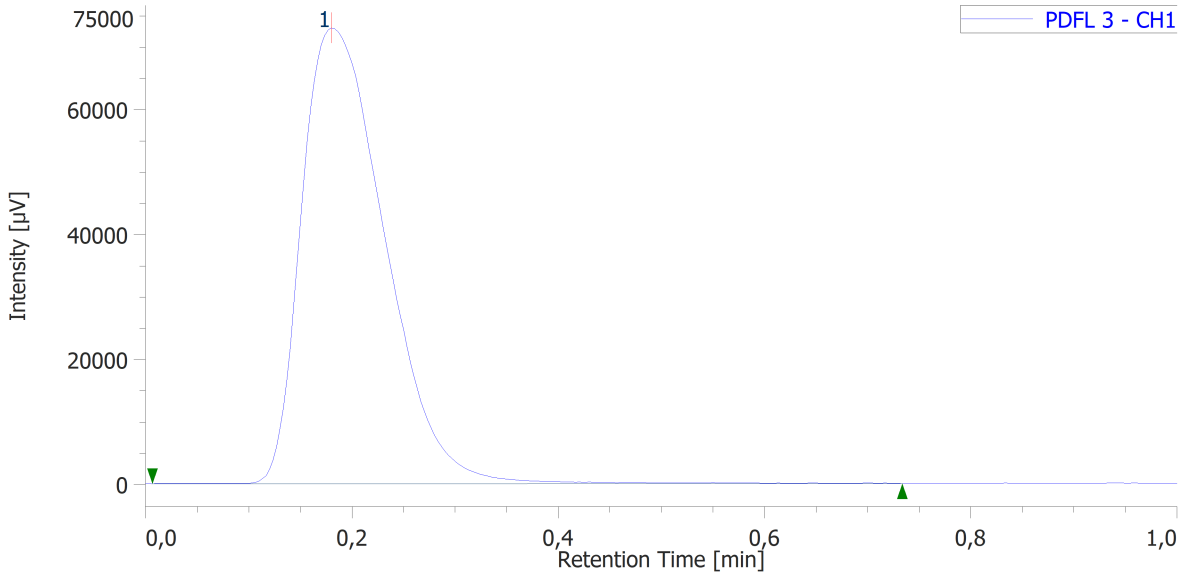

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:31
Description	
HPLC System Name	HP06 - Det FL
Injection Date	28/02/2024 09:46:16
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,180	410071	72920	100,000	100,000	N/A	23	N/A	1,550		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

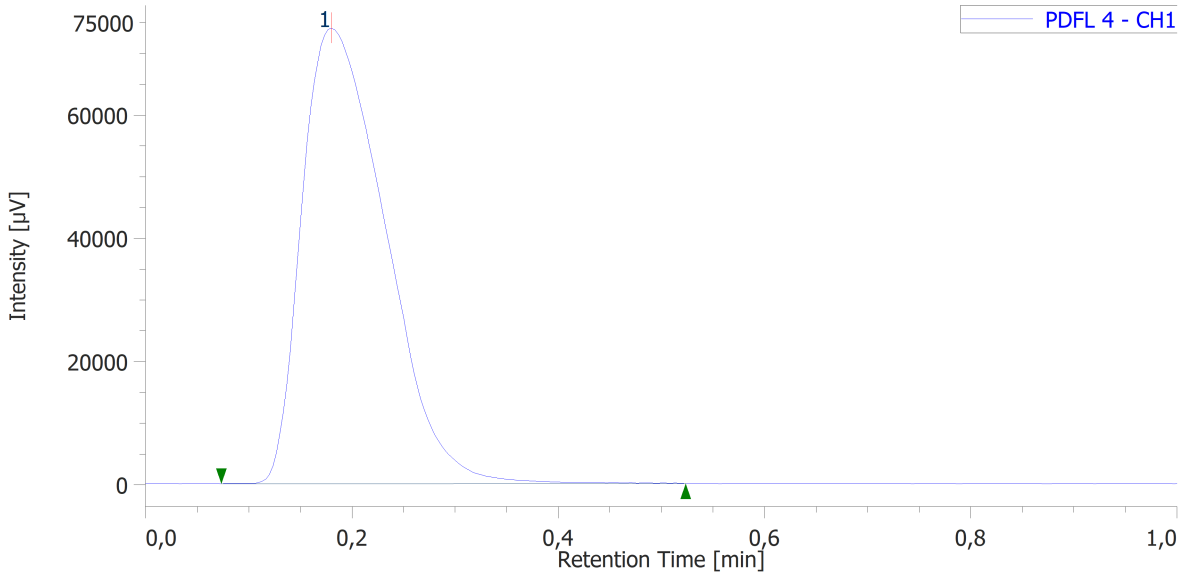

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:31
Description	
HPLC System Name	HP06 - Det FL
Injection Date	28/02/2024 09:48:34
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,180	416589	73941	100,000	100,000	N/A	22	N/A	1,580		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

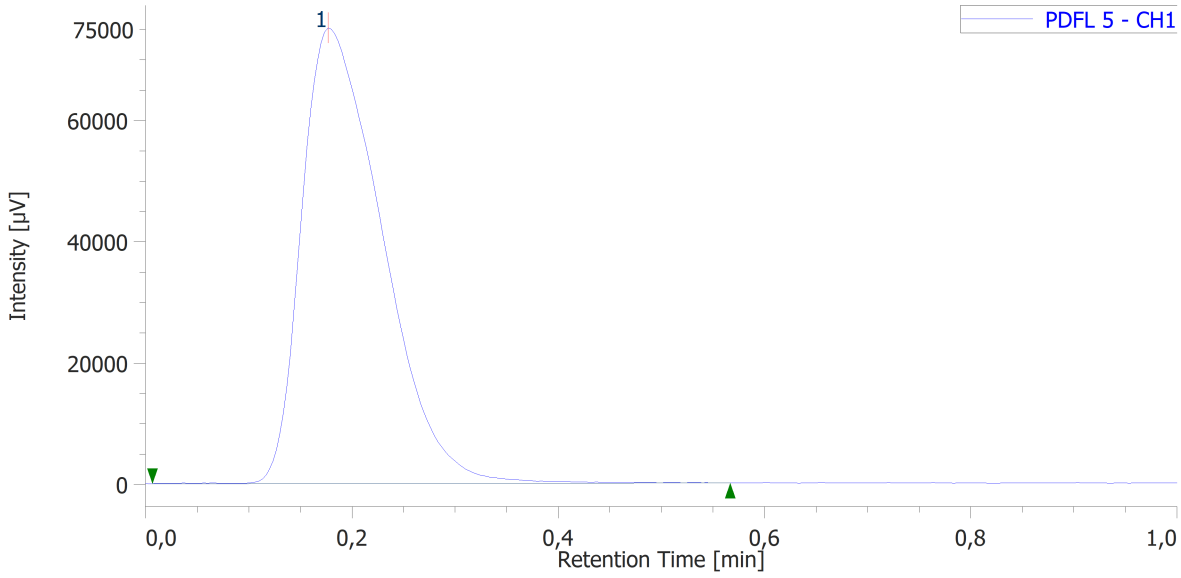

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:31
Description	
HPLC System Name	HP06 – Det FL
Injection Date	28/02/2024 09:50:52
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,177	408283	75063	100,000	100,000	N/A	24	N/A	1,652		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

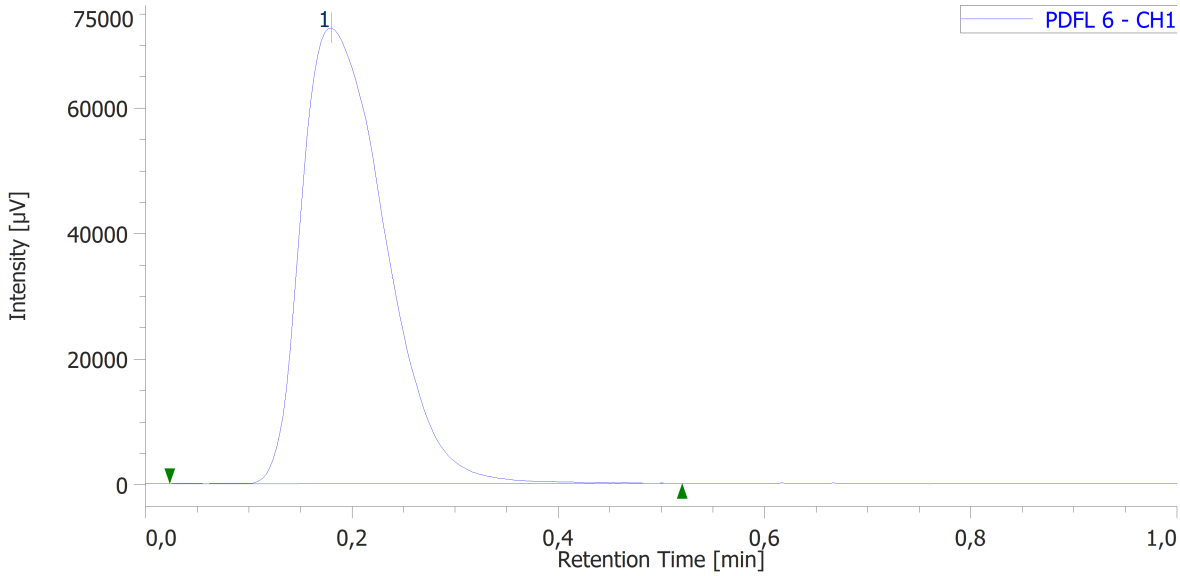

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:01:32
Description	
HPLC System Name	HP06 – Det FL
Injection Date	28/02/2024 09:53:11
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	Sequência Qualificação FL QPack
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,180	408112	72548	100,000	100,000	N/A	23	N/A	1,537		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

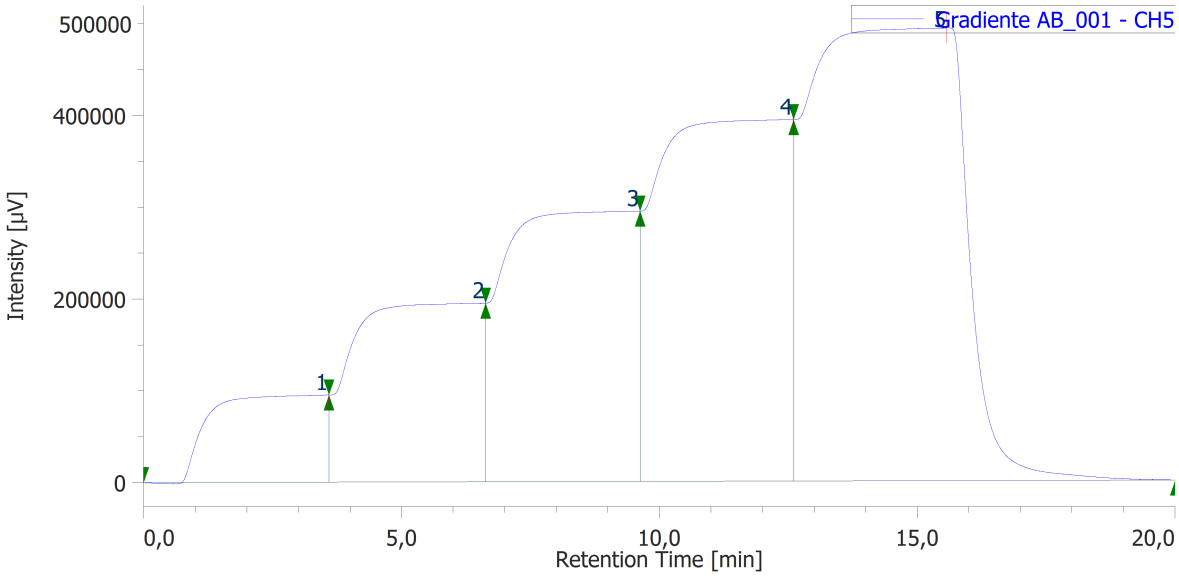

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:02:07
Description	
HPLC System Name	HP06
Injection Date	28/02/2024 10:20:11
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20%	5	3,587	14001084	94916	5,287	6,460	N/A	N/A	N/A	N/A		N/A
2	40%	5	6,623	32424754	194369	12,244	13,228	N/A	N/A	N/A	N/A		N/A
3	60%	5	9,620	50080061	294117	18,910	20,017	N/A	N/A	N/A	N/A		N/A
4	80%	5	12,590	67422178	393345	25,459	26,770	N/A	N/A	N/A	N/A		N/A
5	100%	5	15,572	100900284	492611	38,100	33,526	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA

Chromatogram

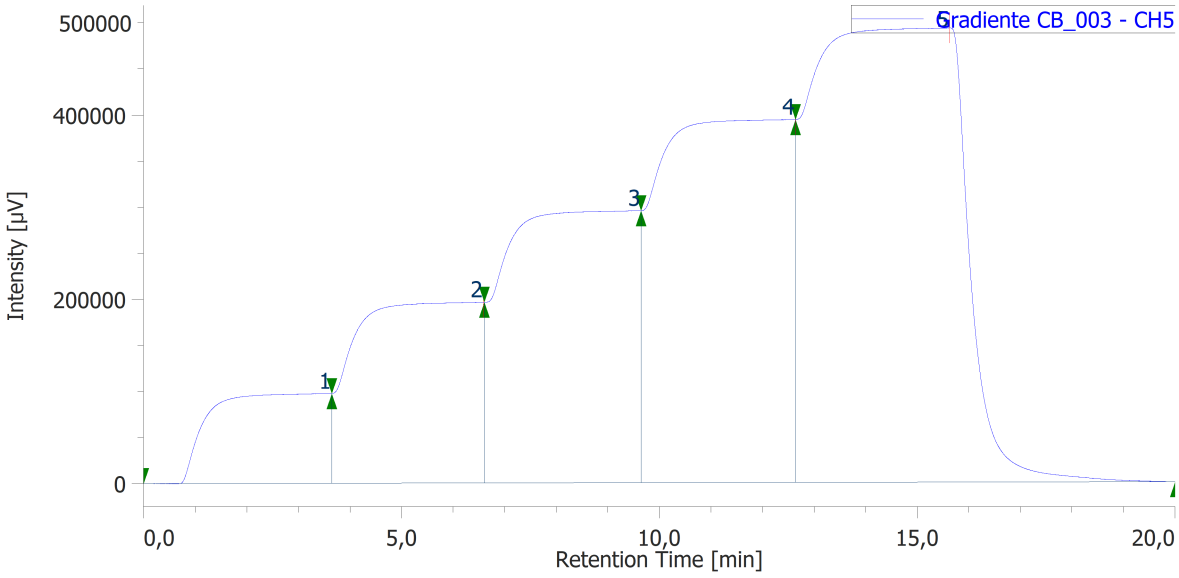

Chromatogram Information	
User Name	QPackSA
Date Modified	28/02/2024 12:02:08
Description	
HPLC System Name	HP06
Injection Date	28/02/2024 11:06:30
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente CB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CB_003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20%	5	3,645	14811347	97322	5,571	6,602	N/A	N/A	N/A	N/A		N/A
2	40%	5	6,585	32133446	196035	12,087	13,298	N/A	N/A	N/A	N/A		N/A
3	60%	5	9,640	50886257	294925	19,141	20,006	N/A	N/A	N/A	N/A		N/A
4	80%	5	12,630	68126395	393442	25,626	26,688	N/A	N/A	N/A	N/A		N/A
5	100%	5	15,623	99888686	492493	37,574	33,407	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer QPackSA
Approver QPackSA