
Chromatogram

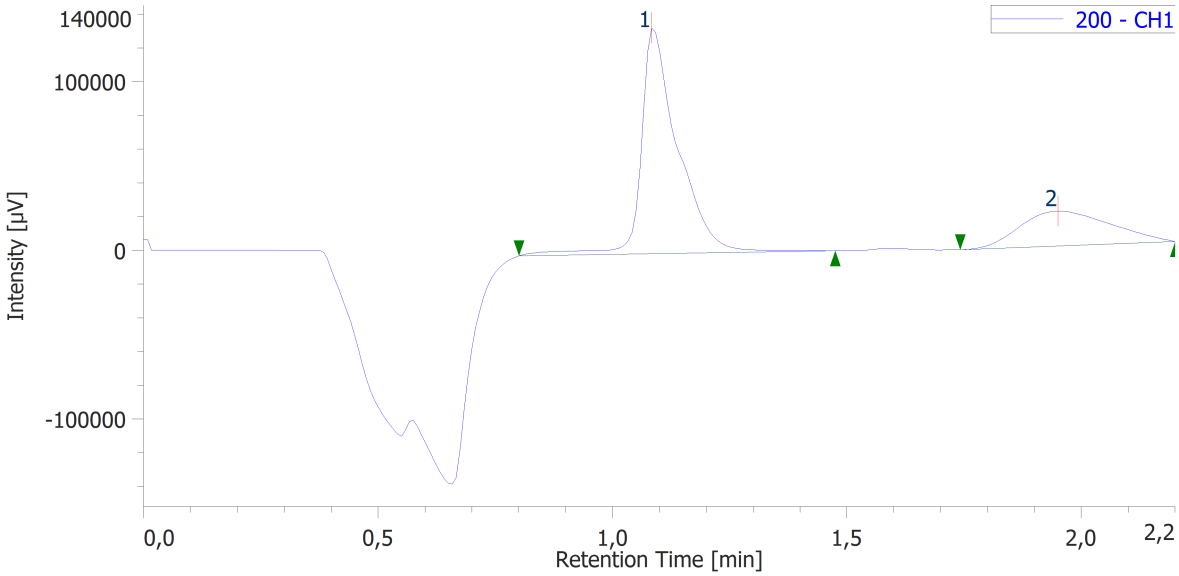

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:15:08
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	200
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	200-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	726485	133762	72,443	86,583	N/A	1291	3,524	1,822	
2	Unknown	1	1,950	276356	20727	27,557	13,417	N/A	438	N/A	1,219	

Creator QPackSA
Reviewer
Approver

Chromatogram

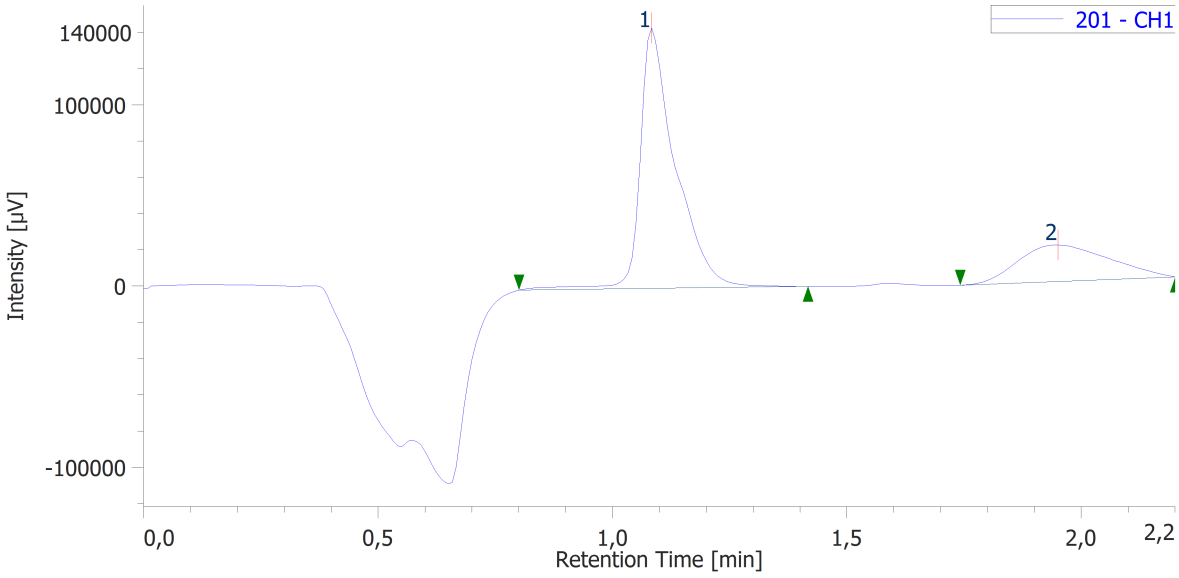

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:19:23
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	201
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	201-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	750884	143681	73,495	87,683	N/A	1321	3,522	1,764	
2	Unknown	1	1,950	270794	20182	26,505	12,317	N/A	434	N/A	1,204	

Creator QPackSA
Reviewer
Approver

Chromatogram

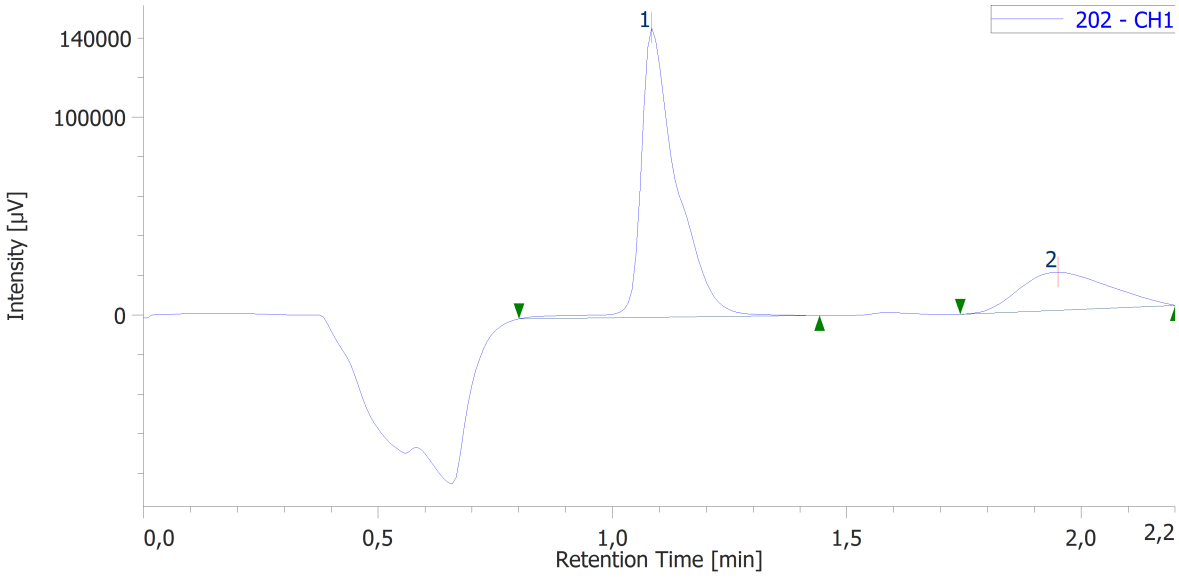

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:23:38
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	202
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	202-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	771991	146129	75,133	88,385	N/A	1311	3,539	1,919	
2	Unknown	1	1,950	255514	19204	24,867	11,615	N/A	441	N/A	1,222	

Creator QPackSA
Reviewer
Approver

Chromatogram

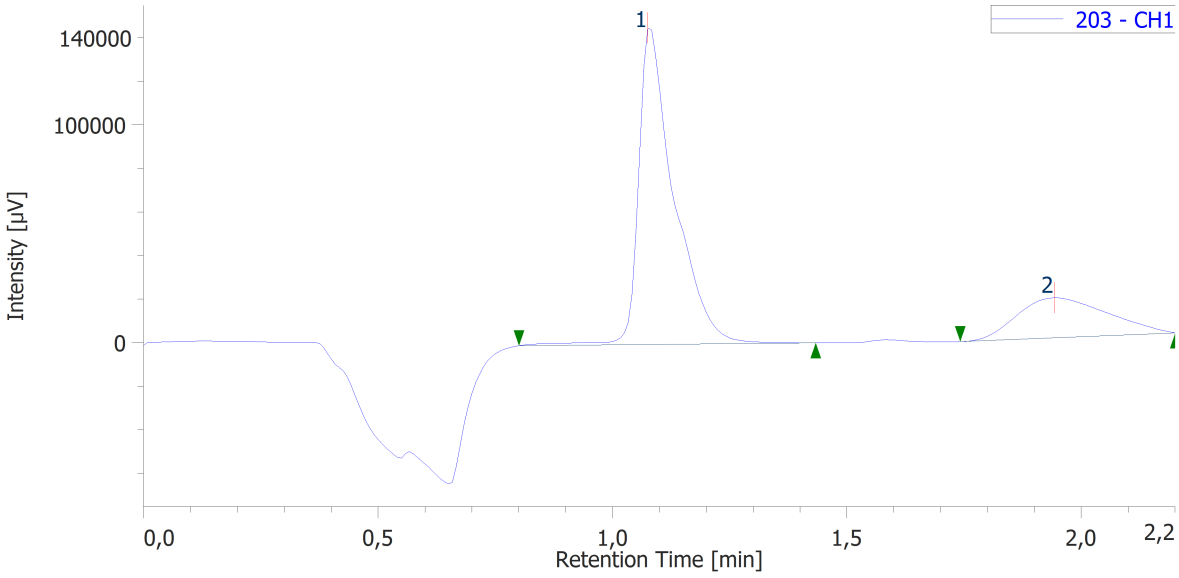

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:27:54
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	203
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	203-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,075	761153	145210	75,578	88,740	N/A	1298	3,539	2,054	
2	Unknown	1	1,942	245956	18426	24,422	11,260	N/A	437	N/A	1,263	

Creator QPackSA
Reviewer
Approver

Chromatogram

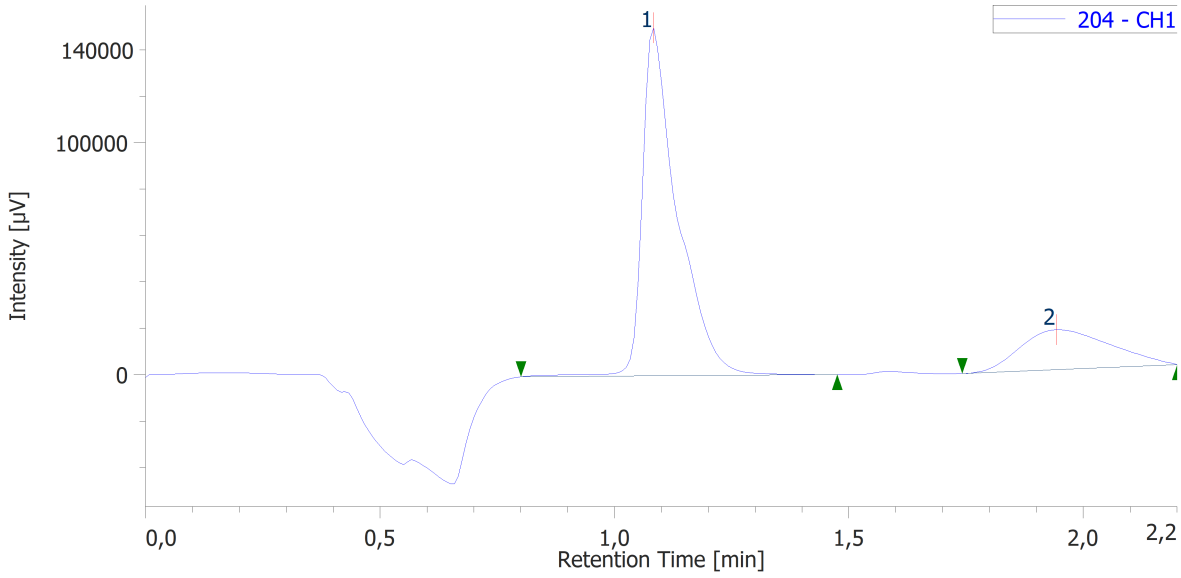

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:32:07
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	204
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	204-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	779860	149925	77,369	89,701	N/A	1338	3,532	1,912	
2	Unknown	1	1,942	228112	17214	22,631	10,299	N/A	443	N/A	1,279	

Creator QPackSA
Reviewer
Approver

Chromatogram

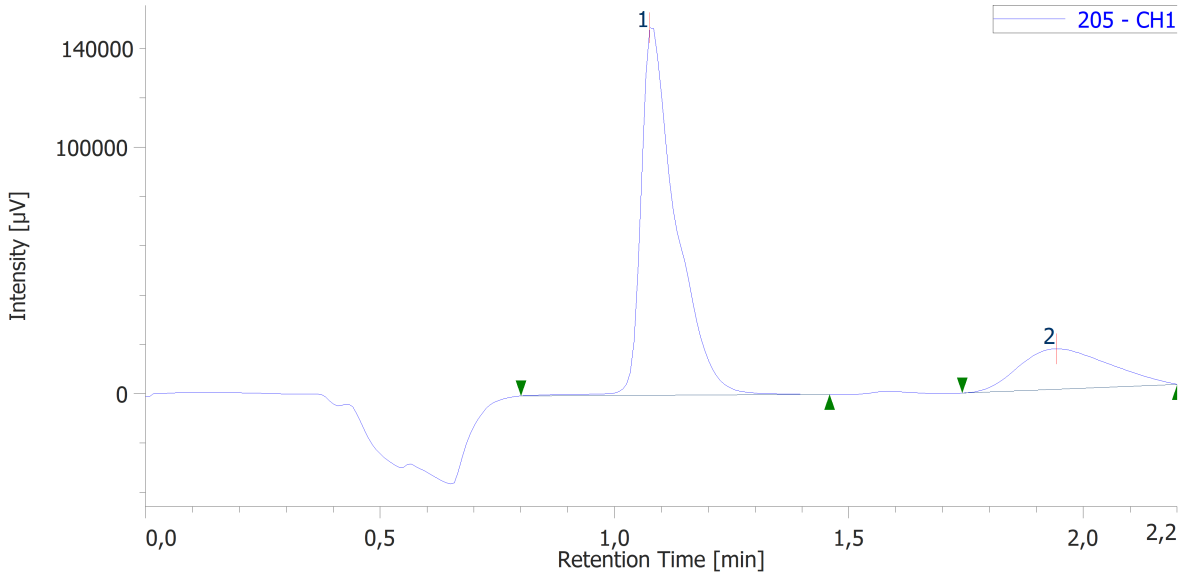

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:36:22
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	205
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	205-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,075	771525	148879	77,868	90,061	N/A	1281	3,536	2,104	
2	Unknown	1	1,942	219288	16430	22,132	9,939	N/A	437	N/A	1,259	

Creator QPackSA
Reviewer
Approver

Chromatogram

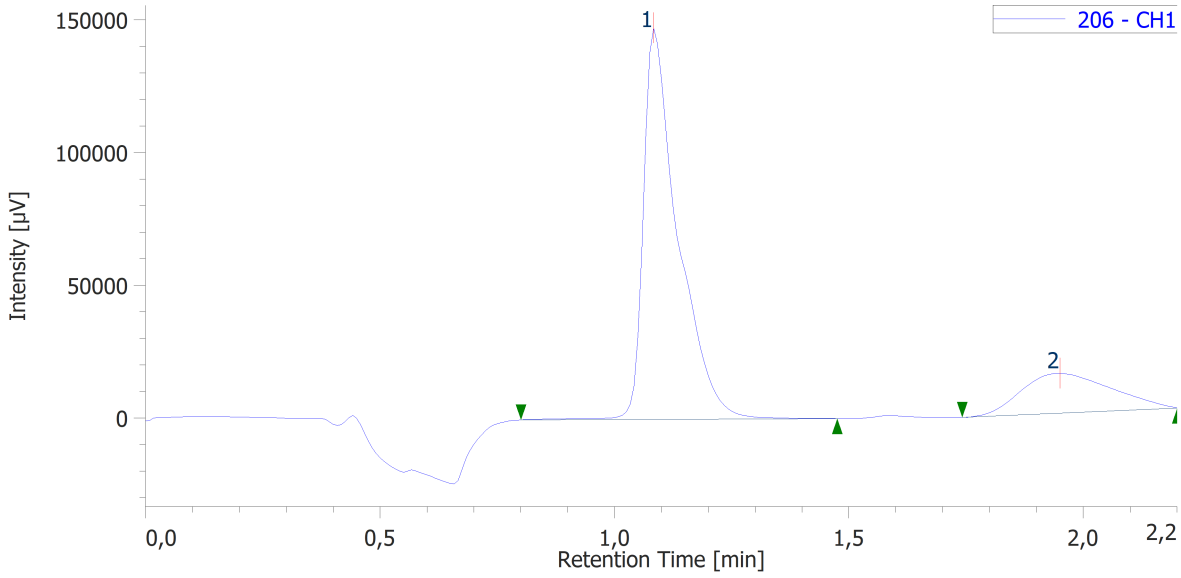

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:40:37
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	206
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	206-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	751959	147408	79,053	90,745	N/A	1342	3,568	1,960	
2	Unknown	1	1,950	199244	15034	20,947	9,255	N/A	447	N/A	1,218	

Creator QPackSA
Reviewer
Approver

Chromatogram

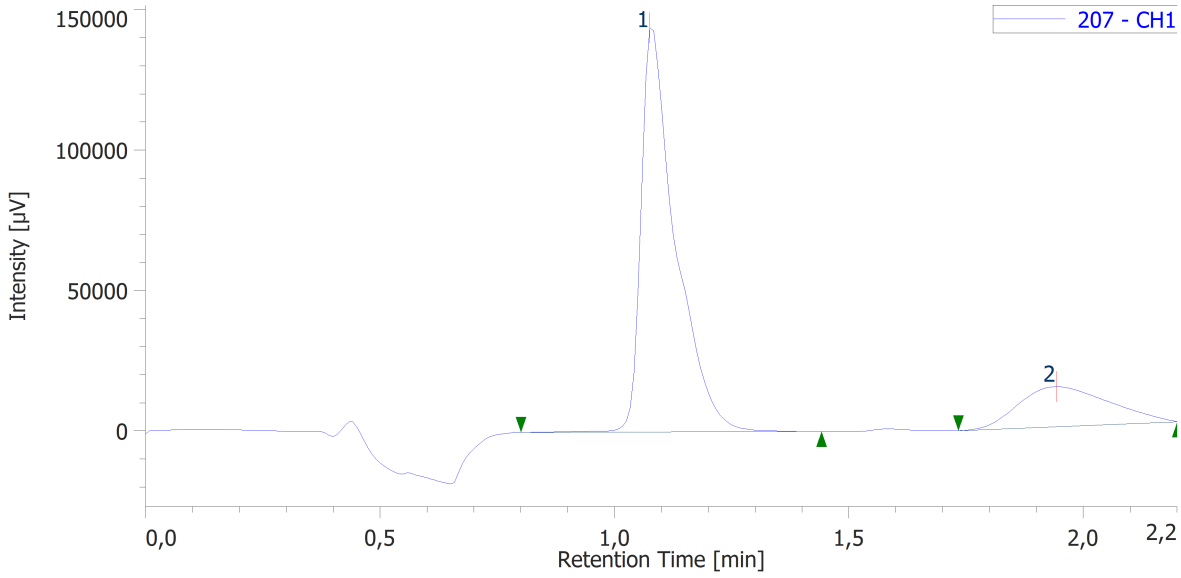

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:44:54
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	207
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	207-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,075	734017	143793	79,459	90,996	N/A	1335	3,562	2,130	
2	Unknown	1	1,942	189747	14229	20,541	9,004	N/A	440	N/A	1,253	

Creator QPackSA
Reviewer
Approver

Chromatogram

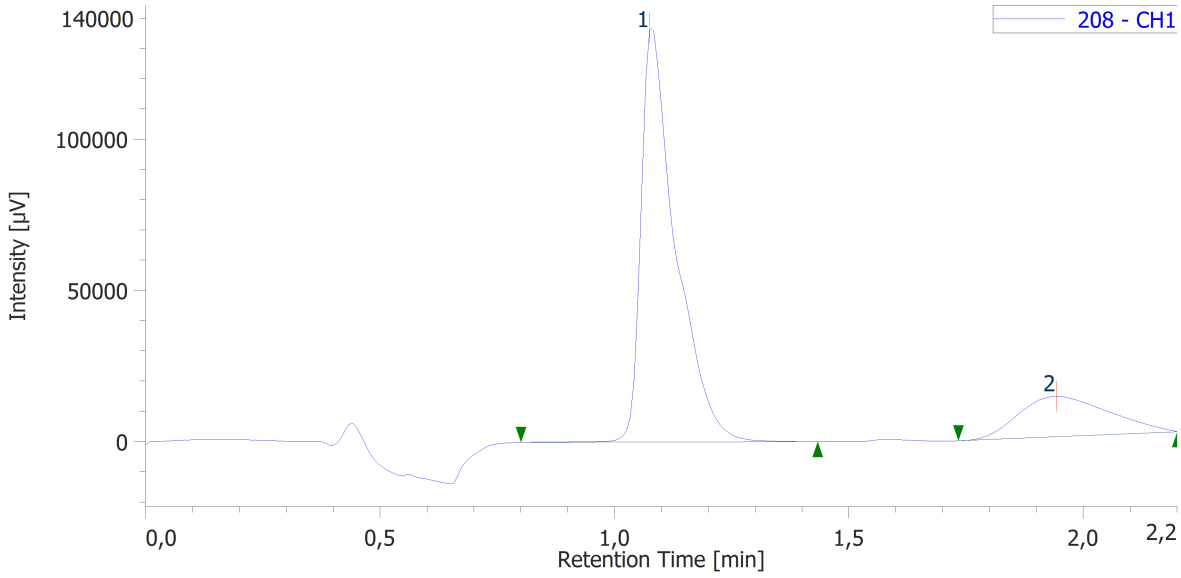

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:49:05
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	208
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	208-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,075	702177	136856	79,778	91,119	N/A	1309	3,552	2,131	
2	Unknown	1	1,942	177987	13339	20,222	8,881	N/A	440	N/A	1,250	

Creator QPackSA
Reviewer
Approver

Chromatogram

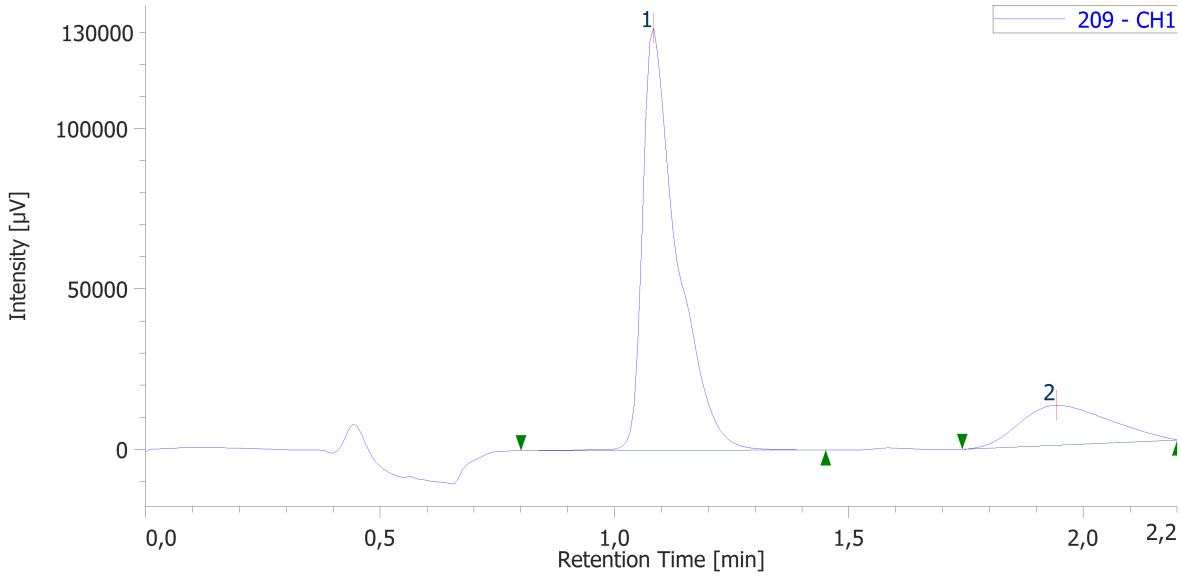

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:53:21
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	209
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	209-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	673223	131612	80,346	91,383	N/A	1360	3,542	1,934	
2	Unknown	1	1,942	164677	12411	19,654	8,617	N/A	444	N/A	1,267	

Creator QPackSA
Reviewer
Approver

Chromatogram

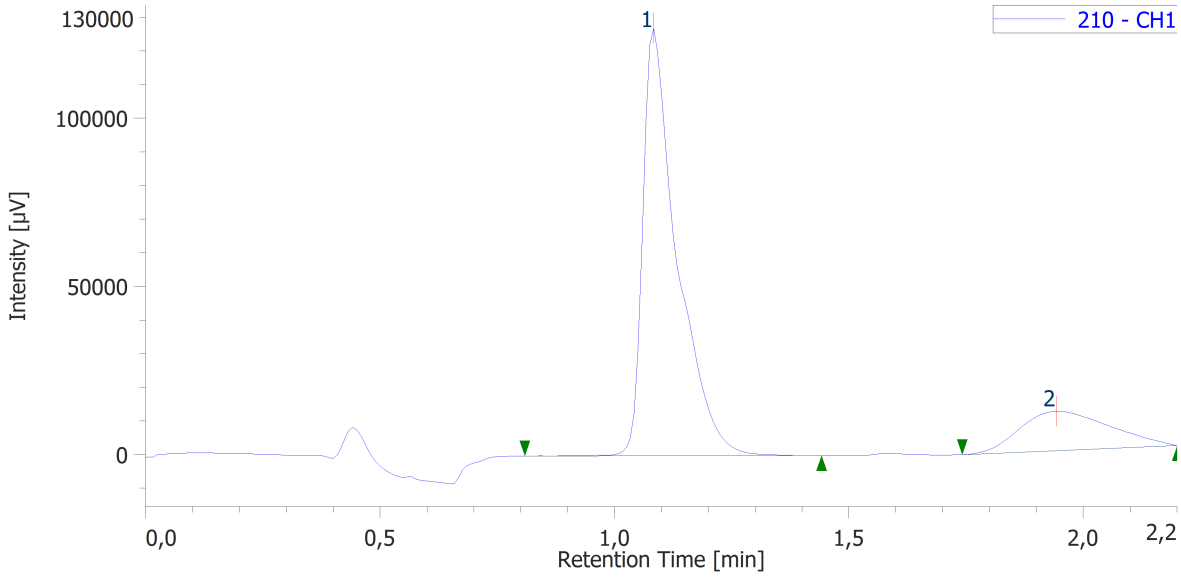

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 09:33:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 16:57:36
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	210
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	210-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	643292	127115	80,575	91,570	N/A	1384	3,554	1,950	
2	Unknown	1	1,942	155083	11703	19,425	8,430	N/A	446	N/A	1,269	

Creator QPackSA
Reviewer
Approver

Chromatogram

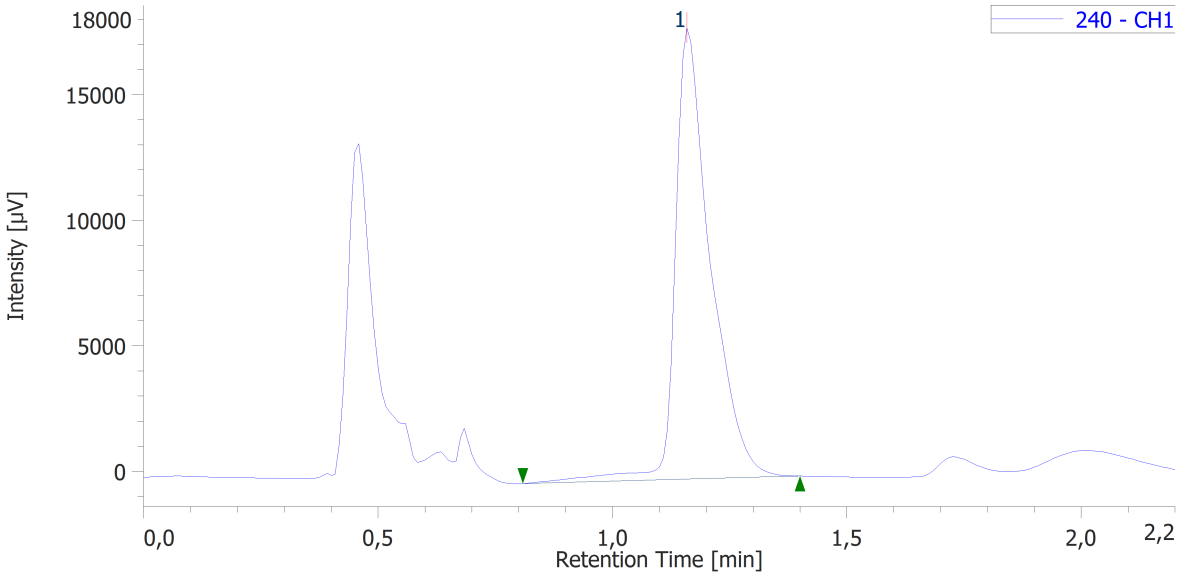

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:06:17
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	240
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	240-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,158	93666	17947	100,000	100,000	N/A	1429	N/A	1,824	

Creator QPackSA
Reviewer
Approver

Chromatogram

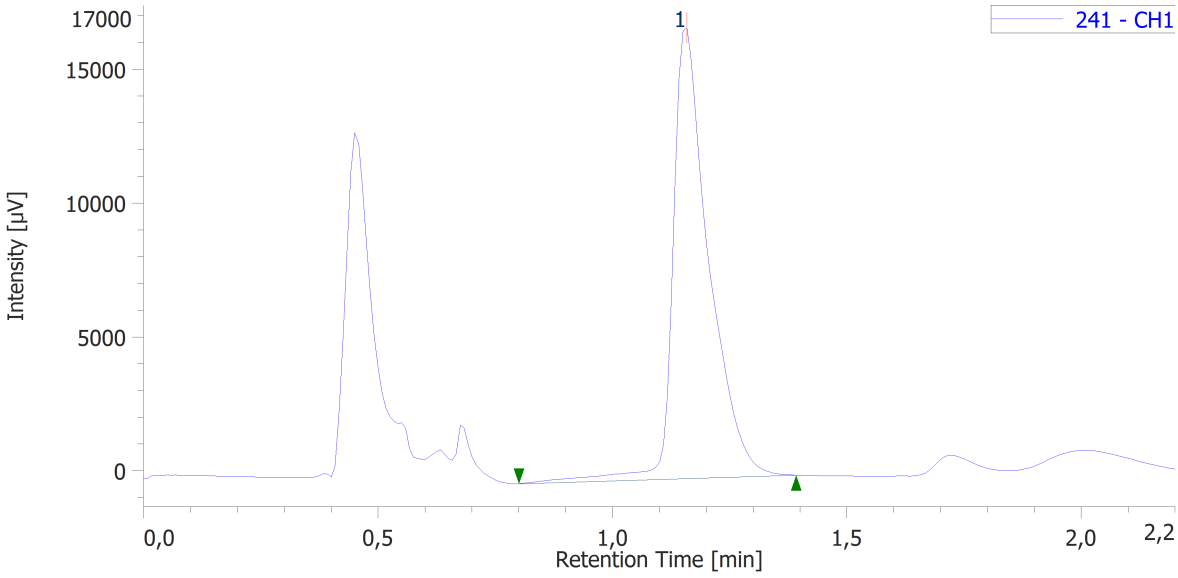

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:10:30
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	241
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	241-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,158	89570	16822	100,000	100,000	N/A	1363	N/A	1,665	

Creator QPackSA
Reviewer
Approver

Chromatogram

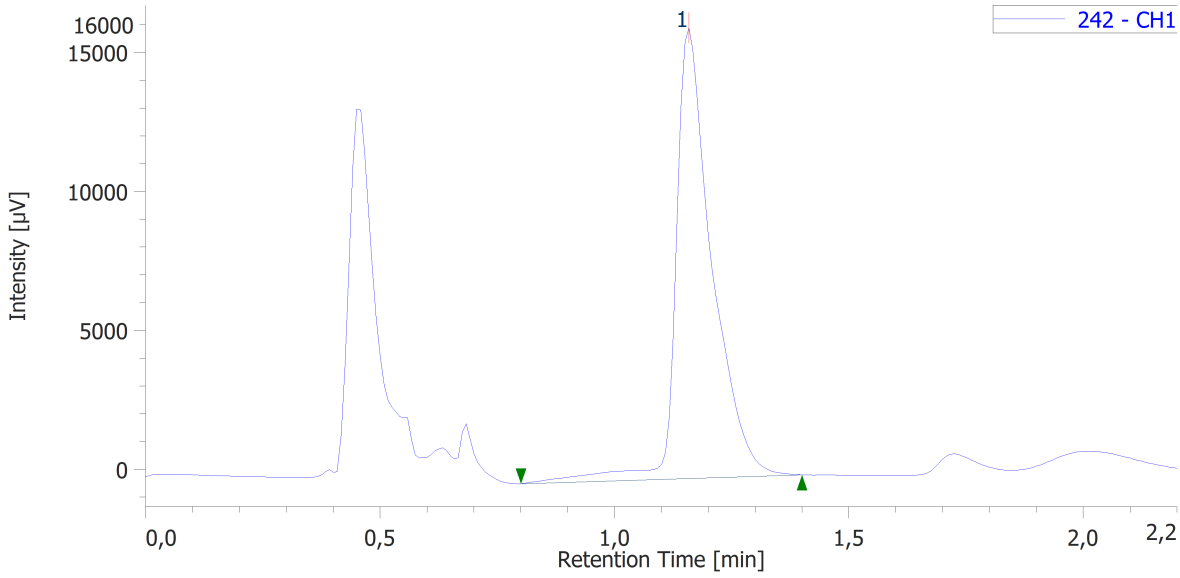

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:14:45
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	242
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	242-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,158	86971	16203	100,000	100,000	N/A	1400	N/A	1,764	

Creator QPackSA
Reviewer
Approver

Chromatogram

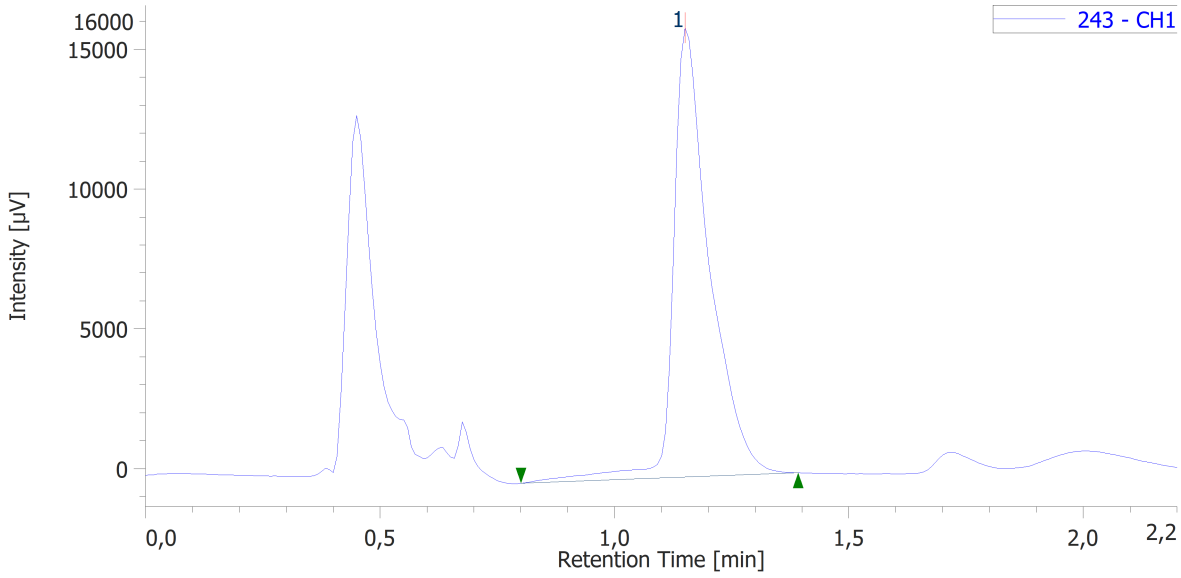

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:18:59
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	243
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	243-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	86187	16049	100,000	100,000	N/A	1404	N/A	1,902	

Creator QPackSA
Reviewer
Approver

Chromatogram

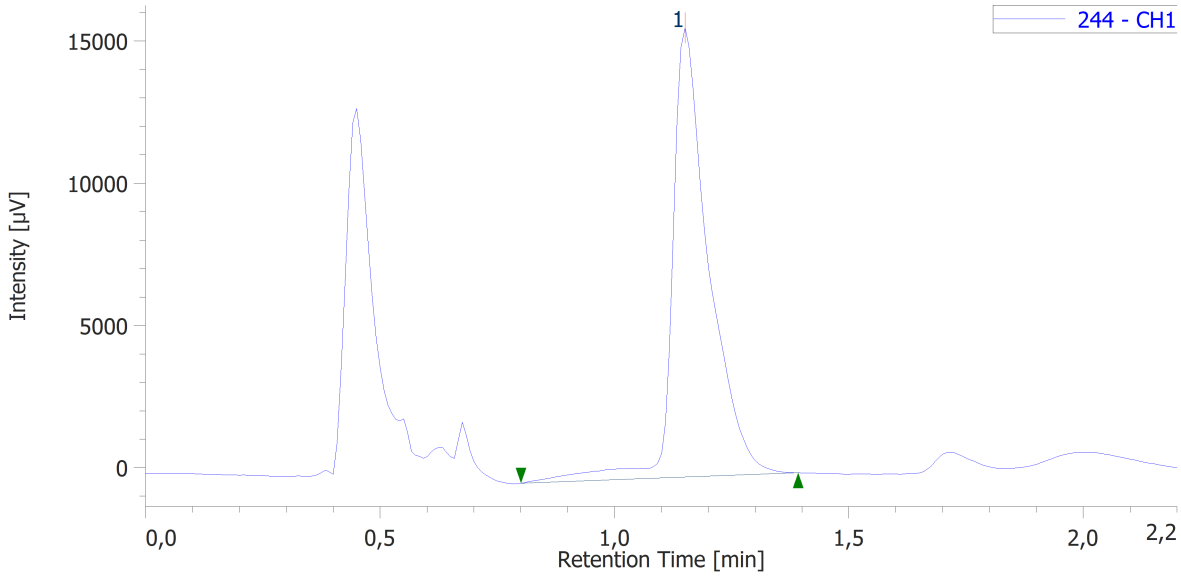

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:23:14
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	244
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	244-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	85736	15773	100,000	100,000	N/A	1391	N/A	1,829	

Creator QPackSA
Reviewer
Approver

Chromatogram

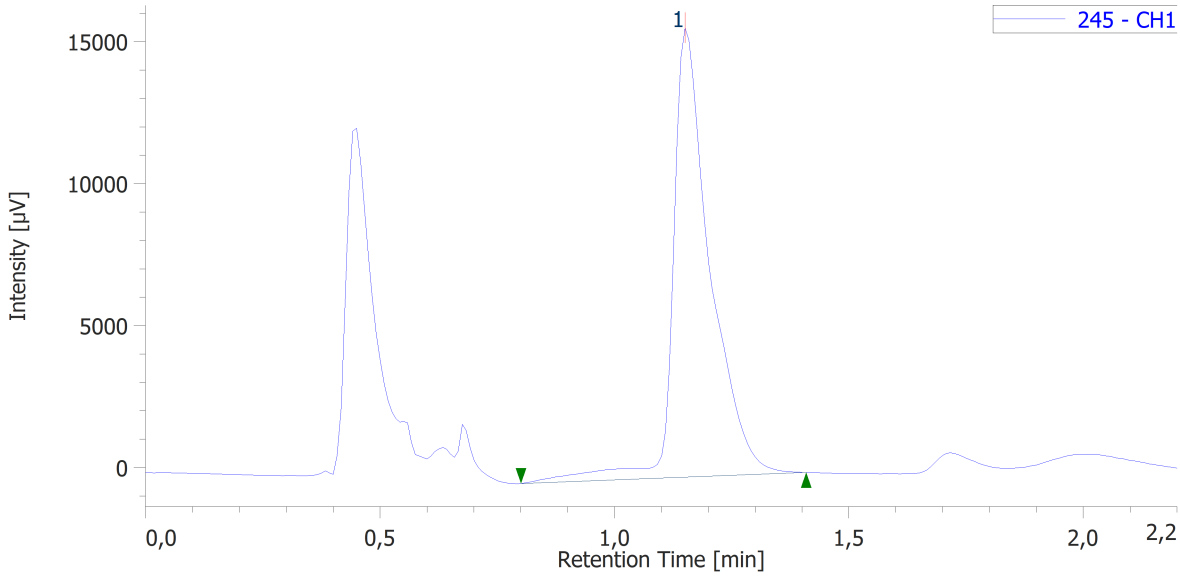

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:27:29
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	245
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	245-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	87005	15812	100,000	100,000	N/A	1399	N/A	1,935	

Creator QPackSA
Reviewer
Approver

Chromatogram

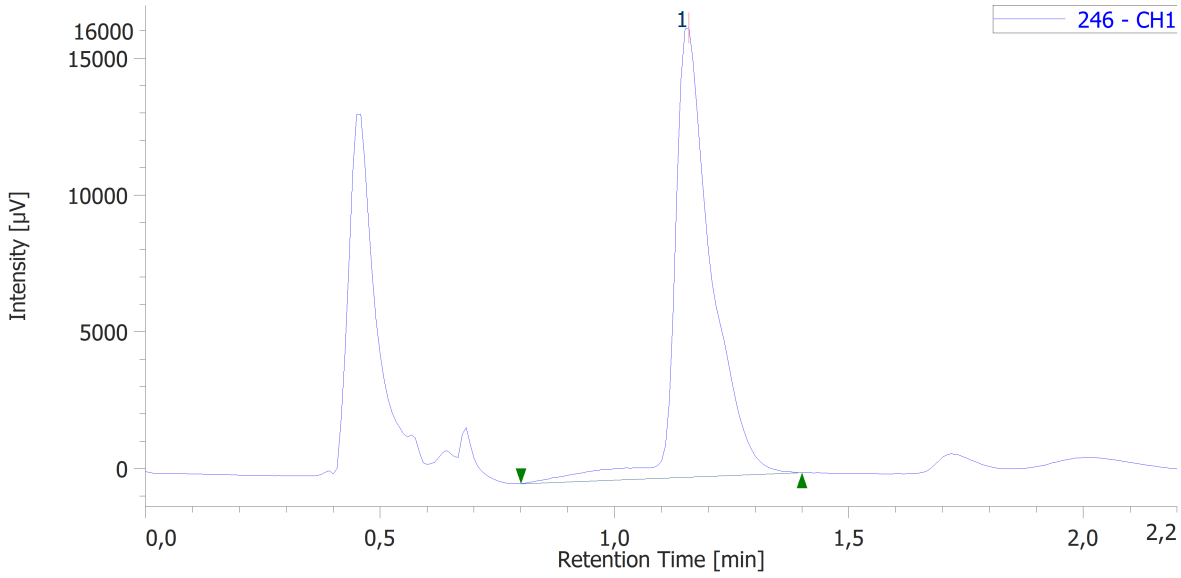

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:31:44
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	246
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	246-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,158	90100	16409	100,000	100,000	N/A	1463	N/A	1,732	

Creator QPackSA
Reviewer
Approver

Chromatogram

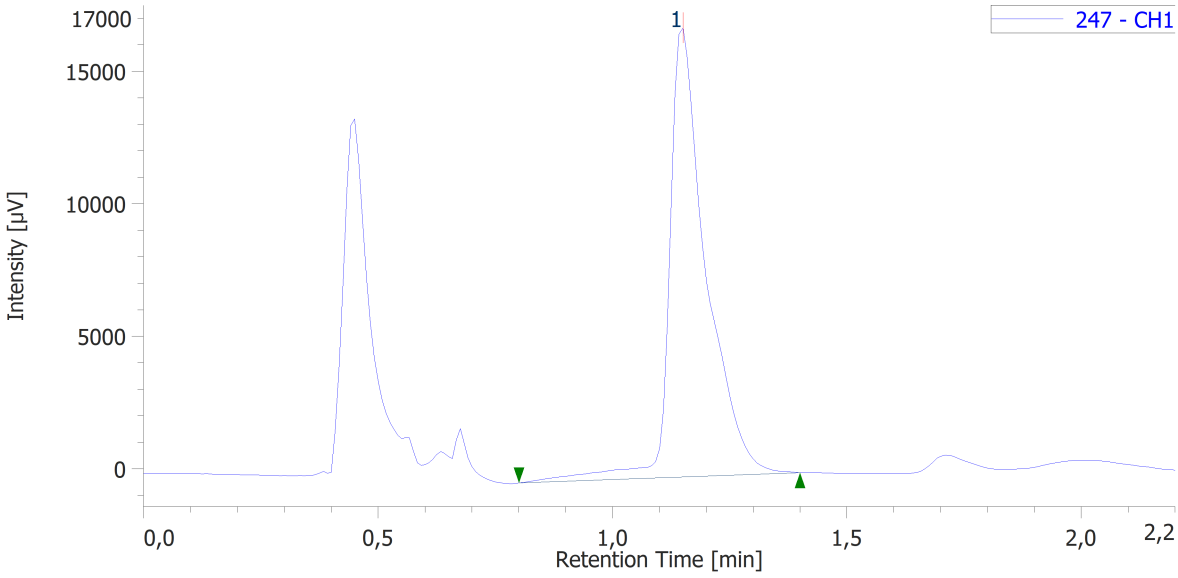

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:28
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:35:57
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	247
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	247-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	92083	16934	100,000	100,000	N/A	1441	N/A	1,781	

Creator QPackSA
Reviewer
Approver

Chromatogram

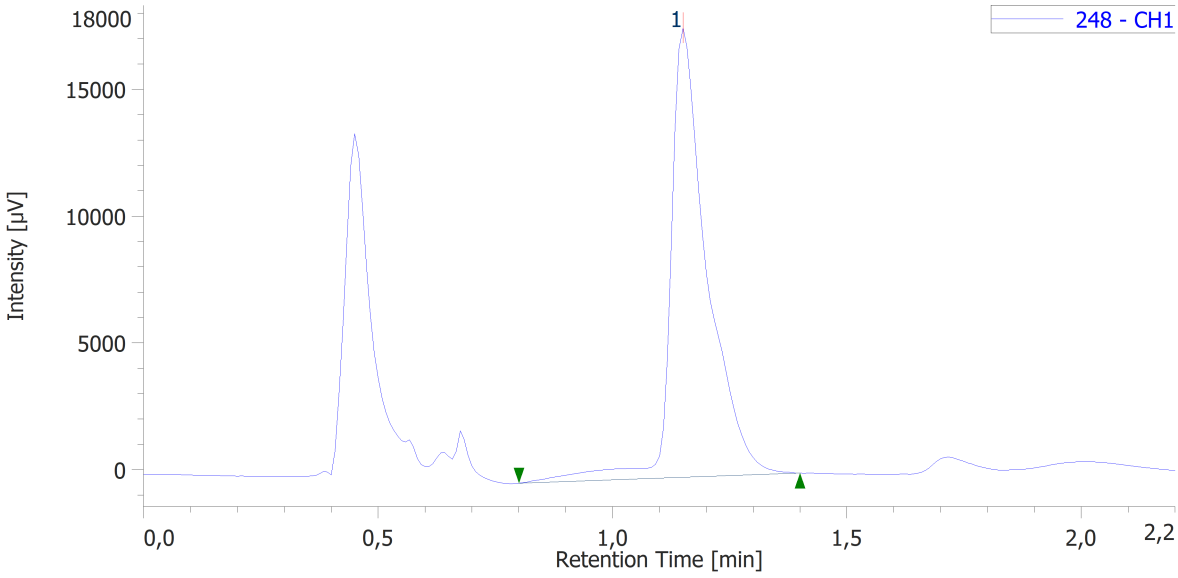

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:29
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:40:12
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	248
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	248-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	95961	17701	100,000	100,000	N/A	1466	N/A	1,919	

Creator QPackSA
Reviewer
Approver

Chromatogram

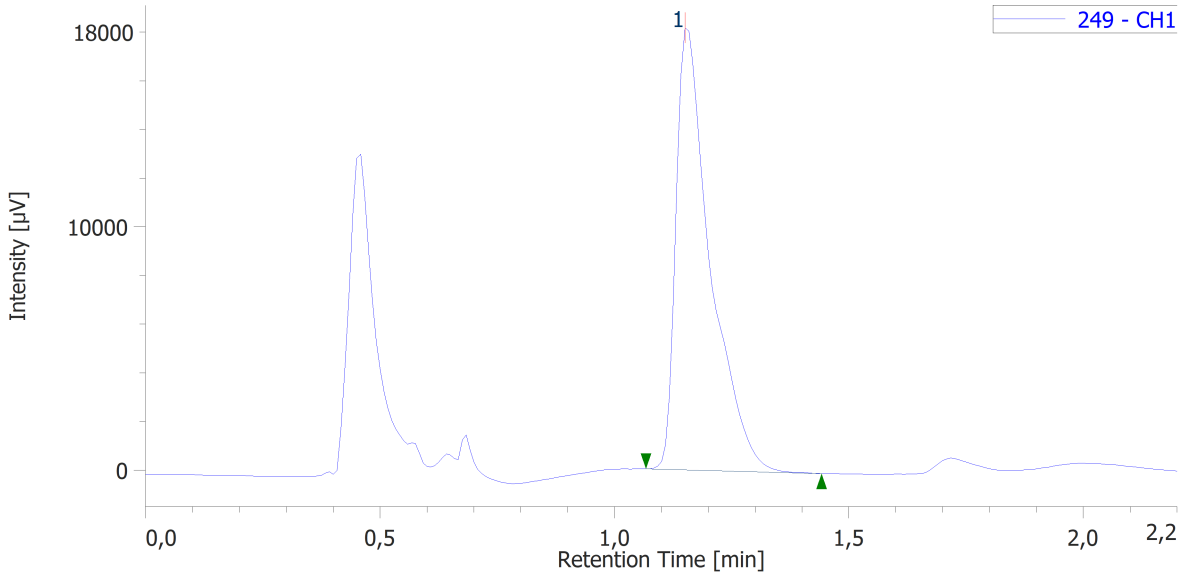

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:29
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:44:27
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	249
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	249-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	92416	18150	100,000	100,000	N/A	1482	N/A	2,174	

Creator QPackSA
Reviewer
Approver

Chromatogram

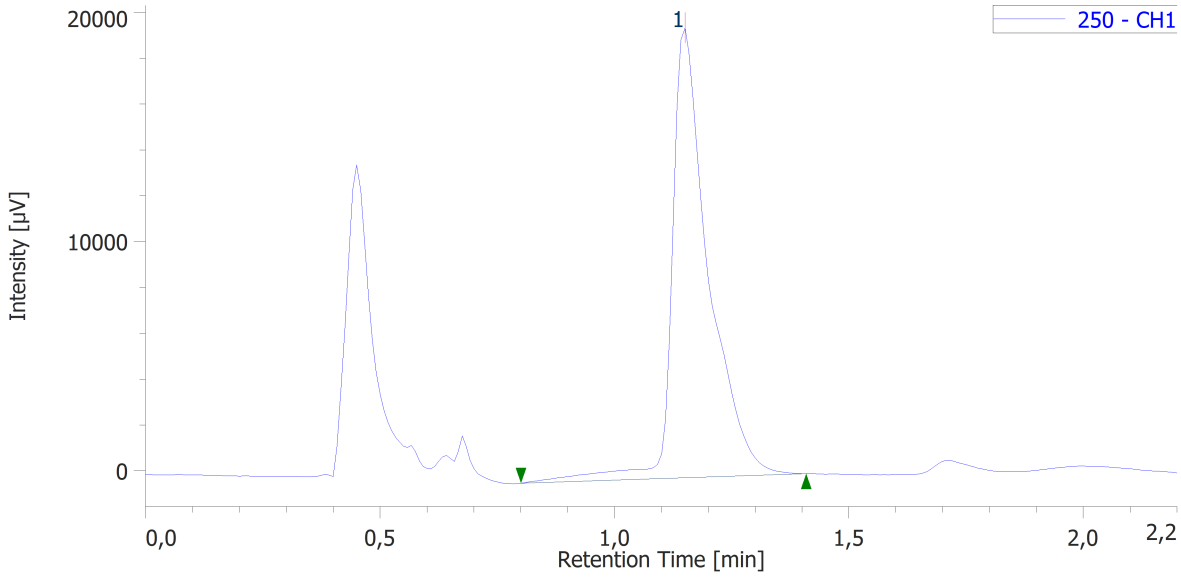

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:53:29
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:48:40
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	250
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	250-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	106114	19611	100,000	100,000	N/A	1462	N/A	1,876	

Creator QPackSA
Reviewer
Approver

Chromatogram

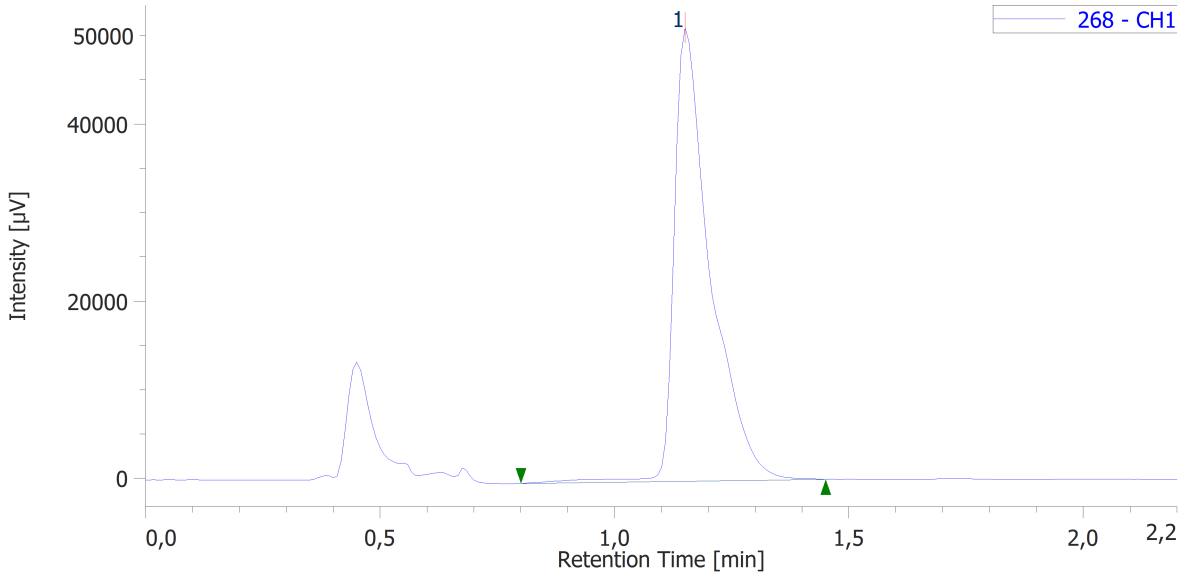

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:55:10
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:52:55
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	268
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	268-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	275386	51145	100,000	100,000	N/A	1401	N/A	2,088	

Creator
Reviewer
Approver

Chromatogram

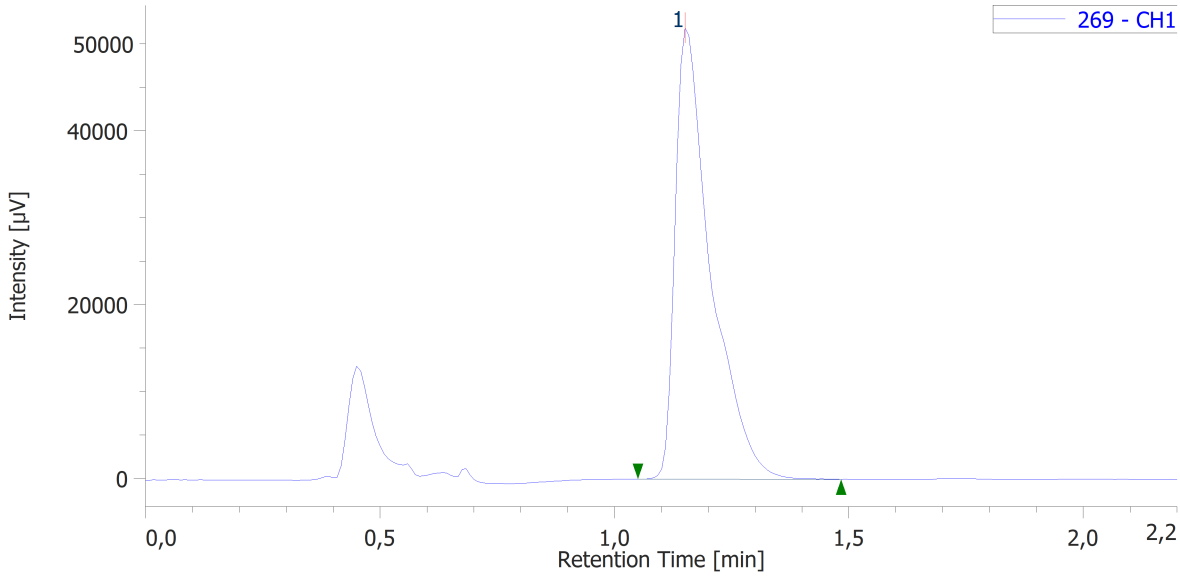

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 10:59:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 10:57:10
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	269
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	269-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	273848	51918	100,000	100,000	N/A	1413	N/A	2,167	

Creator
Reviewer
Approver

Chromatogram

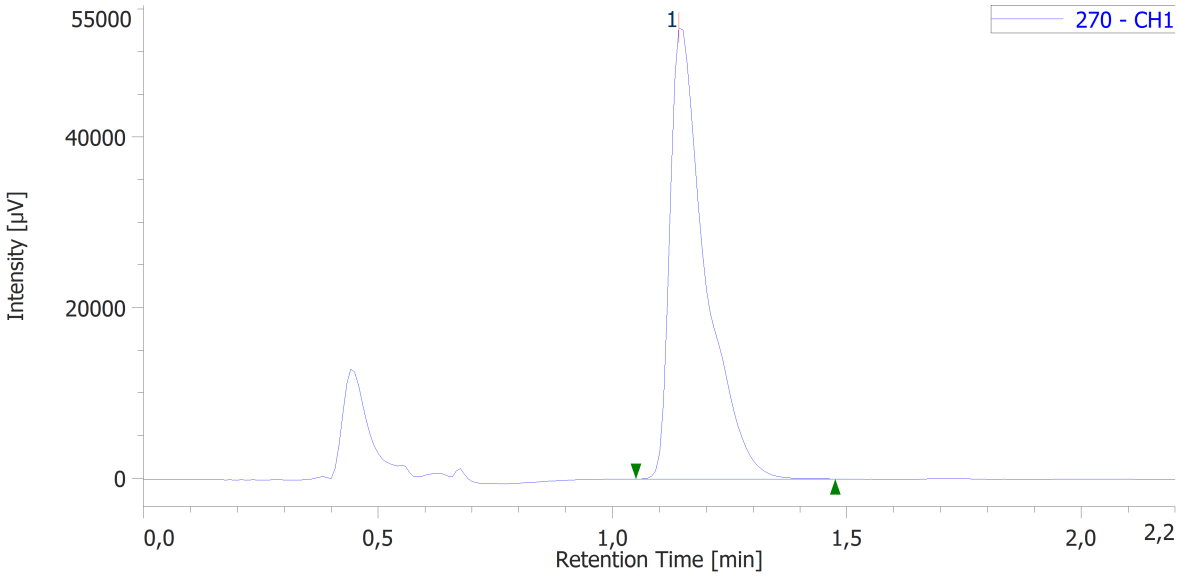

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:03:40
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:01:26
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	270
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	270-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,142	278804	52857	100,000	100,000	N/A	1405	N/A	2,265	

Creator
Reviewer
Approver

Chromatogram

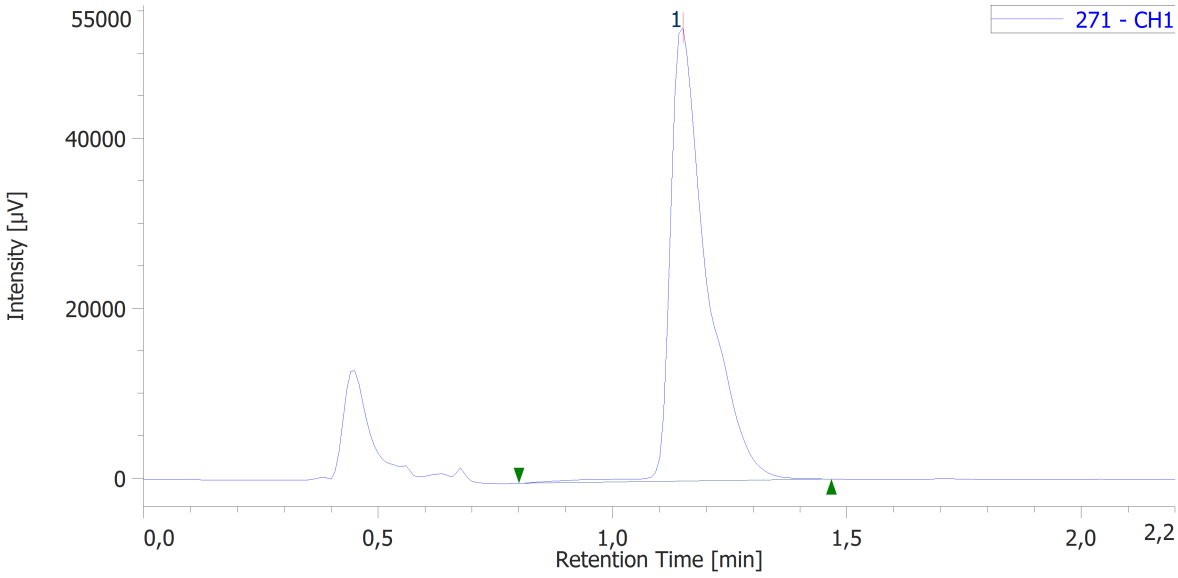

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:07:55
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:05:41
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	271
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	271-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	288249	53300	100,000	100,000	N/A	1387	N/A	1,971	

Creator
Reviewer
Approver

Chromatogram

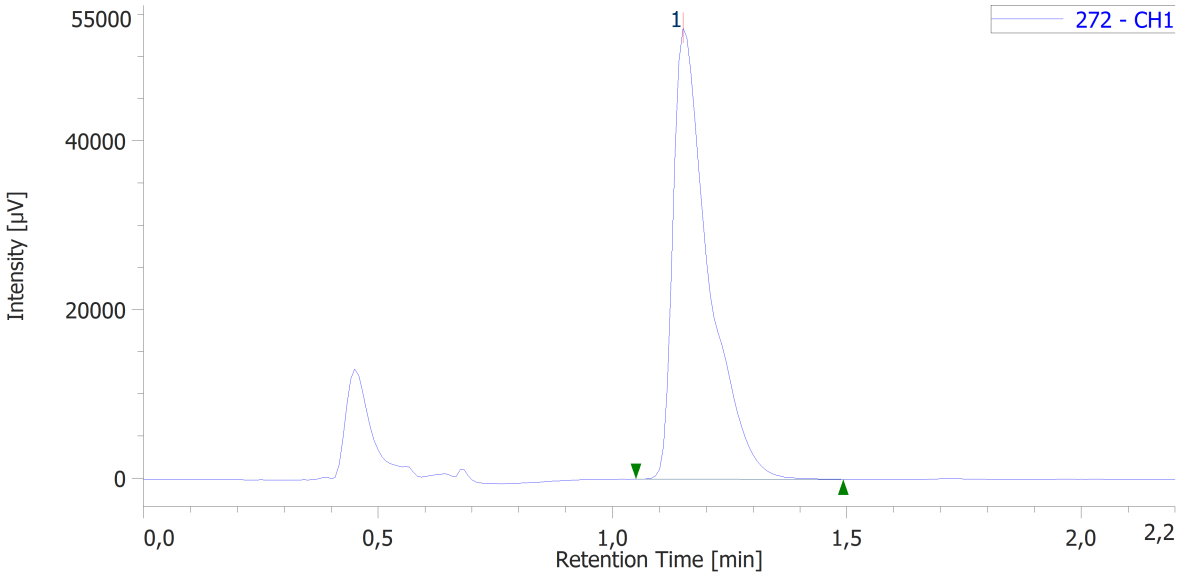

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:12:09
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:09:56
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	272
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	272-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	281934	53465	100,000	100,000	N/A	1407	N/A	2,170	

Creator
Reviewer
Approver

Chromatogram

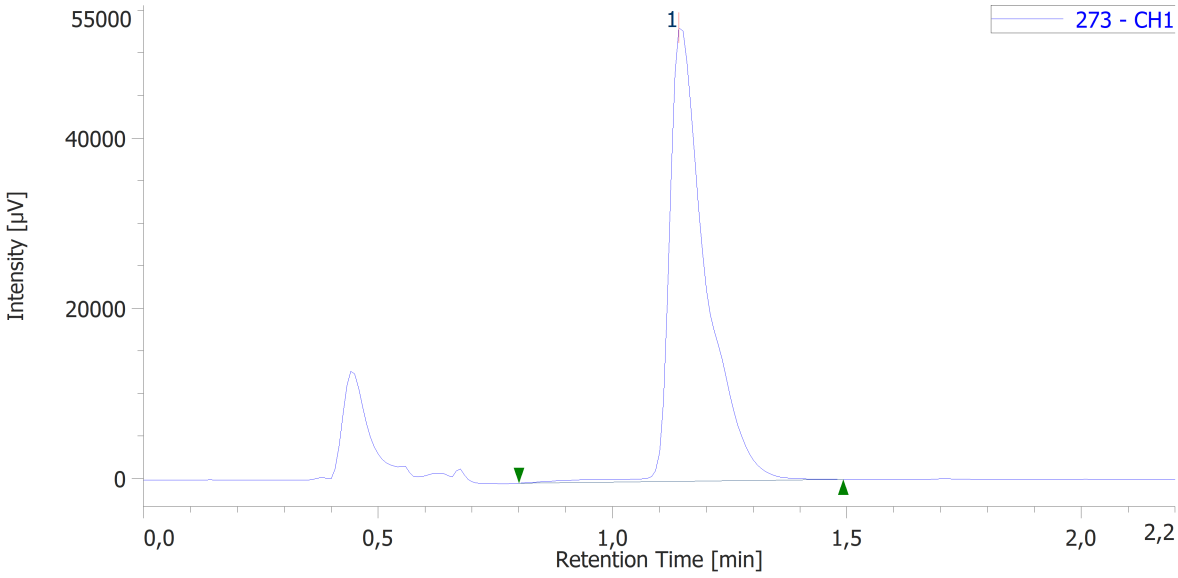

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:17:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:14:11
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	273
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	273-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,142	287408	53236	100,000	100,000	N/A	1384	N/A	2,242	

Creator QPackSA
Reviewer
Approver

Chromatogram

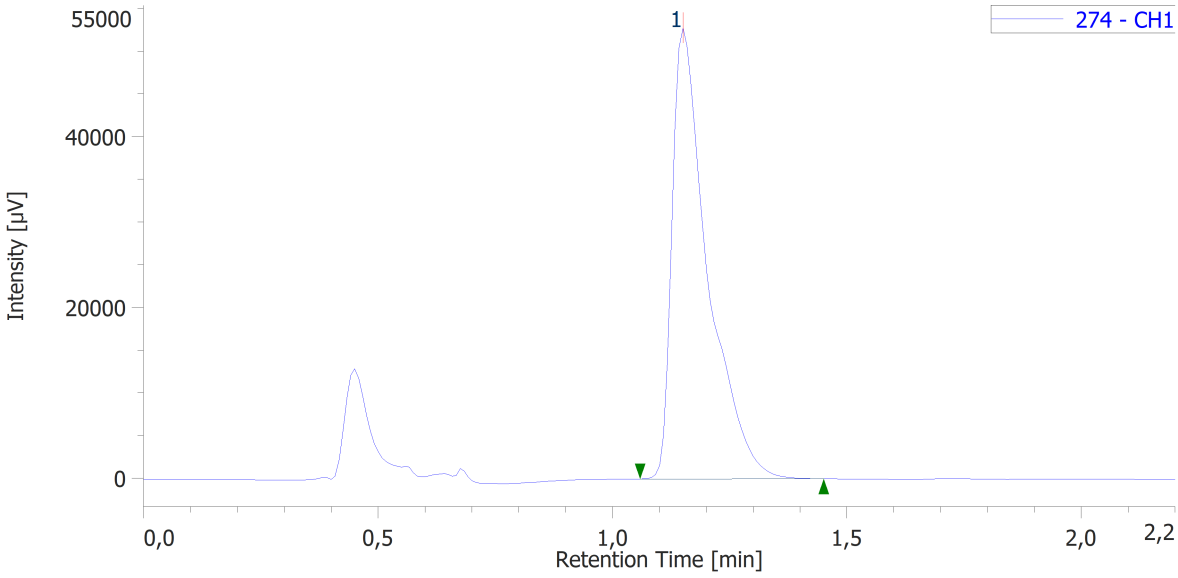

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:41:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:18:26
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	274
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	274-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	278142	52771	100,000	100,000	N/A	1394	N/A	2,080	

Creator QPackSA
Reviewer
Approver

Chromatogram

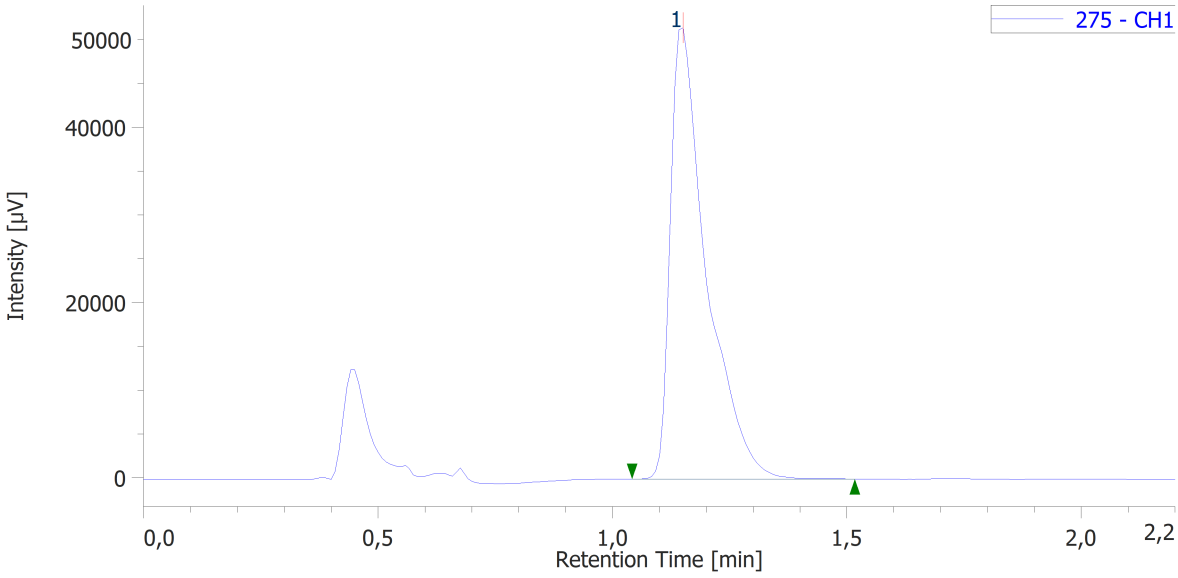

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:41:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:22:41
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	275
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	275-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	275212	51422	100,000	100,000	N/A	1366	N/A	1,966	

Creator QPackSA
Reviewer
Approver

Chromatogram

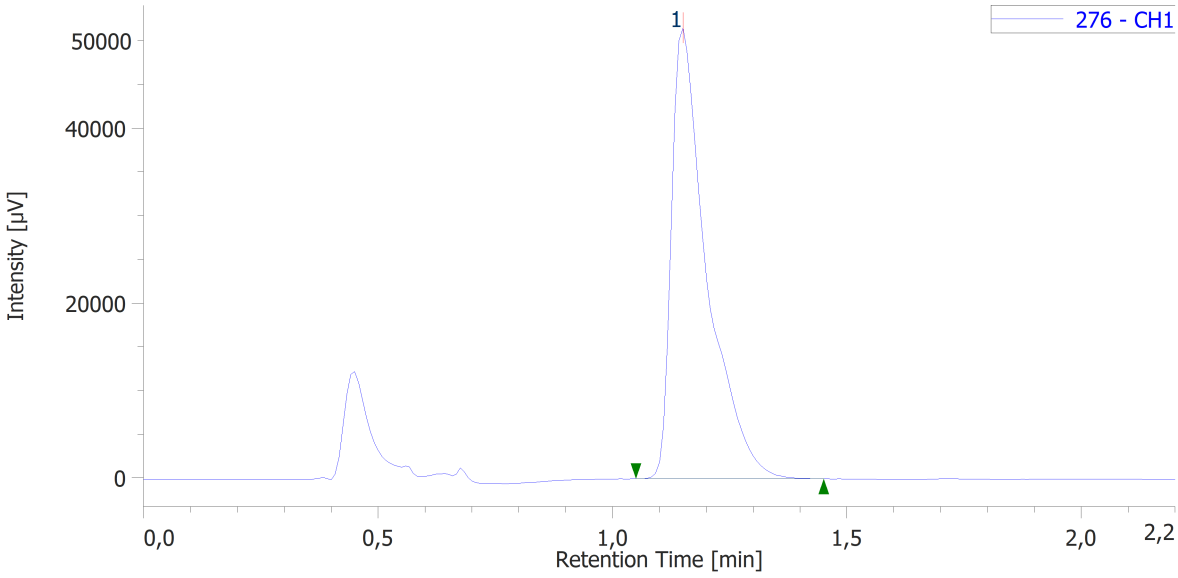

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:41:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:26:57
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	276
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	276-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	270690	51547	100,000	100,000	N/A	1415	N/A	2,043	

Creator QPackSA
Reviewer
Approver

Chromatogram

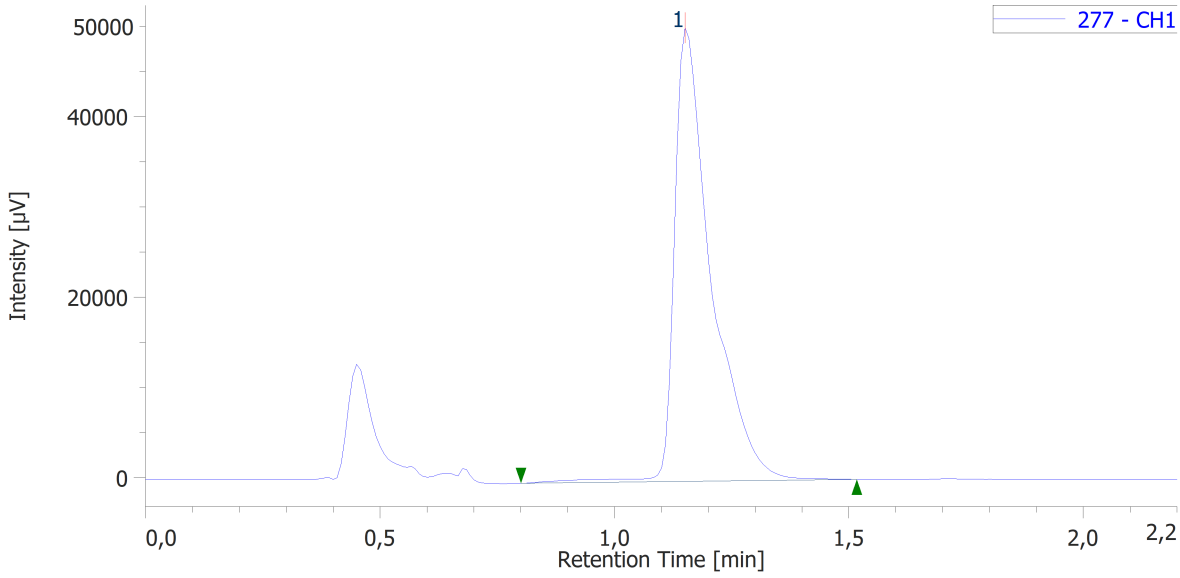

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:41:26
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:31:12
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	277
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	277-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	273416	50193	100,000	100,000	N/A	1386	N/A	2,168	

Creator QPackSA
Reviewer
Approver

Chromatogram

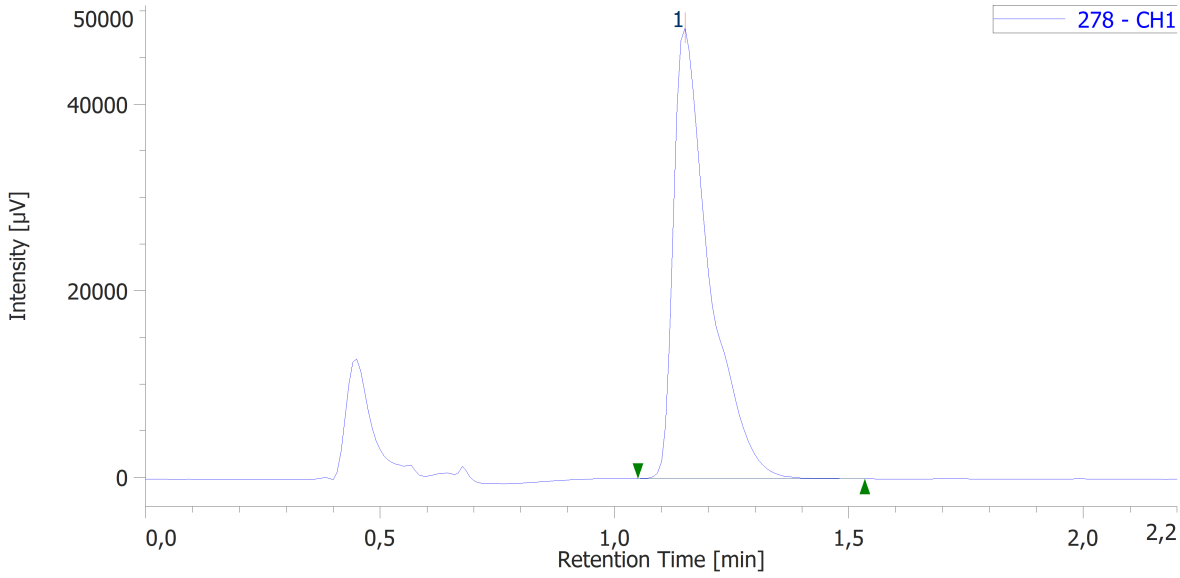

Chromatogram Information	
User Name	QPackSA
Date Modified	12/02/2025 11:41:27
Description	
HPLC System Name	HPLC-0001
Injection Date	12/02/2025 11:35:27
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	EDUV
Control Method	278
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	278-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,150	257314	48291	100,000	100,000	N/A	1366	N/A	2,053	

Creator QPackSA
Reviewer
Approver

Chromatogram

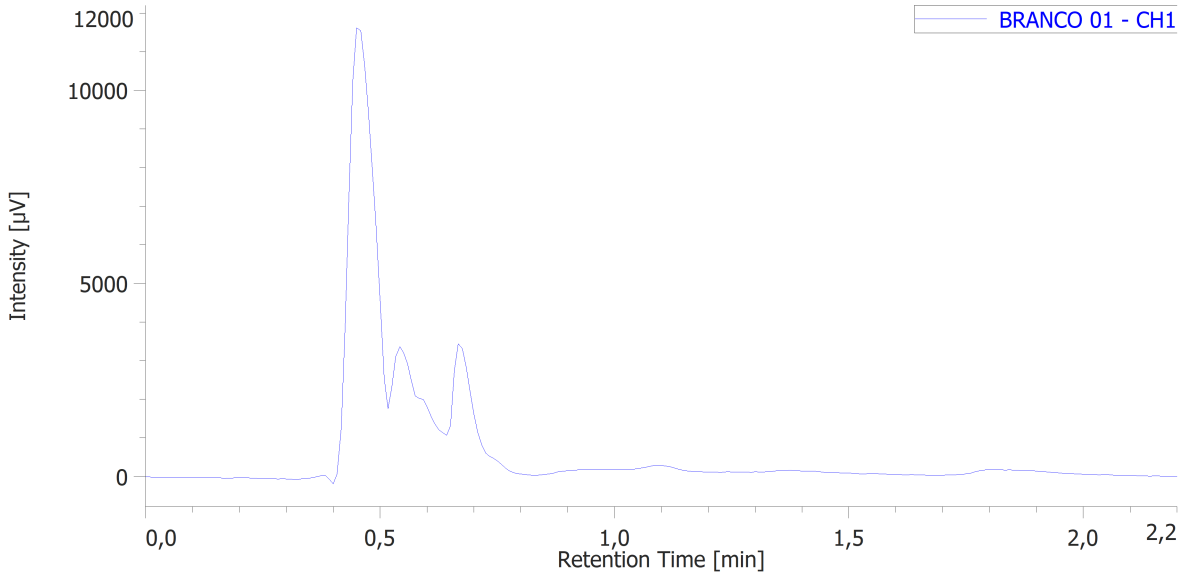


Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:18
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:21:15
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

Creator QPackSA
Reviewer
Approver

Chromatogram

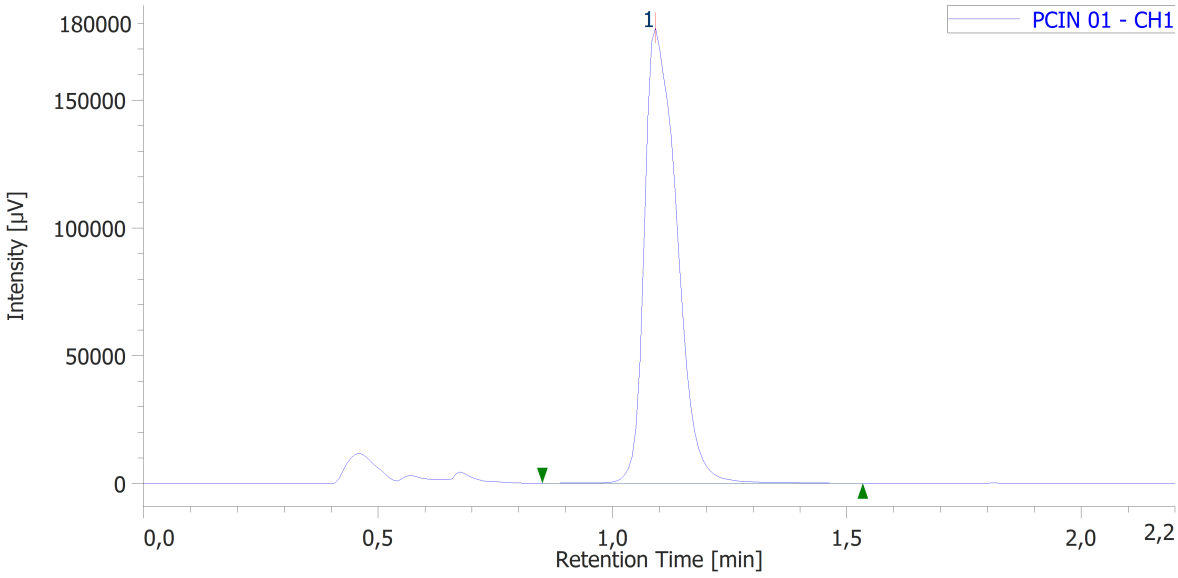

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:18
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:25:31
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,092	856835	178005	100,000	100,000	N/A	1148	N/A	1,465	

Creator QPackSA
Reviewer
Approver

Chromatogram

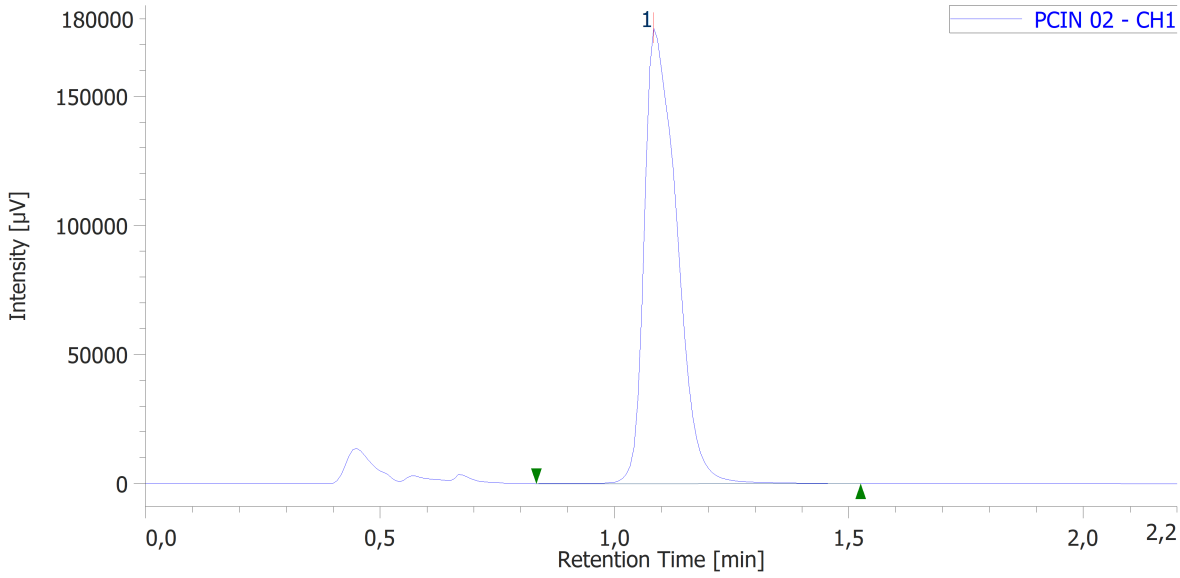

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:18
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:29:48
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	847279	176413	100,000	100,000	N/A	1114	N/A	1,618	

Creator QPackSA
Reviewer
Approver

Chromatogram

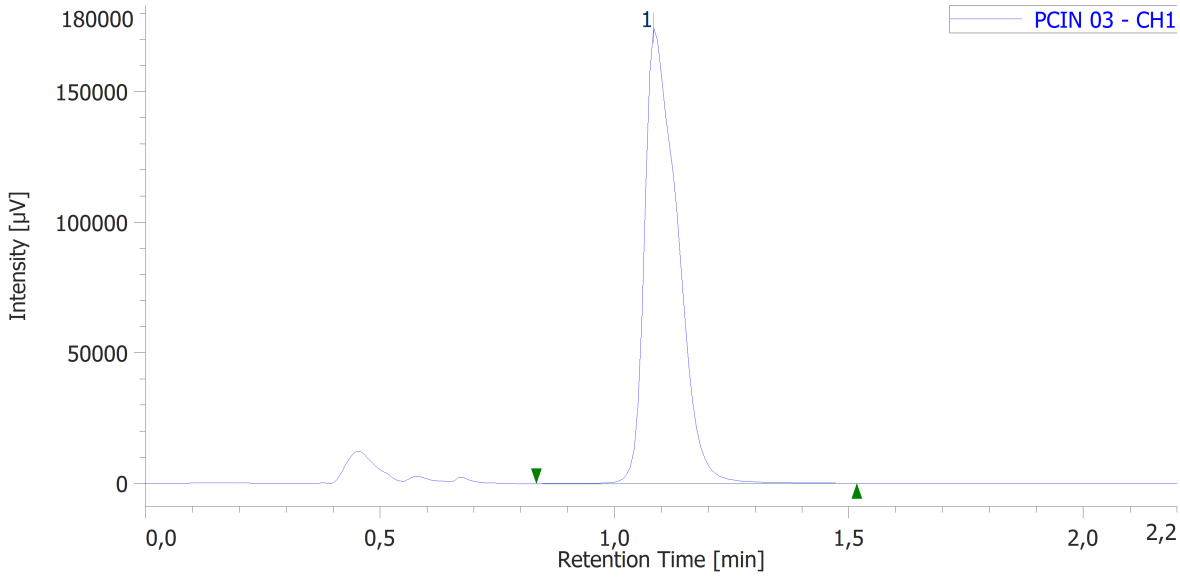

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:18
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:34:03
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	843886	174344	100,000	100,000	N/A	1066	N/A	1,685	

Creator QPackSA
Reviewer
Approver

Chromatogram

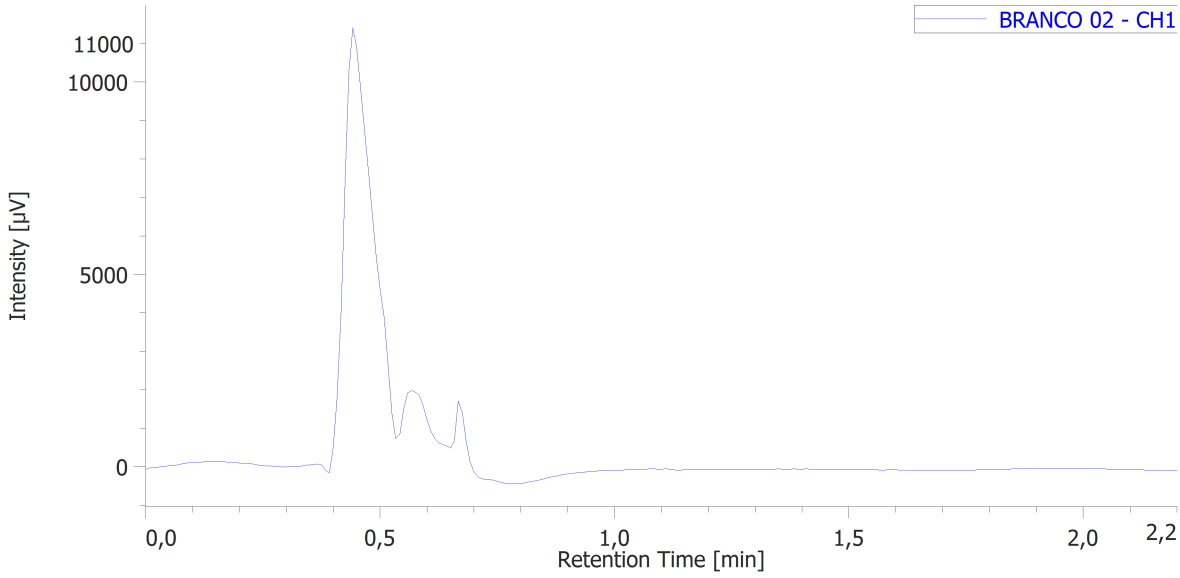


Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:18
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:38:19
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

Creator QPackSA
Reviewer
Approver

Chromatogram

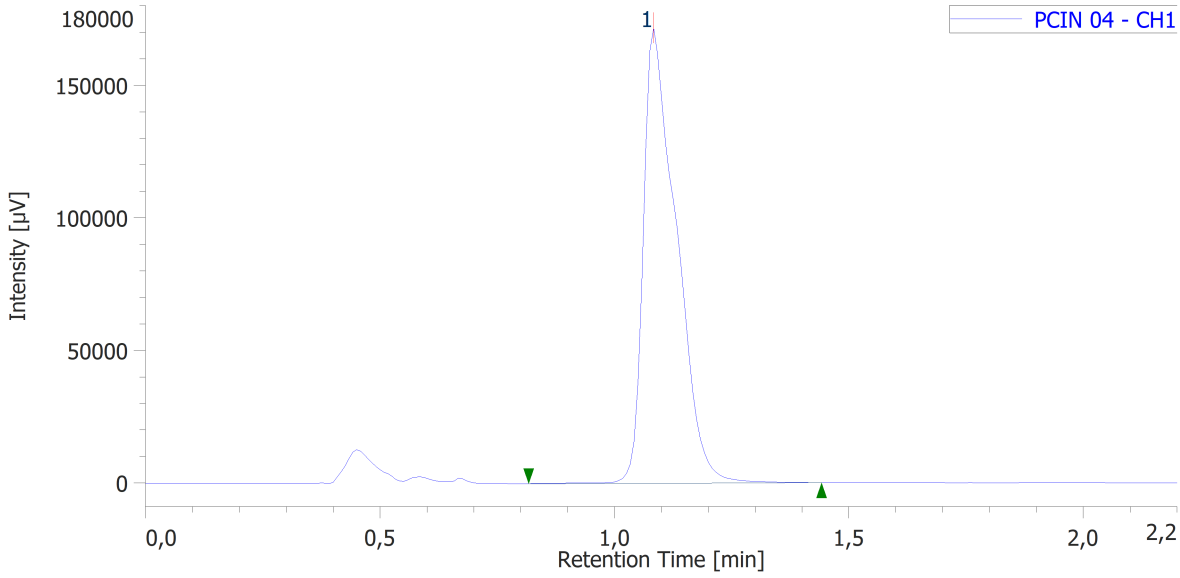

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:19
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:42:36
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	841526	171634	100,000	100,000	N/A	1012	N/A	1,678	

Creator QPackSA
Reviewer
Approver

Chromatogram

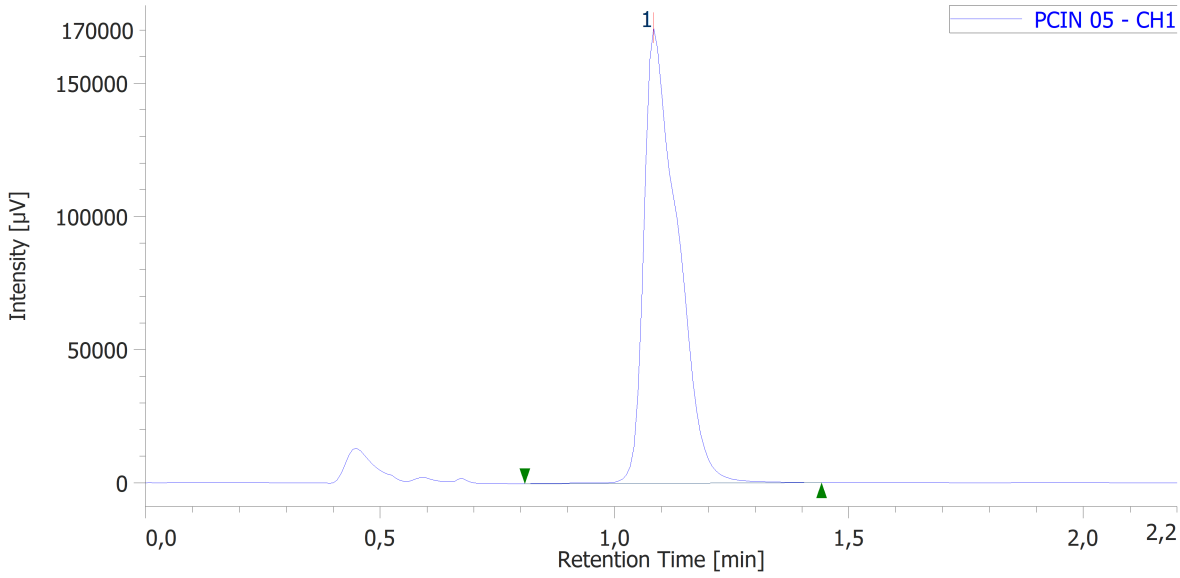

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:19
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:46:51
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	847763	170795	100,000	100,000	N/A	967	N/A	1,736	

Creator QPackSA
Reviewer
Approver

Chromatogram

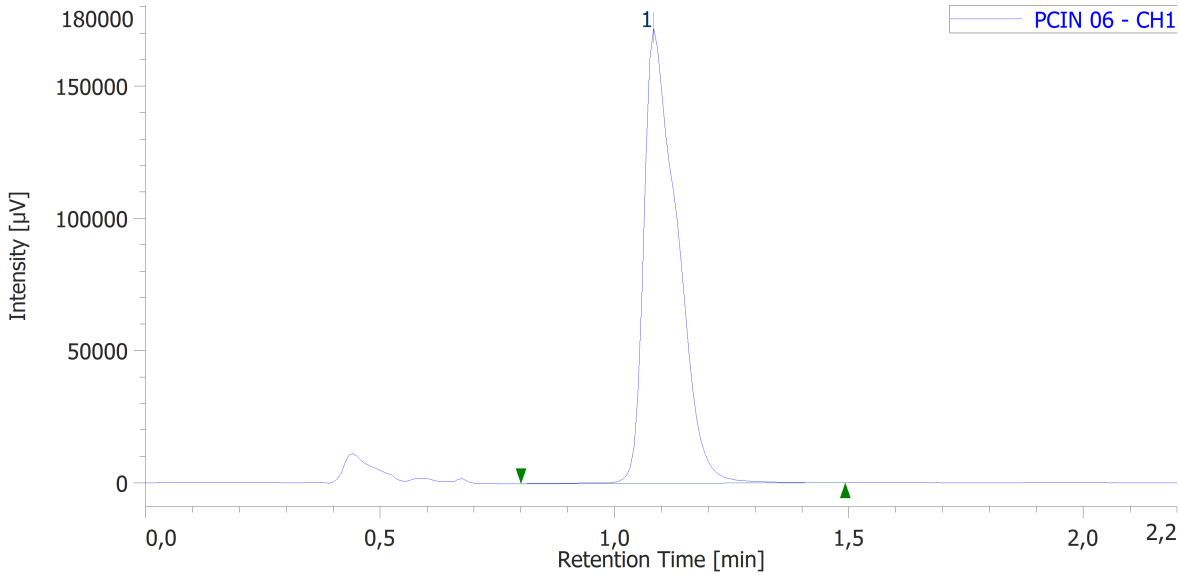

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:19
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:51:07
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	846491	172108	100,000	100,000	N/A	1005	N/A	1,718	

Creator QPackSA
Reviewer
Approver

Chromatogram

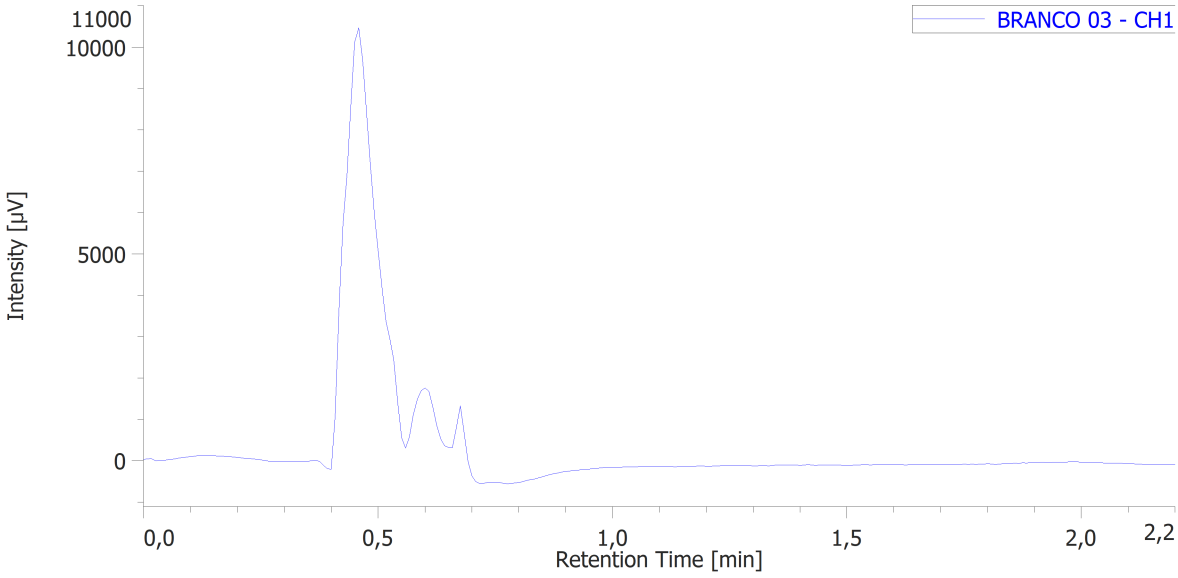


Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 13:19:19
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 12:55:22
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

Creator QPackSA
Reviewer
Approver

Chromatogram

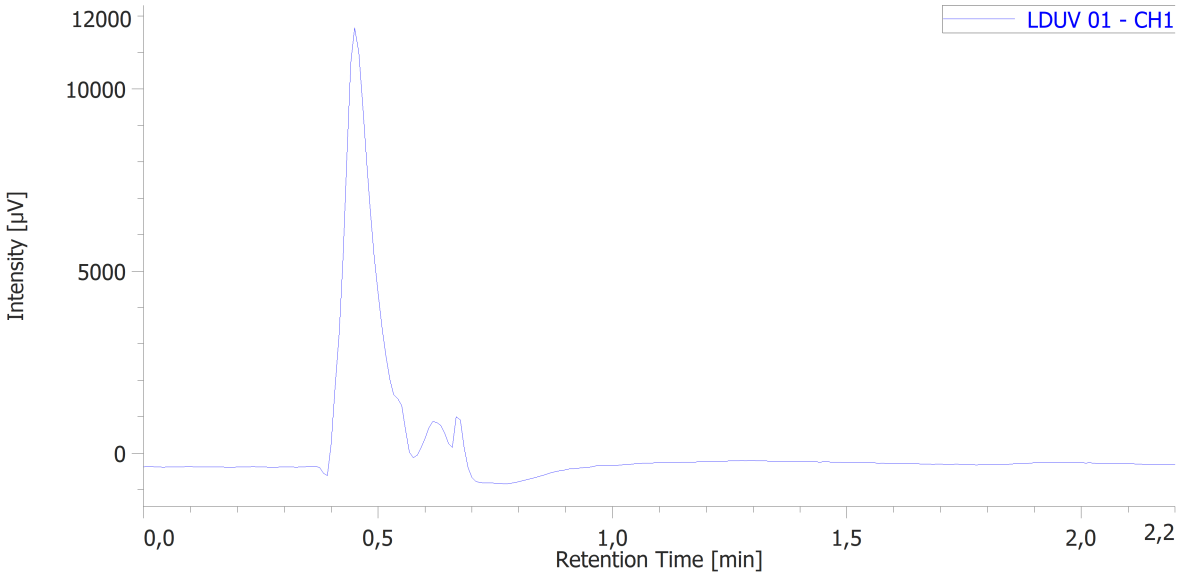


Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 15:31:41
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:05:01
Volume	10,0 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

Creator QPackSA
Reviewer
Approver

Chromatogram

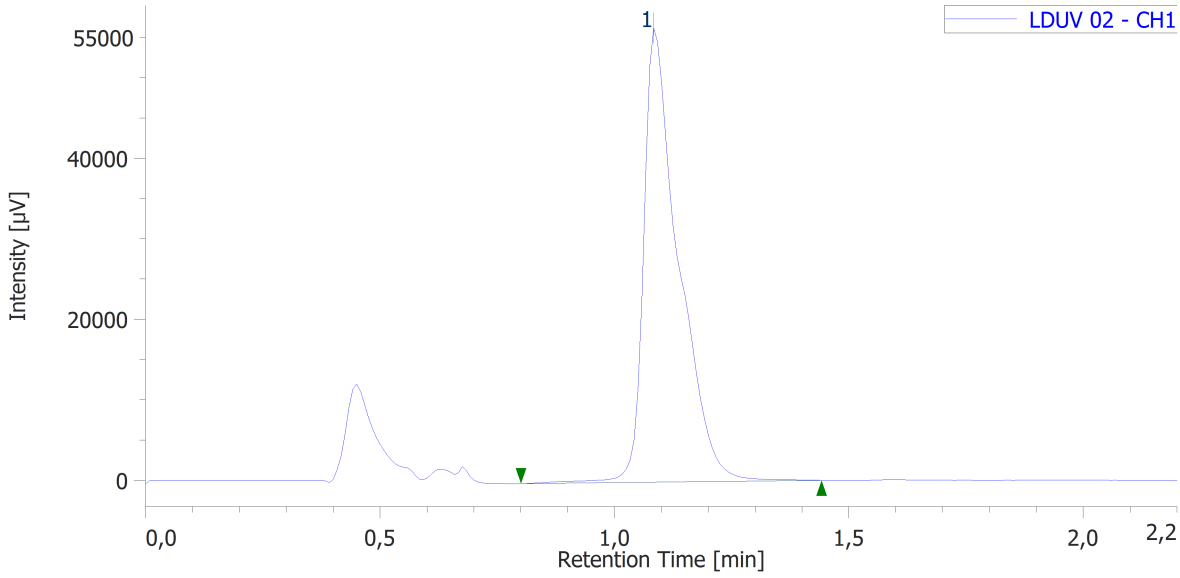

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 15:31:43
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:09:19
Volume	10,0 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	291200	56345	100,000	100,000	N/A	1253	N/A	1,848	

Creator QPackSA
Reviewer
Approver

Chromatogram

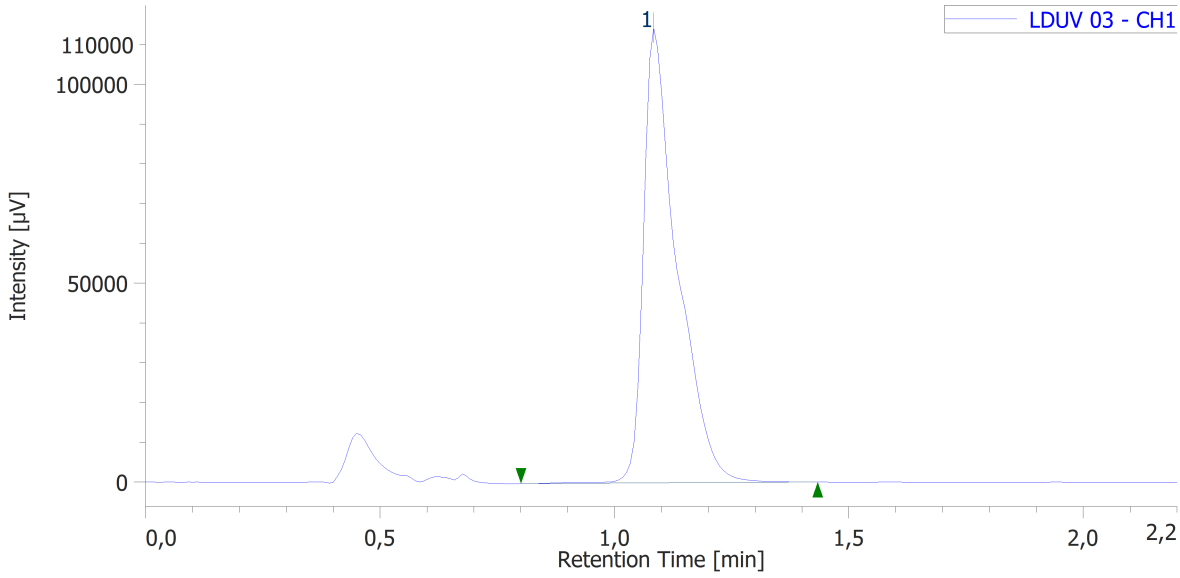

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 15:31:43
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:13:39
Volume	10,0 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	570183	114307	100,000	100,000	N/A	1369	N/A	1,860	

Creator QPackSA
Reviewer
Approver

Chromatogram

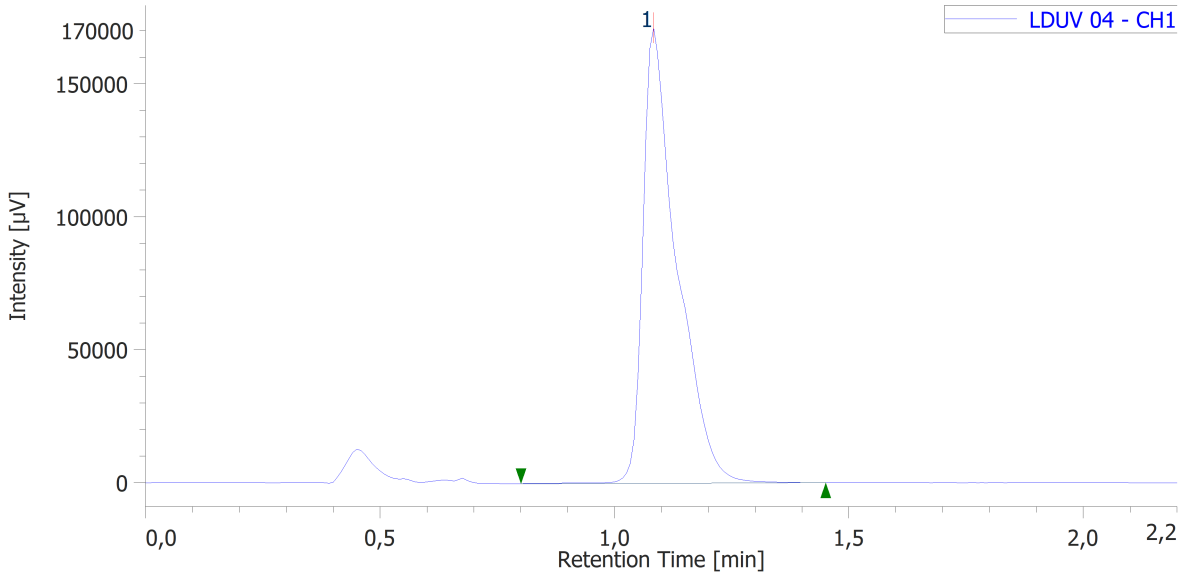

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 15:31:43
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:17:56
Volume	10,0 [µL]
Sample #	7
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	859112	171080	100,000	100,000	N/A	1334	N/A	1,851	

Creator QPackSA
Reviewer
Approver

Chromatogram

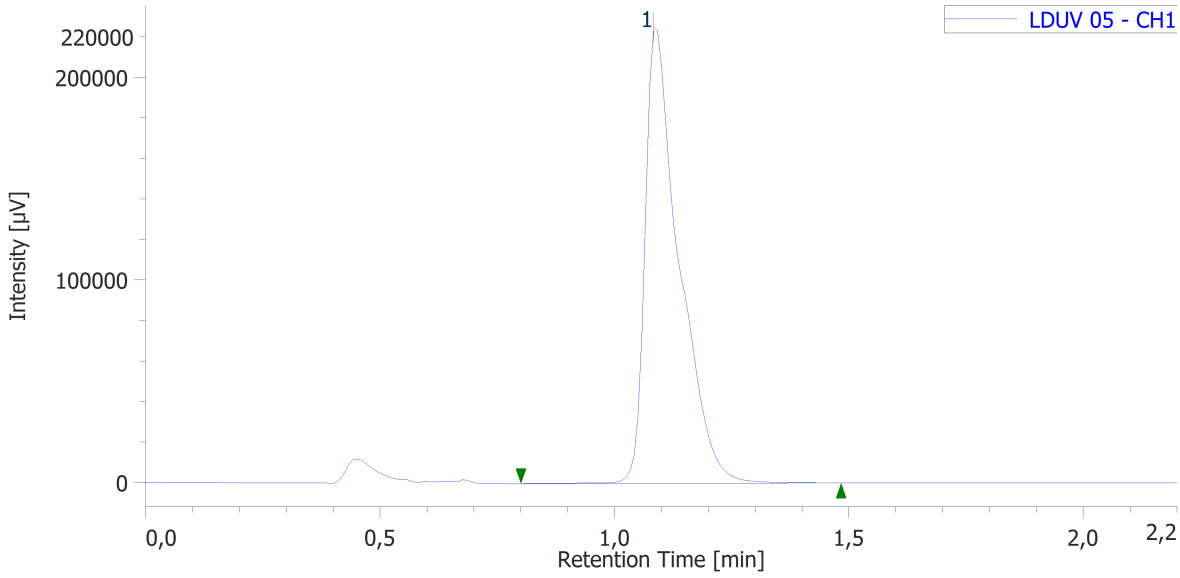

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 15:31:43
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:22:16
Volume	10,0 [µL]
Sample #	8
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	1133781	224595	100,000	100,000	N/A	1283	N/A	2,029	

Creator QPackSA
Reviewer
Approver

Chromatogram

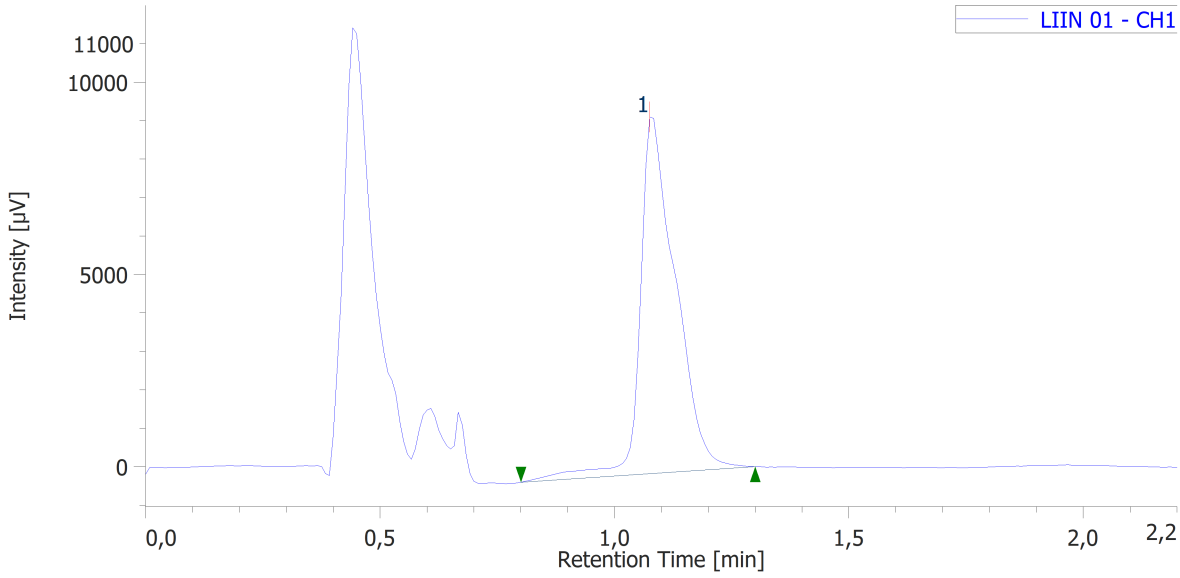

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 14:21:40
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 13:52:11
Volume	0,1 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,075	48776	9259	100,000	100,000	N/A	964	N/A	1,781	

Creator QPackSA
Reviewer
Approver

Chromatogram

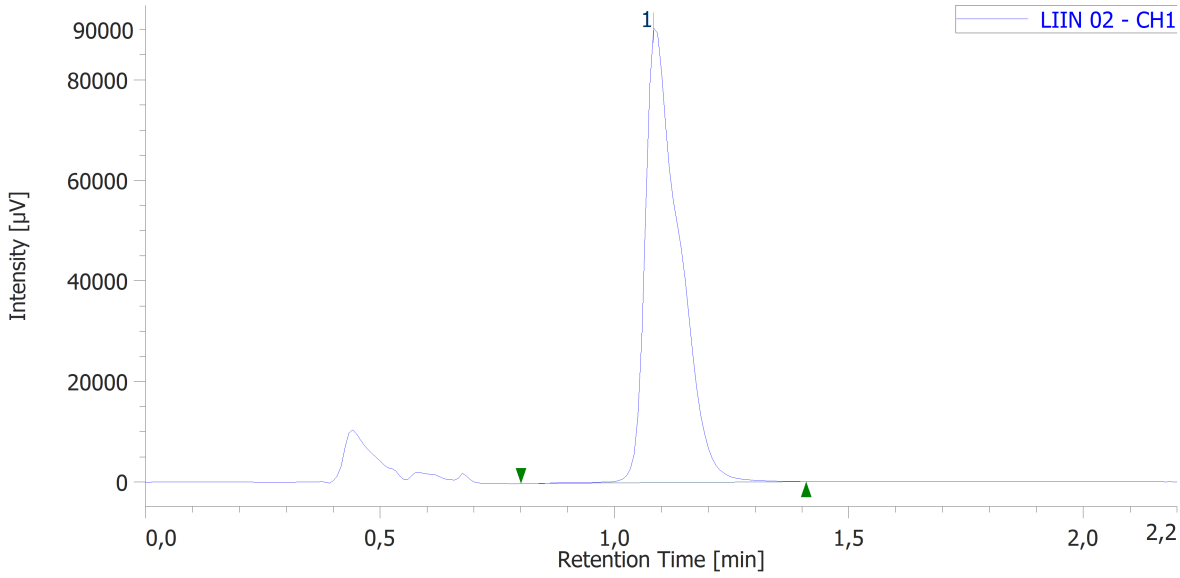

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 14:21:44
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 13:56:23
Volume	5,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	454834	90414	100,000	100,000	N/A	996	N/A	1,905	

Creator QPackSA
Reviewer
Approver

Chromatogram

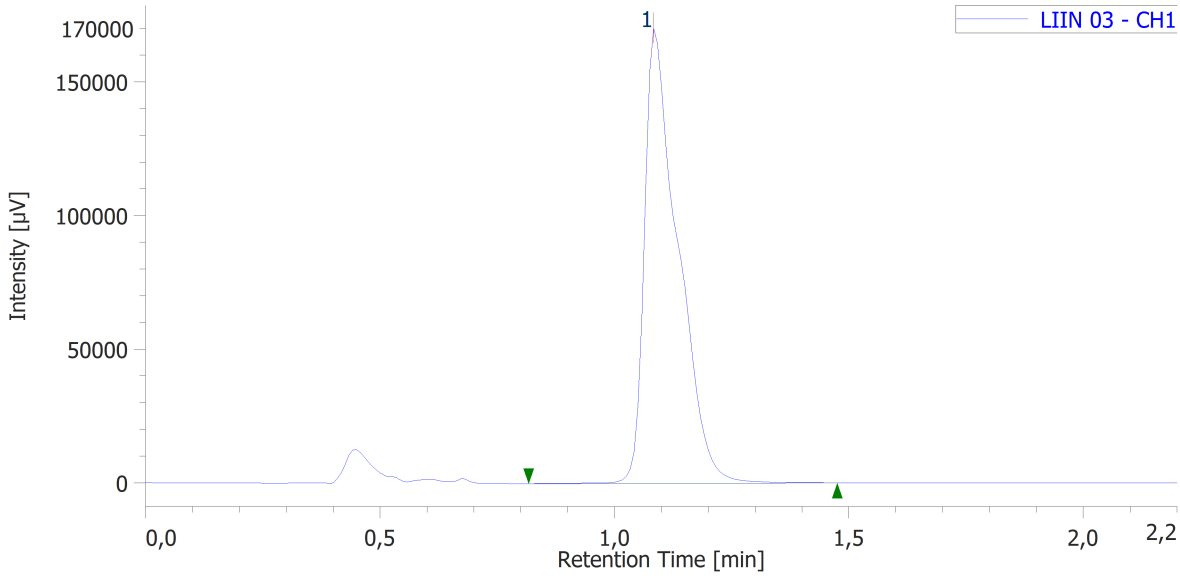

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 14:21:45
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 14:00:43
Volume	10,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	843100	170252	100,000	100,000	N/A	1058	N/A	1,857	

Creator QPackSA
Reviewer
Approver

Chromatogram

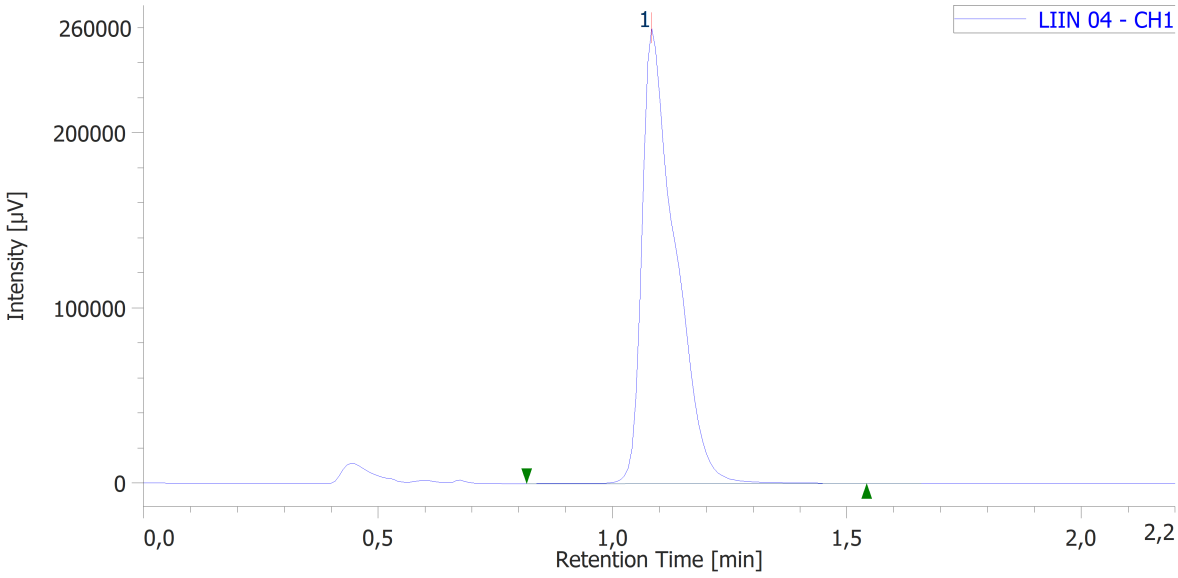

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 14:21:45
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 14:05:08
Volume	15,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	1274464	260114	100,000	100,000	N/A	1100	N/A	1,809	

Creator QPackSA
Reviewer
Approver

Chromatogram

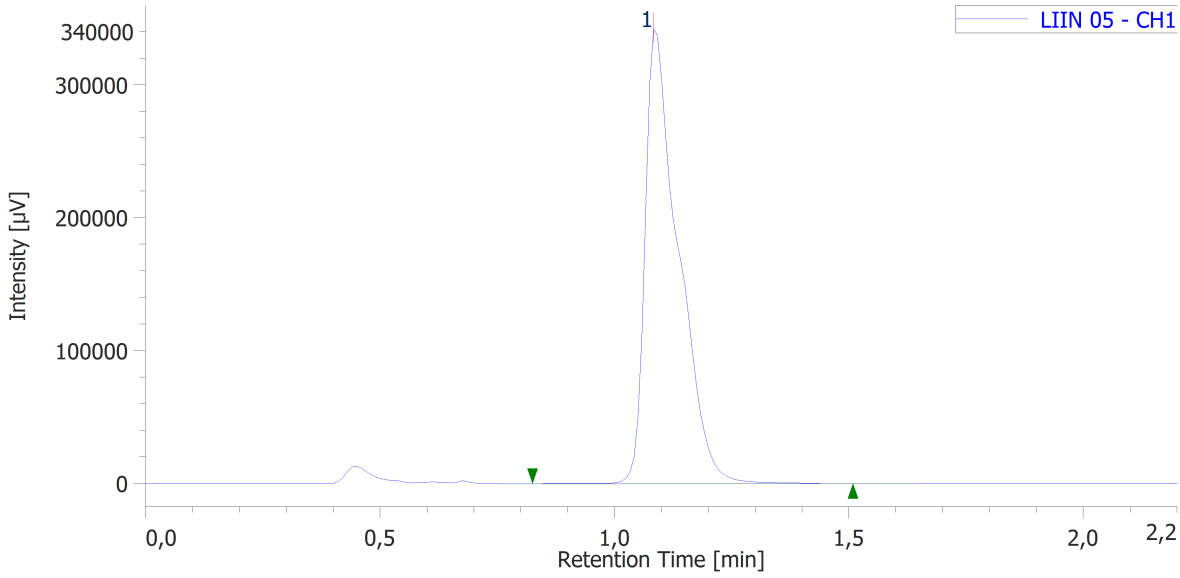

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 14:21:45
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 14:09:40
Volume	20,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,2 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,083	1688576	342755	100,000	100,000	N/A	1119	N/A	1,944	

Creator QPackSA
Reviewer
Approver

Chromatogram

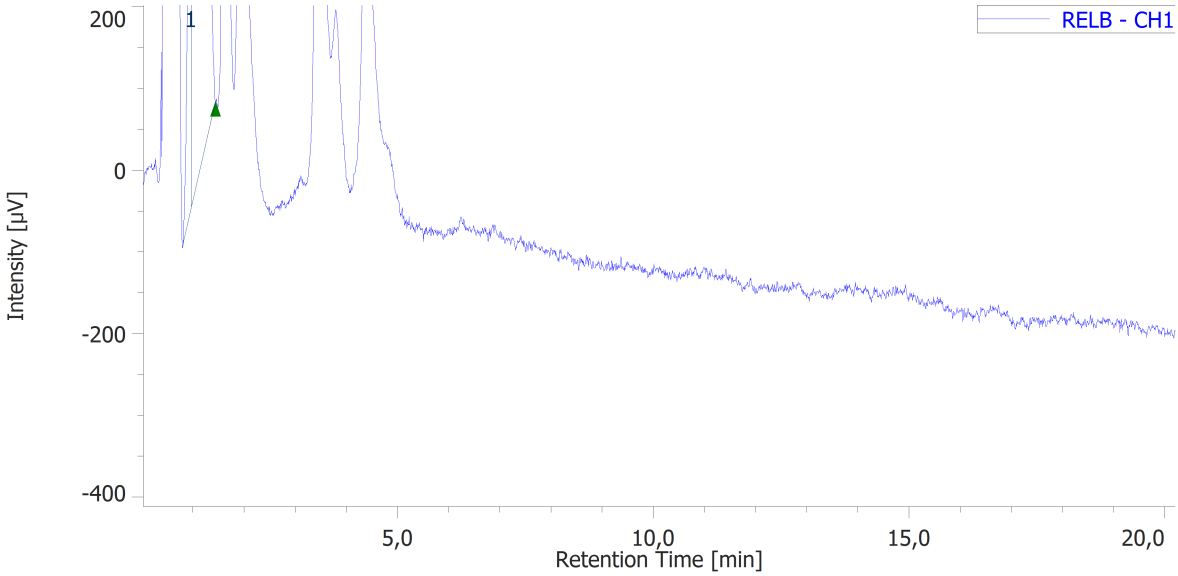

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 16:02:44
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:42:29
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,2 [min]
Acquisition Sequence	RELB
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,092	853296	171158	100,000	100,000	N/A	1494	N/A	1,762	

Creator
Reviewer
Approver

Chromatogram

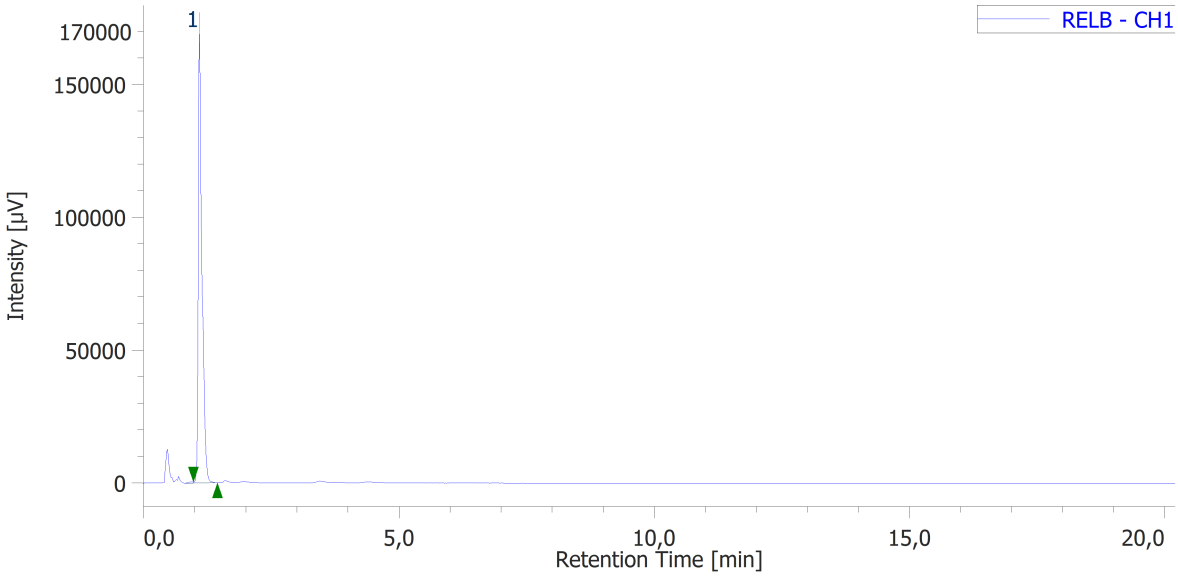

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 16:02:44
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:42:29
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,2 [min]
Acquisition Sequence	RELB
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,092	853296	171158	100,000	100,000	N/A	1494	N/A	1,762	

Creator
Reviewer
Approver

Chromatogram

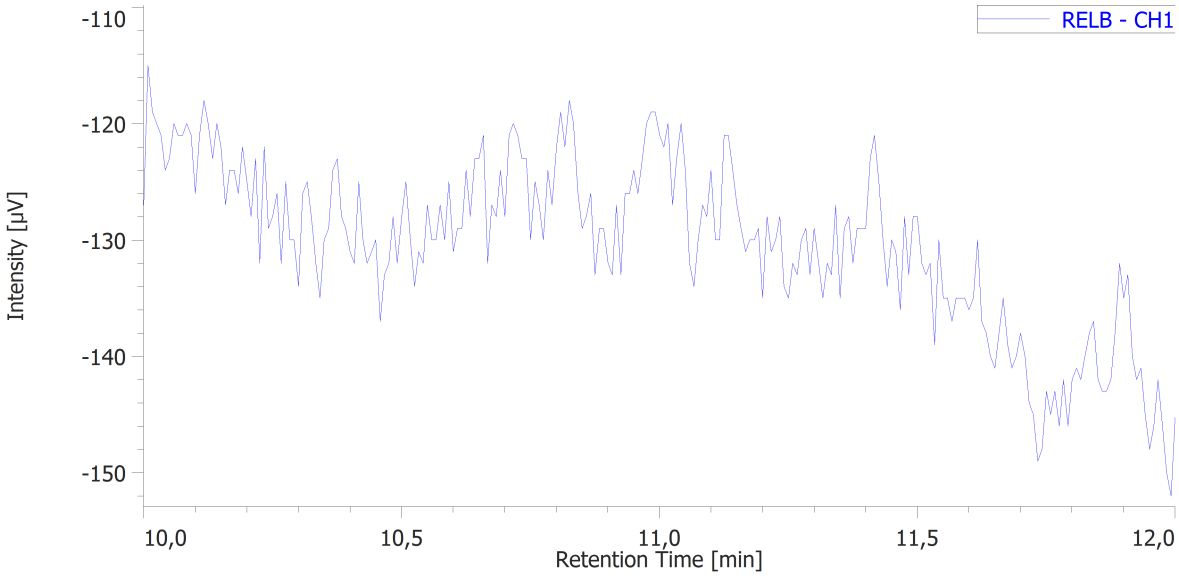

Chromatogram Information	
User Name	QPackSA
Date Modified	11/02/2025 16:02:44
Description	
HPLC System Name	HPLC-0001
Injection Date	11/02/2025 15:42:29
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,2 [min]
Acquisition Sequence	RELB
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína 2025

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,092	853296	171158	100,000	100,000	N/A	1494	N/A	1,762	

Creator
Reviewer
Approver

Chromatogram

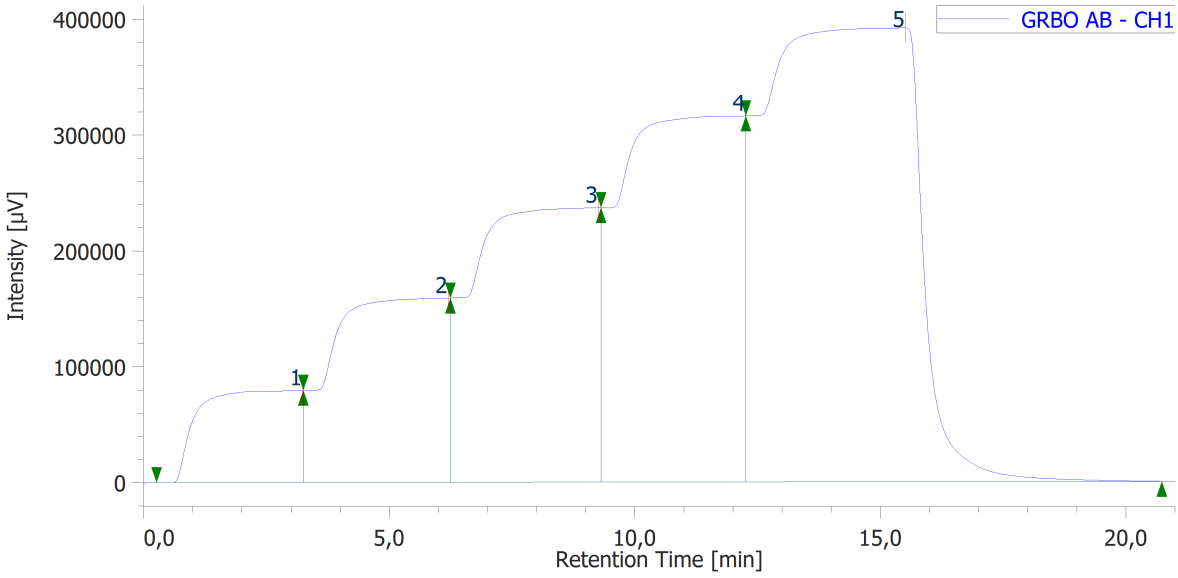

Chromatogram Information

User Name	QPackSA
Date Modified	13/02/2025 11:48:05
Description	
HPLC System Name	HPLC-0001
Injection Date	13/02/2025 11:05:49
Volume	0,1 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	21,0 [min]
Acquisition Sequence	GRBO
Control Method	GRBO AB 2025
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRBO AB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	3,233	10783970	79523	5,063	6,730	N/A	N/A	N/A	N/A	
2	Unknown	1	6,200	25129047	158726	11,799	13,434	N/A	N/A	N/A	N/A	
3	Unknown	1	9,258	40140326	236536	18,847	20,019	N/A	N/A	N/A	N/A	
4	Unknown	1	12,250	52788255	315564	24,786	26,707	N/A	N/A	N/A	N/A	
5	Unknown	1	15,508	84135930	391210	39,505	33,110	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

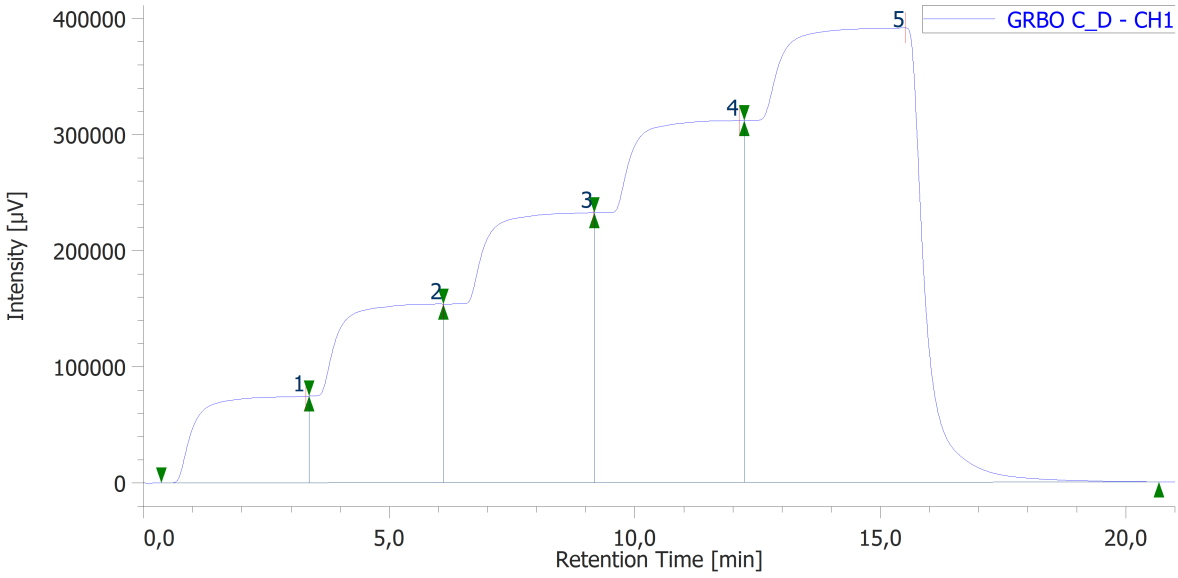

Chromatogram Information

User Name	QPackSA
Date Modified	13/02/2025 12:38:56
Description	
HPLC System Name	HPLC-0001
Injection Date	13/02/2025 11:28:40
Volume	0,1 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	21,0 [min]
Acquisition Sequence	GRBO
Control Method	GRBO CD 2025
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRBO C_D-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	3,300	10485973	74476	5,006	6,405	N/A	N/A	N/A	N/A	
2	Unknown	1	6,092	22485752	153744	10,735	13,221	N/A	N/A	N/A	N/A	
3	Unknown	1	9,158	38814170	232308	18,531	19,977	N/A	N/A	N/A	N/A	
4	Unknown	1	12,125	53328493	311406	25,460	26,779	N/A	N/A	N/A	N/A	
5	Unknown	1	15,508	84342995	390931	40,267	33,618	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver