
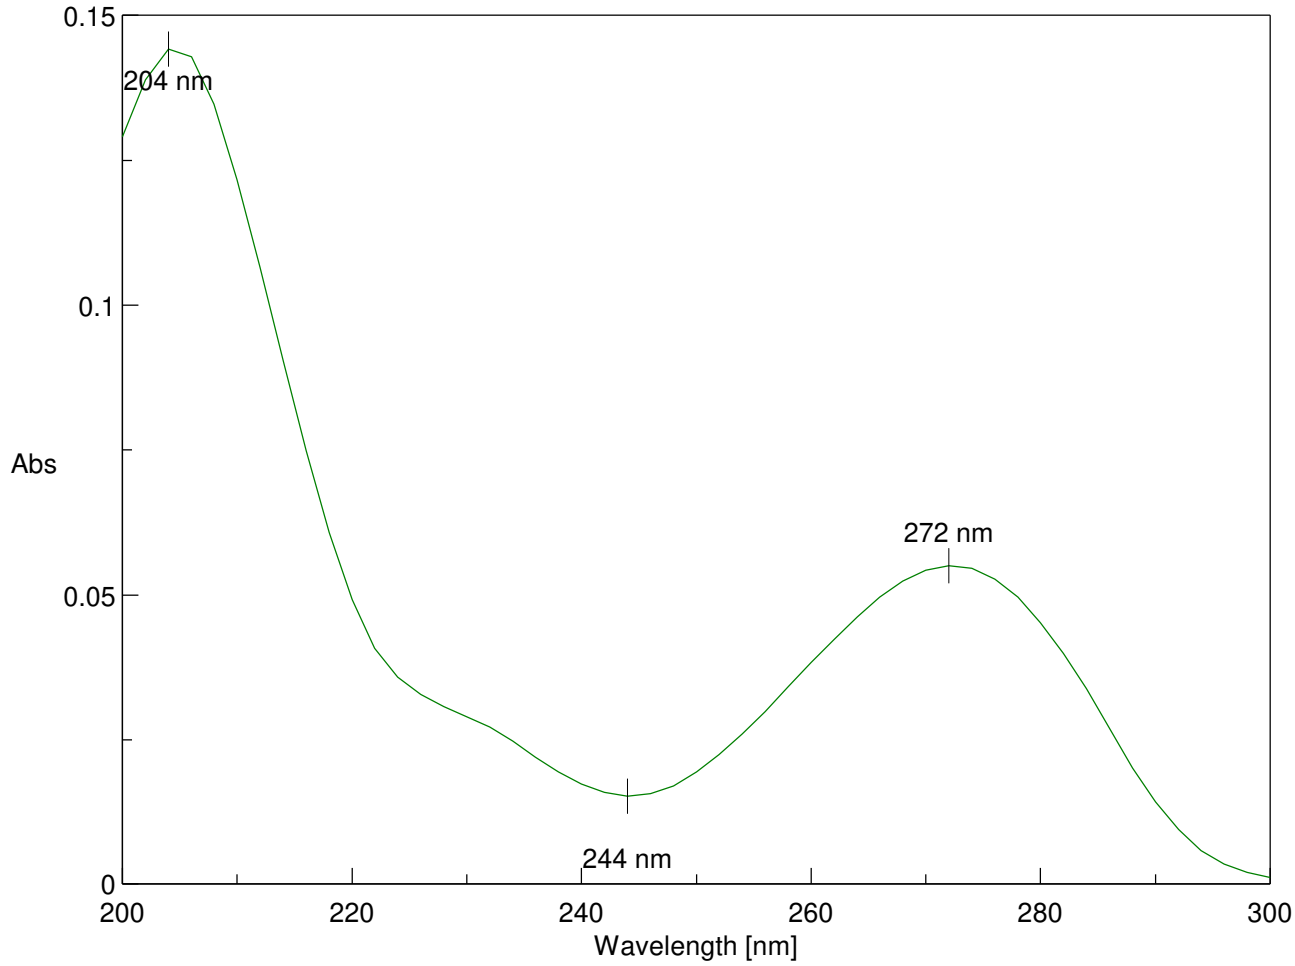


[Comments]	
User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	22/02/2024 10:50

[Measurement Information]	
Model Name	MD-4010
Serial No.	A000661665
ROM version	V1.02.02

[Detailed Information]	
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	2 nm
Data points	51

Chromatogram

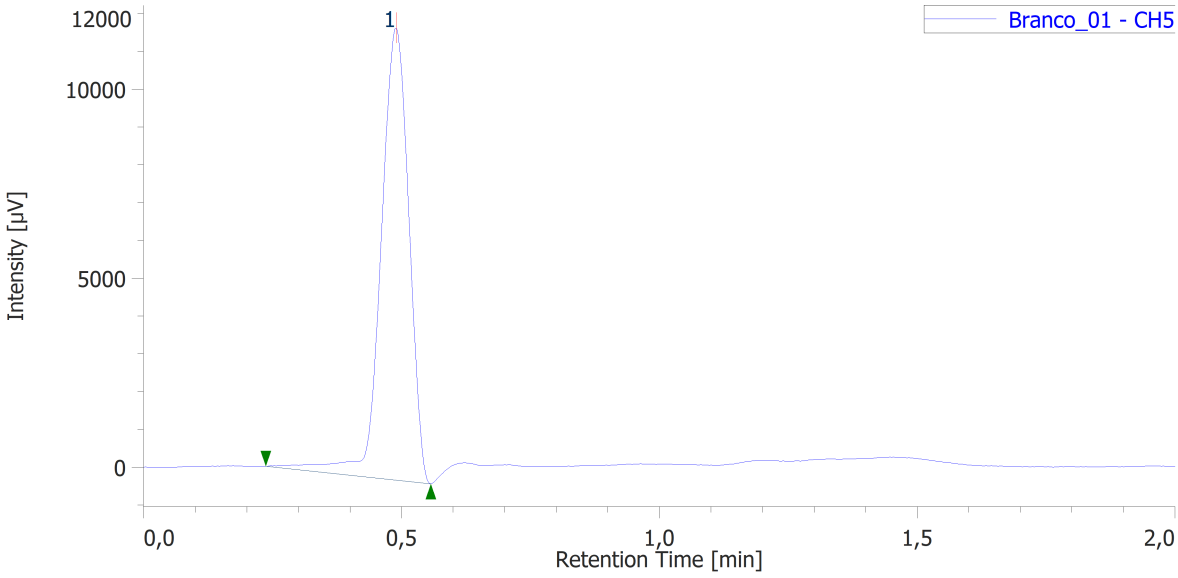

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:24:25
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:22:22
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	Branco_01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,490	45383	11957	100,000	100,000	N/A	393	N/A	0,932	

Creator
Reviewer
Approver

Chromatogram

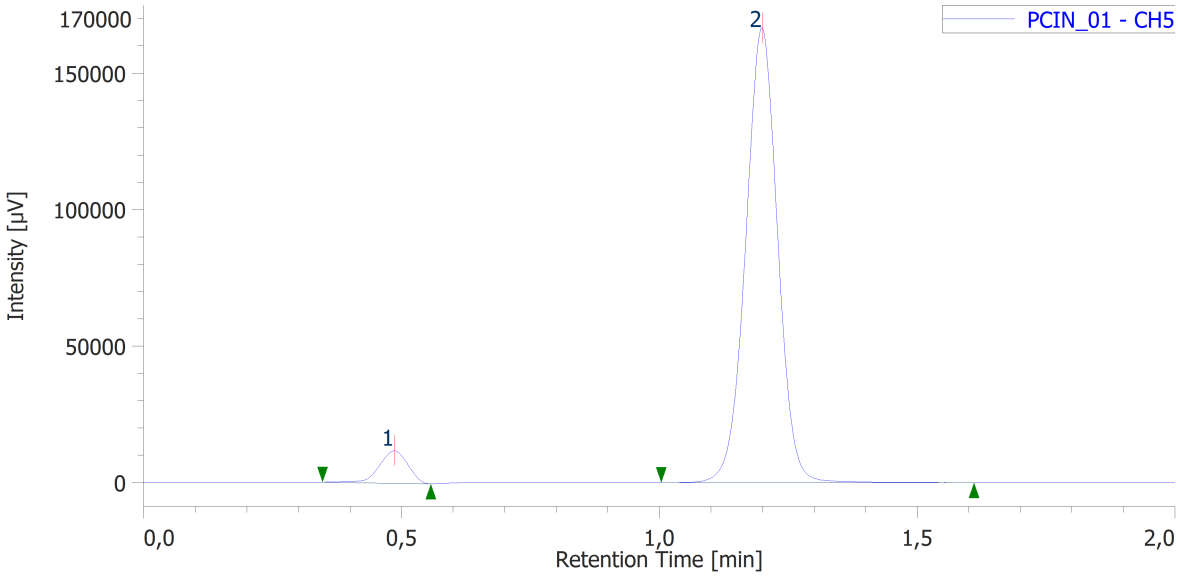

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:27:03
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:25:01
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	PCIN_01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	45592	11933	5,980	6,687	N/A	368	6,713	0,884	
2	Cafeína	5	1,200	716798	166501	94,020	93,313	N/A	1852	N/A	0,971	

Creator
Reviewer
Approver

Chromatogram

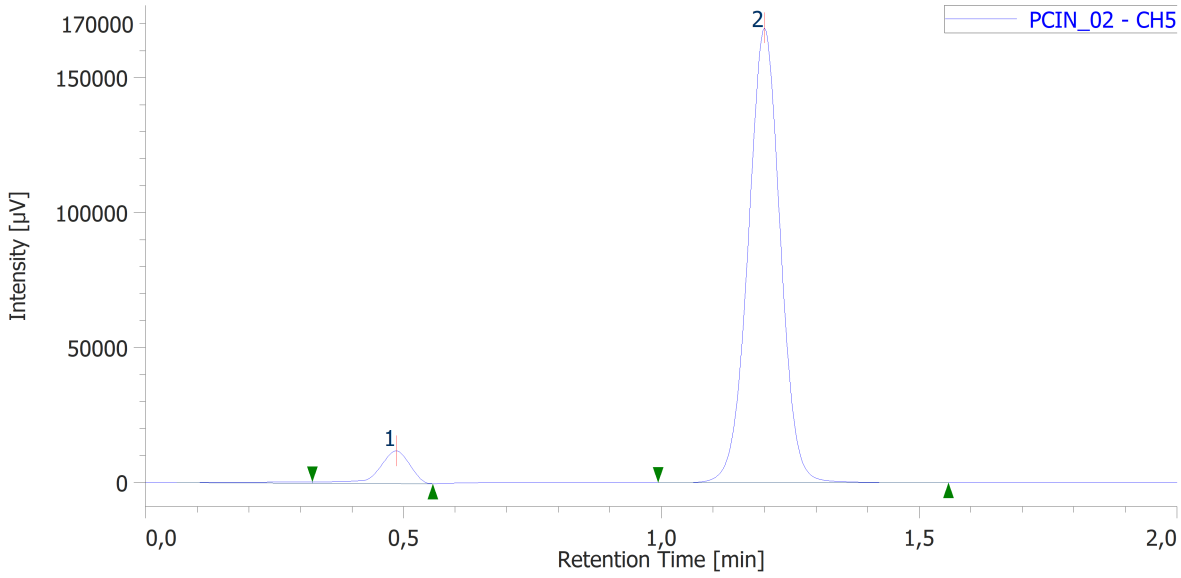

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:29:43
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:27:41
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	PCIN_02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	50222	12138	6,458	6,723	N/A	353	6,635	0,731	
2	Cafeína	5	1,200	727416	168405	93,542	93,277	N/A	1835	N/A	0,992	

Creator
Reviewer
Approver

Chromatogram

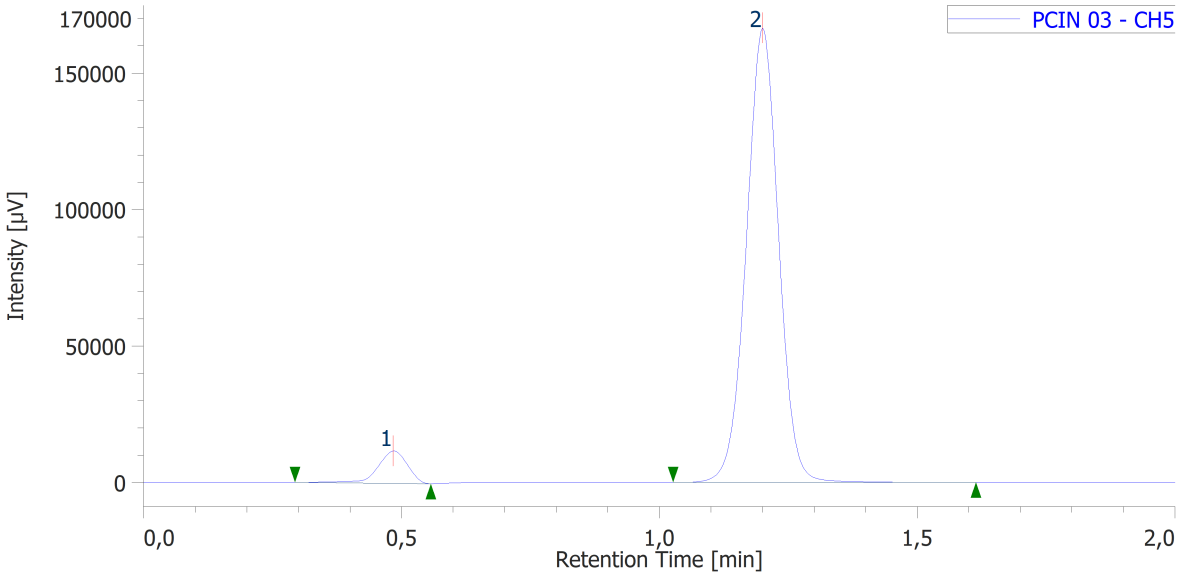

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:32:23
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:30:21
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	PCIN 03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	47065	11900	6,123	6,675	N/A	352	6,670	0,855	
2	Cafeína	5	1,200	721609	166388	93,877	93,325	N/A	1821	N/A	0,996	

Creator
Reviewer
Approver

Chromatogram

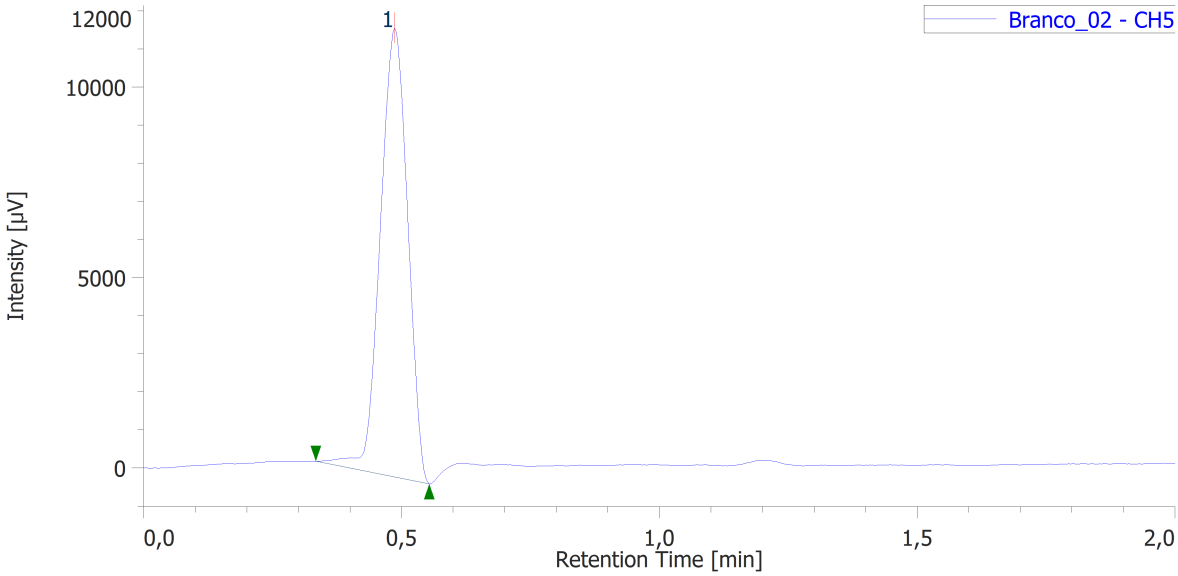

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:35:03
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:33:01
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_02-CH5
Sample Name	Branco_02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	43569	11776	100,000	100,000	N/A	382	N/A	0,962	

Creator
Reviewer
Approver

Chromatogram

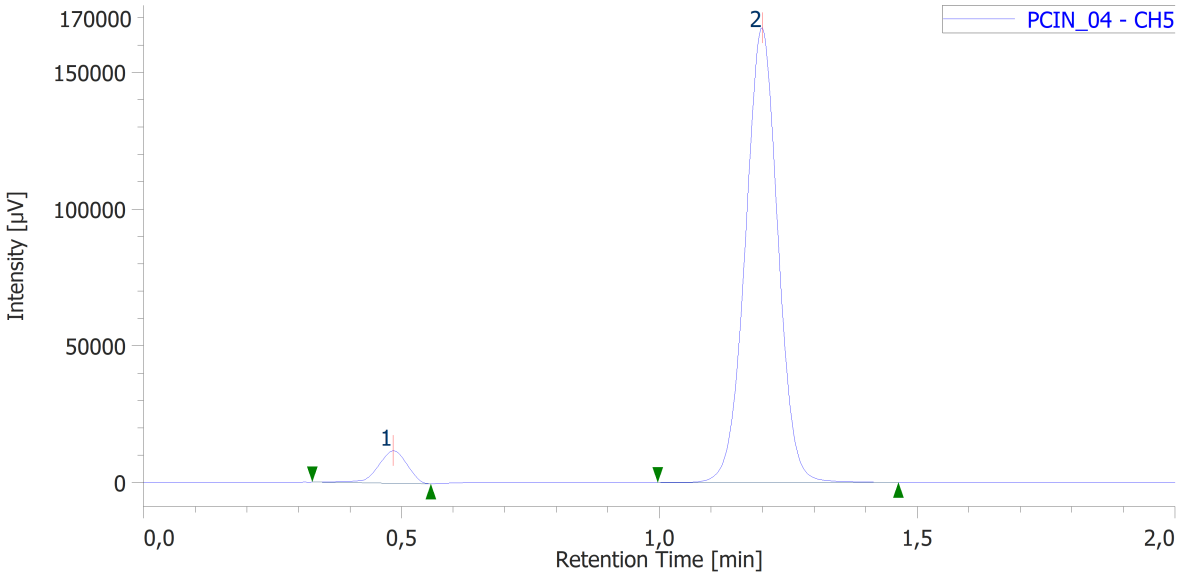

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:37:45
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:35:41
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	PCIN_04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	46432	11902	6,005	6,685	N/A	352	6,632	0,874	
2	Cafeína	5	1,200	726725	166140	93,995	93,315	N/A	1782	N/A	0,977	

Creator
Reviewer
Approver

Chromatogram

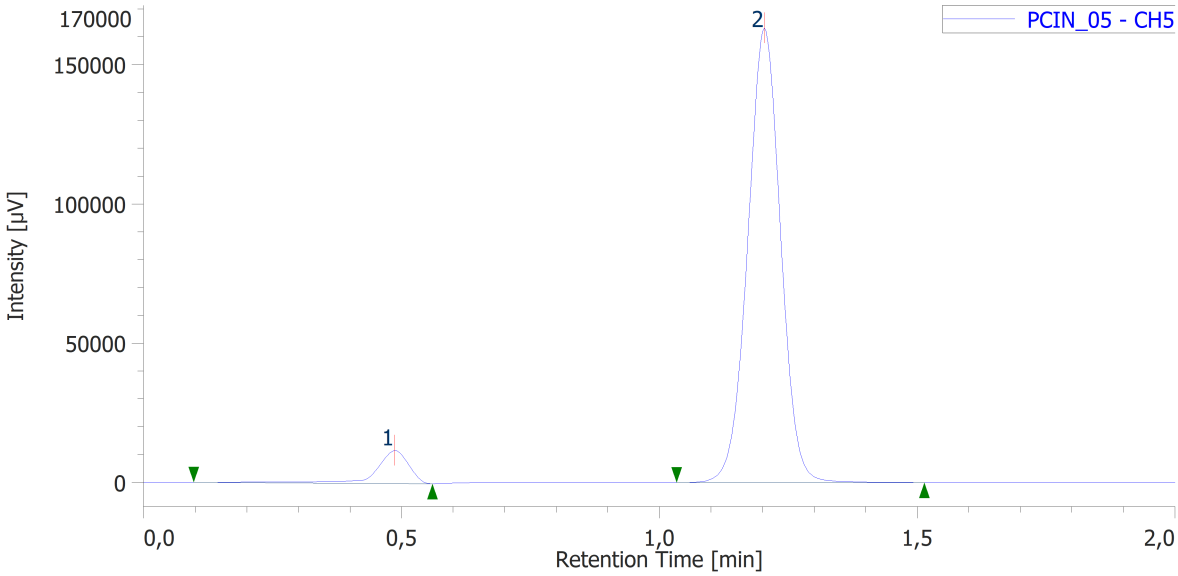

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:40:21
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:38:20
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	PCIN_05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	52851	11899	6,827	6,799	N/A	348	6,549	0,745	
2	Cafeína	5	1,203	721282	163112	93,173	93,201	N/A	1749	N/A	0,995	

Creator
Reviewer
Approver

Chromatogram

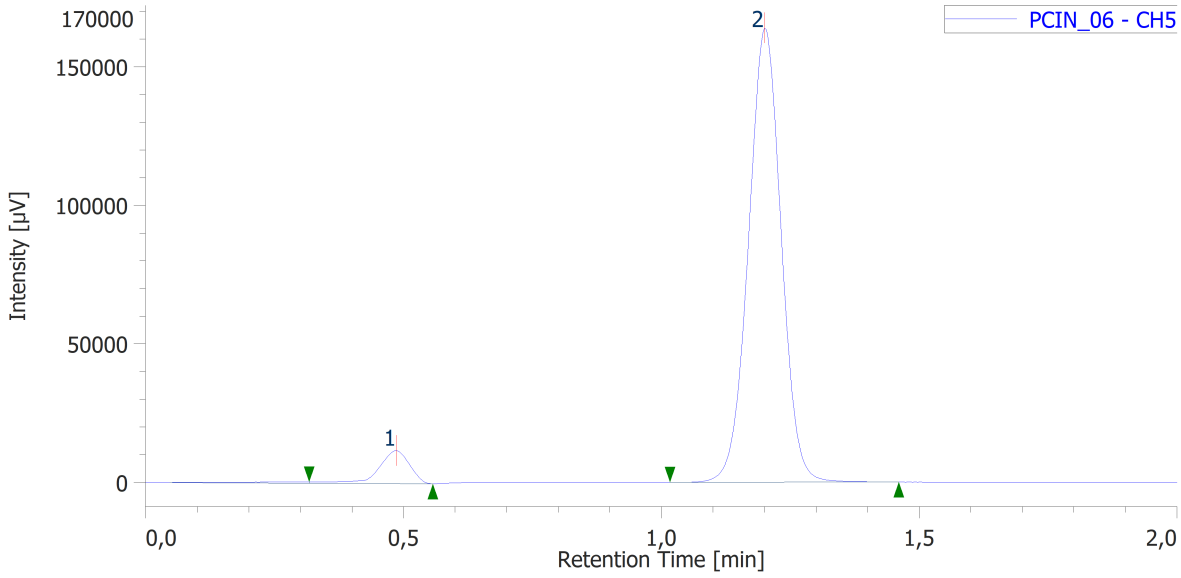

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:43:01
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:41:00
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	PCIN_06
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	49190	11926	6,375	6,784	N/A	349	6,533	0,753	
2	Cafeína	5	1,200	722389	163873	93,625	93,216	N/A	1750	N/A	1,009	

Creator
Reviewer
Approver

Chromatogram

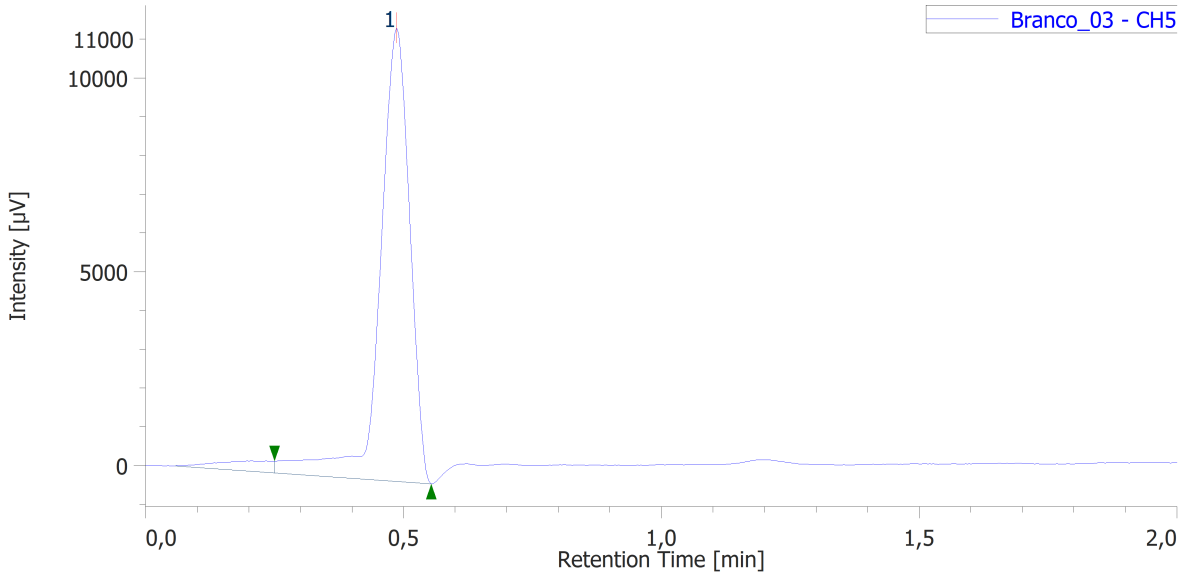

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:45:41
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:43:40
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	Branco_03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	47506	11690	100,000	100,000	N/A	374	N/A	0,898	

Creator
Reviewer
Approver

Chromatogram

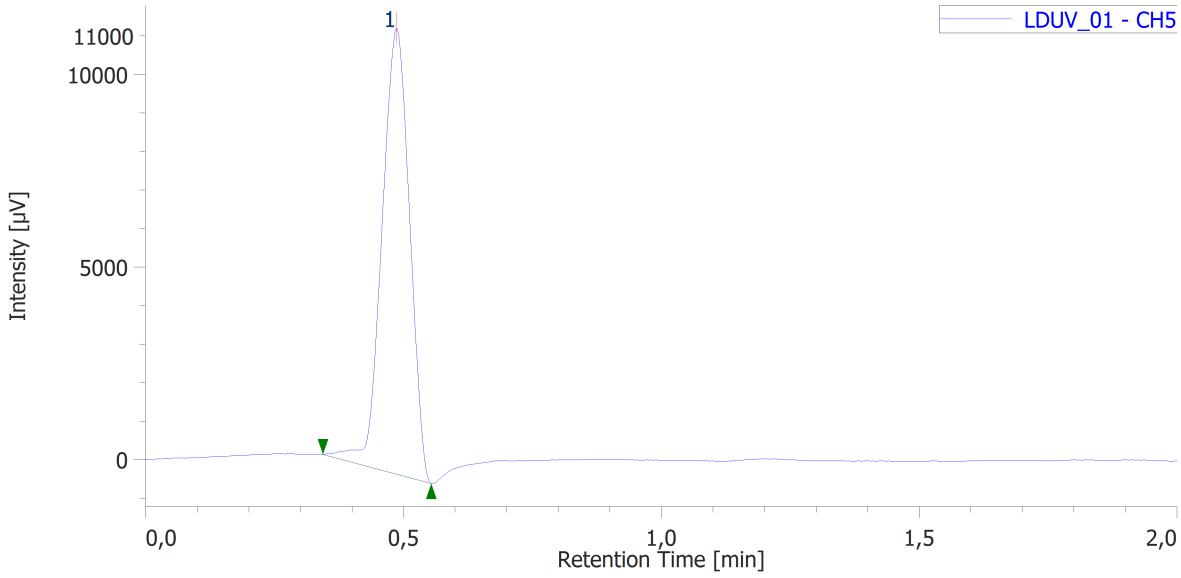

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:48:21
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:46:19
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH5
Sample Name	LDUV_01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	43210	11577	100,000	100,000	N/A	377	N/A	0,956	

Creator
Reviewer
Approver

Chromatogram

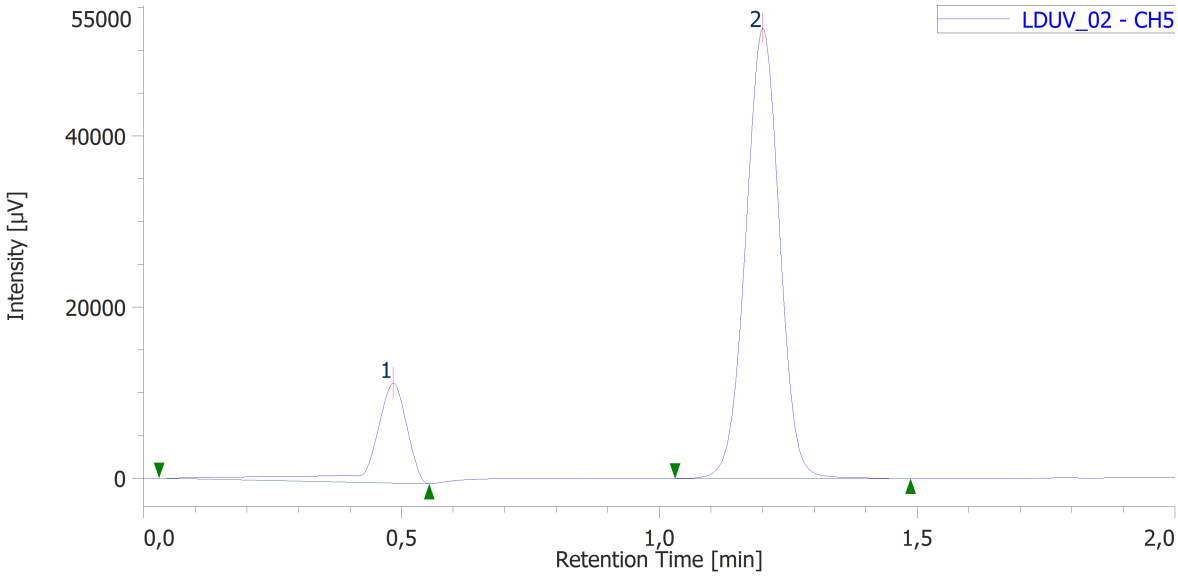

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:51:01
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:48:59
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH5
Sample Name	LDUV_02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	53210	11715	18,170	18,205	N/A	356	6,485	0,670	
2	Cafeína	5	1,200	239631	52636	81,830	81,795	N/A	1621	N/A	1,000	

Creator
Reviewer
Approver

Chromatogram

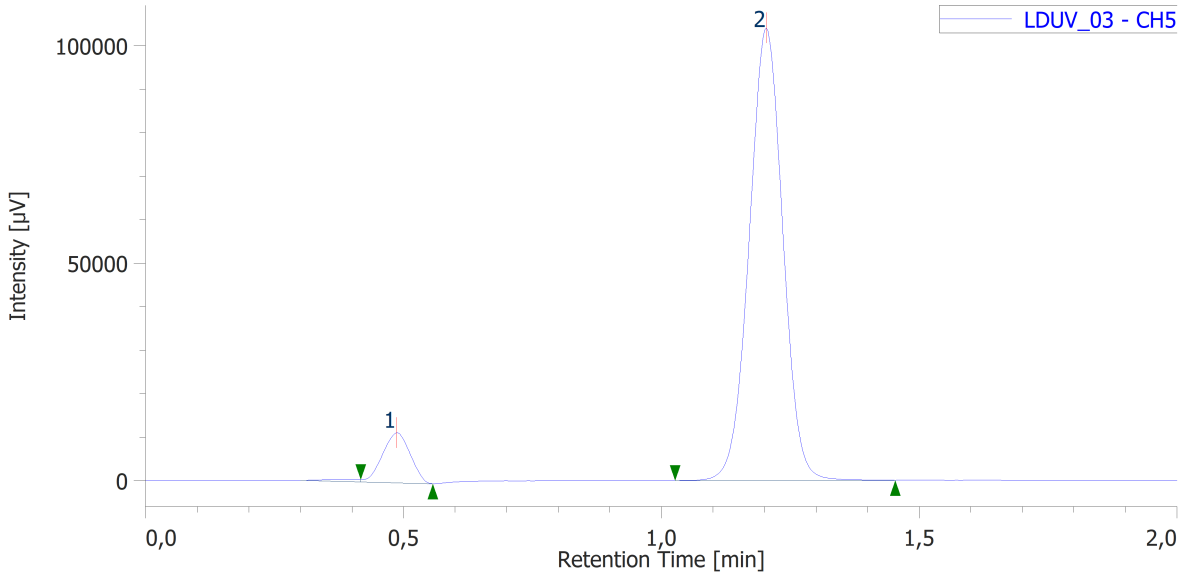

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:53:43
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:51:41
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH5
Sample Name	LDUV_03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	42767	11548	8,342	10,000	N/A	370	6,544	0,945	
2	Cafeína	5	1,203	469883	103937	91,658	90,000	N/A	1653	N/A	0,996	

Creator
Reviewer
Approver

Chromatogram

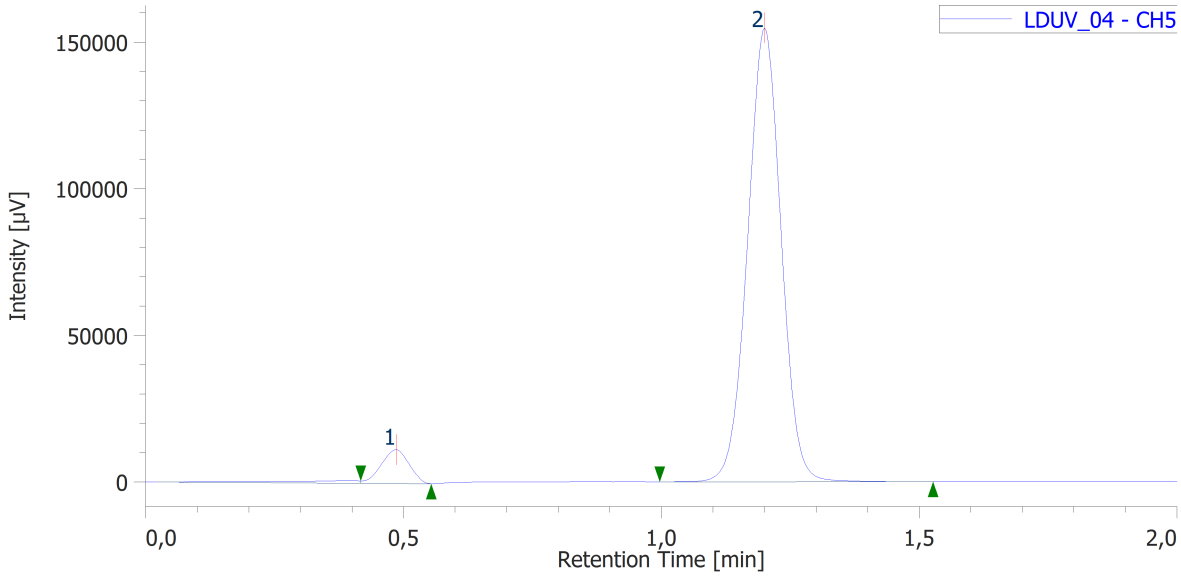

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:56:26
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:54:23
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH5
Sample Name	LDUV_04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	43302	11563	5,851	6,955	N/A	364	6,516	N/A	
2	Cafeína	5	1,200	696823	154681	94,149	93,045	N/A	1667	N/A	0,999	

Creator
Reviewer
Approver

Chromatogram

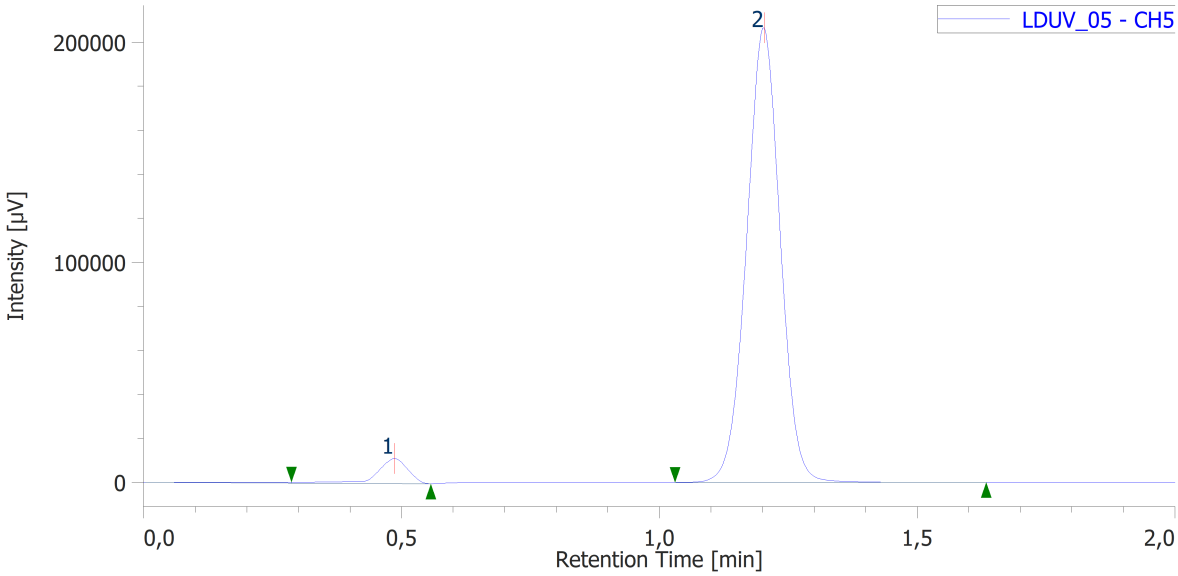

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 16:59:05
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:57:04
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH5
Sample Name	LDUV_05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	47121	11418	4,801	5,244	N/A	367	6,550	0,695	
2	Cafeína	5	1,203	934345	206319	95,199	94,756	N/A	1670	N/A	0,979	

Creator
Reviewer
Approver

Chromatogram

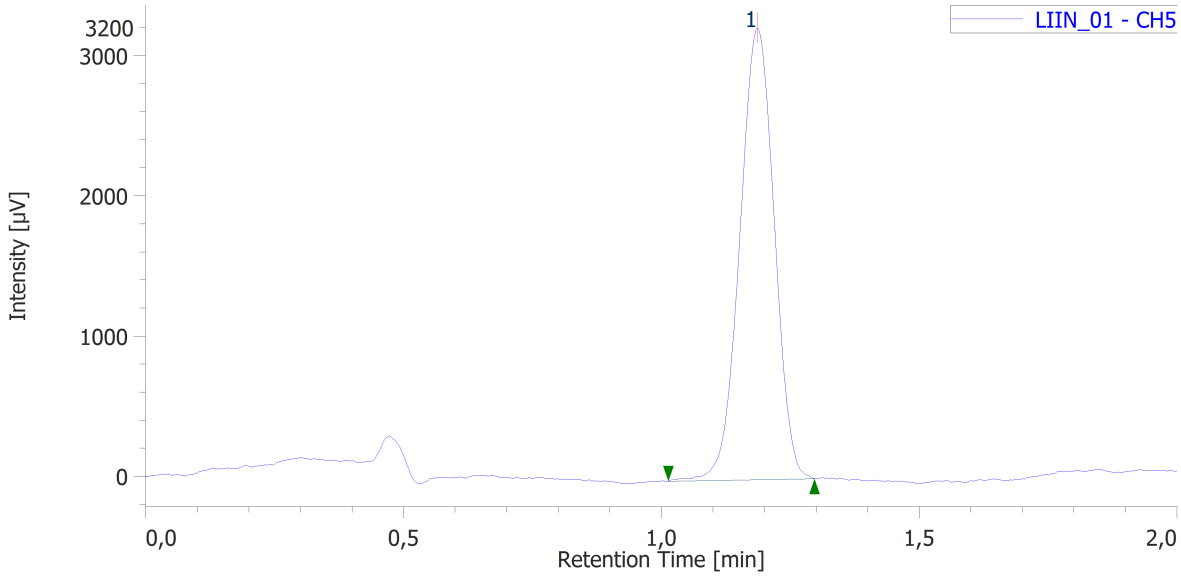

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 17:01:43
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 16:59:42
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	LIIN_01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,187	14980	3220	100,000	100,000	N/A	1483	N/A	0,968	

Creator
Reviewer
Approver

Chromatogram

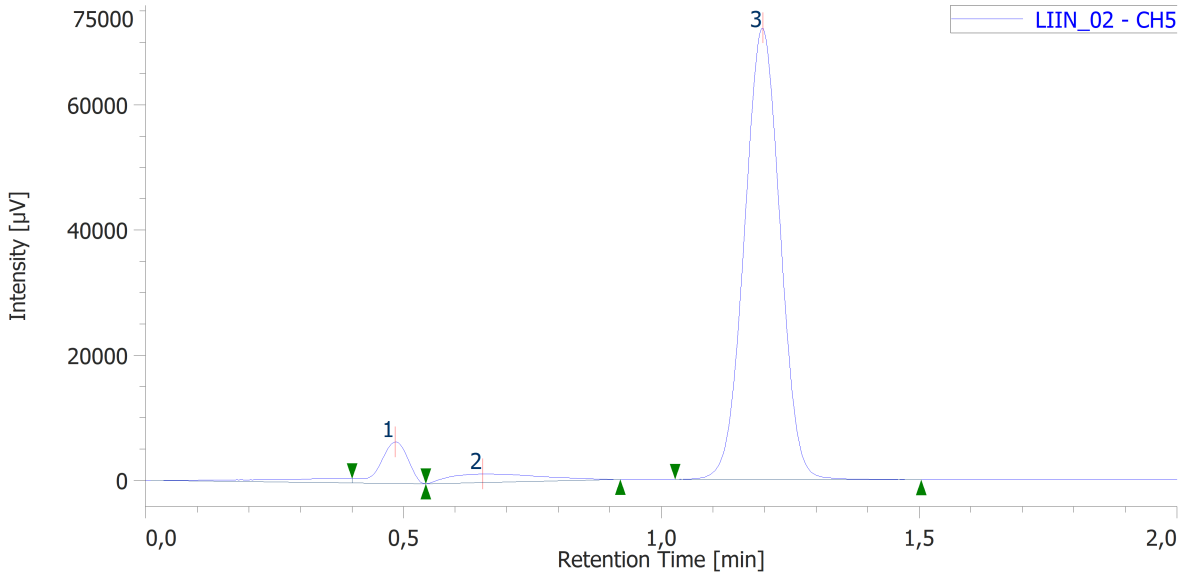

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 17:04:23
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 17:02:22
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	LIIN_02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	24106	6636	6,219	8,285	N/A	414	0,775	N/A	
2	Unknown	5	0,653	16659	1359	4,298	1,697	N/A	57	2,307	1,656	
3	Cafeína	5	1,197	346854	72092	89,483	90,017	N/A	1408	N/A	0,989	

Creator
Reviewer
Approver

Chromatogram

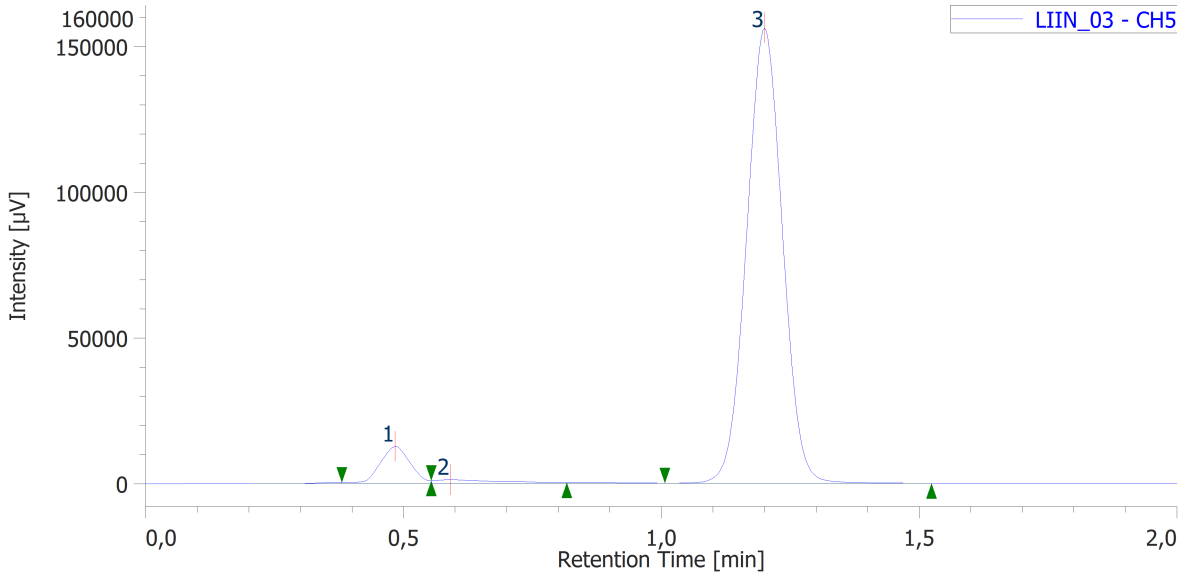

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 17:07:05
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 17:05:02
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	LIIN_03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	51097	12718	6,267	7,476	N/A	324	N/A	N/A	
2	Unknown	5	0,590	11180	1252	1,371	0,736	N/A	N/A	N/A	N/A	
3	Cafeína	5	1,200	753053	156145	92,362	91,788	N/A	1422	N/A	1,015	

Creator
Reviewer
Approver

Chromatogram

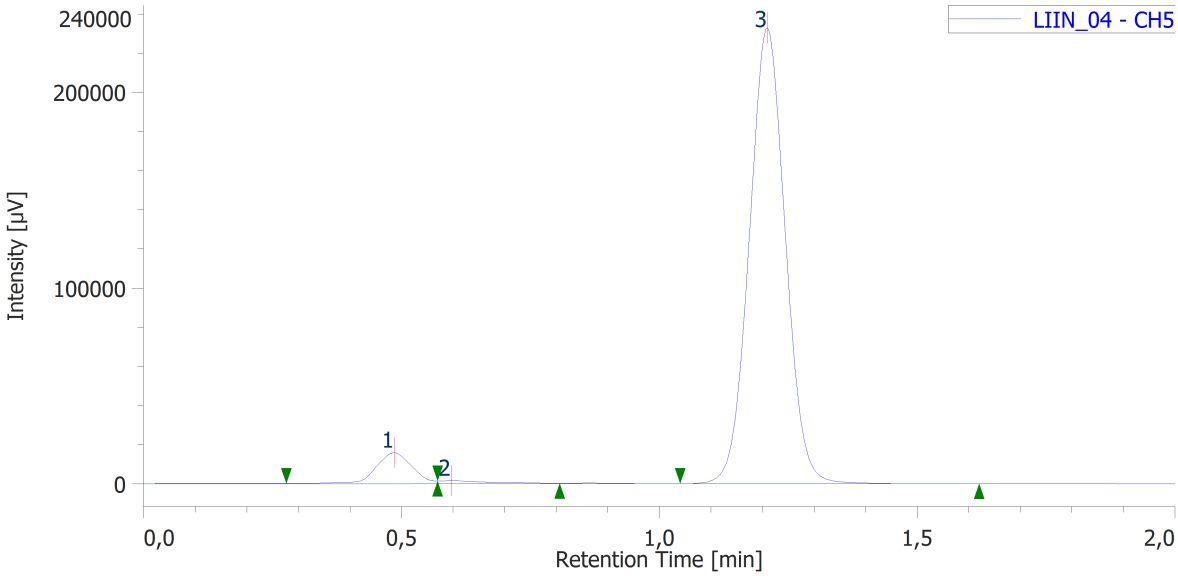

Chromatogram Information

User Name	QPackSA
Date Modified	22/02/2024 17:09:49
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 17:07:47
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	LIIN_04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,487	76332	15809	6,292	6,325	N/A	233	N/A	N/A	
2	Unknown	5	0,597	10485	1496	0,864	0,599	N/A	N/A	N/A	N/A	
3	Cafeína	5	1,210	1126325	232625	92,844	93,076	N/A	1455	N/A	1,016	

Creator
Reviewer
Approver

Chromatogram

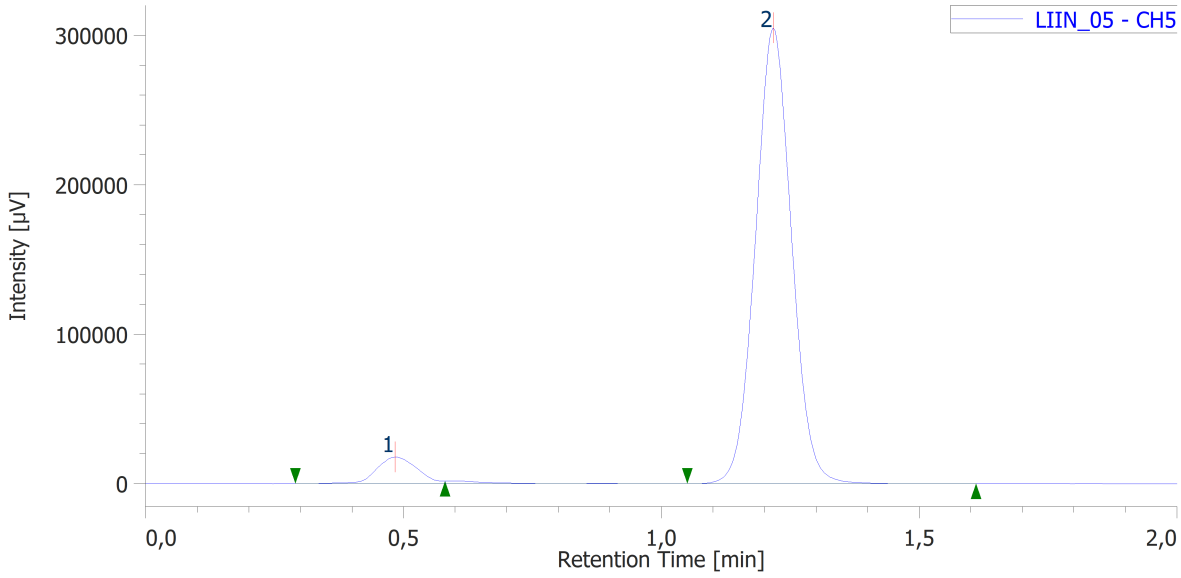

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 17:12:36
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 17:10:35
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH5
Sample Name	LIIN_05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,483	96803	17822	6,132	5,527	N/A	173	5,374	N/A	
2	Cafeína	5	1,217	1481818	304664	93,868	94,473	N/A	1472	N/A	1,041	

Creator
Reviewer
Approver

Chromatogram

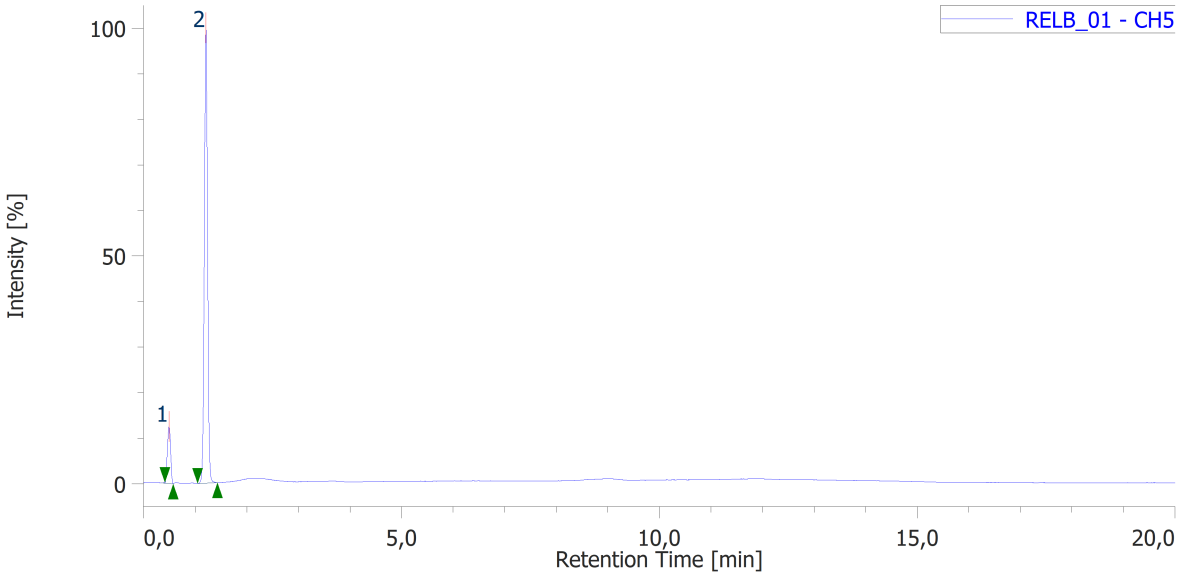

Chromatogram Information

User Name	QPackSA
Date Modified	22/02/2024 15:48:47
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 15:28:45
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_01-CH5
Sample Name	RELB_01
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,490	69933	15951	11,144	11,092	N/A	261	6,113	0,973	
2	Cafeína	5	1,207	557631	127850	88,856	88,908	N/A	1802	N/A	1,005	

Creator
Reviewer
Approver

Chromatogram

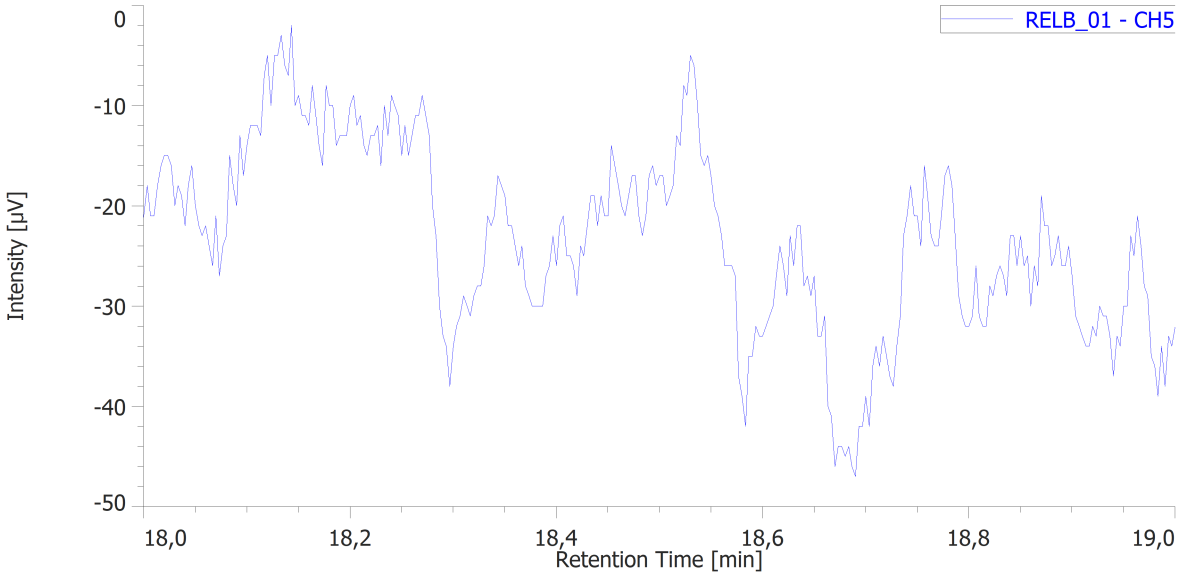

Chromatogram Information	
User Name	QPackSA
Date Modified	22/02/2024 15:48:47
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 15:28:45
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_01-CH5
Sample Name	RELB_01
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,490	69933	15951	11,144	11,092	N/A	261	6,113	0,973	
2	Cafeína	5	1,207	557631	127850	88,856	88,908	N/A	1802	N/A	1,005	

Creator
Reviewer
Approver

Chromatogram

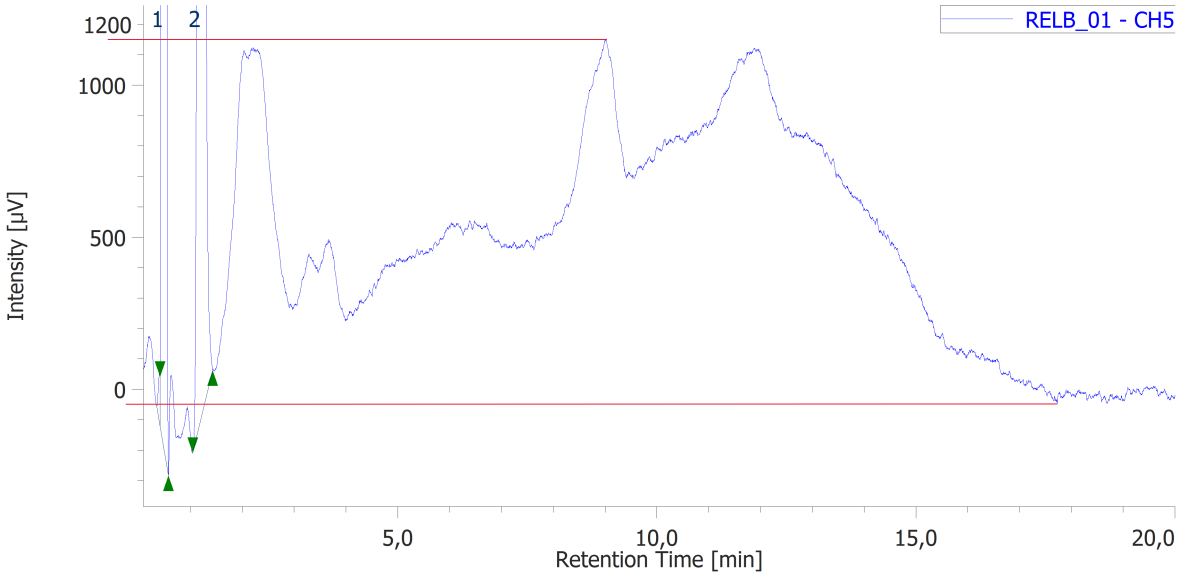

Chromatogram Information

User Name	QPackSA
Date Modified	22/02/2024 15:48:47
Description	
HPLC System Name	HPL09
Injection Date	22/02/2024 15:28:45
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_01-CH5
Sample Name	RELB_01
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificaçãp

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	0,490	69933	15951	11,144	11,092	N/A	261	6,113	0,973	
2	Cafeína	5	1,207	557631	127850	88,856	88,908	N/A	1802	N/A	1,005	

Creator
Reviewer
Approver

Chromatogram

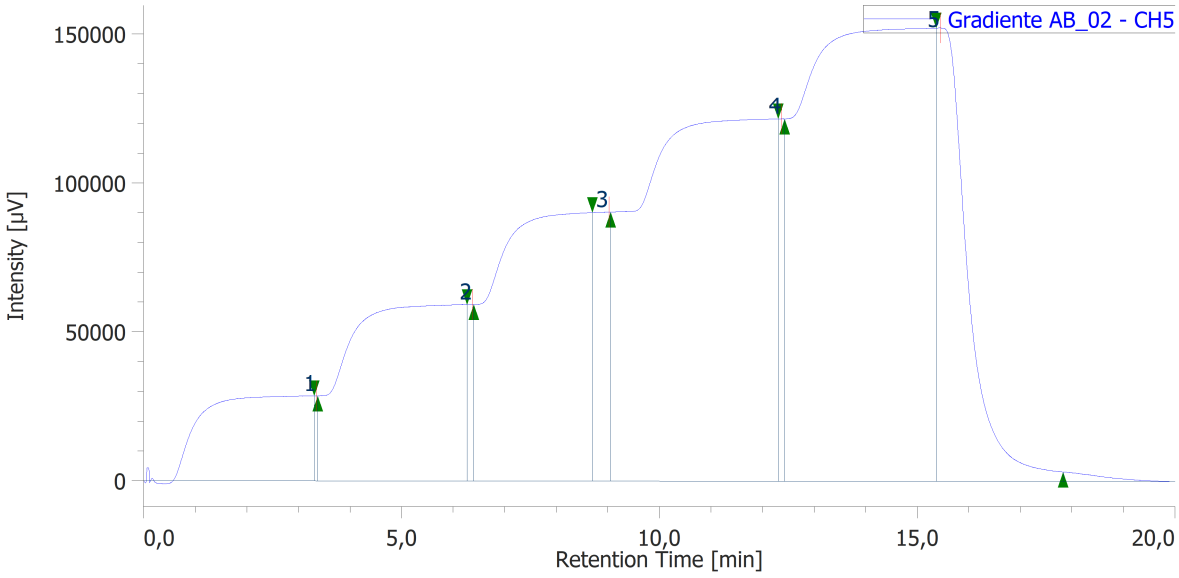

Chromatogram Information

User Name	QPackSA
Date Modified	23/02/2024 12:31:20
Description	
HPLC System Name	HPL09
Injection Date	23/02/2024 12:11:16
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	GRAD AB
Peak ID Table	GradienteAB
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_02-CH5
Sample Name	Gradiente AB
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	GradienteAB

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,353	125466	28531	1,293	6,314	N/A	N/A	N/A	N/A	
2	40%	5	6,377	461811	59228	4,758	13,108	N/A	N/A	N/A	N/A	
3	60%	5	9,023	1894151	90294	19,514	19,983	N/A	N/A	N/A	N/A	
4	80%	5	12,370	899900	121635	9,271	26,918	N/A	N/A	N/A	N/A	
5	100%	5	15,443	6325334	152175	65,165	33,677	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

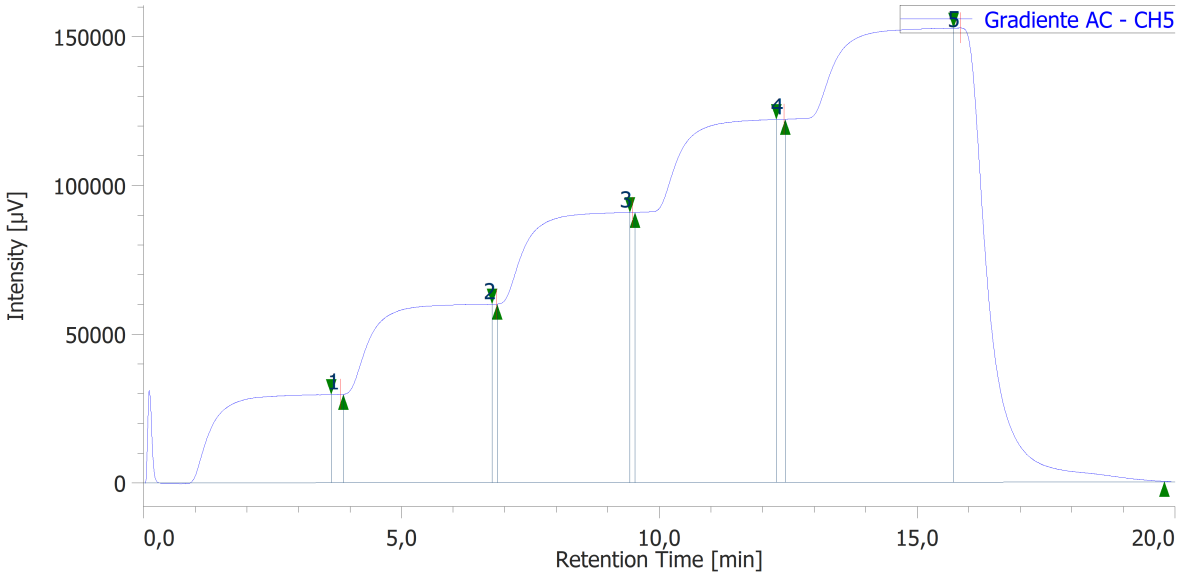

Chromatogram Information	
User Name	QPackSA
Date Modified	23/02/2024 12:10:46
Description	
HPLC System Name	HPL09
Injection Date	23/02/2024 11:50:43
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	GRAD AC
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AC-CH5
Sample Name	Gradiente AC
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Gradiente

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,817	420901	29704	4,480	6,525	N/A	N/A	N/A	N/A	
2	Unknown	5	6,840	359851	60010	3,830	13,181	N/A	N/A	N/A	N/A	
3	Unknown	5	9,483	544629	90798	5,797	19,944	N/A	N/A	N/A	N/A	
4	Unknown	5	12,413	1268935	122063	13,506	26,811	N/A	N/A	N/A	N/A	
5	Unknown	5	15,840	6801167	152691	72,388	33,539	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver