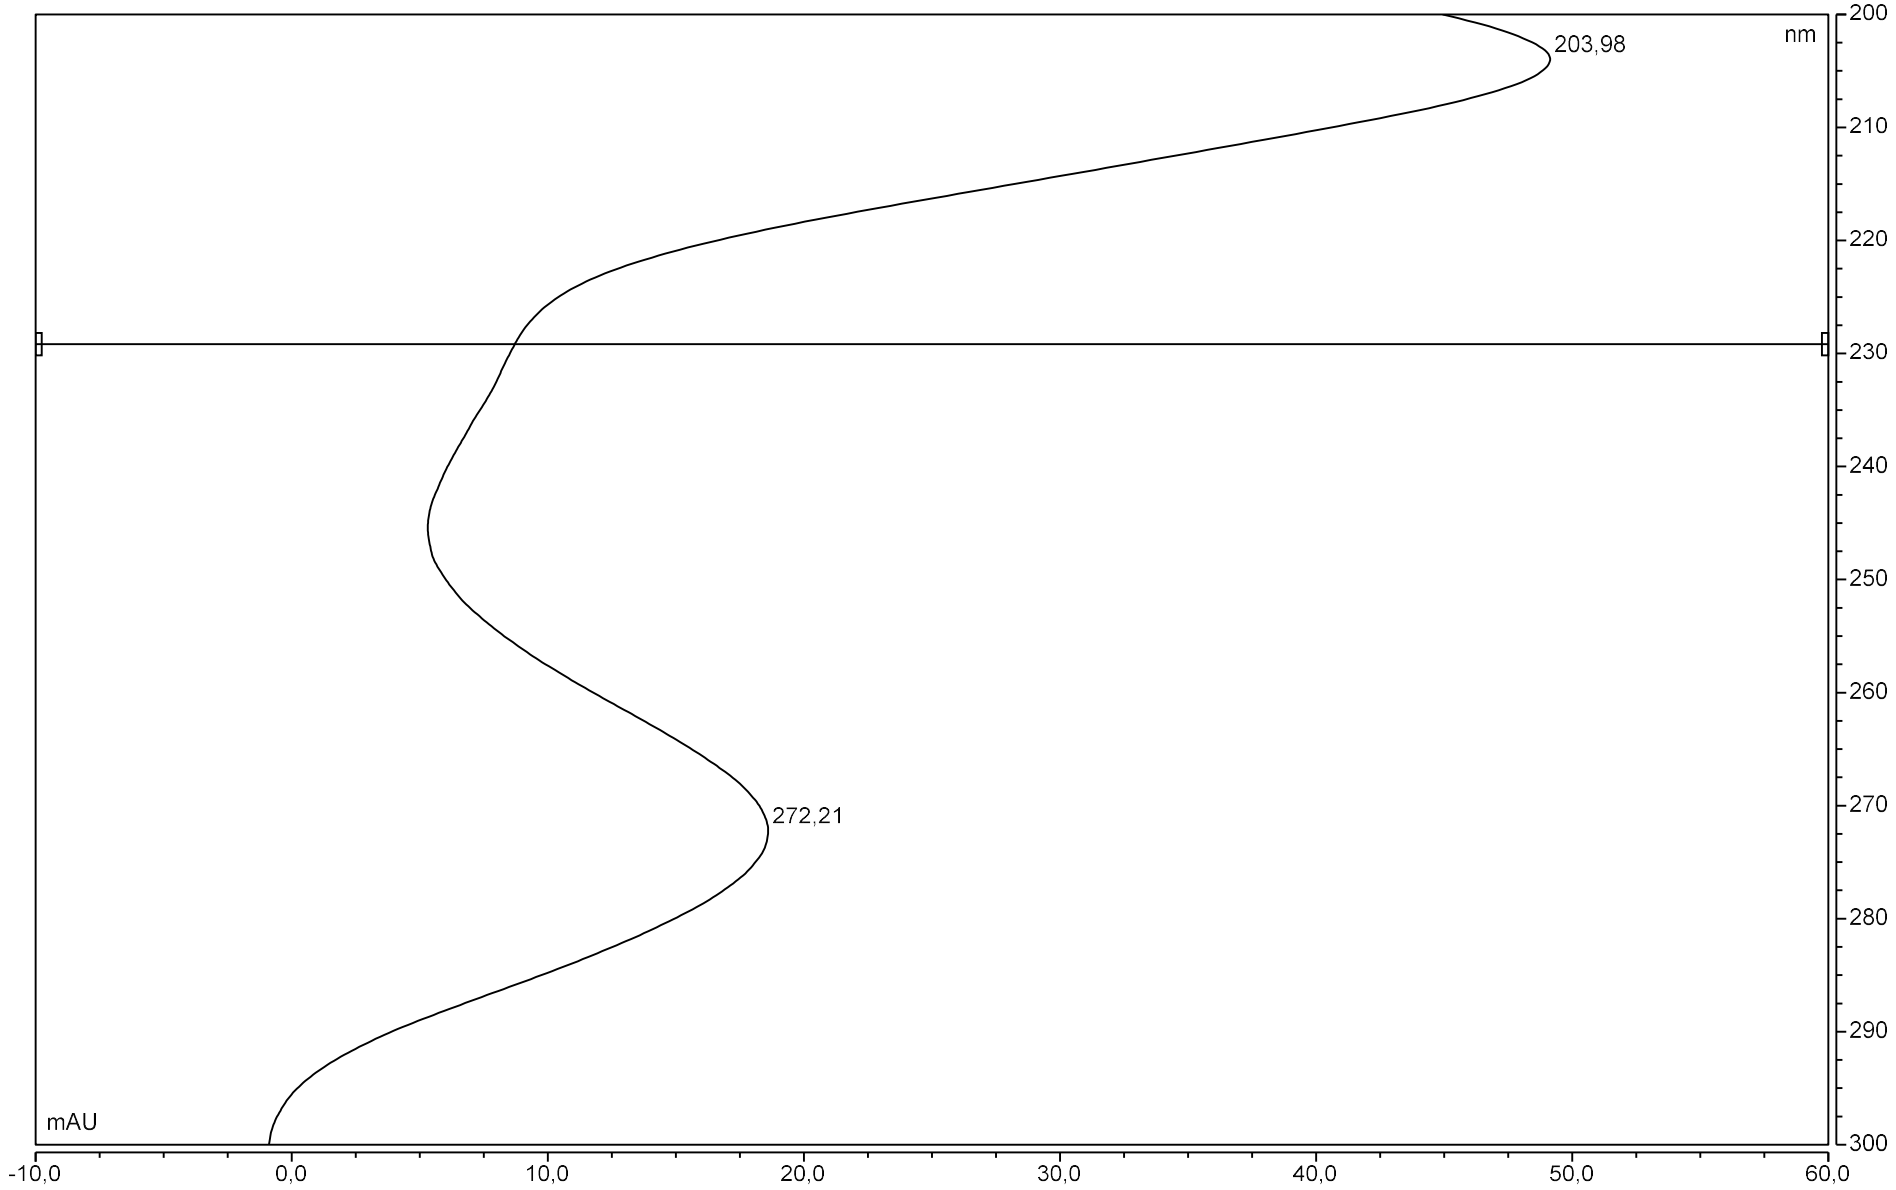
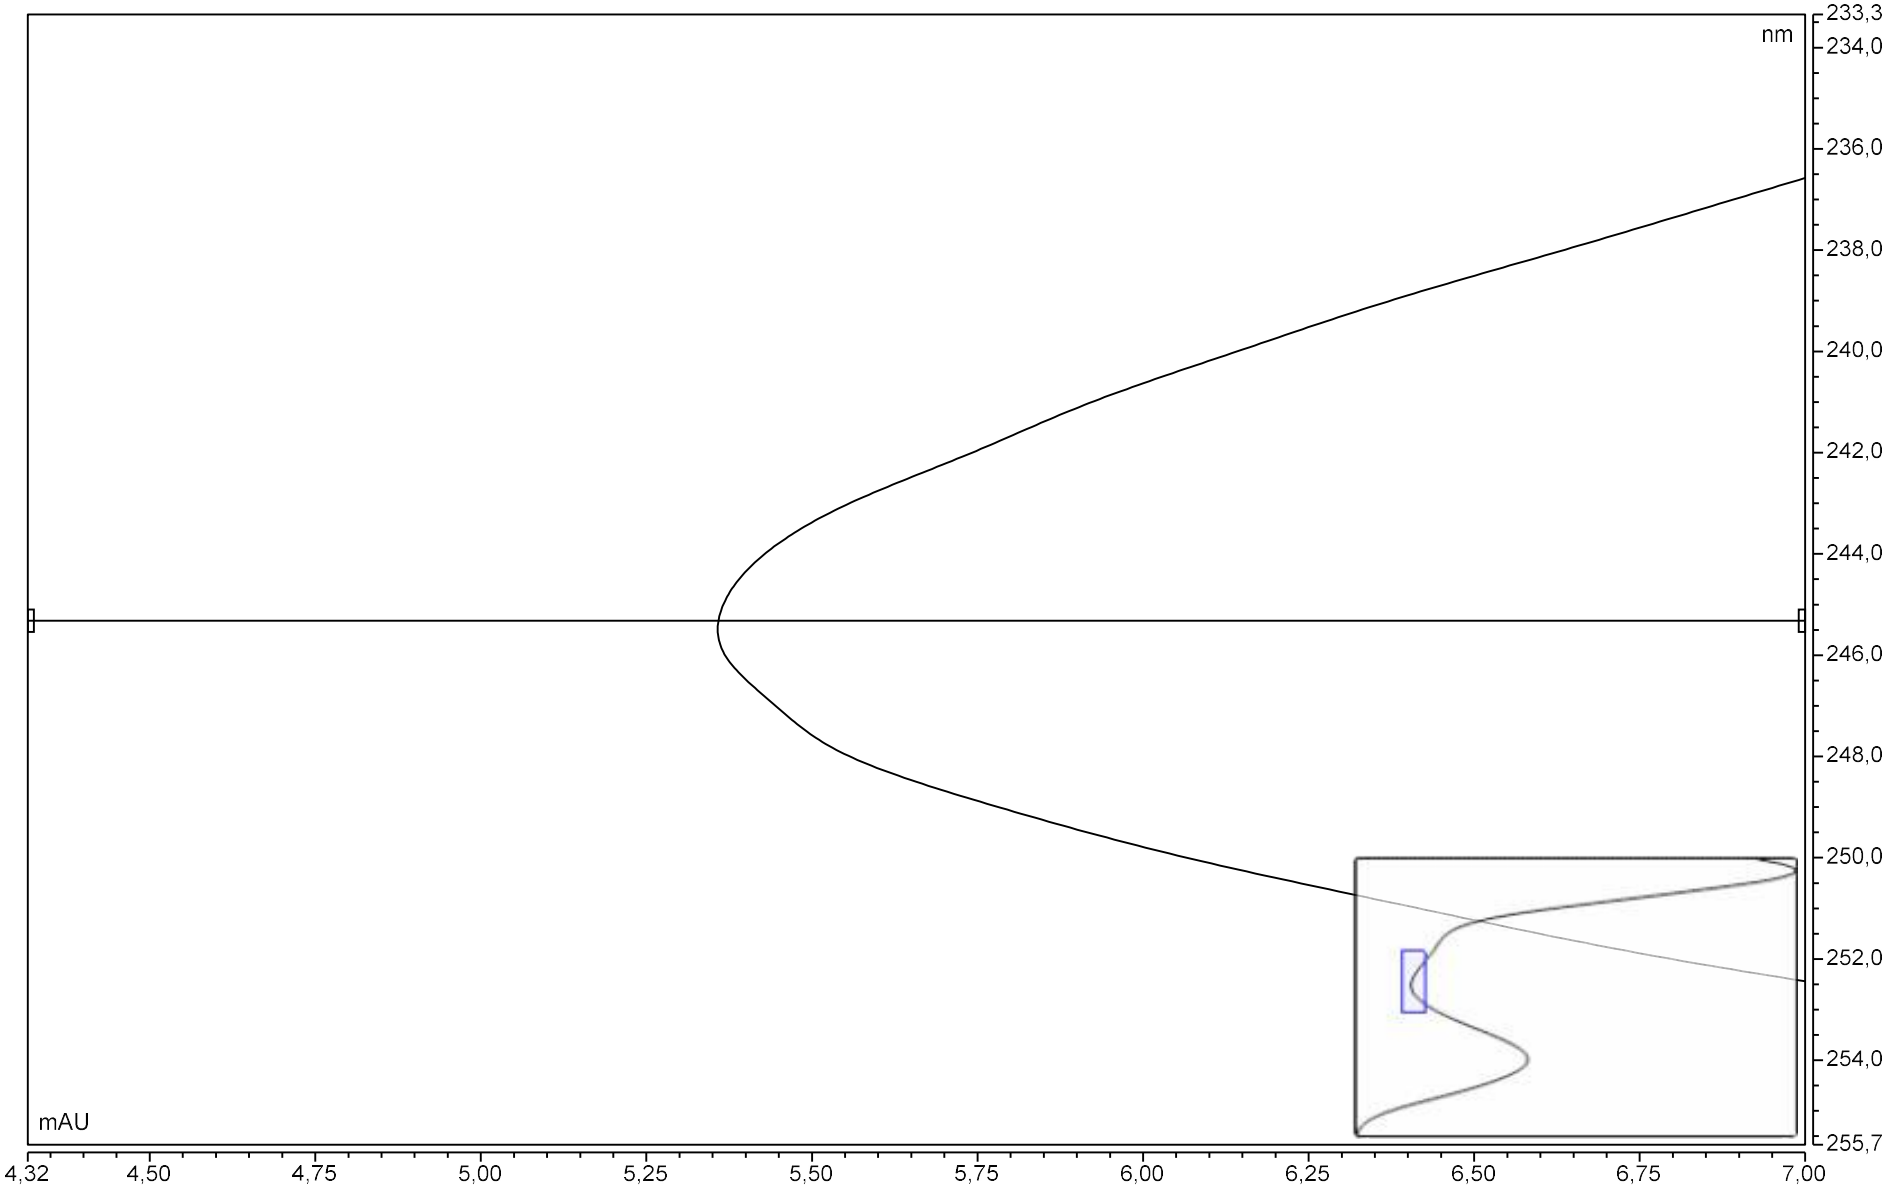

203,98
272,21
nm
mAU
200
210
220
230
240
250
260
270
280
290
300
-10,0
0,0
10,0
20,0
30,0
40,0
50,0
60,0



nm
233,3
234,0
236,0
238,0
240,0
242,0
244,0
246,0
248,0
250,0
252,0
254,0
255,7
mAU
4,32
4,50
4,75
5,00
5,25
5,50
5,75
6,00
6,25
6,50
6,75
7,00

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Left**	*Bandwidth:*	**4**
Processing Method:	**RELB Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 11:03**	*Sample Weight:*	**1,0000**

Chromatogram

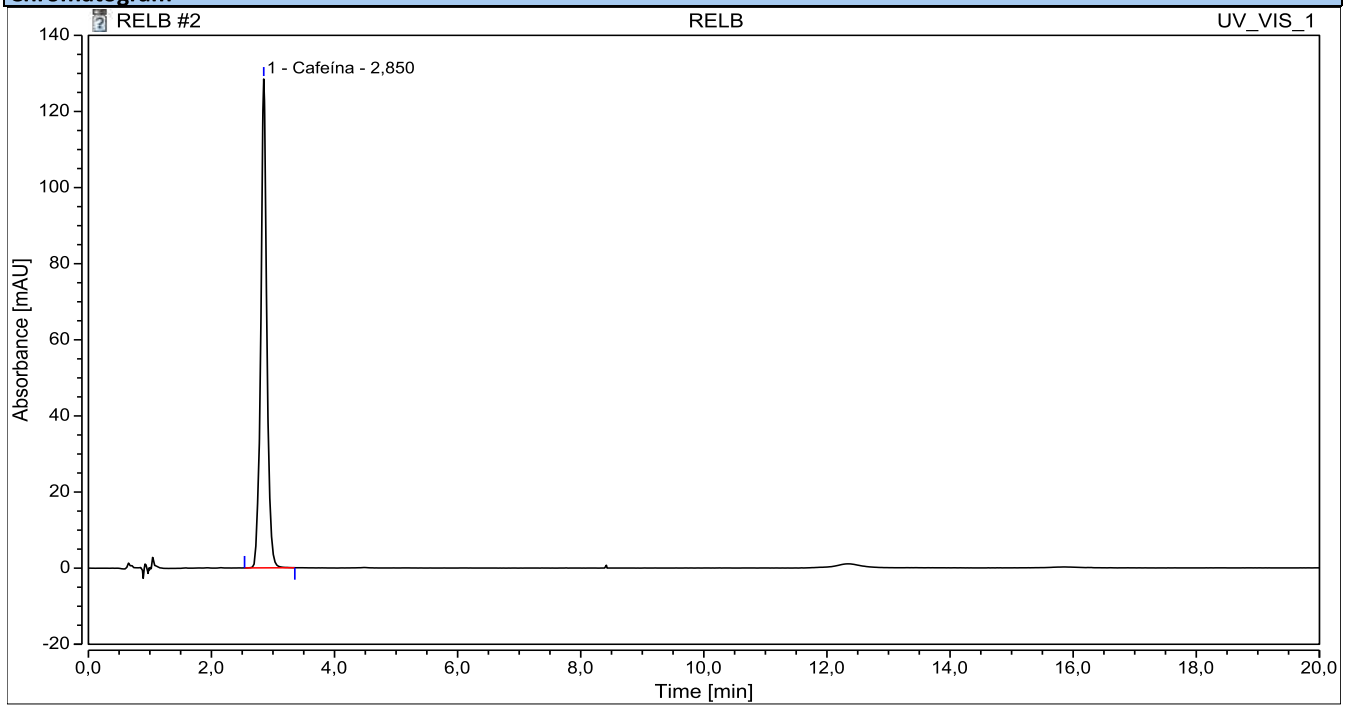

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,850	14,4938	128,454	100,00	100,00	n.a.
Total:			**14,494**	**128,454**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Left**	*Bandwidth:*	**4**
Processing Method:	**RELB Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 11:03**	*Sample Weight:*	**1,0000**

Chromatogram

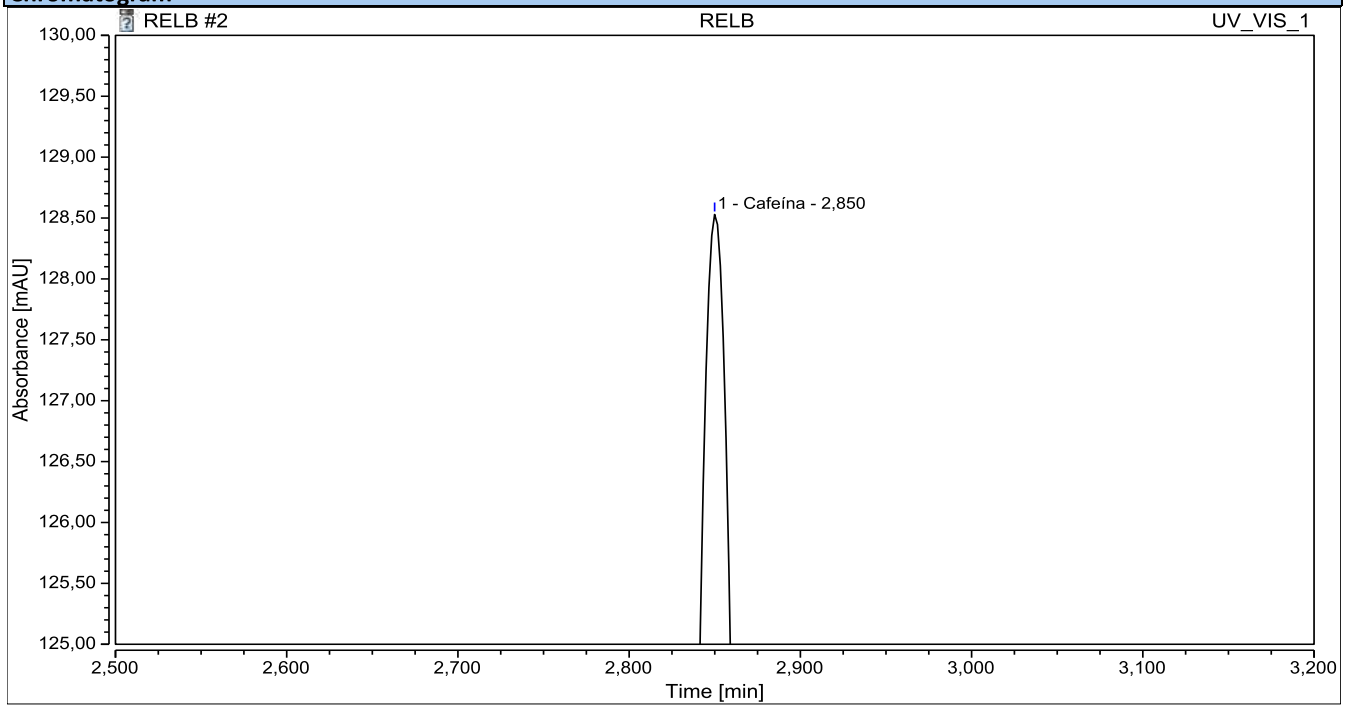

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,850	14,4938	128,454	100,00	100,00	n.a.
Total:			**14,494**	**128,454**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Left**	*Bandwidth:*	**4**
Processing Method:	**RELB Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 11:03**	*Sample Weight:*	**1,0000**

Chromatogram

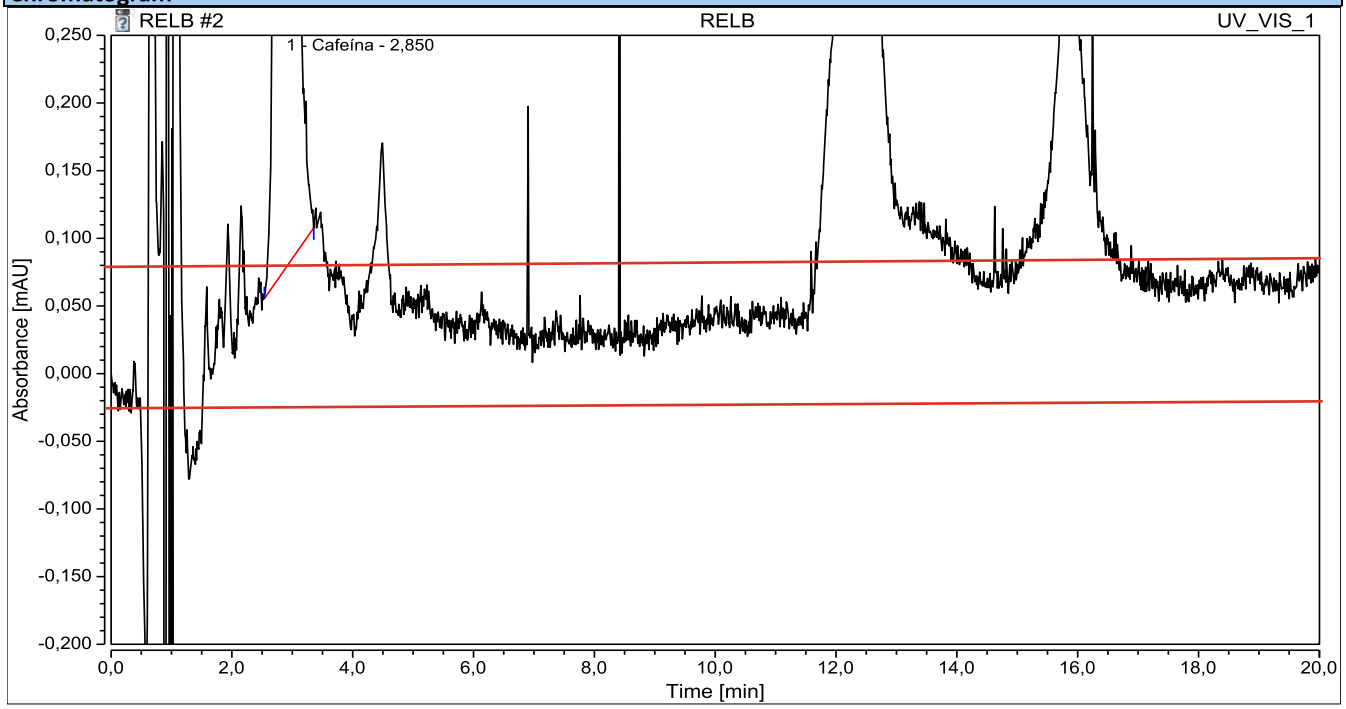

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,850	14,4938	128,454	100,00	100,00	n.a.
Total:			**14,494**	**128,454**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Left**	*Bandwidth:*	**4**
Processing Method:	**RELB Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 11:03**	*Sample Weight:*	**1,0000**

Chromatogram

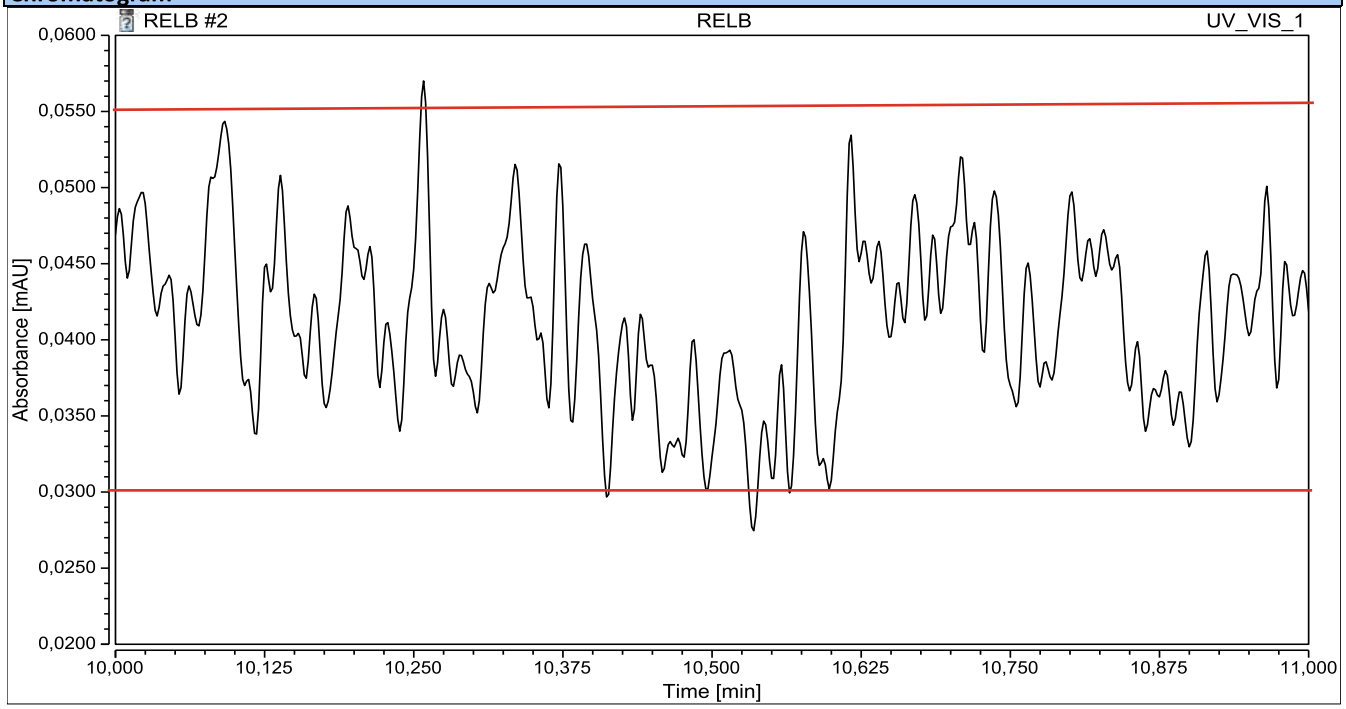

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,850	14,4938	128,454	100,00	100,00	n.a.
Total:			**14,494**	**128,454**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:30**	*Sample Weight:*	**1,0000**

Chromatogram

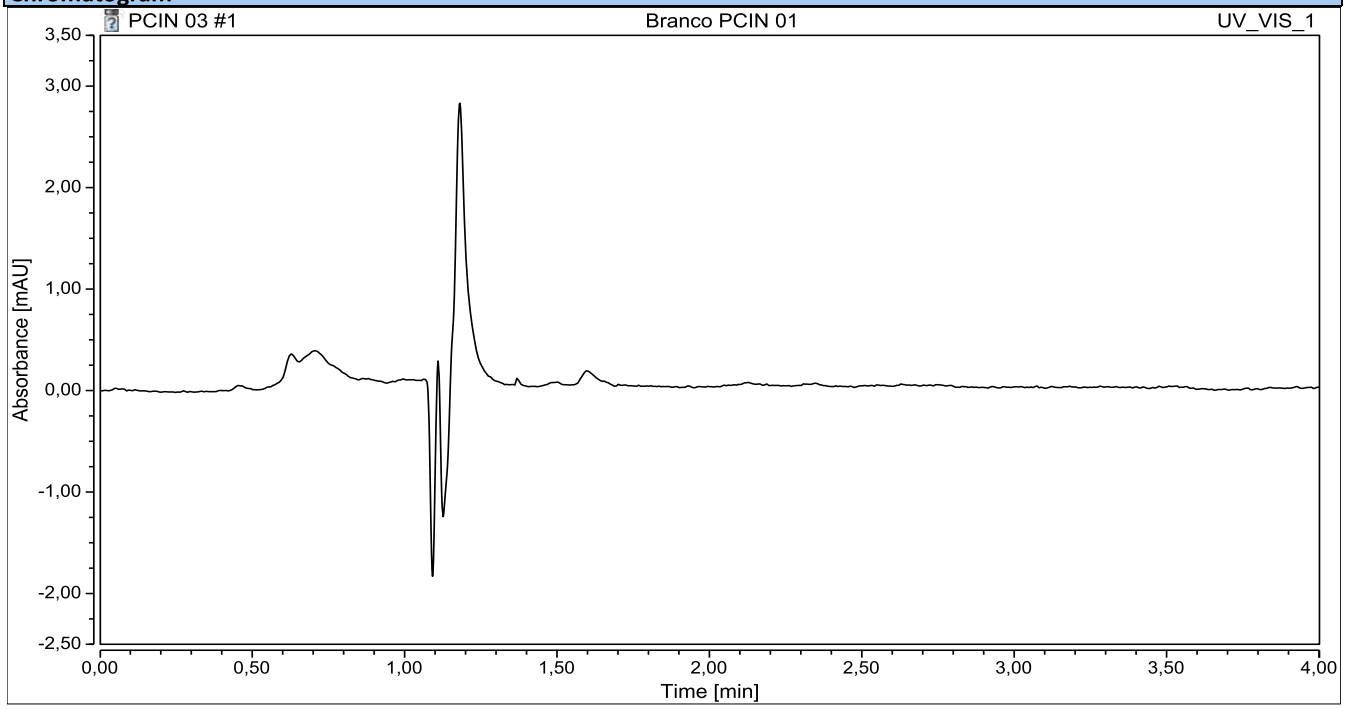

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:35**	*Sample Weight:*	**1,0000**

Chromatogram

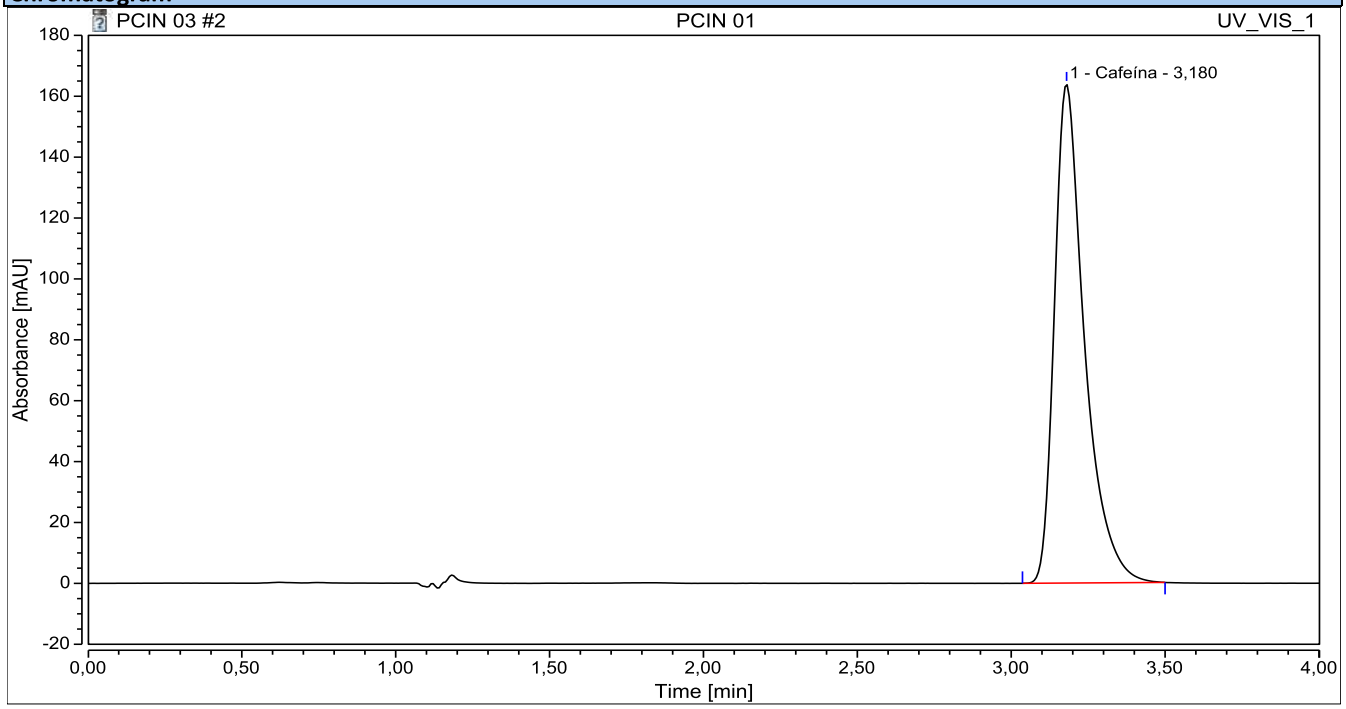

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,180	18,5628	163,959	100,00	100,00	n.a.
Total:			**18,563**	**163,959**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:41**	*Sample Weight:*	**1,0000**

Chromatogram

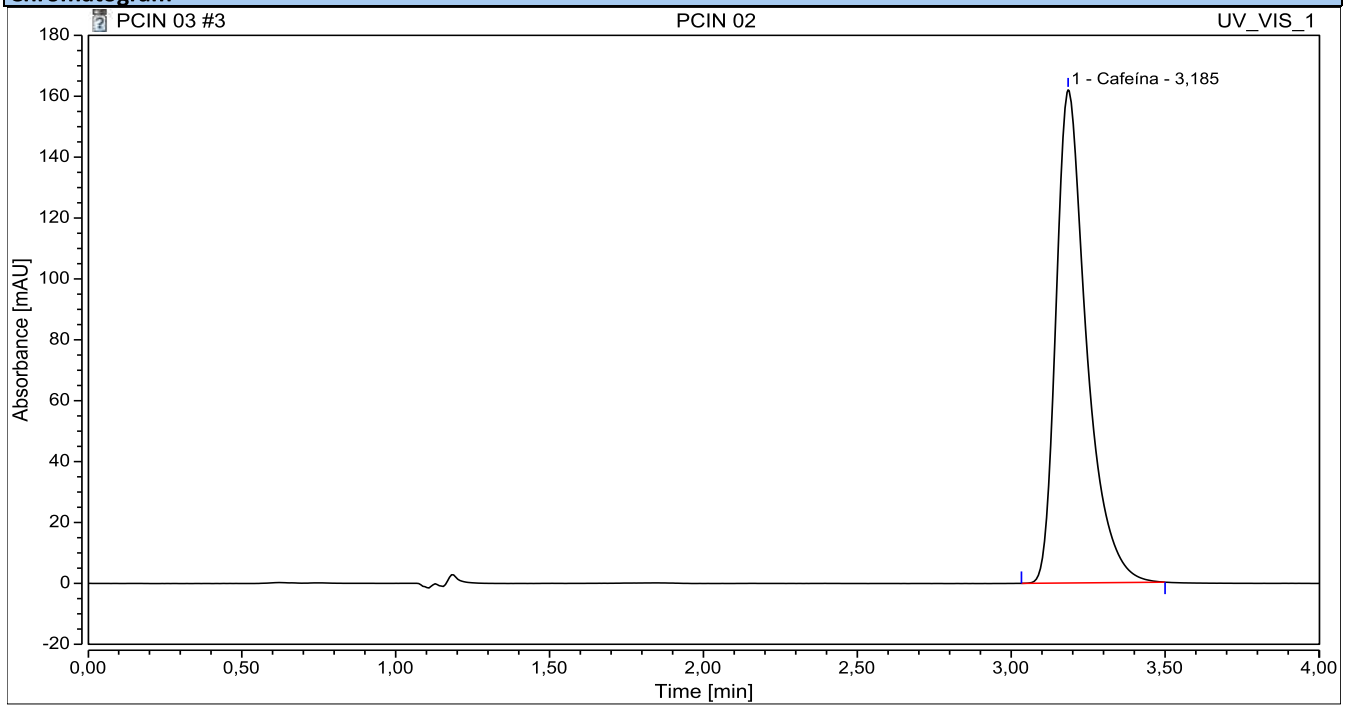

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,185	18,6081	161,979	100,00	100,00	n.a.
Total:			**18,608**	**161,979**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:46**	*Sample Weight:*	**1,0000**

Chromatogram

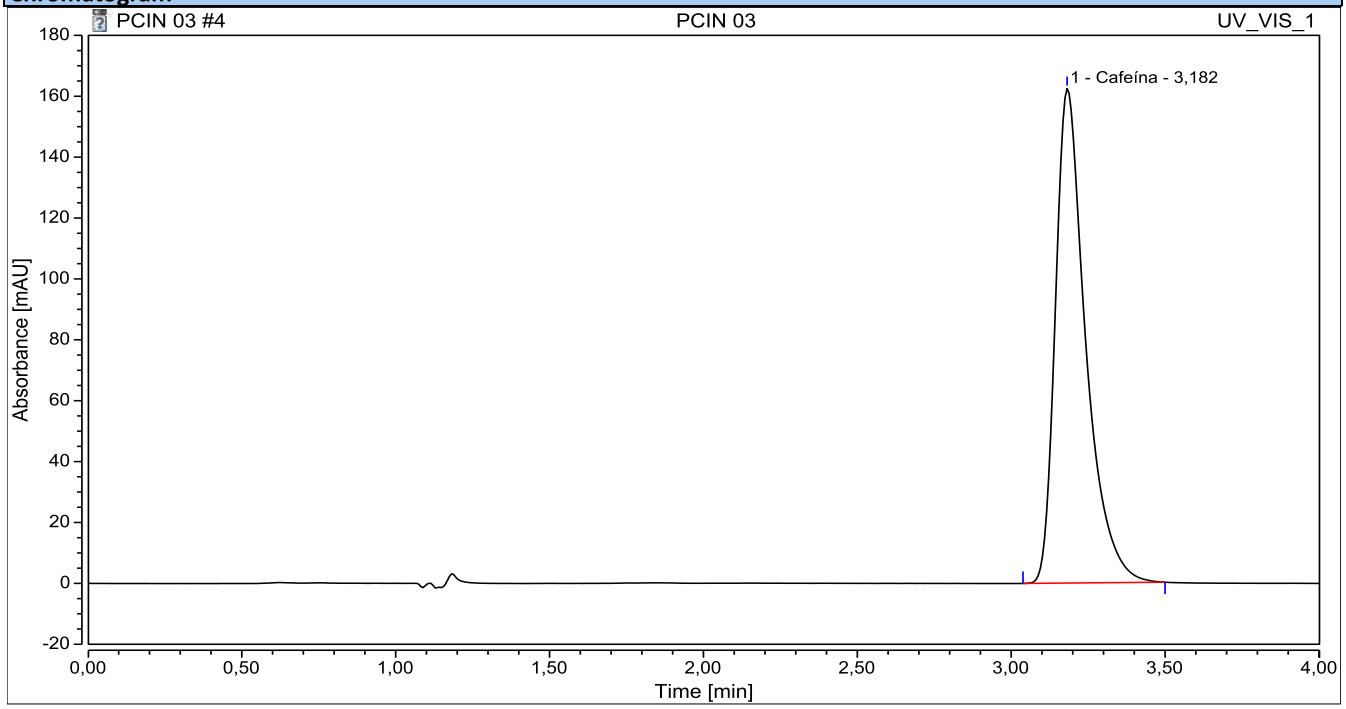

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,182	18,5438	162,421	100,00	100,00	n.a.
Total:			**18,544**	**162,421**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:51**	*Sample Weight:*	**1,0000**

Chromatogram

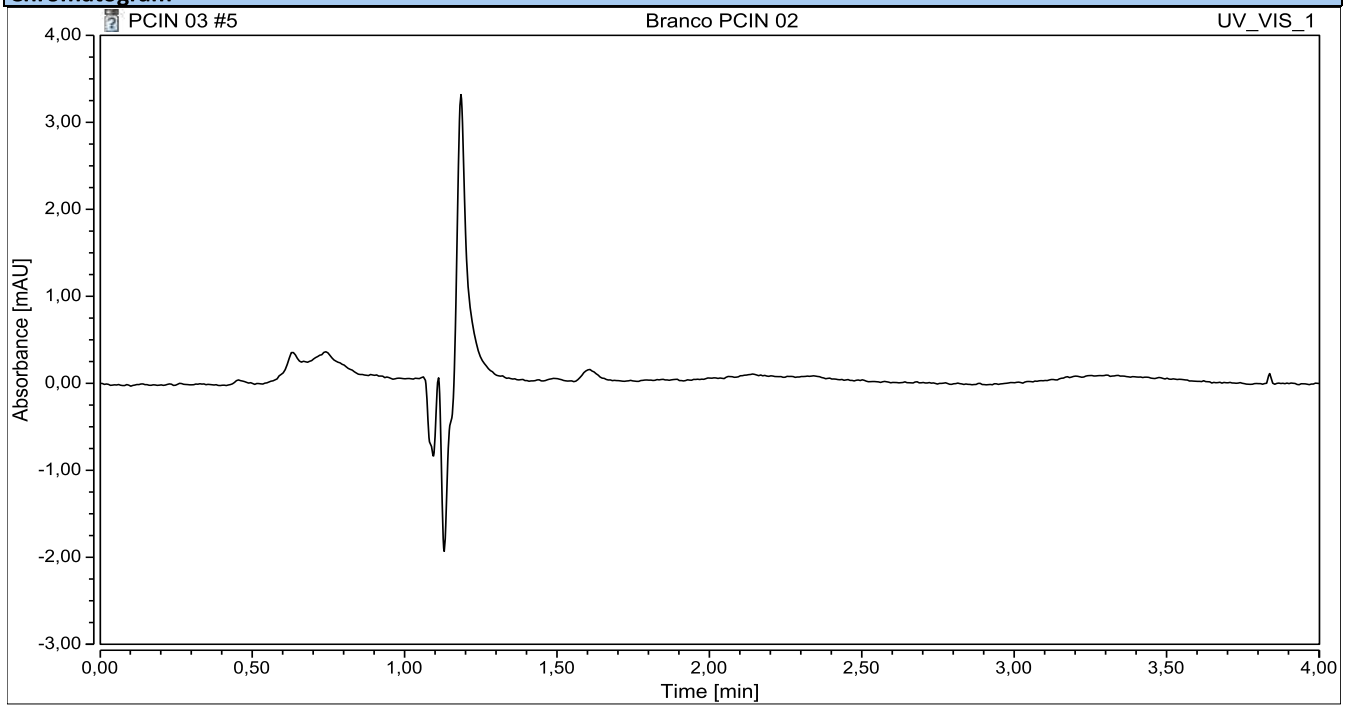

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 14:56**	*Sample Weight:*	**1,0000**

Chromatogram

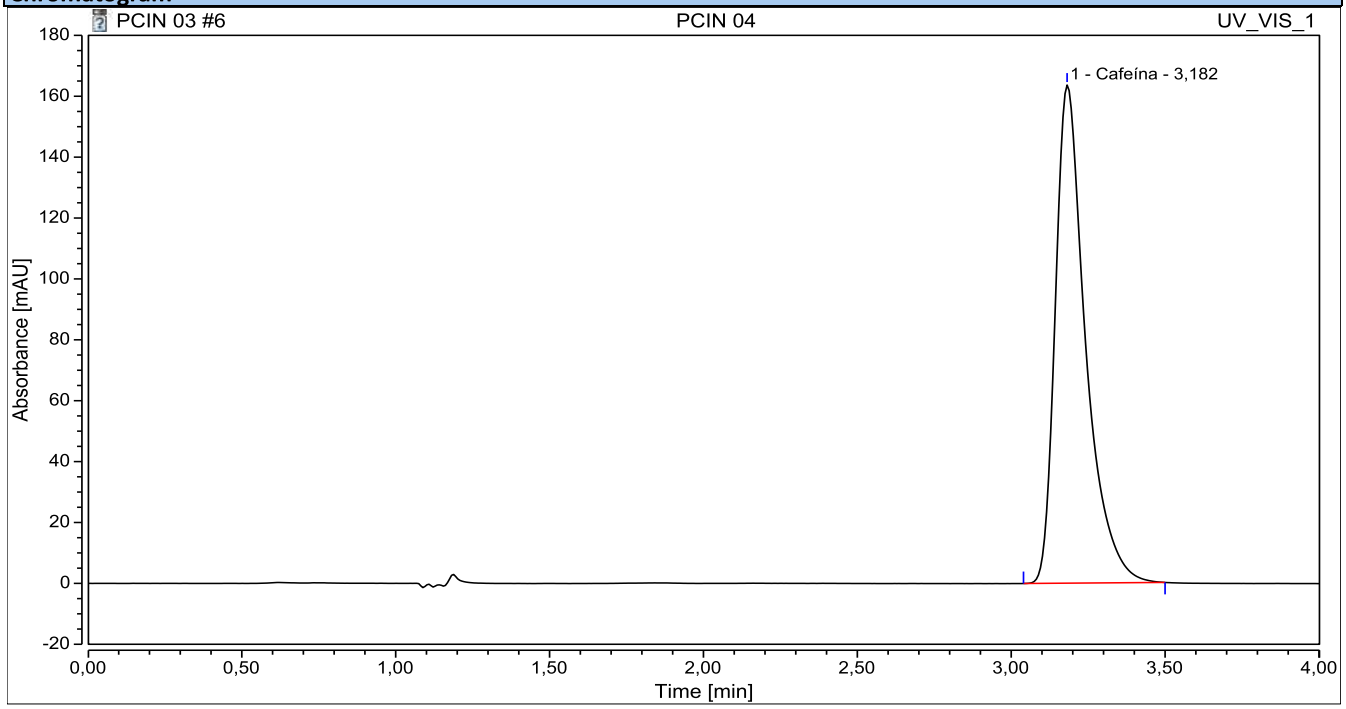

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,182	18,6493	163,619	100,00	100,00	n.a.
Total:			**18,649**	**163,619**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:01**	*Sample Weight:*	**1,0000**

Chromatogram

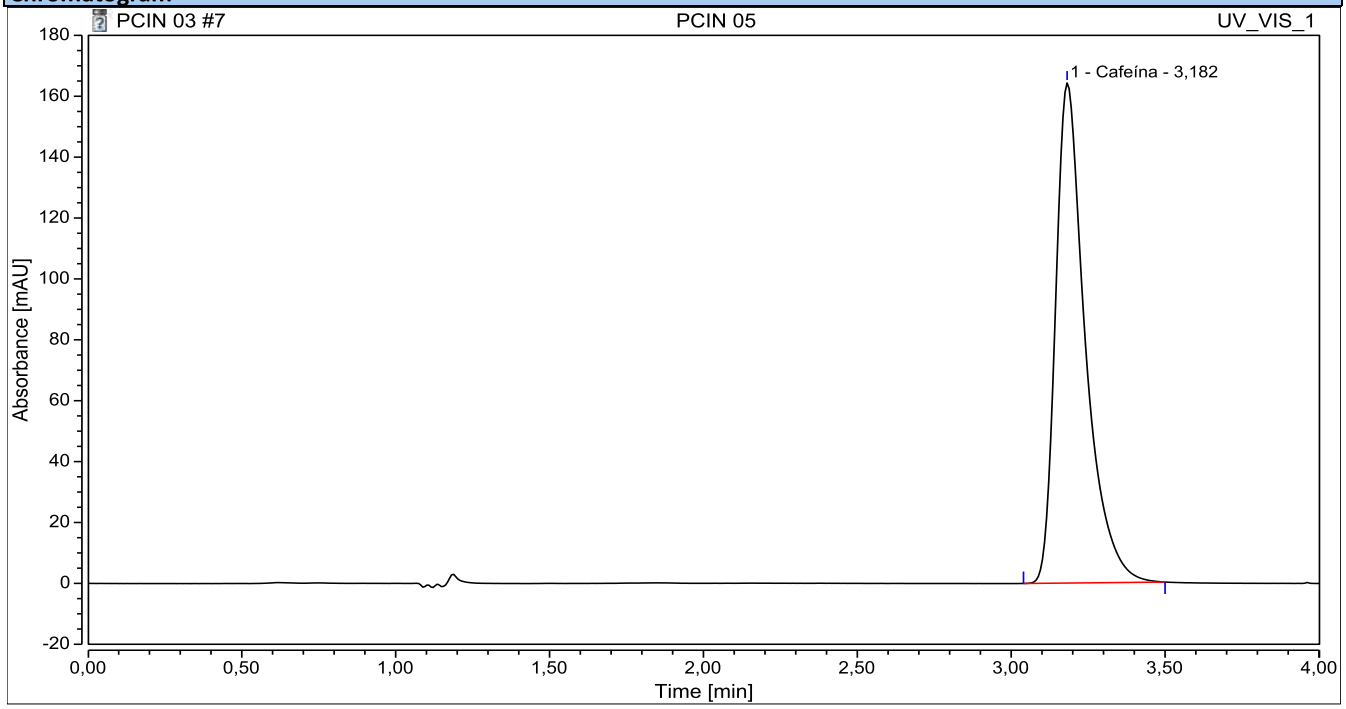

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,182	18,4020	164,243	100,00	100,00	n.a.
Total:			**18,402**	**164,243**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:06**	*Sample Weight:*	**1,0000**

Chromatogram

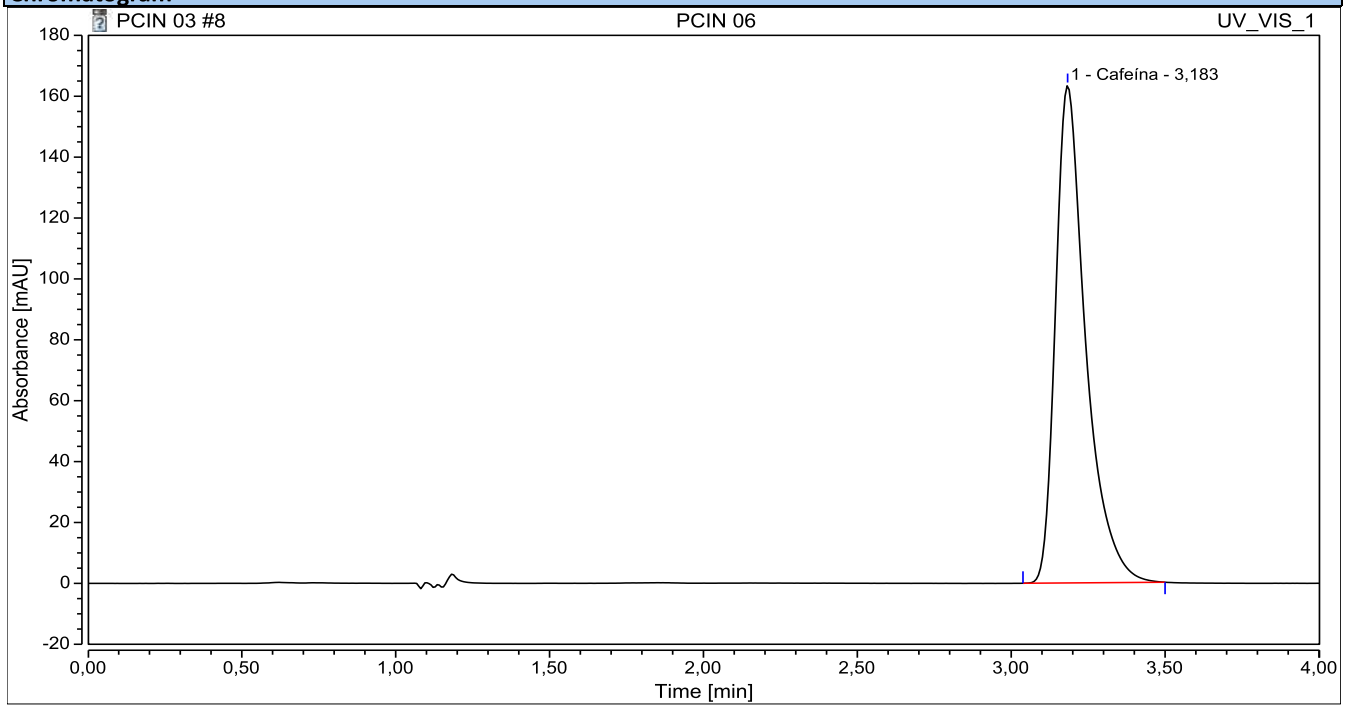

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,183	18,5867	163,388	100,00	100,00	n.a.
Total:			**18,587**	**163,388**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:12**	*Sample Weight:*	**1,0000**

Chromatogram

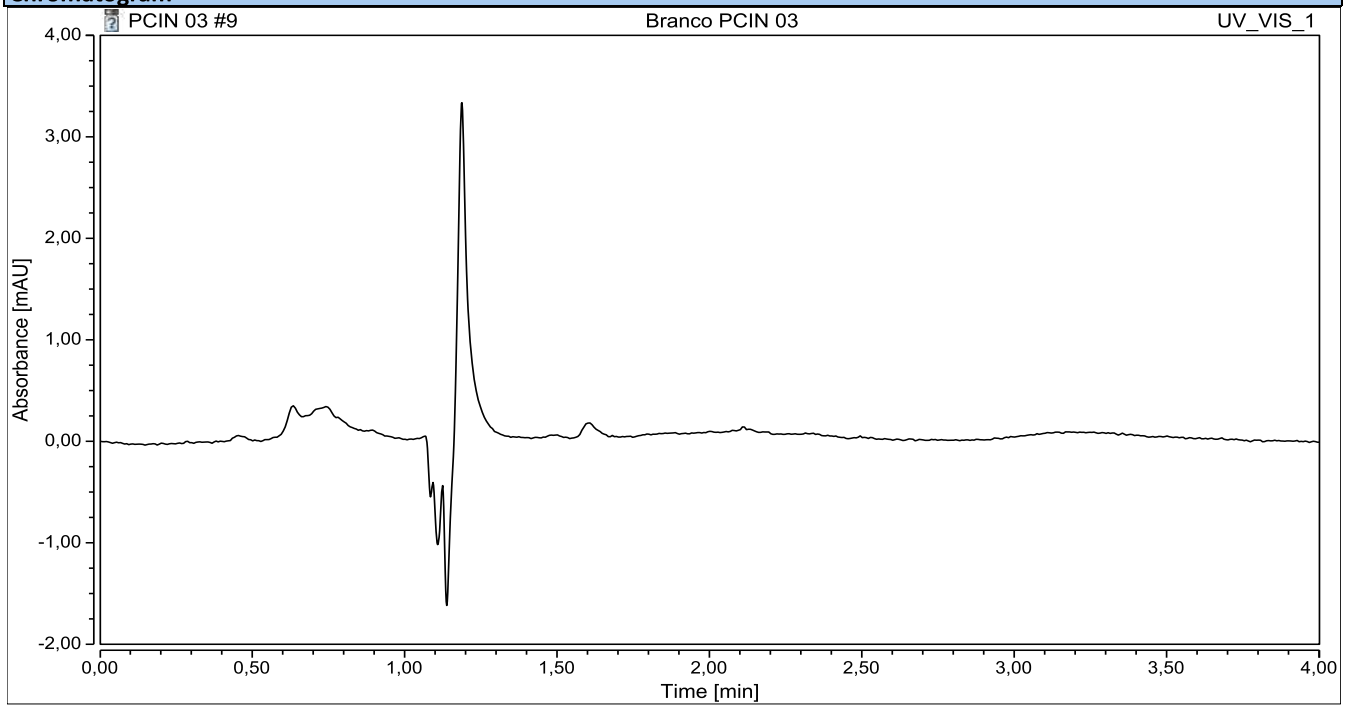

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV L 01**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:17**	*Sample Weight:*	**1,0000**

Chromatogram

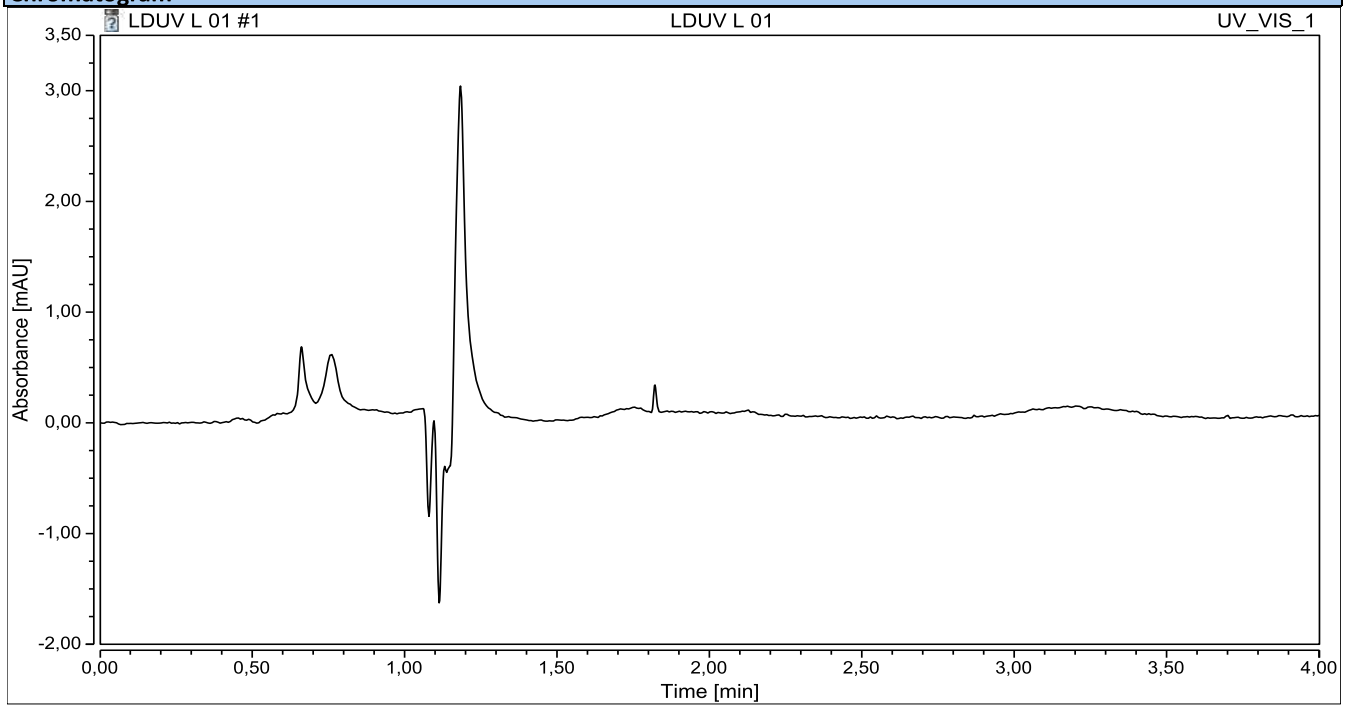

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV L 02**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:22**	*Sample Weight:*	**1,0000**

Chromatogram

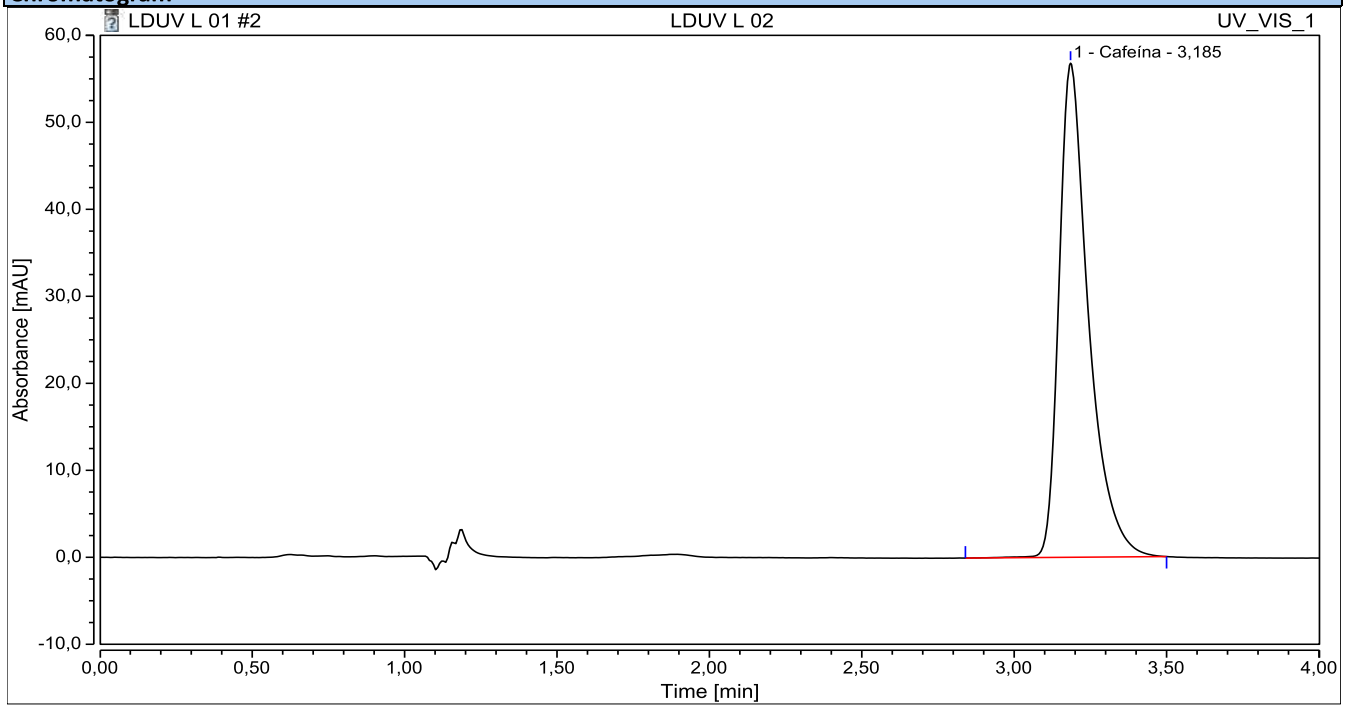

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,185	6,3931	56,807	100,00	100,00	n.a.
Total:			**6,393**	**56,807**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV L 03**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:27**	*Sample Weight:*	**1,0000**

Chromatogram

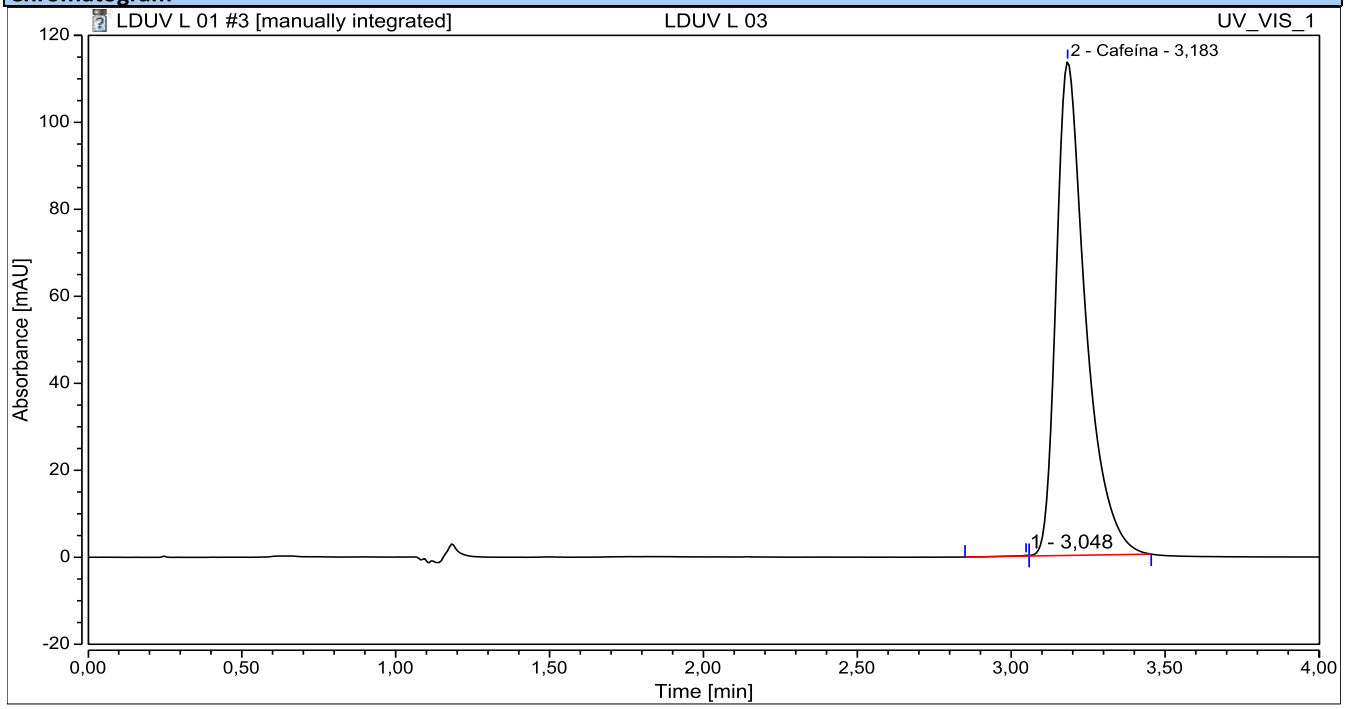

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	Cafeína	3,183	12,6269	113,547	99,94	99,82	n.a.
Total:			**12,627**	**113,547**	**99,942**	**99,824**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV L 04**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:33**	*Sample Weight:*	**1,0000**

Chromatogram

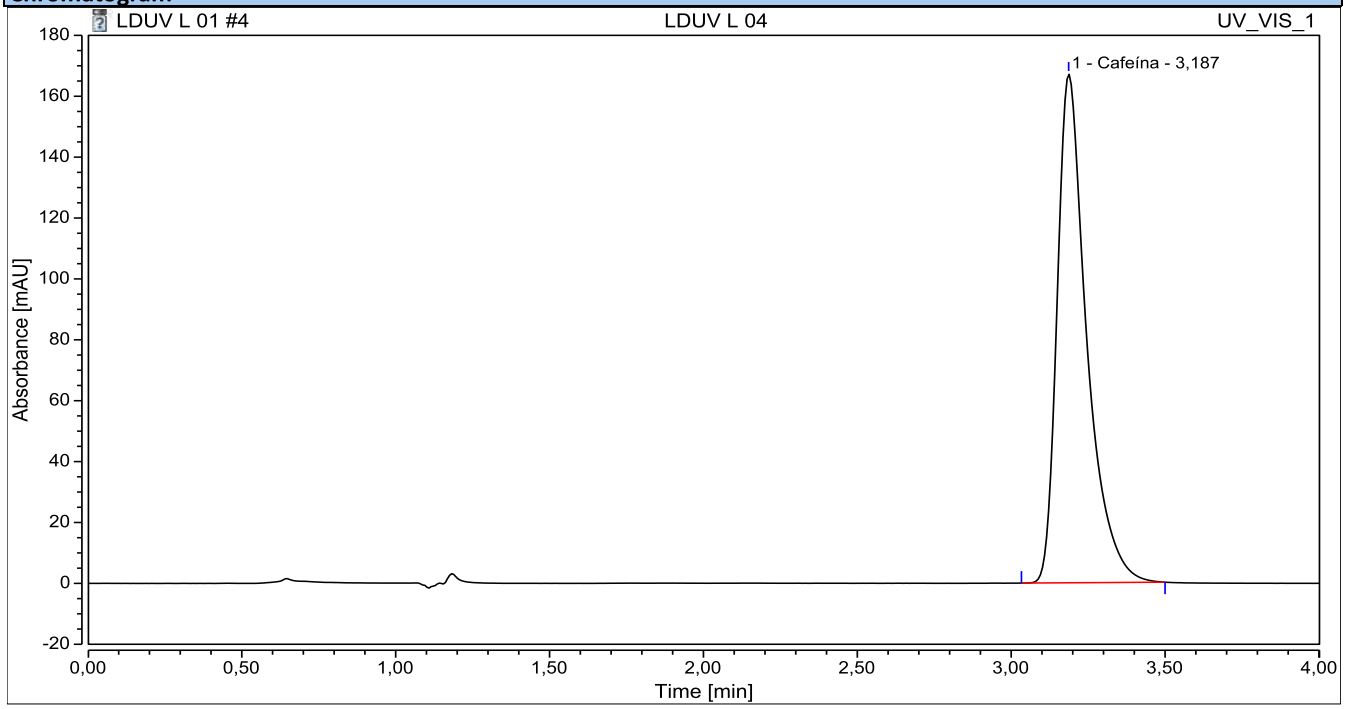

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,187	18,5872	167,121	100,00	100,00	n.a.
Total:			**18,587**	**167,121**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV L 05**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 15:38**	*Sample Weight:*	**1,0000**

Chromatogram

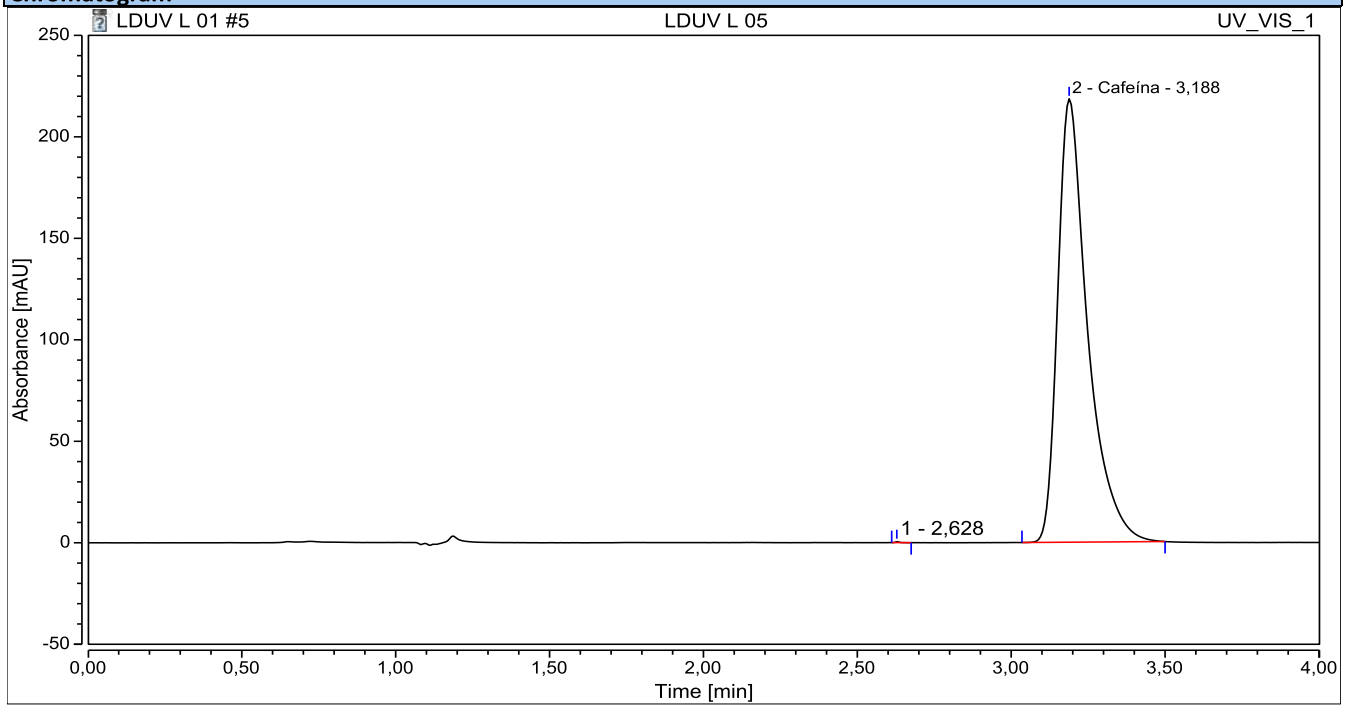

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	Cafeína	3,188	24,6078	218,483	99,97	99,78	n.a.
Total:			**24,608**	**218,483**	**99,971**	**99,777**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 16:11**	*Sample Weight:*	**1,0000**

Chromatogram

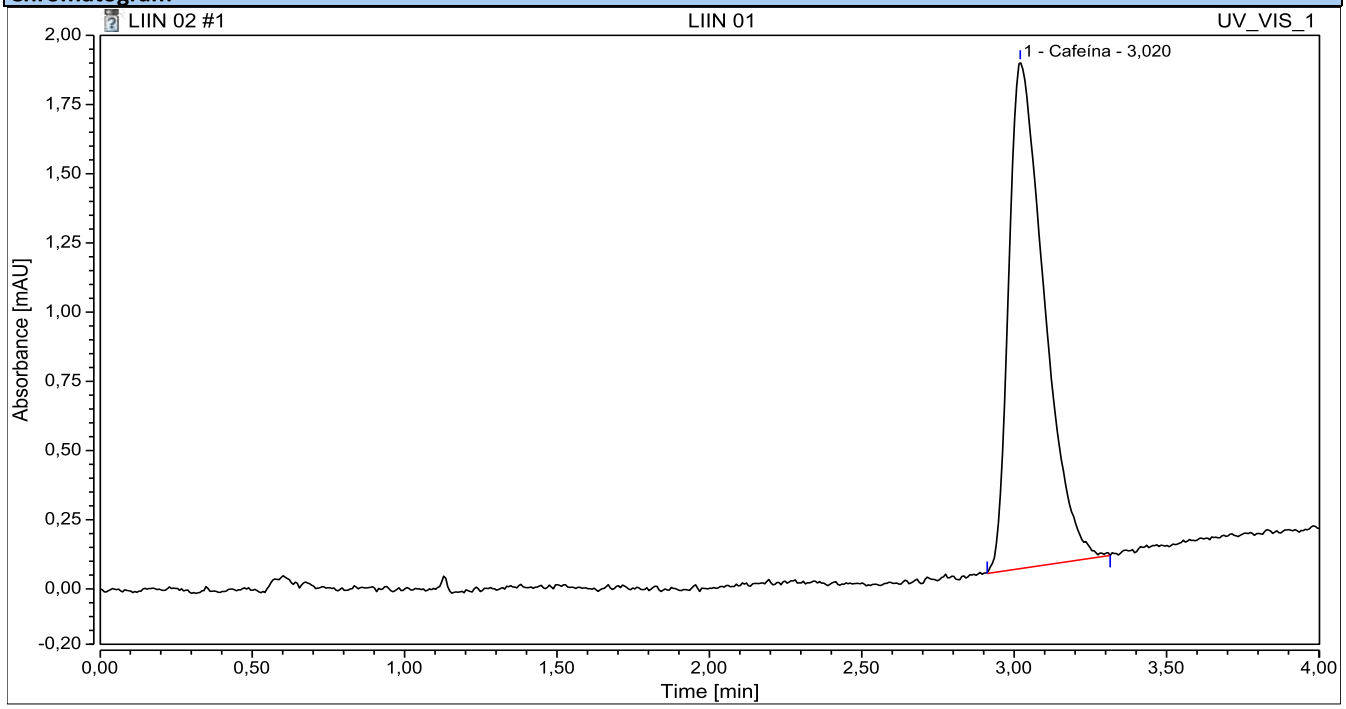

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,020	0,2466	1,829	100,00	100,00	n.a.
Total:			**0,247**	**1,829**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 16:16**	*Sample Weight:*	**1,0000**

Chromatogram

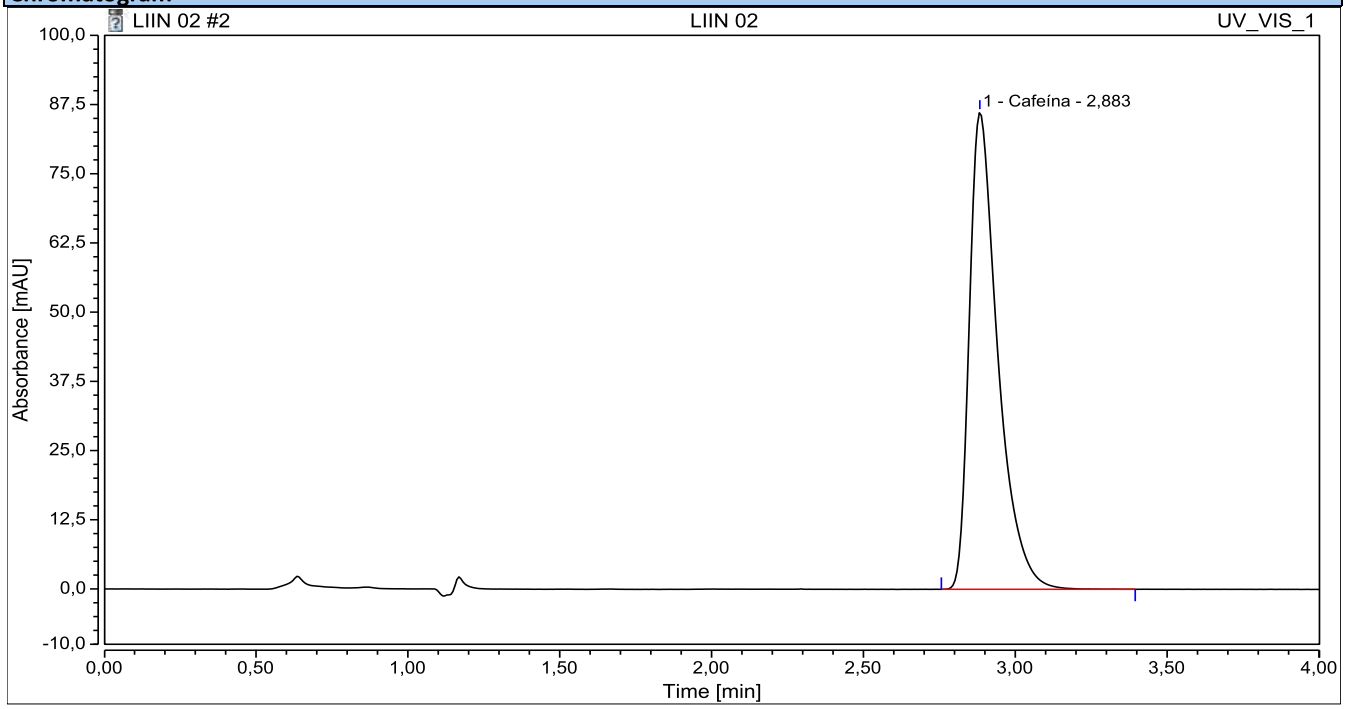

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,883	9,3748	86,198	100,00	100,00	n.a.
Total:			**9,375**	**86,198**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 16:21**	*Sample Weight:*	**1,0000**

Chromatogram

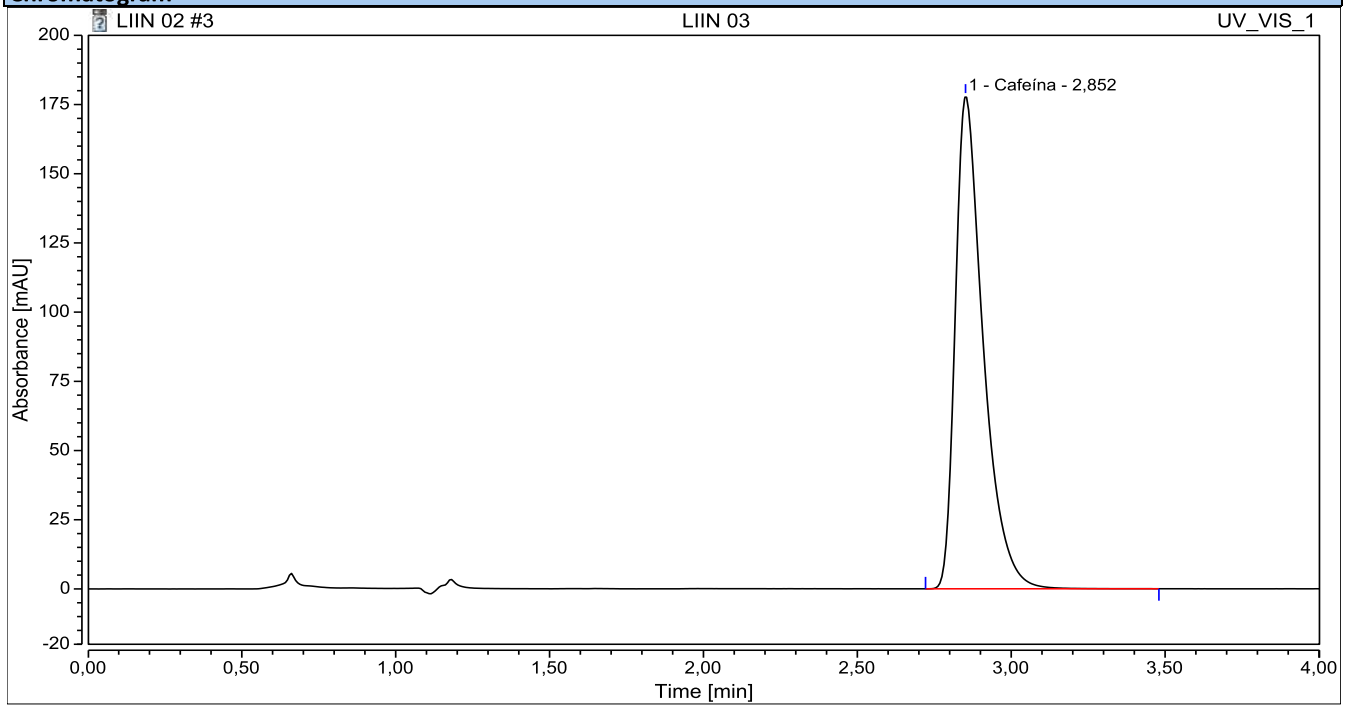

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,852	18,7380	178,023	100,00	100,00	n.a.
Total:			**18,738**	**178,023**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 16:26**	*Sample Weight:*	**1,0000**

Chromatogram

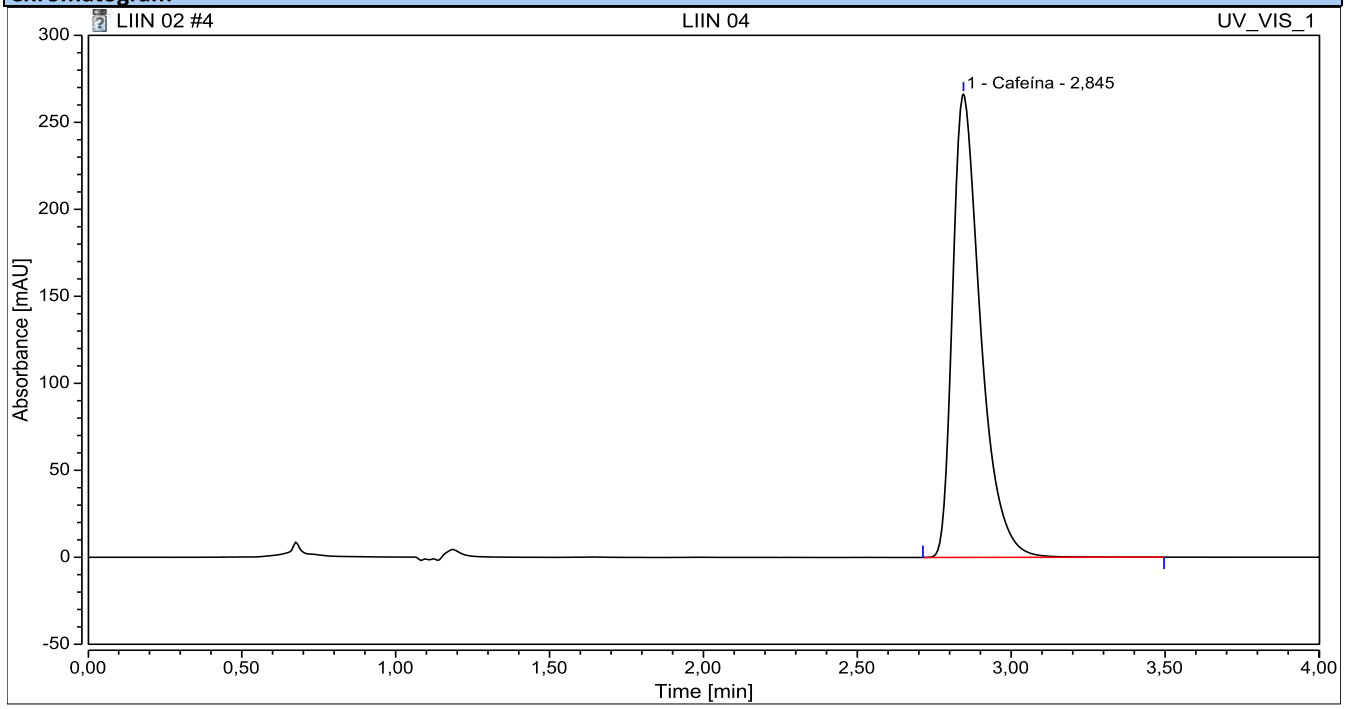

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,845	28,0584	266,299	100,00	100,00	n.a.
Total:			**28,058**	**266,299**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Left**	*Bandwidth:*	**4**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/fev/26 16:32**	*Sample Weight:*	**1,0000**

Chromatogram

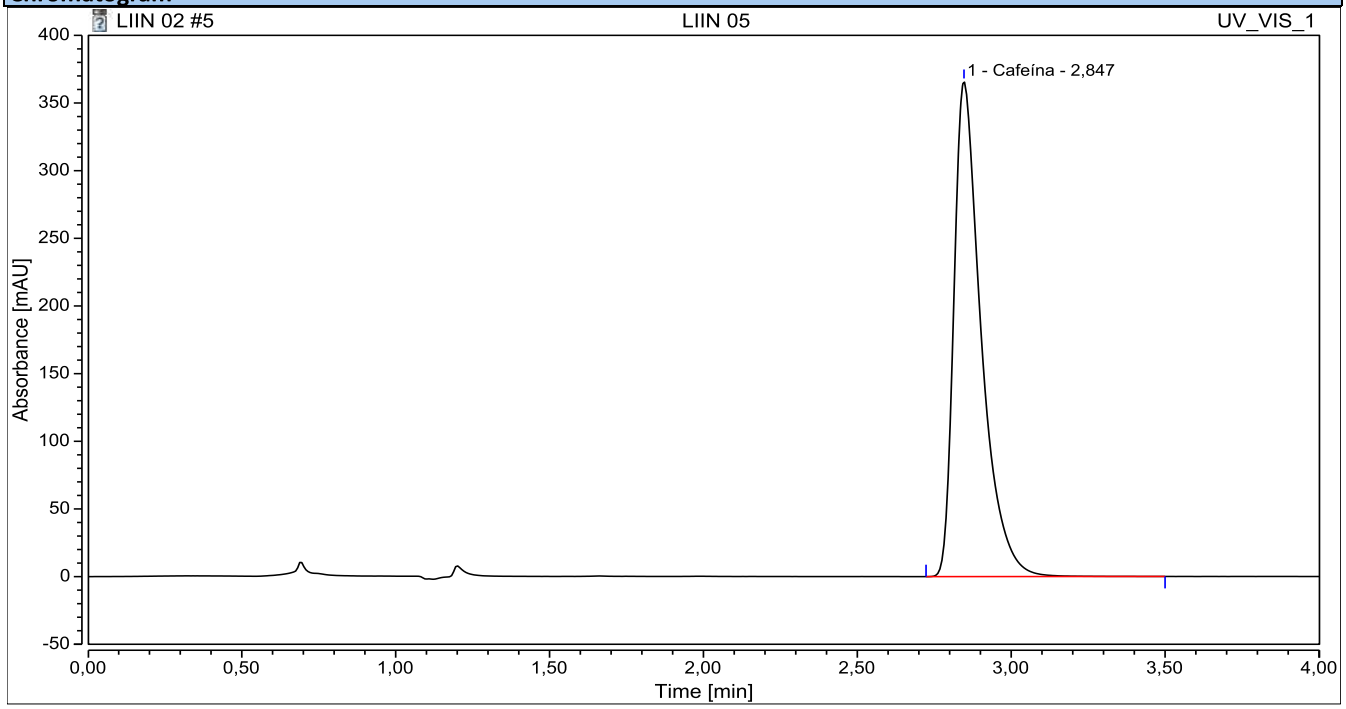


Integration Results


No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,847	37,5062	365,948	100,00	100,00	n.a.
Total:			**37,506**	**365,948**	**100,000**	**100,000**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Contour Spectral View

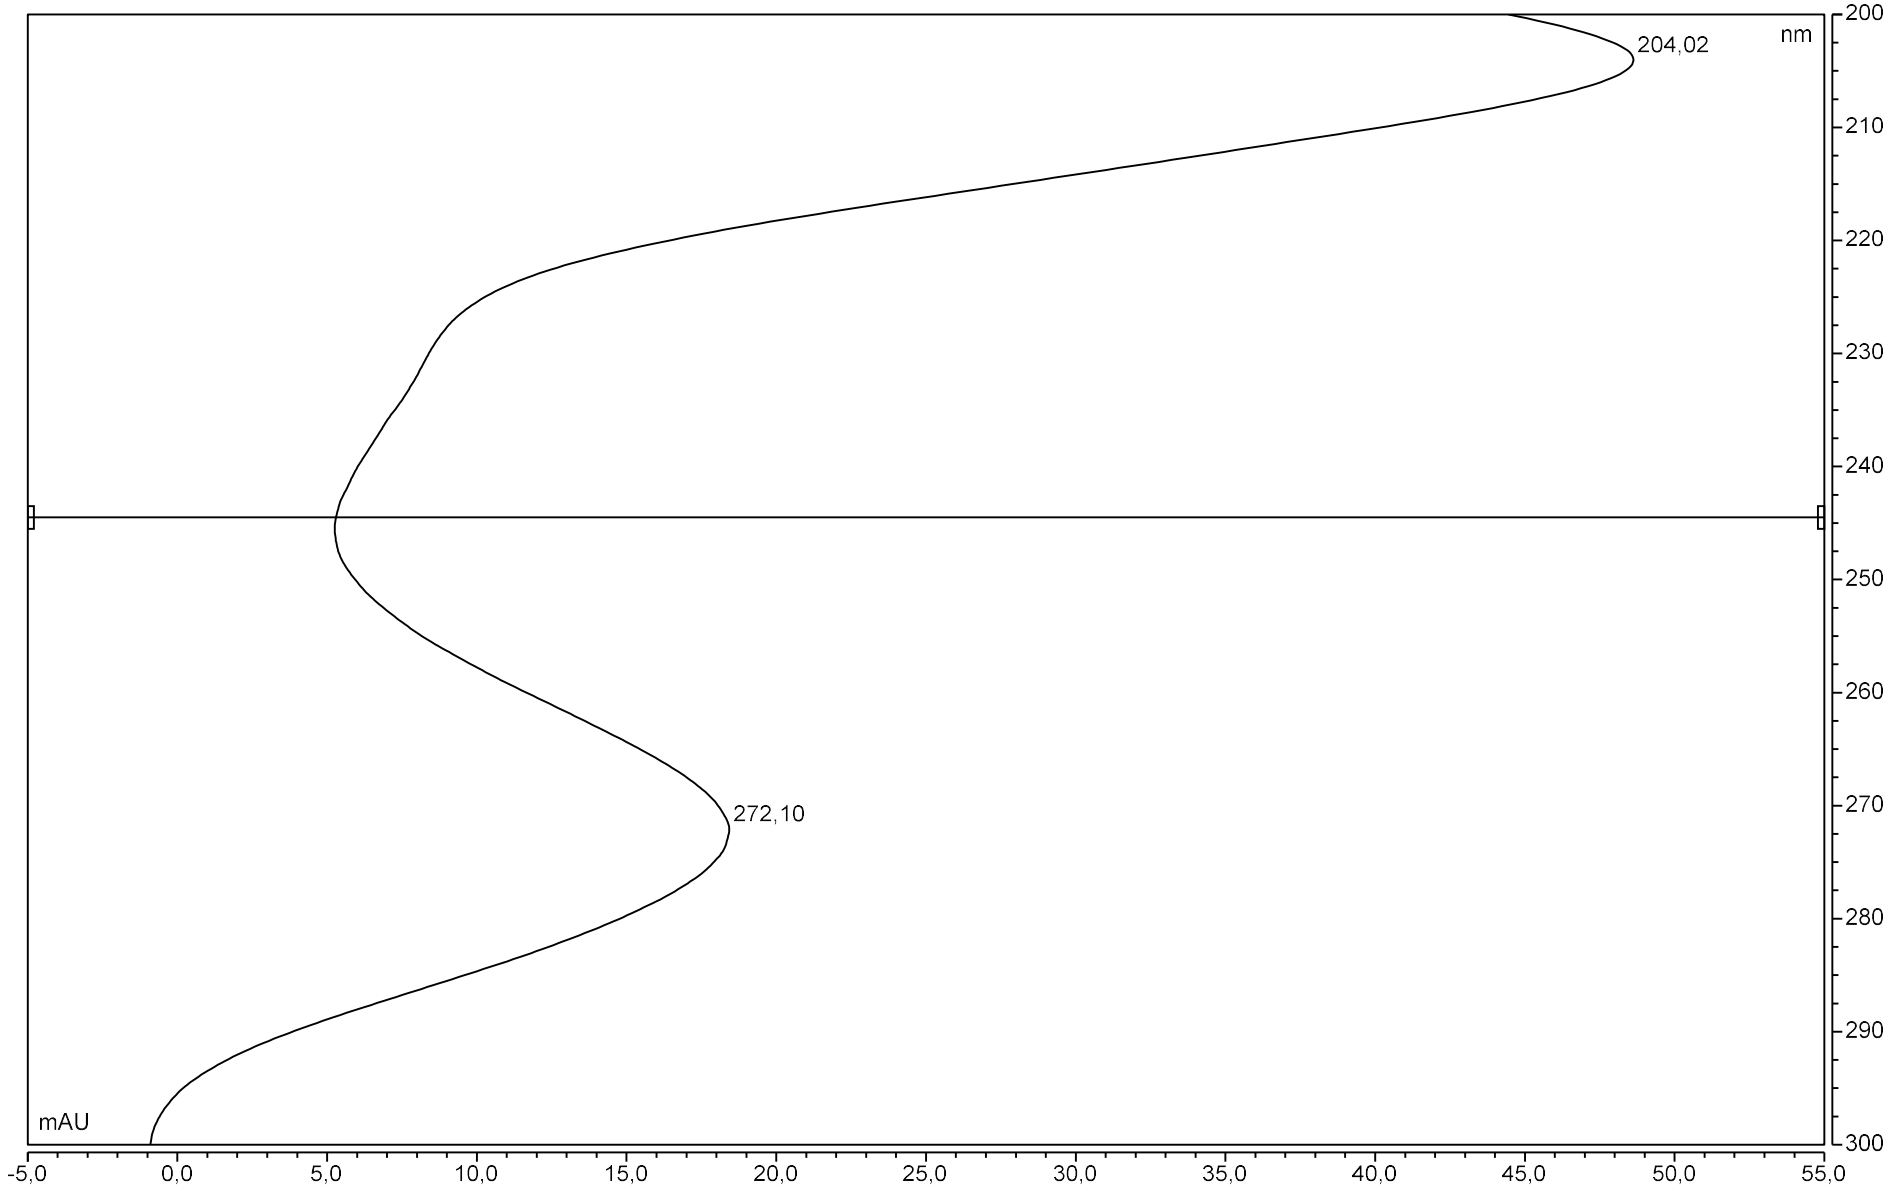

Contour Spectral View

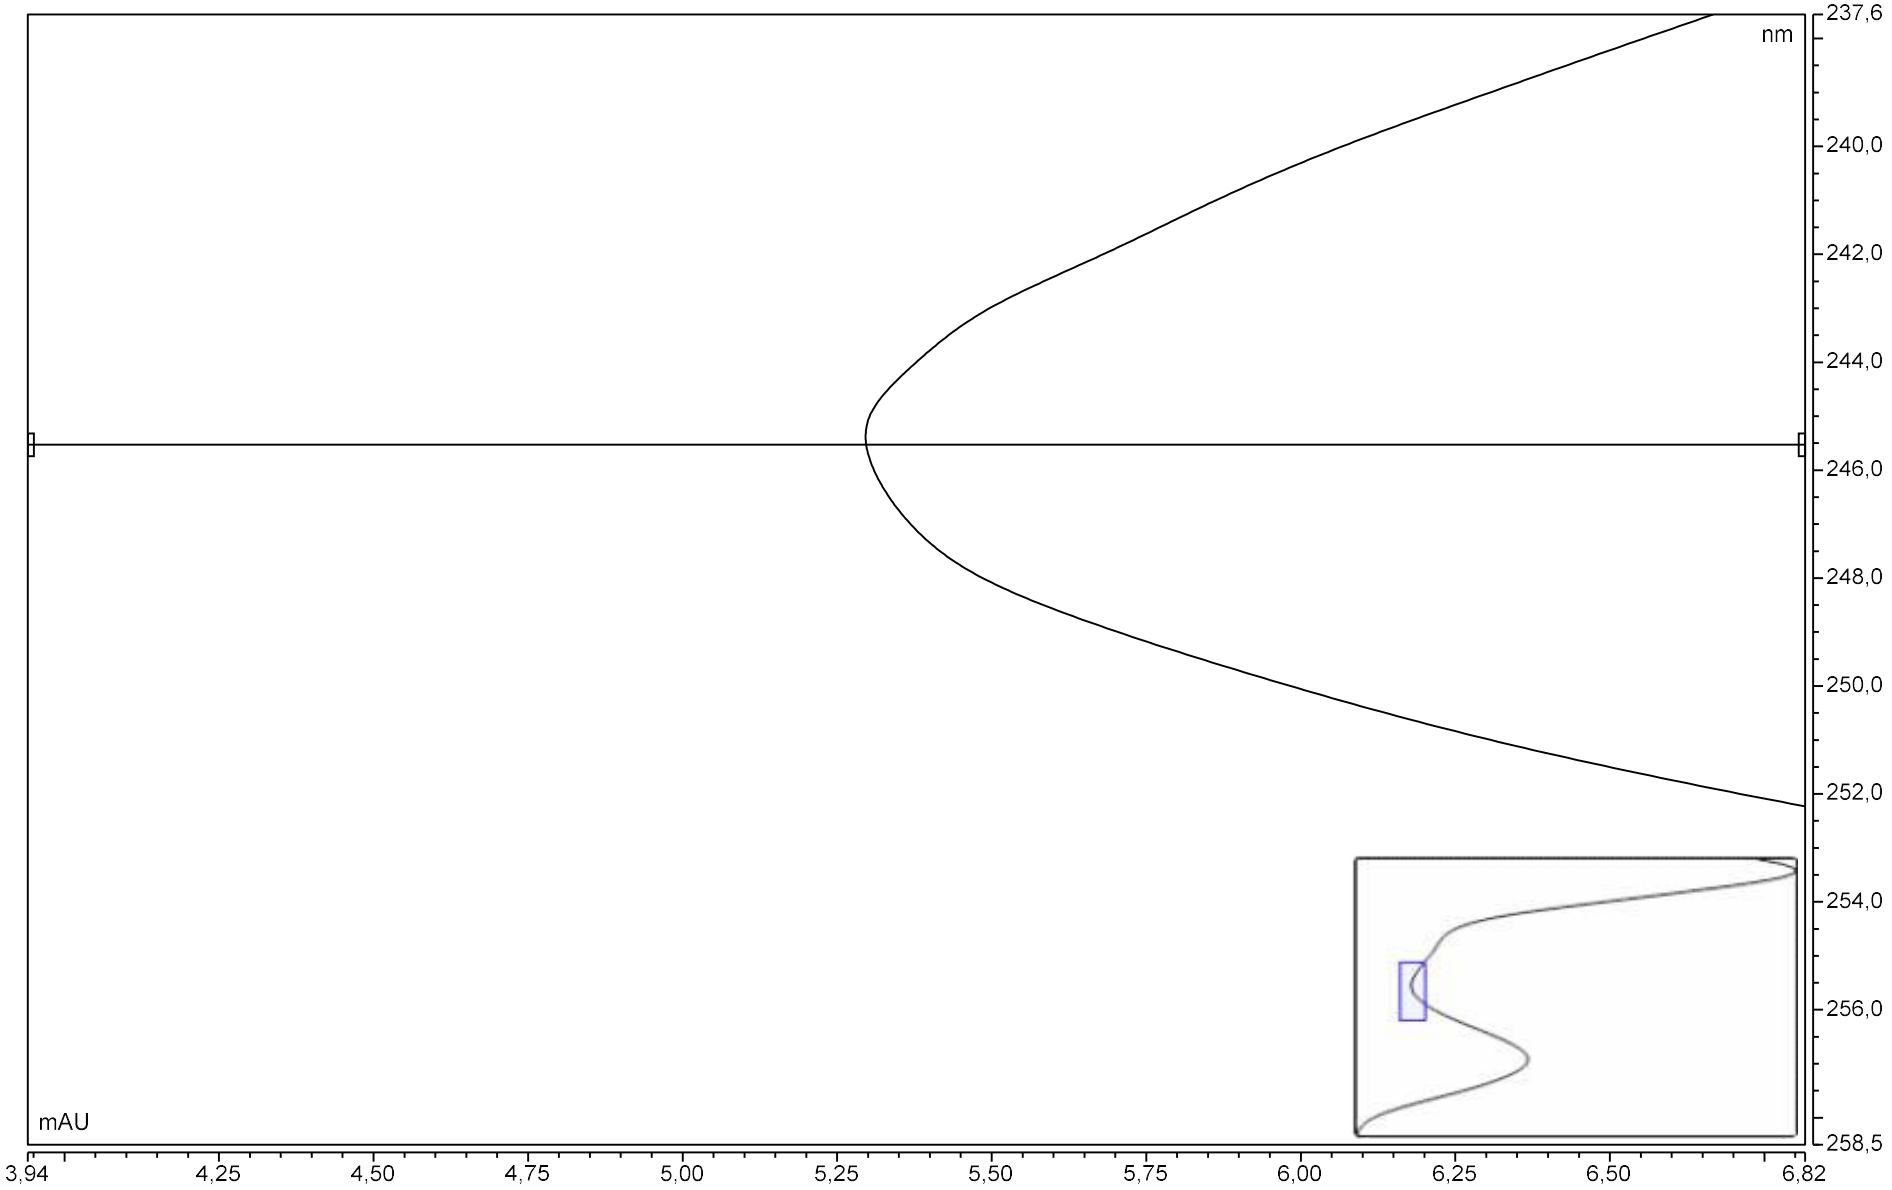


Chromatogram and Results

Injection Details

Injection Name:	**RELB Right**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 08:45**	*Sample Weight:*	**1,0000**

Chromatogram

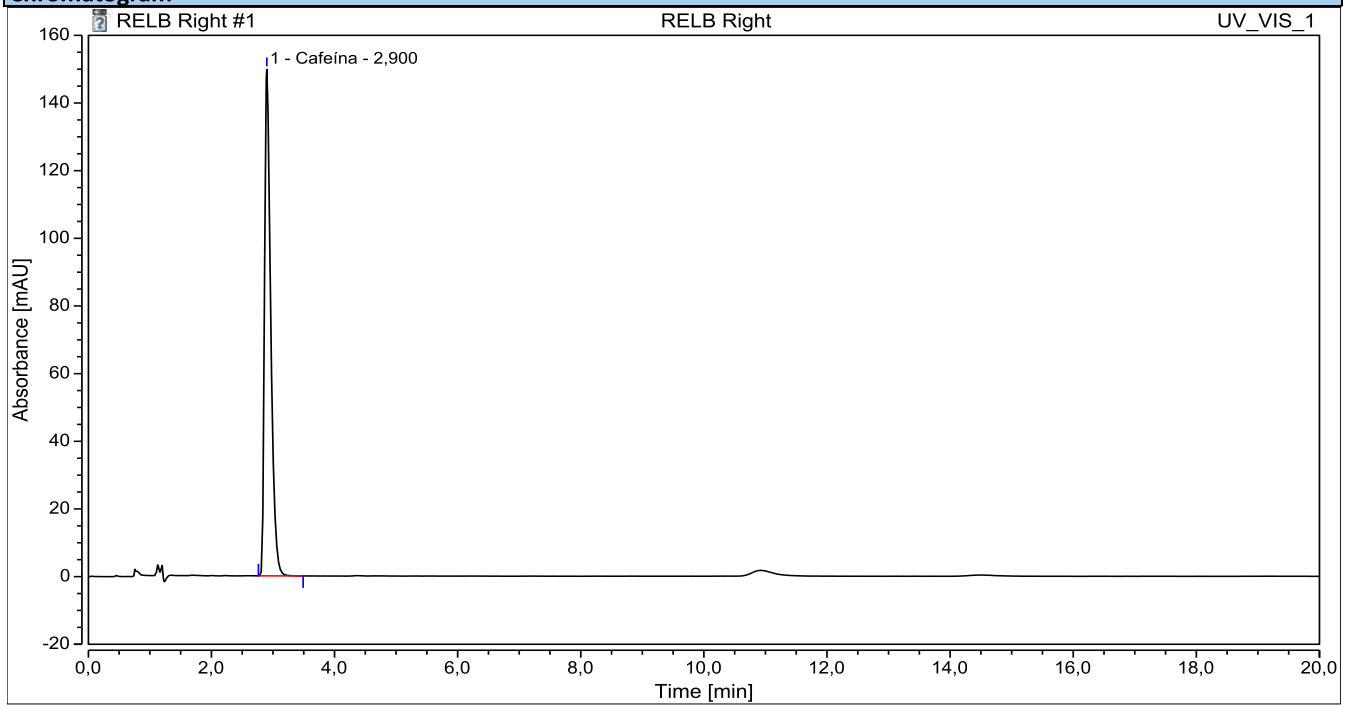

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,900	17,4842	149,743	100,00	100,00	n.a.
Total:			**17,484**	**149,743**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 08:45**	*Sample Weight:*	**1,0000**

Chromatogram

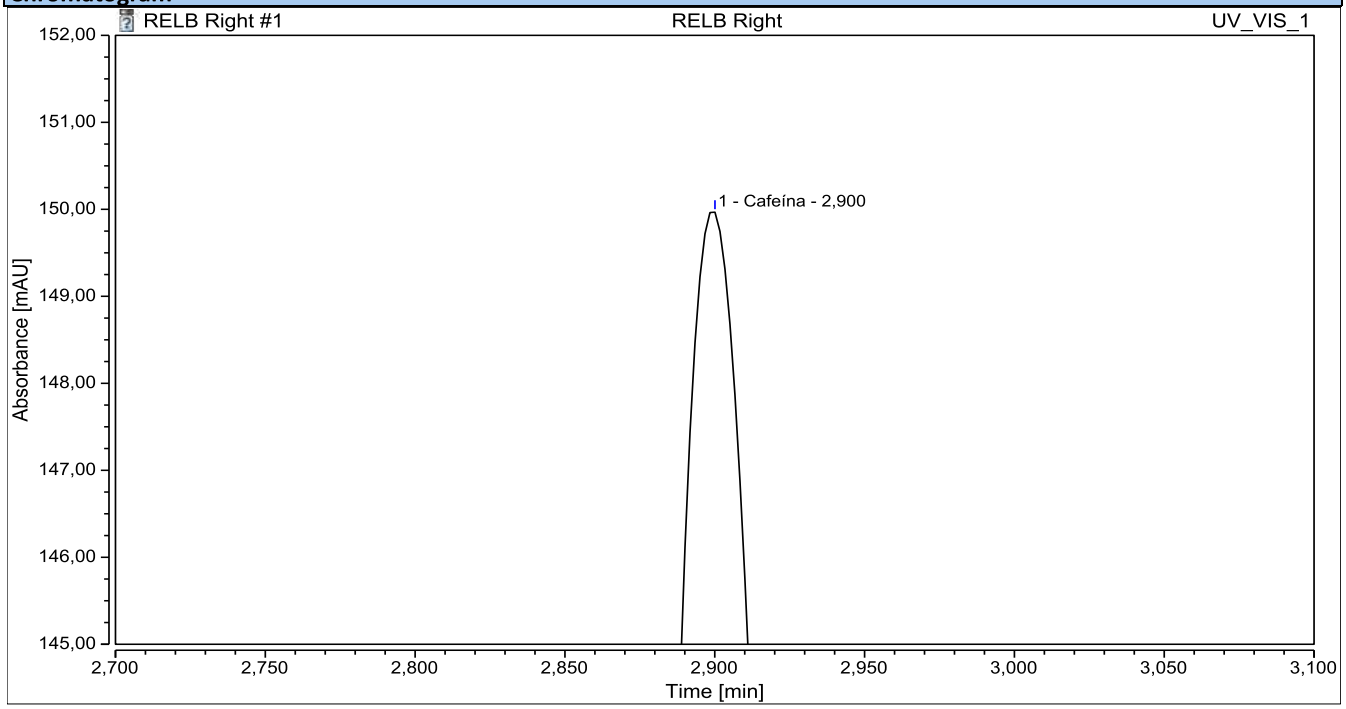

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,900	17,4842	149,743	100,00	100,00	n.a.
Total:			**17,484**	**149,743**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 08:45**	*Sample Weight:*	**1,0000**

Chromatogram

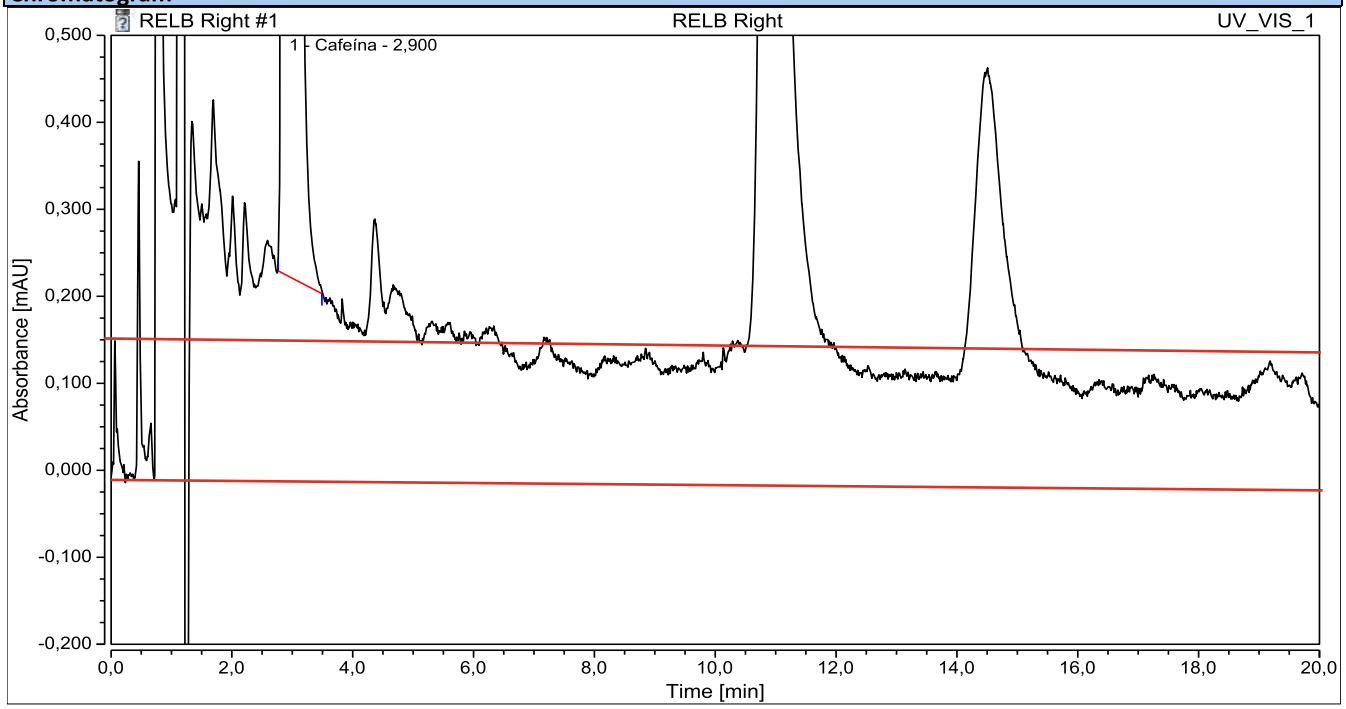

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,900	17,4842	149,743	100,00	100,00	n.a.
Total:			**17,484**	**149,743**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 08:45**	*Sample Weight:*	**1,0000**

Chromatogram

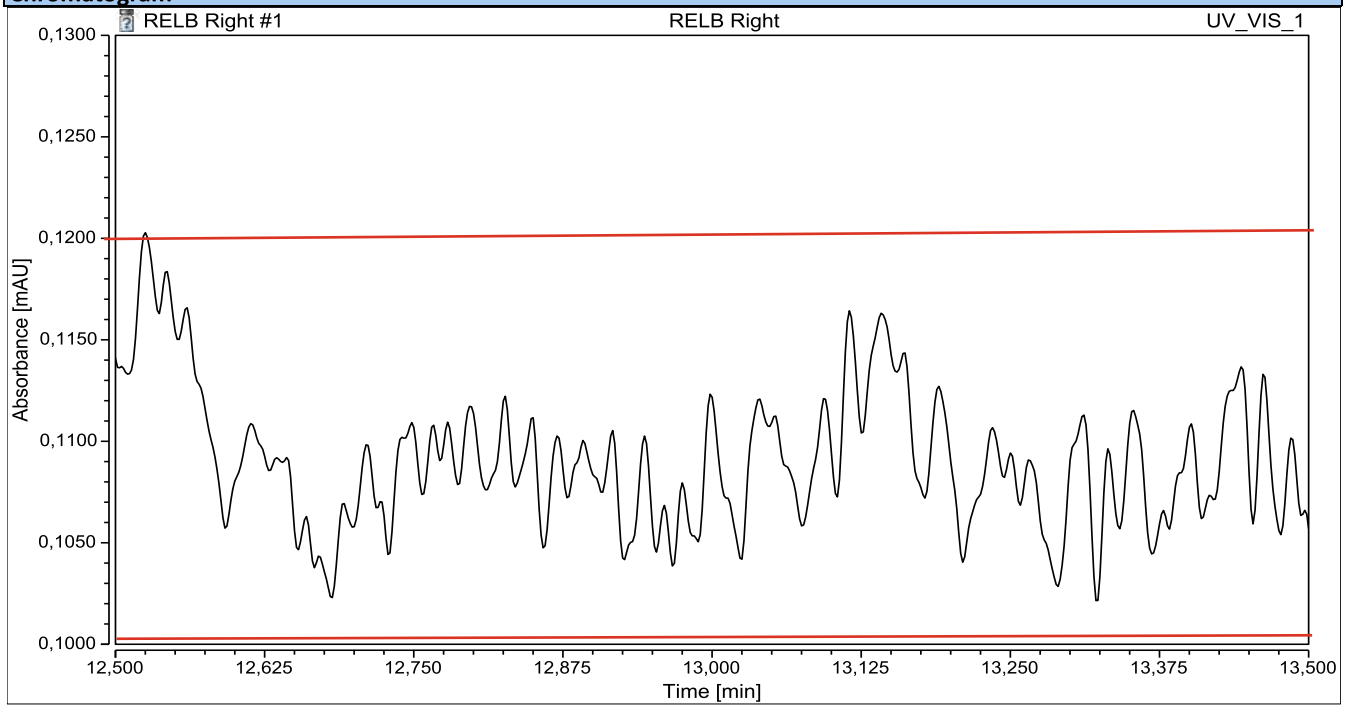

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,900	17,4842	149,743	100,00	100,00	n.a.
Total:			**17,484**	**149,743**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 01**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 10:09**	*Sample Weight:*	**1,0000**

Chromatogram

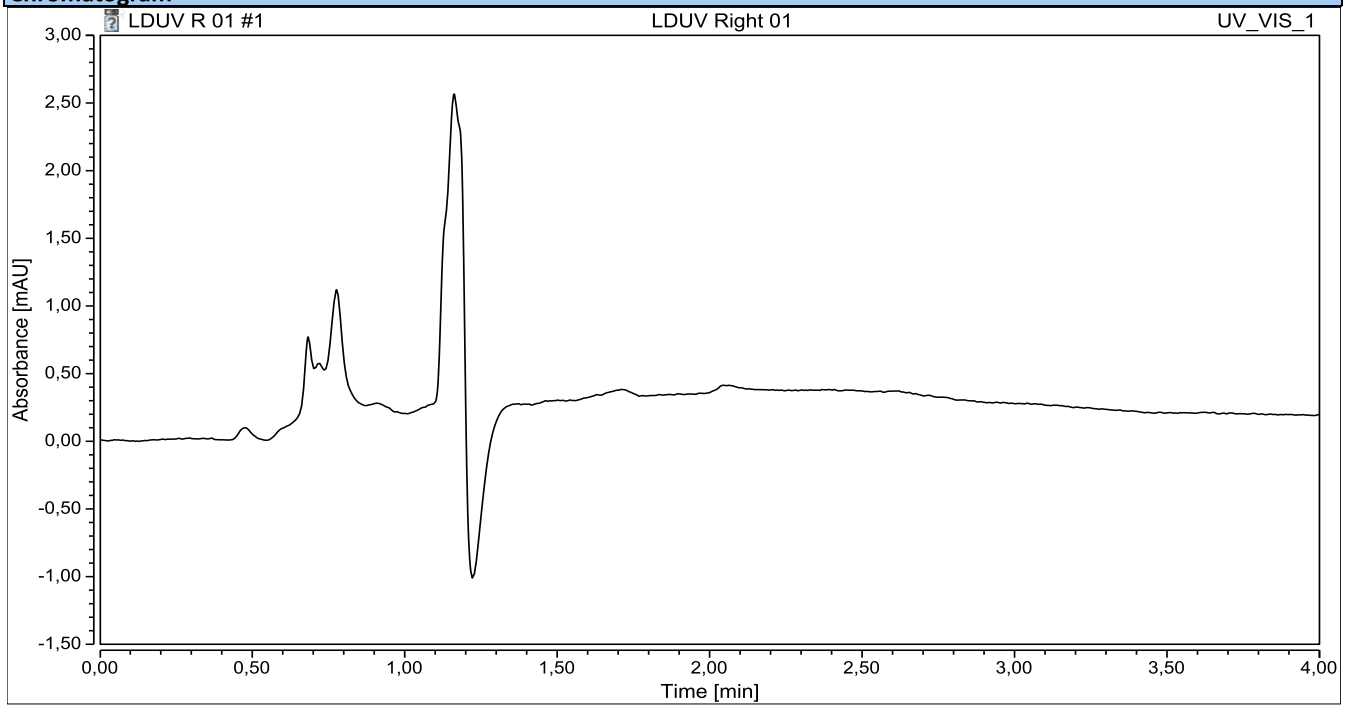

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 02**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 10:14**	*Sample Weight:*	**1,0000**

Chromatogram

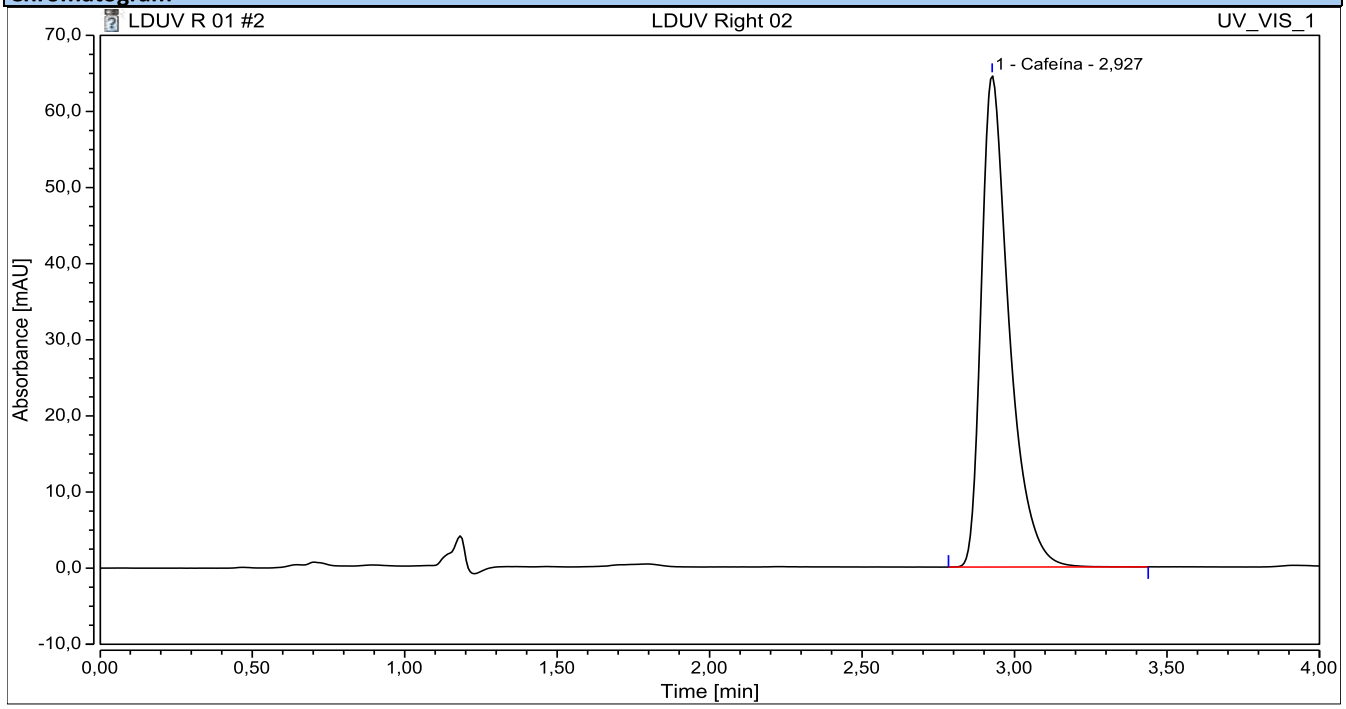

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,927	6,8649	64,608	100,00	100,00	n.a.
Total:			**6,865**	**64,608**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 03**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 10:19**	*Sample Weight:*	**1,0000**

Chromatogram

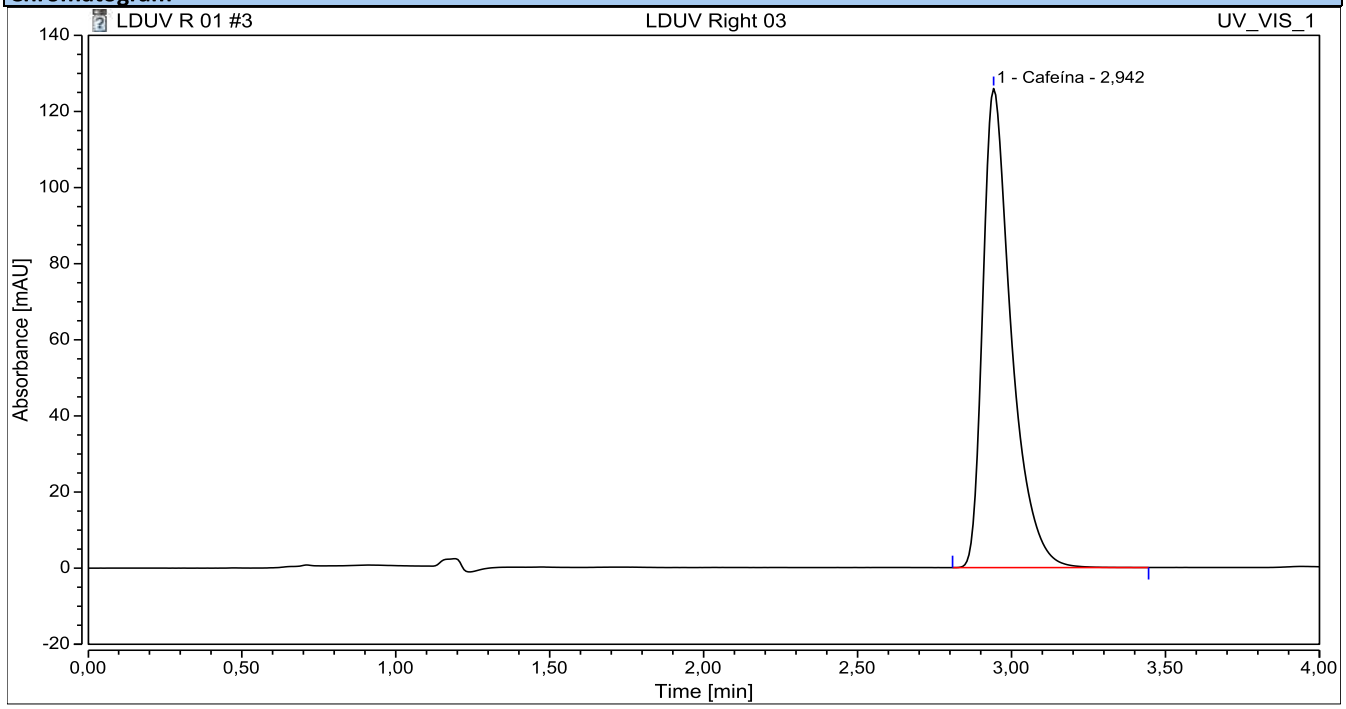

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,942	13,5098	125,897	100,00	100,00	n.a.
Total:			**13,510**	**125,897**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 04**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 10:24**	*Sample Weight:*	**1,0000**

Chromatogram

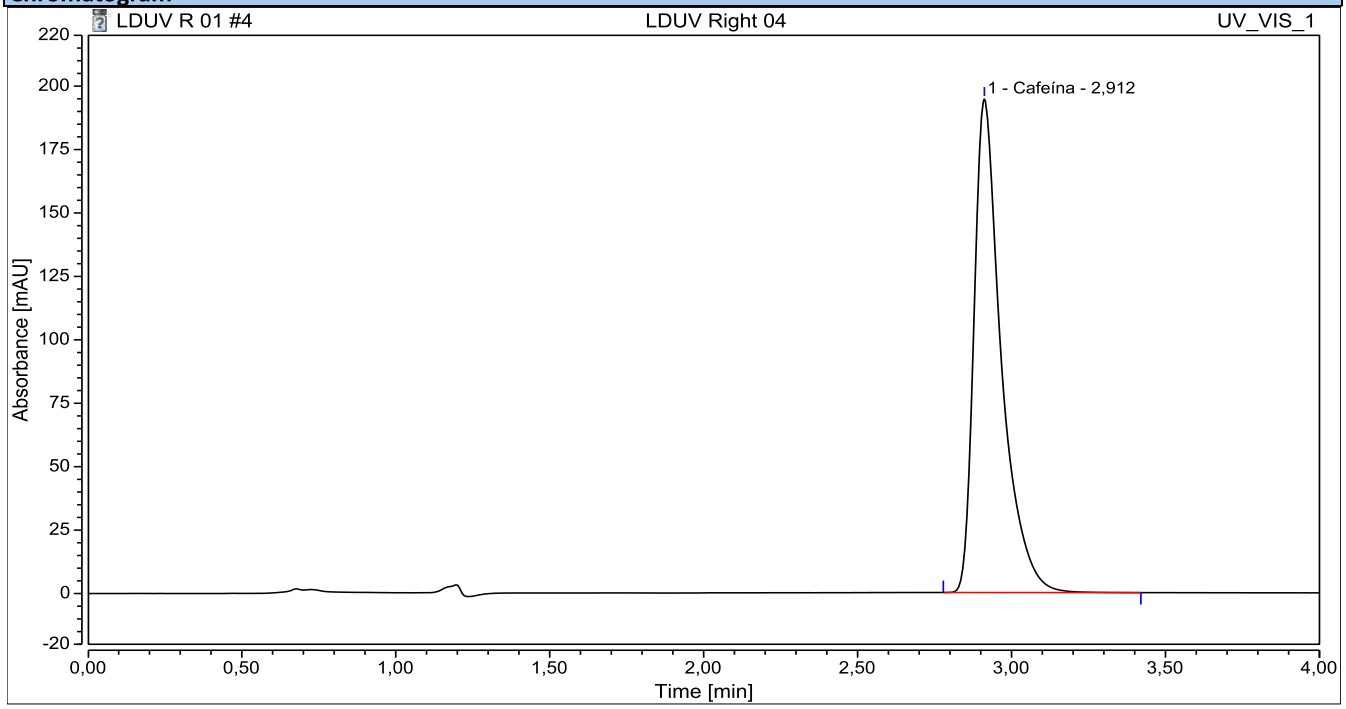

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,912	19,9418	194,500	100,00	100,00	n.a.
Total:			**19,942**	**194,500**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 05**	*Run Time (min):*	**4,00**
Vial Number:	**Y:A8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação Right**	*Bandwidth:*	**n.a.**
Processing Method:	**QPack Reprocesso**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 10:29**	*Sample Weight:*	**1,0000**

Chromatogram

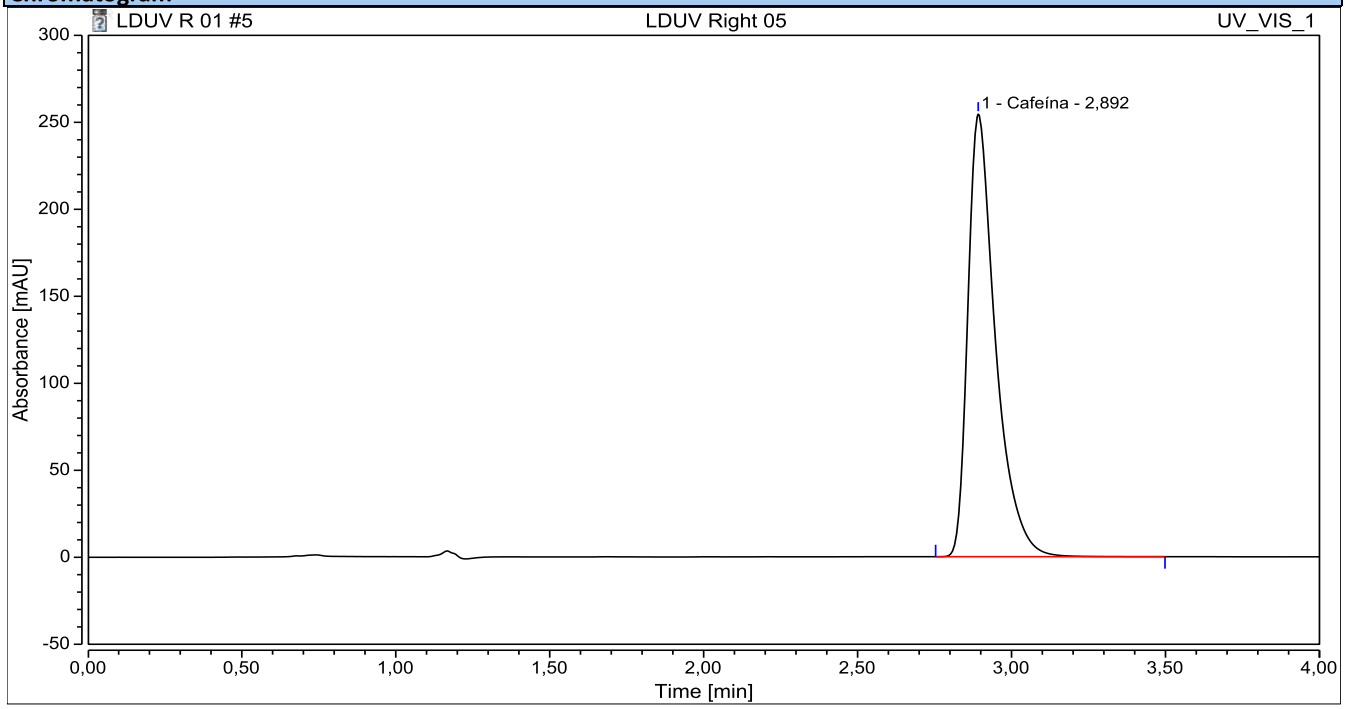

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2,892	26,4377	254,385	100,00	100,00	n.a.
Total:			**26,438**	**254,385**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB L**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB L**	*Bandwidth:*	**4**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 11:11**	*Sample Weight:*	**1,0000**

Chromatogram

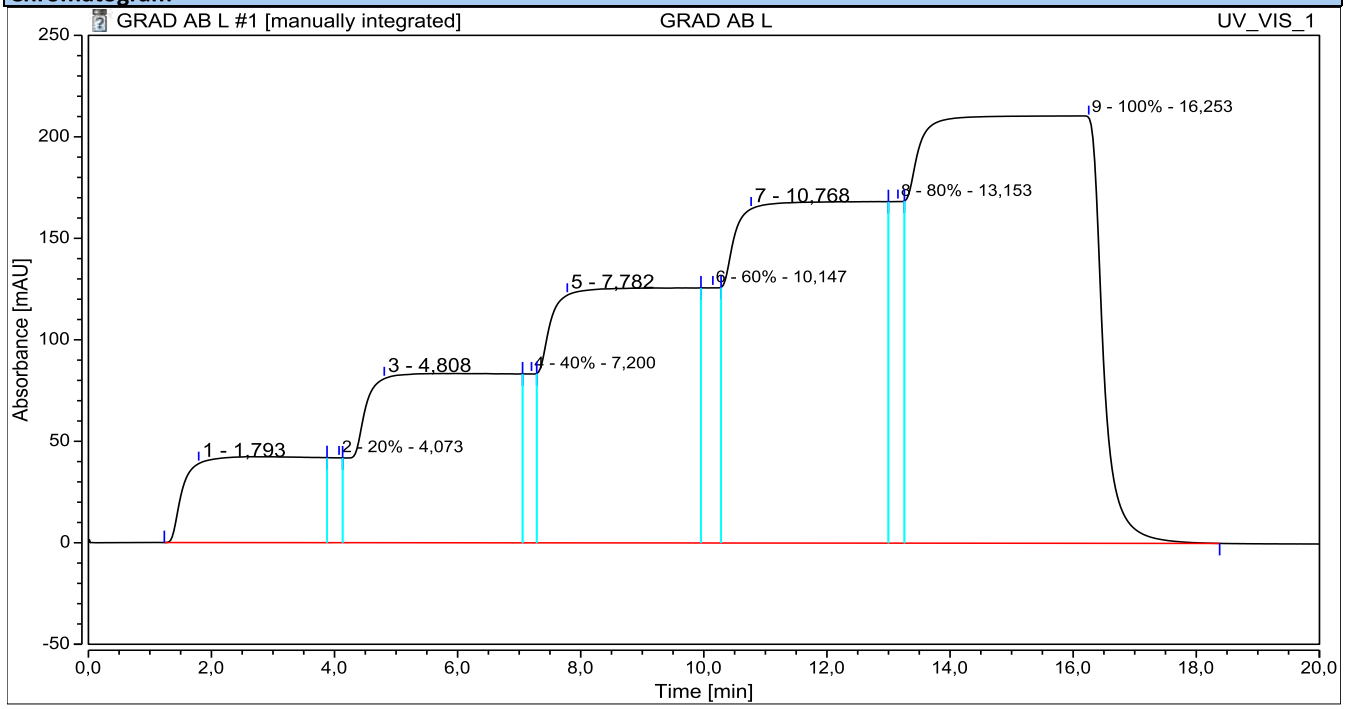

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,073	10,5945	41,802	0,56	4,04	n.a.
4	40%	7,200	19,1392	83,210	1,01	8,04	n.a.
6	60%	10,147	41,0586	125,691	2,17	12,14	n.a.
8	80%	13,153	43,7544	168,298	2,32	16,26	n.a.
9	100%	16,253	676,1843	209,743	35,80	20,26	n.a.
Total:			**790,731**	**628,743**	**41,860**	**60,745**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AC L**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AC L**	*Bandwidth:*	**4**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 11:58**	*Sample Weight:*	**1,0000**

Chromatogram

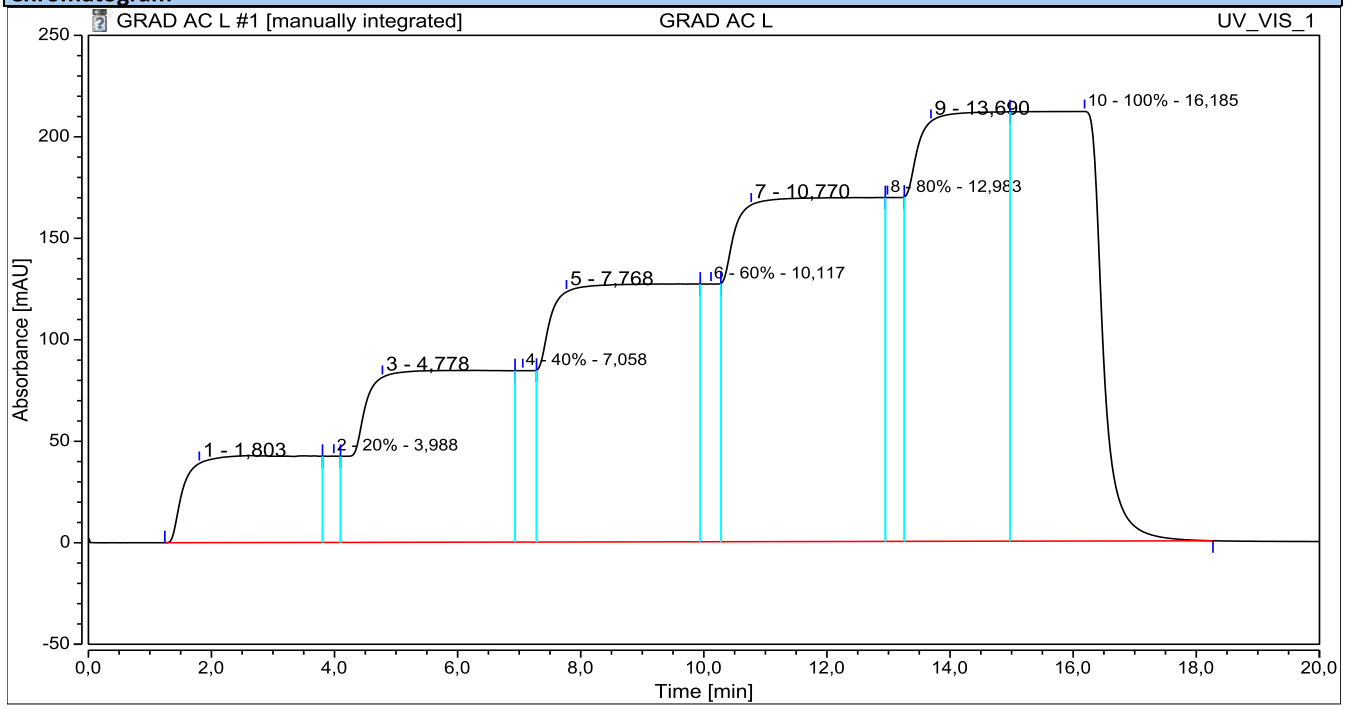

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	3,988	12,3887	42,508	0,65	3,40	n.a.
4	40%	7,058	29,4181	84,465	1,54	6,75	n.a.
6	60%	10,117	42,5312	126,966	2,23	10,15	n.a.
8	80%	12,983	52,2312	169,406	2,74	13,54	n.a.
10	100%	16,185	327,3369	211,623	17,18	16,91	n.a.
Total:			**463,906**	**634,969**	**24,350**	**50,748**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AC R**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AC R**	*Bandwidth:*	**n.a.**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 13:15**	*Sample Weight:*	**1,0000**

Chromatogram

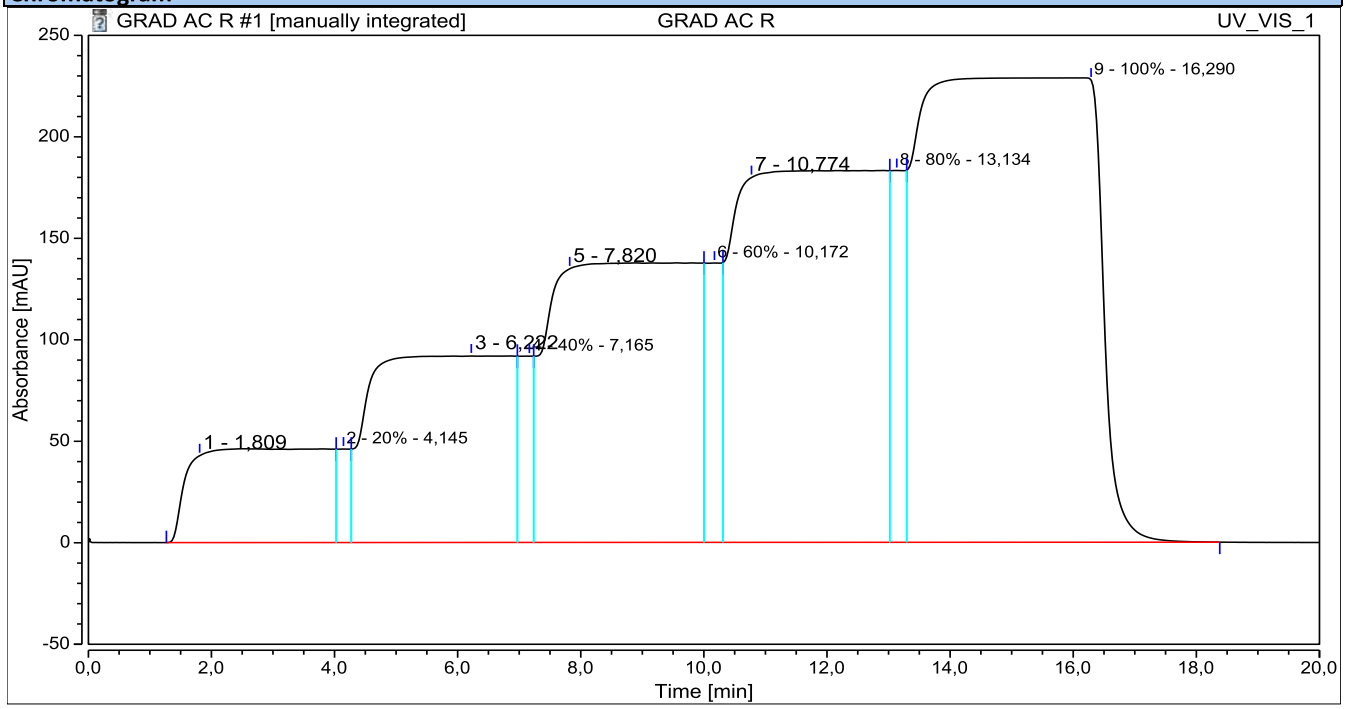

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,145	11,2748	46,062	0,55	4,06	n.a.
4	40%	7,165	24,3195	91,794	1,18	8,08	n.a.
6	60%	10,172	42,4249	137,636	2,06	12,12	n.a.
8	80%	13,134	50,3636	183,188	2,44	16,13	n.a.
9	100%	16,290	731,7791	227,737	35,48	20,05	n.a.
Total:			**860,162**	**686,417**	**41,707**	**60,442**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB R**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB R**	*Bandwidth:*	**n.a.**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/fev/26 12:43**	*Sample Weight:*	**1,0000**

Chromatogram

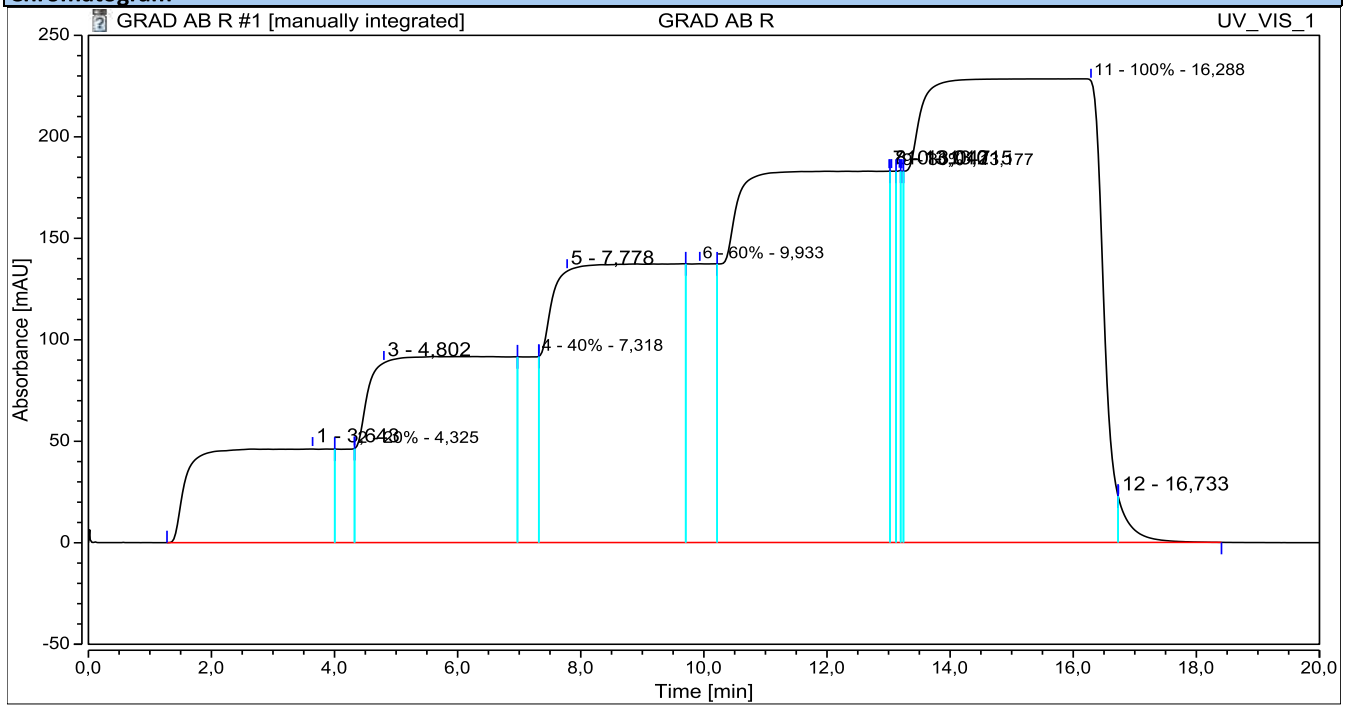

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,325	14,8091	46,338	0,72	3,04	n.a.
4	40%	7,318	31,7127	91,719	1,54	6,01	n.a.
6	60%	9,933	70,0021	137,304	3,40	9,00	n.a.
9	80%	13,177	13,7211	183,178	0,67	12,01	n.a.
11	100%	16,288	735,5168	227,461	35,74	14,91	n.a.
Total:			**865,762**	**686,000**	**42,073**	**44,970**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.