
Peak Find - EDUV PDA_1,2100.JWS

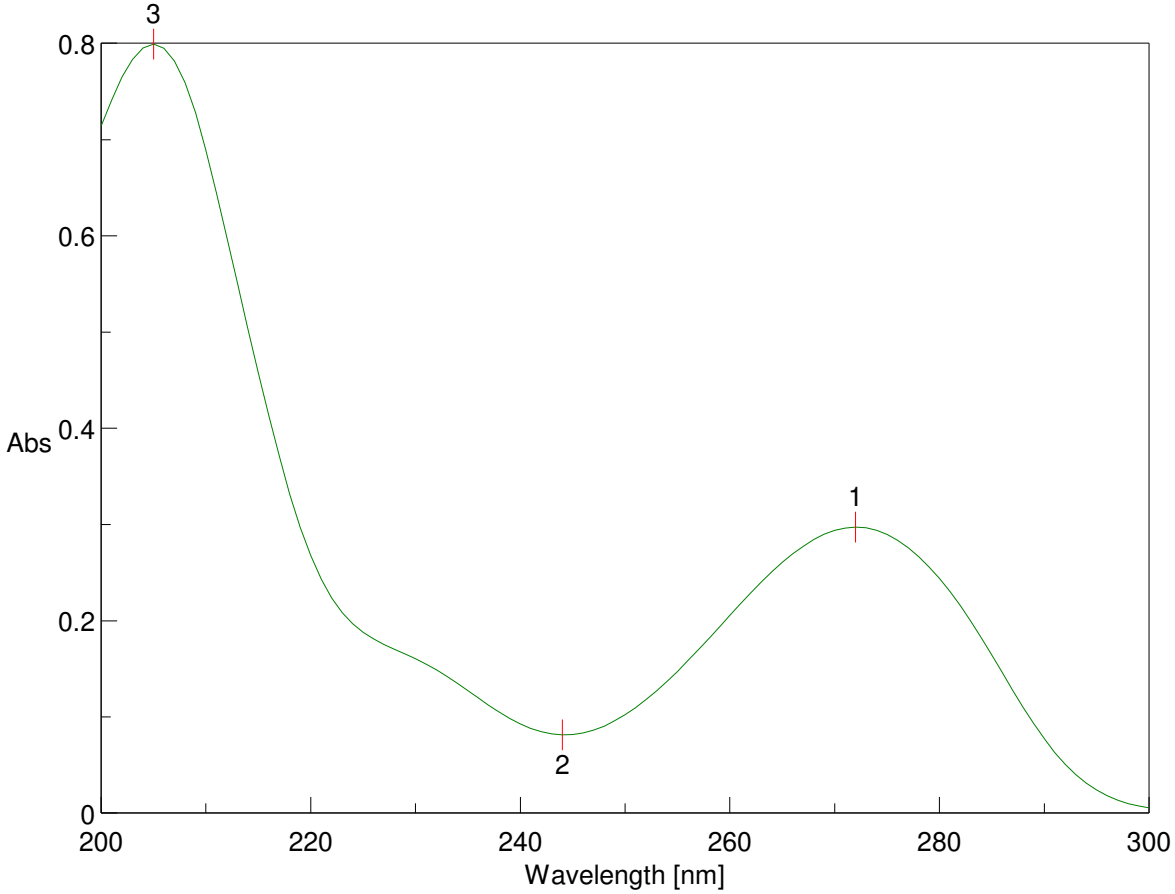

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	19/02/2026 11:37

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.297155	2	244	0.081025
3	205	0.799097			

Chromatogram

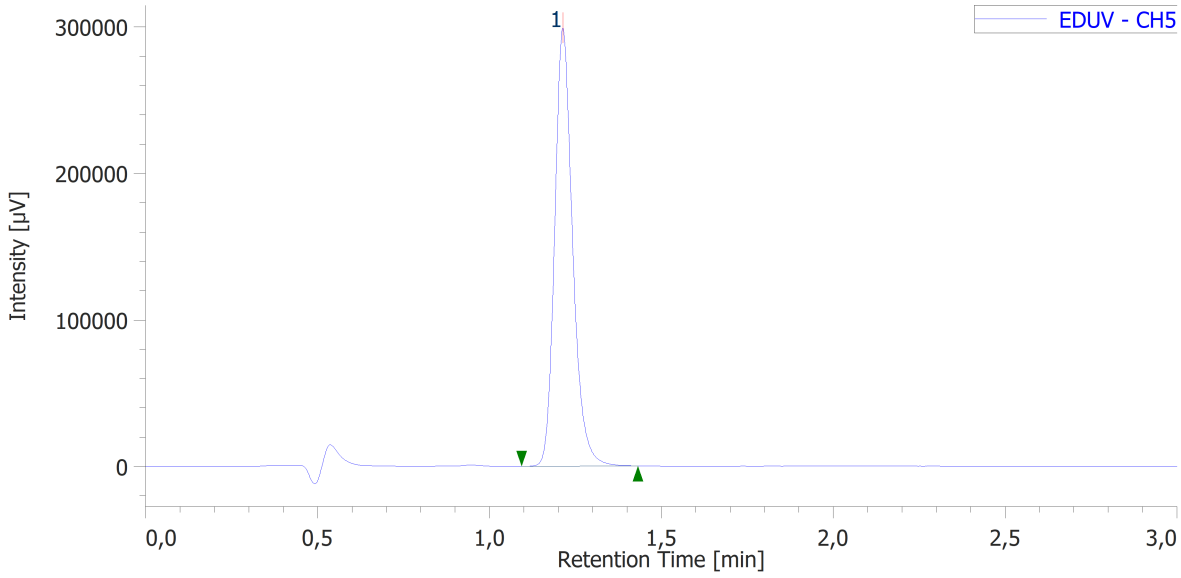

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:40:10
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:37:07
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	EDUV-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,213	1085433	298971	100,000	100,000	N/A	2788	N/A	1,222		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

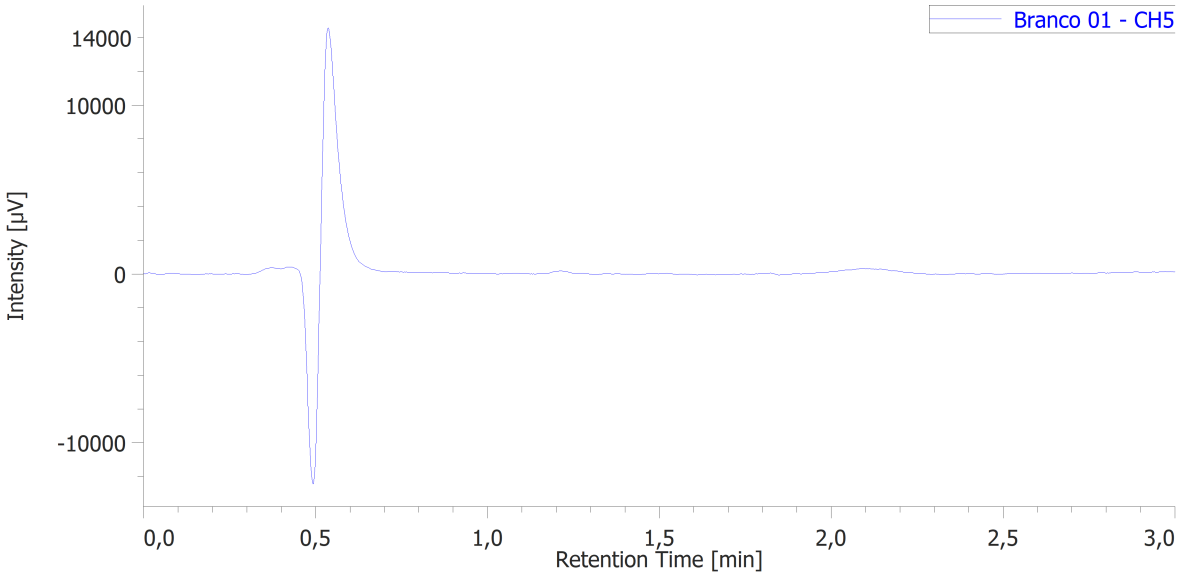


Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:43:22
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:40:19
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

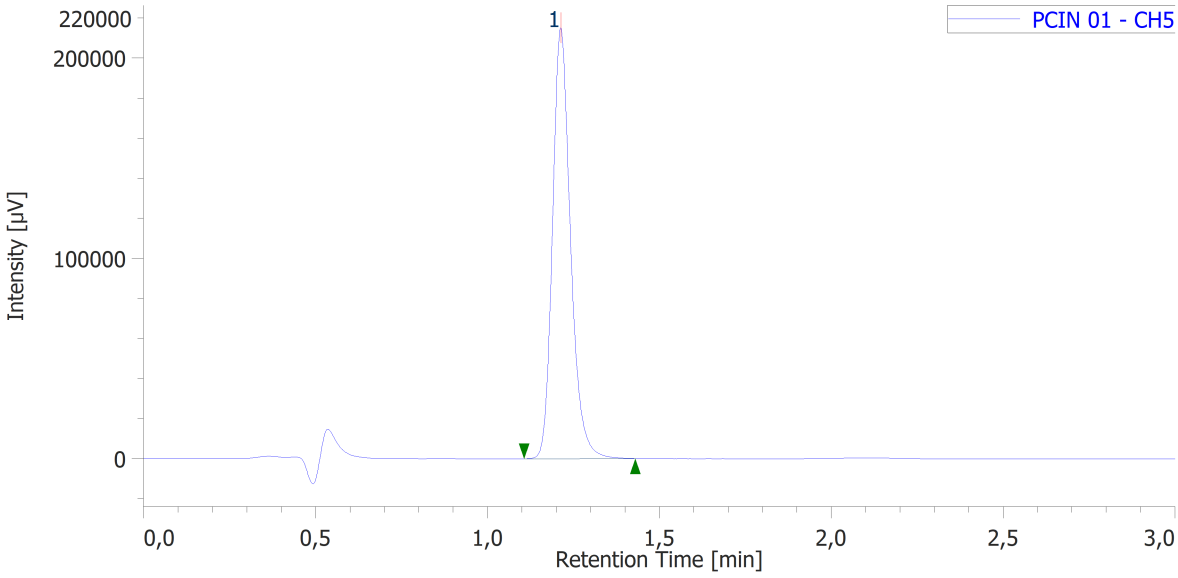

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:46:34
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:43:31
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,213	783416	214904	100,000	100,000	N/A	2760	N/A	1,213		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

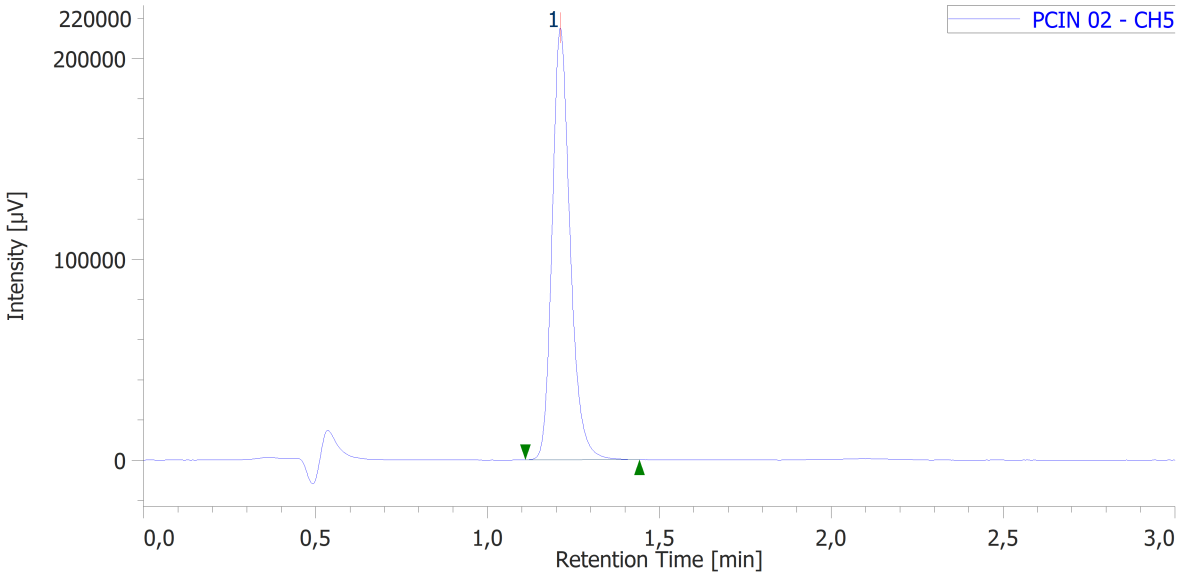

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:49:46
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:46:43
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,212	782547	214988	100,000	100,000	N/A	2765	N/A	1,232		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

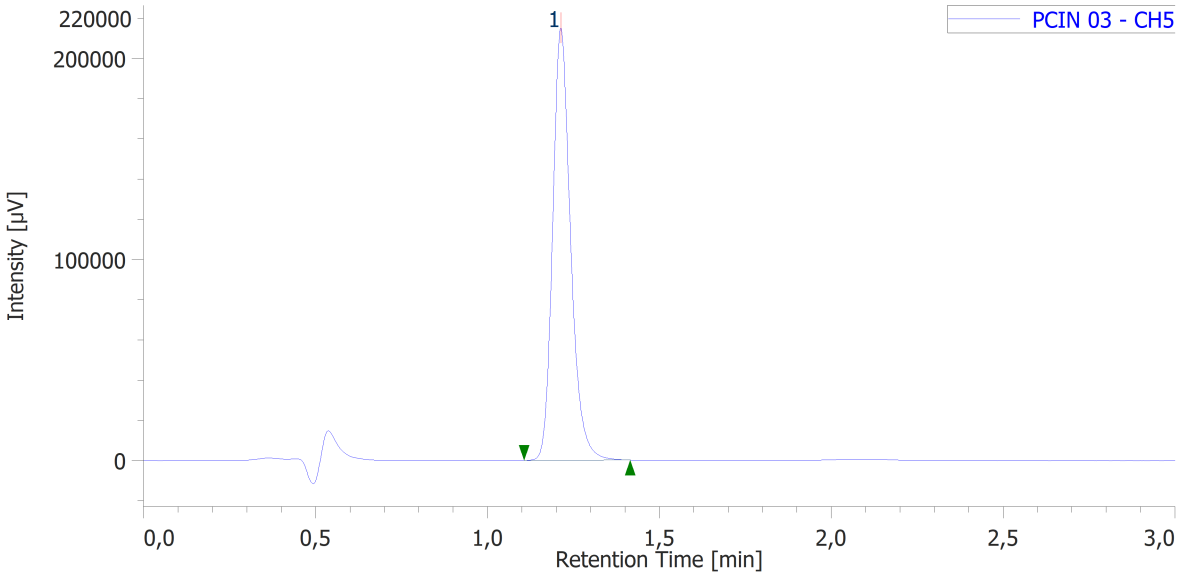

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:52:58
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:49:56
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,213	780975	214868	100,000	100,000	N/A	2777	N/A	1,222		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

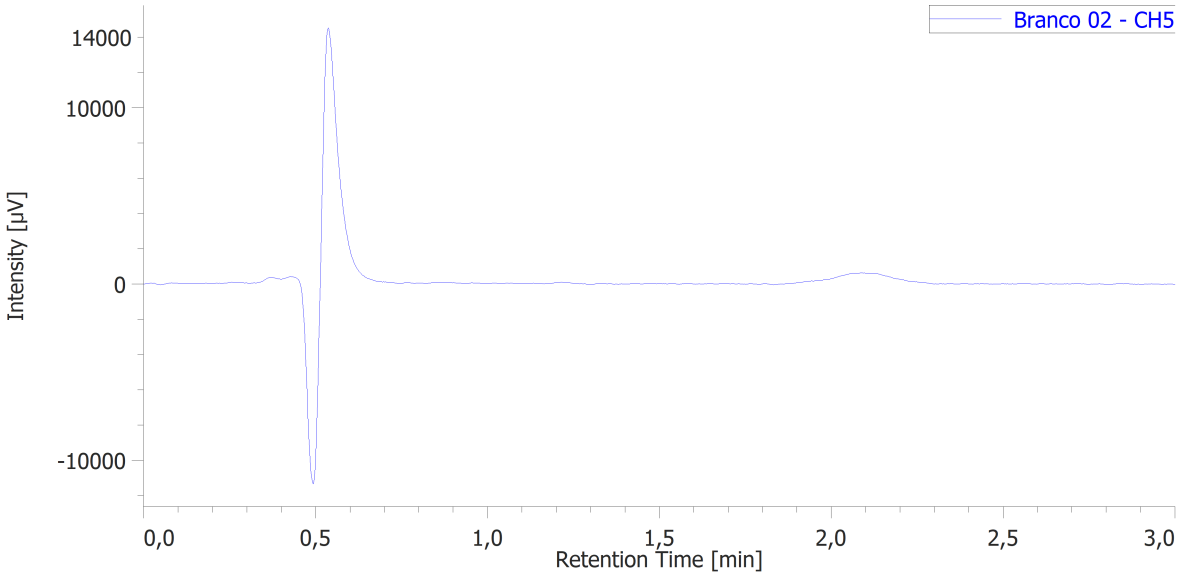


Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:56:10
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:53:08
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

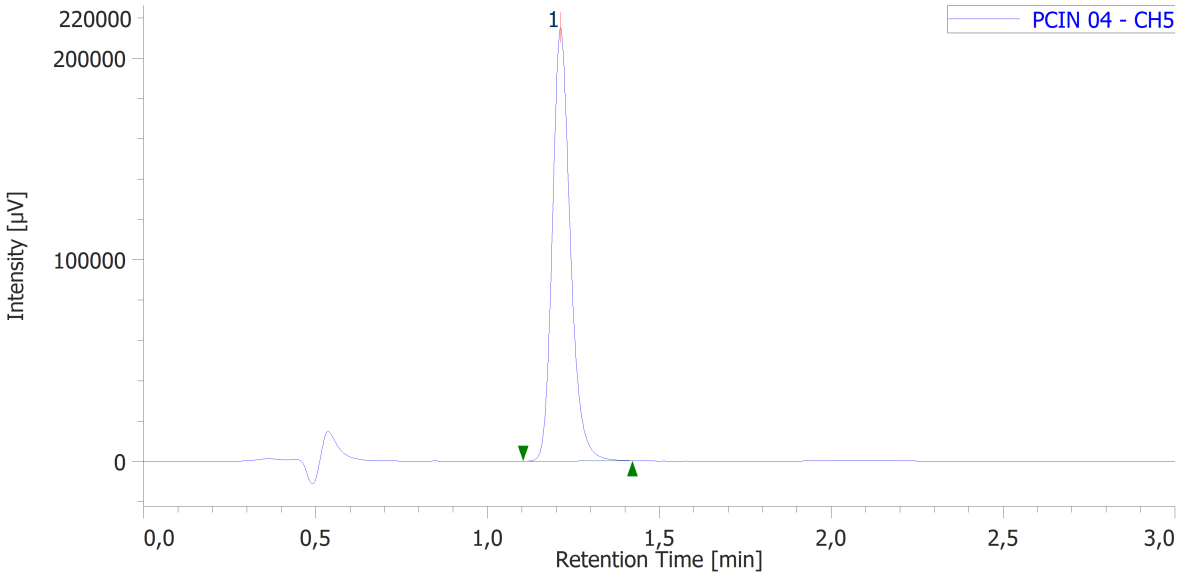

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 11:59:22
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:56:20
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,212	781584	214786	100,000	100,000	N/A	2766	N/A	1,243		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

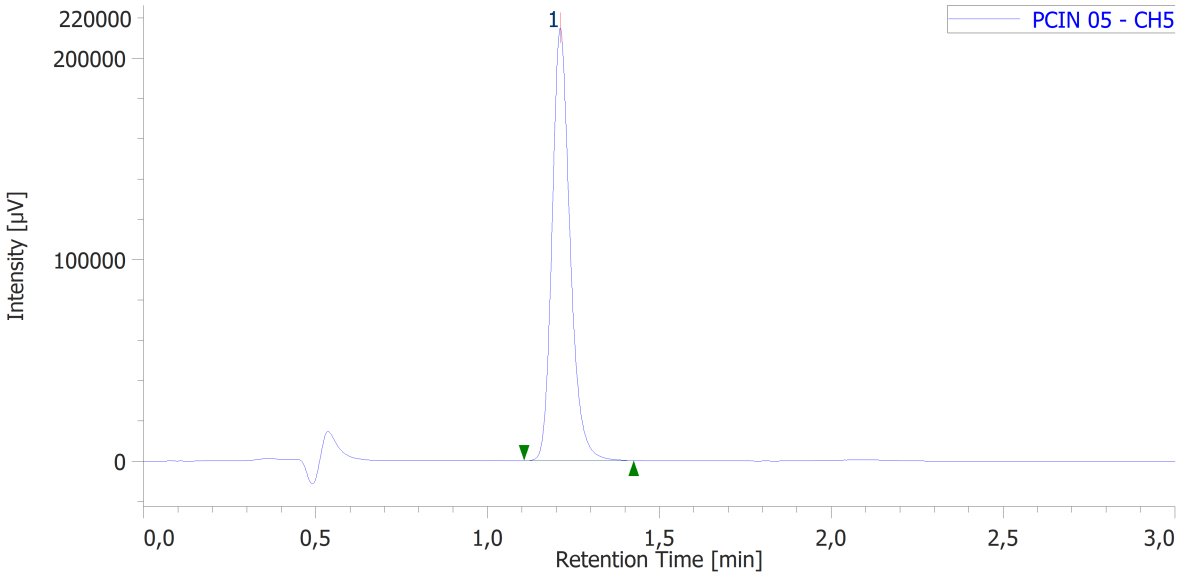

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:02:37
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 11:59:32
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,212	780841	214639	100,000	100,000	N/A	2767	N/A	1,223		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

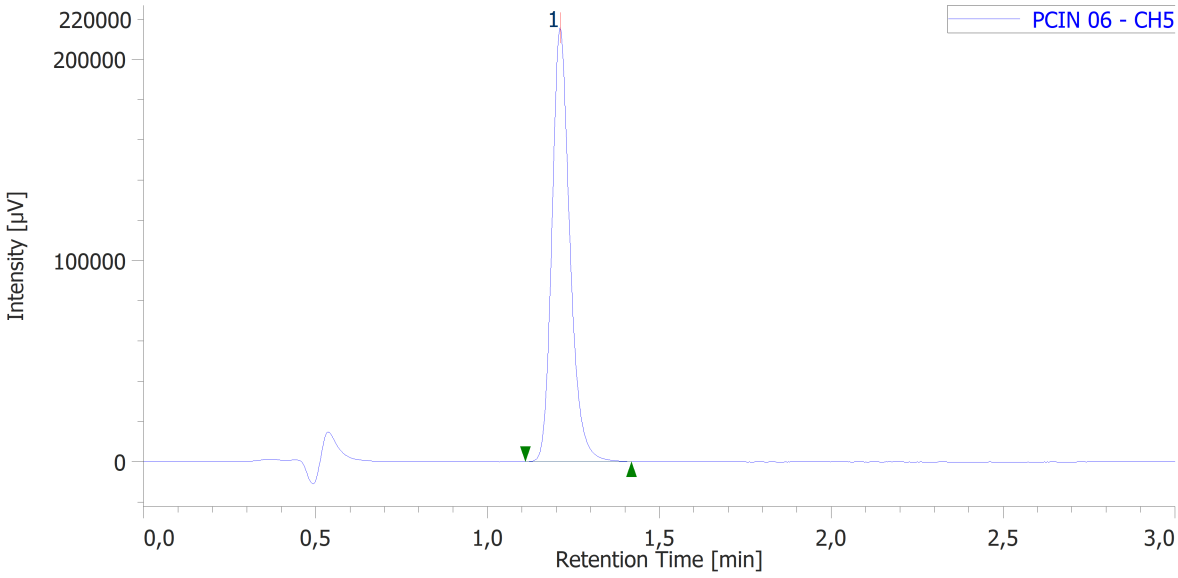

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:12:46
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:09:42
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,212	781794	215421	100,000	100,000	N/A	2779	N/A	1,212		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

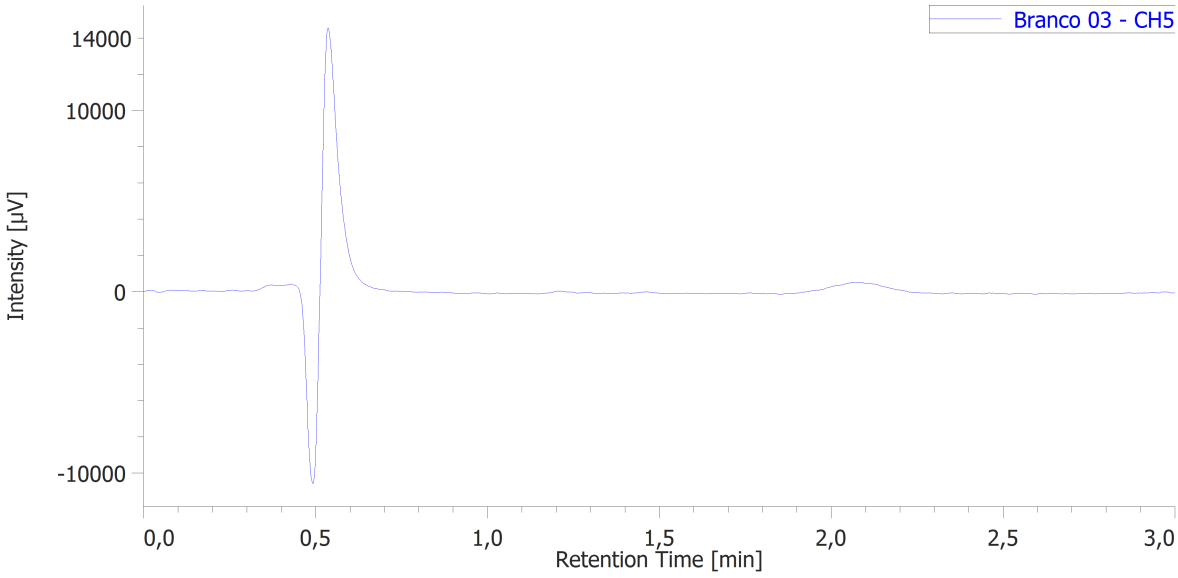


Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:15:58
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:12:55
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

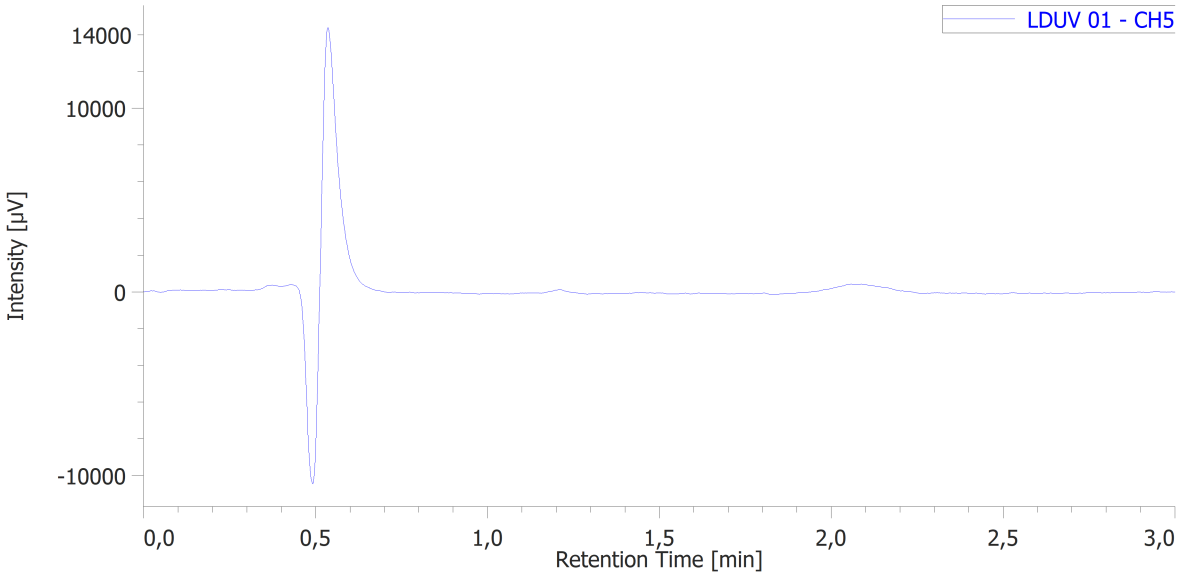


Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:19:10
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:16:07
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

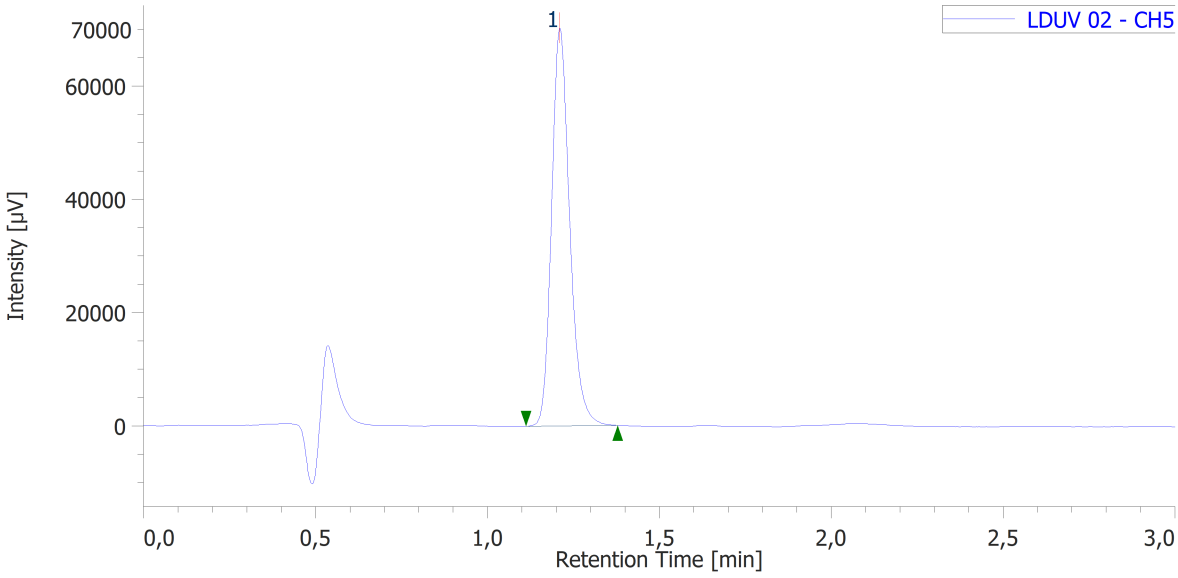

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:22:22
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:19:19
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,210	256897	70239	100,000	100,000	N/A	2694	N/A	1,229		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

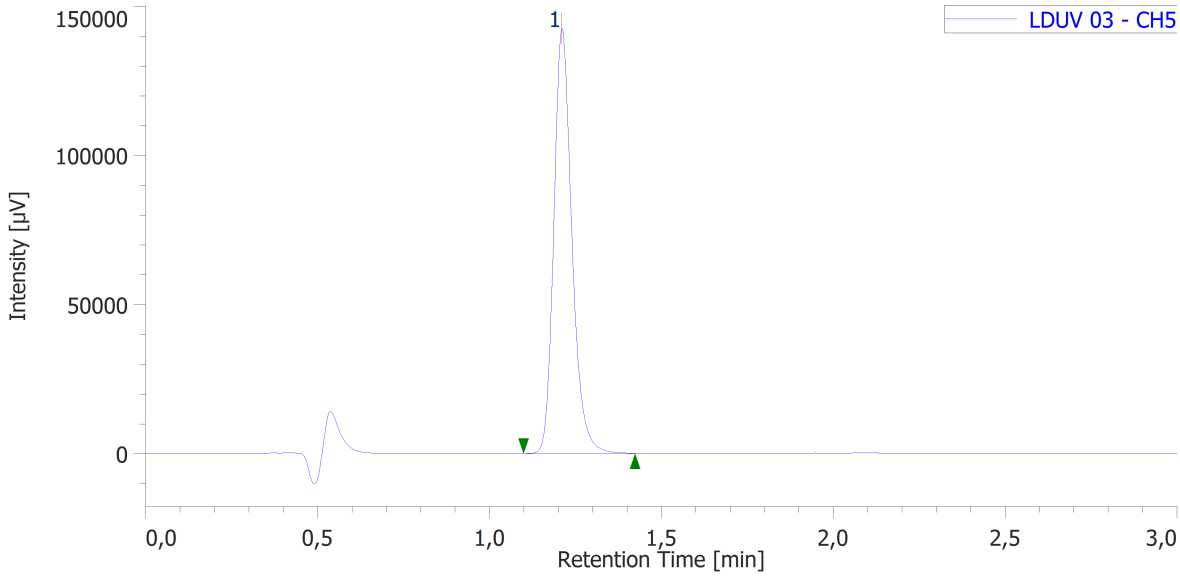

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:25:34
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:22:31
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,210	521620	142604	100,000	100,000	N/A	2724	N/A	1,248		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

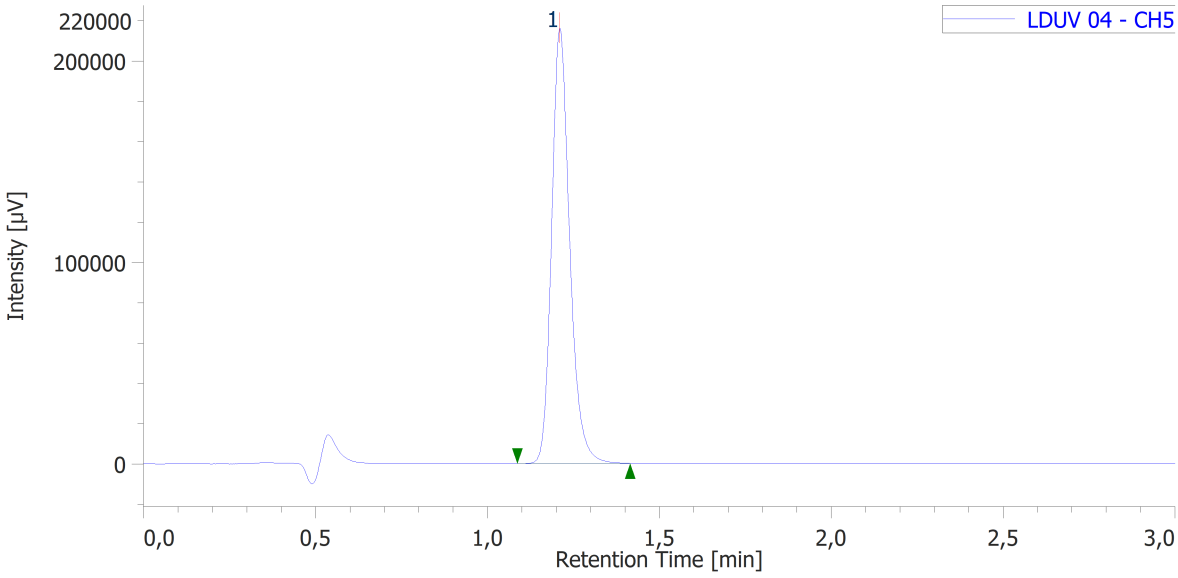

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:28:46
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:25:44
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,210	789222	216173	100,000	100,000	N/A	2740	N/A	1,230		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

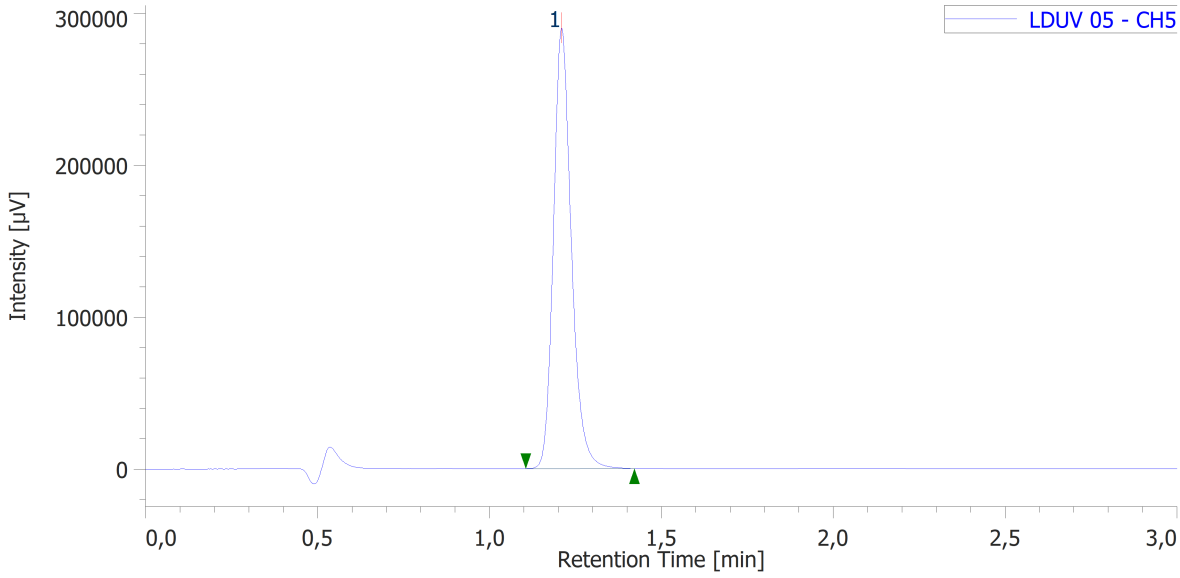

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:31:58
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:28:56
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,210	1049862	290024	100,000	100,000	N/A	2789	N/A	1,207		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

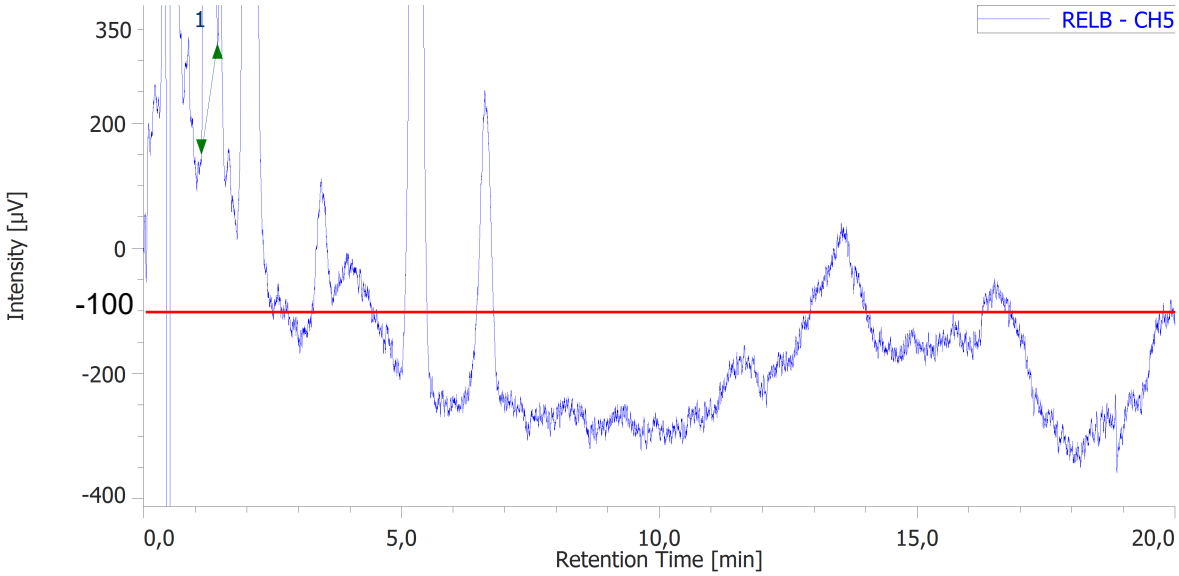

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:58:41
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:32:08
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,225	725394	199815	100,000	100,000	N/A	2854	N/A	1,224		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

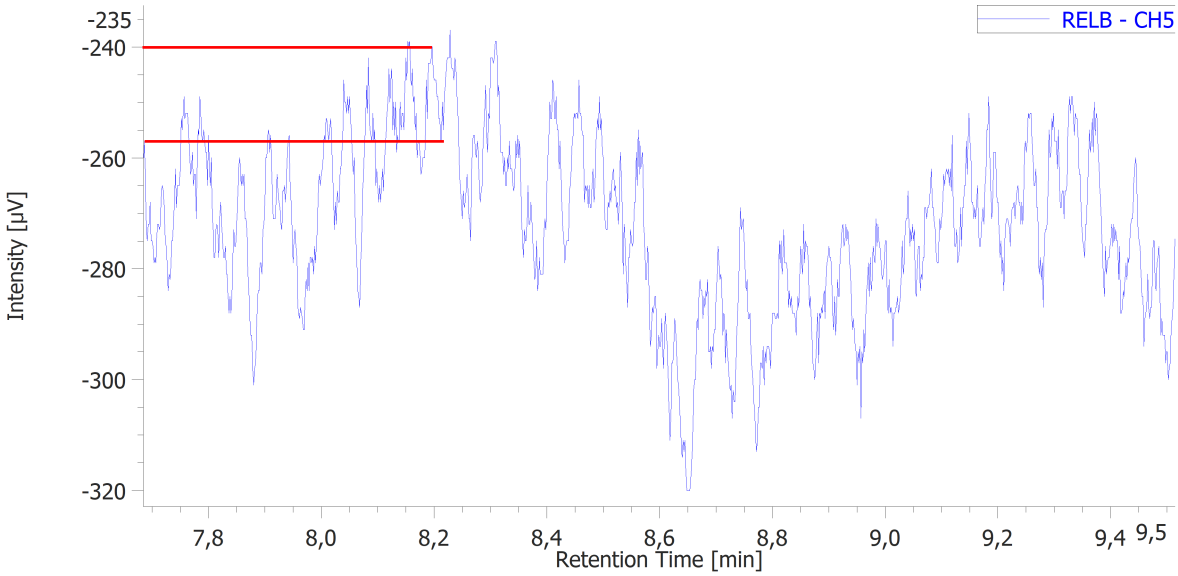

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:58:41
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:32:08
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,225	725394	199815	100,000	100,000	N/A	2854	N/A	1,224		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

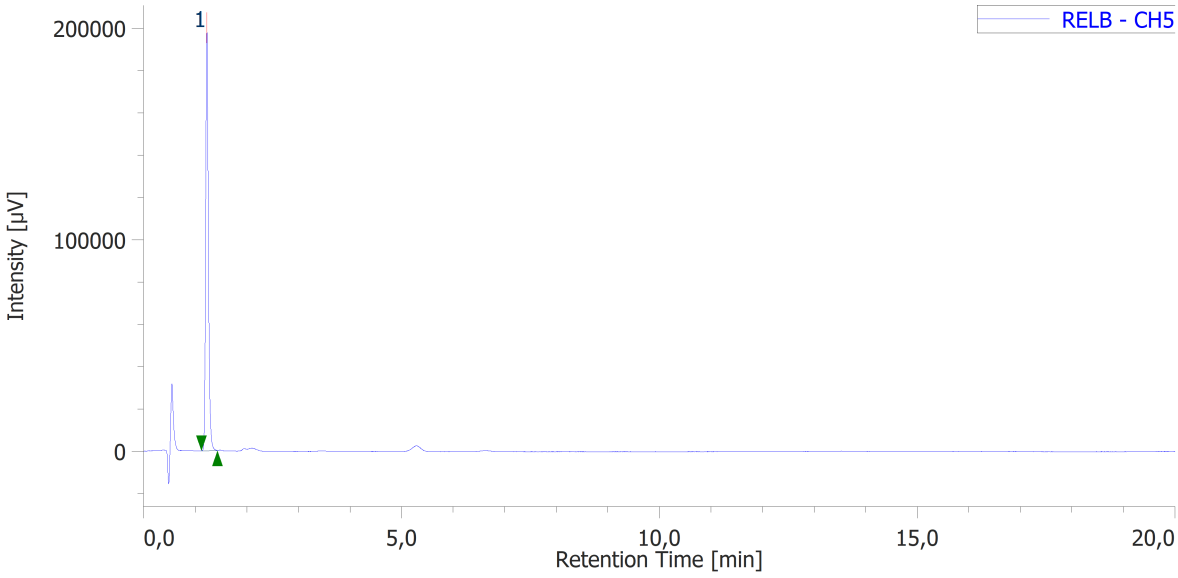

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:58:41
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:32:08
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,225	725394	199815	100,000	100,000	N/A	2854	N/A	1,224		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

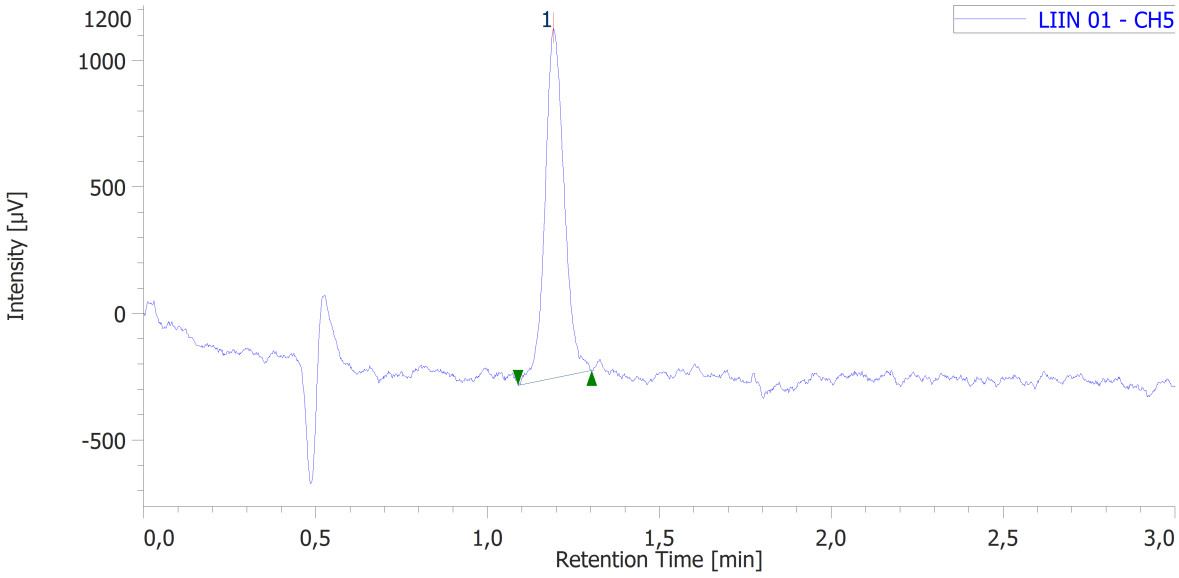

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 13:03:46
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:52:20
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,192	5352	1383	100,000	100,000	N/A	2376	N/A	1,096		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

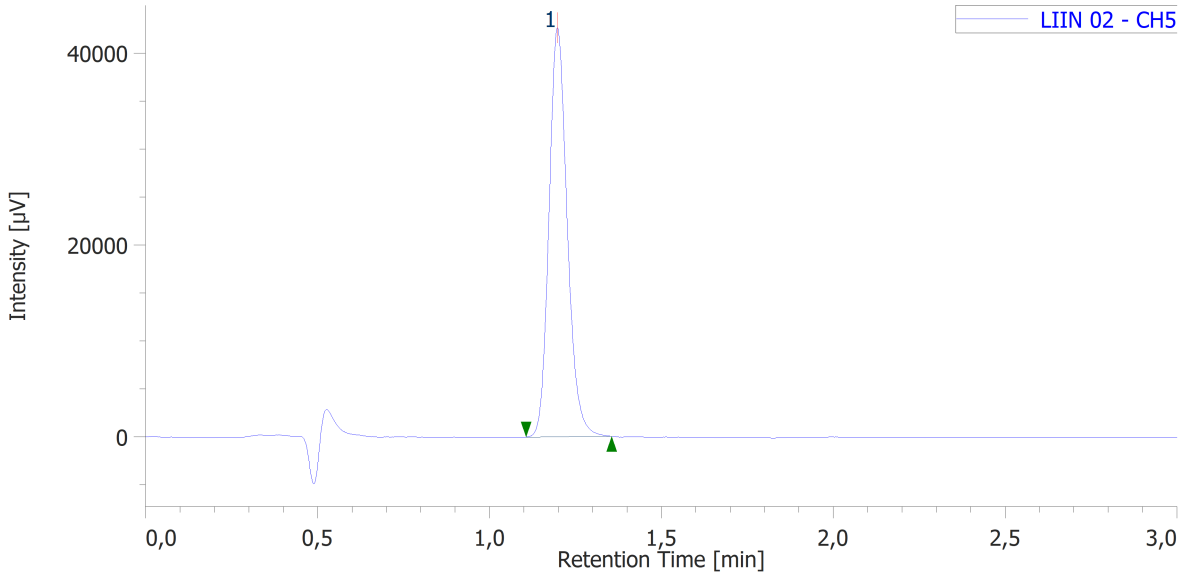

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 12:58:34
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:55:32
Volume	2,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,197	157096	42588	100,000	100,000	N/A	2540	N/A	1,195		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

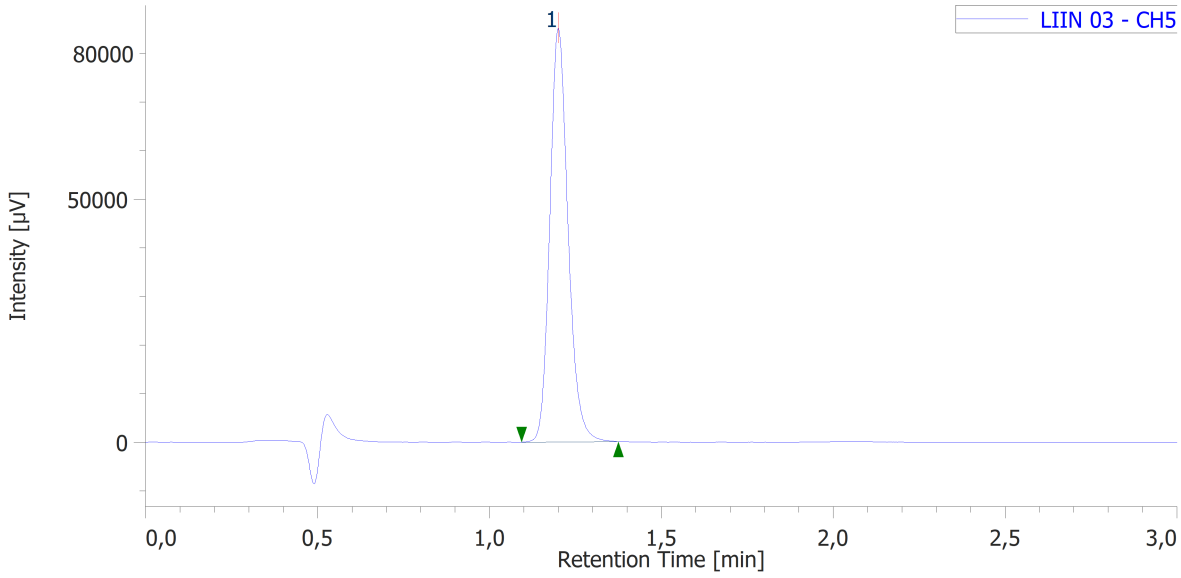

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 13:01:48
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 12:58:44
Volume	4,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,200	313514	85116	100,000	100,000	N/A	2587	N/A	1,181		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

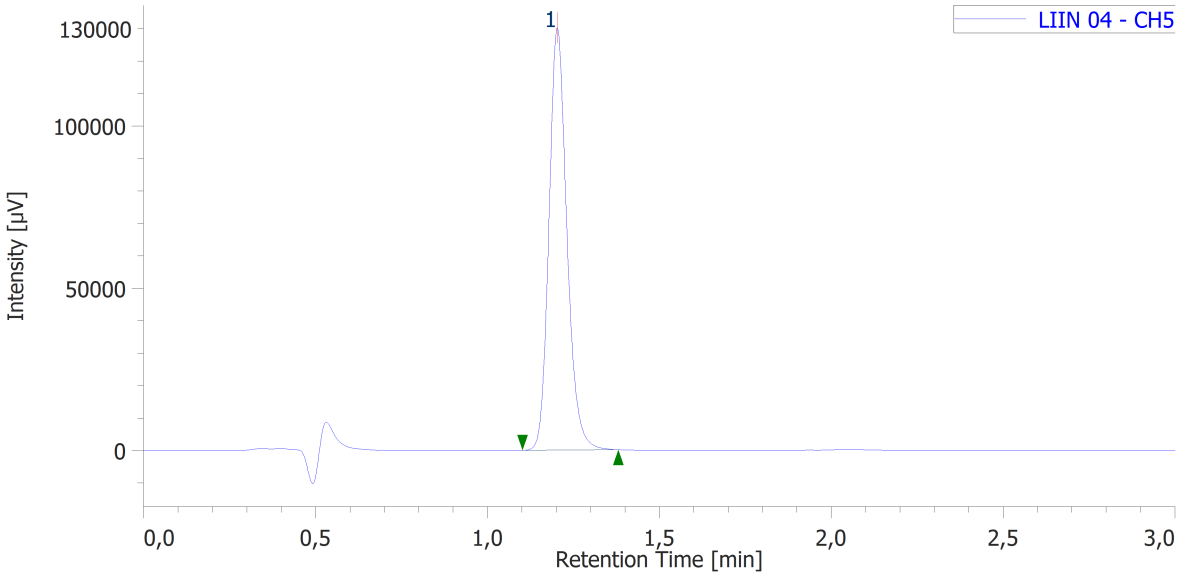

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 13:05:00
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 13:01:57
Volume	6,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,203	472113	130045	100,000	100,000	N/A	2691	N/A	1,172		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

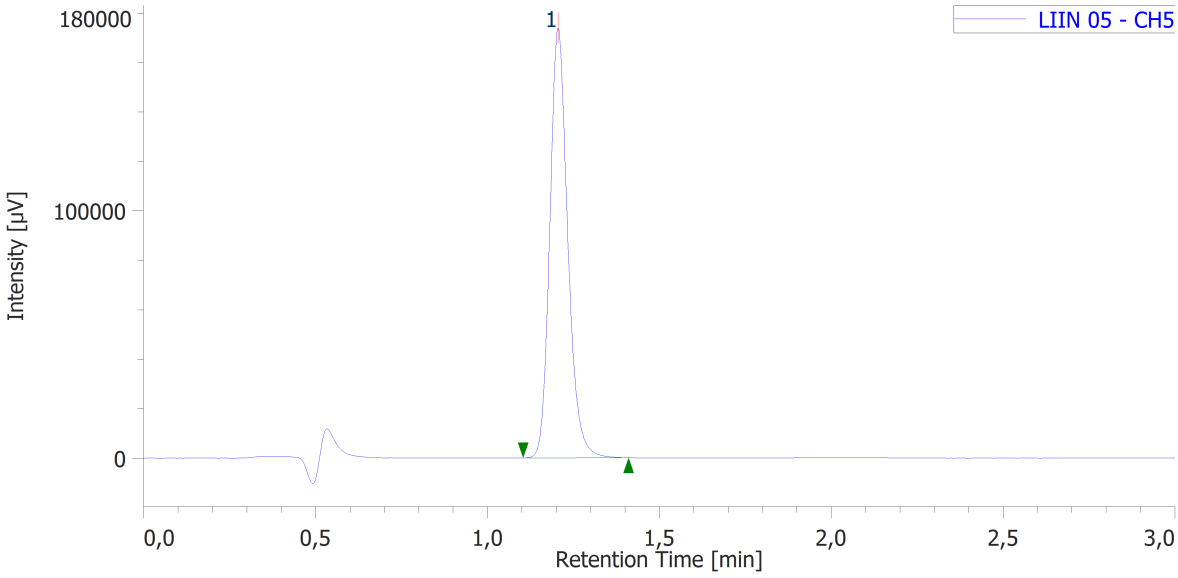

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 13:08:12
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 13:05:09
Volume	8,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,205	630201	173792	100,000	100,000	N/A	2724	N/A	1,197		N/A

Creator QPackSA
Reviewer
Approver

Peak Find - HP06 - Det FL FPEm_20260219T141259-0300.jws

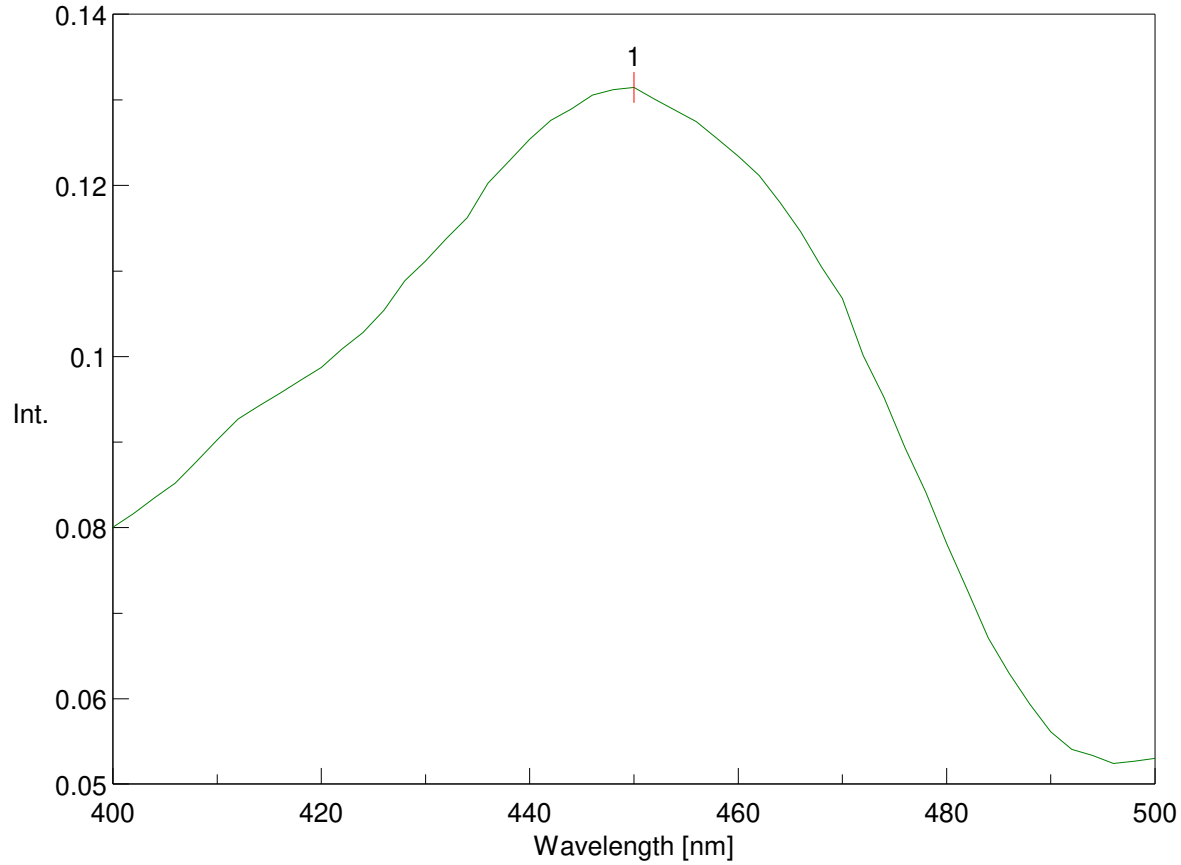

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	19/02/2026 14:12

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	0.131439			

Chromatogram

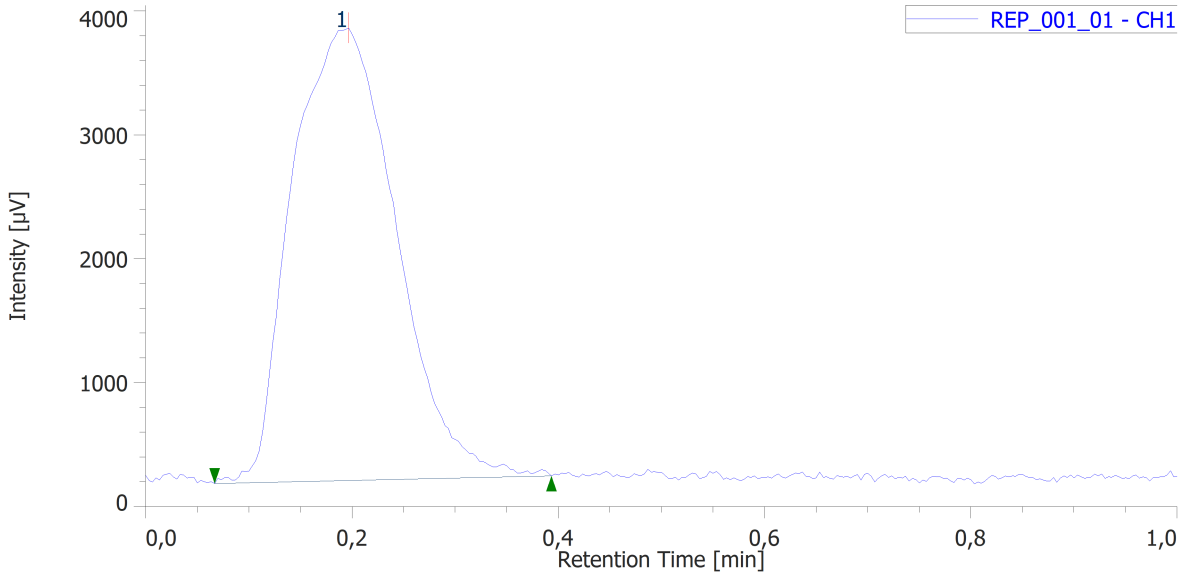

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:45
Description	
HPLC System Name	HP06 – Det FL
Injection Date	19/02/2026 15:19:54
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,197	25594	3651	100,000	100,000	N/A	16	N/A	1,181		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

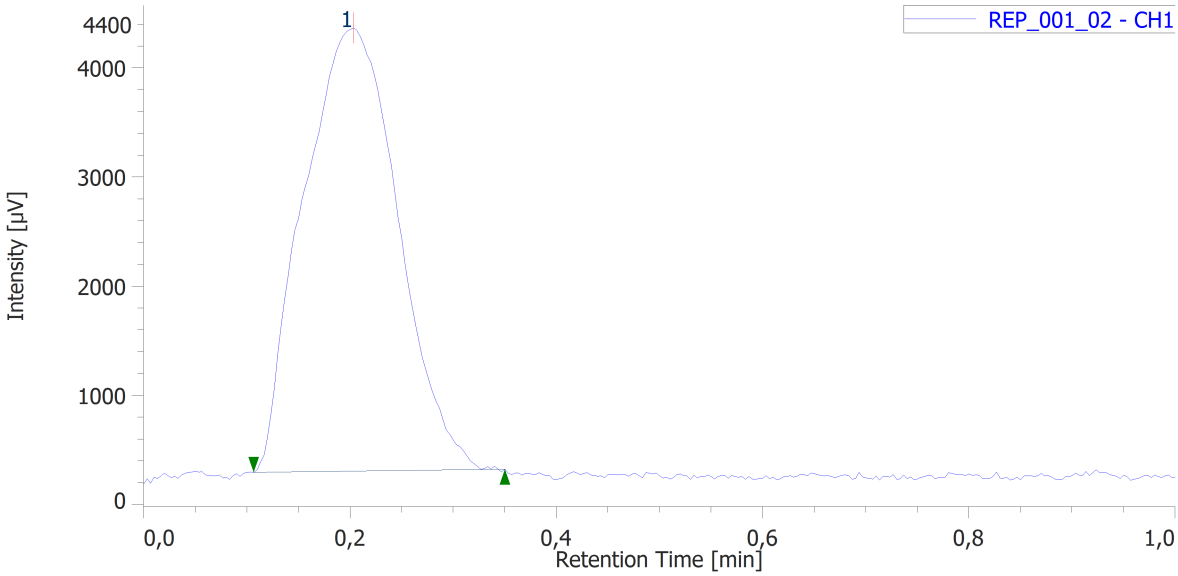

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:45
Description	
HPLC System Name	HP06 - Det FL
Injection Date	19/02/2026 15:22:23
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,203	25920	4058	100,000	100,000	N/A	20	N/A	1,107		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

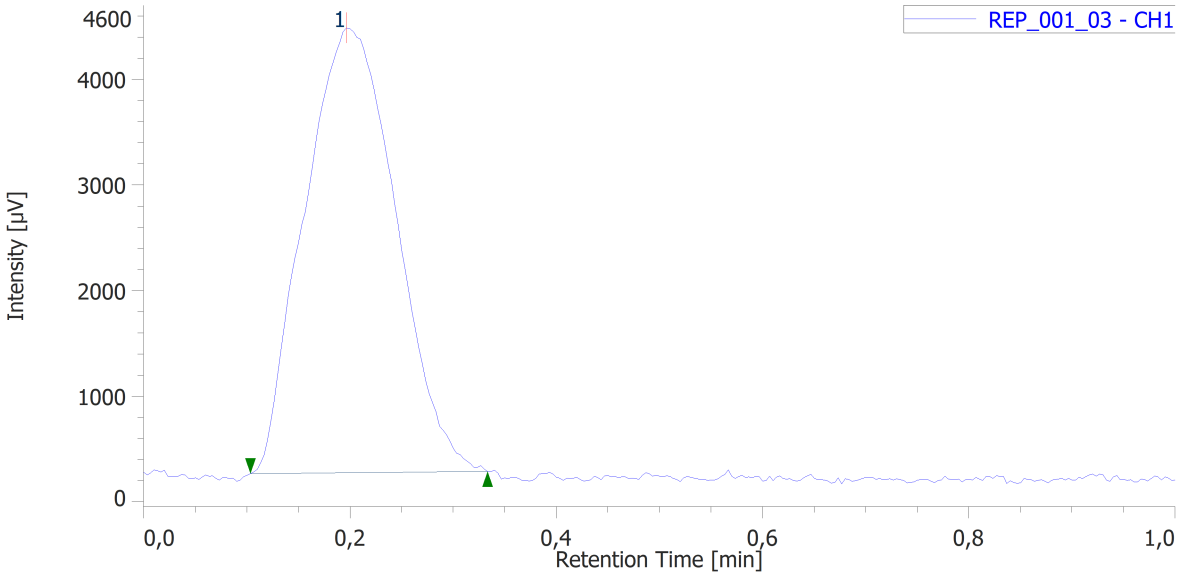

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:45
Description	
HPLC System Name	HP06 - Det FL
Injection Date	19/02/2026 15:24:51
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,197	25946	4210	100,000	100,000	N/A	21	N/A	1,157		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

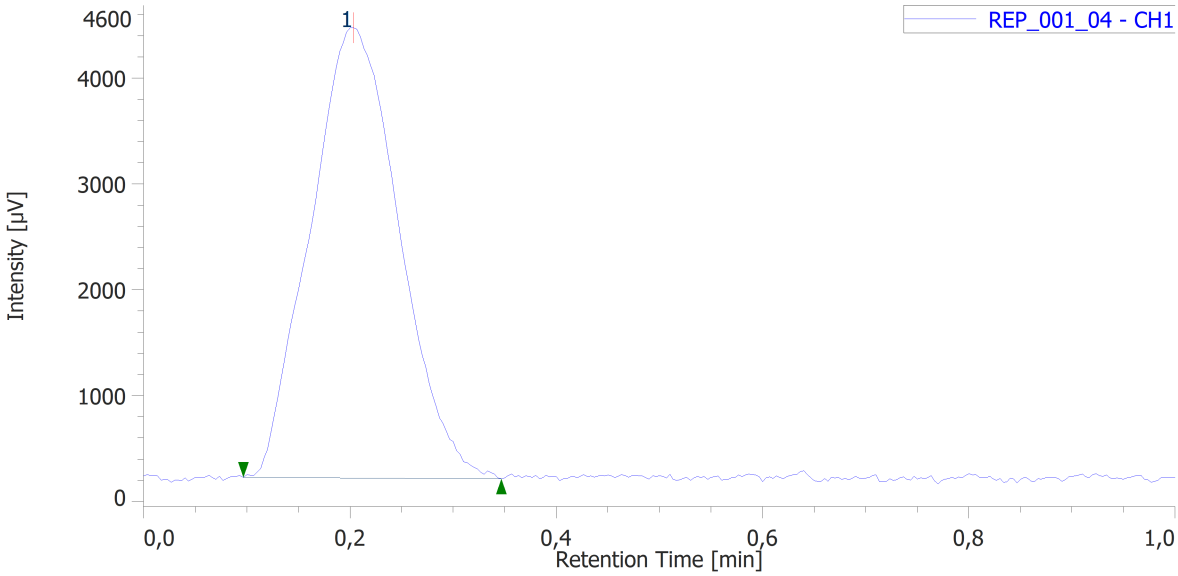

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:46
Description	
HPLC System Name	HP06 – Det FL
Injection Date	19/02/2026 15:27:19
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,203	25518	4251	100,000	100,000	N/A	26	N/A	1,108		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

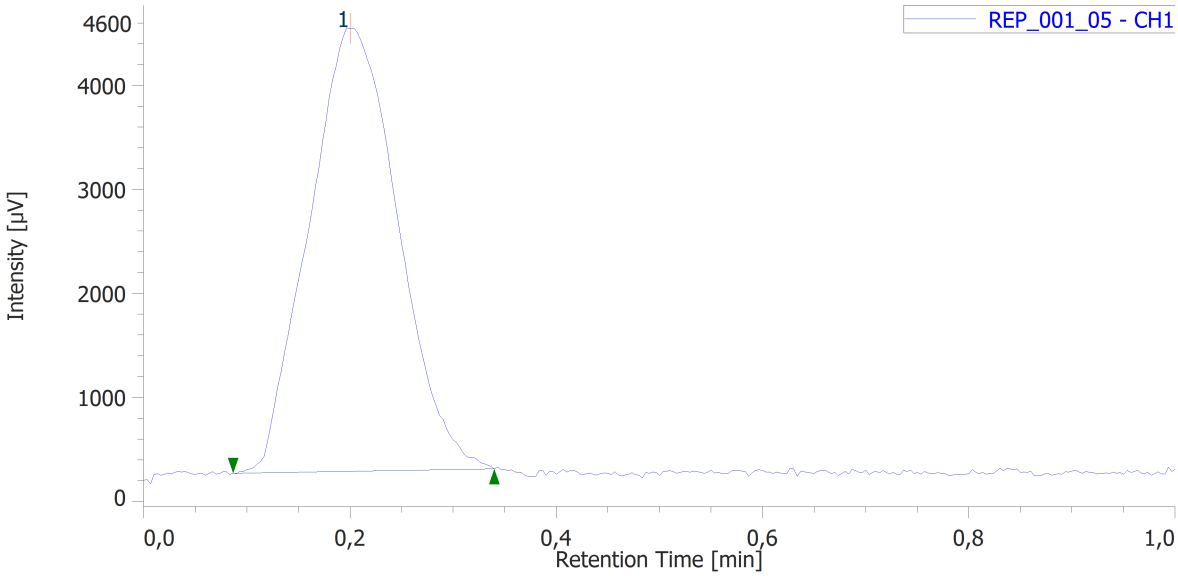

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:46
Description	
HPLC System Name	HP06 – Det FL
Injection Date	19/02/2026 15:29:47
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,200	25562	4255	100,000	100,000	N/A	25	N/A	1,148		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

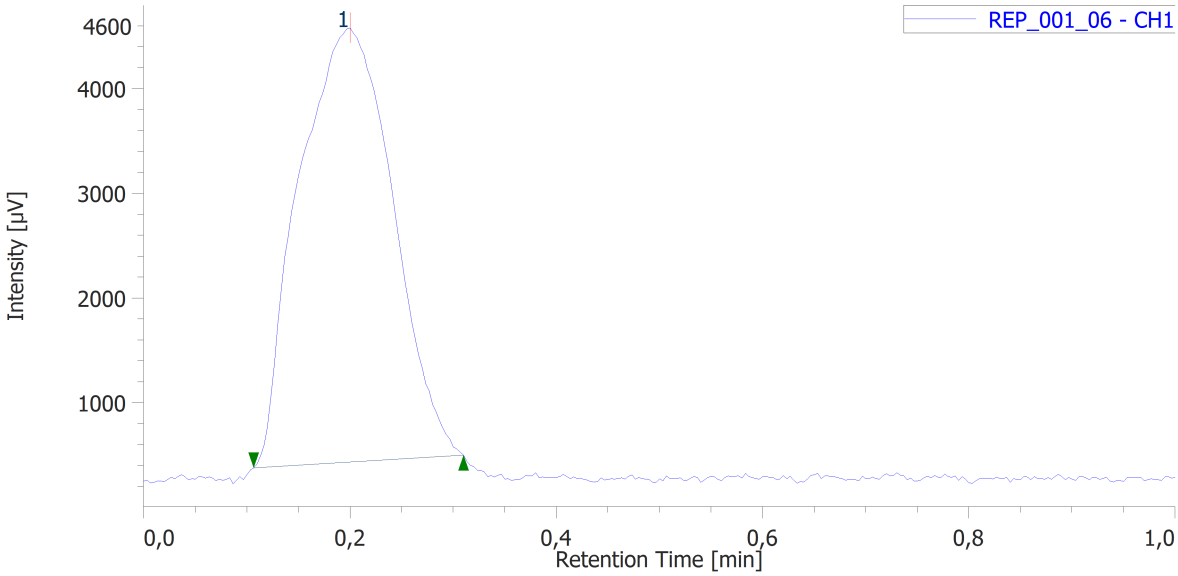

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 15:34:46
Description	
HPLC System Name	HP06 – Det FL
Injection Date	19/02/2026 15:32:15
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	REP_001_06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,200	26199	4144	100,000	100,000	N/A	18	N/A	1,057		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

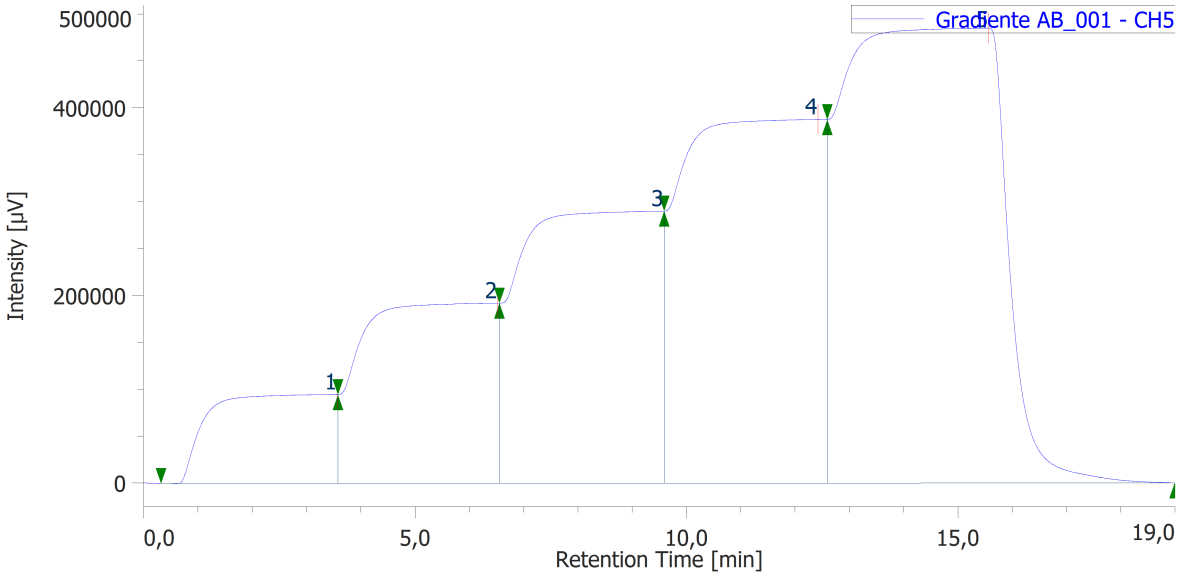

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 16:19:04
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 15:55:54
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20%	5	3,572	14414129	94743	5,529	6,539	N/A	N/A	N/A	N/A		N/A
2	40%	5	6,520	31665215	191989	12,145	13,251	N/A	N/A	N/A	N/A		N/A
3	60%	5	9,587	50016678	289830	19,184	20,003	N/A	N/A	N/A	N/A		N/A
4	80%	5	12,420	67203913	387486	25,776	26,743	N/A	N/A	N/A	N/A		N/A
5	100%	5	15,565	97419613	484867	37,366	33,464	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

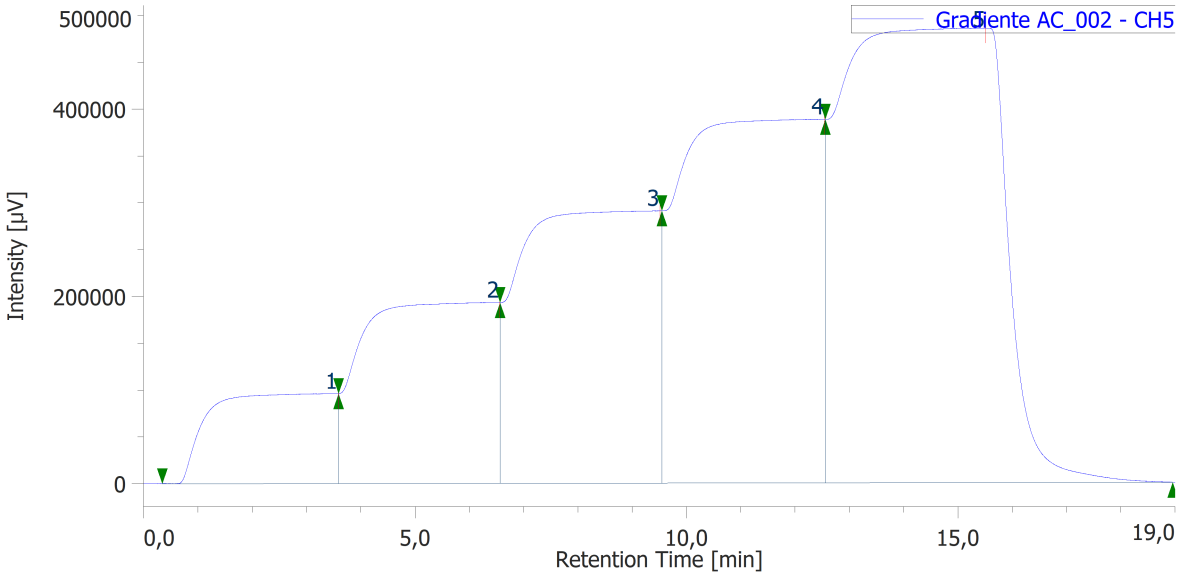

Chromatogram Information	
User Name	QPackSA
Date Modified	19/02/2026 16:38:01
Description	
HPLC System Name	HP06
Injection Date	19/02/2026 16:17:21
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Gradiente AC
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AC_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20%	5	3,585	14649992	95952	5,599	6,603	N/A	N/A	N/A	N/A		N/A
2	40%	5	6,558	31917391	193013	12,199	13,283	N/A	N/A	N/A	N/A		N/A
3	60%	5	9,507	49245699	290606	18,822	19,999	N/A	N/A	N/A	N/A		N/A
4	80%	5	12,535	67333213	388151	25,735	26,712	N/A	N/A	N/A	N/A		N/A
5	100%	5	15,505	98495166	485365	37,645	33,402	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver