
Peak Find - Exploratoria_002 UV_tR2.00 D.jws

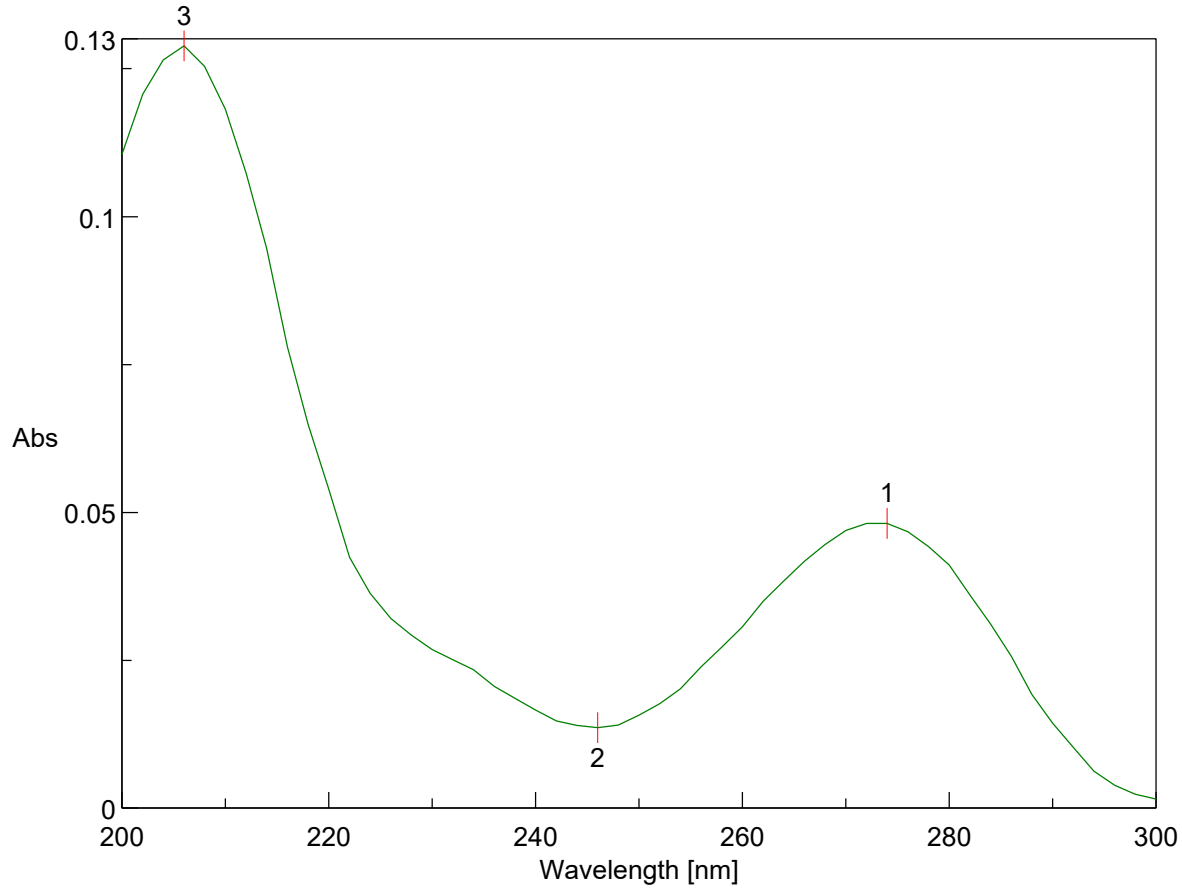

[Comments]

User	Administrator
Division	---
Company	Qpack
Creation date	08/05/2020 10:42

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	X-LC 3075UV
Model Name	X-LC 3075UV
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0480855	2	246	0.0135725
3	206	0.12879			

Chromatogram

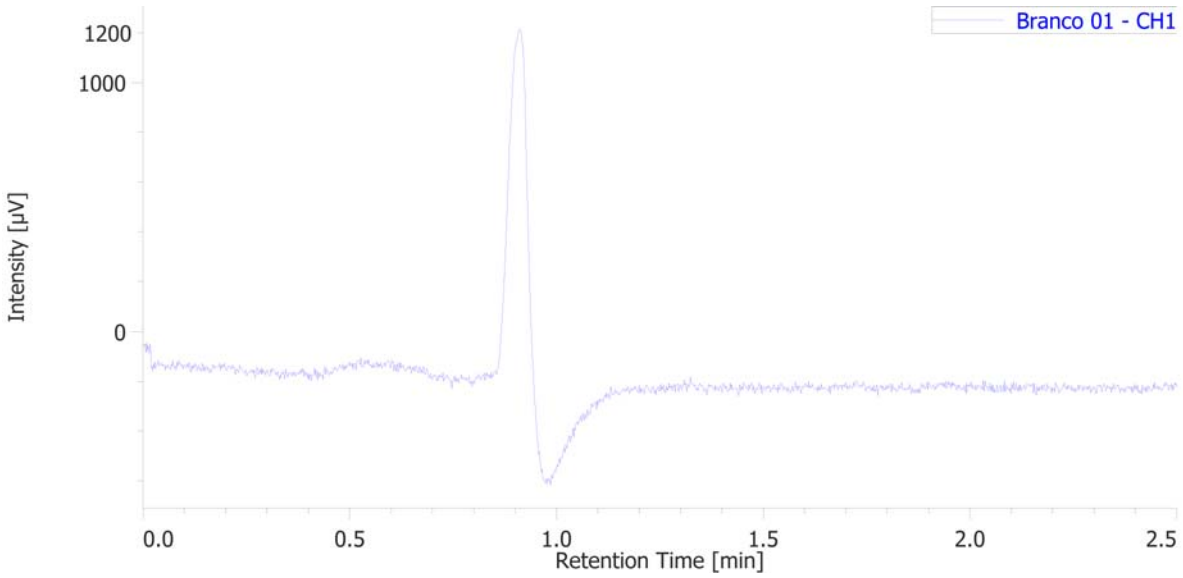


Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:38:20
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:35:47
Volume	10.00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator Administrator
Reviewer
Approver

Chromatogram

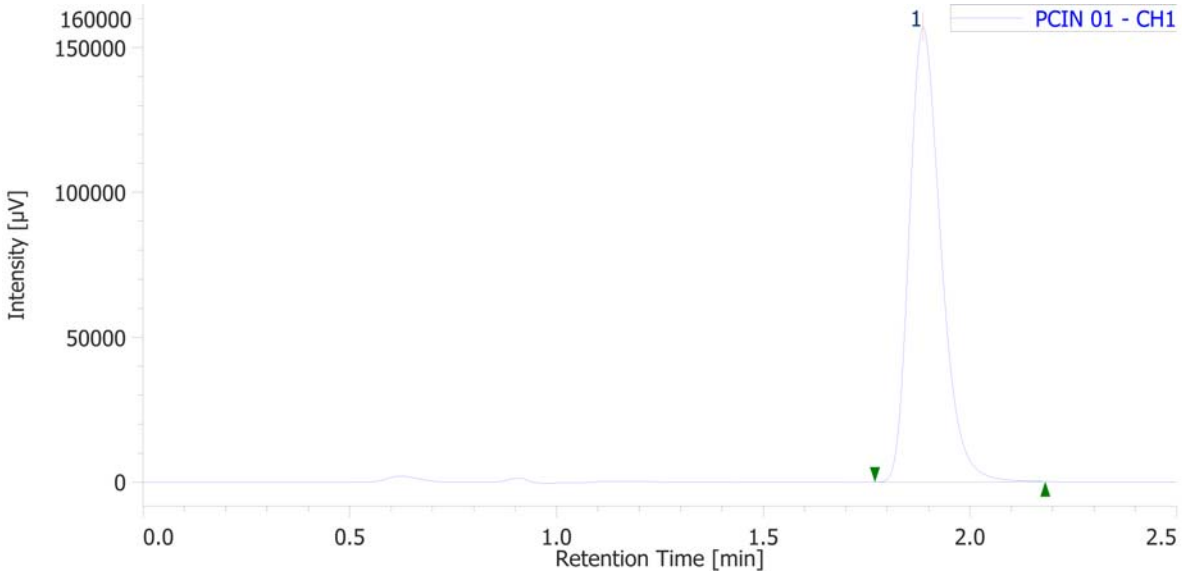

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:41:36
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:39:03
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.887	835931	157105	100.000	100.000	N/A	3004	N/A	1.301	

Creator Administrator
Reviewer
Approver

Chromatogram

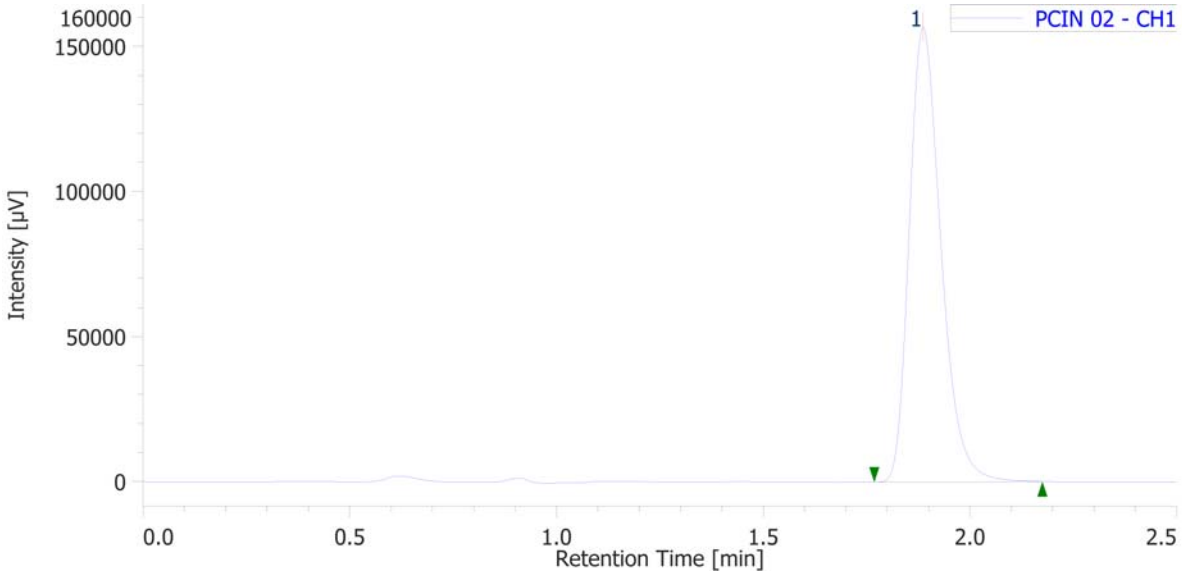

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:44:52
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:42:20
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.887	833977	156799	100.000	100.000	N/A	3008	N/A	1.302	

Creator Administrator
Reviewer
Approver

Chromatogram

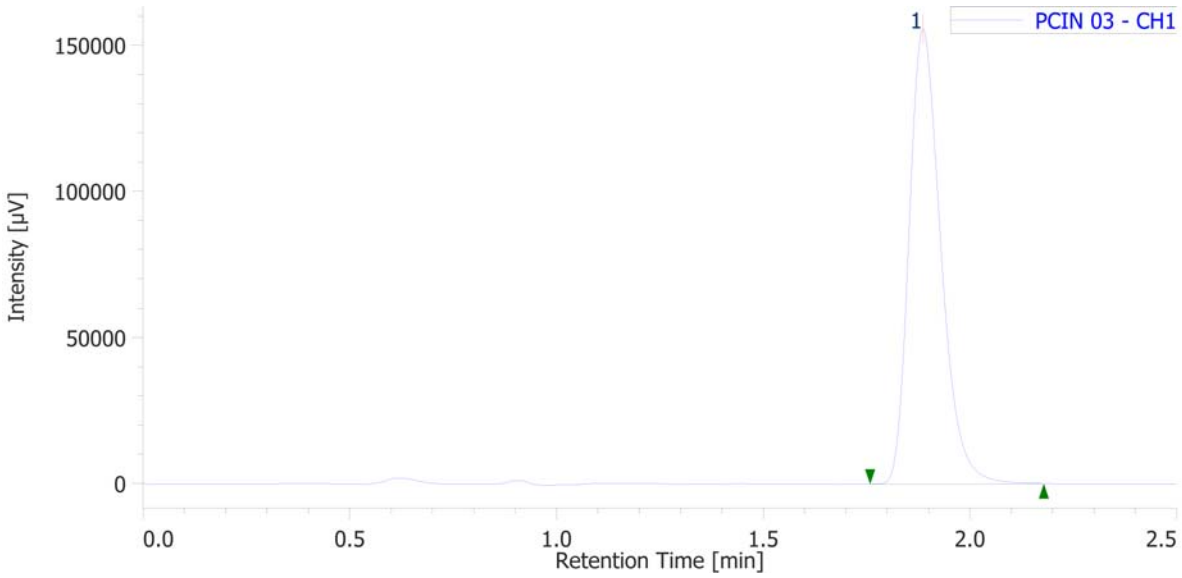

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:48:10
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:45:37
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.887	830153	155655	100.000	100.000	N/A	2989	N/A	1.296	

Creator Administrator
Reviewer
Approver

Chromatogram

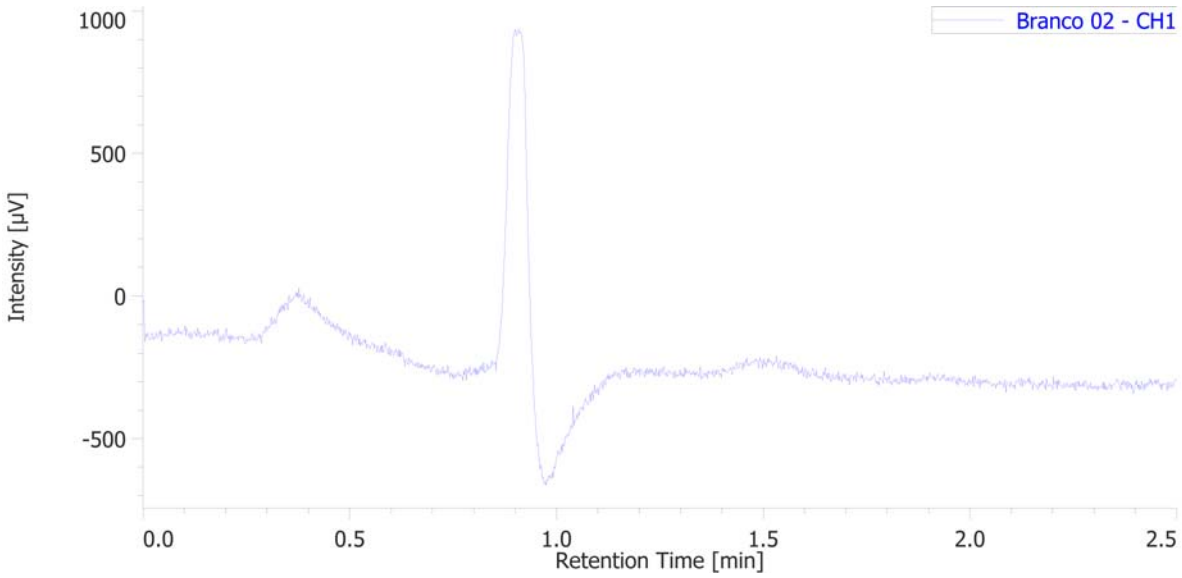


Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:51:28
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:48:54
Volume	10.00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator Administrator
Reviewer
Approver

Chromatogram

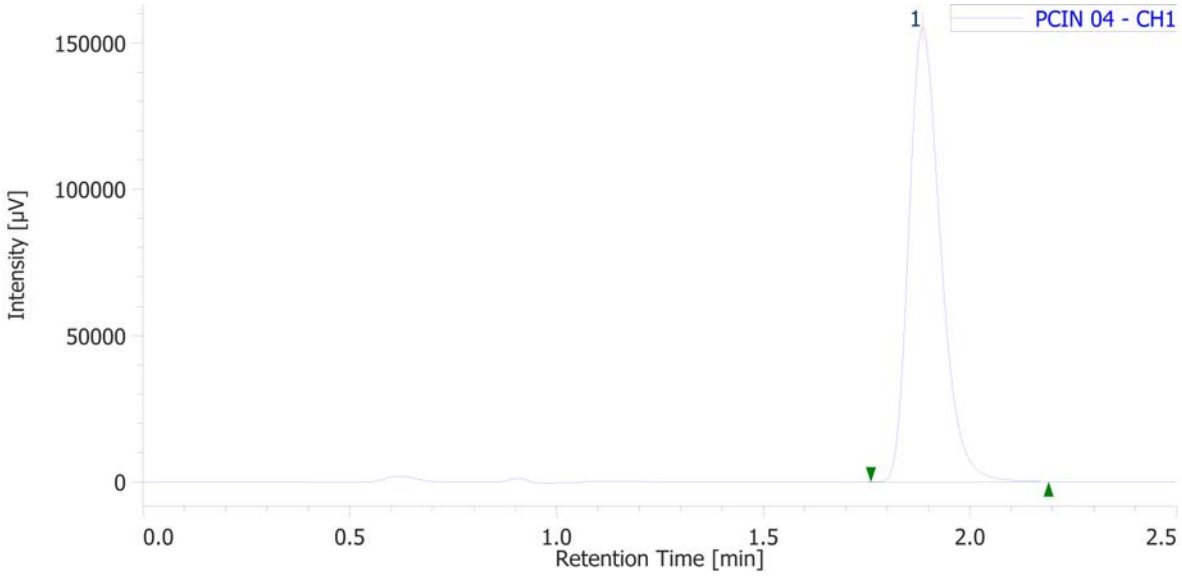

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:54:44
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:52:11
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	830365	155482	100.000	100.000	N/A	2978	N/A	1.316	

Creator Administrator
Reviewer
Approver

Chromatogram

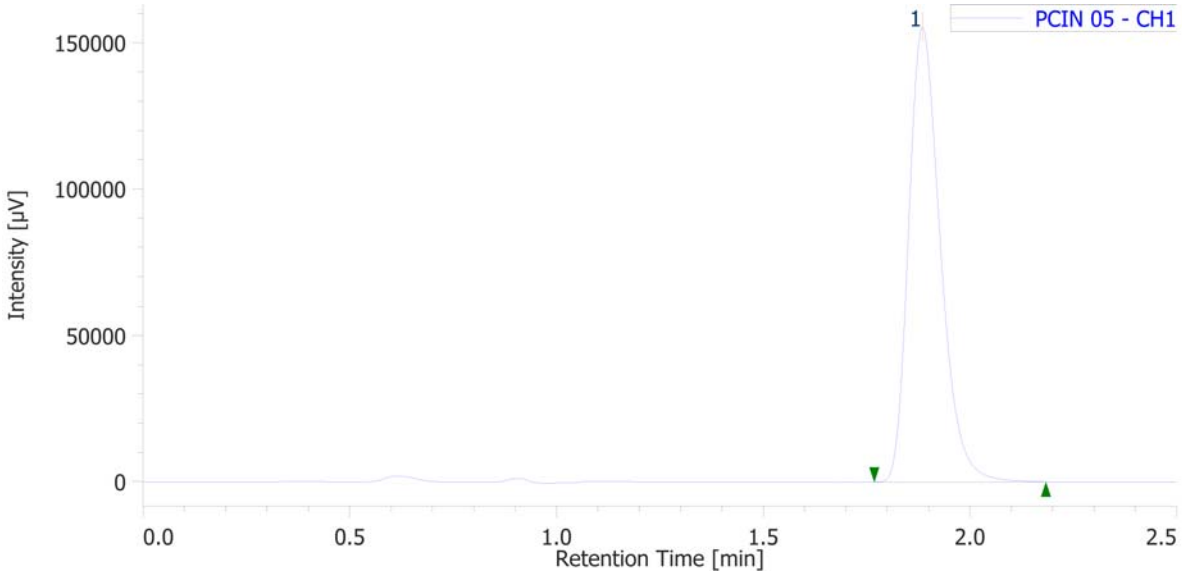

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 11:58:00
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:55:28
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	830846	155430	100.000	100.000	N/A	2972	N/A	1.306	

Creator Administrator
Reviewer
Approver

Chromatogram

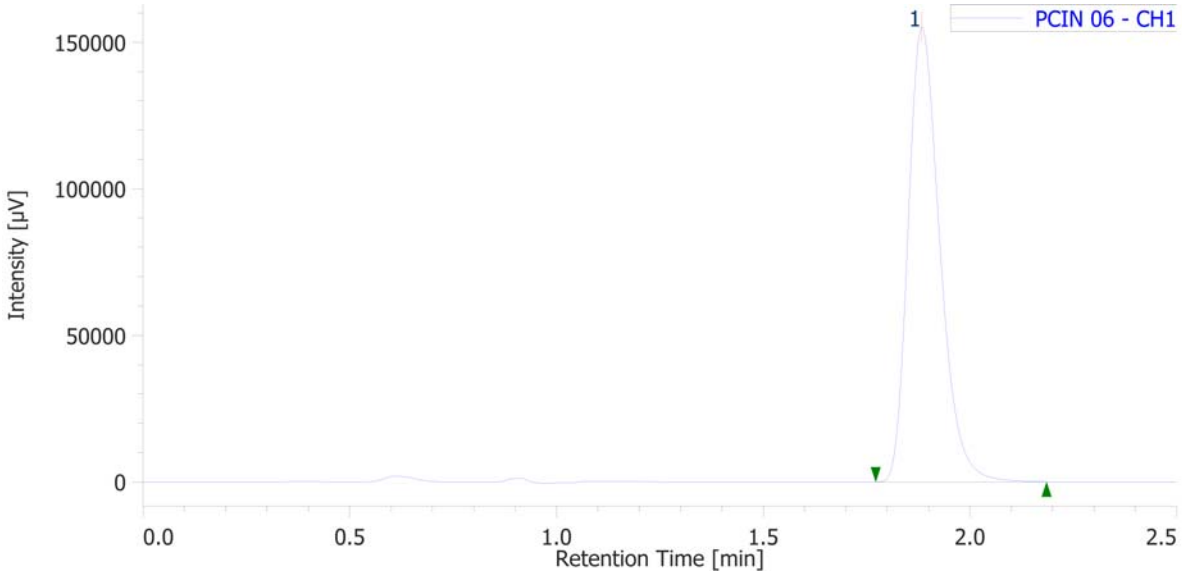

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 12:01:18
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 11:58:45
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.883	829759	155286	100.000	100.000	N/A	2963	N/A	1.311	

Creator Administrator
Reviewer
Approver

Chromatogram

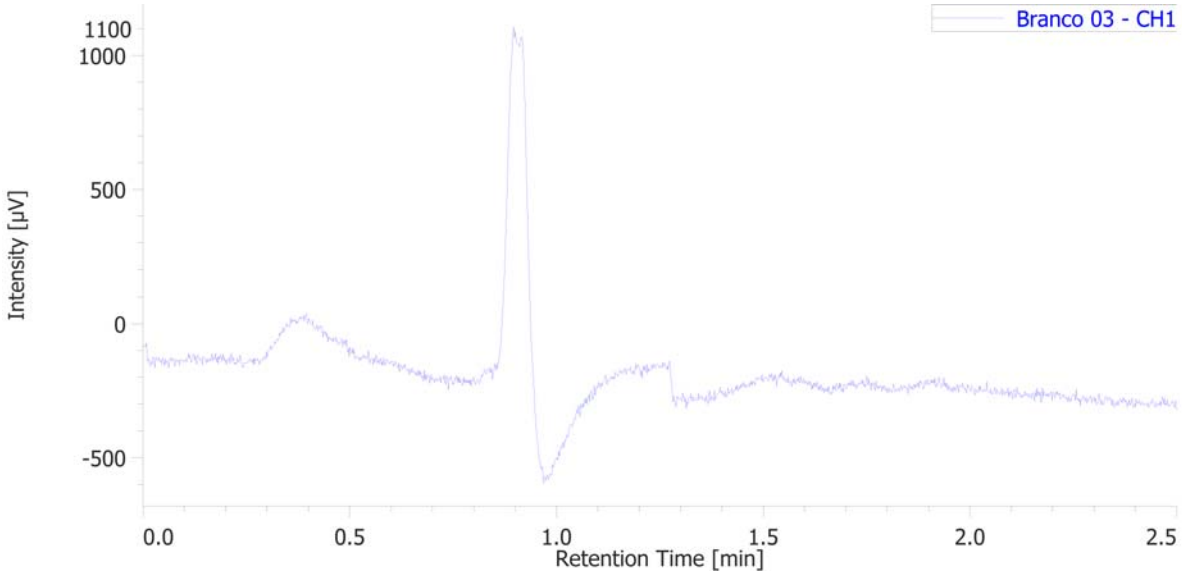


Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:28:53
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:02:02
Volume	10.00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator	Administrator
Reviewer	
Approver	

Chromatogram

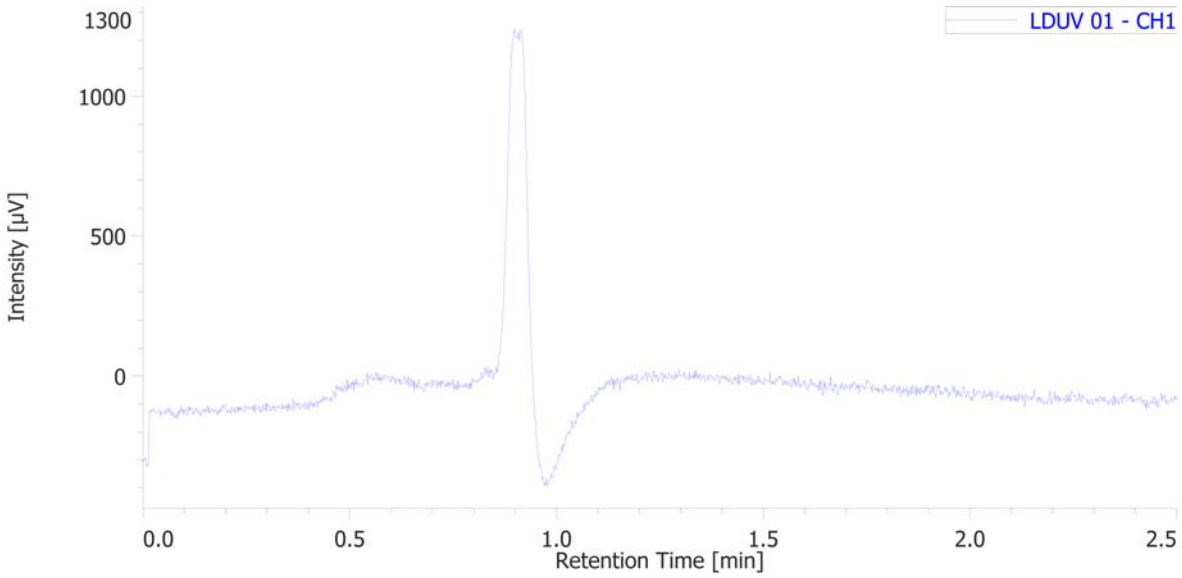


Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:56:28
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:09:13
Volume	10.00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator Administrator
Reviewer
Approver

Chromatogram

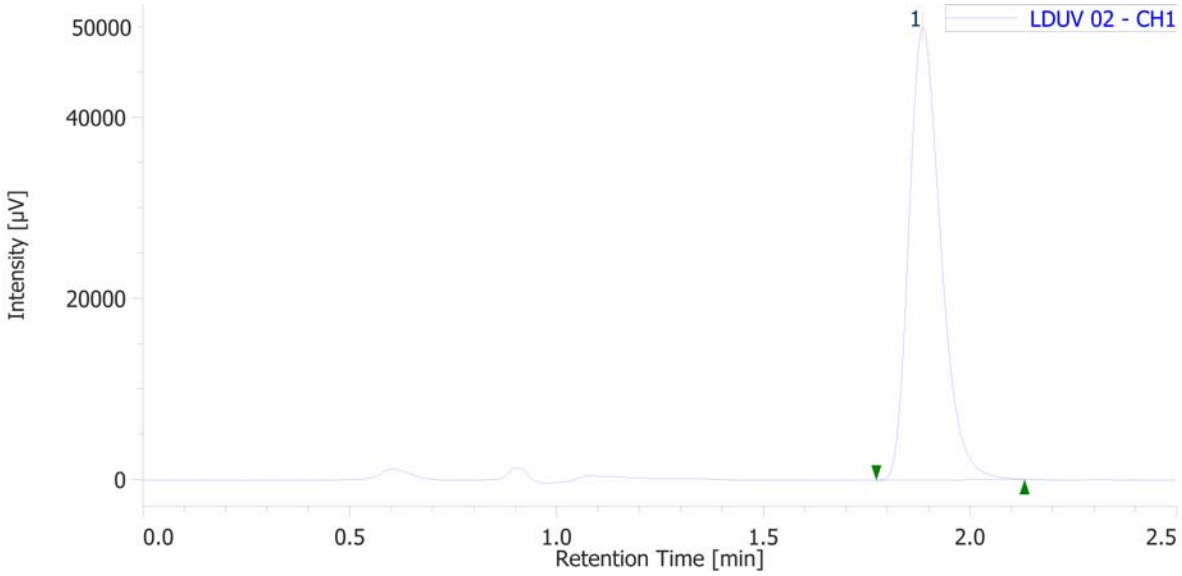

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:56:28
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:12:30
Volume	10.00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	267516	50054	100.000	100.000	N/A	2955	N/A	1.314	

Creator Administrator
Reviewer
Approver

Chromatogram

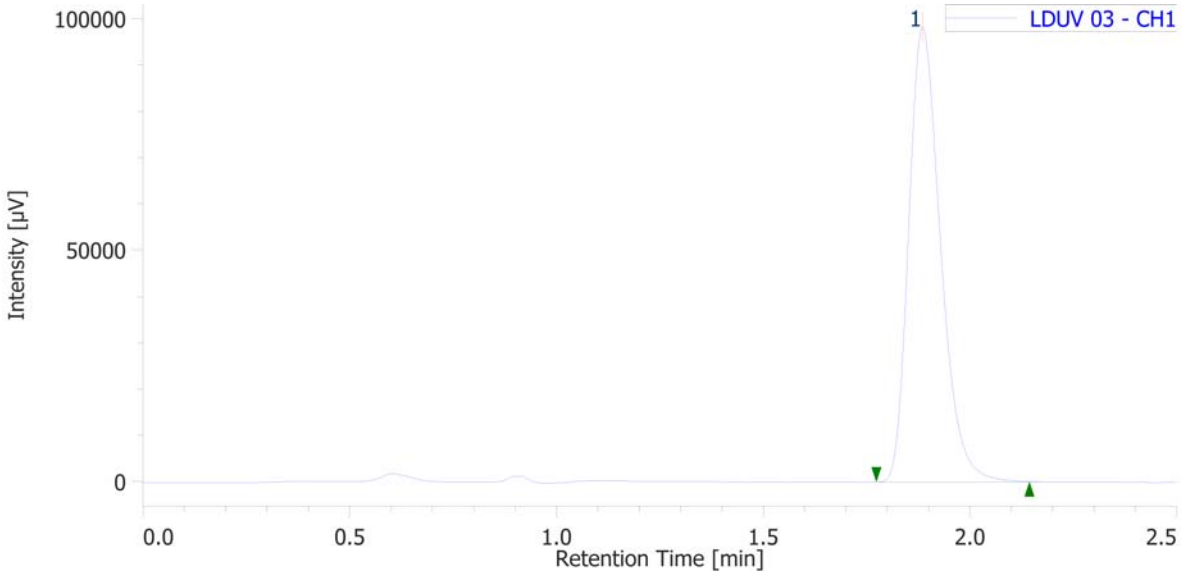

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:56:29
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:15:46
Volume	10.00 [μL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	525608	98227	100.000	100.000	N/A	2957	N/A	1.304	

Creator Administrator
Reviewer
Approver

Chromatogram

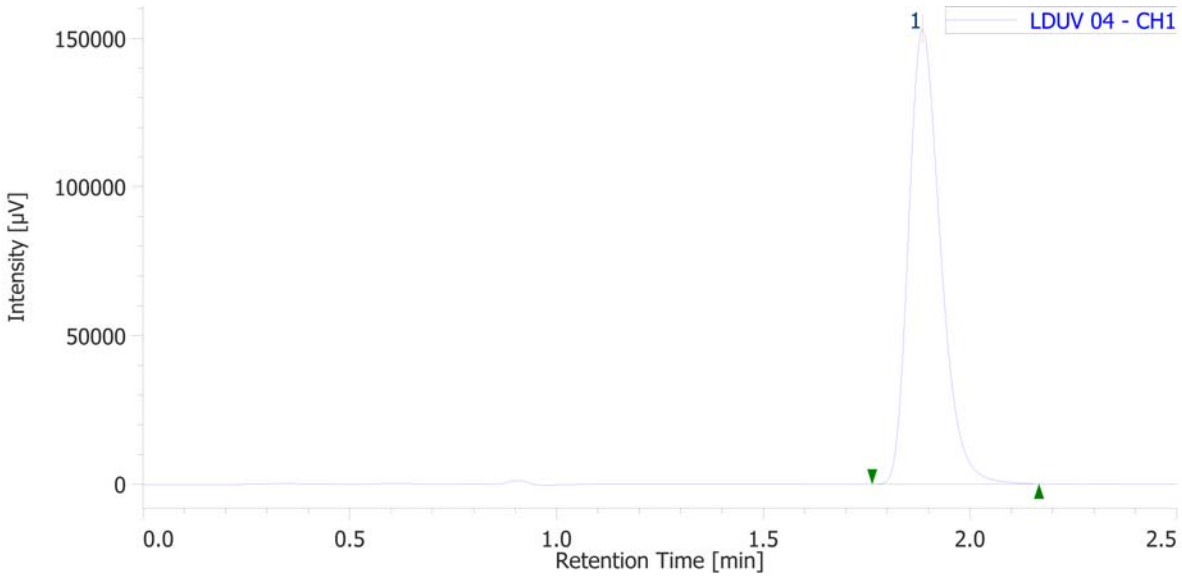

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:56:29
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:19:06
Volume	10.00 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	822662	153110	100.000	100.000	N/A	2929	N/A	1.305	

Creator Administrator
Reviewer
Approver

Chromatogram

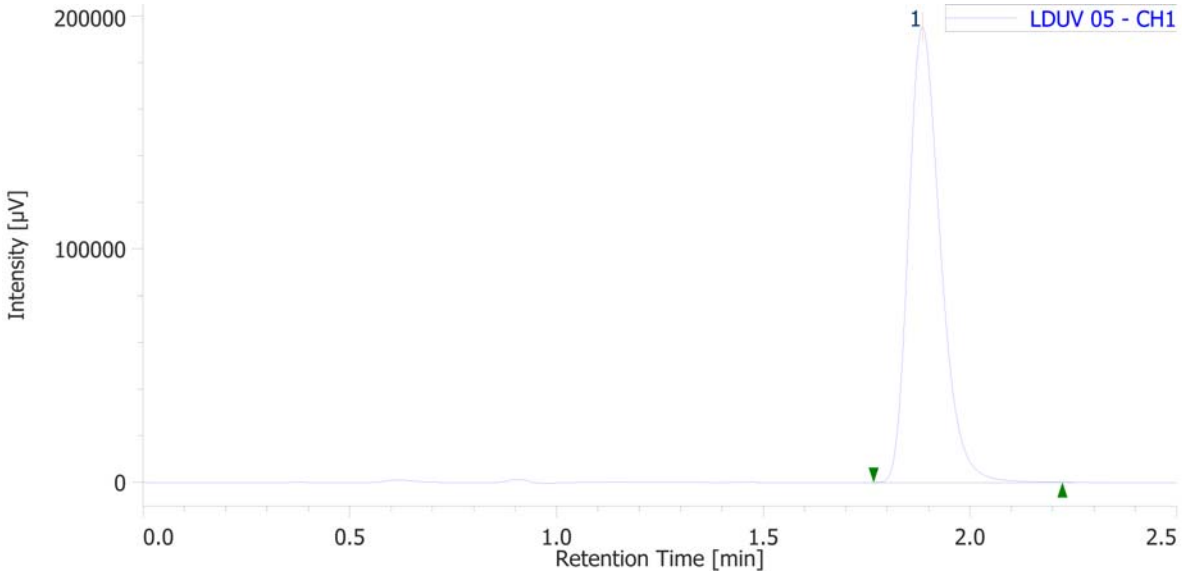

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:56:21
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:22:26
Volume	10.00 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.885	1049023	195310	100.000	100.000	N/A	2943	N/A	1.301	

Creator Administrator
Reviewer
Approver

Chromatogram

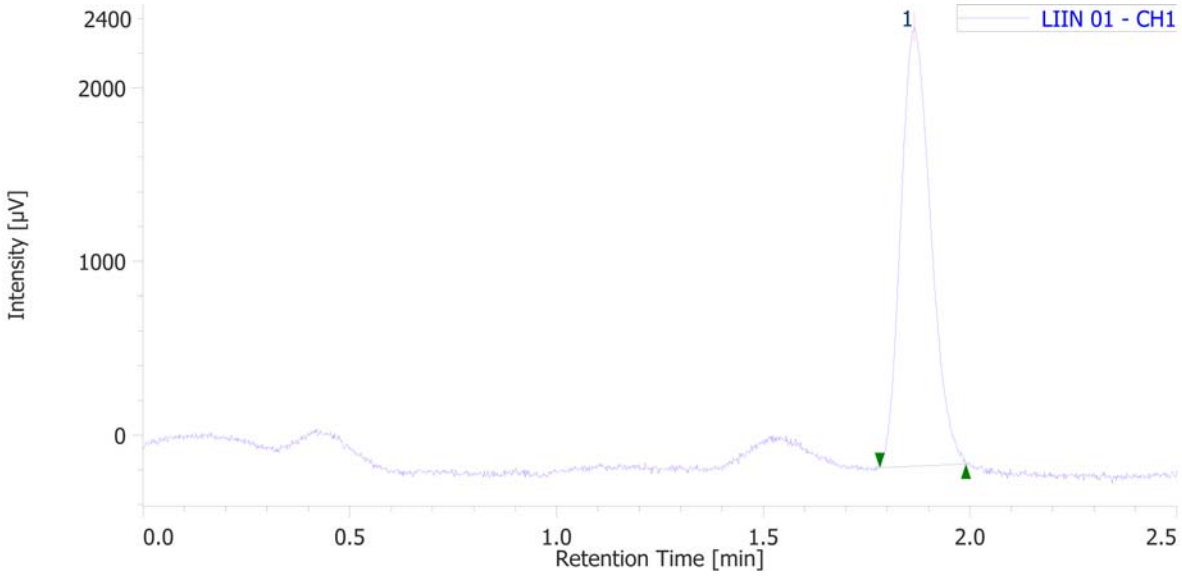

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 14:07:55
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:25:40
Volume	0.10 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.865	12701	2529	100.000	100.000	N/A	3089	N/A	1.228	

Creator Administrator
Reviewer
Approver

Chromatogram

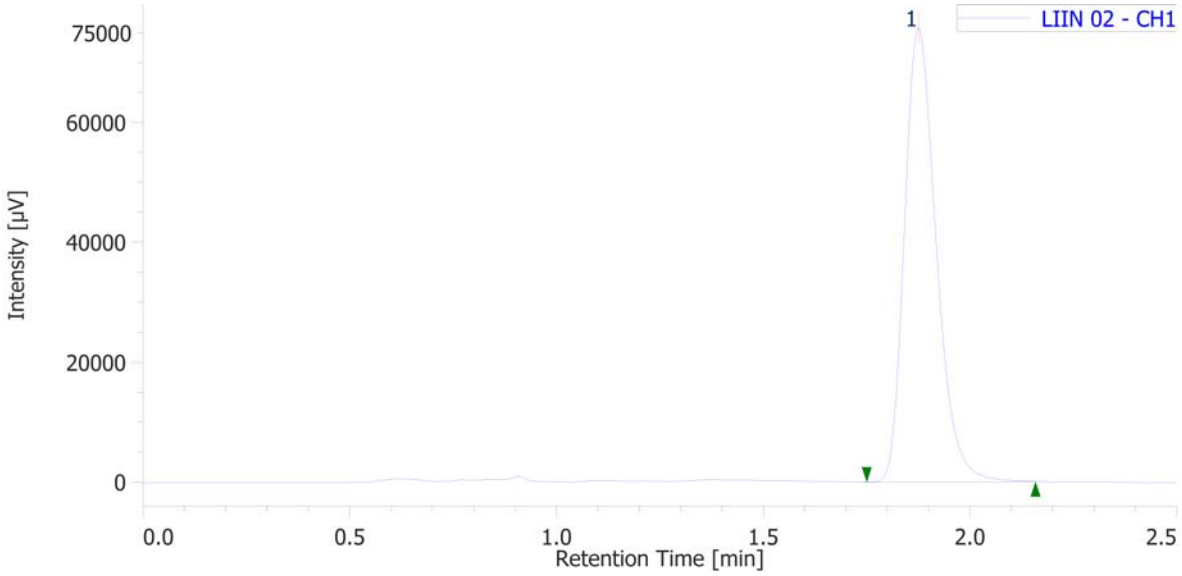

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:59:17
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:28:56
Volume	5.00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.875	404783	75922	100.000	100.000	N/A	2953	N/A	1.291	

Creator Administrator
Reviewer
Approver

Chromatogram

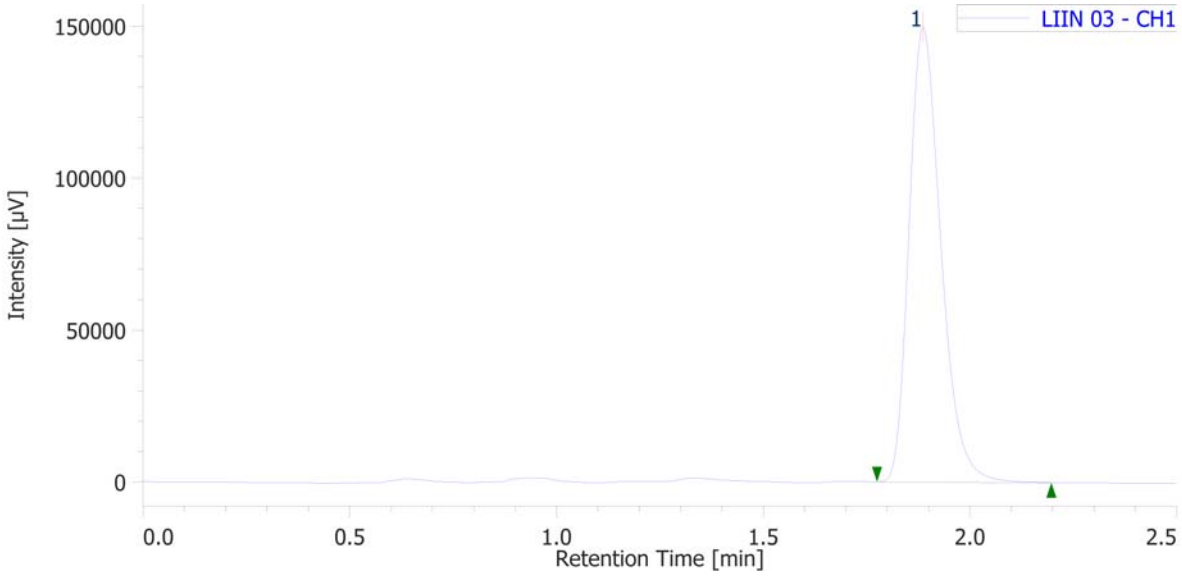

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:59:17
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:32:16
Volume	10.00 [μL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.887	801400	149716	100.000	100.000	N/A	2959	N/A	1.290	

Creator Administrator
Reviewer
Approver

Chromatogram

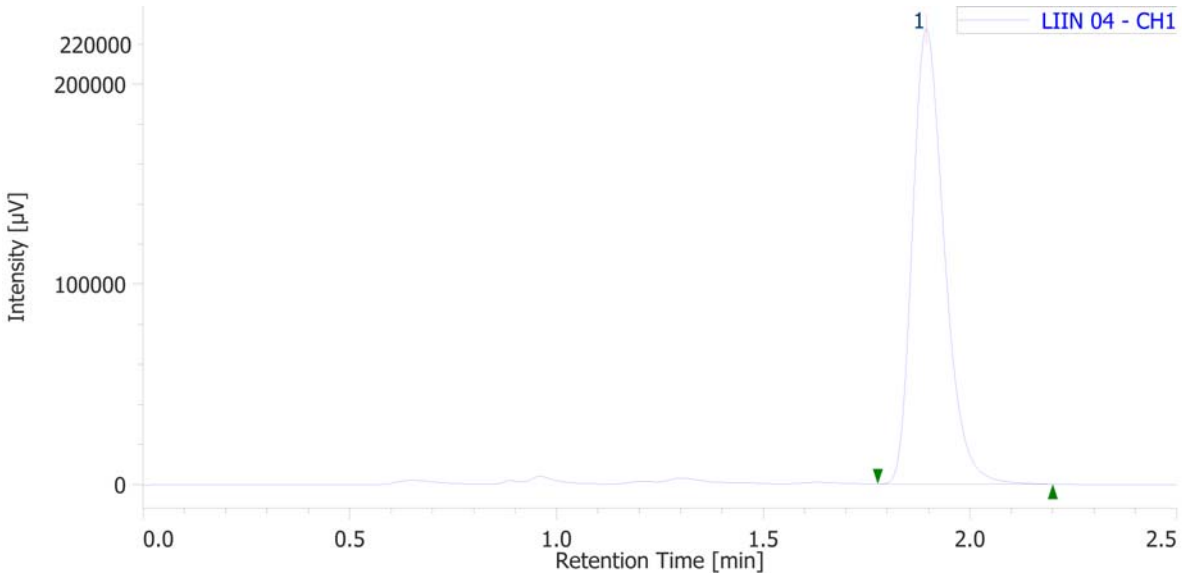

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:59:18
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:35:38
Volume	15.00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.893	1219087	227231	100.000	100.000	N/A	2975	N/A	1.327	

Creator Administrator
Reviewer
Approver

Chromatogram

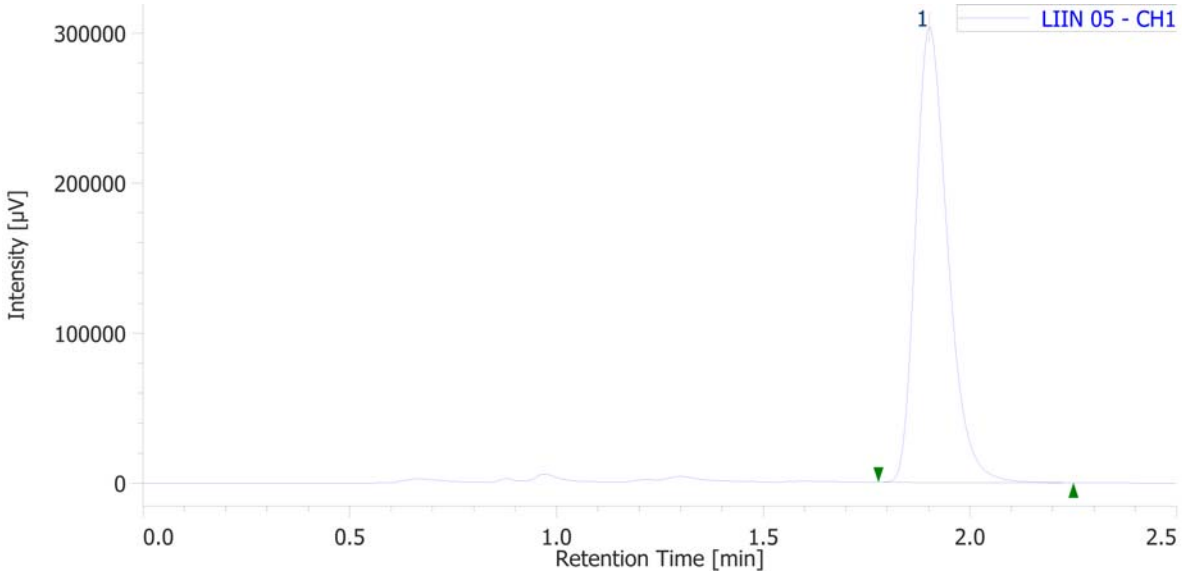

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 13:59:19
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 12:39:03
Volume	20.00 [μL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Id
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.902	1638947	303460	100.000	100.000	N/A	2970	N/A	1.325	

Creator Administrator
Reviewer
Approver

Chromatogram

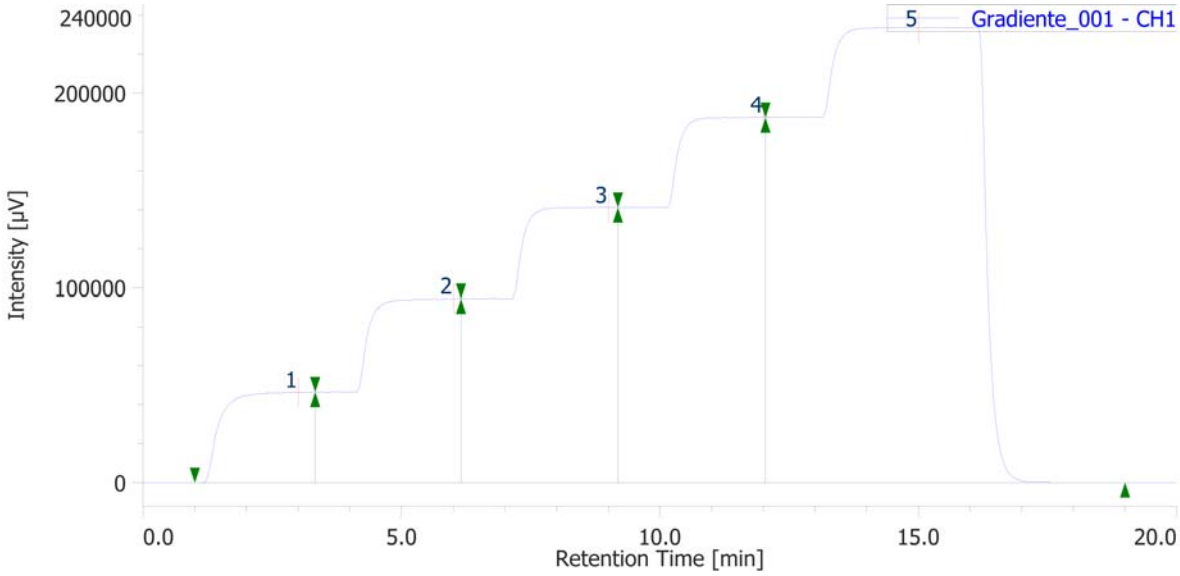

Chromatogram Information	
User Name	Administrator
Date Modified	08/05/2020 15:19:12
Description	
HPLC System Name	HPL20
Injection Date	08/05/2020 14:45:58
Volume	0.00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.000	5210017	46488	4.122	6.613	N/A	N/A	N/A	N/A	
2	40%	1	6.000	13050674	94374	10.325	13.426	N/A	N/A	N/A	N/A	
3	60%	1	9.000	22348500	141072	17.681	20.069	N/A	N/A	N/A	N/A	
4	80%	1	12.000	28903029	187432	22.866	26.665	N/A	N/A	N/A	N/A	
5	100%	1	15.000	56888156	233558	45.006	33.227	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver