
Peak Find - EDUV 01_025 PDA_1,4750.JWS

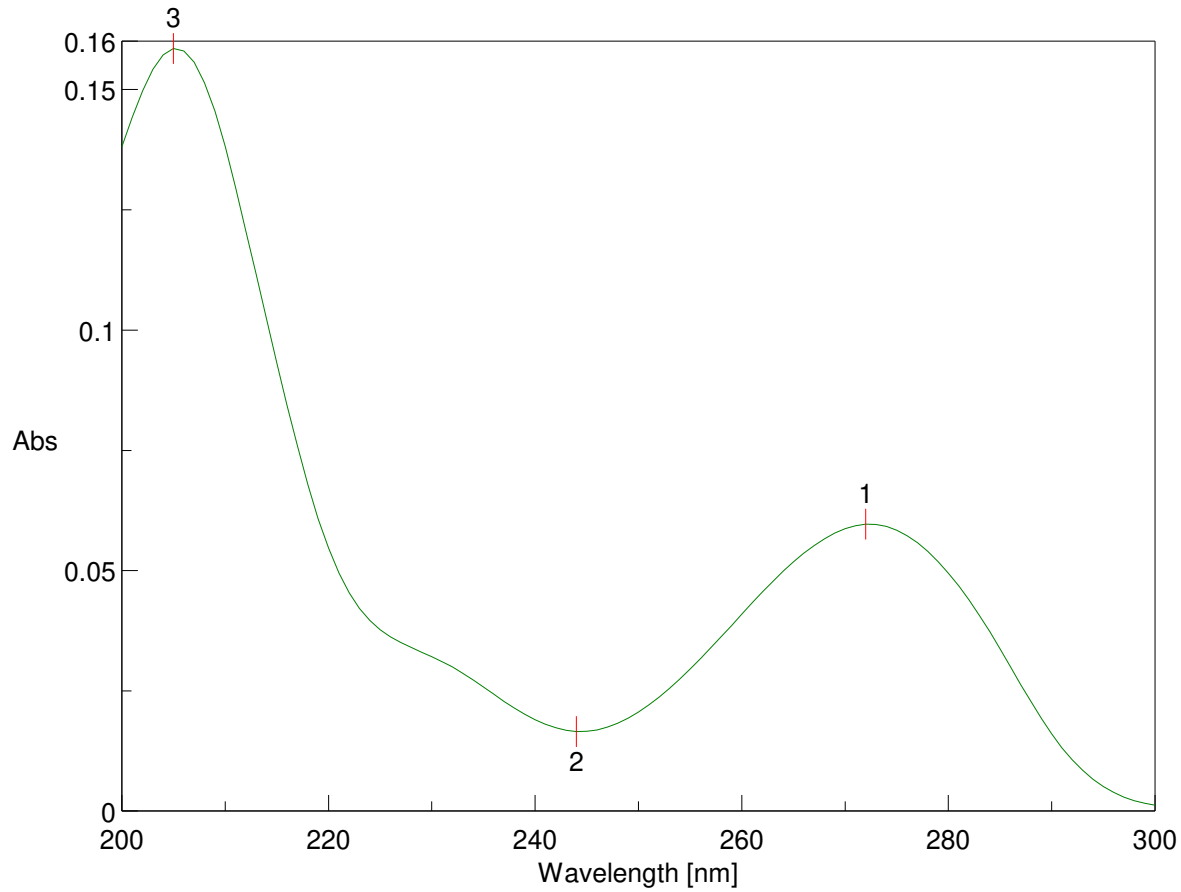

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	20/02/2025 17:12
Date modified	20/02/2025 17:17

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.059591	2	244	0.016532
3	205	0.158459			

Chromatogram

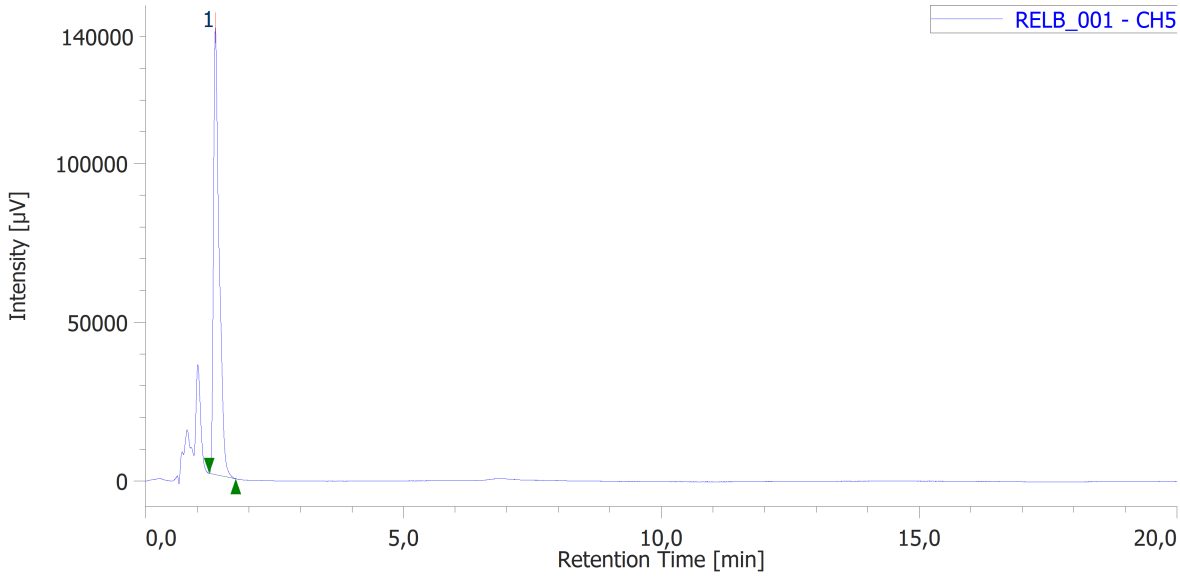

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 20:07:47
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:44:19
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_001-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,350	1076916	140570	100,000	100,000	N/A	810	N/A	1,708		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

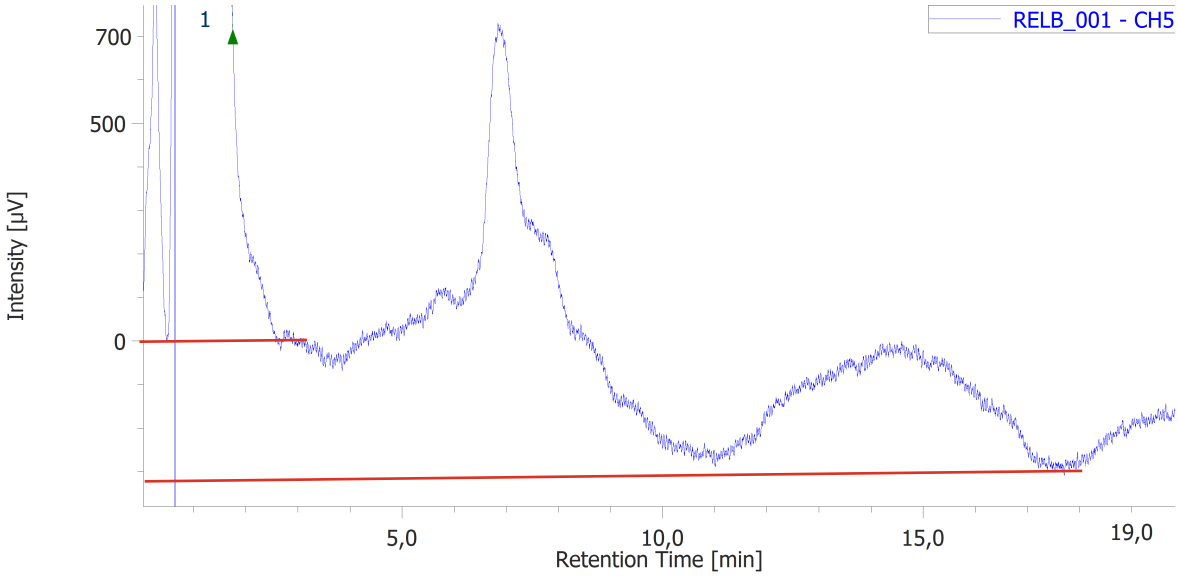

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 20:07:47
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:44:19
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_001-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,350	1076916	140570	100,000	100,000	N/A	810	N/A	1,708		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

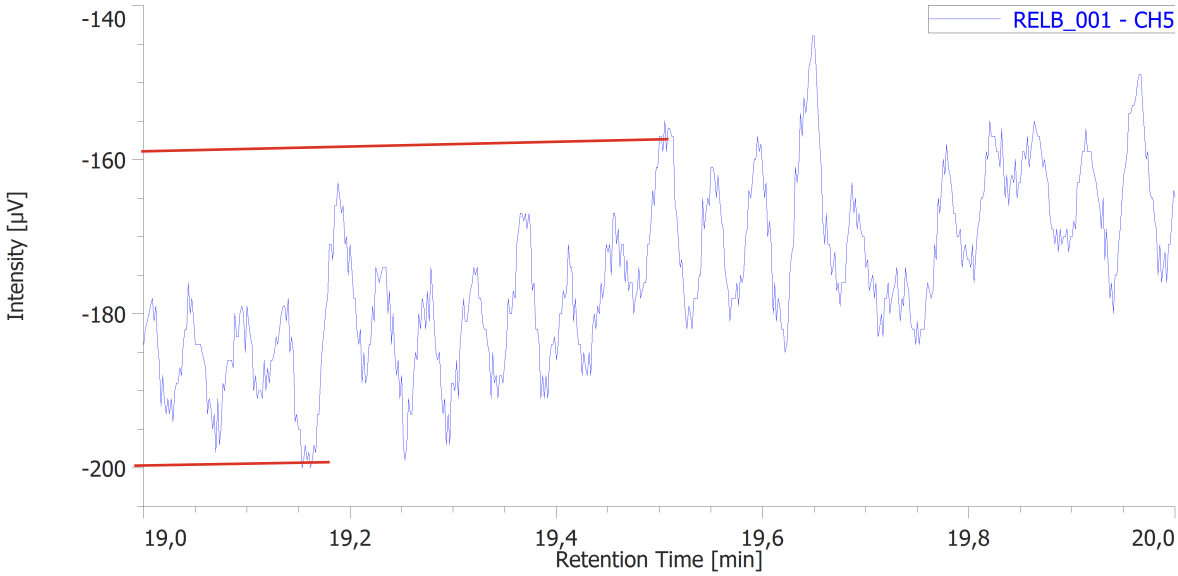

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 20:07:47
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:44:19
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_001-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,350	1076916	140570	100,000	100,000	N/A	810	N/A	1,708		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

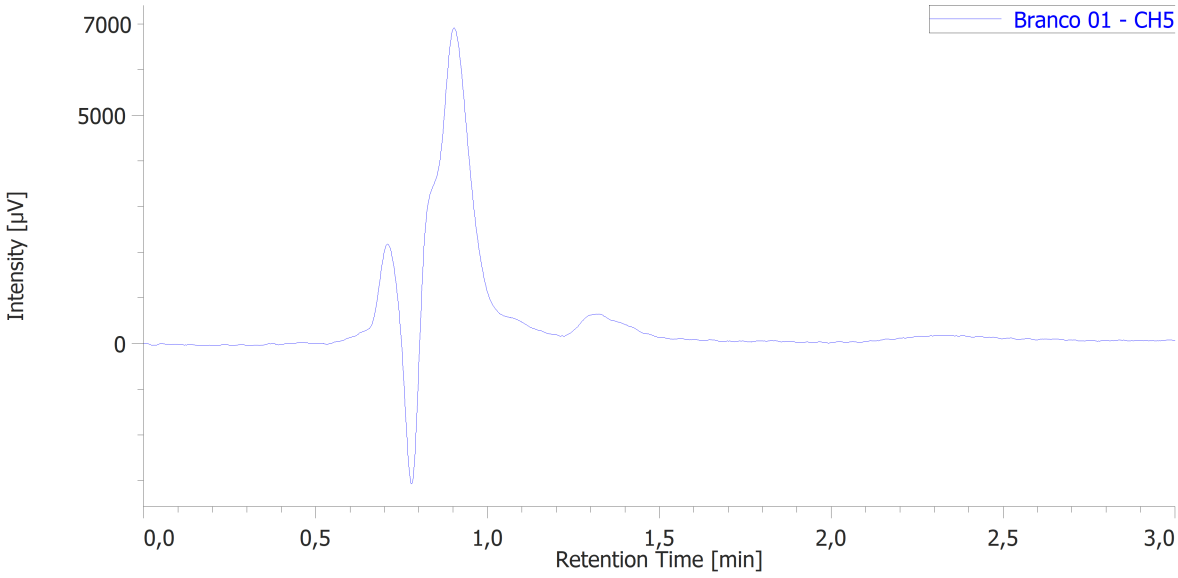


Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:10:40
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:07:38
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

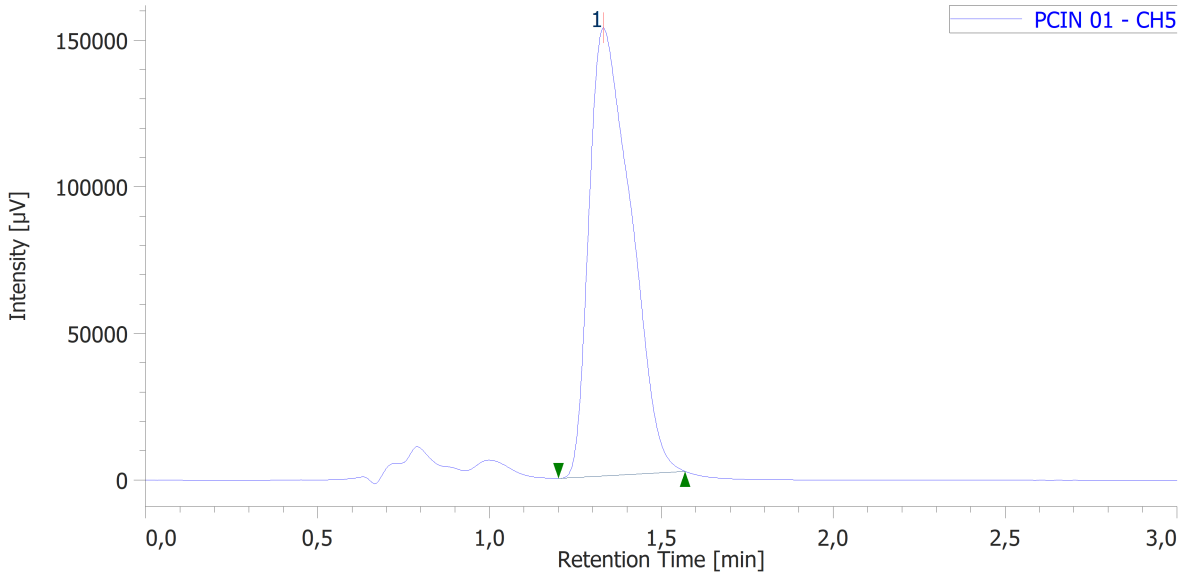

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:45:55
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:10:51
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,332	1292044	152643	100,000	100,000	N/A	491	N/A	1,526		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

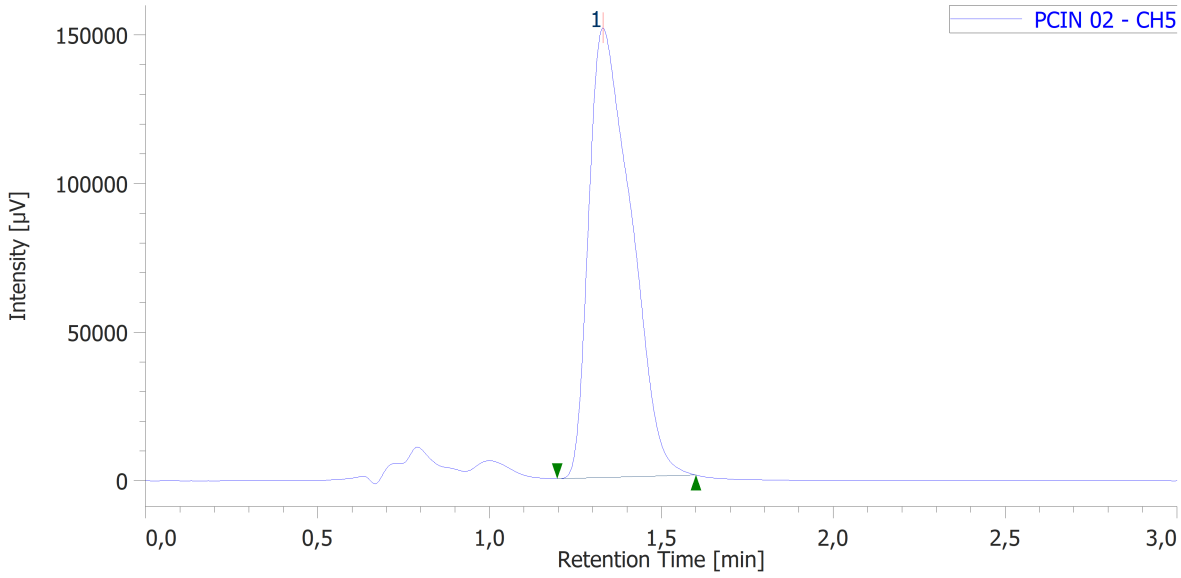

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:45:57
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:14:03
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,330	1290965	151106	100,000	100,000	N/A	483	N/A	1,576		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

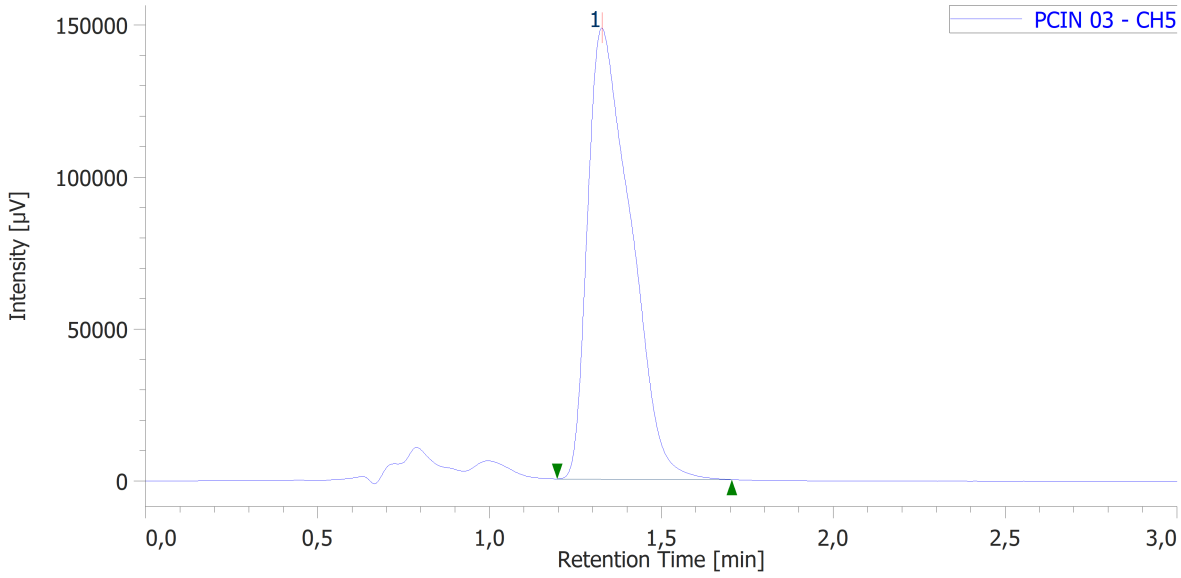

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:20:18
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:17:15
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,327	1291074	148324	100,000	100,000	N/A	469	N/A	1,622		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

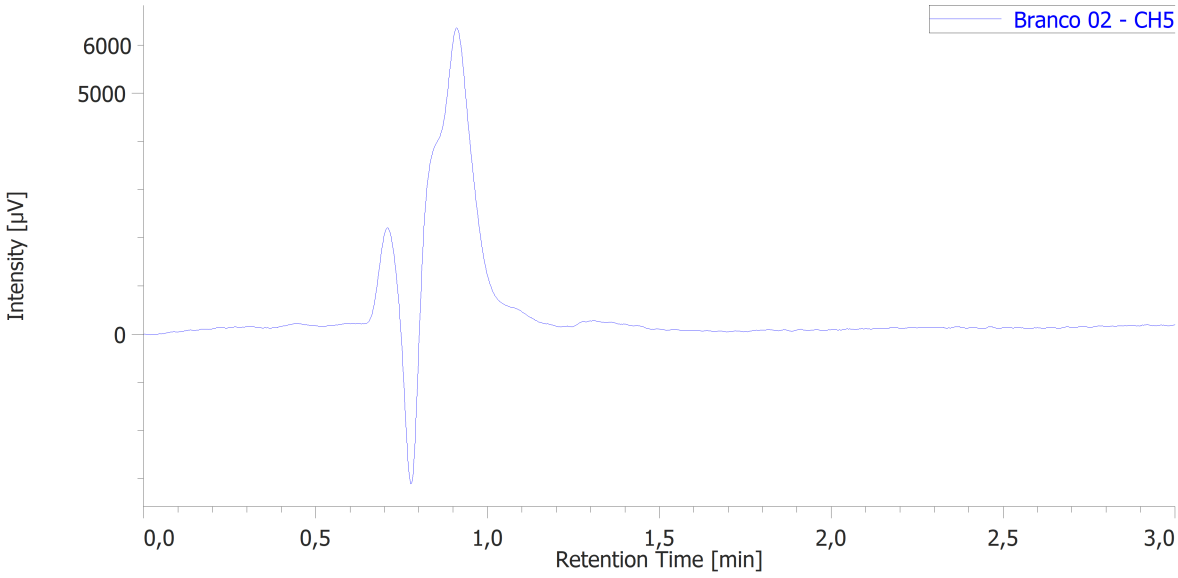


Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:23:30
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:20:27
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

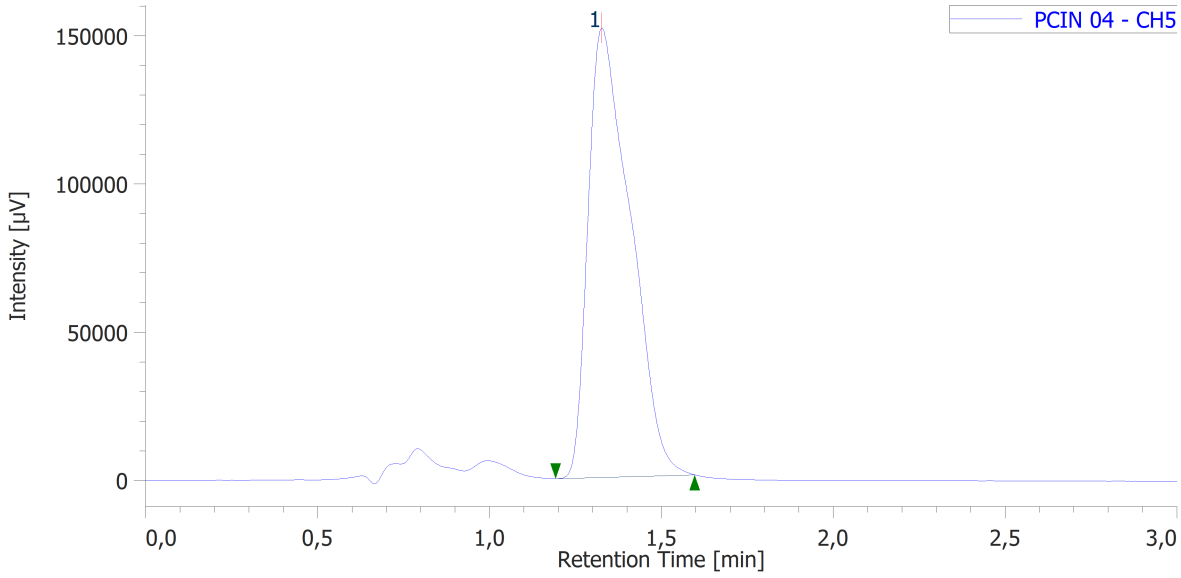

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:45:57
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:23:40
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,327	1298722	151466	100,000	100,000	N/A	470	N/A	1,634		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

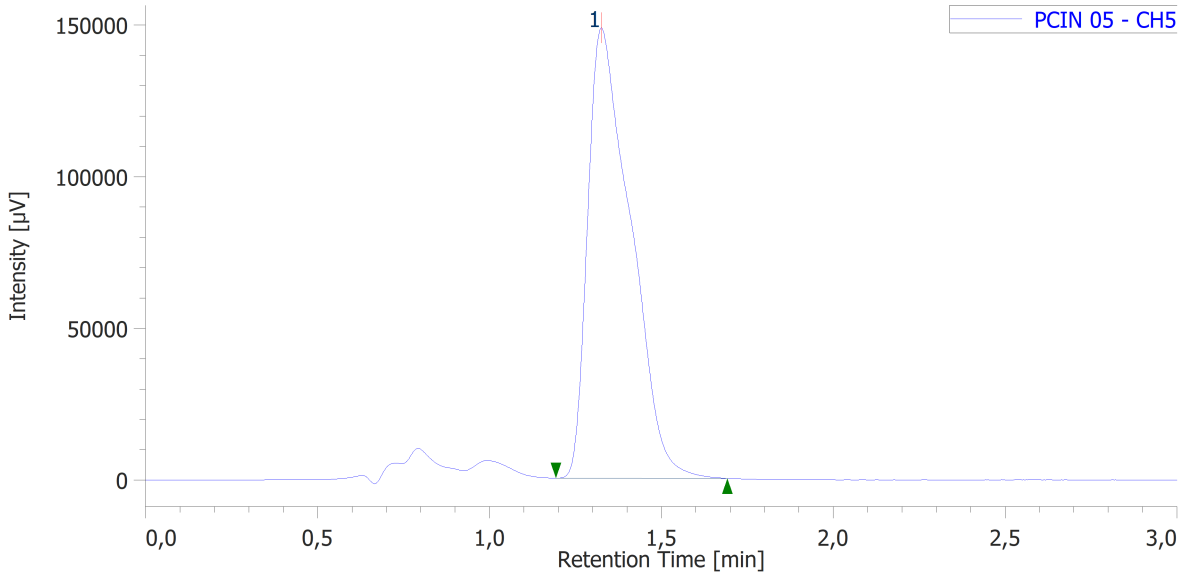

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:29:54
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:26:52
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,325	1288256	148360	100,000	100,000	N/A	461	N/A	1,691		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

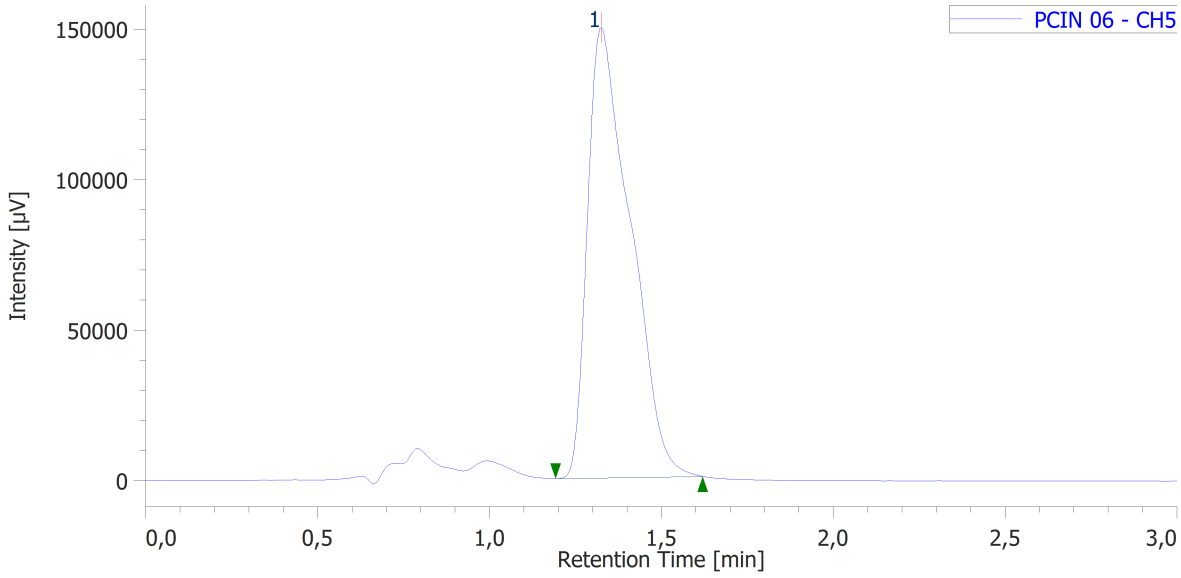

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:45:58
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:30:04
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,325	1296264	149348	100,000	100,000	N/A	457	N/A	1,679		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

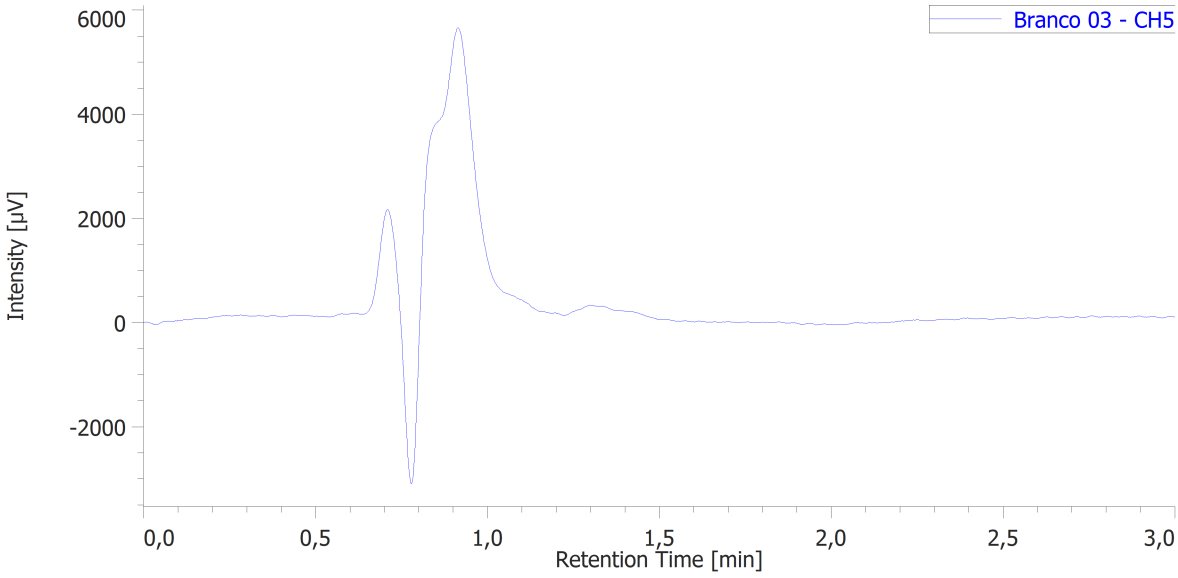


Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 18:36:18
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 18:33:16
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

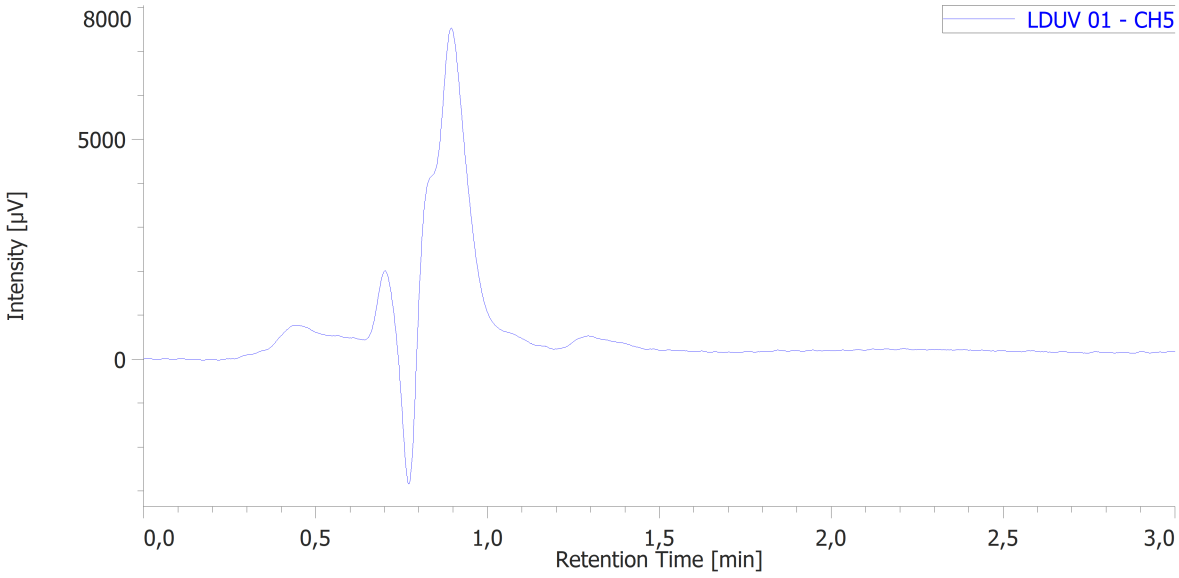


Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:05:24
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:02:22
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

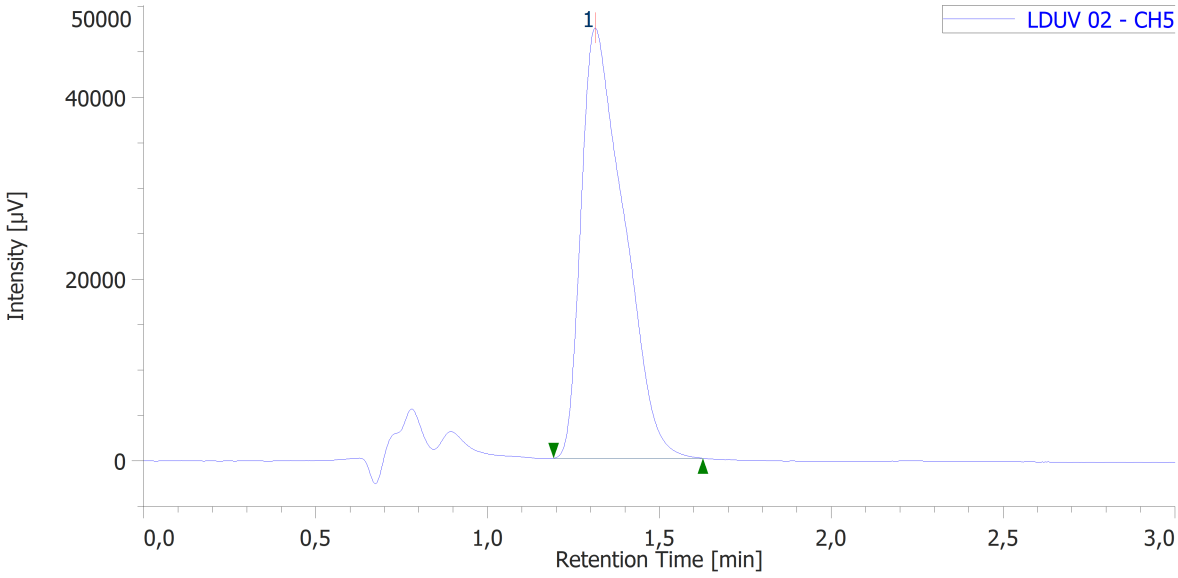

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:08:36
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:05:34
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,313	408943	47344	100,000	100,000	N/A	476	N/A	1,637		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

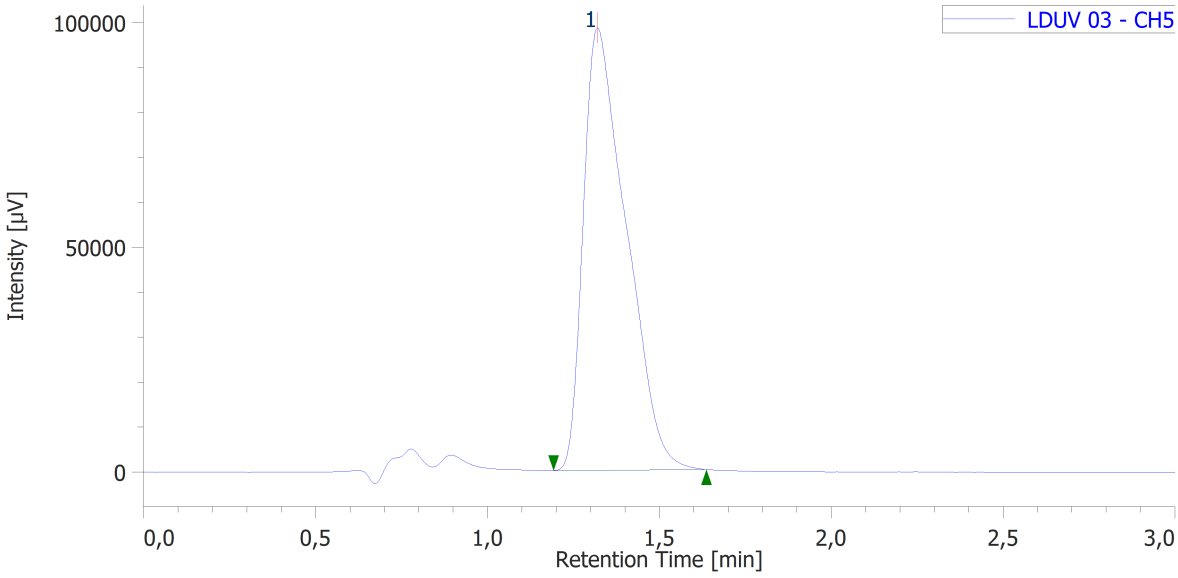

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:11:48
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:08:46
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,320	852857	98380	100,000	100,000	N/A	492	N/A	1,649		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

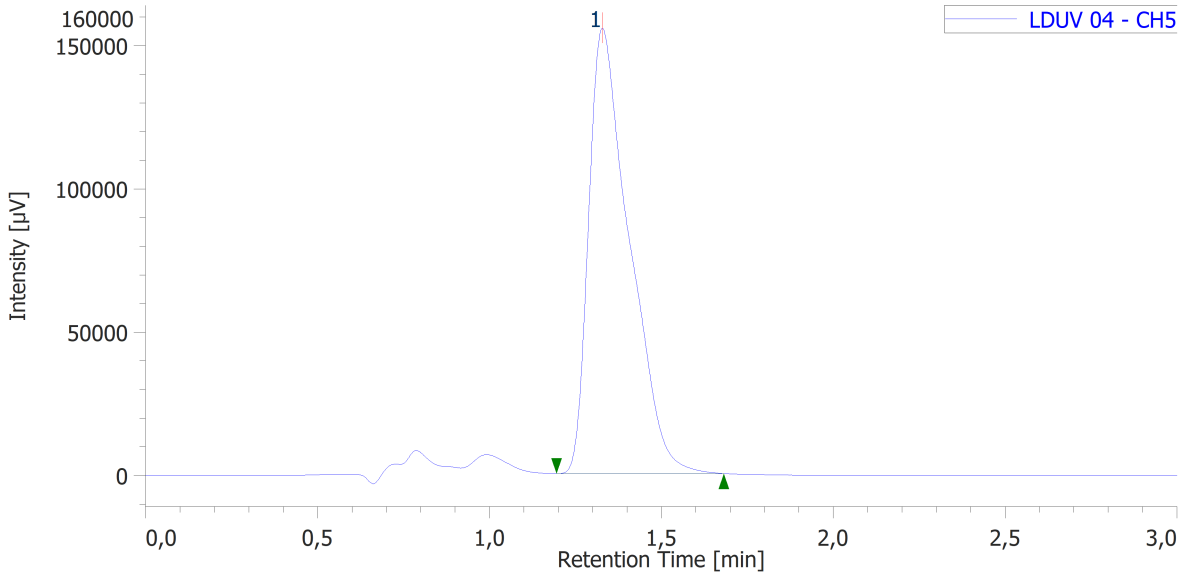

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:15:00
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:11:58
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,328	1280196	155425	100,000	100,000	N/A	599	N/A	1,659		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

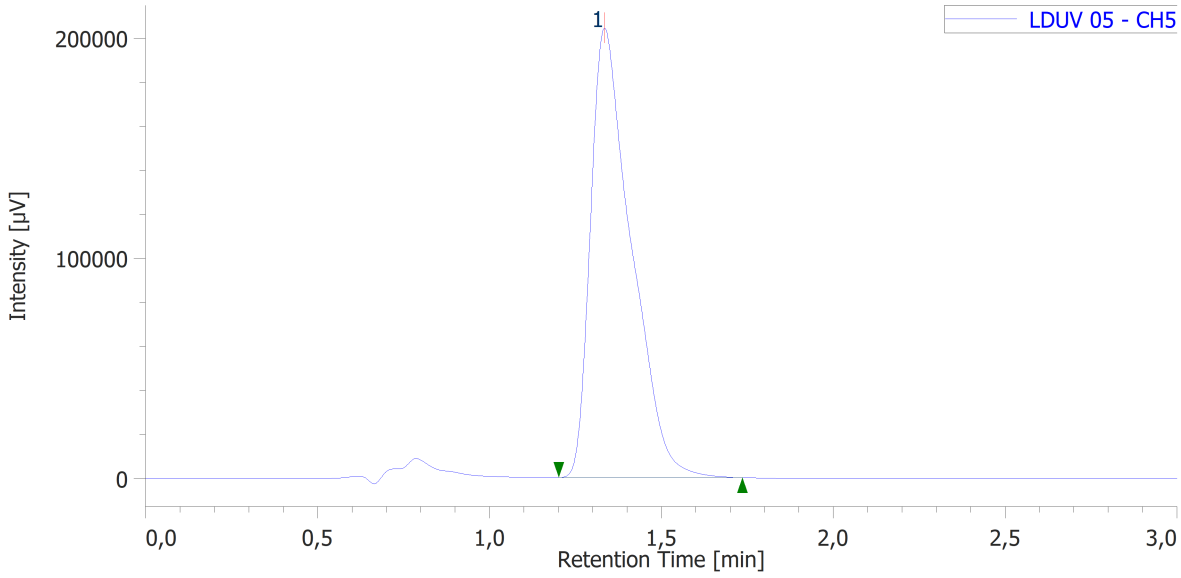

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:18:14
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:15:10
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Sequência Qualificação QPack
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,335	1677592	204125	100,000	100,000	N/A	621	N/A	1,622		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

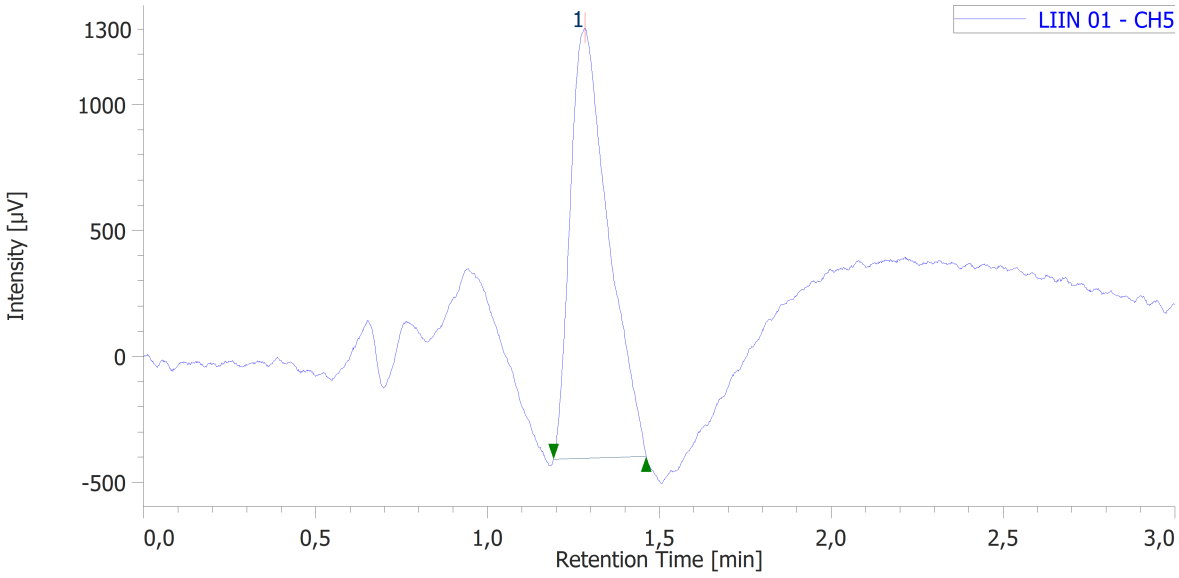

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:26:22
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:23:19
Volume	0,1 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,283	13176	1708	100,000	100,000	N/A	649	N/A	1,515		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

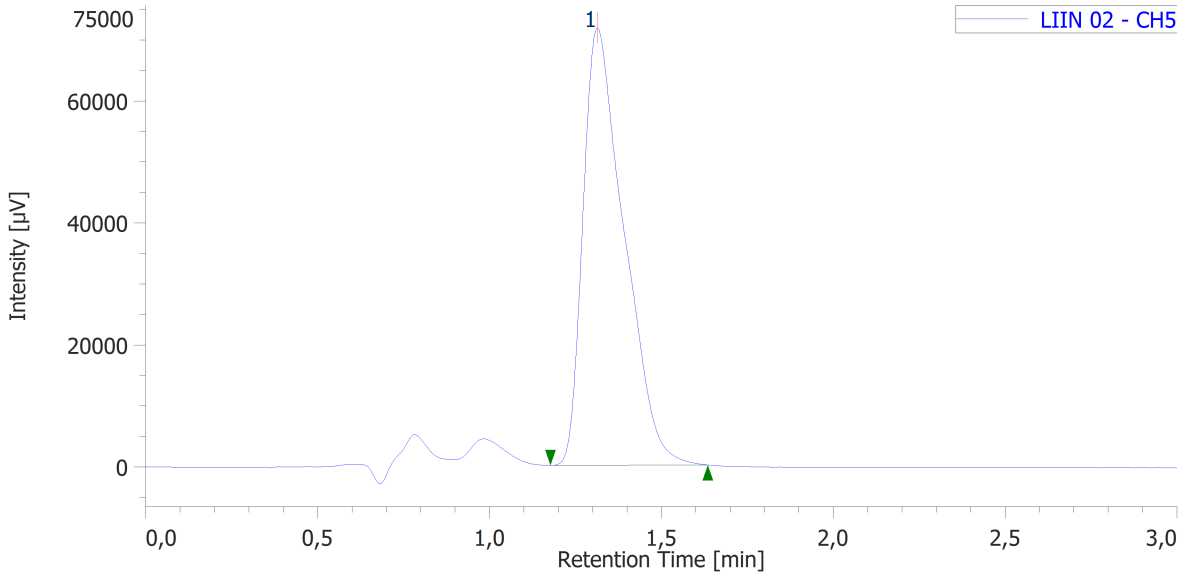

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:29:34
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:26:32
Volume	5,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,313	595374	71671	100,000	100,000	N/A	560	N/A	1,600		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

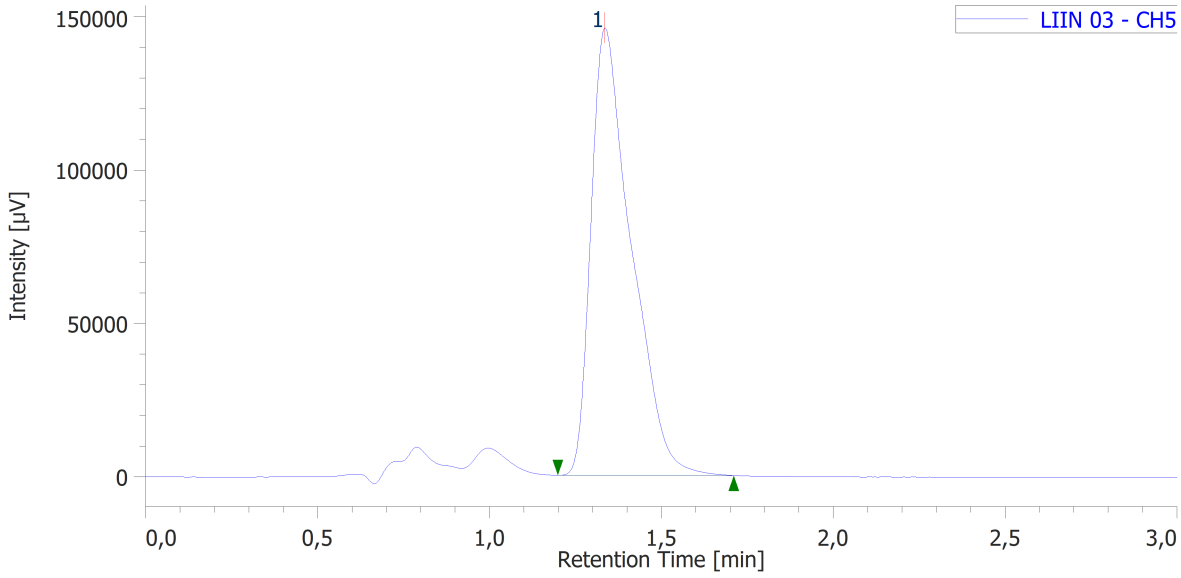

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:32:46
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:29:44
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,335	1184909	145770	100,000	100,000	N/A	646	N/A	1,644		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

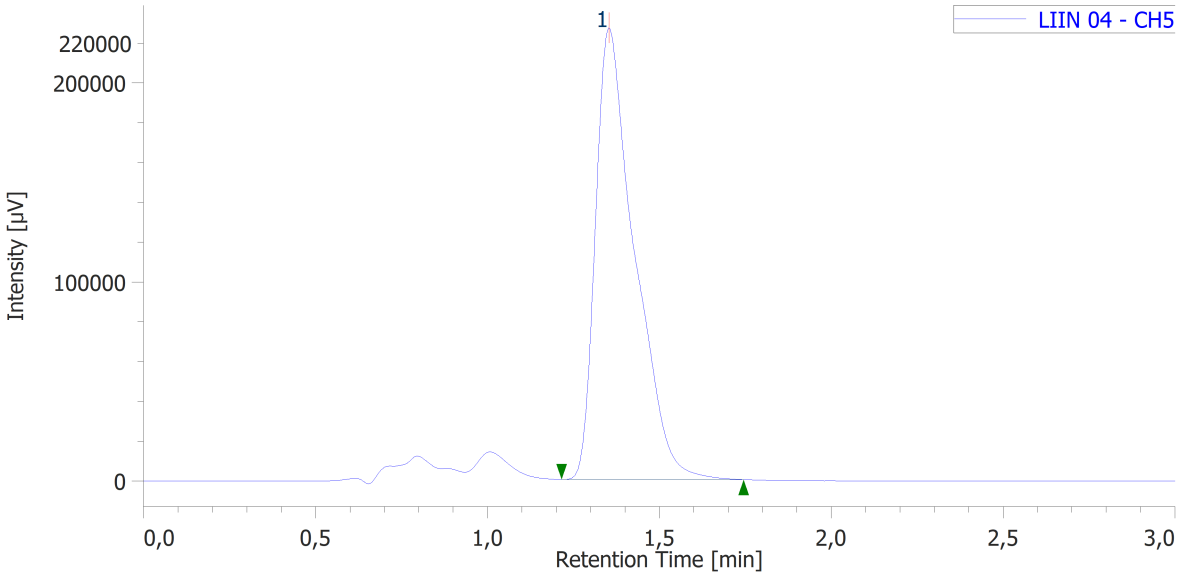

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:35:58
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:32:56
Volume	15,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,353	1787723	226652	100,000	100,000	N/A	734	N/A	1,636		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

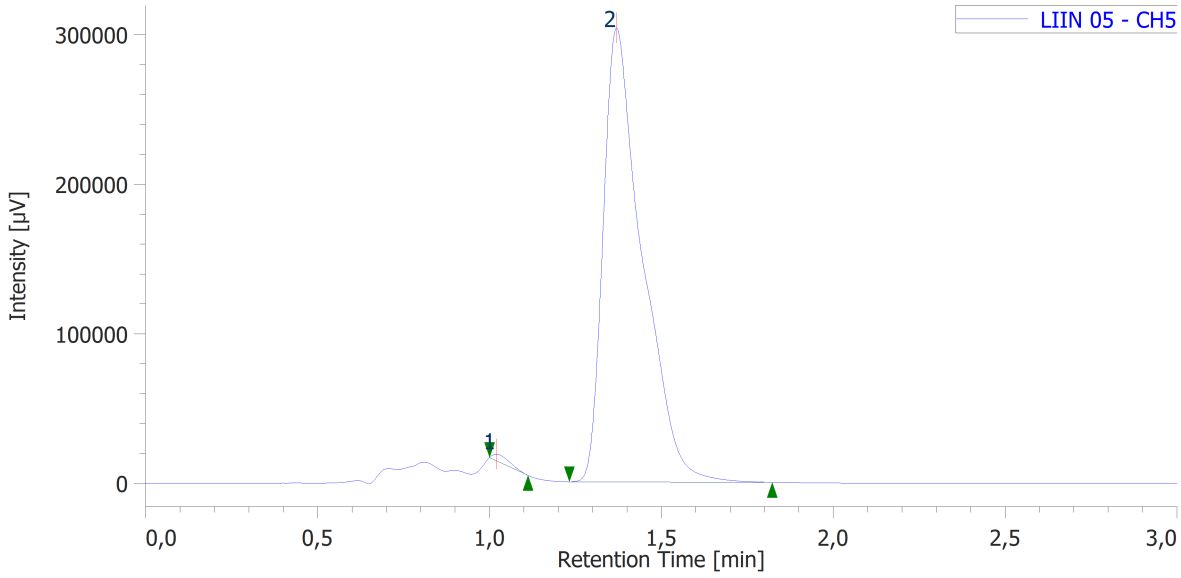

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 19:39:10
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 19:36:08
Volume	20,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	5	1,020	16634	4359	0,690	1,416	N/A	1542	2,338	2,544		N/A
2	Cafeína	5	1,370	2395018	303383	99,310	98,584	N/A	779	N/A	1,664		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

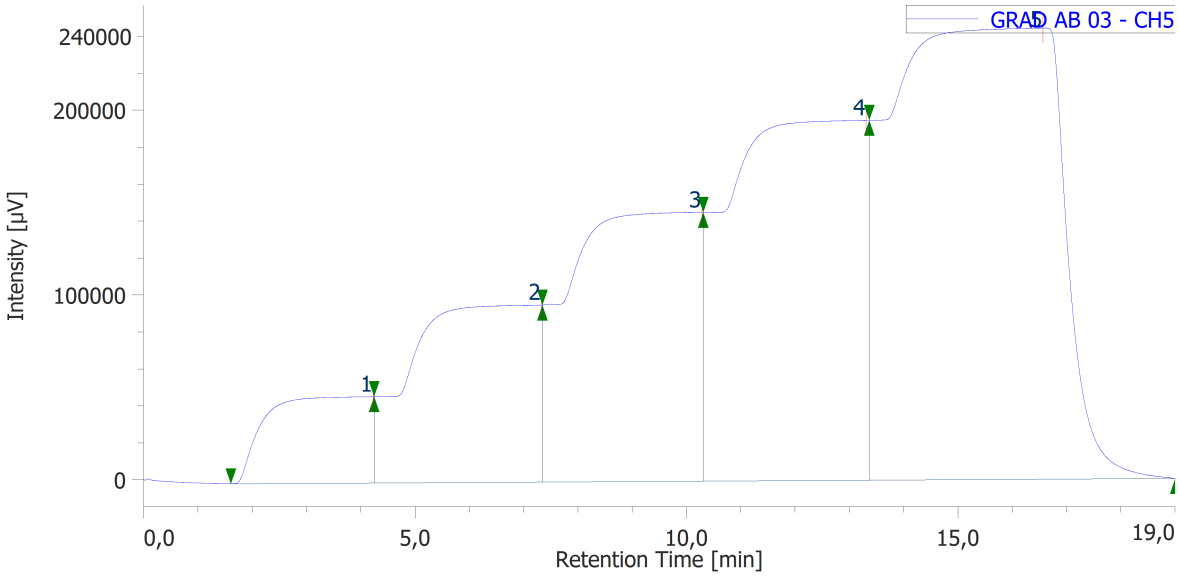

Chromatogram Information	
User Name	QPackSA
Date Modified	21/02/2025 09:01:06
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 21:05:49
Volume	0,1 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Sequência Gradiente
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20%	5	4,227	6002493	46634	4,588	6,421	N/A	N/A	N/A	N/A		N/A
2	40%	5	7,325	15289129	95737	11,687	13,183	N/A	N/A	N/A	N/A		N/A
3	60%	5	10,285	23599848	145322	18,039	20,010	N/A	N/A	N/A	N/A		N/A
4	80%	5	13,305	33385199	194582	25,519	26,793	N/A	N/A	N/A	N/A		N/A
5	100%	5	16,560	52548509	243962	40,167	33,593	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

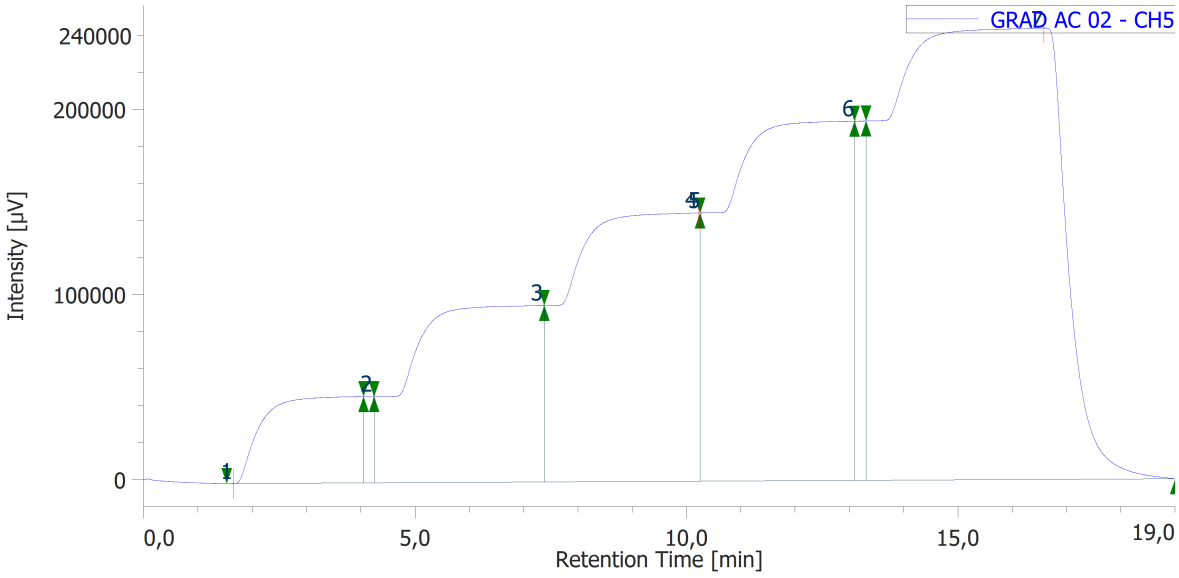

Chromatogram Information	
User Name	QPackSA
Date Modified	20/02/2025 22:03:15
Description	
HPLC System Name	HP06
Injection Date	20/02/2025 21:44:13
Volume	0,1 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Sequência Gradiente
Control Method	Gradiente AC
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD AC 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	5	1,653	-1799	121	N/A	0,014	N/A	1439	N/A	0,672		N/A
2	20%	5	4,228	540314	46610	0,432	5,360	N/A	N/A	N/A	N/A		N/A
3	40%	5	7,367	15466173	95342	12,376	10,965	N/A	N/A	N/A	N/A		N/A
4	60%	5	10,208	22772606	144892	18,222	16,663	N/A	N/A	N/A	N/A		N/A
5	Unknown	5	10,262	30681922	144854	24,551	16,659	N/A	N/A	N/A	N/A		N/A
6	80%	5	13,103	2463546	193928	1,971	22,302	N/A	N/A	N/A	N/A		N/A
7	100%	5	16,582	53050411	243788	42,449	28,037	N/A	N/A	N/A	N/A		N/A

Creator
Reviewer
Approver