
Peak Find - EDUV_009 PDA_2,7967.JWS

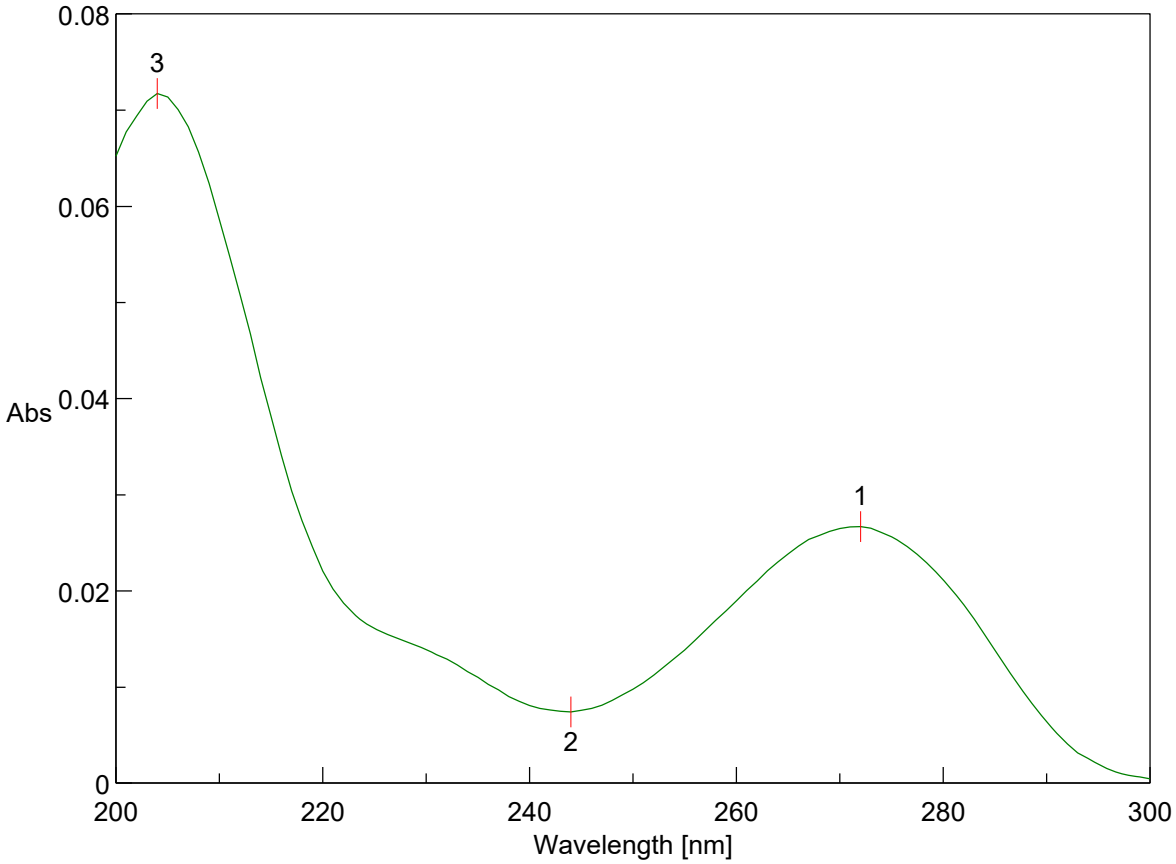

[Comments]

User	Administrator
Division	---
Company	QPack
Creation date	28/03/2022 15:40

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A031161665
ROM version	V1.02.03

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.026675	2	244	0.007396
3	204	0.071701			

Chromatogram

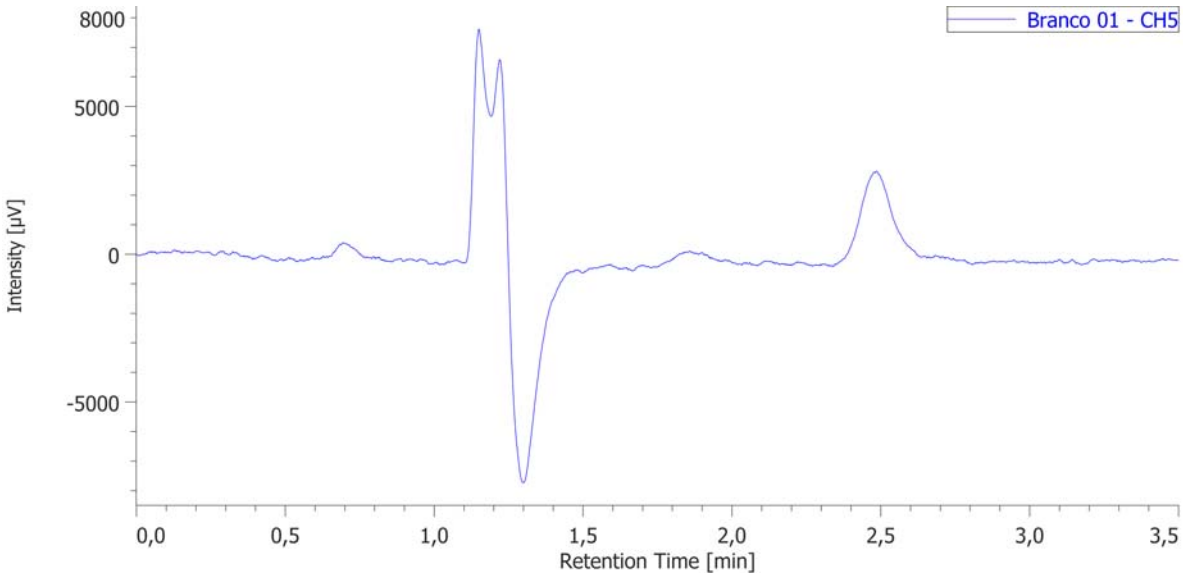


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:35
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 15:53:35
Volume	10,0 [µL]
Sample #	1
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Chromatogram

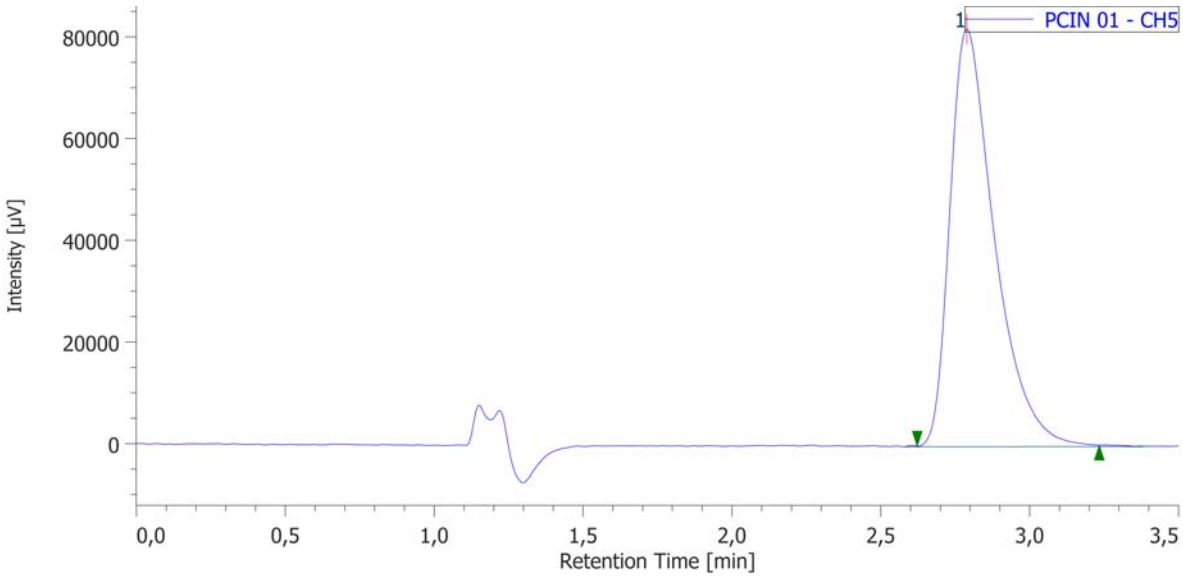


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 15:58:25
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,788	855447	82089	100,000	100,000	N/A	1791	N/A	1,591	

Chromatogram

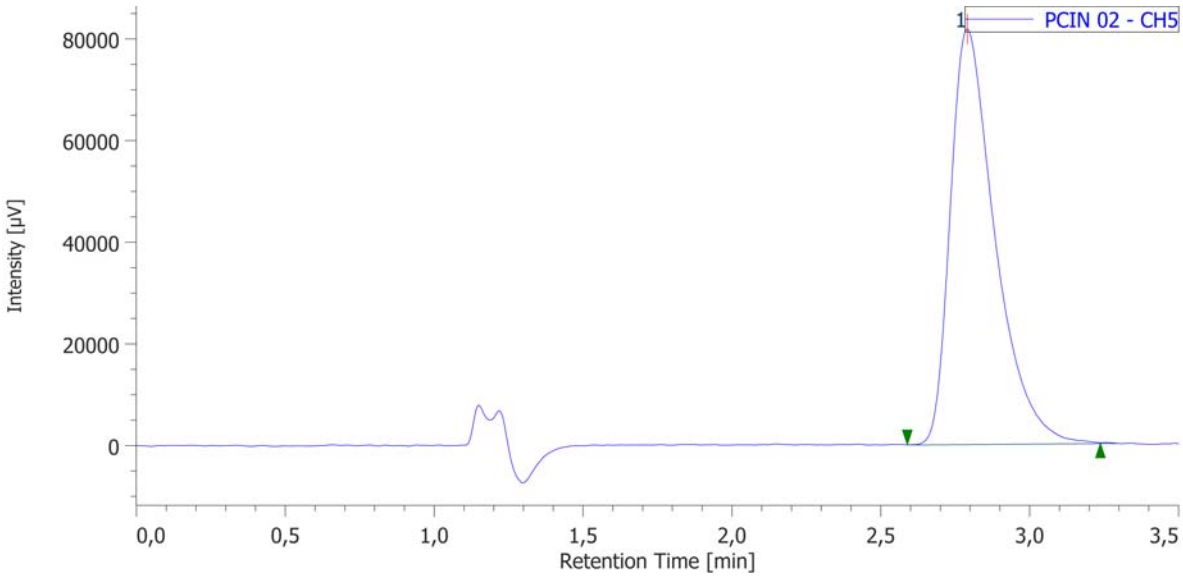


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:03:12
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,790	852908	81700	100,000	100,000	N/A	1786	N/A	1,588	

Chromatogram

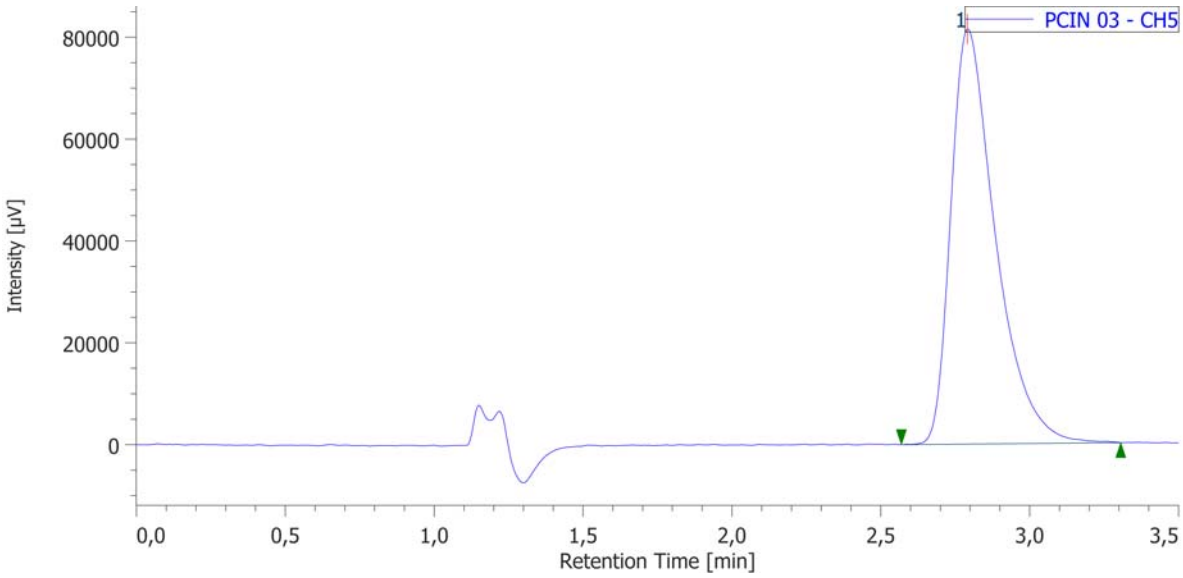


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:07:55
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,790	850030	81454	100,000	100,000	N/A	1789	N/A	1,619	

Chromatogram

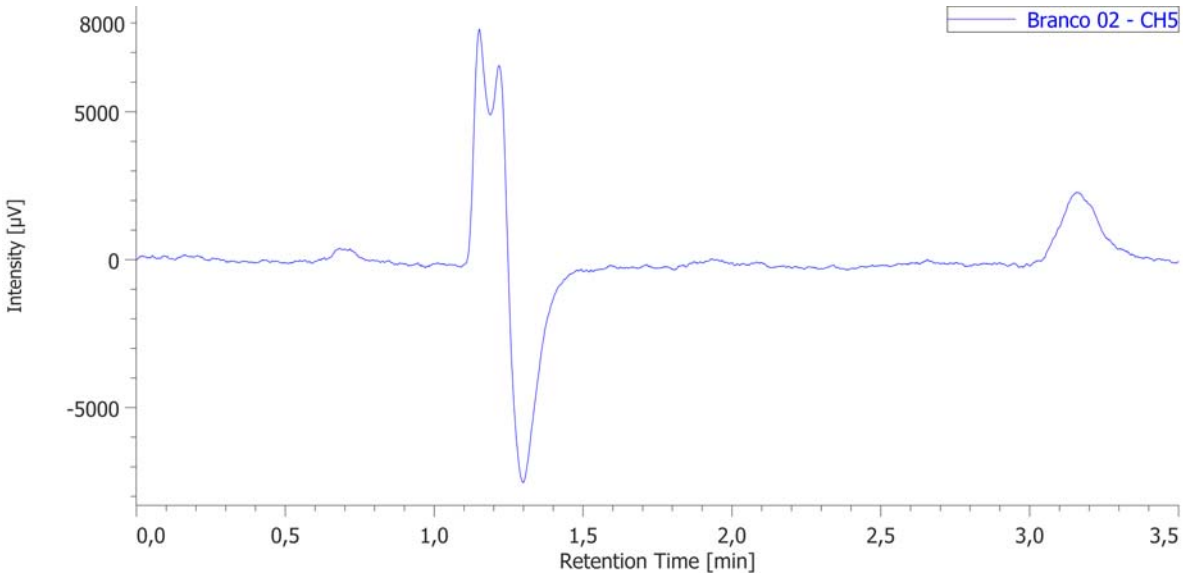


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:12:37
Volume	10,0 [µL]
Sample #	1
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Chromatogram

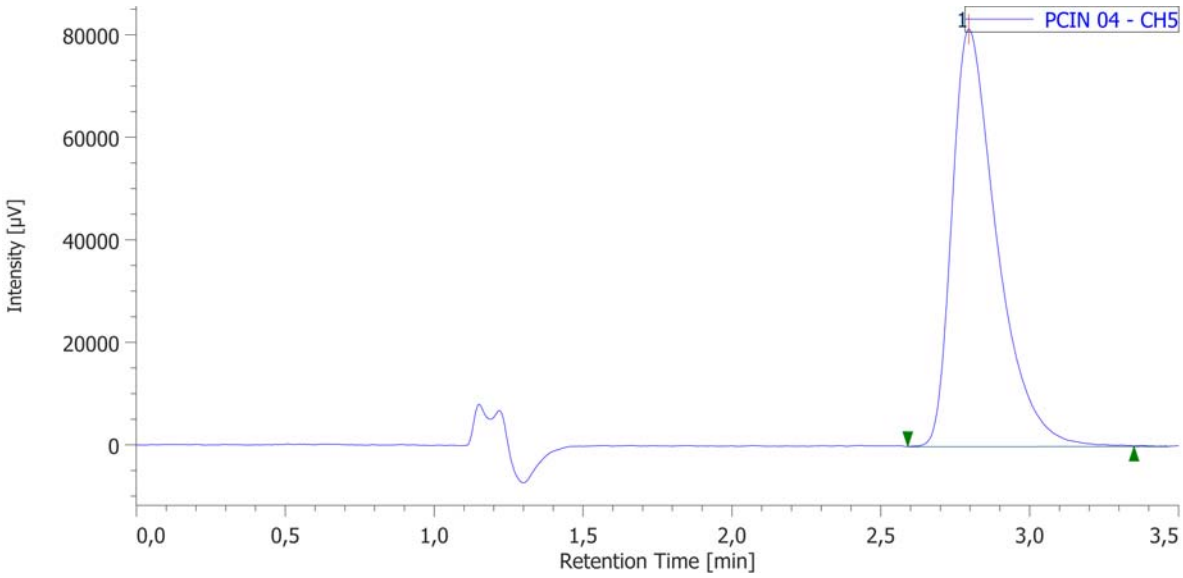


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:17:20
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,795	854472	81443	100,000	100,000	N/A	1791	N/A	1,606	

Chromatogram

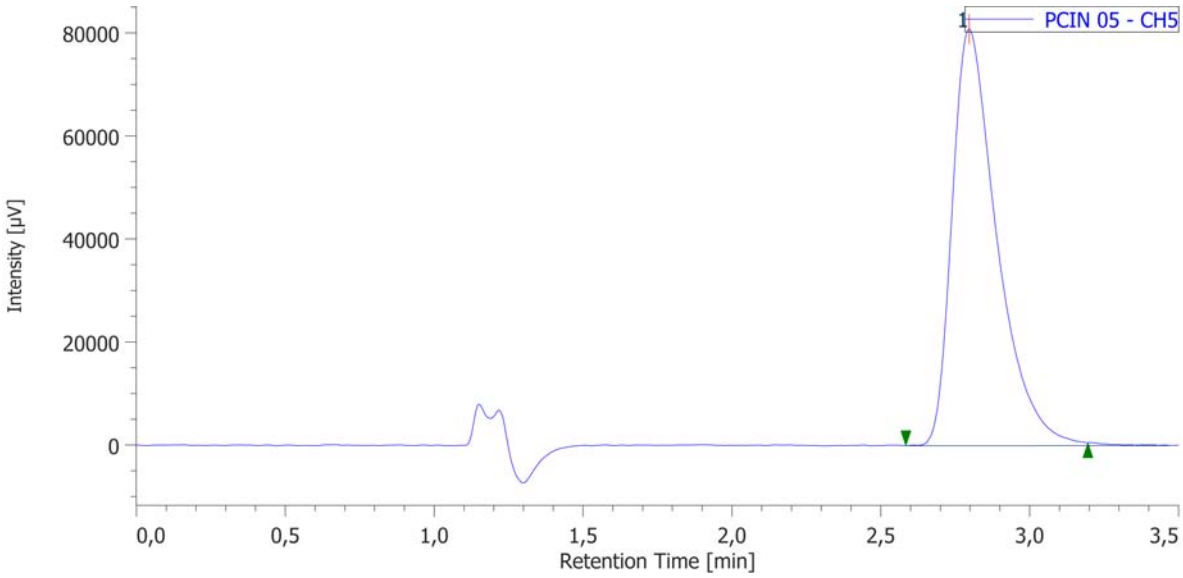


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:22:03
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,797	846009	80862	100,000	100,000	N/A	1793	N/A	1,583	

Chromatogram

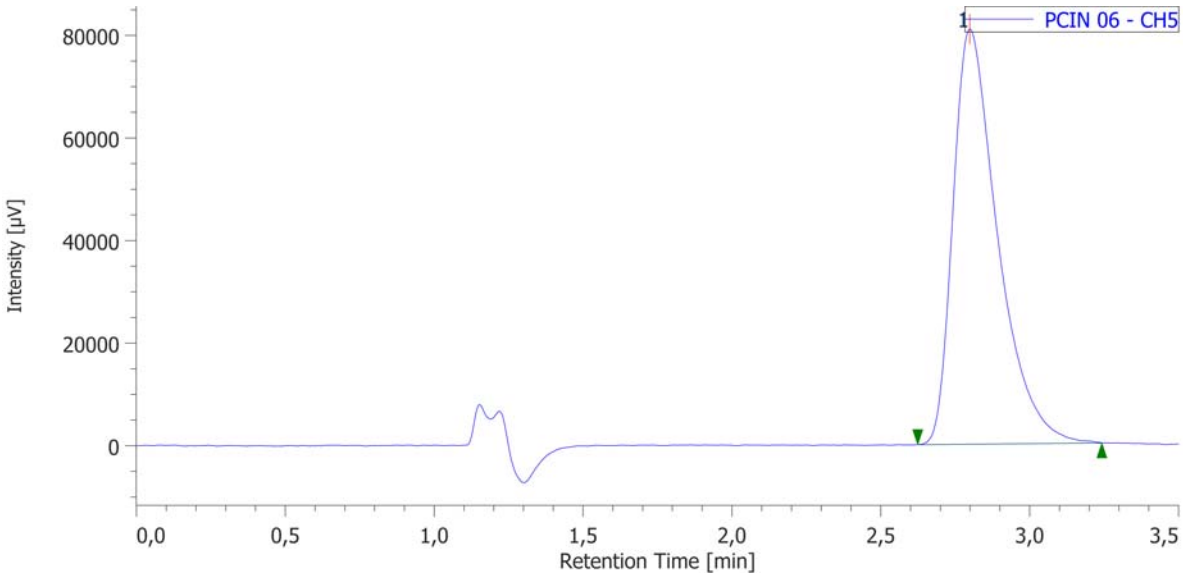


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:26:46
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,798	843127	80918	100,000	100,000	N/A	1797	N/A	1,598	

Chromatogram

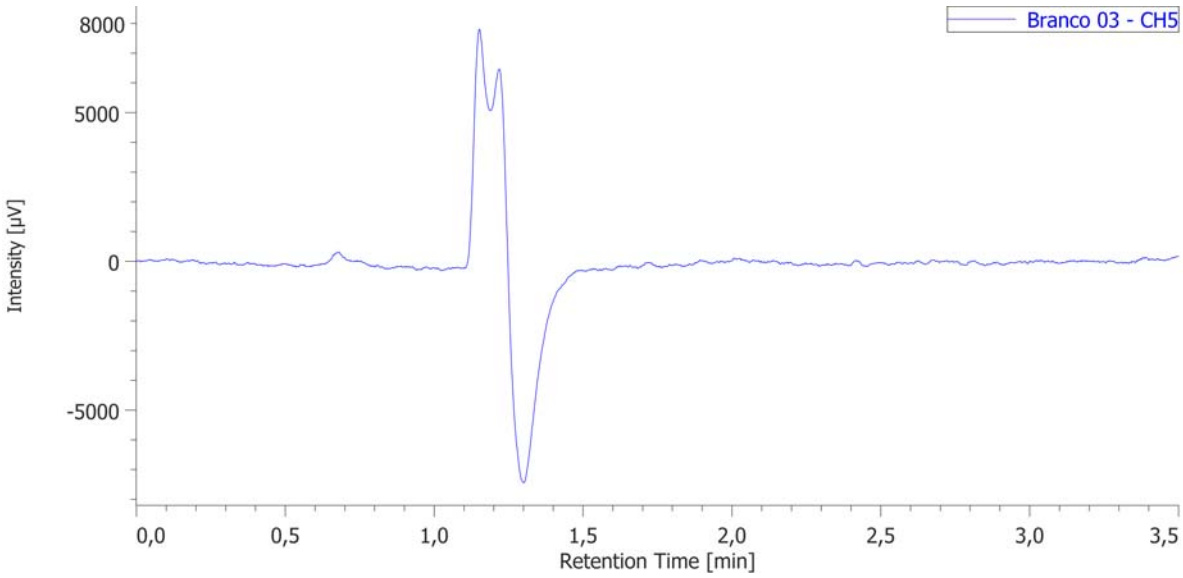


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:31:34
Volume	10,0 [µL]
Sample #	1
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Chromatogram

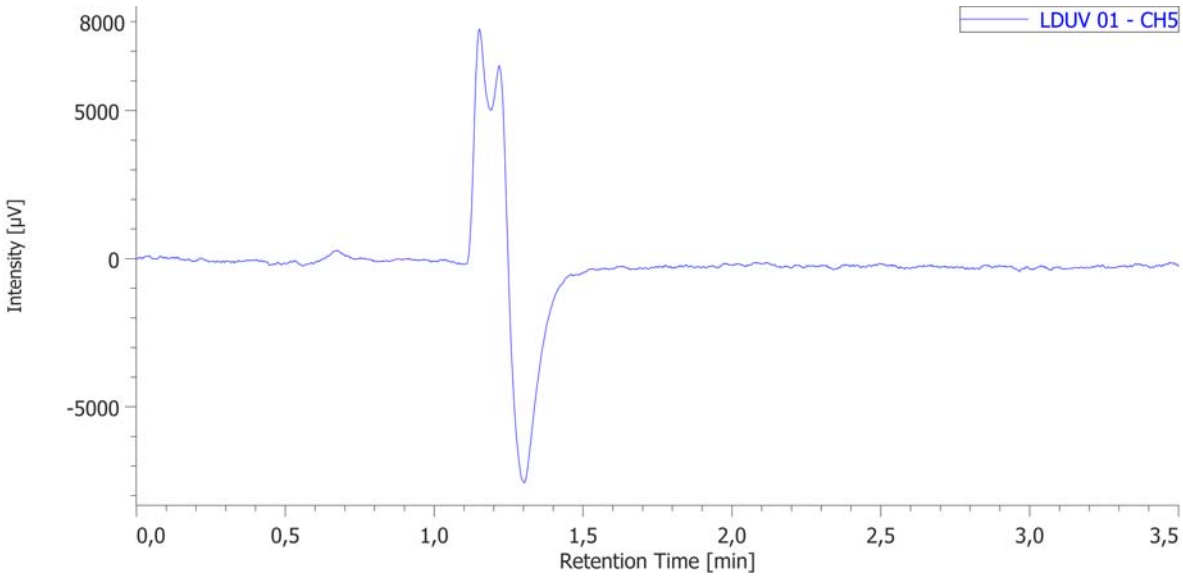


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:36:22
Volume	10,0 [µL]
Sample #	1
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Chromatogram

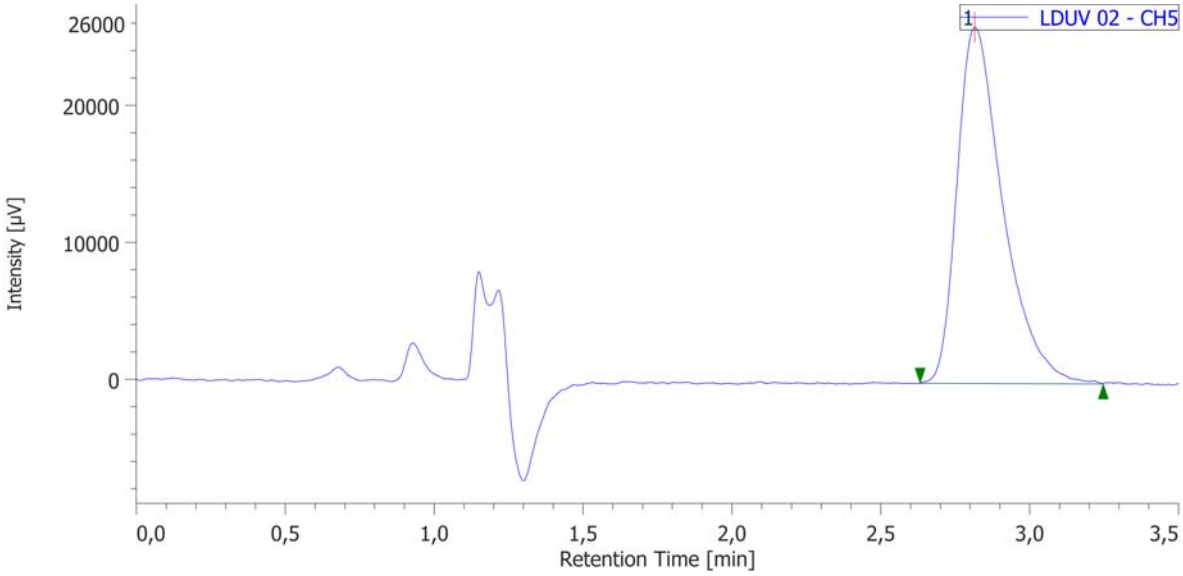


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:36
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:41:07
Volume	10,0 [µL]
Sample #	2
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,815	278659	26015	100,000	100,000	N/A	1732	N/A	1,546	

Chromatogram

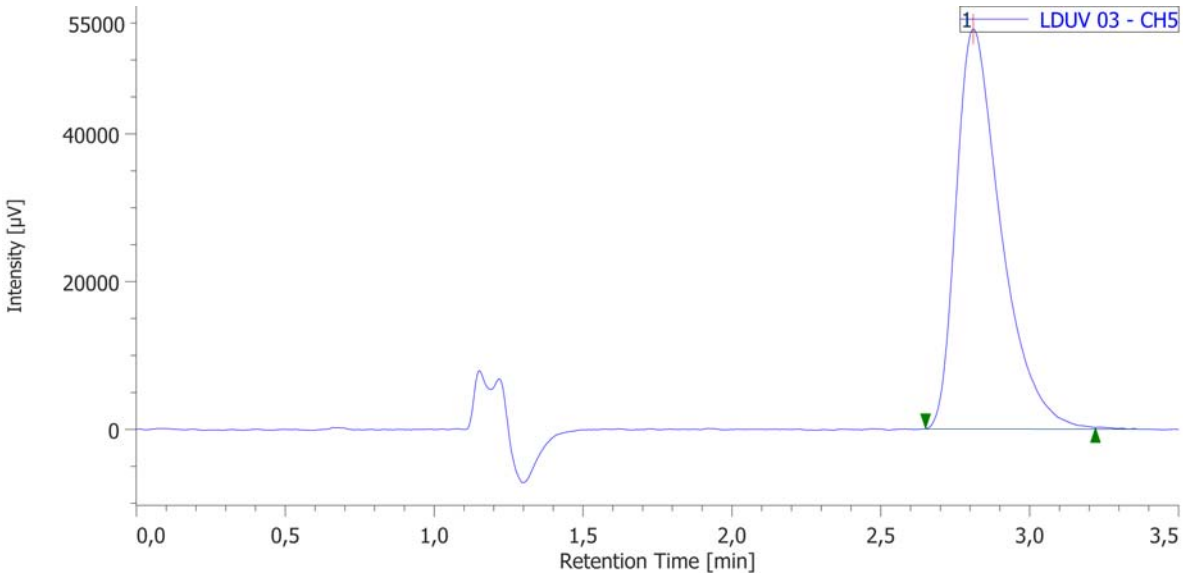


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:45:51
Volume	10,0 [µL]
Sample #	3
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,810	568168	54107	100,000	100,000	N/A	1786	N/A	1,577	

Chromatogram

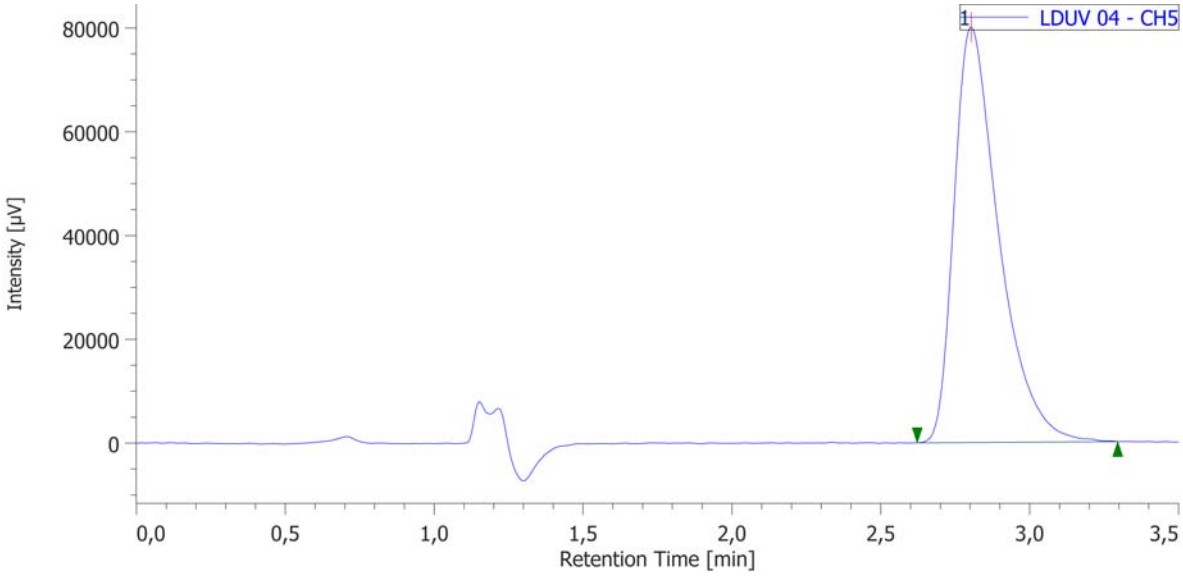


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:50:41
Volume	10,0 [µL]
Sample #	4
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,803	838505	80041	100,000	100,000	N/A	1790	N/A	1,578	

Chromatogram

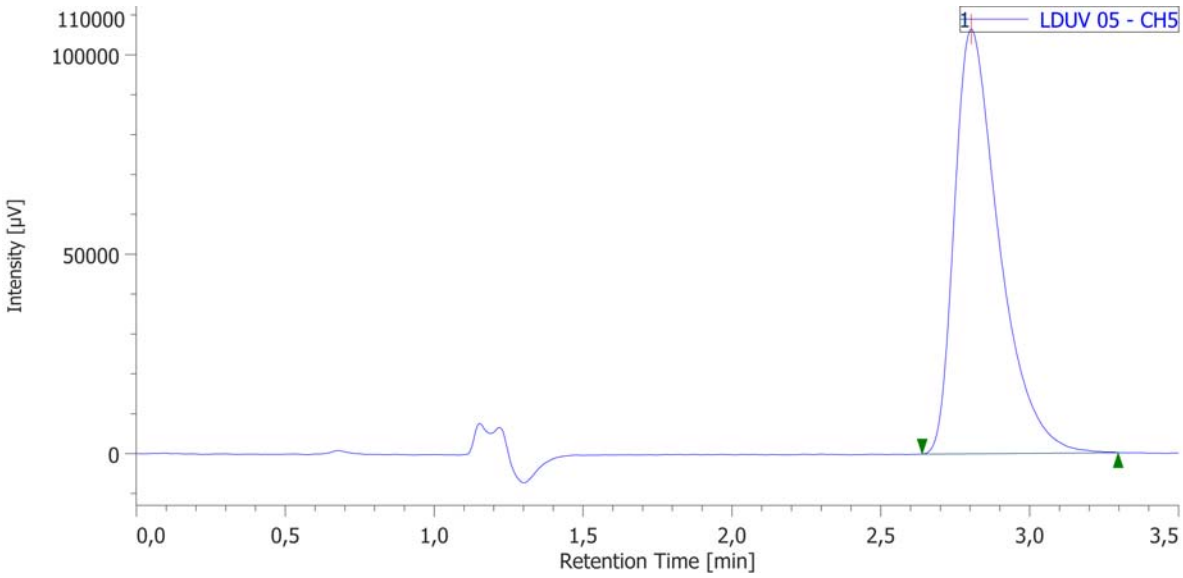


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 16:55:28
Volume	10,0 [µL]
Sample #	5
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,803	1112800	106490	100,000	100,000	N/A	1790	N/A	1,607	

Chromatogram

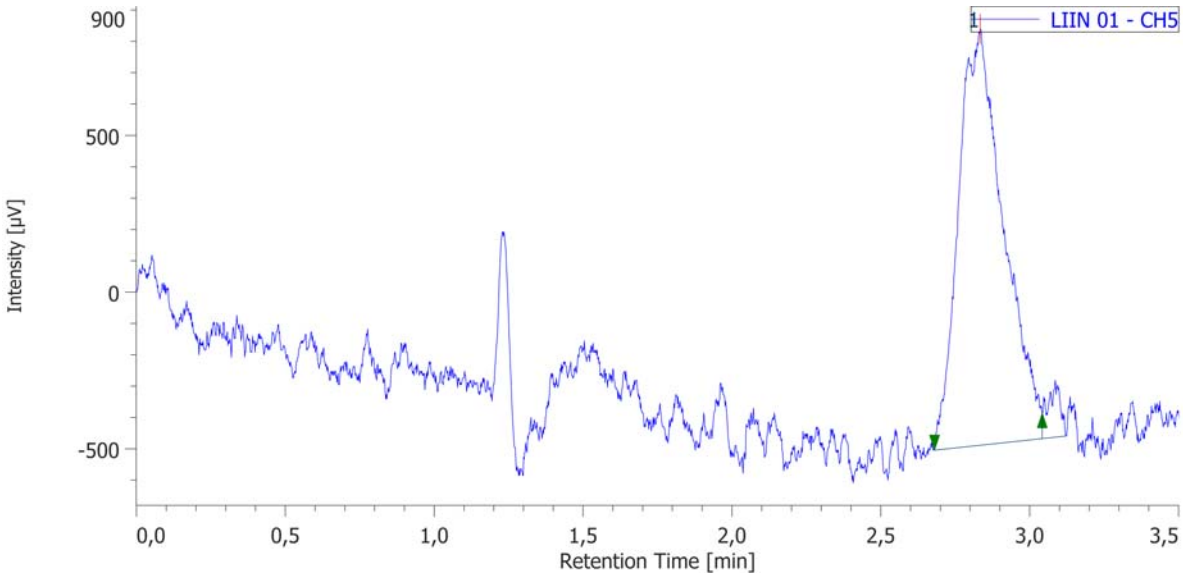


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:00:07
Volume	0,1 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,833	13970	1327	100,000	100,000	N/A	1695	N/A	N/A	

Chromatogram

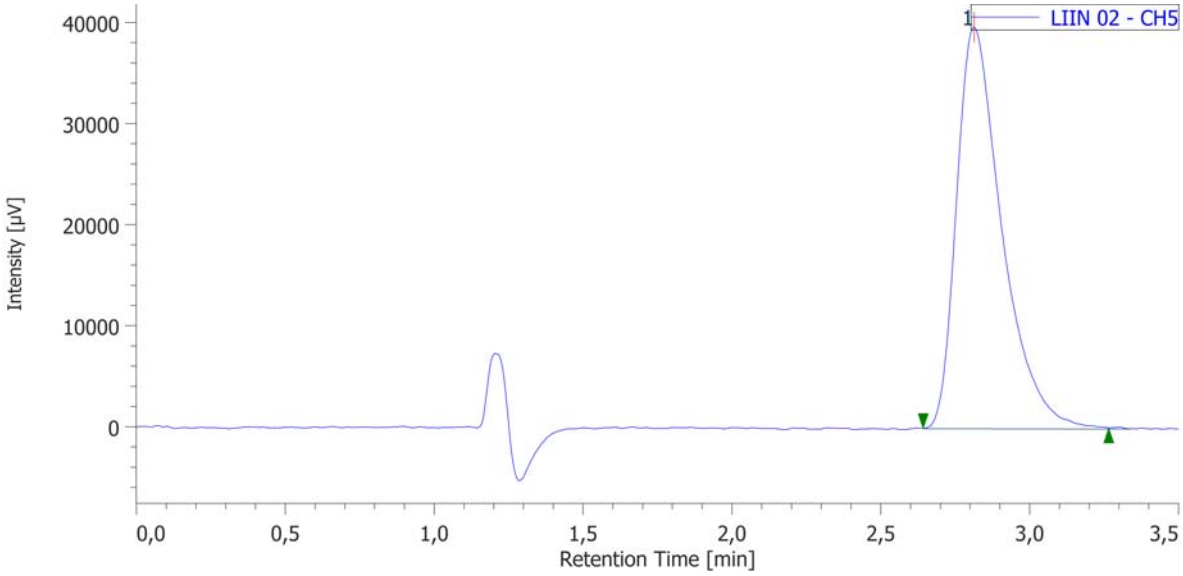


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:04:47
Volume	5,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,813	421244	39726	100,000	100,000	N/A	1774	N/A	1,547	

Chromatogram

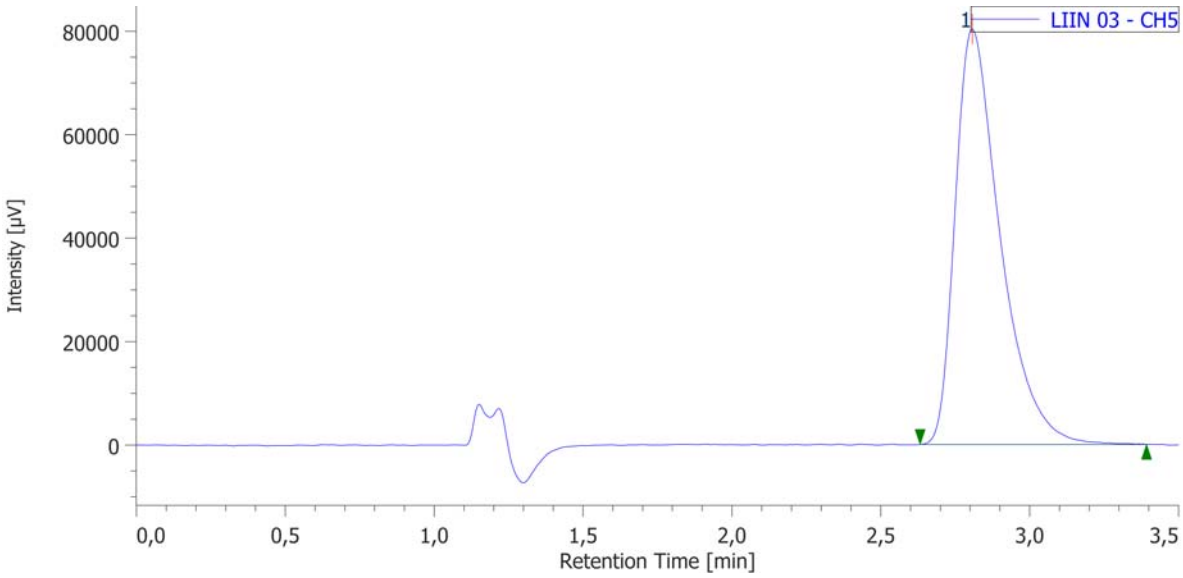


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:09:31
Volume	10,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,807	846113	80282	100,000	100,000	N/A	1776	N/A	1,601	

Chromatogram

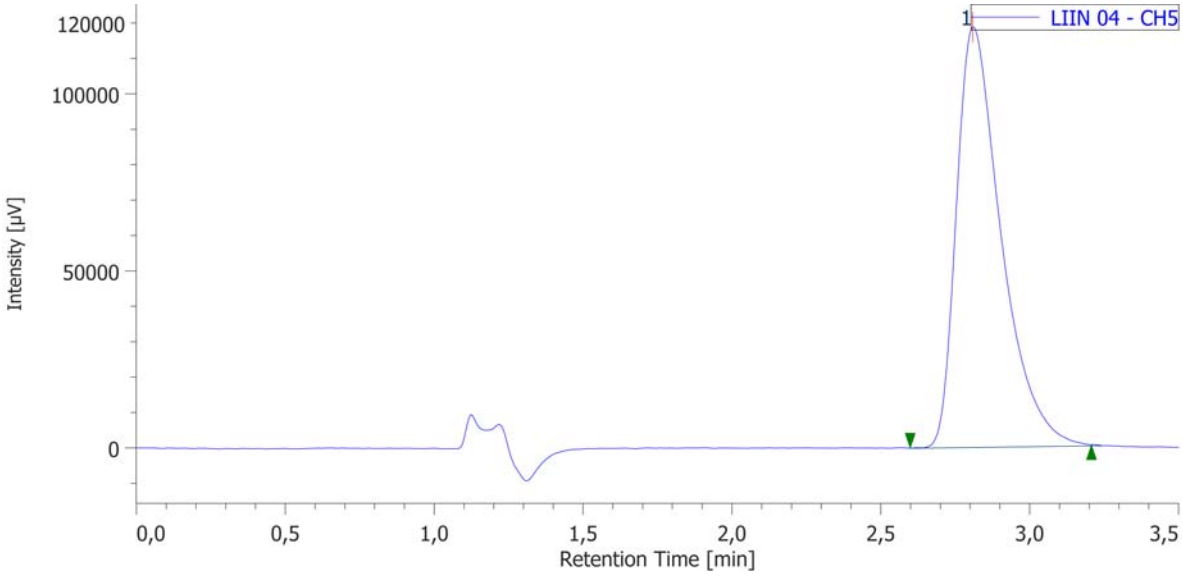


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:14:15
Volume	15,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,808	1240424	118676	100,000	100,000	N/A	1787	N/A	1,637	

Chromatogram

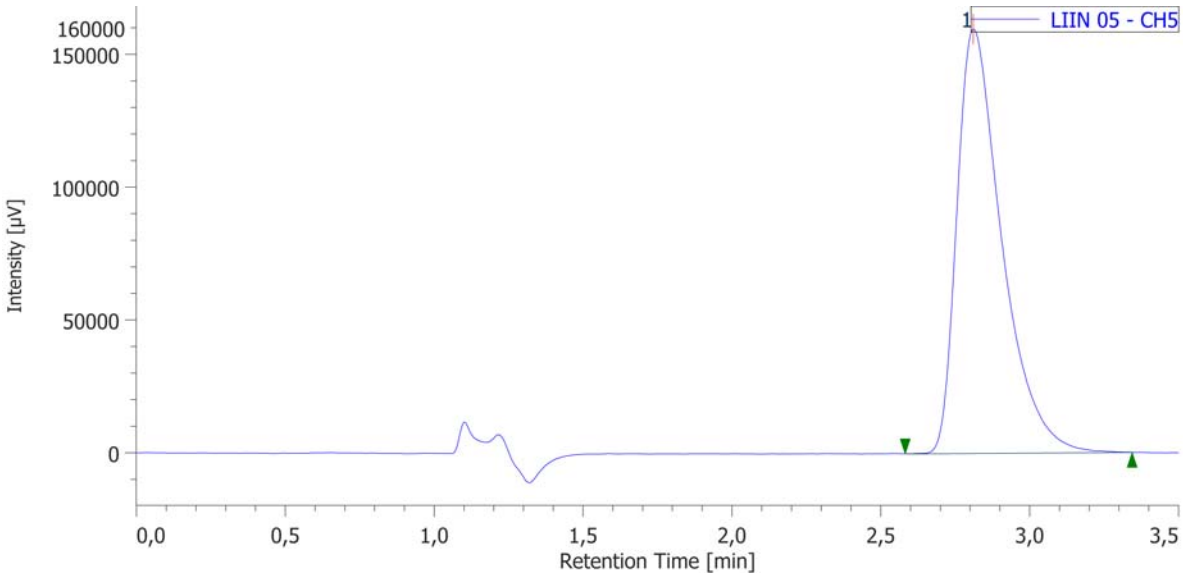


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:28:37
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:19:01
Volume	20,0 [µL]
Sample #	6
Project Name	HPL 02
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,810	1677240	159743	100,000	100,000	N/A	1787	N/A	1,663	

Chromatogram

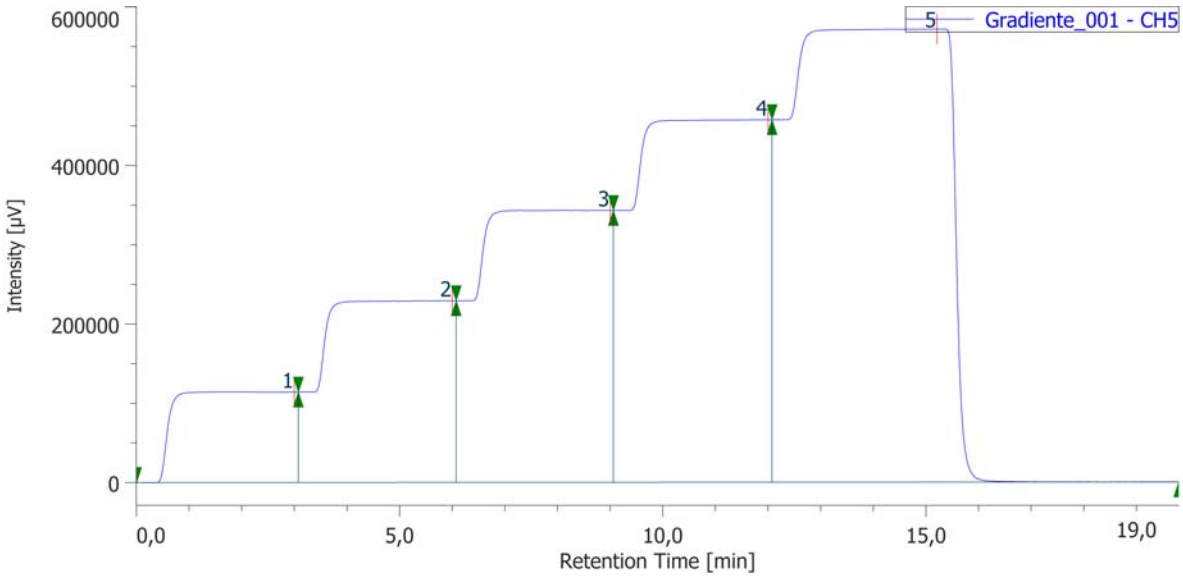

Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2022 08:54:21
Description	
HPLC System Name	HPL 02
Injection Date	28/03/2022 17:51:15
Volume	10,0 [µL]
Sample #	–
Project Name	HPL 02
Acquisition Time	19,8 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,000	17012172	114015	5,509	6,650	N/A	N/A	N/A	N/A	
2	40%	5	6,000	37699874	229055	12,209	13,360	N/A	N/A	N/A	N/A	
3	60%	5	9,000	57940348	342921	18,763	20,002	N/A	N/A	N/A	N/A	
4	80%	5	12,000	78999937	457039	25,583	26,658	N/A	N/A	N/A	N/A	
5	100%	5	15,210	117146375	571441	37,936	33,330	N/A	N/A	N/A	N/A	