
Chromatogram

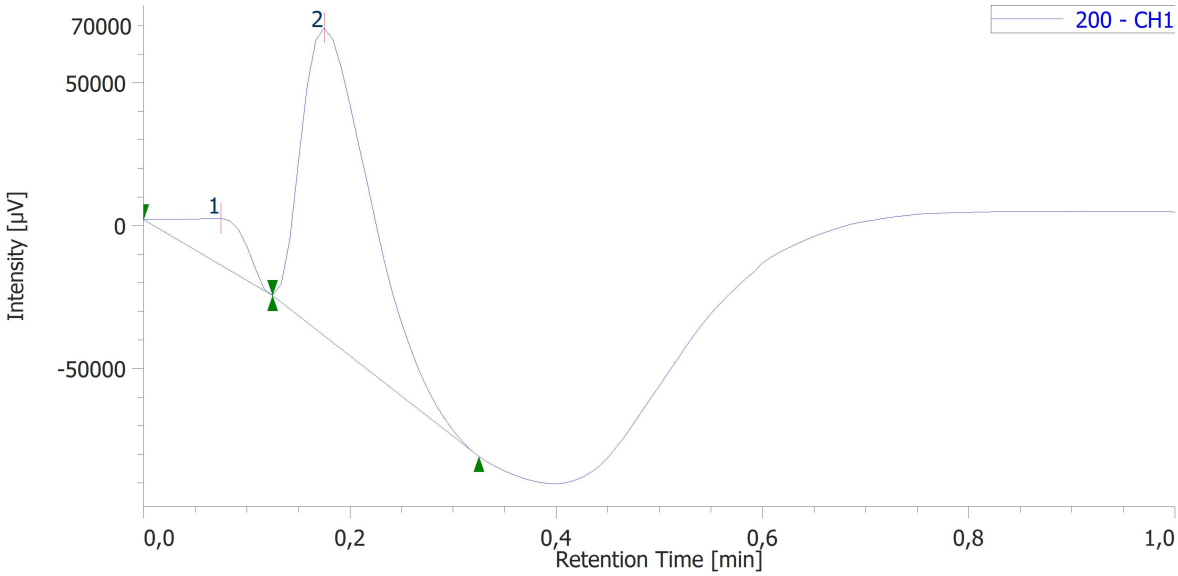

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:04:19
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:03:16
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	200
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	200-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,075	66571	16309	11,553	13,156	N/A	7	0,829	0,789	
2	Cafeína	1	0,175	509659	107664	88,447	86,844	N/A	30	N/A	1,797	

Creator
Reviewer
Approver

Chromatogram

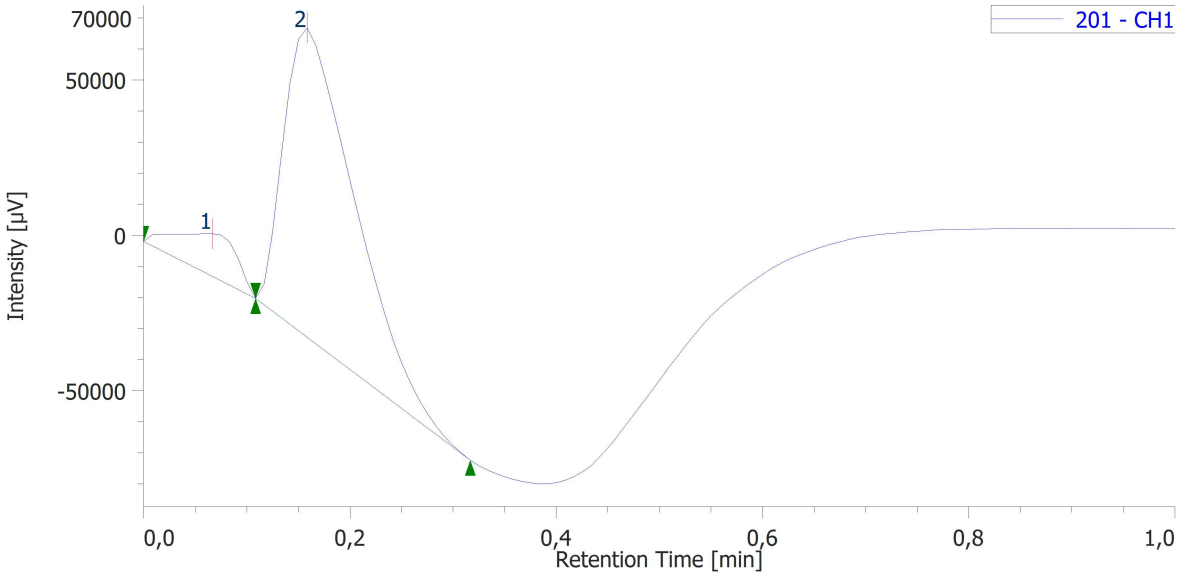

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:08:55
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:07:52
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	201
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	201-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,067	55968	13682	10,384	12,092	N/A	5	0,739	0,809	
2	Cafeína	1	0,158	483031	99462	89,616	87,908	N/A	23	N/A	1,816	

Creator
Reviewer
Approver

Chromatogram

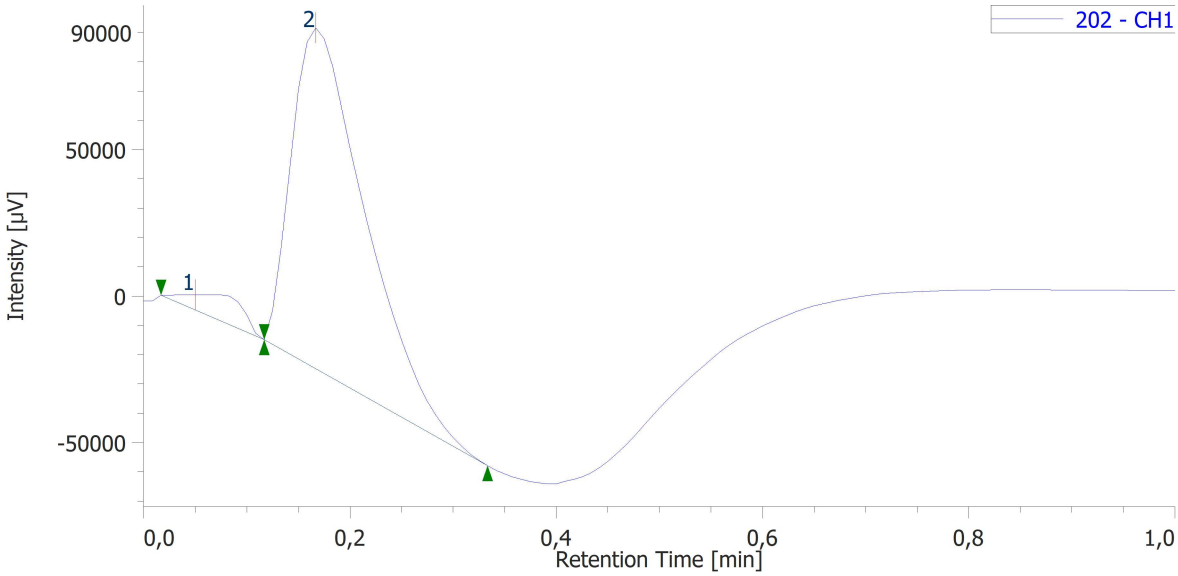

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:13:31
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:12:28
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	202
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	202-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,050	30872	5194	5,018	4,275	N/A	3	0,916	1,518	
2	Cafeína	1	0,167	584309	116298	94,982	95,725	N/A	25	N/A	1,825	

Creator
Reviewer
Approver

Chromatogram

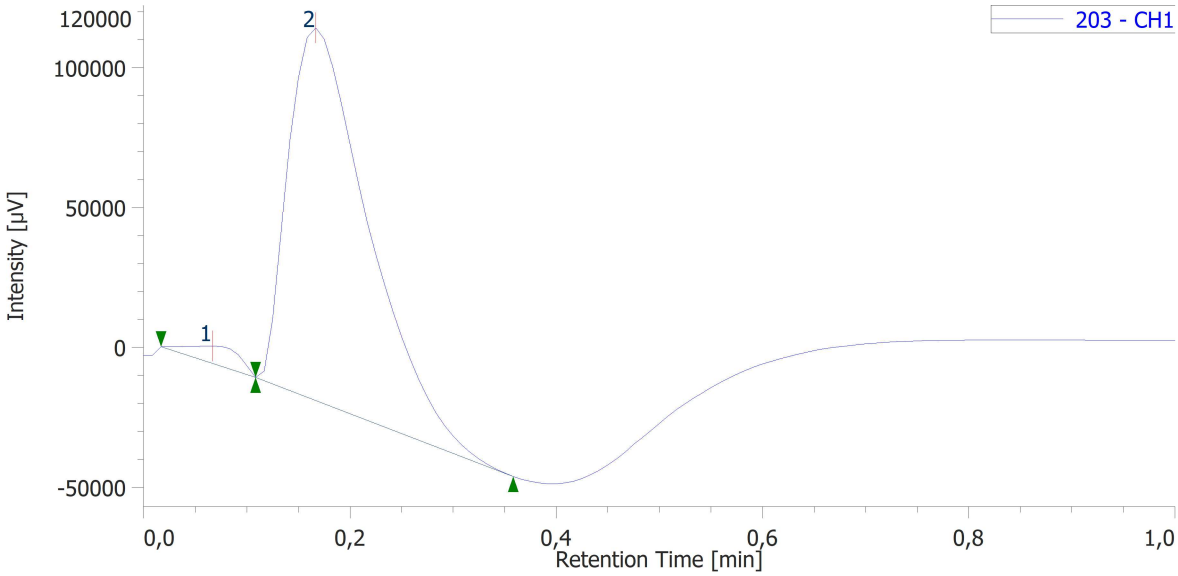

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:18:07
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:17:04
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	203
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	203-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,067	22569	6179	3,021	4,436	N/A	7	0,828	0,930	
2	Cafeína	1	0,167	724554	133125	96,979	95,564	N/A	22	N/A	1,853	

Creator
Reviewer
Approver

Chromatogram

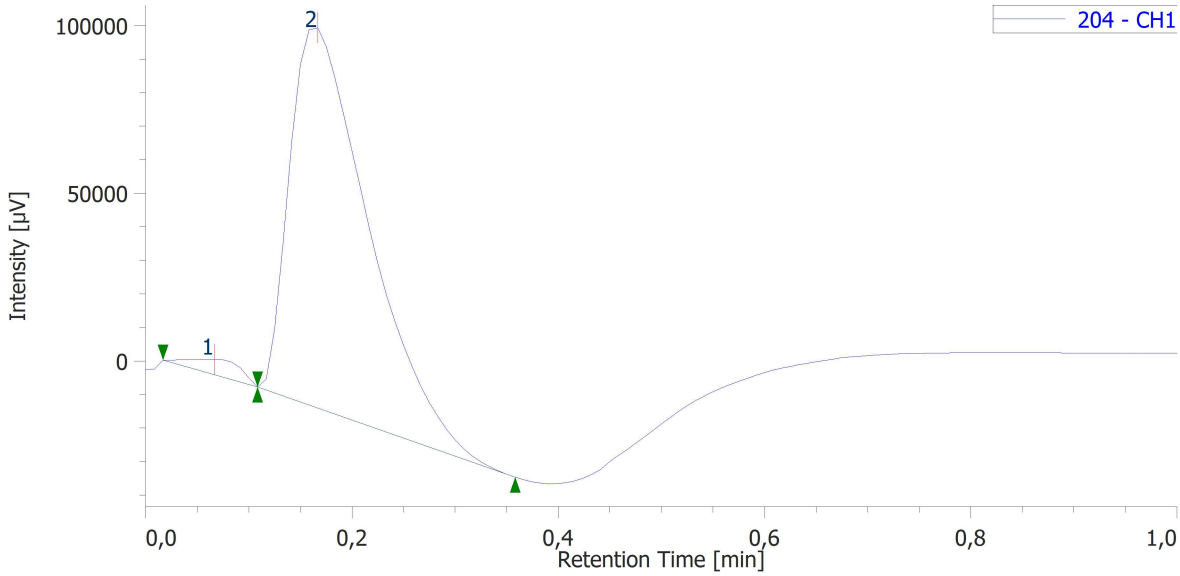

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:22:43
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:21:40
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	204
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	204-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,067	16352	4550	2,626	3,862	N/A	7	0,842	0,929	
2	Cafeína	1	0,167	606408	113269	97,374	96,138	N/A	22	N/A	1,835	

Creator
Reviewer
Approver

Chromatogram

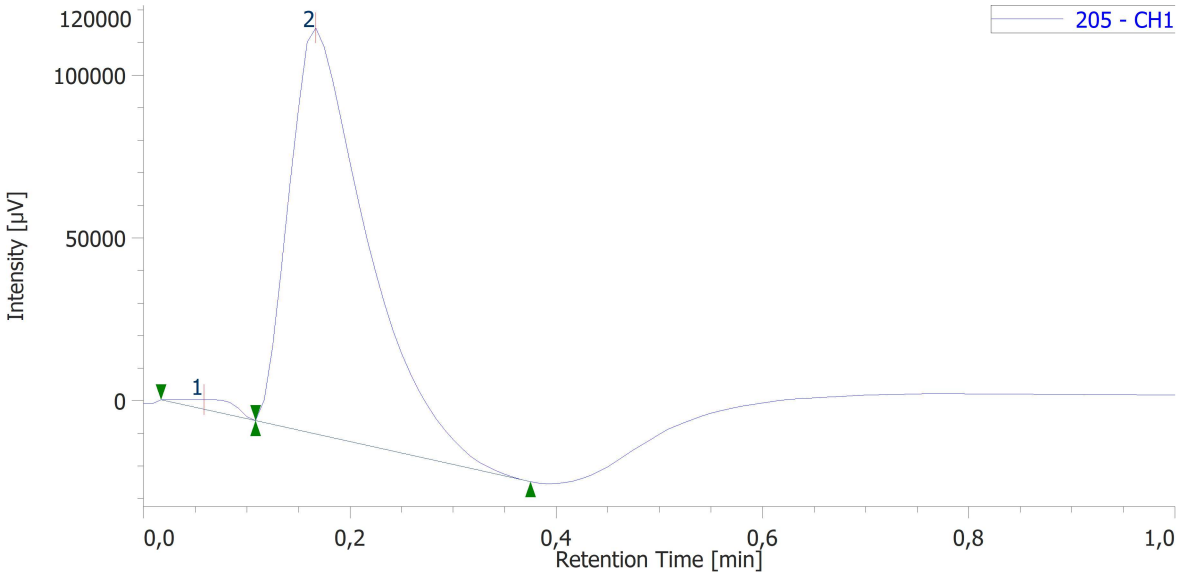

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:27:19
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:26:16
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	205
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	205-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,058	11643	2909	1,736	2,282	N/A	5	0,922	1,103	
2	Cafeína	1	0,167	659107	124557	98,264	97,718	N/A	24	N/A	1,865	

Creator
Reviewer
Approver

Chromatogram

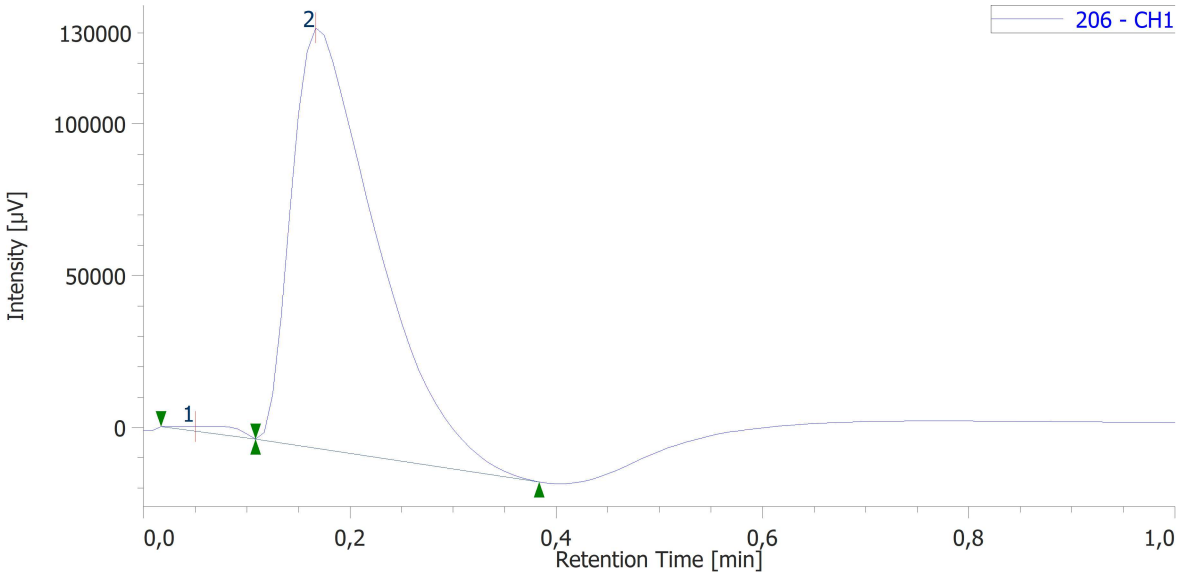

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:31:55
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:30:52
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	206
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	206-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,050	8730	1548	1,081	1,106	N/A	3	0,867	1,415	
2	Cafeína	1	0,167	798568	138399	98,919	98,894	N/A	20	N/A	2,122	

Creator
Reviewer
Approver

Chromatogram

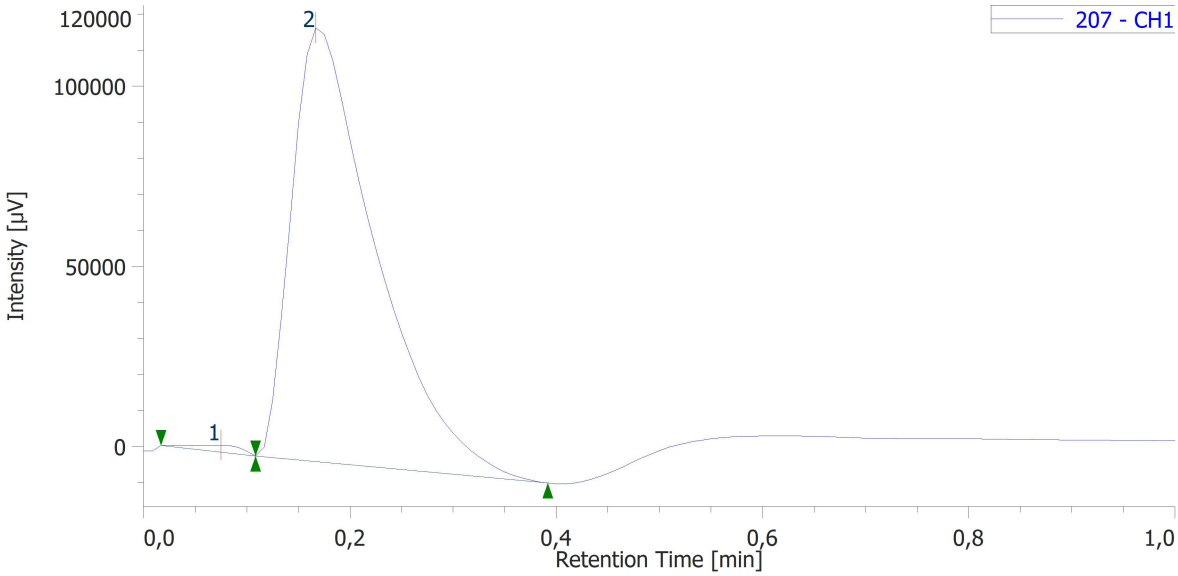

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:36:31
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:35:28
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	207
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	207-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,075	6422	1957	0,928	1,600	N/A	11	0,773	0,794	
2	Cafeína	1	0,167	685384	120329	99,072	98,400	N/A	21	N/A	2,127	

Creator
Reviewer
Approver

Chromatogram

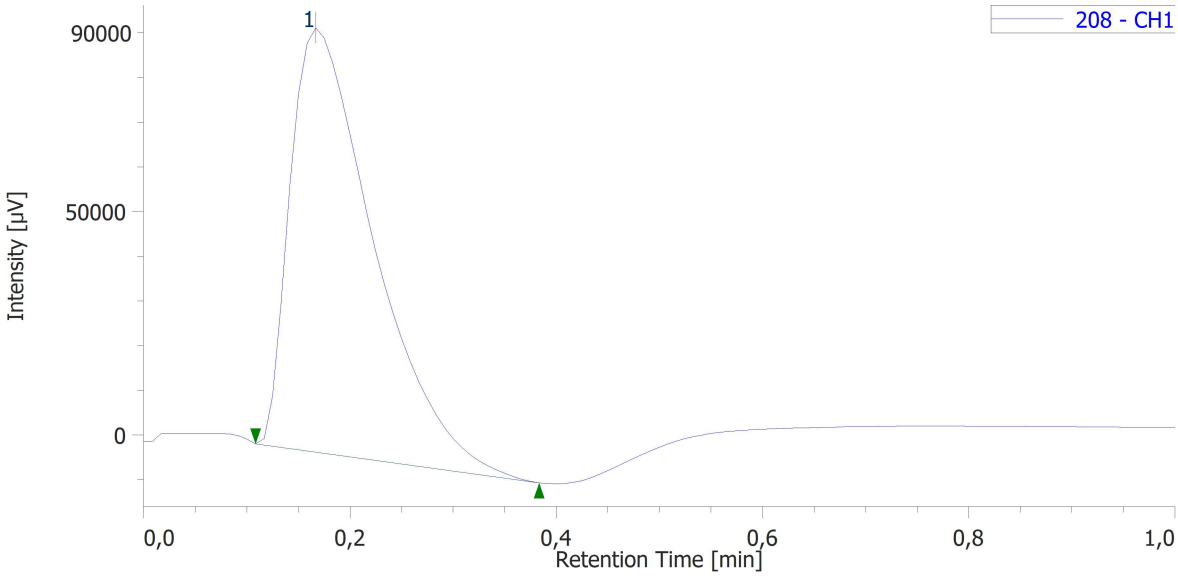

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:41:07
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:40:04
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	208
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	208-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	536120	94806	100,000	100,000	N/A	21	N/A	2,051	

Creator
Reviewer
Approver

Chromatogram

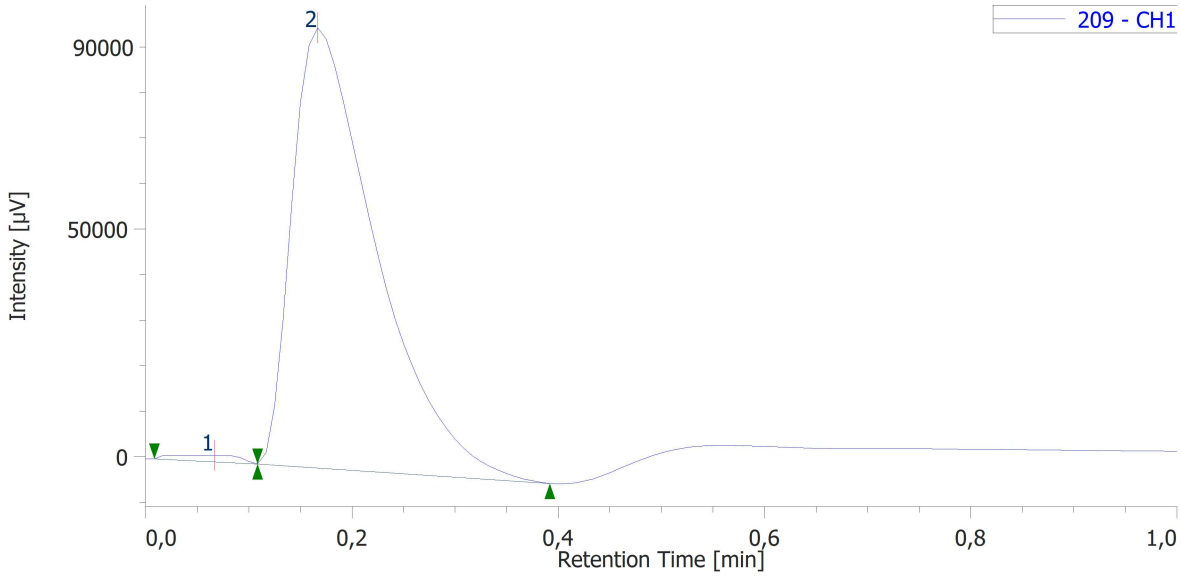

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:45:43
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:44:40
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	209
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	209-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,067	6258	1422	1,129	1,452	N/A	4	0,705	0,850	
2	Cafeína	1	0,167	548162	96567	98,871	98,548	N/A	21	N/A	2,062	

Creator
Reviewer
Approver

Chromatogram

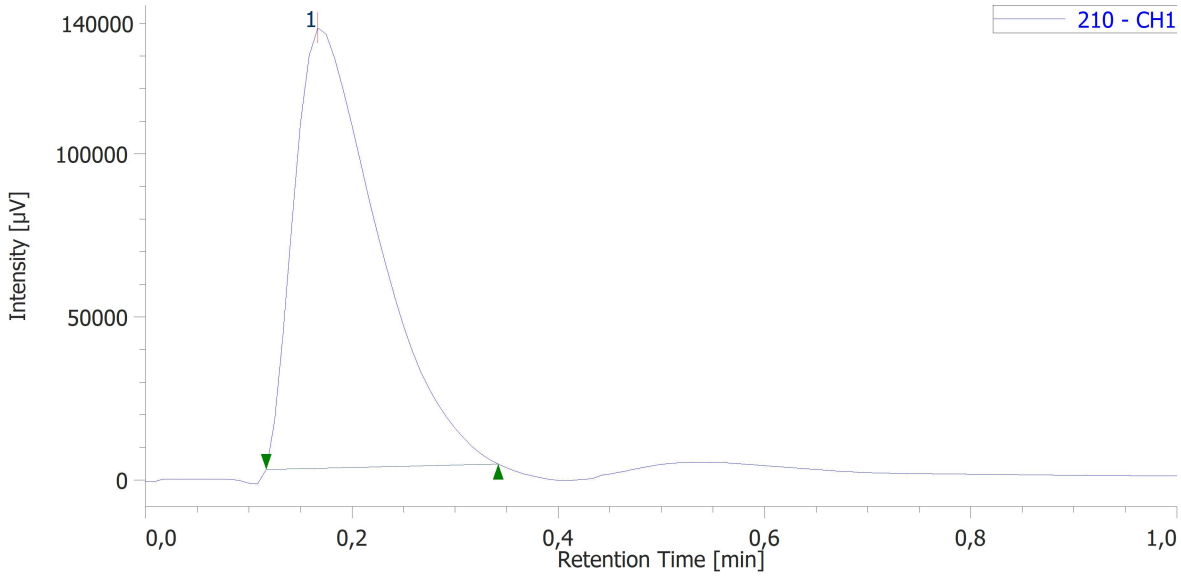

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:50:19
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:49:16
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	210
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	210-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	765077	134929	100,000	100,000	N/A	20	N/A	2,081	

Creator
Reviewer
Approver

Chromatogram

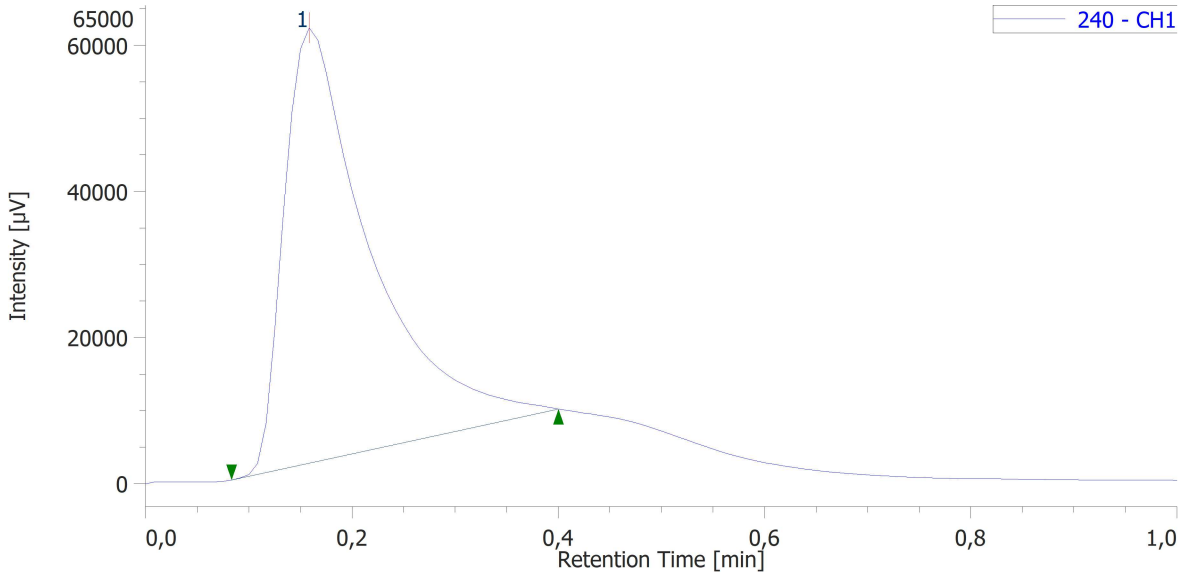

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:54:54
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:53:52
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	240
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	240-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	347327	59545	100,000	100,000	N/A	21	N/A	2,478	

Creator
Reviewer
Approver

Chromatogram

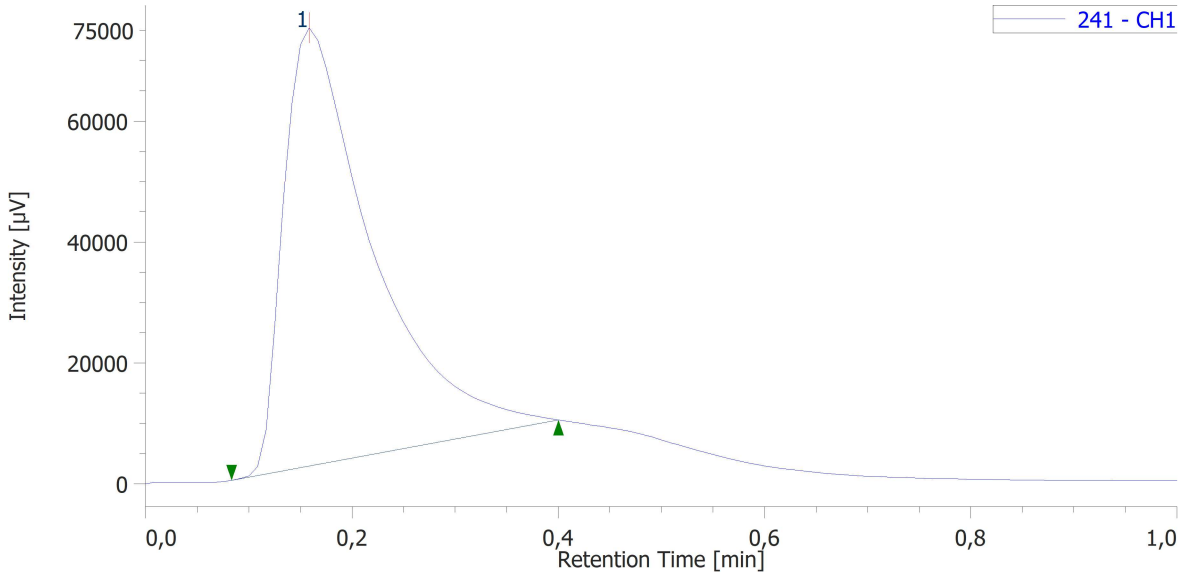

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 12:59:30
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 12:58:28
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	241
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	241-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	434922	72425	100,000	100,000	N/A	19	N/A	2,492	

Creator
Reviewer
Approver

Chromatogram

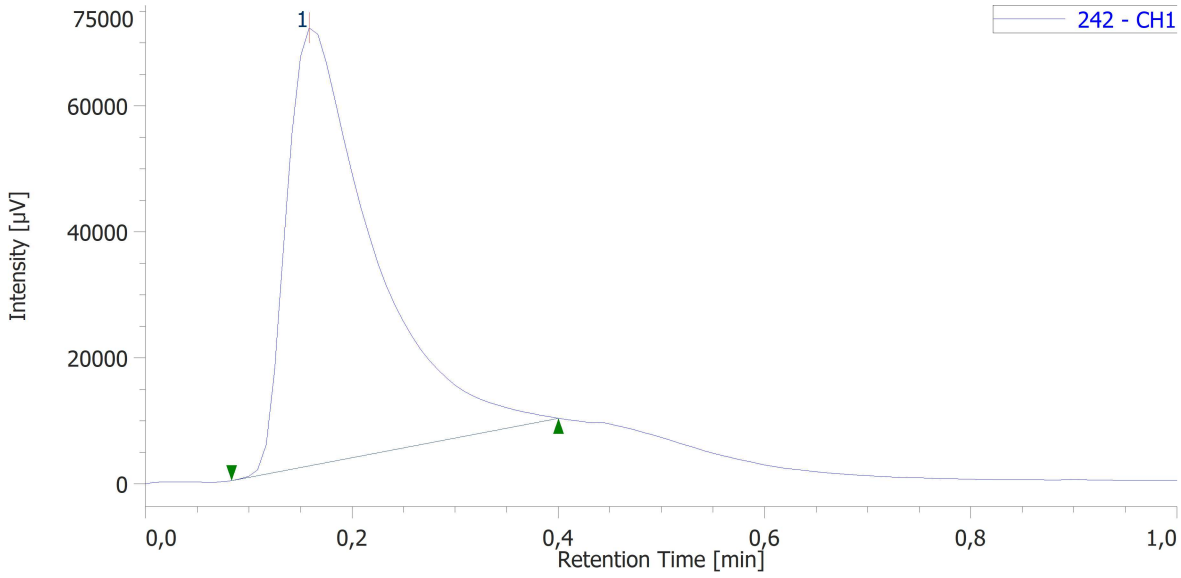

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:04:06
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:03:04
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	242
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	242-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	408048	69481	100,000	100,000	N/A	20	N/A	2,625	

Creator
Reviewer
Approver

Chromatogram

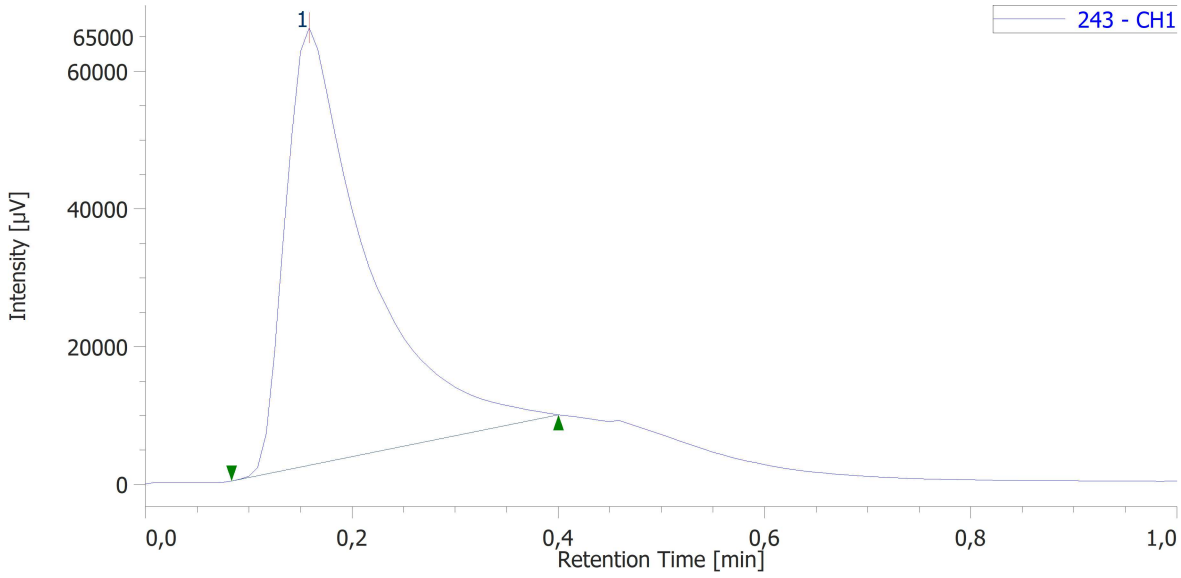

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:08:42
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:07:40
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	243
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	243-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	349506	63483	100,000	100,000	N/A	25	N/A	2,508	

Creator
Reviewer
Approver

Chromatogram

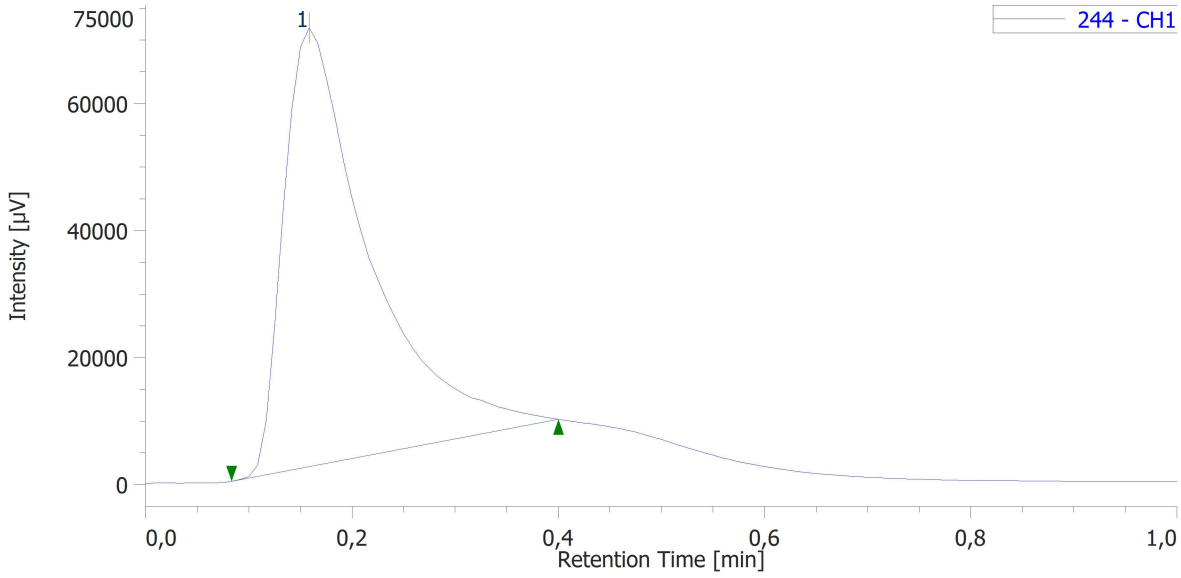

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:13:18
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:12:16
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	244
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	244-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	399405	69039	100,000	100,000	N/A	22	N/A	2,457	

Creator
Reviewer
Approver

Chromatogram

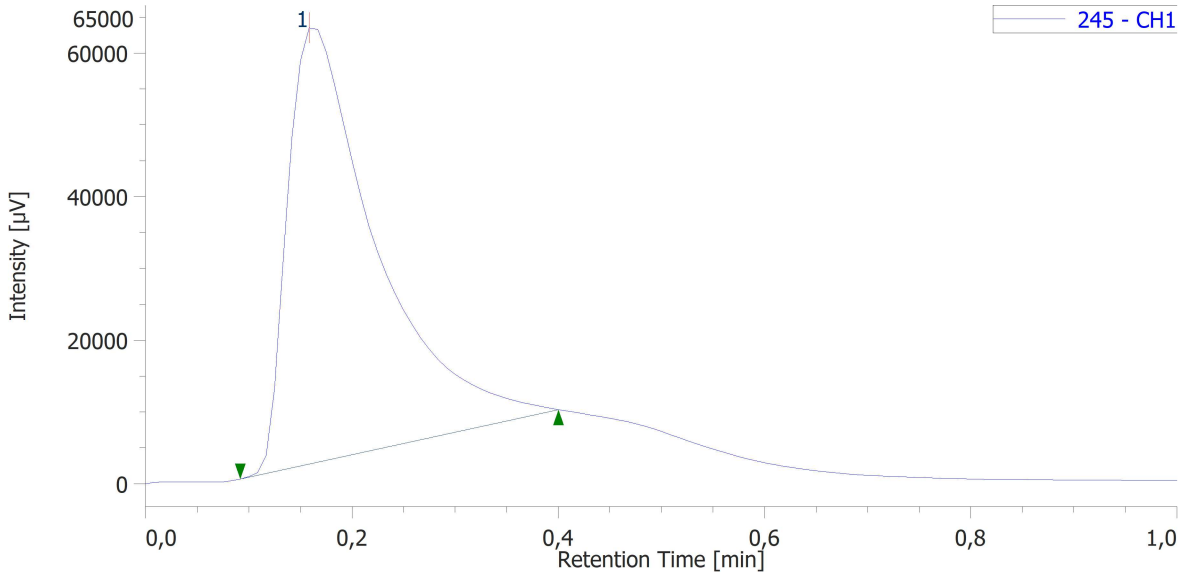

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:17:54
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:16:52
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	245
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	245-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	364237	60700	100,000	100,000	N/A	19	N/A	2,839	

Creator
Reviewer
Approver

Chromatogram

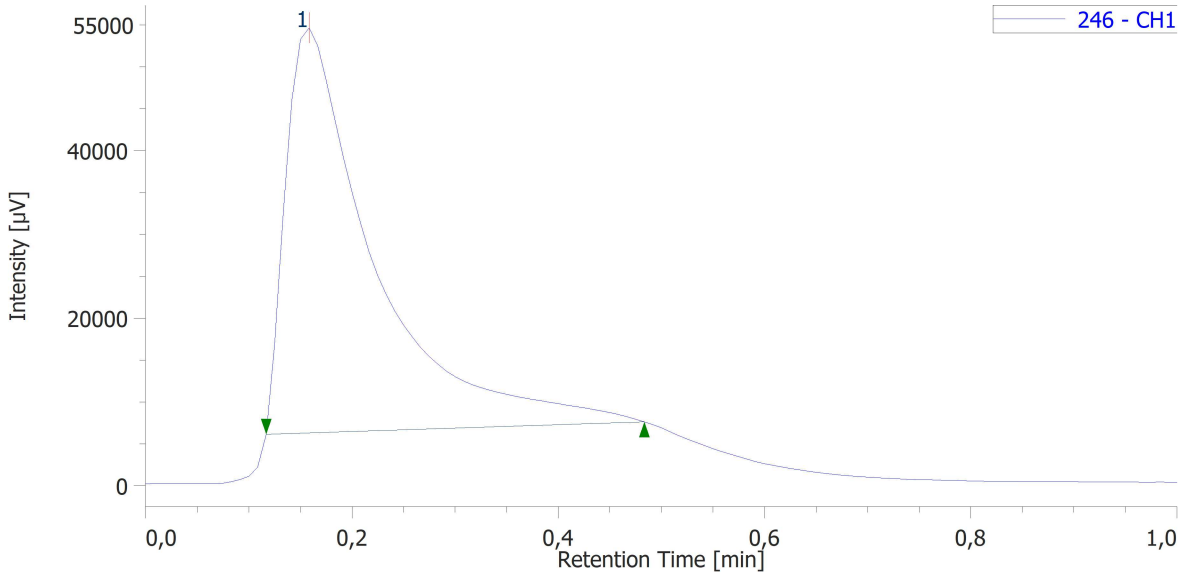

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:22:30
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:21:28
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	246
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	246-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	287217	48314	100,000	100,000	N/A	23	N/A	3,578	

Creator
Reviewer
Approver

Chromatogram

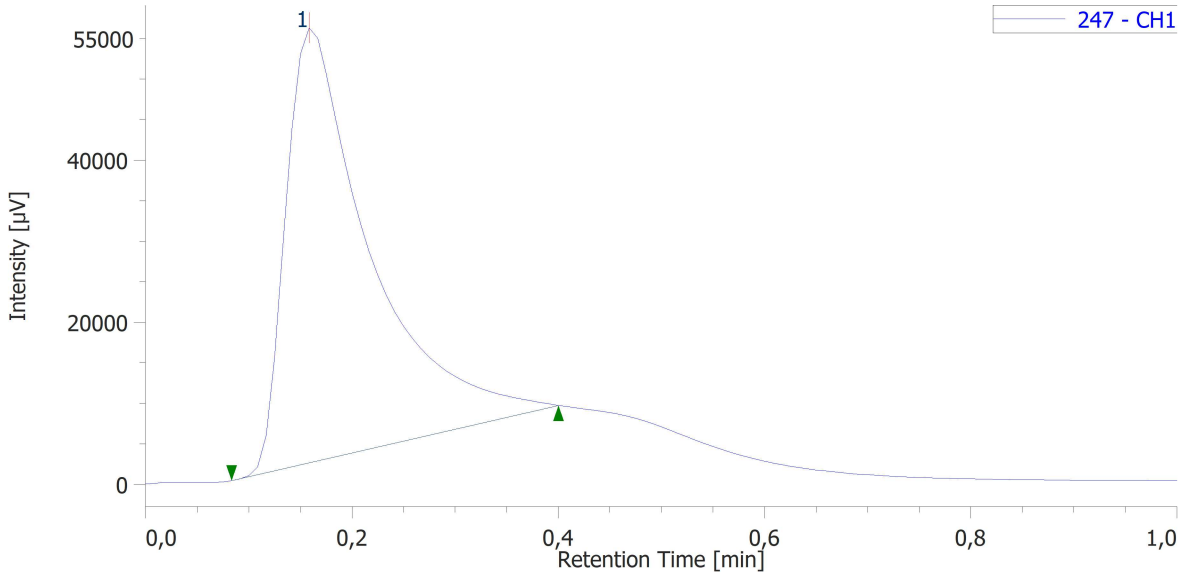

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:27:06
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:26:04
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	247
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	247-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	306468	53647	100,000	100,000	N/A	23	N/A	2,570	

Creator
Reviewer
Approver

Chromatogram

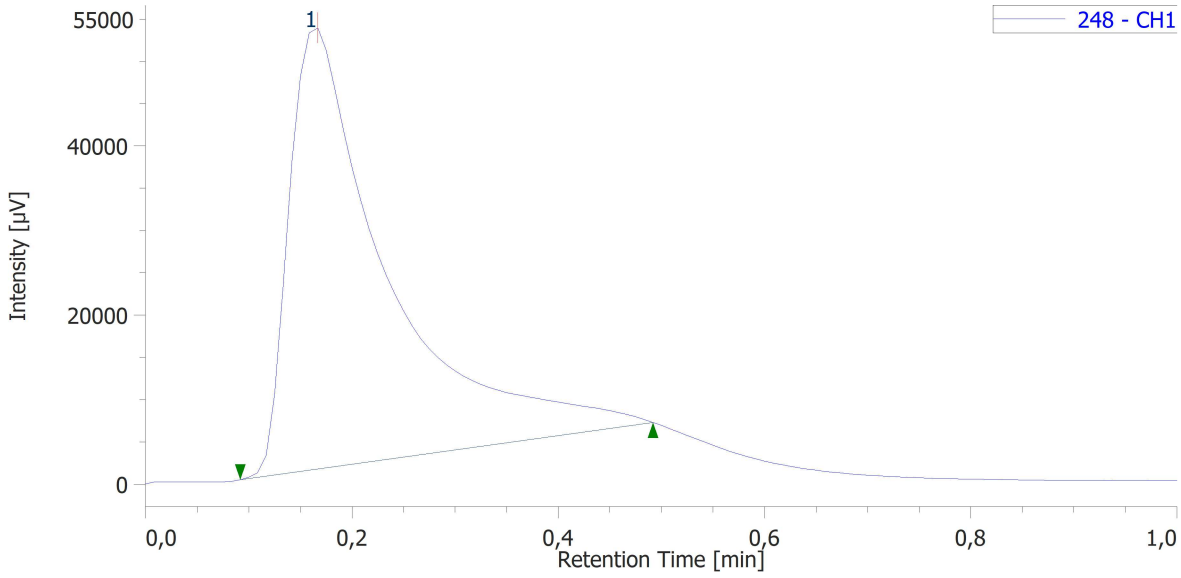

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:31:43
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:30:40
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	248
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	248-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	348544	52117	100,000	100,000	N/A	21	N/A	3,212	

Creator
Reviewer
Approver

Chromatogram

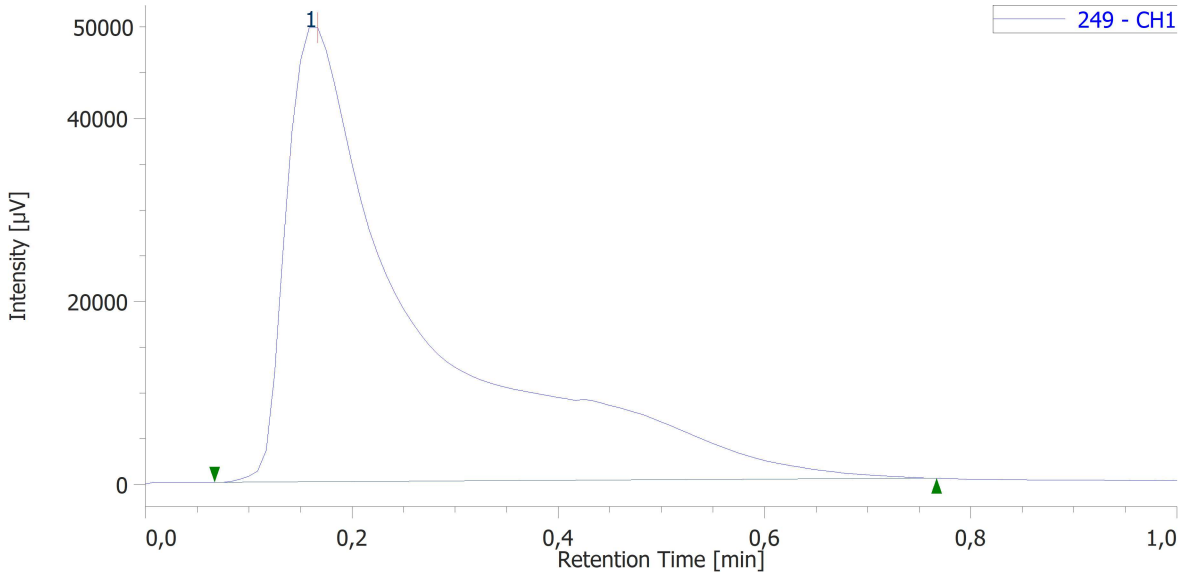

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:36:18
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:35:16
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	249
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	249-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	449755	49553	100,000	100,000	N/A	18	N/A	4,410	

Creator
Reviewer
Approver

Chromatogram

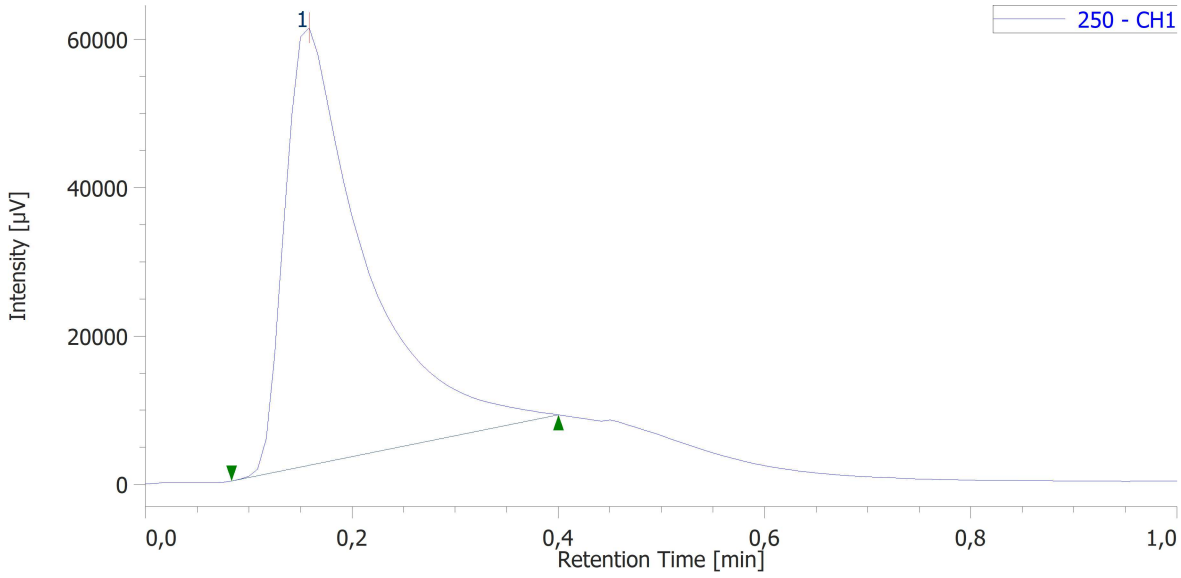

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 13:40:54
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 13:39:52
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	250
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	250-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	319819	58960	100,000	100,000	N/A	26	N/A	2,525	

Creator
Reviewer
Approver

Chromatogram

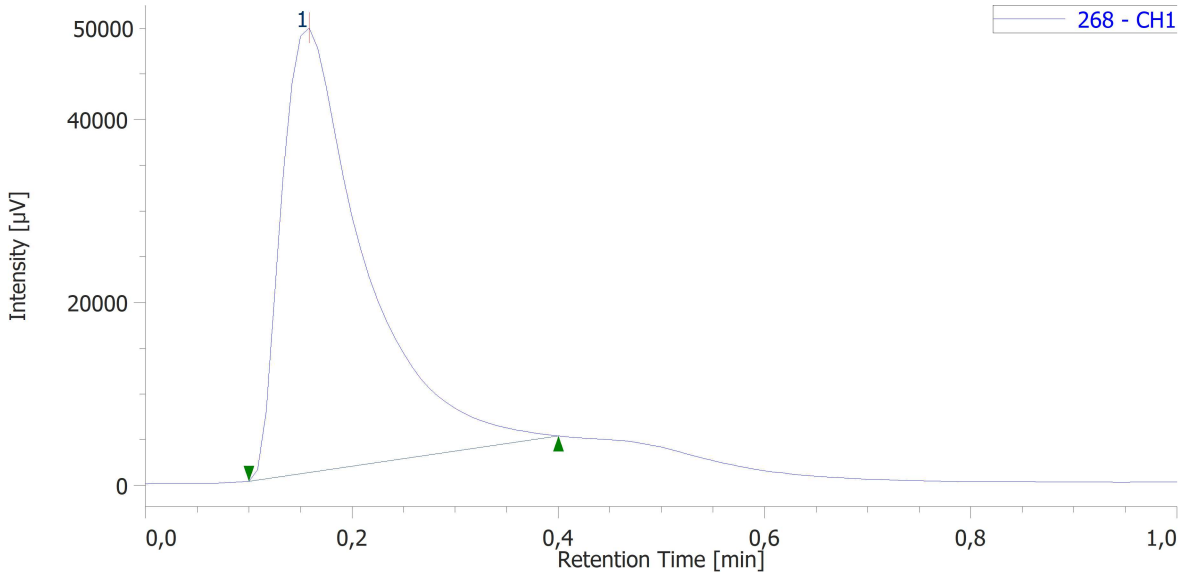

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:28:58
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:27:55
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	268
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	268-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	273956	48562	100,000	100,000	N/A	22	N/A	2,320	

Creator
Reviewer
Approver

Chromatogram

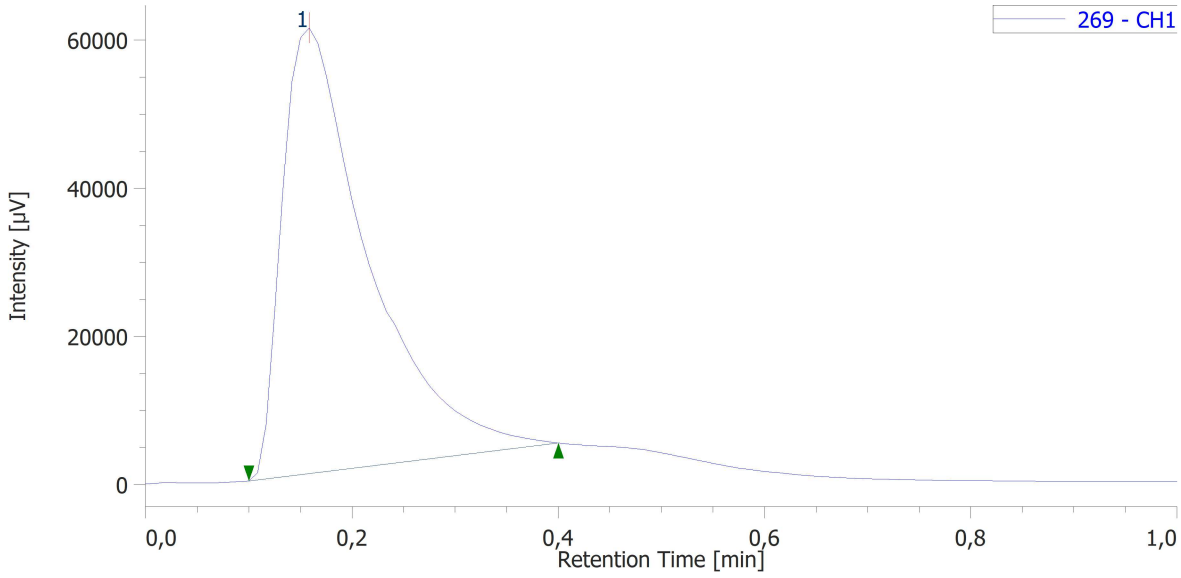

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:33:34
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:32:31
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	269
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	269-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	349357	60119	100,000	100,000	N/A	21	N/A	2,357	

Creator
Reviewer
Approver

Chromatogram

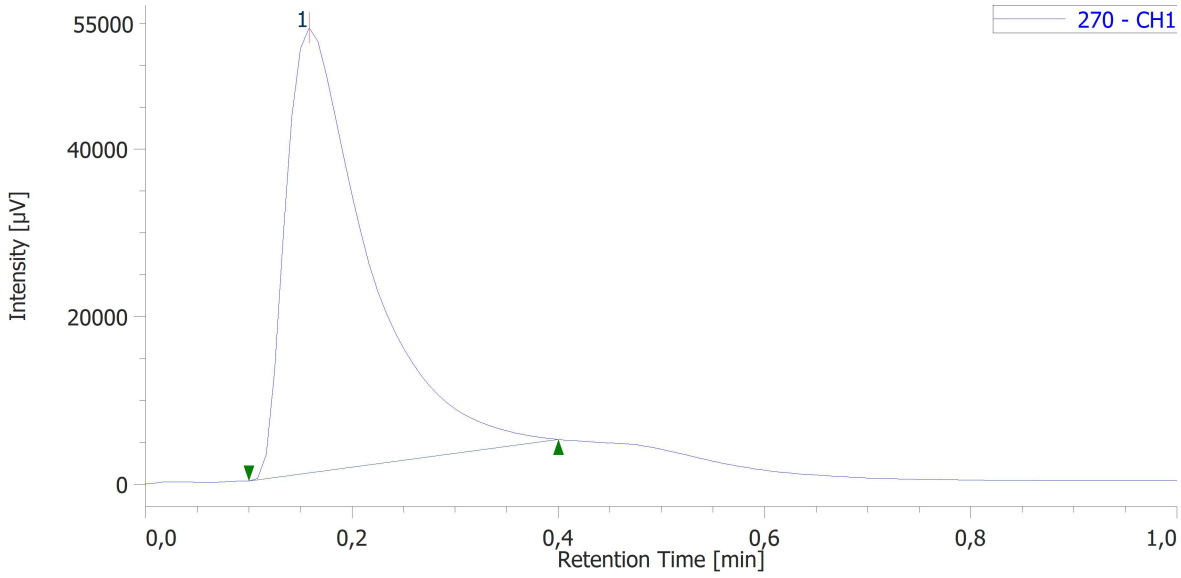

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:38:10
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:37:07
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	270
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	270-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	295827	53085	100,000	100,000	N/A	22	N/A	2,581	

Creator
Reviewer
Approver

Chromatogram

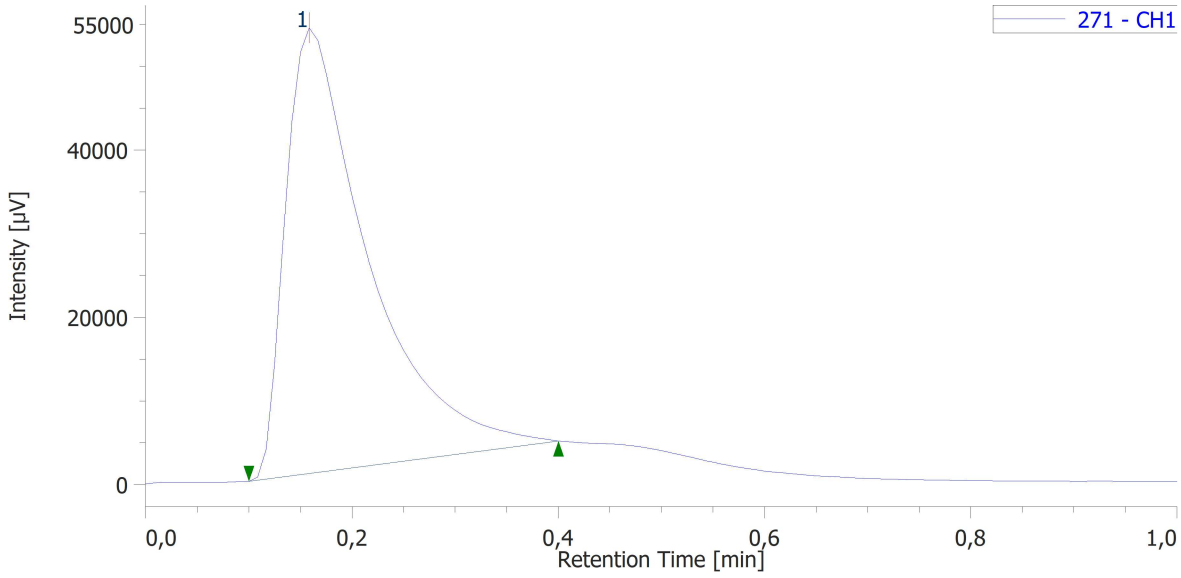

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:42:46
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:41:43
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	271
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	271-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	296943	53229	100,000	100,000	N/A	22	N/A	2,495	

Creator
Reviewer
Approver

Chromatogram

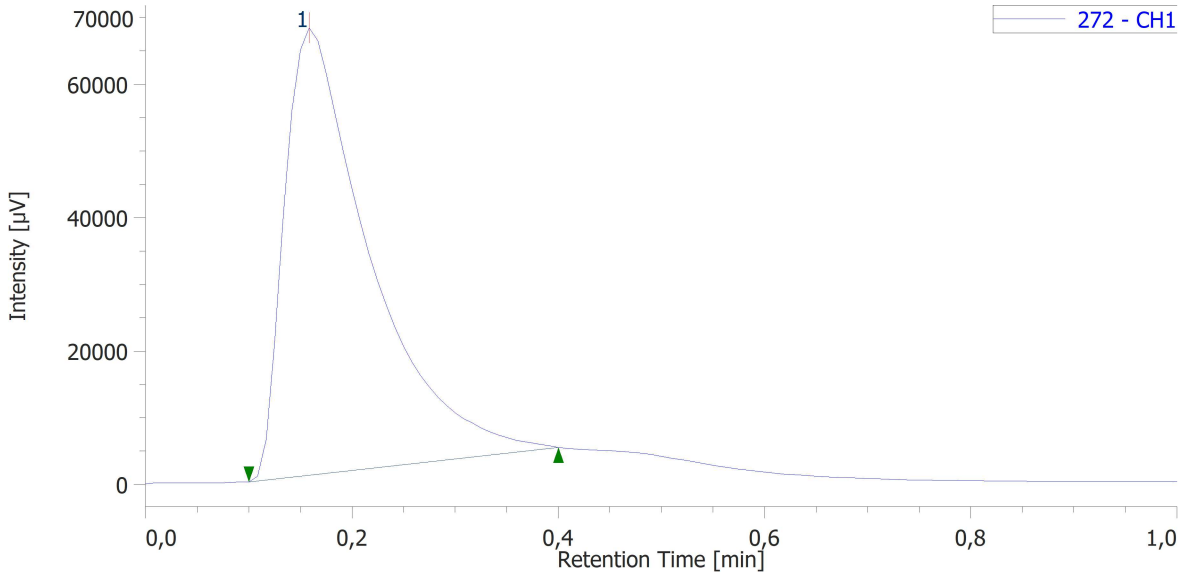

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:47:22
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:46:19
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	272
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	272-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	386794	67033	100,000	100,000	N/A	20	N/A	2,423	

Creator
Reviewer
Approver

Chromatogram

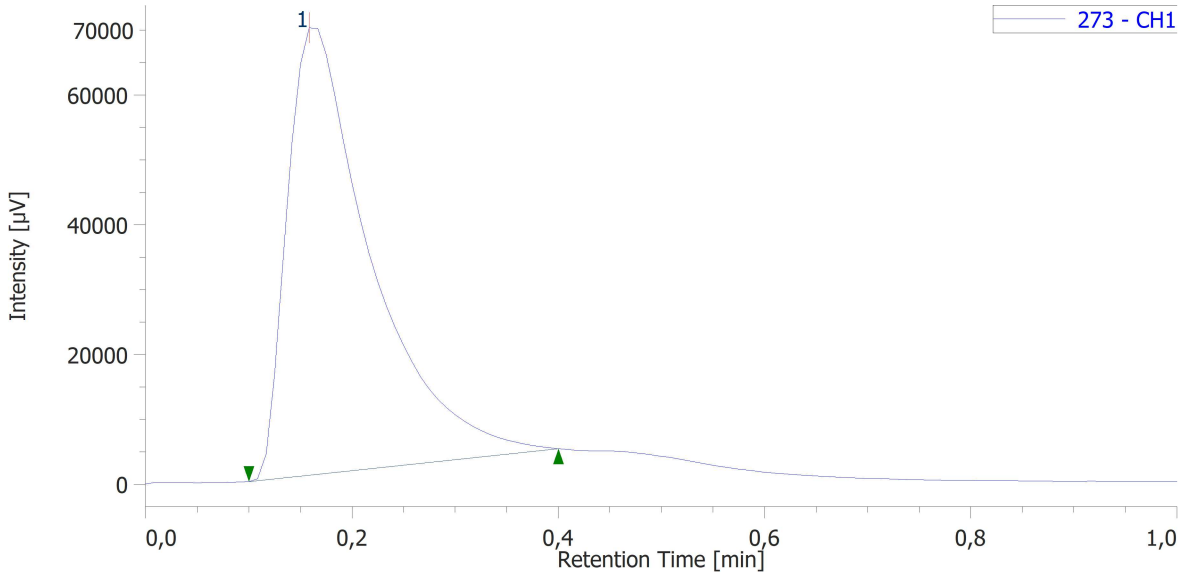

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:51:58
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:50:55
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	273
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	273-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	391133	68912	100,000	100,000	N/A	21	N/A	2,523	

Creator
Reviewer
Approver

Chromatogram

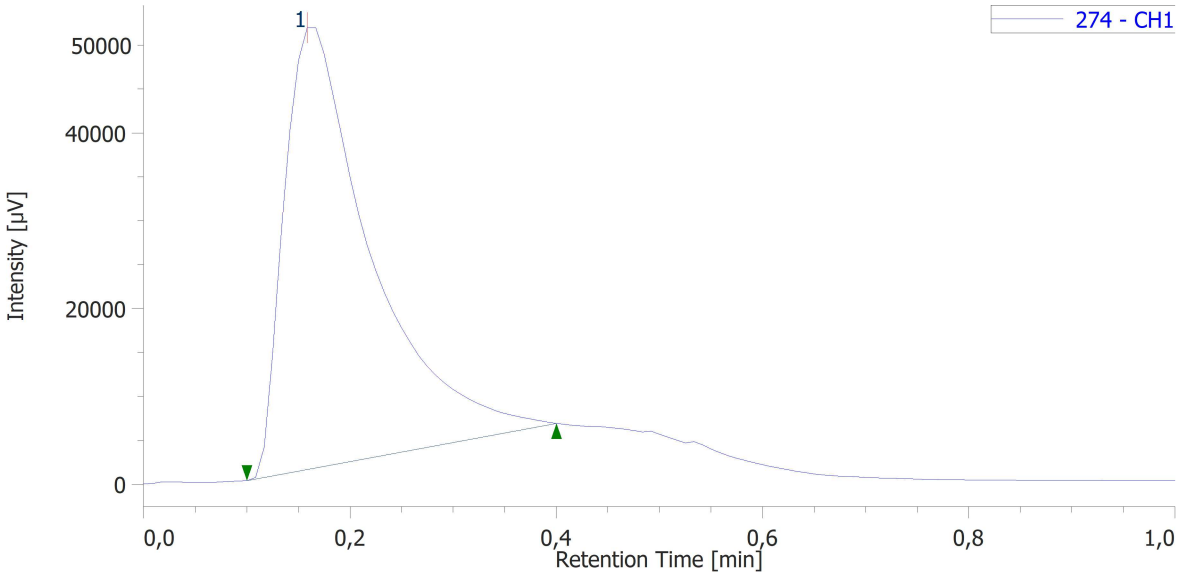

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 14:56:34
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 14:55:32
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	274
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	274-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	295988	50262	100,000	100,000	N/A	20	N/A	2,613	

Creator
Reviewer
Approver

Chromatogram

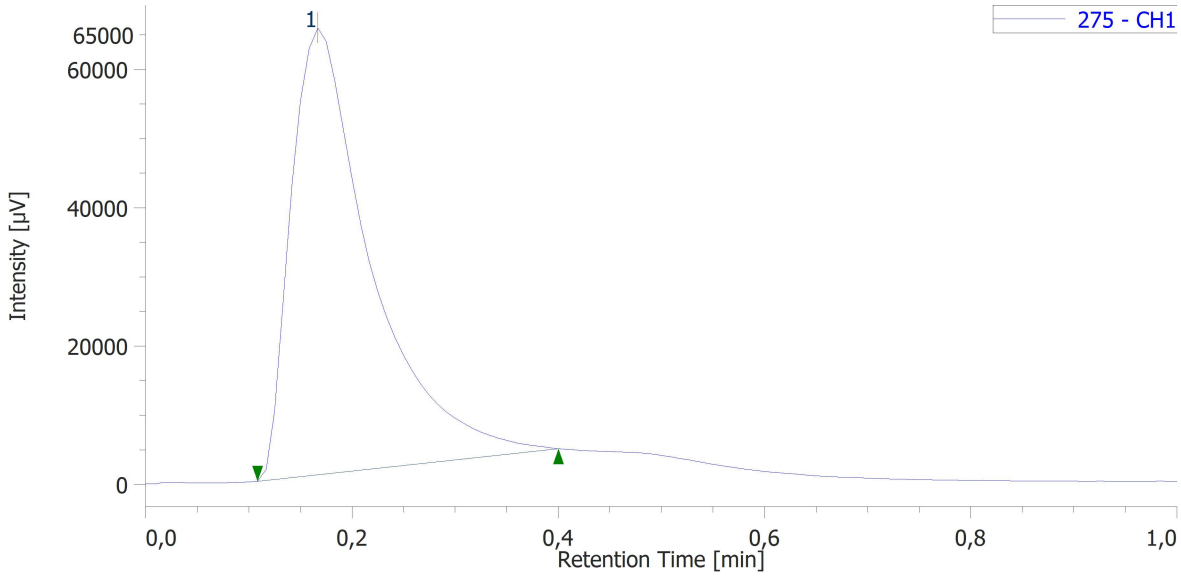

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 15:01:12
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 15:00:09
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	275
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	275-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	349433	64552	100,000	100,000	N/A	26	N/A	2,190	

Creator
Reviewer
Approver

Chromatogram

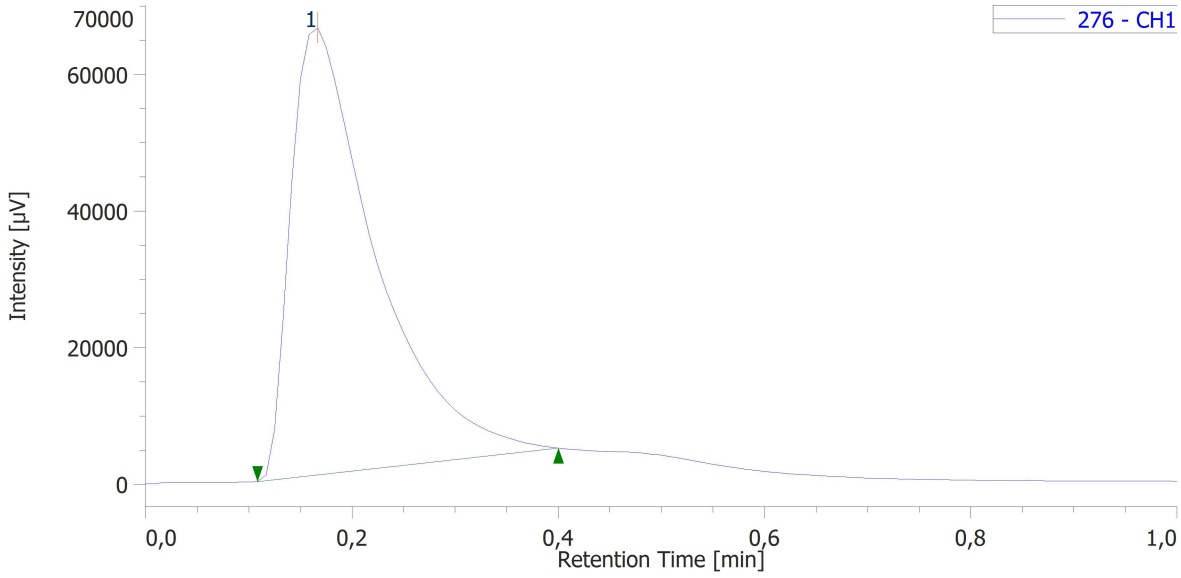

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 15:05:48
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 15:04:45
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	276
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	276-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,167	375131	65400	100,000	100,000	N/A	23	N/A	2,320	

Creator
Reviewer
Approver

Chromatogram

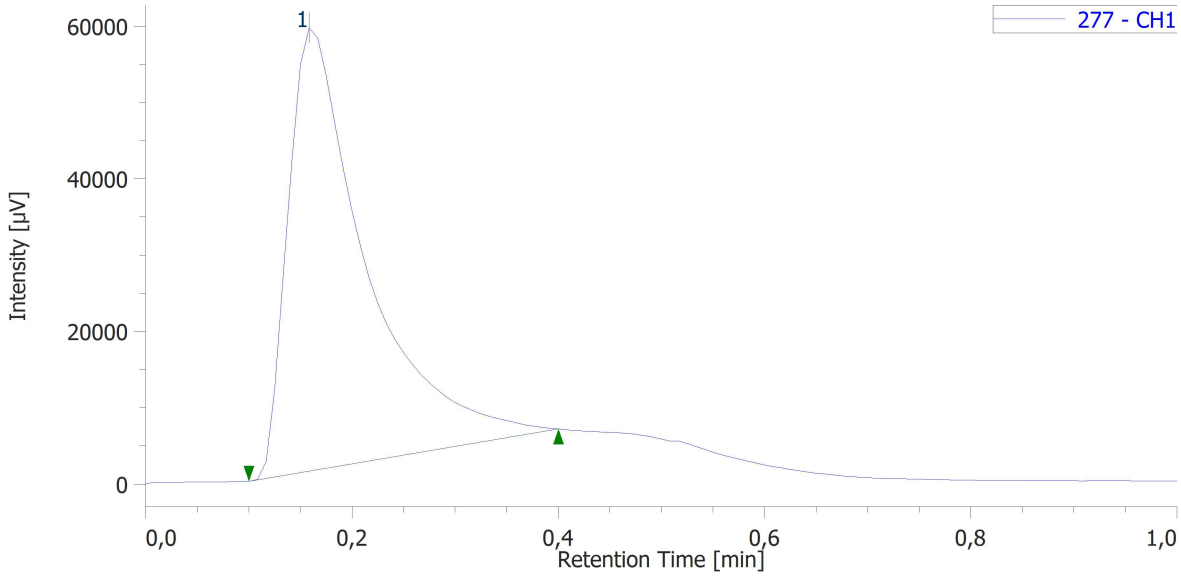

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 15:10:24
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 15:09:21
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	277
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	277-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	306636	58040	100,000	100,000	N/A	27	N/A	2,686	

Creator
Reviewer
Approver

Chromatogram

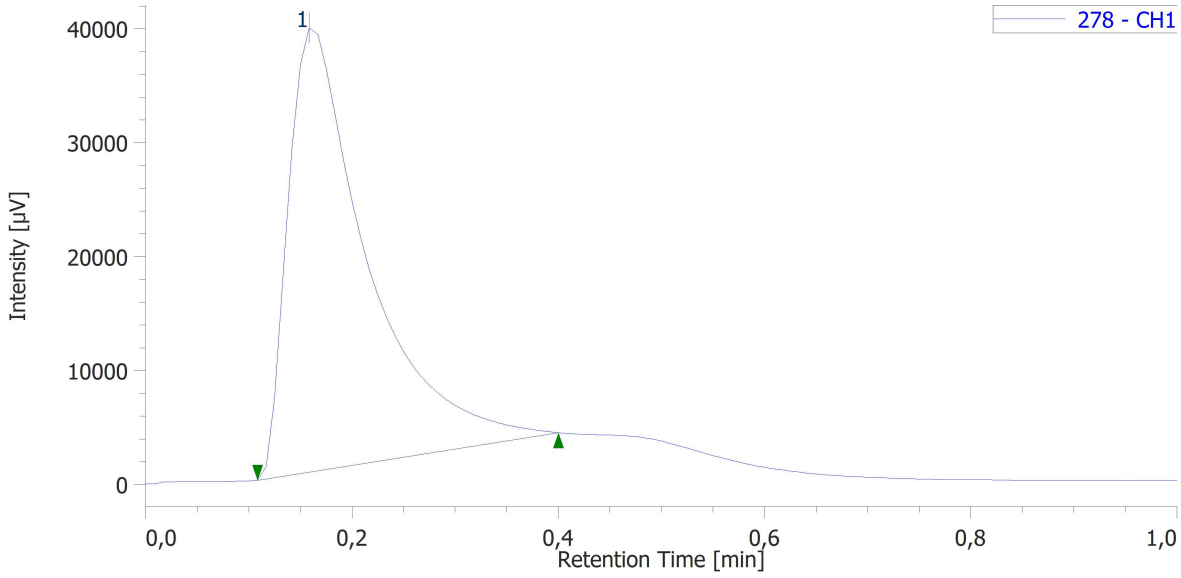

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 15:15:00
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 15:13:57
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	278
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	278-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	EDUV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,158	209501	38957	100,000	100,000	N/A	25	N/A	2,688	

Creator
Reviewer
Approver

Chromatogram

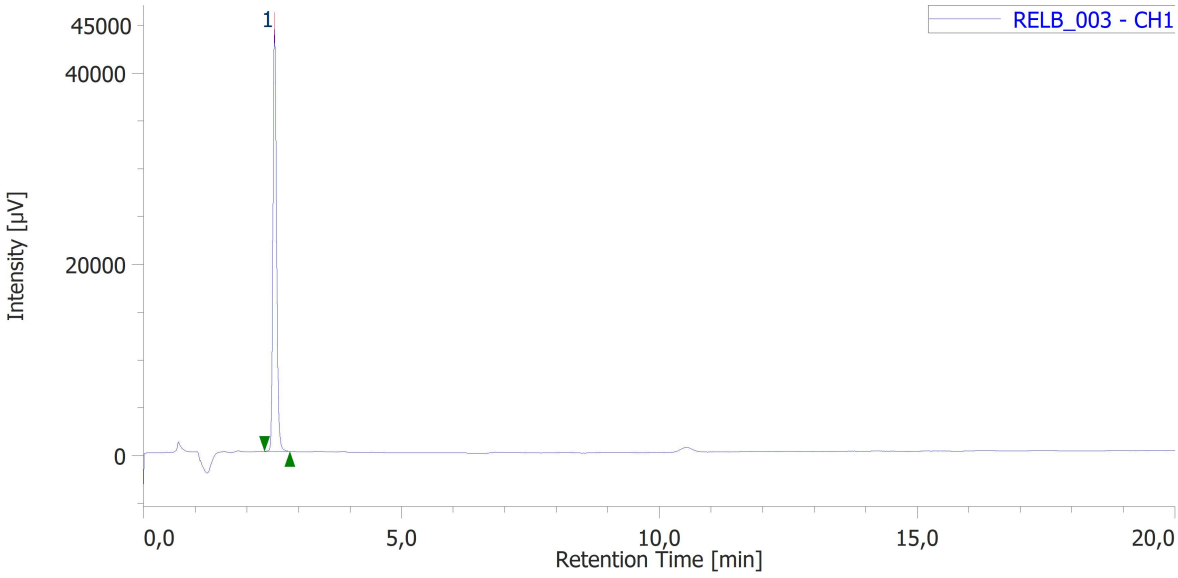

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 16:35:39
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 16:15:36
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,533	217858	44250	100,000	100,000	N/A	6406	N/A	1,265	

Creator
Reviewer
Approver

Chromatogram

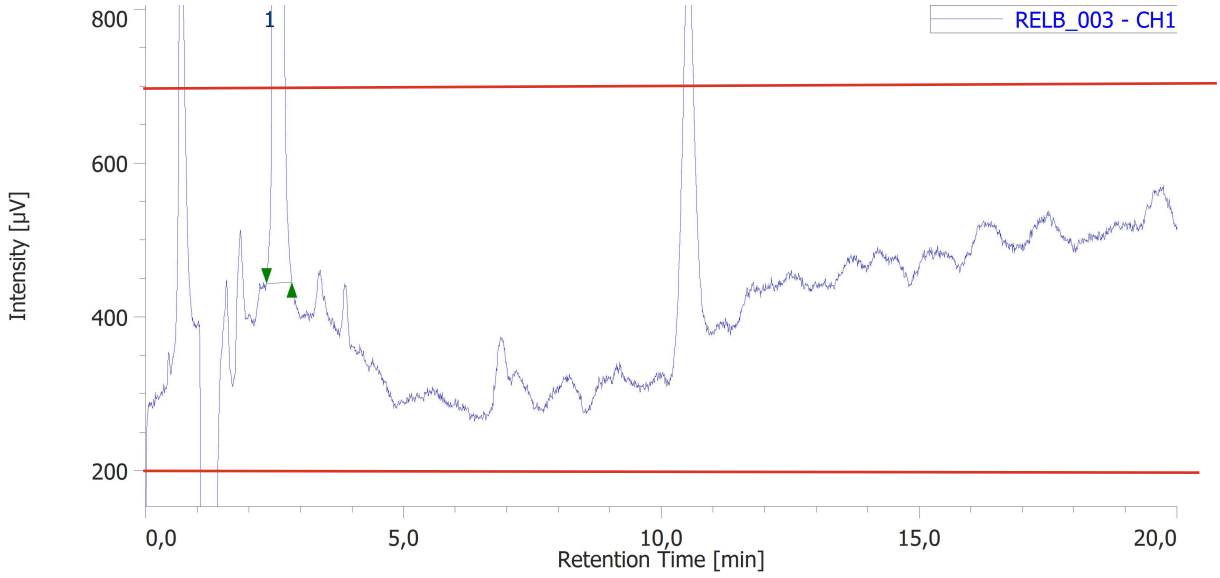

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 16:35:39
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 16:15:36
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,533	217858	44250	100,000	100,000	N/A	6406	N/A	1,265	

Creator
Reviewer
Approver

Chromatogram

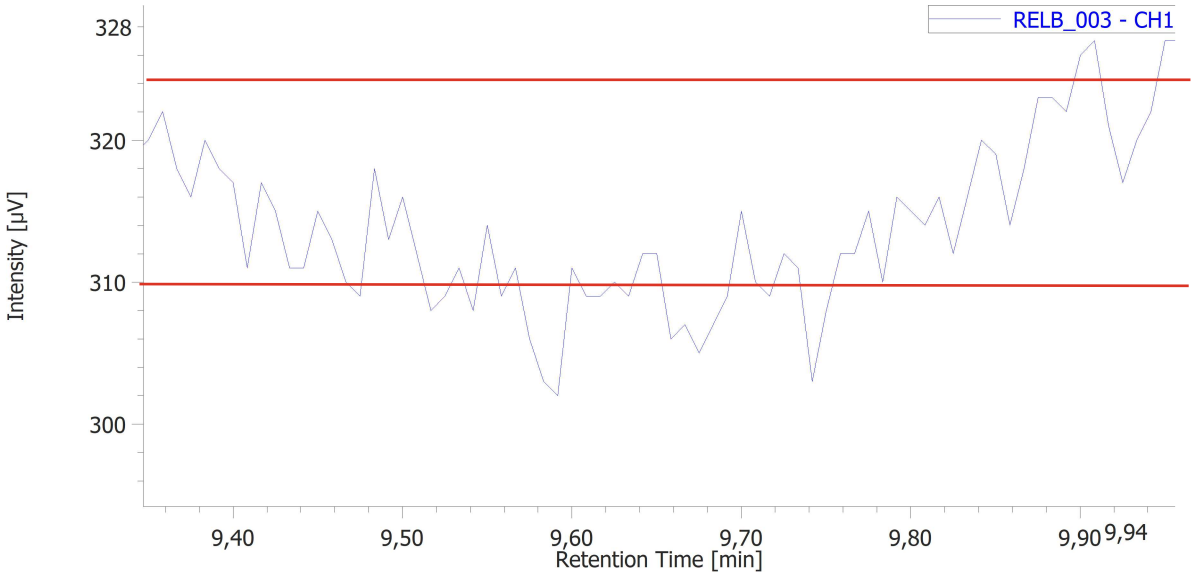

Chromatogram Information	
User Name	QPackSA
Date Modified	25/02/2026 16:35:39
Description	
HPLC System Name	HPLC-0001
Injection Date	25/02/2026 16:15:36
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	SRELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,533	217858	44250	100,000	100,000	N/A	6406	N/A	1,265	

Creator
Reviewer
Approver

Chromatogram

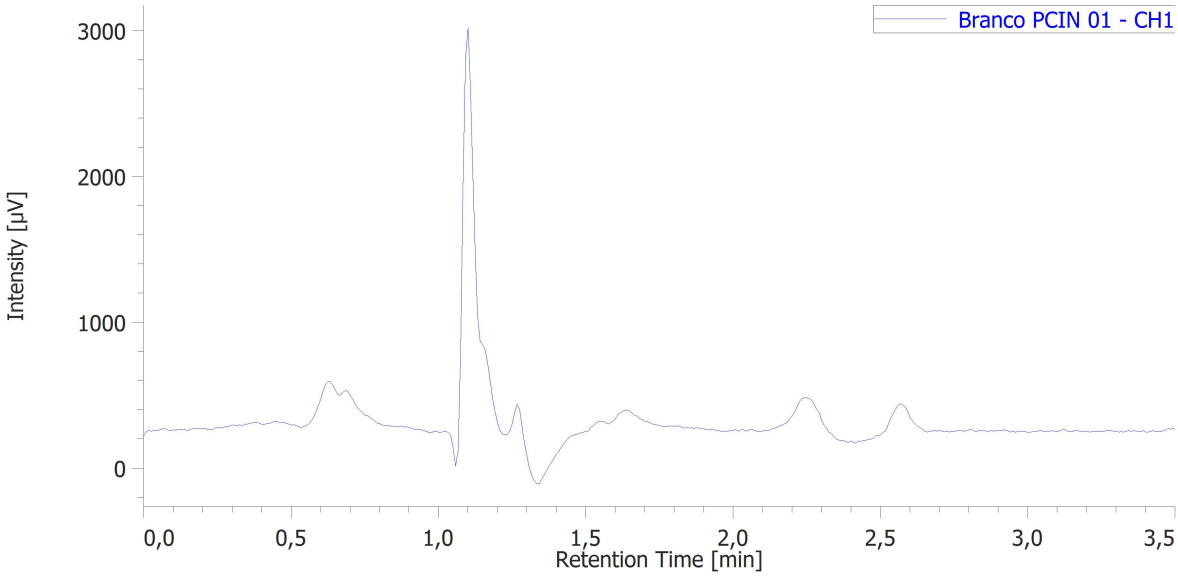


Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 12:31:25
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:27:52
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

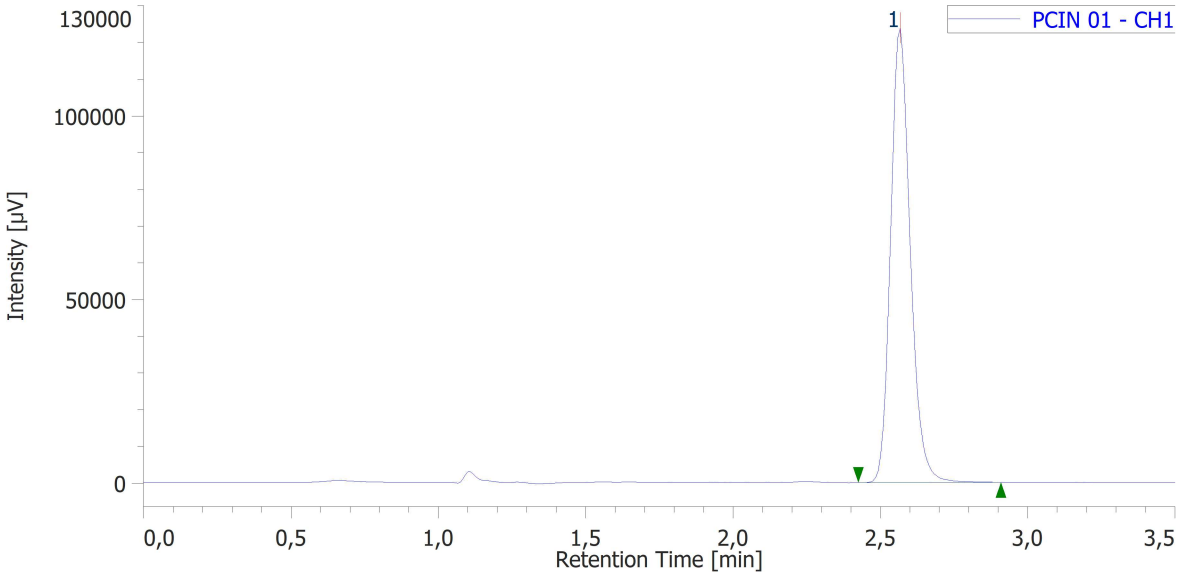

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 12:36:57
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:33:25
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	571985	123709	100,000	100,000	N/A	7468	N/A	1,156	

Creator QPackSA
Reviewer
Approver

Chromatogram

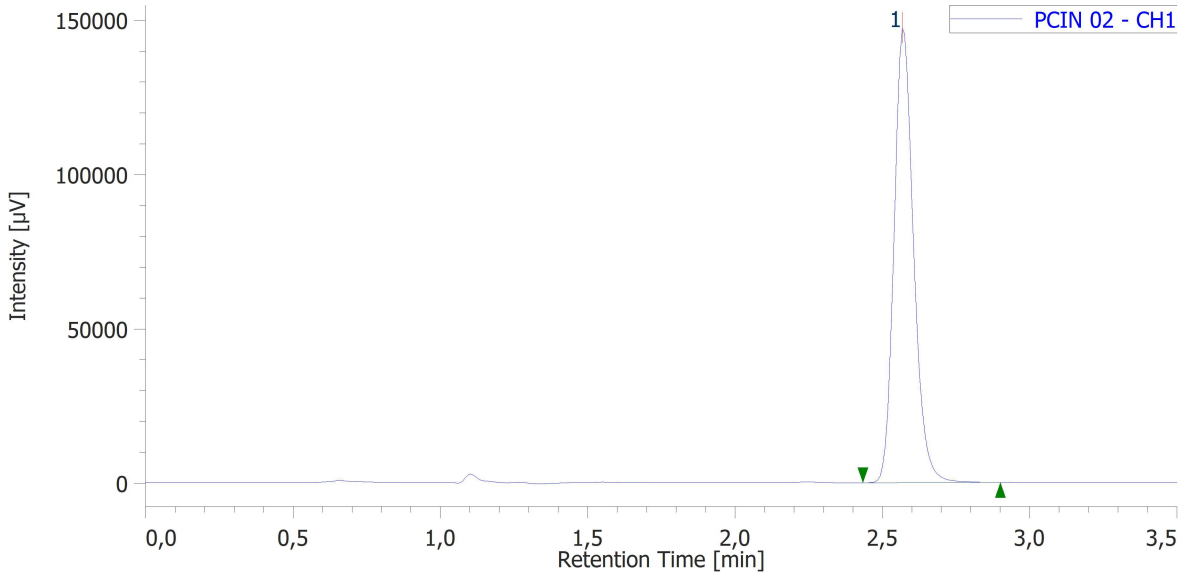

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 12:42:33
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:39:01
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	566395	122257	100,000	100,000	N/A	7526	N/A	1,242	

Creator QPackSA
Reviewer
Approver

Chromatogram

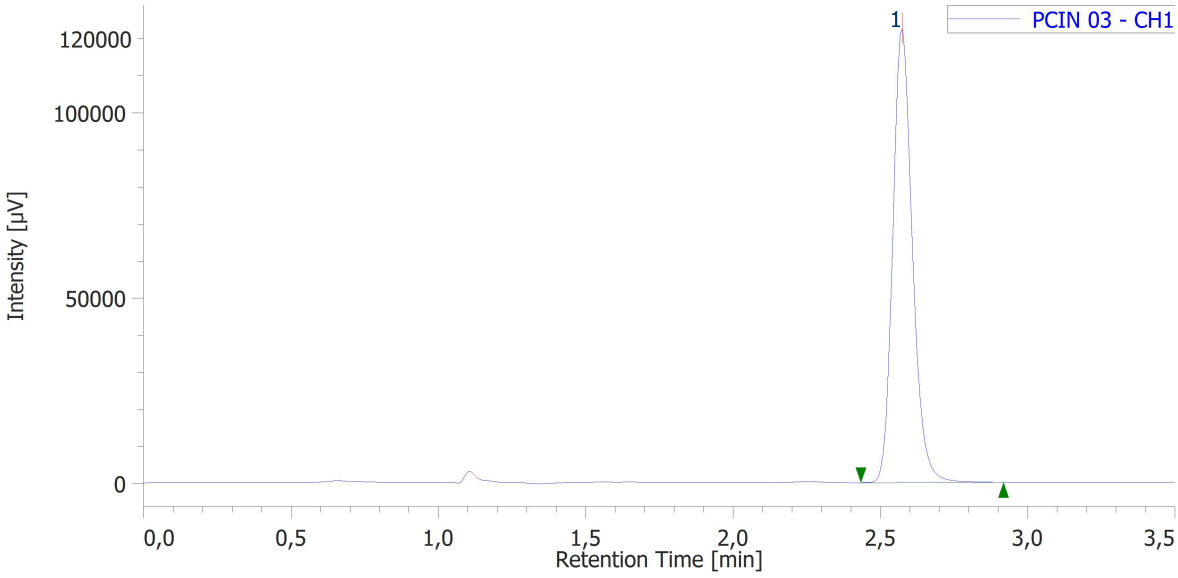

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 12:48:07
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:44:34
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,575	566363	122646	100,000	100,000	N/A	7552	N/A	1,140	

Creator QPackSA
Reviewer
Approver

Chromatogram

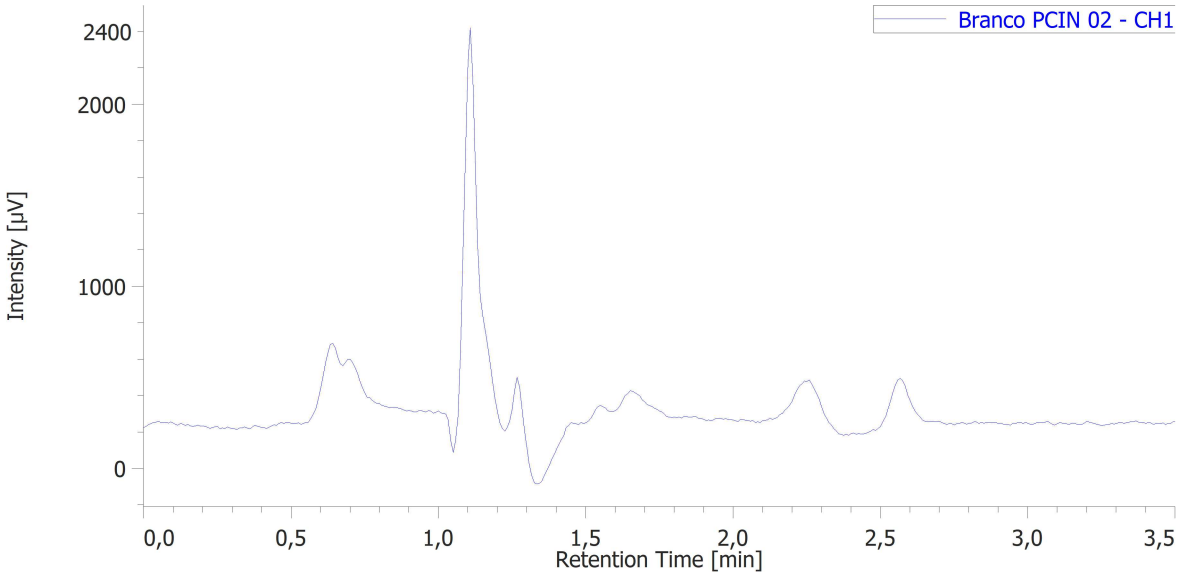


Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 12:53:39
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:50:07
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

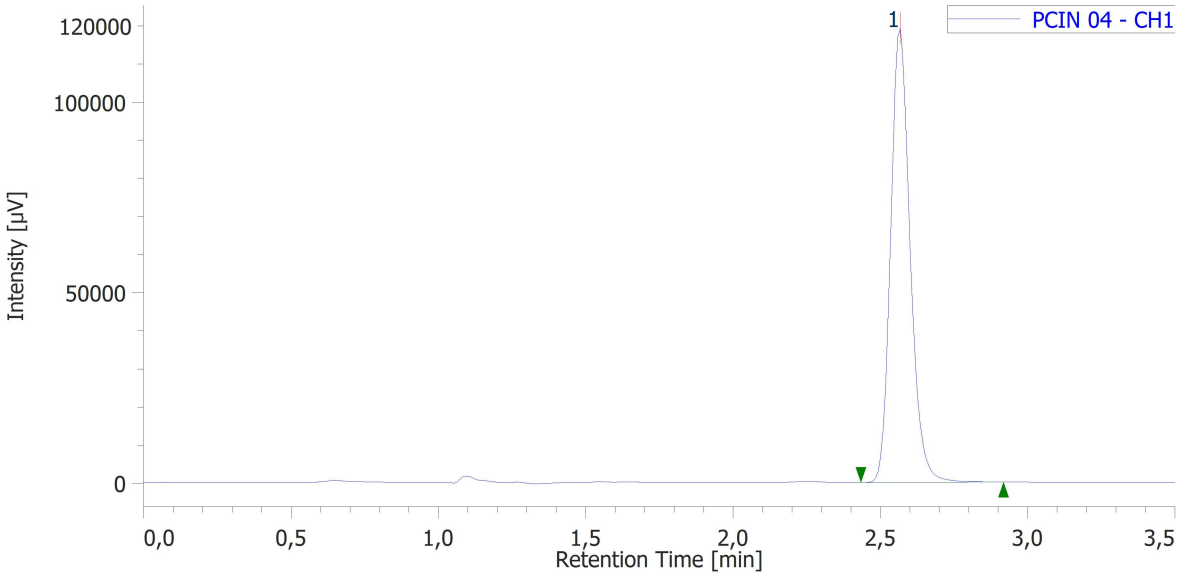

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 12:59:15
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 12:55:43
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	566704	122210	100,000	100,000	N/A	7610	N/A	1,157	

Creator QPackSA
Reviewer
Approver

Chromatogram

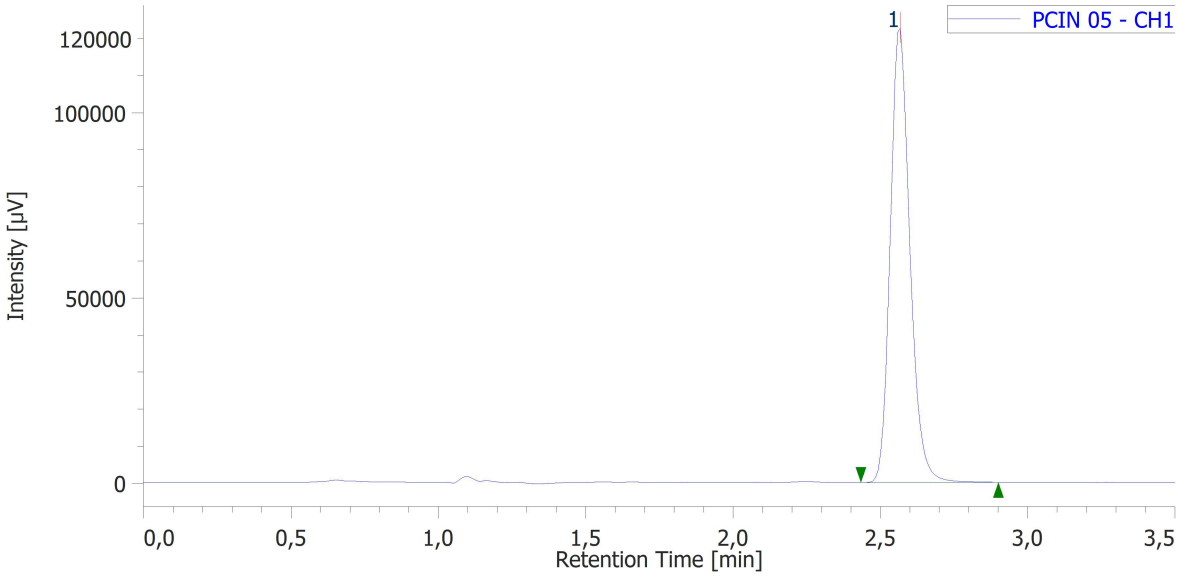

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:04:51
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:01:19
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	566283	122642	100,000	100,000	N/A	7507	N/A	1,138	

Creator QPackSA
Reviewer
Approver

Chromatogram

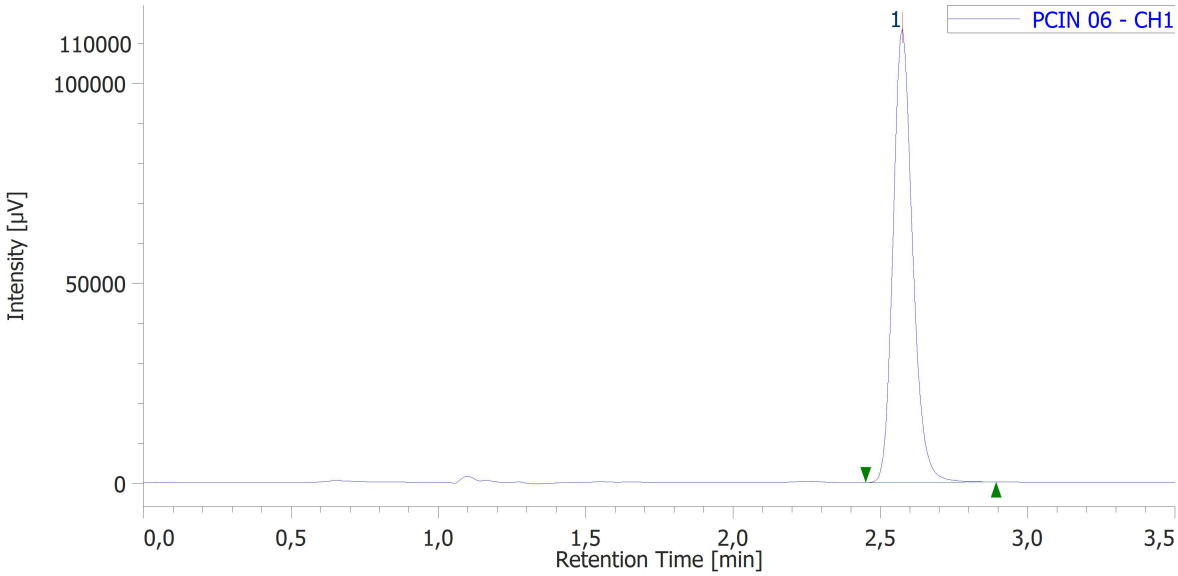

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:10:25
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:06:52
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,575	561561	122562	100,000	100,000	N/A	7625	N/A	1,157	

Creator QPackSA
Reviewer
Approver

Chromatogram

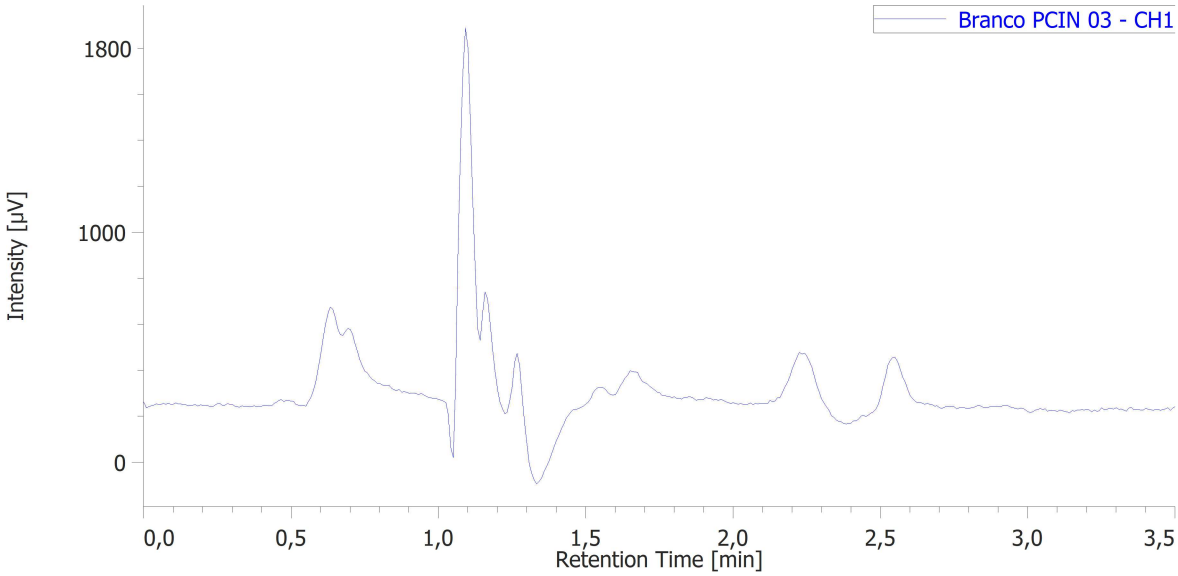


Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:15:57
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:12:25
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

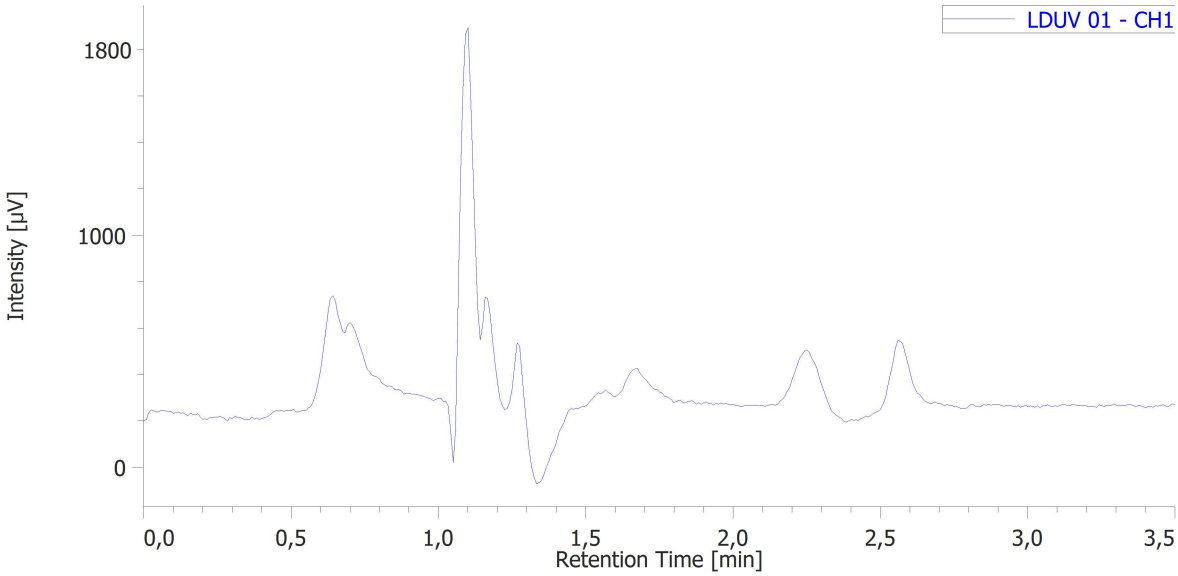


Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:21:33
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:18:01
Volume	10,0 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

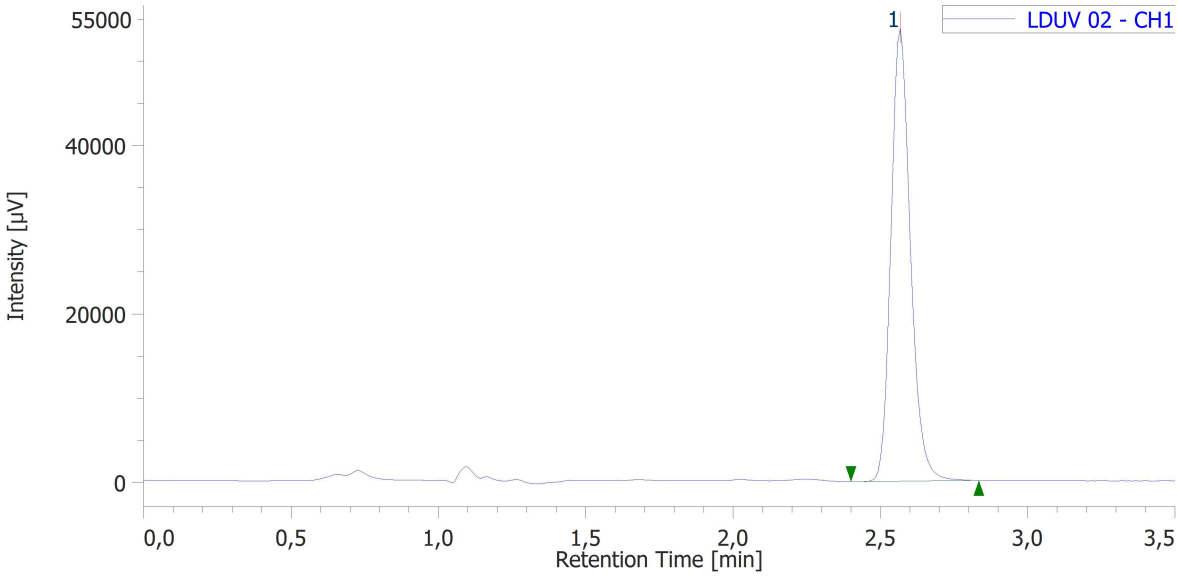

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:27:09
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:23:36
Volume	10,0 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	246742	53753	100,000	100,000	N/A	7582	N/A	1,177	

Creator QPackSA
Reviewer
Approver

Chromatogram

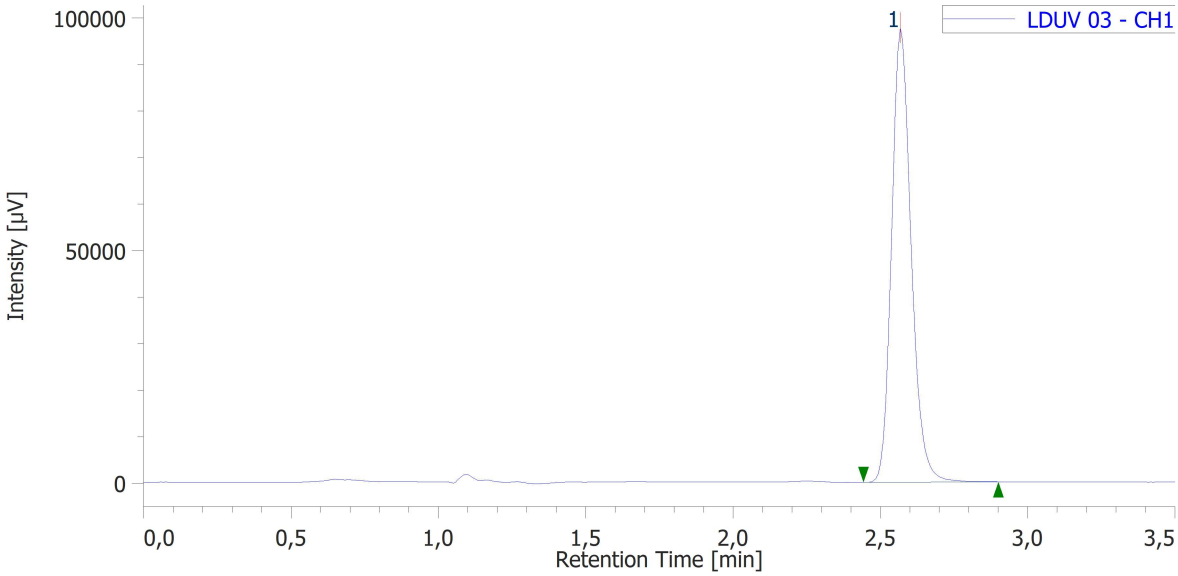

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:32:47
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:29:14
Volume	10,0 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	479178	97582	100,000	100,000	N/A	7535	N/A	1,217	

Creator QPackSA
Reviewer
Approver

Chromatogram

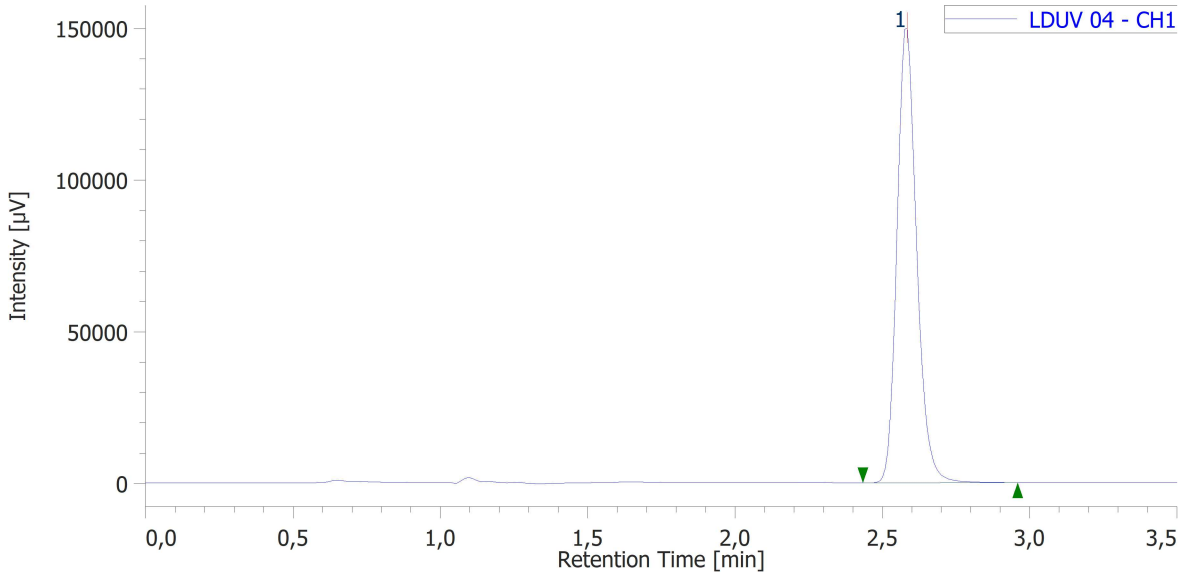

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:38:23
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:34:50
Volume	10,0 [µL]
Sample #	7
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,583	734503	149816	100,000	100,000	N/A	7572	N/A	1,128	

Creator QPackSA
Reviewer
Approver

Chromatogram

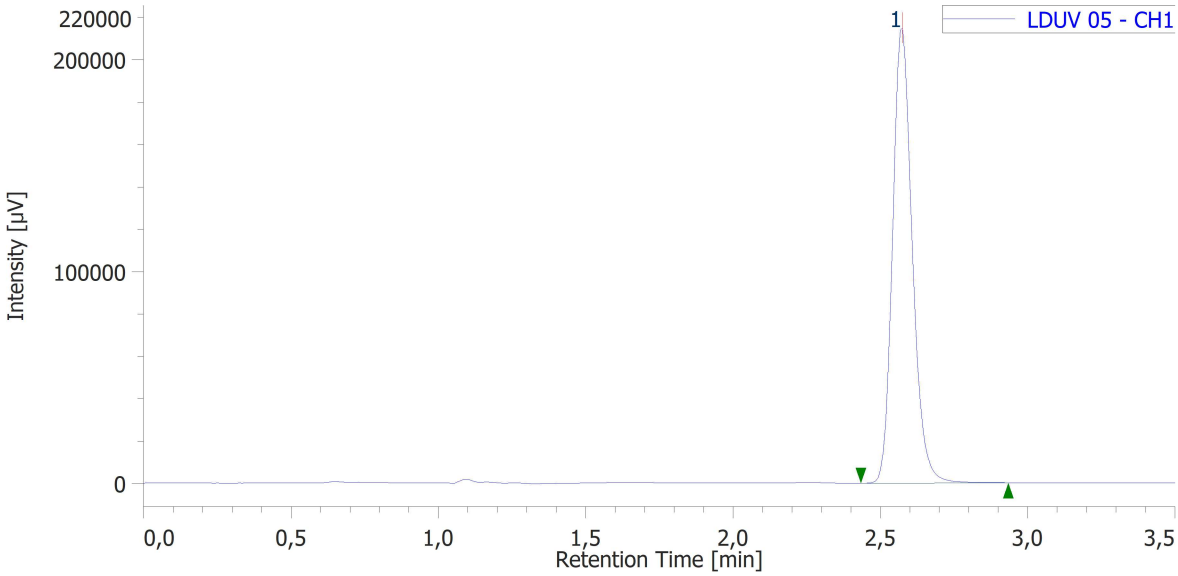

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:44:01
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:40:28
Volume	10,0 [µL]
Sample #	8
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,575	996078	214660	100,000	100,000	N/A	7480	N/A	1,132	

Creator QPackSA
Reviewer
Approver

Chromatogram

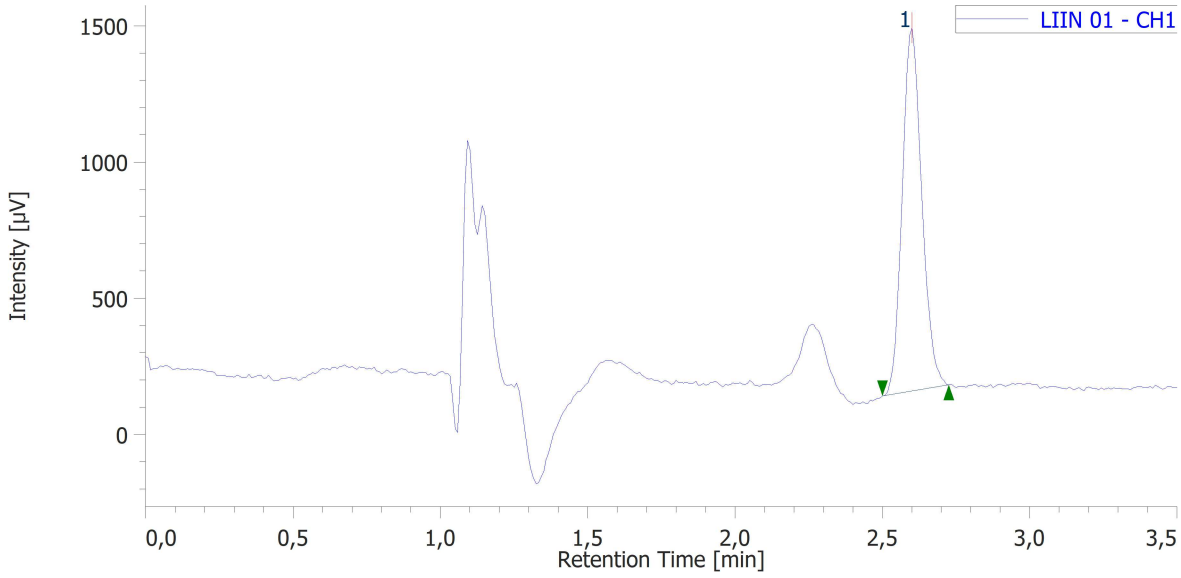

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:49:29
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:45:56
Volume	0,1 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,600	6134	1332	100,000	100,000	N/A	7455	N/A	1,110	

Creator QPackSA
Reviewer
Approver

Chromatogram

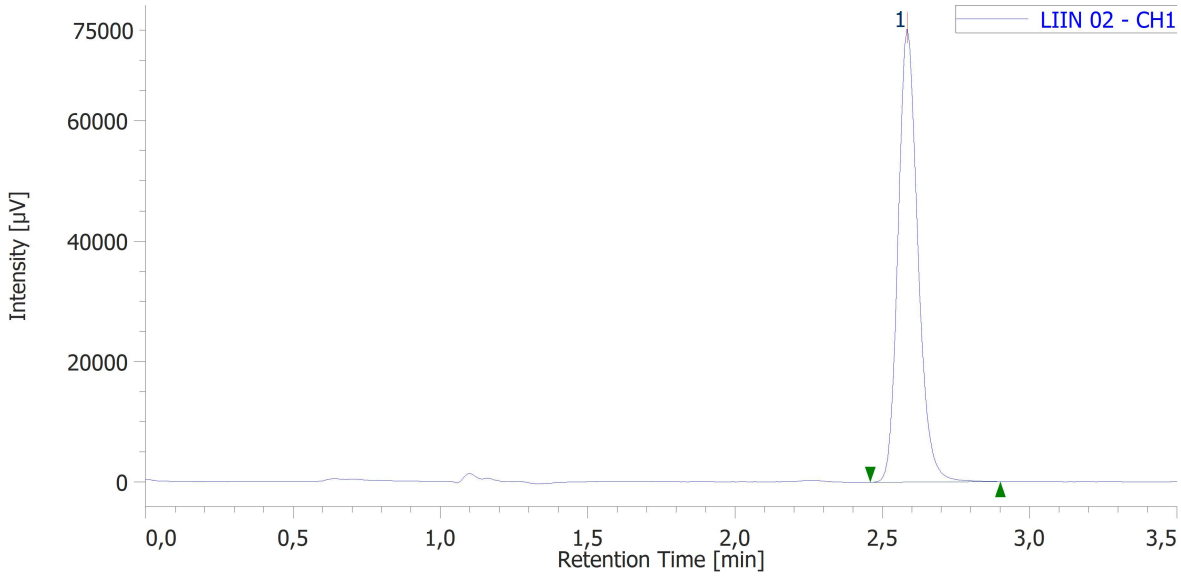

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 13:54:59
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:51:27
Volume	5,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,583	350073	75317	100,000	100,000	N/A	7473	N/A	1,196	

Creator QPackSA
Reviewer
Approver

Chromatogram

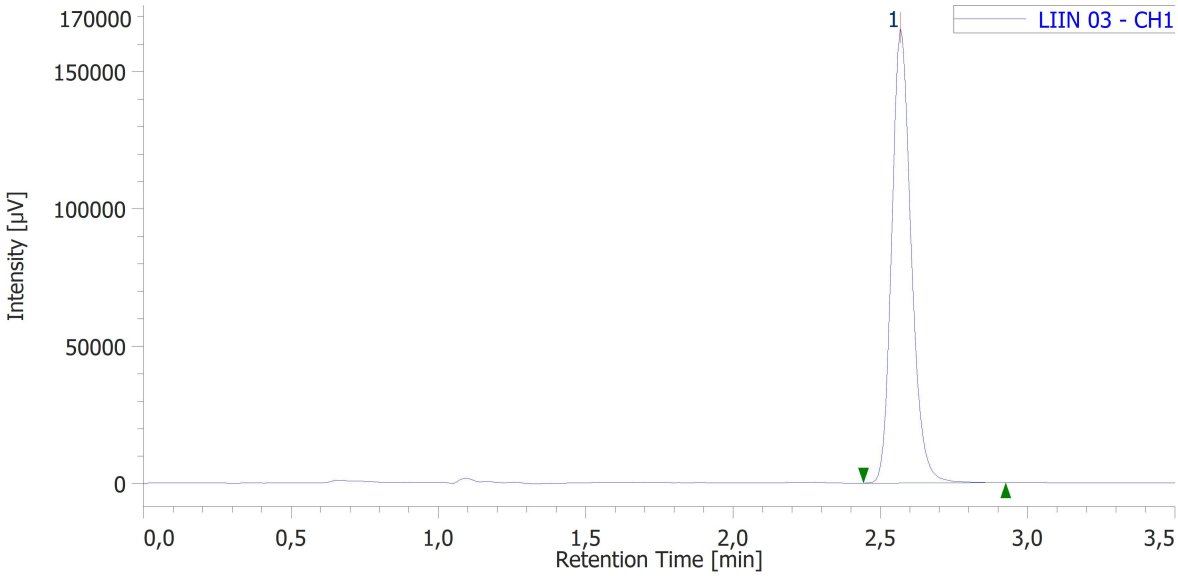

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 14:00:39
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 13:57:05
Volume	10,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,567	709250	165578	100,000	100,000	N/A	7589	N/A	1,223	

Creator QPackSA
Reviewer
Approver

Chromatogram

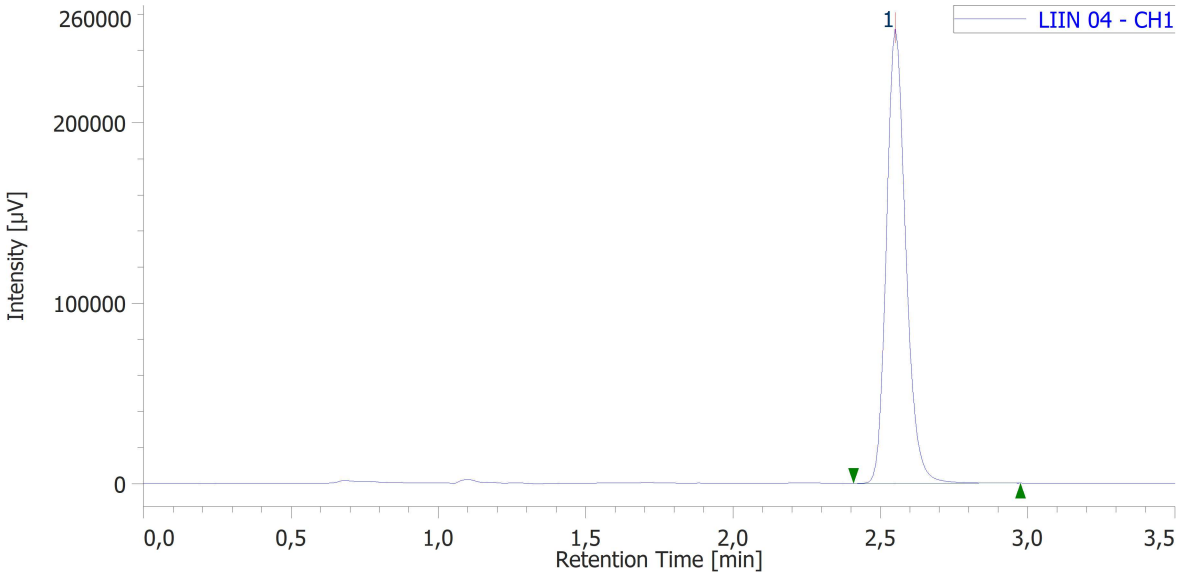

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 14:06:21
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 14:02:48
Volume	15,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,550	1045398	252098	100,000	100,000	N/A	7636	N/A	1,199	

Creator QPackSA
Reviewer
Approver

Chromatogram

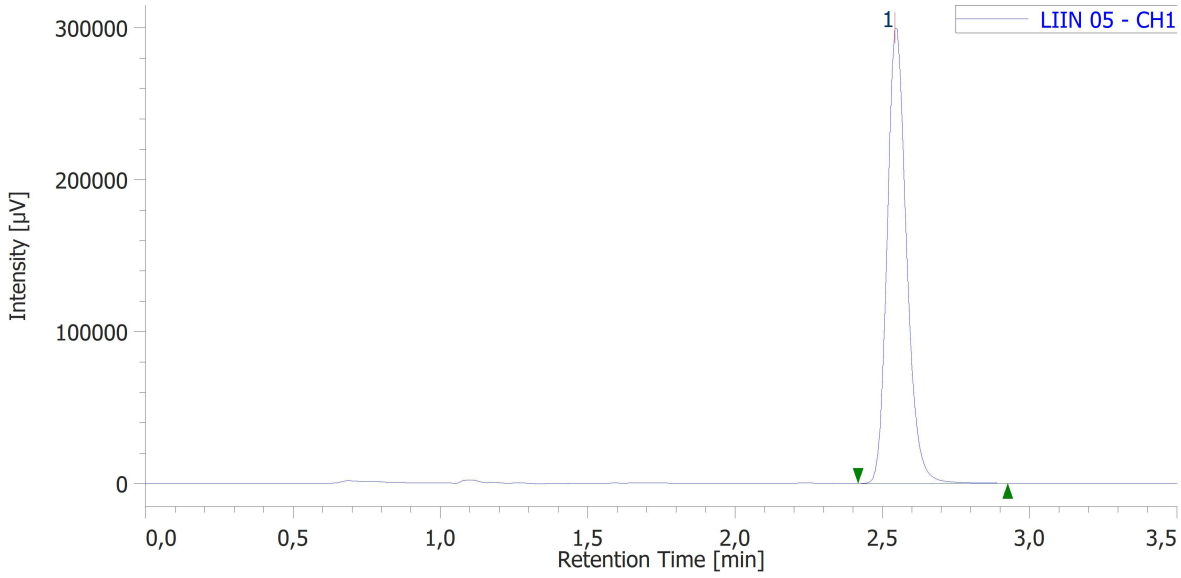

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 14:12:11
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 14:08:39
Volume	20,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,542	1367384	299528	100,000	100,000	N/A	7537	N/A	1,281	

Creator QPackSA
Reviewer
Approver

Chromatogram

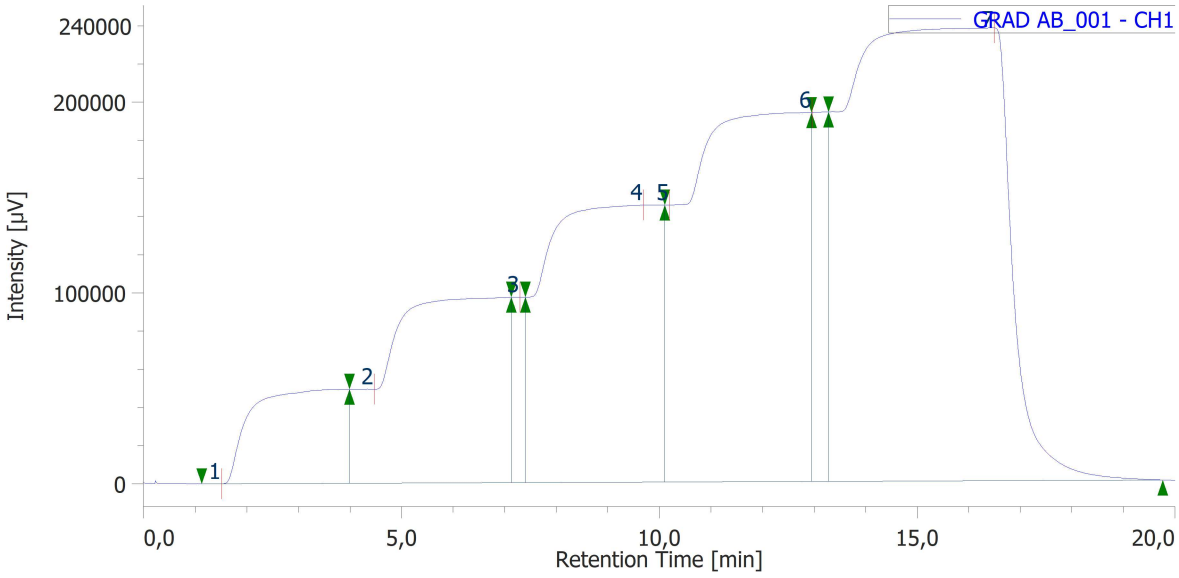

Chromatogram Information

User Name	QPackSA
Date Modified	26/02/2026 14:59:52
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 14:39:50
Volume	0,0 [µL]
Sample #	-
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	GRBO AB
Peak ID Table	GRAD
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,508	-11577	63	N/A	0,007	N/A	287	N/A	0,579	
2	20%	1	4,467	15593831	49131	12,588	5,669	N/A	N/A	N/A	N/A	
3	40%	1	7,292	1601450	97030	1,293	11,196	N/A	N/A	N/A	N/A	
4	60%	1	9,683	22018857	145126	17,774	16,745	N/A	N/A	N/A	N/A	
5	Unknown	1	10,192	30698474	145048	24,781	16,736	N/A	N/A	N/A	N/A	
6	80%	1	12,958	3770405	193173	3,044	22,289	N/A	N/A	N/A	N/A	
7	100%	1	16,492	50207855	237106	40,530	27,358	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

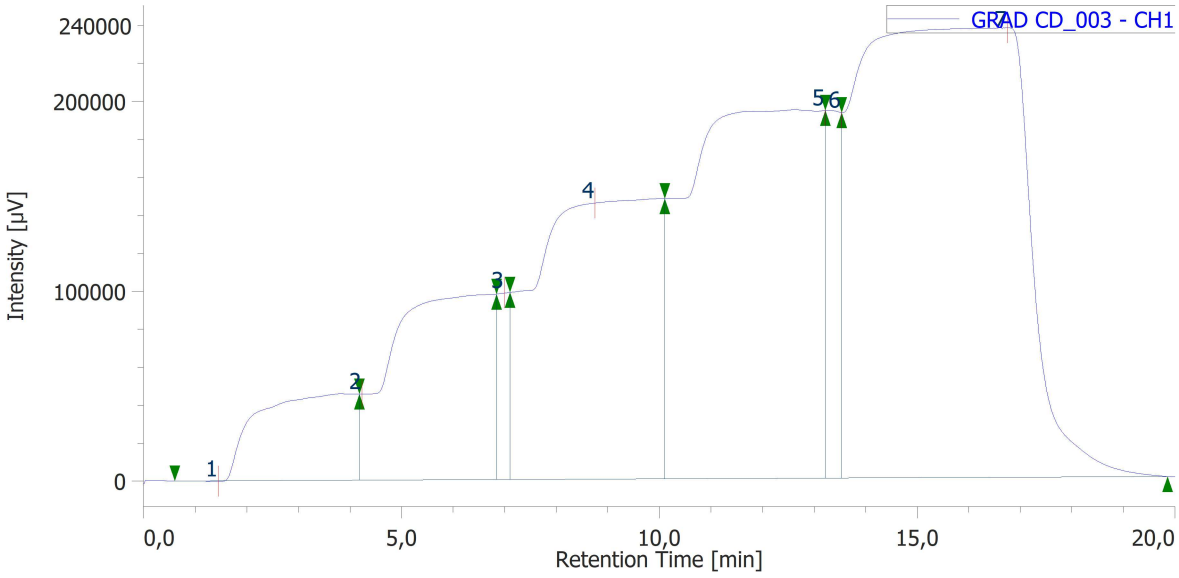

Chromatogram Information	
User Name	QPackSA
Date Modified	26/02/2026 16:10:08
Description	
HPLC System Name	HPLC-0001
Injection Date	26/02/2026 15:50:06
Volume	0,0 [µL]
Sample #	-
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	GRBO CD
Peak ID Table	GRAD
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD CD_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,450	-3100	270	N/A	0,030	N/A	49	N/A	0,583	
2	20%	1	4,233	13191089	45330	10,175	4,974	N/A	N/A	N/A	N/A	
3	40%	1	6,992	1519650	98113	1,172	10,765	N/A	N/A	N/A	N/A	
4	Unknown	1	8,750	24152498	145330	18,631	15,946	N/A	N/A	N/A	N/A	
5	80%	1	13,208	34103990	193485	26,307	21,229	N/A	N/A	N/A	N/A	
6	Unknown	1	13,525	3670636	192362	2,831	21,106	N/A	N/A	N/A	N/A	
7	100%	1	16,742	53002100	236521	40,885	25,951	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver