
Chromatogram

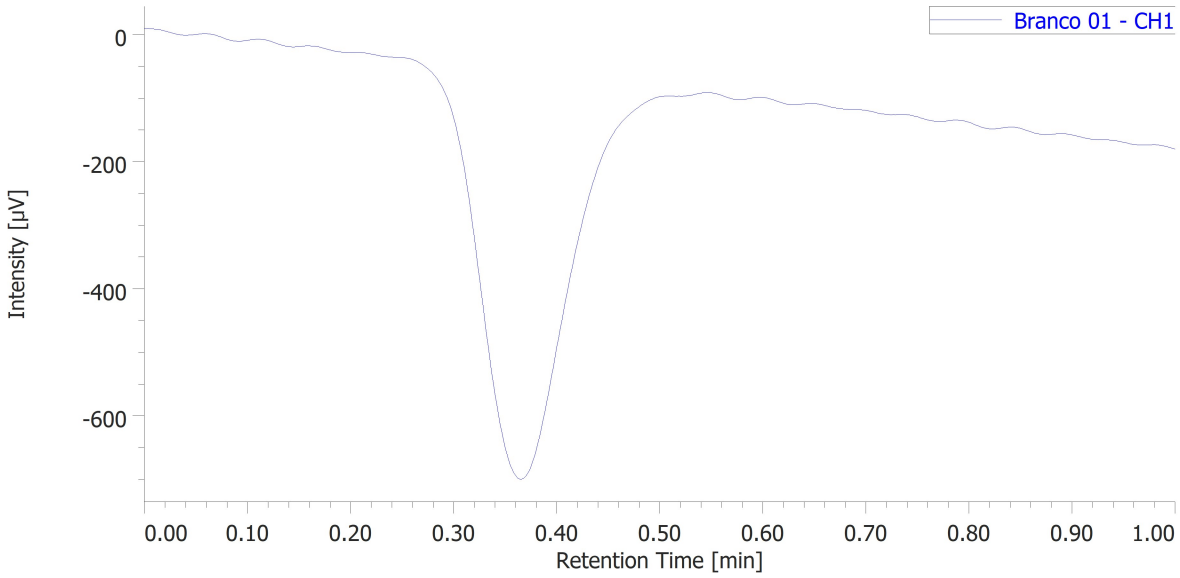


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:40:38 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:33:35 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração (Manual)

Chromatogram

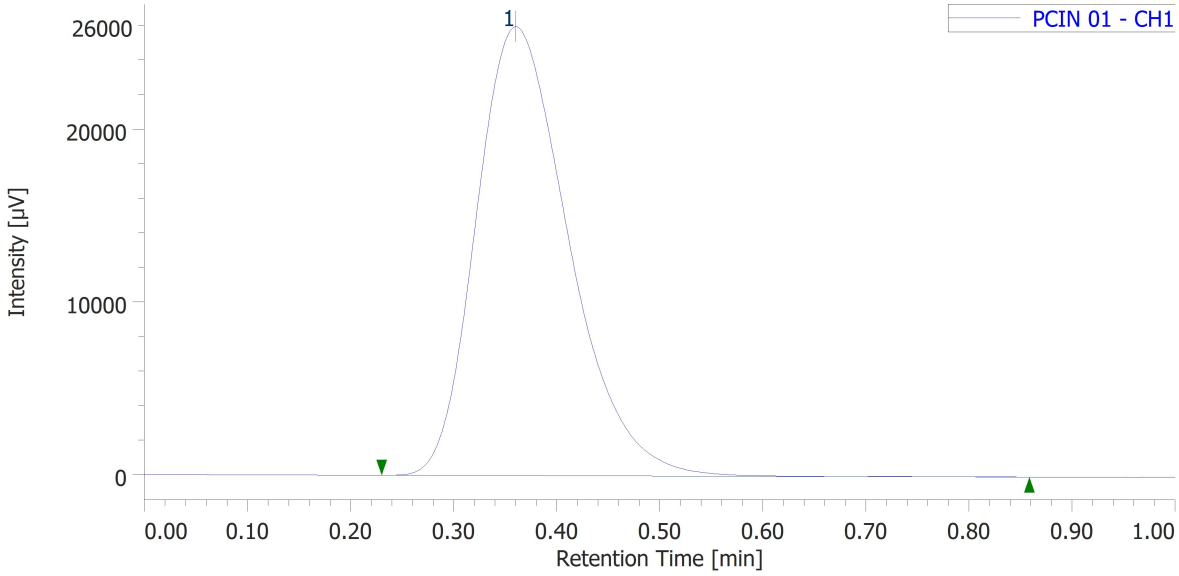


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:40:38 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:35:56 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.360	1799312	288427	100.000	100.000	N/A	78	N/A	1.314	

Chromatogram

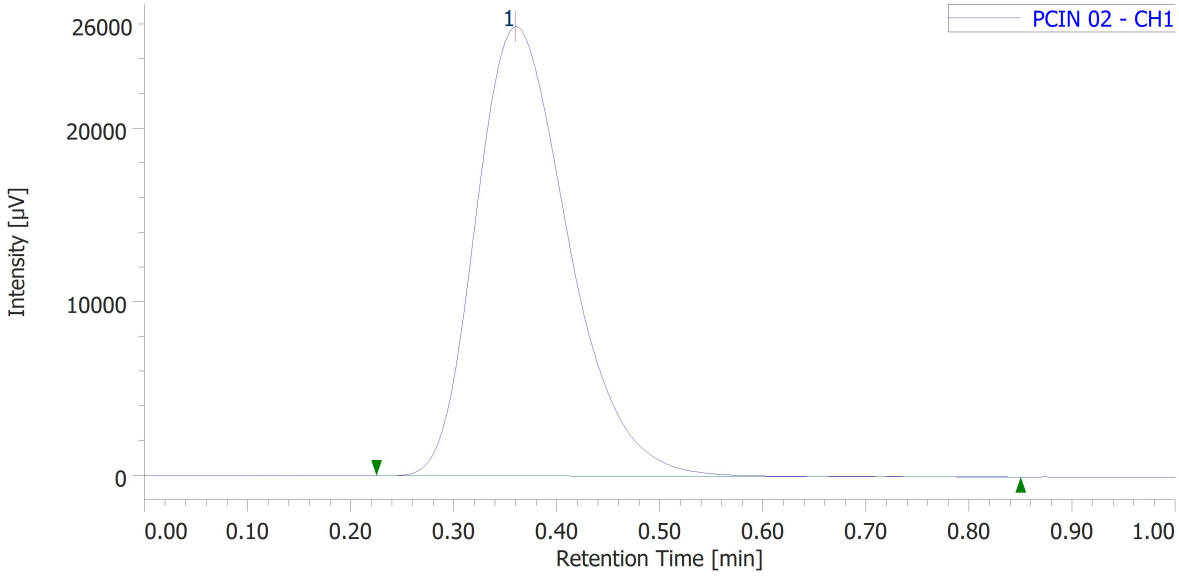


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:40:38 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:38:16 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.360	1795299	287478	100.000	100.000	N/A	78	N/A	1.313	

Chromatogram

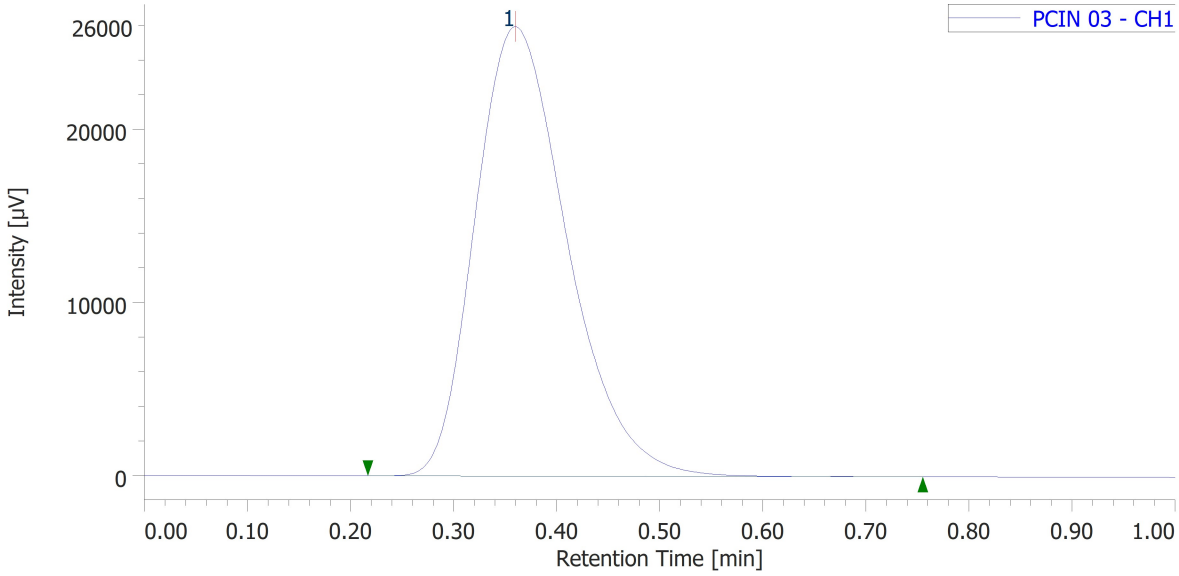


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:43:15 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:40:36 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.360	1791243	288217	100.000	100.000	N/A	79	N/A	1.301	

Chromatogram

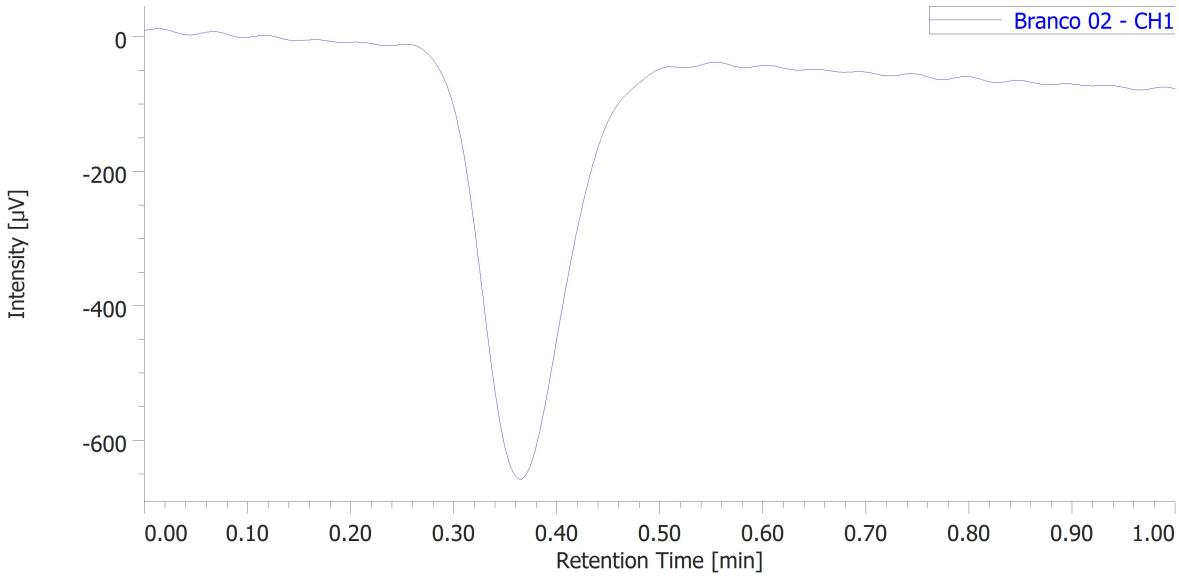


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:47:18 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:42:55 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração (Manual)

Chromatogram

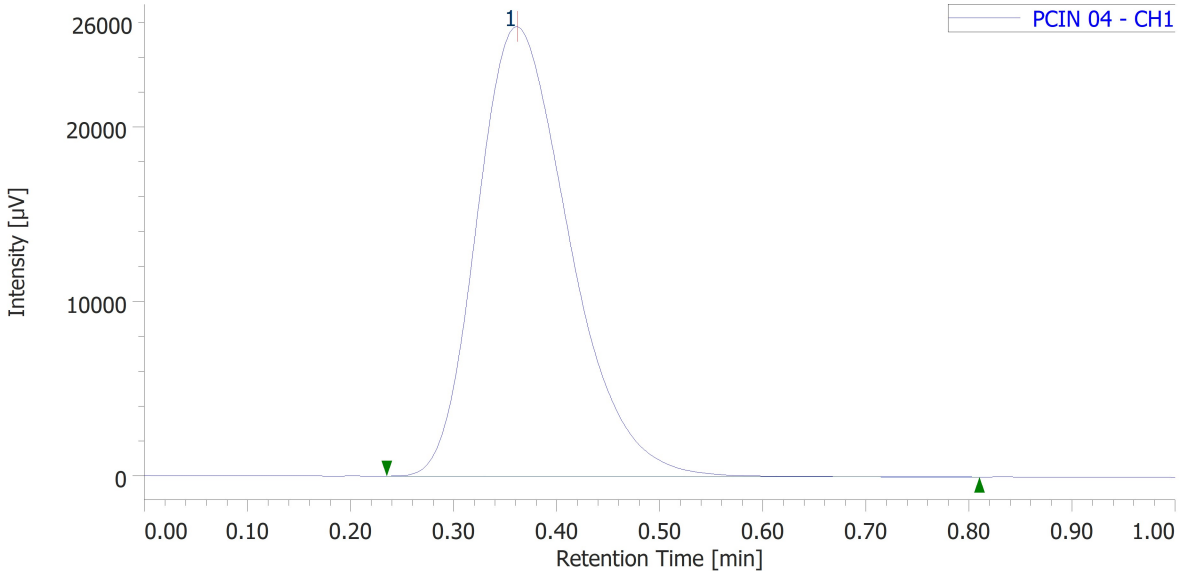


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:47:18 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:45:16 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.362	1782371	286170	100.000	100.000	N/A	79	N/A	1.296	

Chromatogram

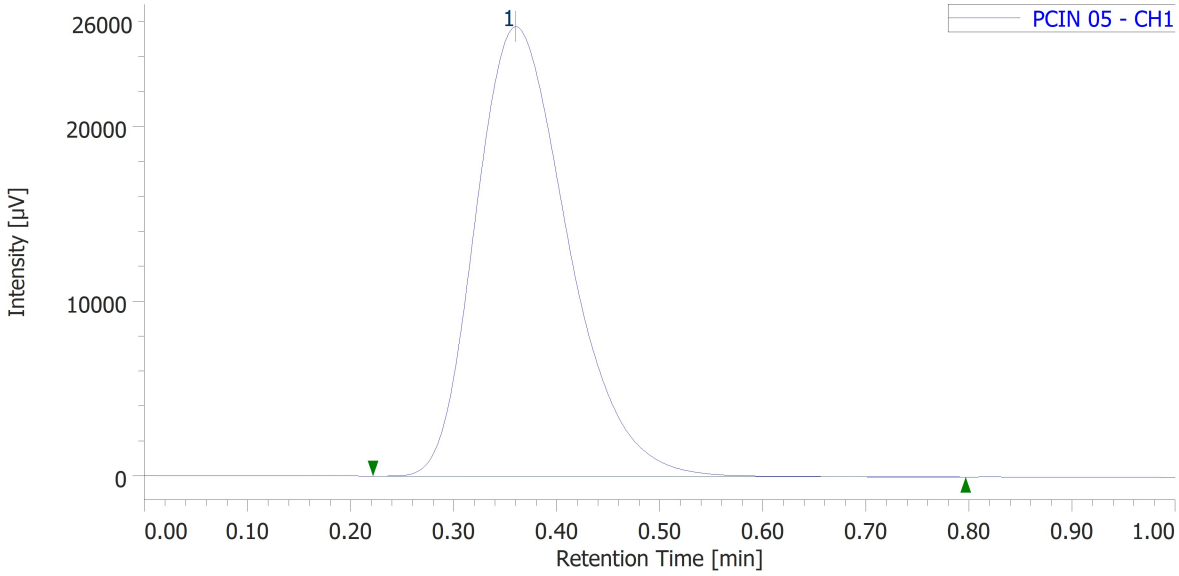


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:49:54 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:47:37 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.360	1783108	285768	100.000	100.000	N/A	78	N/A	1.307	

Chromatogram

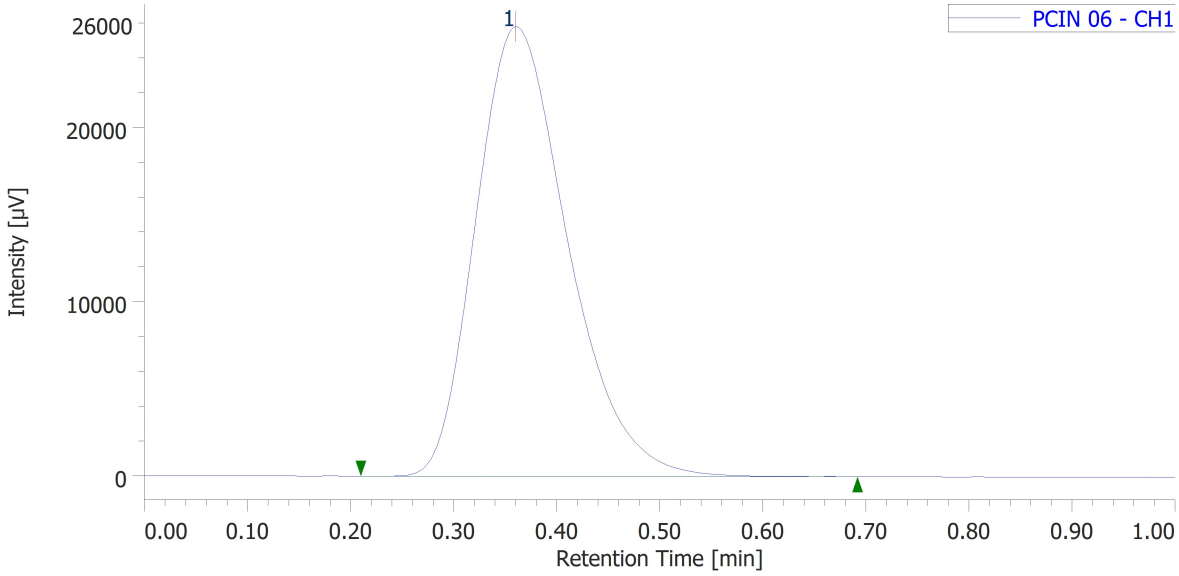


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:51:44 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:49:57 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.360	1776284	286588	100.000	100.000	N/A	79	N/A	1.306	

Chromatogram

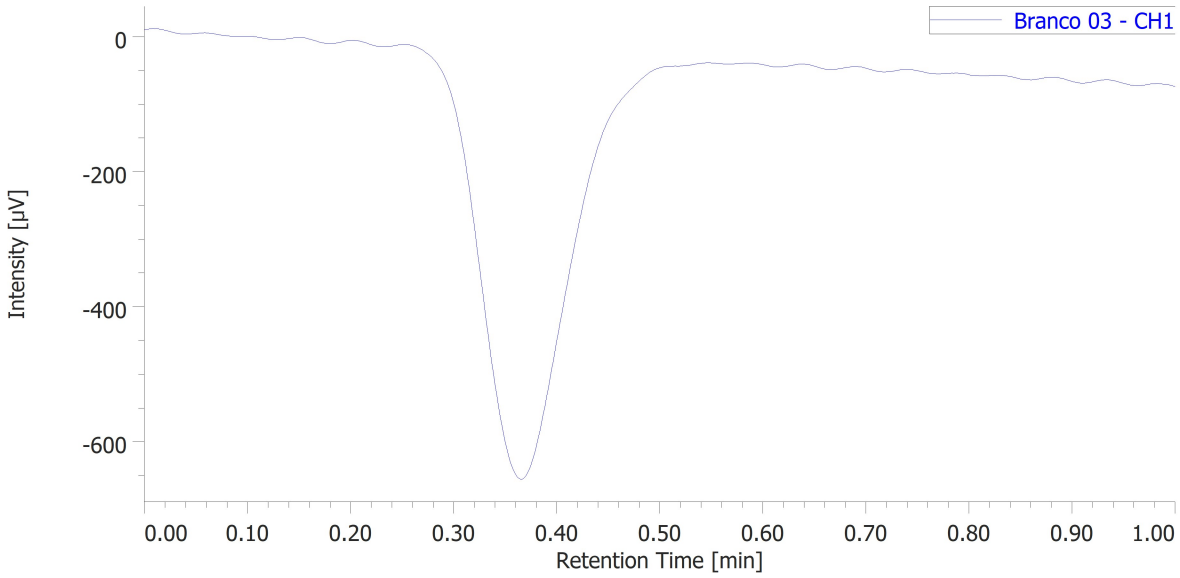


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:58:21 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:52:16 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração (Manual)

Chromatogram

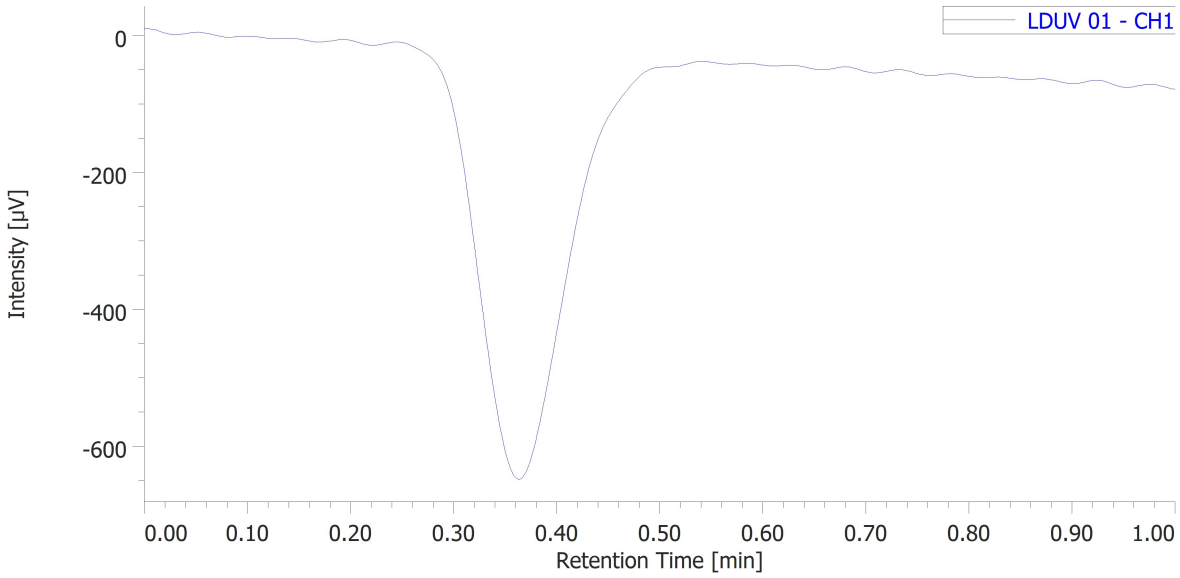


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 12:59:14 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:54:36 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração (Manual)

Chromatogram

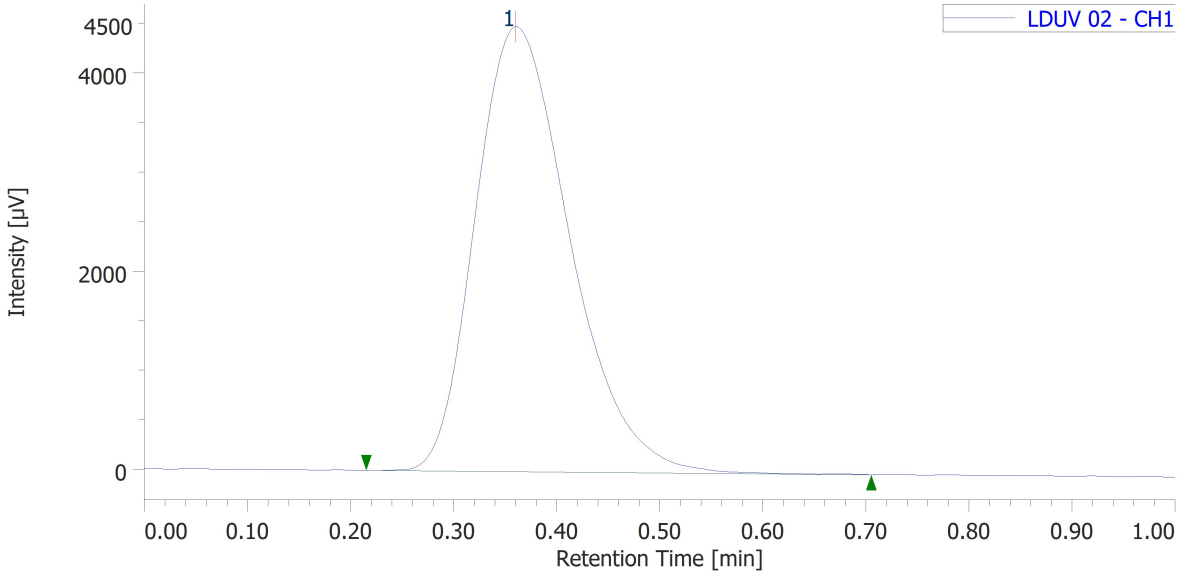


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:06:50 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:56:57 PM
Volume	2.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.360	318607	49909	100.000	100.000	N/A	74	N/A	1.321	

Chromatogram

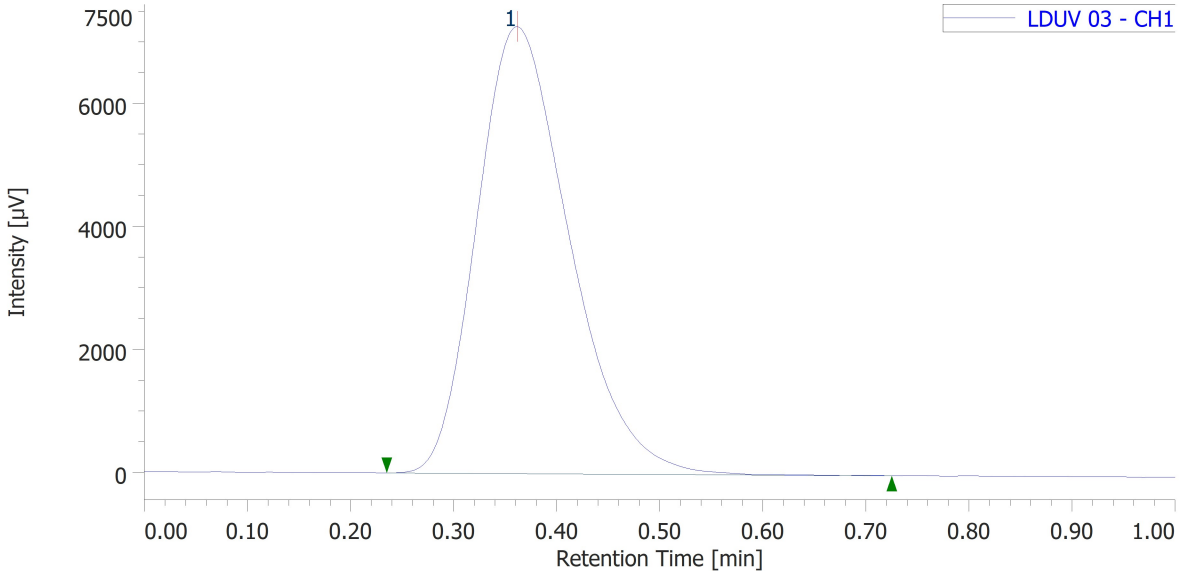


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:06:50 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 12:59:15 PM
Volume	2.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.362	505091	80701	100.000	100.000	N/A	78	N/A	1.289	

Chromatogram

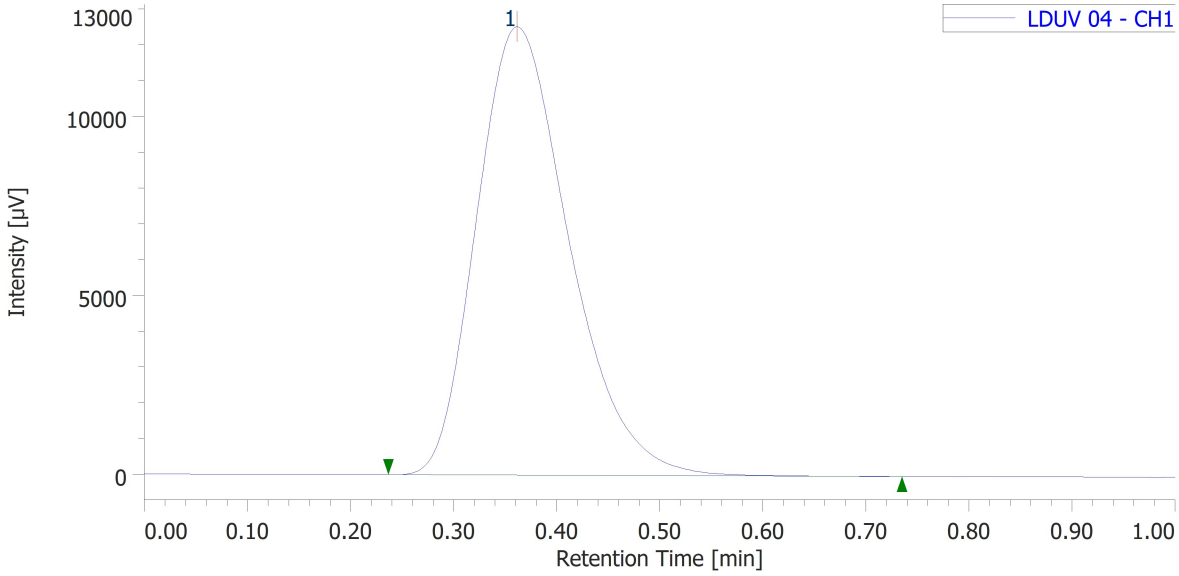


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:06:50 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:01:35 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.362	868610	139136	100.000	100.000	N/A	79	N/A	1.295	

Chromatogram

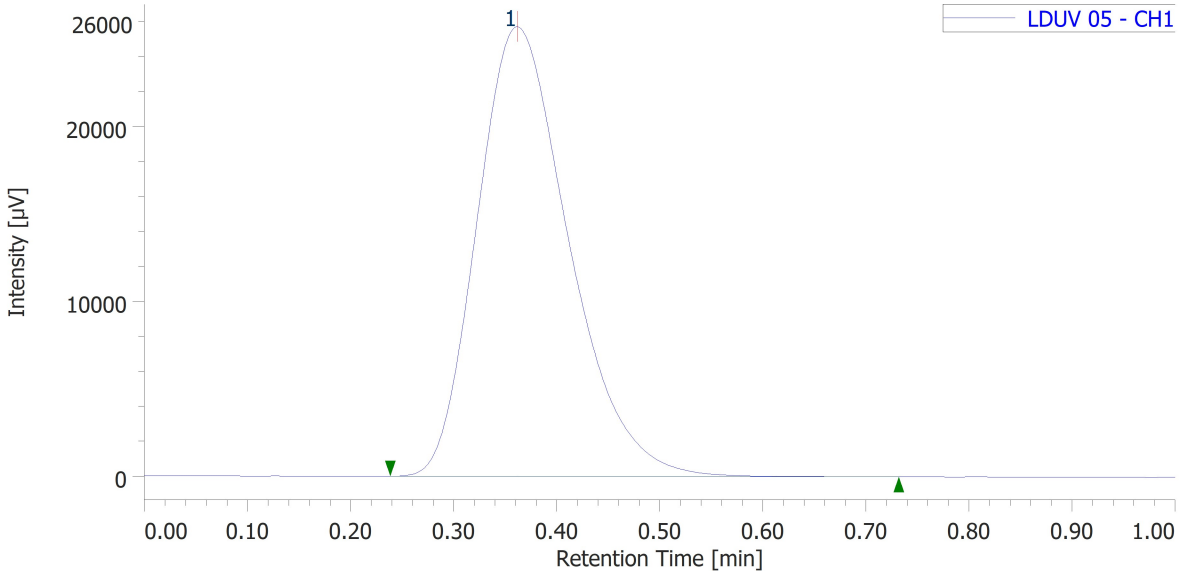


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:06:49 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:03:55 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.362	1768377	285737	100.000	100.000	N/A	80	N/A	1.289	

Chromatogram

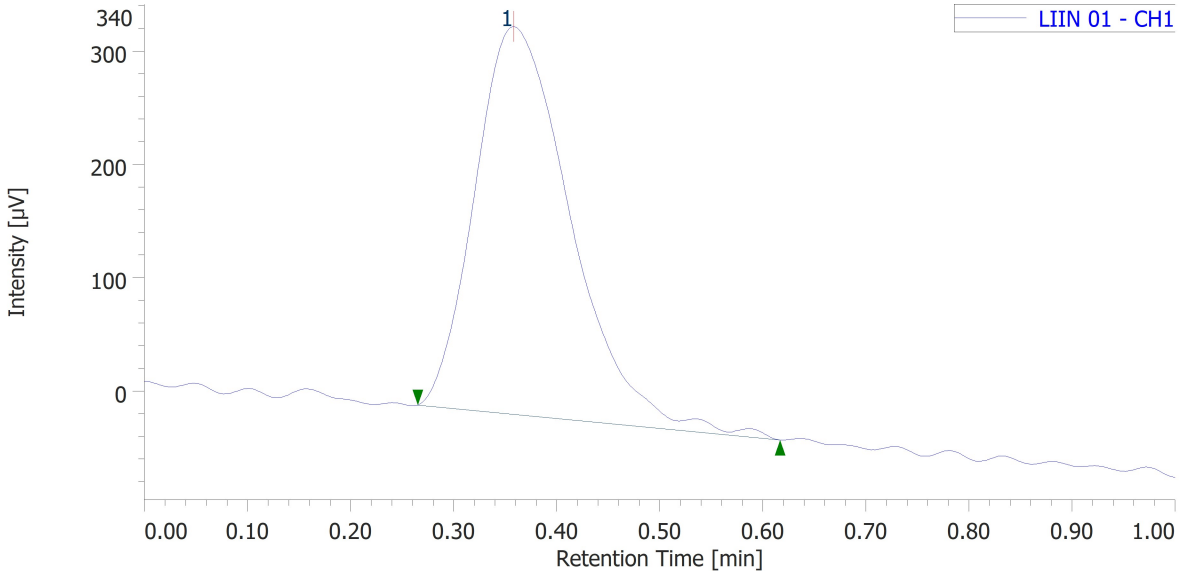


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:18:28 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:06:14 PM
Volume	0.1 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.358	24645	3800	100.000	100.000	N/A	74	N/A	1.380	

Chromatogram

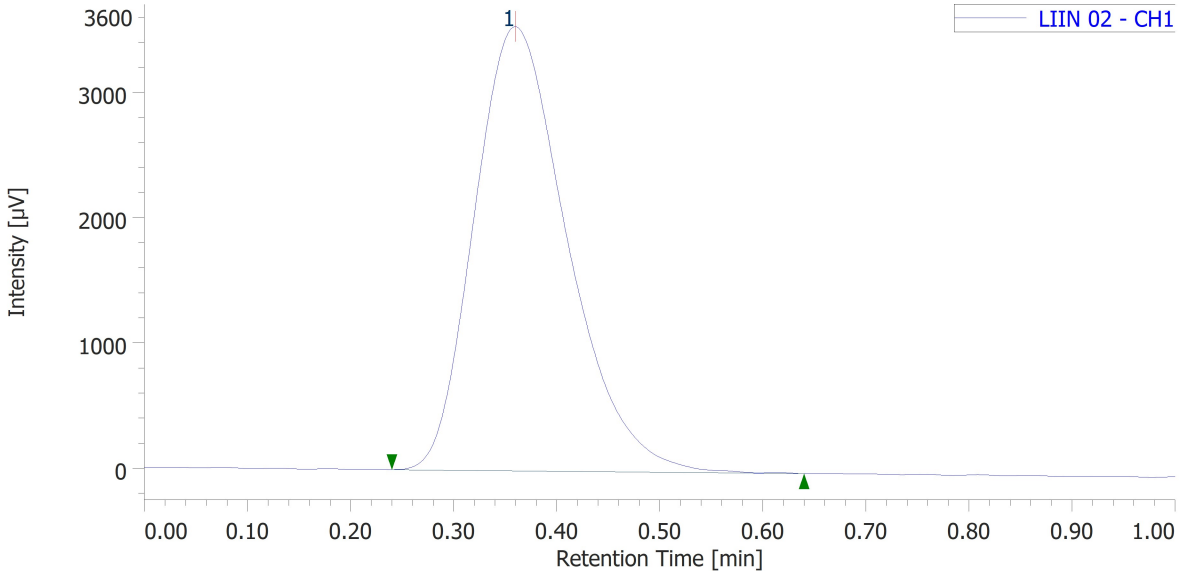


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:18:28 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:08:32 PM
Volume	1.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.360	247132	39363	100.000	100.000	N/A	77	N/A	1.285	

Chromatogram

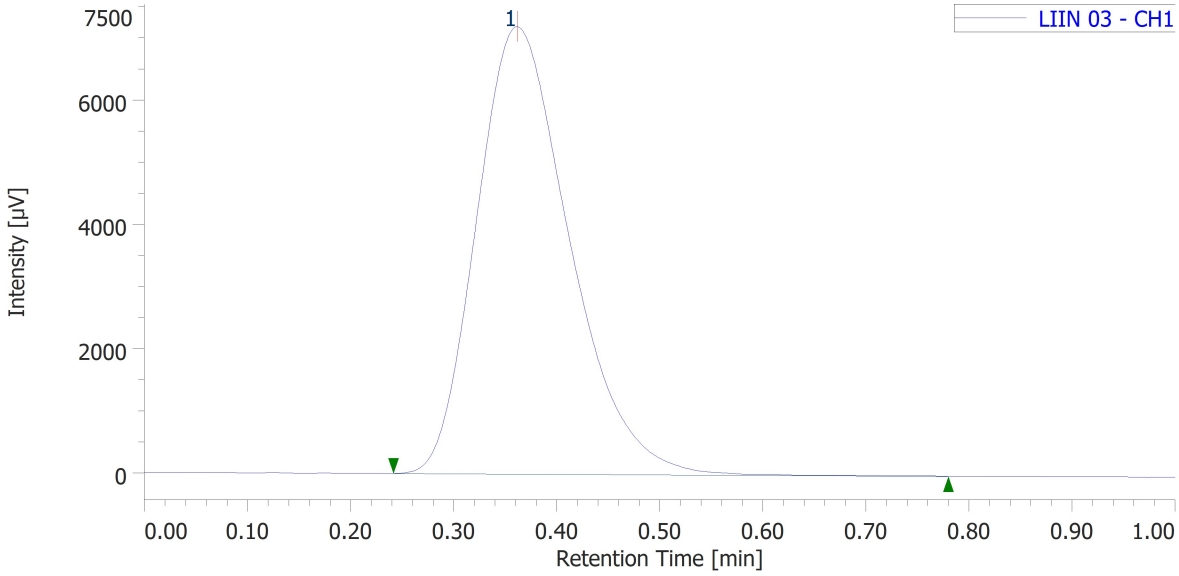


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:18:28 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:10:53 PM
Volume	2.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.362	501867	79931	100.000	100.000	N/A	78	N/A	1.291	

Chromatogram

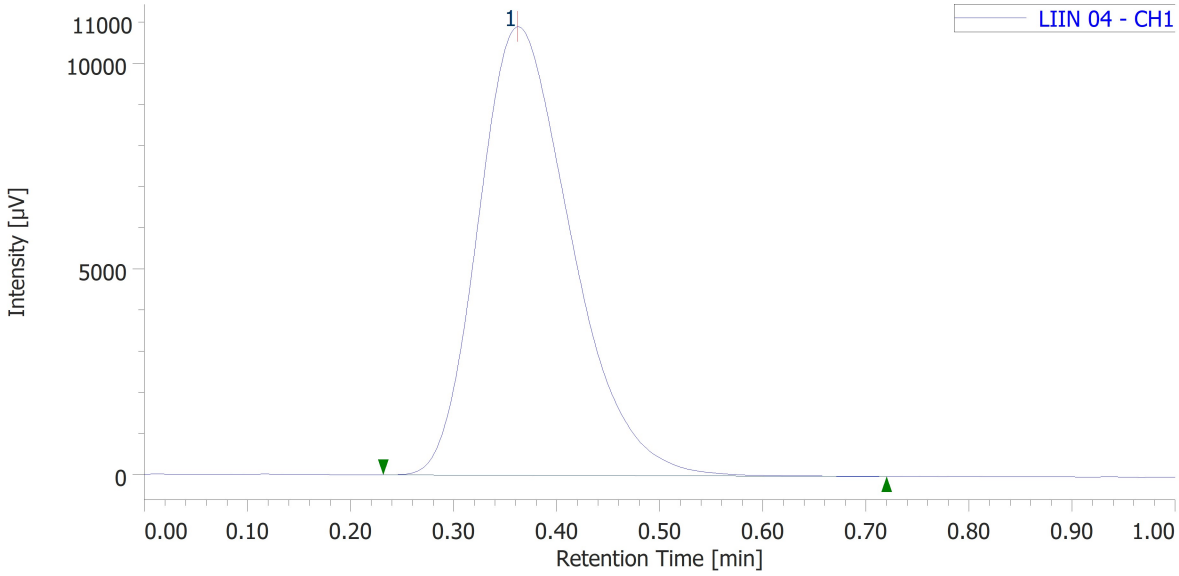


Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:18:29 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:13:13 PM
Volume	3.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.362	760438	121108	100.000	100.000	N/A	78	N/A	1.317	

Chromatogram

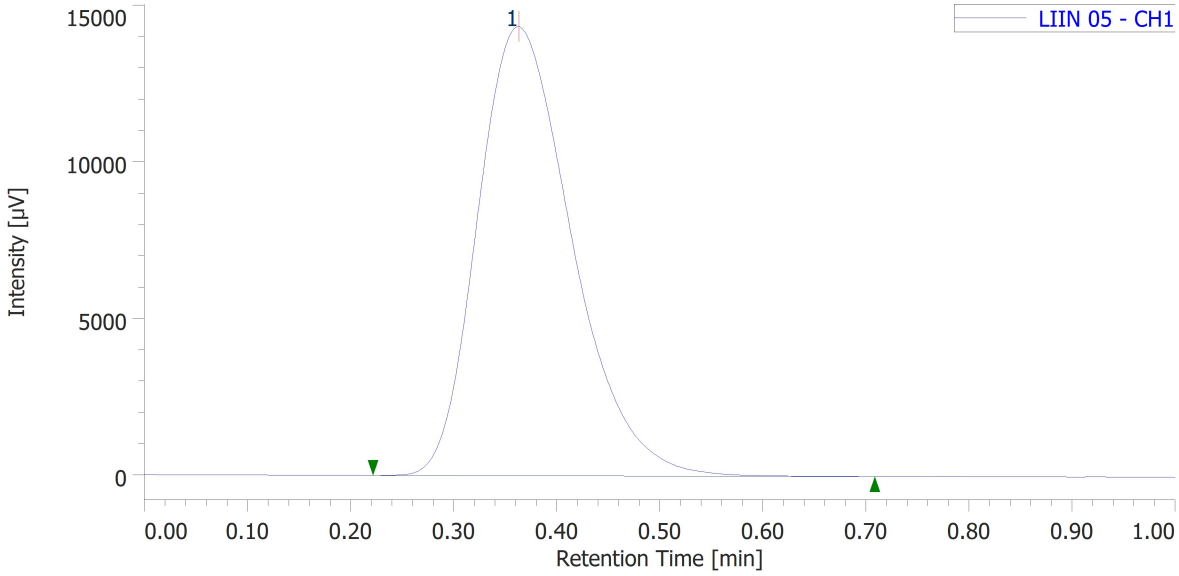

Chromatogram Information	
User Name	QPackSA
Date Modified	2/21/2025 1:18:29 PM
Description	
HPLC System Name	HPLC 01
Injection Date	2/21/2025 1:15:34 PM
Volume	4.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.363	1013605	159238	100.000	100.000	N/A	76	N/A	1.296	