
Peak Find - EDUV HPL37 2023.jws

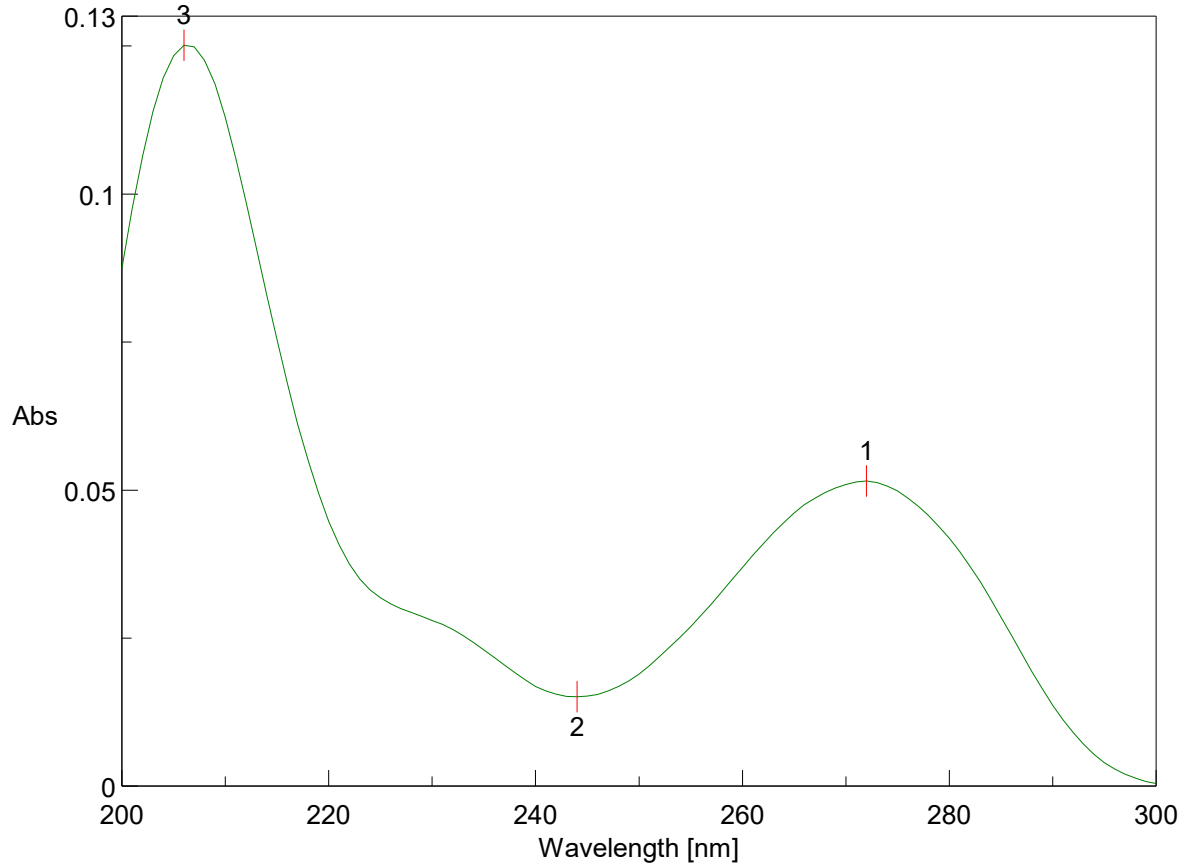

[Comments]

User	Administrator
Workgroup	Jasco
Division	
Company	Valer Laboratorios
Creation date	08/03/2023 14:20


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	300 nm	
Data interval	1 nm	
Data points	101	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.051526	2	244	0.015059
3	206	0.125107			

Creation	Administrator
Review	
Approval	

Chromatogram

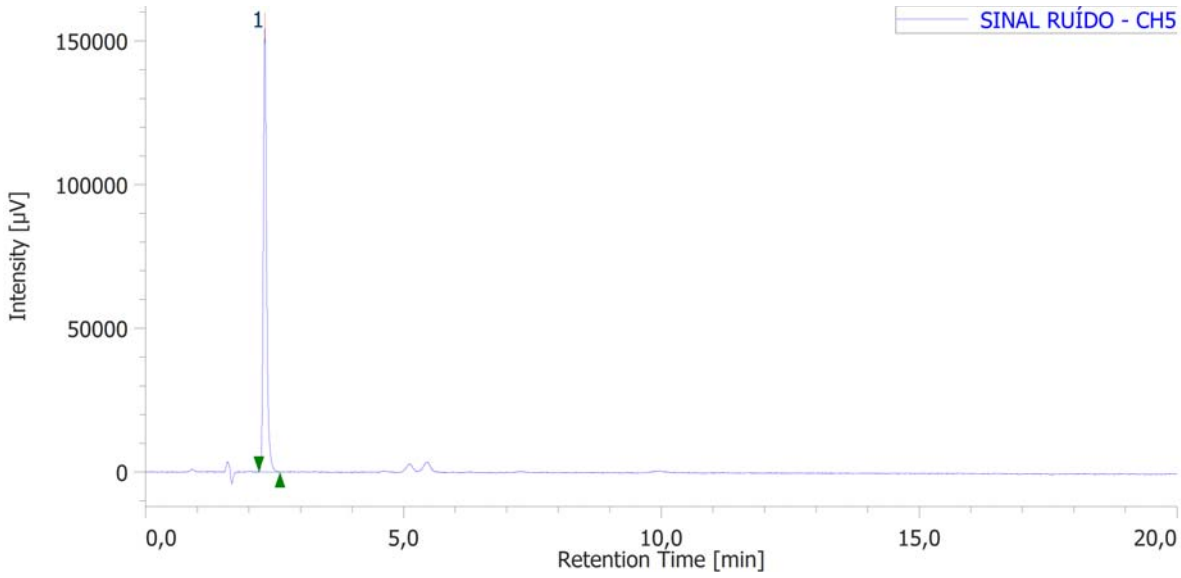

Chromatogram Information	
User Name	QPackSA
Date Modified	08/03/2023 15:59:44
Description	
HPLC System Name	HPL37
Injection Date	08/03/2023 15:39:42
Volume	20,0 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	SINAL RUÍDO_2023
Control Method	SINAL RUÍDO -2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	SINAL RUÍDO-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO 2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,308	692722	154312	100,000	100,000	N/A	6983	N/A	1,294	


Creator
Reviewer
Approver

Relatório SRELB

Detector DAD – X-LC 3110MD – N/S A002661329	Data: 07/03/2023
Ruído:	
Valor máximo: -0.340 mAU	**Diferença: 0.046 mAU**
Valor mínimo: -0.386 mAU	

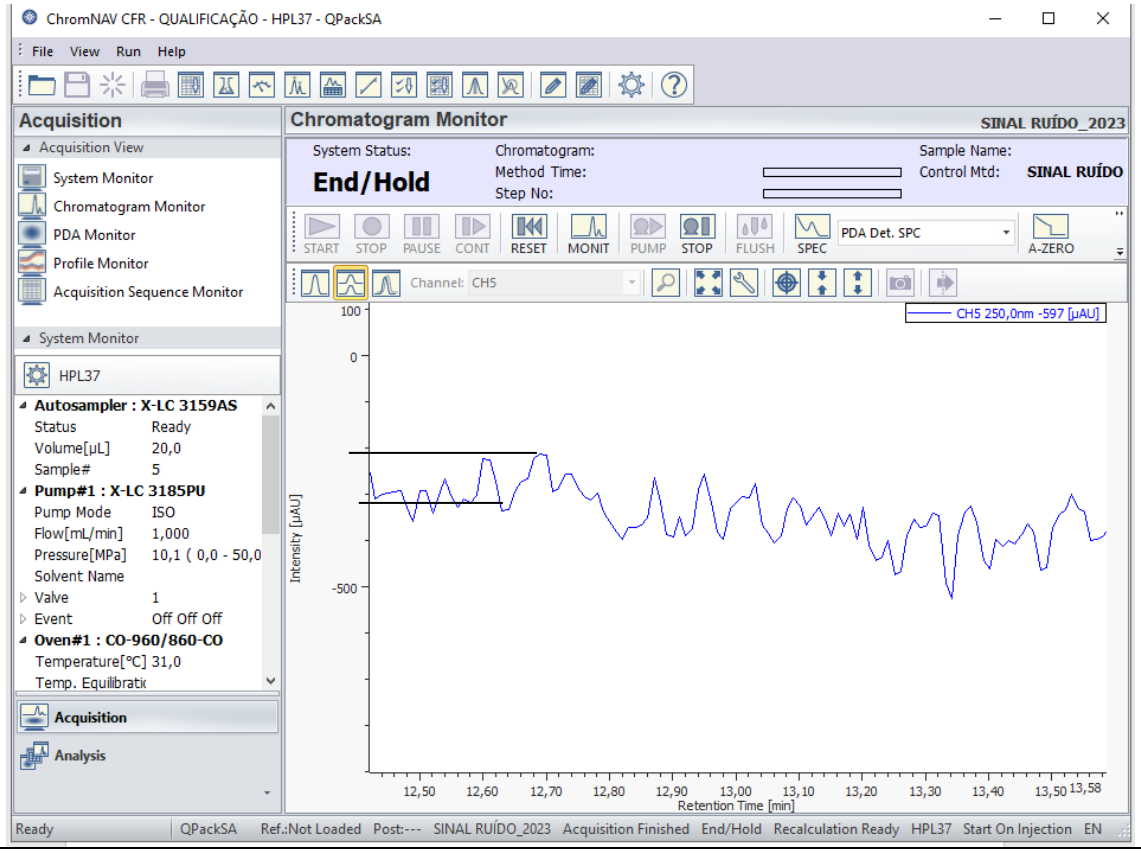


Estabilidade da Linha de Base:	
Valor máximo: -0.070 mAU	**Diferença (em 20 minutos): 0.742mAU**
Valor mínimo: -0.812 mAU	**Diferença (em 60 minutos): 0.742 x 3 = 2.226 mAU**

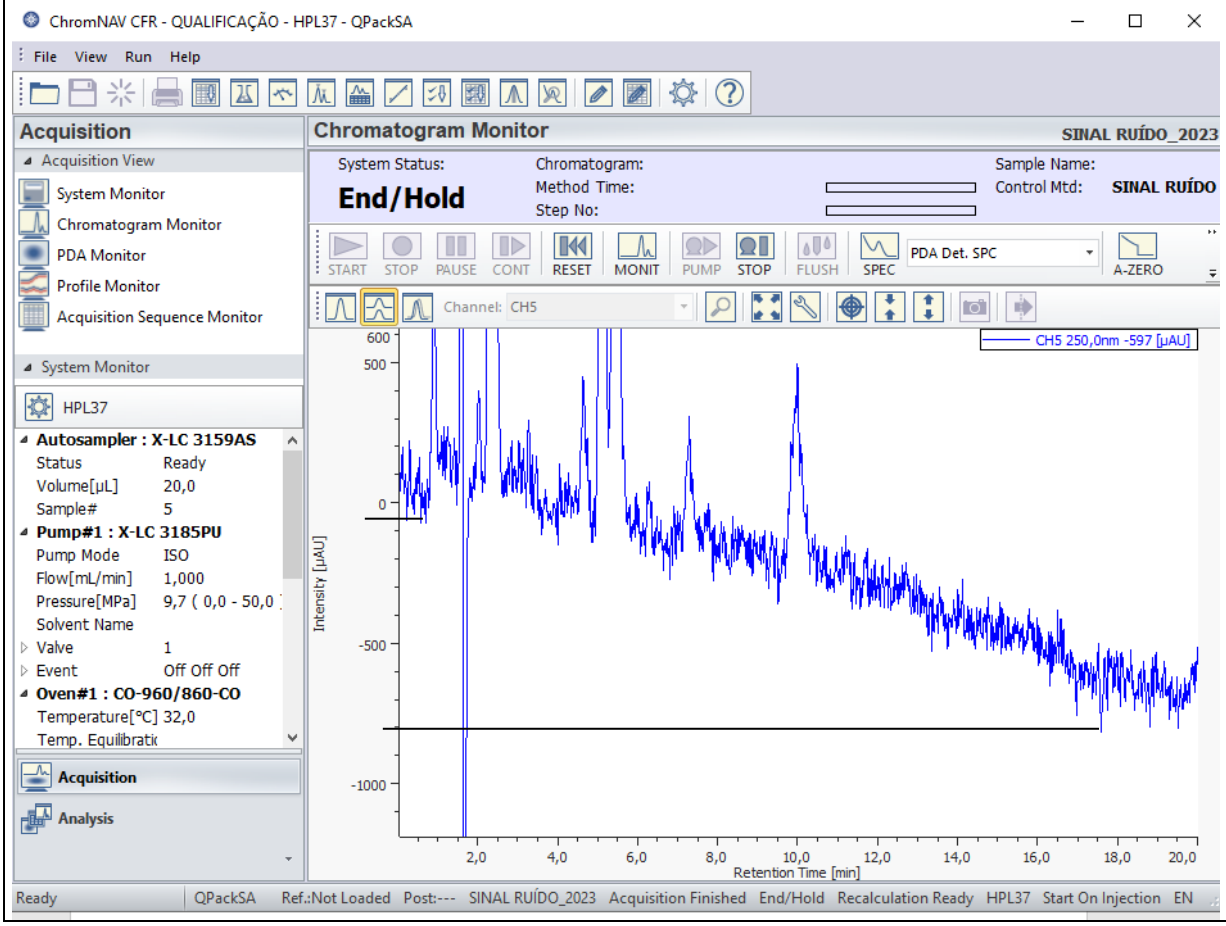


Altura do Pico:

Valor: 153.590 mAU

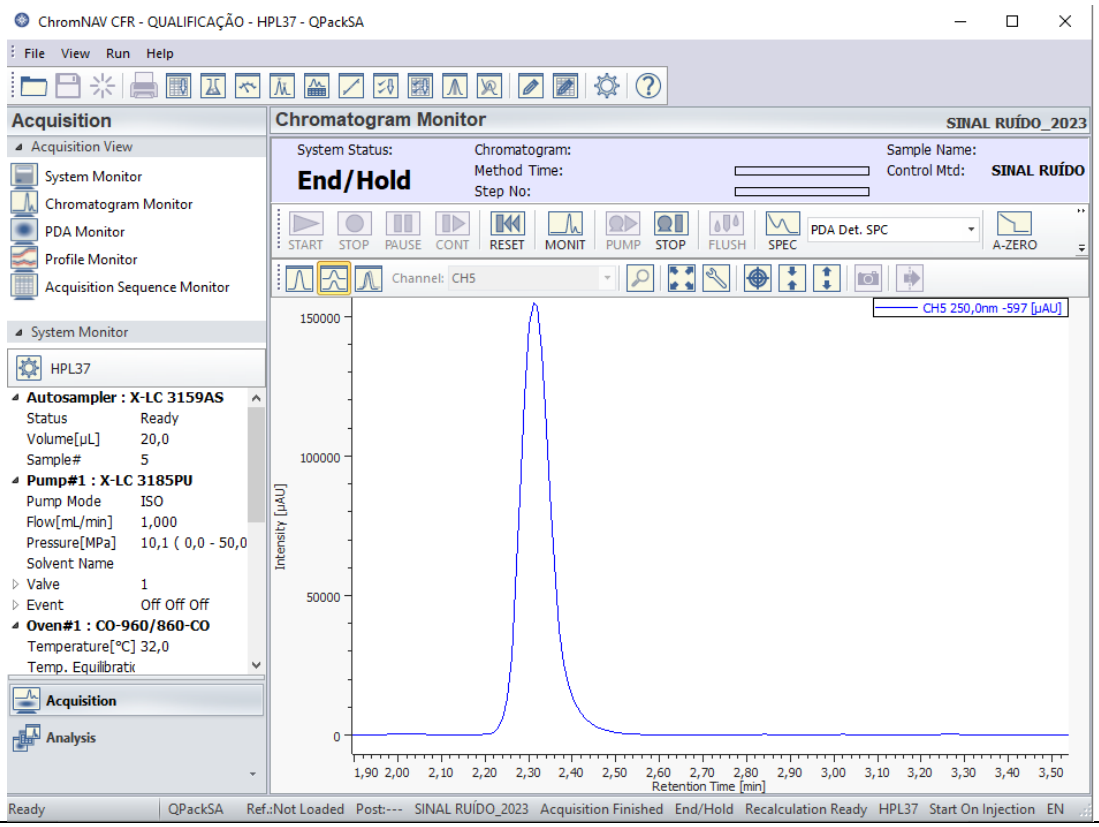

Chromatogram

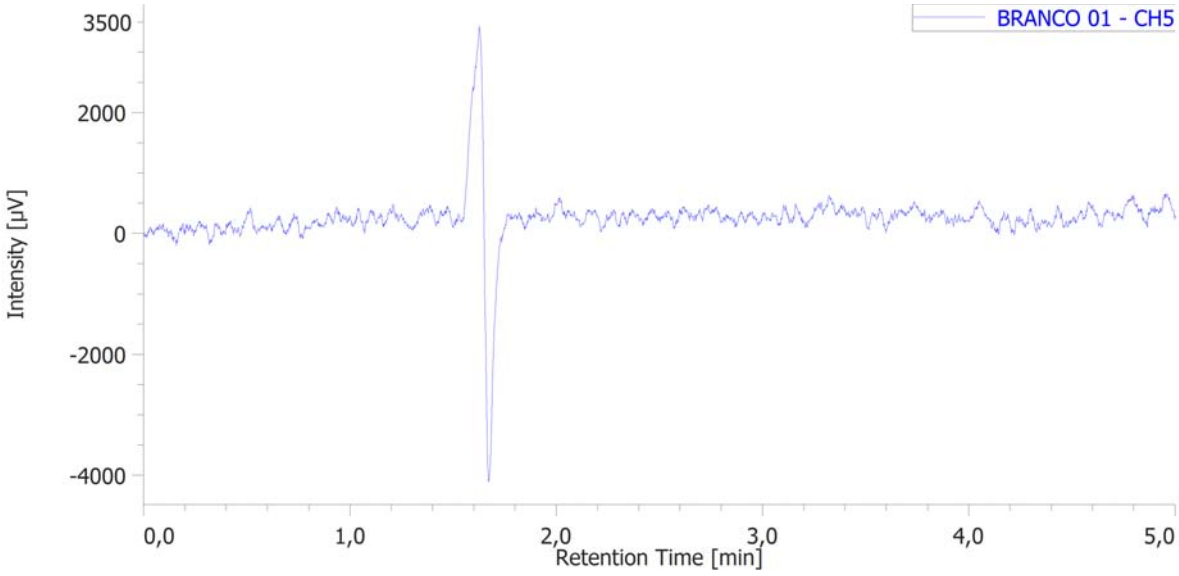


Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:19:21
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:14:18
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 01-CH5
Sample Name	BRANCO 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO 2023

Creator
Reviewer
Approver

Chromatogram

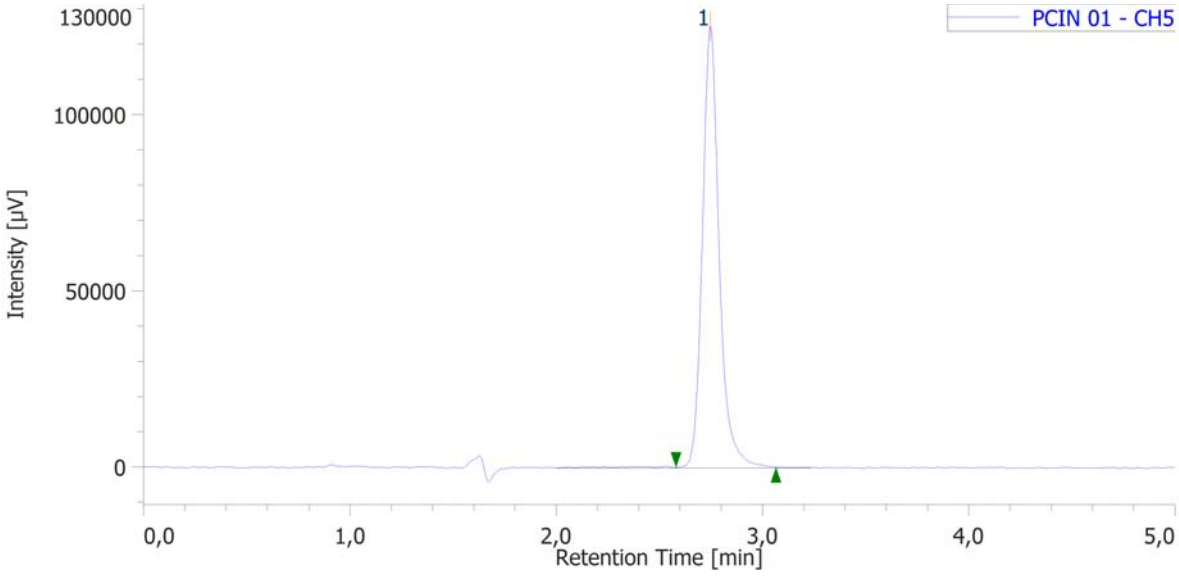

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:24:33
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:19:31
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	PCIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO 2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	710872	125281	100,000	100,000	N/A	6178	N/A	1,213	

Creator
Reviewer
Approver

Chromatogram

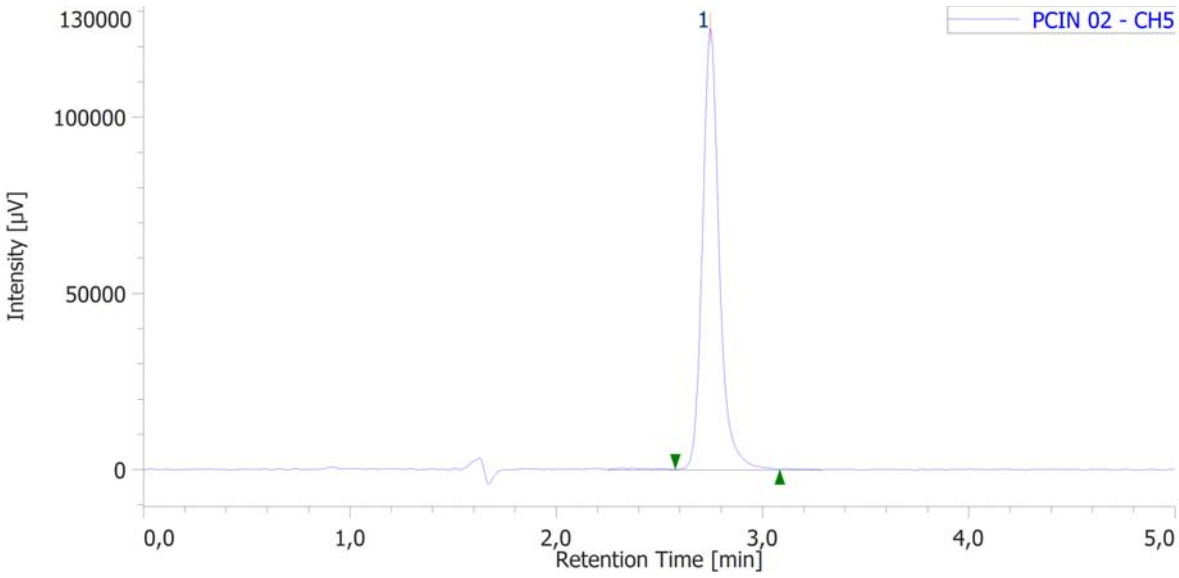

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:29:44
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:24:43
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	PCIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO-2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	711549	125263	100,000	100,000	N/A	6198	N/A	1,211	

Creator
Reviewer
Approver

Chromatogram

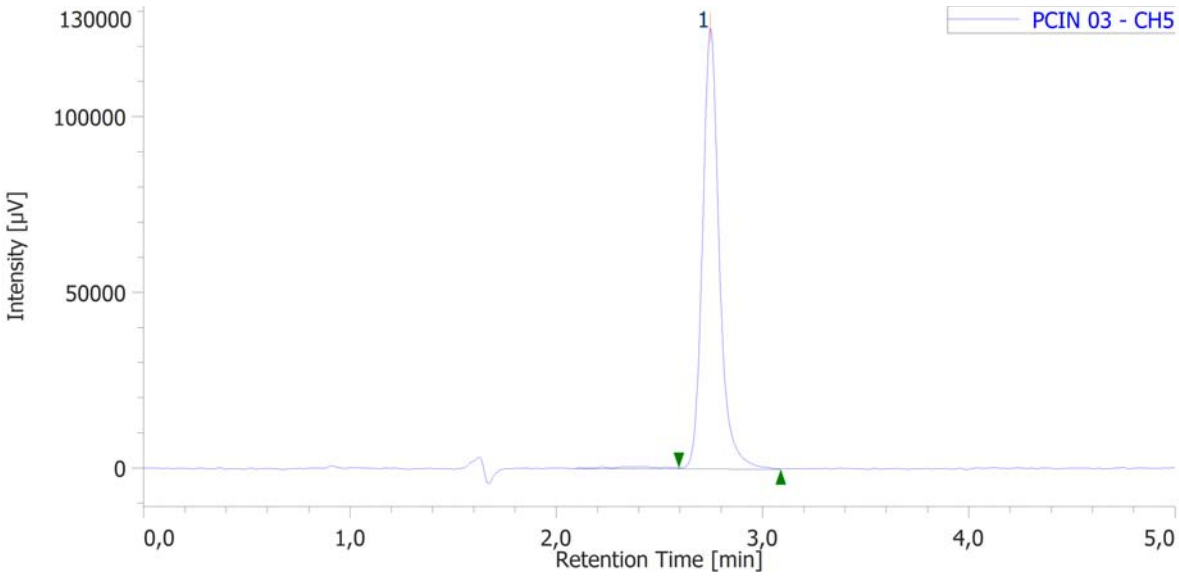

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:34:58
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:29:56
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	PCIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO-2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	710839	125390	100,000	100,000	N/A	6168	N/A	1,218	

Creator
Reviewer
Approver

Chromatogram

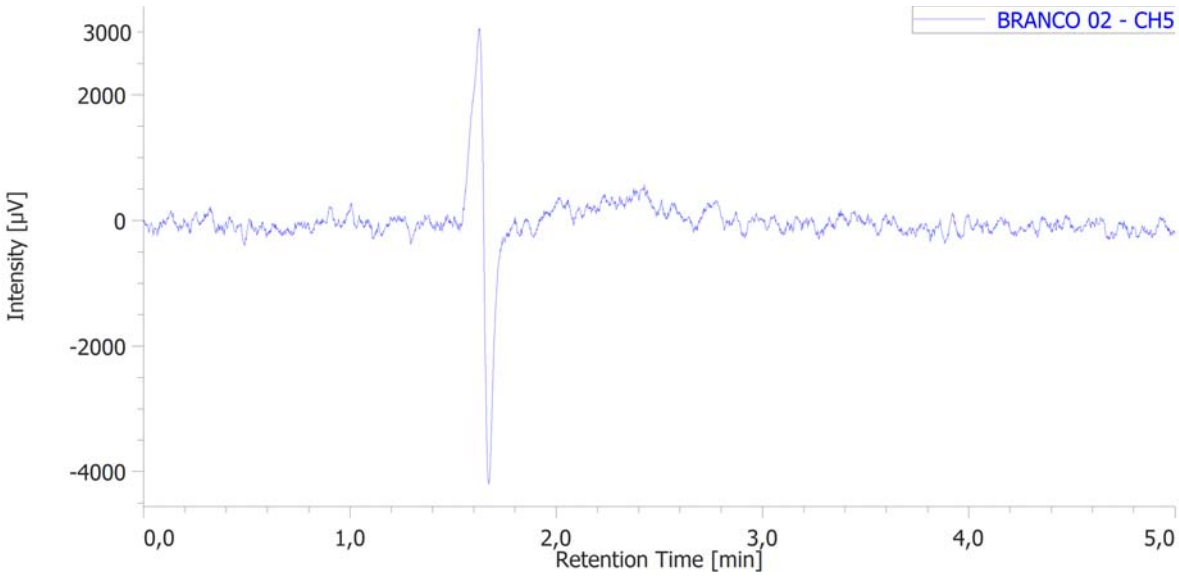


Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:40:10
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:35:08
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 02-CH5
Sample Name	BRANCO 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

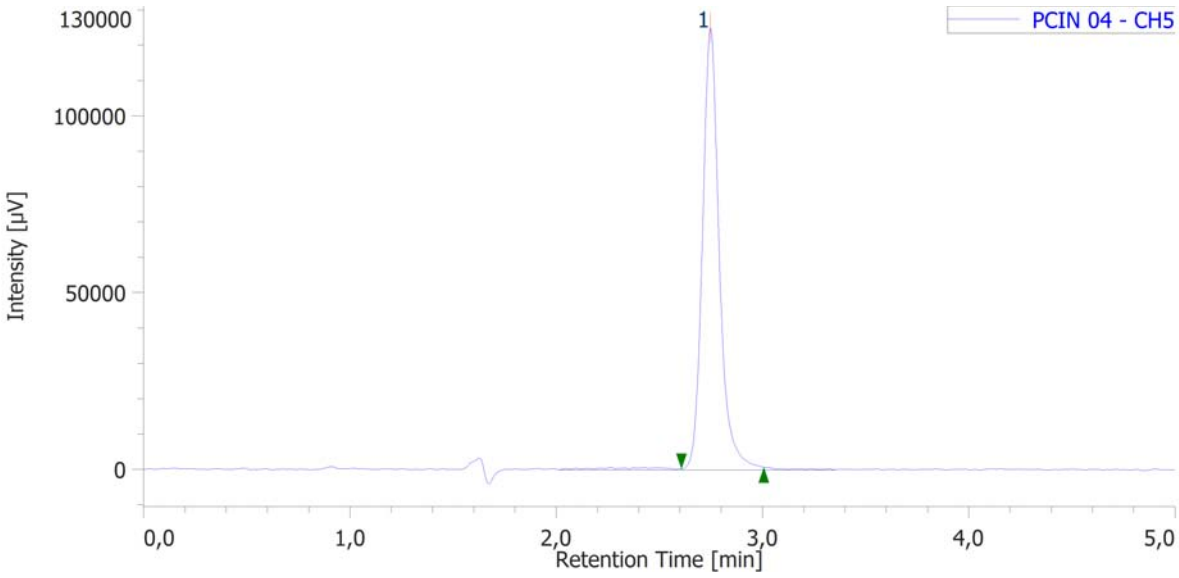

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:45:22
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:40:21
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	PCIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO 2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	710410	124846	100,000	100,000	N/A	6125	N/A	1,220	

Creator
Reviewer
Approver

Chromatogram

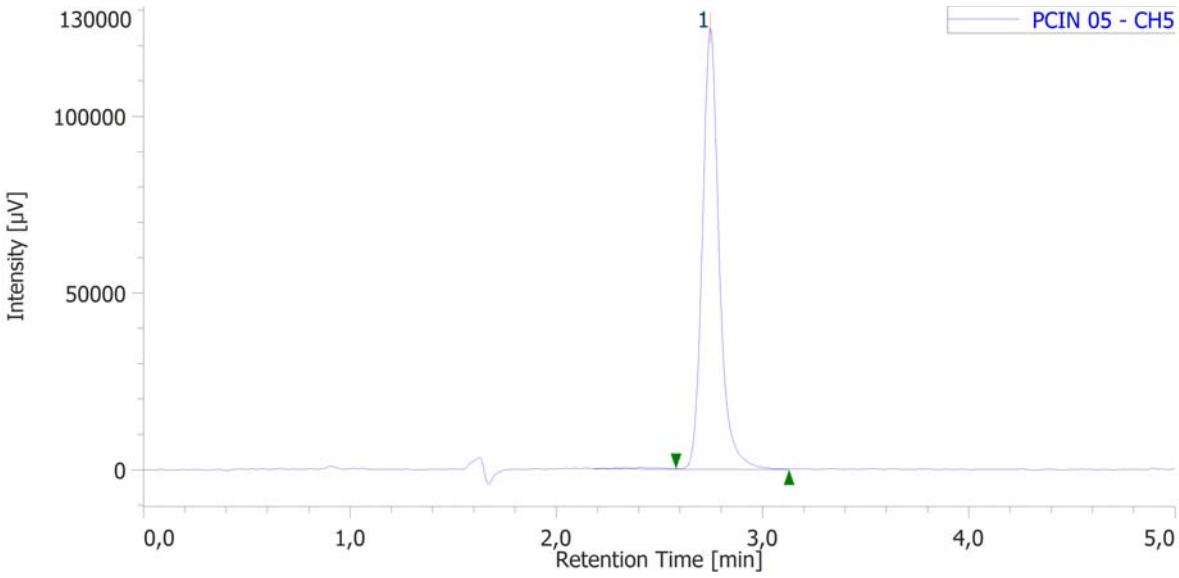

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:50:34
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:45:33
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	PCIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	707479	124720	100,000	100,000	N/A	6133	N/A	1,209	

Creator
Reviewer
Approver

Chromatogram

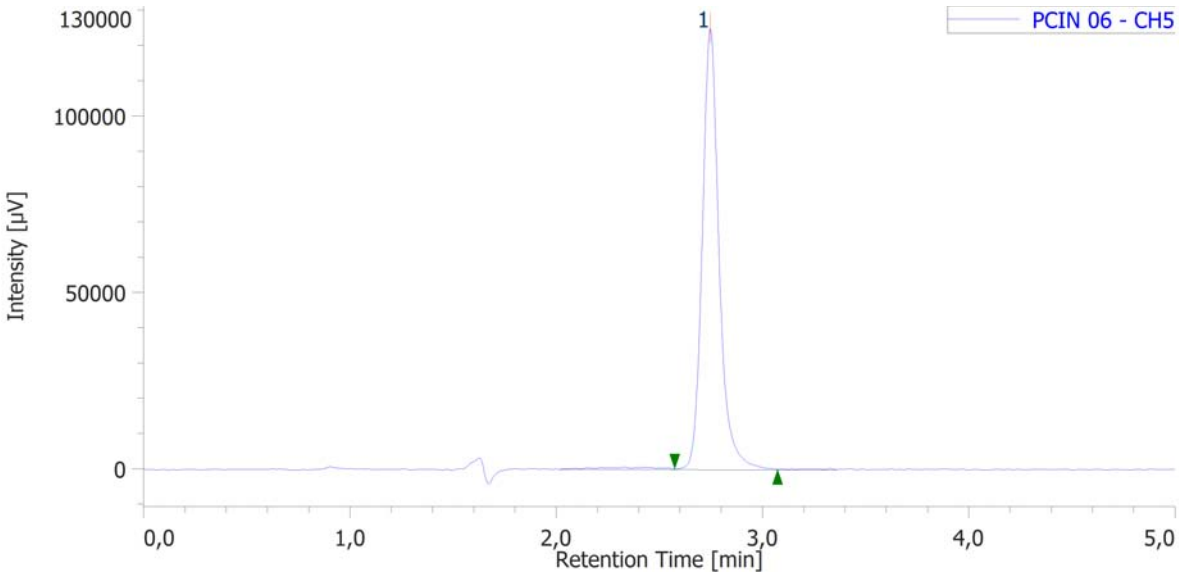

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 10:55:48
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:50:46
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	PCIN 06
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO_2023

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	711148	125037	100,000	100,000	N/A	6156	N/A	1,199	

Creator
Reviewer
Approver

Chromatogram

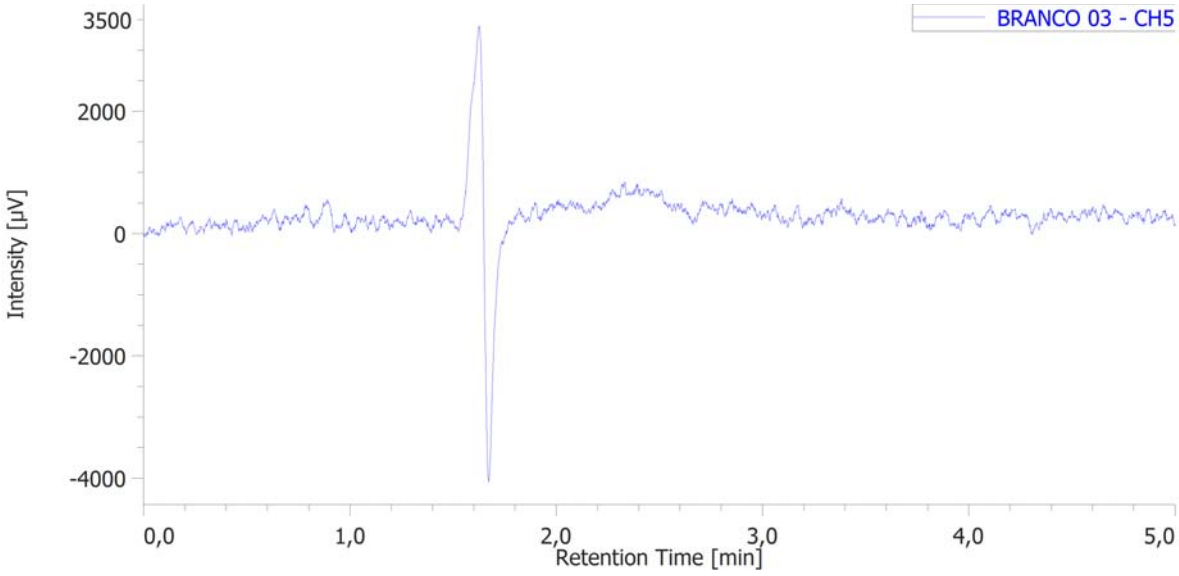


Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:01:00
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 10:55:58
Volume	10,0 [µL]
Sample #	11
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2023
Control Method	QUALIFICAÇÃO_2023
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 03-CH5
Sample Name	BRANCO 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

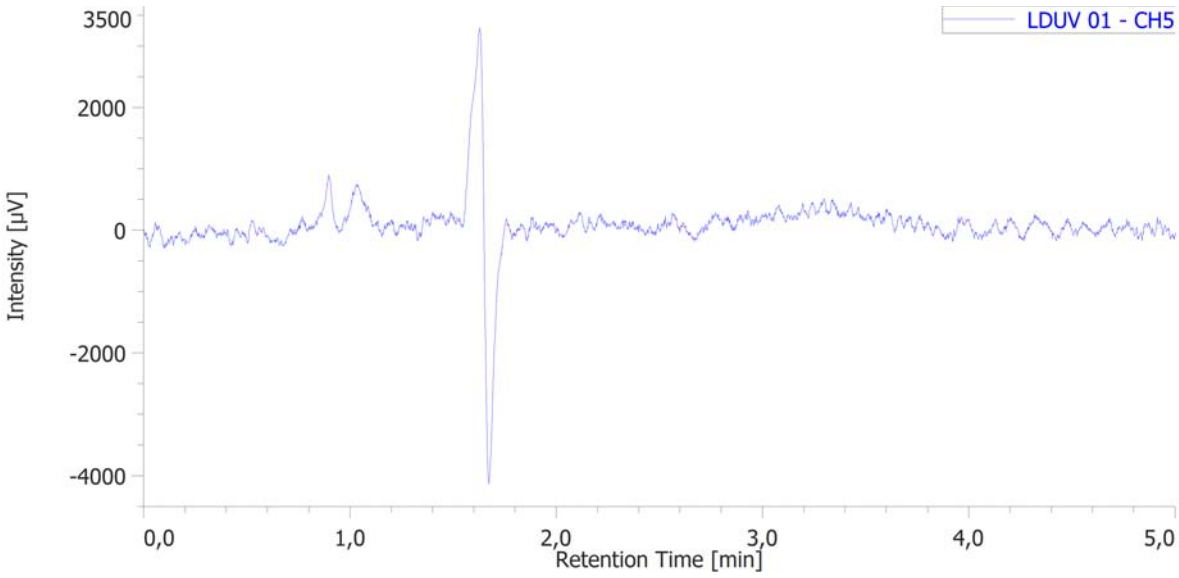


Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:17:00
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:11:58
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LDUV_2023
Control Method	QUALIFICAÇÃO - 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	LDUV 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO_2023

Creator
Reviewer
Approver

Chromatogram

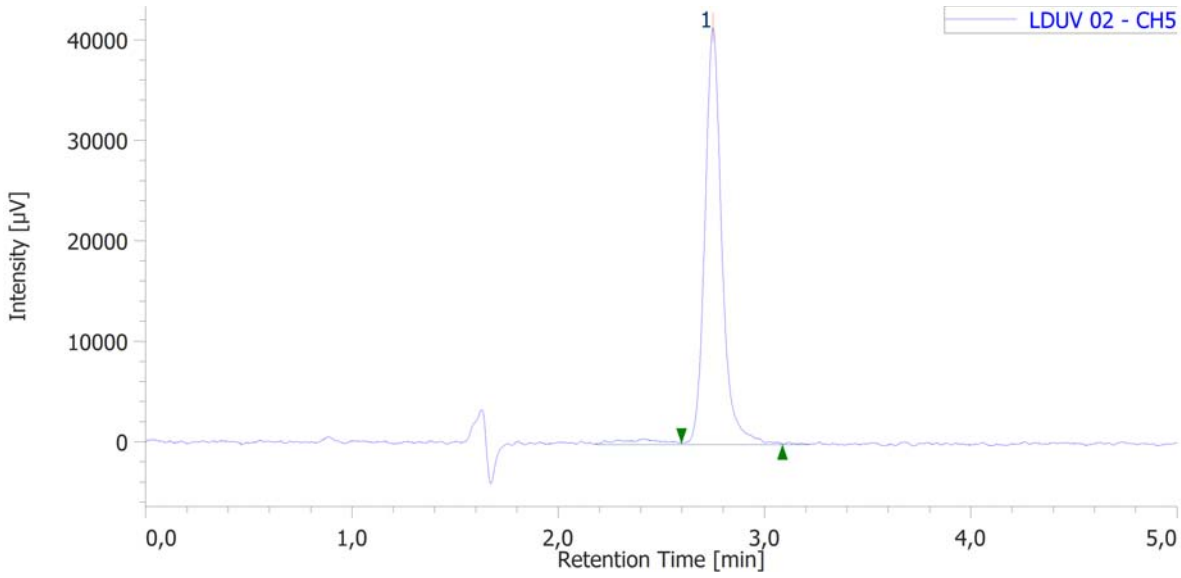

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:22:12
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:17:11
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LDUV_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	LDUV 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,750	237720	41408	100,000	100,000	N/A	6066	N/A	1,181	

Creator
Reviewer
Approver

Chromatogram

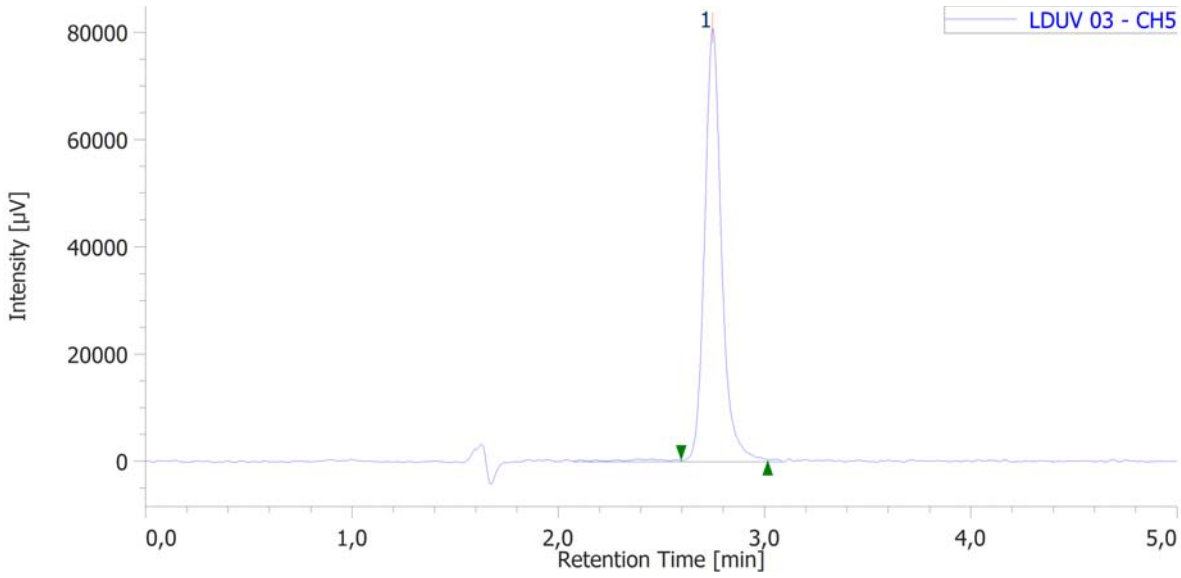

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:27:26
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:22:23
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LDUV_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	LDUV 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,748	462655	80836	100,000	100,000	N/A	6062	N/A	1,198	

Creator
Reviewer
Approver

Chromatogram

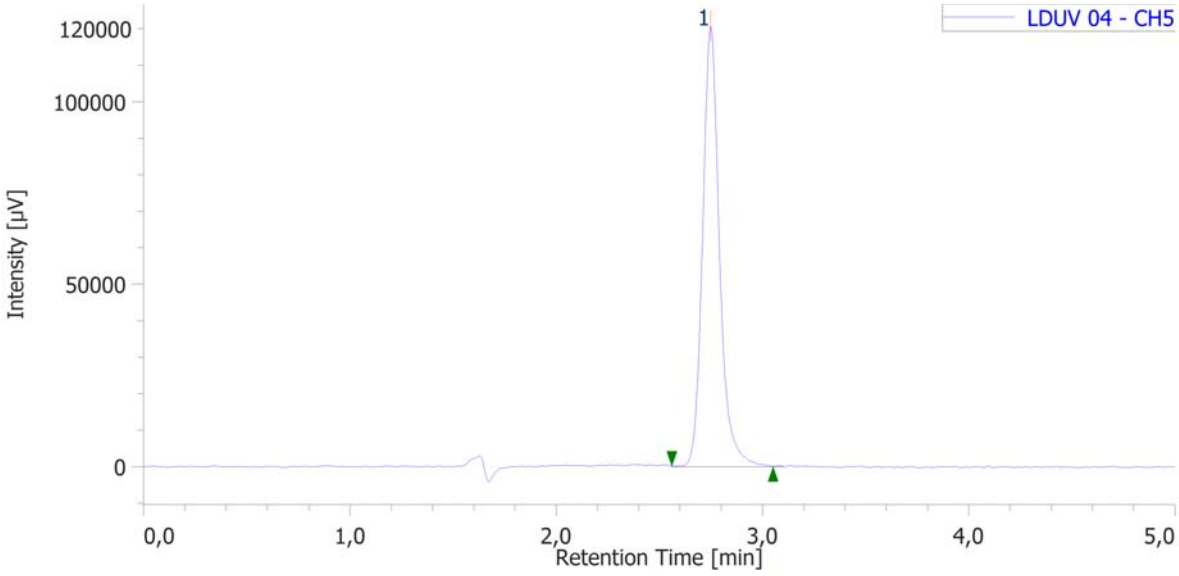

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:32:38
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:27:36
Volume	10,0 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LDUV_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04–CH5
Sample Name	LDUV 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,748	686576	120595	100,000	100,000	N/A	6072	N/A	1,199	

Creator
Reviewer
Approver

Chromatogram

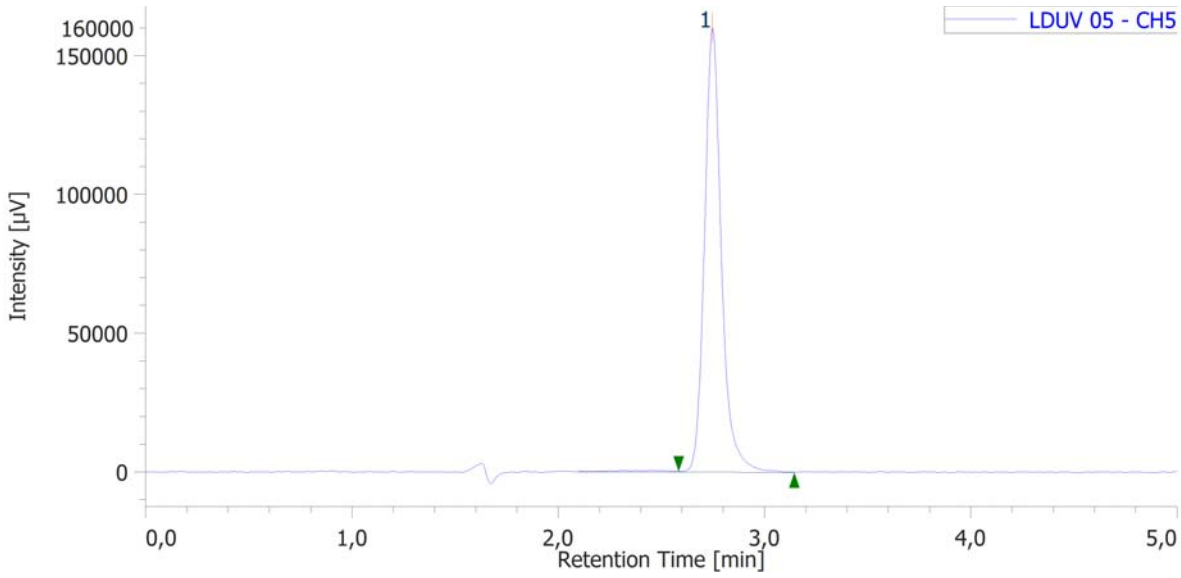

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:37:50
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:32:48
Volume	10,0 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LDUV_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	LDUV 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,747	914542	159868	100,000	100,000	N/A	6042	N/A	1,220	

Creator
Reviewer
Approver

Chromatogram

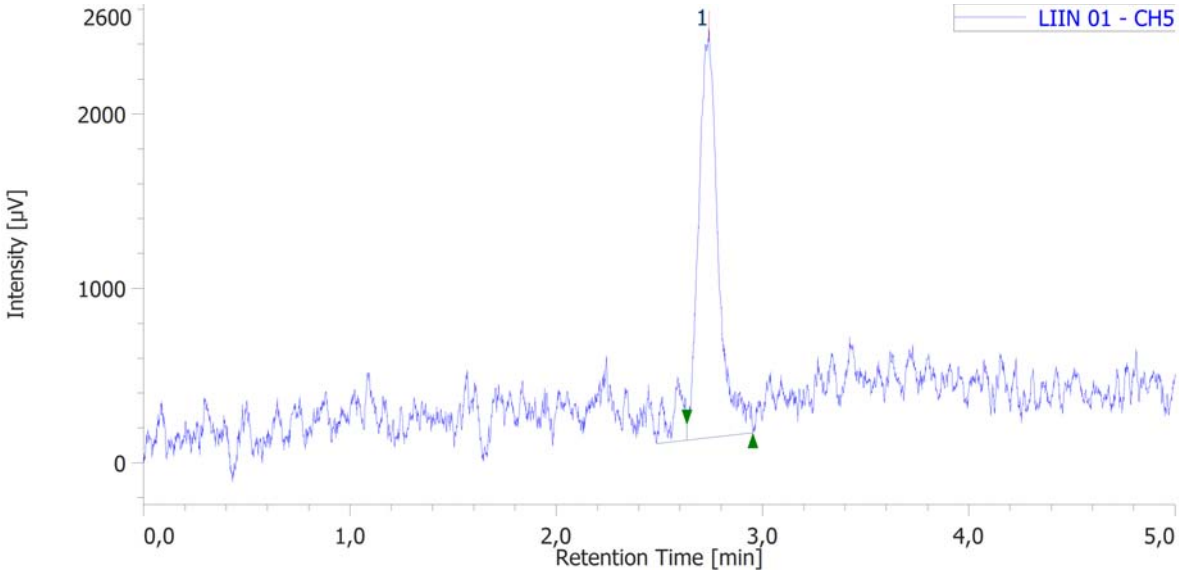

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:52:52
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:47:49
Volume	0,1 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LIIN_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	LIIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,740	15400	2357	100,000	100,000	N/A	4818	N/A	1,479	

Creator
Reviewer
Approver

Chromatogram

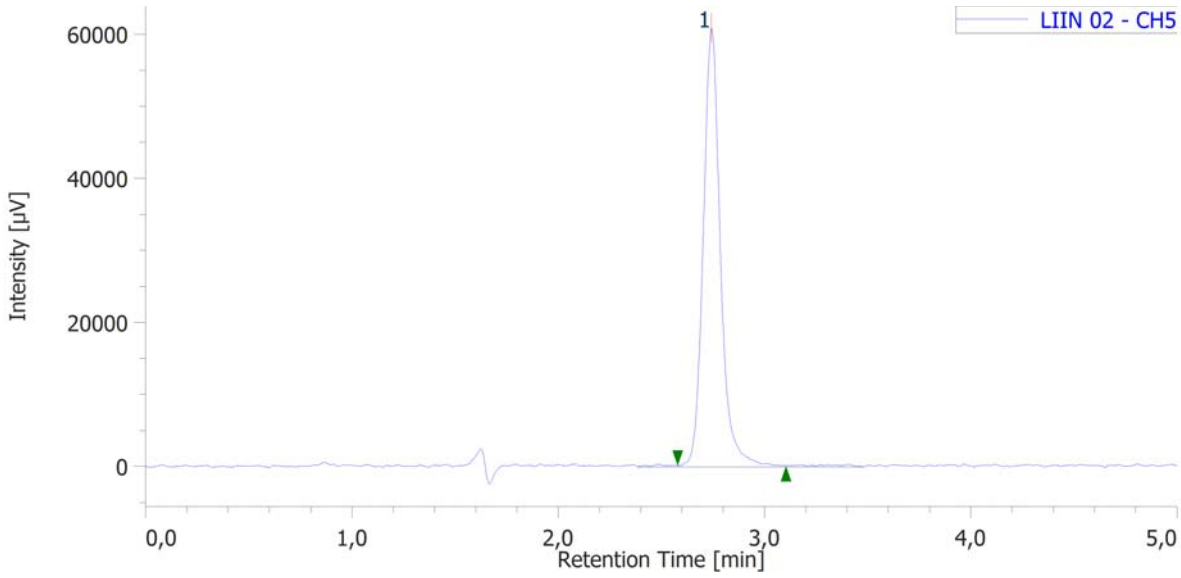

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 11:58:04
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:53:01
Volume	5,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LIIN_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	LIIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,742	354734	60881	100,000	100,000	N/A	5848	N/A	1,189	

Creator
Reviewer
Approver

Chromatogram

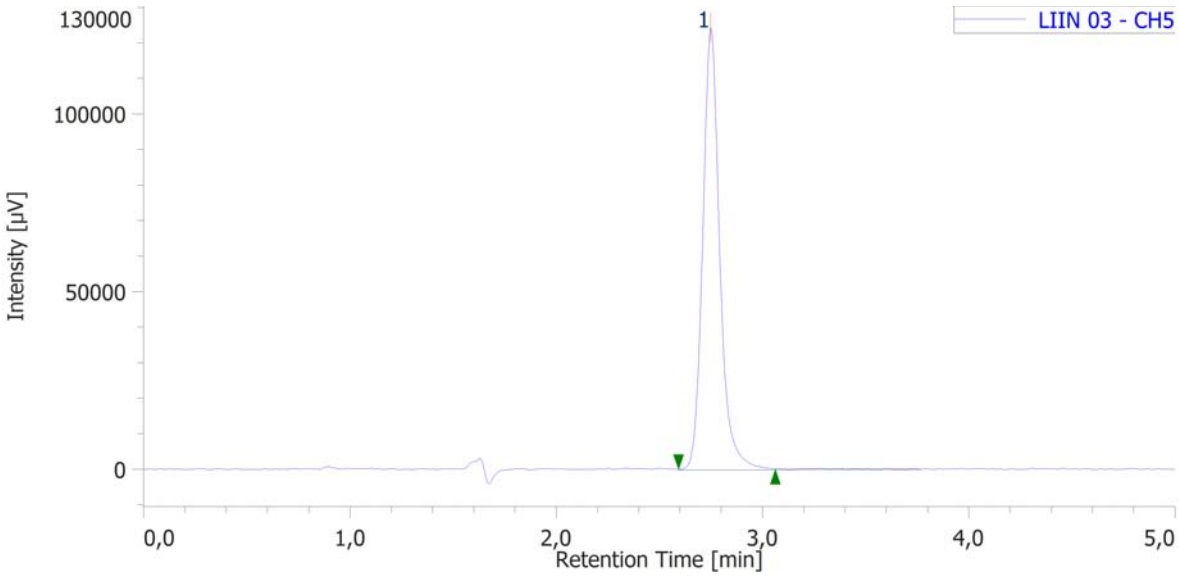

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 12:03:16
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 11:58:14
Volume	10,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LIIN_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	LIIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,748	713022	124166	100,000	100,000	N/A	5969	N/A	1,198	

Creator
Reviewer
Approver

Chromatogram

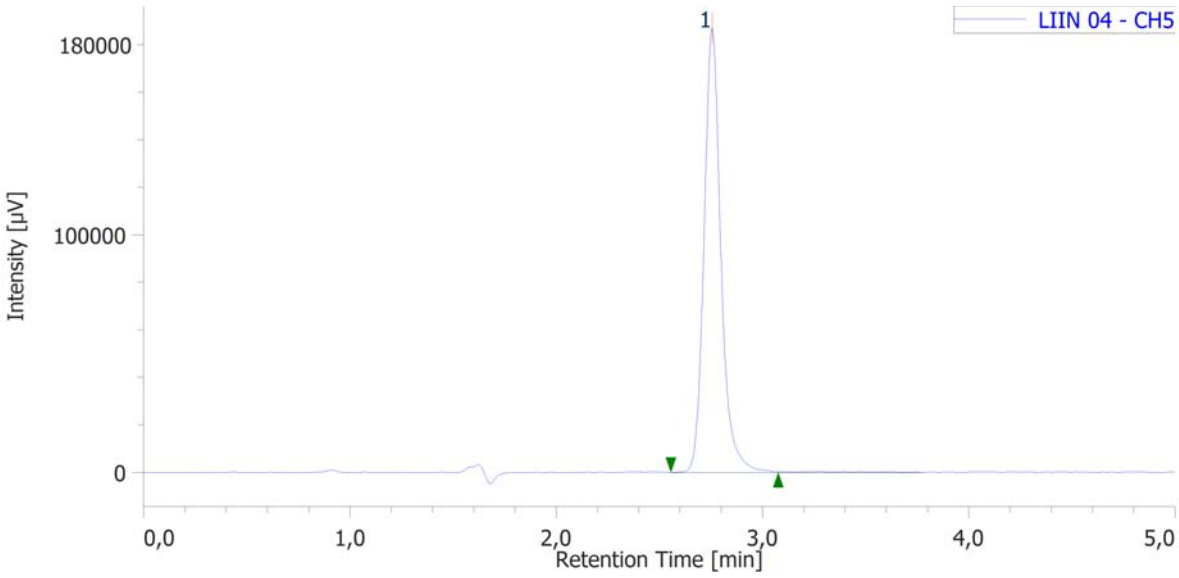

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 12:08:28
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 12:03:26
Volume	15,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LIIN_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	LIIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,755	1067584	186996	100,000	100,000	N/A	6098	N/A	1,197	

Creator
Reviewer
Approver

Chromatogram

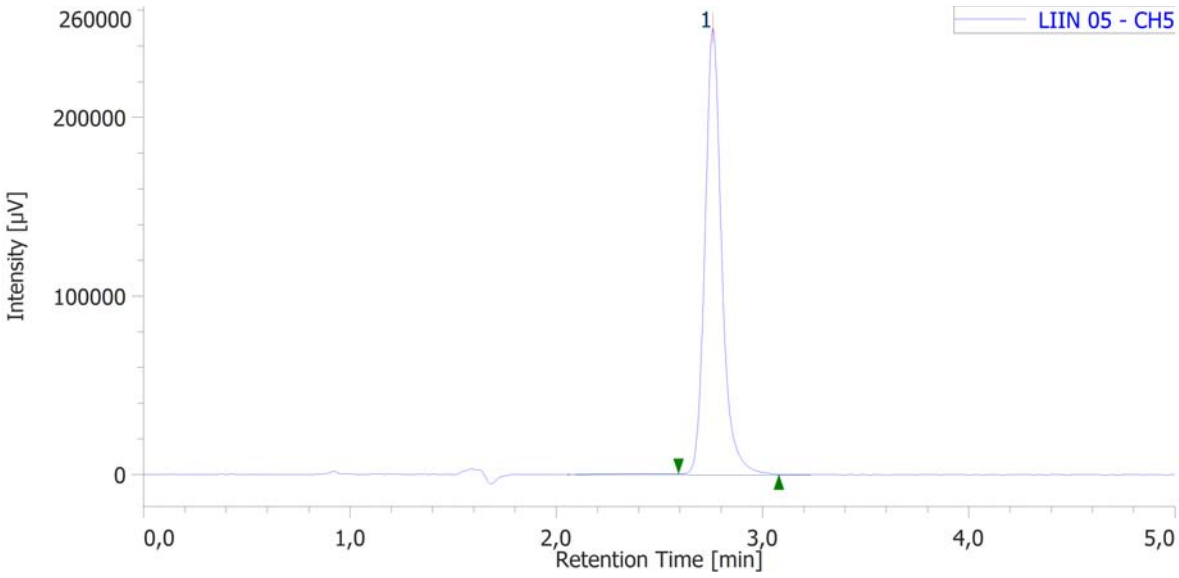

Chromatogram Information	
User Name	QPackSA
Date Modified	09/03/2023 12:13:42
Description	
HPLC System Name	HPL37
Injection Date	09/03/2023 12:08:39
Volume	20,0 [µL]
Sample #	12
Project Name	QUALIFICAÇÃO
Acquisition Time	5,0 [min]
Acquisition Sequence	LIIN_2023
Control Method	QUALIFICAÇÃO – 2023
Peak ID Table	Qualificação 2023
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	LIIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	QUALIFICAÇÃO

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,758	1414985	250001	100,000	100,000	N/A	6191	N/A	1,217	

Creator
Reviewer
Approver