

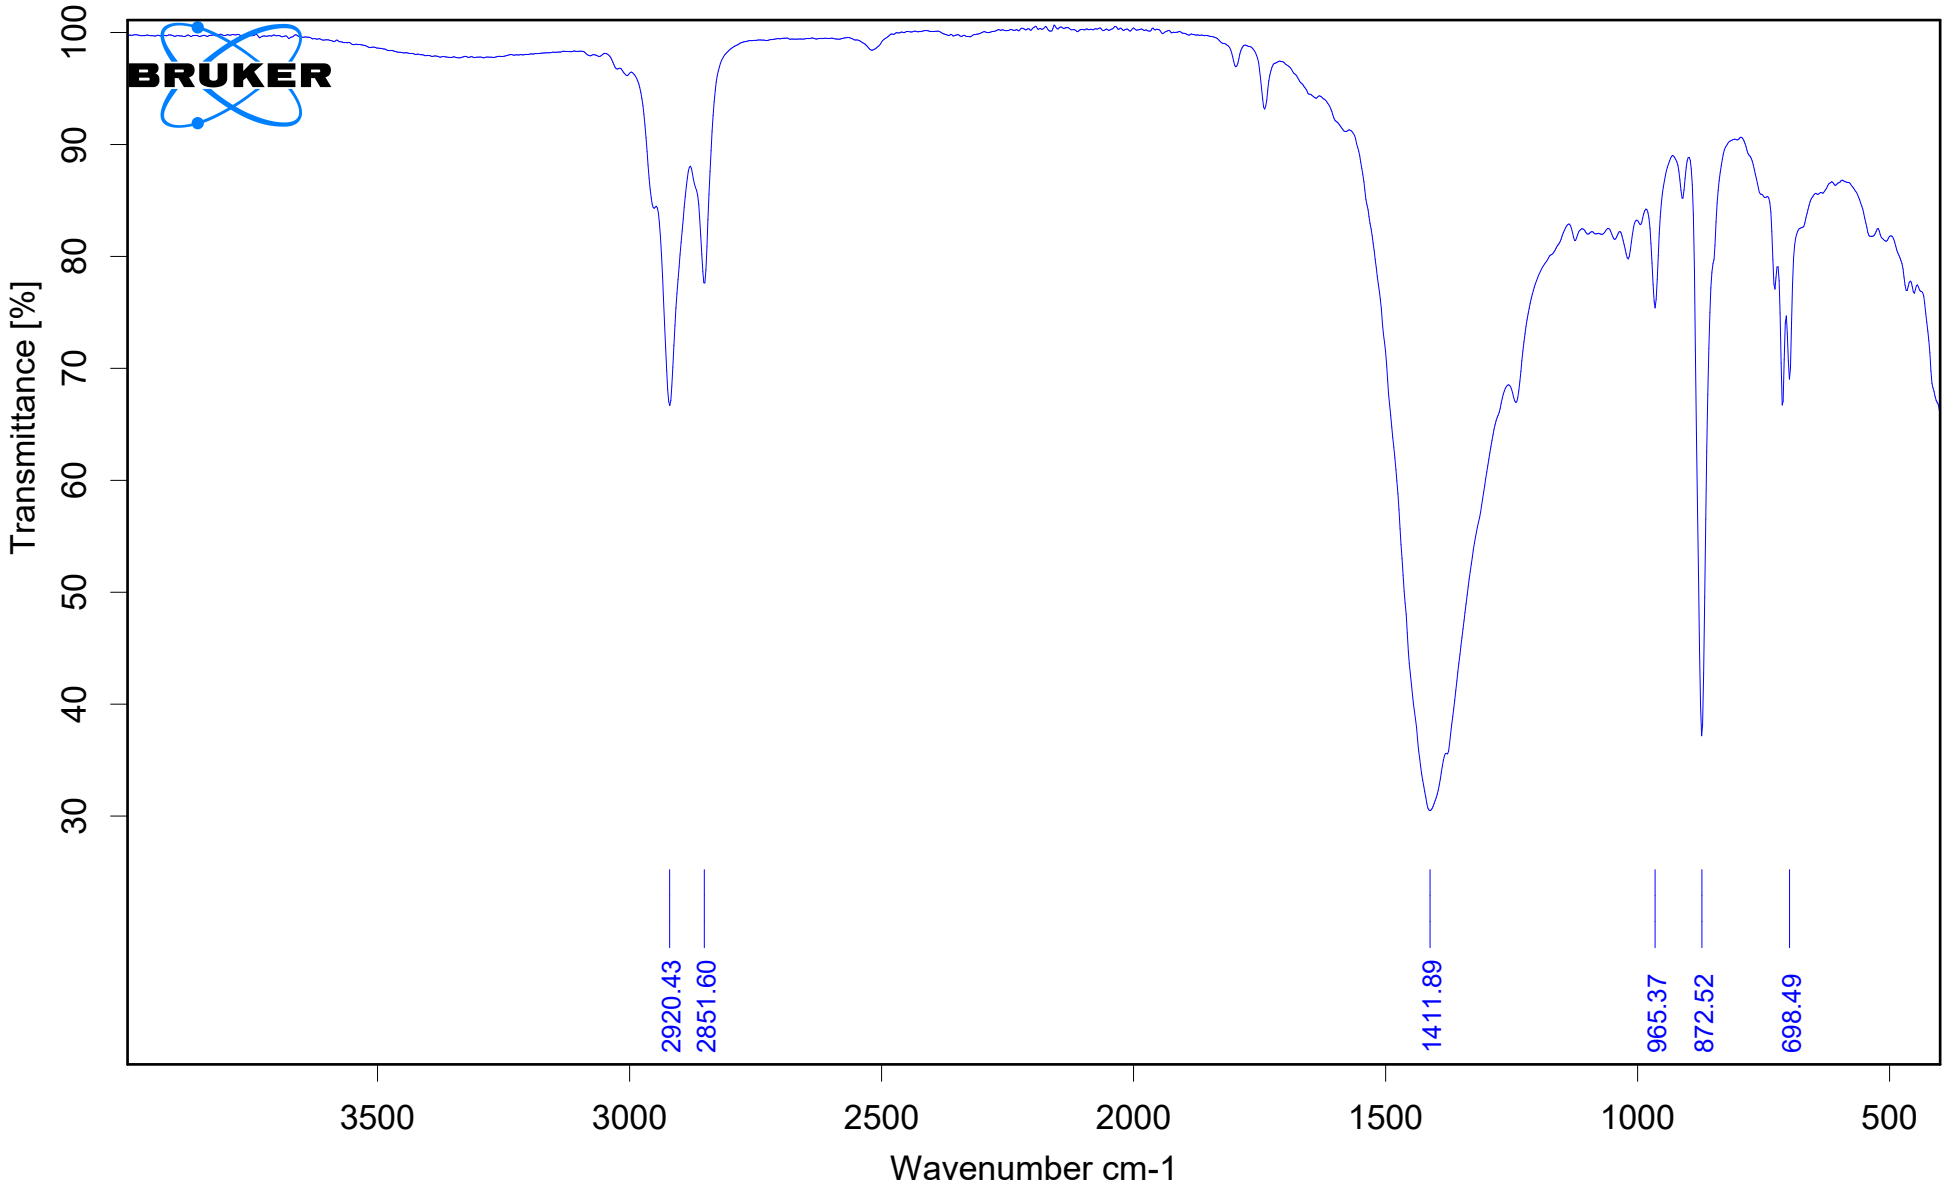



C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\.5	Instrument type and / or accessory	10/03/2026

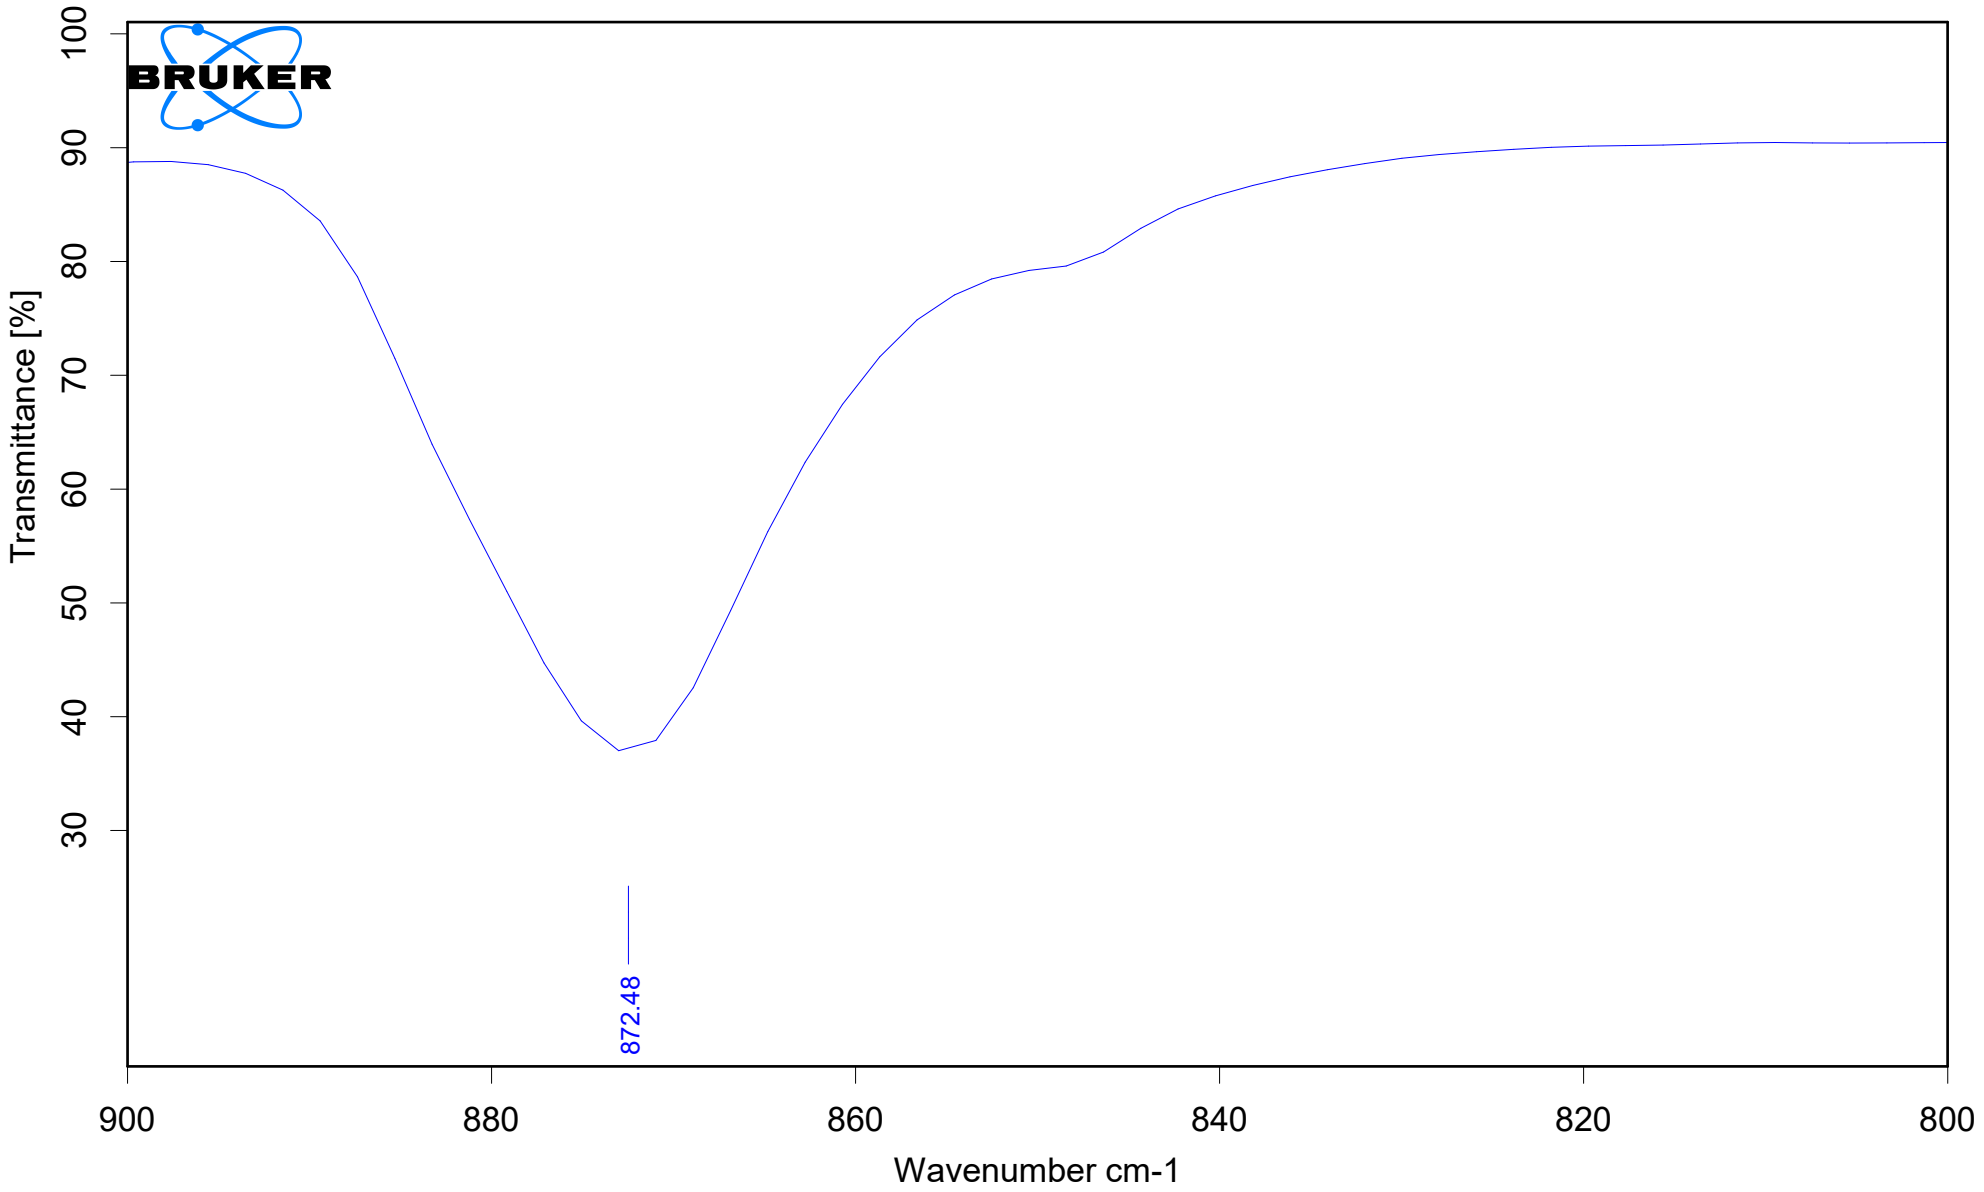


C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Resolução.0	Resolução	Instrument type and / or accessory	10/03/2026

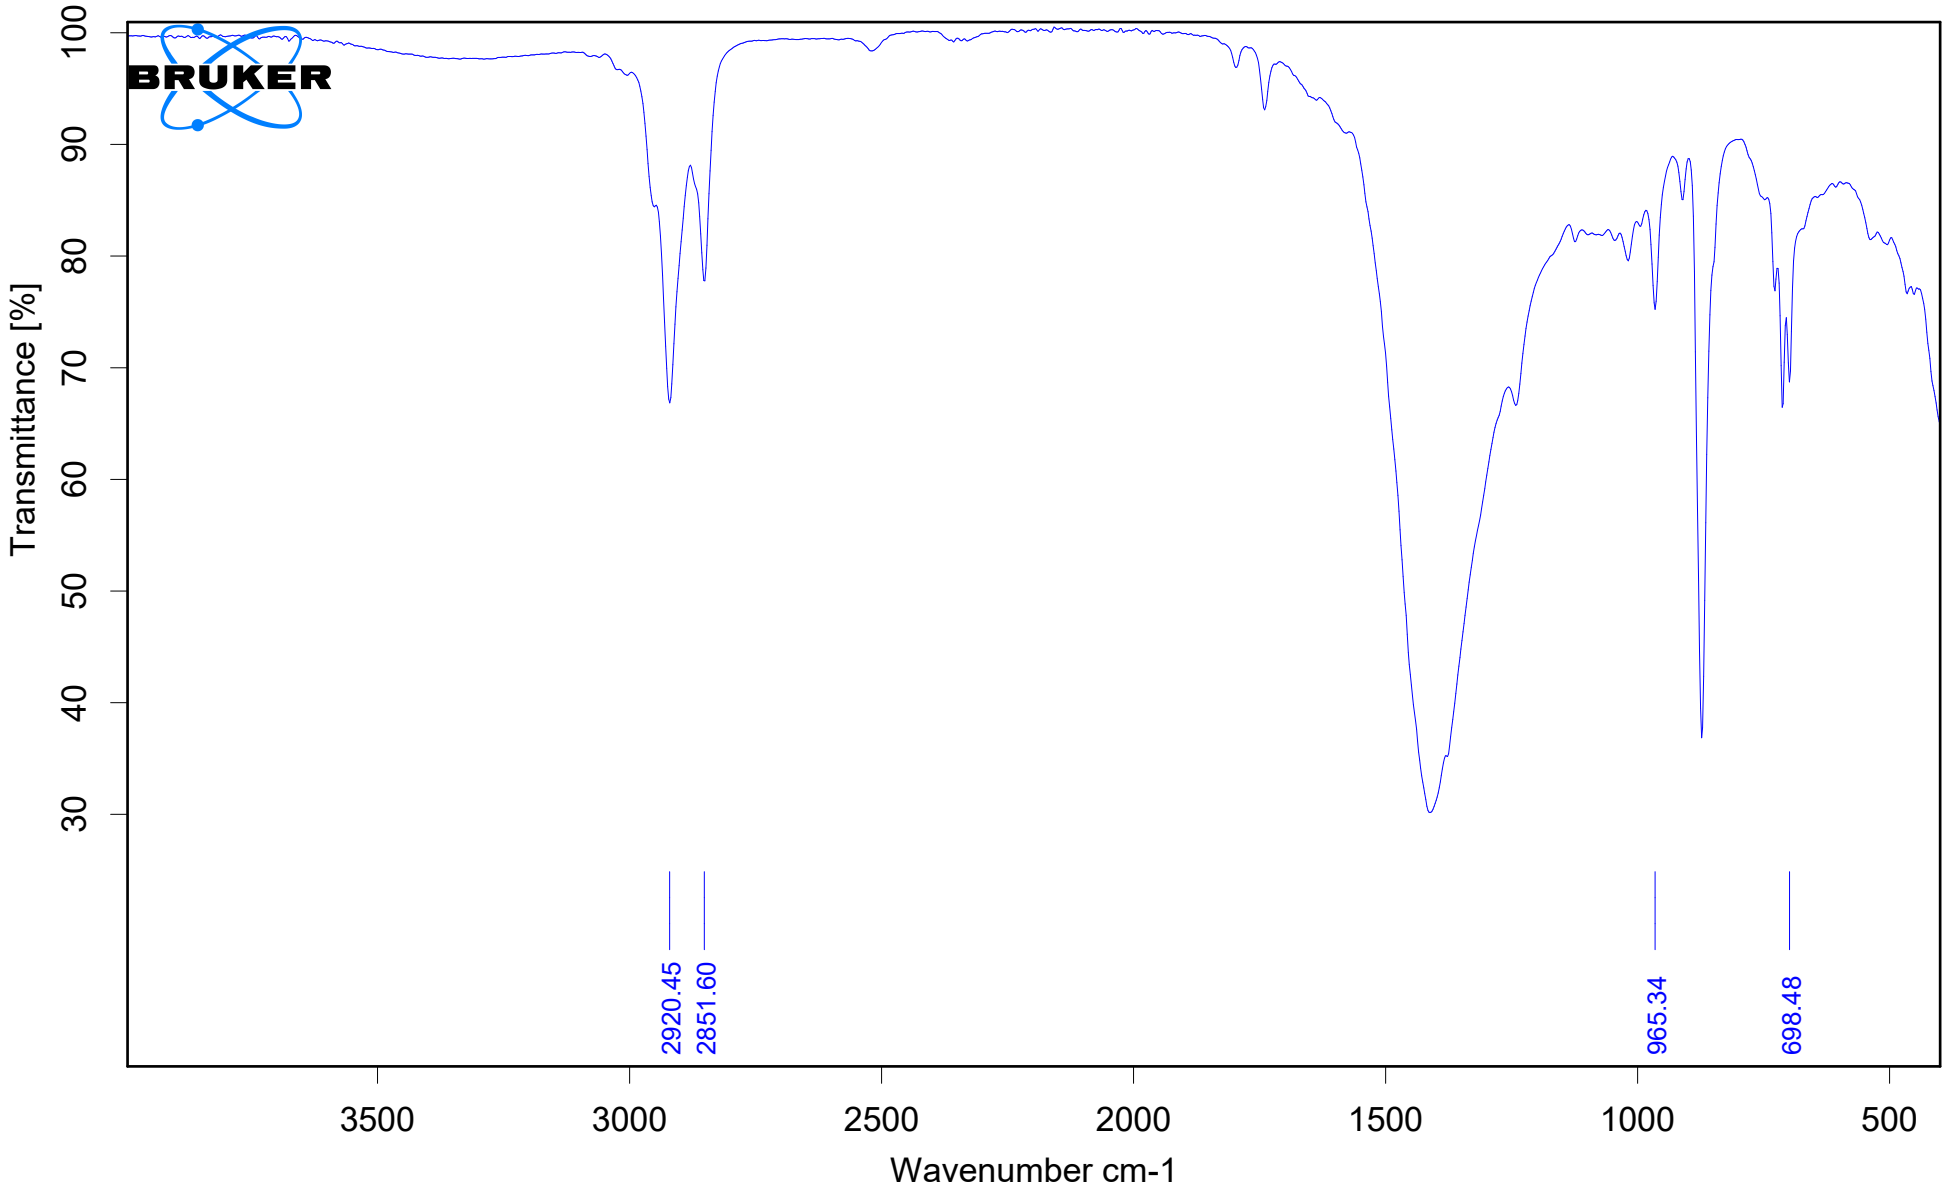


C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade do número de onda 1-2.0	Repetibilidade do número de onda 1-	10/03/2026

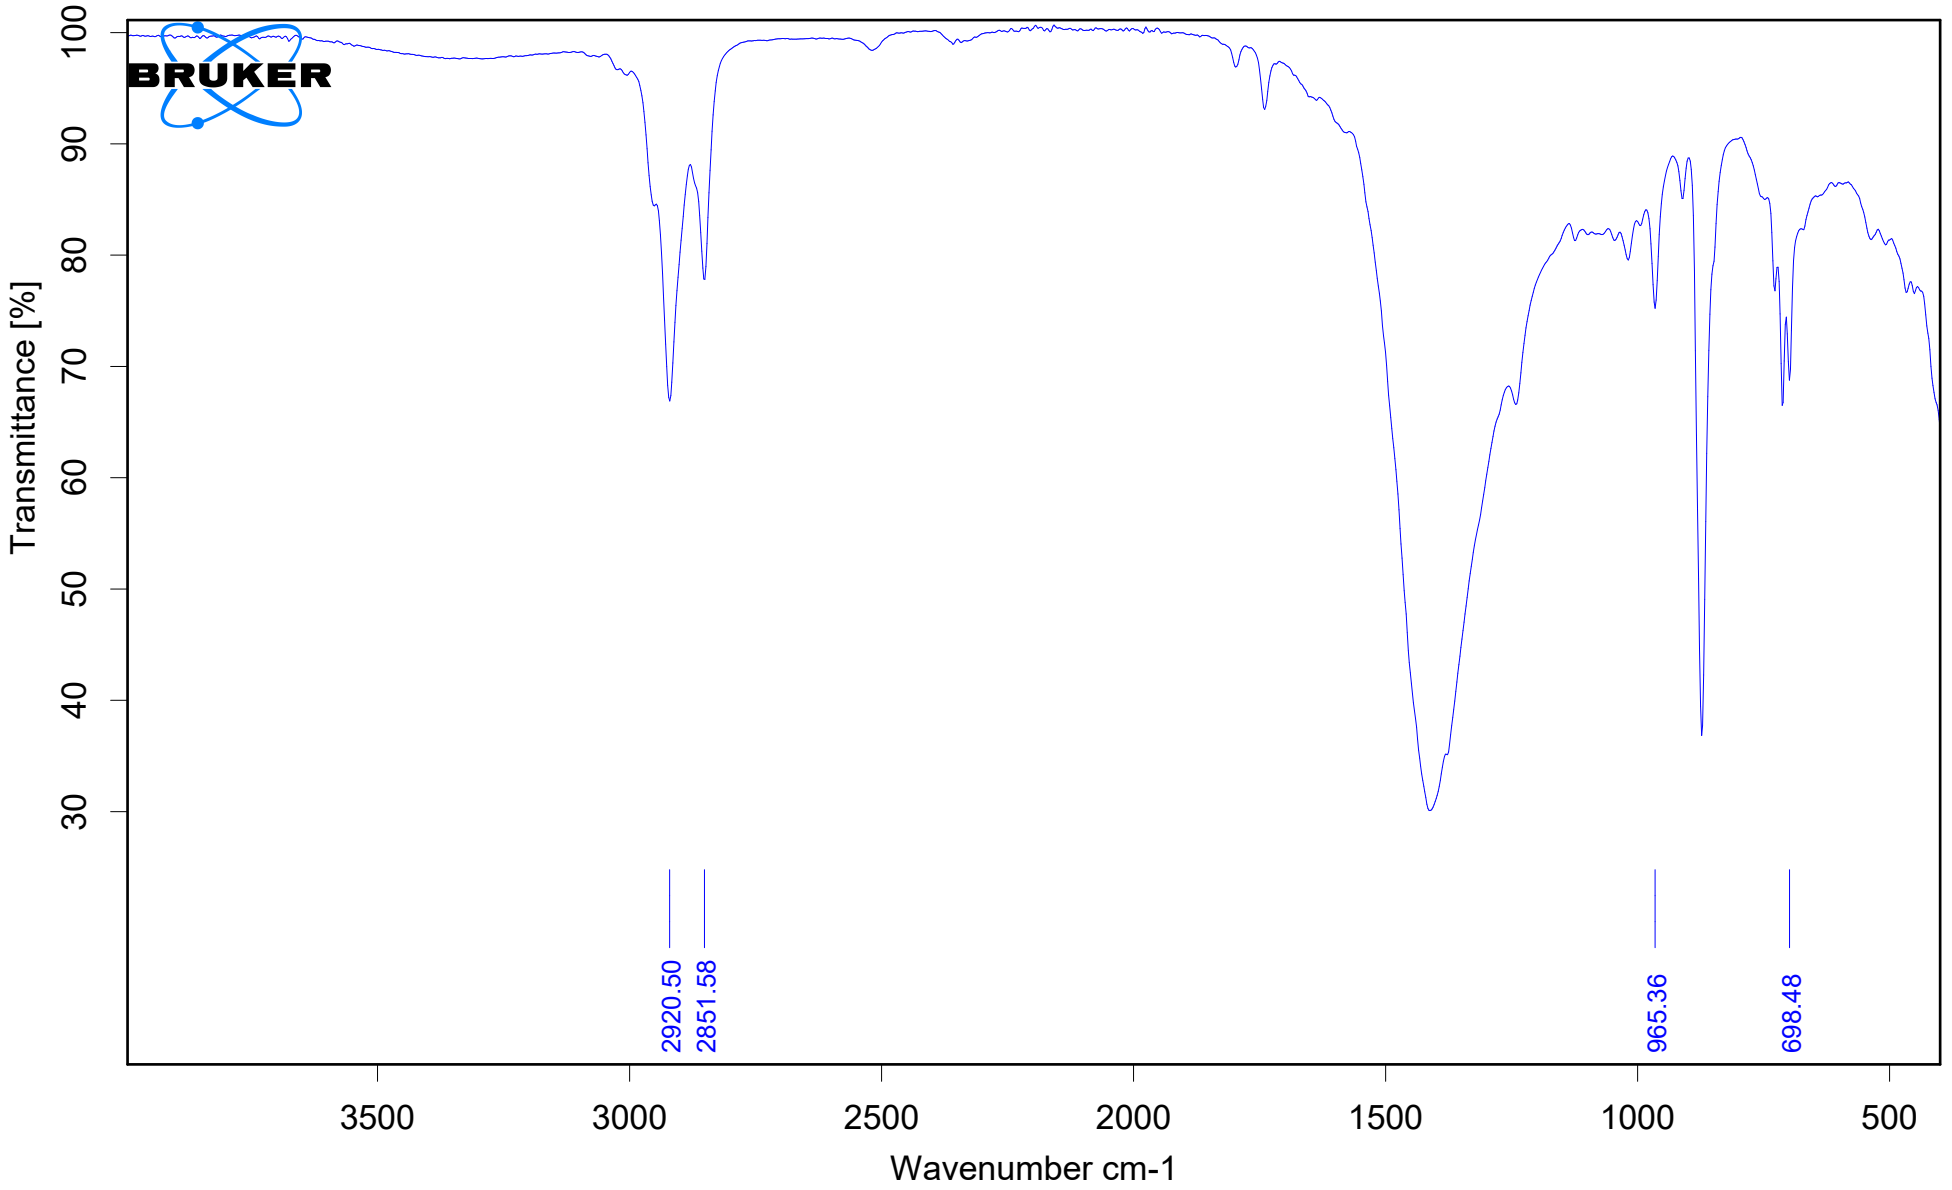

C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade do número de onda 2-2.0	Repetibilidade do número de onda 2-	10/03/2026

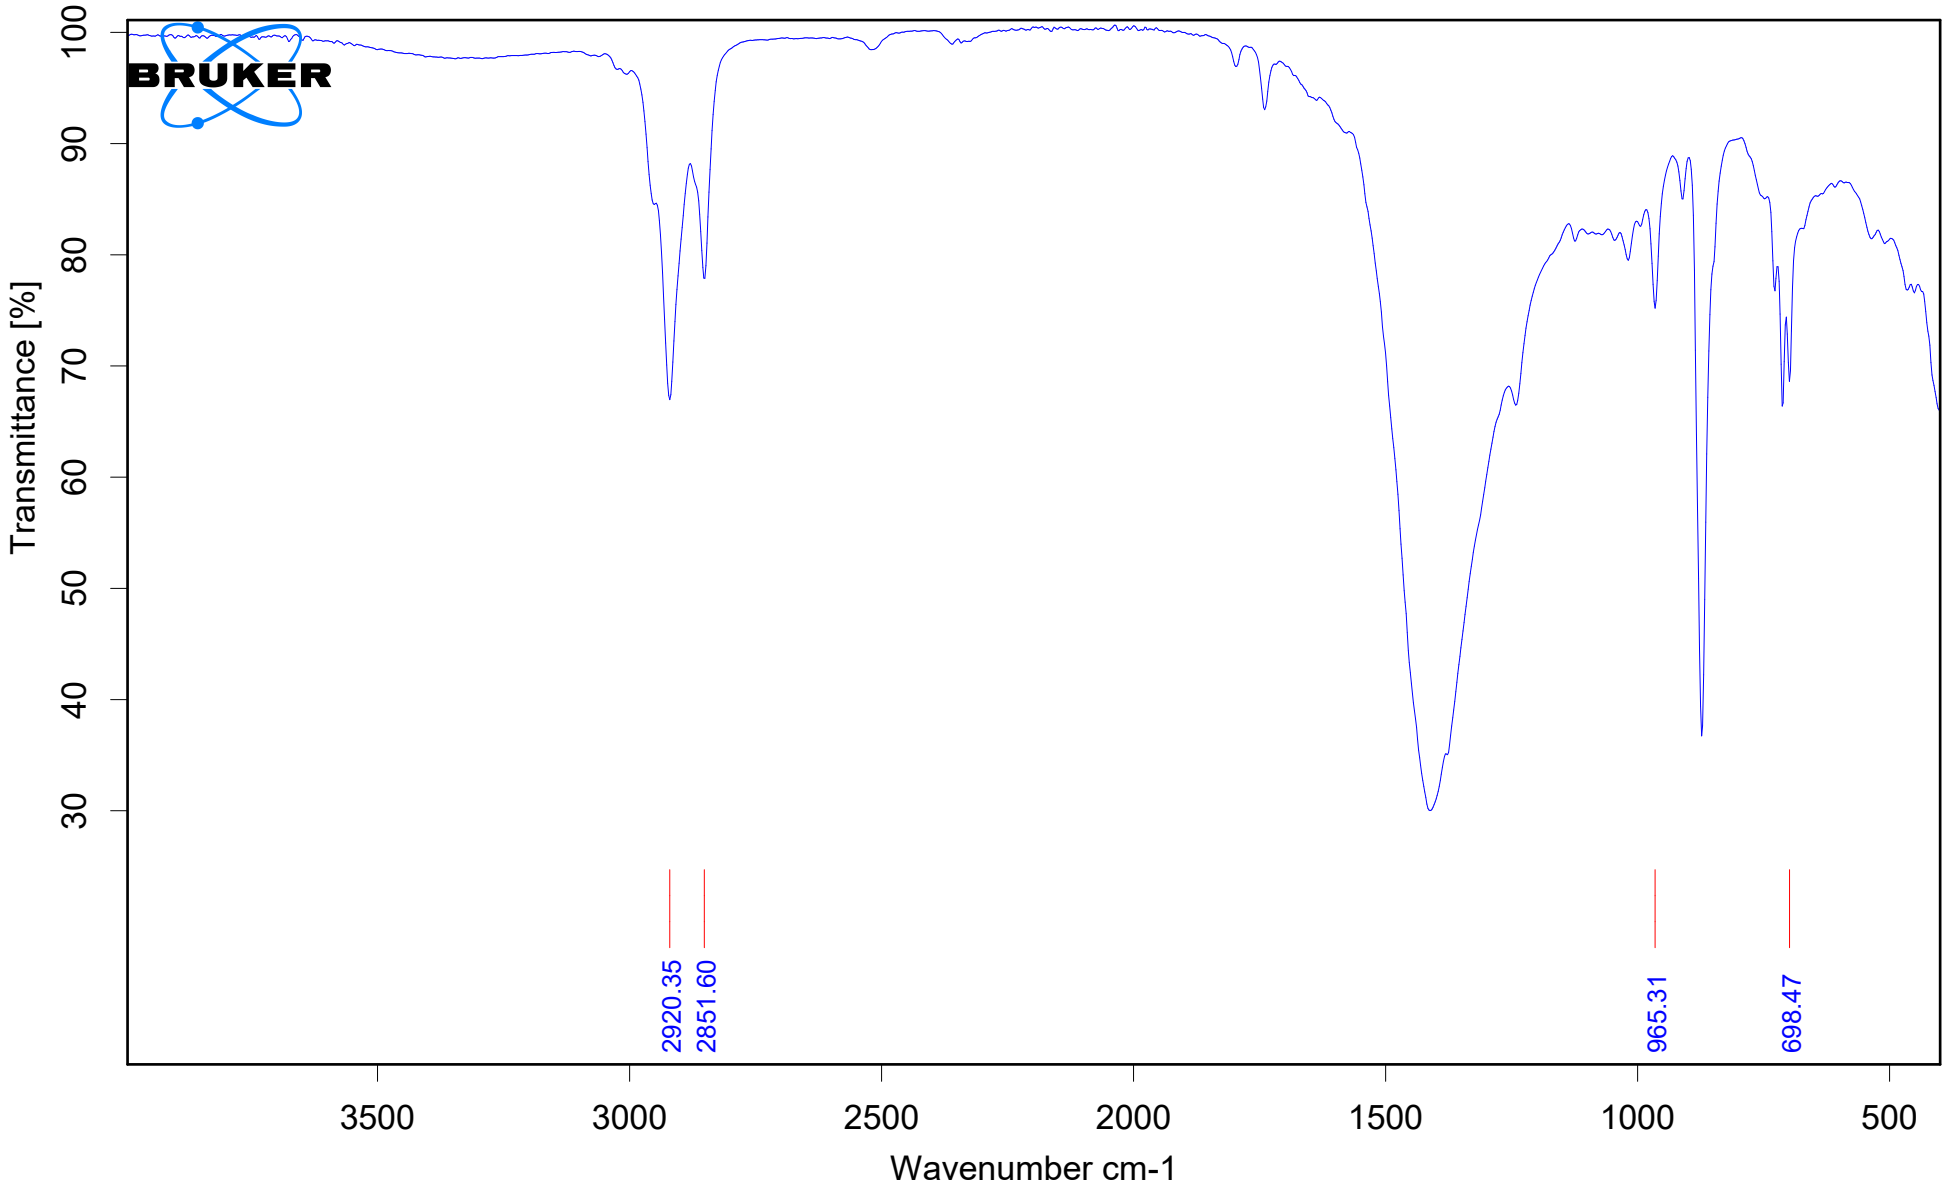


C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade fotométrica 1-2.0	Repetibilidade fotométrica 1-2	Instrume	10/03/2026

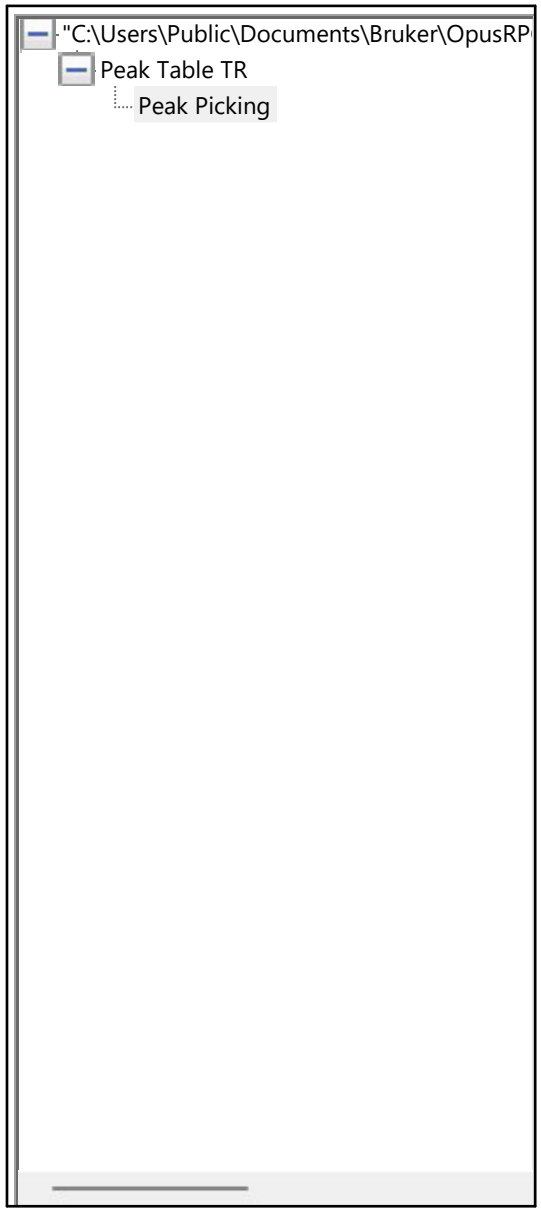


Peak Picking	Values
Method:	Standard
Searched for minima:	Yes
Number of peaks:	4
Sensitivity > [%]:	0.000000
From:	2993.045549
to:	623.446014
Absolute peak height >	0.000000
Relative peak height < [%]	0.000000
Absolute peak height <	0.000000

Wavenumber	Abs. intensity	Rel. intensity	Width	Found if threshold <	Shoulder
2920.3522	0.670	0.333	48.6486	111.043243	0
2851.6013	0.778	0.109	15.6953	32.447472	0
965.3107	0.752	0.105	14.7431	64.787254	0
698.4689	0.686	0.067	6.8930	27.187277	0

C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade fotométrica 1-2.0 Repetibilidade fotom

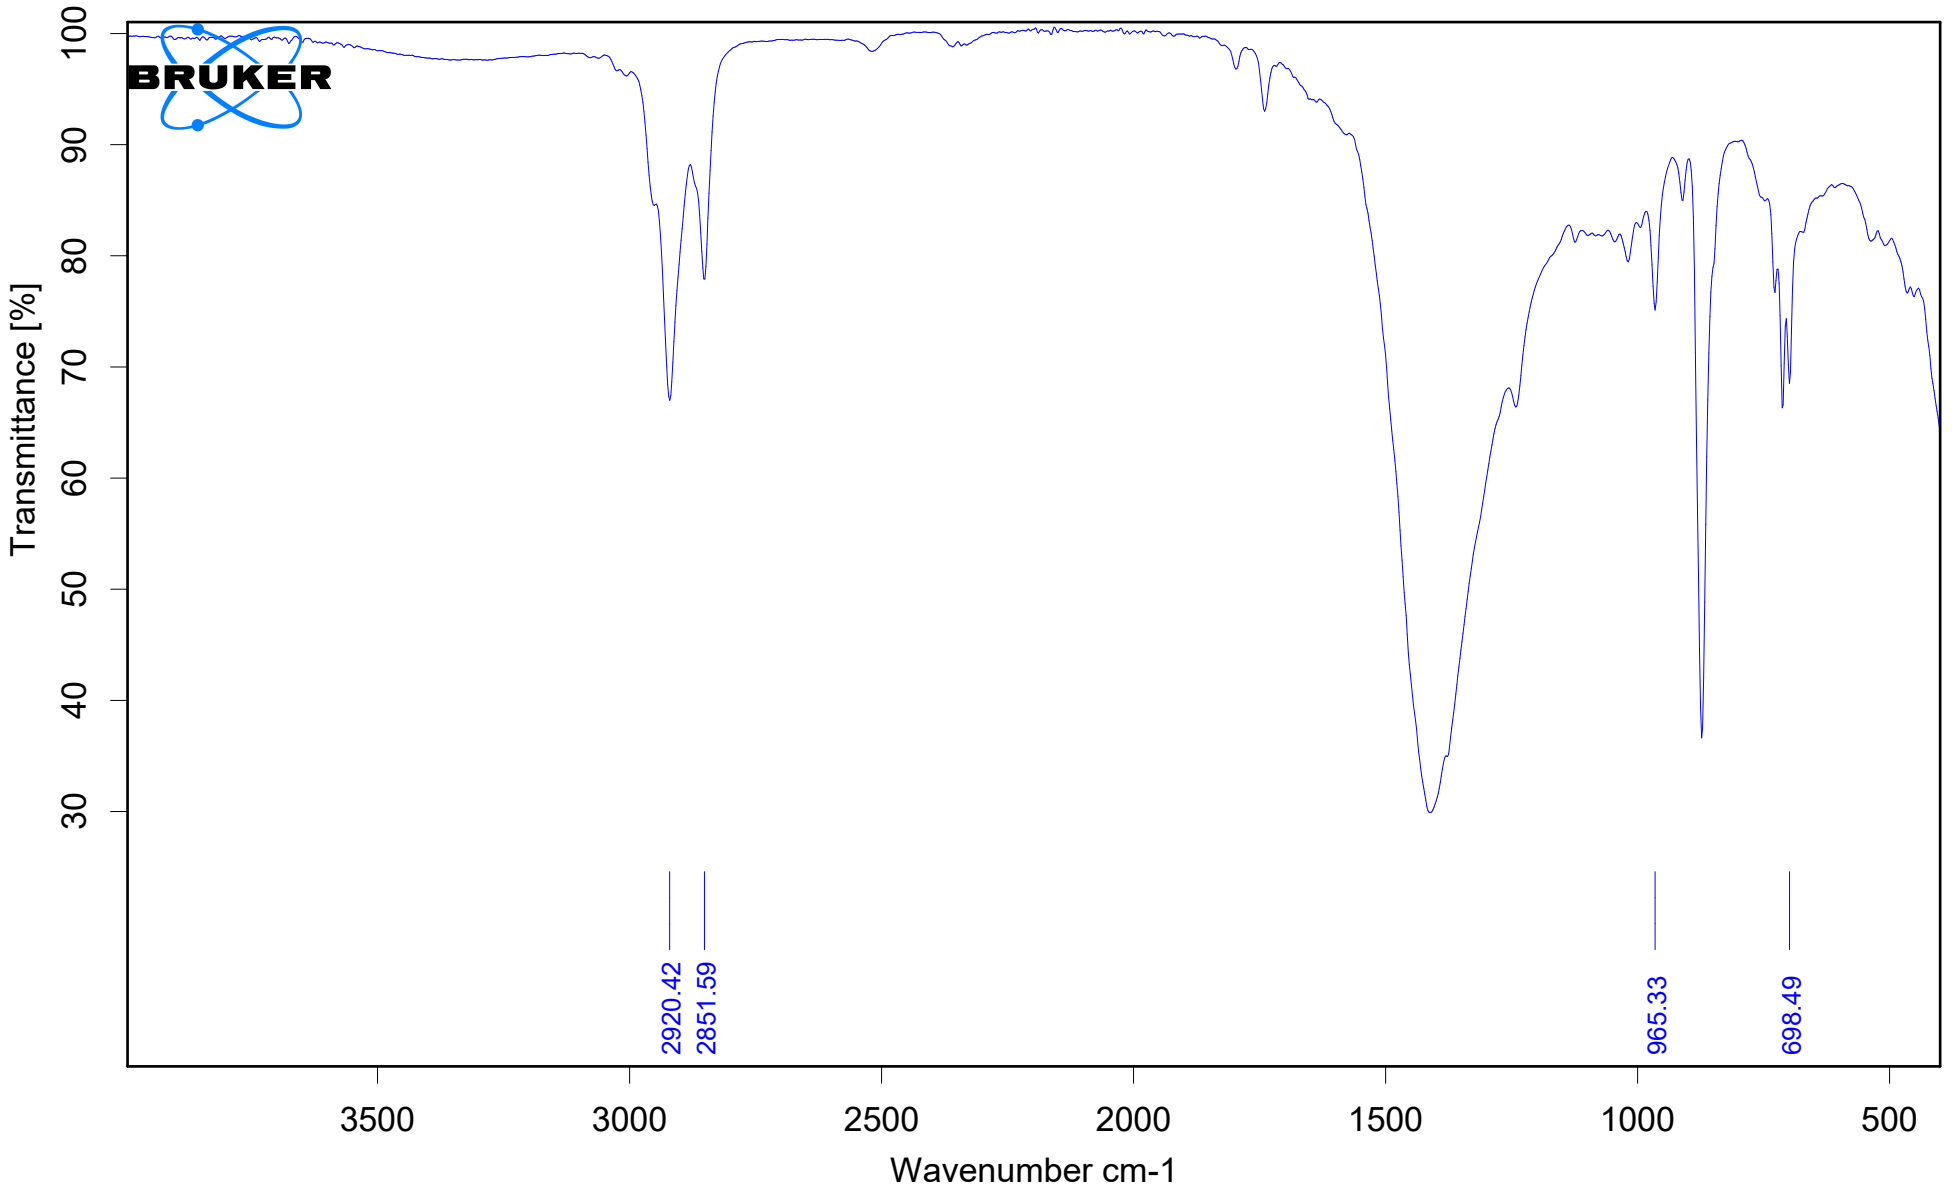


C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade fotométrica 2-2.0	Repetibilidade fotométrica 2-2	Instrume	10/03/2026

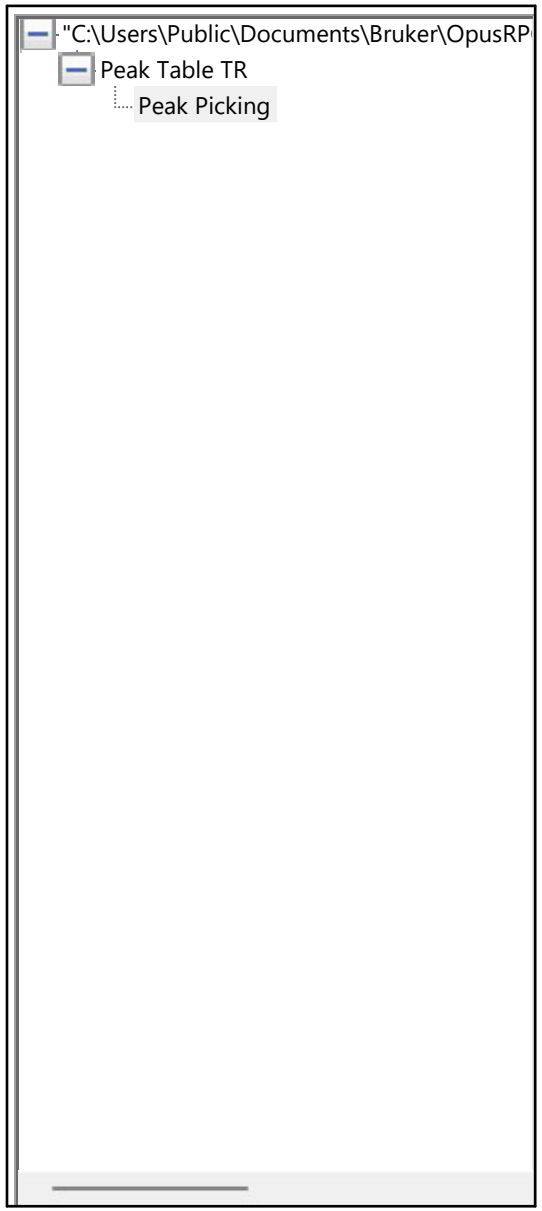


Peak Picking	Values
Method:	Standard
Searched for minima:	Yes
Number of peaks:	4
Sensitivity > [%]:	0.000000
From:	2993.045549
to:	625.604827
Absolute peak height >	0.000000
Relative peak height < [%]	0.000000
Absolute peak height <	0.000000

Wavenumber	Abs. intensity	Rel. intensity	Width	Found if threshold <	Shoulder
2920.4157	0.670	0.332	48.4303	111.017365	0
2851.5869	0.778	0.109	15.8225	32.531891	0
965.3282	0.751	0.105	14.6873	64.815216	0
698.4867	0.685	0.067	6.9056	27.017778	0

C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Repetibilidade fotométrica 2-2.0 Repetibilidade fotom

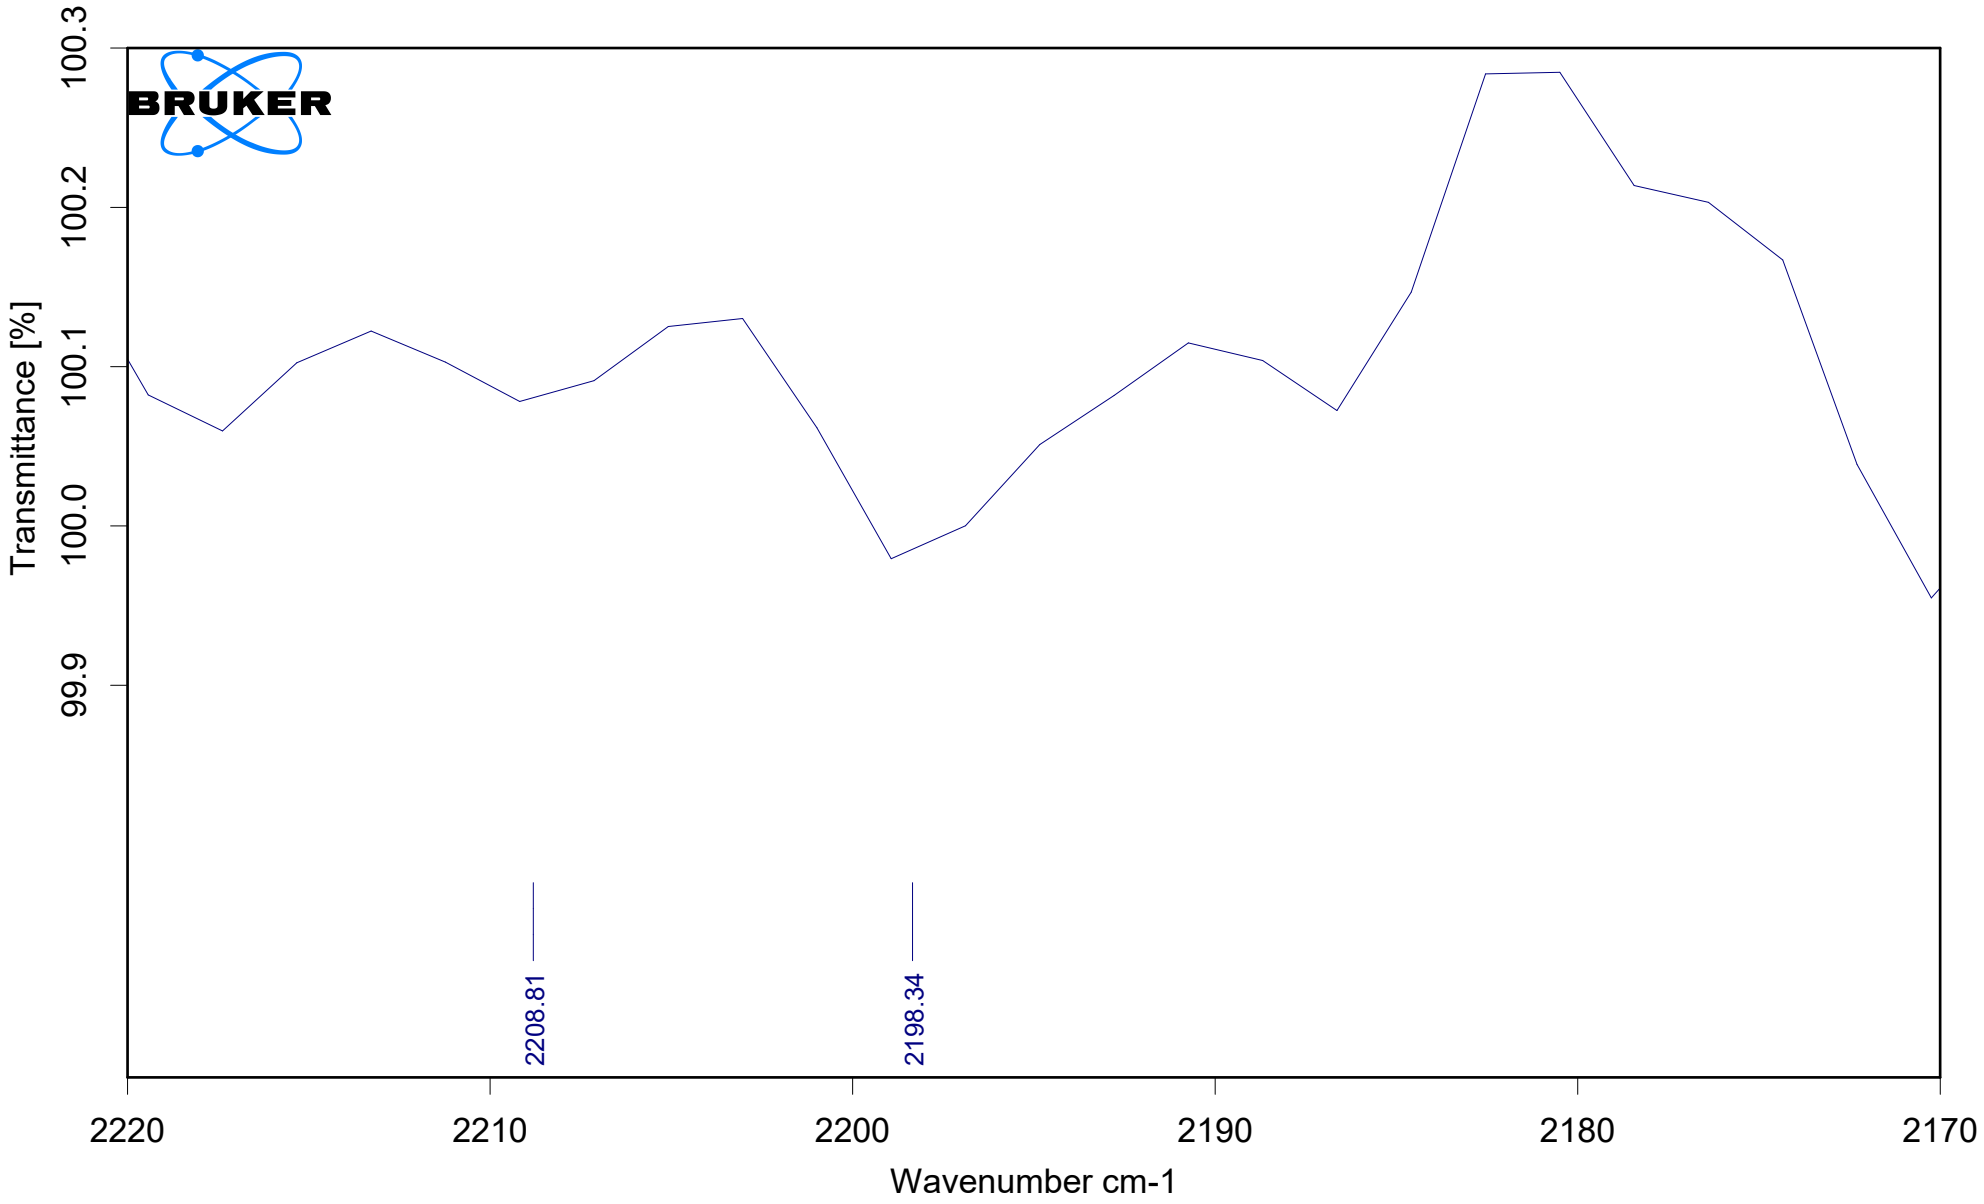

C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Sensibilidade.0	Sensibilidade	Instrument type and / or accessory	10/03/2026

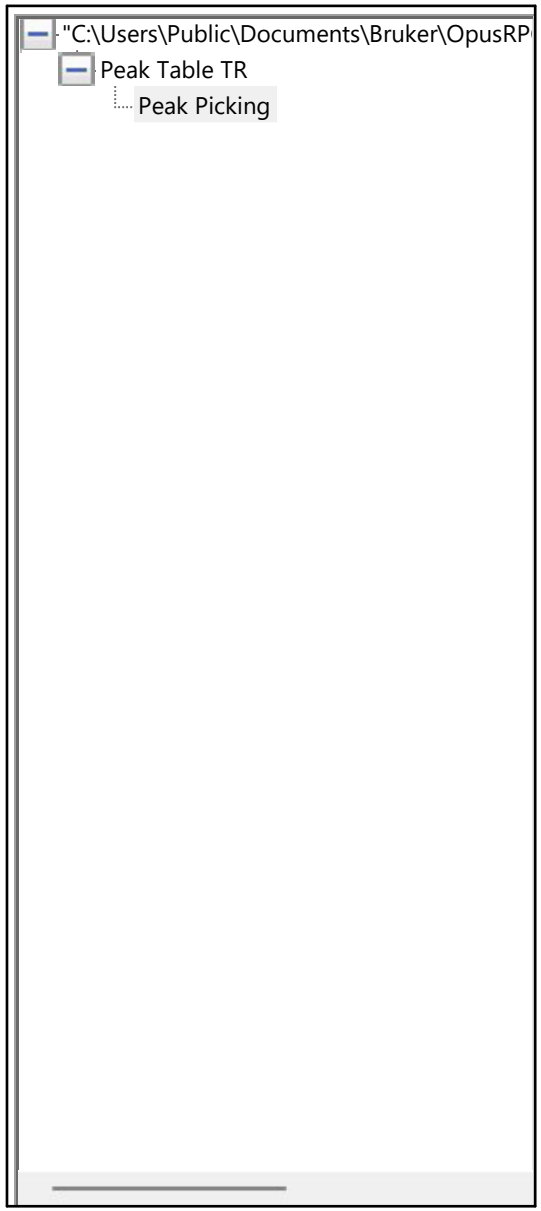

Peak Picking	Values
Method:	Standard
Searched for minima:	Yes
Number of peaks:	2
Sensitivity > [%]:	0.000000
From:	2210.165666
to:	2197.871549
Absolute peak height >	0.000000
Relative peak height < [%]	0.000000
Absolute peak height <	0.000000

Wavenumber	Abs. intensity	Rel. intensity	Width	Found if threshold <	Shoulder
2208.8074	1.001	0.001	5.1497	95.520119	0
2198.3447	1.000	0.003	10.9234	137.642731	0

C:\Users\Public\Documents\Bruker\OpusRPC_5.1.19.199\Data\MEAS\Sensibilidade.0 Sensibilidade Instrument type ar