
Chromatogram

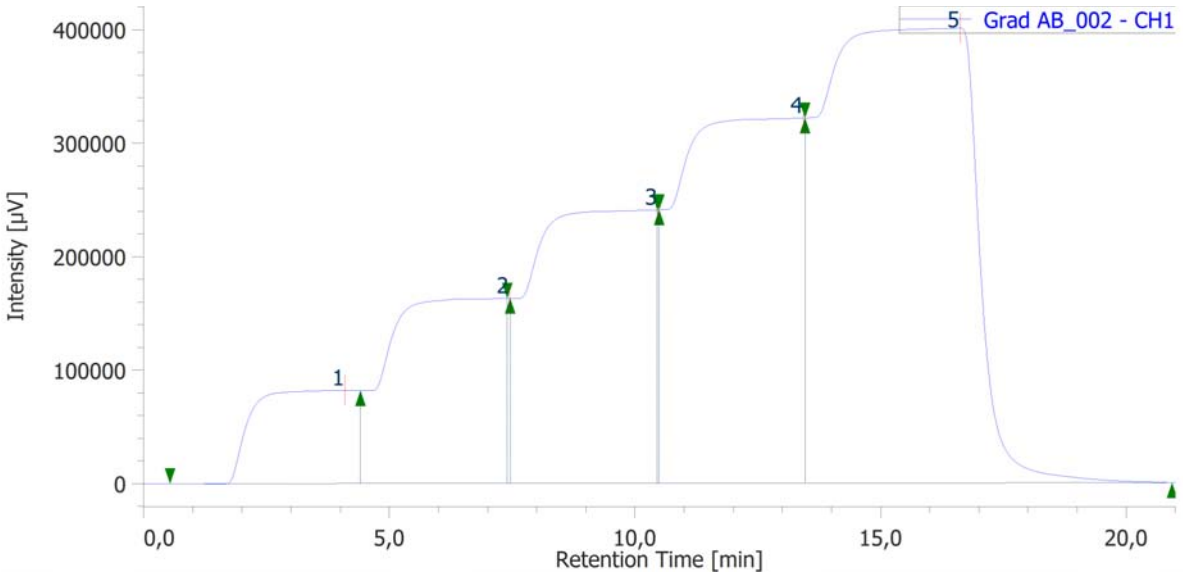

Chromatogram Information	
User Name	QPackSA
Date Modified	18/03/2024 14:38:03
Description	
HPLC System Name	HPLC-0004
Injection Date	18/03/2024 13:05:42
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20 %	1	4,100	11463136	82001	7,559	6,790	N/A	N/A	N/A	N/A		N/A
2	40 %	1	7,442	570369	162974	0,376	13,494	N/A	N/A	N/A	N/A		N/A
3	60 %	1	10,467	601849	240735	0,397	19,933	N/A	N/A	N/A	N/A		N/A
4	80 %	1	13,425	54336993	321540	35,831	26,624	N/A	N/A	N/A	N/A		N/A
5	100 %	1	16,617	84677756	400467	55,838	33,159	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

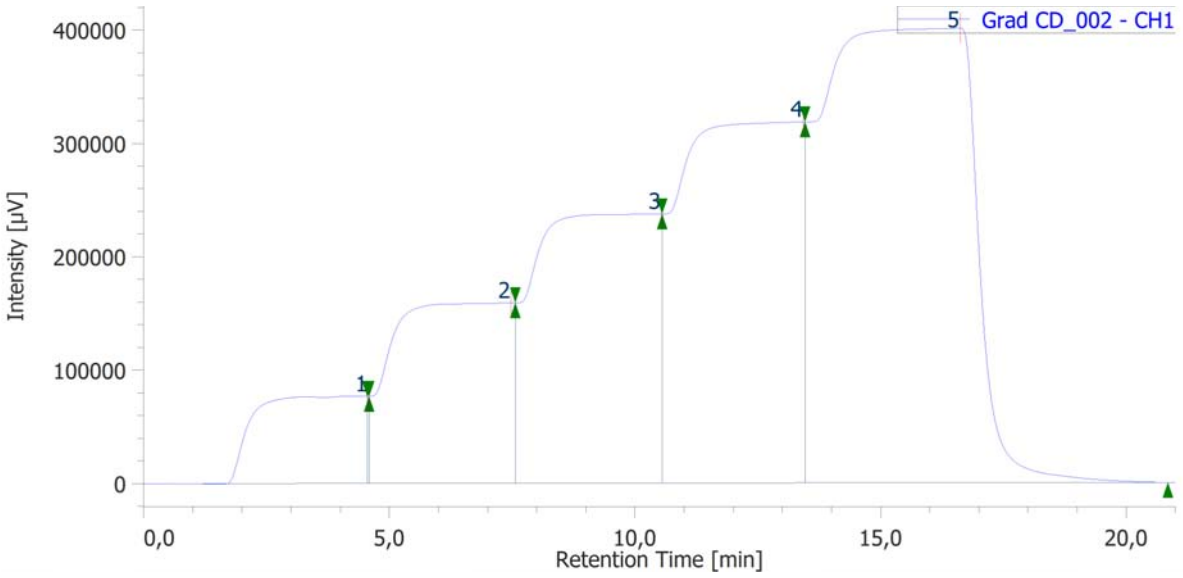

Chromatogram Information

User Name	QPackSA
Date Modified	18/03/2024 14:45:54
Description	
HPLC System Name	HPLC-0004
Injection Date	18/03/2024 14:14:14
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20 %	1	4,567	153466	76733	0,075	6,441	N/A	N/A	N/A	N/A		N/A
2	40 %	1	7,475	25994279	158856	12,770	13,334	N/A	N/A	N/A	N/A		N/A
3	60 %	1	10,533	40230087	237286	19,764	19,918	N/A	N/A	N/A	N/A		N/A
4	80 %	1	13,425	52897190	318048	25,987	26,697	N/A	N/A	N/A	N/A		N/A
5	100 %	1	16,617	84276566	400420	41,403	33,611	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver