
Peak Find - EDFL_003 FPEm_tR0,31 D.jws

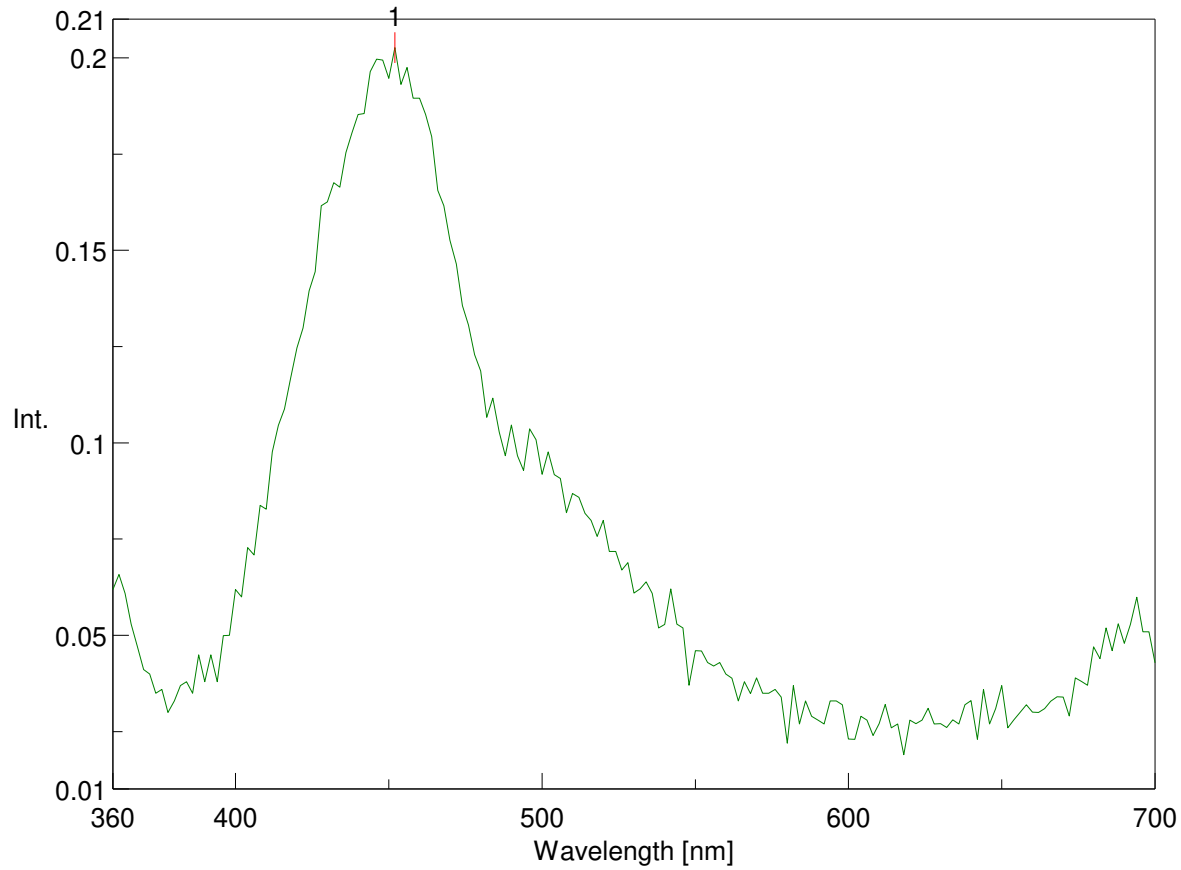

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	05/03/2025 15:25

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	FP-1520
Model Name	FP-1520
Serial No.	XXXXX
ROM version	V1.42
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	452	0.202591			

Chromatogram

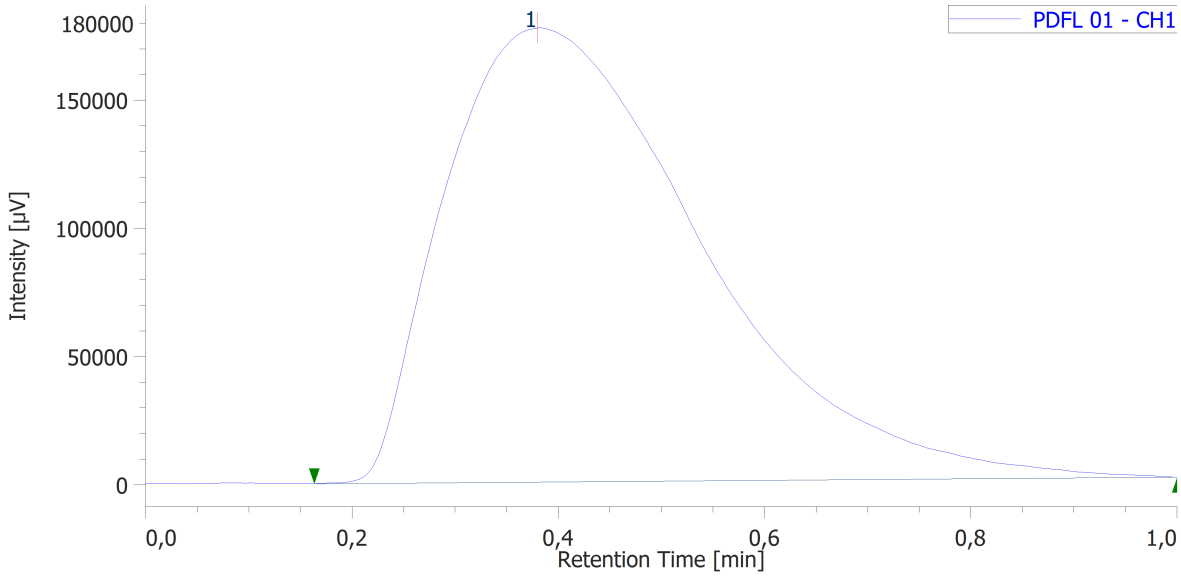

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:20
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:47:14
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,380	3067284	177024	100,000	100,000	N/A	11	N/A	1,809		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

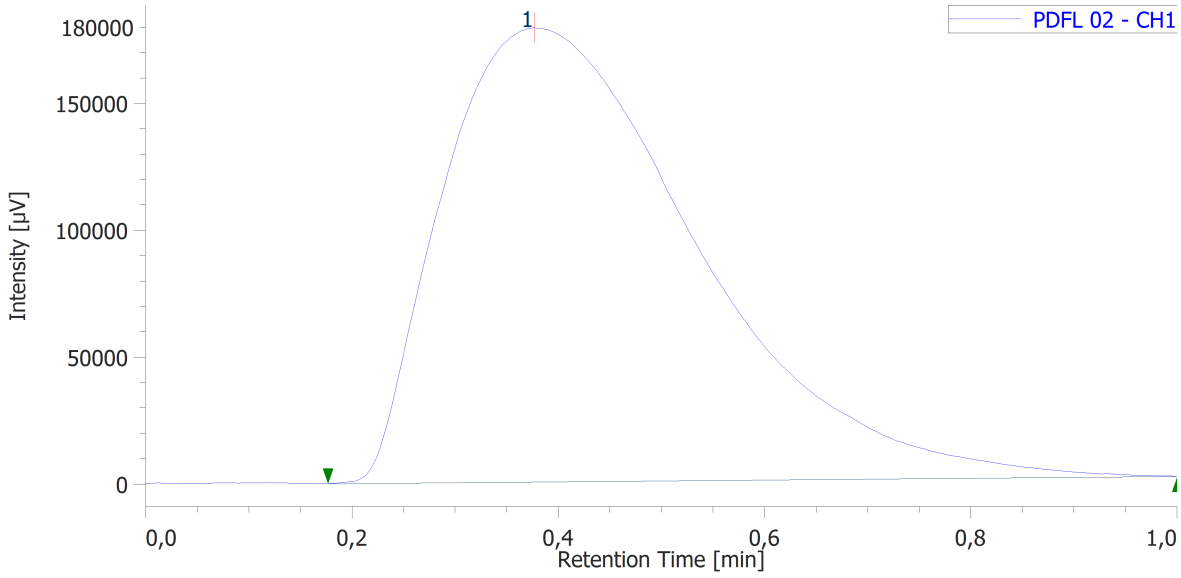

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:20
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:49:37
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,377	3062181	178742	100,000	100,000	N/A	11	N/A	1,811		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

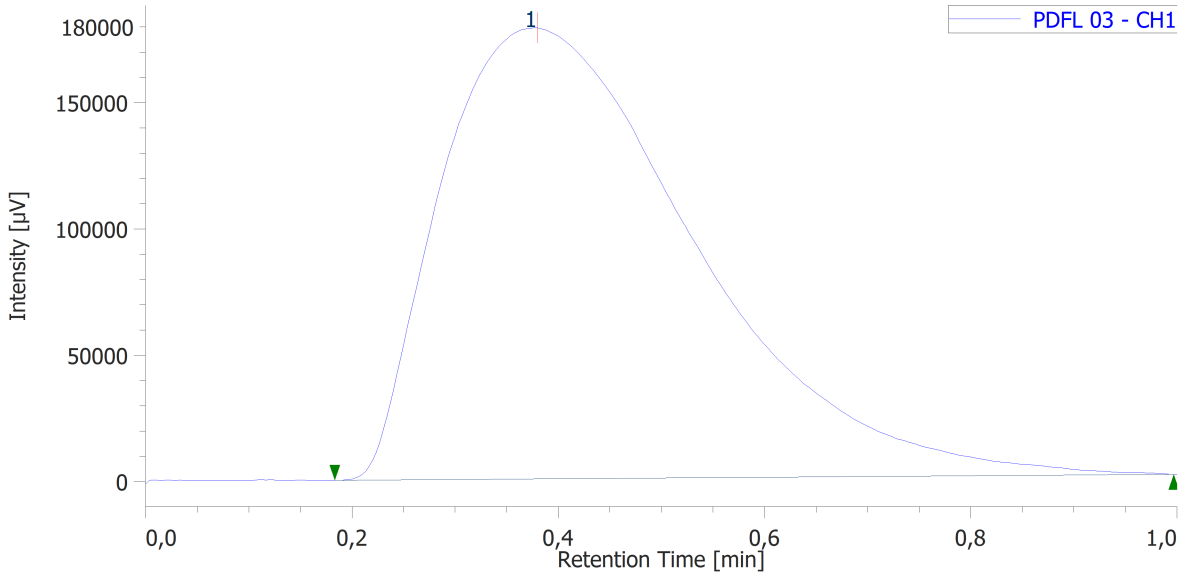

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:20
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:52:01
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,380	3061713	178329	100,000	100,000	N/A	11	N/A	1,763		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

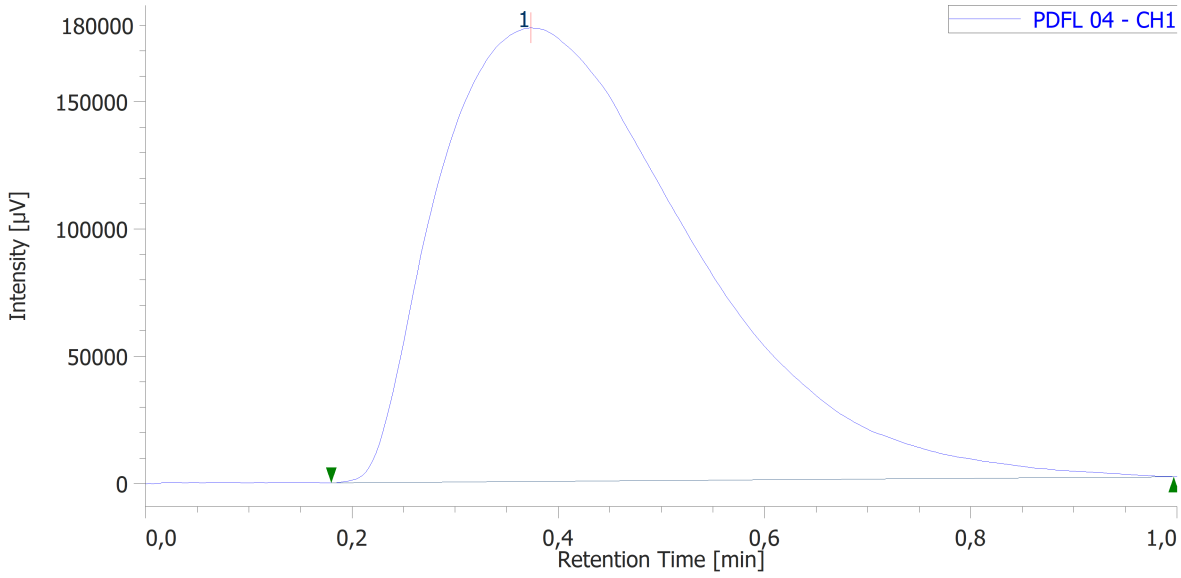

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:20
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:54:24
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,373	3061194	178011	100,000	100,000	N/A	11	N/A	1,833		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

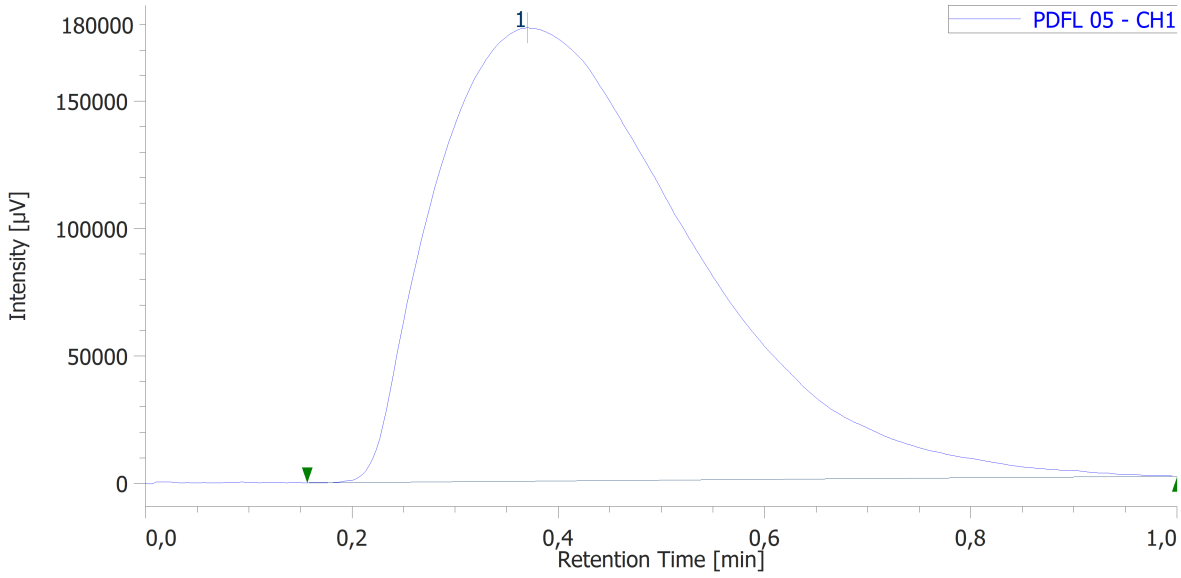

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:21
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:56:47
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,370	3070033	177792	100,000	100,000	N/A	10	N/A	1,865		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

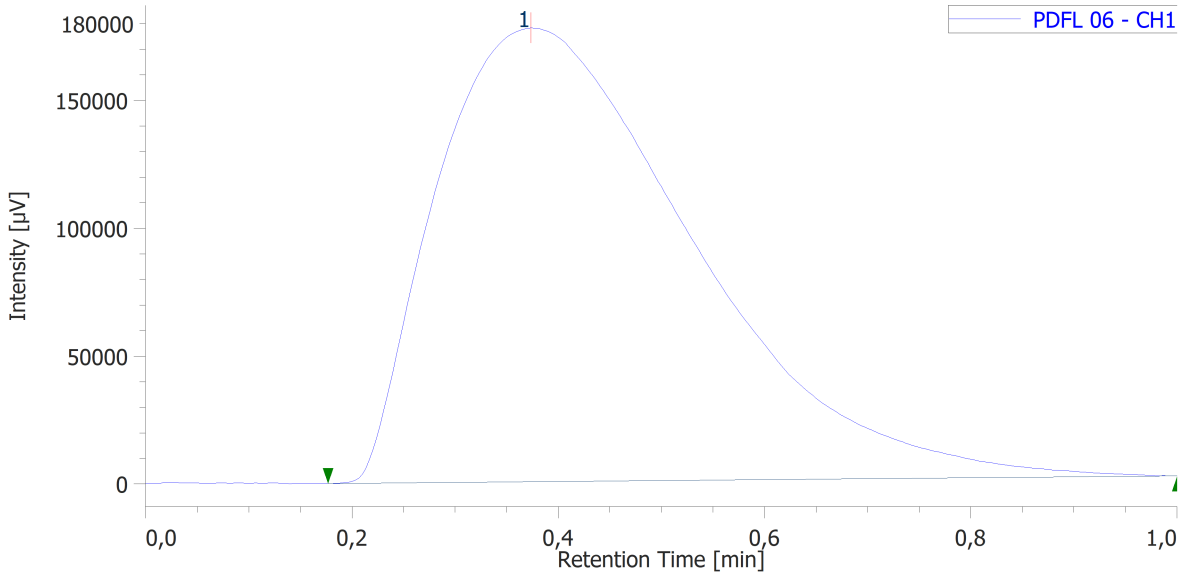

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2025 16:10:21
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2025 15:59:11
Volume	10,0 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PDFL 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,373	3071689	177444	100,000	100,000	N/A	10	N/A	1,804		N/A

Creator QPackSA
Reviewer
Approver