

EDUV | DAD1 Scan RT=1,122 Minutes | 2025-03-10 12-48-39-03-00-01.dx
rel. Response [%]
100
80
60
40
20
0
205
273
190
195
200
205
210
215
220
225
230
235
240
245
250
255
260
265
270
275
280
285
290
295
300
Wavelength [nm]

Single Injection Report

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 12-48-39-03-00-01.dx		
Sample name:	EDUV		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A1
Injection date:	2025-03-10 12:49:35-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

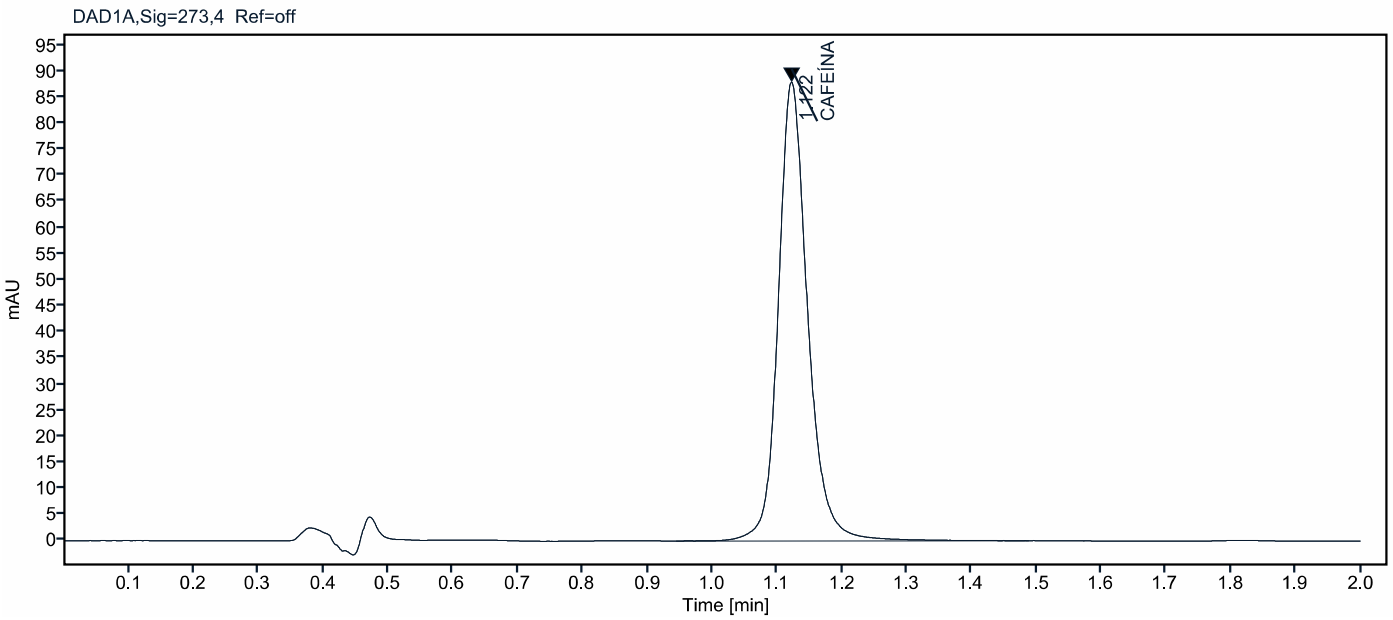

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
EDUV	CAFEÍNA	1.122	278.3414			87.919

Agilent - Data Analysis

Home | Processing | Audit/E-Sign | Chromatograms

Open Method | Save Method | Close Method — Methods

Reprocess All | Save All Results — Processing

Print All | View PDF — Reports

Layouts | Copy | Delete | Reset — Layouts

Acquisition Setpoints | Injection List | Peak Details | UV Spectrum
Calibration Curve | Injection Results | Sample Information | Isoabsorbance
Chromatograms | Processing Method | Peak Explorer — Windows

essing

2025-03-10 12-48-32-03-00
V - 2025-03-10 12-48-39-03-00-01.dx *
NCO 01 - 2025-03-10 12-51-38-03-00-02.dx *
01 - 2025-03-10 12-54-36-03-00-03.dx *
02 - 2025-03-10 12-57-32-03-00-04.dx *
03 - 2025-03-10 13-00-30-03-00-05.dx *
NCO 02 - 2025-03-10 13-03-26-03-00-06.dx *
04 - 2025-03-10 13-06-24-03-00-07.dx *
05 - 2025-03-10 13-09-21-03-00-08.dx *
06 - 2025-03-10 13-12-17-03-00-09.dx *
NCO 03 - 2025-03-10 13-15-15-03-00-10.dx *
V 01 - 2025-03-10 13-18-12-03-00-11.dx *


273,4 Ref=off

Traces

uantitative_DefaultMethod


UV Spectrum

Display mode: Separate

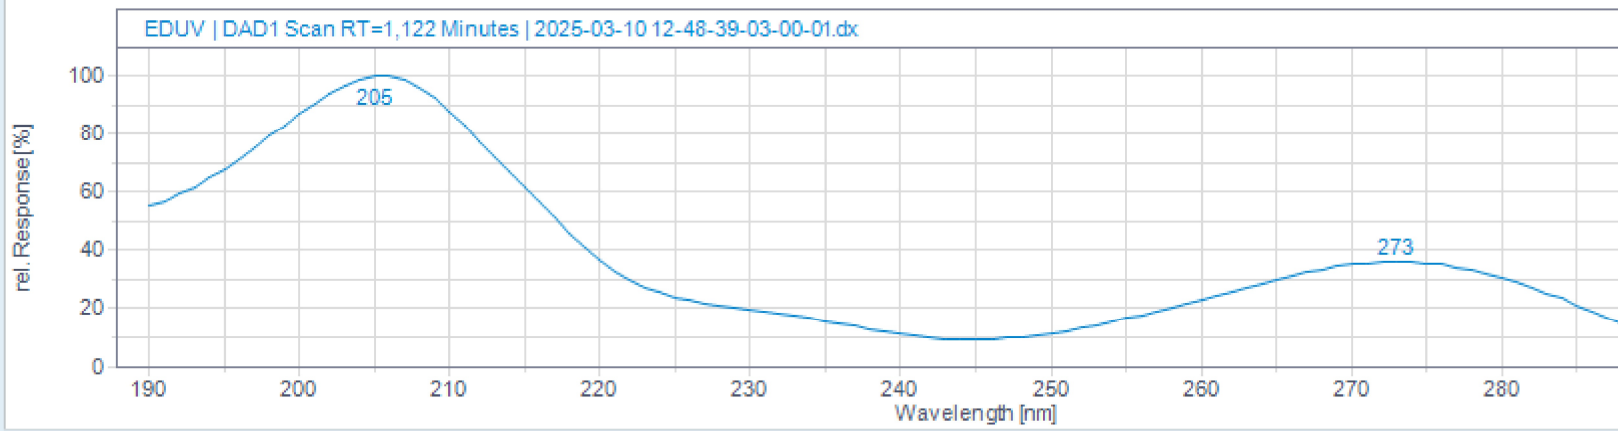


Chromatograms

Display mode: Overlaid

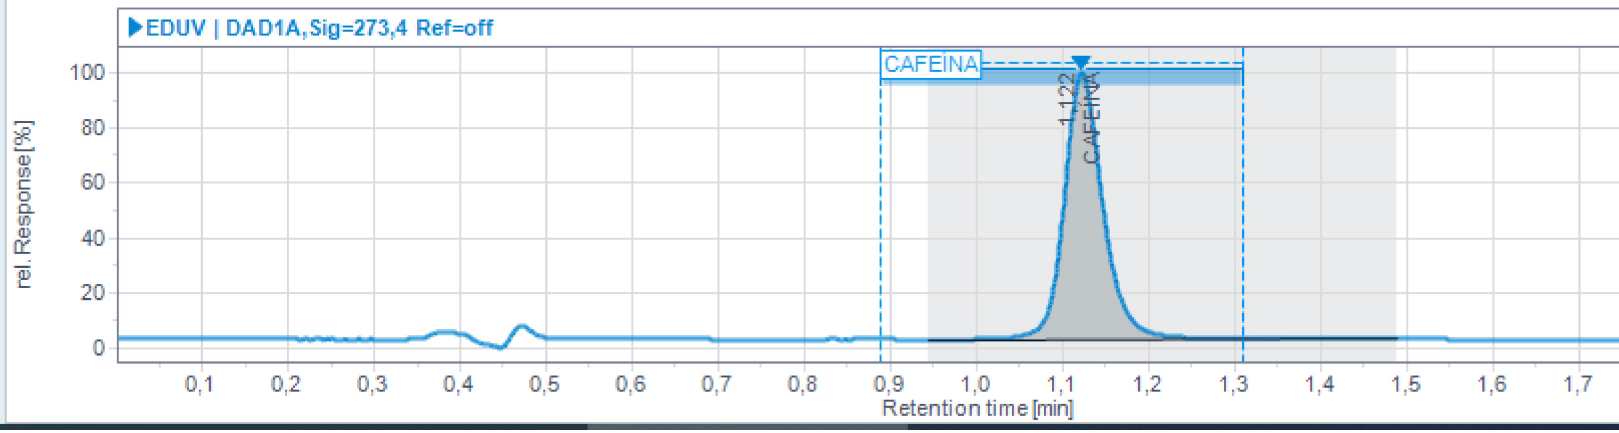

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 12-51-38-03-00-02.dx		
Sample name:	BRANCO 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A2
Injection date:	2025-03-10 12:52:33-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

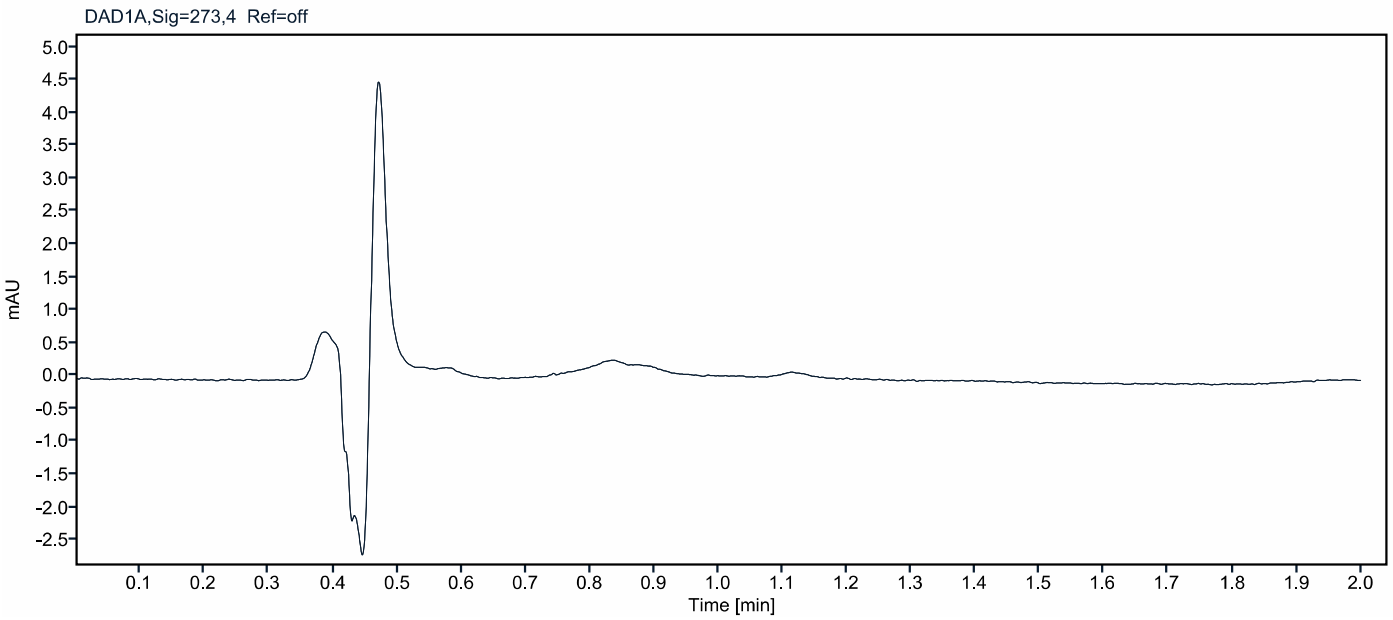

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height

Single Injection Report

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 12-54-36-03-00-03.dx		
Sample name:	PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 12:55:30-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

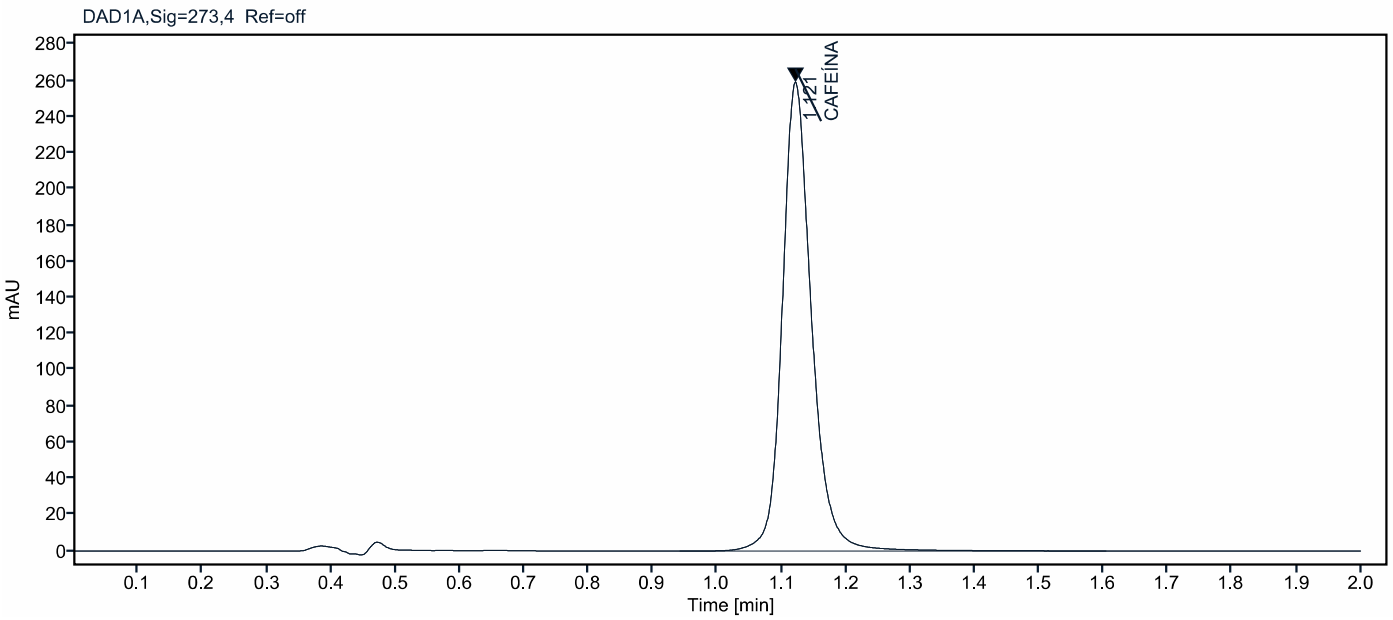


Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 01	CAFEÍNA	1.121	822.9856			259.307

Single Injection Report

Agilent


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 12-57-32-03-00-04.dx		
Sample name:	PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 12:58:27-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

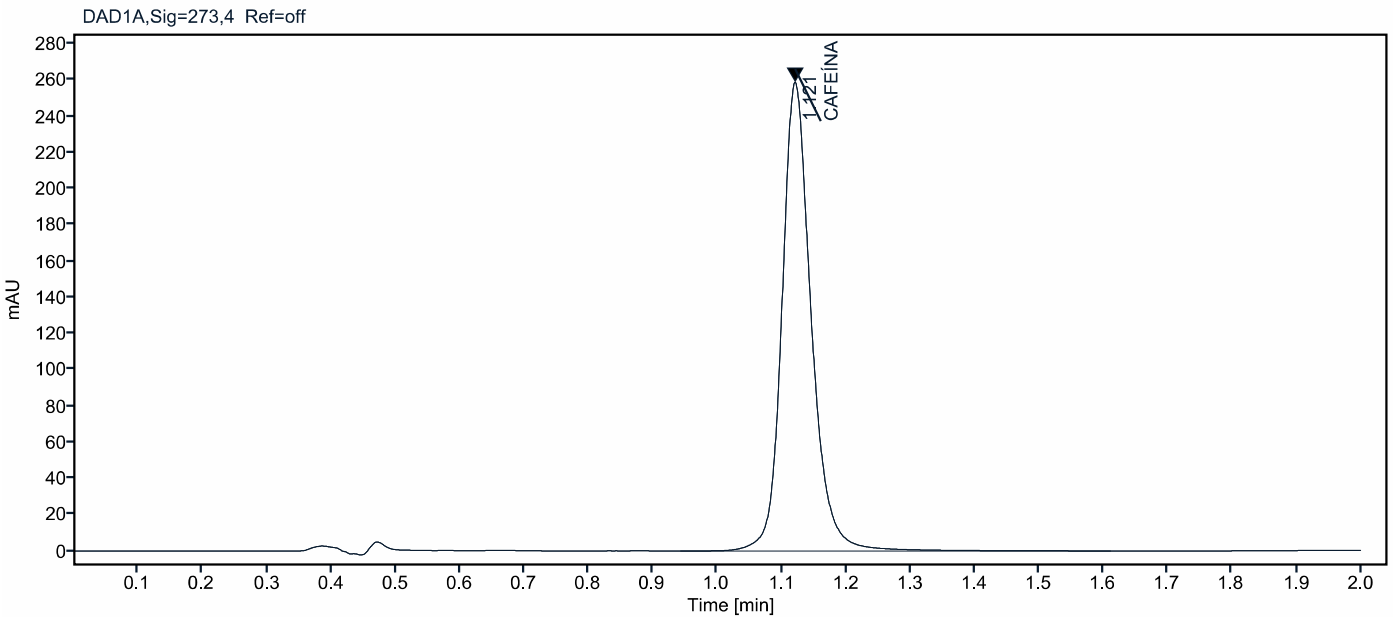

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 02	CAFEÍNA	1.121	822.9728			258.924

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-00-30-03-00-05.dx		
Sample name:	PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 13:01:24-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

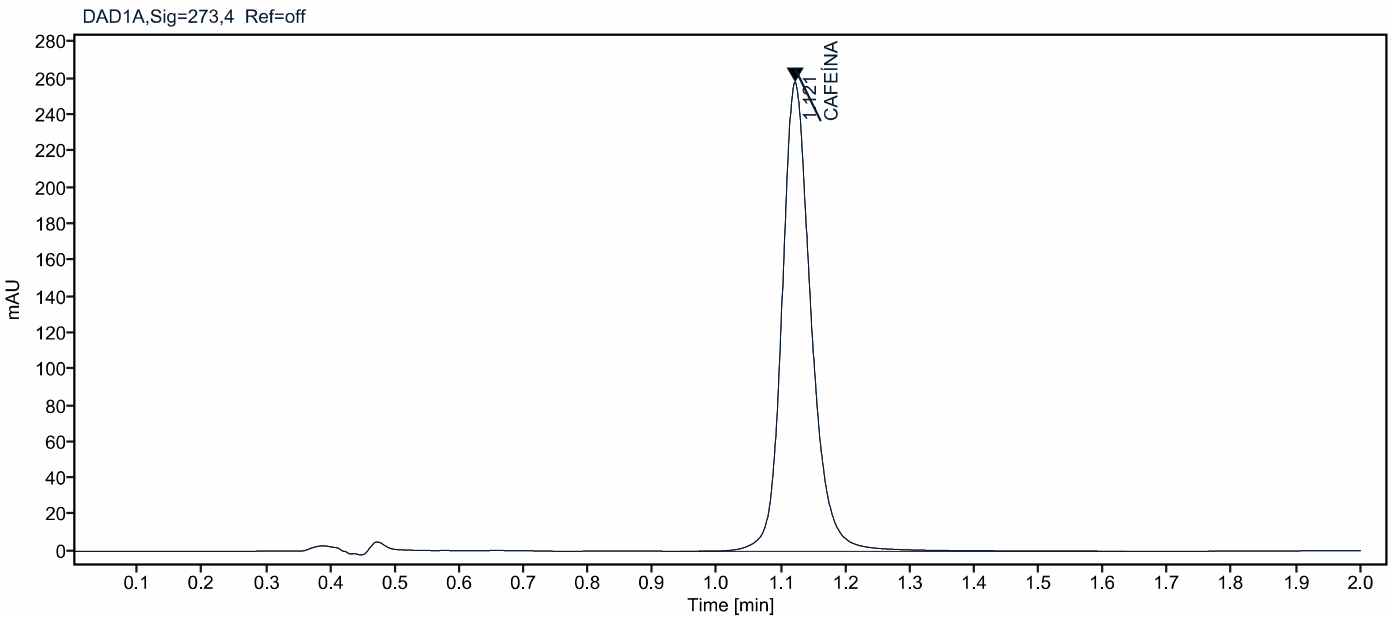

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 03	CAFEÍNA	1.121	821.9561			258.221

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-03-26-03-00-06.dx		
Sample name:	BRANCO 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A2
Injection date:	2025-03-10 13:04:22-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

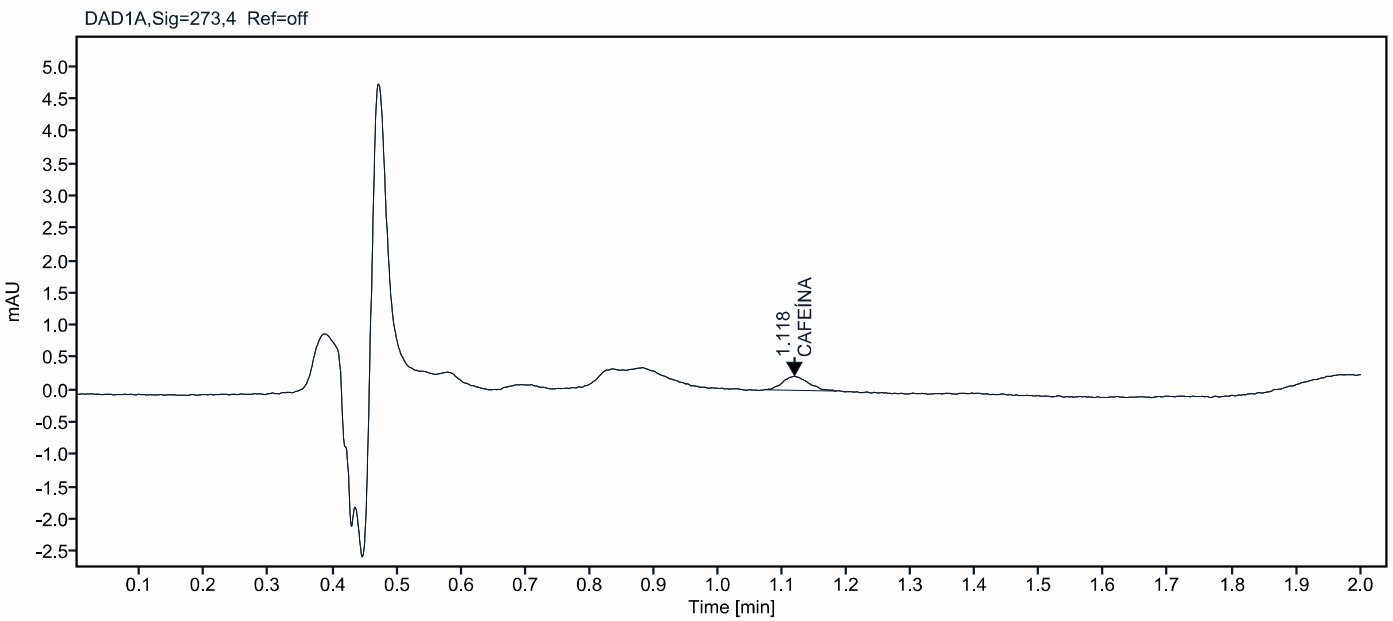

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
BRANCO 02	CAFEÍNA	1.118	0.5981			0.215

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-06-24-03-00-07.dx		
Sample name:	PCIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 13:07:18-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

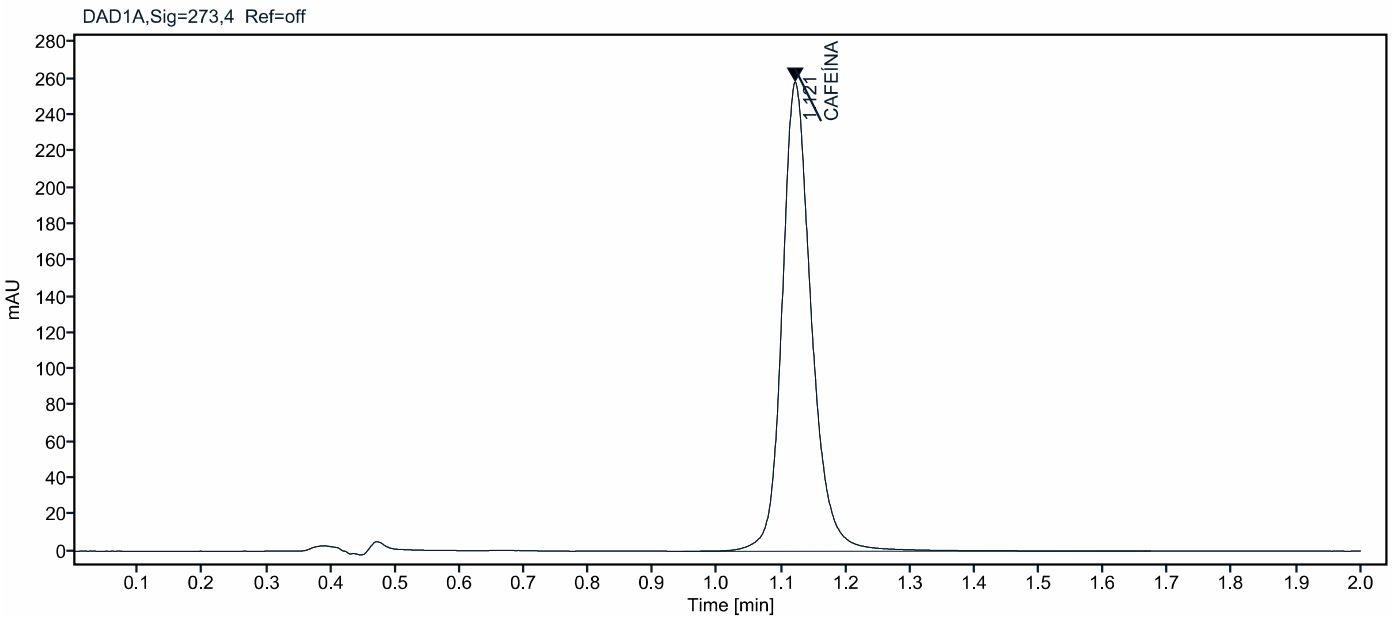

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 04	CAFEÍNA	1.121	822.7704			258.139

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-09-21-03-00-08.dx		
Sample name:	PCIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 13:10:15-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

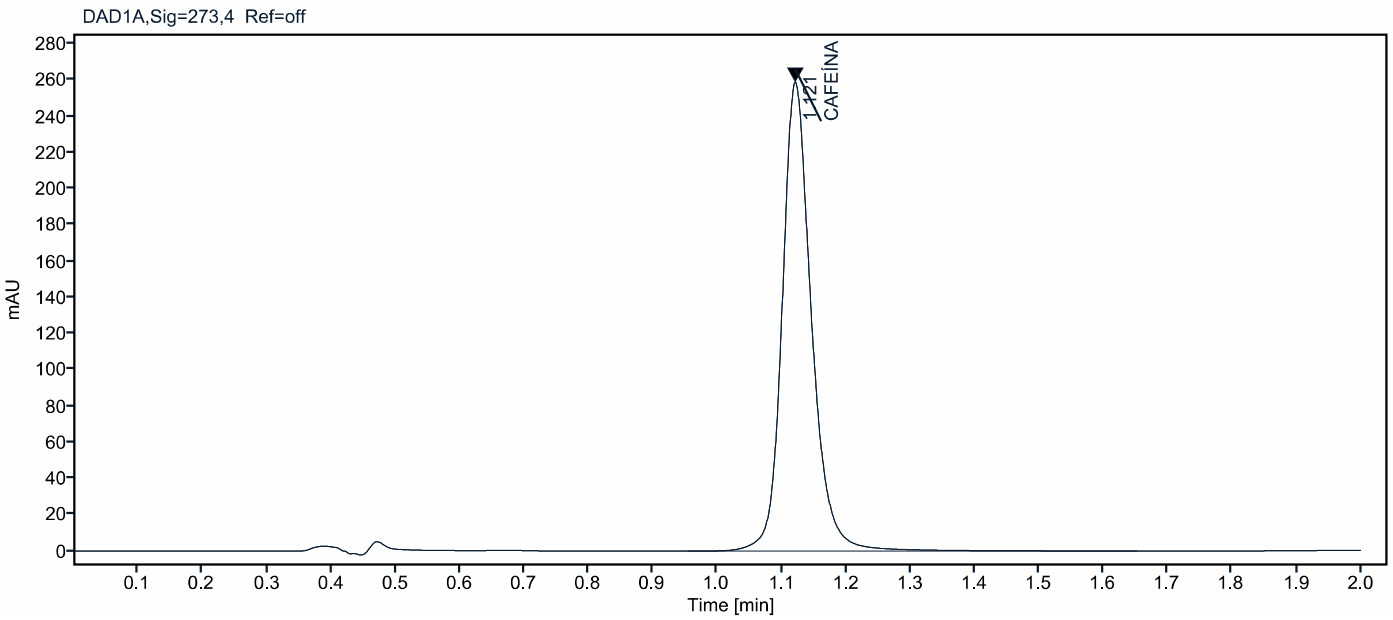

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 05	CAFEÍNA	1.121	823.6893			258.855

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-12-17-03-00-09.dx		
Sample name:	PCIN 06		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A3
Injection date:	2025-03-10 13:13:12-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

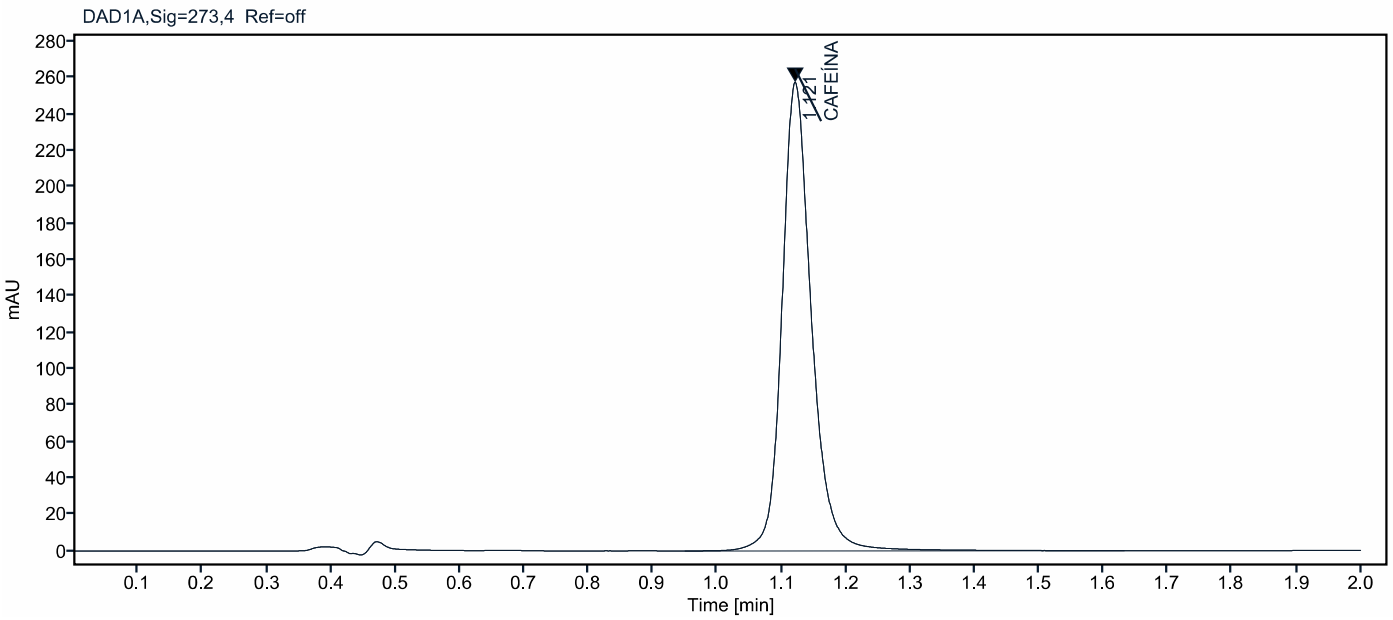

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
PCIN 06	CAFEÍNA	1.121	825.5265			257.831

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-15-15-03-00-10.dx		
Sample name:	BRANCO 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A2
Injection date:	2025-03-10 13:16:09-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

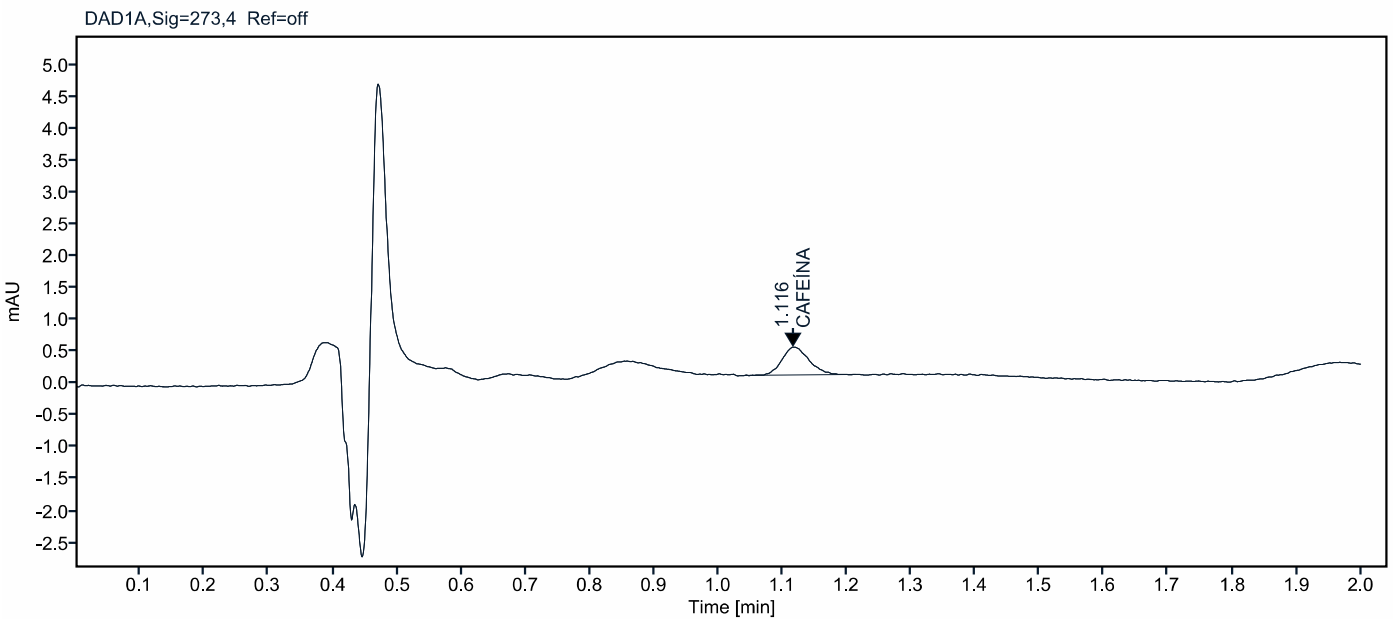

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
BRANCO 03	CAFEÍNA	1.116	1.2664			0.437

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-18-12-03-00-11.dx		
Sample name:	LDUV 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A4
Injection date:	2025-03-10 13:19:06-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

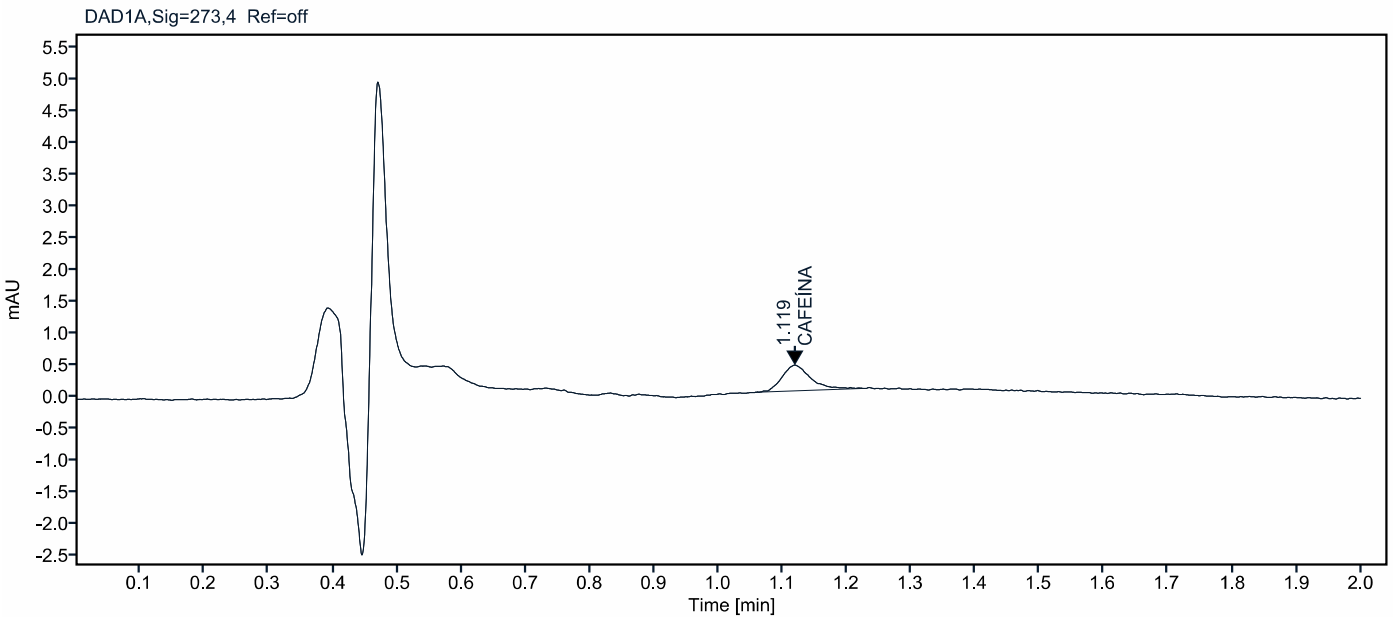

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LDUV 01	CAFEÍNA	1.119	1.2549			0.404

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-21-09-03-00-12.dx		
Sample name:	LDUV 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A5
Injection date:	2025-03-10 13:22:03-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

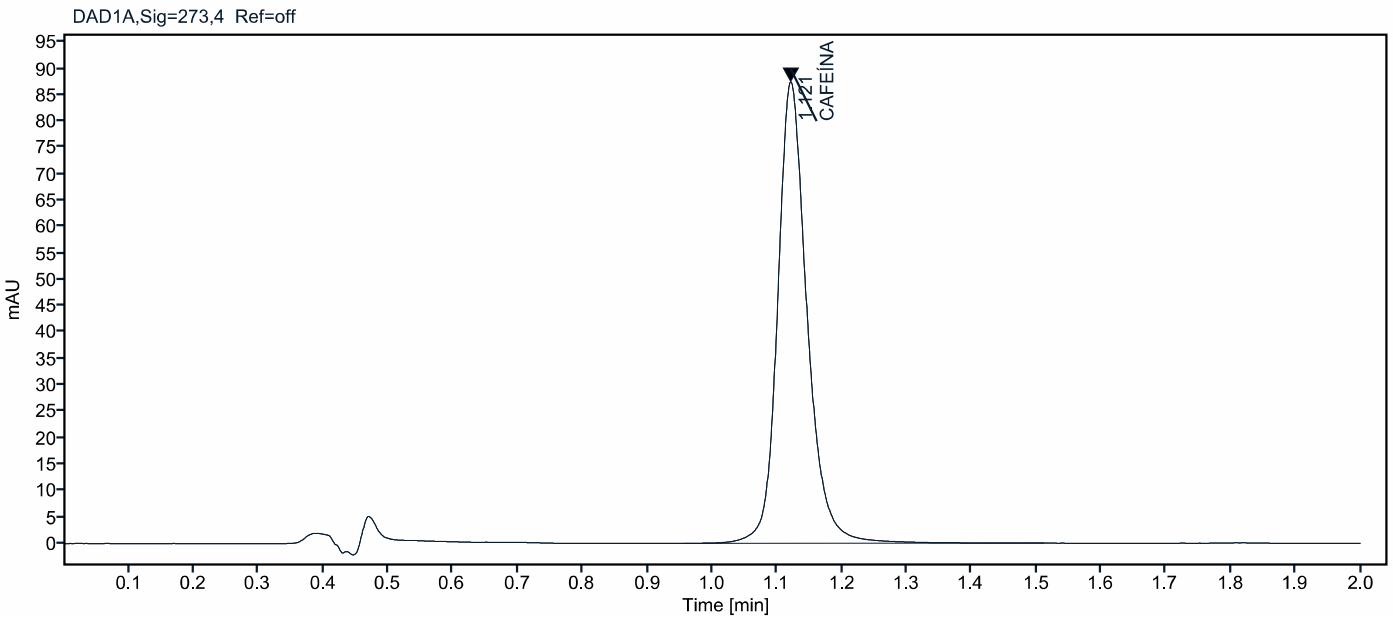

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LDUV 02	CAFEÍNA	1.121	277.9510			87.437

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-24-05-03-00-13.dx		
Sample name:	LDUV 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A6
Injection date:	2025-03-10 13:24:58-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

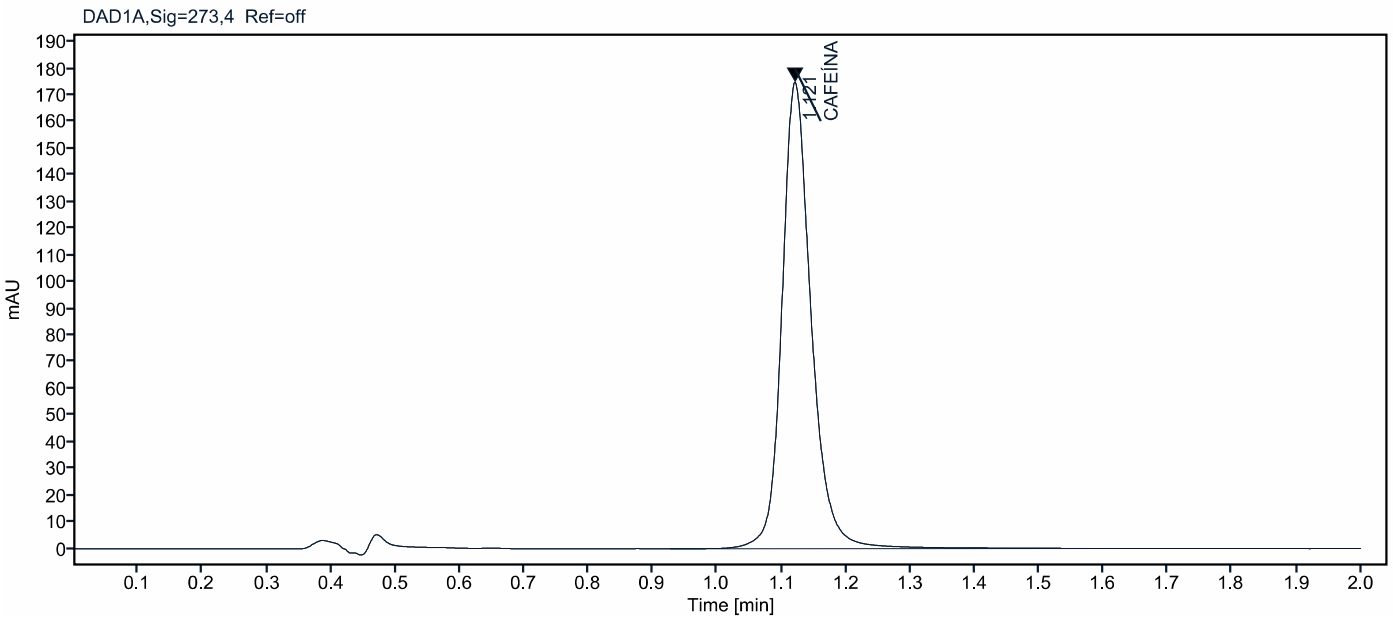

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LDUV 03	CAFEÍNA	1.121	557.1583			174.890

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-27-01-03-00-14.dx		
Sample name:	LDUV 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A7
Injection date:	2025-03-10 13:27:55-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

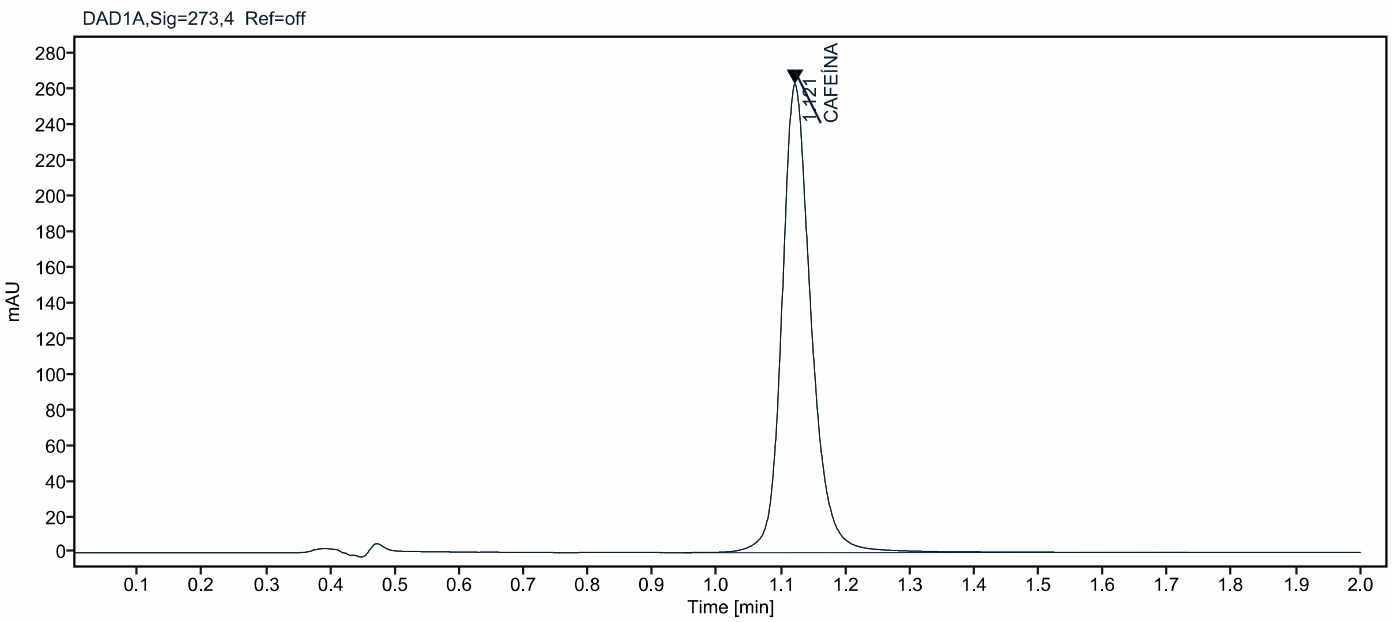

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LDUV 04	CAFEÍNA	1.121	838.8400			262.758

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-29-56-03-00-15.dx		
Sample name:	LDUV 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A8
Injection date:	2025-03-10 13:30:50-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

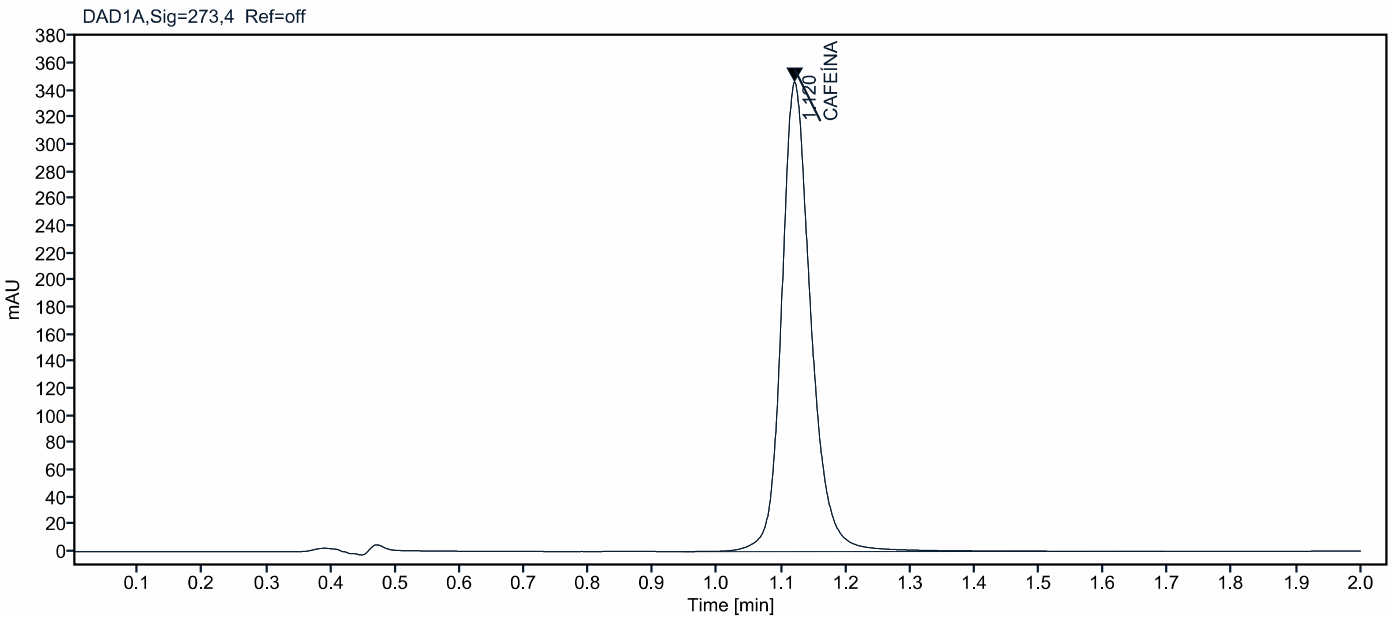

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LDUV 05	CAFEÍNA	1.120	1105.5620			346.260

Single Injection Report

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-32-53-03-00-16.dx		
Sample name:	LIIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A9
Injection date:	2025-03-10 13:33:42-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	0.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

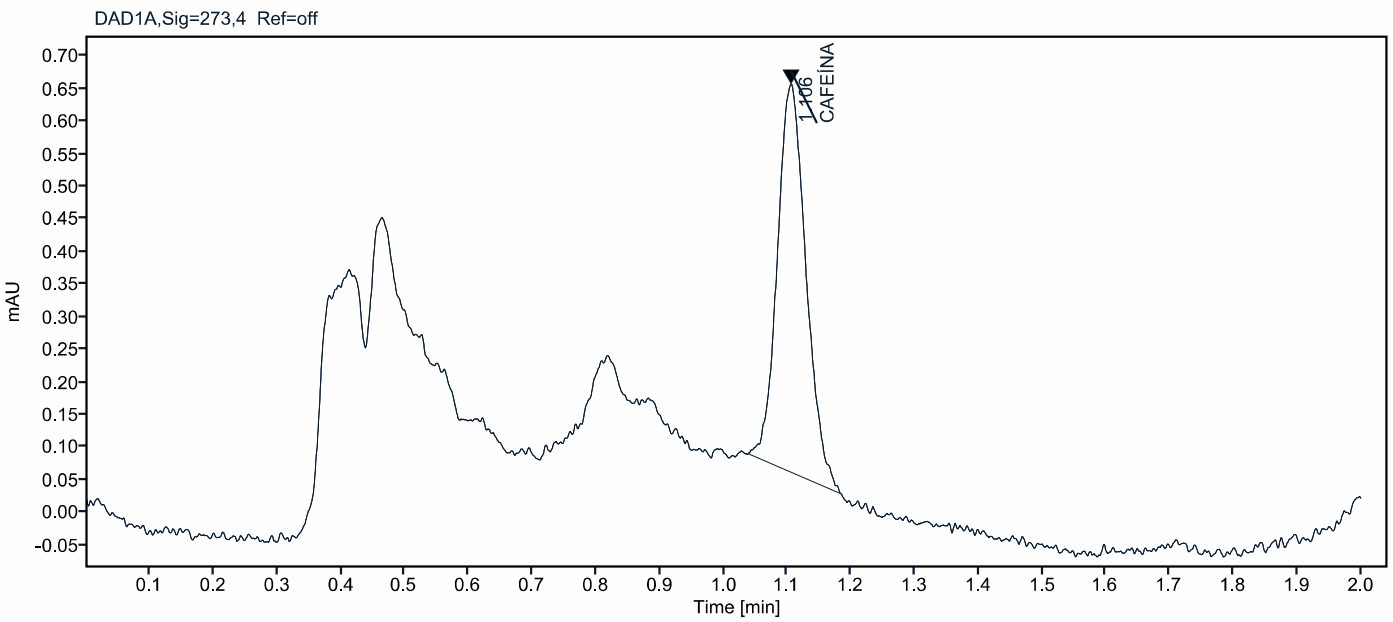


Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LIIN 01	CAFEÍNA	1.106	1.8699			0.596

Single Injection Report

Agilent


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-35-44-03-00-17.dx		
Sample name:	LIIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A9
Injection date:	2025-03-10 13:36:32-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	5.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

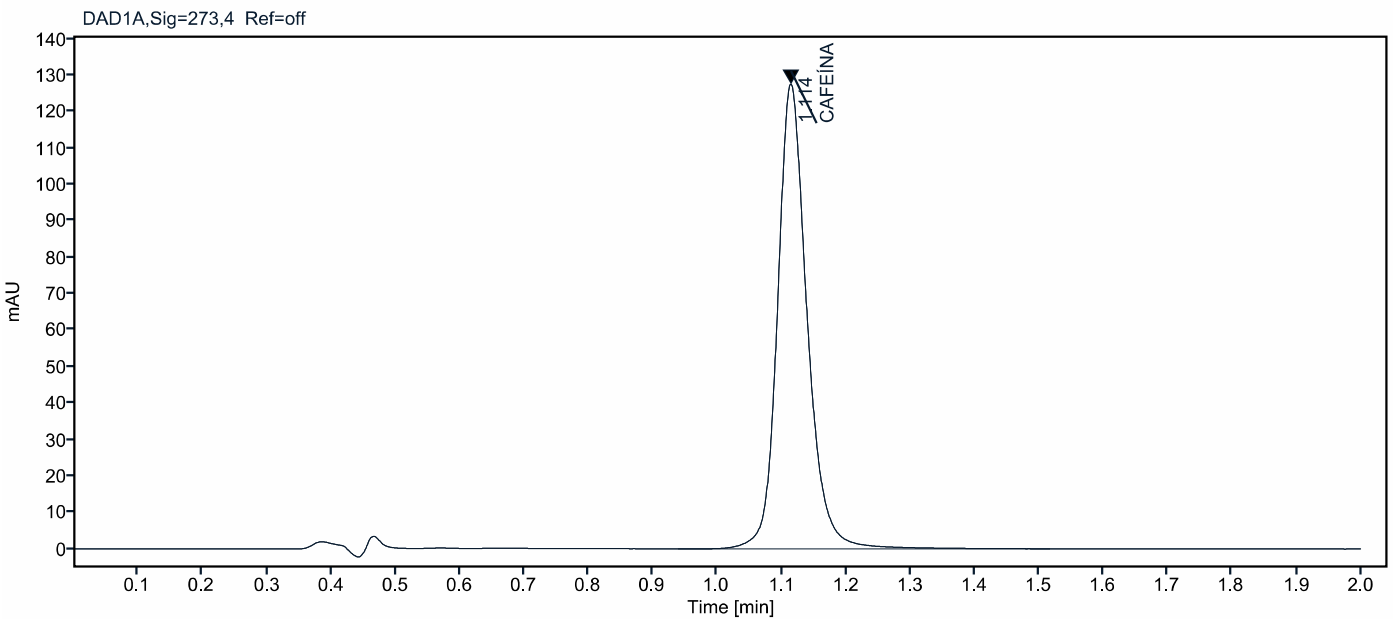

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LIIN 02	CAFEÍNA	1.114	409.6585			127.577

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-38-35-03-00-18.dx		
Sample name:	LIIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A9
Injection date:	2025-03-10 13:39:28-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

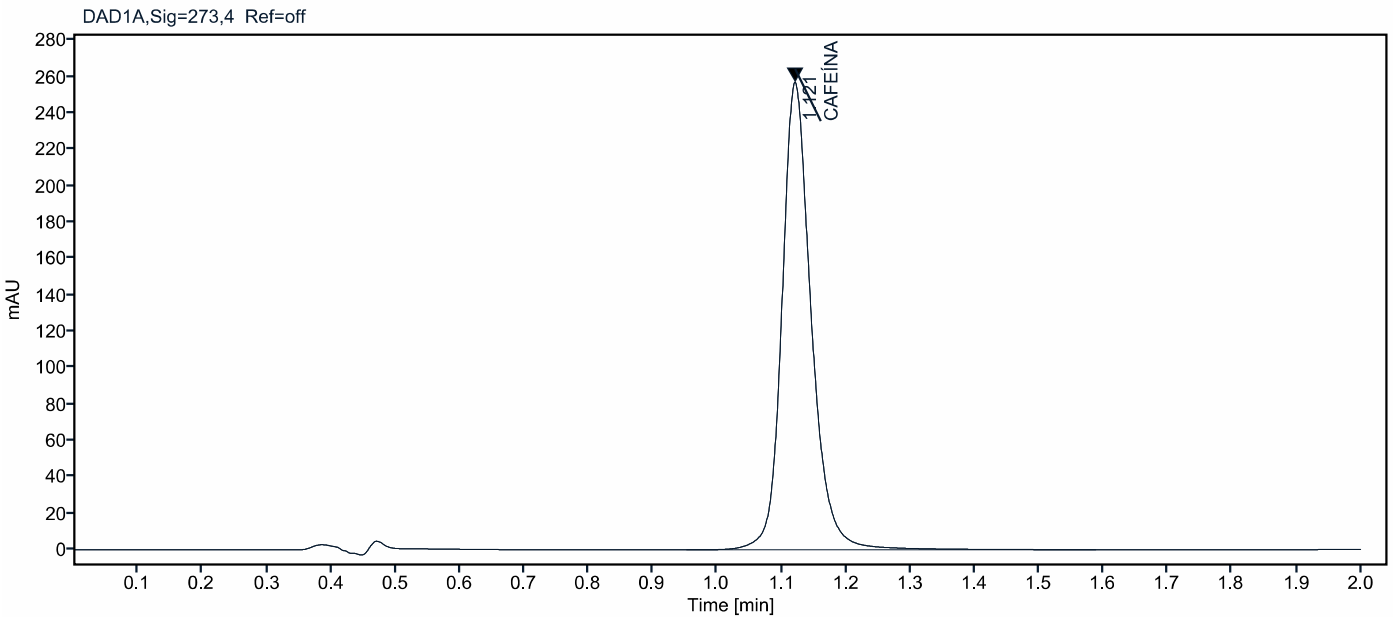

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LIIN 03	CAFEÍNA	1.121	817.3894			256.907

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-41-31-03-00-19.dx		
Sample name:	LIIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A9
Injection date:	2025-03-10 13:42:29-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	15.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

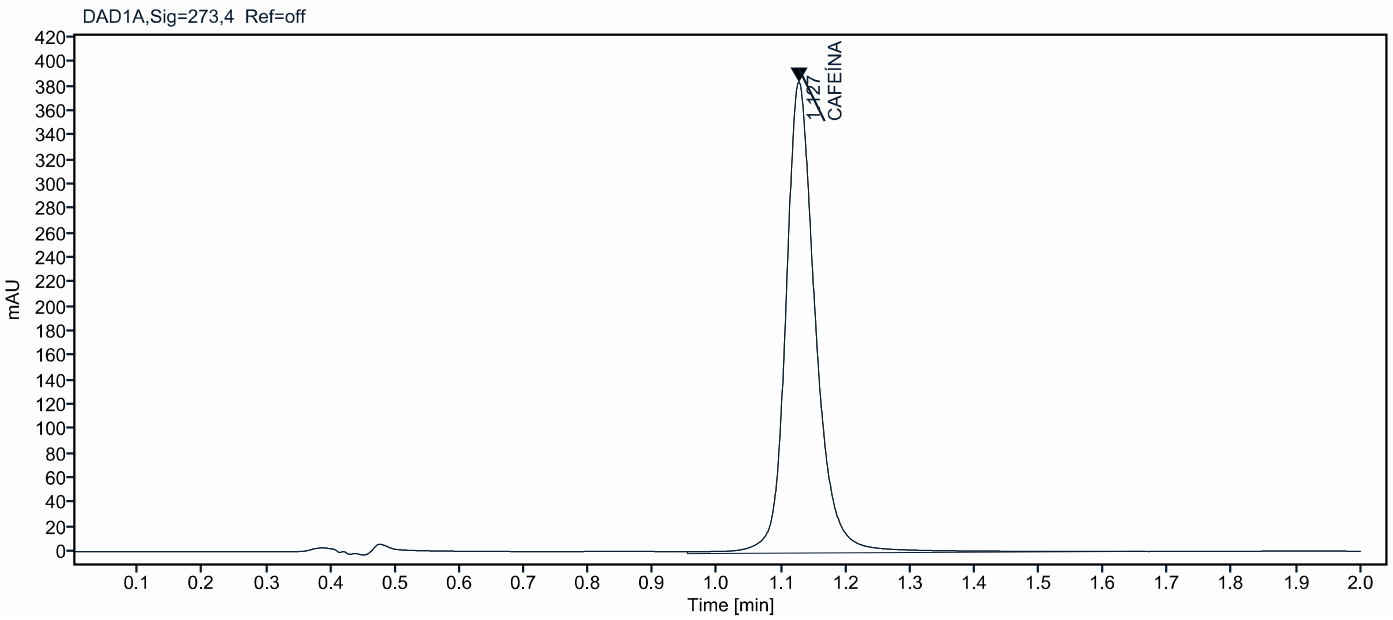

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LIIN 04	CAFEÍNA	1.127	1258.1254			384.994

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 12-48-32-03-00.rslt\2025-03-10 13-44-31-03-00-20.dx		
Sample name:	LIIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A9
Injection date:	2025-03-10 13:45:33-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO 2025.amx	**Injection volume:**	20.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:17:38-03:00		

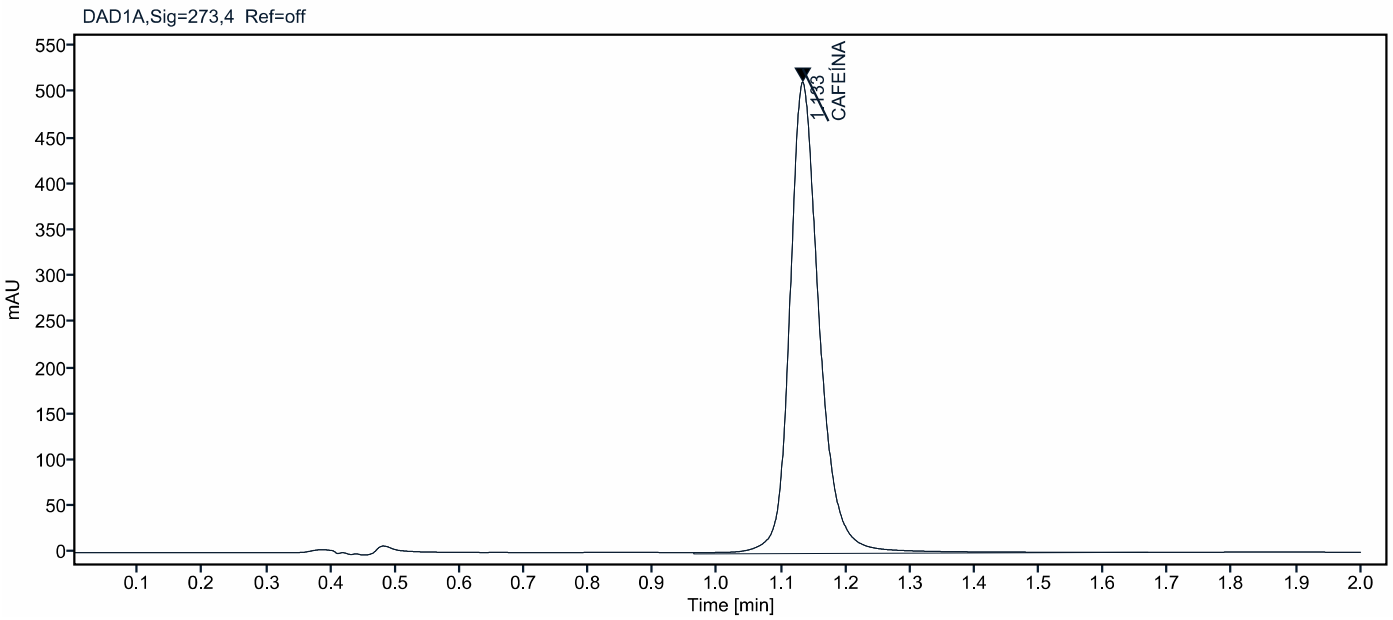

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
LIIN 05	CAFEÍNA	1.133	1663.2899			511.684

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 17-00-44-03-00.rslt\2025-03-10 17-00-52-03-00-21.dx		
Sample name:	RELB		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A10
Injection date:	2025-03-10 17:01:57-03:00	**Injection:**	1 of 1
Acq. method:	RELB 2025.amx	**Injection volume:**	20.000 µL
Analysis method:	QPACK.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:48:21-03:00		

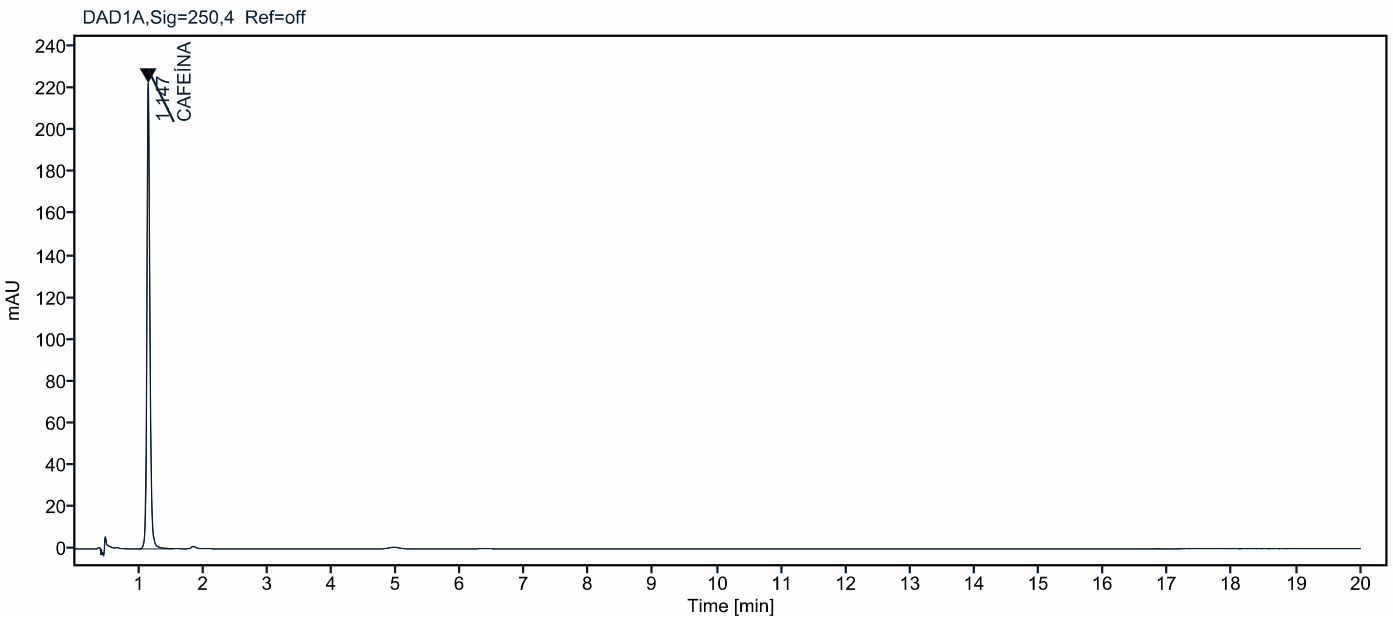

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
RELB	CAFEÍNA	1.147	751.8053			222.834

Single Injection Report

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 17-00-44-03-00.rslt\2025-03-10 17-00-52-03-00-21.dx		
Sample name:	RELB		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A10
Injection date:	2025-03-10 17:01:57-03:00	**Injection:**	1 of 1
Acq. method:	RELB 2025.amx	**Injection volume:**	20.000 µL
Analysis method:	QPACK.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:48:21-03:00		

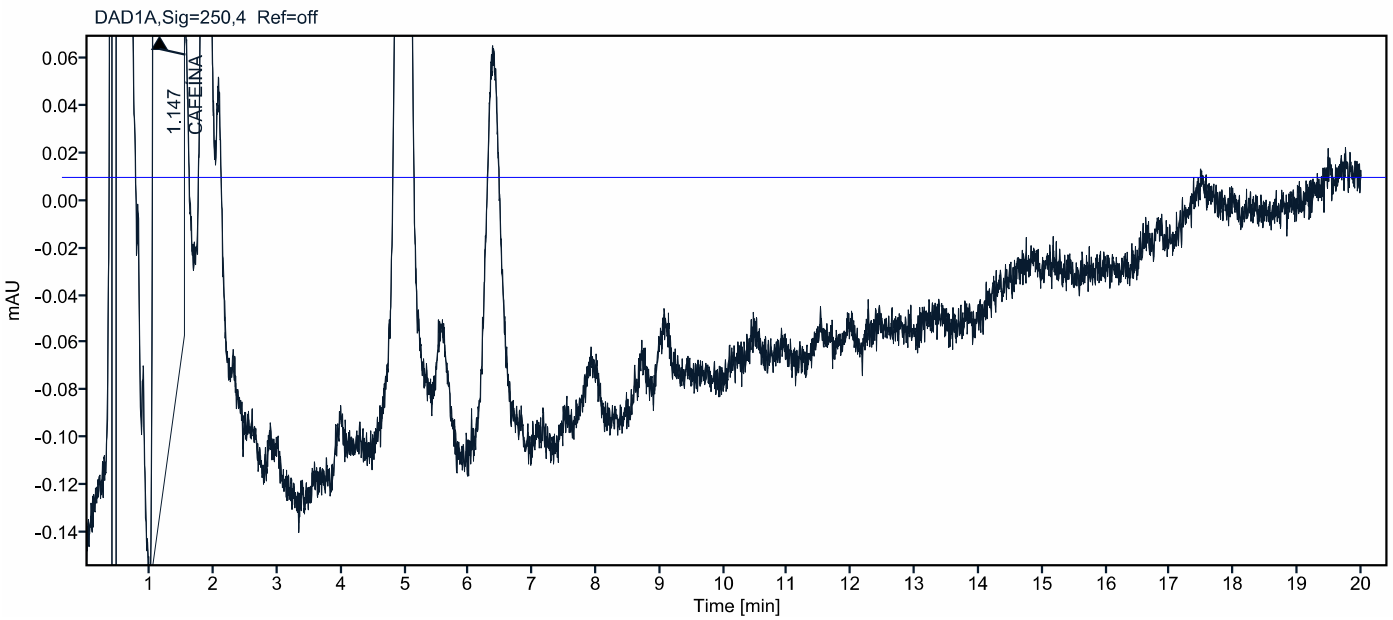


Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
RELB	CAFEÍNA	1.147	751.8053			222.834

Single Injection Report

Agilent

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\CMLI-009-2025-03-10 17-00-44-03-00.rslt\2025-03-10 17-00-52-03-00-21.dx		
Sample name:	RELB		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A10
Injection date:	2025-03-10 17:01:57-03:00	**Injection:**	1 of 1
Acq. method:	RELB 2025.amx	**Injection volume:**	20.000 µL
Analysis method:	QPACK.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-10 17:48:21-03:00		

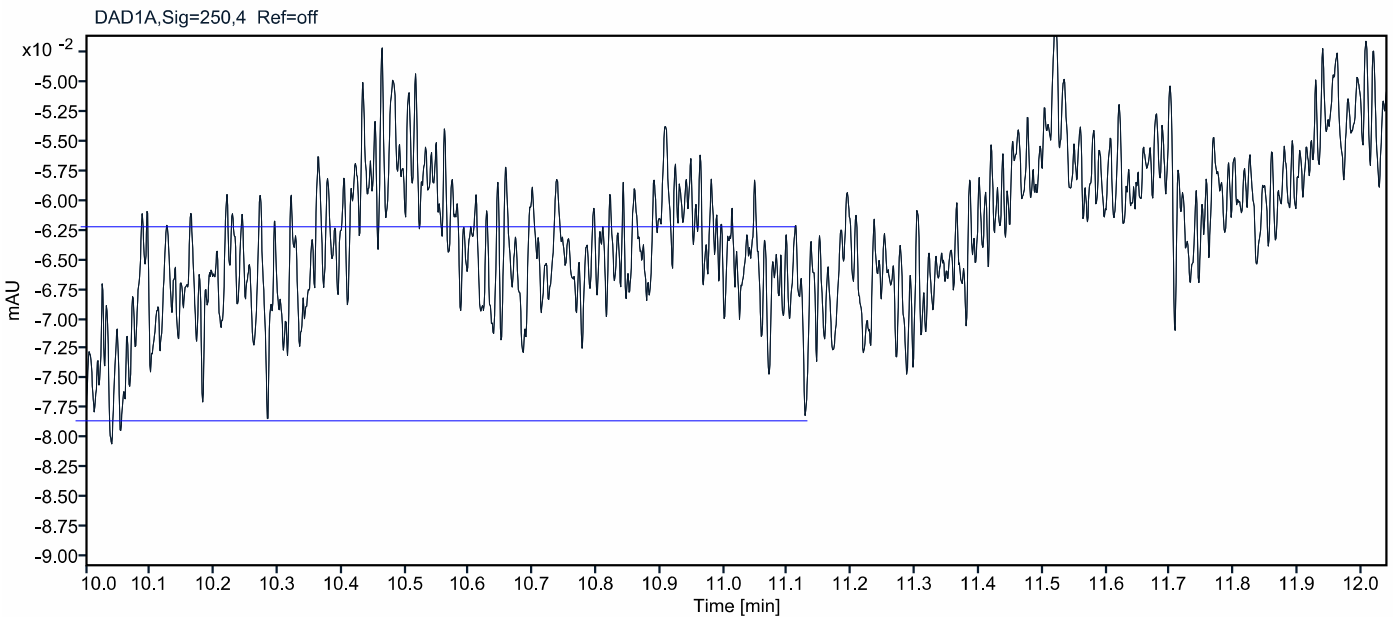


Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
RELB	CAFEÍNA	1.147	751.8053			222.834

Single Injection Report

Agilent

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\GRABO\CMLI-009-2025-03-11 11-11-46-03-00.rslt\2025-03-11 11-11-53-03-00-22.dx		
Sample name:	GRABO AB		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A1
Injection date:	2025-03-11 11:12:51-03:00	**Injection:**	1 of 1
Acq. method:	Gradiente AB.amx	**Injection volume:**	0.000 µL
Analysis method:	*QPACK.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-11 12:42:30-03:00		

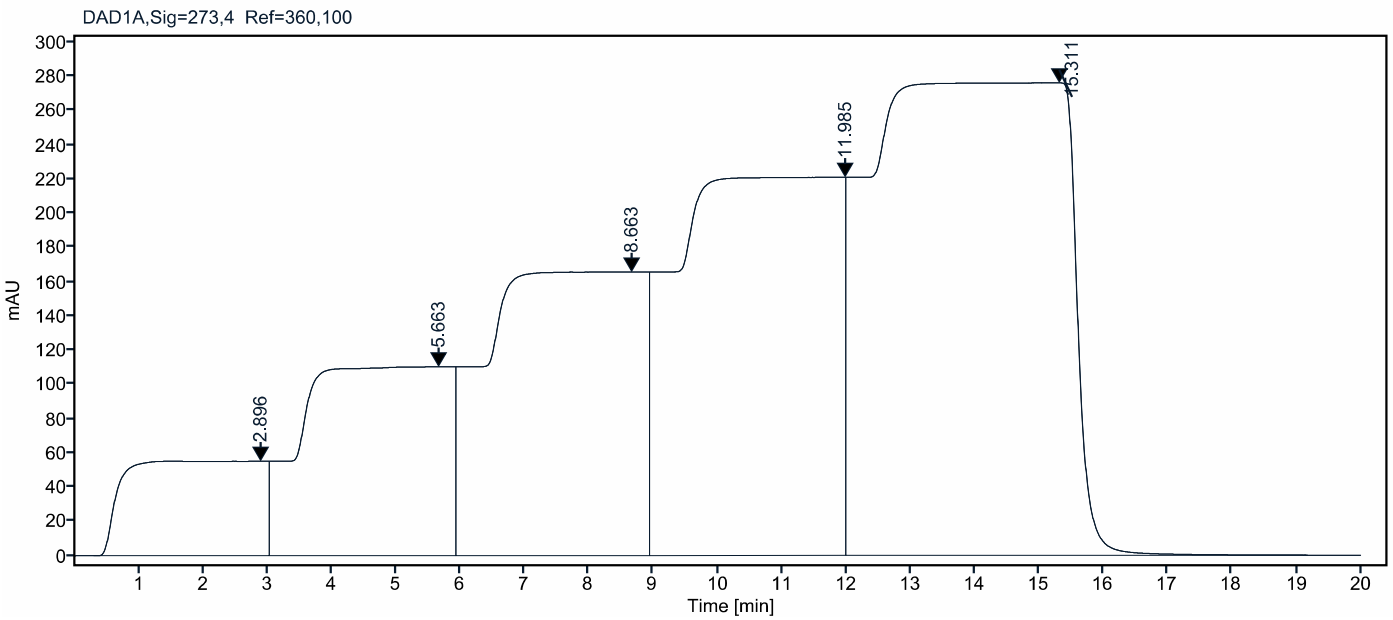


Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
GRABO AB		2.896	7930.5270			55.176
GRABO AB		5.663	17199.2810			110.391
GRABO AB		8.663	27622.9675			165.761
GRABO AB		11.985	38154.5785			220.995
GRABO AB		15.311	58219.9109			276.121

Single Injection Report

Agilent

Data file:	C:\CDSProjects\Agilent\Results\QUALIFIÇÃO 2025\GRABO\CMLI-009-2025-03-11 11-11-46-03-00.rslt\2025-03-11 11-53-53-03-00-24.dx		
Sample name:	GRABO CD		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI-009	**Location:**	P1-A1
Injection date:	2025-03-11 11:54:51-03:00	**Injection:**	1 of 1
Acq. method:	Gradiente CD.amx	**Injection volume:**	0.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2025-03-11 12:49:31-03:00		

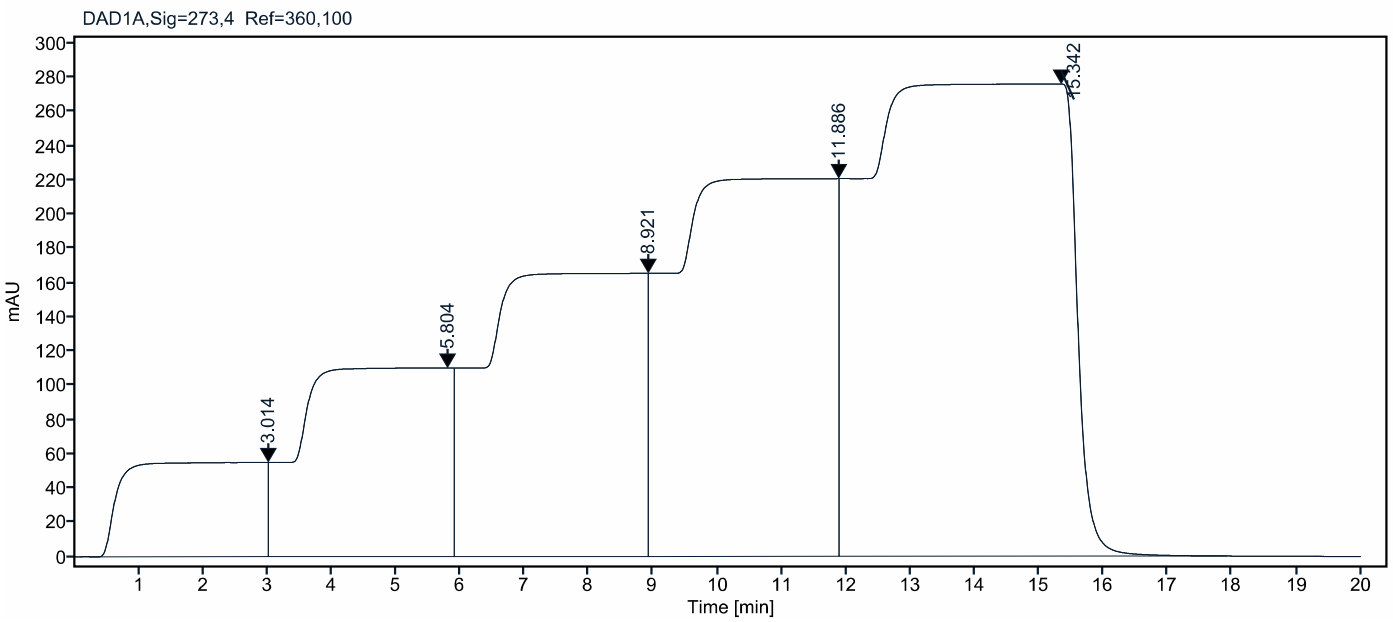

Sample Name	Name	RT	Area	Noise	Signal To Noise	Height
GRABO CD		3.014	7853.9709			55.075
GRABO CD		5.804	17085.6248			110.204
GRABO CD		8.921	27527.6410			165.476
GRABO CD		11.886	36923.9340			220.712
GRABO CD		15.342	59494.4822			275.884