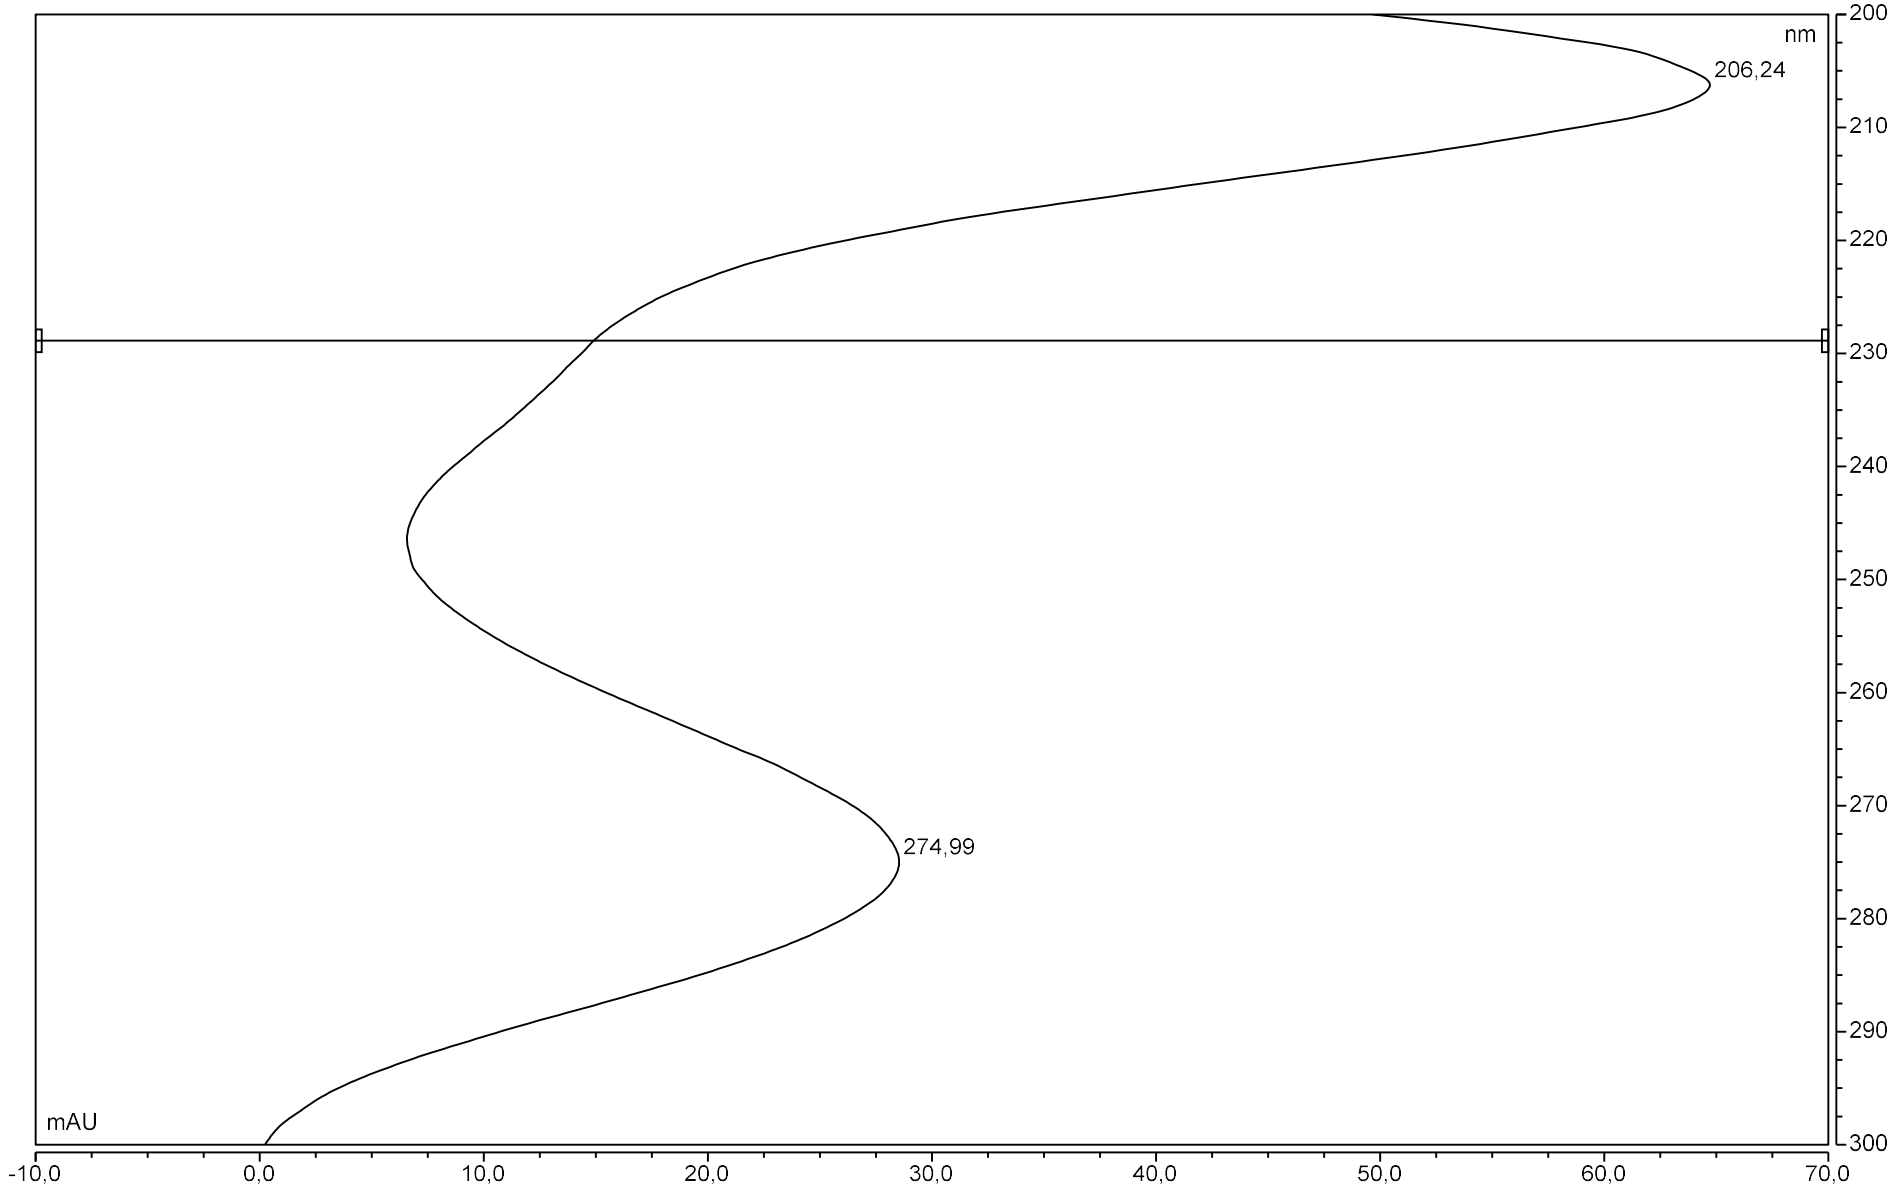
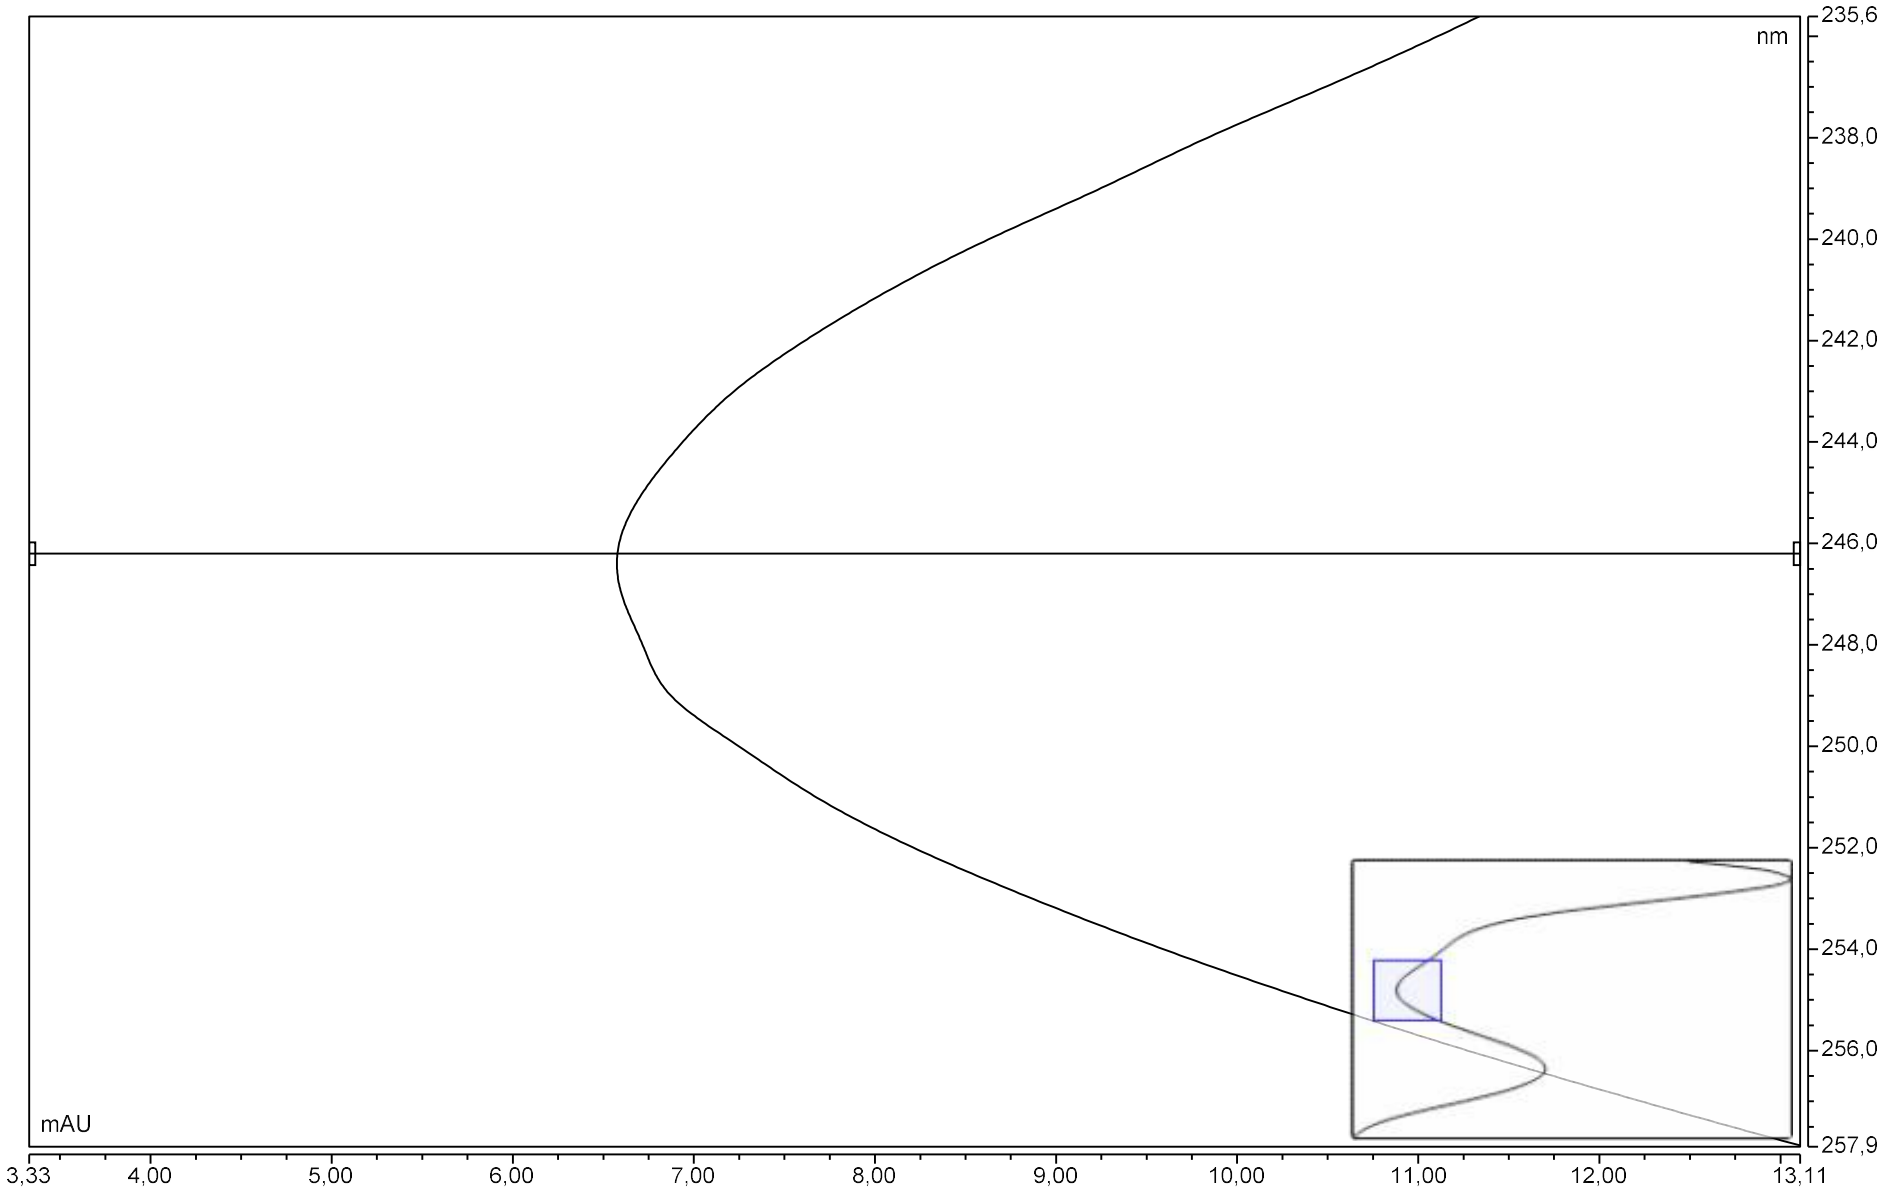

nm
206,24
274,99
mAU
200
210
220
230
240
250
260
270
280
290
300
-10,0
0,0
10,0
20,0
30,0
40,0
50,0
60,0
70,0



nm
235,6
238,0
240,0
242,0
244,0
246,0
248,0
250,0
252,0
254,0
256,0
257,9
mAU
3,33
4,00
5,00
6,00
7,00
8,00
9,00
10,00
11,00
12,00
13,11

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BA7**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**1**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 11:53**	*Sample Weight:*	**1,0000**

Chromatogram

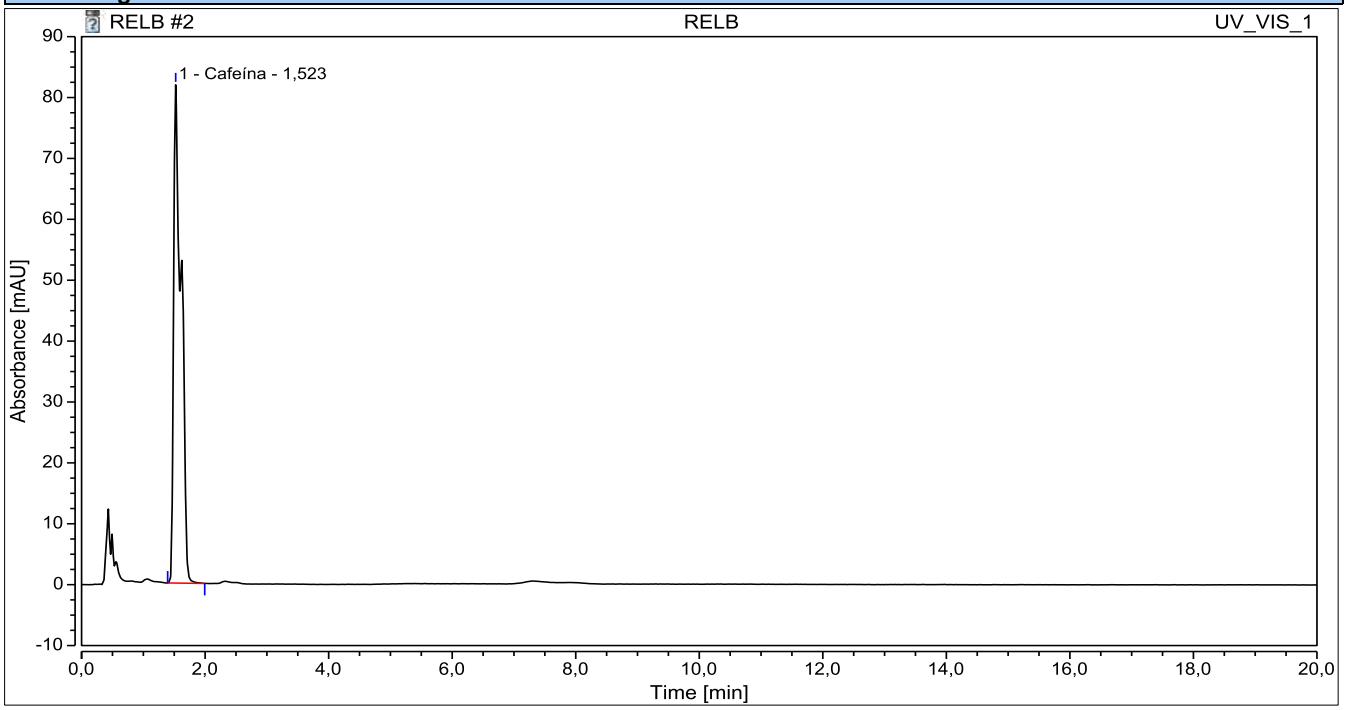

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,523	11,5908	81,821	100,00	100,00	n.a.
Total:			**11,591**	**81,821**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BA7**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**1**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 11:53**	*Sample Weight:*	**1,0000**

Chromatogram

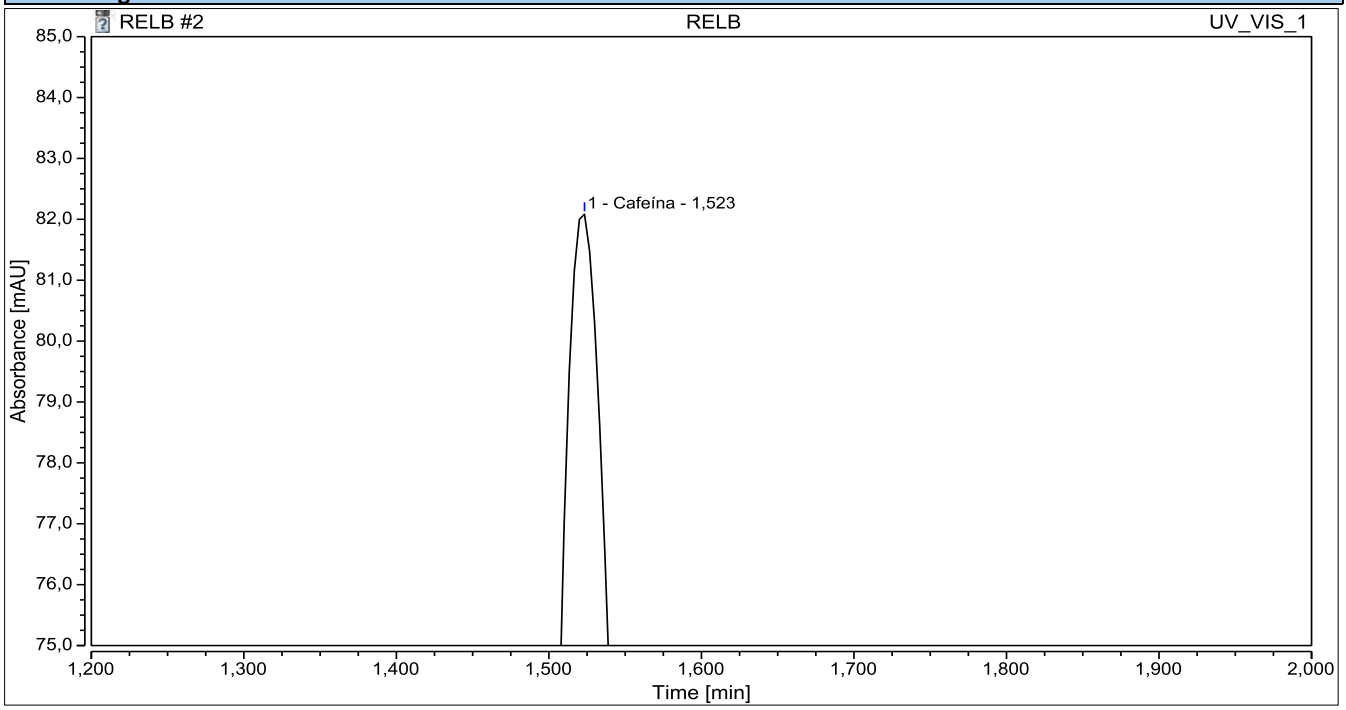

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,523	11,5908	81,821	100,00	100,00	n.a.
Total:			**11,591**	**81,821**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BA7**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**1**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 11:53**	*Sample Weight:*	**1,0000**

Chromatogram

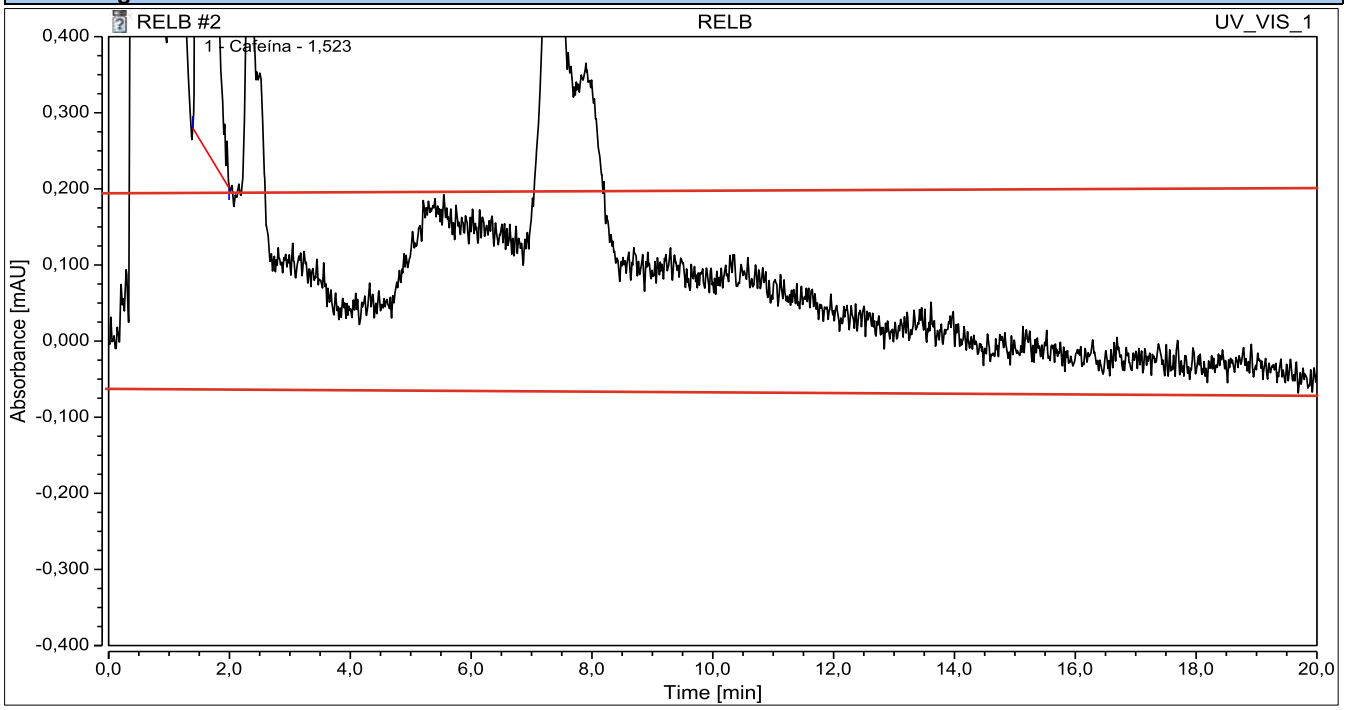

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,523	11,5908	81,821	100,00	100,00	n.a.
Total:			**11,591**	**81,821**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BA7**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**1**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 11:53**	*Sample Weight:*	**1,0000**

Chromatogram

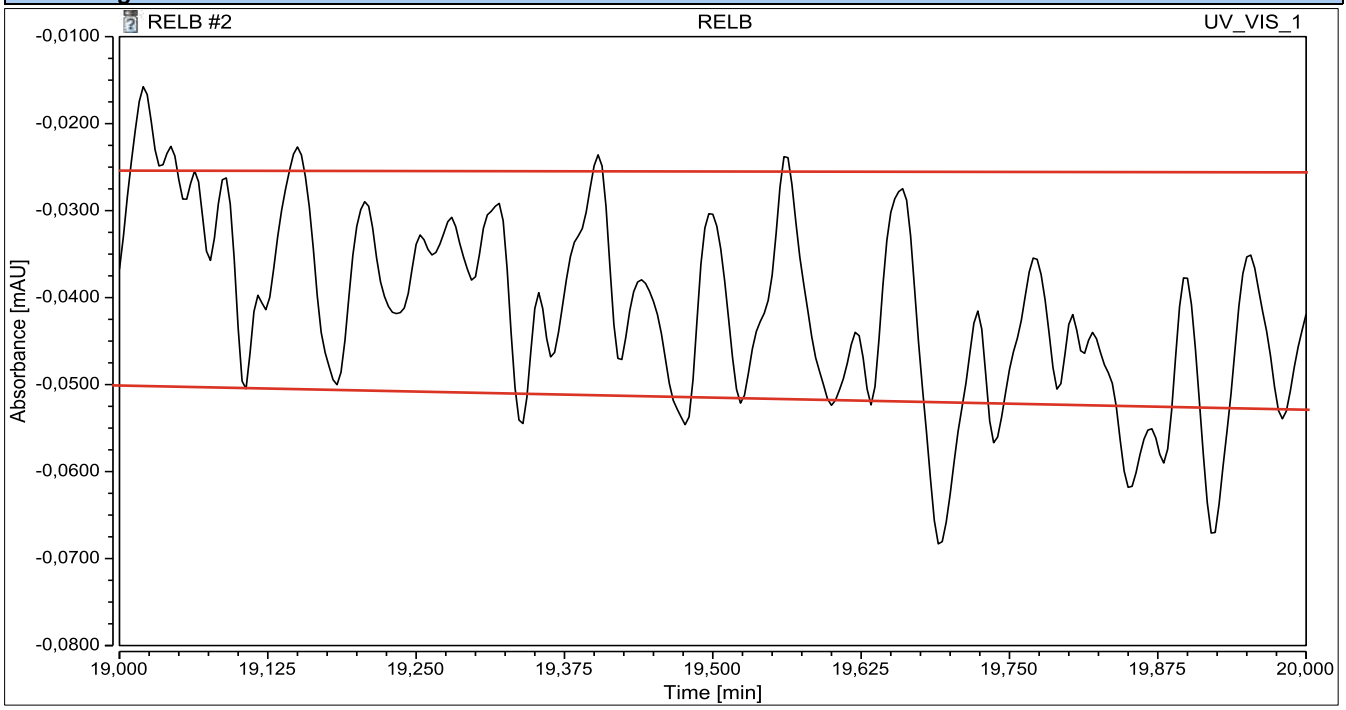

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,523	11,5908	81,821	100,00	100,00	n.a.
Total:			**11,591**	**81,821**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**2,50**
Vial Number:	**BA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 14:28**	*Sample Weight:*	**1,0000**

Chromatogram

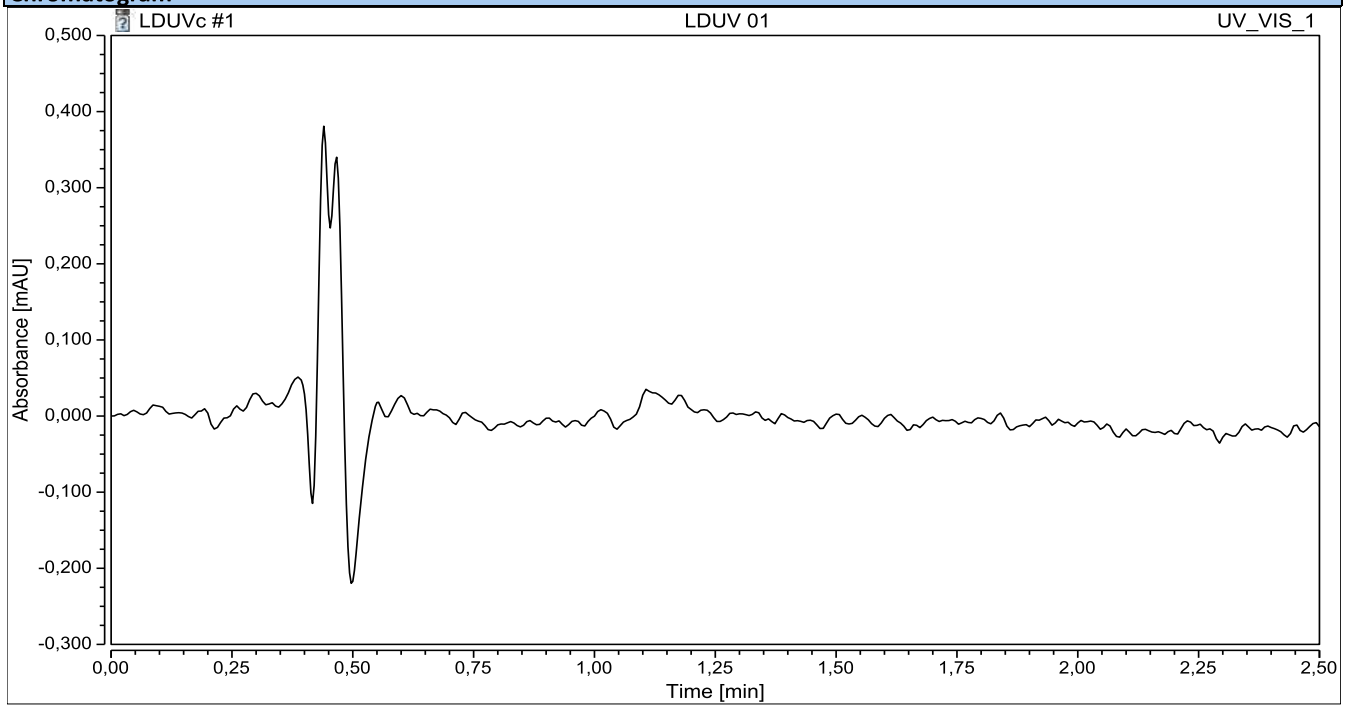

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**2,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 14:32**	*Sample Weight:*	**1,0000**

Chromatogram

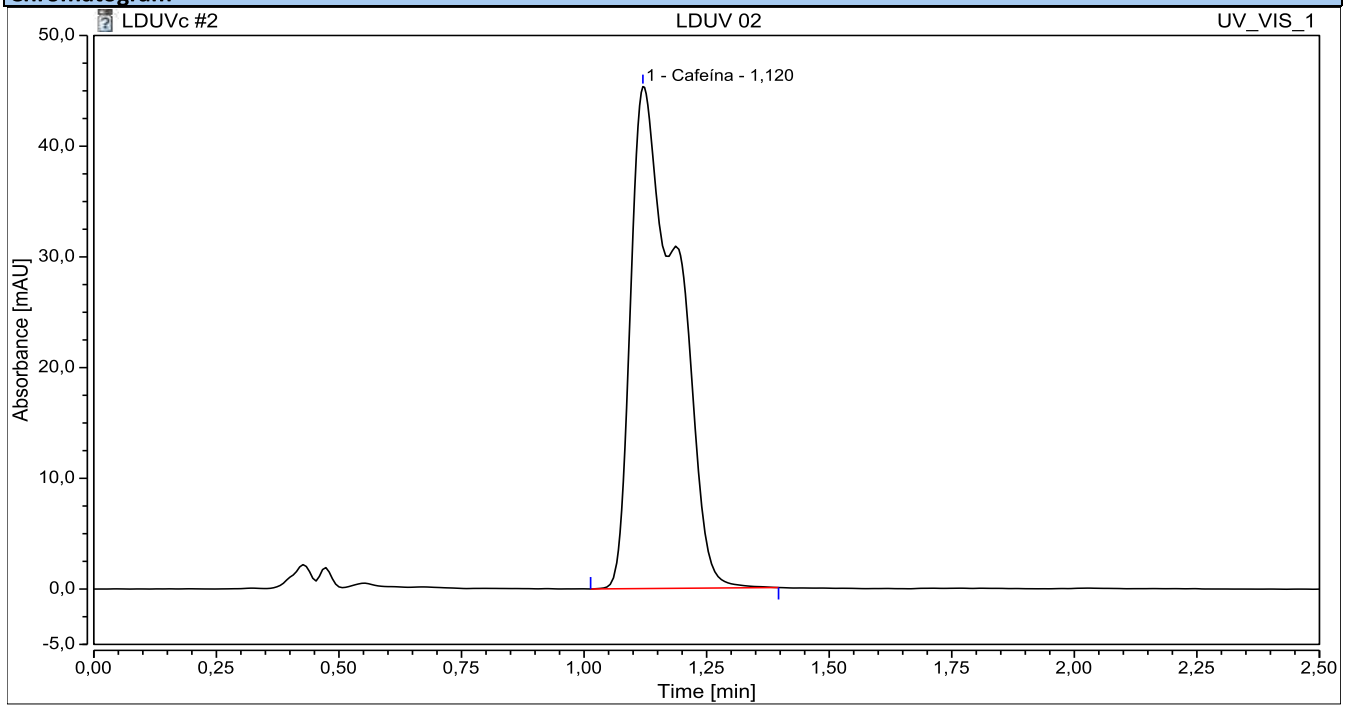

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,120	4,9637	45,344	100,00	100,00	n.a.
Total:			**4,964**	**45,344**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**2,50**
Vial Number:	**BA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 14:35**	*Sample Weight:*	**1,0000**

Chromatogram

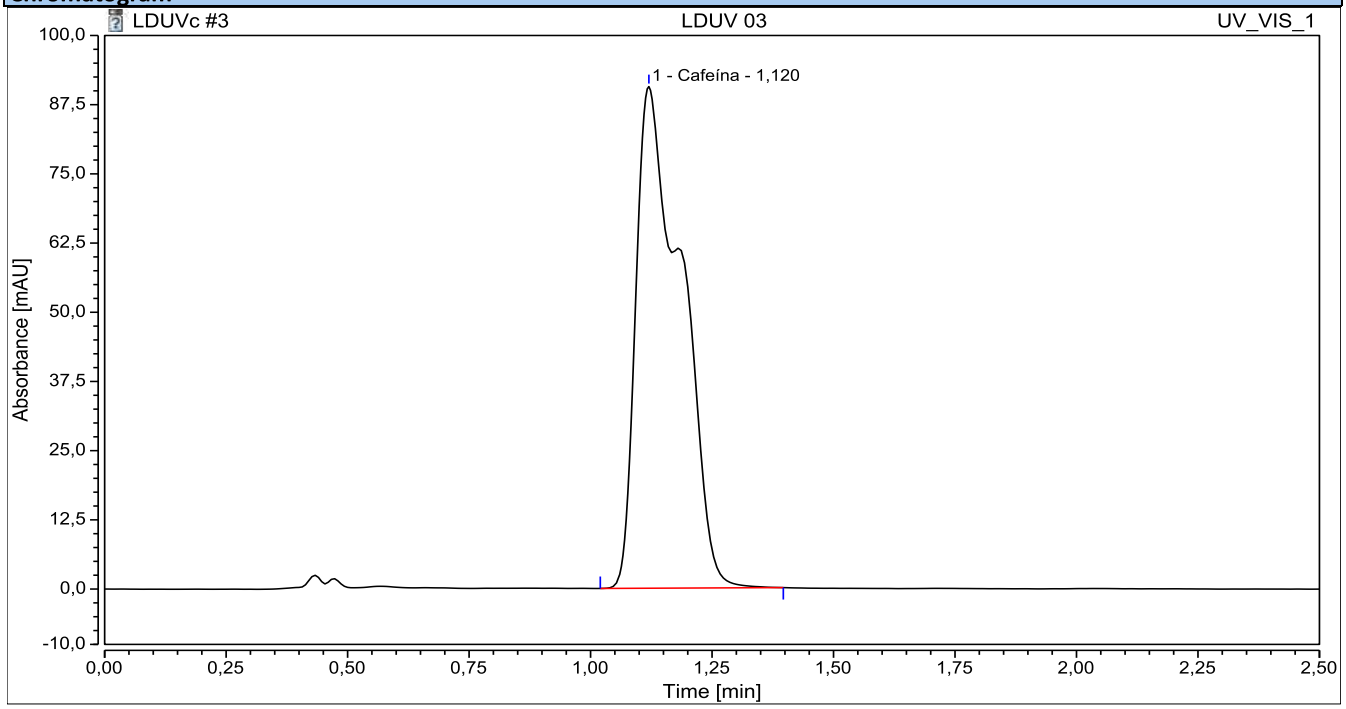

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,120	9,8166	90,626	100,00	100,00	n.a.
Total:			**9,817**	**90,626**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**2,50**
Vial Number:	**BA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 14:38**	*Sample Weight:*	**1,0000**

Chromatogram

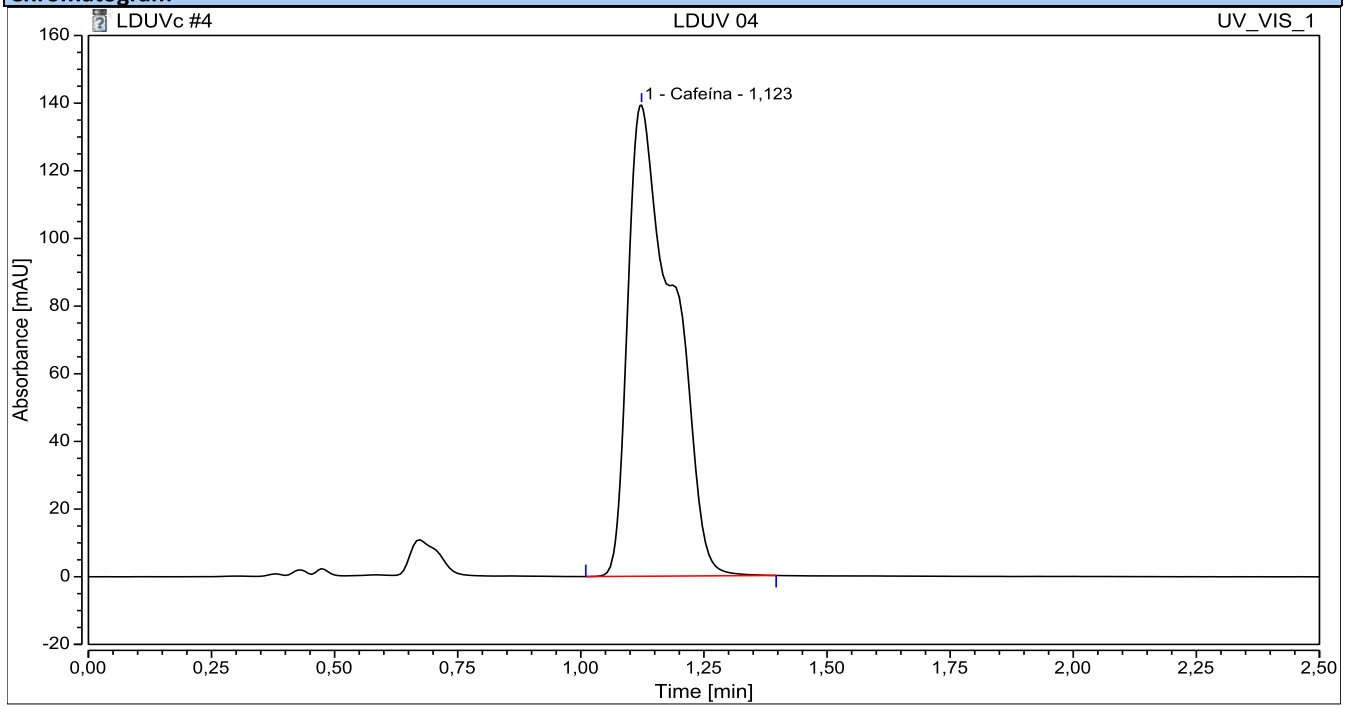

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,123	14,8270	139,279	100,00	100,00	n.a.
Total:			**14,827**	**139,279**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**2,50**
Vial Number:	**BA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**RELB**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 14:42**	*Sample Weight:*	**1,0000**

Chromatogram

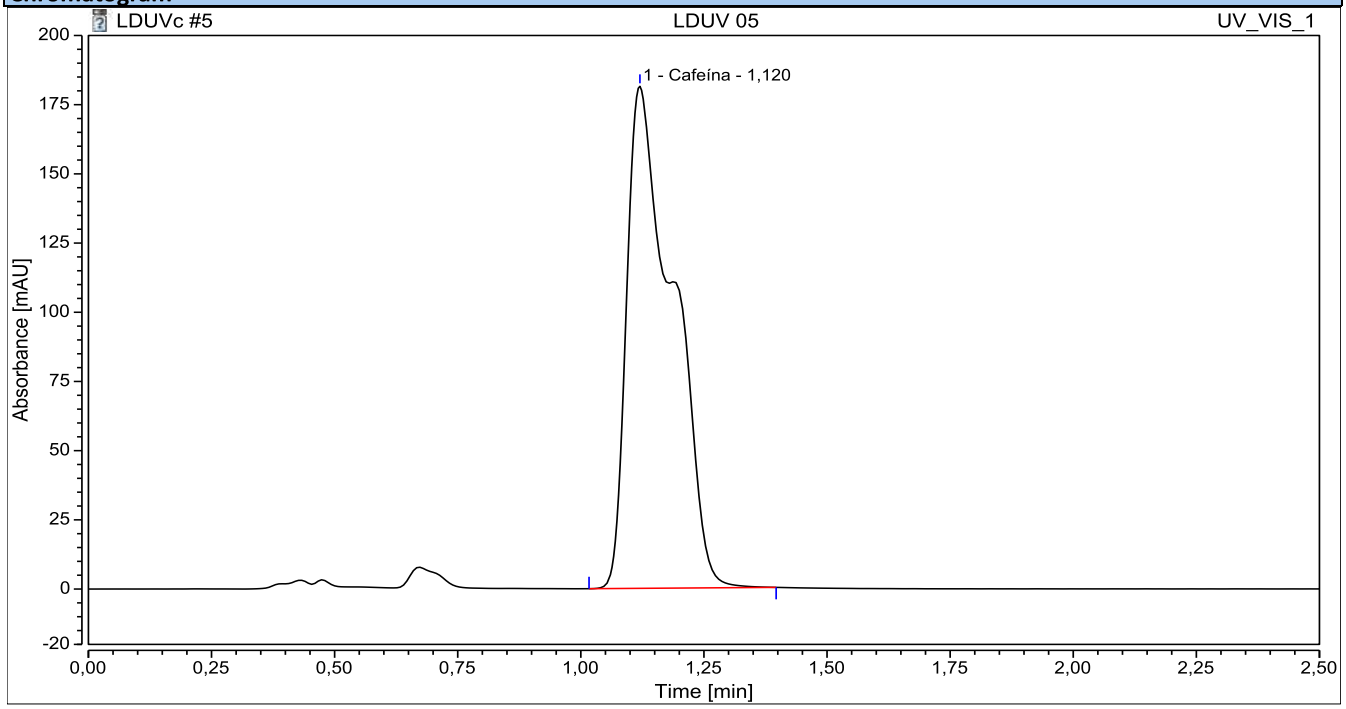

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,120	19,7401	181,393	100,00	100,00	n.a.
Total:			**19,740**	**181,393**	**100,000**	**100,000**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.