

Contour Spectral View

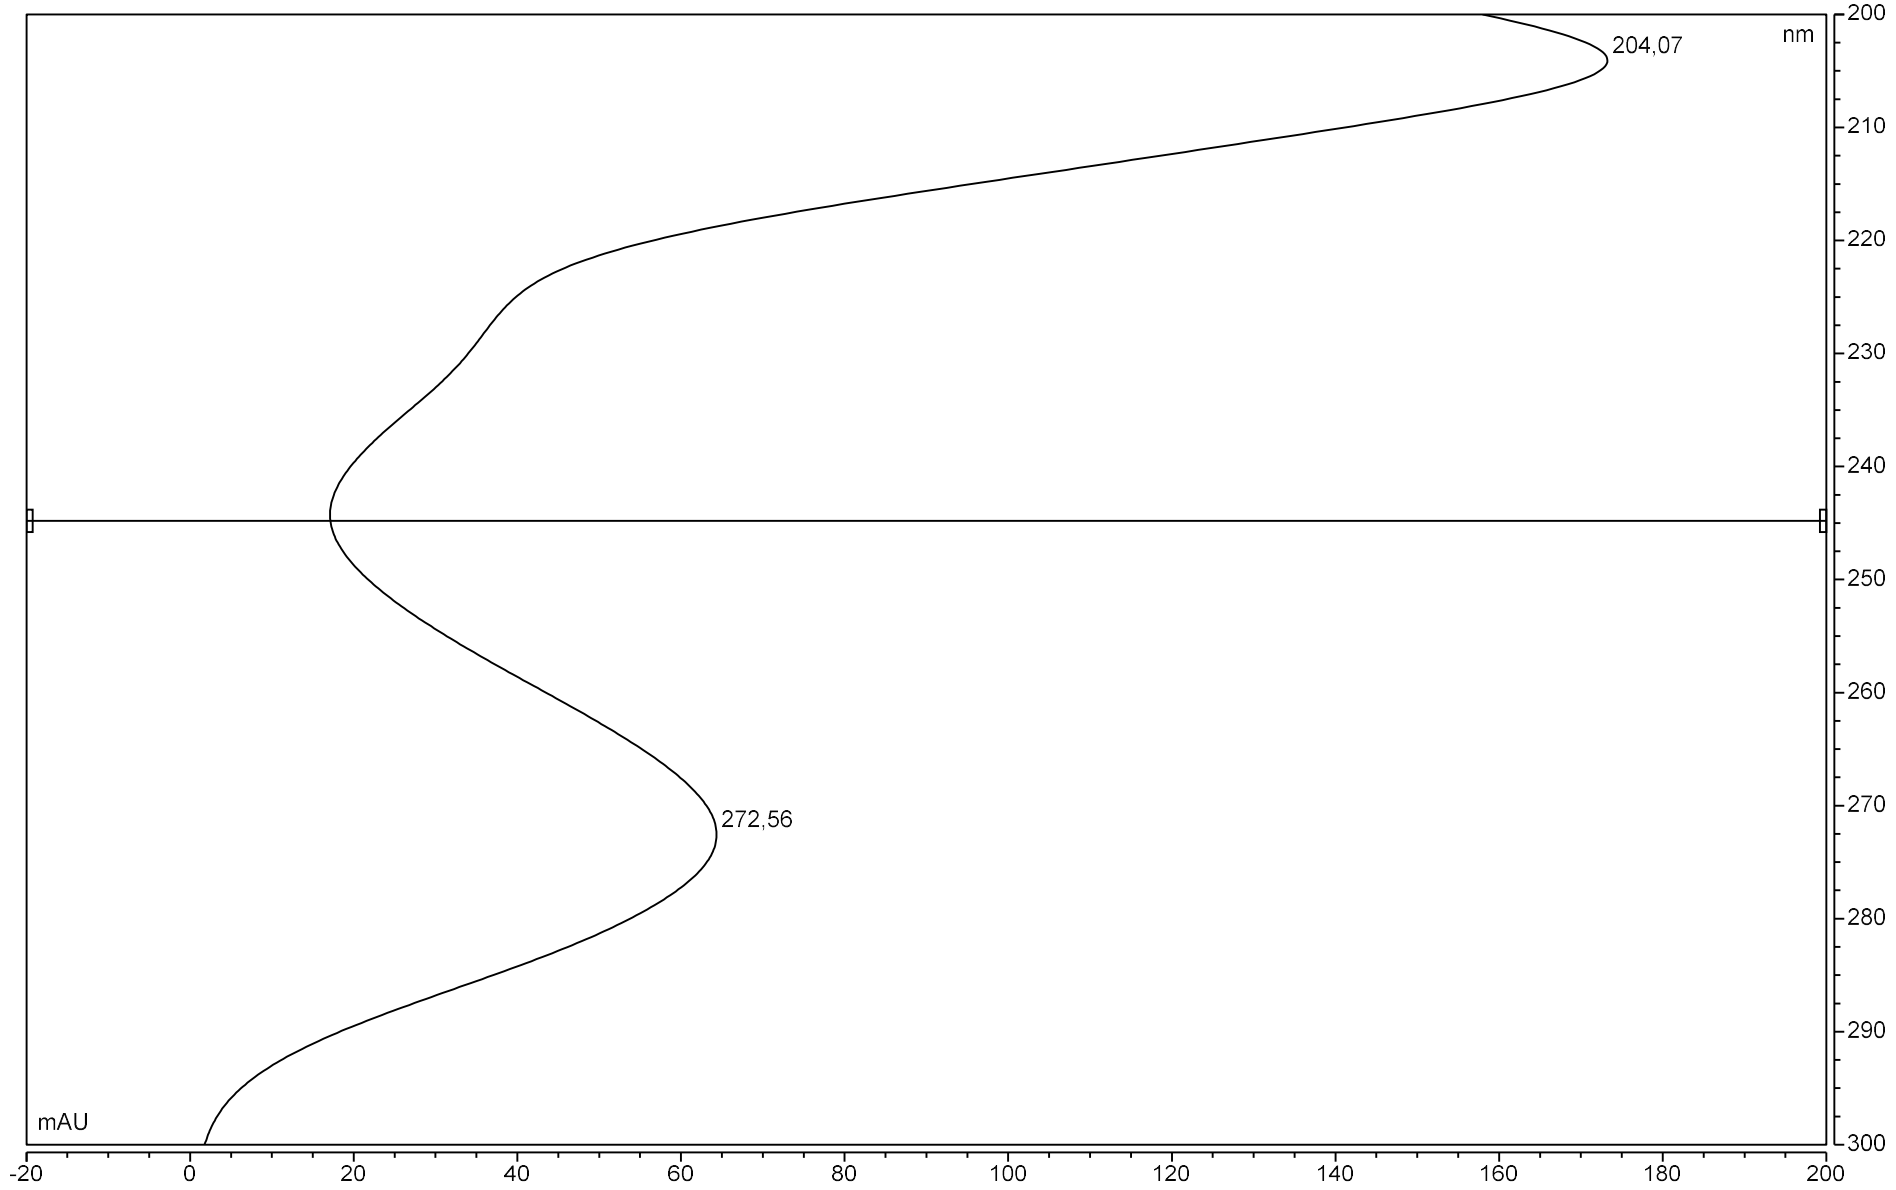

Contour Spectral View

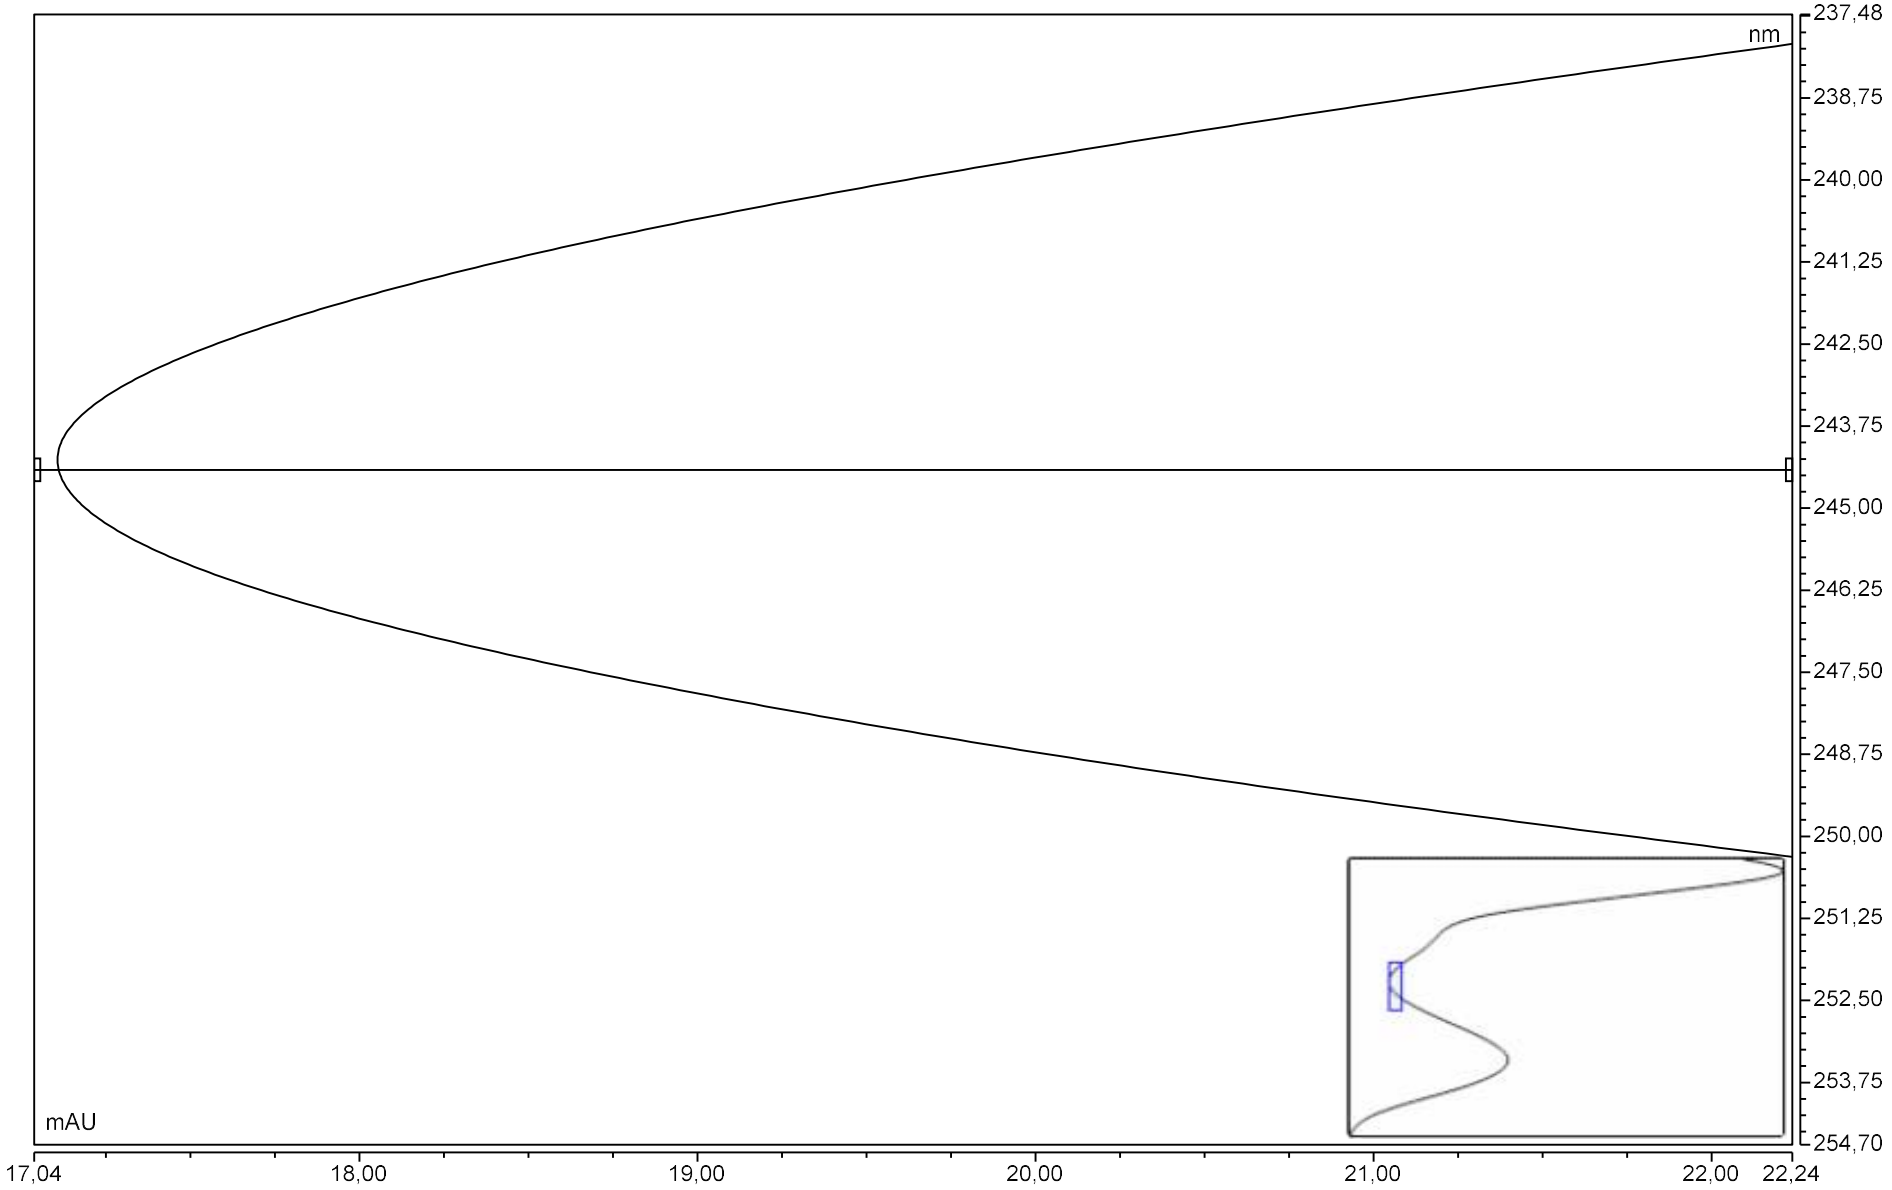


Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 16:36**	*Sample Weight:*	**1,0000**

Chromatogram

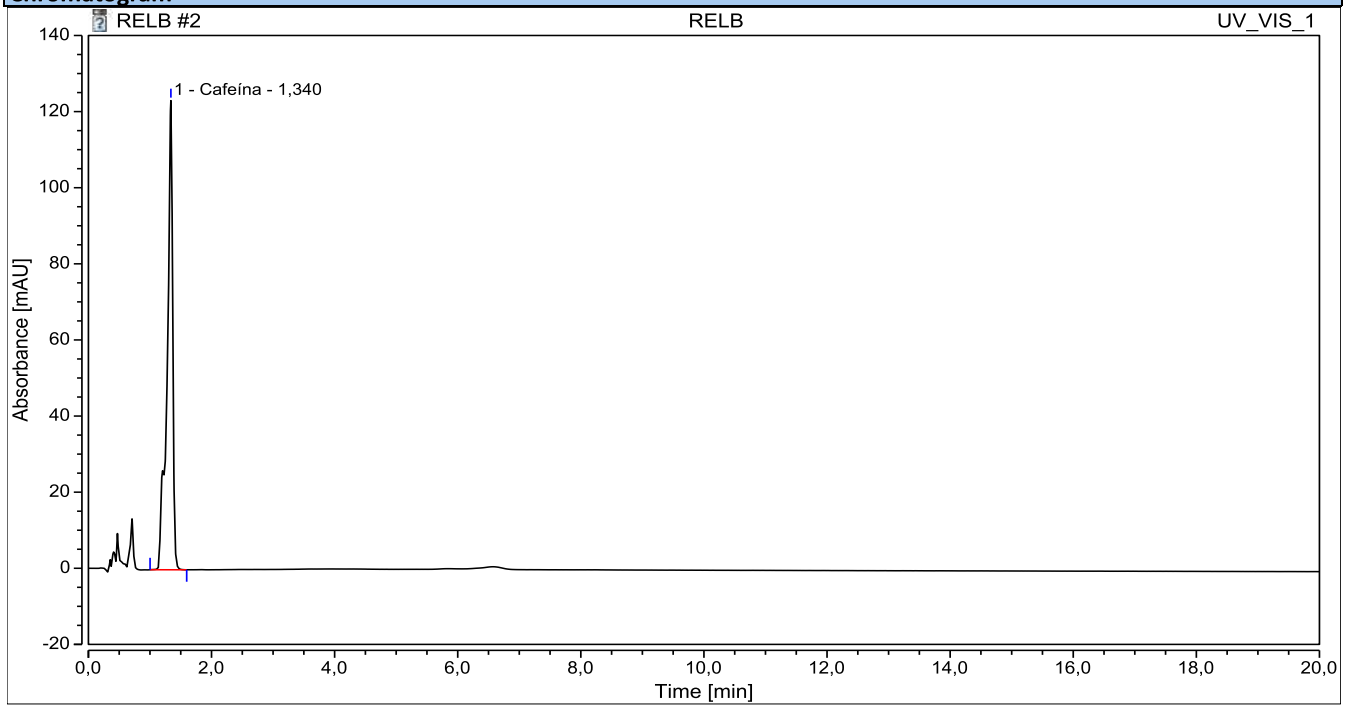

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,340	12,7863	123,275	100,00	100,00	n.a.
Total:			**12,786**	**123,275**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 16:36**	*Sample Weight:*	**1,0000**

Chromatogram

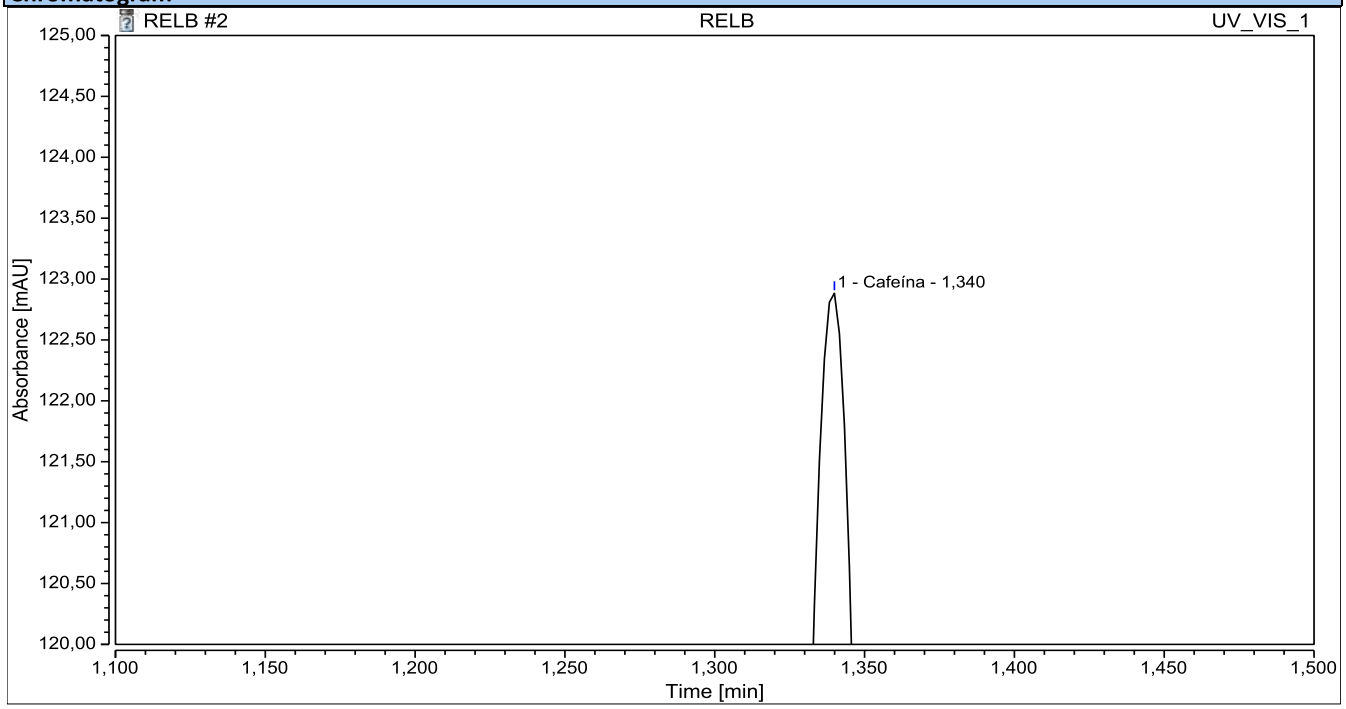

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,340	12,7863	123,275	100,00	100,00	n.a.
Total:			**12,786**	**123,275**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 16:36**	*Sample Weight:*	**1,0000**

Chromatogram

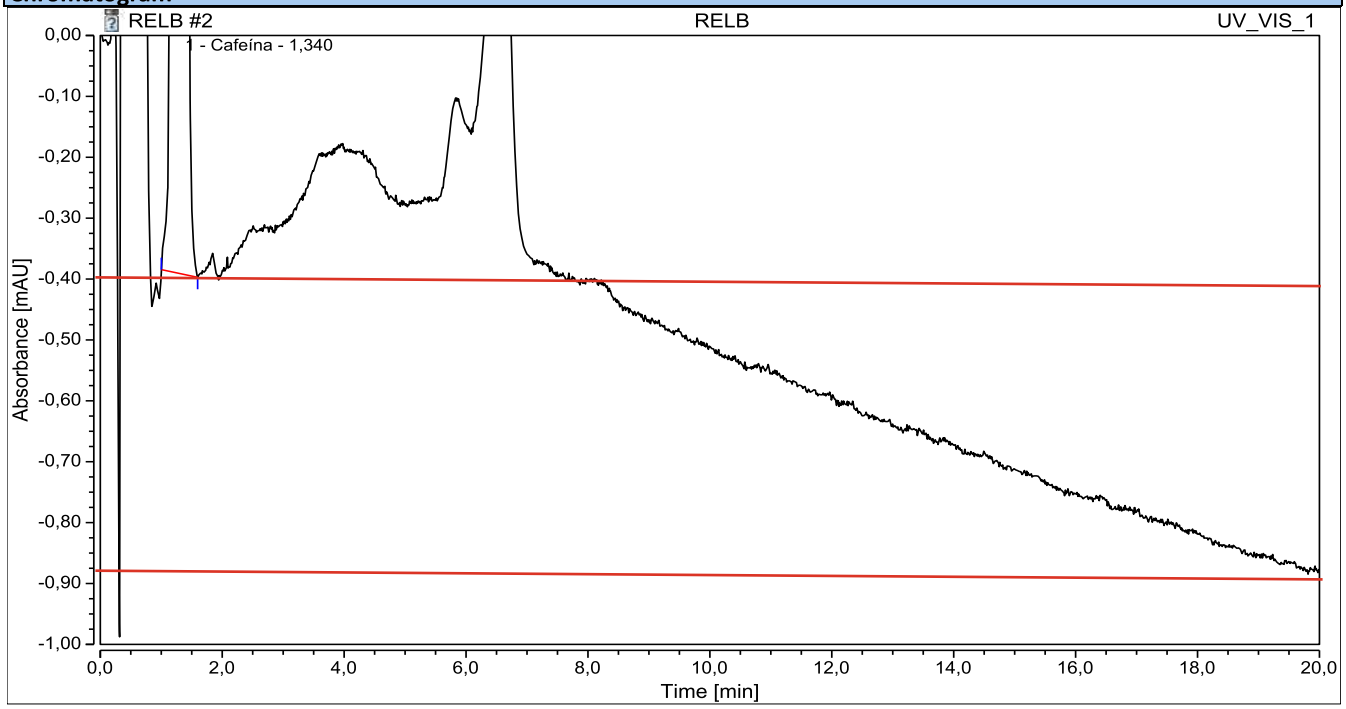

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,340	12,7863	123,275	100,00	100,00	n.a.
Total:			**12,786**	**123,275**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 16:36**	*Sample Weight:*	**1,0000**

Chromatogram

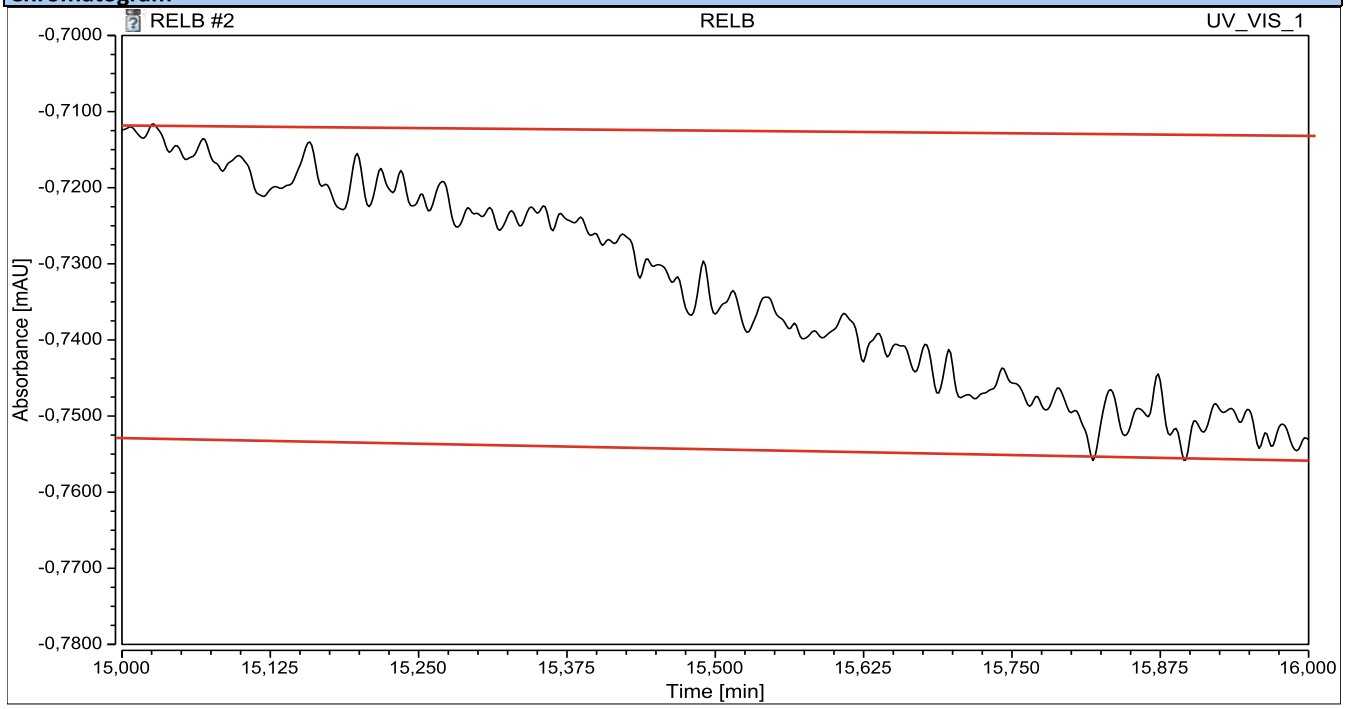

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,340	12,7863	123,275	100,00	100,00	n.a.
Total:			**12,786**	**123,275**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**4**
Processing Method:	**HPLC 04**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 17:38**	*Sample Weight:*	**1,0000**

Chromatogram

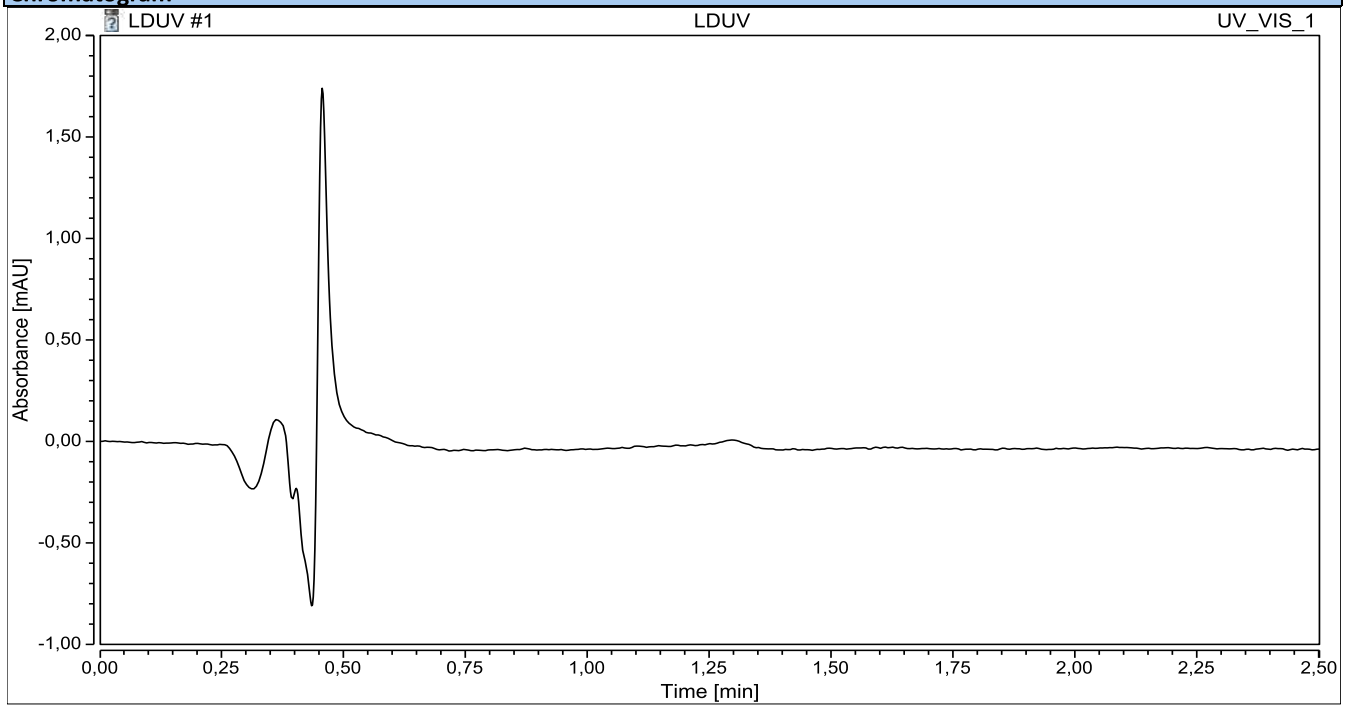

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**4**
Processing Method:	**HPLC 04**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 17:41**	*Sample Weight:*	**1,0000**

Chromatogram

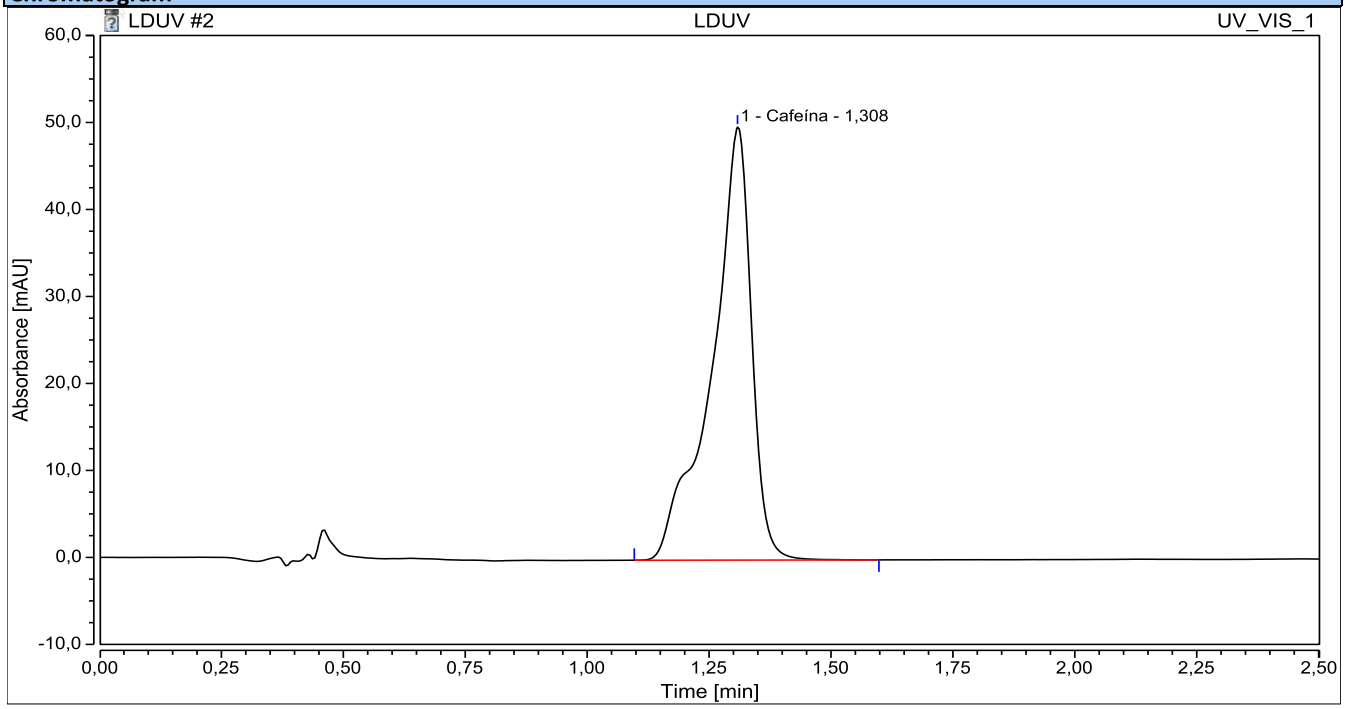

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,308	4,6619	49,784	100,00	100,00	n.a.
Total:			**4,662**	**49,784**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**4**
Processing Method:	**HPLC 04**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 17:44**	*Sample Weight:*	**1,0000**

Chromatogram

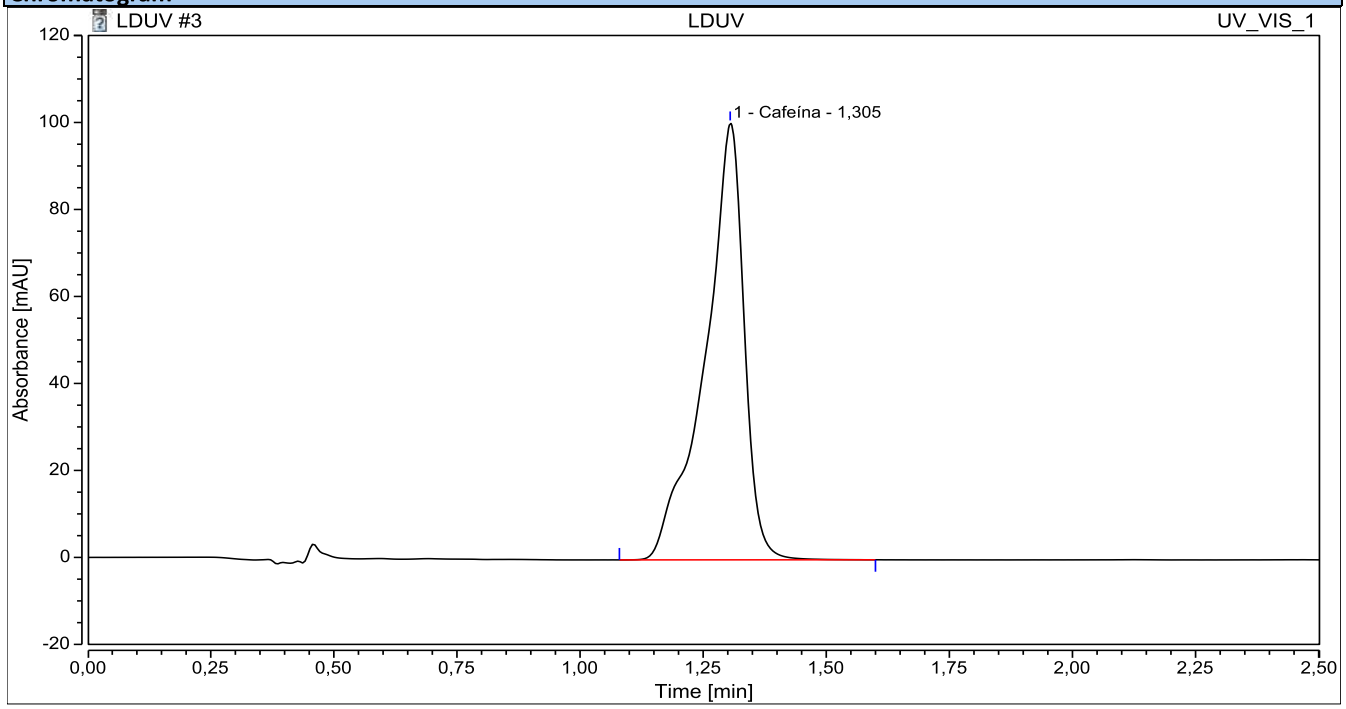

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,305	9,2310	100,346	100,00	100,00	n.a.
Total:			**9,231**	**100,346**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**4**
Processing Method:	**HPLC 04**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 17:48**	*Sample Weight:*	**1,0000**

Chromatogram

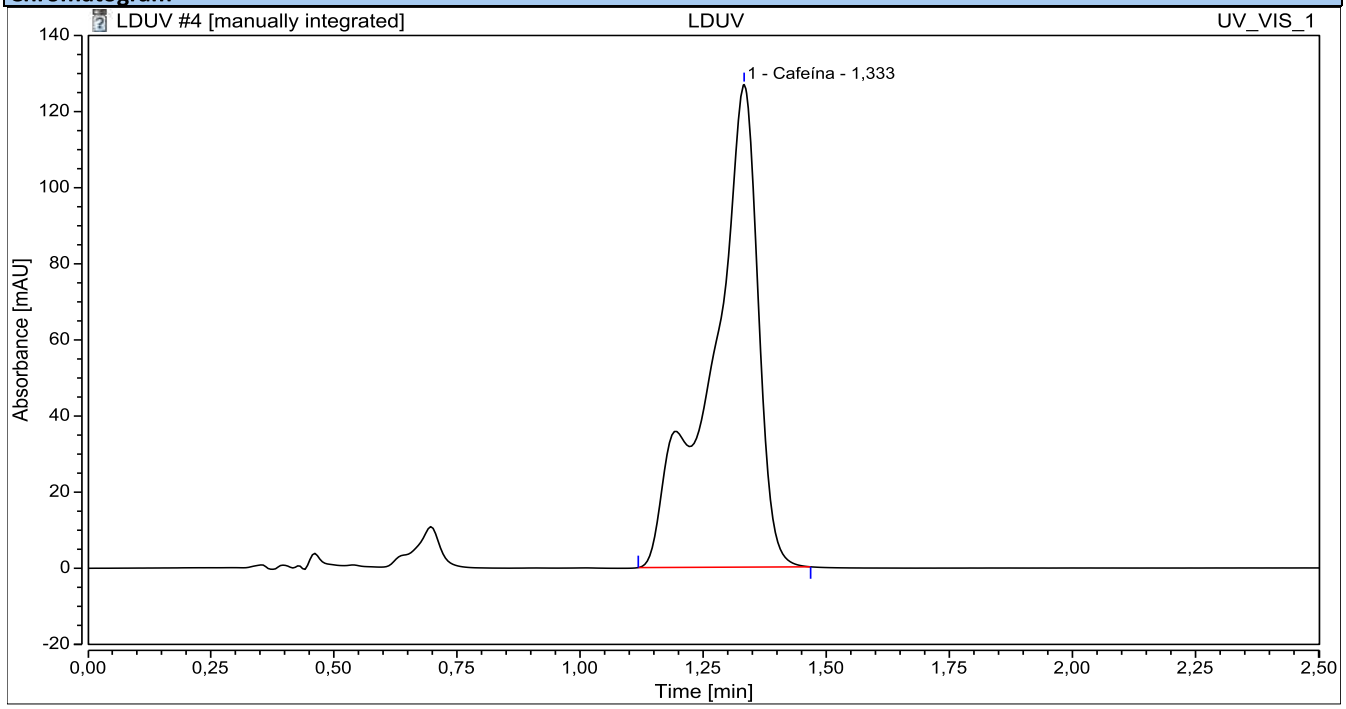

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,333	13,8141	126,802	100,00	100,00	n.a.
Total:			**13,814**	**126,802**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**4**
Processing Method:	**HPLC 04**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/mar/25 17:51**	*Sample Weight:*	**1,0000**

Chromatogram

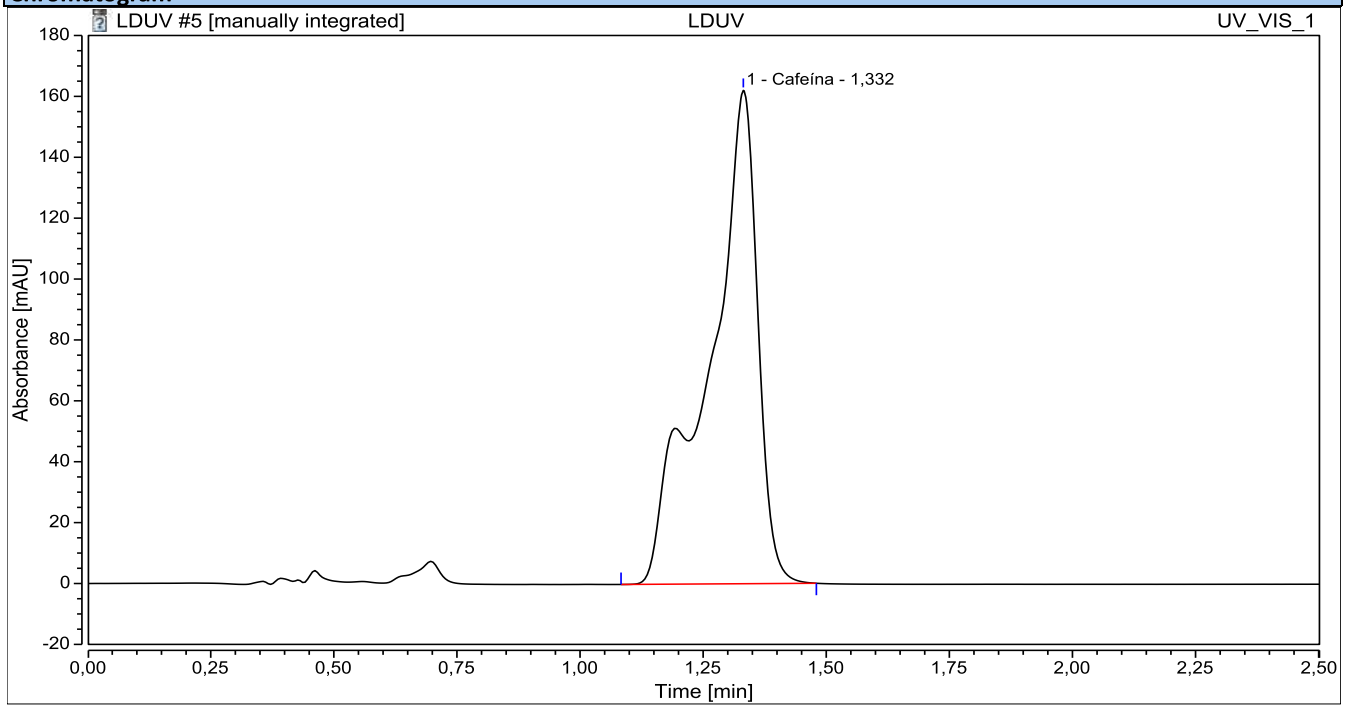

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,332	18,5174	162,034	100,00	100,00	n.a.
Total:			**18,517**	**162,034**	**100,000**	**100,000**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.