
Chromatogram

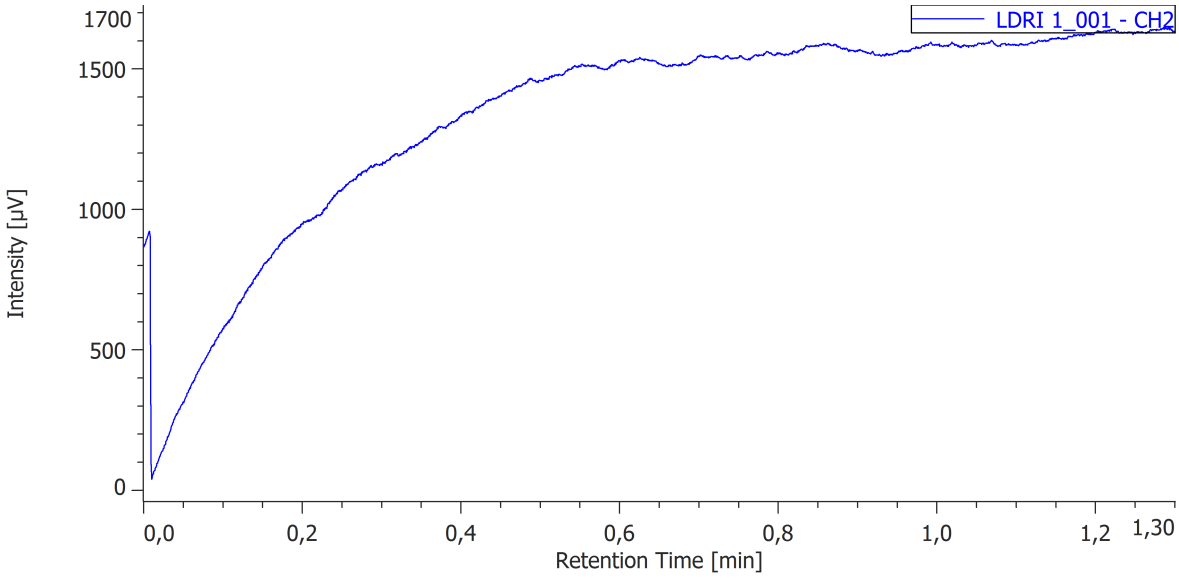


Chromatogram Information	
User Name	QPackSA
Date Modified	28/03/2024 09:51:09
Description	
HPLC System Name	HPL08 RI
Injection Date	28/03/2024 09:21:02
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,3 [min]
Acquisition Sequence	
Control Method	Qualificação_RID
Peak ID Table	LDRI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 1_001-CH2
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	LDRI

Creator QPackSA
Reviewer
Approver

Chromatogram

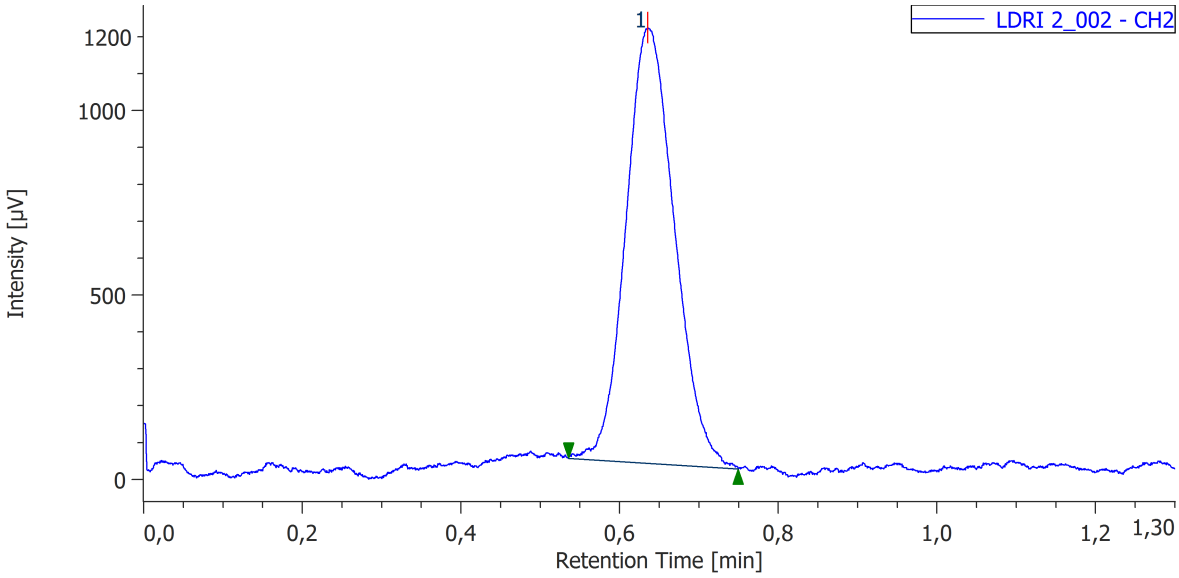

Chromatogram Information	
User Name	QPackSA
Date Modified	28/03/2024 09:51:09
Description	
HPLC System Name	HPL08 RI
Injection Date	28/03/2024 09:26:06
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	1,3 [min]
Acquisition Sequence	
Control Method	Qualificação_RID
Peak ID Table	LDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 2_002-CH2
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	LDRI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	LDRI	2	0,635	5049	1181	100,000	100,000	N/A	510	N/A	1,137	

Creator QPackSA
Reviewer
Approver

Chromatogram

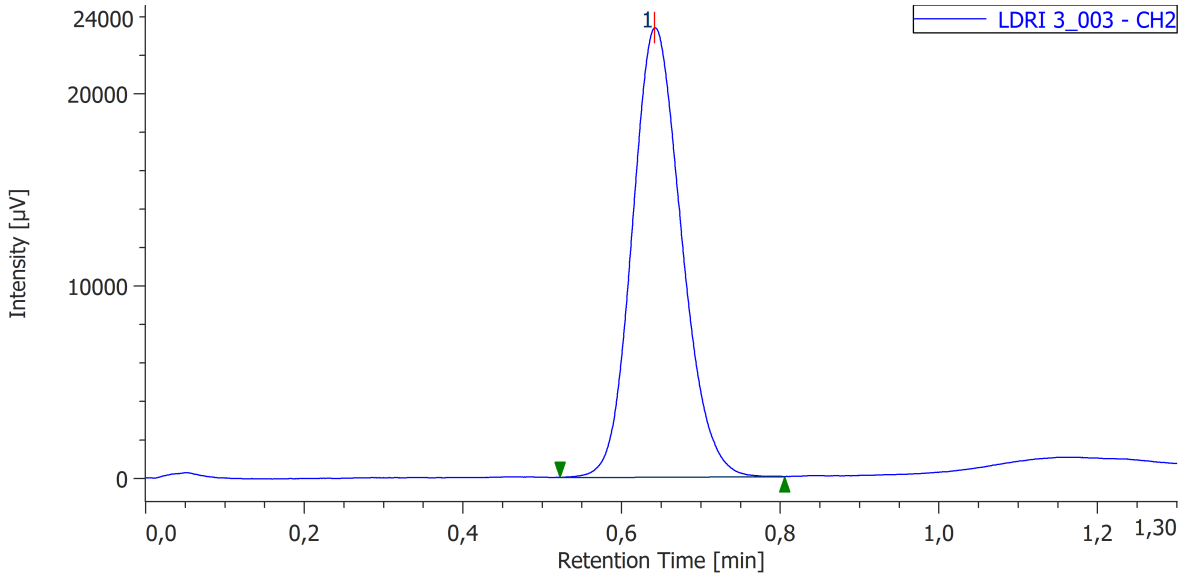

Chromatogram Information	
User Name	QPackSA
Date Modified	28/03/2024 09:51:09
Description	
HPLC System Name	HPL08 RI
Injection Date	28/03/2024 09:31:15
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	1,3 [min]
Acquisition Sequence	
Control Method	Qualificação_RID
Peak ID Table	LDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 3_003-CH2
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	LDRI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	LDRI	2	0,641	10042	23355	100,000	100,000	N/A	515	N/A	1,156	

Creator QPackSA
Reviewer
Approver

Chromatogram

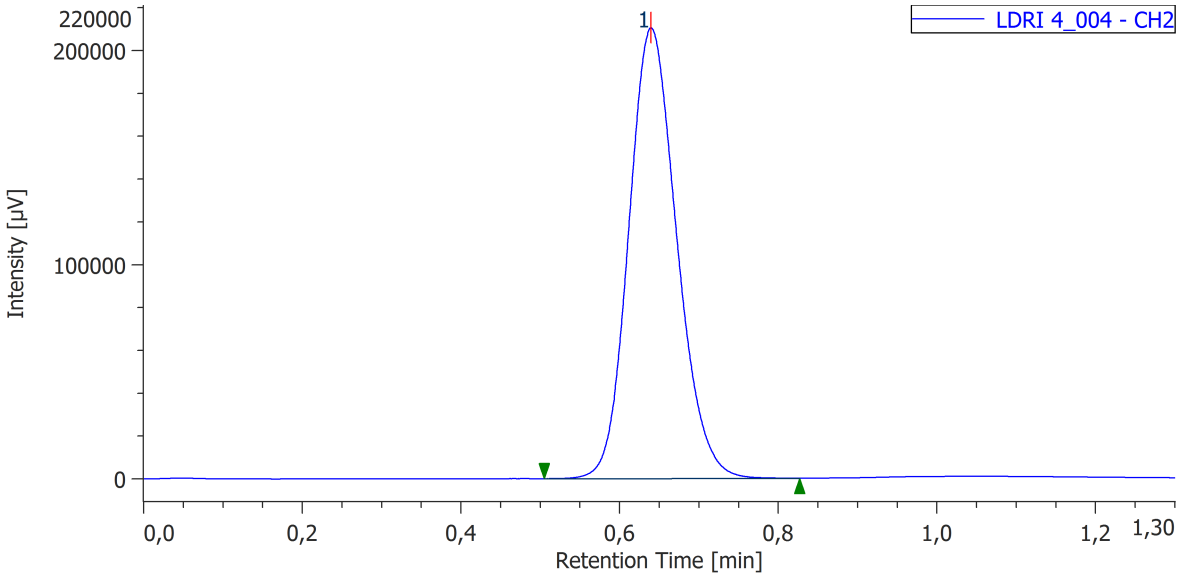


Channel & Peak Information Table

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning

Creator QPackSA
Reviewer
Approver

Chromatogram

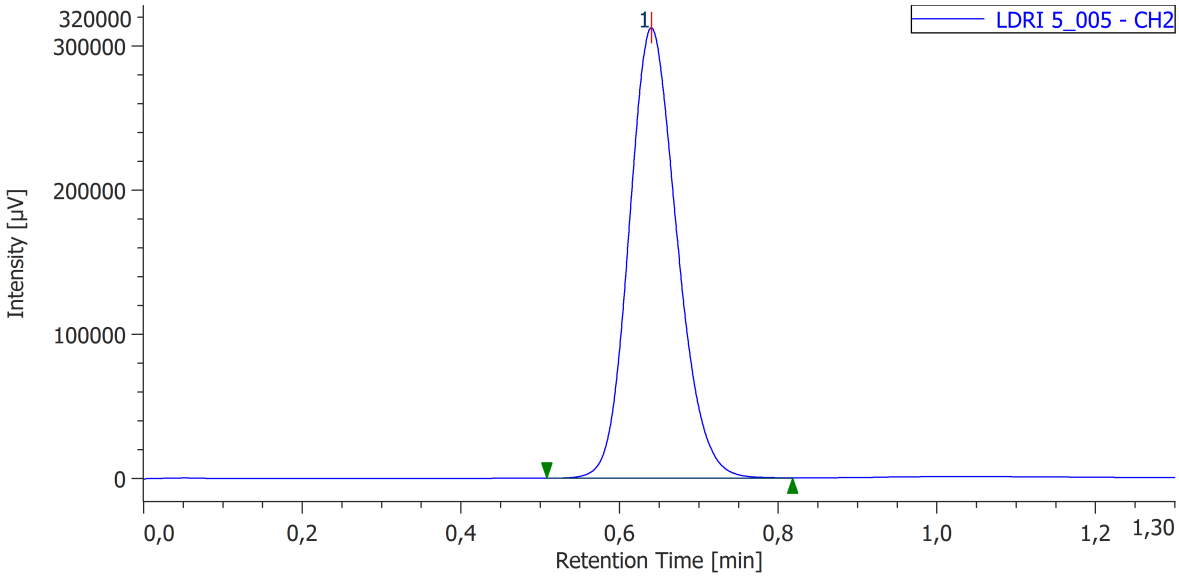

Chromatogram Information	
User Name	QPackSA
Date Modified	28/03/2024 09:51:10
Description	
HPLC System Name	HPL08 RI
Injection Date	28/03/2024 09:41:44
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,3 [min]
Acquisition Sequence	
Control Method	Qualificação_RID
Peak ID Table	LDRI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 5_005-CH2
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	LDRI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	LDRI	2	0,640	19675	312184	100,000	100,000	N/A	540	N/A	1,144	

Creator QPackSA
Reviewer
Approver