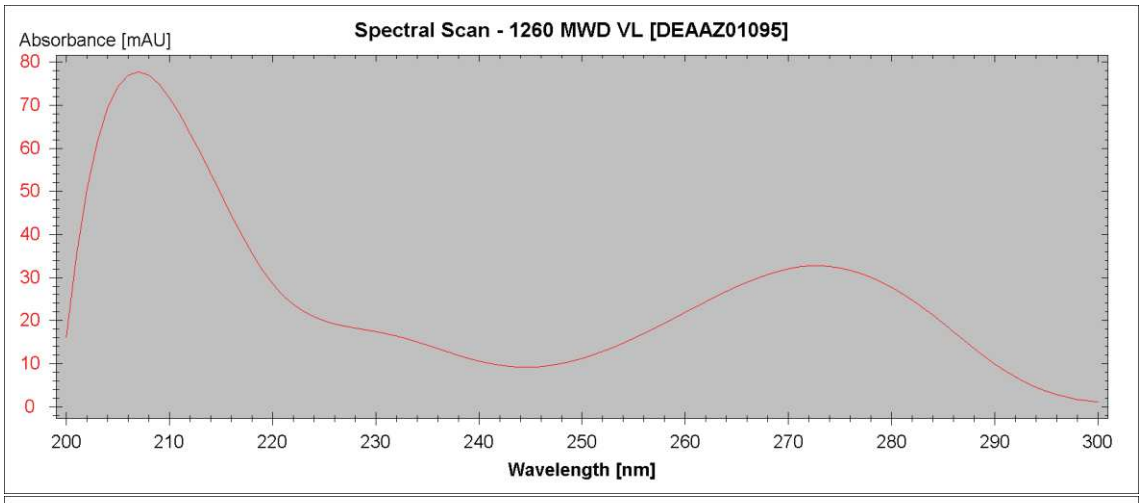
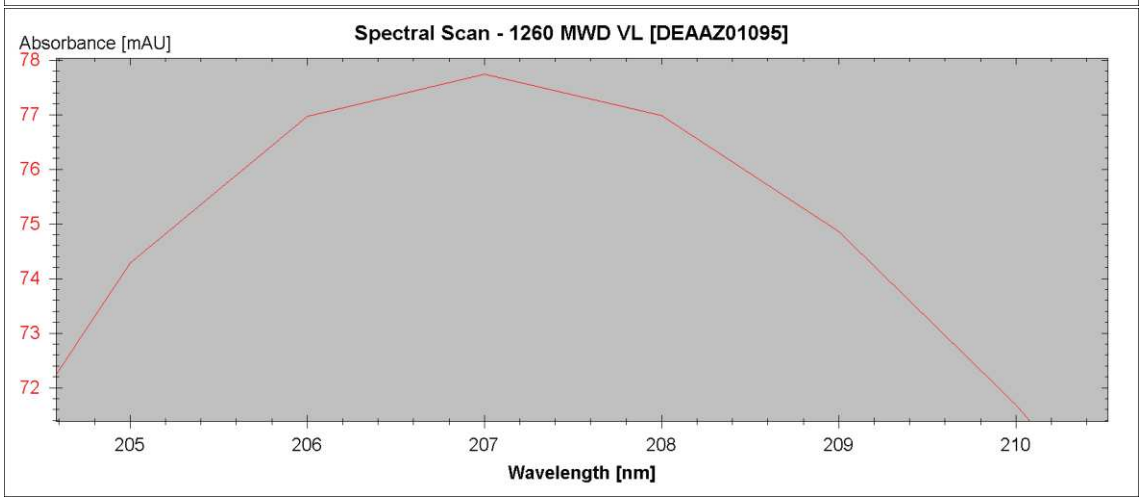
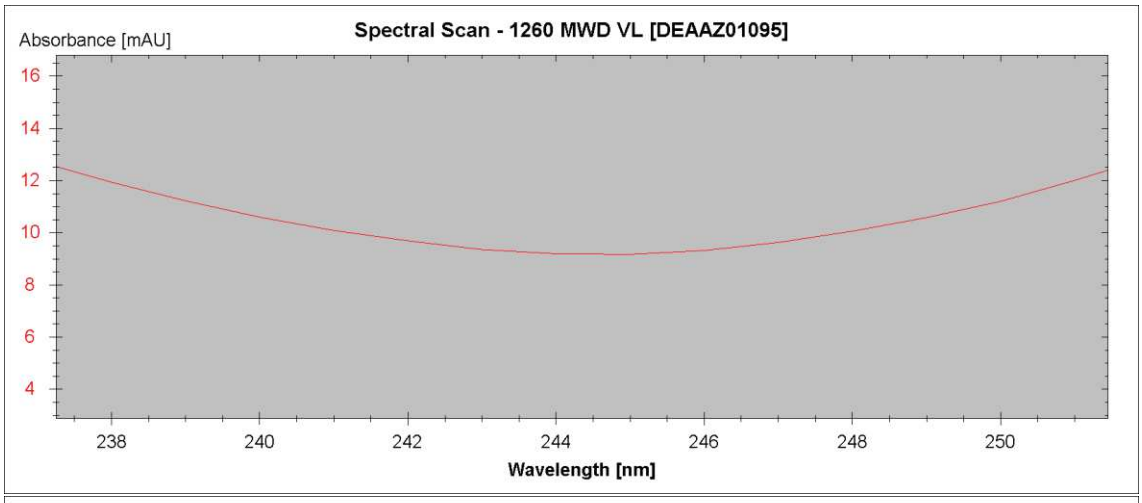
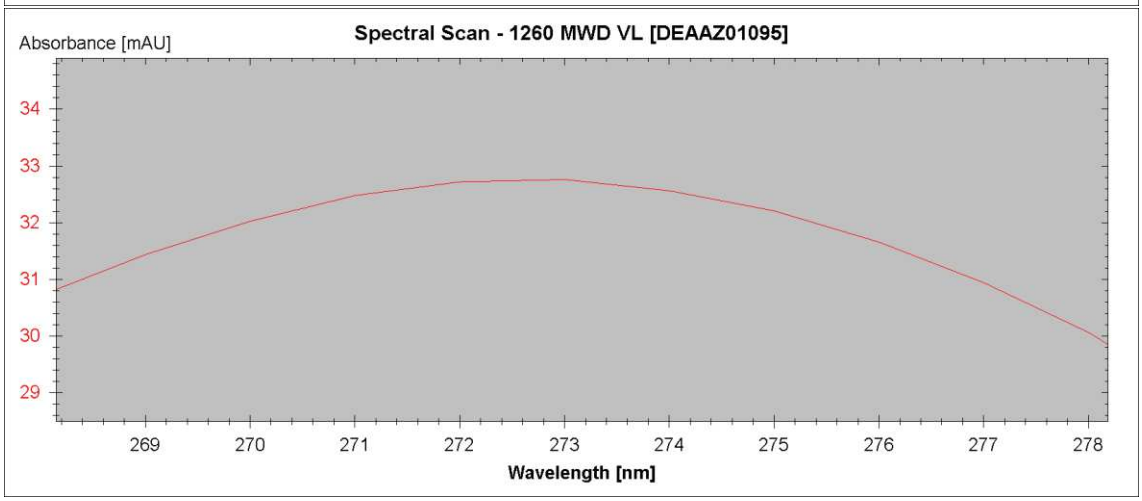

Spectral Scan - 1260 MWD VL [DEAAZ01095]
Absorbance [mAU]
80
70
60
50
40
30
20
10
0
200
210
220
230
240
250
260
270
280
290
300
Wavelength [nm]



Spectral Scan - 1260 MWD VL [DEAAZ01095]
Absorbance [mAU]
78
77
76
75
74
73
72
205
206
207
208
209
210
Wavelength [nm]


Spectral Scan - 1260 MWD VL [DEAAZ01095]
Absorbance [mAU]
16
14
12
10
8
6
4
238
240
242
244
246
248
250
Wavelength [nm]


Spectral Scan - 1260 MWD VL [DEAAZ01095]
Absorbance [mAU]
34
33
32
31
30
29
269
270
271
272
273
274
275
276
277
278
Wavelength [nm]

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0101.D
Sample Name: BR PCIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   1
Acq. Instrument : HPLC SALMIX                       Location :   92
Injection Date  : 6/8/2021 10:59:40 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 10:58:45 AM by SISTEMA
```

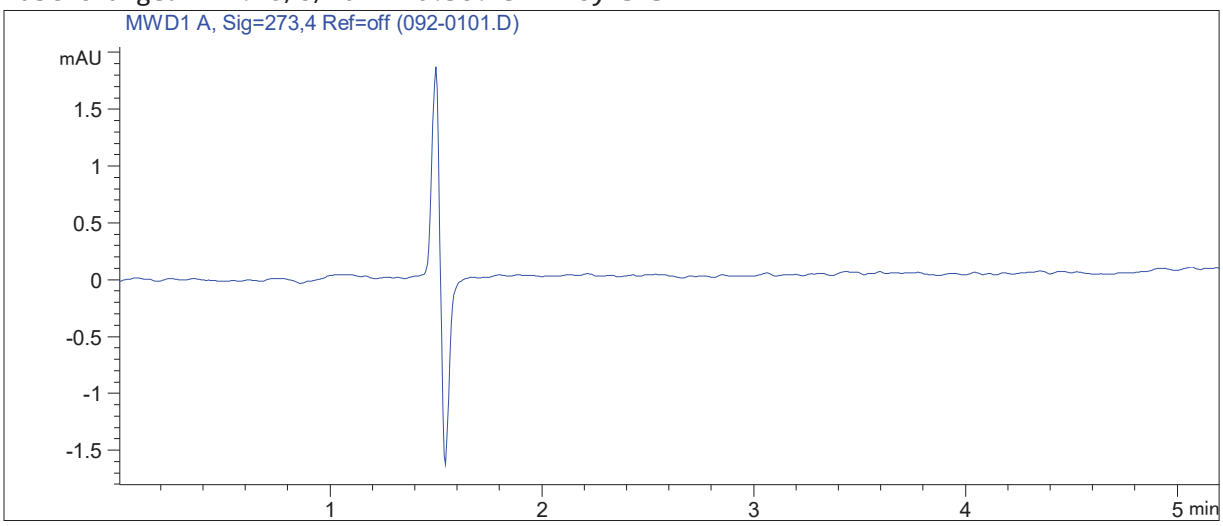


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      6/8/2021 10:56:45 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.160            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0101.D
Sample Name: BR PCIN 001

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : 6/8/2021 10:56:45 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	4.160		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0201.D
Sample Name: PCIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC SALMIX                       Location :   93
Injection Date  : 6/8/2021 11:05:53 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M
Last changed    : 6/8/2021 10:58:45 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:03 AM by SISTEMA
                  (modified after loading)
```

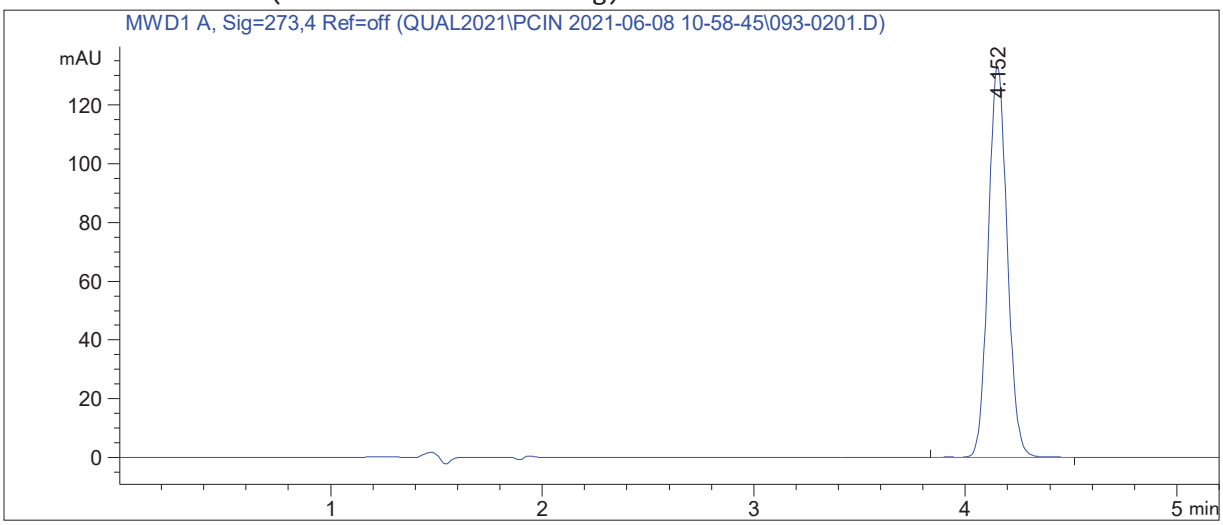


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152 BB      826.73206 1.20958e-3    1.00000    Cafeína

Totals :                                1.00000


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0301.D
Sample Name: PCIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   3
Acq. Instrument : HPLC SALMIX                     Location :   93
Injection Date  : 6/8/2021 11:12:05 AM                 Inj :   1
                                                Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Acq. Method     : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M
Last changed    : 6/8/2021 10:58:45 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

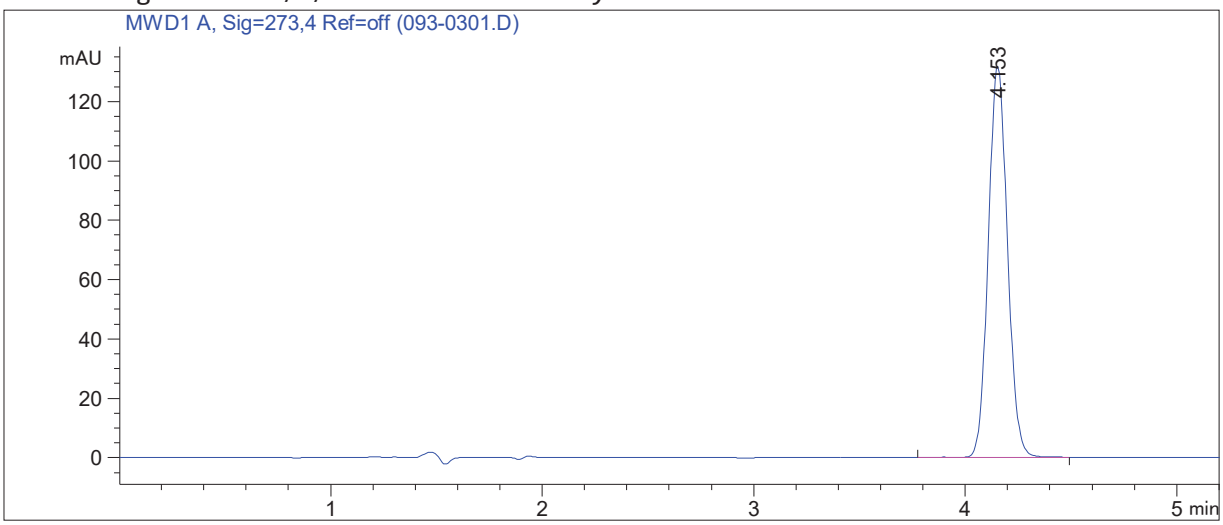


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.153 BB      826.39124 1.20958e-3 9.99588e-1    Cafeína

Totals :                              9.99588e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0401.D
Sample Name: PCIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   4
Acq. Instrument : HPLC SALMIX                       Location :   93
Injection Date  : 6/8/2021 11:18:18 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

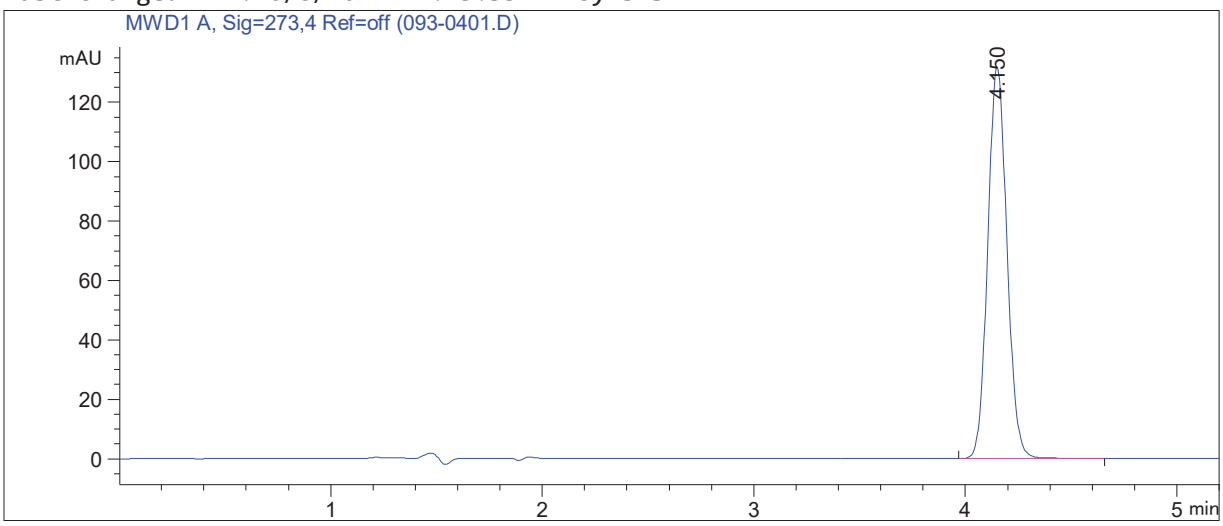


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.150 VB      827.38568 1.20958e-3    1.00079    Cafeína

Totals :                                1.00079


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0501.D
Sample Name: BR PCIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   5
Acq. Instrument : HPLC SALMIX                       Location :   92
Injection Date  : 6/8/2021 11:24:28 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

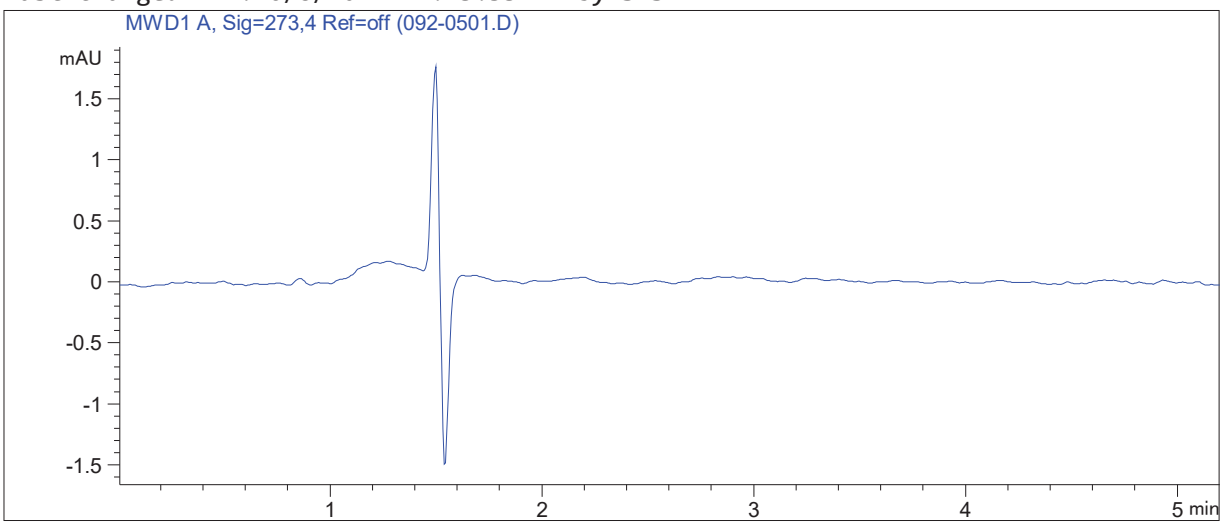


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0501.D
Sample Name: BR PCIN 002

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Tuesday, June 08, 2021 11:13:03 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	4.152		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0601.D
Sample Name: PCIN 004

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   6
Acq. Instrument : HPLC SALMIX                       Location :   93
Injection Date  : 6/8/2021 11:30:41 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

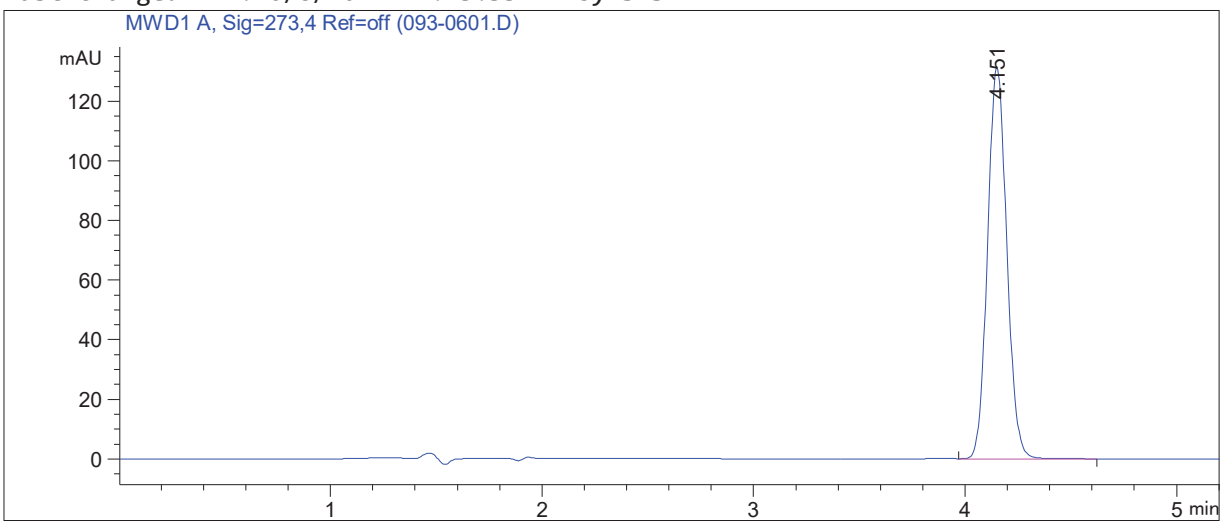


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.151 BB      825.18939 1.20958e-3 9.98134e-1    Cafeína

Totals :                              9.98134e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0701.D
Sample Name: PCIN 005

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   7
Acq. Instrument : HPLC SALMIX                       Location :   93
Injection Date  : 6/8/2021 11:36:53 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

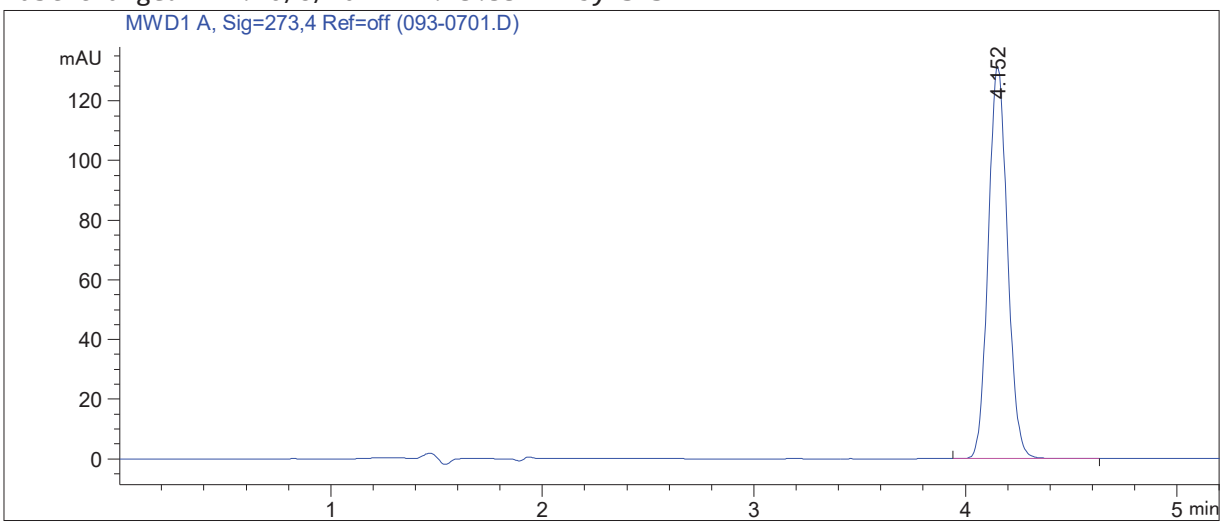


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152 BB      826.58148 1.20958e-3 9.99818e-1    Cafeína

Totals :                              9.99818e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\093-0801.D
Sample Name: PCIN 006

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   8
Acq. Instrument : HPLC SALMIX                       Location :   93
Injection Date  : 6/8/2021 11:43:06 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

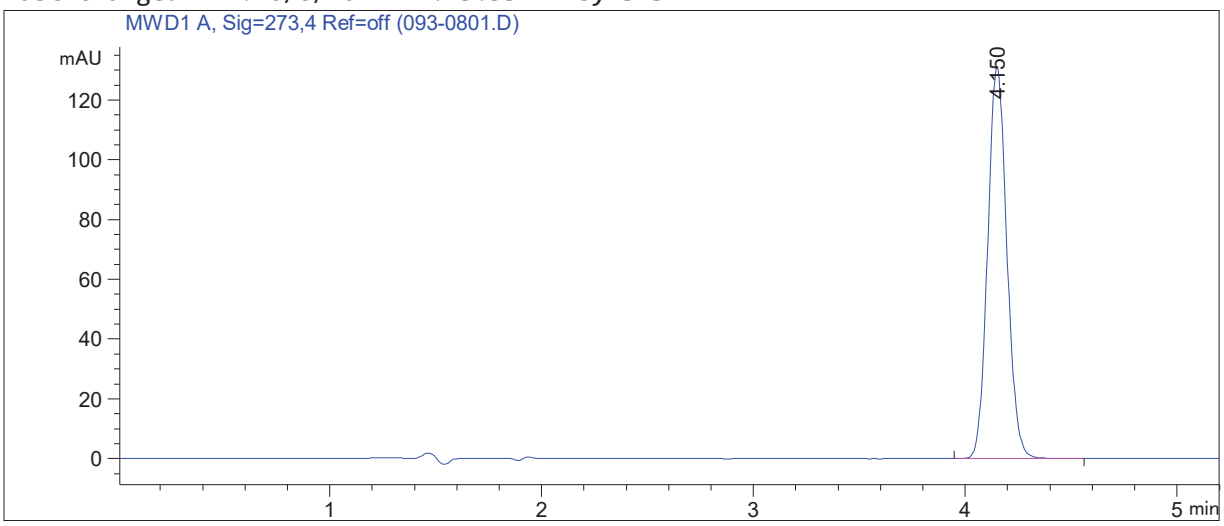


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.150 BB      826.18530 1.20958e-3 9.99339e-1    Cafeína

Totals :                              9.99339e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0901.D
Sample Name: BR PCIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   9
Acq. Instrument : HPLC SALMIX                       Location :   92
Injection Date  : 6/8/2021 11:49:16 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\PCIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 11:13:53 AM by SISTEMA
```

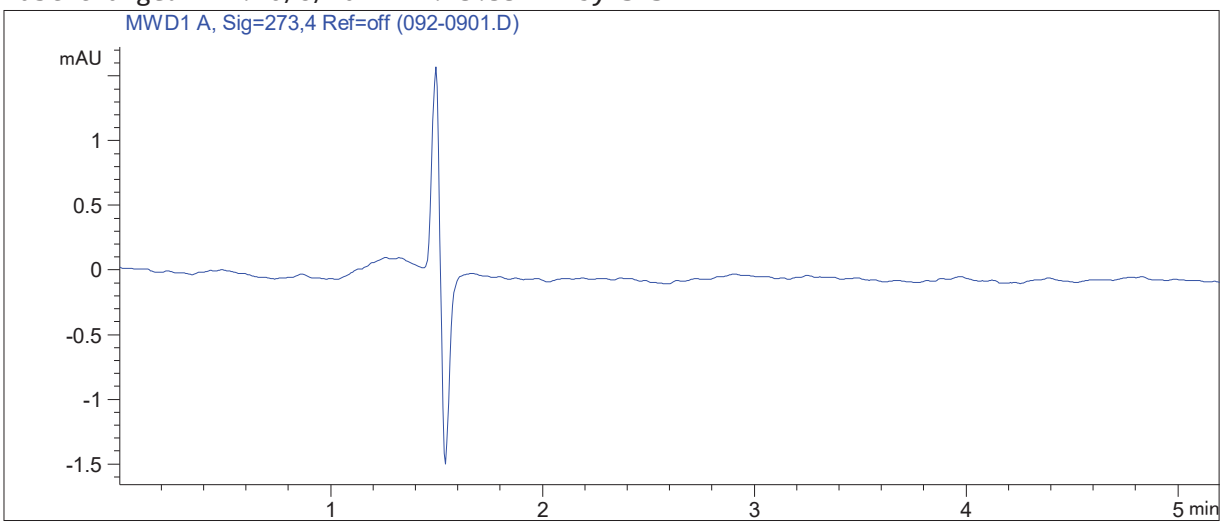


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area      Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2021\PCIN 2021-06-08 10-58-45\092-0901.D
Sample Name: BR PCIN 003

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Tuesday, June 08, 2021 11:13:03 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	4.152		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\094-0101.D
Sample Name: LDUV 001

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   1
Acq. Instrument : HPLC SALMIX                       Location :   94
Injection Date  : 6/8/2021 12:43:43 PM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\LDUV.S
Method          : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 12:42:45 PM by SISTEMA
```

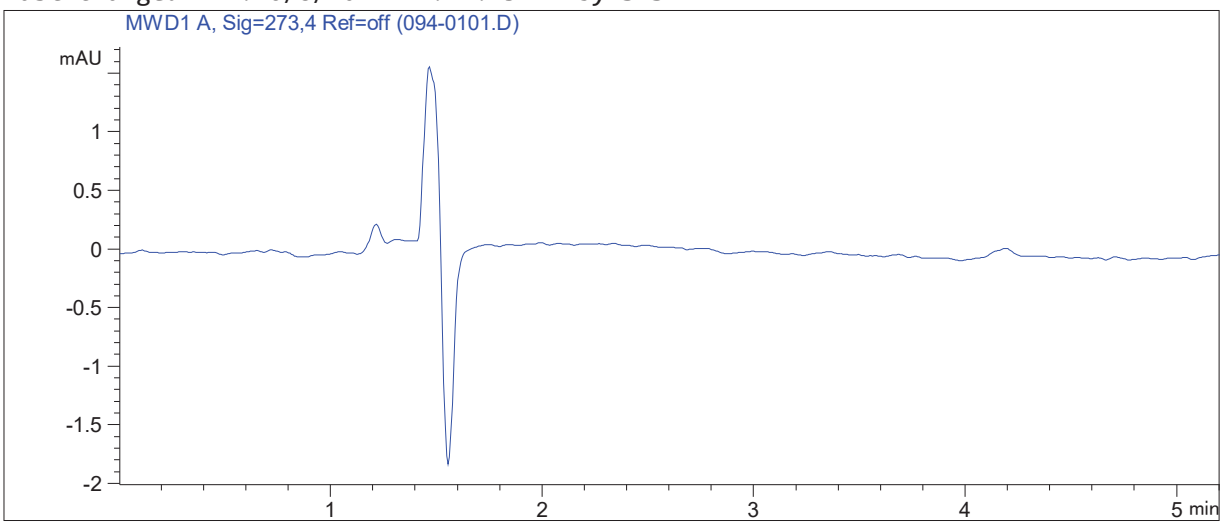


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area      Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\094-0101.D
Sample Name: LDUV 001

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Tuesday, June 08, 2021 11:13:03 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	4.152		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\095-0201.D
Sample Name: LDUV 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC SALMIX                       Location :   95
Injection Date  : 6/8/2021 12:49:54 PM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\LDUV.S
Method          : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 12:42:45 PM by SISTEMA
```

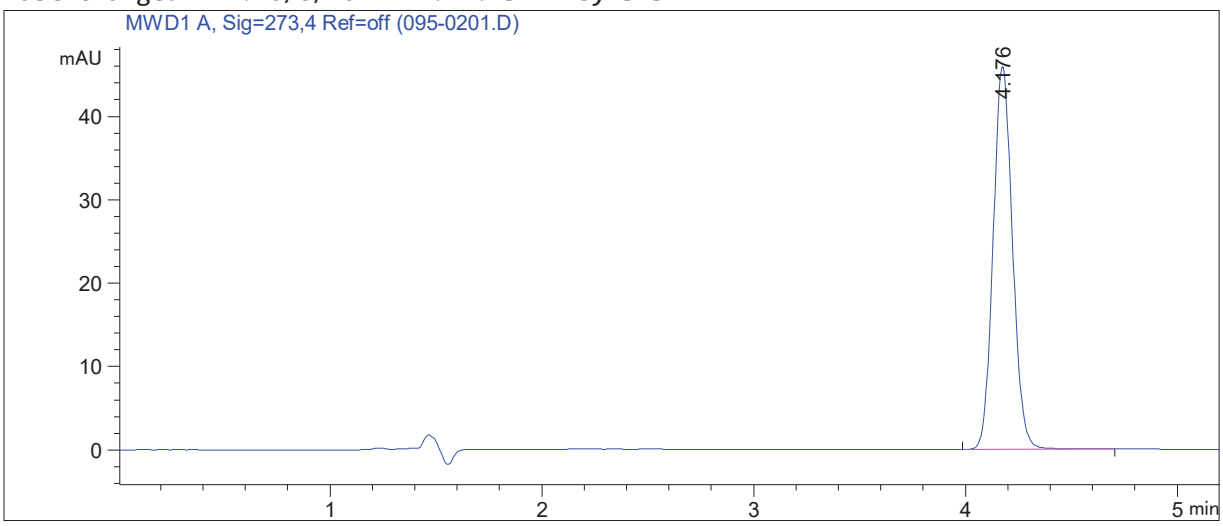


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.176 BB      291.65143 1.20958e-3 3.52776e-1    Cafeína

Totals :                              3.52776e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\096-0301.D
Sample Name: LDUV 003

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   3
Acq. Instrument : HPLC SALMIX                     Location :   96
Injection Date  : 6/8/2021 12:56:06 PM                Inj :   1
                                                 Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\LDUV.S
Method          : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 12:42:45 PM by SISTEMA
```

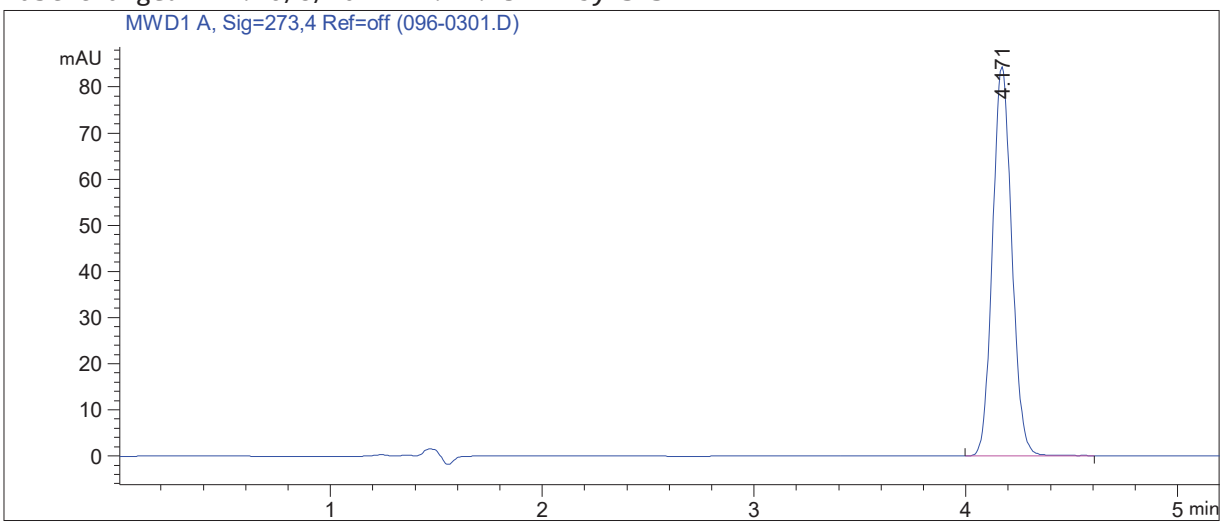


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.171 BB      532.83807 1.20958e-3 6.44511e-1    Cafeína

Totals :                              6.44511e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\097-0401.D
Sample Name: LDUV 004

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   4
Acq. Instrument : HPLC SALMIX                     Location :   97
Injection Date  : 6/8/2021 1:02:17 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\LDUV.S
Method          : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 12:42:45 PM by SISTEMA
```

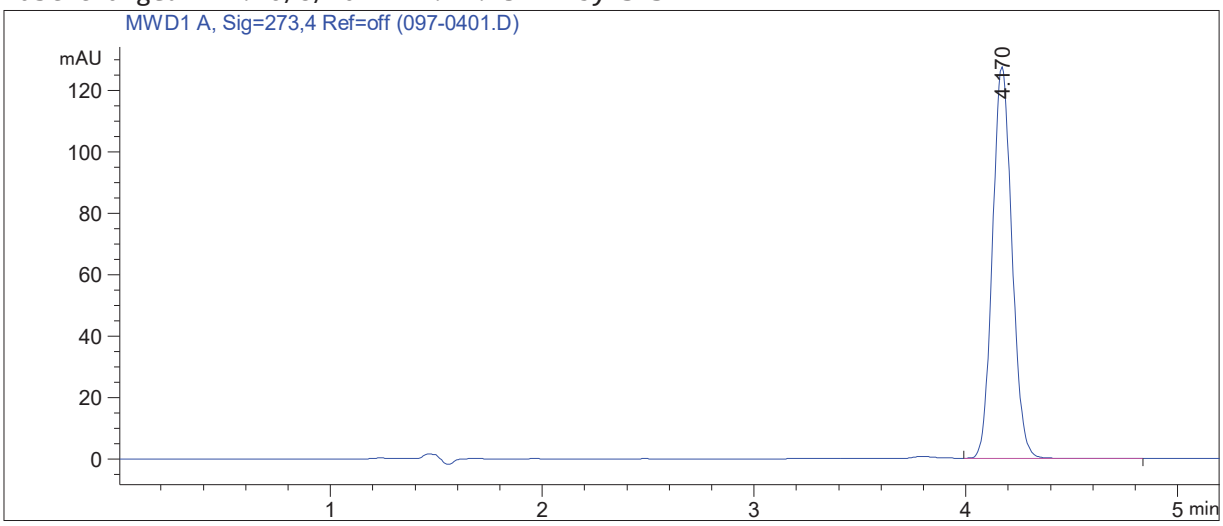


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.170 VB      818.17084 1.20958e-3 9.89645e-1    Cafeína

Totals :                              9.89645e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\098-0501.D
Sample Name: LDUV 005

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   5
Acq. Instrument : HPLC SALMIX                    Location :   98
Injection Date  : 6/8/2021 1:08:29 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M
Last changed    : 6/8/2021 12:42:45 PM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2021\LDUV 2021-06-08 12-42-45\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:18:43 PM by SISTEMA
Additional Info : Peak(s) manually integrated
```

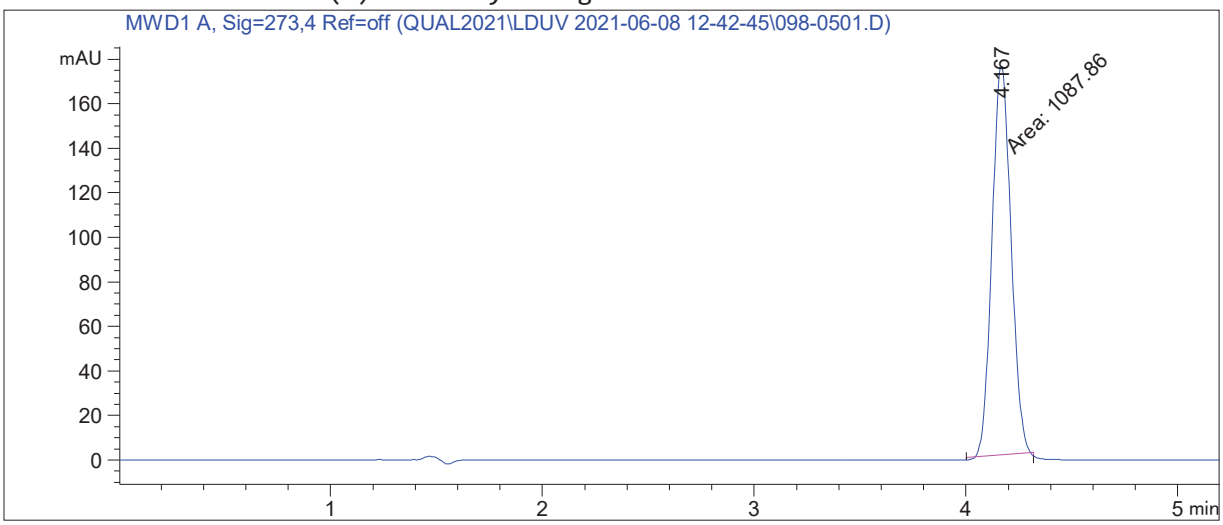


```
==================================================================
                    External Standard Report
==================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.167 MM     1087.86426 1.20958e-3    1.31586    Cafeína

Totals :                                1.31586


==================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0101.D
Sample Name: LIIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   1
Acq. Instrument : HPLC SALMIX                       Location :   99
Injection Date  : 6/8/2021 1:20:04 PM                    Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Sequence File   : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\LIIN.S
Method          : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:19:48 PM by SISTEMA
```

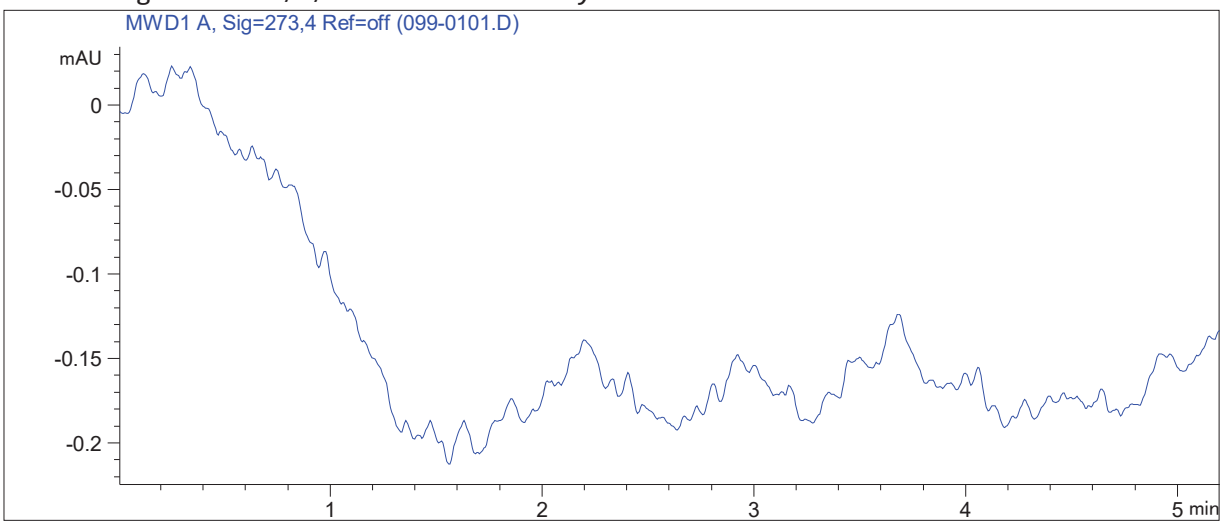


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.152            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0101.D
Sample Name: LIIN 001

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Tuesday, June 08, 2021 11:13:03 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	4.152		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0201.D
Sample Name: LIIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC SALMIX                       Location :   99
Injection Date  : 6/8/2021 1:26:19 PM                    Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 5.000 µl
Method          : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:19:48 PM by SISTEMA
```

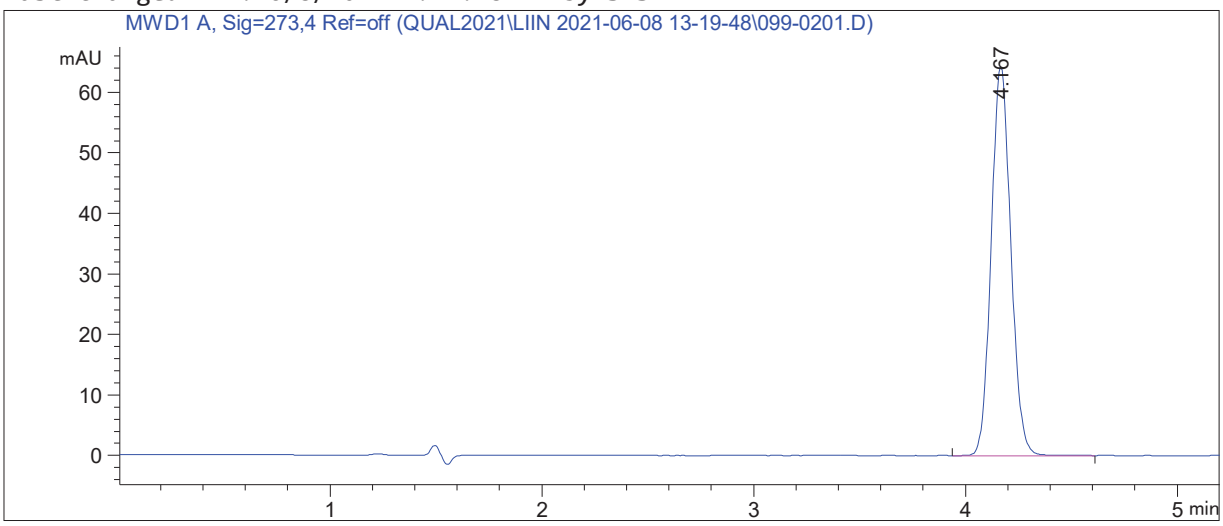


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.167 BB      413.71439 1.20958e-3 5.00421e-1    Cafeína

Totals :                              5.00421e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0301.D
Sample Name: LIIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   3
Acq. Instrument : HPLC SALMIX                       Location :   99
Injection Date  : 6/8/2021 1:32:31 PM                    Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:19:48 PM by SISTEMA
```

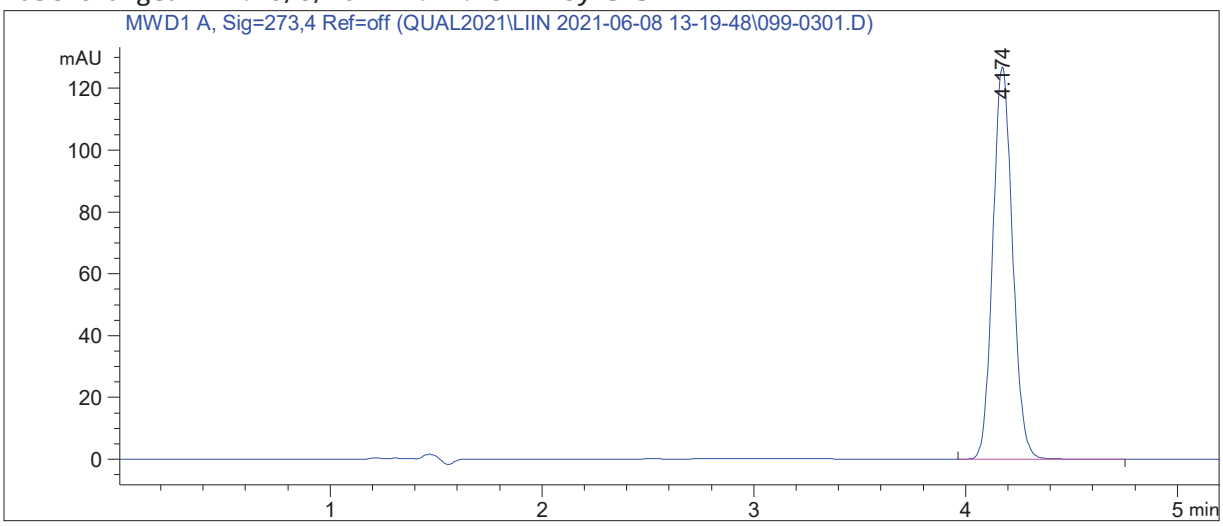


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.174 BB      820.19989 1.20958e-3 9.92099e-1    Cafeína

Totals :                              9.92099e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0401.D
Sample Name: LIIN 004

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   4
Acq. Instrument : HPLC SALMIX                    Location :   99
Injection Date  : 6/8/2021 1:38:45 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Method          : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:19:48 PM by SISTEMA
```

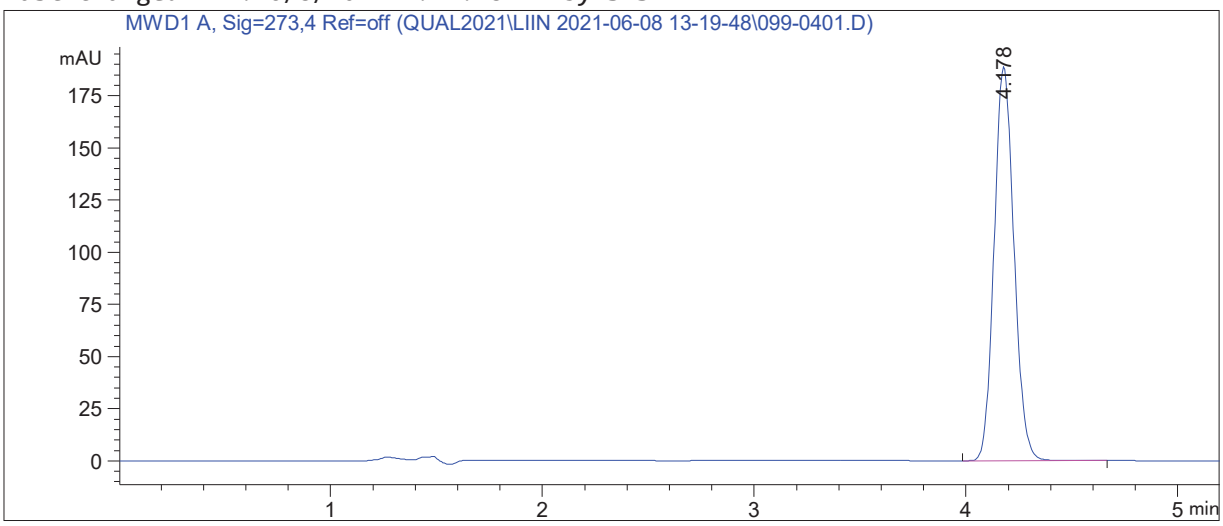


```
==================================================================
                    External Standard Report
==================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.178 BB     1229.14294 1.20958e-3    1.48675    Cafeína

Totals :                                1.48675


==================================================================
                        *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\099-0501.D
Sample Name: LIIN 005

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   5
Acq. Instrument : HPLC SALMIX                       Location :   99
Injection Date  : 6/8/2021 1:45:02 PM                    Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Method          : C:\Chem32\1\DATA\QUAL2021\LIIN 2021-06-08 13-19-48\Qualificação QPack.M (
                  Sequence Method)
Last changed    : 6/8/2021 1:19:48 PM by SISTEMA
```

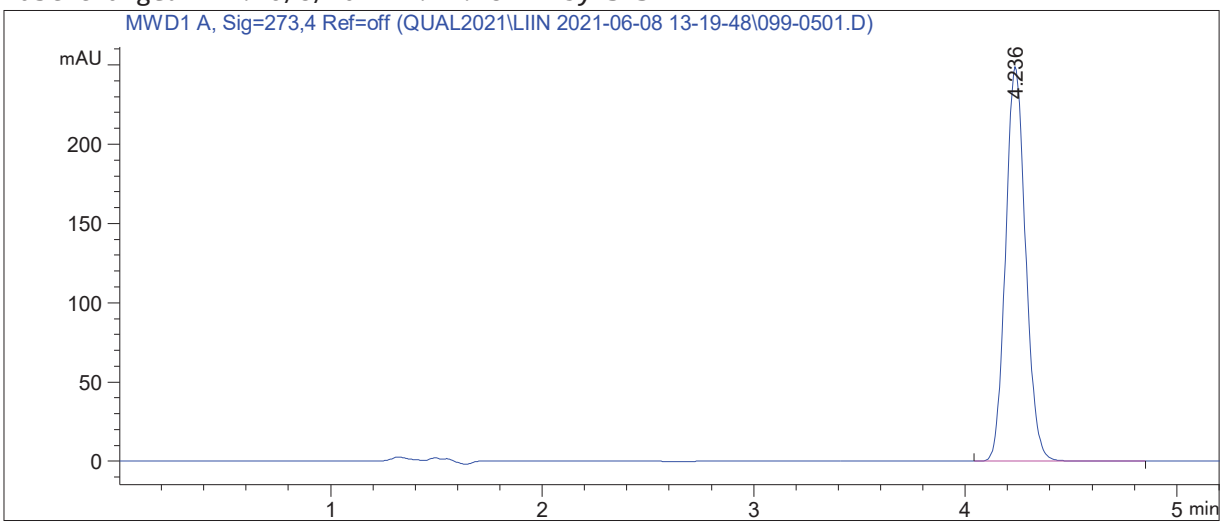


```
==========================================================================
                     External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Tuesday, June 08, 2021 11:13:03 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  4.236 BB     1632.30957 1.20958e-3    1.97441    Cafeína

Totals :                                1.97441


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2021\GRAD AB 2021-06-08 14-27-59.D
Sample Name: GRAD AB

```
==========================================================================
Acq. Operator   : SISTEMA
Sample Operator : SISTEMA
Acq. Instrument : HPLC SALMIX                    Location :     -
Injection Date  : 6/8/2021 2:28:12 PM
                                                 Inj Volume : No inj
Method          : C:\CHEM32\1\METHODS\GRAD AB.M
Last changed    : 6/8/2021 2:23:36 PM by SISTEMA
Additional Info : Peak(s) manually integrated
```

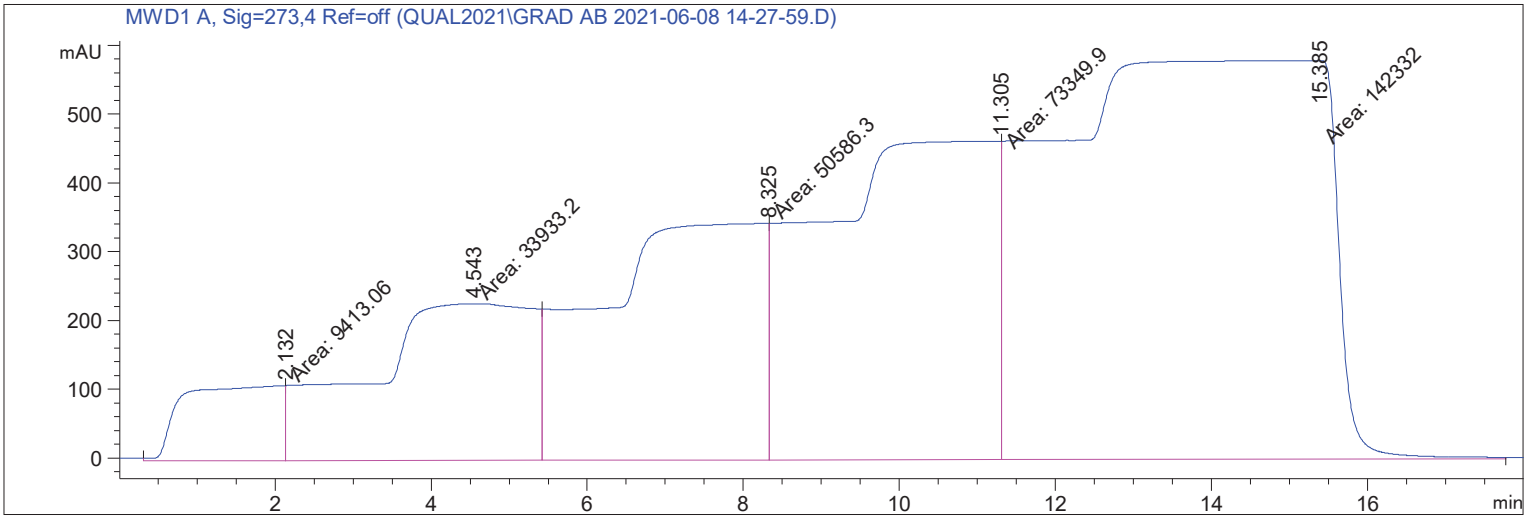


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: MWD1 A, Sig=273,4 Ref=off
```

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.132	MF	1.4359	9413.06055	109.25942	3.0403
2	4.543	FM	2.4811	3.39332e4	227.94623	10.9598
3	8.325	FM	2.4513	5.05863e4	343.94830	16.3385
4	11.305	FM	2.6394	7.33499e4	463.16663	23.6908
5	15.385	FM	4.0925	1.42332e5	579.65027	45.9706


Data File C:\Chem32\1\DATA\QUAL2021\GRAD AB 2021-06-08 14-27-59.D
Sample Name: GRAD AB

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
Totals :				3.09614e5	1723.97085	

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2021\GRAD CD 2021-06-08 14-54-15.D
Sample Name: GRAD CD

```
==========================================================================
Acq. Operator   : SISTEMA
Sample Operator : SISTEMA
Acq. Instrument : HPLC SALMIX                    Location :     -
Injection Date  : 6/8/2021 2:54:28 PM
                                                 Inj Volume : No inj
Method          : C:\CHEM32\1\METHODS\GRAD CD.M
Last changed    : 6/8/2021 2:47:53 PM by SISTEMA
Additional Info : Peak(s) manually integrated
```

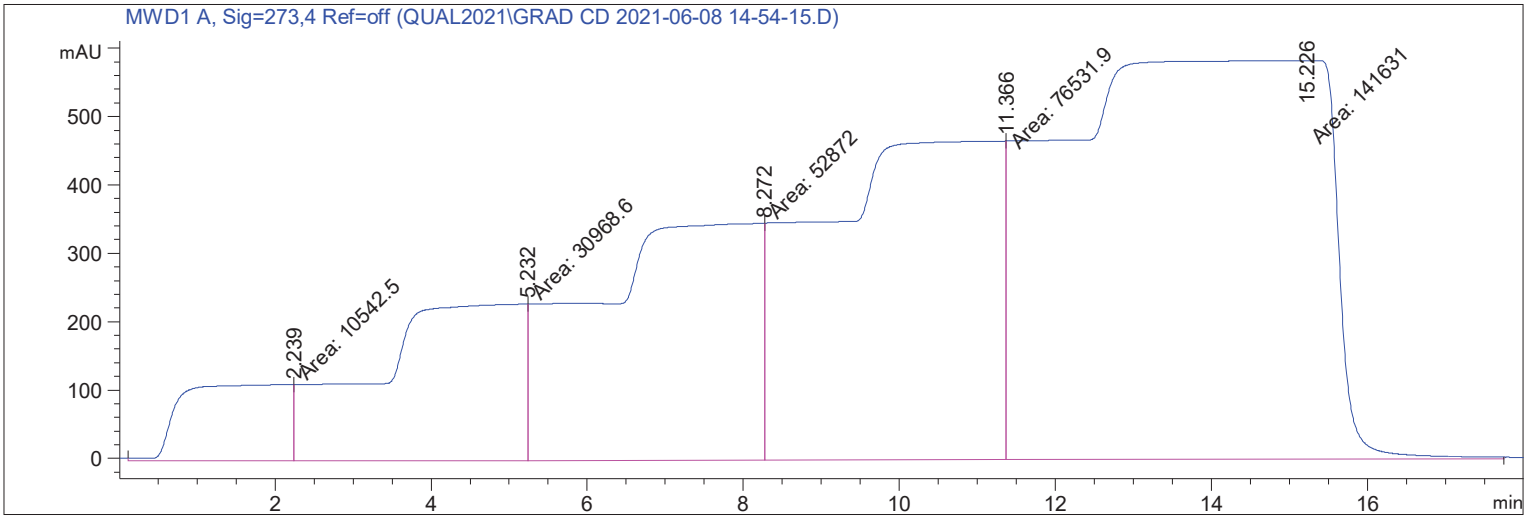


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.239 MF    1.5762 1.05425e4   111.47382   3.3731
   2   5.232 FM    2.2562 3.09686e4   228.76566   9.9085
   3   8.272 FM    2.5426 5.28720e4   346.57452  16.9166
   4  11.366 FM    2.7366 7.65319e4   466.10770  24.4866
   5  15.226 FM    4.0469 1.41631e5   583.28809  45.3153
```

Data File C:\Chem32\1\DATA\QUAL2021\GRAD CD 2021-06-08 14-54-15.D
Sample Name: GRAD CD

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
Totals :				3.12546e5	1736.20979	

==========

*** End of Report ***