
Peak Find - EDFL.jws

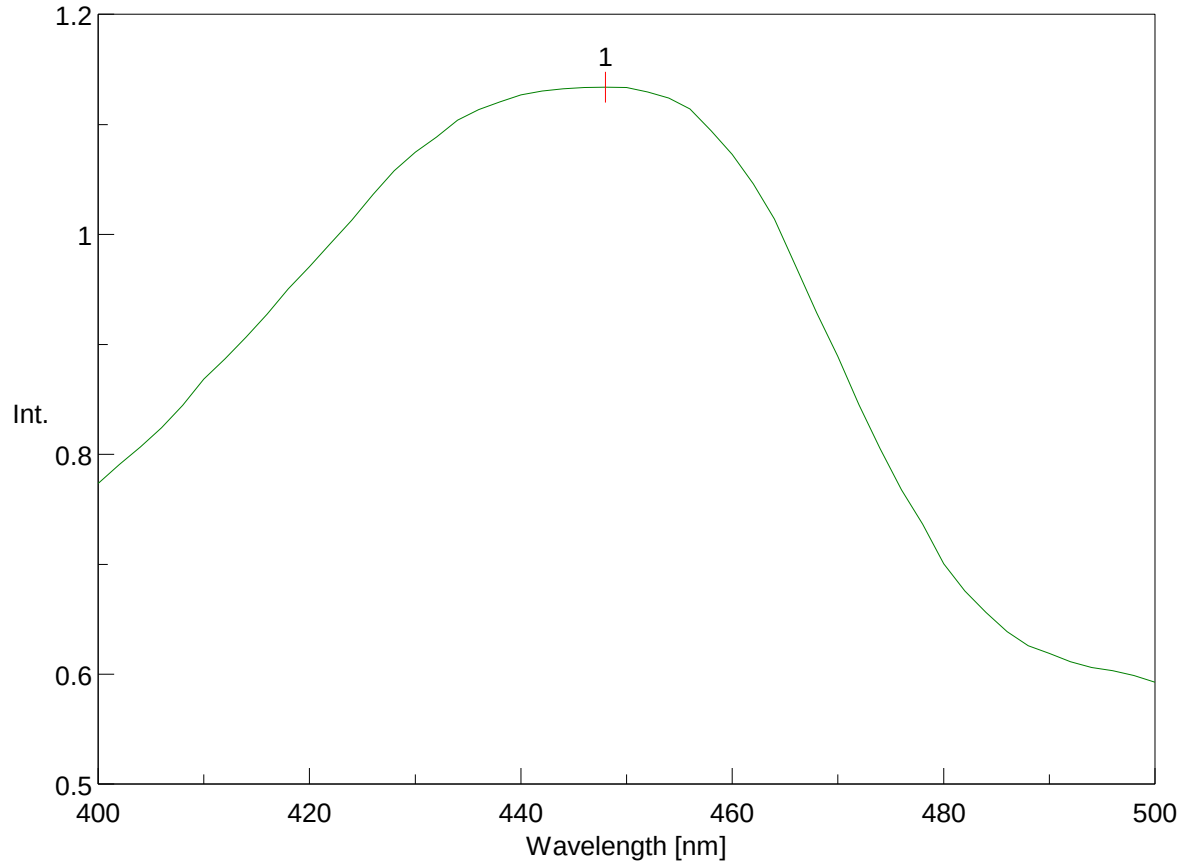

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	05/03/2026 09:40

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Model Name	FP-1520
Serial No.	XXXXX
ROM version	V1.42
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	448	1.13363			

Chromatogram

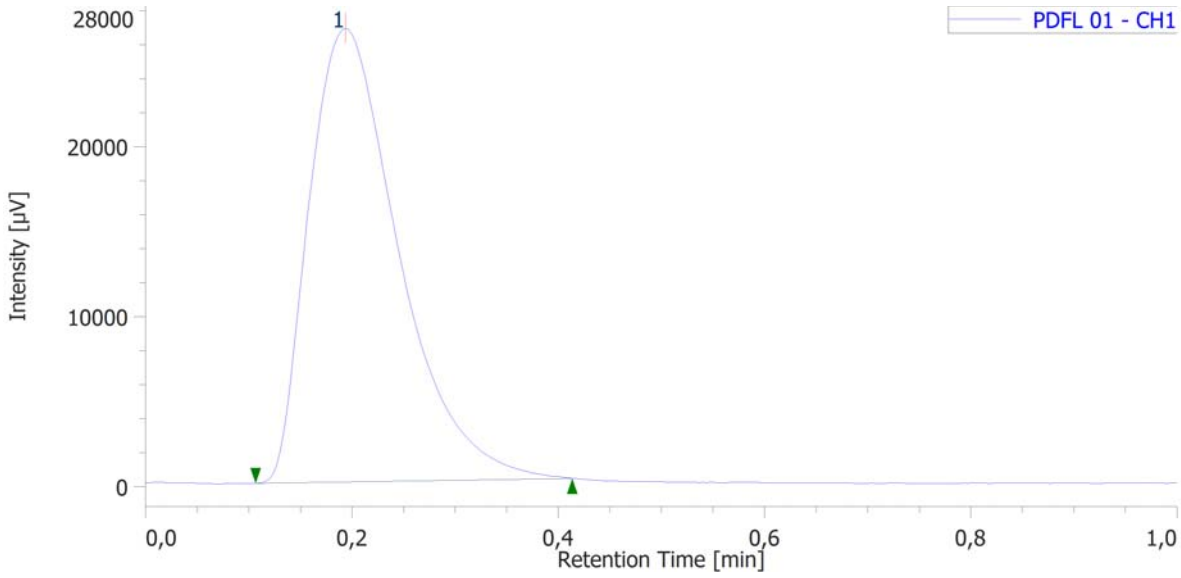

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:32
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2026 10:07:40
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,193	161075	26673	100,000	100,000	N/A	24	N/A	1,573		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

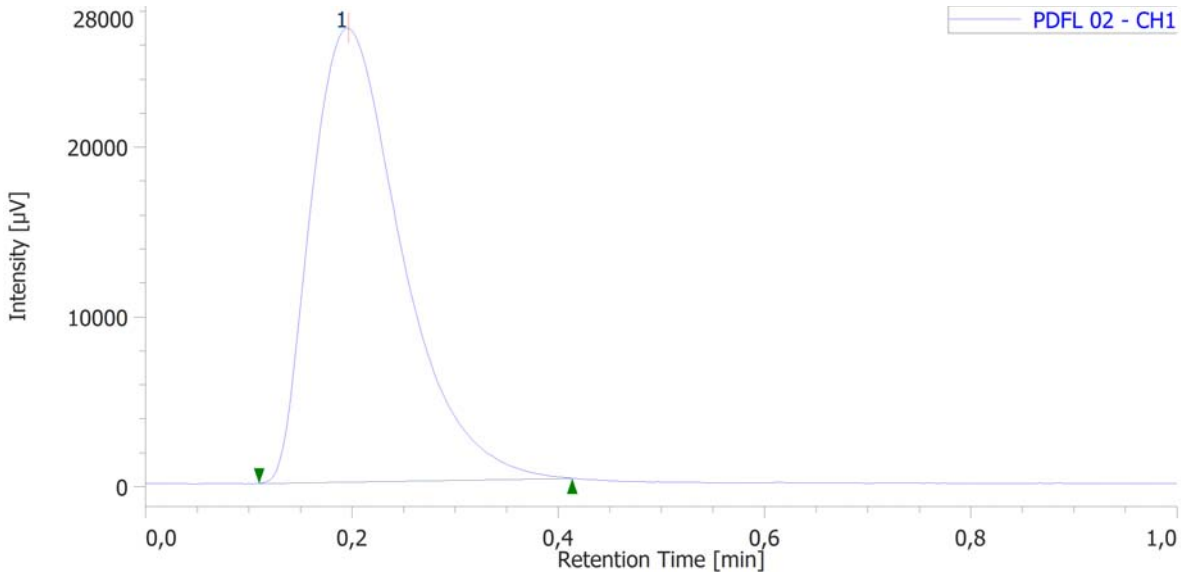

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:34
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2026 10:09:55
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,197	163243	26707	100,000	100,000	N/A	24	N/A	1,556		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

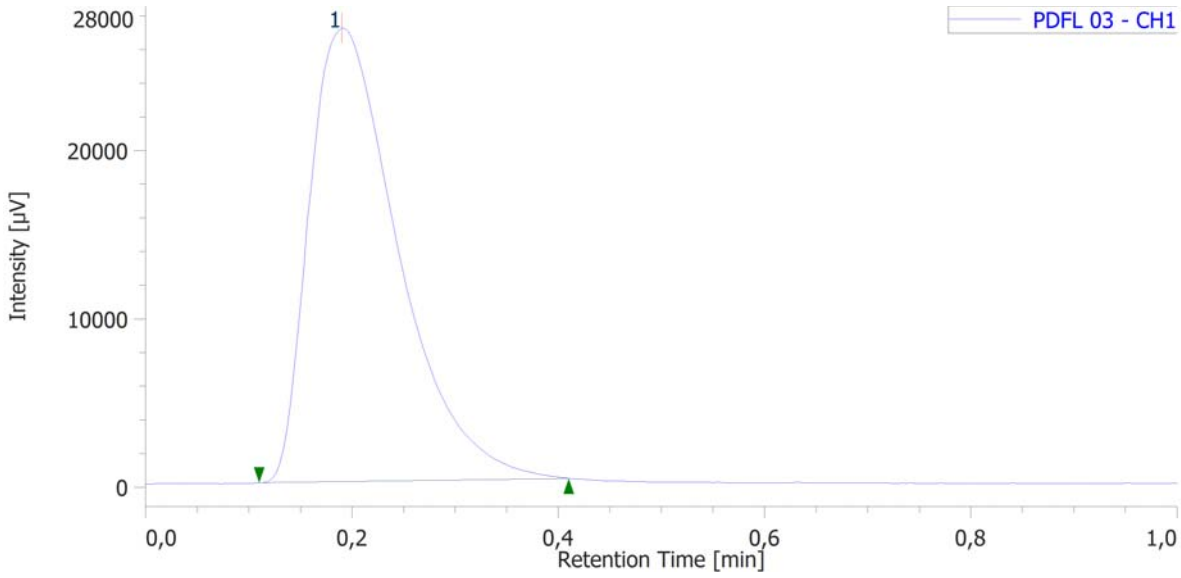

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:34
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2026 10:12:11
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,190	161506	26918	100,000	100,000	N/A	24	N/A	1,726		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

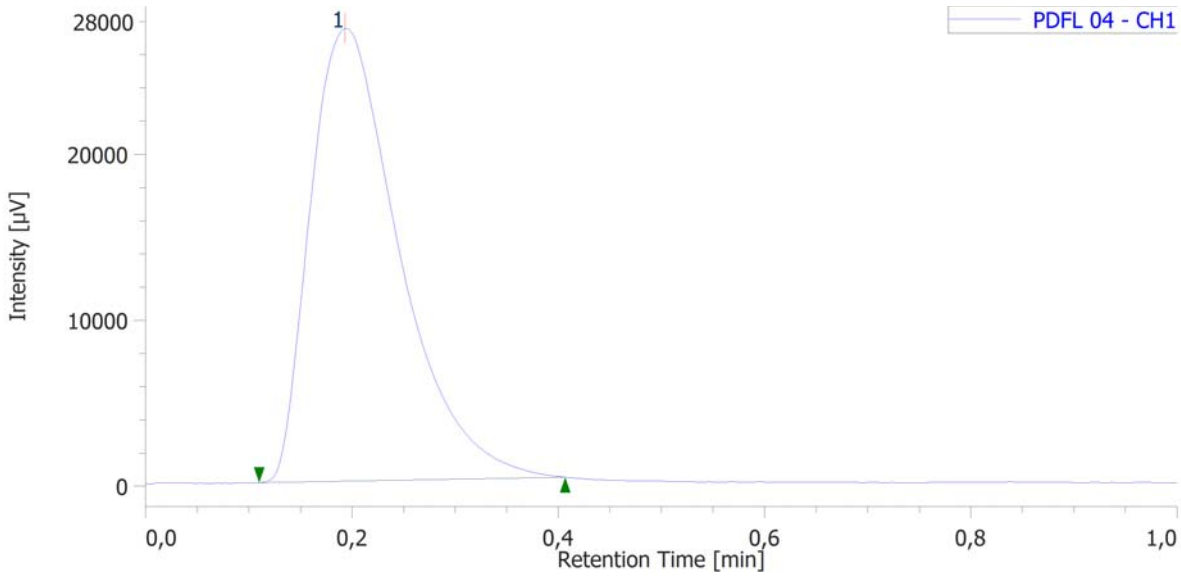

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:34
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2026 10:14:28
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,193	163439	27274	100,000	100,000	N/A	25	N/A	1,630		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

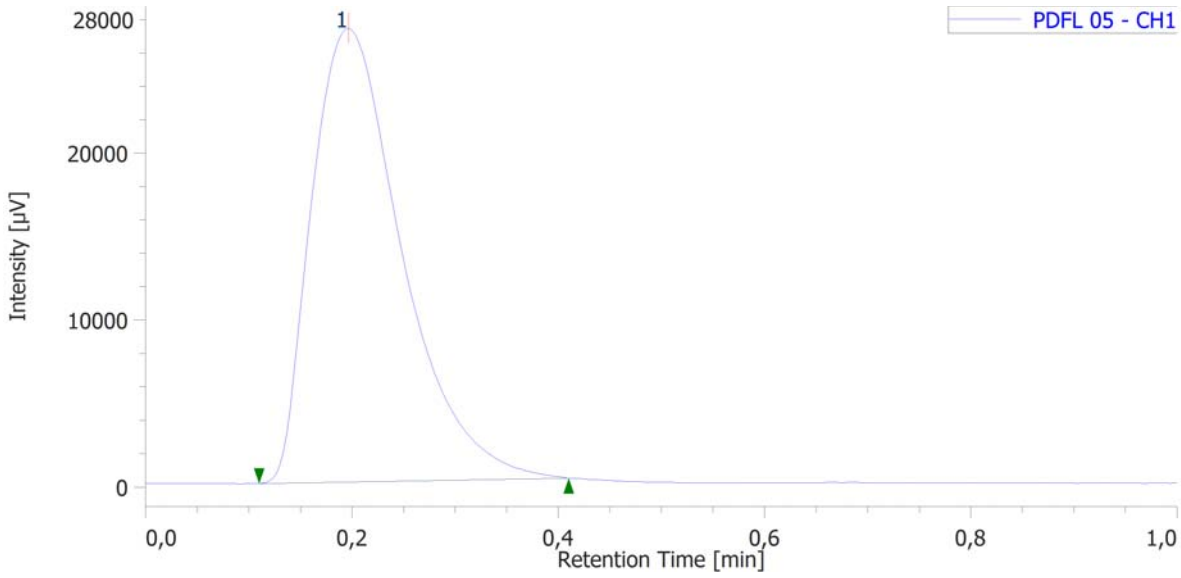

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:34
Description	
HPLC System Name	HP06 – Det FL
Injection Date	05/03/2026 10:16:43
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,197	165317	27161	100,000	100,000	N/A	24	N/A	1,572		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

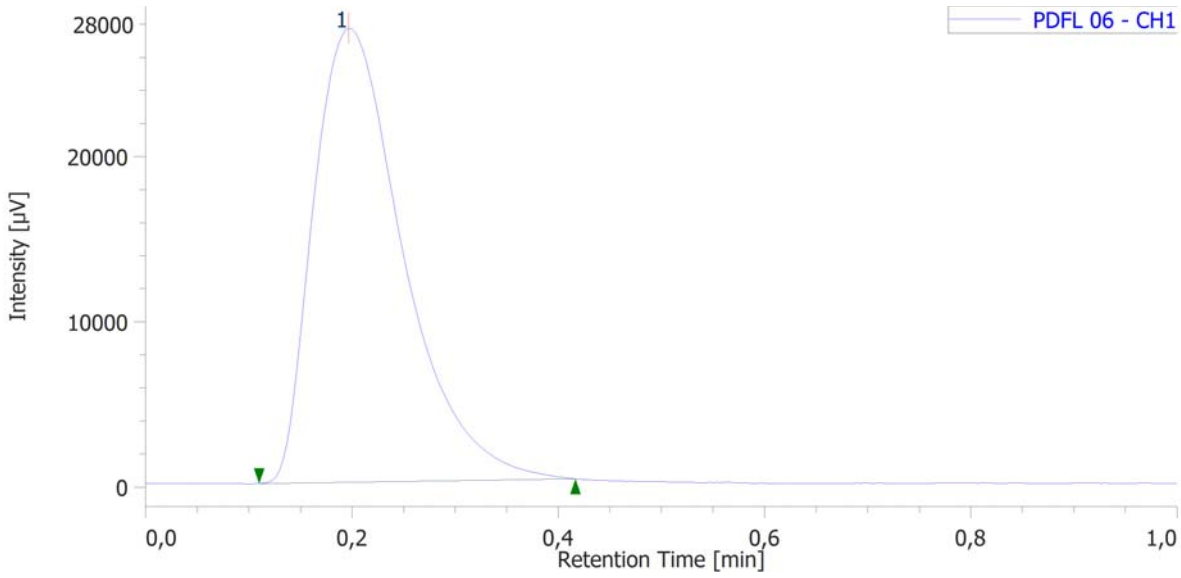

Chromatogram Information	
User Name	QPackSA
Date Modified	05/03/2026 10:31:35
Description	
HPLC System Name	HP06 - Det FL
Injection Date	05/03/2026 10:18:59
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PDFL 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,197	165882	27459	100,000	100,000	N/A	25	N/A	1,613		N/A

Creator QPackSA
Reviewer
Approver