Lab Advisor Diagnostic Result — Samix II

G7114A — Holmium Oxide Test — Passed

DEACX11868
D.07.25[0013]
1260 VWD

The test measures the Holmium spectrum from the built-in Holmium filter. The spectrum is evaluated for peaks at different wavelengths.


Results

Started at 6/10/2021 10:37:10 AM by Salmix-Lab\Salmix on SALMIX-LAB using Agilent Lab Advisor - Version B.02.10 [253] SP1 - Basic

Item	Value	Result
Accumulated UV Lamp Burn Time	2312.82 h	Done
UV Lamp On-Time	22.16 h	Done
Holmium Deviation to 360.8 nm	-0.20 nm	
Holmium Deviation Limit	*-1 ... 1 nm*	Passed
Holmium Deviation to 418.5 nm	-0.10 nm	
Holmium Deviation Limit	*-1 ... 1 nm*	Passed
Holmium Deviation to 536.4 nm	-0.10 nm	
Holmium Deviation Limit	*-1 ... 1 nm*	Passed

Finished at 6/10/2021 10:38:30 AM


Signals

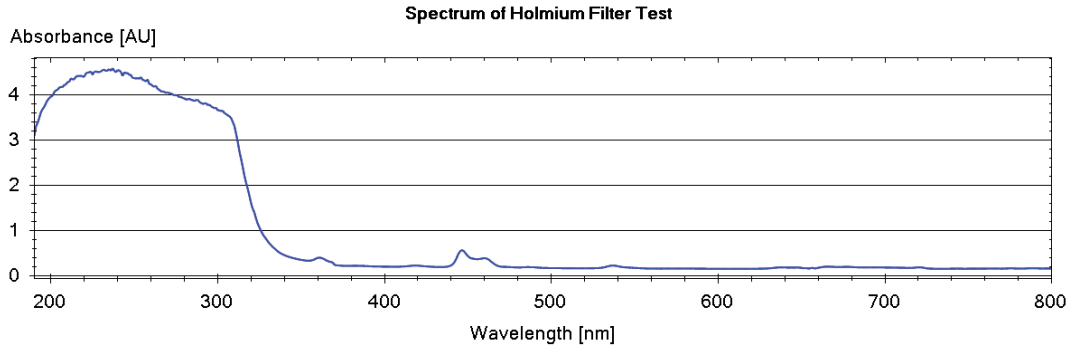

Signature: .....

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AA-0101.D
Sample Name: Branco PCIN 001

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   1
Acq. Instrument : HPLC Salmix II                 Location :   P2-A1
Injection Date  : 6/10/2021 11:06:33 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

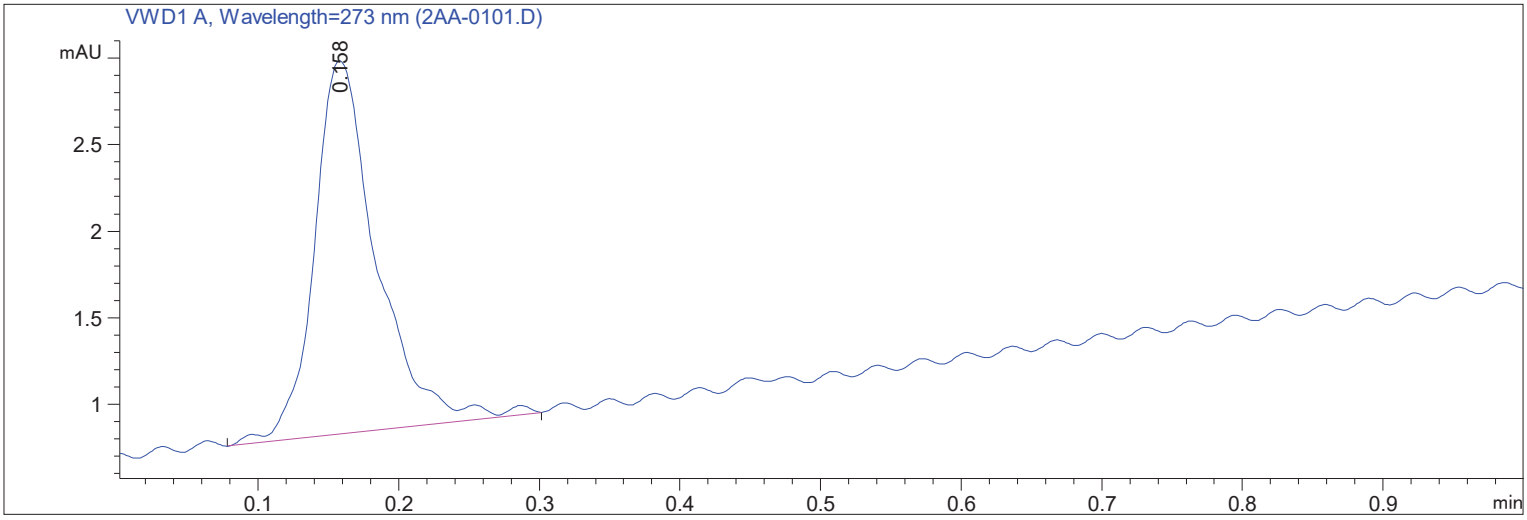


```
==================================================================
                        Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.158 VV R  0.0456    6.67642    2.15895 100.0000

Totals :                    6.67642    2.15895

==================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0201.D
Sample Name: PCIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   2
Acq. Instrument : HPLC Salmix II                  Location :   P2-A2
Injection Date  : 6/10/2021 11:08:17 AM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

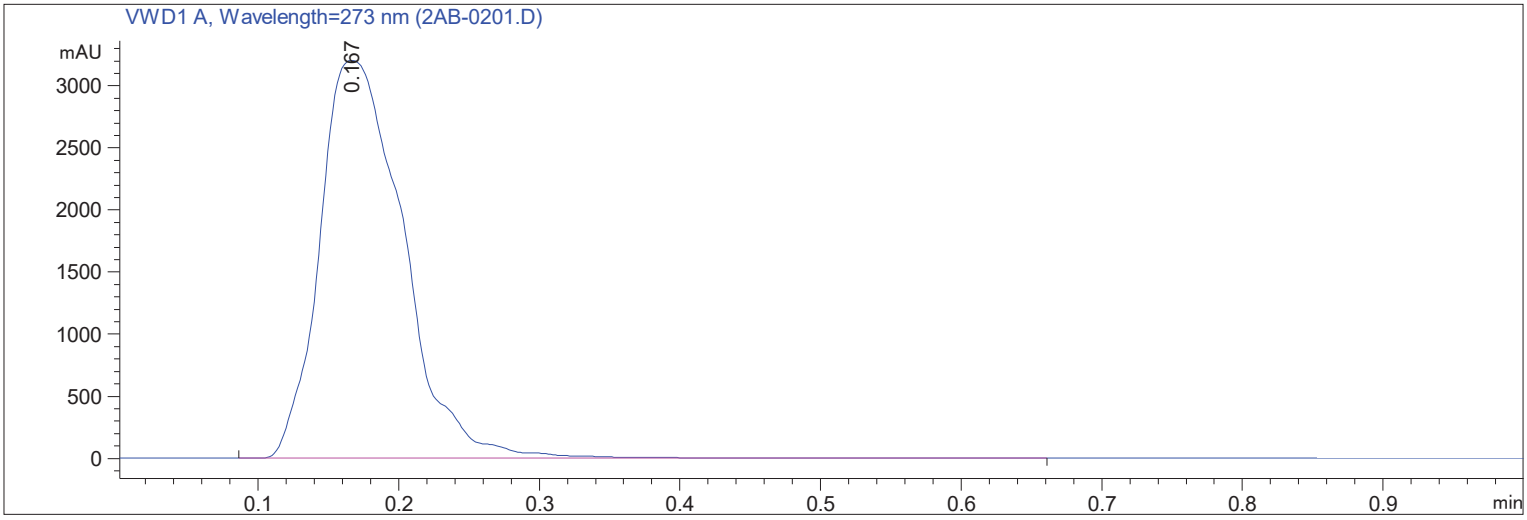


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.167 BV R  0.0601 1.32212e4  3204.77075 100.0000

Totals :                  1.32212e4  3204.77075


==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0301.D
Sample Name: PCIN 002

```
=====================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   3
Acq. Instrument : HPLC Salmix II                 Location :   P2-A2
Injection Date  : 6/10/2021 11:10:01 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

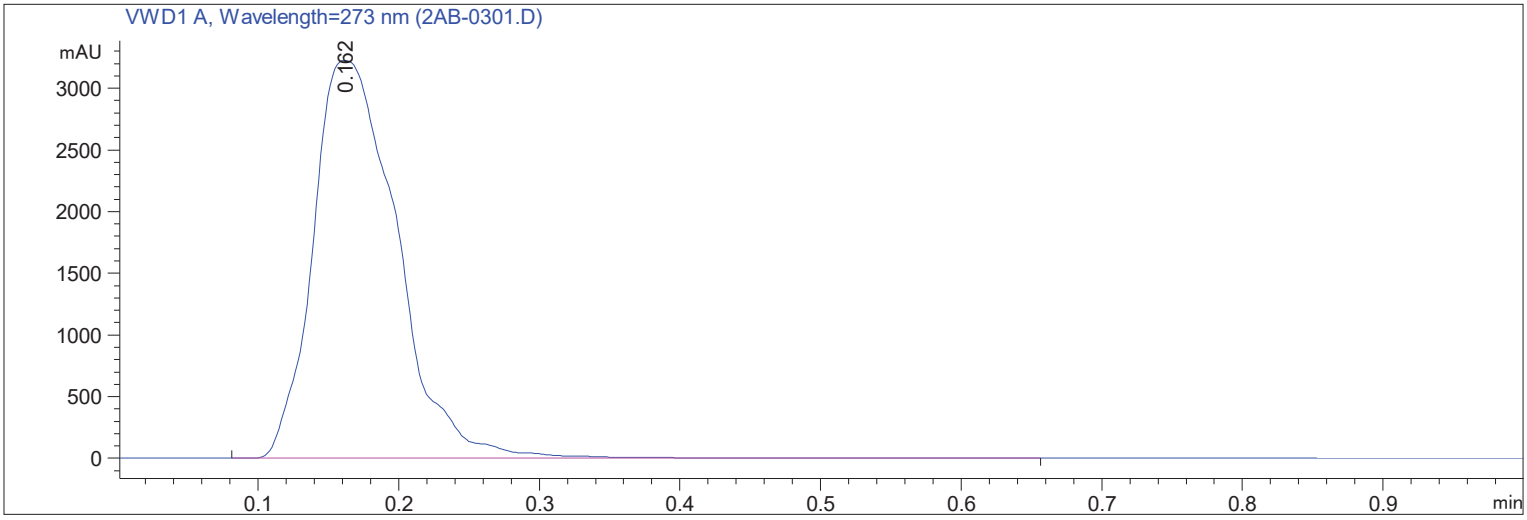


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.162 BV R  0.0604 1.33709e4  3225.66968 100.0000

Totals :                  1.33709e4  3225.66968


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0401.D
Sample Name: PCIN 003

```
=====================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   4
Acq. Instrument : HPLC Salmix II                 Location :   P2-A2
Injection Date  : 6/10/2021 11:11:44 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

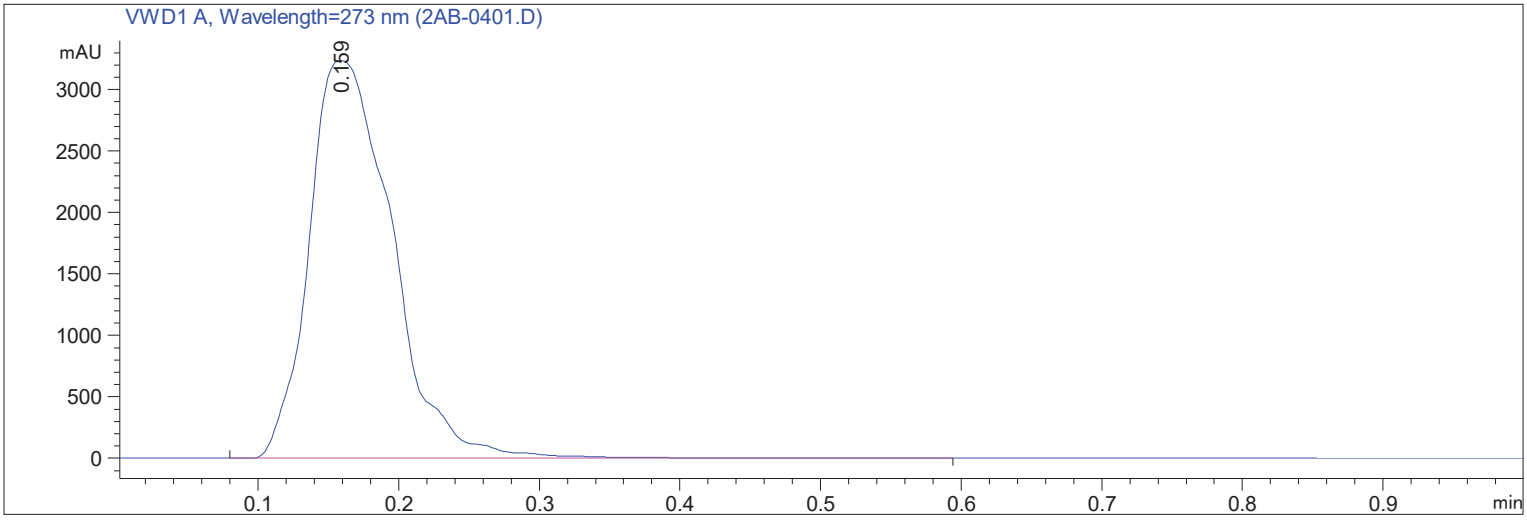


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.159 BV R  0.0598 1.32678e4  3237.51758 100.0000

Totals :                  1.32678e4  3237.51758


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AA-0501.D
Sample Name: Branco PCIN 002

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   5
Acq. Instrument : HPLC Salmix II                 Location :   P2-A1
Injection Date  : 6/10/2021 11:13:27 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

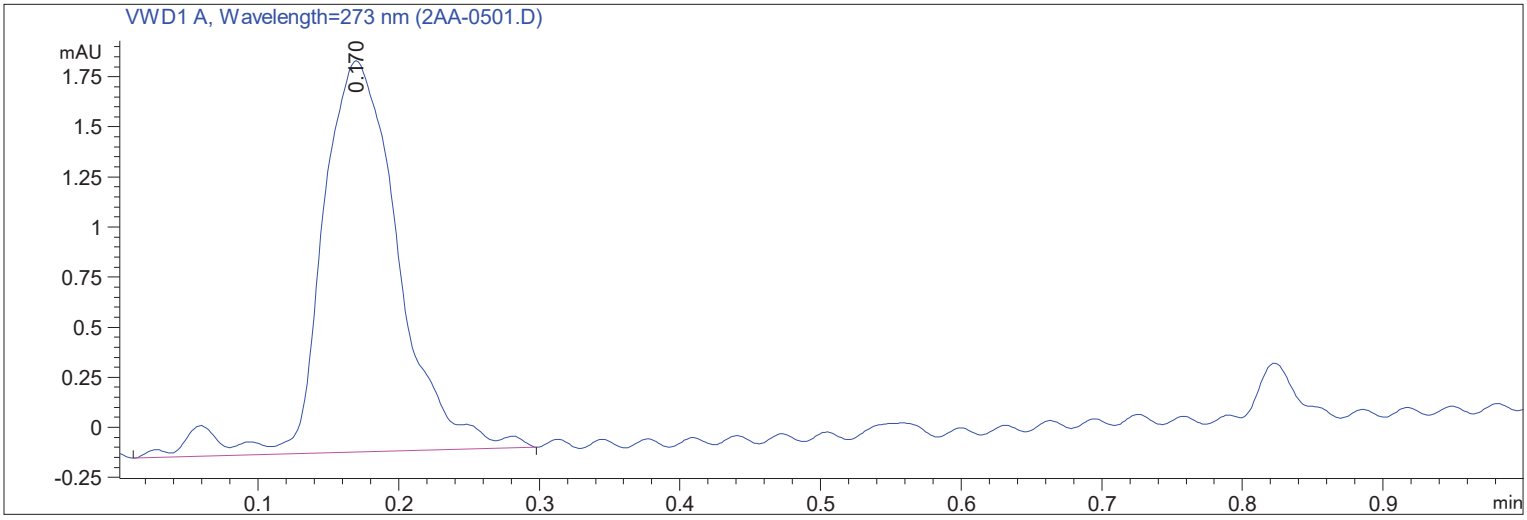


```
==================================================================
                        Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.170 VV R  0.0558    7.50664    1.95554 100.0000

Totals :                    7.50664    1.95554

==================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0601.D
Sample Name: PCIN 004

```
=====================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   6
Acq. Instrument : HPLC Salmix II                  Location :   P2-A2
Injection Date  : 6/10/2021 11:15:10 AM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

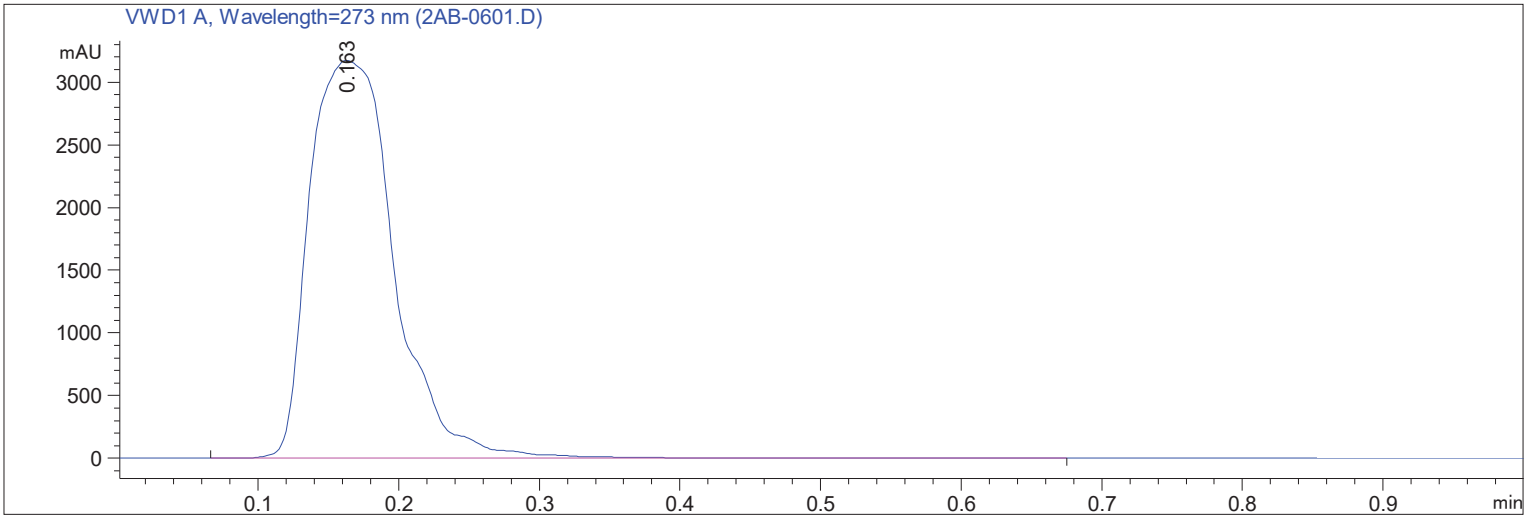


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.163 BV R  0.0670 1.33169e4  3173.01709 100.0000

Totals :                  1.33169e4  3173.01709


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0701.D
Sample Name: PCIN 005

```
=====================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   7
Acq. Instrument : HPLC Salmix II                 Location :   P2-A2
Injection Date  : 6/10/2021 11:16:54 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

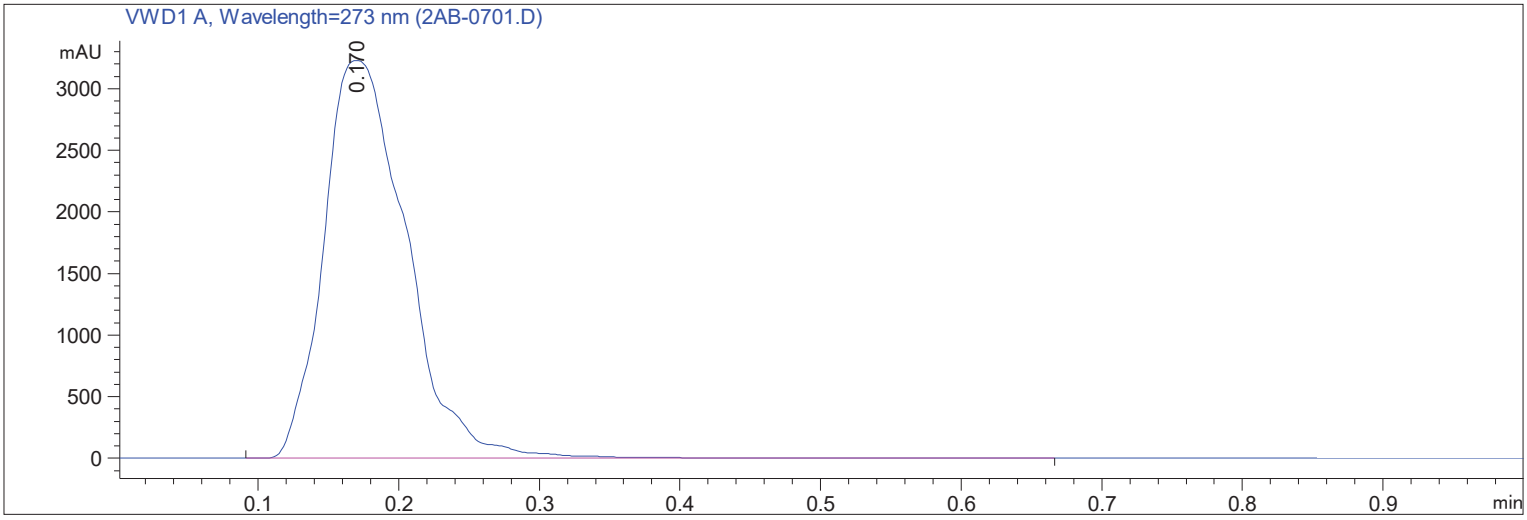


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.170 BV R  0.0595 1.31602e4  3229.98340 100.0000

Totals :                  1.31602e4  3229.98340


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AB-0801.D
Sample Name: PCIN 006

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   8
Acq. Instrument : HPLC Salmix II                 Location :   P2-A2
Injection Date  : 6/10/2021 11:18:38 AM               Inj :   1
                                               Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

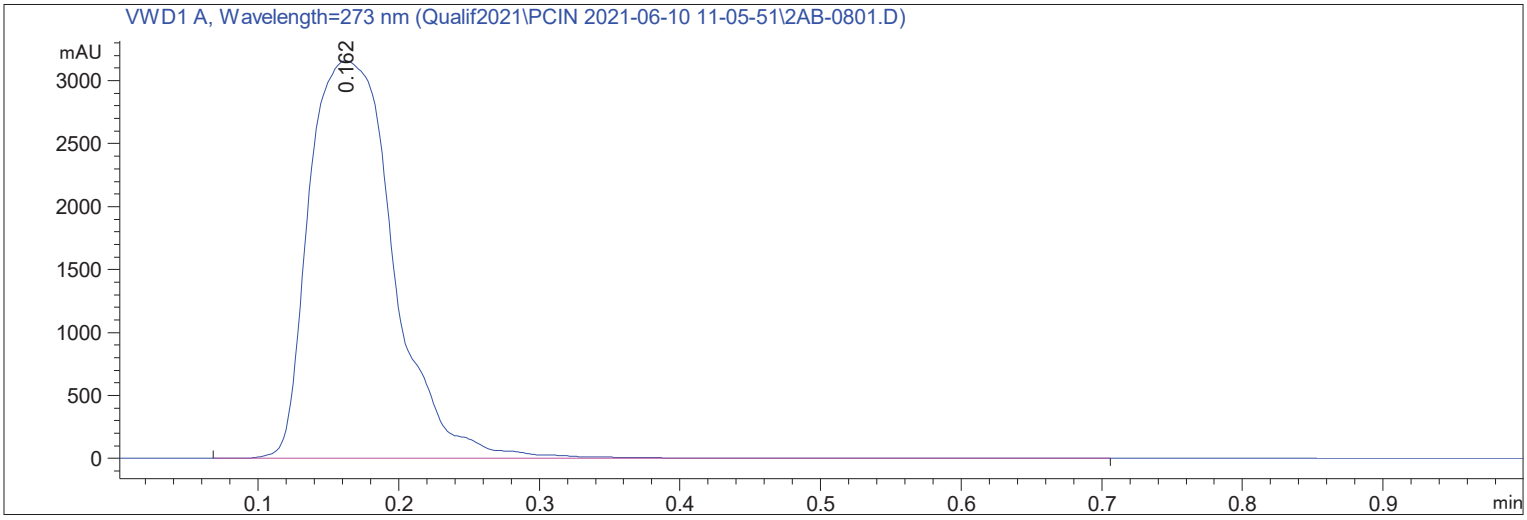


```
==================================================================
                        Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.162 BV R  0.0669 1.32415e4  3160.59033 100.0000

Totals :                  1.32415e4  3160.59033


==================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\2AA-0901.D
Sample Name: Branco PCIN 003

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   9
Acq. Instrument : HPLC Salmix II                 Location :   P2-A1
Injection Date  : 6/10/2021 11:20:22 AM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\PCIN.S
Method          : C:\Chem32\2\Data\Qualif2021\PCIN 2021-06-10 11-05-51\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 11:05:51 AM by SISTEMA
```

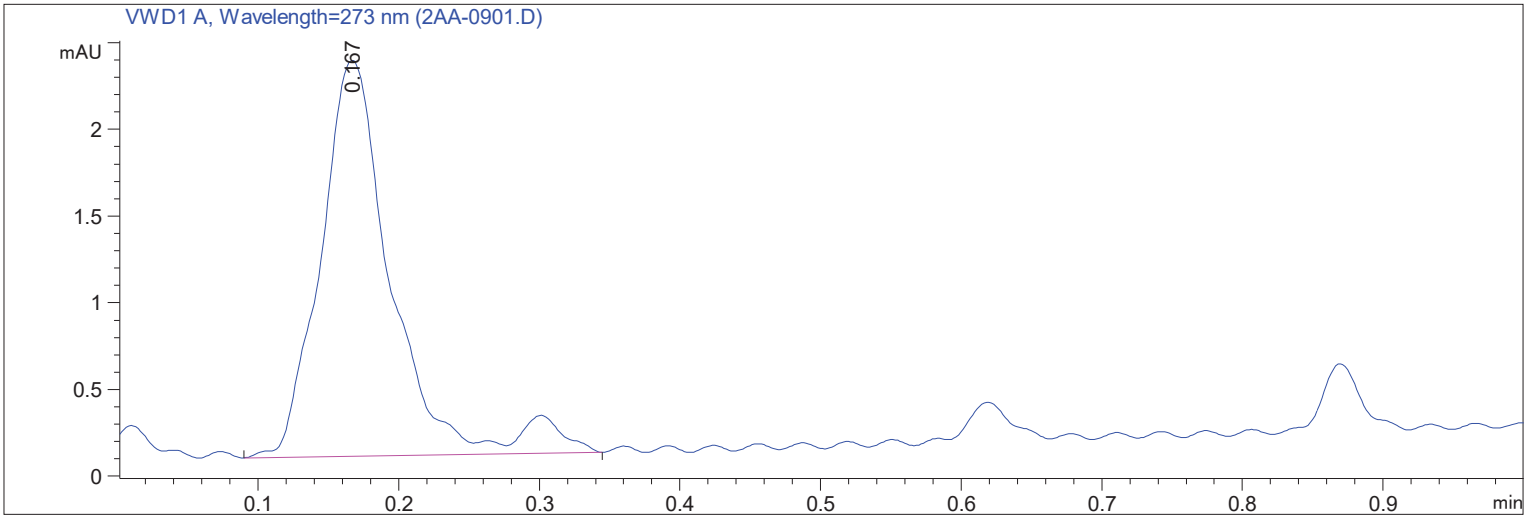


```
==================================================================
                        Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.167 BV R  0.0514    8.09517    2.28317 100.0000

Totals :                    8.09517    2.28317


==================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\2AA-0101.D
Sample Name: LDUV 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   1
Acq. Instrument : HPLC Salmix II                  Location :   P2-A1
Injection Date  : 6/10/2021 12:04:57 PM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\LDUV.S
Method          : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:04:18 PM by SISTEMA
```

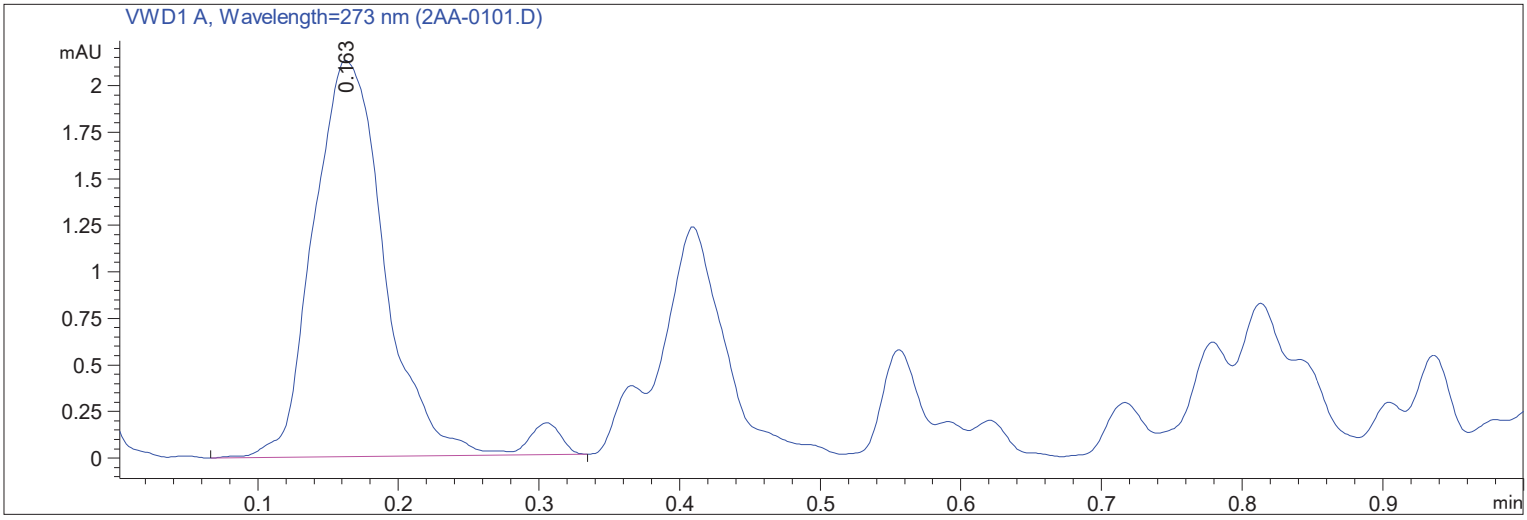


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.163 BV R  0.0532    7.69961    2.12895 100.0000

Totals :                    7.69961    2.12895

==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\2AB-0201.D
Sample Name: LDUV 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC Salmix II                    Location :   P2-A2
Injection Date  : 6/10/2021 12:06:39 PM                 Inj :   1
                                                  Inj Volume : 5.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\LDUV.S
Method          : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:04:18 PM by SISTEMA
```

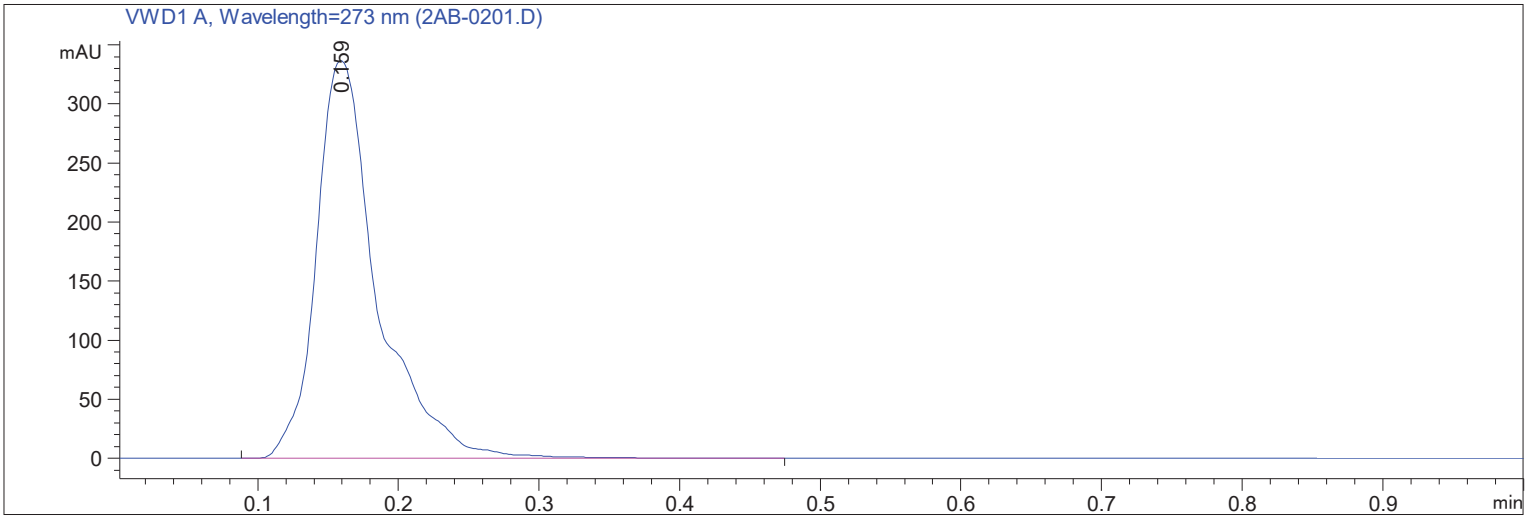


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.159 BV R  0.0453 1020.21893  337.17578 100.0000

Totals :                  1020.21893  337.17578


==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\2AC-0301.D
Sample Name: LDUV 003

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   3
Acq. Instrument : HPLC Salmix II                  Location :   P2-A3
Injection Date  : 6/10/2021 12:08:21 PM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\LDUV.S
Method          : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:04:18 PM by SISTEMA
```

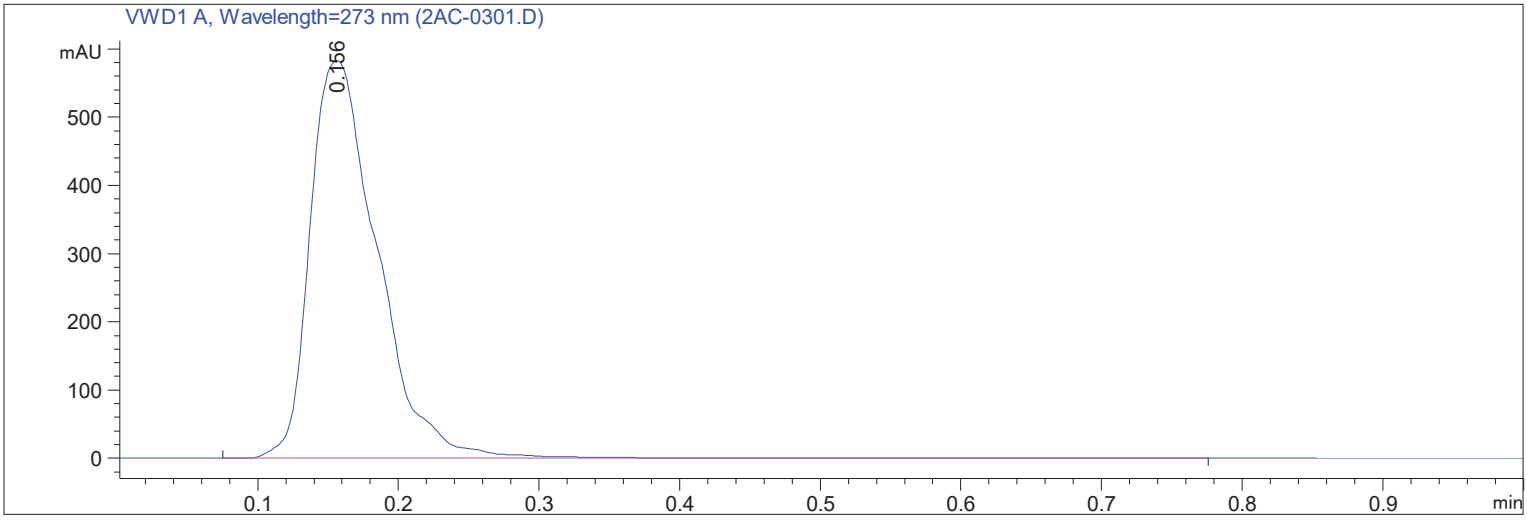


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.156 BV R  0.0493 1939.65417  583.42700 100.0000

Totals :                  1939.65417  583.42700


==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\2AD-0401.D
Sample Name: LDUV 004

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   4
Acq. Instrument : HPLC Salmix II                  Location :   P2-A4
Injection Date  : 6/10/2021 12:10:06 PM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\LDUV.S
Method          : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:04:18 PM by SISTEMA
```

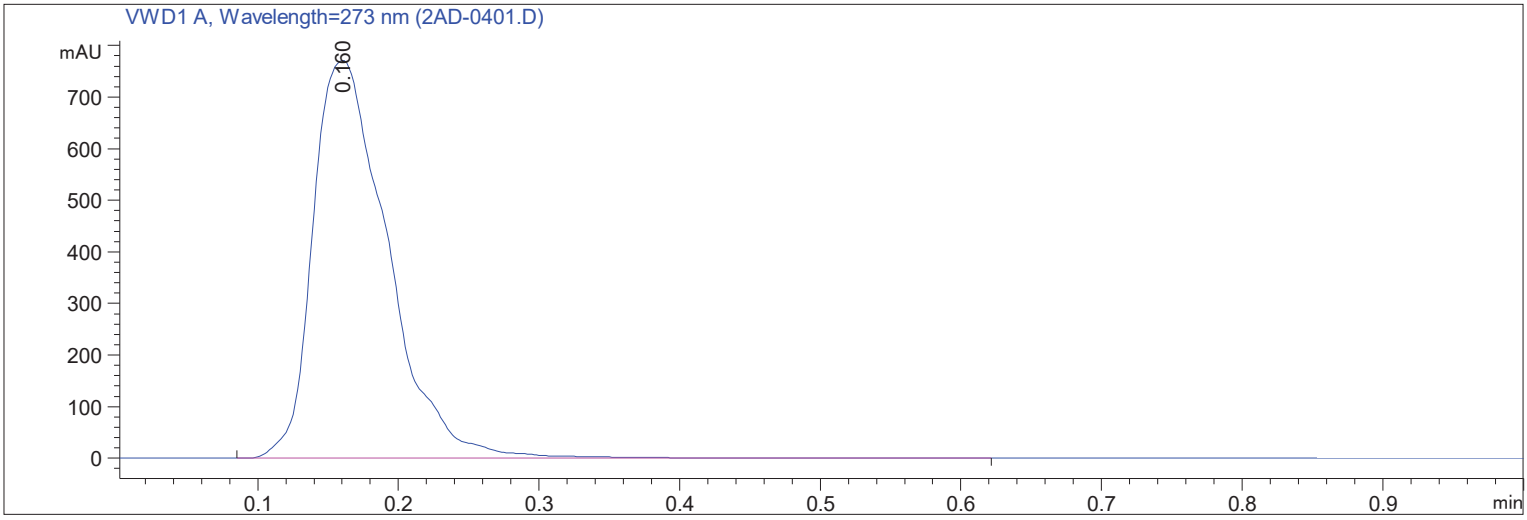


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.160 BB    0.0542 2856.99365  771.29572 100.0000

Totals :                  2856.99365  771.29572

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\2AE-0501.D
Sample Name: LDUV 005

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   5
Acq. Instrument : HPLC Salmix II                  Location :   P2-A5
Injection Date  : 6/10/2021 12:11:54 PM               Inj :   1
                                                Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\LDUV.S
Method          : C:\Chem32\2\Data\Qualif2021\LDUV 2021-06-10 12-04-18\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:04:18 PM by SISTEMA
```

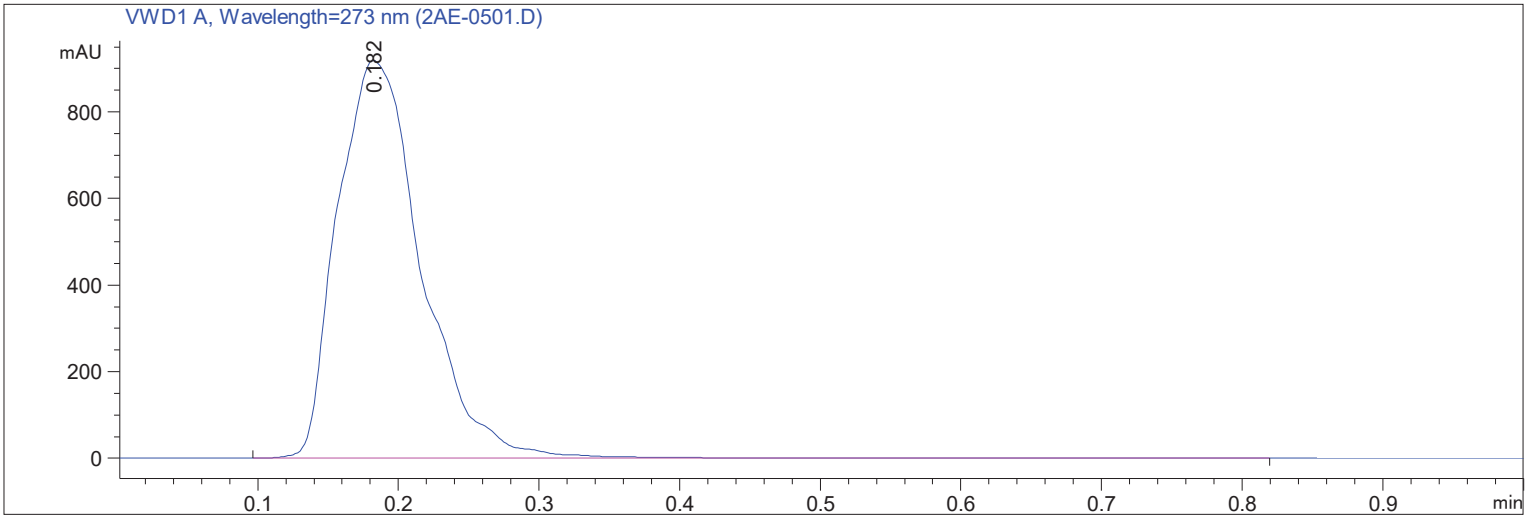


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.182 BV R  0.0599 3812.09351  919.20471 100.0000

Totals :                  3812.09351  919.20471

==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\2AF-0101.D
Sample Name: LIIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   1
Acq. Instrument : HPLC Salmix II                  Location :   P2-A6
Injection Date  : 6/10/2021 12:20:09 PM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\LIIN.S
Method          : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:19:27 PM by SISTEMA
```

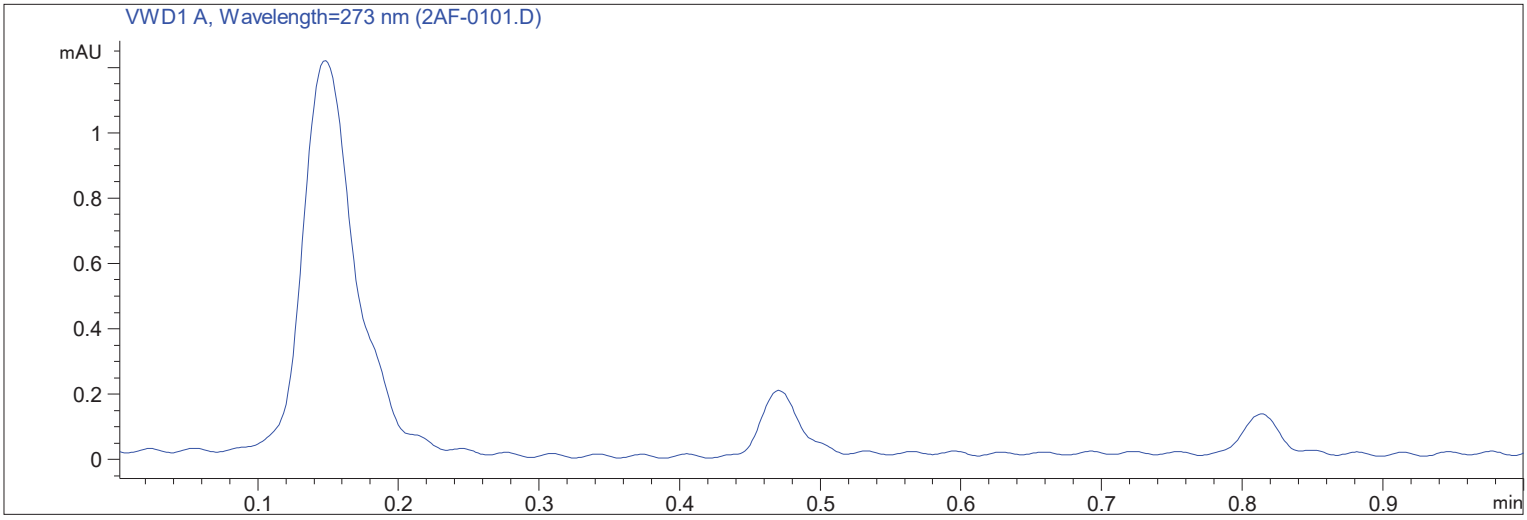


```
==========================================================================
                        Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\2AF-0201.D
Sample Name: LIIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC Salmix II                    Location :   P2-A6
Injection Date  : 6/10/2021 12:21:48 PM                 Inj :   1
                                                  Inj Volume : 5.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\LIIN.S
Method          : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:19:27 PM by SISTEMA
```

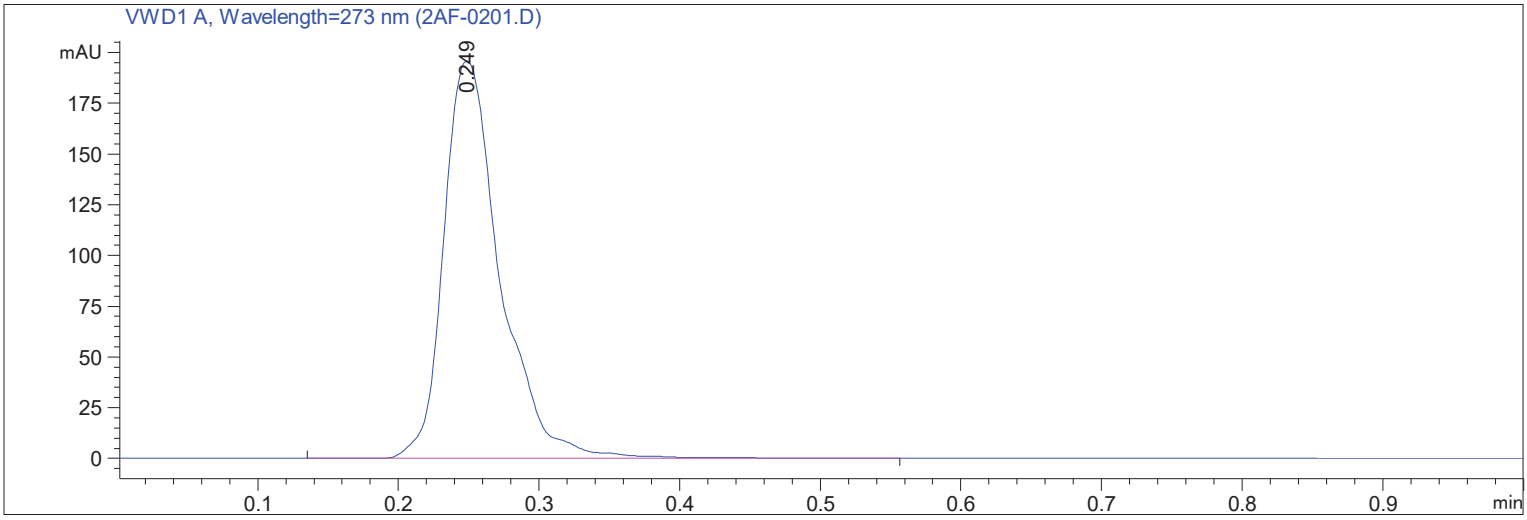


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.249 BV R  0.0420  546.79694  196.05177 100.0000

Totals :                   546.79694  196.05177


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\2AF-0301.D
Sample Name: LIIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   3
Acq. Instrument : HPLC Salmix II                    Location :   P2-A6
Injection Date  : 6/10/2021 12:23:30 PM                 Inj :   1
                                                  Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 10.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\LIIN.S
Method          : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:19:27 PM by SISTEMA
```

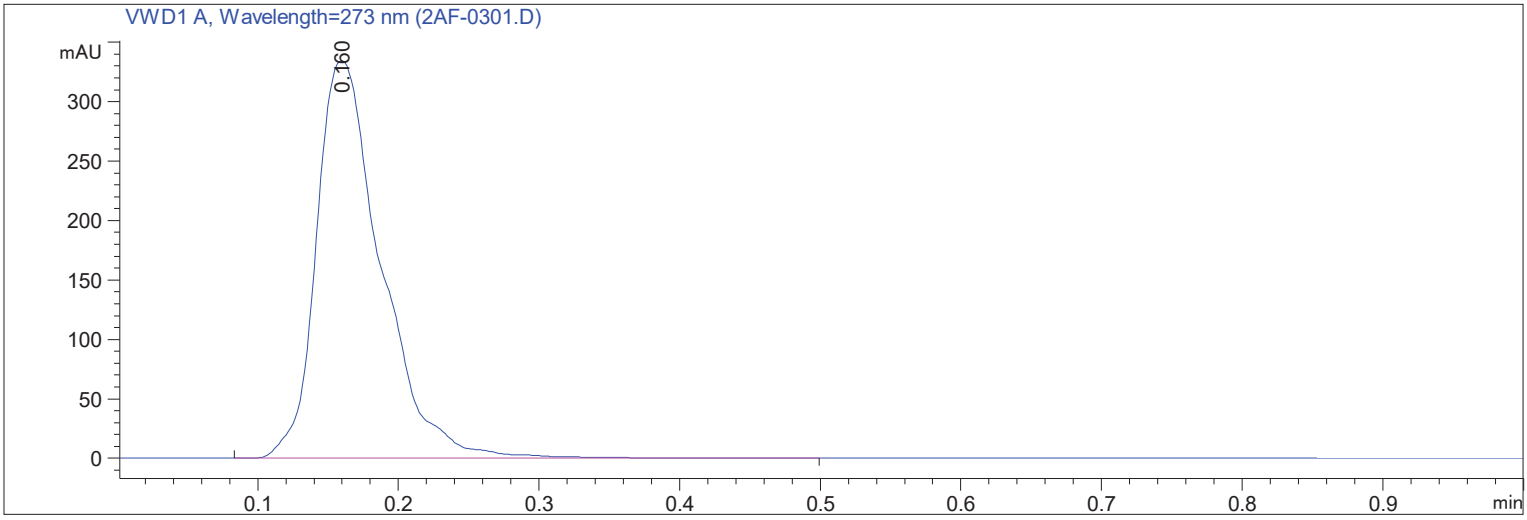


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.160 BB    0.0479 1072.09119  334.77274 100.0000

Totals :                  1072.09119  334.77274


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\2AF-0401.D
Sample Name: LIIN 004

```
=====================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   4
Acq. Instrument : HPLC Salmix II                  Location :   P2-A6
Injection Date  : 6/10/2021 12:25:16 PM               Inj :   1
                                                 Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\LIIN.S
Method          : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:19:27 PM by SISTEMA
```

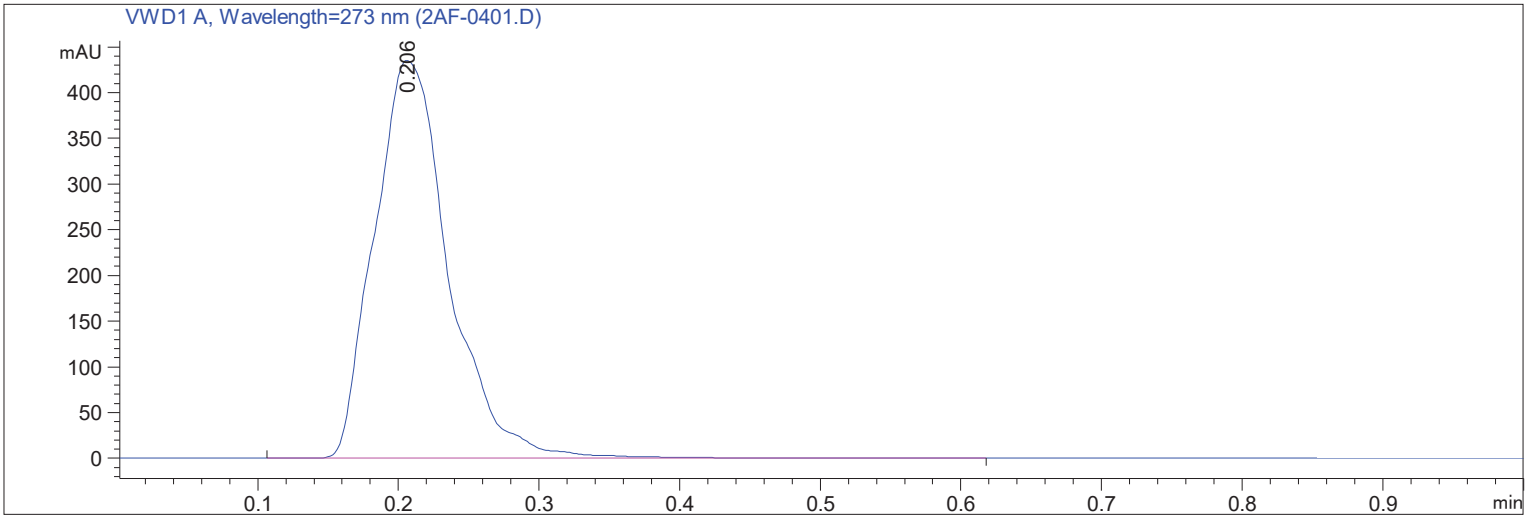


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.206 BB    0.0539 1599.49658  435.30353 100.0000

Totals :                  1599.49658  435.30353


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\2AF-0501.D
Sample Name: LIIN 005

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   5
Acq. Instrument : HPLC Salmix II                 Location :   P2-A6
Injection Date  : 6/10/2021 12:27:04 PM               Inj :   1
                                               Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Sequence File   : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\LIIN.S
Method          : C:\Chem32\2\Data\Qualif2021\LIIN 2021-06-10 12-19-27\QUALIFICAÇÃO.M (
                  Sequence Method)
Last changed    : 6/10/2021 12:19:27 PM by SISTEMA
```

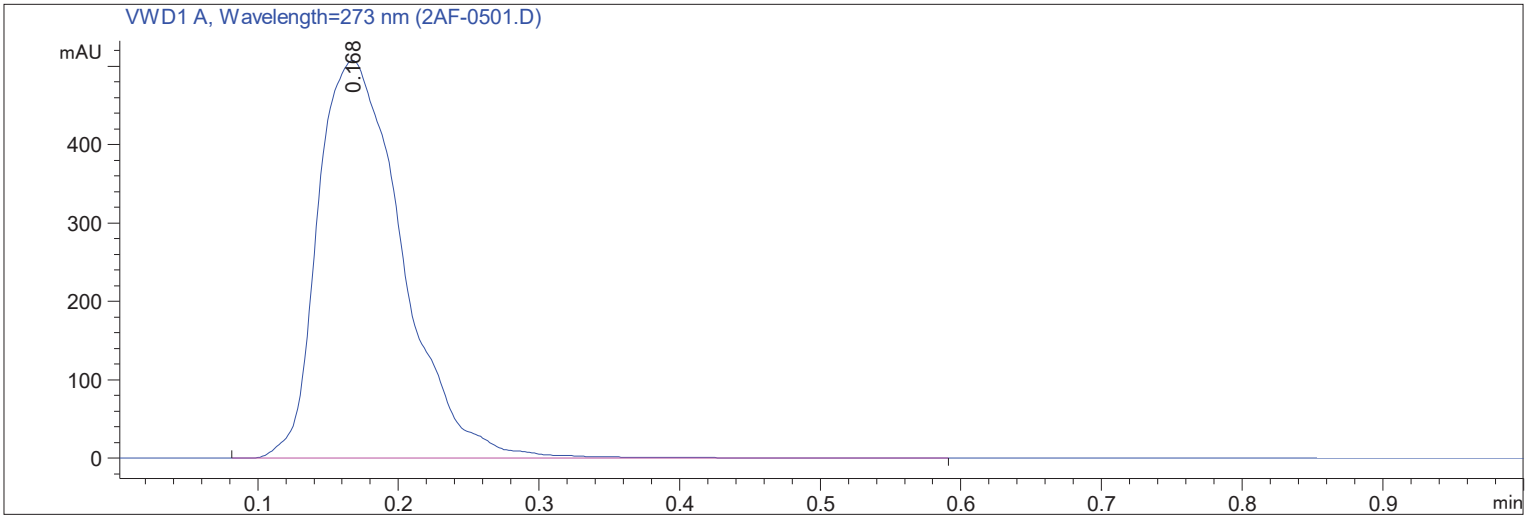


```
==================================================================
                        Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.168 BV R  0.0604 2126.95117  507.64133 100.0000

Totals :                  2126.95117  507.64133


==================================================================
                        *** End of Report ***
```