
Chromatogram

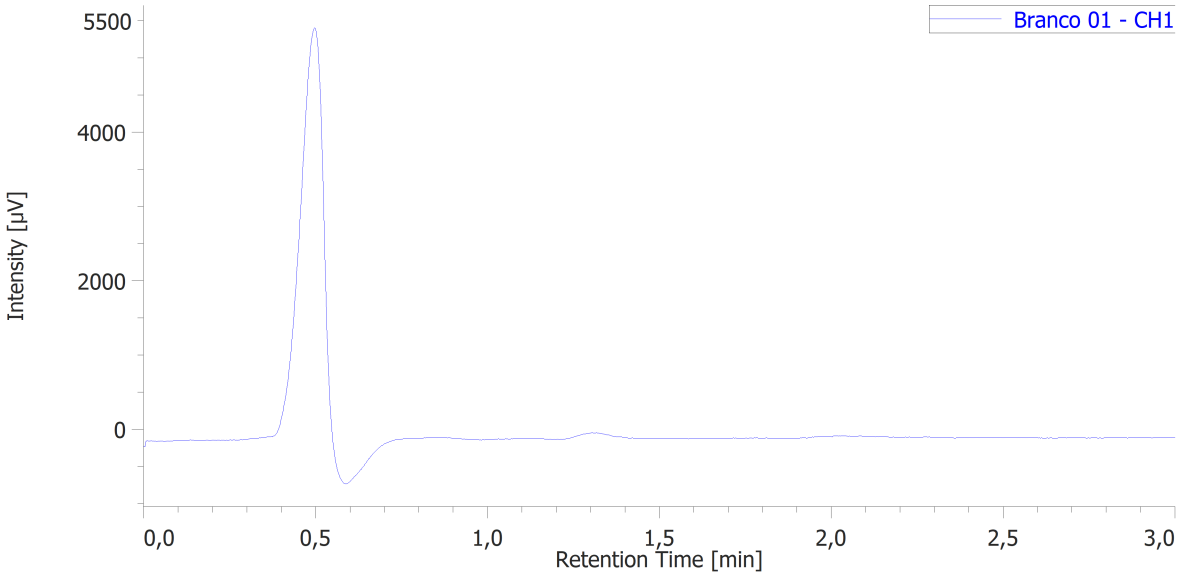


Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:17:34
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:04:38
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

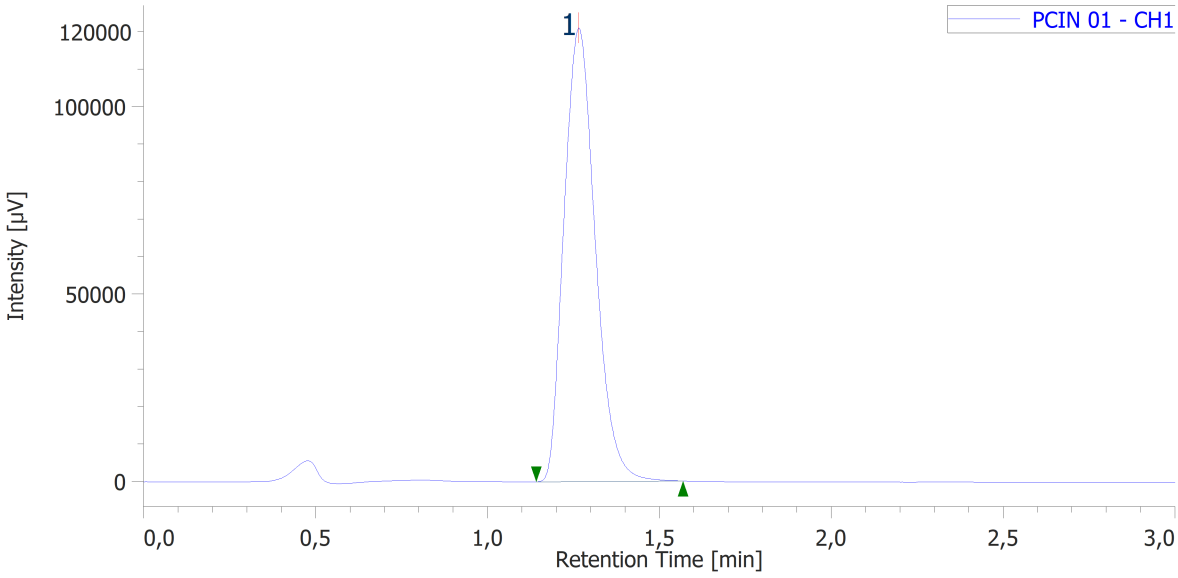

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:17:34
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:08:59
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,265	764908	120945	100,000	100,000	N/A	912	N/A	1,230	

Creator QPackSA
Reviewer
Approver

Chromatogram

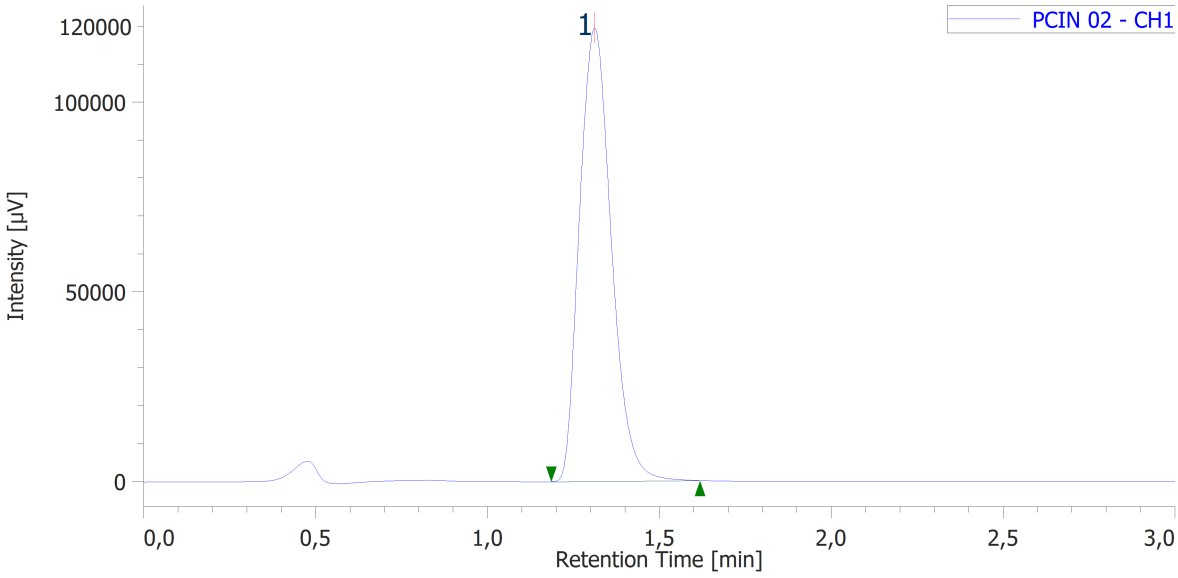

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:17:35
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:13:20
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,312	768901	119489	100,000	100,000	N/A	941	N/A	1,220	

Creator QPackSA
Reviewer
Approver

Chromatogram

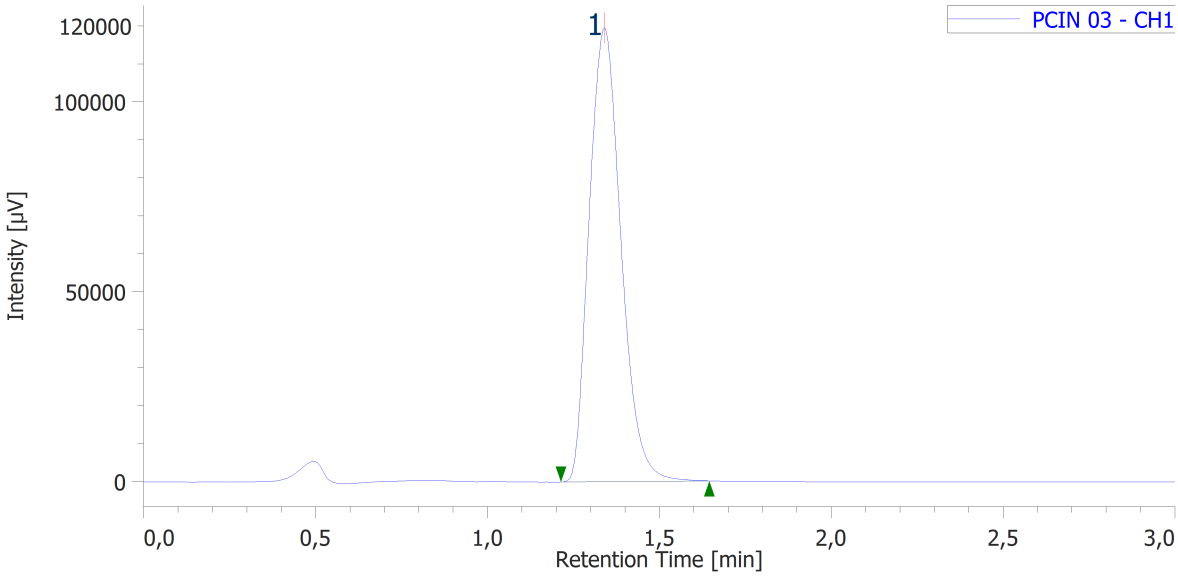

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:21:36
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:17:38
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,340	768356	119452	100,000	100,000	N/A	981	N/A	1,208	

Creator QPackSA
Reviewer
Approver

Chromatogram

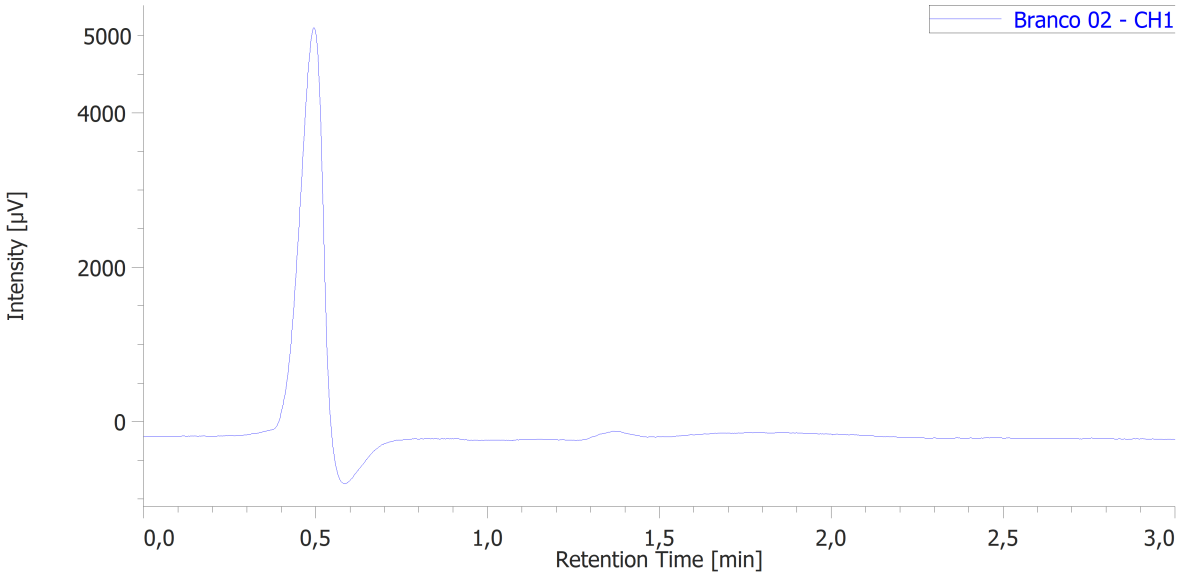


Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:30:42
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:21:56
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

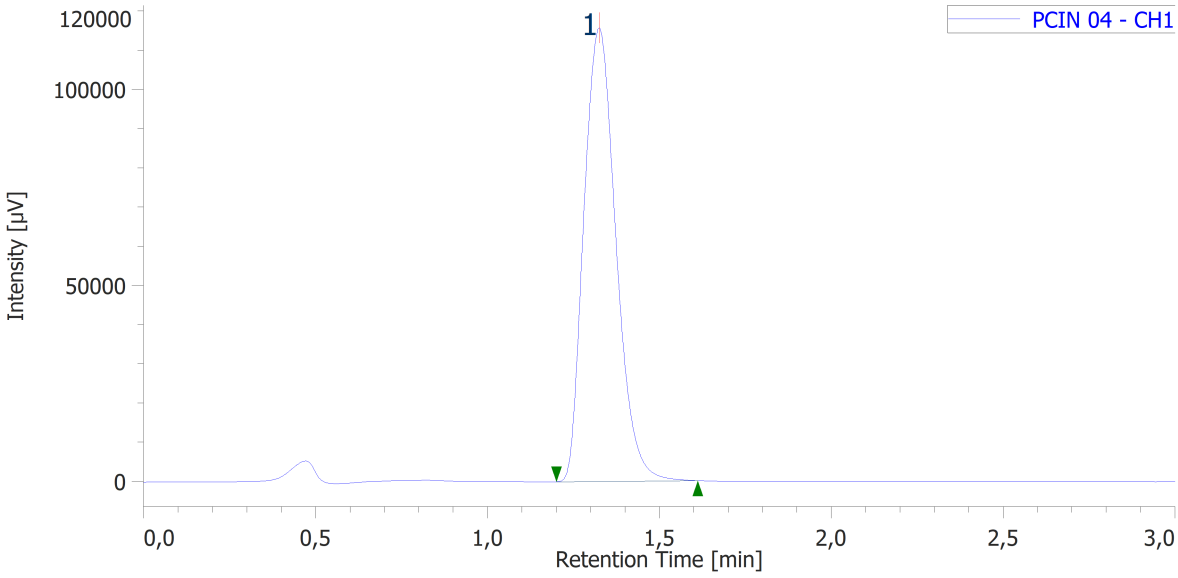

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:30:42
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:26:17
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,325	749135	115638	100,000	100,000	N/A	942	N/A	1,213	

Creator QPackSA
Reviewer
Approver

Chromatogram

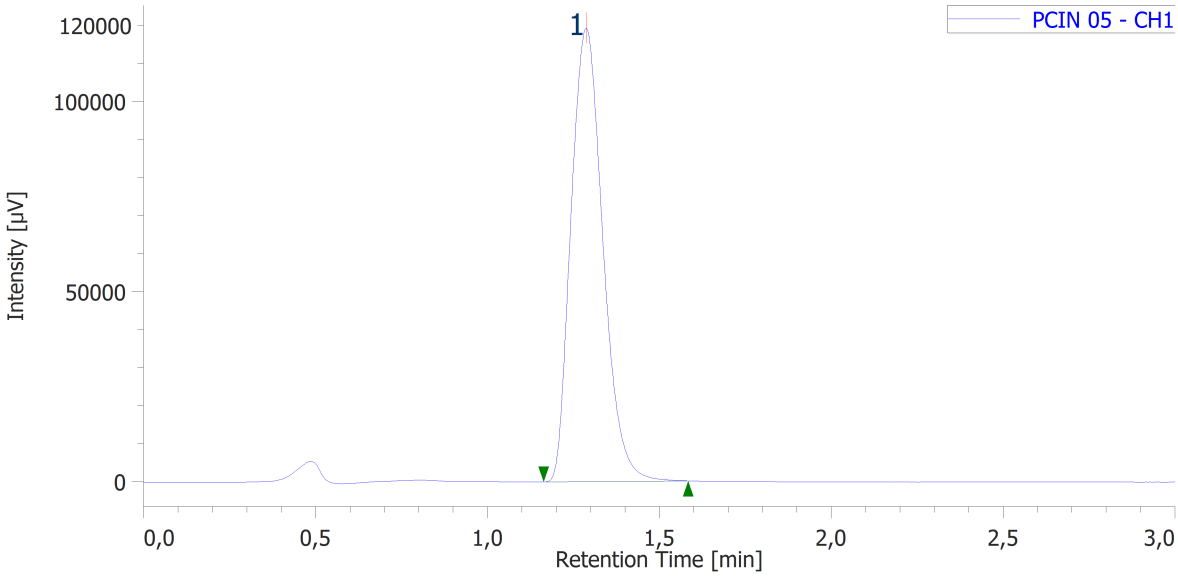

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:34:10
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:30:36
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,287	766989	119253	100,000	100,000	N/A	903	N/A	1,221	

Creator QPackSA
Reviewer
Approver

Chromatogram

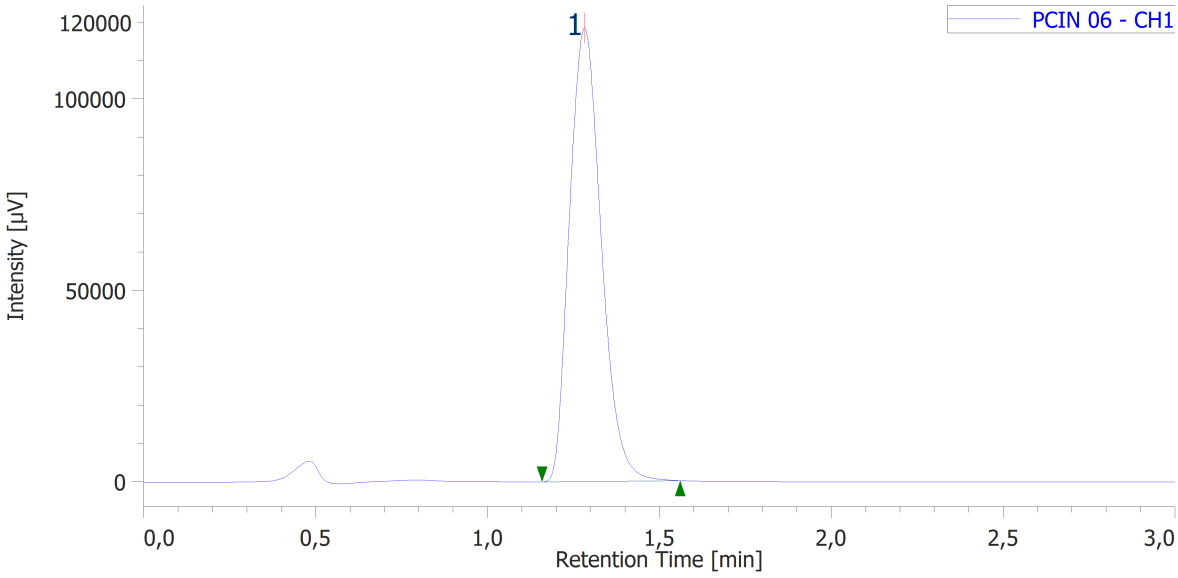

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 14:38:14
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:34:54
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,282	760305	118482	100,000	100,000	N/A	899	N/A	1,226	

Creator QPackSA
Reviewer
Approver

Chromatogram

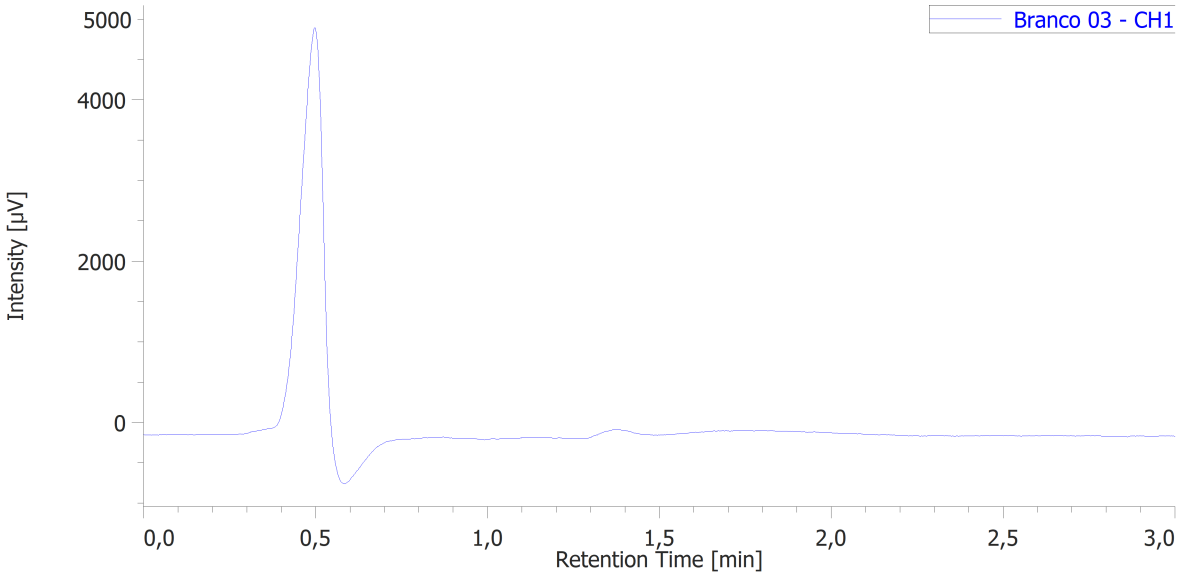


Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:21:23
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 14:39:12
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

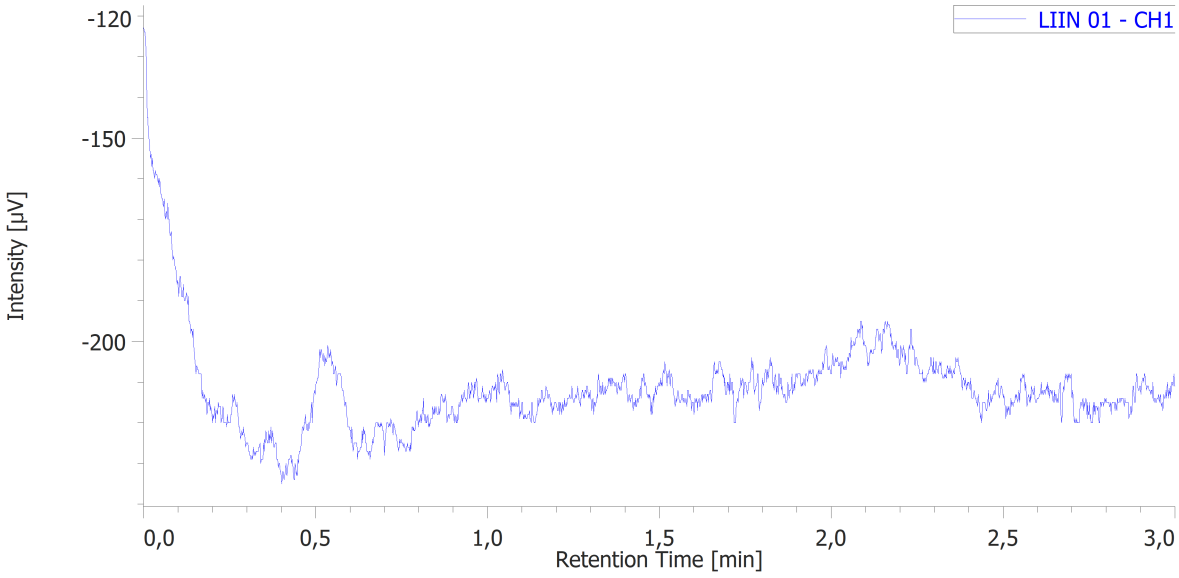


Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:36:09
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 17:17:44
Volume	0,1 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

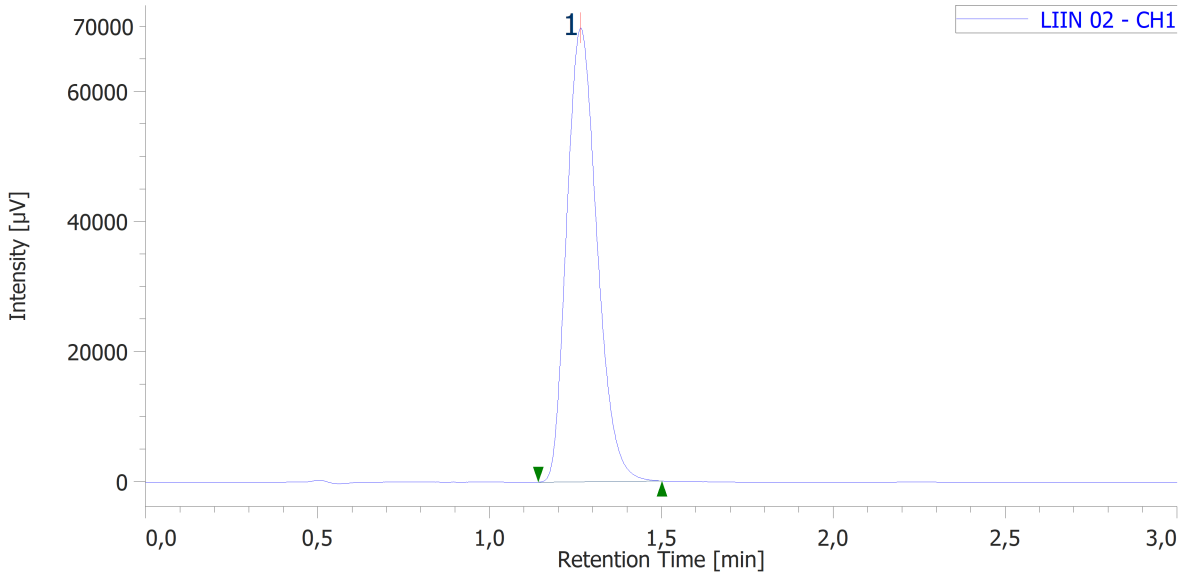

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:36:09
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 17:21:23
Volume	5,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,265	426944	69740	100,000	100,000	N/A	976	N/A	1,227	

Creator QPackSA
Reviewer
Approver

Chromatogram

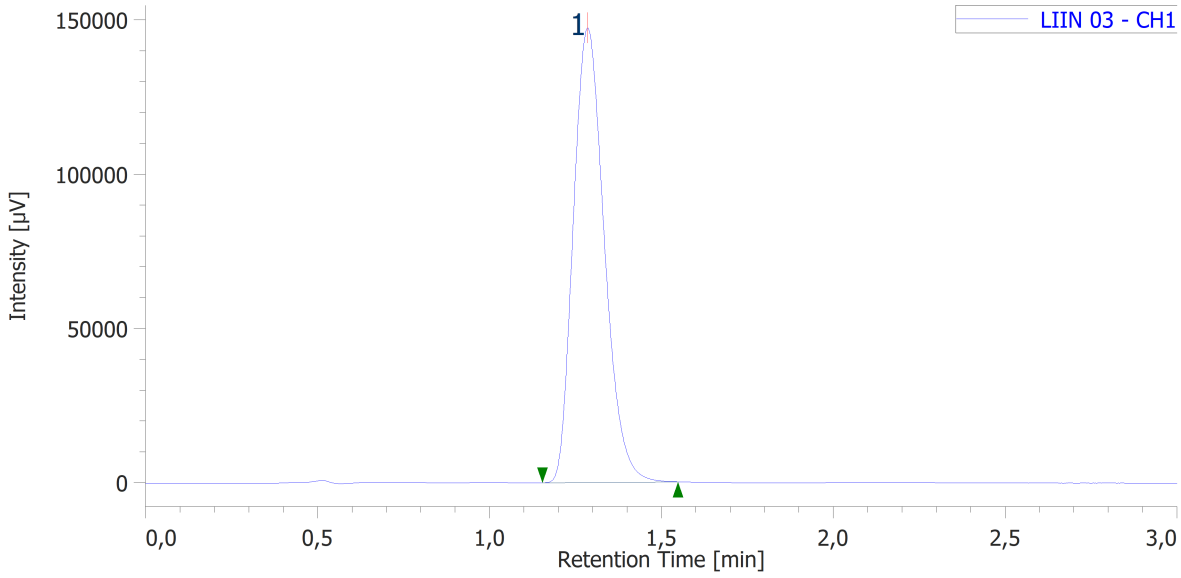

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:36:09
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 17:25:05
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,285	921593	147243	100,000	100,000	N/A	962	N/A	1,235	

Creator QPackSA
Reviewer
Approver

Chromatogram

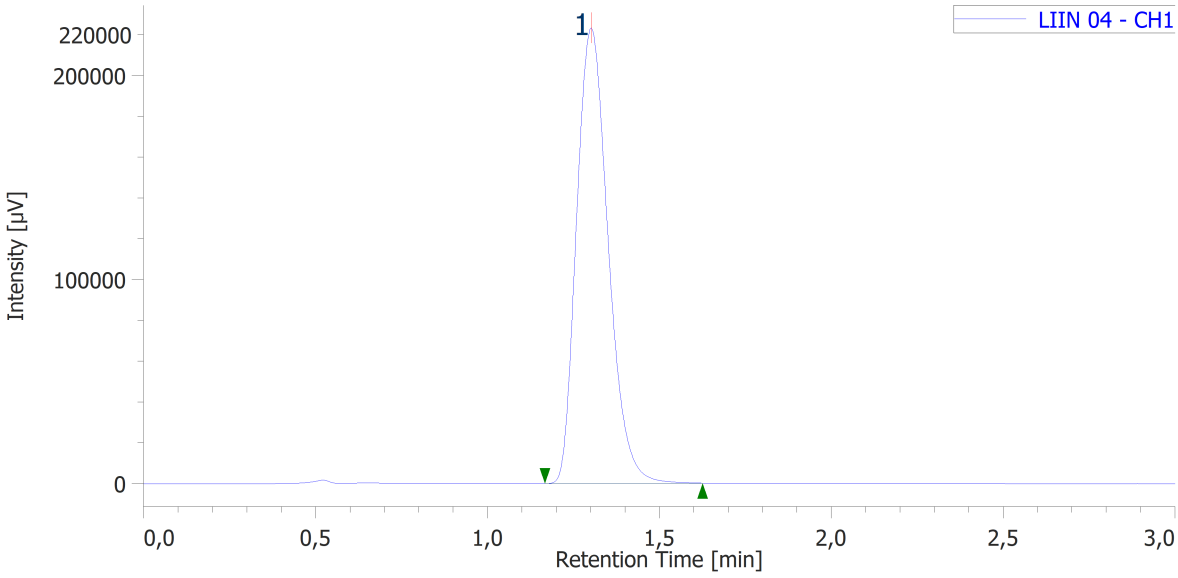

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:36:09
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 17:28:50
Volume	15,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,302	1425288	223157	100,000	100,000	N/A	952	N/A	1,236	

Creator QPackSA
Reviewer
Approver

Chromatogram

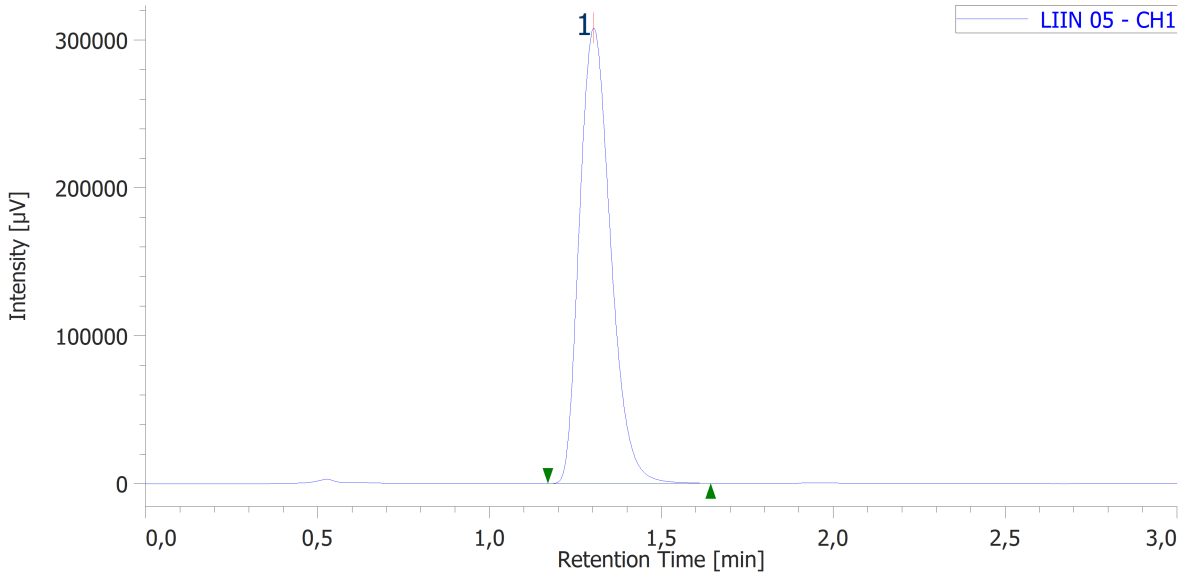

Chromatogram Information	
User Name	QPackSA
Date Modified	20/03/2025 17:36:09
Description	
HPLC System Name	01-HP-02
Injection Date	20/03/2025 17:32:36
Volume	20,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor Sistema 02
Control Method	Qualificação HPLC 02
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,303	1932902	307980	100,000	100,000	N/A	988	N/A	1,252	

Creator QPackSA
Reviewer
Approver