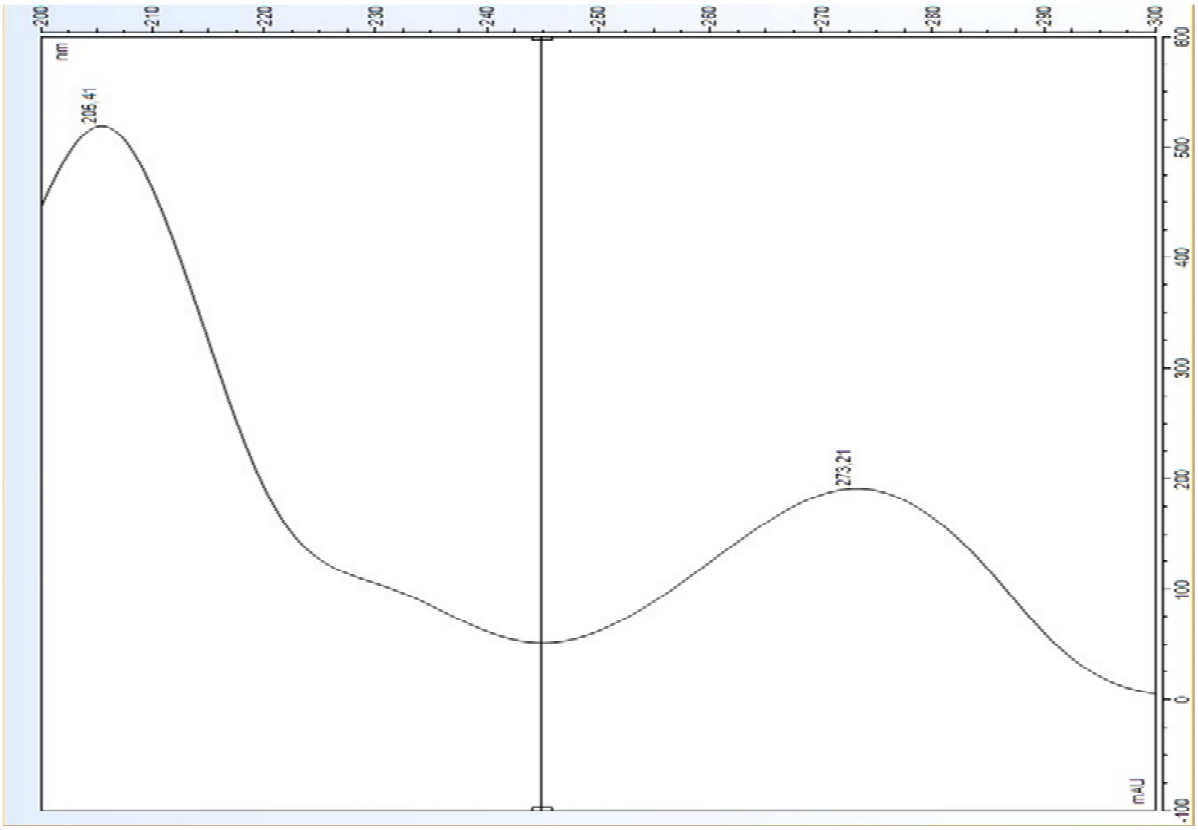


File Path chrom://clbap1358/ChromeleonLocal/Qualificação/Qualificação 2019/EDUV.seq/322.smp/3DFIELD.field
Channel UV_VIS_1

Injection Information:
Data Vault ChromeleonLocal
Injection EDUV
Injection Number 1
Position GA2
Comment
Processing Method
Instrument Method Qualificação
Type Unknown
Status Finished
Injection Date 21/05/2019
Injection Time 14:48:11
Injection Volume (µl) 10,000
Dilution Factor 1,0000
Weight 1,0000

Raw Data Information:
Data Points 101
Wavelength Min. (nm) 200,000000
Wavelength Max. (nm) 300,000000
Retention Time (min) 1,683333

Raw Data:


Wavelength (nm)	Value (mAU)
200,0	446,394470
201,0	467,625050
202,0	486,742049
203,0	502,051085
204,0	512,833685
205,0	518,304081
206,0	517,750711
207,0	511,278839
208,0	499,203116
209,0	482,298165
210,0	461,395947
211,0	437,433388
212,0	411,156560
213,0	383,180641
214,0	354,184112
215,0	324,416657
216,0	294,755834
217,0	265,681759
218,0	238,638058
219,0	213,731778
220,0	191,692304
221,0	172,896932
222,0	157,139370
223,0	144,491562
224,0	134,426840
225,0	126,602300
226,0	120,547063
227,0	115,723498
228,0	111,747629
229,0	108,275420
230,0	105,017191
231,0	101,683921
232,0	98,002618
233,0	93,980199
234,0	89,551156
235,0	84,771400
236,0	79,828029
237,0	74,910586
238,0	70,154850
239,0	65,686945
240,0	61,690871
241,0	58,230761
242,0	55,365804
243,0	53,220216
244,0	51,879647
245,0	51,429573
246,0	51,880720
247,0	53,214851
248,0	55,388514
249,0	58,347050
250,0	62,023465
251,0	66,368286
252,0	71,249310
253,0	76,629226
254,0	82,510953
255,0	88,788872
256,0	95,394379
257,0	102,318472
258,0	109,500892
259,0	116,829819
260,0	124,243803
261,0	131,667324
262,0	139,019736
263,0	146,251747
264,0	153,187403
265,0	159,782002
266,0	166,011224
267,0	171,769808
268,0	176,970373
269,0	181,484591
270,0	185,240518
271,0	188,131820
272,0	190,013837
273,0	190,827977
274,0	190,481257
275,0	188,926410
276,0	186,181139
277,0	182,266842
278,0	177,299450
279,0	171,378325
280,0	164,568553
281,0	156,769523
282,0	148,166844
283,0	138,734885
284,0	128,480323
285,0	117,513008
286,0	106,107241
287,0	94,363576
288,0	82,614844
289,0	71,234528
290,0	60,445610
291,0	50,373974
292,0	41,376355
293,0	33,423545
294,0	26,507856
295,0	20,747961
296,0	15,979649
297,0	12,137831
298,0	9,107471
299,0	6,764770
300,0	5,000055

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 15:47*
Created By:	*Michael Careli*

Chromatogram

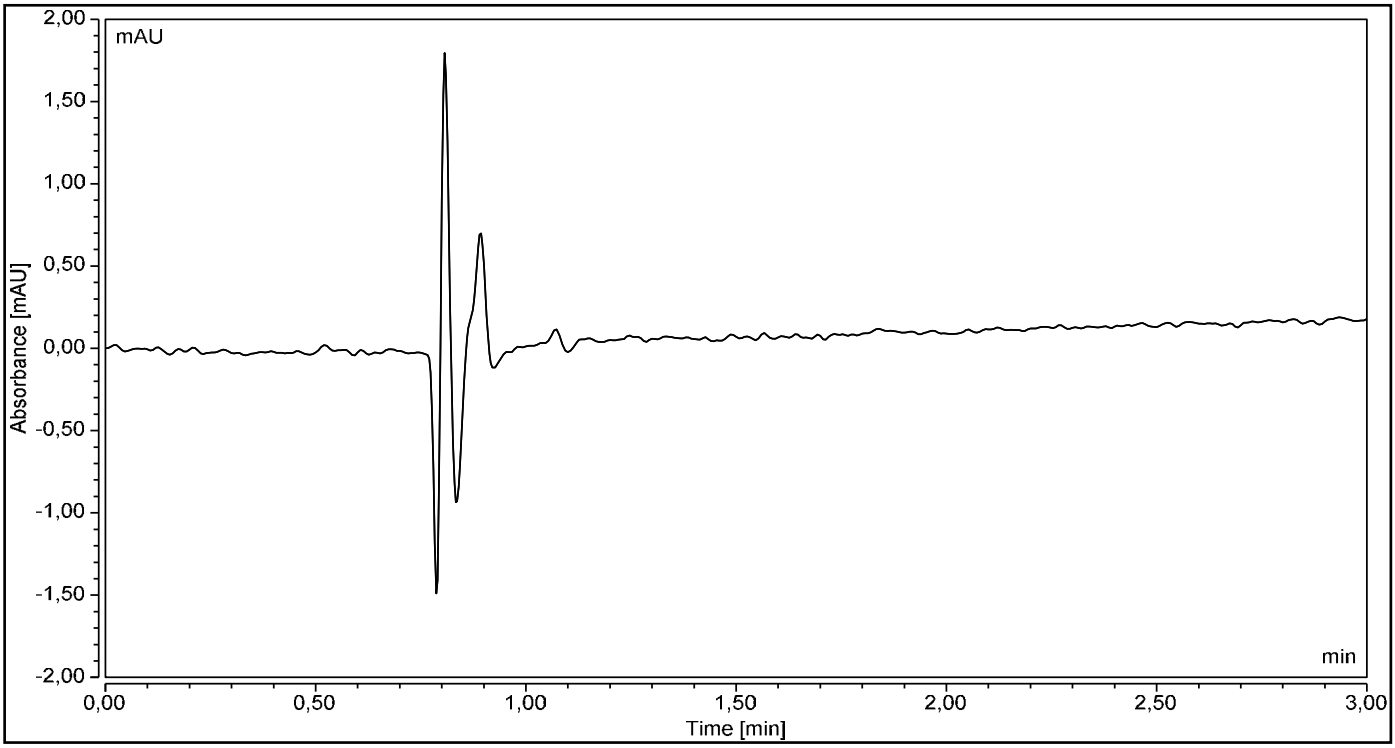

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 15:51*
Created By:	*Michael Careli*

Chromatogram

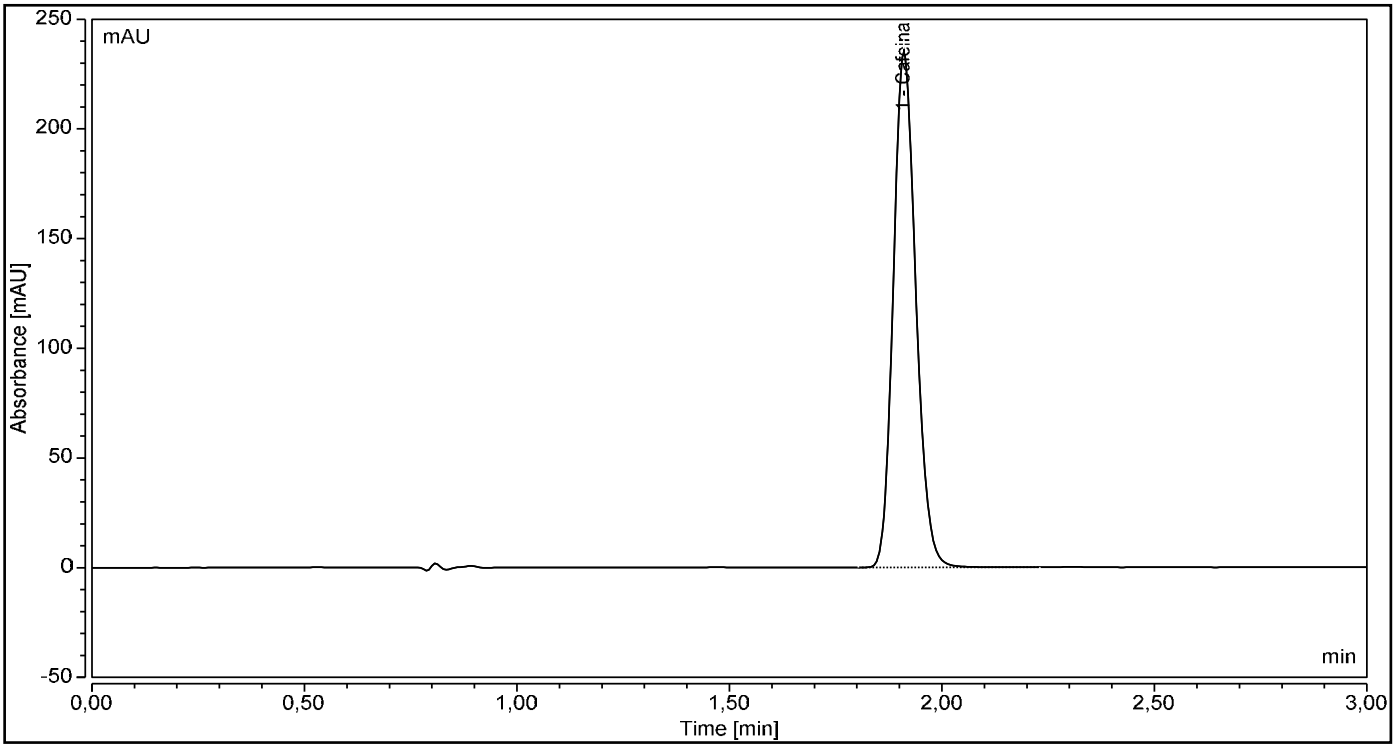

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,910	14,4640863

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 15:56*
Created By:	*Michael Careli*

Chromatogram

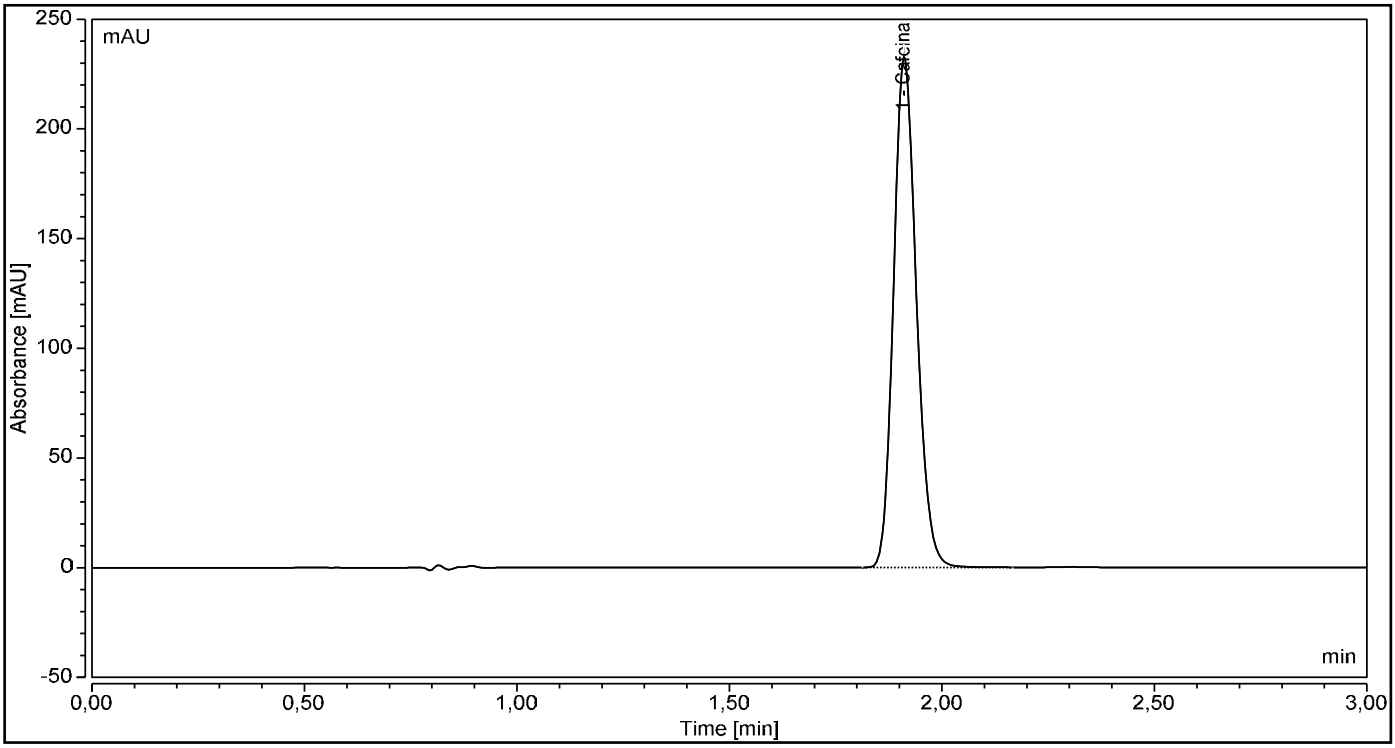

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,910	14,4816520

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:00*
Created By:	*Michael Careli*

Chromatogram

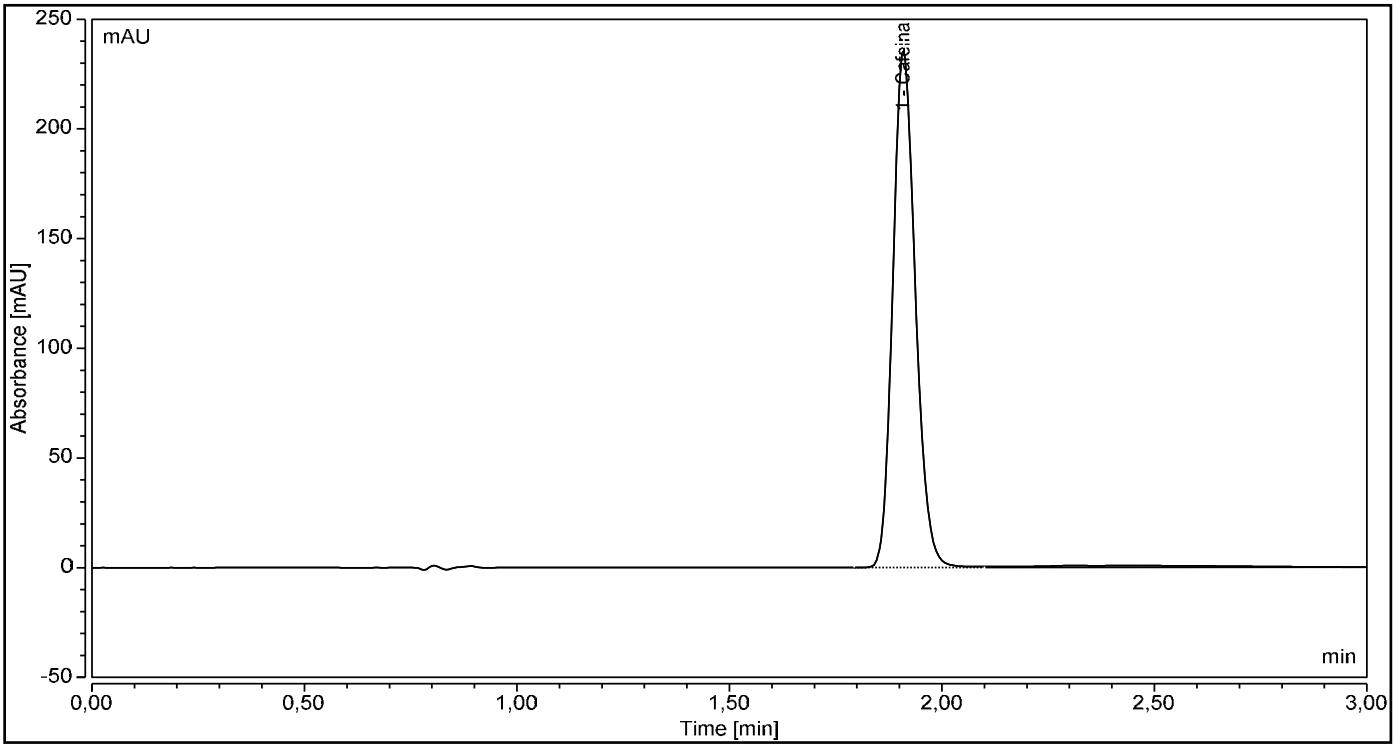

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,910	14,5277018

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:04*
Created By:	*Michael Careli*

Chromatogram

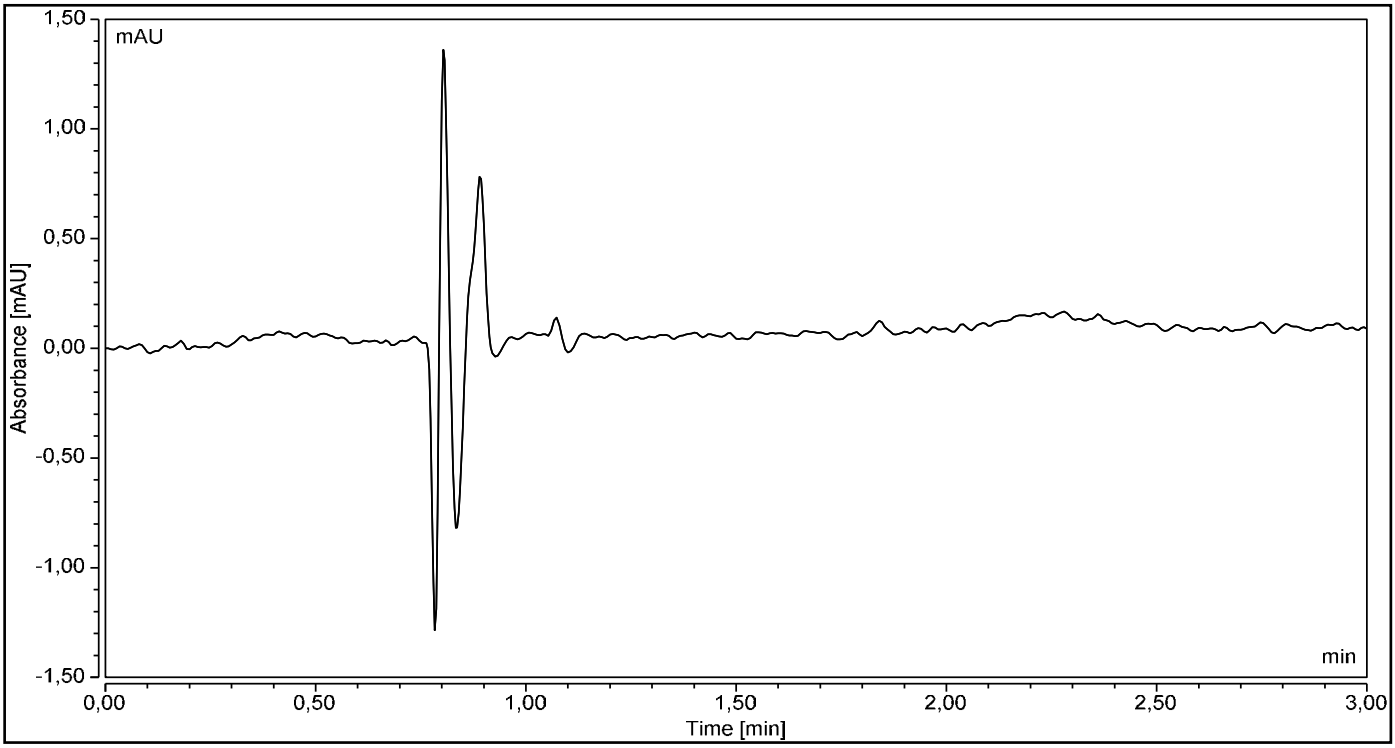

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 4*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:08*
Created By:	*Michael Careli*

Chromatogram

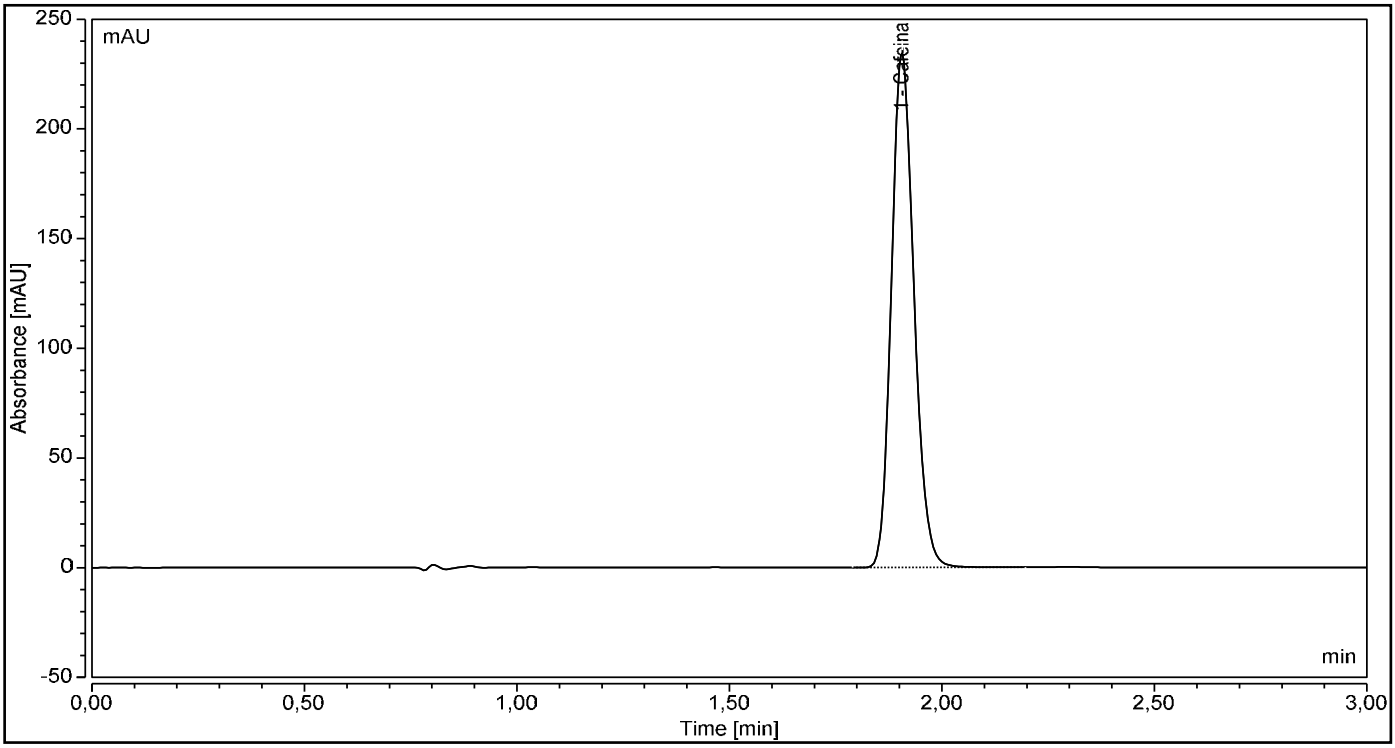

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,4591363

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 5*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:13*
Created By:	*Michael Careli*

Chromatogram

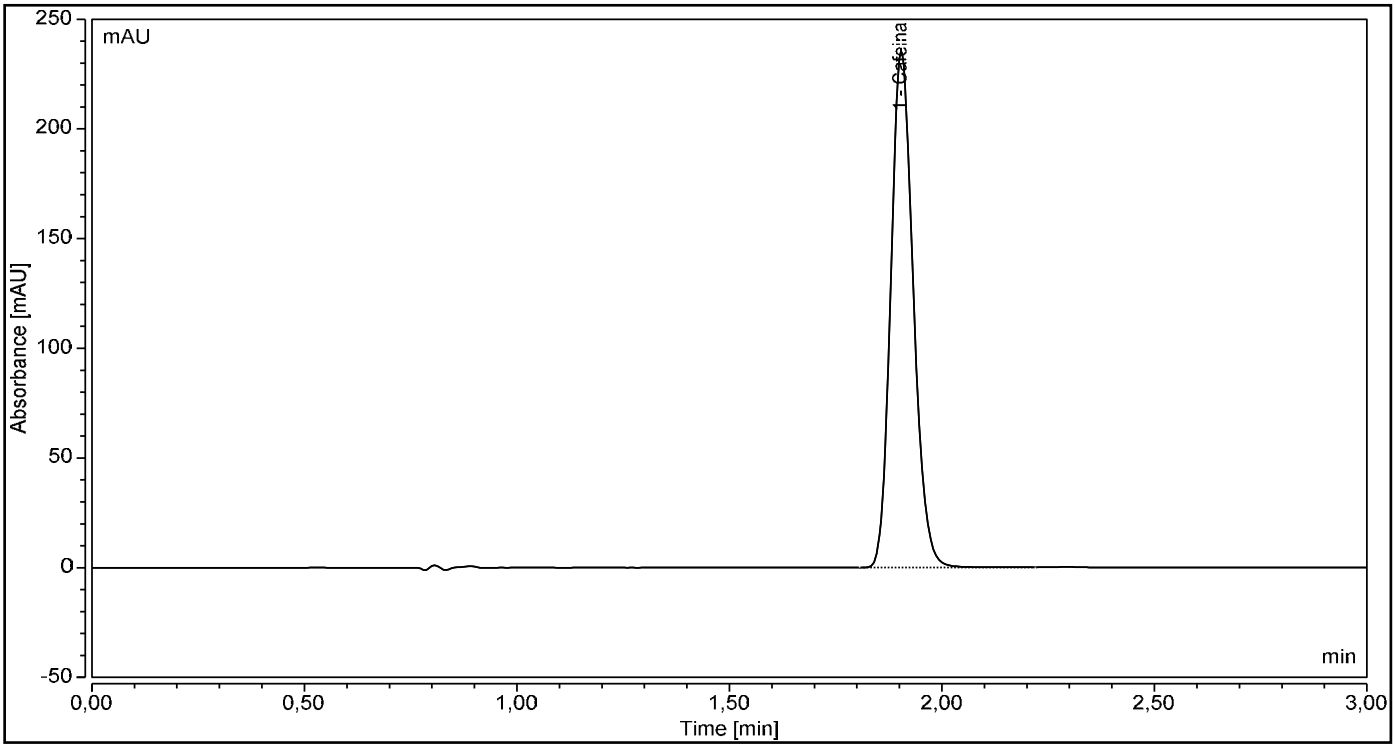

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,903	14,4637254

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 6*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:17*
Created By:	*Michael Careli*

Chromatogram

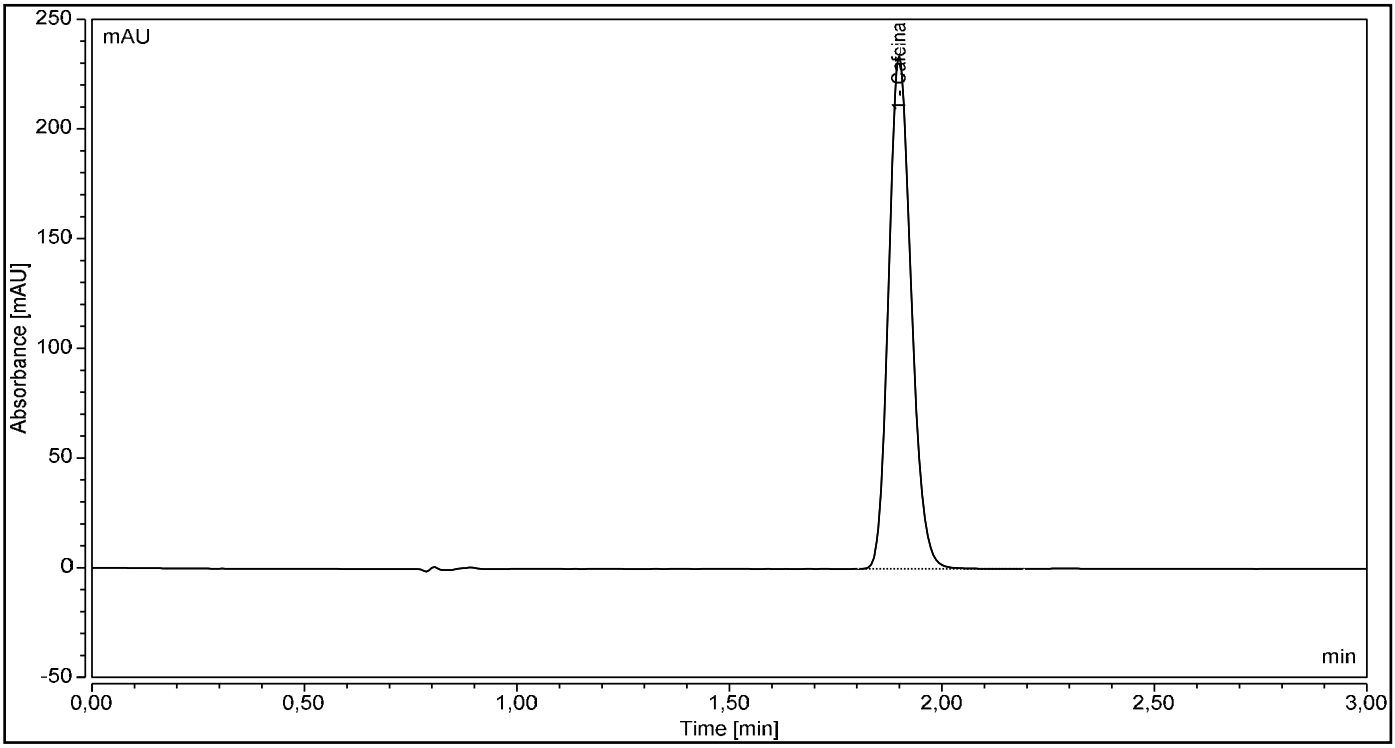

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,900	14,4606542

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:21*
Created By:	*Michael Careli*

Chromatogram

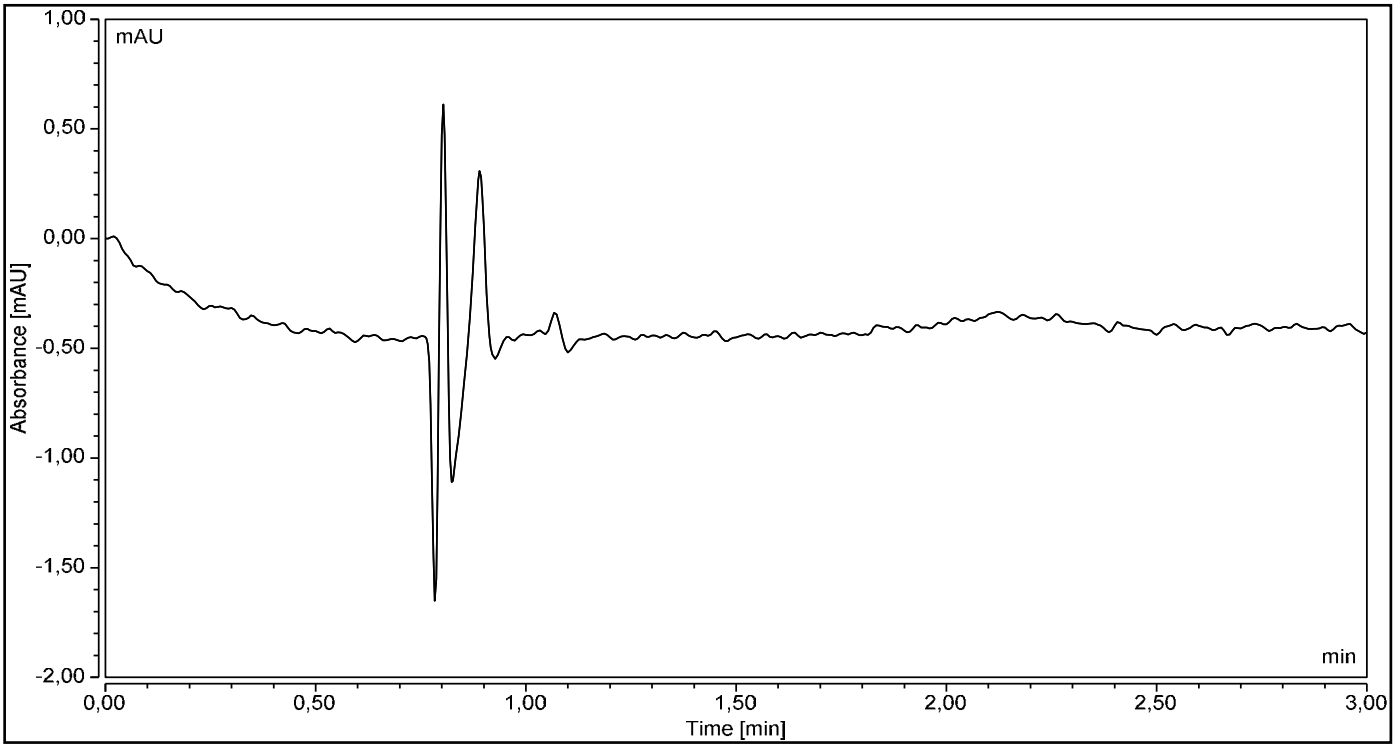

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:26*
Created By:	*Michael Careli*

Chromatogram

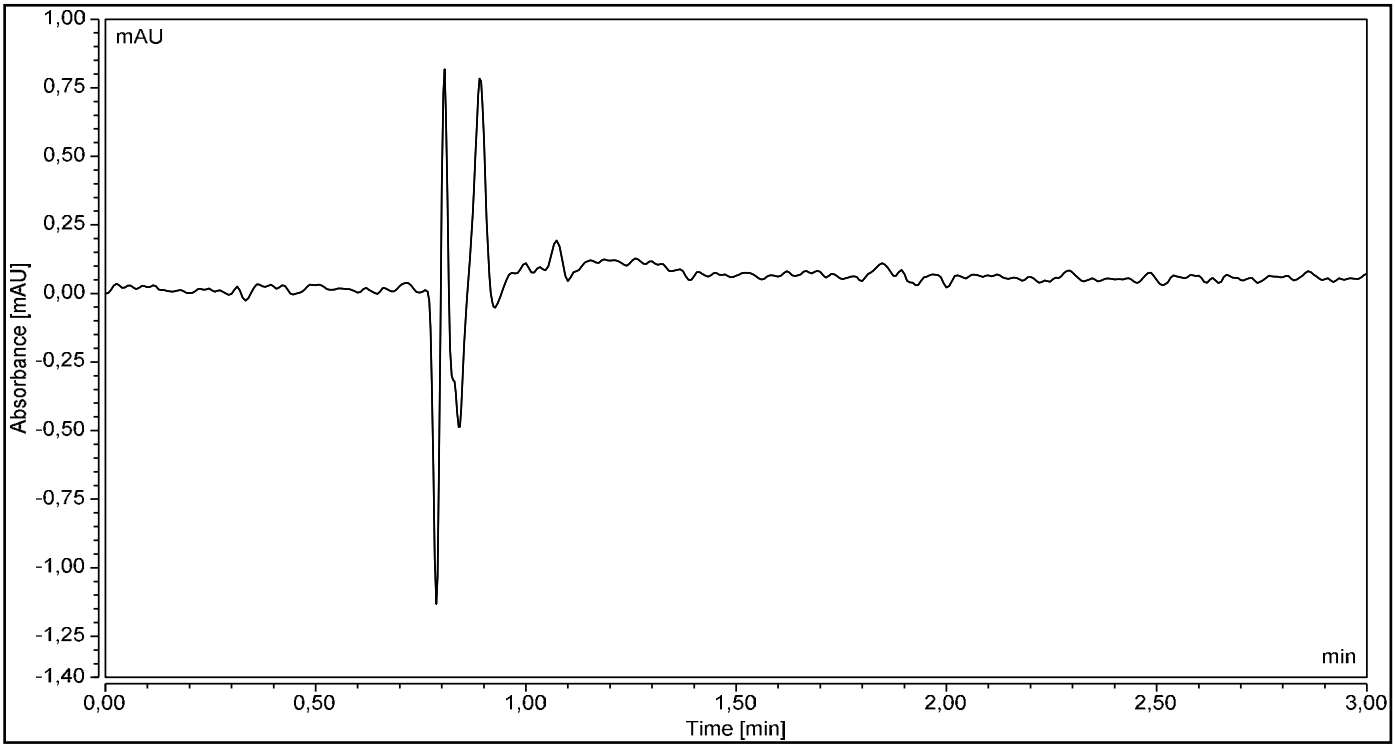

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:31*
Created By:	*Michael Careli*

Chromatogram

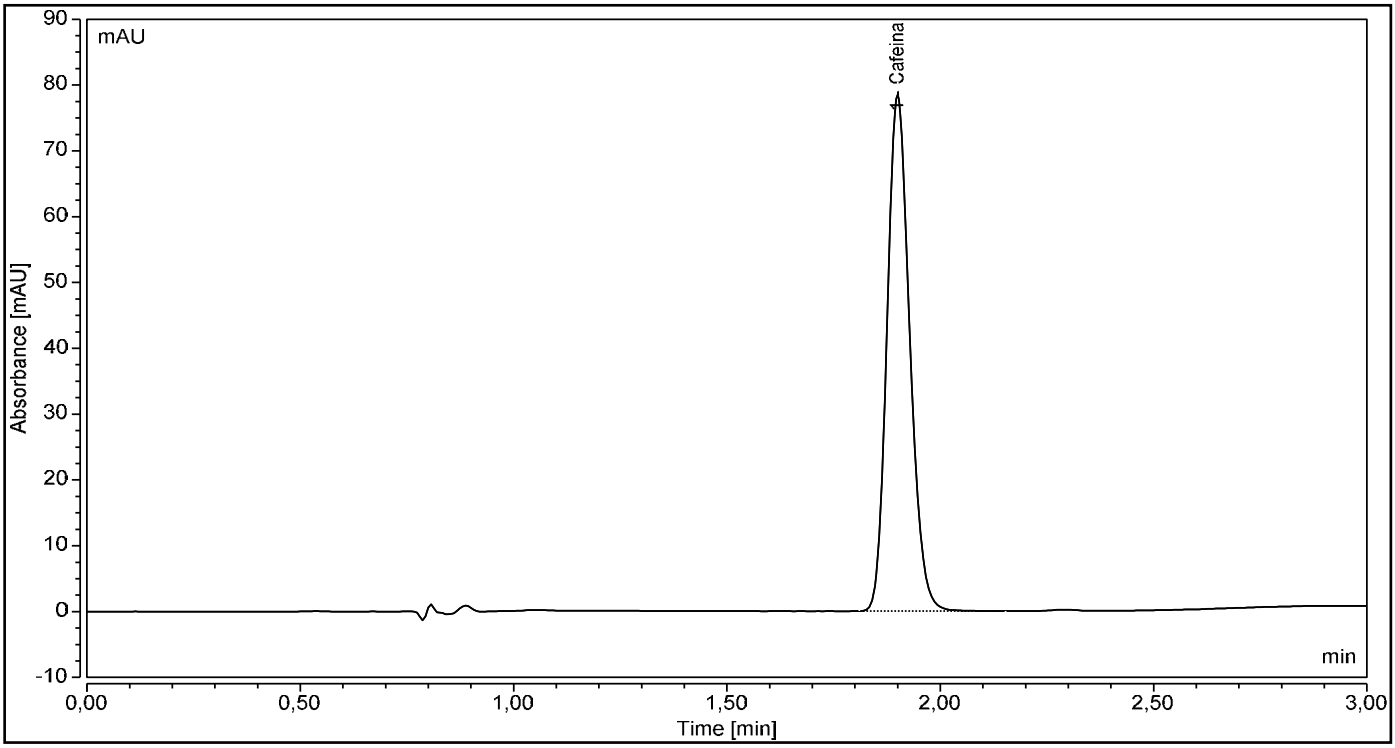

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,900	4,8478423

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:35*
Created By:	*Michael Careli*

Chromatogram

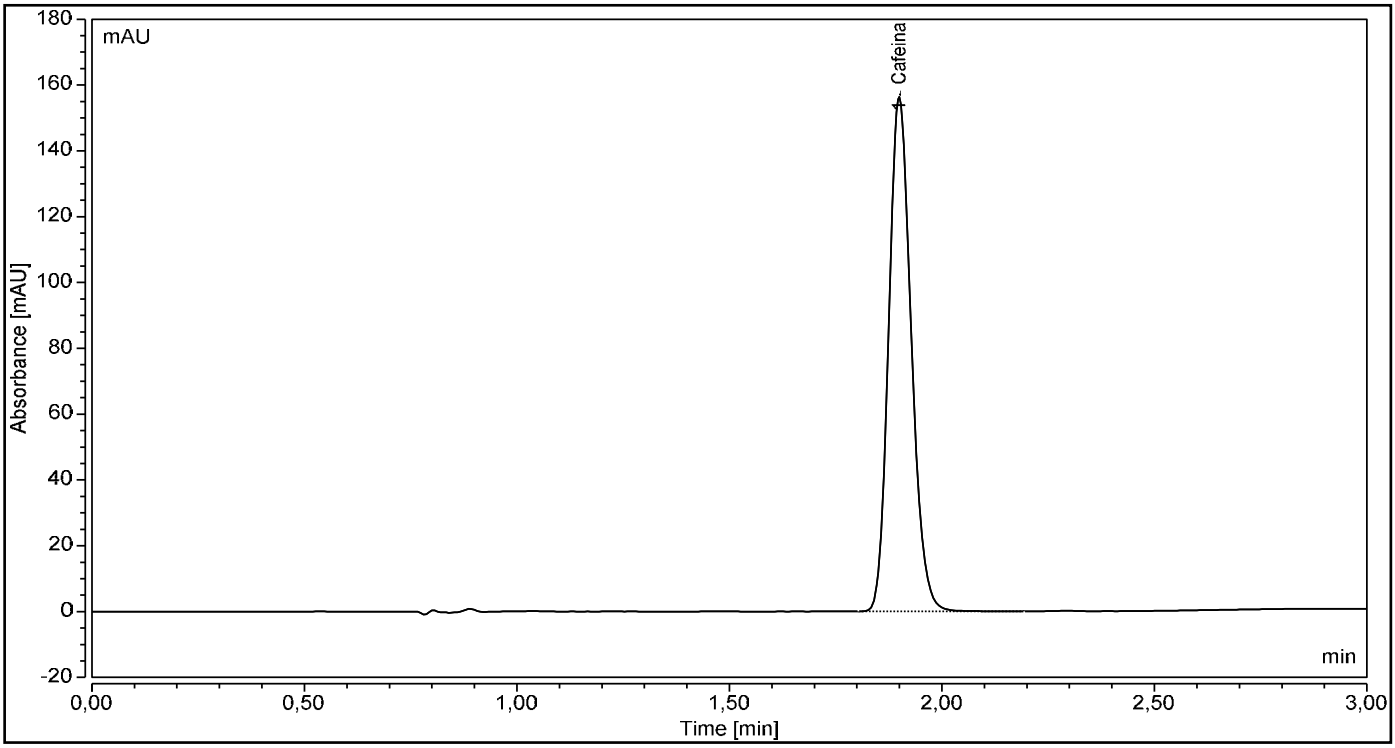

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,900	9,6223767

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 4*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:39*
Created By:	*Michael Careli*

Chromatogram

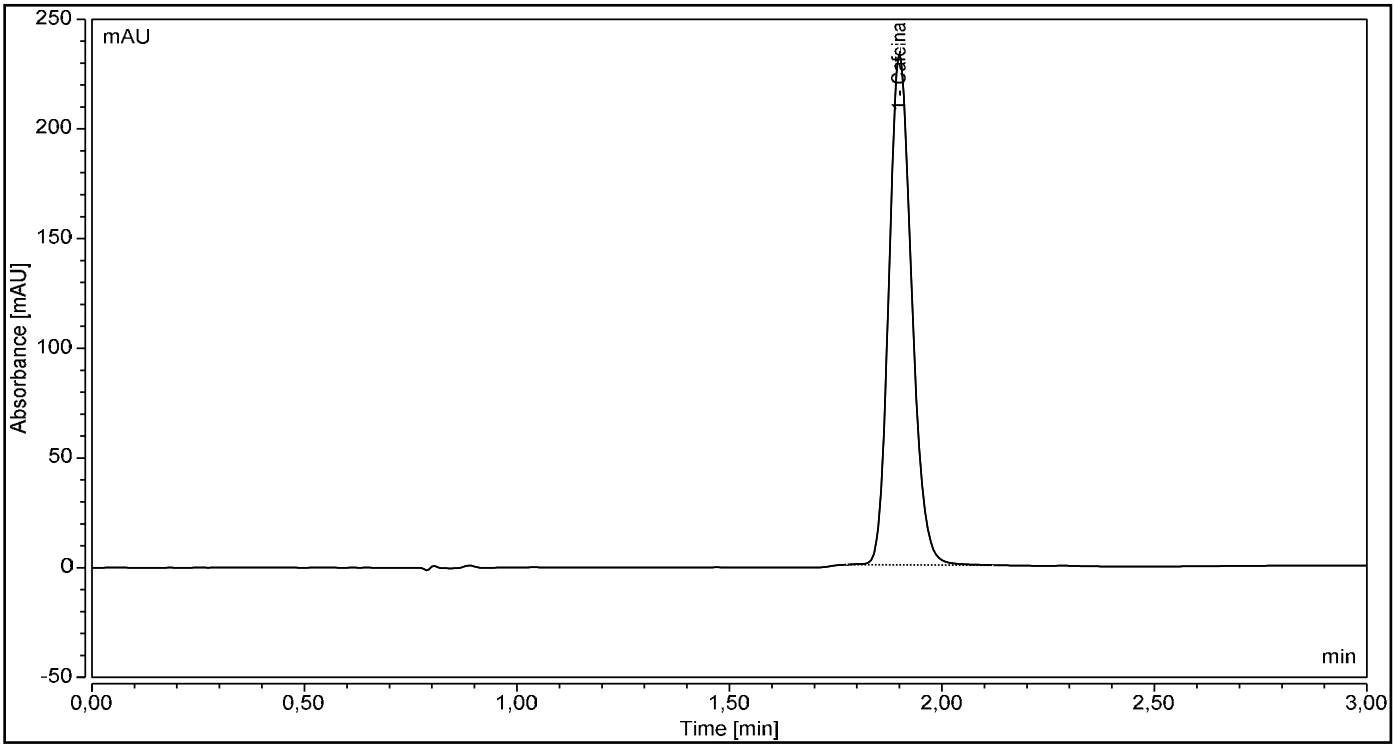

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,900	14,4921424

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 5*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*21/mai/19 16:43*
Created By:	*Michael Careli*

Chromatogram

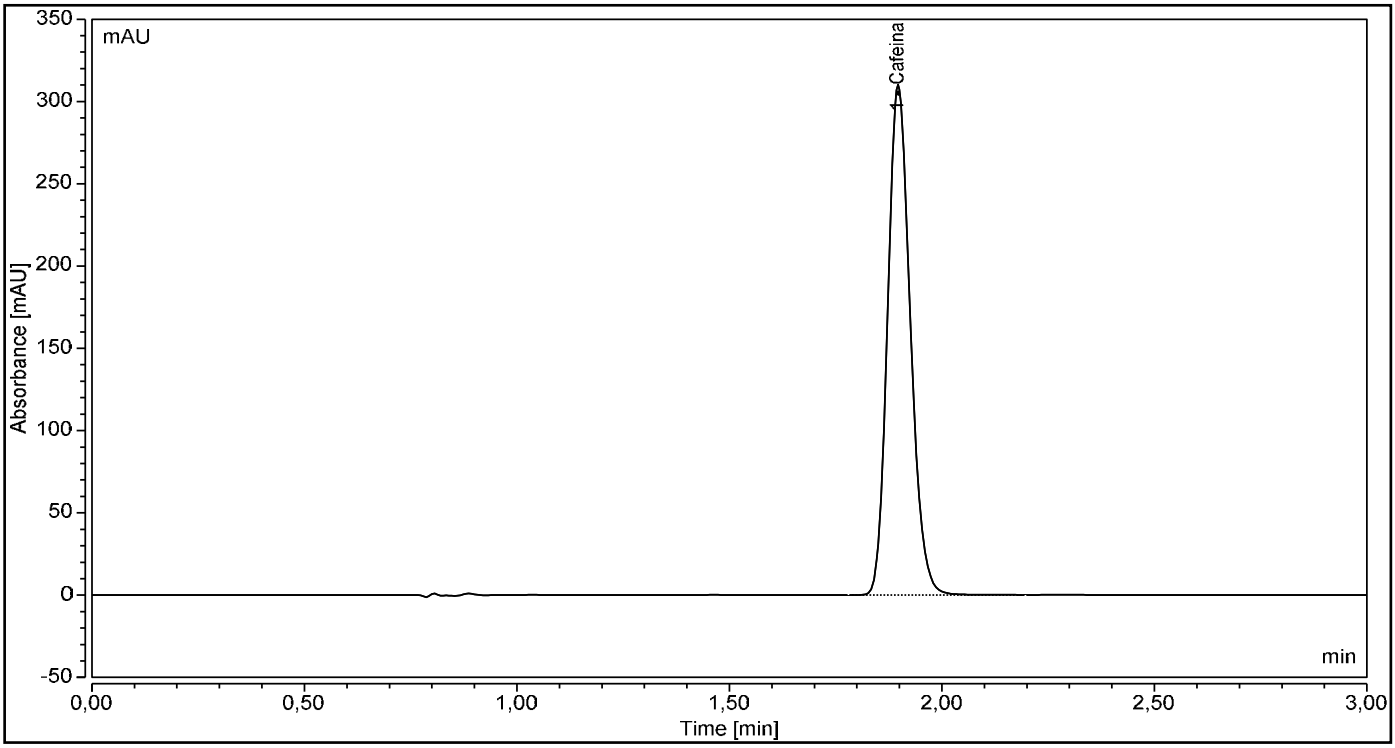

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,897	19,2098088

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 1*
Run Time (min):	*3,00*
Injection Volume:	*0,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*22/mai/19 08:34*
Created By:	*Michael Careli*

Chromatogram

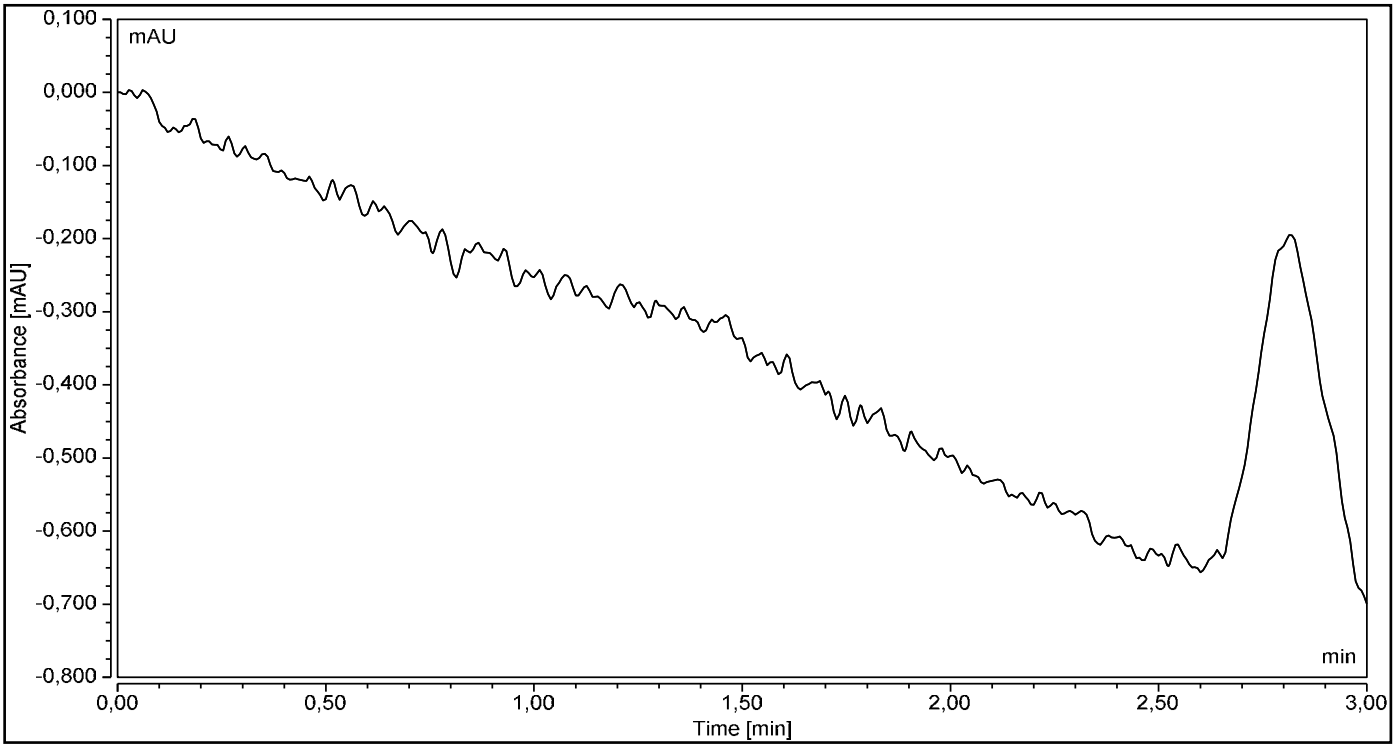

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 2*
Run Time (min):	*3,00*
Injection Volume:	*5,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*22/mai/19 08:38*
Created By:	*Michael Careli*

Chromatogram

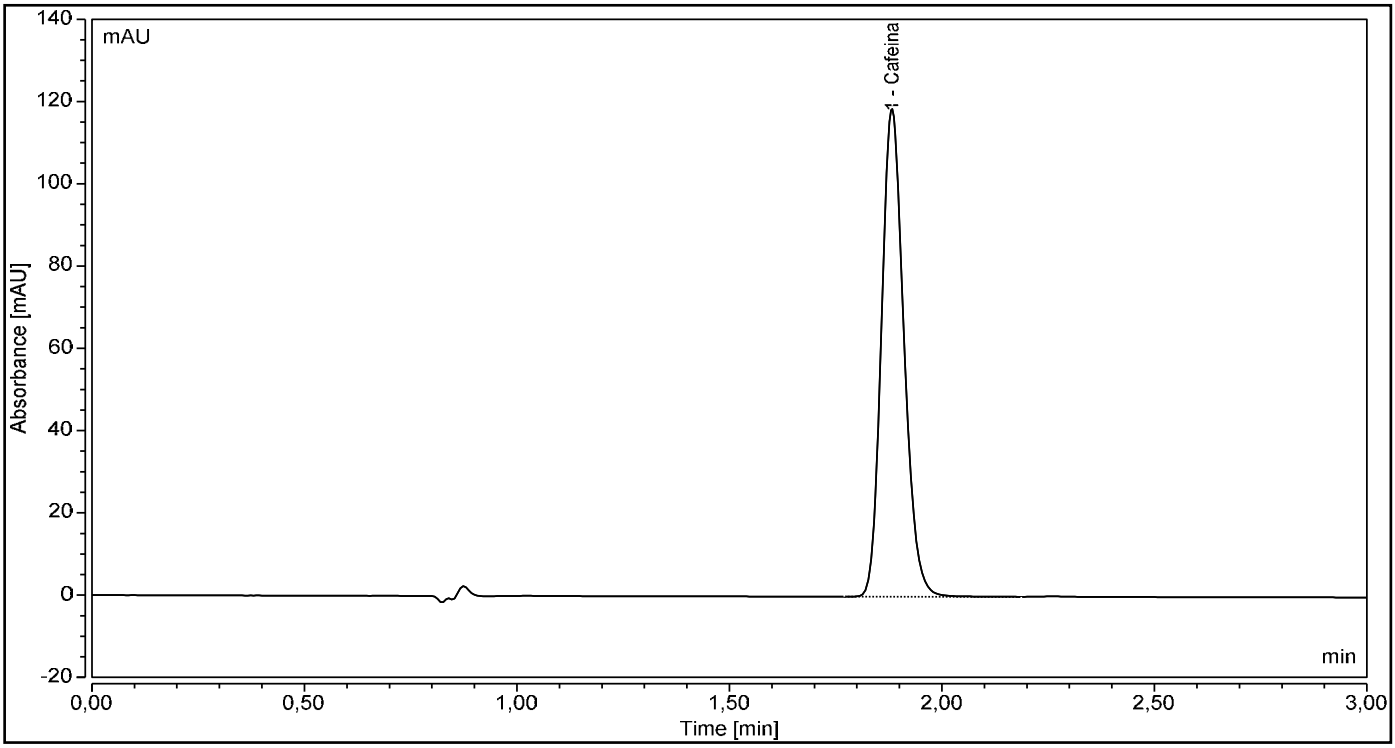

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,883	7,2646524

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*22/mai/19 08:42*
Created By:	*Michael Careli*

Chromatogram

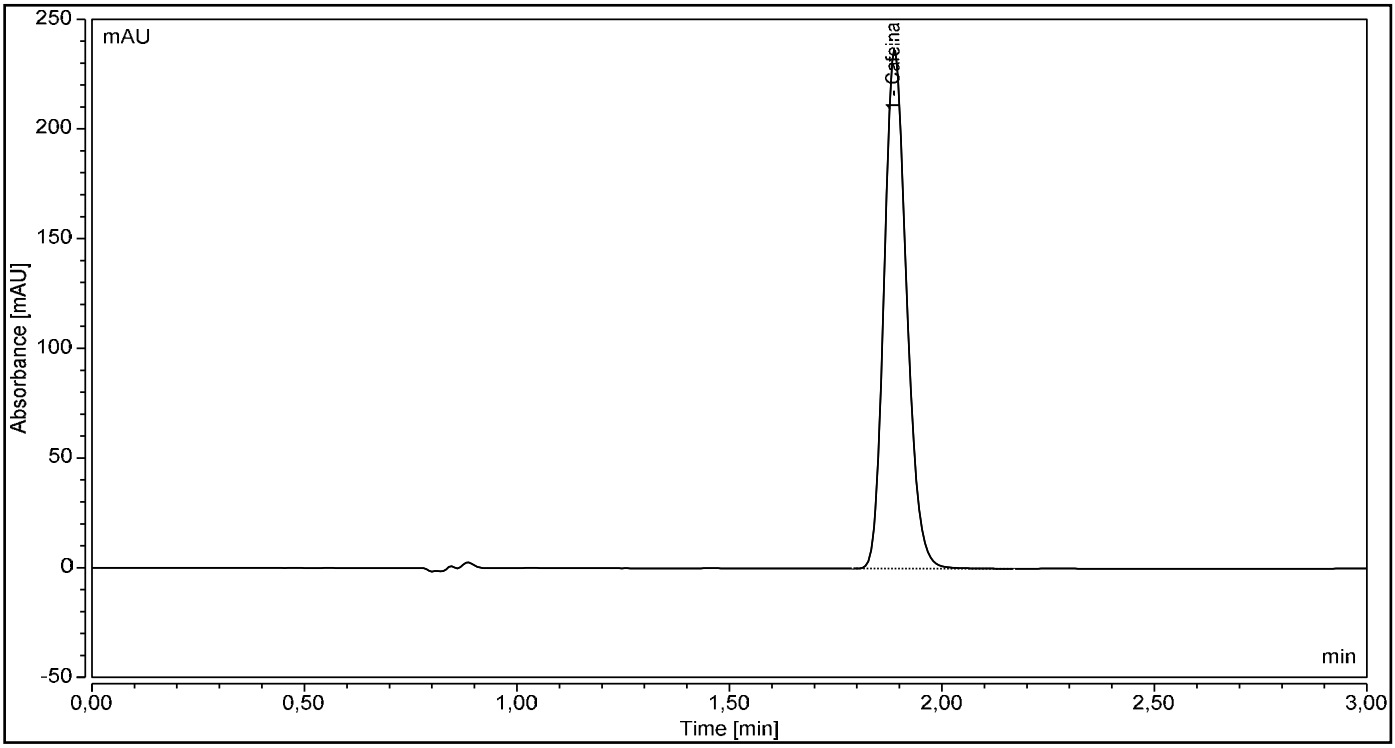

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,887	14,5091882

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 4*
Run Time (min):	*3,00*
Injection Volume:	*15,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*22/mai/19 08:46*
Created By:	*Michael Careli*

Chromatogram

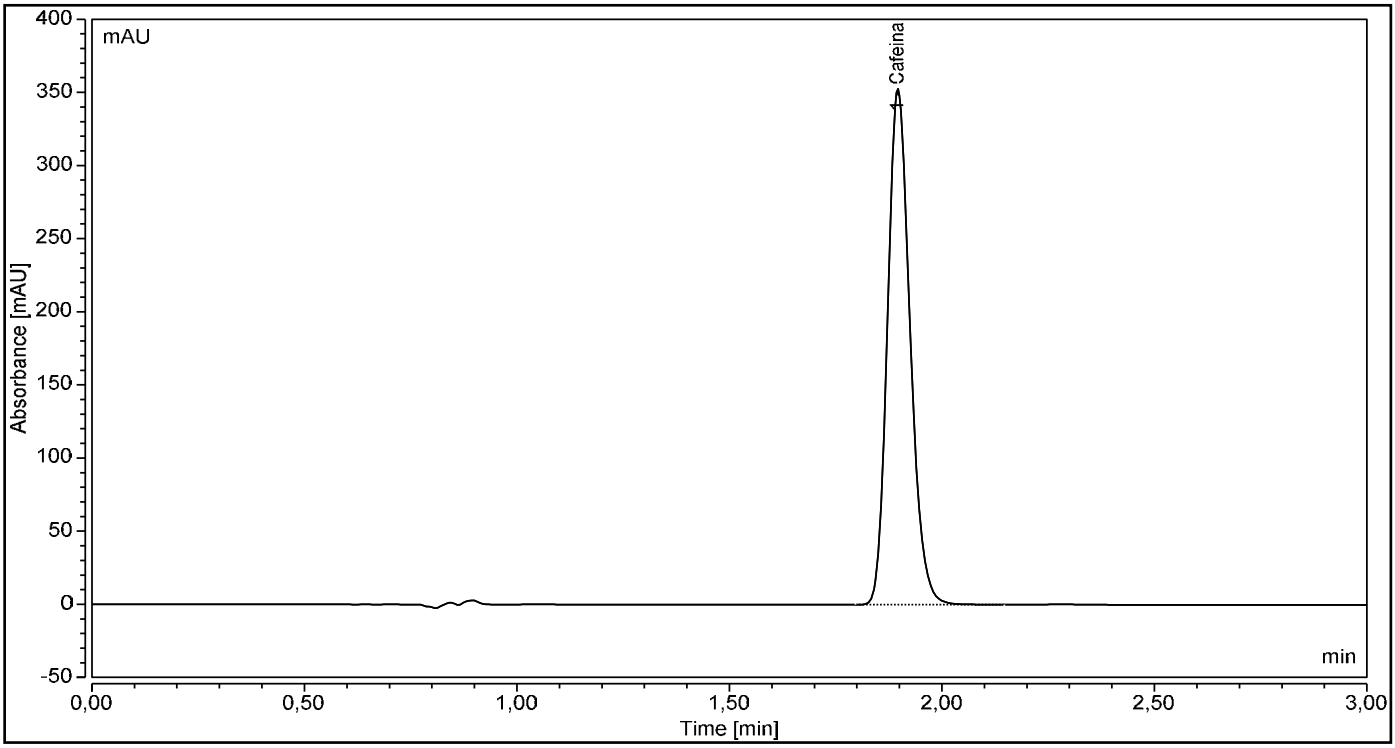

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,897	21,7307380

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 5*
Run Time (min):	*3,00*
Injection Volume:	*20,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*22/mai/19 08:51*
Created By:	*Michael Careli*

Chromatogram

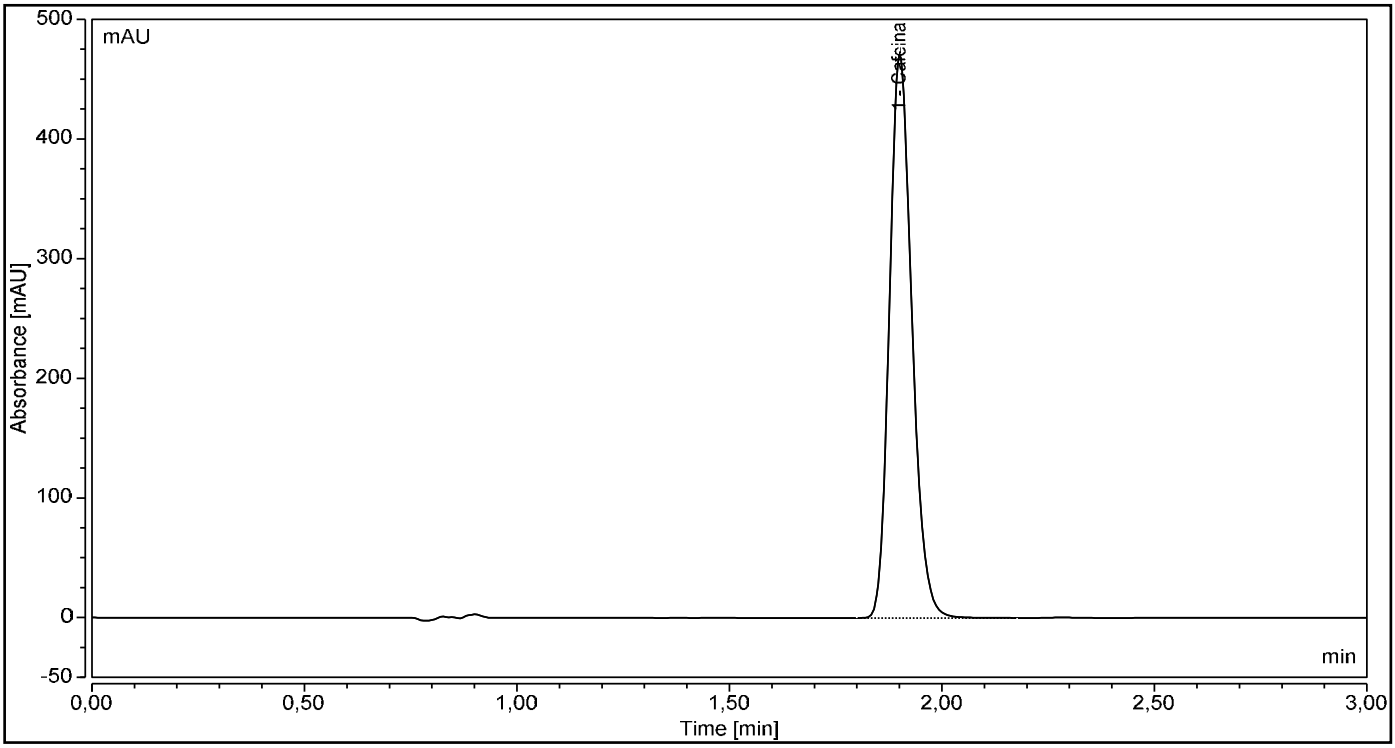

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,900	28,9774621

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Grad AB*
Run Time (min):	*19,00*
Injection Volume:	*0,00*
Instrument Method:	*Grad AB*
Processing Method:	*Gradiente*
Injection Date/Time:	*22/mai/19 09:43*
Created By:	*Michael Careli*

Chromatogram

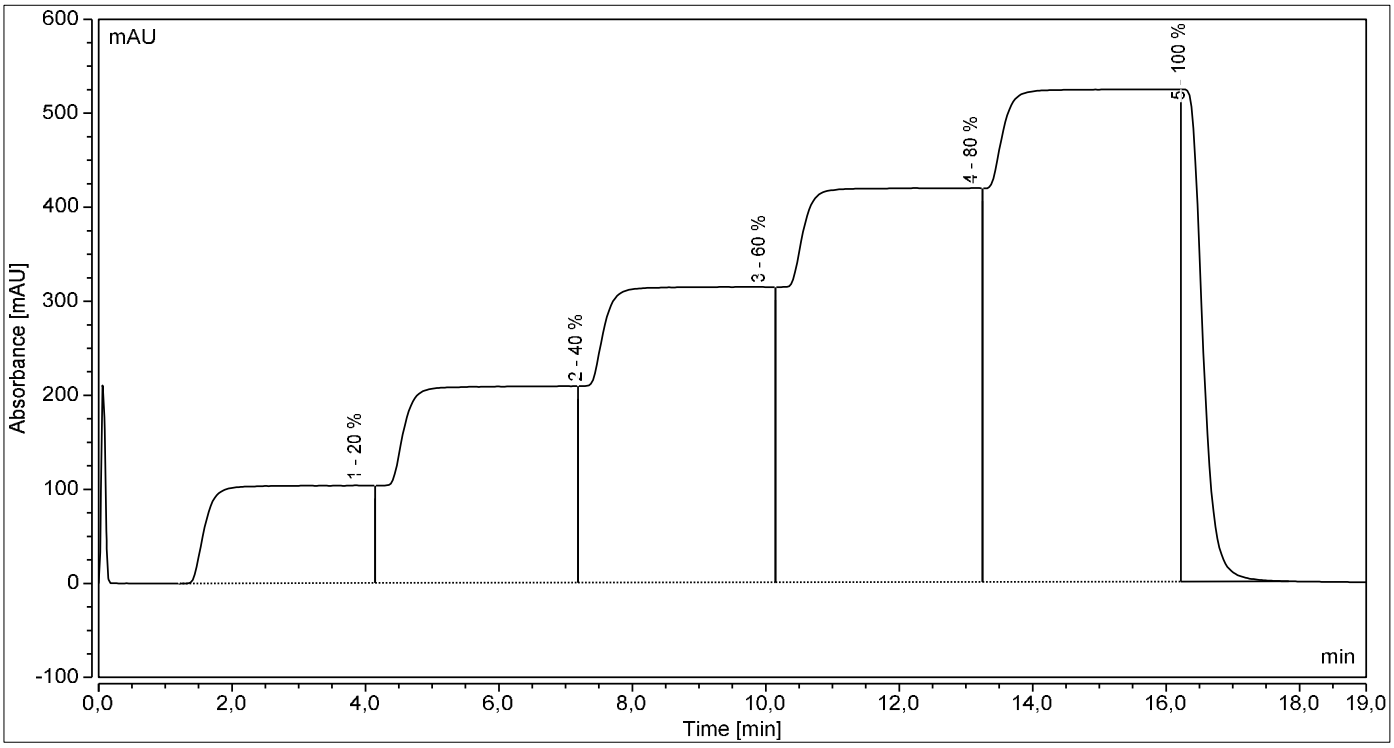

Integration Results


No.	Peak Name	Retention Time min	Height mAU
1	20 %	3,853	103,842
2	40 %	7,163	209,013
3	60 %	9,903	314,246
4	80 %	13,083	418,790
5	100 %	16,200	523,414

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Grad CD*
Run Time (min):	*19,00*
Injection Volume:	*0,00*
Instrument Method:	*Grad CD*
Processing Method:	*Gradiente*
Injection Date/Time:	*22/mai/19 10:19*
Created By:	*Michael Careli*

Chromatogram

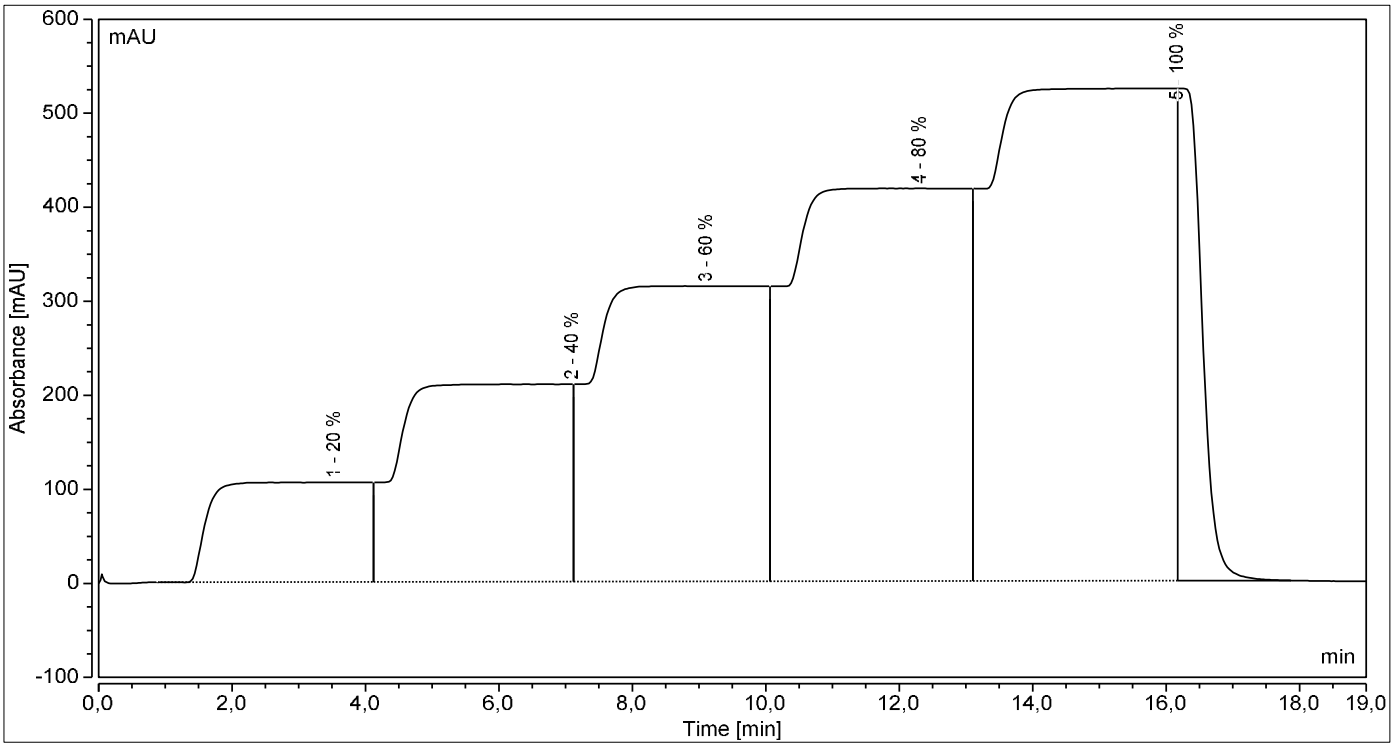

Integration Results

No.	Peak Name	Retention Time min	Height mAU
1	20 %	3,533	106,007
2	40 %	7,103	210,019
3	60 %	9,110	314,074
4	80 %	12,310	417,639
5	100 %	16,173	523,492