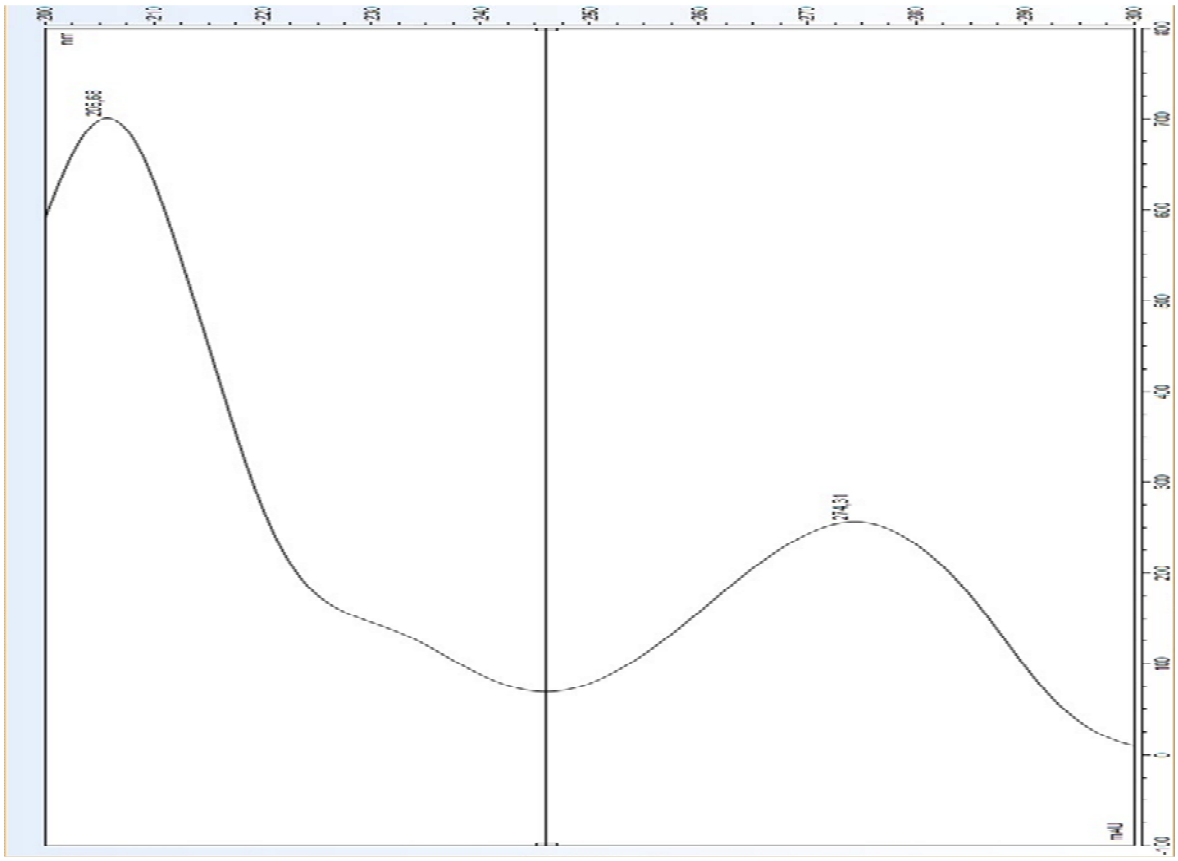


File Path chrom://clbap1357/ChromeleonLocal/Qualificação/Qualificação 2019/EDUV.seq/409.smp/3DFIELD.field
Channel UV_VIS_1

Injection Information:
Data Vault ChromeleonLocal
Injection EDUV
Injection Number 1
Position GA2
Comment
Processing Method Qualificação
Instrument Method Qualificação
Type Unknown
Status Finished
Injection Date 23/05/2019
Injection Time 08:59:57
Injection Volume (µl) 10,000
Dilution Factor 1,0000
Weight 1,0000

Raw Data Information:
Data Points 101
Wavelength Min. (nm) 200,000000
Wavelength Max. (nm) 300,000000
Retention Time (min) 1,893333

Raw Data:


Wavelength (nm)	Value (mAU)
200,0	590,887105
201,0	621,702350
202,0	649,244228
203,0	672,324042
204,0	689,012747
205,0	698,697251
206,0	700,215560
207,0	693,684679
208,0	679,582934
209,0	658,075908
210,0	630,016782
211,0	597,581184
212,0	562,221382
213,0	525,014372
214,0	487,370341
215,0	449,358192
216,0	410,568798
217,0	372,357629
218,0	335,189124
219,0	300,629157
220,0	269,660608
221,0	242,666319
222,0	219,942404
223,0	201,378357
224,0	186,636161
225,0	175,224613
226,0	166,446159
227,0	159,645329
228,0	154,112467
229,0	149,442324
230,0	145,236799
231,0	141,104587
232,0	136,715778
233,0	131,803044
234,0	126,270719
235,0	120,130010
236,0	113,570041
237,0	106,822437
238,0	100,107974
239,0	93,660599
240,0	87,703472
241,0	82,398777
242,0	77,823822
243,0	74,108963
244,0	71,313683
245,0	69,613699
246,0	69,085185
247,0	69,722657
248,0	71,526591
249,0	74,446206
250,0	78,398650
251,0	83,312457
252,0	89,077299
253,0	95,589703
254,0	102,827734
255,0	110,630400
256,0	119,050987
257,0	127,923615
258,0	137,139269
259,0	146,754393
260,0	156,602928
261,0	166,555534
262,0	176,554750
263,0	186,404418
264,0	196,010899
265,0	205,328596
266,0	214,129520
267,0	222,368075
268,0	229,973628
269,0	236,896589
270,0	242,917373
271,0	247,907832
272,0	251,884595
273,0	254,574850
274,0	255,837277
275,0	255,536869
276,0	253,624752
277,0	250,141397
278,0	245,114460
279,0	238,709345
280,0	230,897023
281,0	221,907092
282,0	211,738182
283,0	200,414968
284,0	187,879335
285,0	174,220453
286,0	159,643600
287,0	144,153365
288,0	128,154703
289,0	112,160332
290,0	96,534973
291,0	81,735079
292,0	68,085078
293,0	55,770937
294,0	45,042637
295,0	35,742047
296,0	28,039517
297,0	21,732391
298,0	16,611696
299,0	12,638868
300,0	9,544433

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:13*
Created By:	*Michael Careli*

Chromatogram

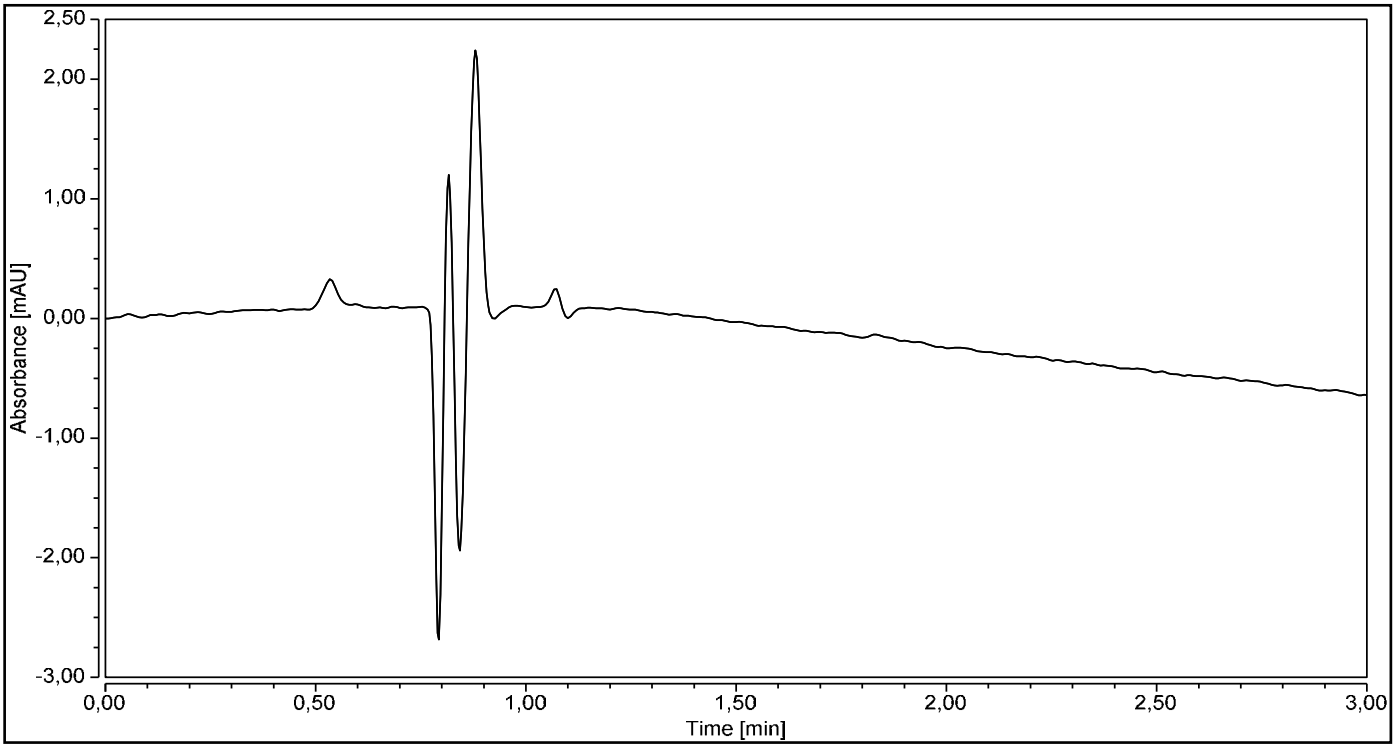

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:17*
Created By:	*Michael Careli*

Chromatogram

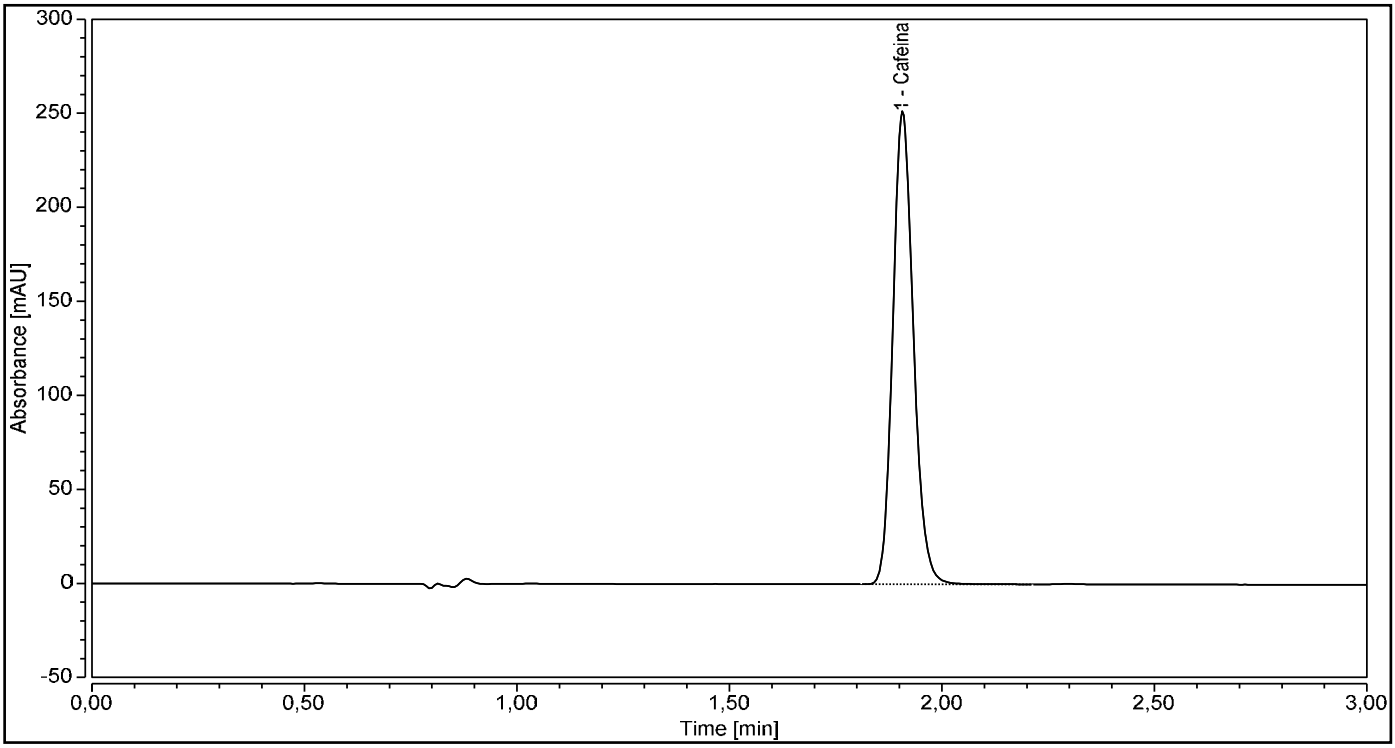

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,1202250

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:21*
Created By:	*Michael Careli*

Chromatogram

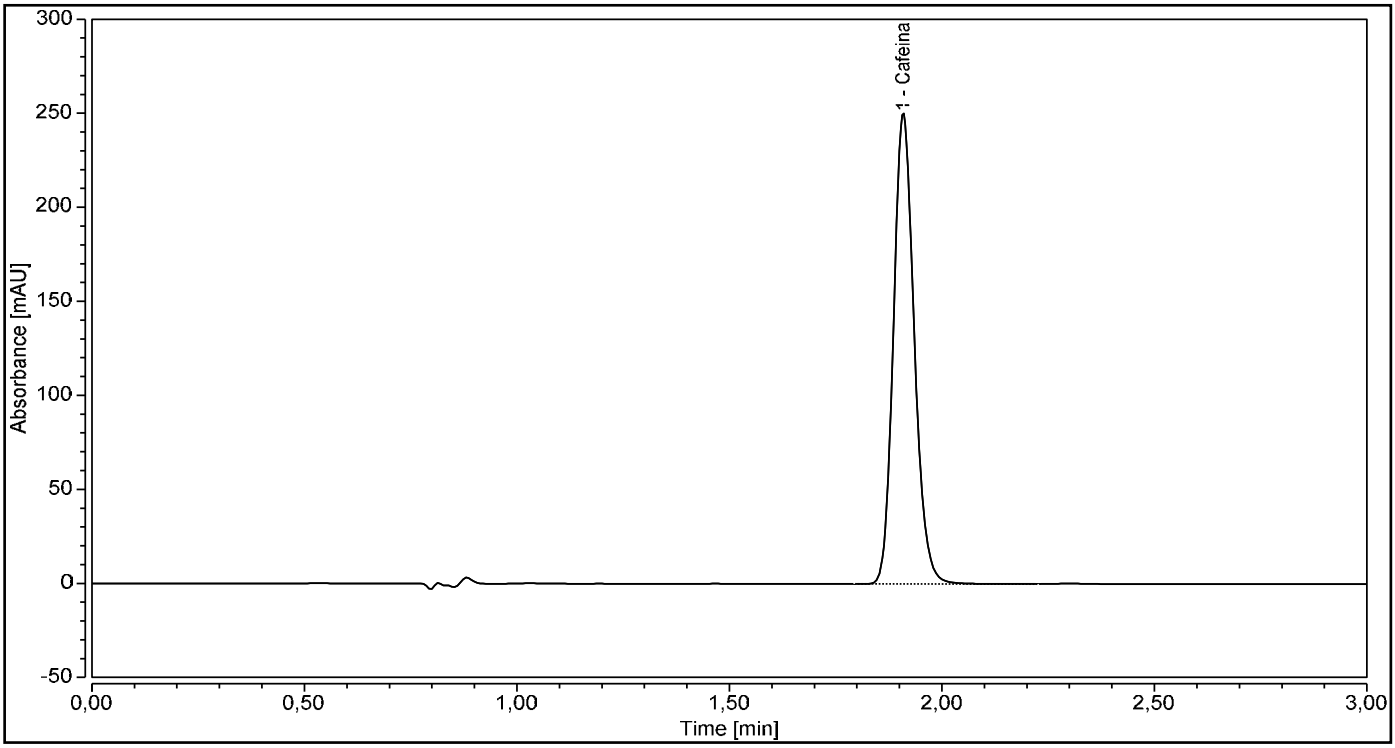

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,910	14,1629750

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:26*
Created By:	*Michael Careli*

Chromatogram

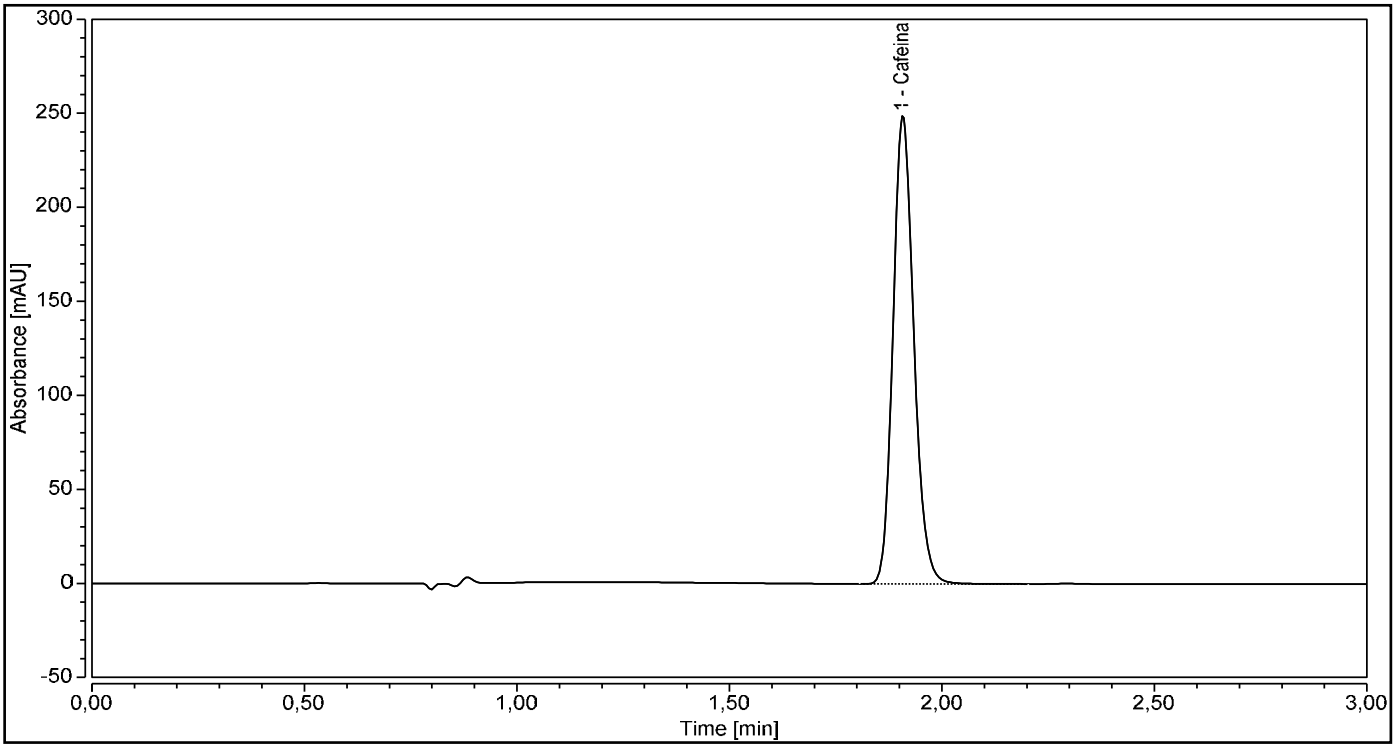

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,1283611

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:30*
Created By:	*Michael Careli*

Chromatogram

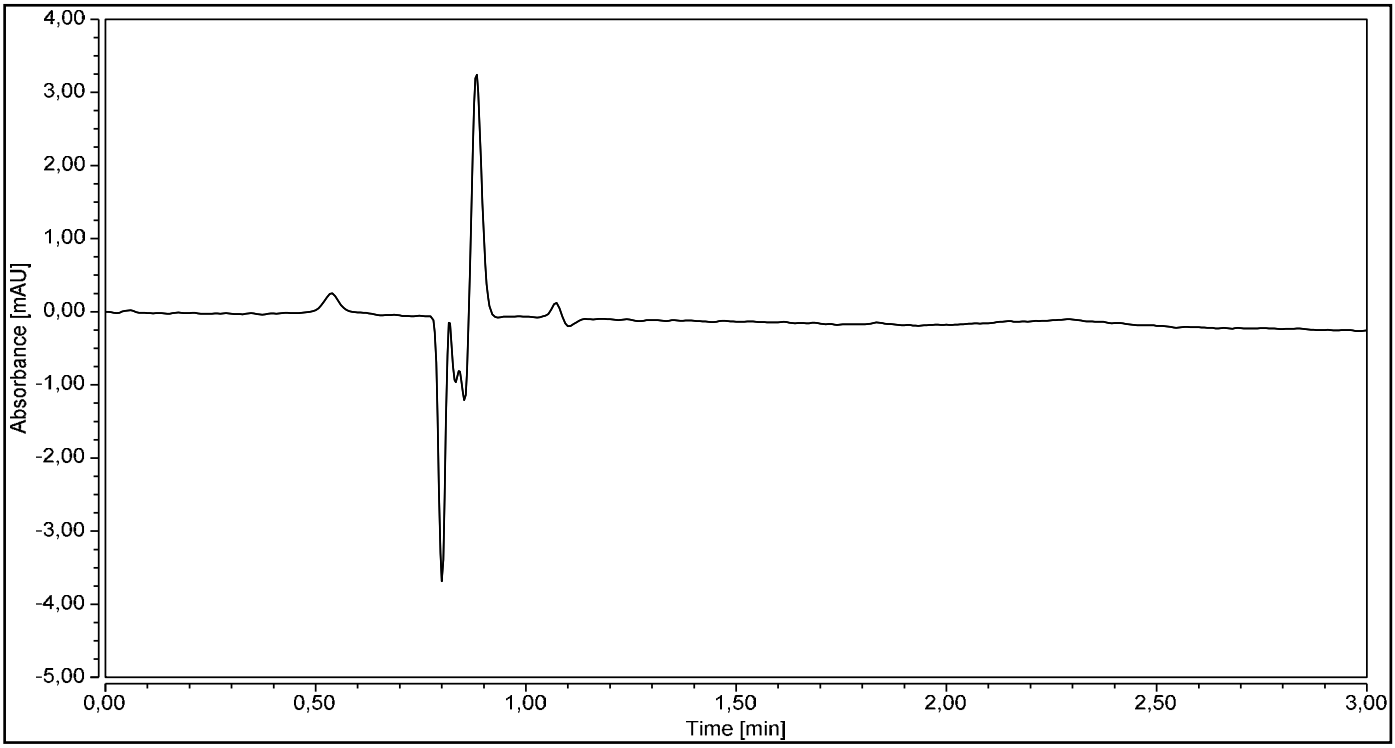

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 4*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:34*
Created By:	*Michael Careli*

Chromatogram

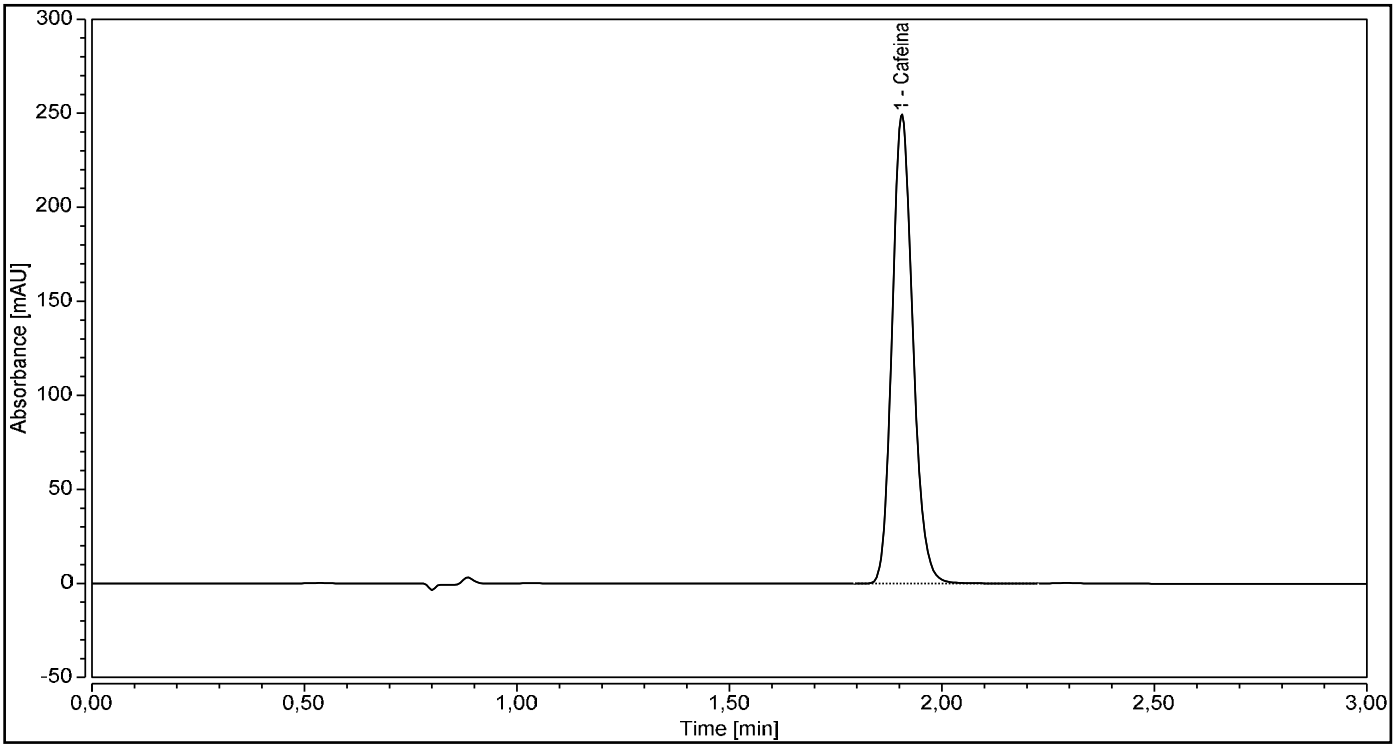

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,1423129

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 5*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:38*
Created By:	*Michael Careli*

Chromatogram

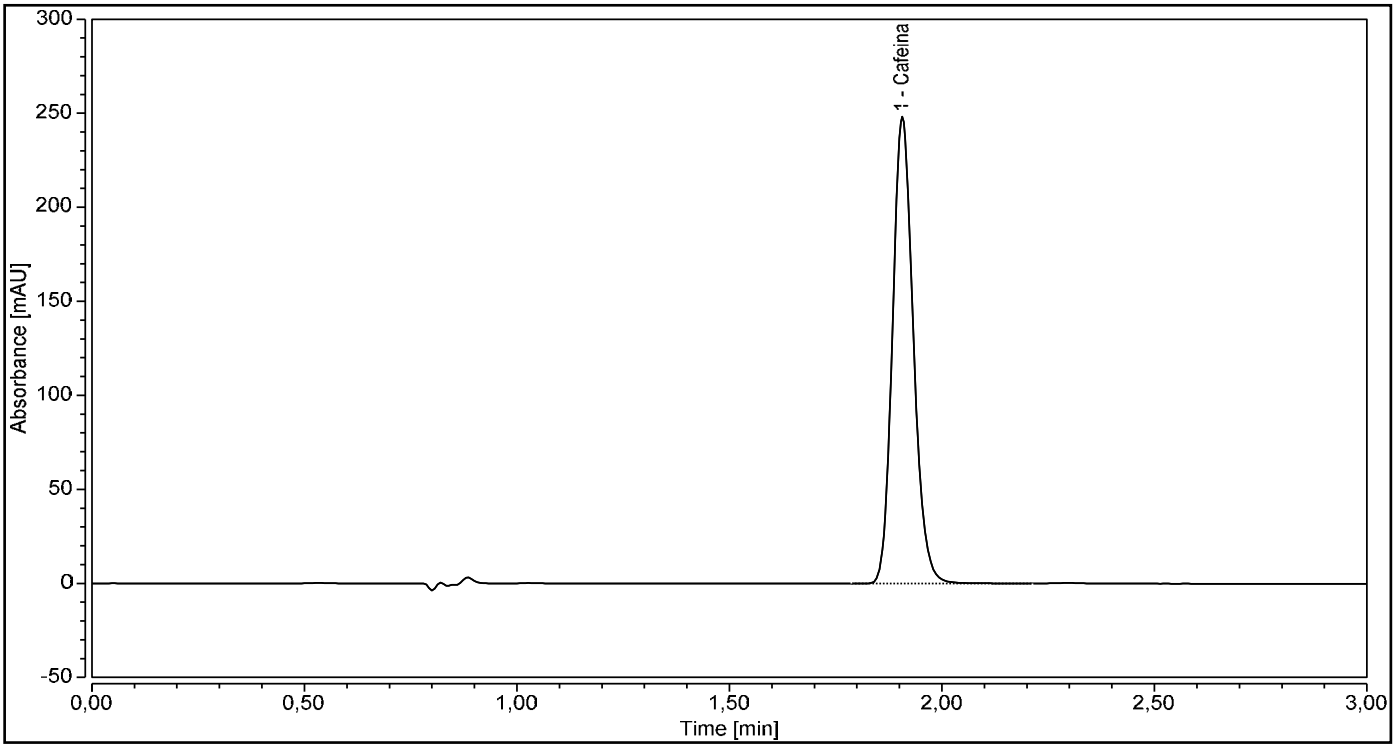

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,0904453

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*PCIN 6*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:43*
Created By:	*Michael Careli*

Chromatogram

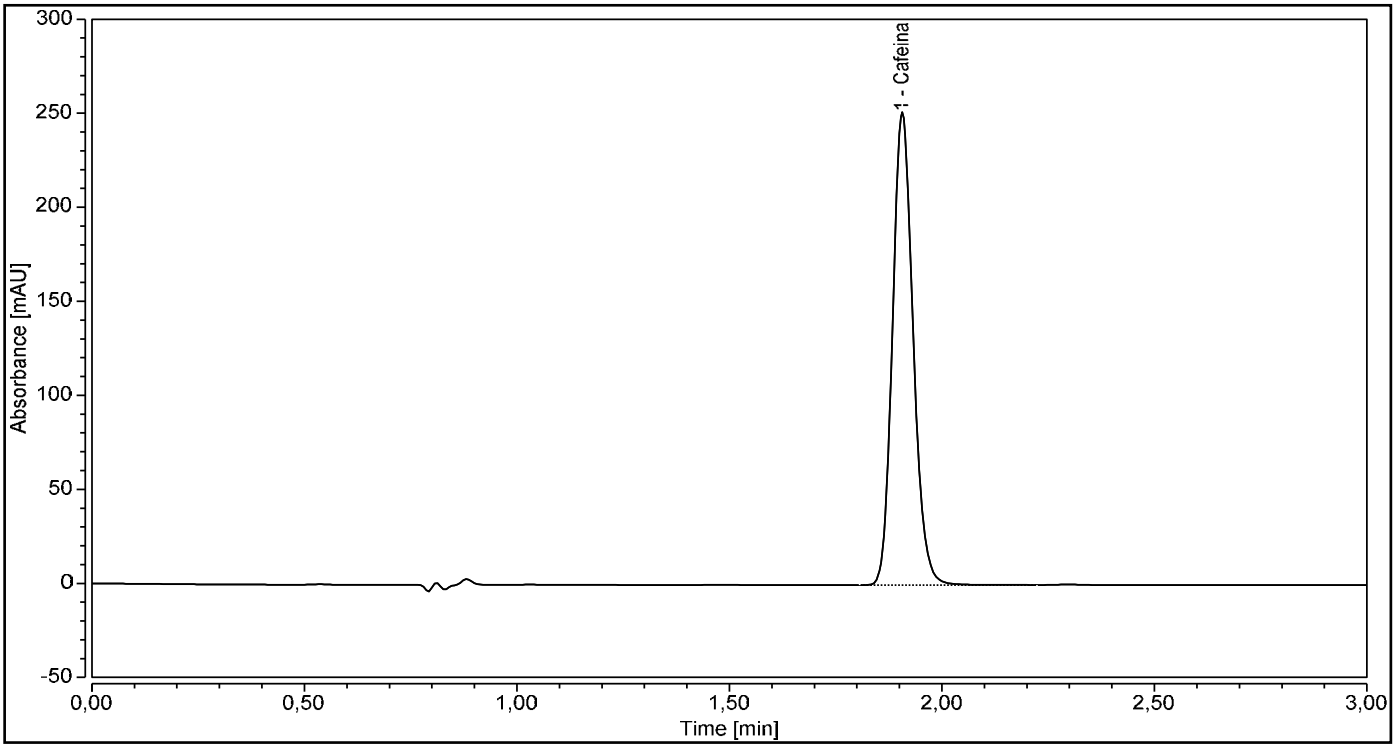

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,907	14,1126109

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Branco 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:47*
Created By:	*Michael Careli*

Chromatogram

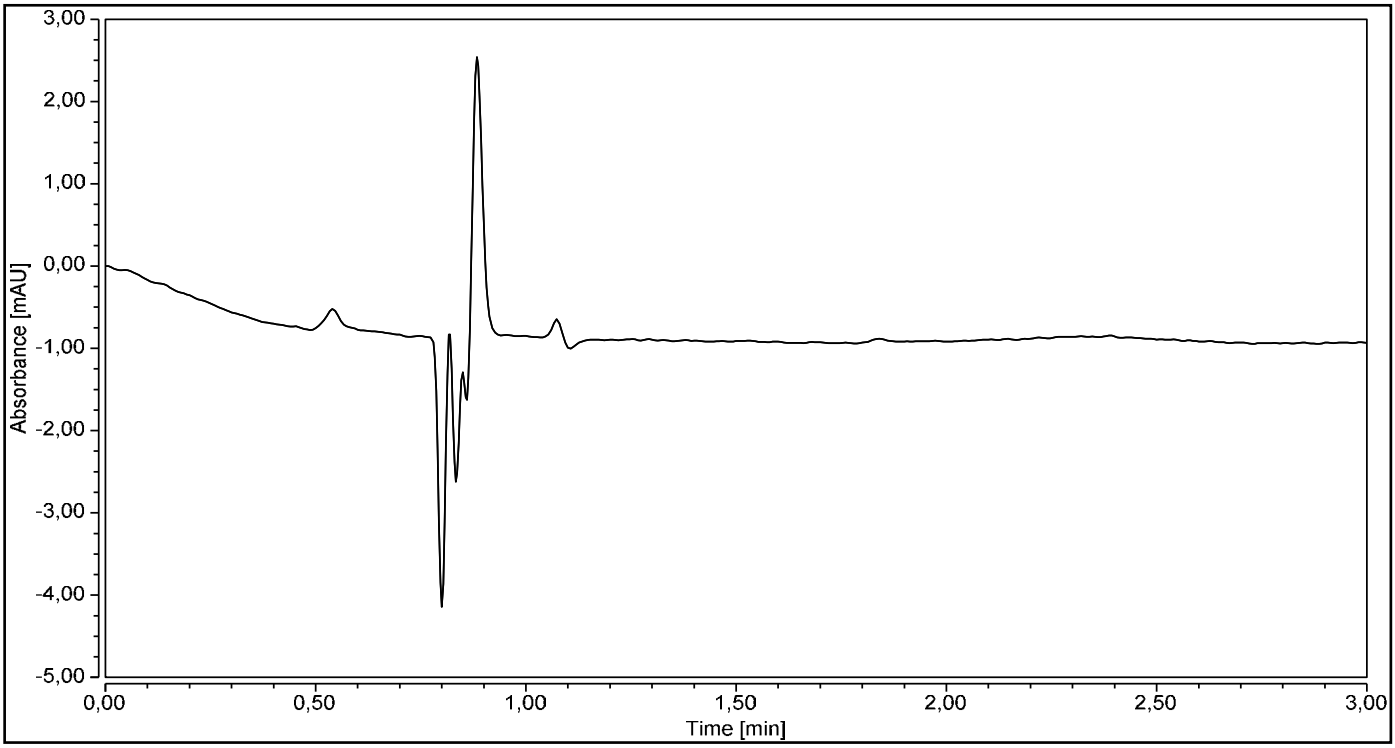

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 1*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:54*
Created By:	*Michael Careli*

Chromatogram

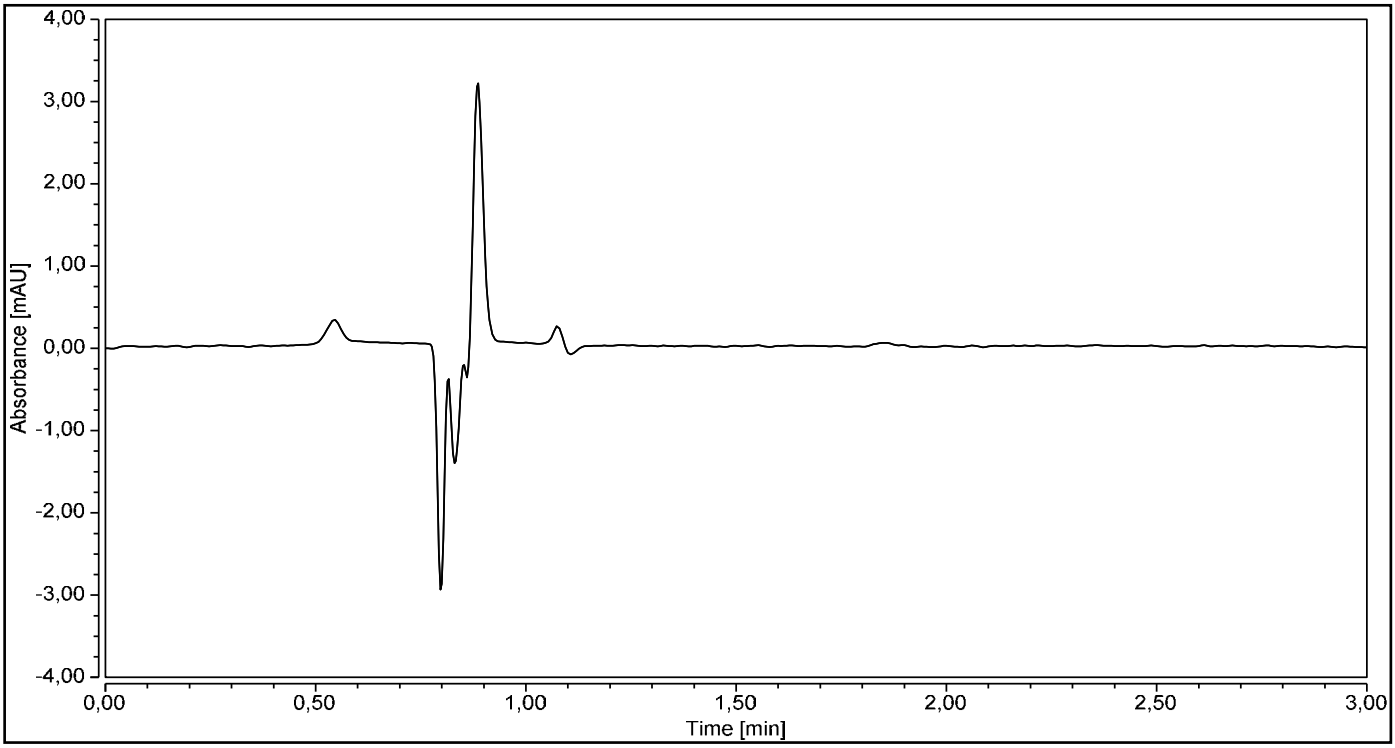

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 2*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 09:58*
Created By:	*Michael Careli*

Chromatogram

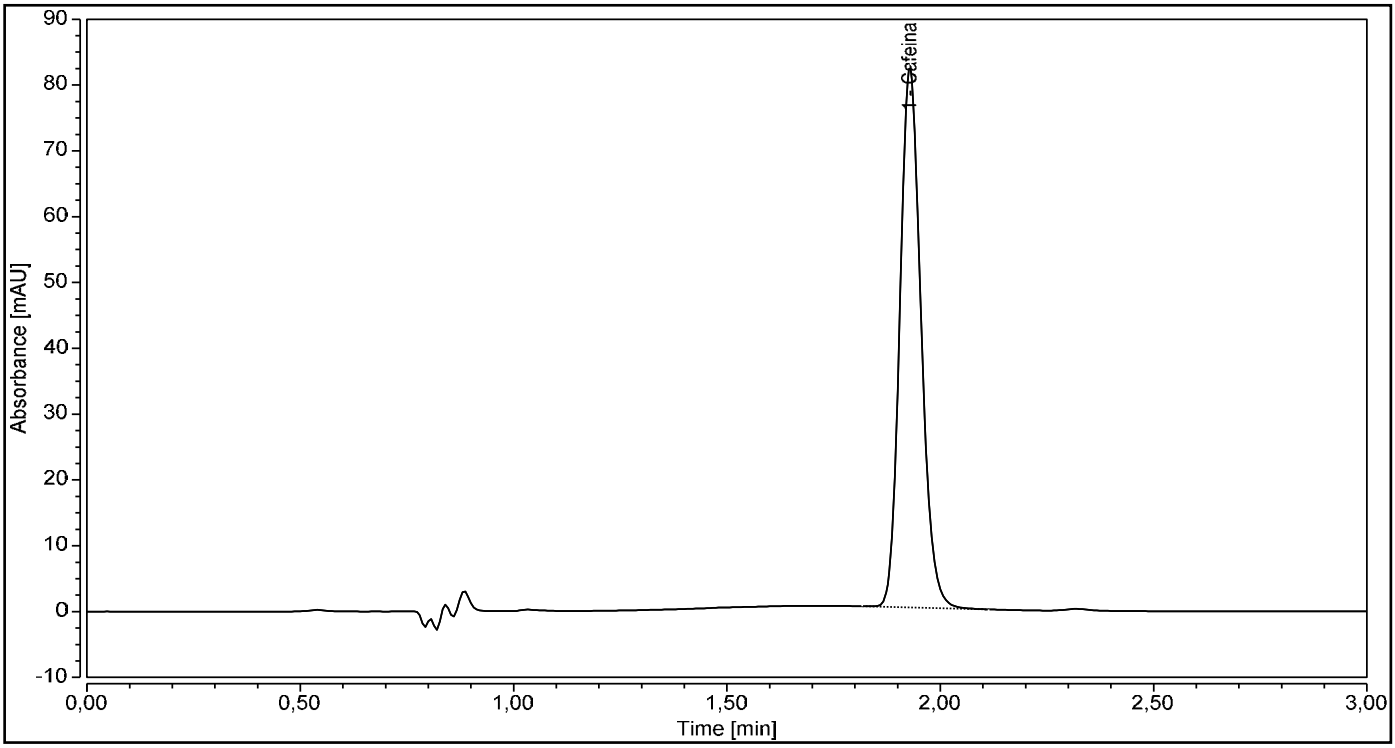

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,930	4,7188921

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:02*
Created By:	*Michael Careli*

Chromatogram

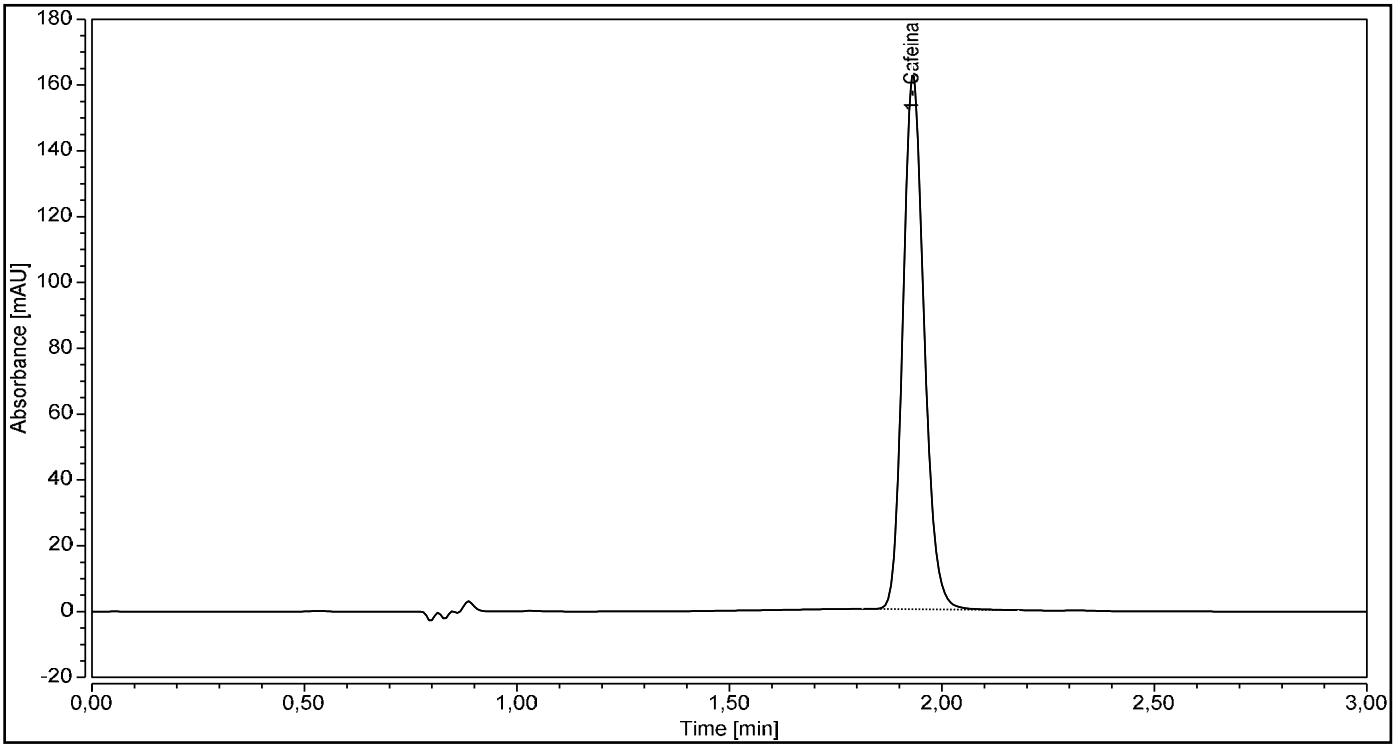

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,930	9,4291751

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 4*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:06*
Created By:	*Michael Careli*

Chromatogram

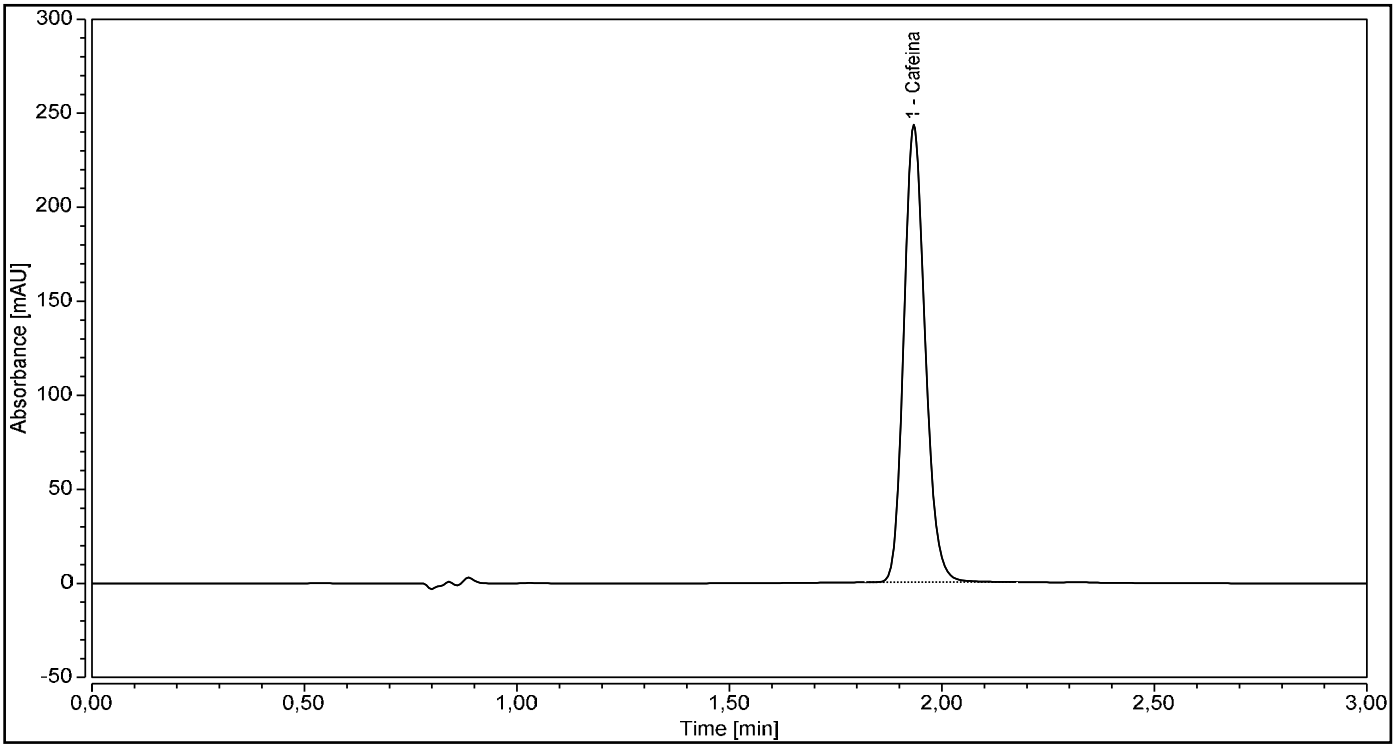

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,933	14,1394324

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LDUV 5*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:11*
Created By:	*Michael Careli*

Chromatogram

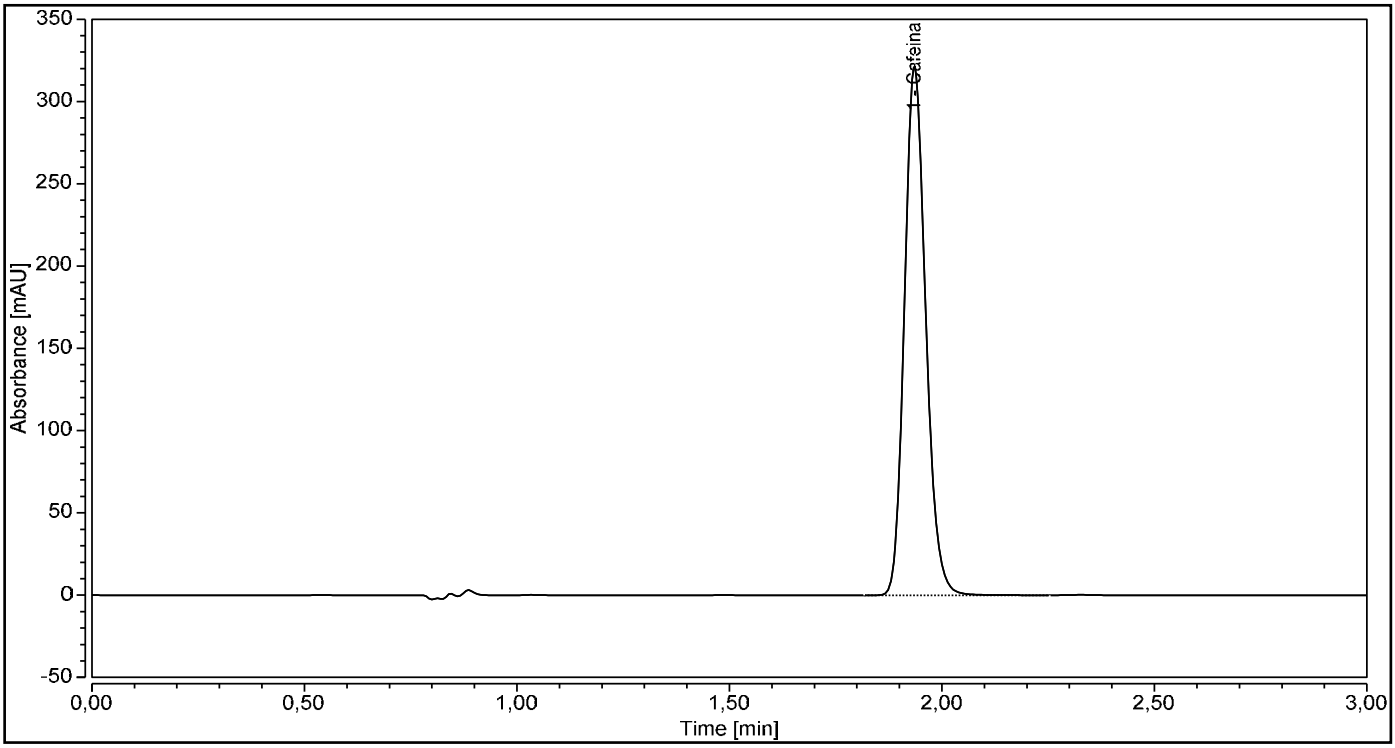

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,937	18,6774856

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 1*
Run Time (min):	*3,00*
Injection Volume:	*0,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:20*
Created By:	*Michael Careli*

Chromatogram

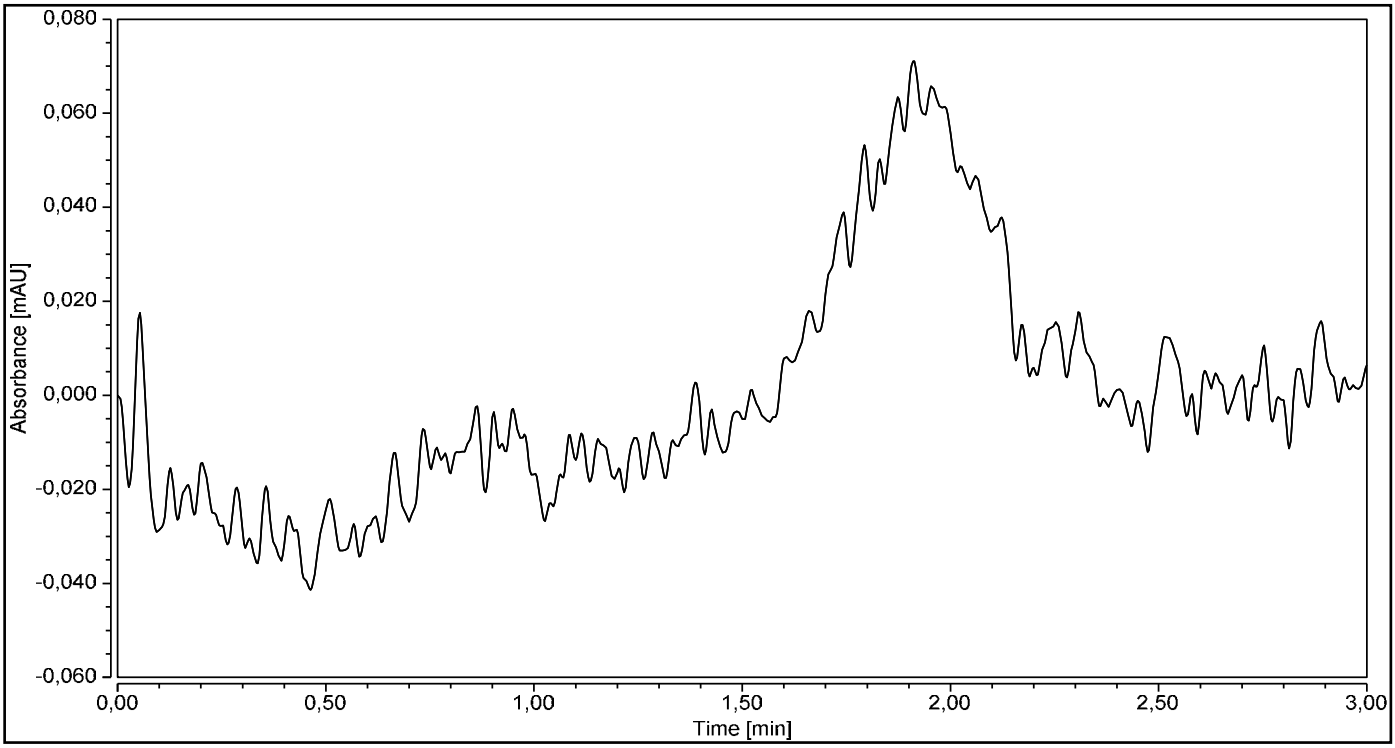

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 2*
Run Time (min):	*3,00*
Injection Volume:	*5,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:24*
Created By:	*Michael Careli*

Chromatogram

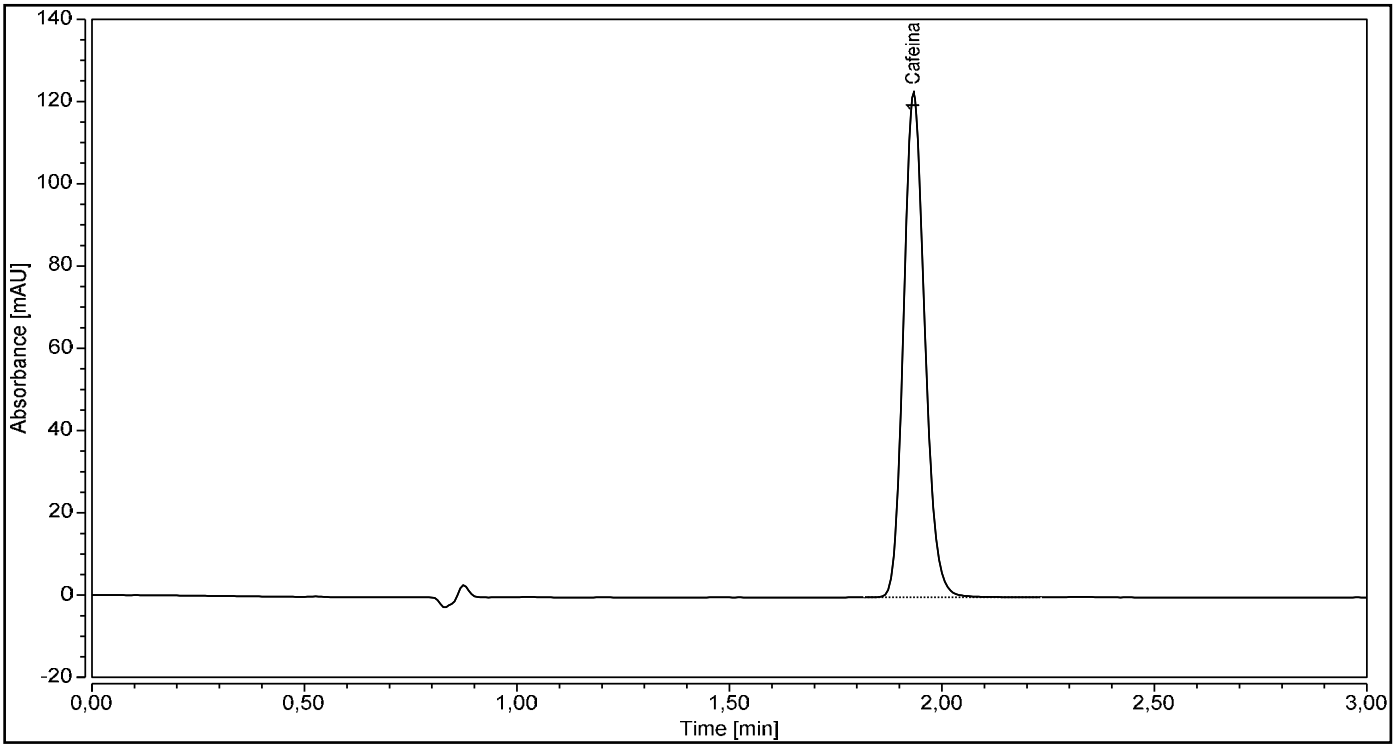

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,933	7,1092422

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 3*
Run Time (min):	*3,00*
Injection Volume:	*10,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:29*
Created By:	*Michael Careli*

Chromatogram

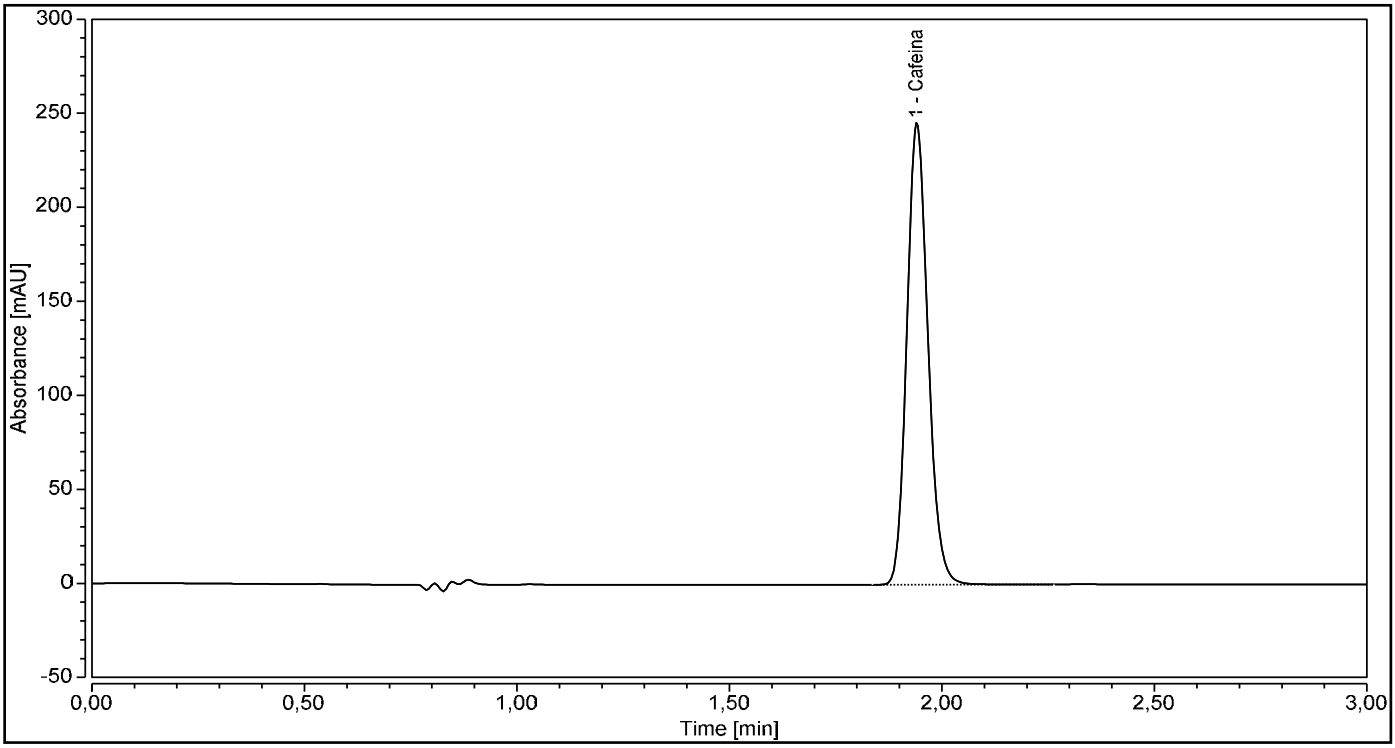

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,940	14,1561589

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 4*
Run Time (min):	*3,00*
Injection Volume:	*15,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:33*
Created By:	*Michael Careli*

Chromatogram

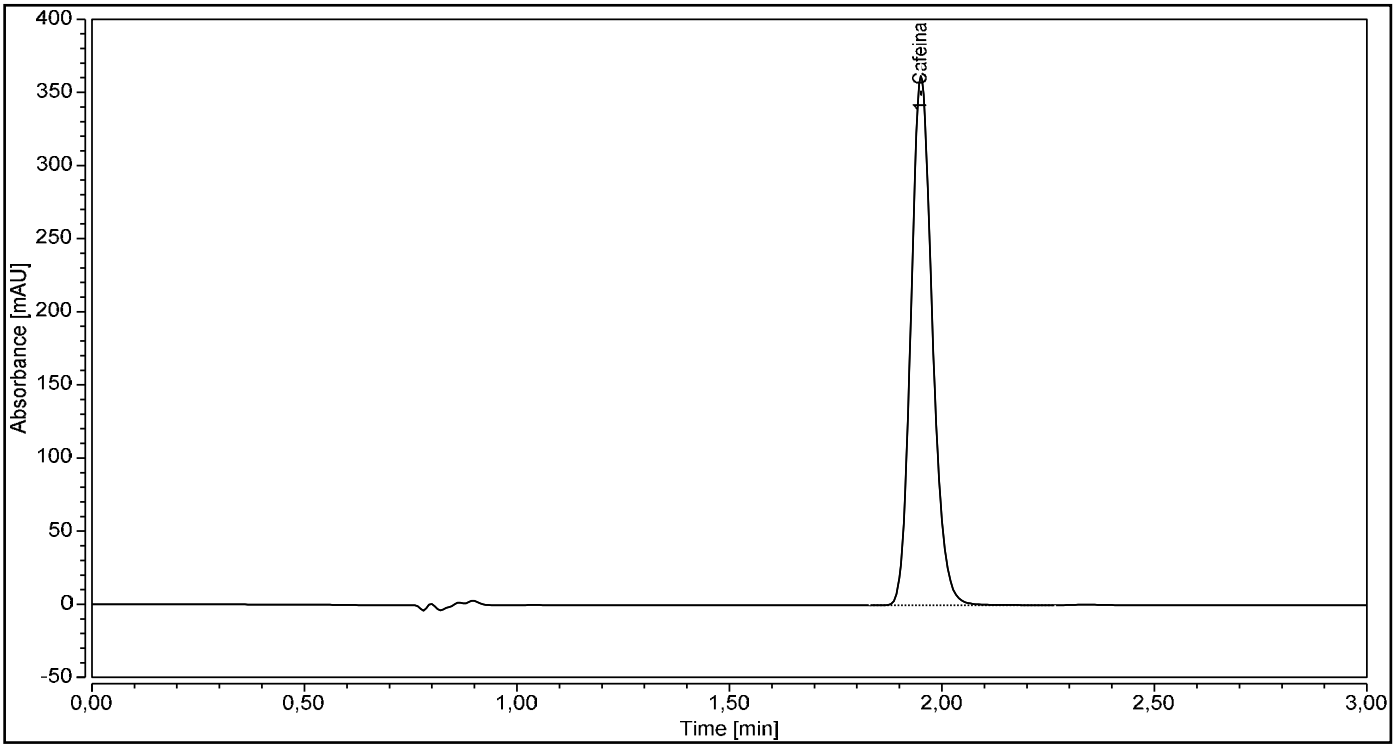

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,950	21,1737132

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*LIIN 5*
Run Time (min):	*3,00*
Injection Volume:	*20,00*
Instrument Method:	*Qualificação*
Processing Method:	*Qualificação*
Injection Date/Time:	*23/mai/19 10:37*
Created By:	*Michael Careli*

Chromatogram

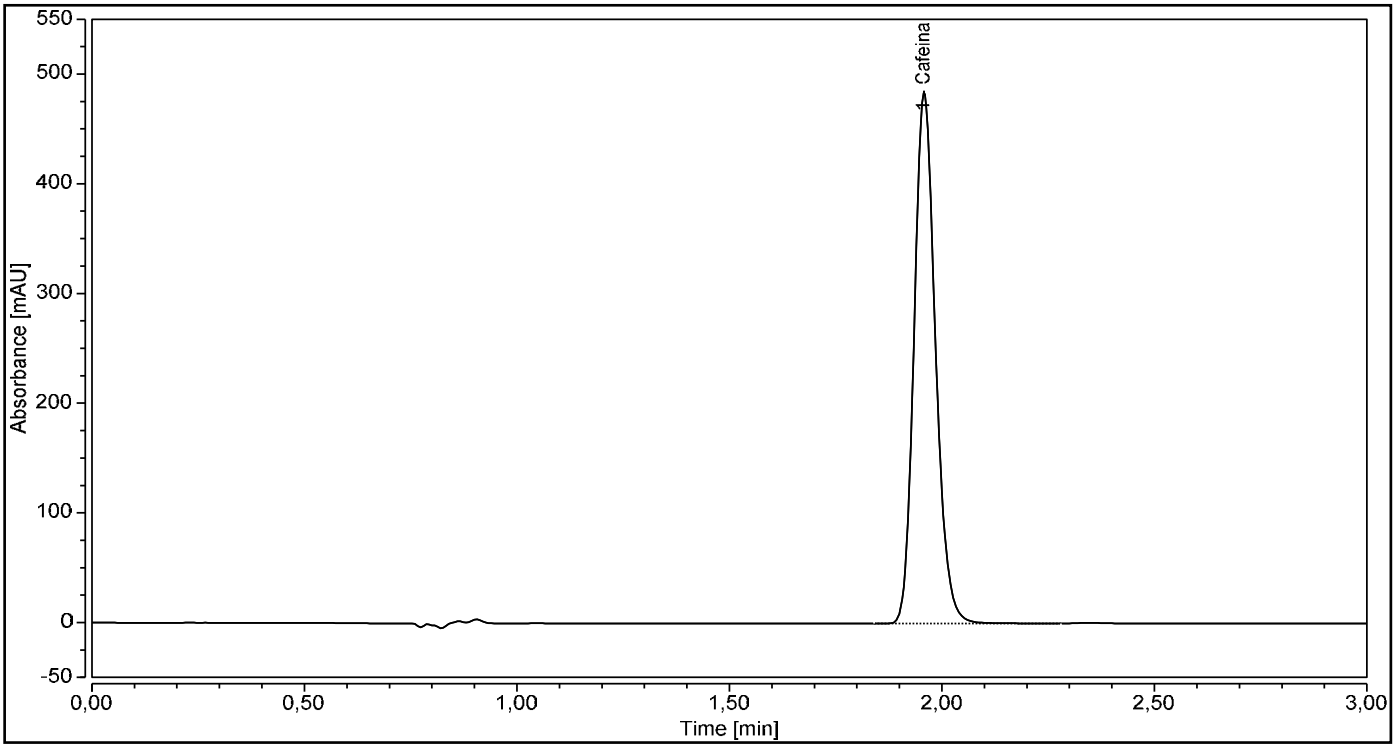

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min
1	Cafeina	1,957	28,2934266

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Grad AB*
Run Time (min):	*19,00*
Injection Volume:	*0,00*
Instrument Method:	*Grad AB*
Processing Method:	*Gradiente*
Injection Date/Time:	*23/mai/19 11:03*
Created By:	*Michael Careli*

Chromatogram

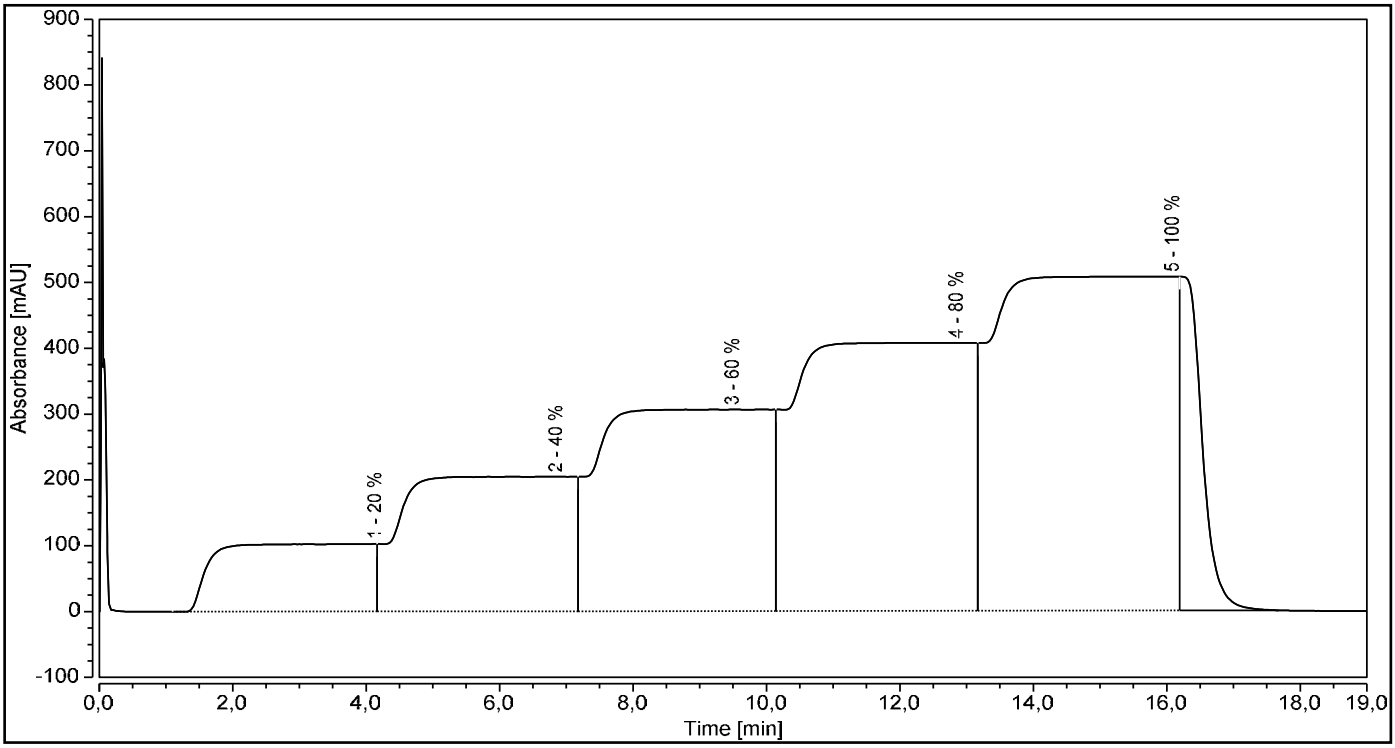

Integration Results


No.	Peak Name	Retention Time min	Height mAU
1	20 %	4,140	102,669
2	40 %	6,847	204,692
3	60 %	9,493	306,343
4	80 %	12,860	407,102
5	100 %	16,093	507,163

CLARION®
LABORATÓRIO DE ALTA TECNOLOGIA

Injection Details

Injection Name:	*Grad CD*
Run Time (min):	*19,00*
Injection Volume:	*0,00*
Instrument Method:	*Grad CD*
Processing Method:	*Gradiente*
Injection Date/Time:	*23/mai/19 11:34*
Created By:	*Michael Careli*

Chromatogram

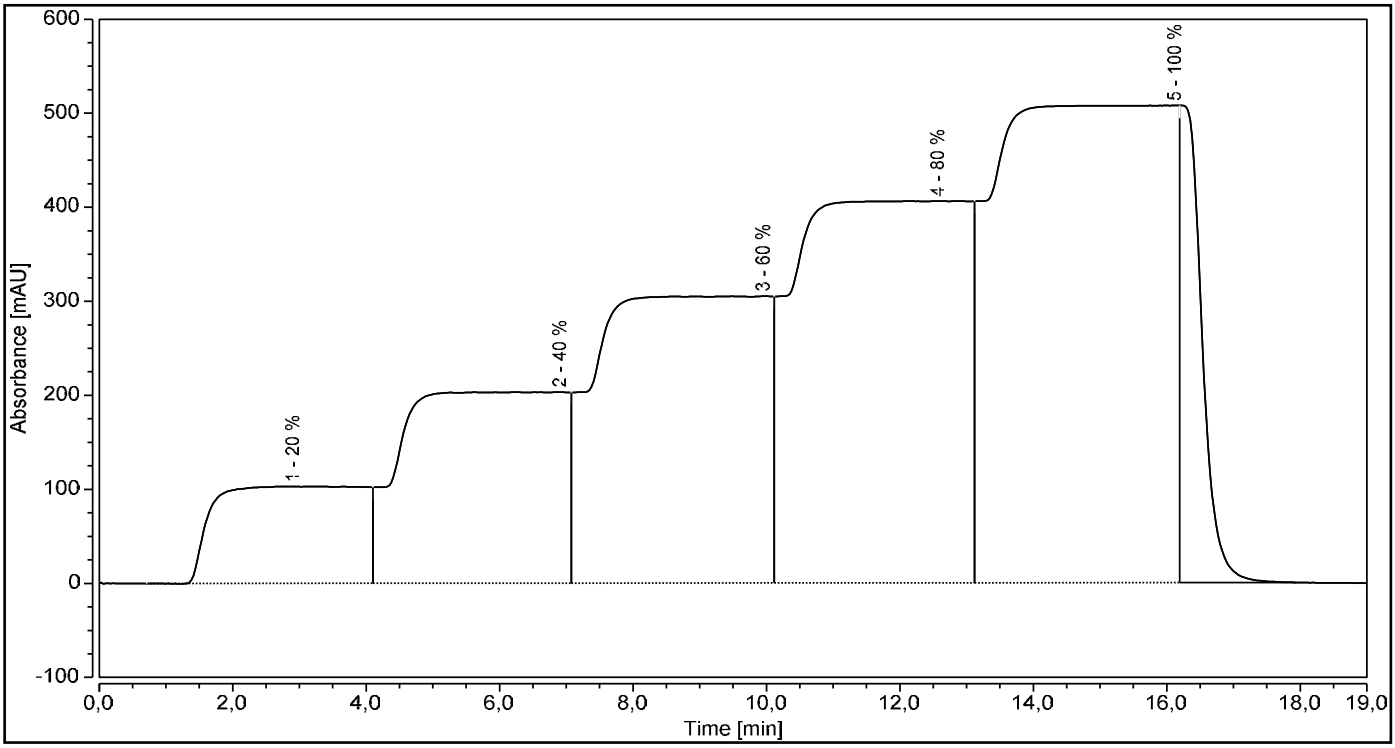

Integration Results

No.	Peak Name	Retention Time min	Height mAU
1	20 %	2,917	103,047
2	40 %	6,910	203,177
3	60 %	9,960	304,990
4	80 %	12,577	405,936
5	100 %	16,130	507,309