
SAMPLE INFORMATION

Sample Name:	B01	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,1	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:11:46 AM BRT -03:00
Date Processed: 7/3/2018 1:02:04 PM BRT -03:00

Auto-Scaled Chromatogram

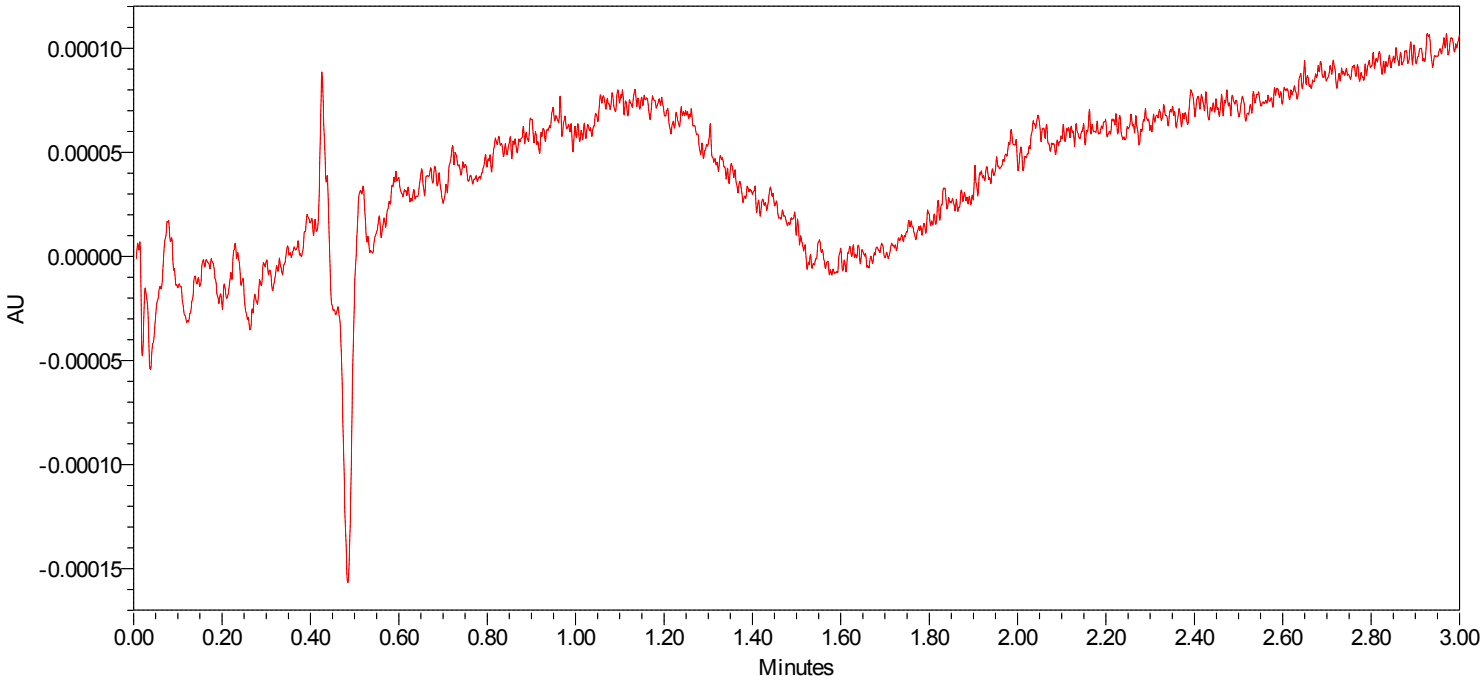

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522				

SAMPLE INFORMATION

Sample Name:	B02	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,1	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:26:32 AM BRT -03:00
Date Processed: 7/3/2018 12:56:17 PM BRT -03:00

Auto-Scaled Chromatogram

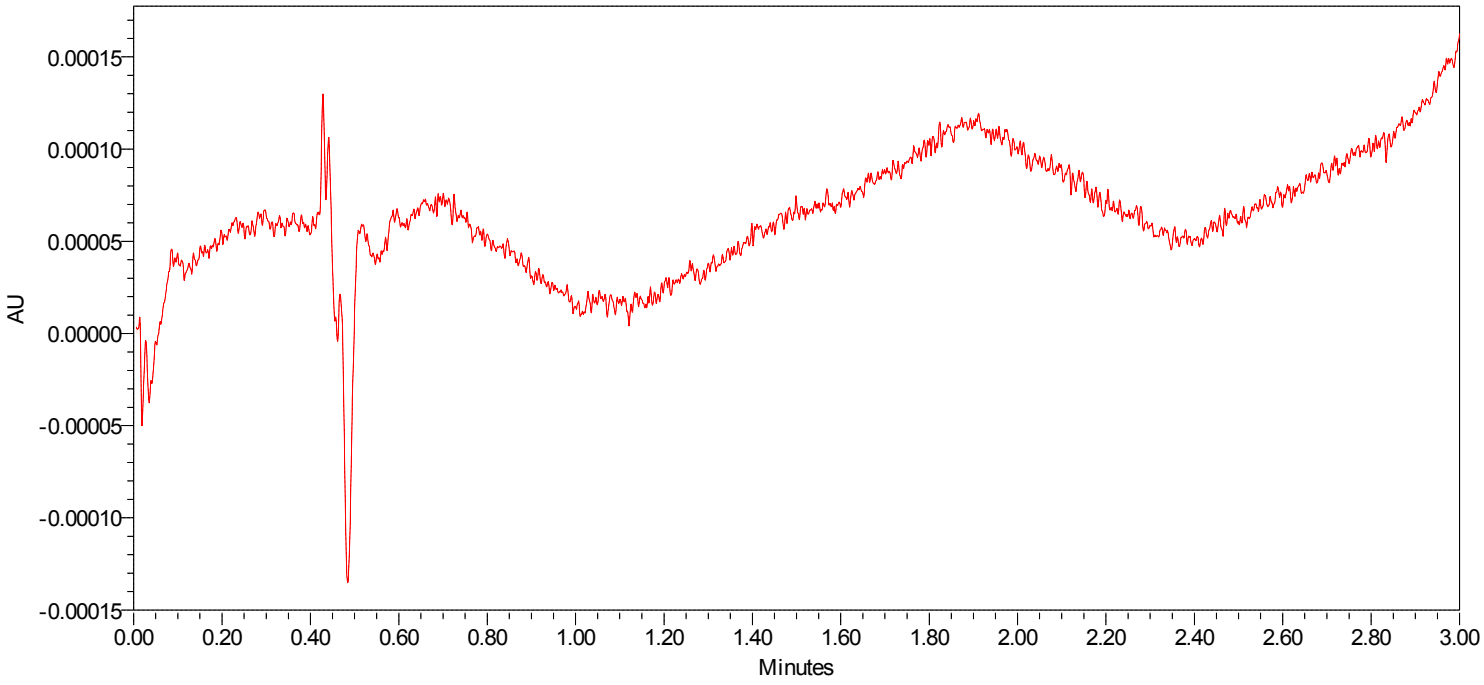

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522				

SAMPLE INFORMATION

Sample Name:	B03	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,1	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:41:16 AM BRT -03:00
Date Processed: 7/3/2018 1:01:29 PM BRT -03:00

Auto-Scaled Chromatogram

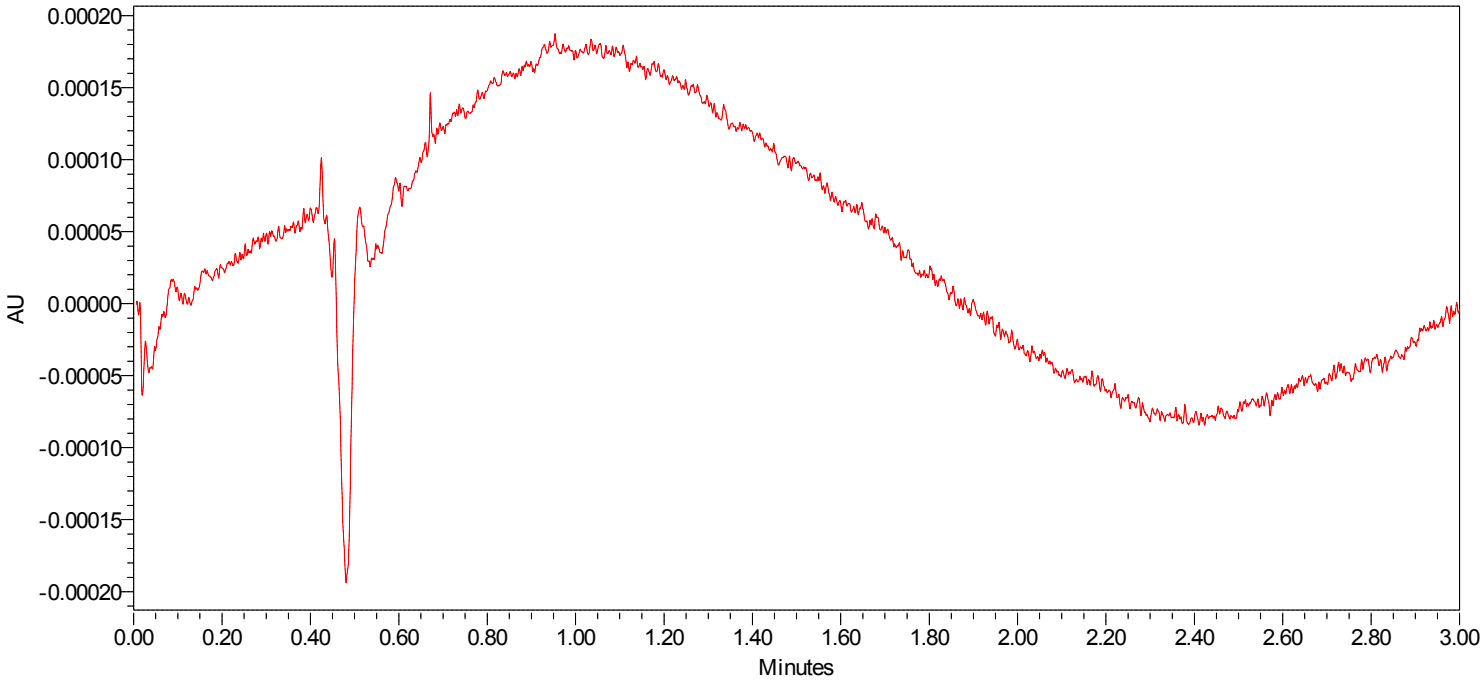

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522				

SAMPLE INFORMATION

Sample Name:	Gradiente AB	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	1:A,1	Acq. Method Set:	Qualificacao Gradiente
Injection #:	2	Processing Method:	Gradiente AB
Injection Volume:	0.10 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	15.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 3:38:36 PM BRT -03:00
Date Processed: 7/3/2018 3:56:57 PM BRT -03:00

Auto-Scaled Chromatogram

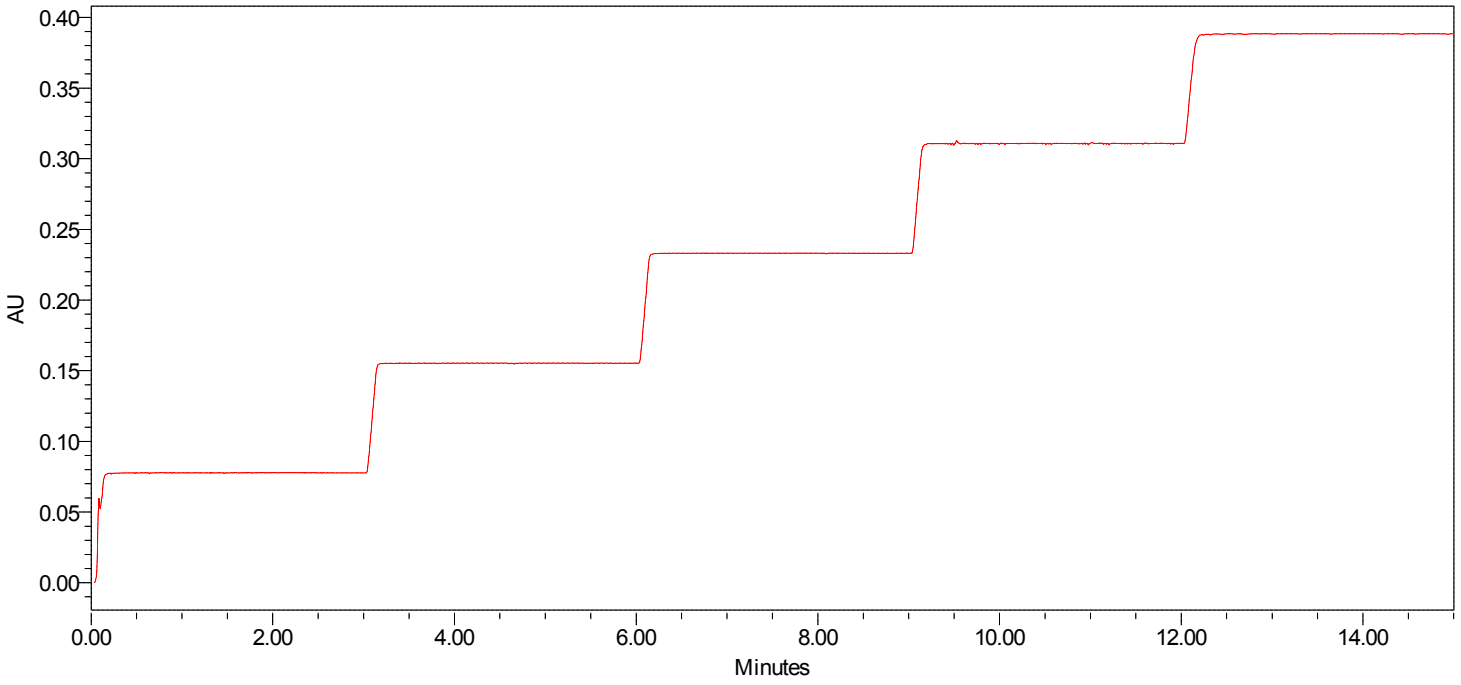

Peak Results


	Name	RT	Area	Height	Amount	Units
1						

SAMPLE INFORMATION

Sample Name:	LDUV01	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LDUV
Vial:	1:A,1	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 12:42:12 PM BRT -03:00
Date Processed: 7/3/2018 1:04:48 PM BRT -03:00

Auto-Scaled Chromatogram

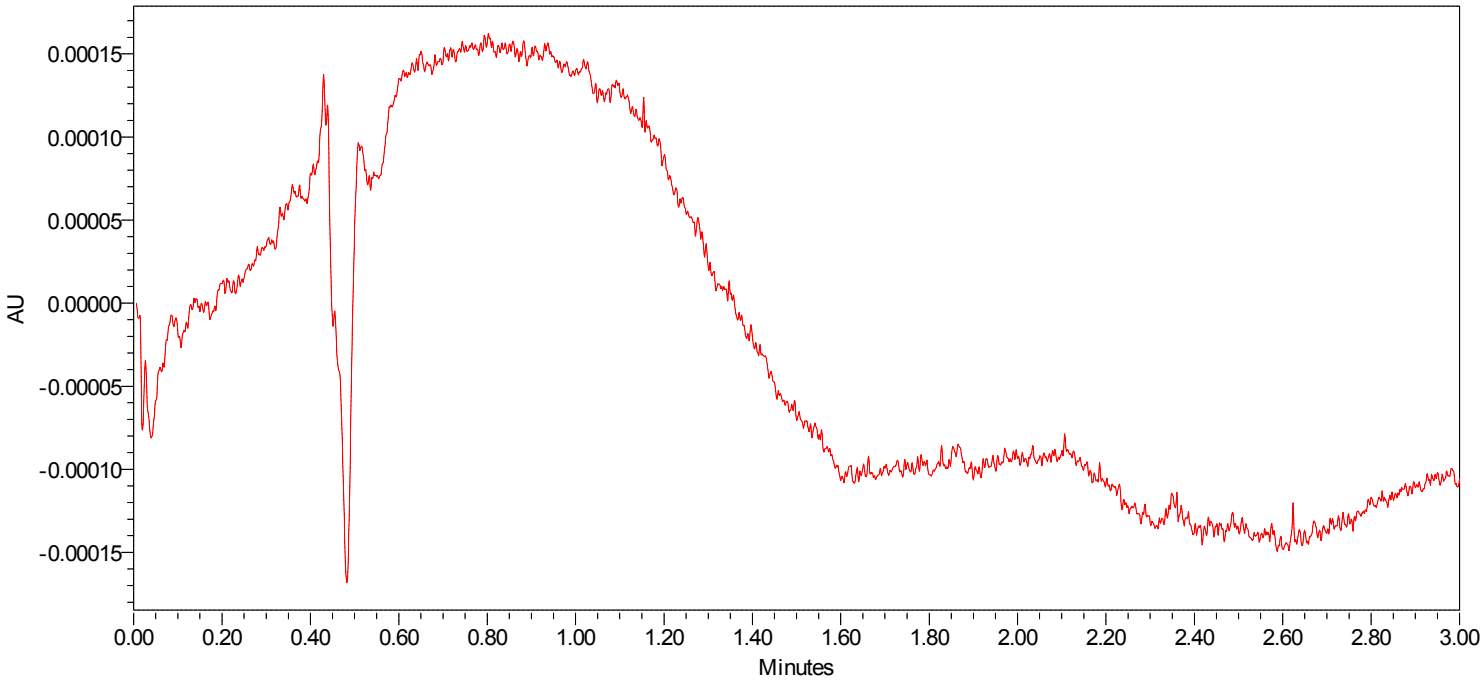

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522				

SAMPLE INFORMATION

Sample Name:	LDUV02	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LDUV
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 12:45:55 PM BRT -03:00
Date Processed: 7/3/2018 1:05:27 PM BRT -03:00

Auto-Scaled Chromatogram

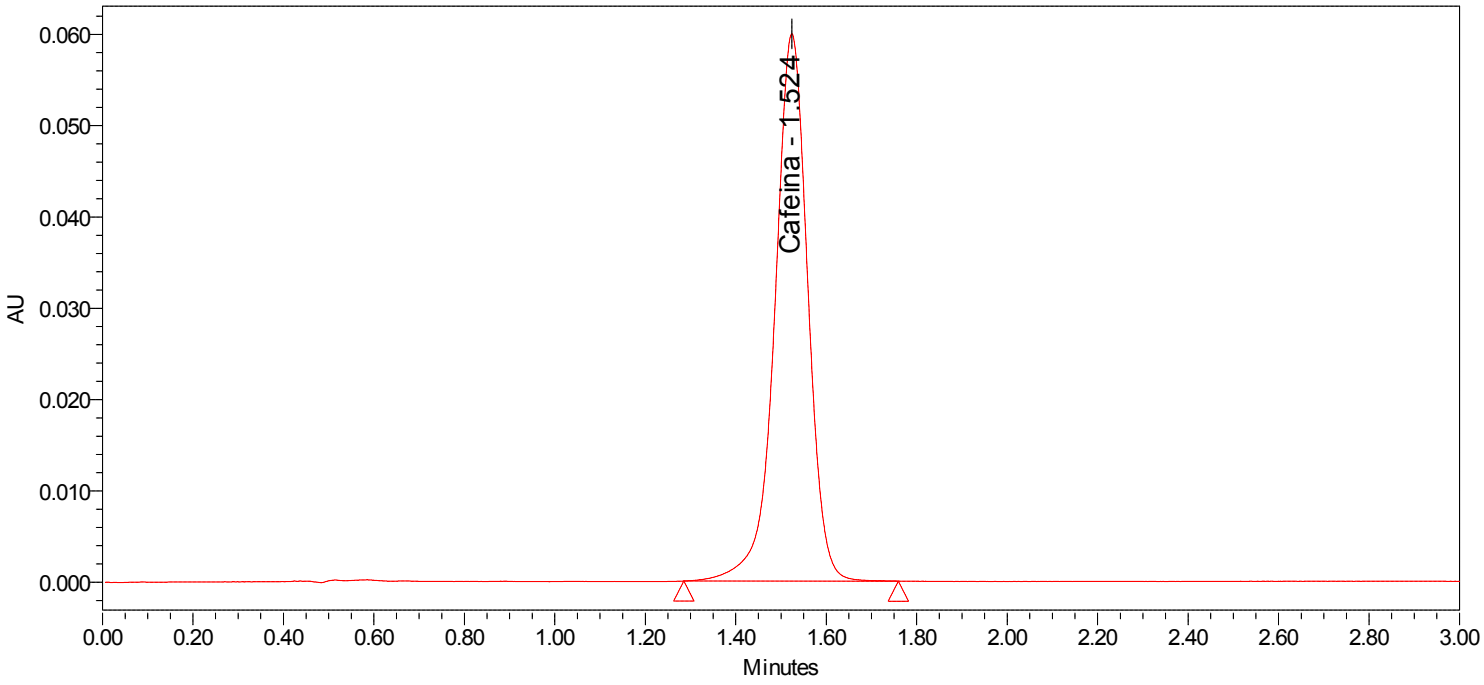

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.524	303193	59945		

SAMPLE INFORMATION

Sample Name:	LDUV03	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LDUV
Vial:	1:A,3	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 12:49:35 PM BRT -03:00
Date Processed: 7/3/2018 1:06:13 PM BRT -03:00

Auto-Scaled Chromatogram

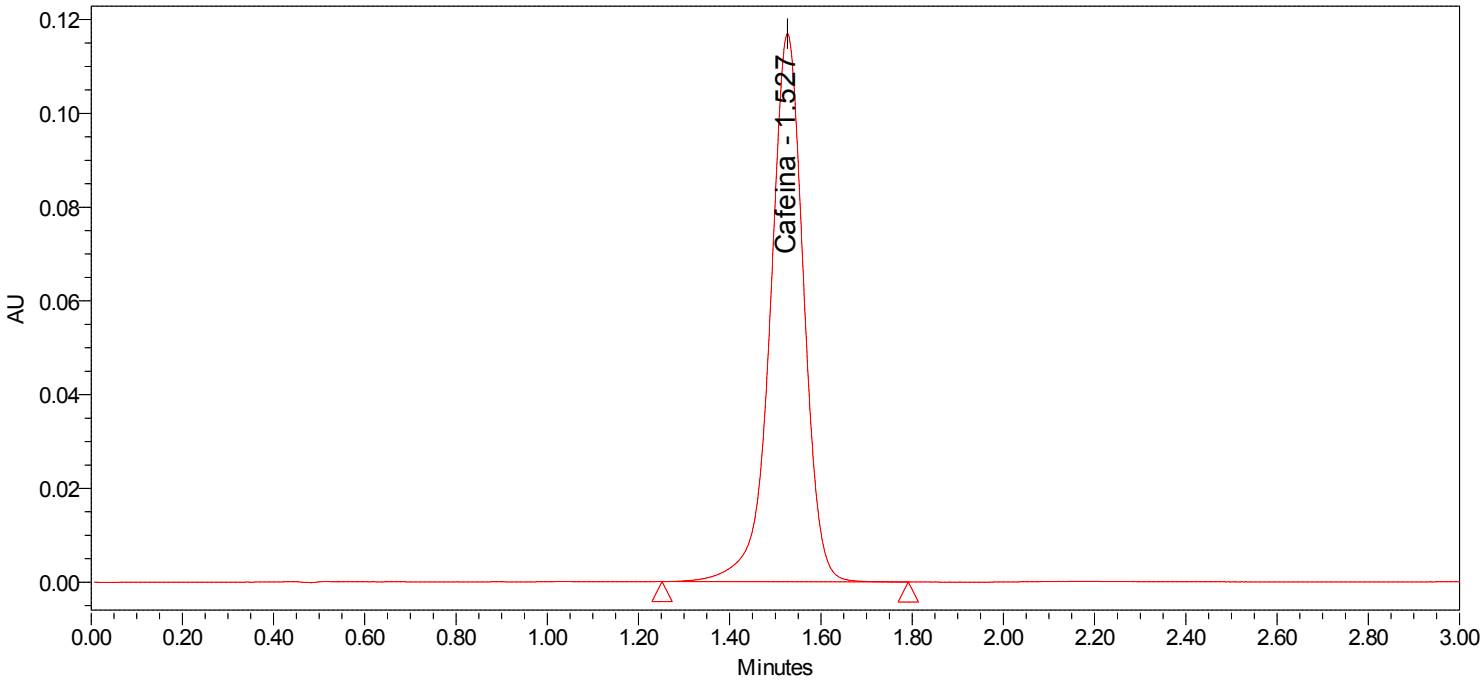

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.527	593238	116933		

SAMPLE INFORMATION

Sample Name:	LDUV04	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LDUV
Vial:	1:A,4	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 12:53:19 PM BRT -03:00
Date Processed: 7/3/2018 1:06:51 PM BRT -03:00

Auto-Scaled Chromatogram

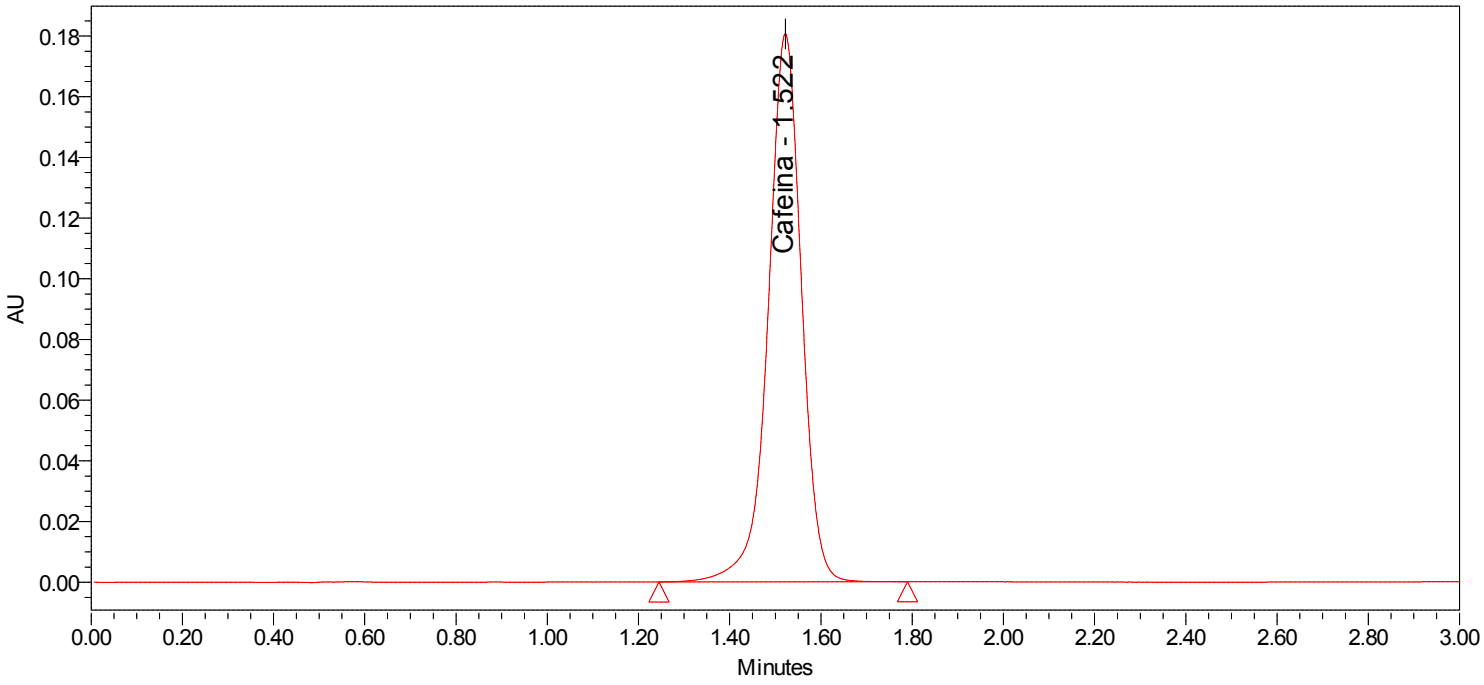

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522	912542	180669		

SAMPLE INFORMATION

Sample Name:	LDUV05	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LDUV
Vial:	1:A,5	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 12:56:59 PM BRT -03:00
Date Processed: 7/3/2018 1:07:27 PM BRT -03:00

Auto-Scaled Chromatogram

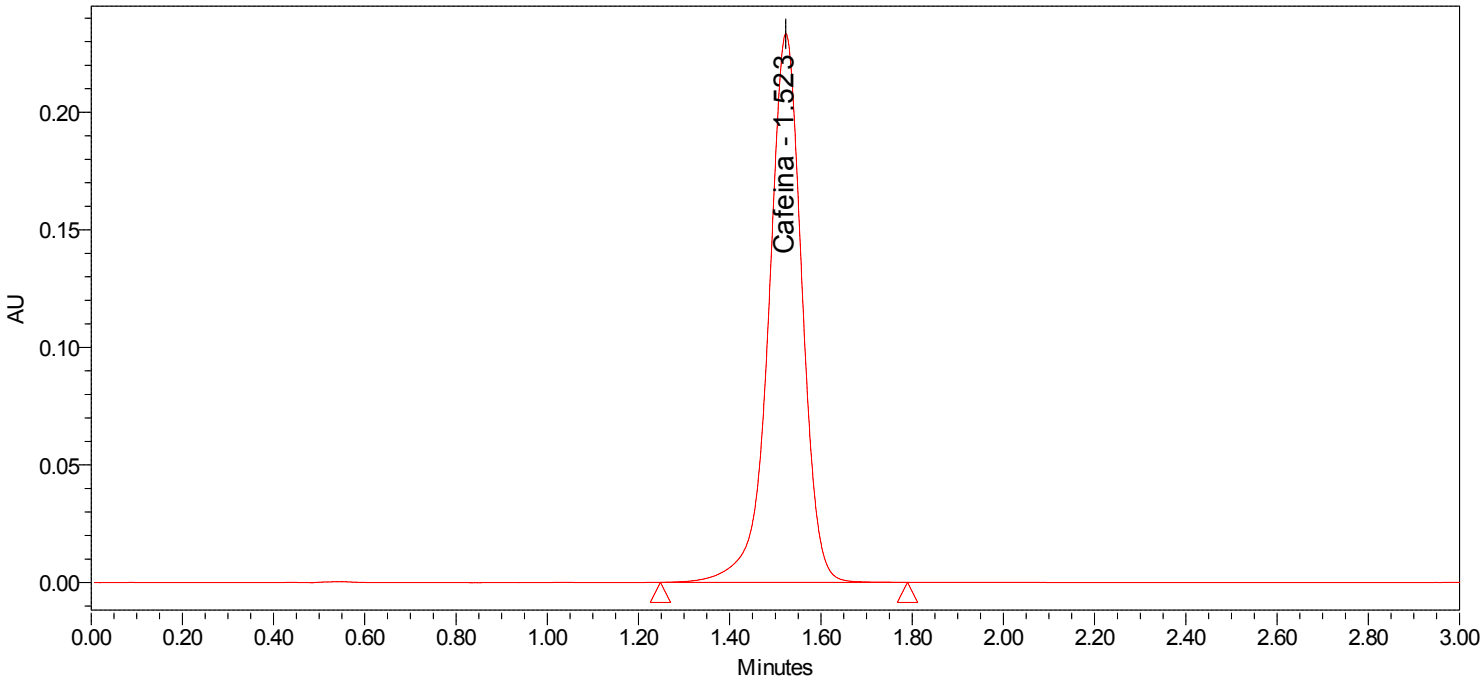

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.523	1178967	233326		

SAMPLE INFORMATION

Sample Name:	LIIN01	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LIIN
Vial:	1:A,6	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	2.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 1:30:40 PM BRT -03:00
Date Processed: 7/3/2018 4:01:38 PM BRT -03:00

Auto-Scaled Chromatogram

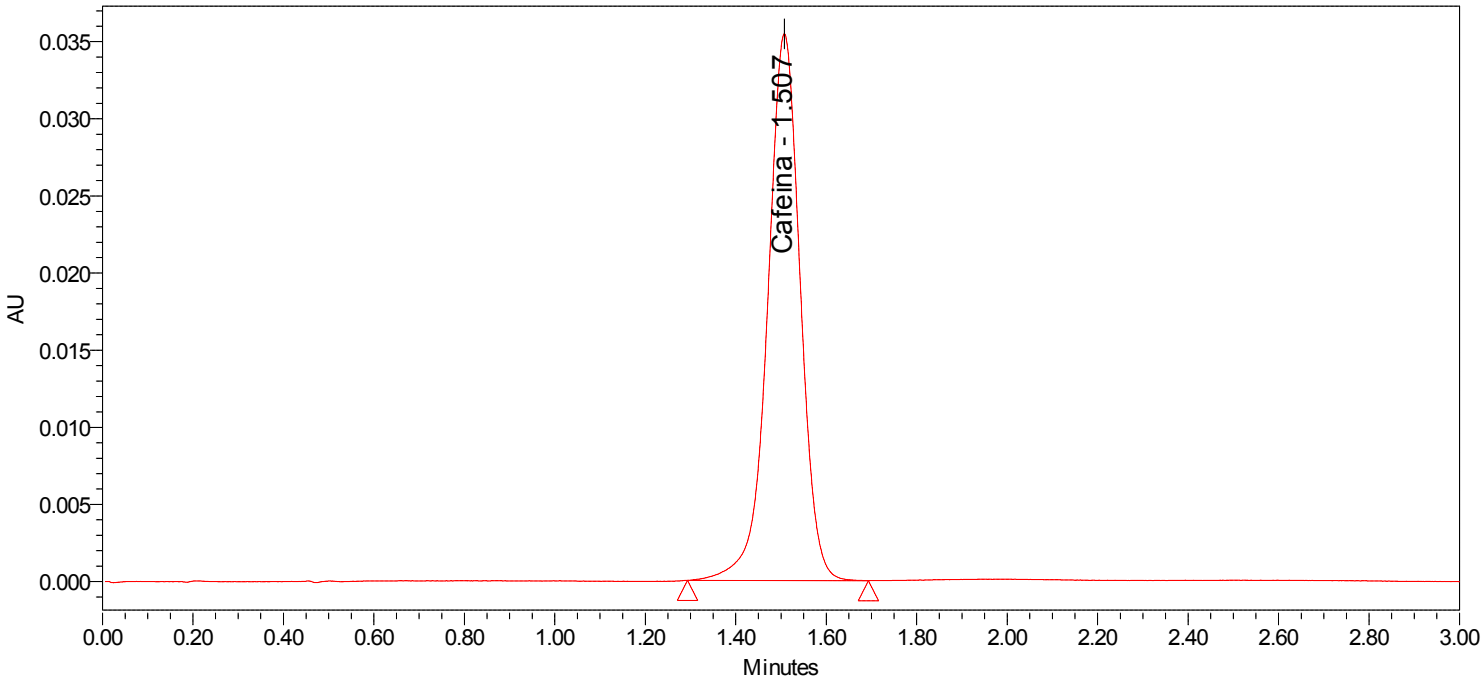

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.507	177367	35451		

SAMPLE INFORMATION

Sample Name:	LIIN02	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LIIN
Vial:	1:A,6	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	4.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 1:34:09 PM BRT -03:00
Date Processed: 7/3/2018 4:02:23 PM BRT -03:00

Auto-Scaled Chromatogram

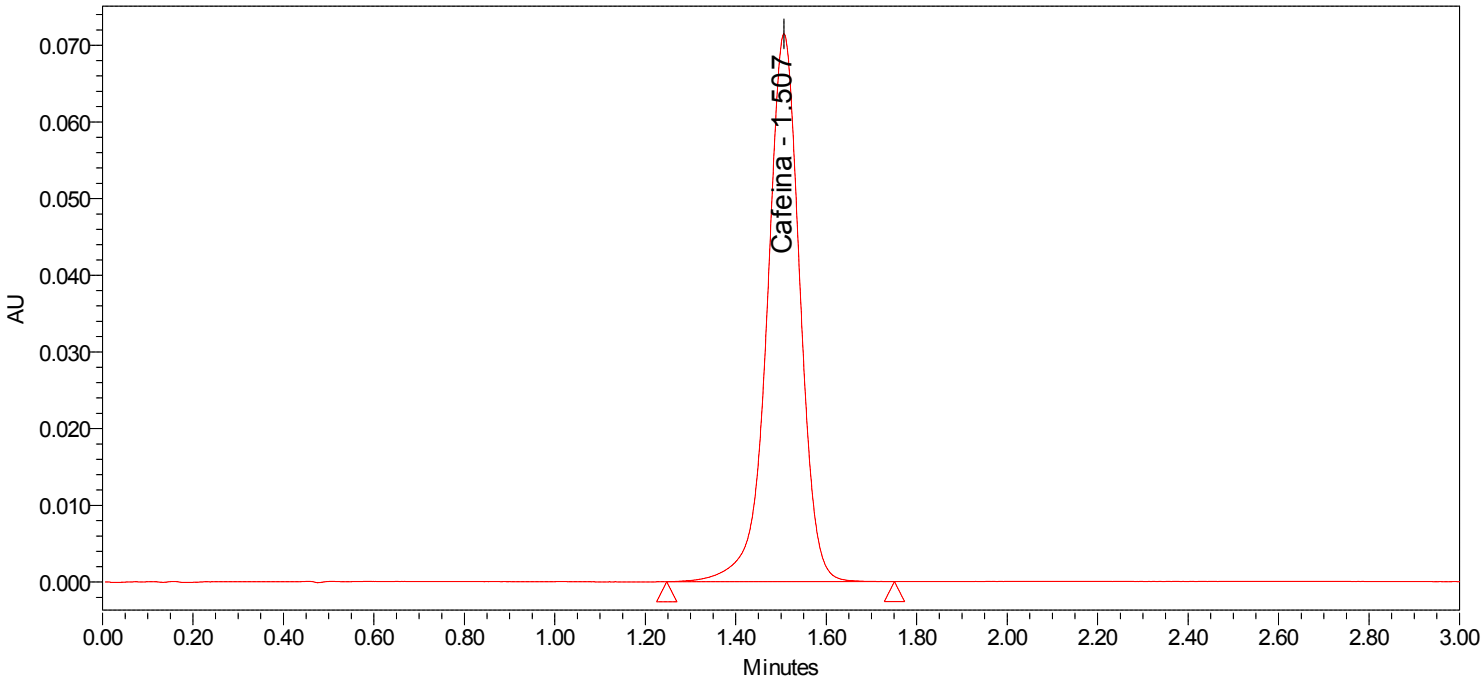

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.507	358996	71470		

SAMPLE INFORMATION

Sample Name:	LIIN03	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LIIN
Vial:	1:A,6	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	6.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 1:37:42 PM BRT -03:00
Date Processed: 7/3/2018 4:03:00 PM BRT -03:00

Auto-Scaled Chromatogram

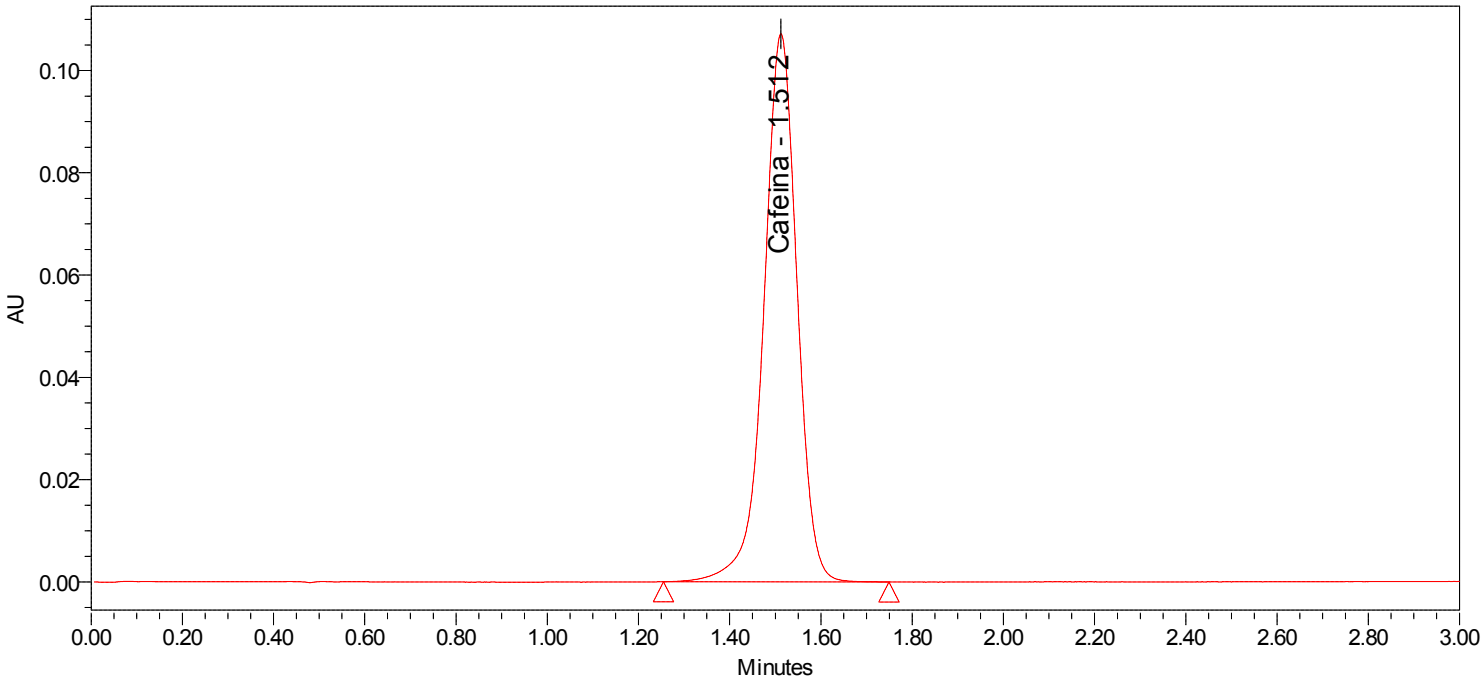

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.512	541259	107194		

SAMPLE INFORMATION

Sample Name:	LIIN04	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LIIN
Vial:	1:A,6	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	8.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 1:41:19 PM BRT -03:00
Date Processed: 7/3/2018 4:03:32 PM BRT -03:00

Auto-Scaled Chromatogram

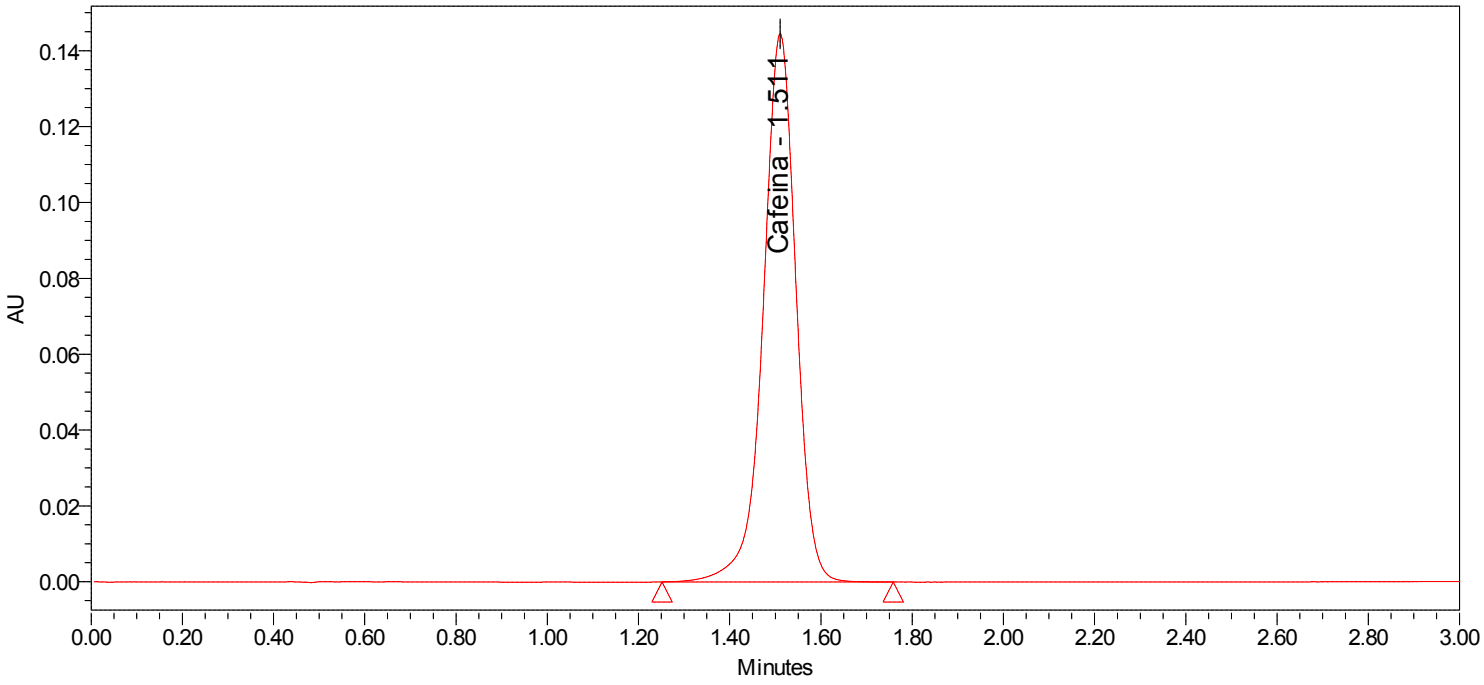

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.511	720974	144567		

SAMPLE INFORMATION

Sample Name:	LIIN05	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	LIIN
Vial:	1:A,6	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 1:44:59 PM BRT -03:00
Date Processed: 7/3/2018 4:04:06 PM BRT -03:00

Auto-Scaled Chromatogram

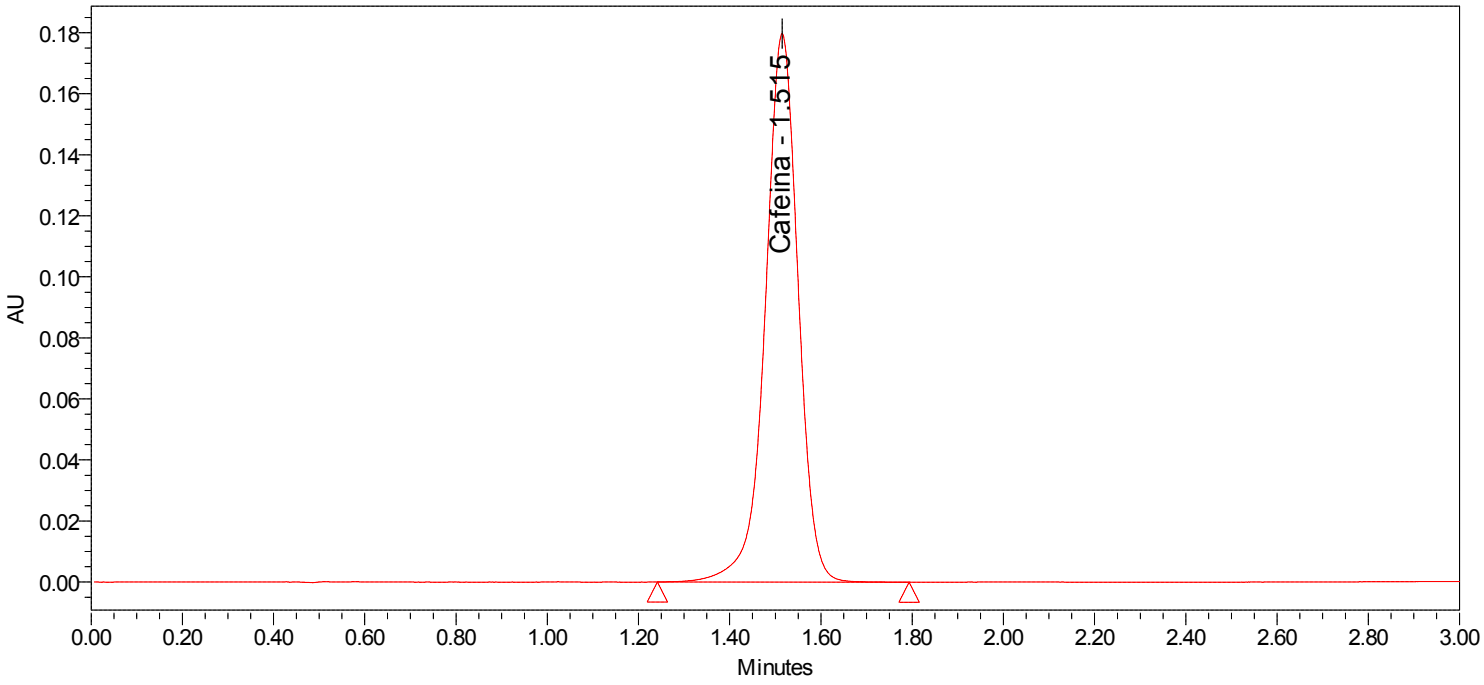

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.515	899959	179754		

SAMPLE INFORMATION

Sample Name:	PCIN01	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:15:28 AM BRT -03:00
Date Processed: 7/3/2018 12:42:47 PM BRT -03:00

Auto-Scaled Chromatogram

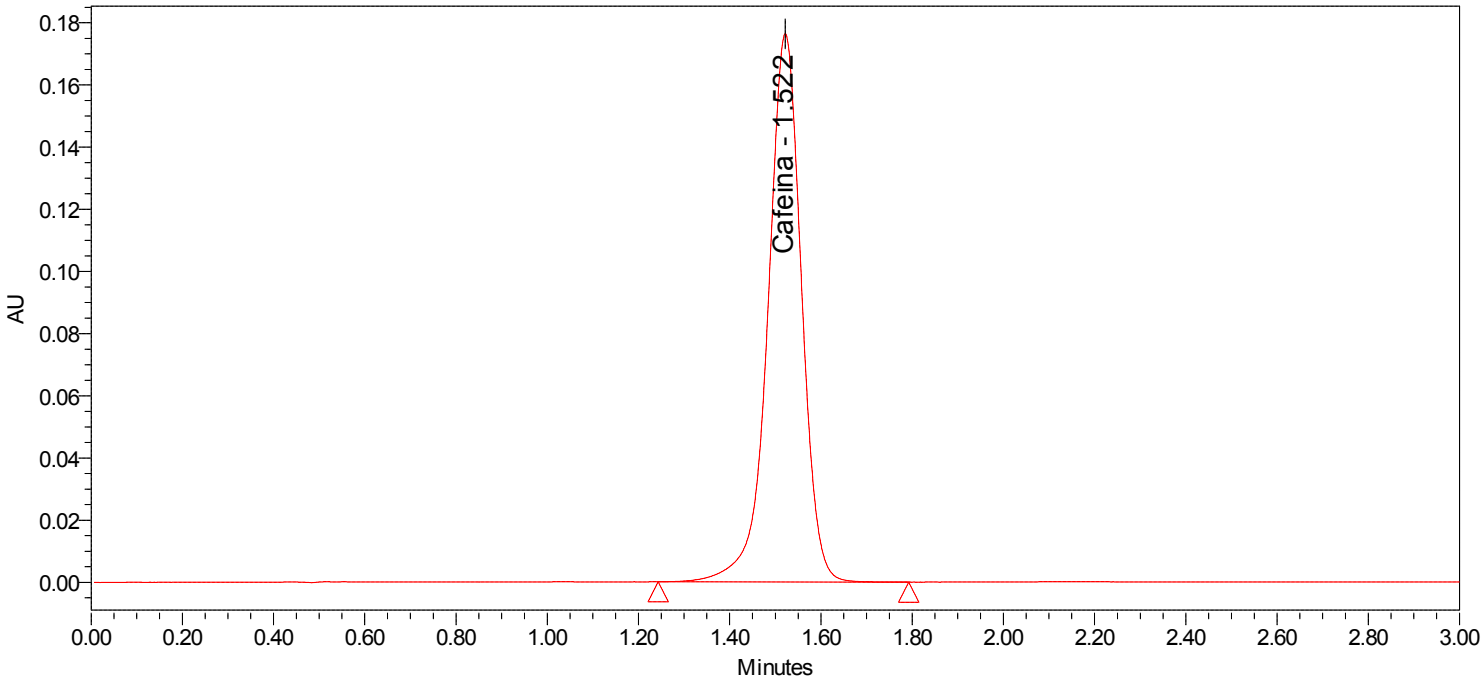

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.522	900295	176387		

SAMPLE INFORMATION

Sample Name:	PCIN02	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:19:08 AM BRT -03:00
Date Processed: 7/3/2018 1:03:04 PM BRT -03:00

Auto-Scaled Chromatogram

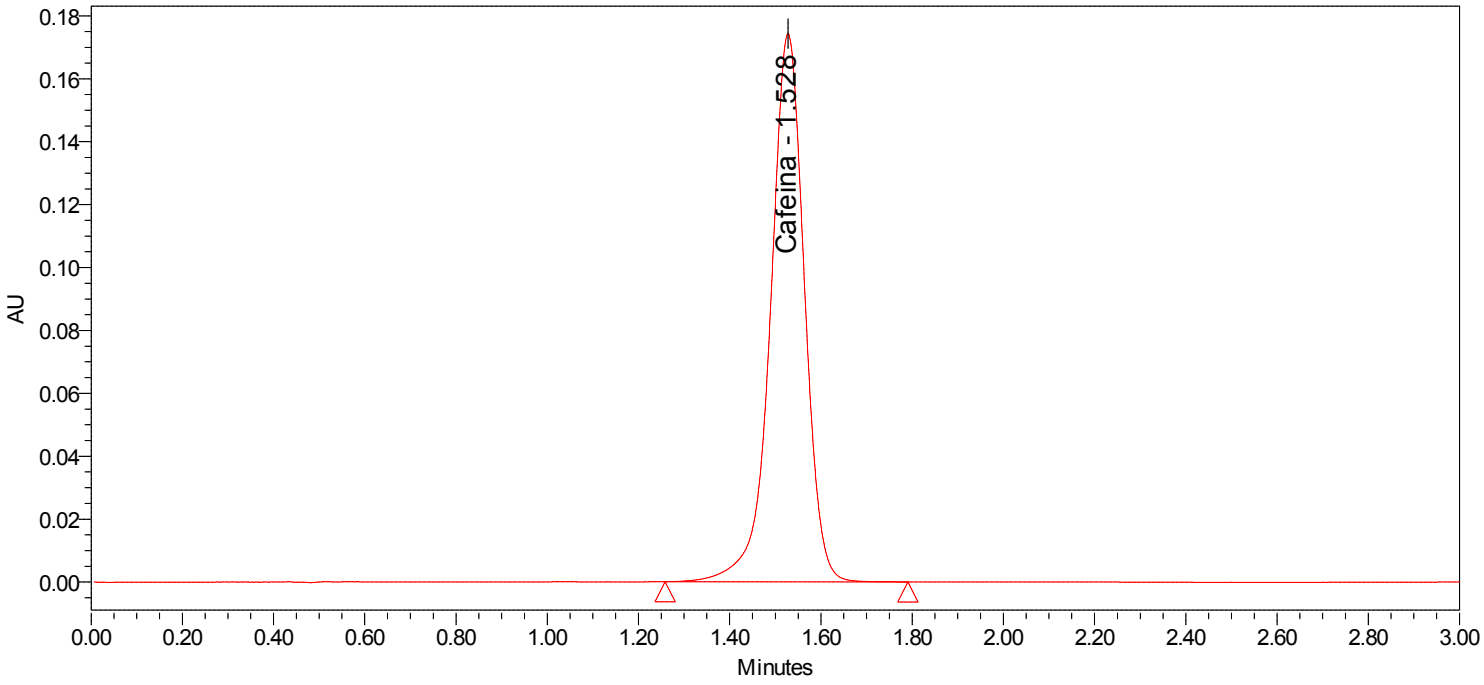

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.528	900744	174295		

SAMPLE INFORMATION

Sample Name:	PCIN03	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:22:50 AM BRT -03:00
Date Processed: 7/3/2018 12:52:13 PM BRT -03:00

Auto-Scaled Chromatogram

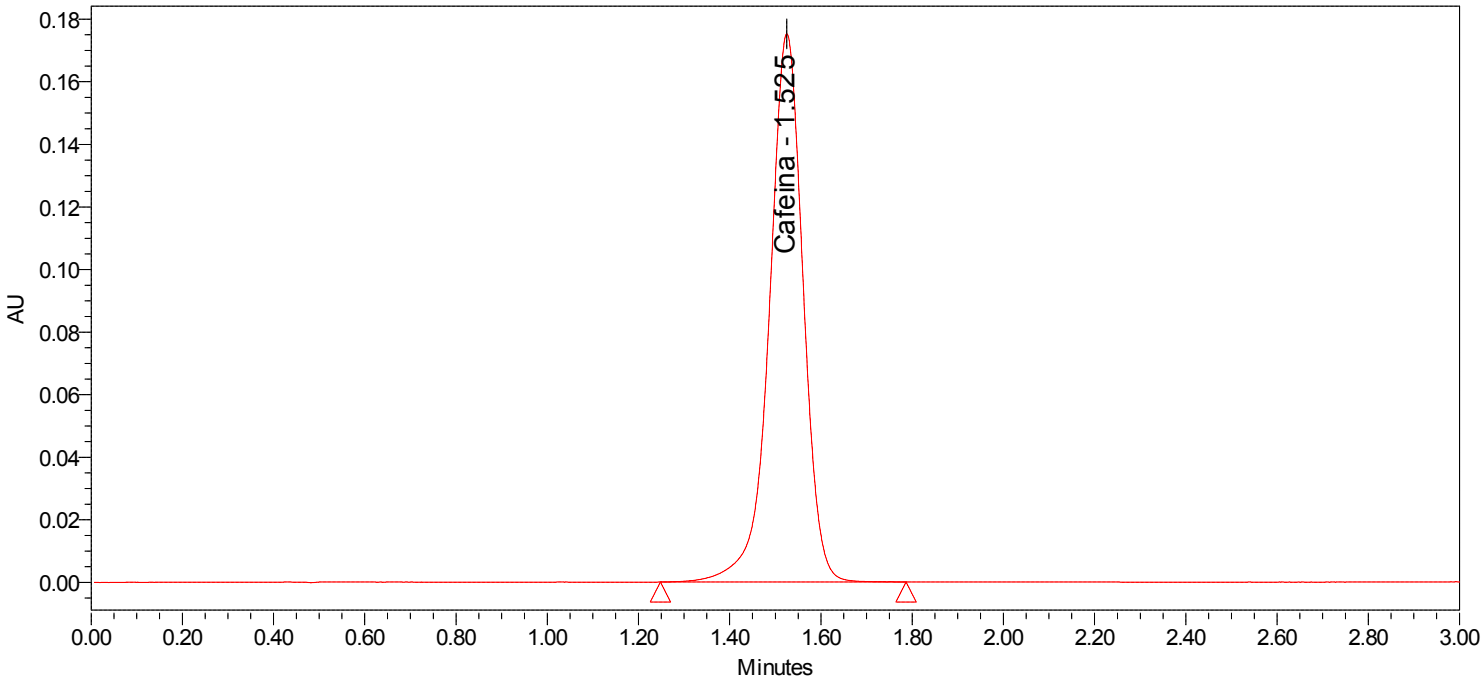

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.525	901272	175267		

SAMPLE INFORMATION

Sample Name:	PCIN04	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:30:12 AM BRT -03:00
Date Processed: 7/3/2018 12:57:22 PM BRT -03:00

Auto-Scaled Chromatogram

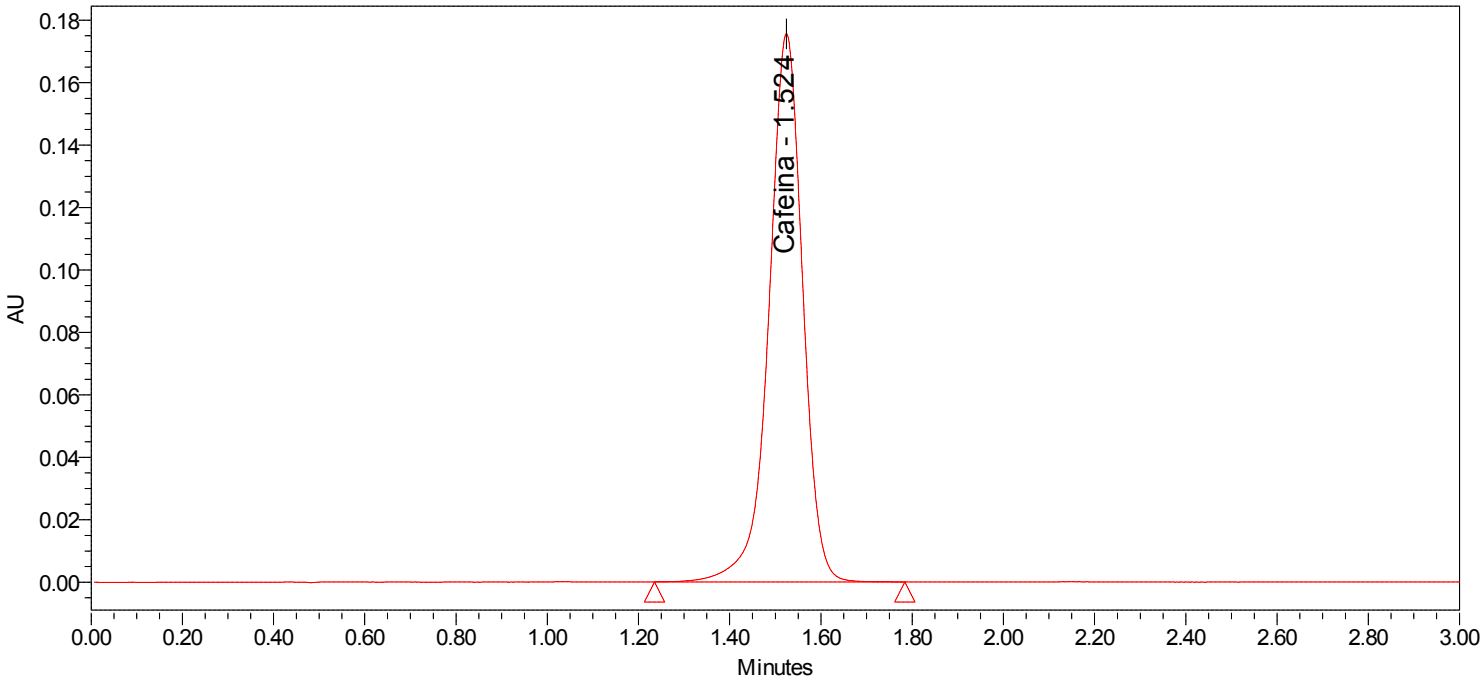

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.524	901489	175587		

SAMPLE INFORMATION

Sample Name:	PCIN05	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm

Date Acquired: 7/3/2018 11:33:55 AM BRT -03:00
Date Processed: 7/3/2018 12:58:13 PM BRT -03:00

Auto-Scaled Chromatogram

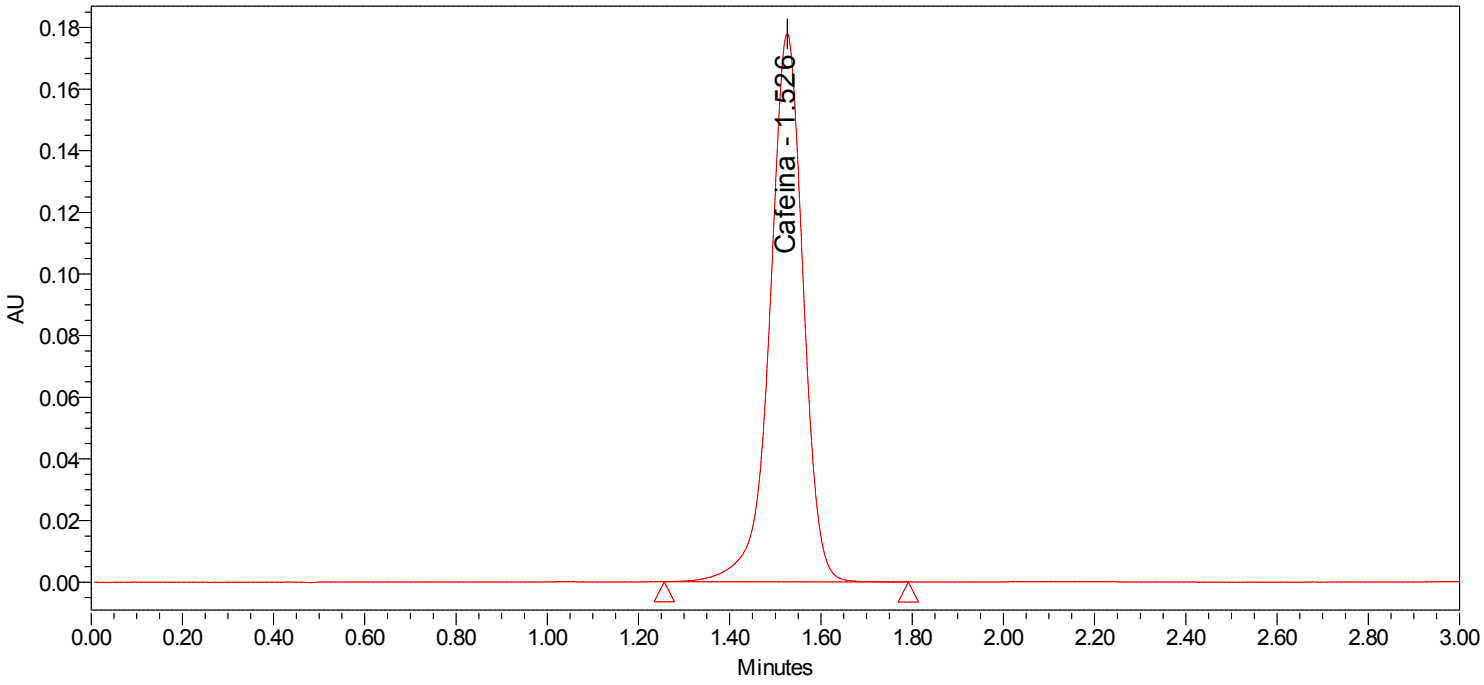

Peak Results


	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.526	900296	177879		

SAMPLE INFORMATION

Sample Name:	PCIN06	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	PCIN
Vial:	1:A,2	Acq. Method Set:	Qualificacao
Injection #:	1	Processing Method:	ID Cafeina
Injection Volume:	10.00 ul	Channel Name:	ACQUITY TUV ChA
Run Time:	3.0 Minutes	Proc. Chnl. Descr.:	ACQUITY TUV ChA 273nm


Date Acquired: 7/3/2018 11:37:36 AM BRT -03:00
Date Processed: 7/3/2018 1:00:05 PM BRT -03:00

Auto-Scaled Chromatogram

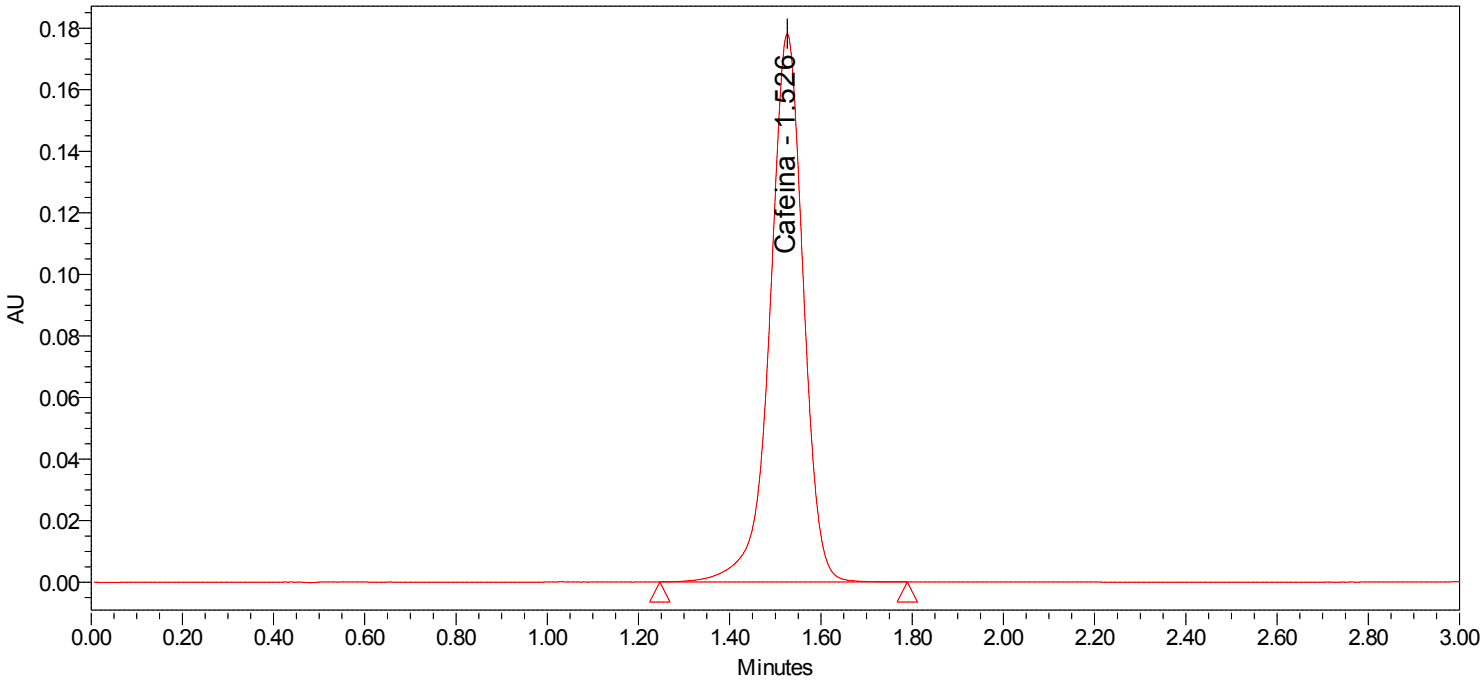

Peak Results

	Name	RT	Area	Height	Amount	Units
1	Cafeina	1.526	902896	178120		

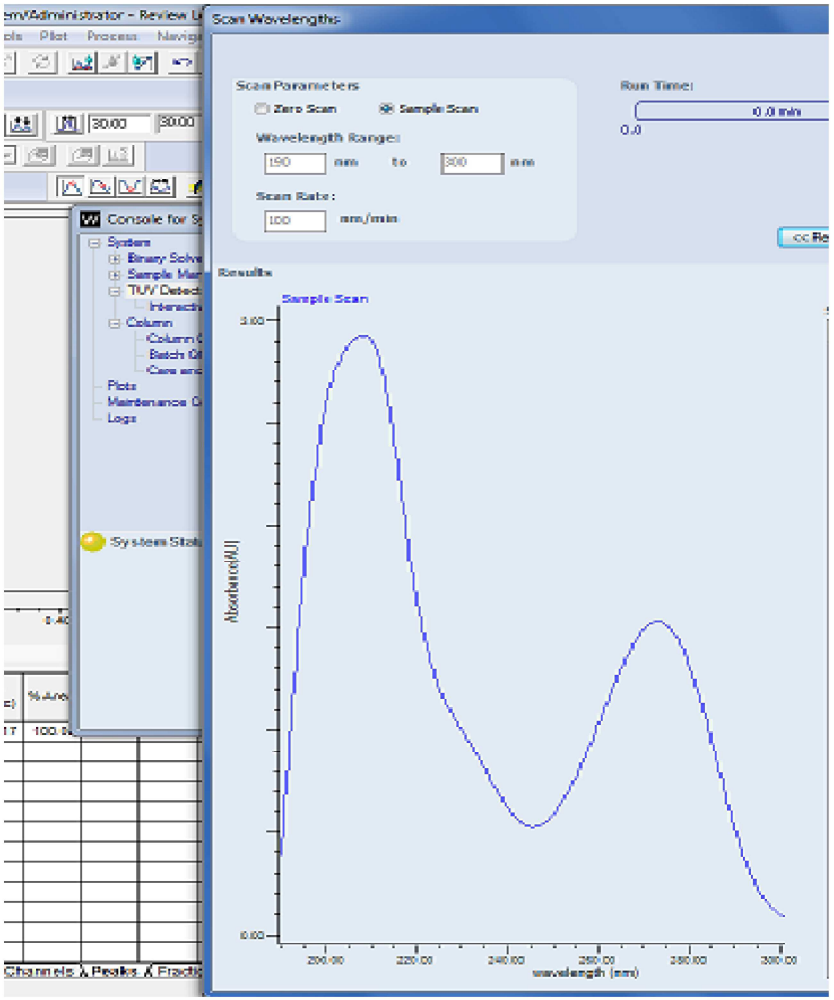
Scan Wavelengths
Scan Parameters
Zero Scan
Sample Scan
Wavelength Range:
190
nm
to
800
nm
Scan Rate:
100
nm/min
Run Time:
0.0 min
0.0
Results
Sample Scan
Absorbance(AU)
wavelength (nm)
Console for
System
Plots
Logs
Channels
Peaks
Fracti