
Chromatogram

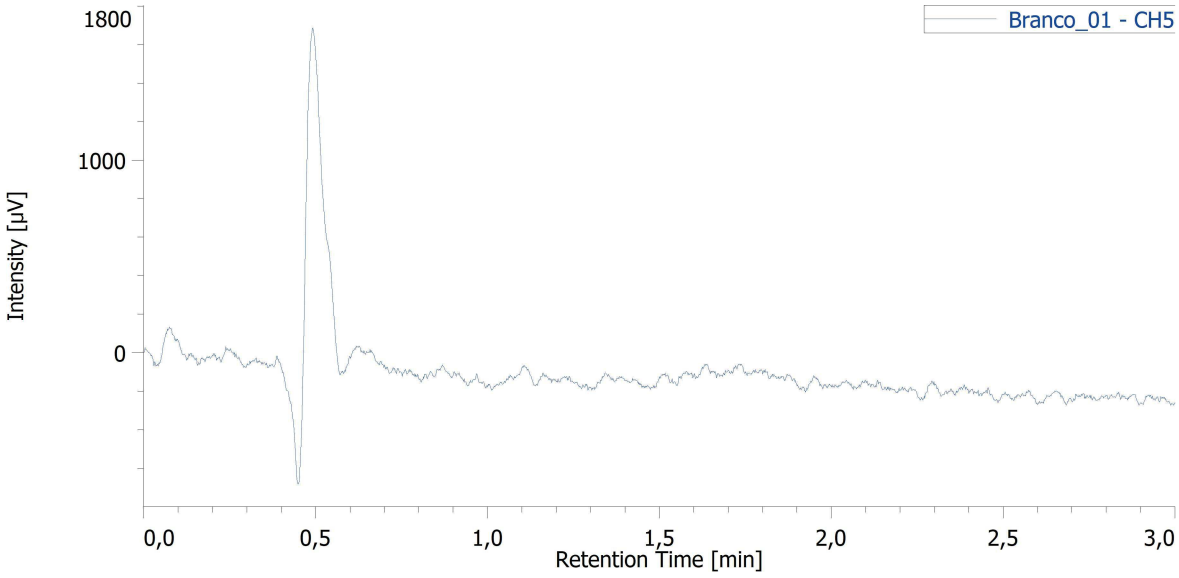


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 10:49:44
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 10:46:42
Volume	10,0 [µL]
Sample #	172
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

Creator
Reviewer
Approver

Chromatogram

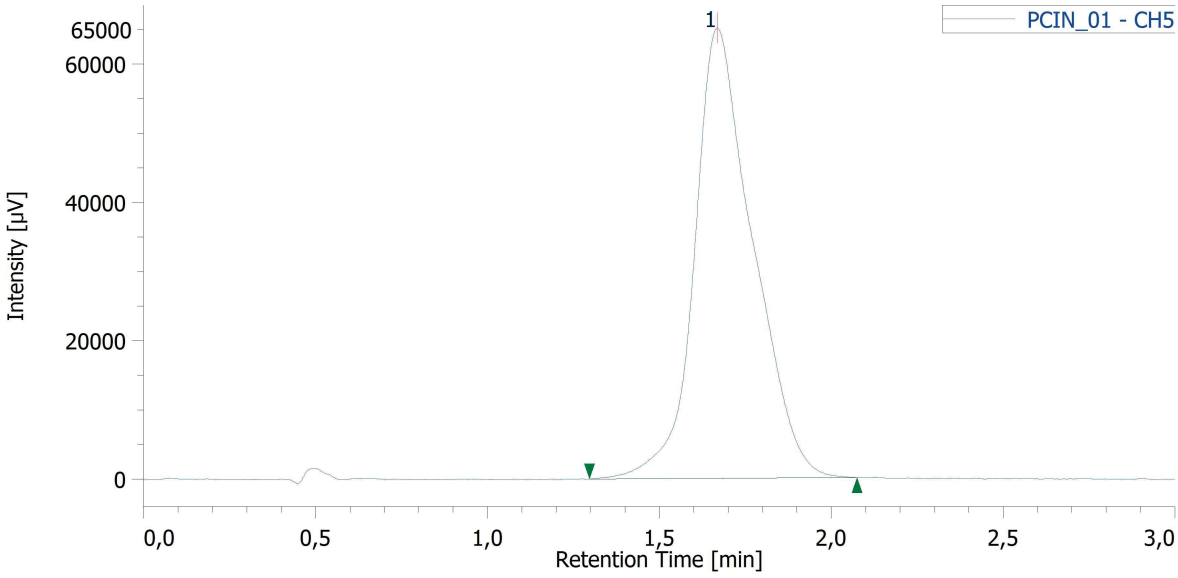

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 10:53:00
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 10:49:57
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,668	767696	65053	100,000	100,000	N/A	494	N/A	1,174	

Creator
Reviewer
Approver

Chromatogram

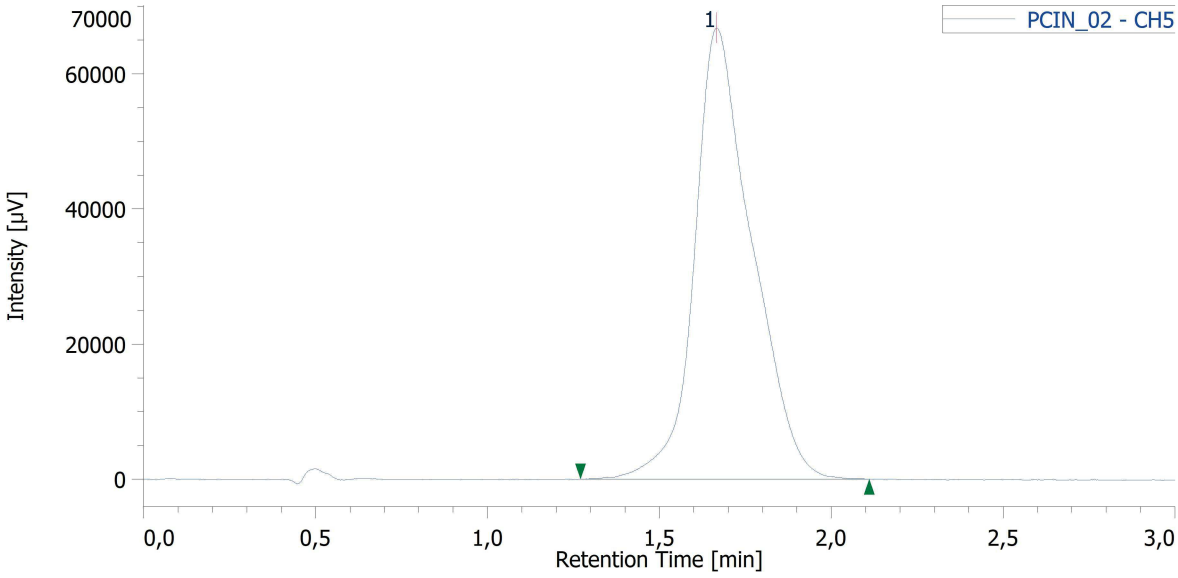

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 10:56:14
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 10:53:13
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,667	776343	66750	100,000	100,000	N/A	508	N/A	1,193	

Creator
Reviewer
Approver

Chromatogram

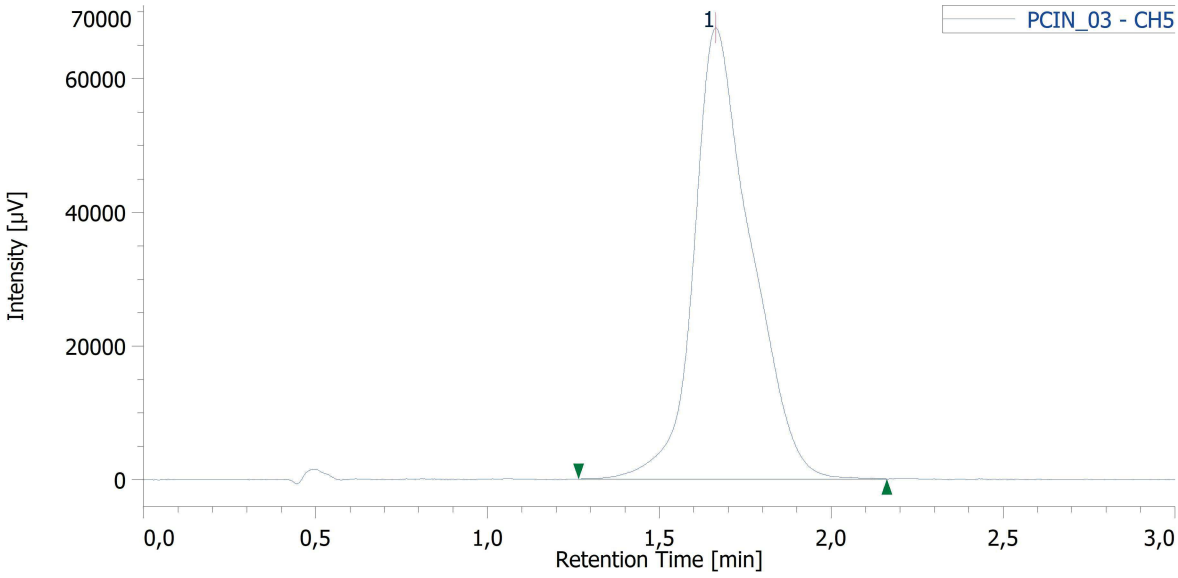

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 10:59:30
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 10:56:28
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,663	778796	67446	100,000	100,000	N/A	516	N/A	1,210	

Creator
Reviewer
Approver

Chromatogram

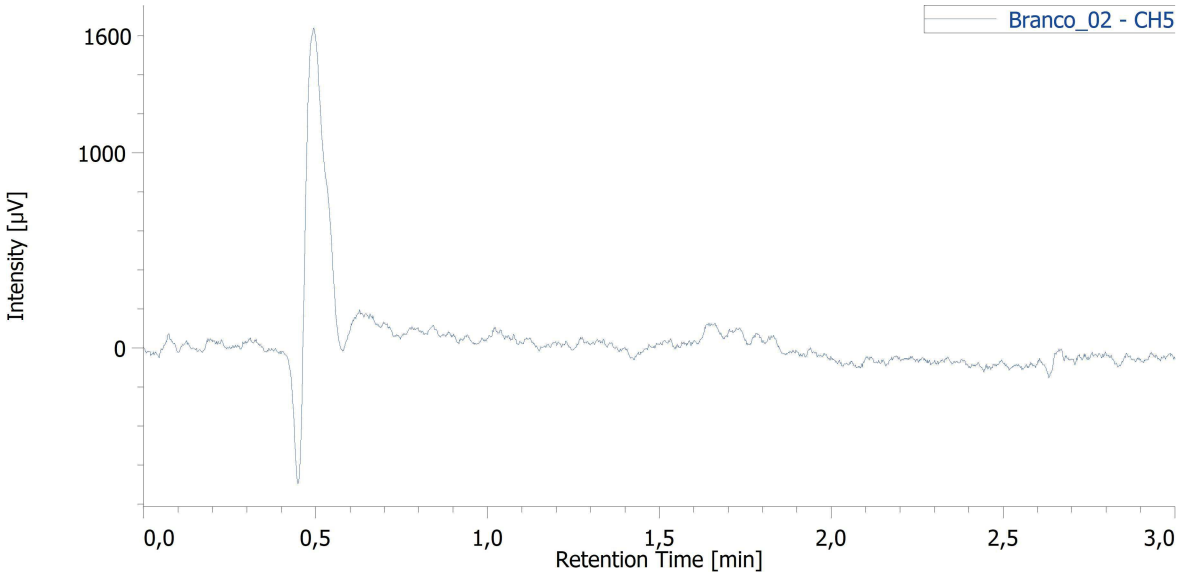


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 11:02:46
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 10:59:44
Volume	10,0 [µL]
Sample #	172
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

Creator
Reviewer
Approver

Chromatogram

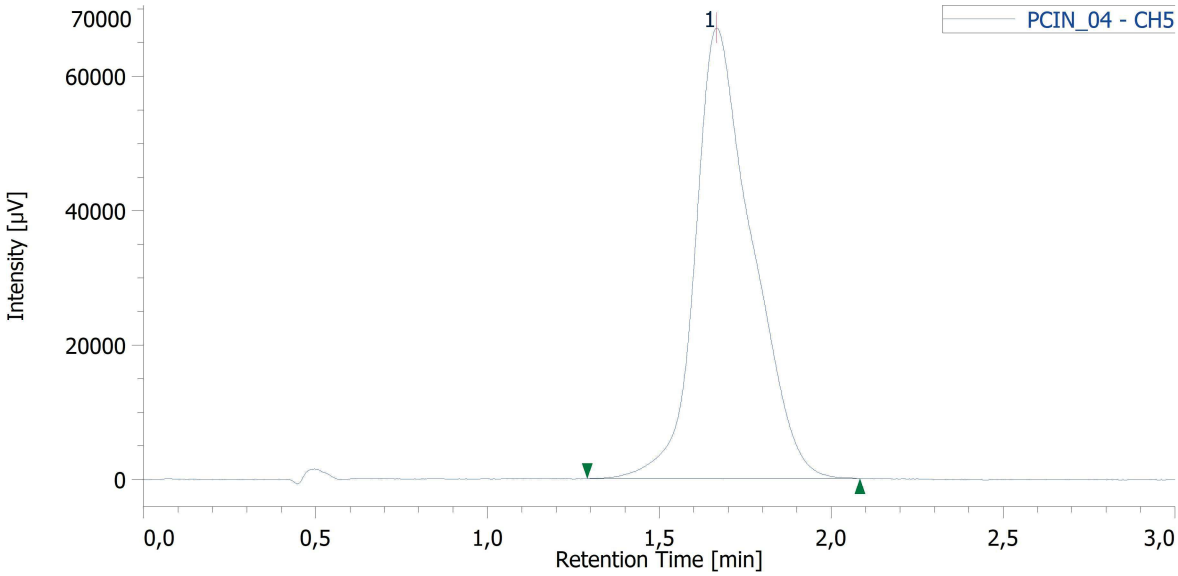

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 11:06:00
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 11:02:59
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,667	772777	67014	100,000	100,000	N/A	507	N/A	1,230	

Creator
Reviewer
Approver

Chromatogram

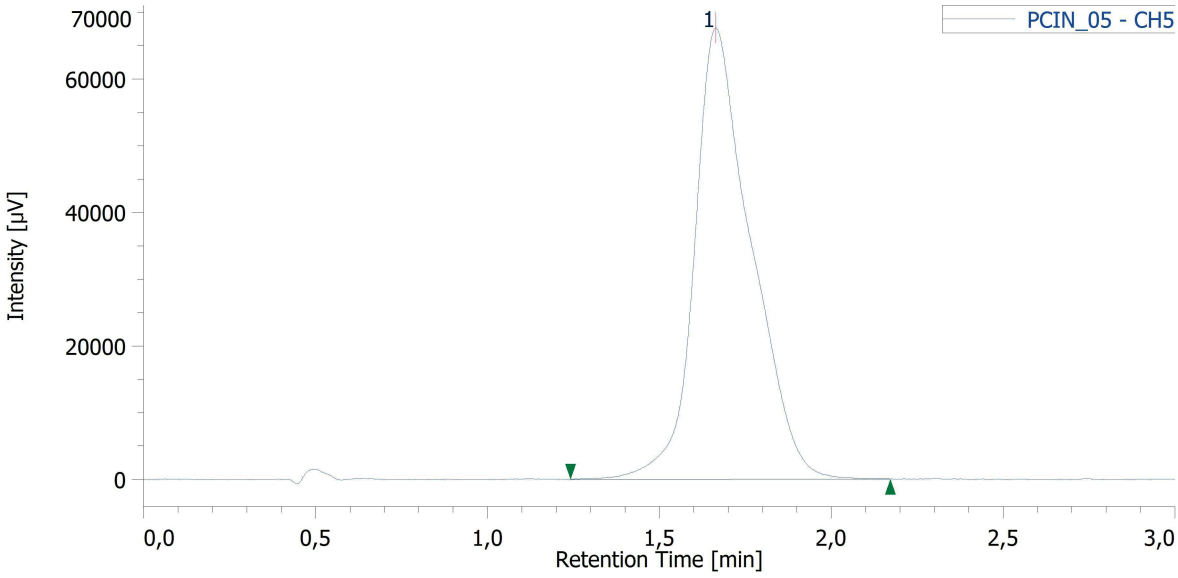

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 11:09:16
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 11:06:14
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,663	777120	67603	100,000	100,000	N/A	515	N/A	1,242	

Creator
Reviewer
Approver

Chromatogram

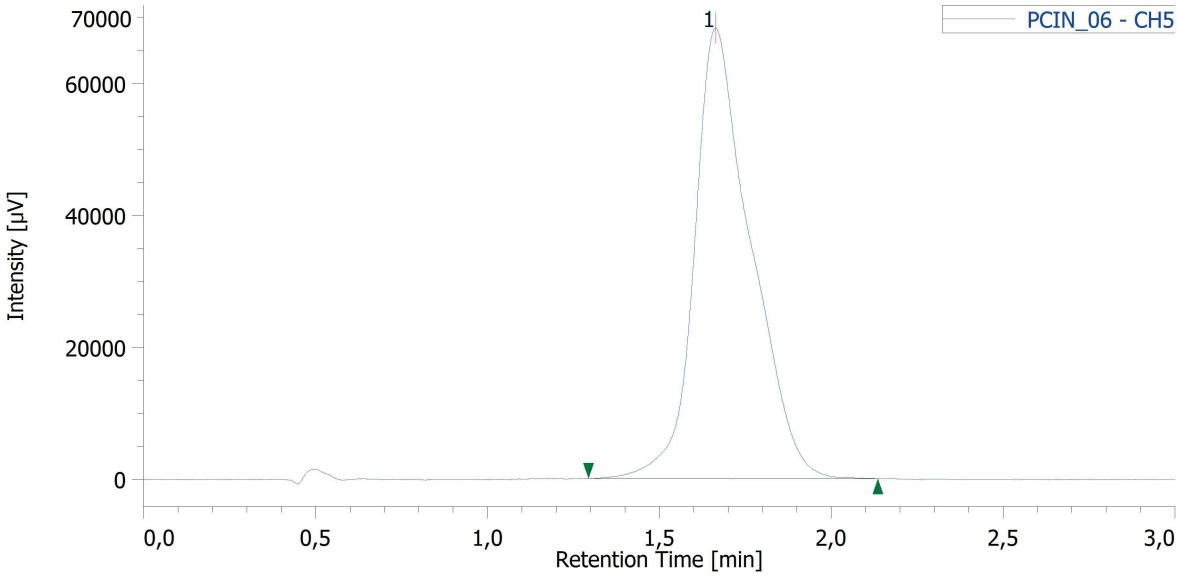

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 11:12:32
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 11:09:30
Volume	10,0 [µL]
Sample #	173
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,663	780464	68295	100,000	100,000	N/A	519	N/A	1,256	

Creator
Reviewer
Approver

Chromatogram

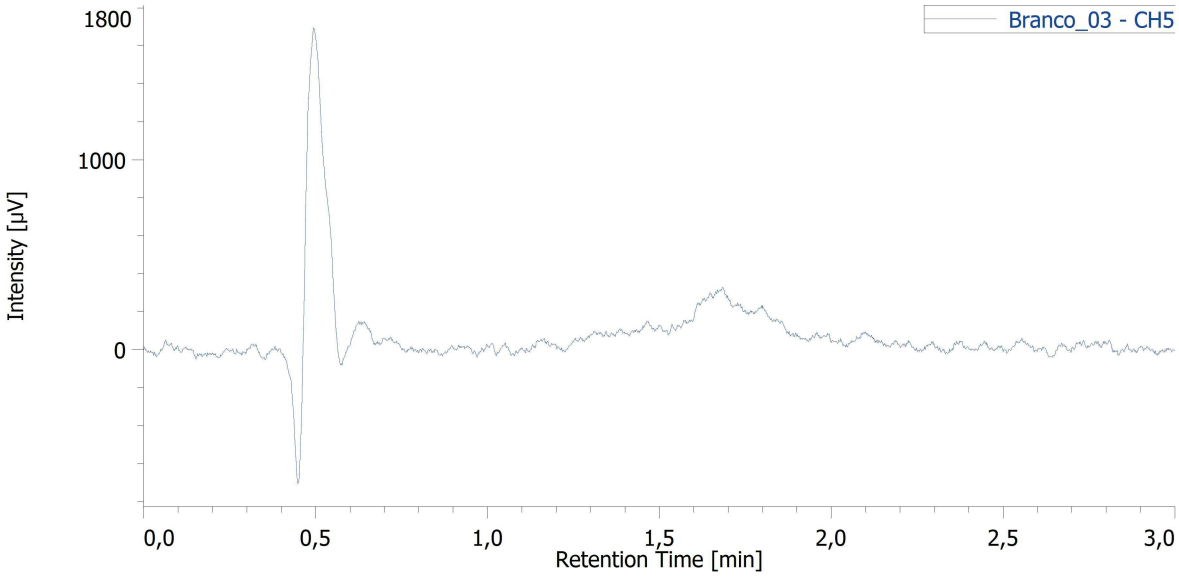


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 11:15:48
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 11:12:46
Volume	10,0 [µL]
Sample #	172
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

Creator
Reviewer
Approver

Chromatogram

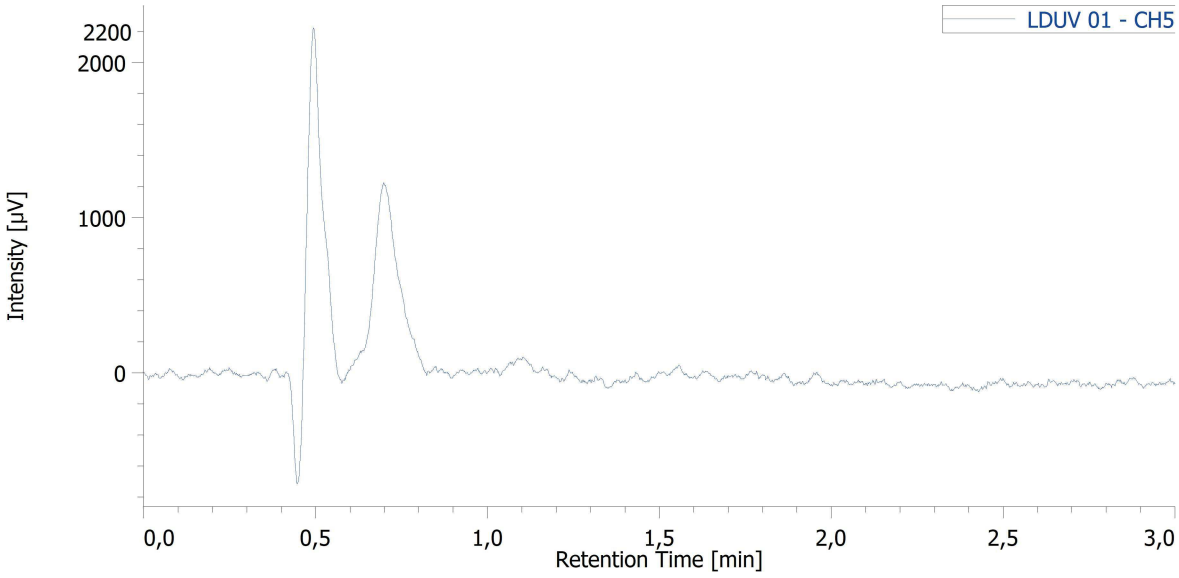


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 13:26:57
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 13:23:55
Volume	10,0 [µL]
Sample #	174
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

Creator
Reviewer
Approver

Chromatogram

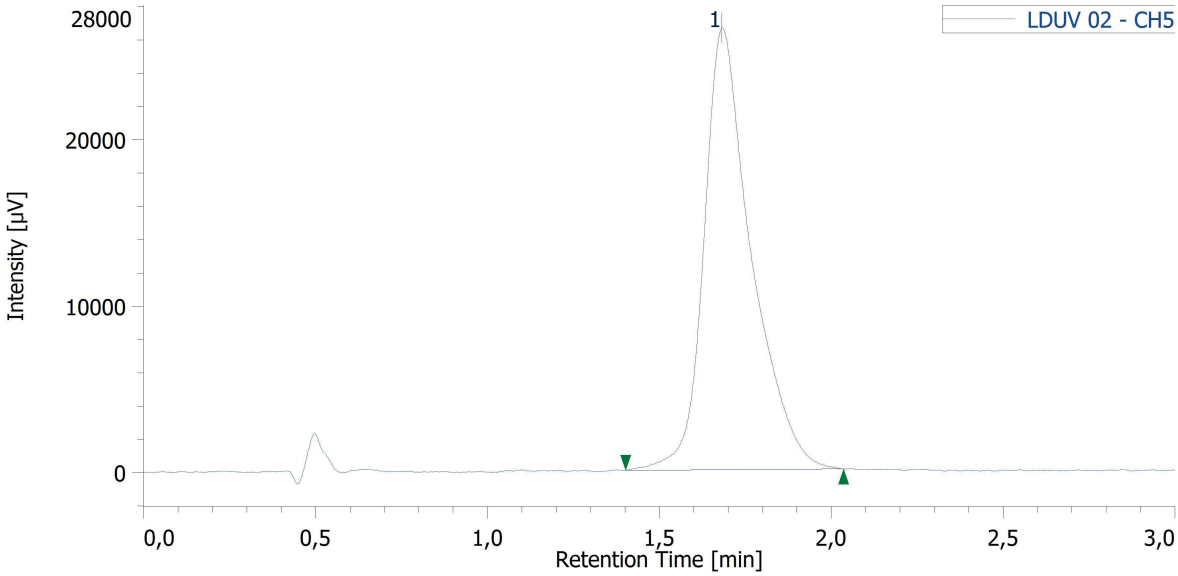

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 13:30:13
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 13:27:10
Volume	10,0 [µL]
Sample #	175
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,682	254700	26533	100,000	100,000	N/A	846	N/A	1,401	

Creator
Reviewer
Approver

Chromatogram

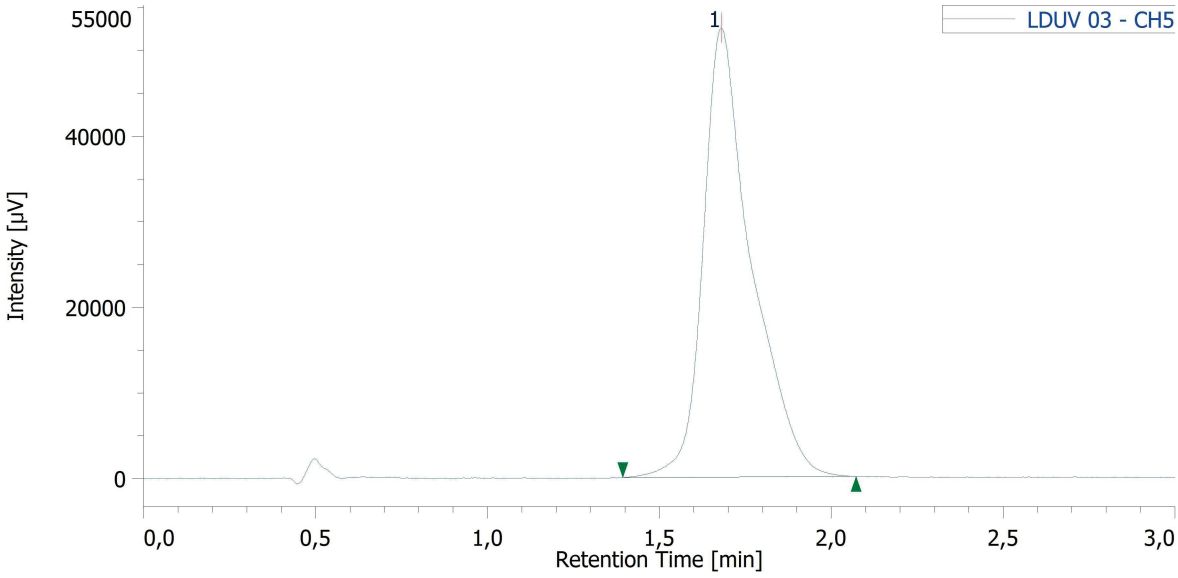

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 13:33:26
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 13:30:25
Volume	10,0 [µL]
Sample #	176
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,680	512185	52467	100,000	100,000	N/A	859	N/A	1,436	

Creator
Reviewer
Approver

Chromatogram

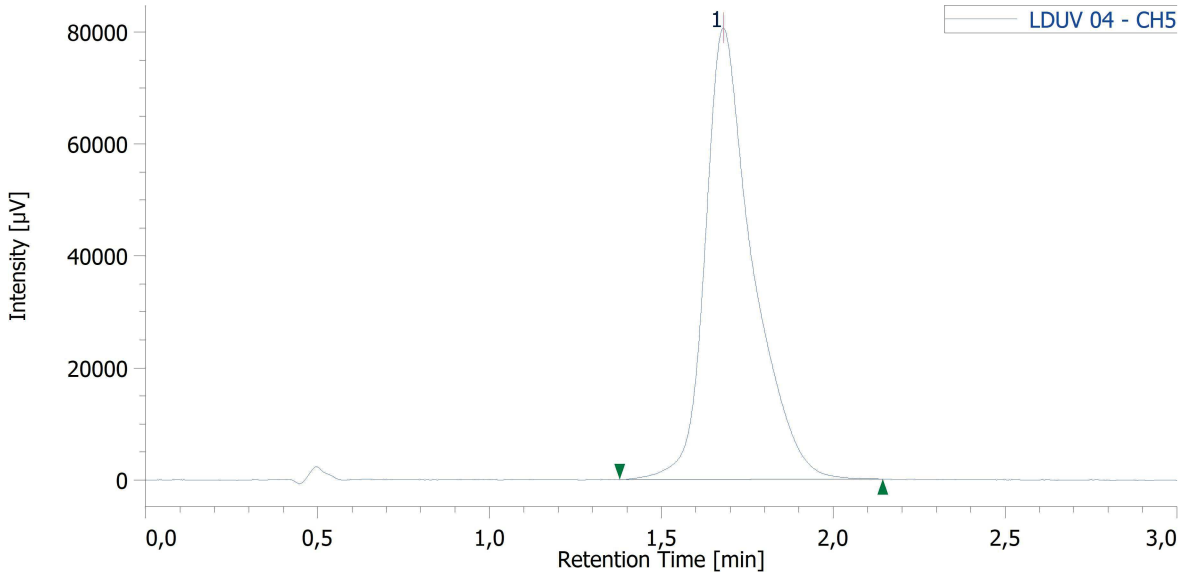

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 13:36:42
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 13:33:41
Volume	10,0 [µL]
Sample #	177
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,680	773020	80578	100,000	100,000	N/A	863	N/A	1,416	

Creator
Reviewer
Approver

Chromatogram

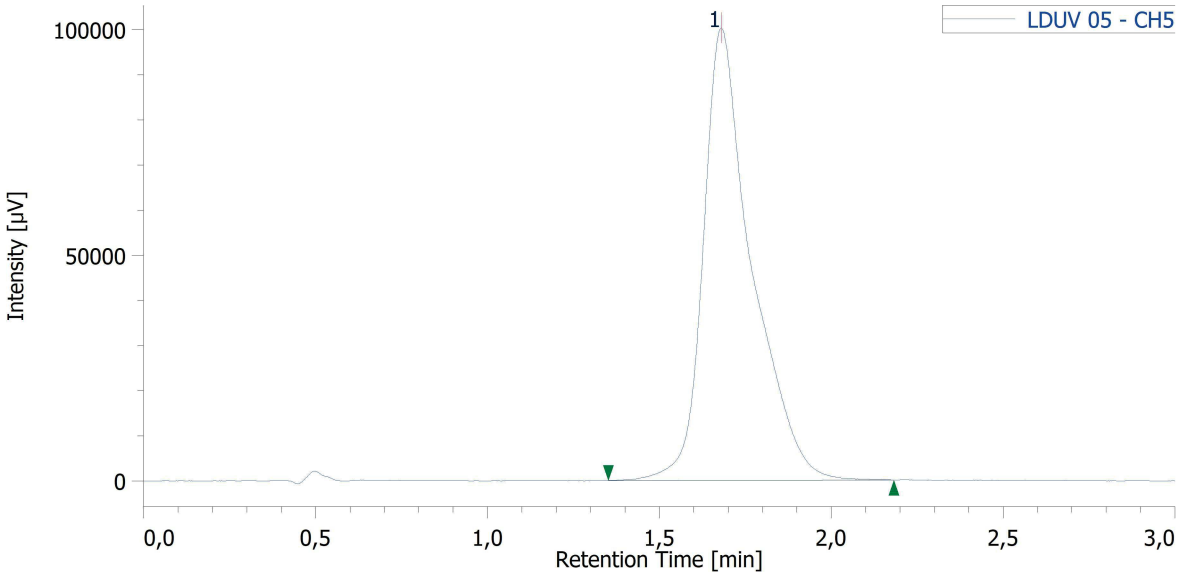

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 13:39:58
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 13:36:56
Volume	10,0 [µL]
Sample #	178
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,680	983344	100243	100,000	100,000	N/A	861	N/A	1,455	

Creator
Reviewer
Approver

Chromatogram

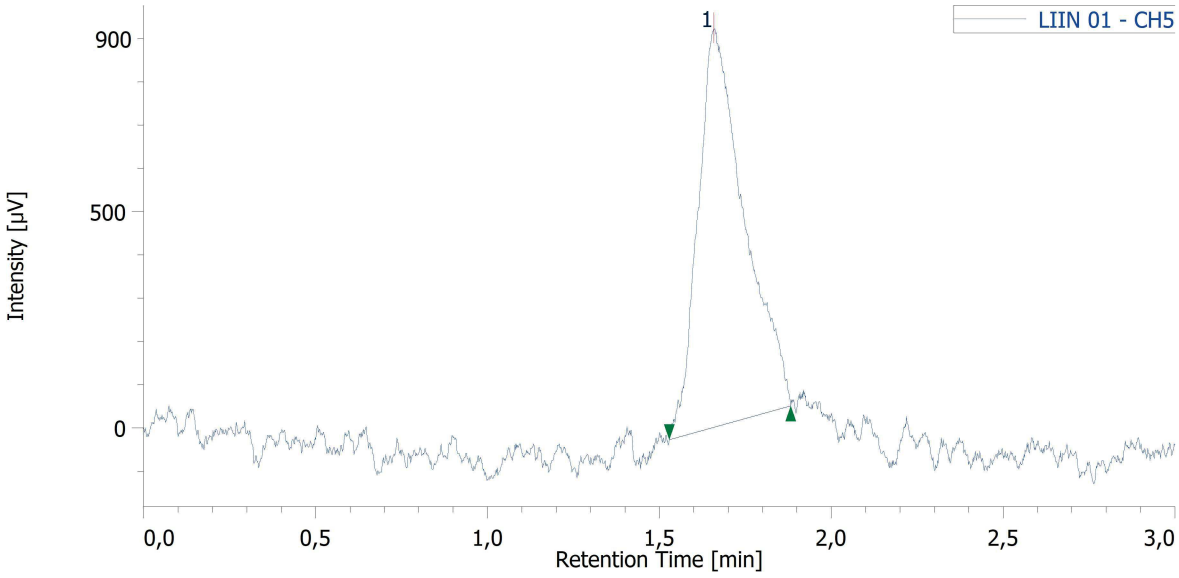

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 12:19:11
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 12:16:10
Volume	0,1 [µL]
Sample #	179
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,658	8632	922	100,000	100,000	N/A	779	N/A	1,456	

Creator
Reviewer
Approver

Chromatogram

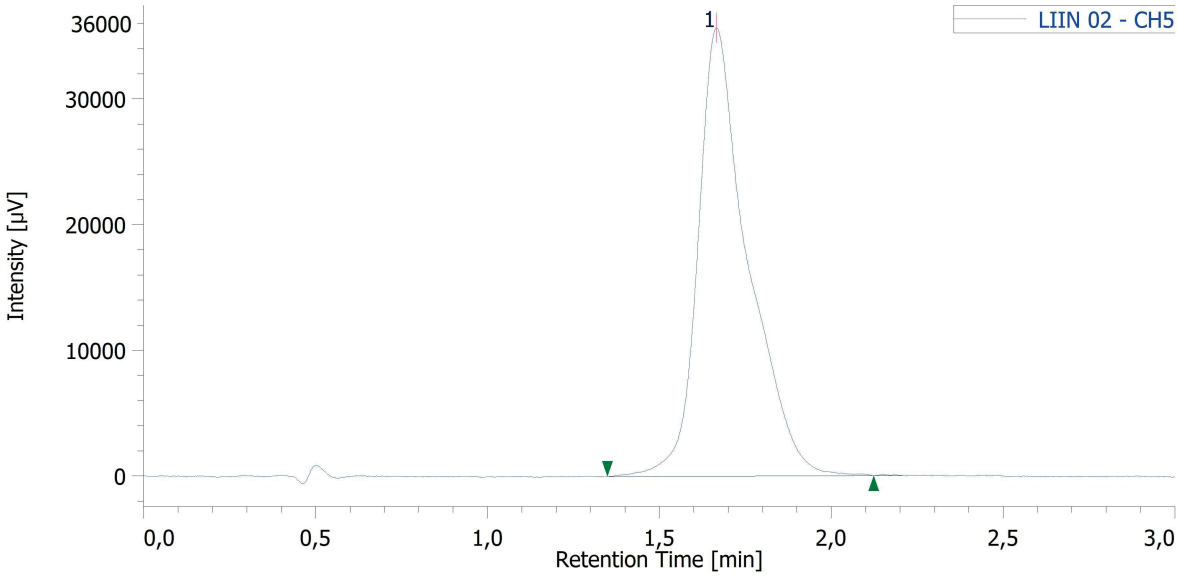

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 12:22:23
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 12:19:22
Volume	5,0 [µL]
Sample #	179
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,665	360802	35634	100,000	100,000	N/A	784	N/A	1,413	

Creator
Reviewer
Approver

Chromatogram

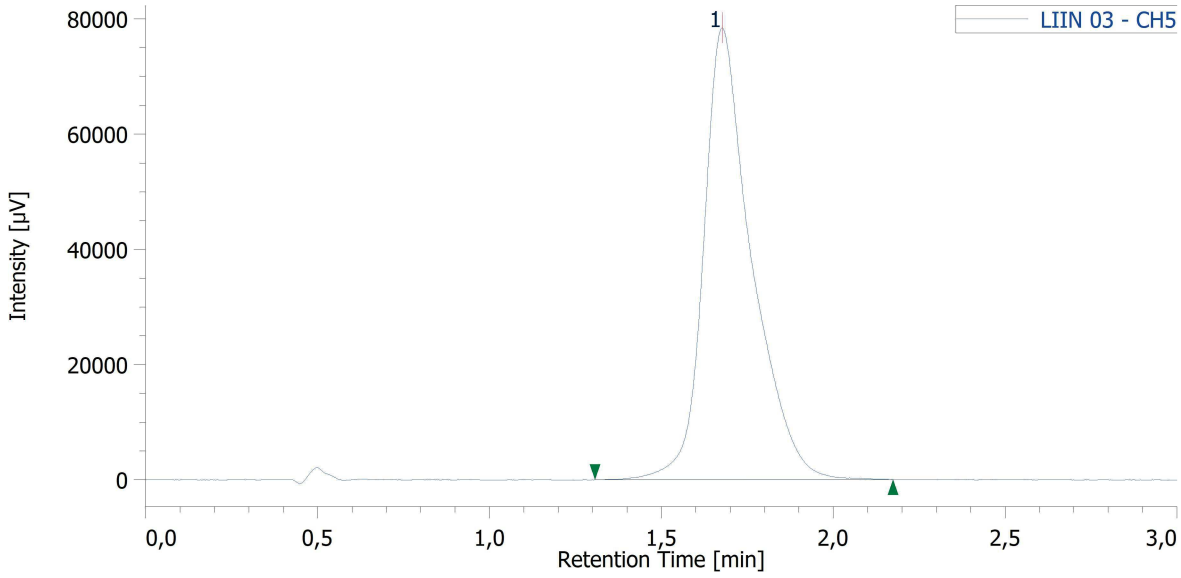

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 12:25:39
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 12:22:37
Volume	10,0 [µL]
Sample #	179
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,677	763247	78366	100,000	100,000	N/A	816	N/A	1,360	

Creator
Reviewer
Approver

Chromatogram

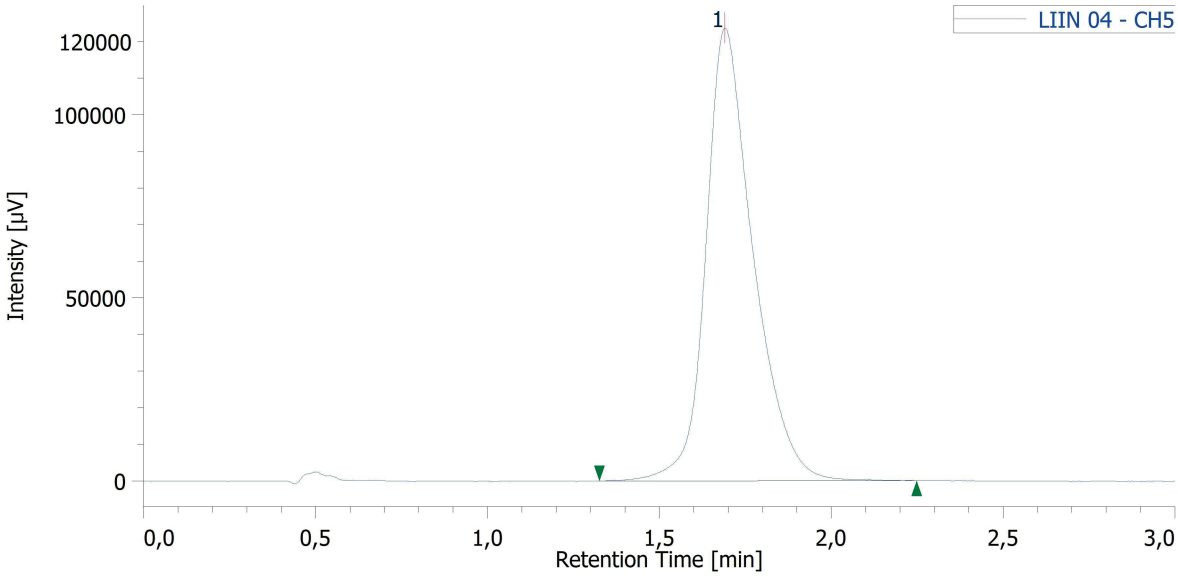

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 12:29:09
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 12:26:07
Volume	15,0 [µL]
Sample #	179
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,690	1184783	123590	100,000	100,000	N/A	817	N/A	1,296	

Creator
Reviewer
Approver

Chromatogram

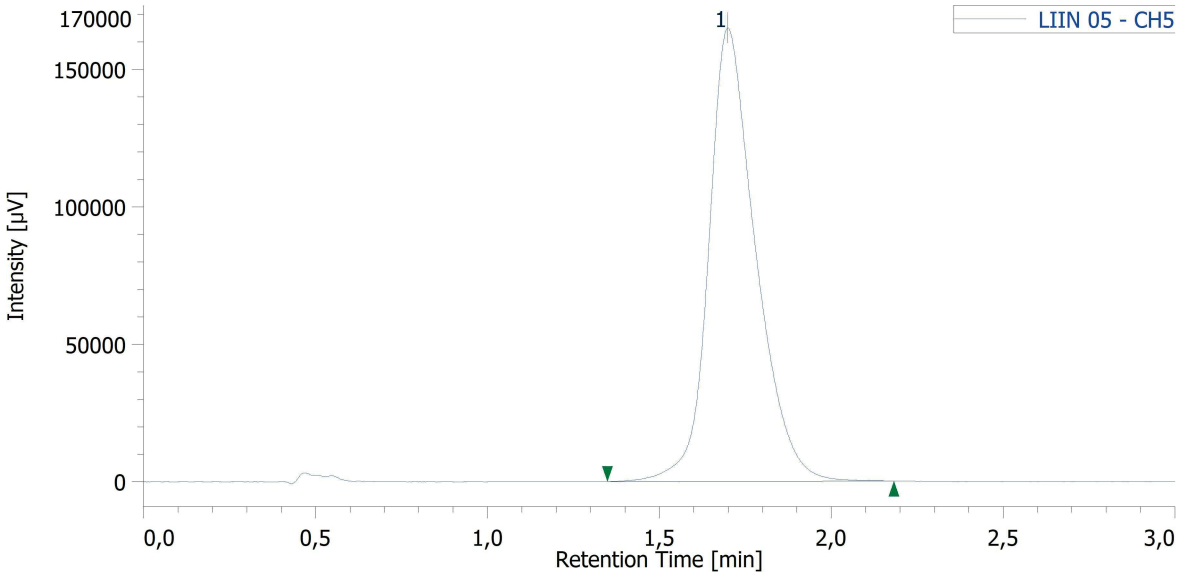

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 12:32:55
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 12:29:52
Volume	20,0 [µL]
Sample #	179
Project Name	Qualificação Operacional
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak Method Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,698	1565316	164883	100,000	100,000	N/A	822	N/A	1,260	

Creator
Reviewer
Approver

Chromatogram

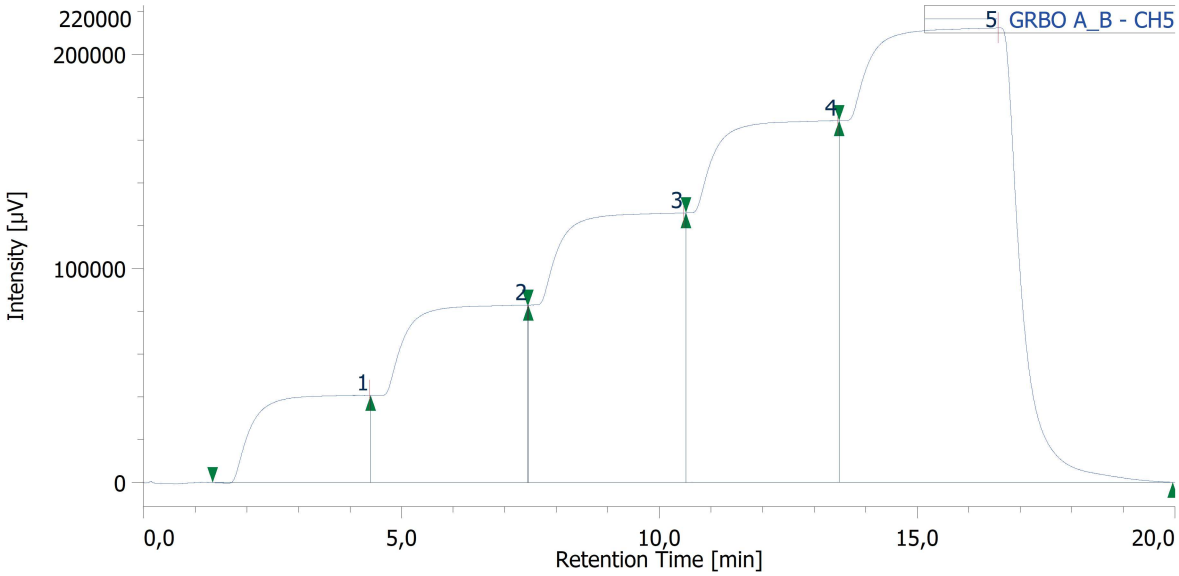

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 14:58:02
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 14:38:00
Volume	0,1 [µL]
Sample #	172
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRBO A_B-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,383	5672986	40710	5,666	6,457	N/A	N/A	N/A	N/A	
2	Unknown	5	7,450	82878	82885	0,083	13,146	N/A	N/A	N/A	N/A	
3	Unknown	5	10,470	21512813	125829	21,487	19,957	N/A	N/A	N/A	N/A	
4	Unknown	5	13,460	28669147	168931	28,635	26,793	N/A	N/A	N/A	N/A	
5	Unknown	5	16,563	44181435	212141	44,129	33,647	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

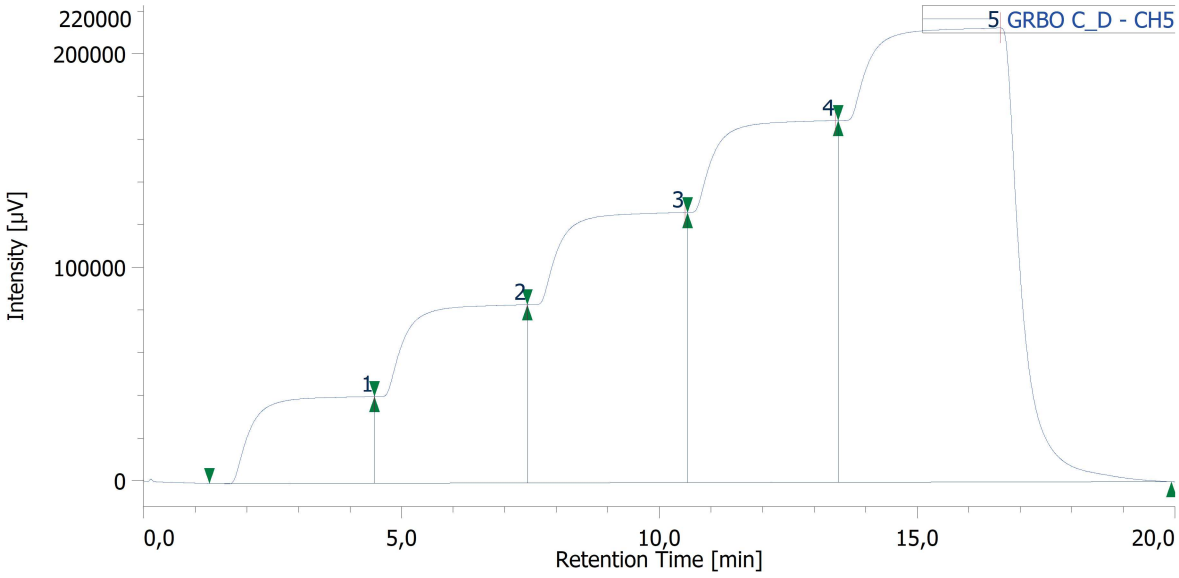

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2022 15:18:14
Description	
HPLC System Name	HPL19
Injection Date	04/05/2022 14:58:12
Volume	0,1 [µL]
Sample #	172
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRBO C_D-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,467	5820642	40514	5,110	6,405	N/A	N/A	N/A	N/A	
2	Unknown	5	7,433	13324059	83447	11,696	13,193	N/A	N/A	N/A	N/A	
3	Unknown	5	10,497	21956529	126510	19,274	20,001	N/A	N/A	N/A	N/A	
4	Unknown	5	13,407	28347003	169414	24,884	26,784	N/A	N/A	N/A	N/A	
5	Unknown	5	16,610	44466822	212634	39,035	33,617	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver