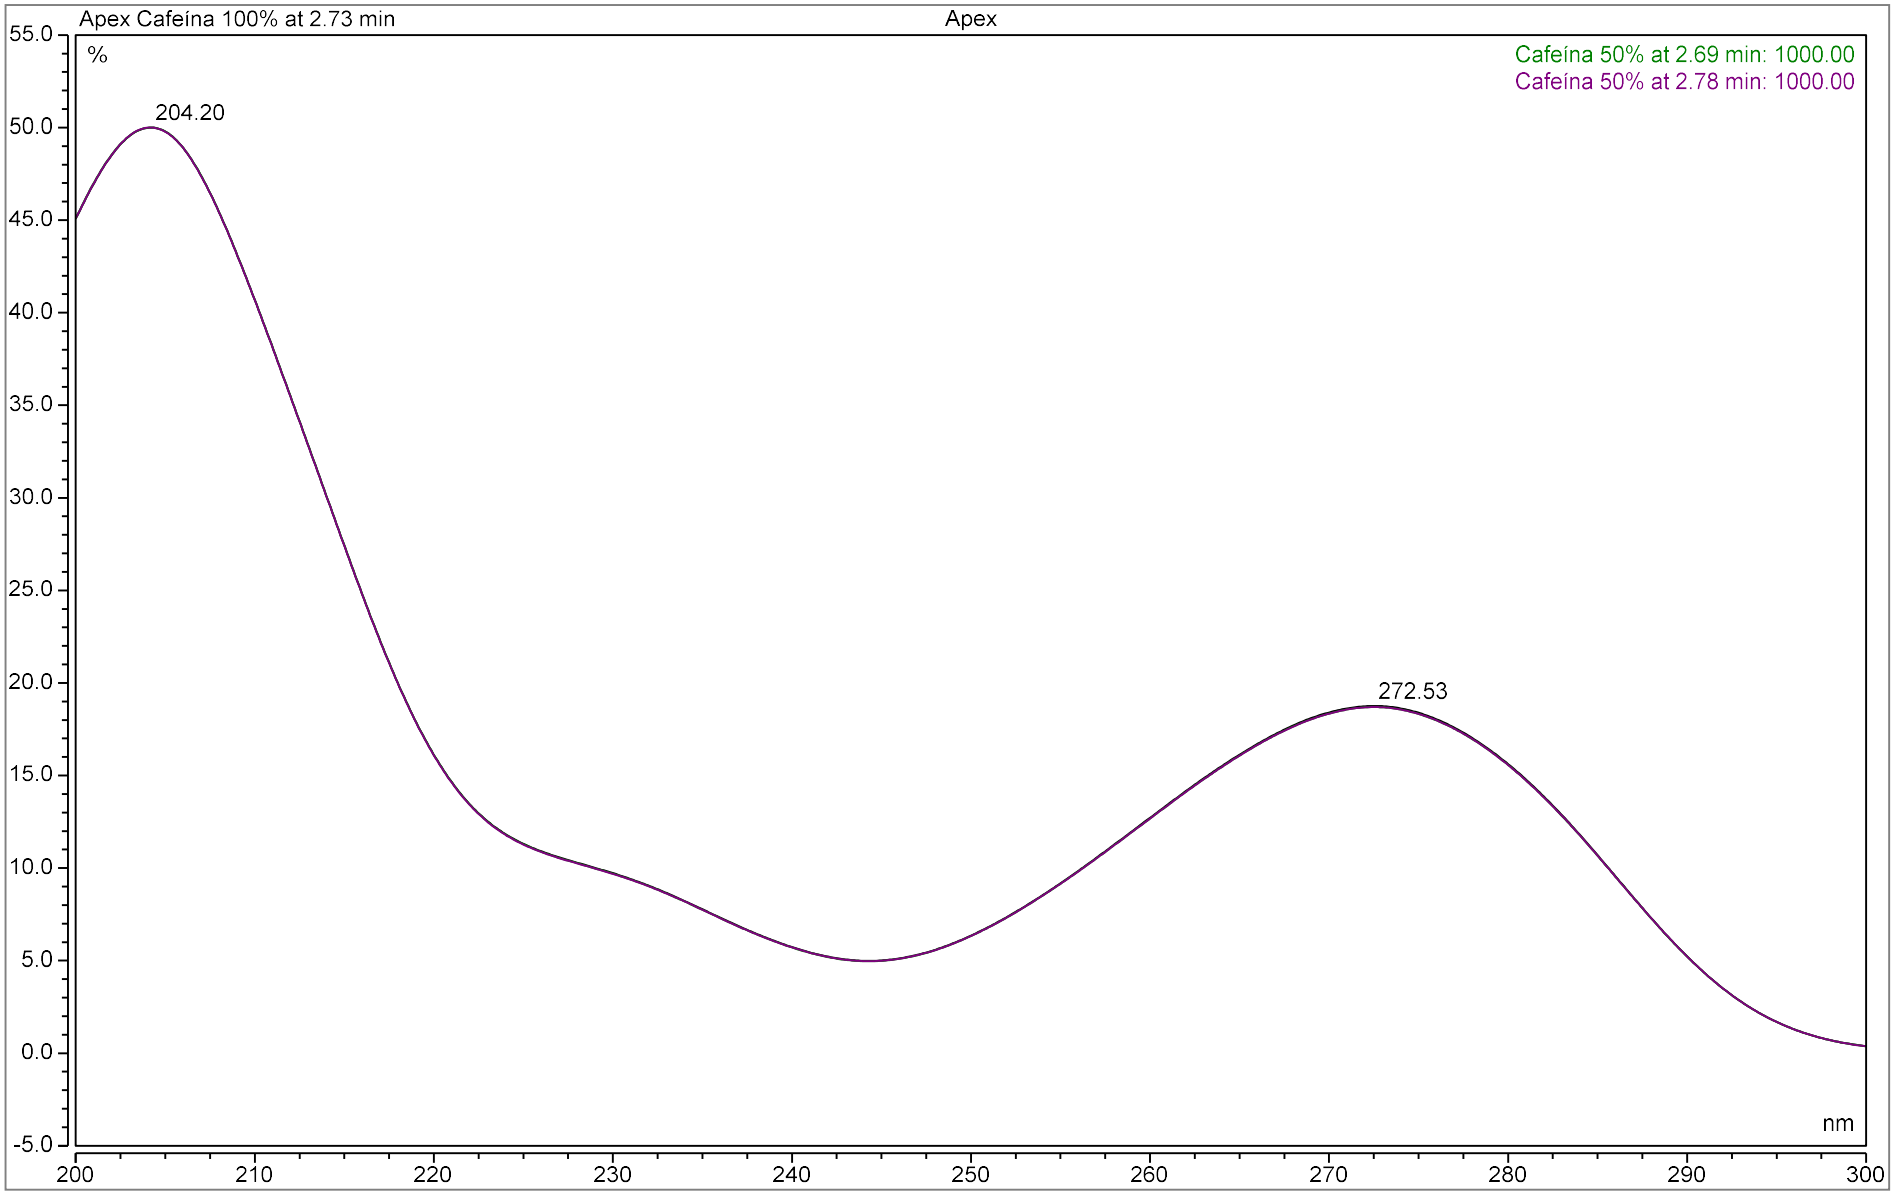
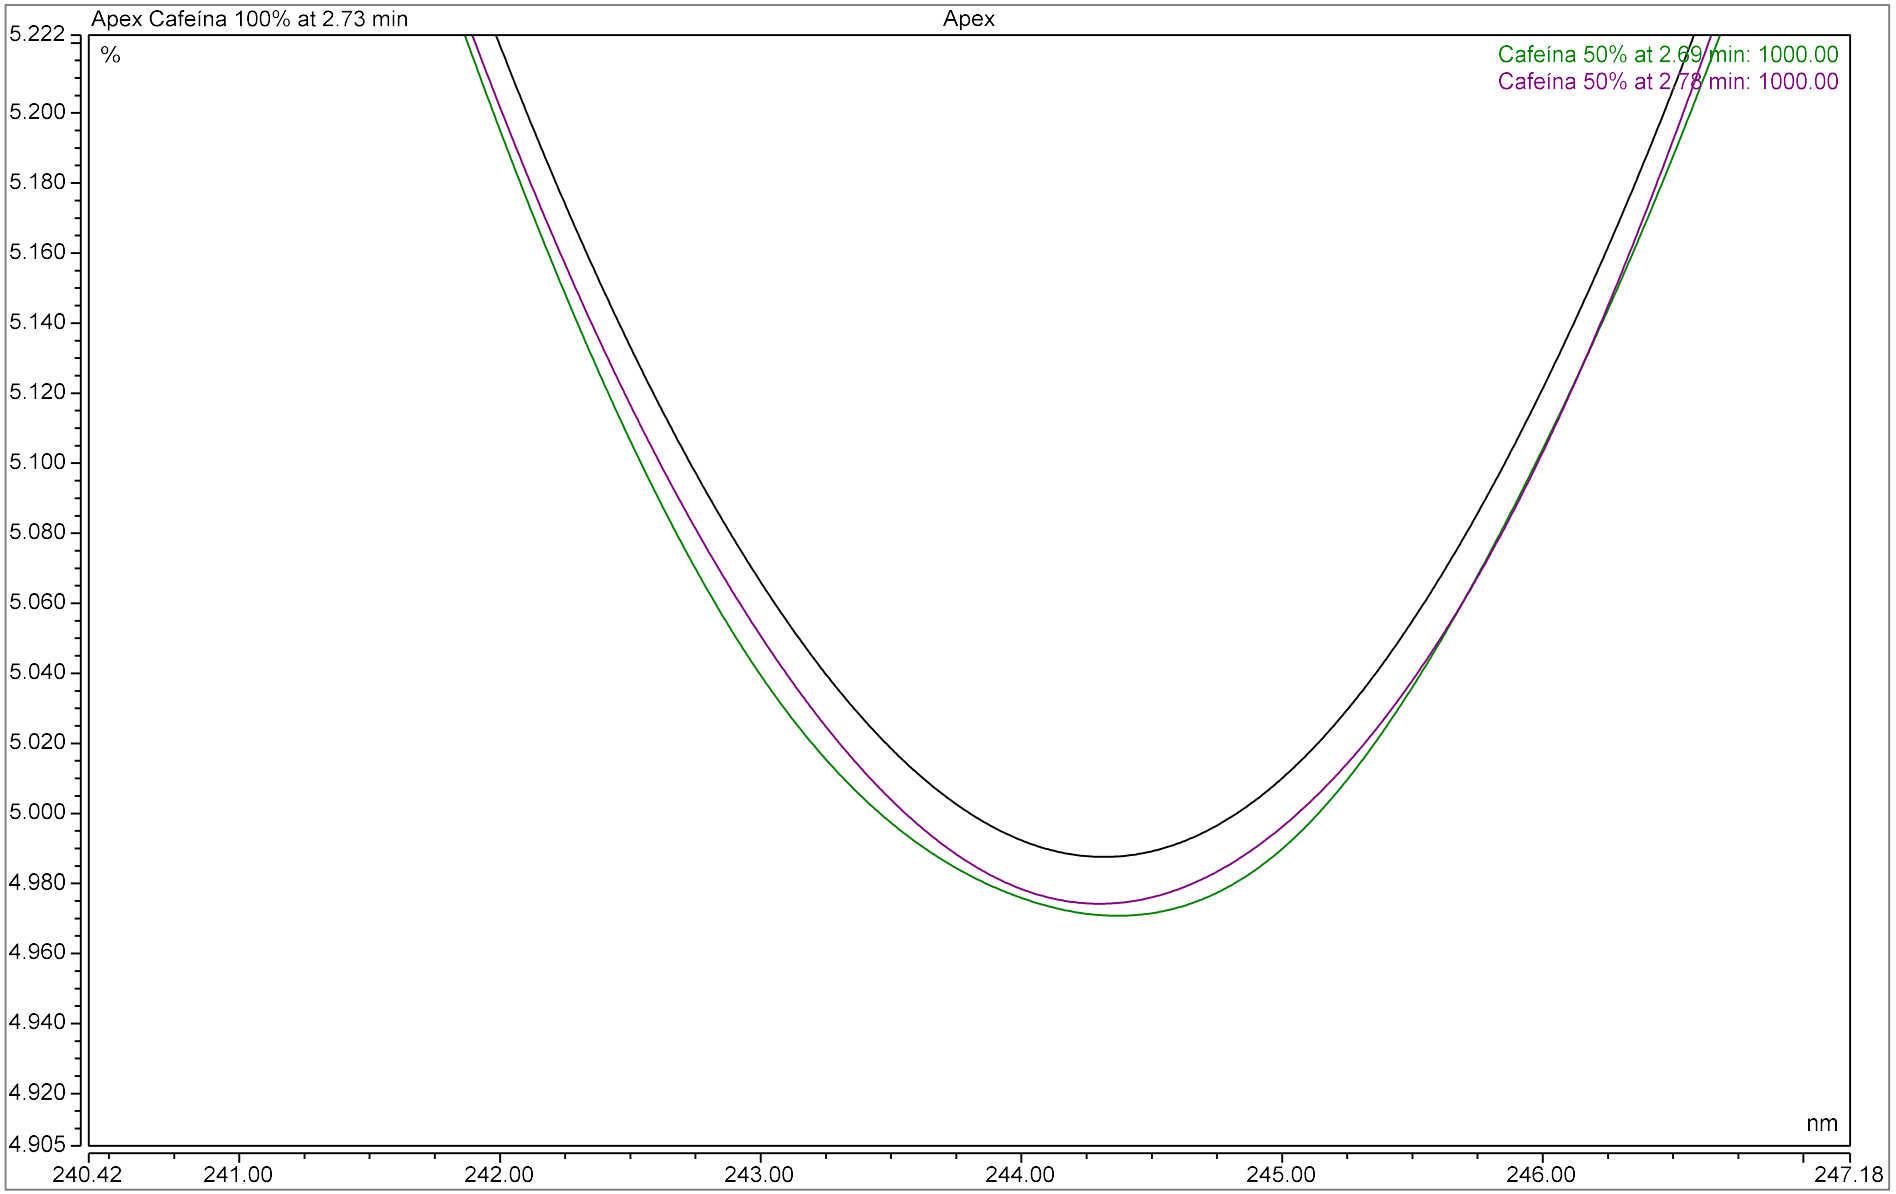

Apex Cafeína 100% at 2.73 min
Apex
%
Cafeína 50% at 2.69 min: 1000.00
Cafeína 50% at 2.78 min: 1000.00
204.20
272.53
nm
55.0
50.0
45.0
40.0
35.0
30.0
25.0
20.0
15.0
10.0
5.0
0.0
-5.0
200
210
220
230
240
250
260
270
280
290
300



Apex Cafeína 100% at 2.73 min
Apex
%
Cafeína 50% at 2.69 min: 1000.00
Cafeína 50% at 2.78 min: 1000.00
5.222
5.200
5.180
5.160
5.140
5.120
5.100
5.080
5.060
5.040
5.020
5.000
4.980
4.960
4.940
4.920
4.905
nm
240.42
241.00
242.00
243.00
244.00
245.00
246.00
247.18

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20.00**
Vial Number:	**B:B1**	*Injection Volume:*	**20.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB 04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 15:16**	*Sample Weight:*	**1.0000**

Chromatogram

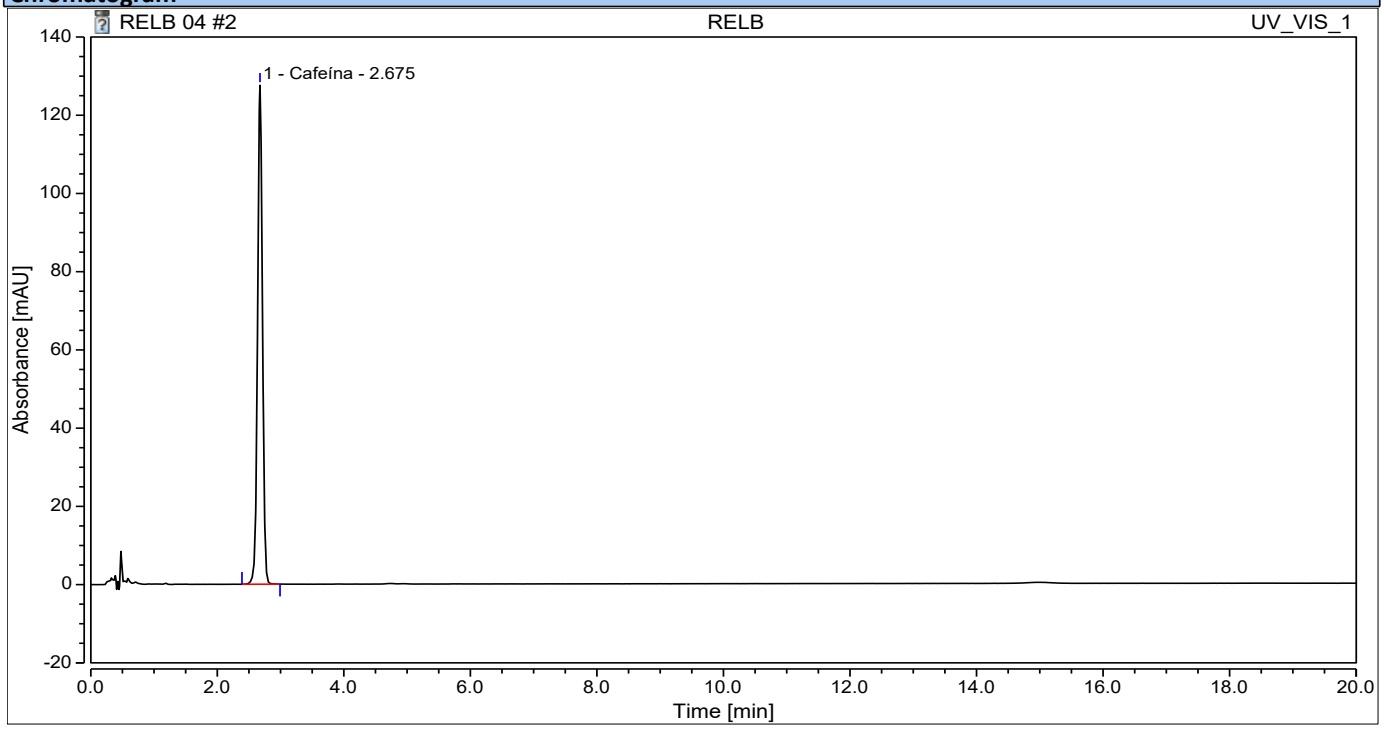

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.675	11.3950	127.564	100.00	100.00	n.a.
Total:			**11.395**	**127.564**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20.00**
Vial Number:	**B:B1**	*Injection Volume:*	**20.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB 04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 15:16**	*Sample Weight:*	**1.0000**

Chromatogram

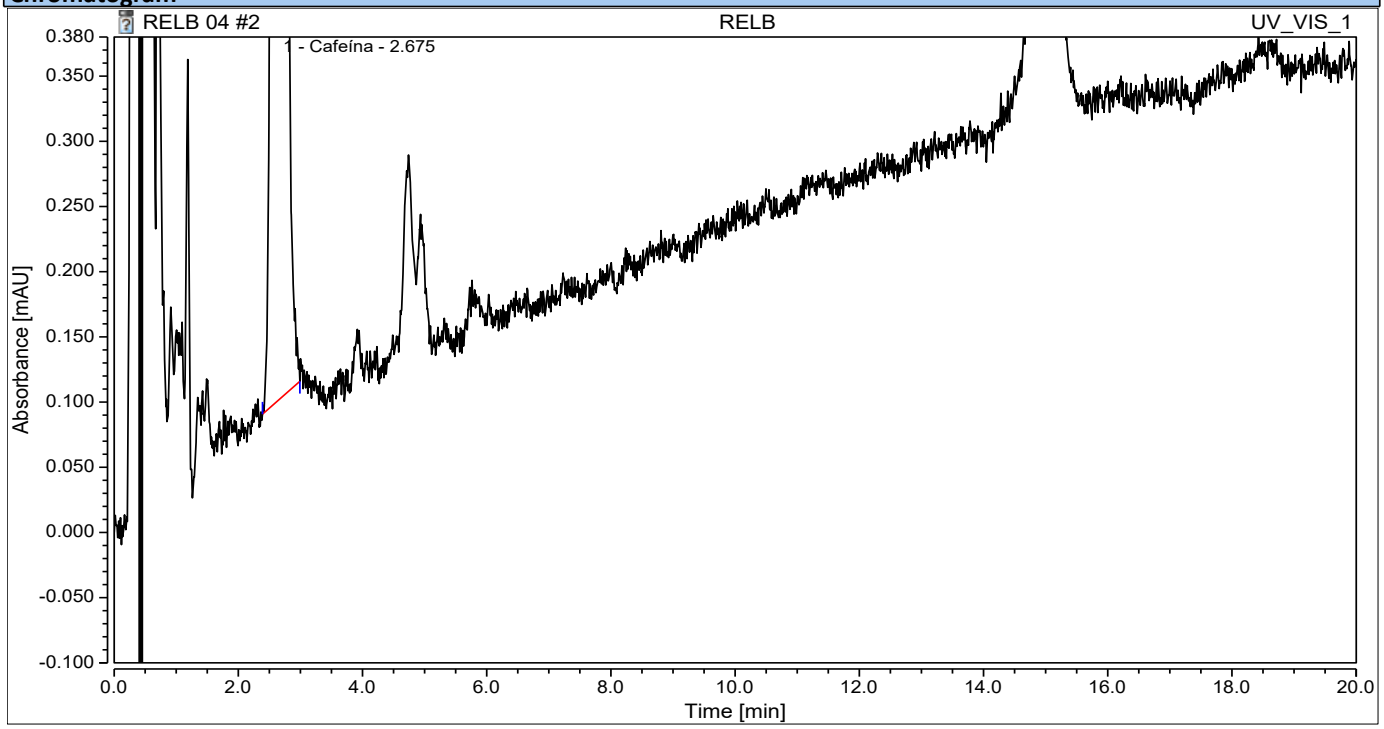

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.675	11.3950	127.564	100.00	100.00	n.a.
Total:			**11.395**	**127.564**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20.00**
Vial Number:	**B:B1**	*Injection Volume:*	**20.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB 04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 15:16**	*Sample Weight:*	**1.0000**

Chromatogram

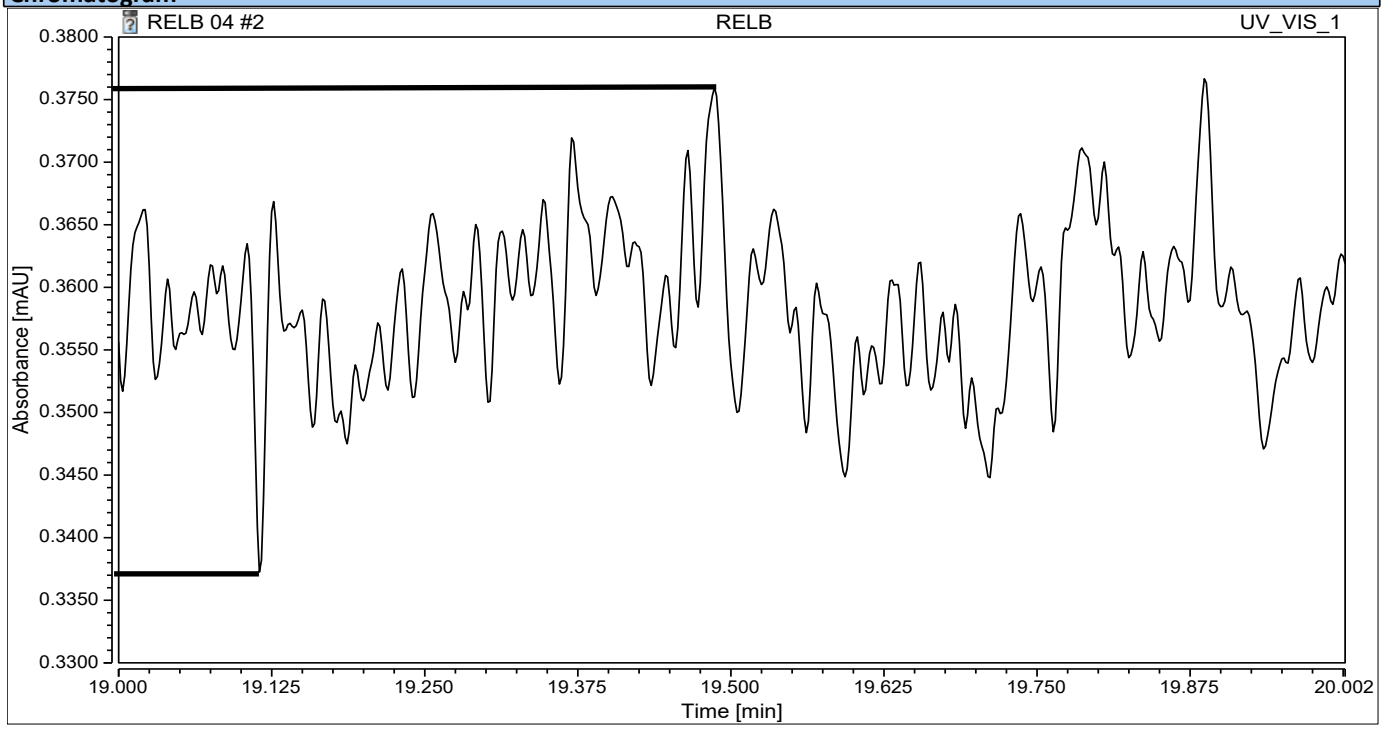

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.675	11.3950	127.564	100.00	100.00	n.a.
Total:			**11.395**	**127.564**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**EDUV**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:06**	*Sample Weight:*	**1.0000**

Chromatogram

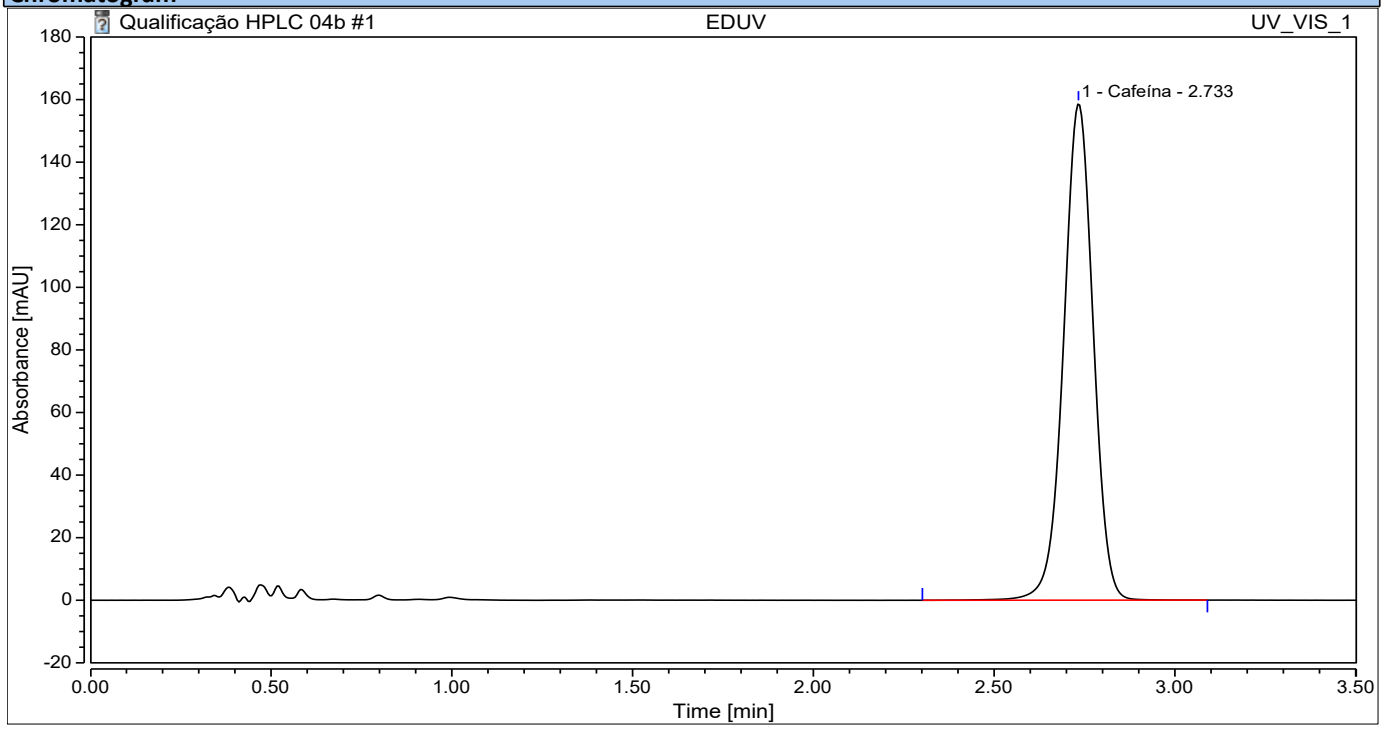

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.733	15.0567	158.759	100.00	100.00	n.a.
Total:			**15.057**	**158.759**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**3.50**
Vial Number:	**B:A2**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:10**	*Sample Weight:*	**1.0000**

Chromatogram

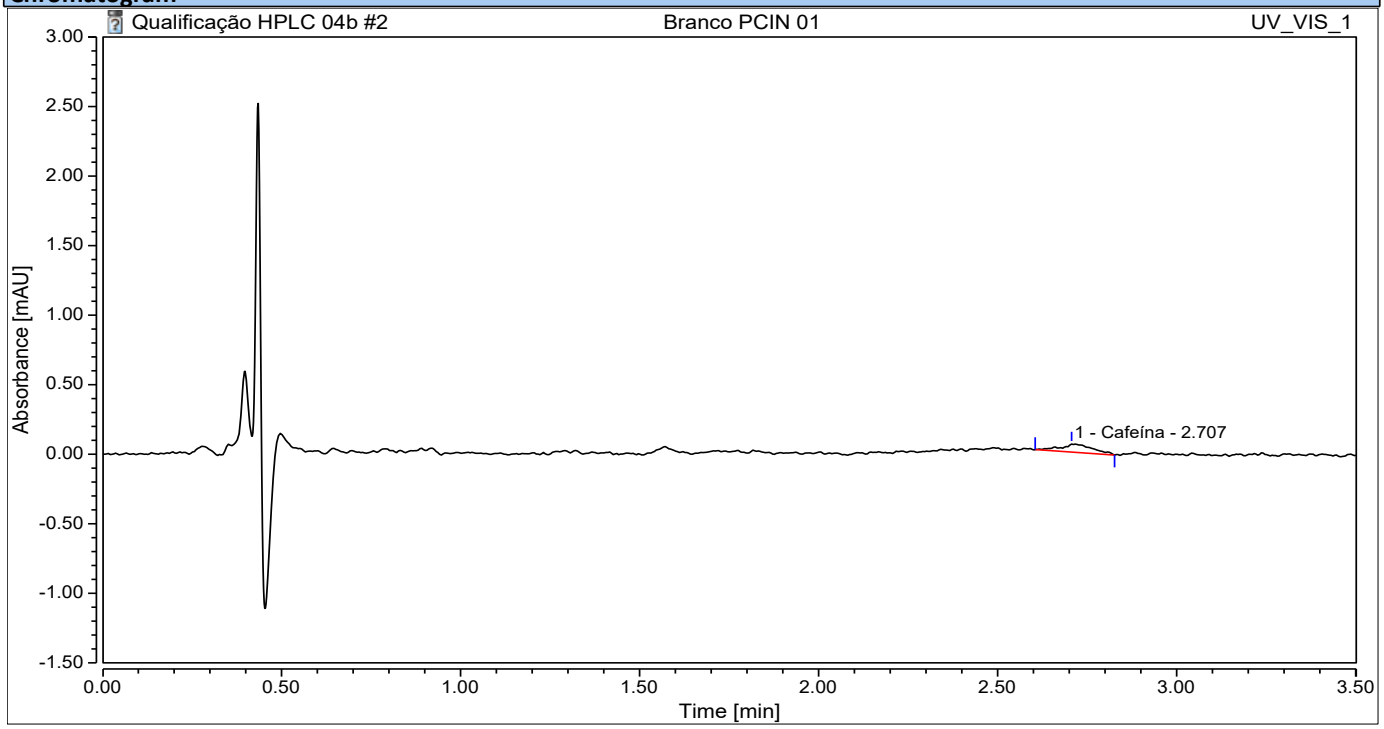

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.707	0.0063	0.058	100.00	100.00	n.a.
Total:			**0.006**	**0.058**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:14**	*Sample Weight:*	**1.0000**

Chromatogram

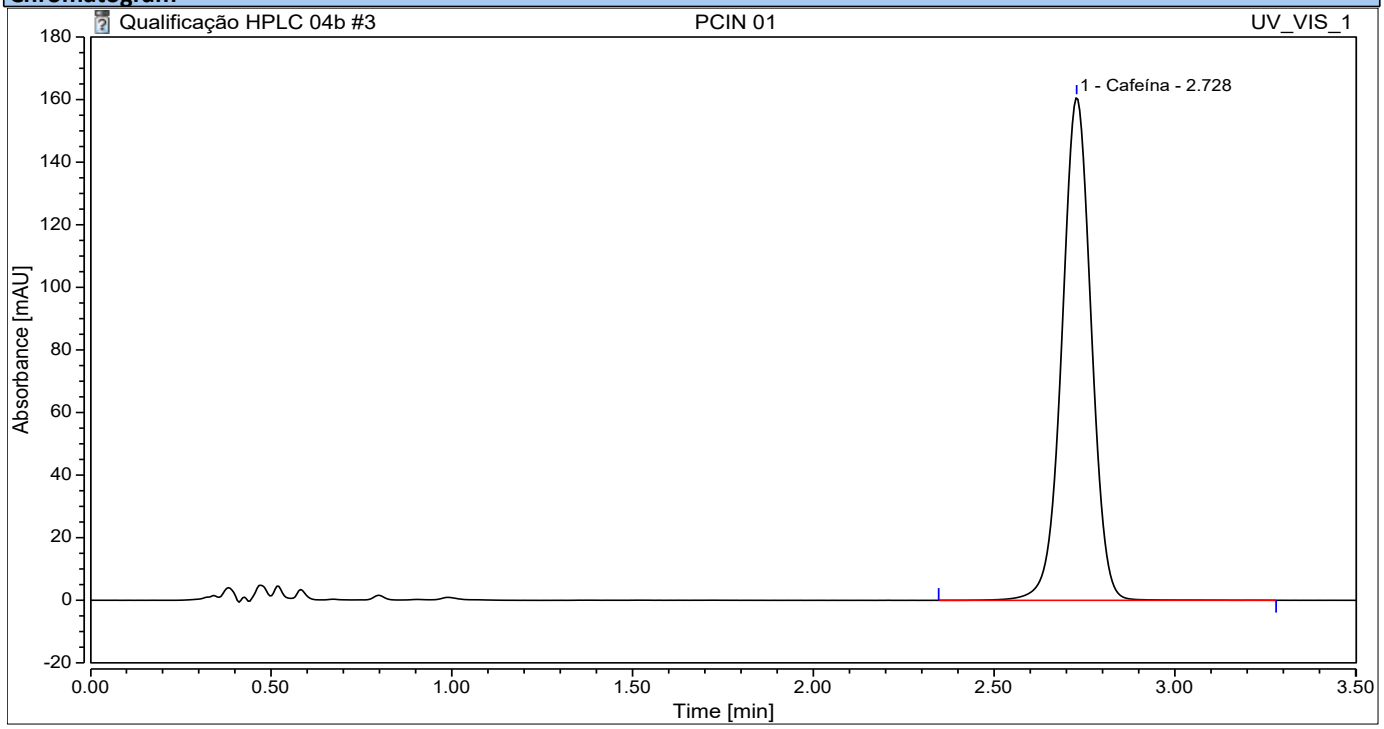

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.728	15.0919	160.760	100.00	100.00	n.a.
Total:			**15.092**	**160.760**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:19**	*Sample Weight:*	**1.0000**

Chromatogram

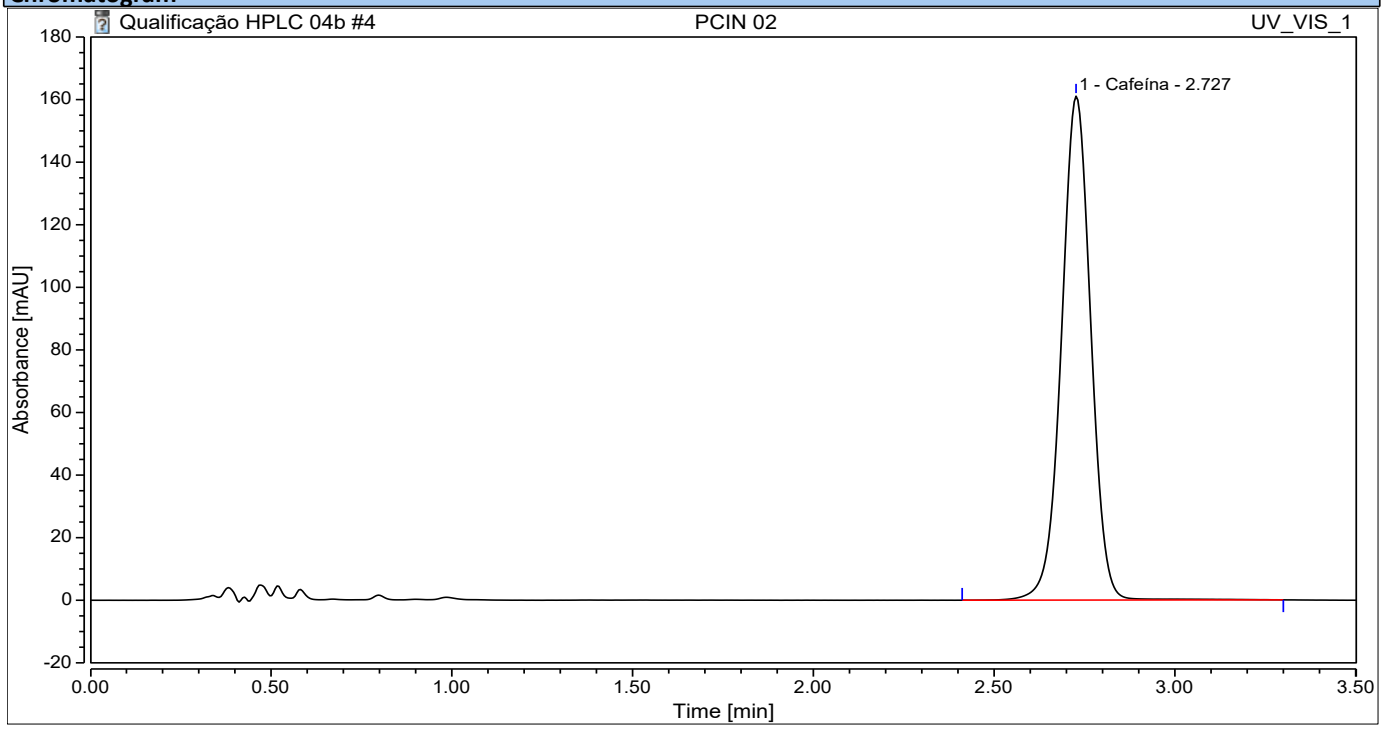

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.727	15.1229	161.047	100.00	100.00	n.a.
Total:			**15.123**	**161.047**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:23**	*Sample Weight:*	**1.0000**

Chromatogram

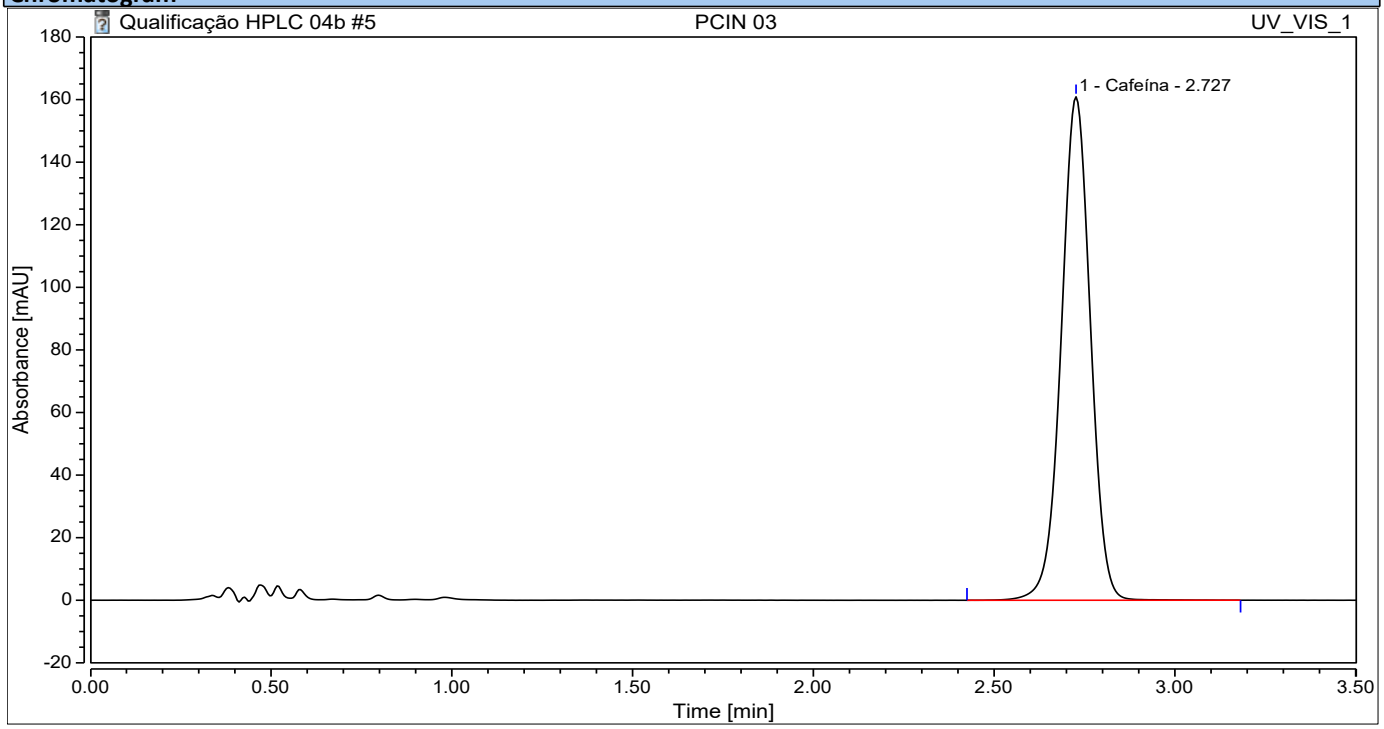

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.727	15.0452	160.896	100.00	100.00	n.a.
Total:			**15.045**	**160.896**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**3.50**
Vial Number:	**B:A2**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:27**	*Sample Weight:*	**1.0000**

Chromatogram

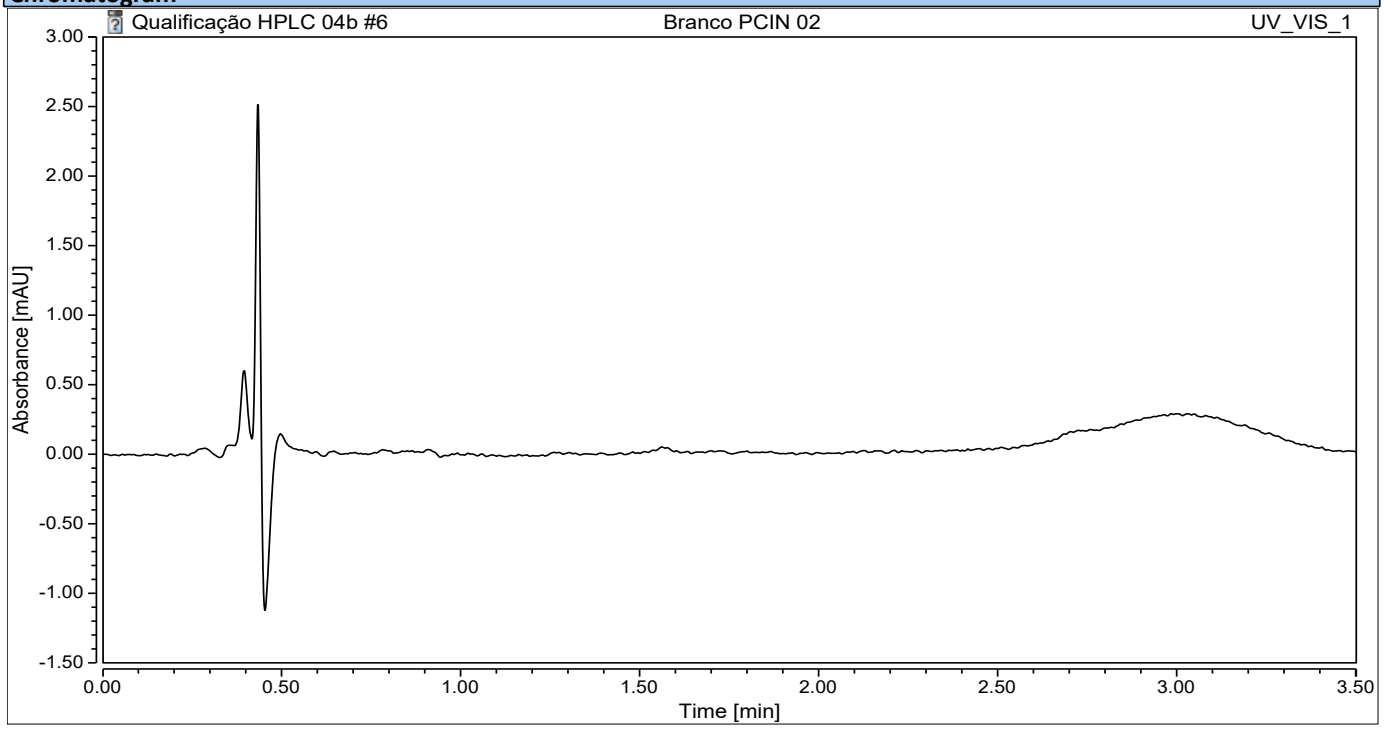

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.000**	**0.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:31**	*Sample Weight:*	**1.0000**

Chromatogram

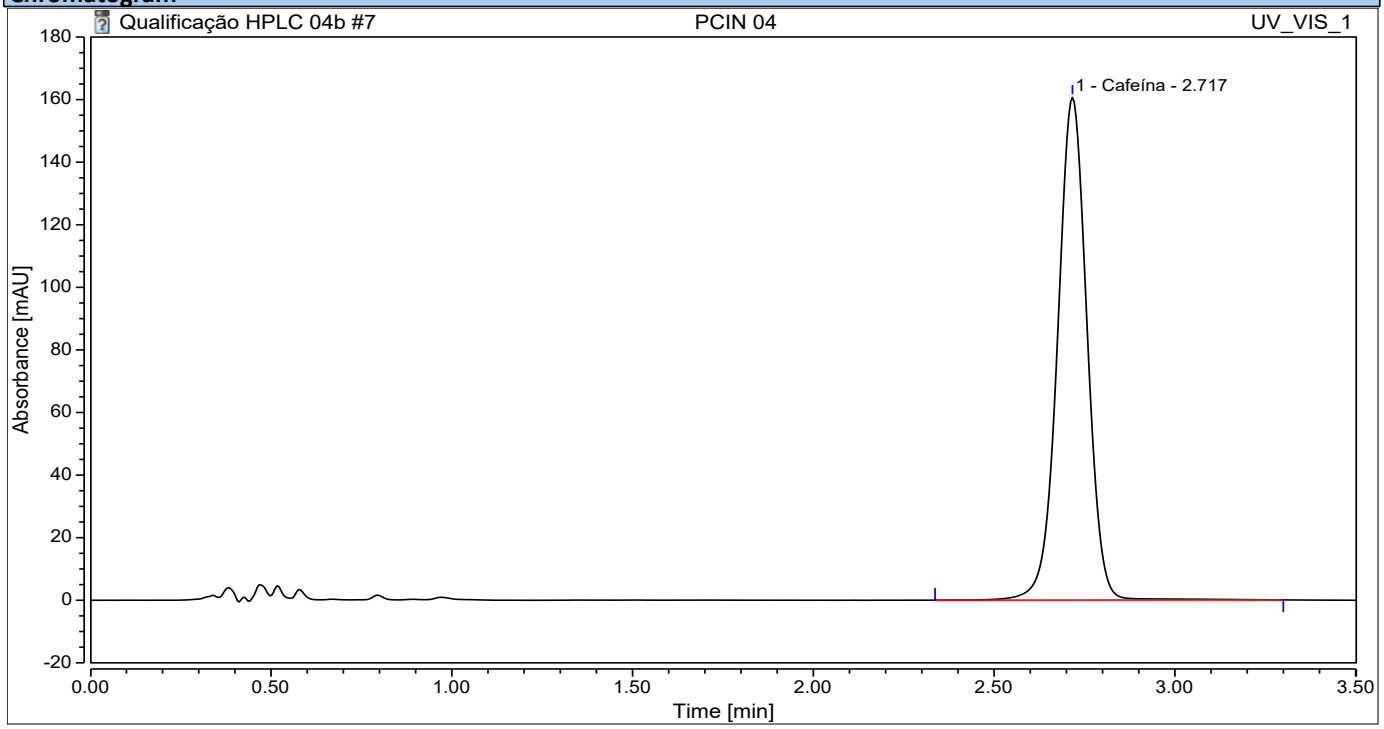

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.717	15.1800	160.648	100.00	100.00	n.a.
Total:			**15.180**	**160.648**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:35**	*Sample Weight:*	**1.0000**

Chromatogram

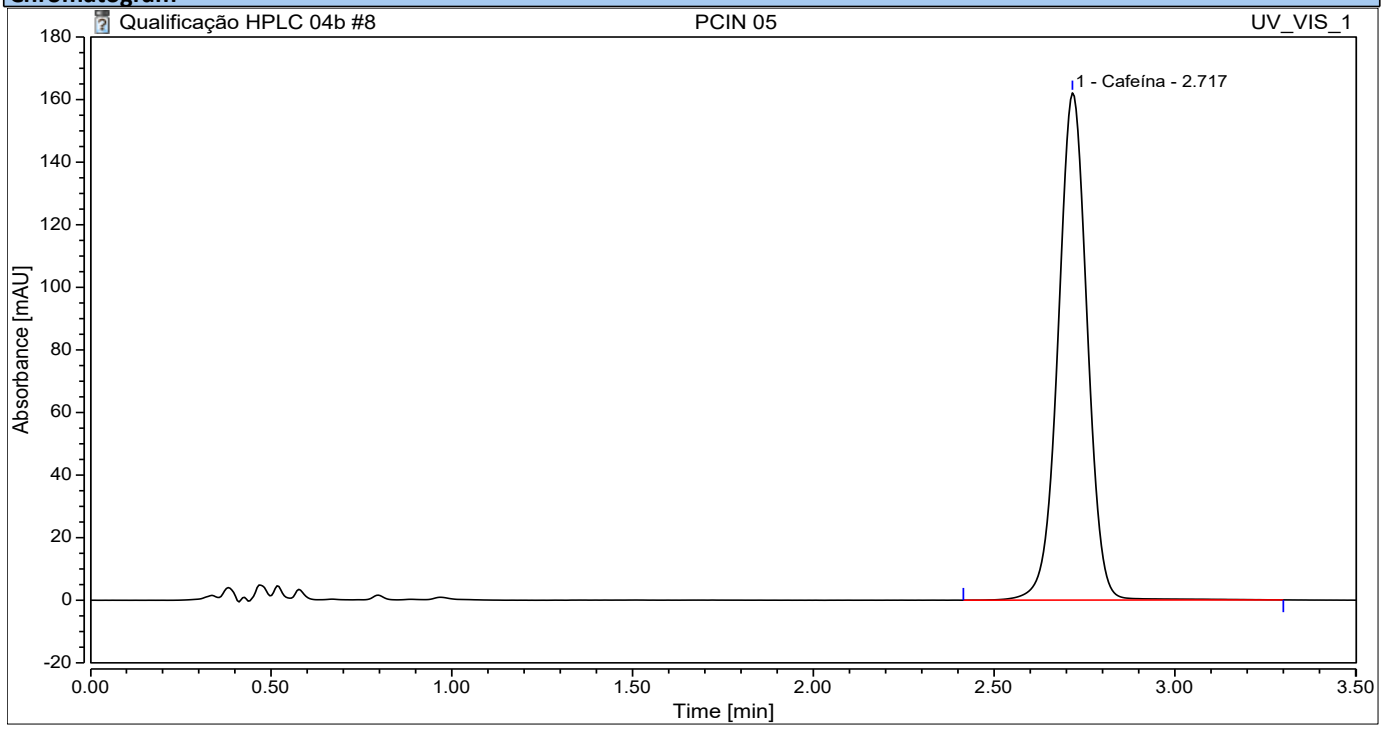

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.717	15.1410	162.100	100.00	100.00	n.a.
Total:			**15.141**	**162.100**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**3.50**
Vial Number:	**B:A3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:39**	*Sample Weight:*	**1.0000**

Chromatogram

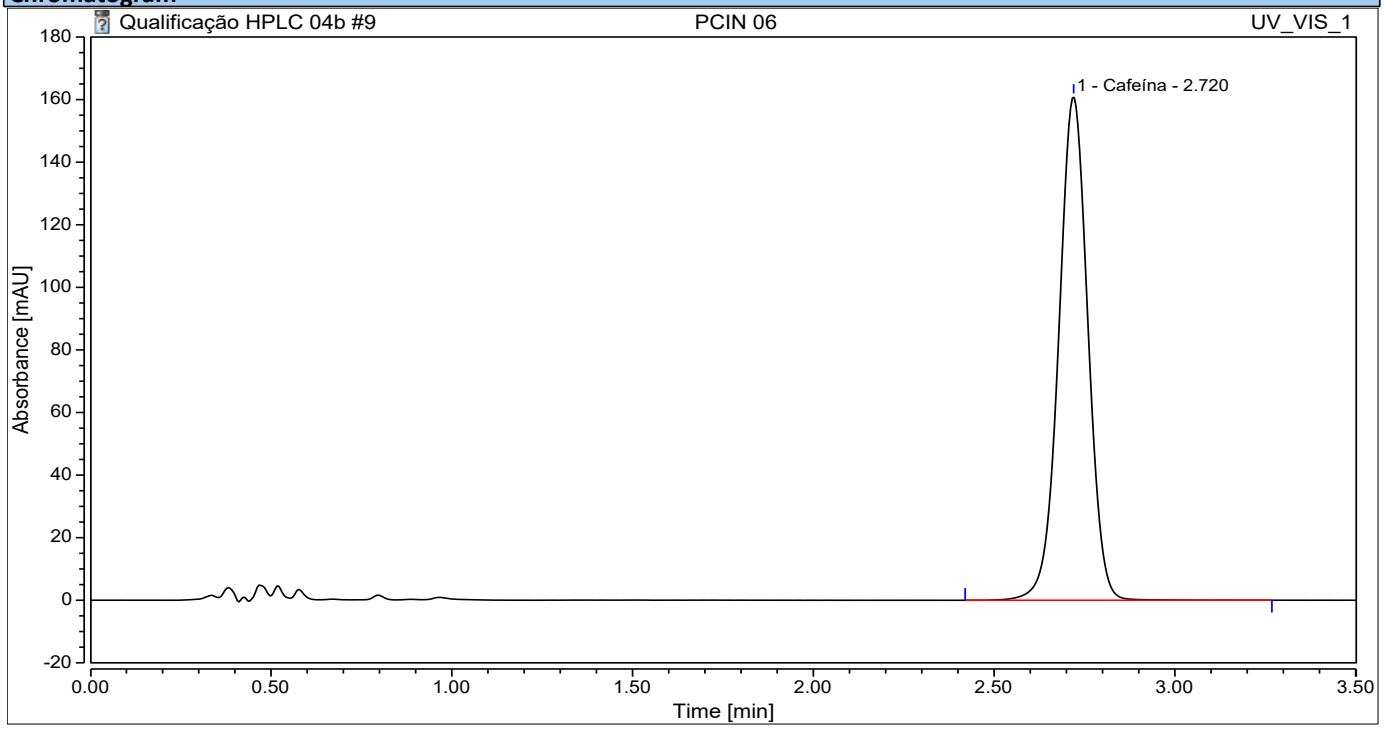

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.720	15.0460	160.999	100.00	100.00	n.a.
Total:			**15.046**	**160.999**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**3.50**
Vial Number:	**B:A2**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:44**	*Sample Weight:*	**1.0000**

Chromatogram

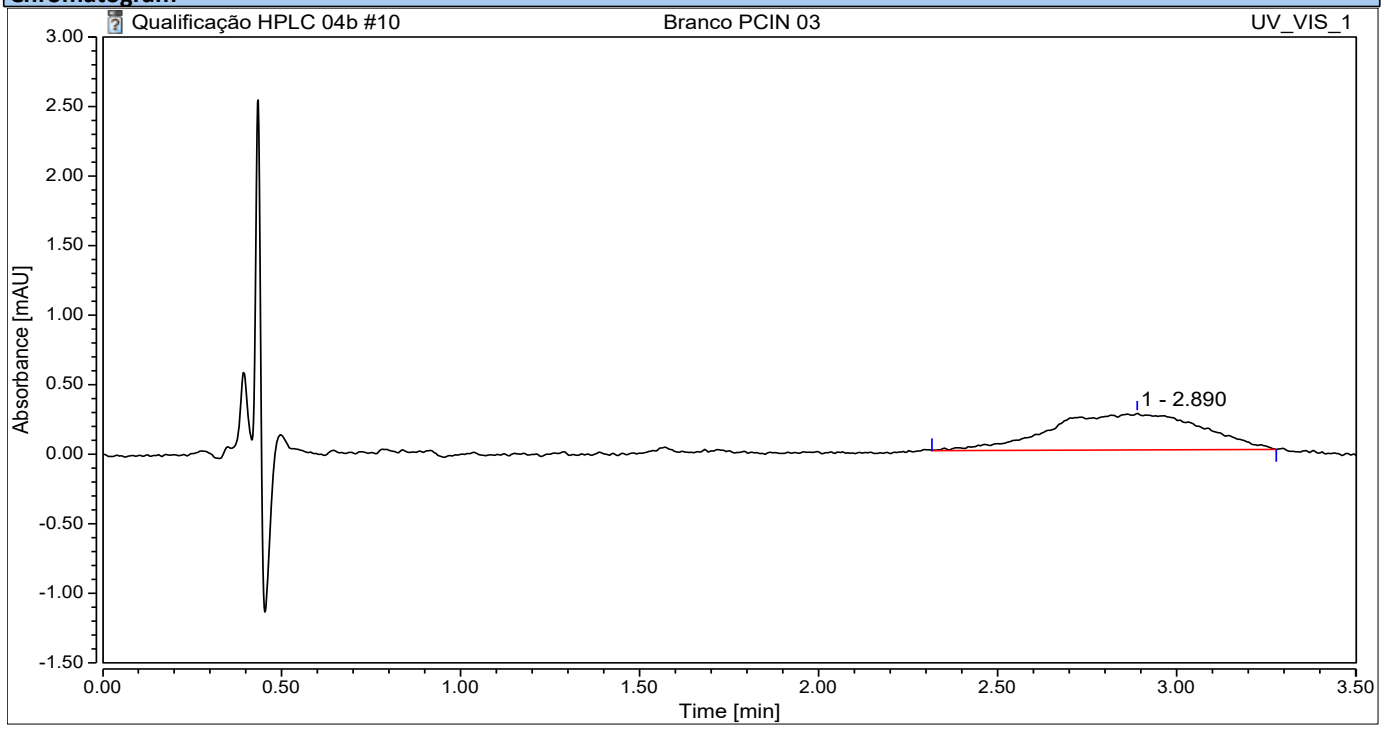

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.000**	**0.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**3.50**
Vial Number:	**B:A4**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:48**	*Sample Weight:*	**1.0000**

Chromatogram

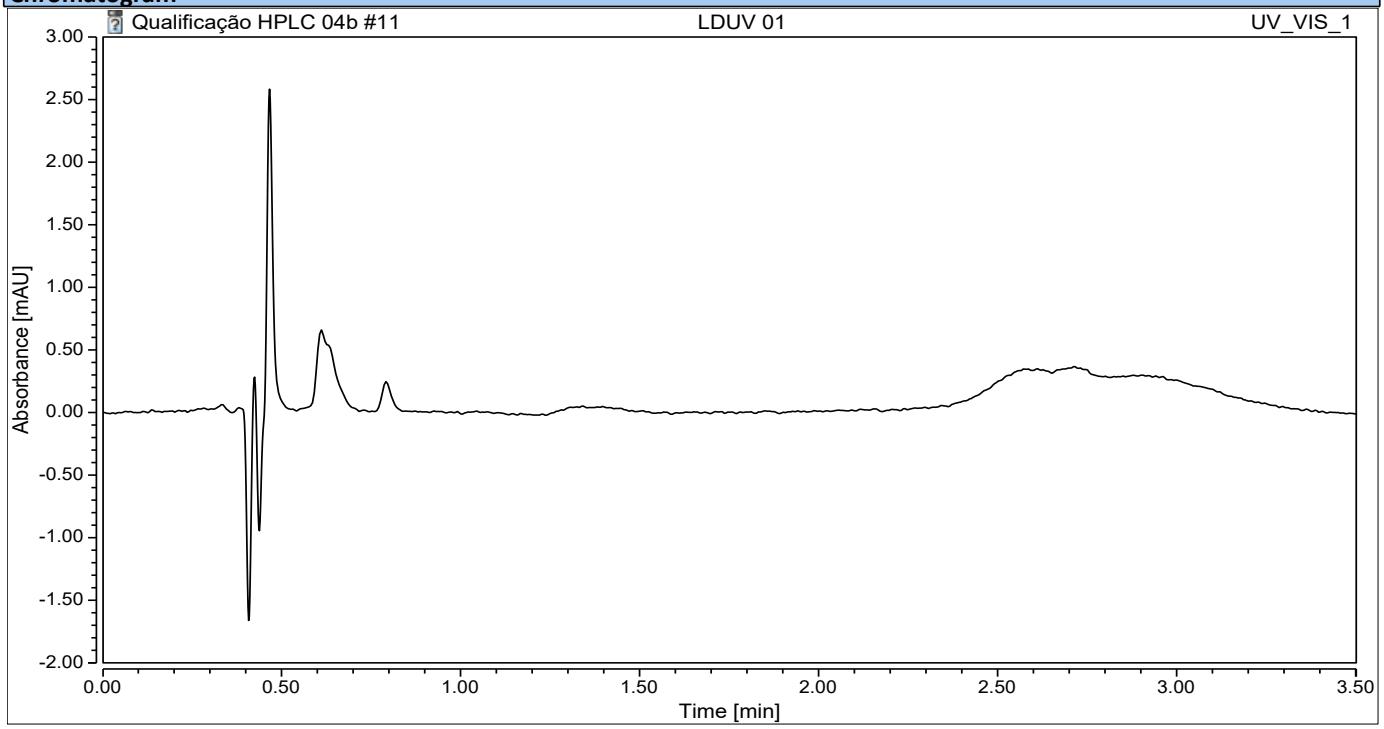

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.000**	**0.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**3.50**
Vial Number:	**B:A5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:52**	*Sample Weight:*	**1.0000**

Chromatogram

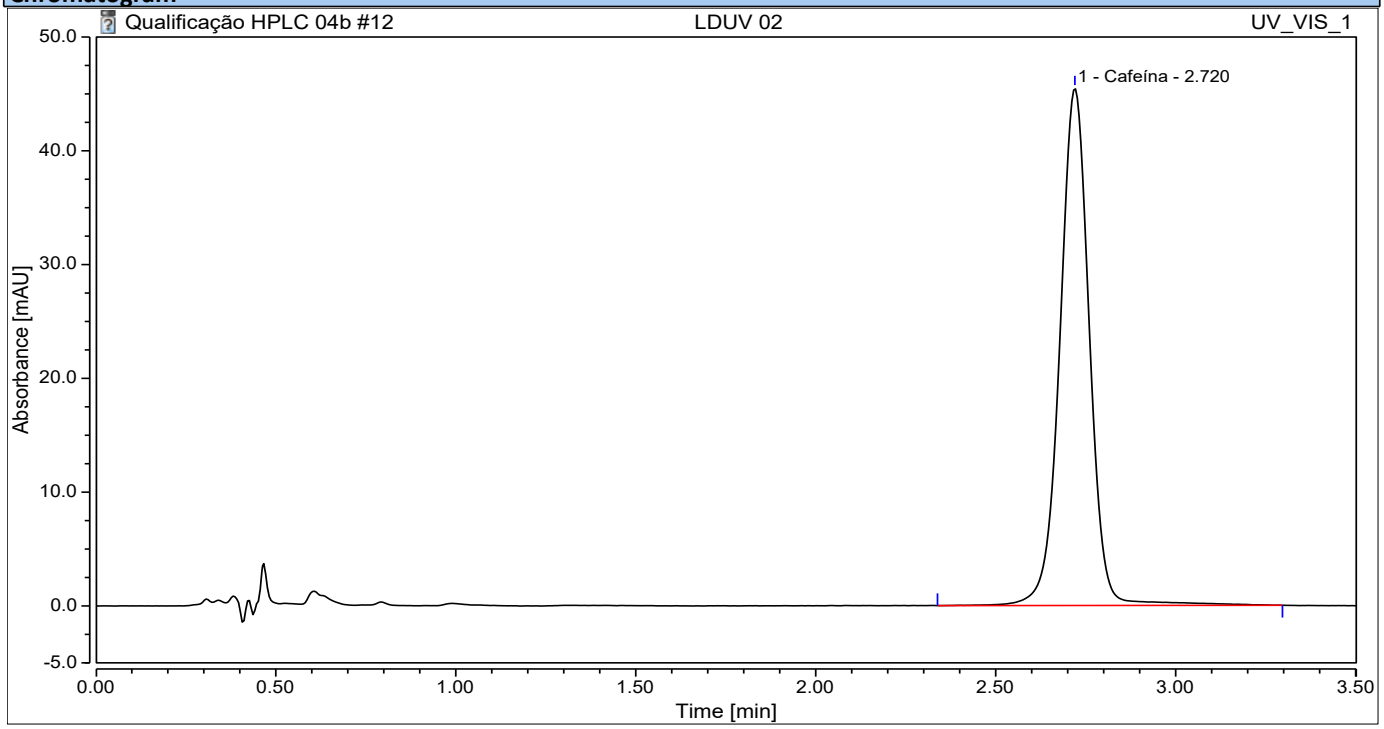

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.720	4.3309	45.469	100.00	100.00	n.a.
Total:			**4.331**	**45.469**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**3.50**
Vial Number:	**B:A6**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 12:56**	*Sample Weight:*	**1.0000**

Chromatogram

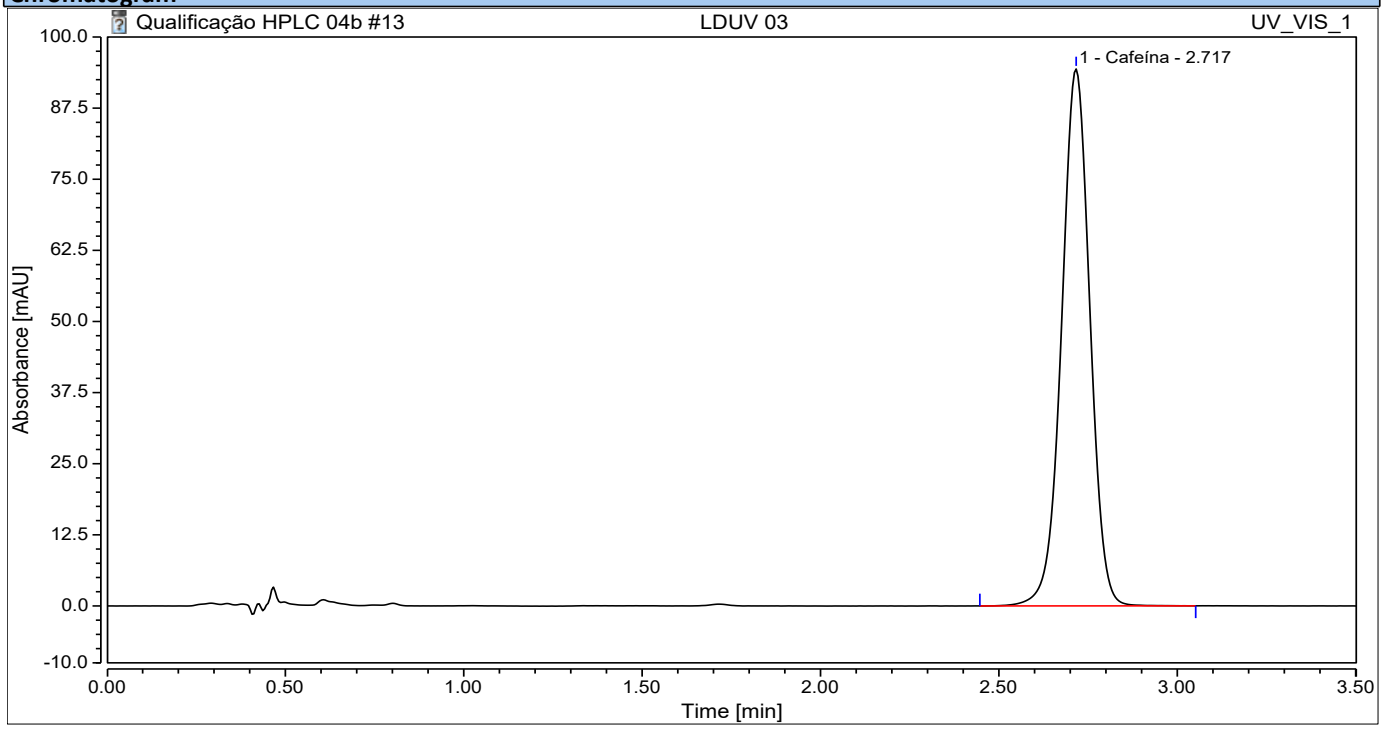

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.717	8.6718	94.375	100.00	100.00	n.a.
Total:			**8.672**	**94.375**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**3.50**
Vial Number:	**B:A7**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:00**	*Sample Weight:*	**1.0000**

Chromatogram

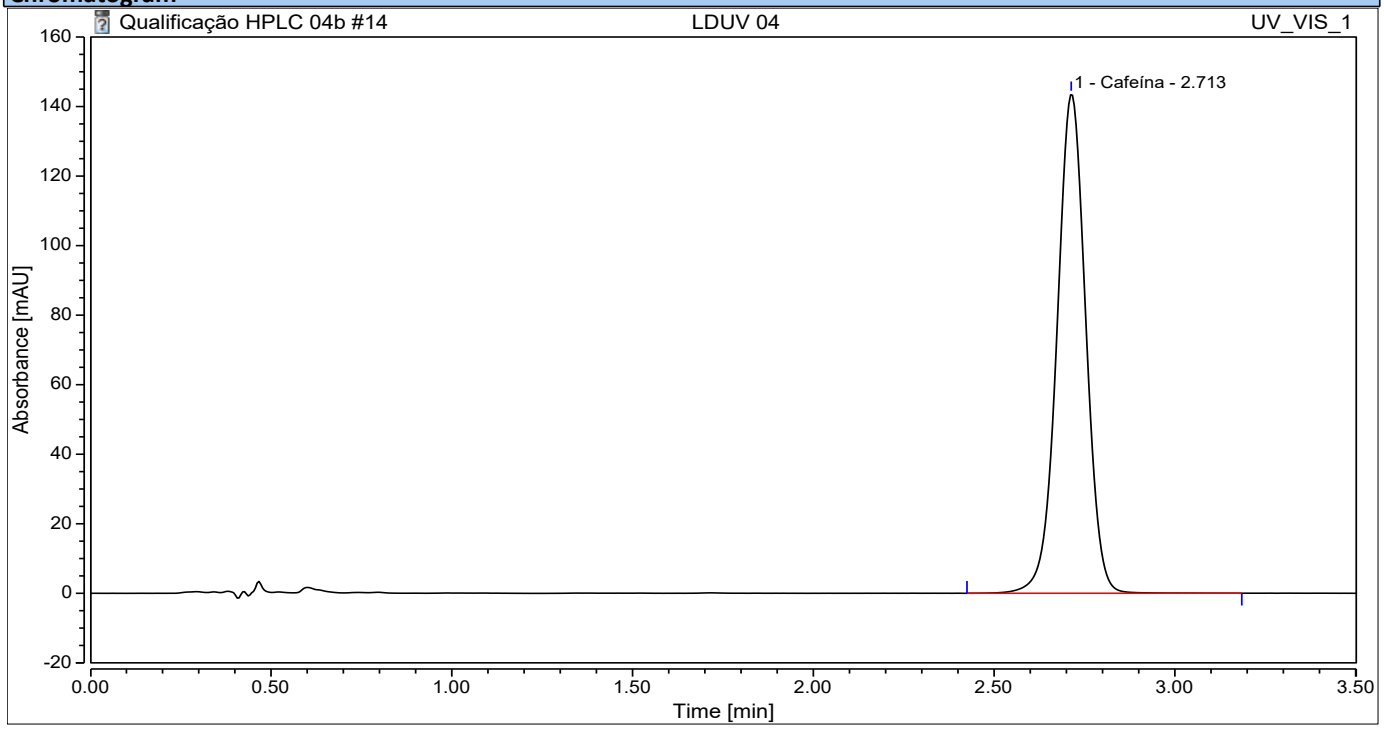

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.713	13.2460	143.657	100.00	100.00	n.a.
Total:			**13.246**	**143.657**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**3.50**
Vial Number:	**B:A8**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:04**	*Sample Weight:*	**1.0000**

Chromatogram

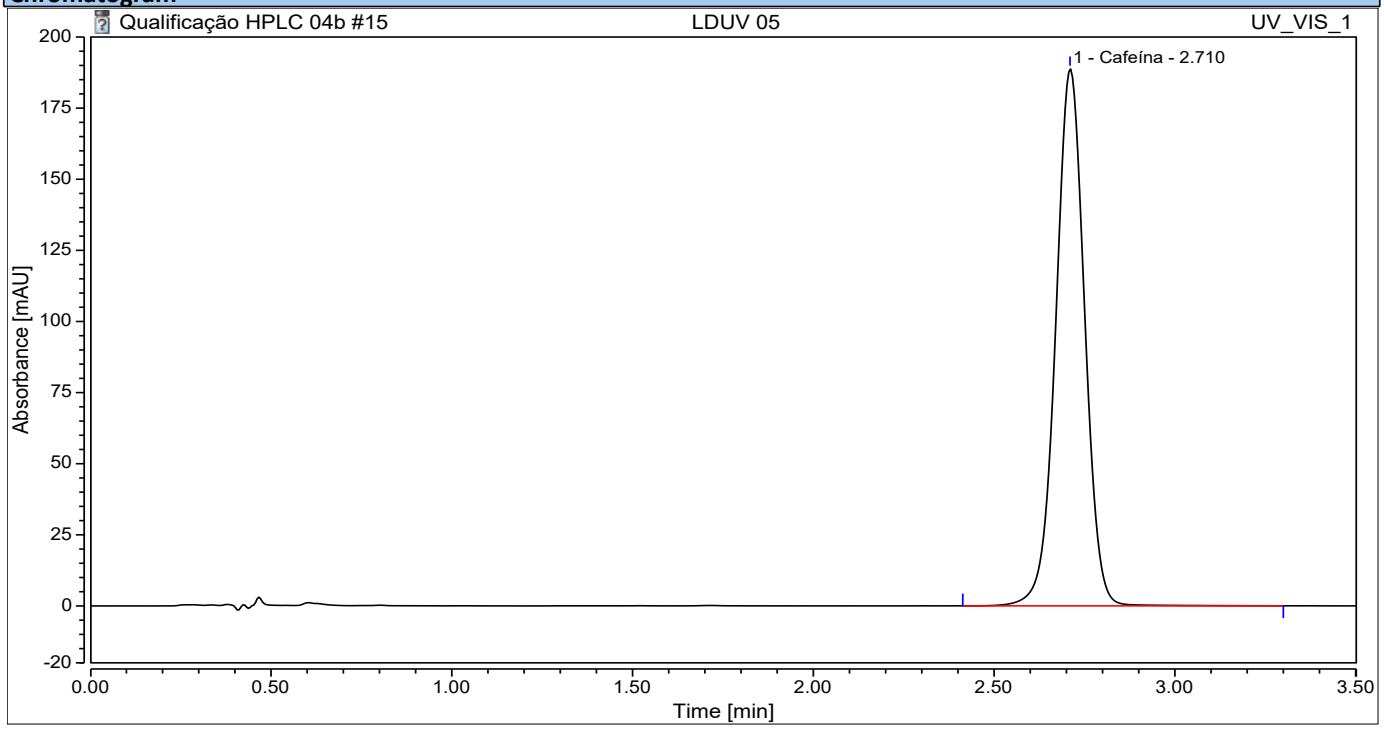

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.710	17.5018	188.807	100.00	100.00	n.a.
Total:			**17.502**	**188.807**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**3.50**
Vial Number:	**B:A9**	*Injection Volume:*	**0.10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:08**	*Sample Weight:*	**1.0000**

Chromatogram

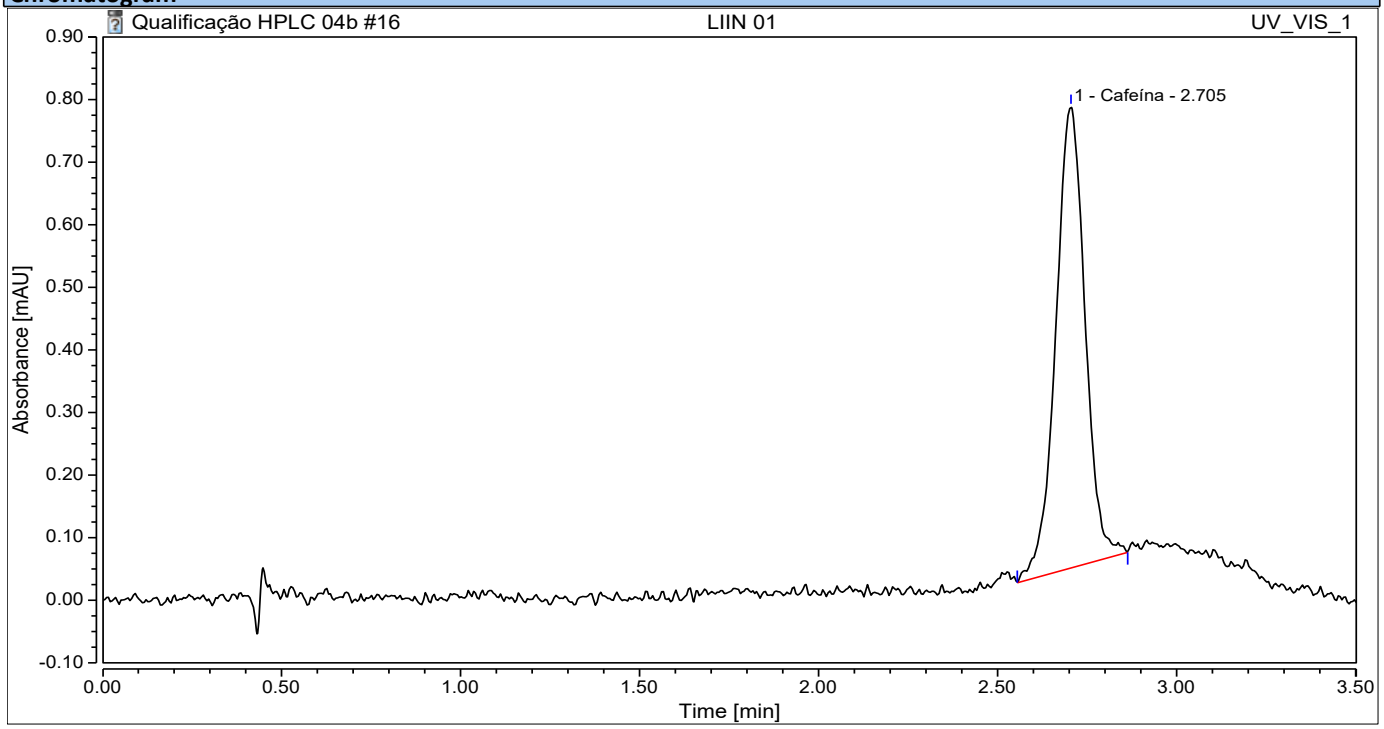

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.705	0.0700	0.737	100.00	100.00	n.a.
Total:			**0.070**	**0.737**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**3.50**
Vial Number:	**B:A9**	*Injection Volume:*	**5.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:13**	*Sample Weight:*	**1.0000**

Chromatogram

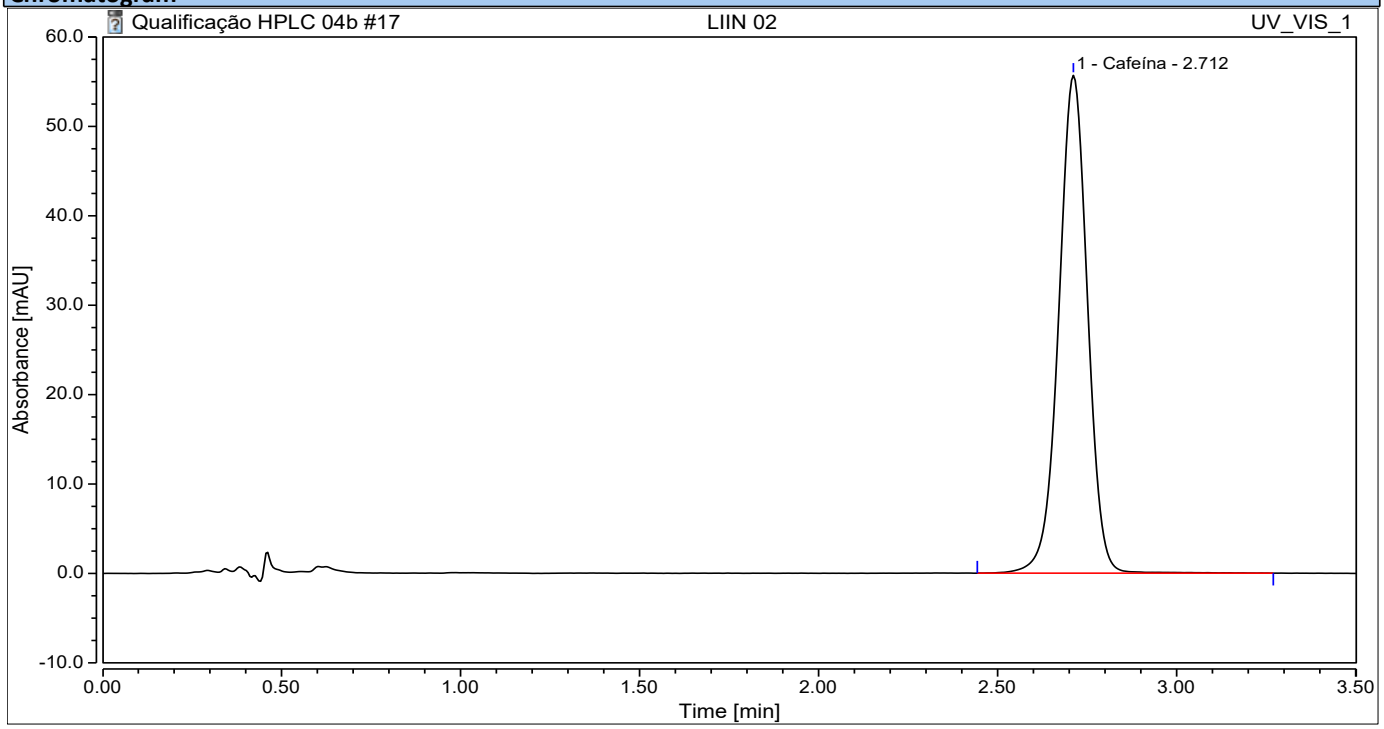

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.712	5.1896	55.680	100.00	100.00	n.a.
Total:			**5.190**	**55.680**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**3.50**
Vial Number:	**B:A9**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:17**	*Sample Weight:*	**1.0000**

Chromatogram

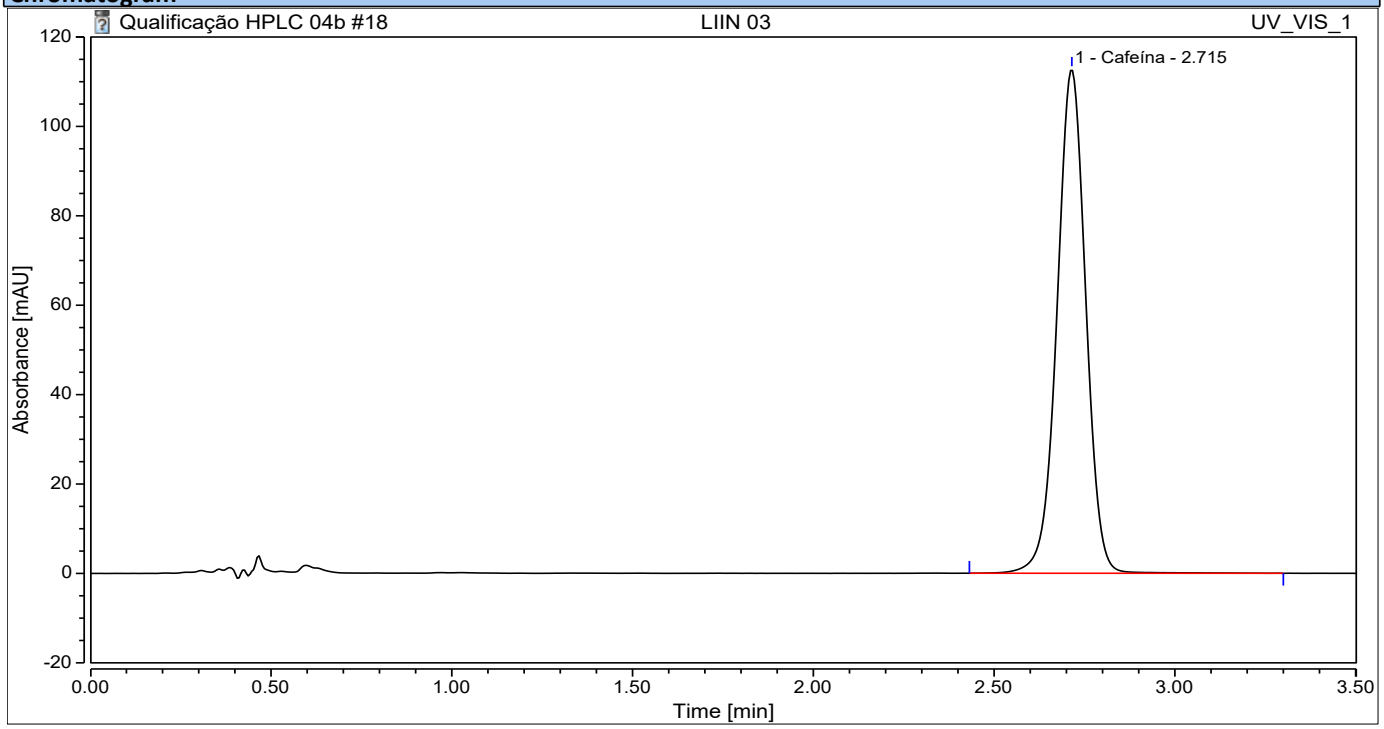

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.715	10.3935	112.743	100.00	100.00	n.a.
Total:			**10.394**	**112.743**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**3.50**
Vial Number:	**B:A9**	*Injection Volume:*	**15.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:21**	*Sample Weight:*	**1.0000**

Chromatogram

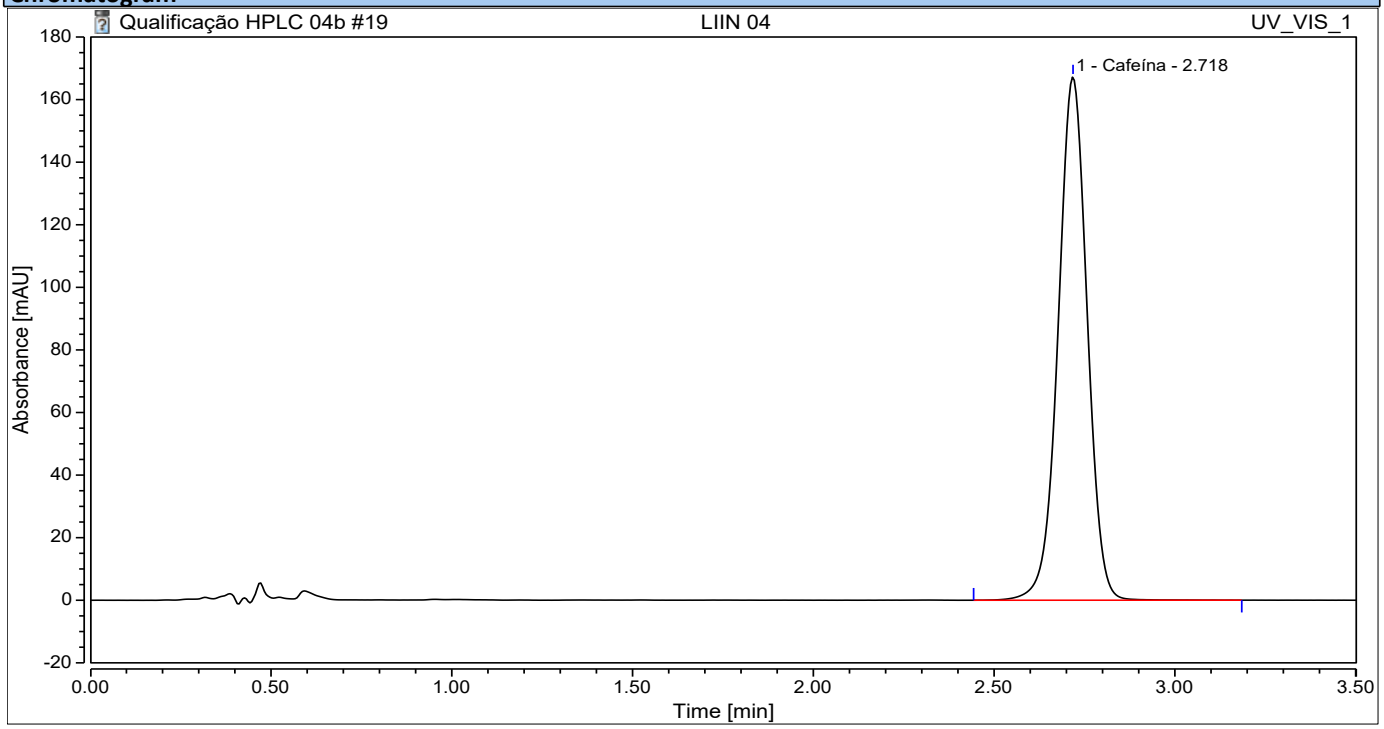

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.718	15.5369	167.197	100.00	100.00	n.a.
Total:			**15.537**	**167.197**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**3.50**
Vial Number:	**B:A9**	*Injection Volume:*	**20.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 13:25**	*Sample Weight:*	**1.0000**

Chromatogram

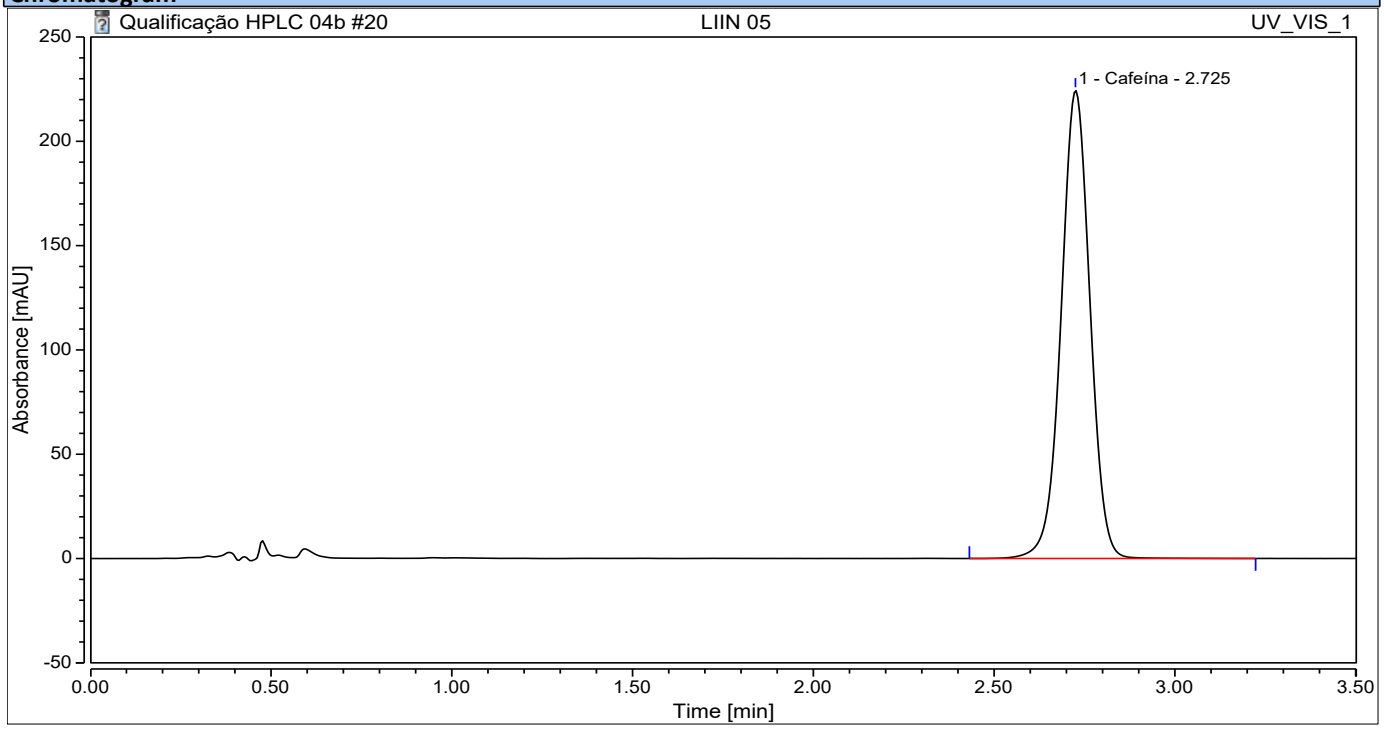

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	2.725	20.7405	224.430	100.00	100.00	n.a.
Total:			**20.740**	**224.430**	**100.000**	**100.000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB**	*Run Time (min):*	**19.00**
Vial Number:	**B:A2**	*Injection Volume:*	**0.10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB 04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 16:57**	*Sample Weight:*	**1.0000**

Chromatogram

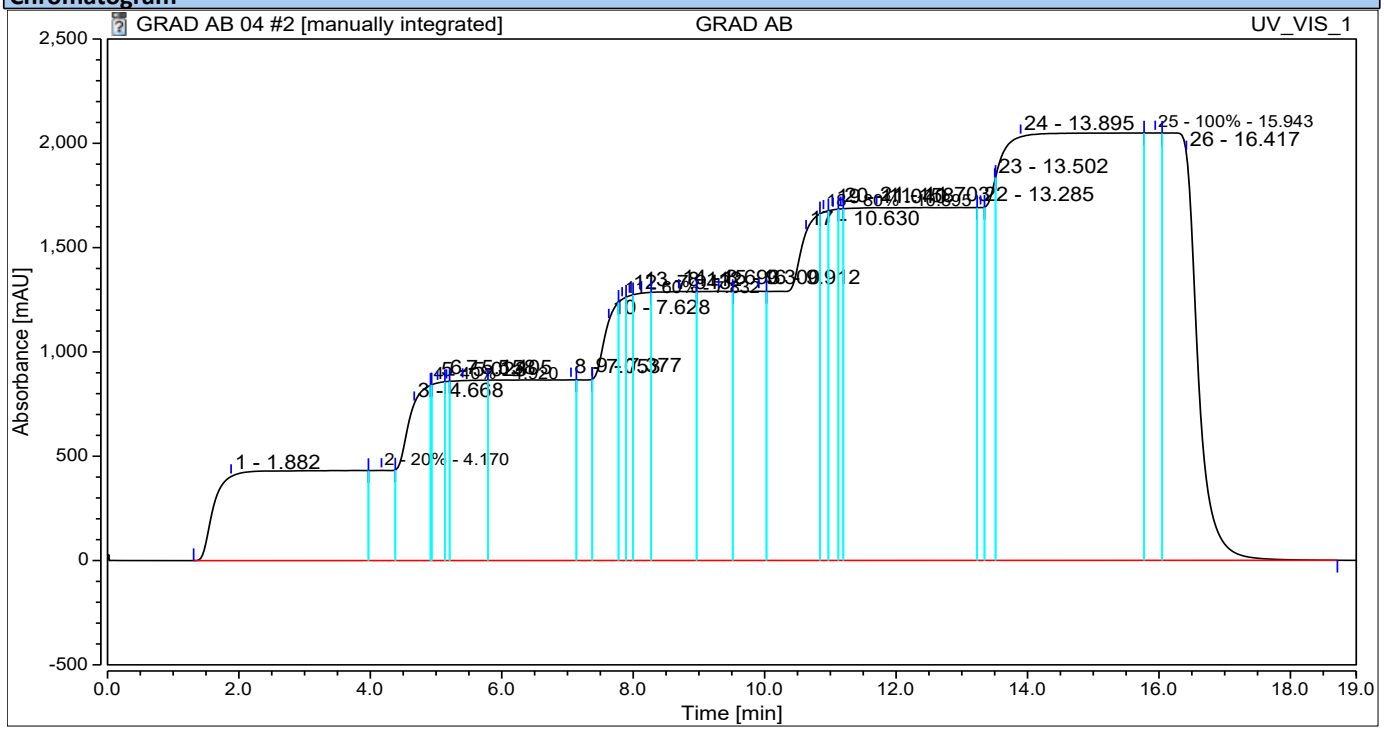

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4.170	176.2926	432.063	0.93	1.29	n.a.
4	40%	4.920	14.0194	840.508	0.07	2.52	n.a.
11	60%	7.832	143.9209	1251.763	0.76	3.75	n.a.
18	80%	10.895	214.2677	1669.026	1.13	5.00	n.a.
25	100%	15.943	563.3049	2048.953	2.96	6.14	n.a.
Total:			**1111.805**	**6242.313**	**5.851**	**18.691**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD CD**	*Run Time (min):*	**19.00**
Vial Number:	**B:A2**	*Injection Volume:*	**0.10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD 04**	*Bandwidth:*	**4**
Processing Method:	**Basic Quantitative**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**05/Apr/24 17:16**	*Sample Weight:*	**1.0000**

Chromatogram

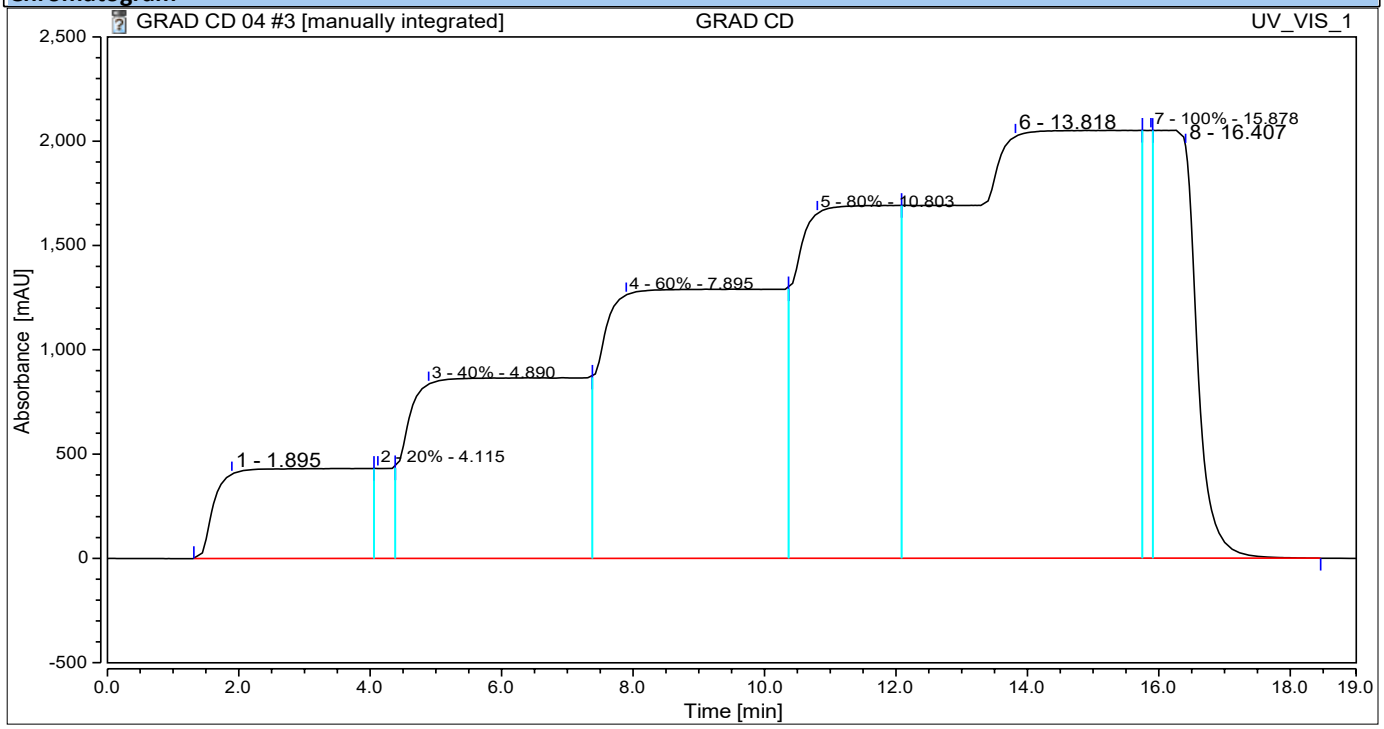

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4.115	139.5888	431.845	0.73	4.06	n.a.
3	40%	4.890	2493.8001	836.727	13.12	7.86	n.a.
4	60%	7.895	3752.0644	1253.849	19.74	11.87	n.a.
5	80%	10.803	2817.1770	1654.557	14.82	15.54	n.a.
7	100%	15.878	321.3226	2051.407	1.69	19.27	n.a.
Total:			**9523.953**	**6238.386**	**50.096**	**58.609**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.