
Peak Find - EDUV.jws

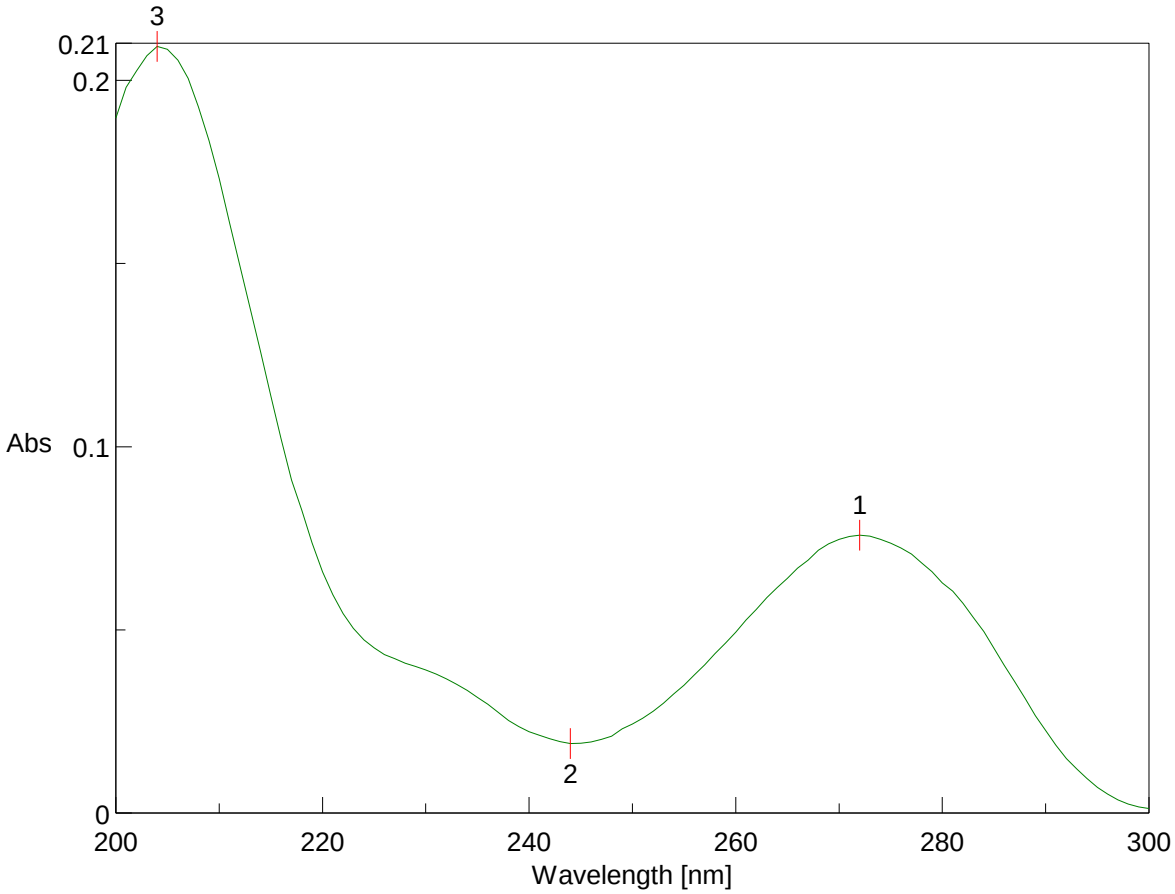

[Comments]

User	QPackSA
Division	---
Company	As Ervas Curam
Creation date	02/04/2025 13:22

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.075814	2	244	0.01899
3	204	0.209095			

Chromatogram

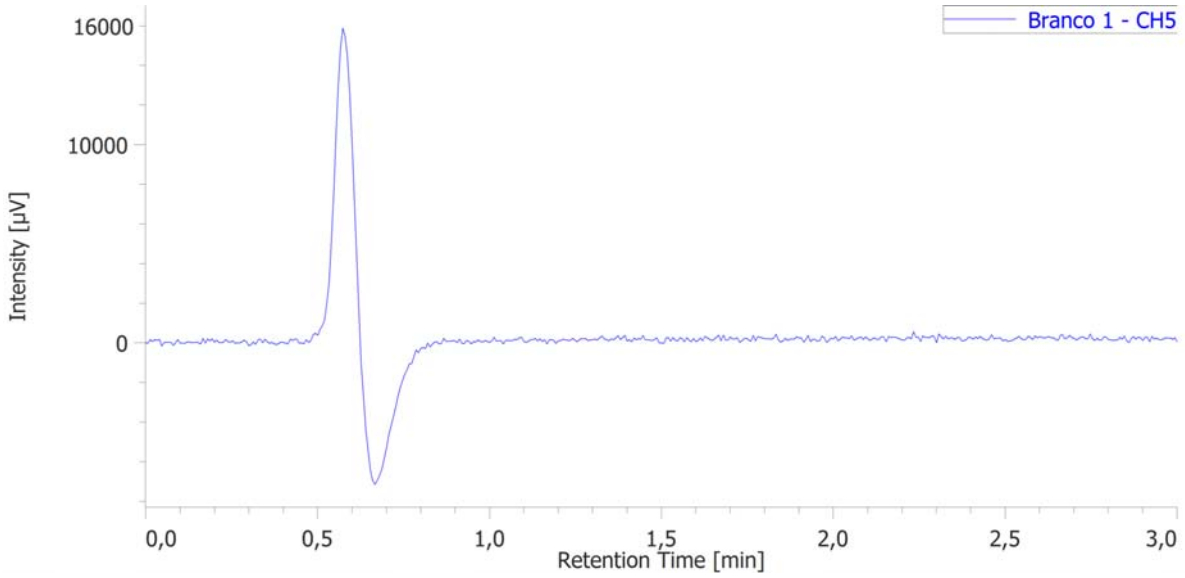


Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:30:13
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:27:10
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

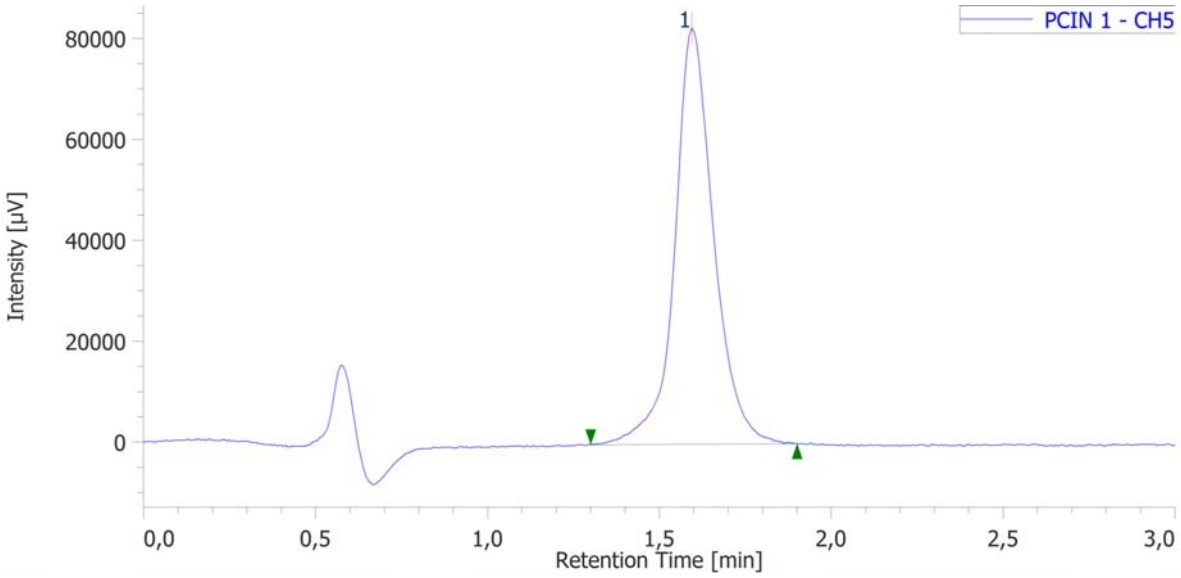

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:35:04
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:32:03
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,593	650004	82424	100,000	100,000	N/A	1122	N/A	1,063	

Creator QPackSA
Reviewer
Approver

Chromatogram

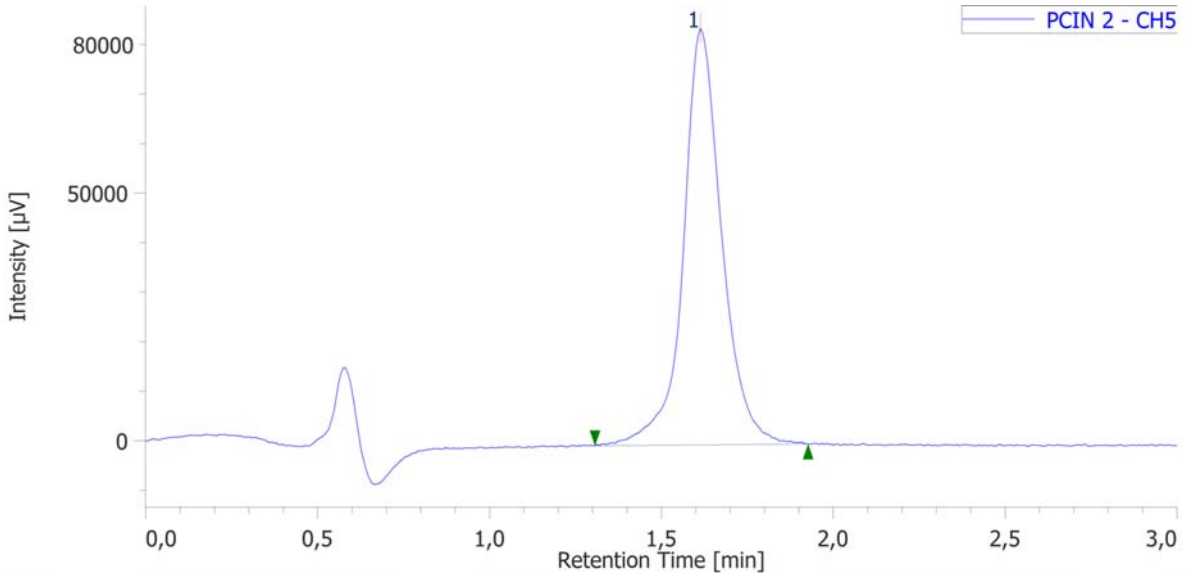

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:39:56
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:36:55
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.613	653550	84014	100.000	100.000	N/A	1192	N/A	1.034	

Creator QPackSA
Reviewer
Approver

Chromatogram

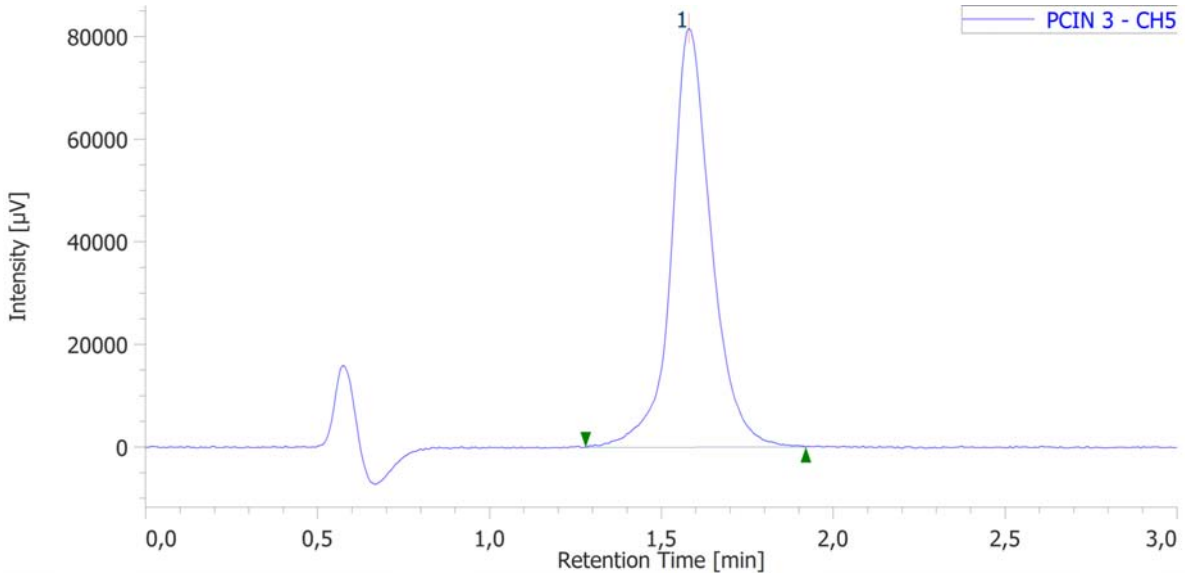

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:44:50
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:41:48
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,580	659952	81565	100,000	100,000	N/A	1060	N/A	1,063	

Creator QPackSA
Reviewer
Approver

Chromatogram

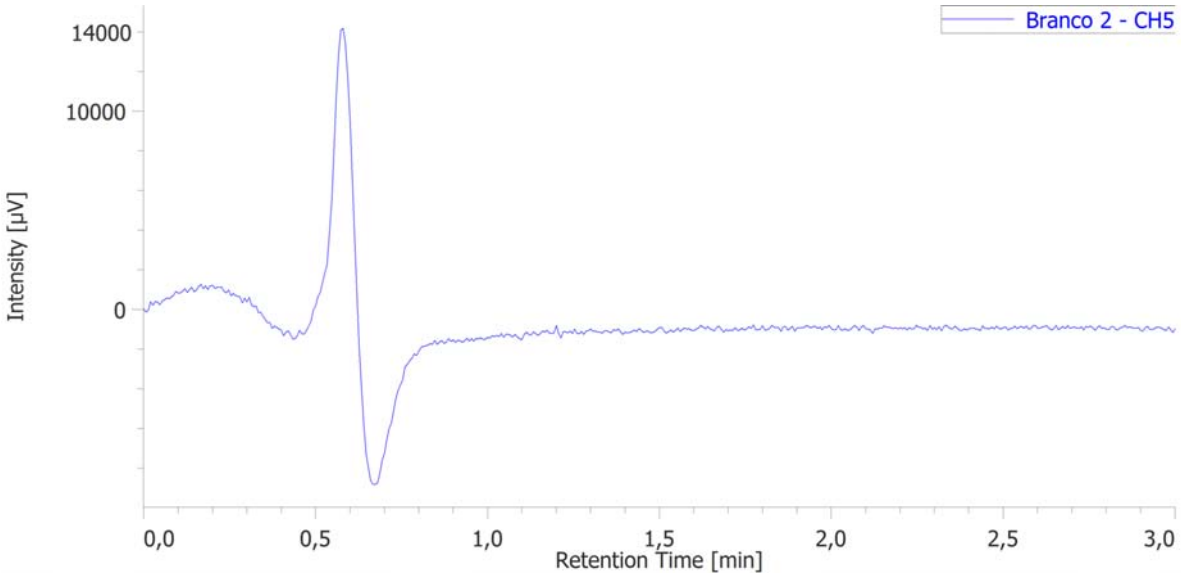


Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:49:42
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:46:41
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

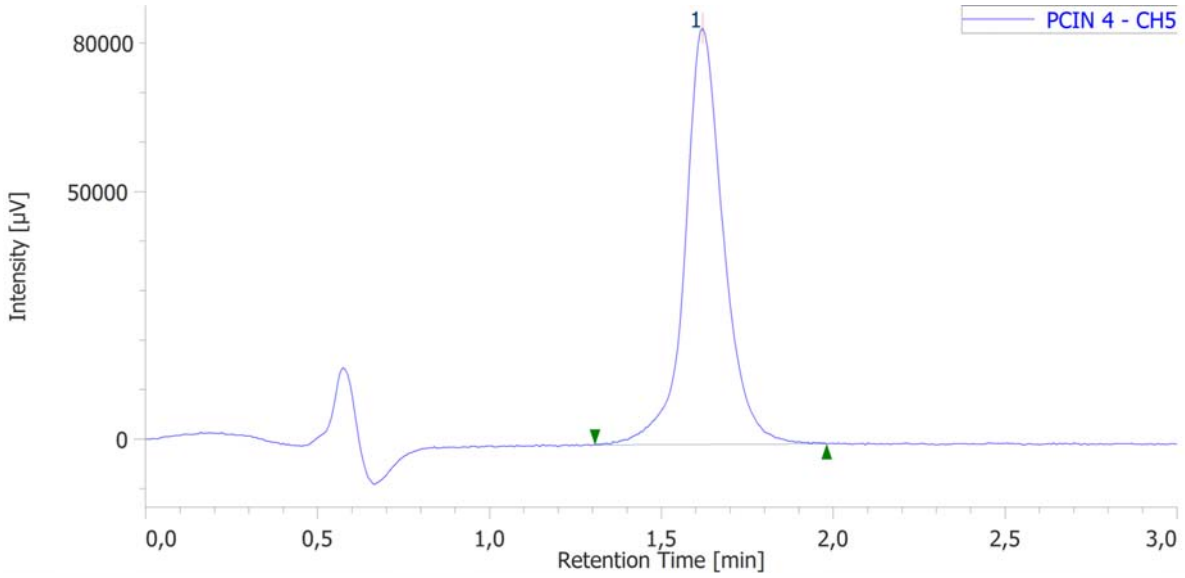

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:54:35
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:51:33
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.620	656735	84029	100.000	100.000	N/A	1198	N/A	1.021	

Creator QPackSA
Reviewer
Approver

Chromatogram

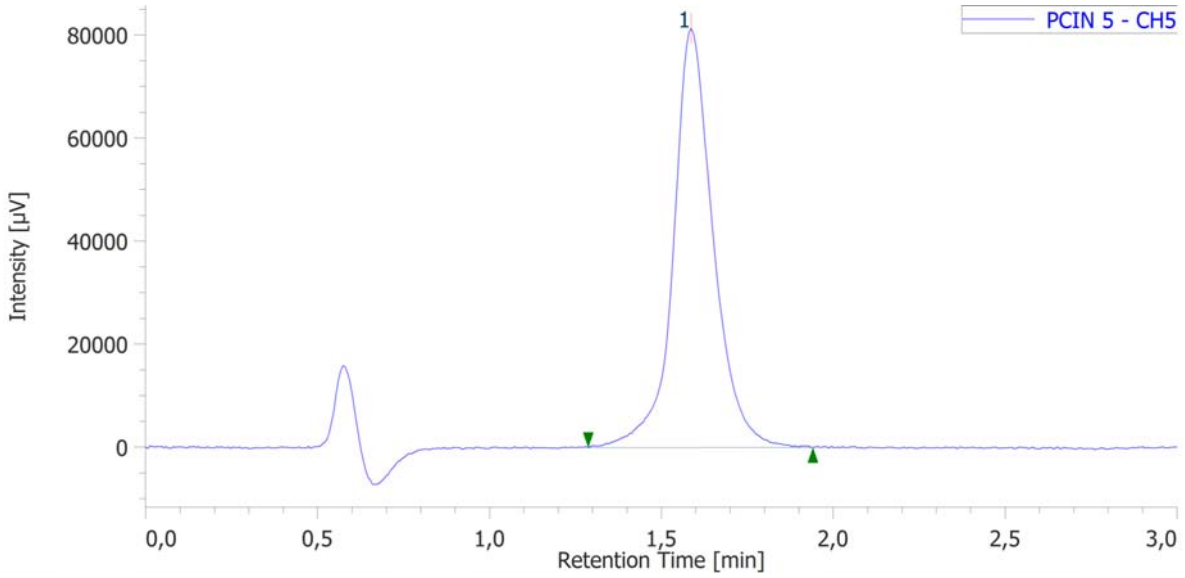

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 14:59:28
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 14:56:26
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.587	658746	81348	100.000	100.000	N/A	1068	N/A	1.044	

Creator QPackSA
Reviewer
Approver

Chromatogram

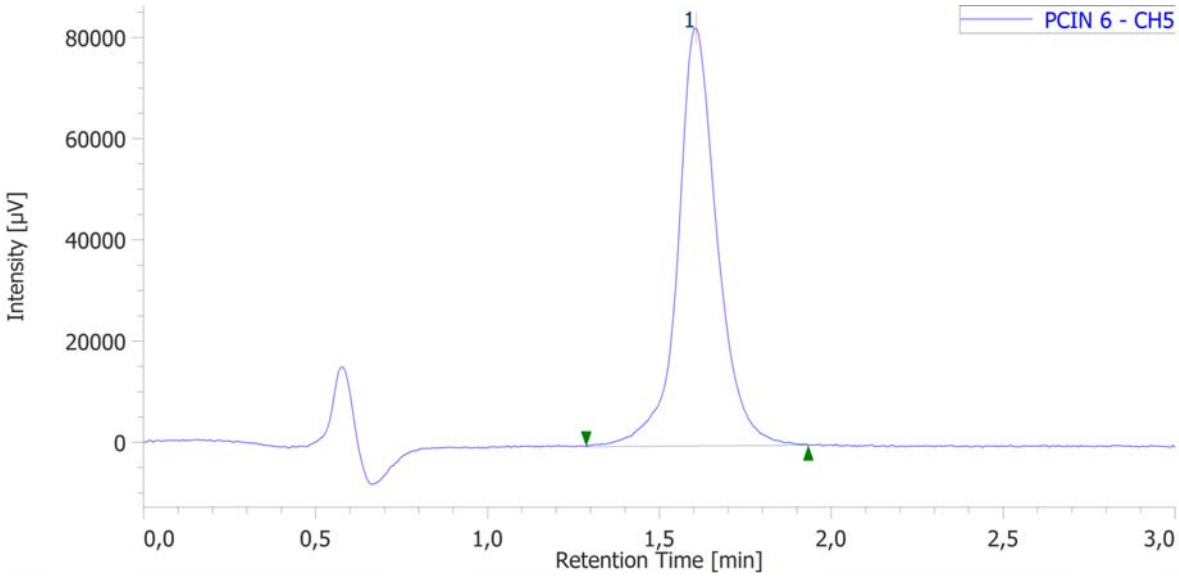

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 15:04:20
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 15:01:18
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.607	658821	82489	100.000	100.000	N/A	1135	N/A	1.025	

Creator QPackSA
Reviewer
Approver

Chromatogram

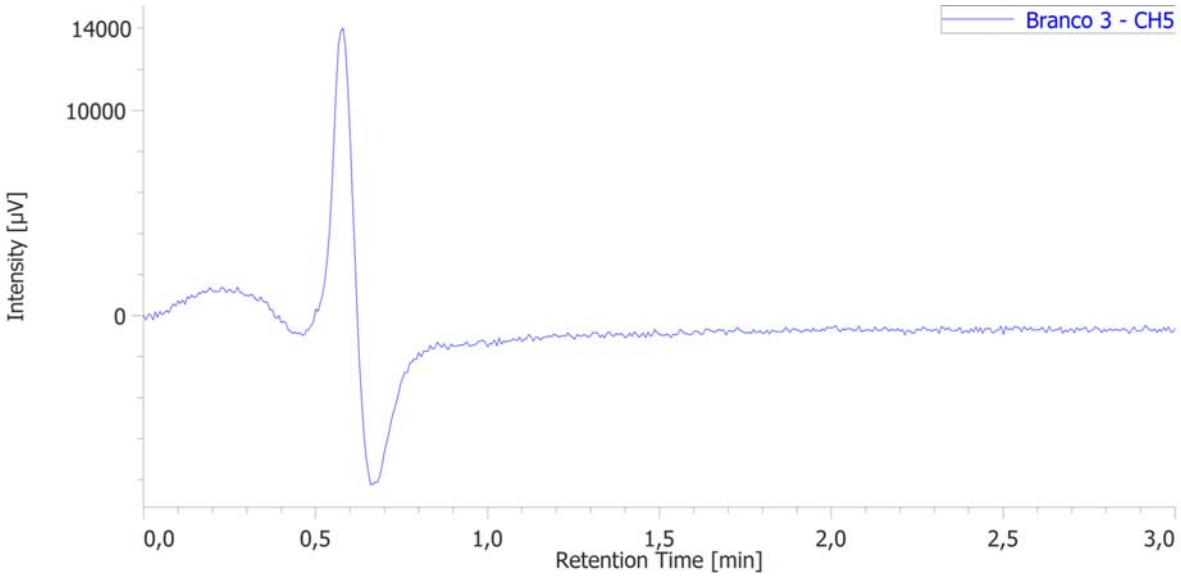


Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 15:09:10
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 15:06:08
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

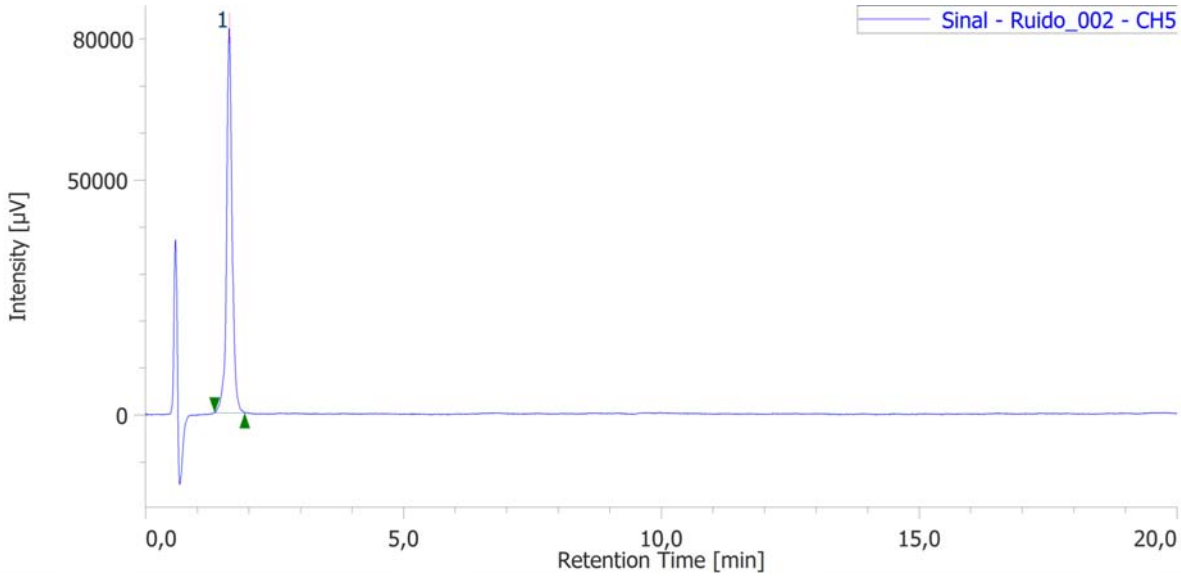

Chromatogram Information	
User Name	QPackSA
Date Modified	02/04/2025 16:02:24
Description	
HPLC System Name	11.XI.05
Injection Date	02/04/2025 15:42:22
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Sinal - Ruido_002-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,620	607486	81758	100,000	100,000	N/A	1343	N/A	0,999	

Creator
Reviewer
Approver

Certificado Nº: 149/25 - RELB	Início da Qualificação: 02/04/2025	Página 1 de 3

Resultado obtido na altura do pico


	ALTURA DO PICO (mAU)
Resultado:	81.7580

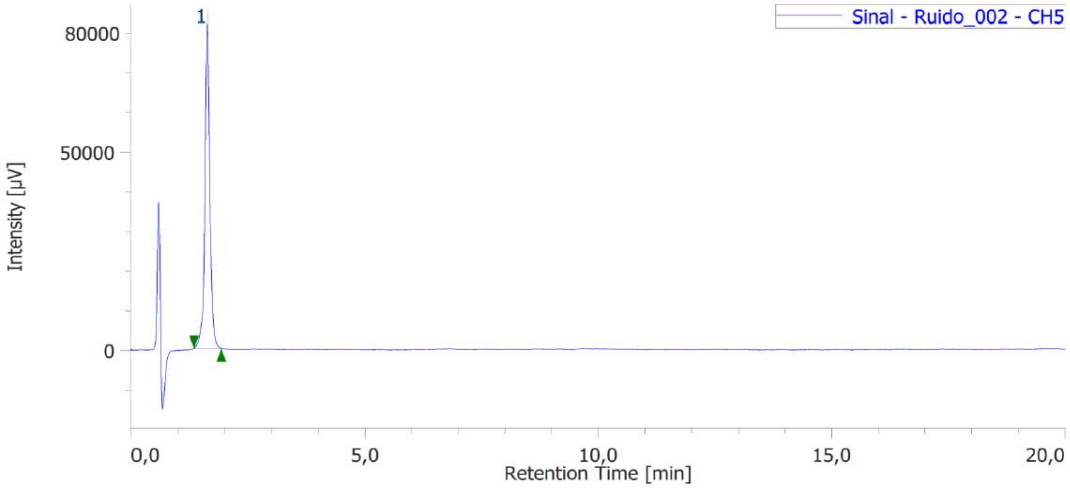

Certificado Nº: 149/25 - RELB	Início da Qualificação: 02/04/2025	Página 2 de 3

Resultado obtido no teste de sinal/ruído


Resultado:	Ruído (mAU)
VALOR MÁXIMO:	0.0276
VALOR MÍNIMO:	0.0188
	Ruído
	0.0088

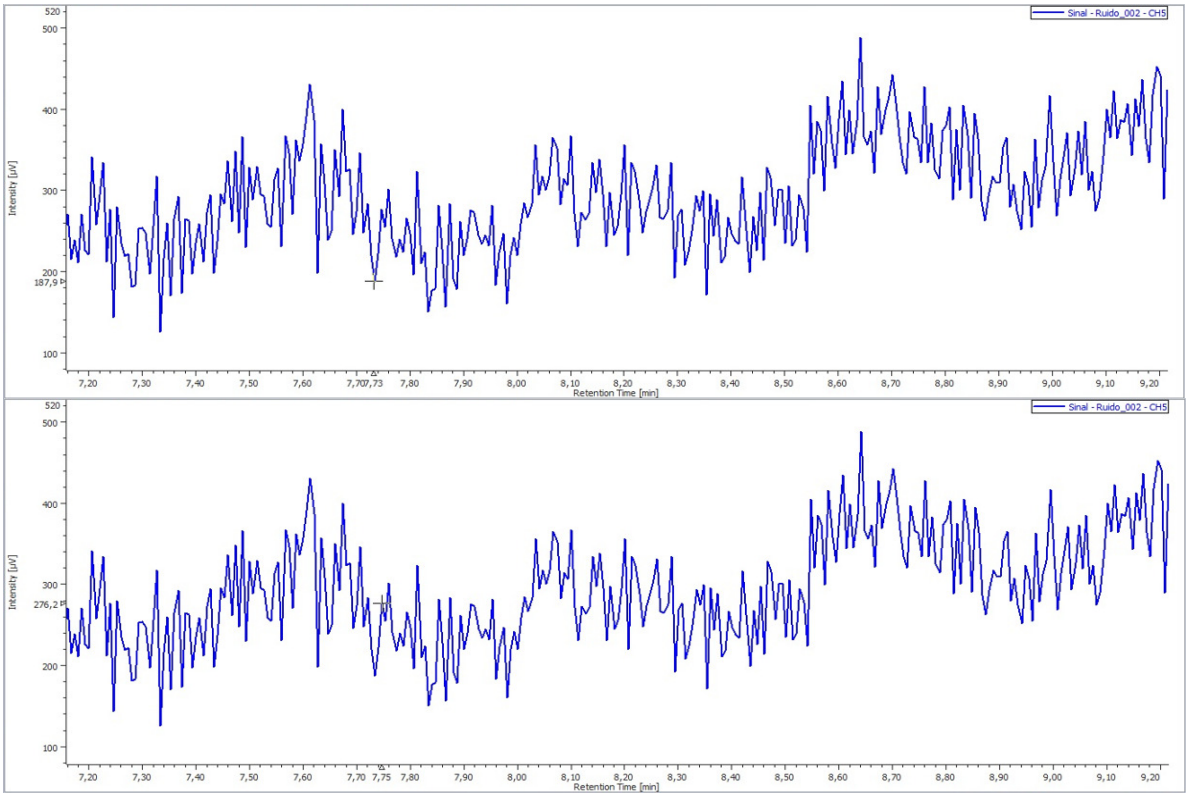


Certificado Nº: 149/25 - RELB	Início da Qualificação: 02/04/2025	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	0.36260	1.07919
VALOR MÍNIMO:	0.00287	
Resultado:	0.35973	

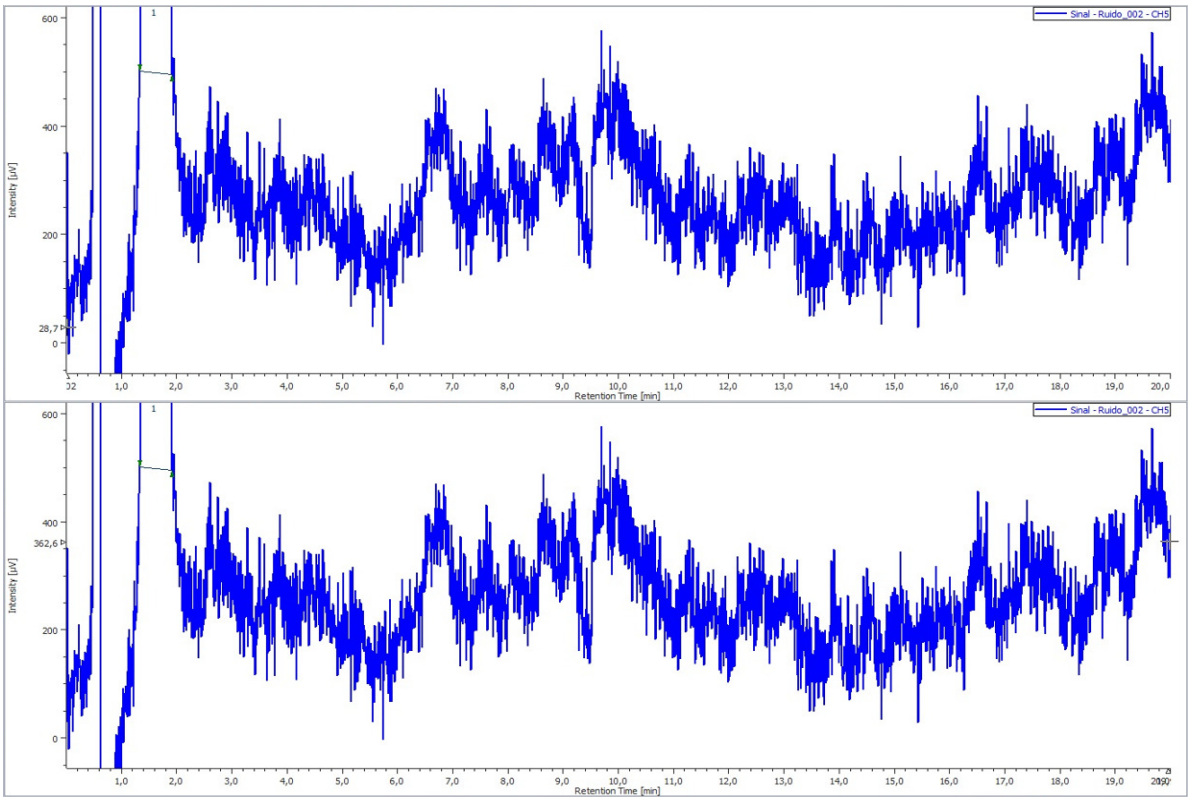

Chromatogram

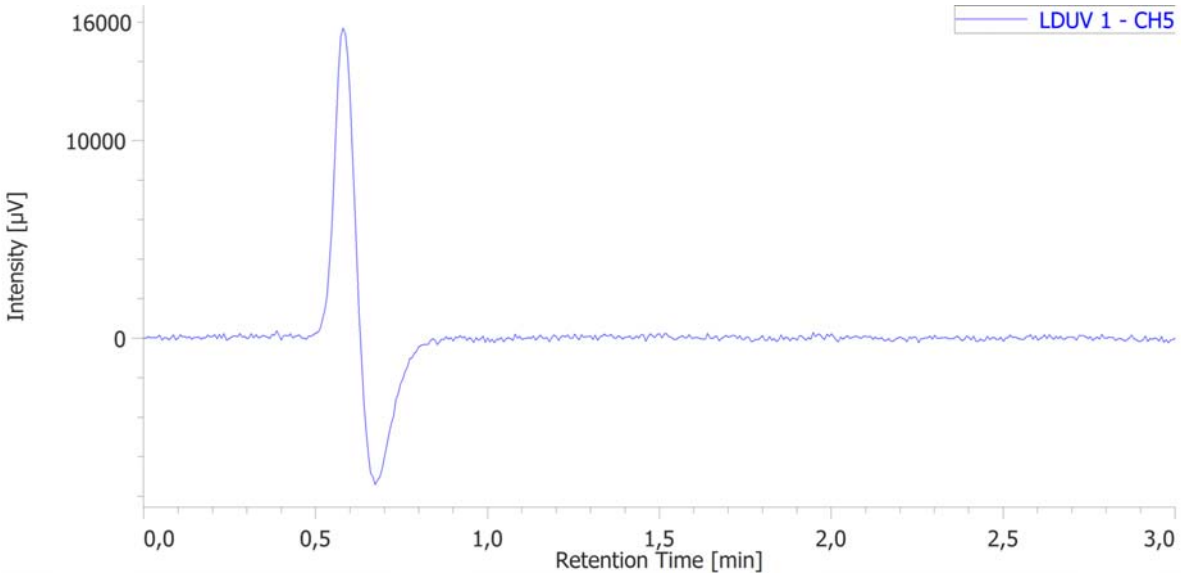


Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:02:52
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 10:36:24
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

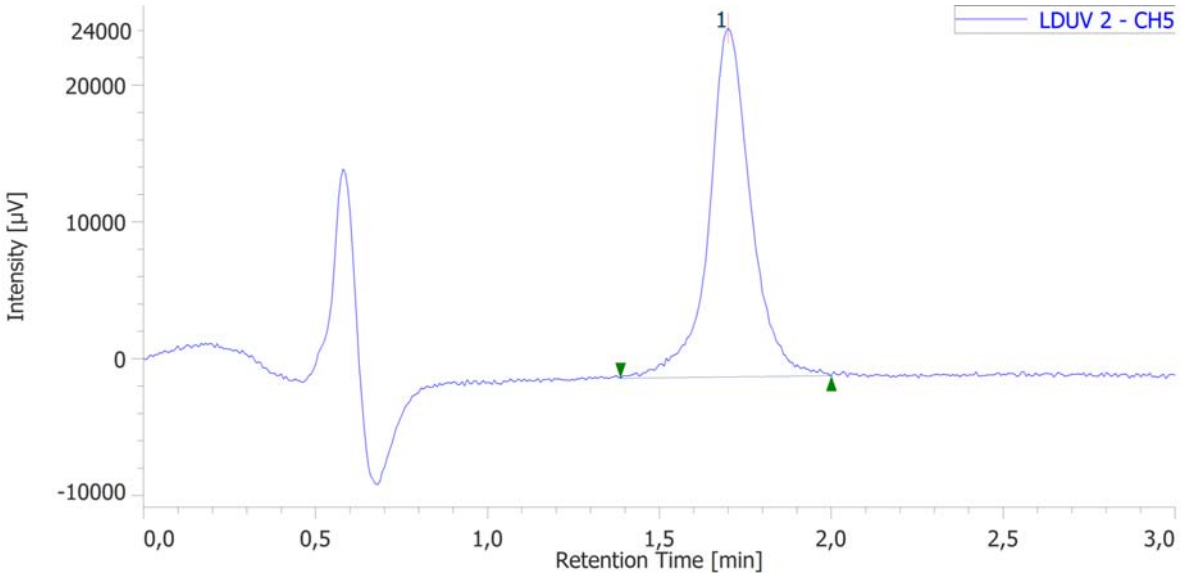

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:02:52
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 10:41:18
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.700	216067	25481	100.000	100.000	N/A	1171	N/A	0.973	

Creator QPackSA
Reviewer
Approver

Chromatogram

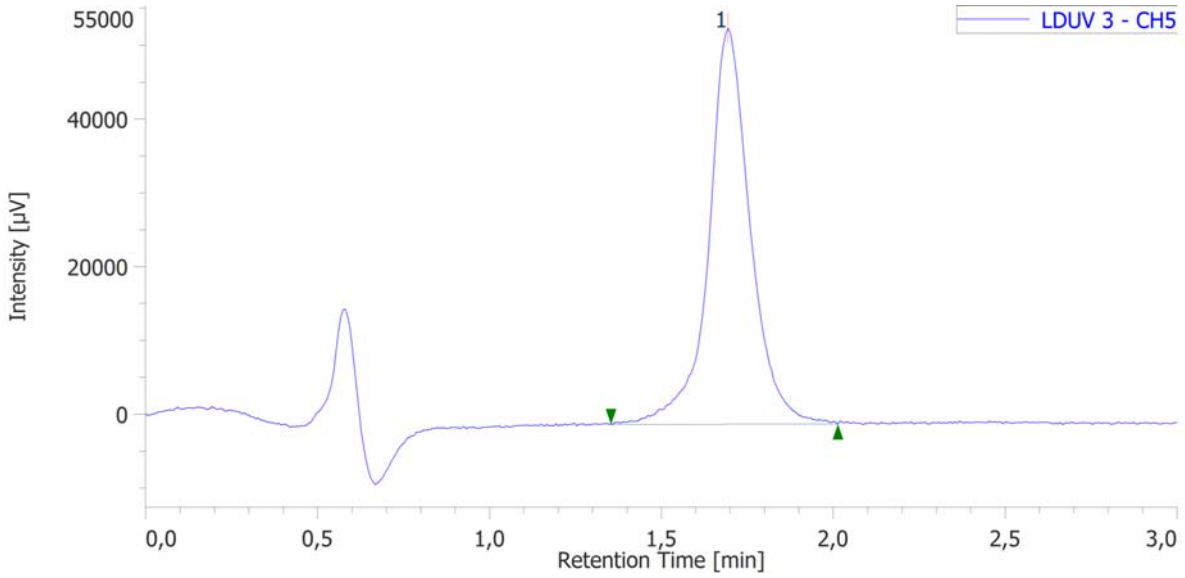

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:02:52
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 10:46:12
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.693	451448	53635	100.000	100.000	N/A	1158	N/A	0.994	

Creator QPackSA
Reviewer
Approver

Chromatogram

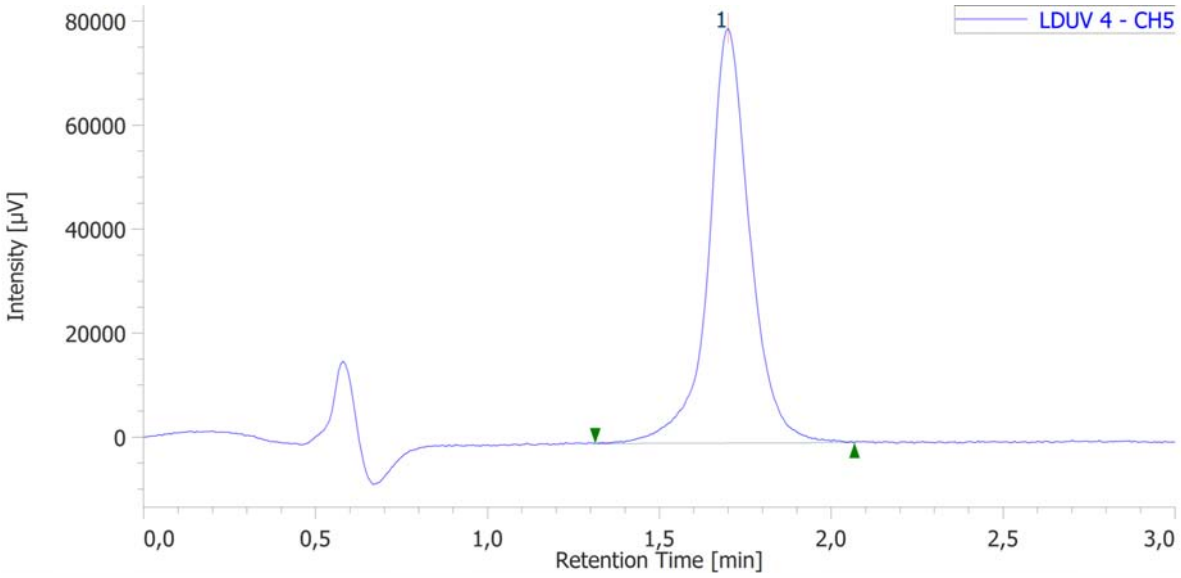

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:02:52
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 10:51:06
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.700	667780	79736	100.000	100.000	N/A	1179	N/A	0.989	

Creator QPackSA
Reviewer
Approver

Chromatogram

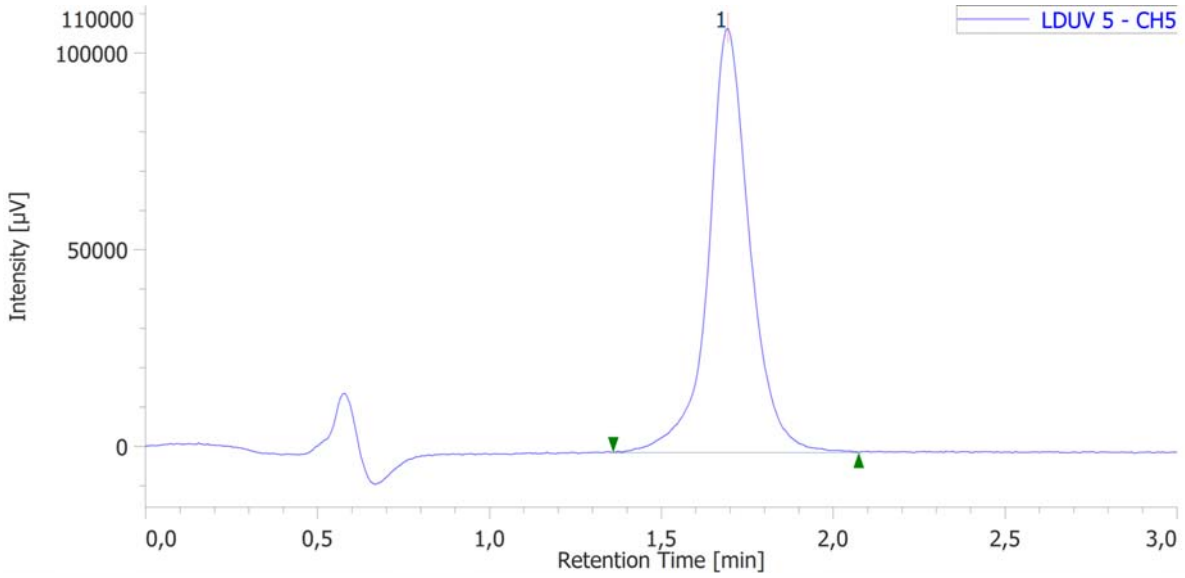

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:02:52
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 10:56:02
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.693	902614	107836	100.000	100.000	N/A	1164	N/A	0.999	

Creator QPackSA
Reviewer
Approver

Chromatogram

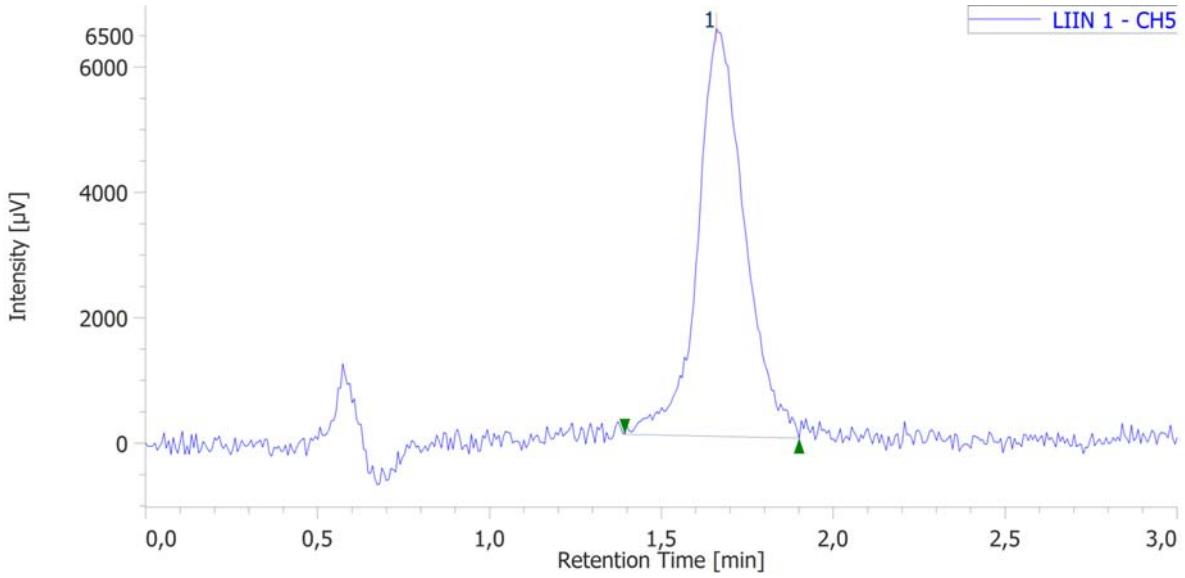

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:10:53
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 11:07:51
Volume	1.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.660	61571	6503	100.000	100.000	N/A	820	N/A	1.113	

Creator QPackSA
Reviewer
Approver

Chromatogram

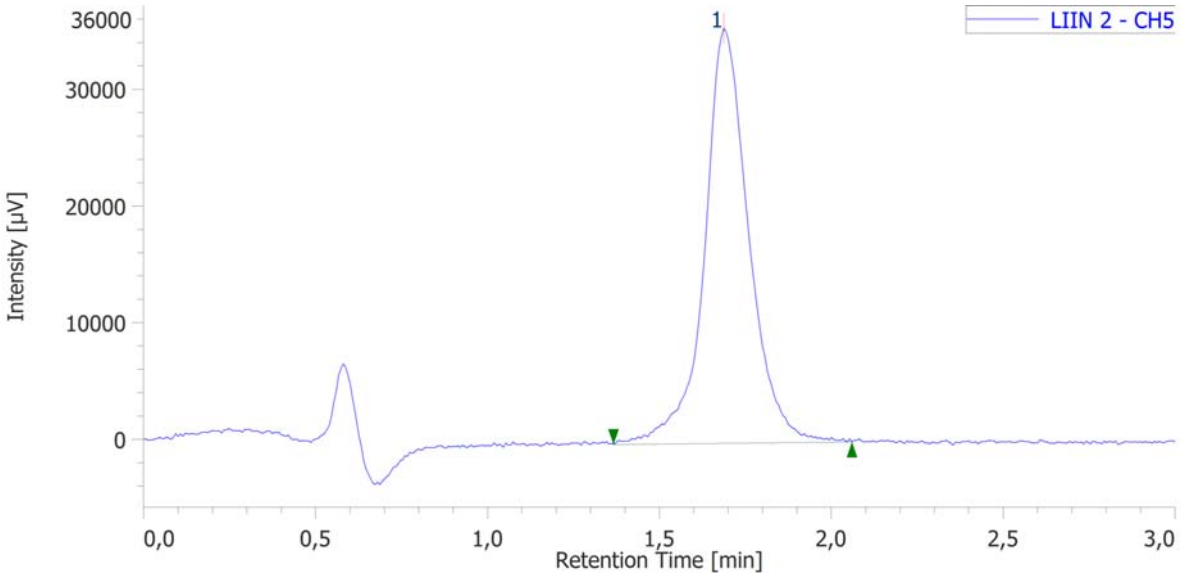

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:15:41
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 11:12:38
Volume	5.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.687	318324	35542	100.000	100.000	N/A	991	N/A	1.042	

Creator QPackSA
Reviewer
Approver

Chromatogram

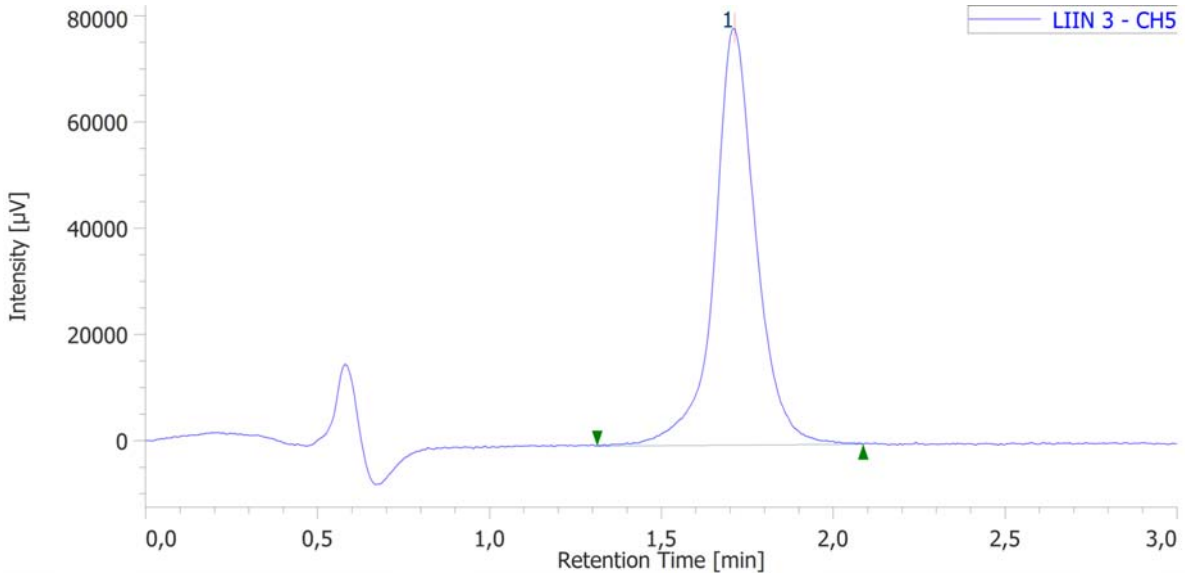

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:20:31
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 11:17:30
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.713	660068	78455	100.000	100.000	N/A	1193	N/A	0.968	

Creator QPackSA
Reviewer
Approver

Chromatogram

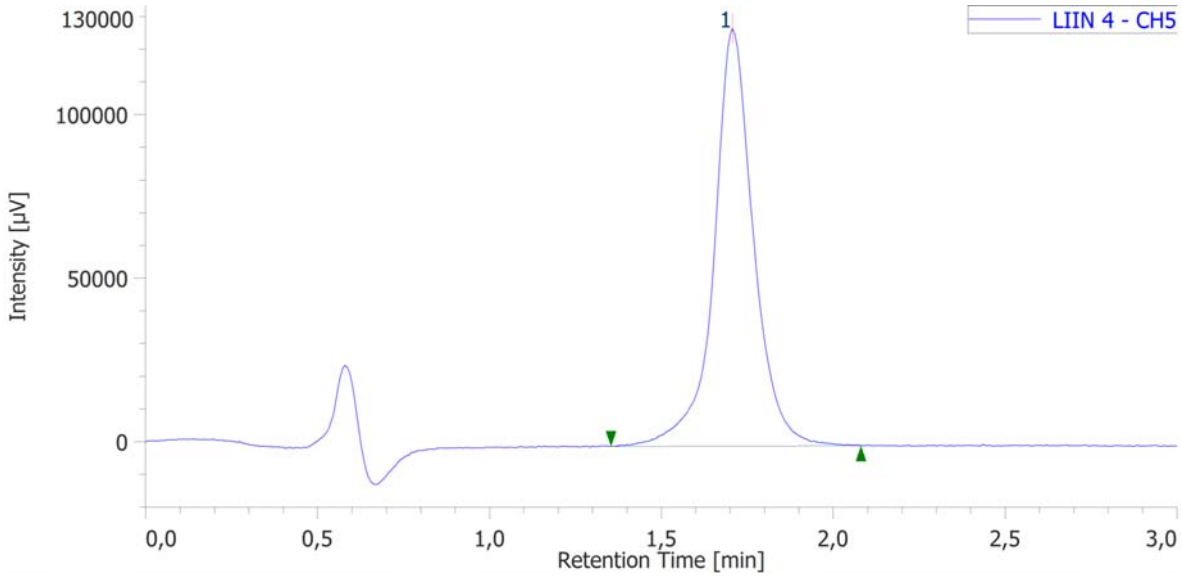

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:25:29
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 11:22:26
Volume	15.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.707	1024029	127730	100.000	100.000	N/A	1300	N/A	0.987	

Creator QPackSA
Reviewer
Approver

Chromatogram

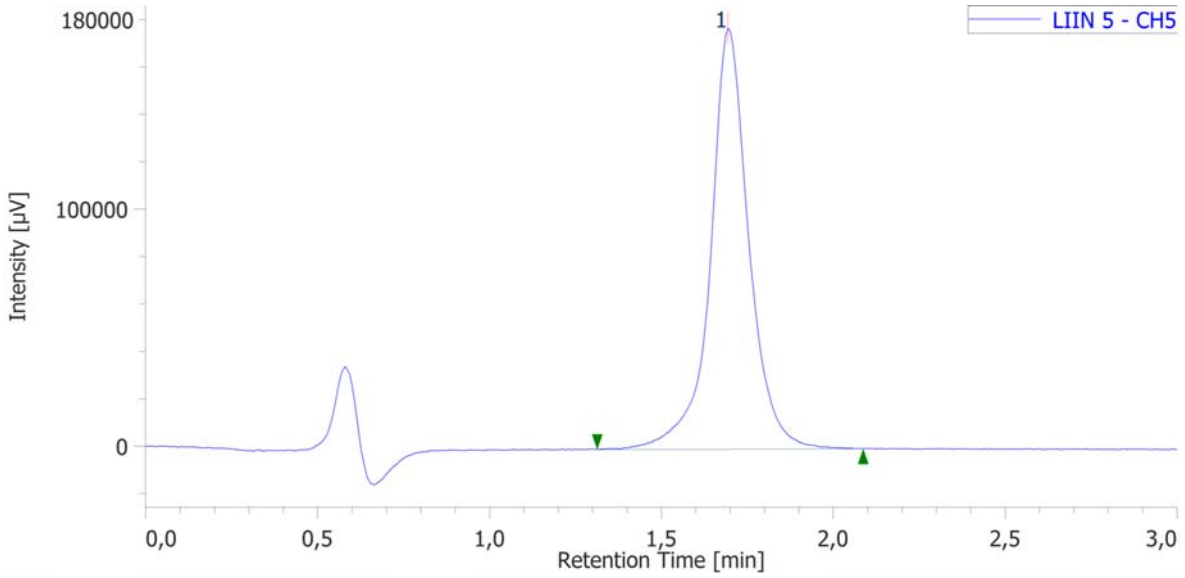

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 11:30:29
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 11:27:27
Volume	20.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	400 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.693	1383812	177467	100.000	100.000	N/A	1370	N/A	0.987	

Creator QPackSA
Reviewer
Approver

Chromatogram

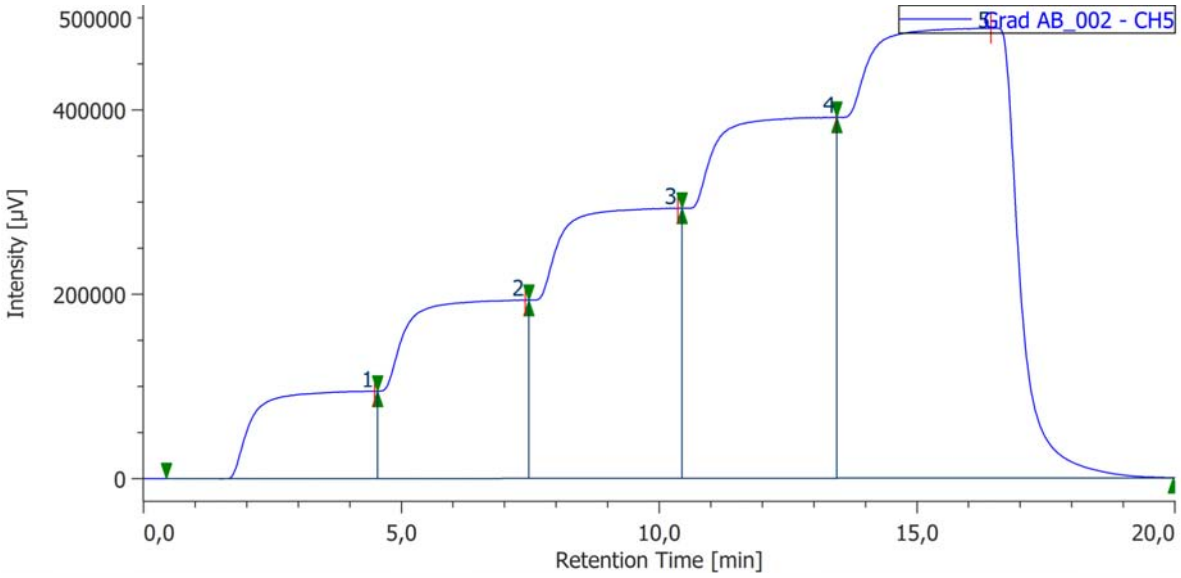

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 15:19:05
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 14:57:29
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	GRAD
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,480	13936362	94638	5,310	6,484	N/A	N/A	N/A	N/A	
2	40%	5	7,400	30887445	193229	11,769	13,238	N/A	N/A	N/A	N/A	
3	60%	5	10,360	48671258	292693	18,546	20,052	N/A	N/A	N/A	N/A	
4	80%	5	13,427	66780415	391262	25,446	26,805	N/A	N/A	N/A	N/A	
5	100%	5	16,427	102161060	487835	38,928	33,421	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

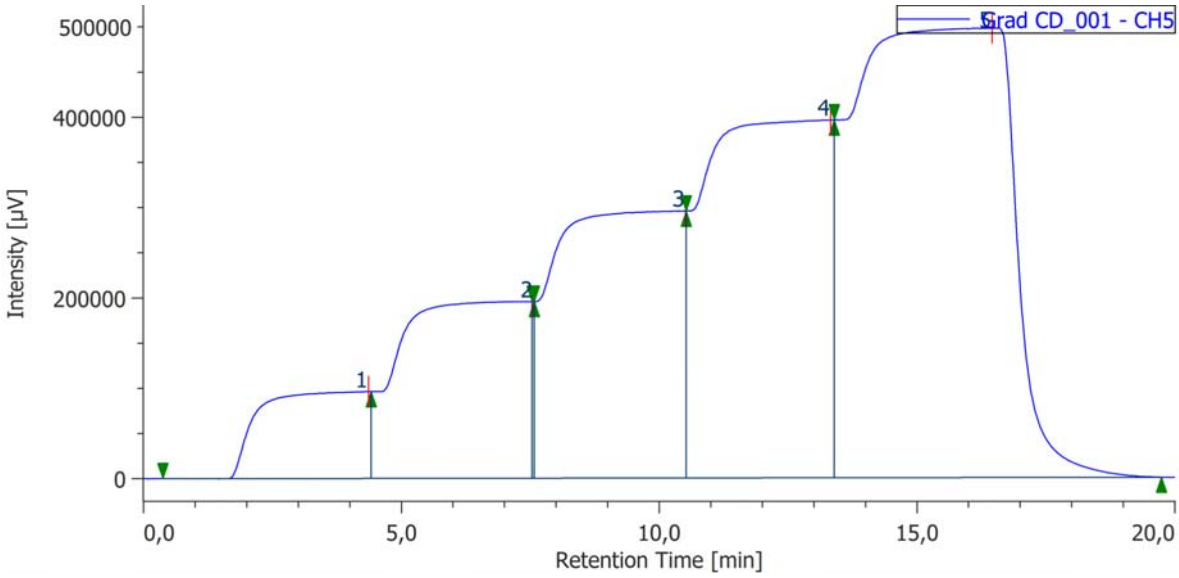

Chromatogram Information	
User Name	QPackSA
Date Modified	03/04/2025 15:59:55
Description	
HPLC System Name	11.XI.05
Injection Date	03/04/2025 15:37:26
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	GRAD
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,360	13402273	95981	5,751	6,489	N/A	N/A	N/A	N/A	
2	40%	5	7,560	468639	195194	0,201	13,196	N/A	N/A	N/A	N/A	
3	60%	5	10,507	49268027	295318	21,143	19,964	N/A	N/A	N/A	N/A	
4	80%	5	13,320	64818834	395708	27,816	26,751	N/A	N/A	N/A	N/A	
5	100%	5	16,453	105068140	497024	45,089	33,600	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver