


HPLC SALMIX - Agilent Lab Advisor
Agilent Lab Advisor for LC & CE
Service & Diagnostics
Basic Version
Tasks
Spectral scan
HPLC SALMIX » HPLC SALMIX » G1365D:DEAAZ01095
Lab Advisor
System Overview
Configuration
Apps
Firmware Update
Logs & Results
HPLC SALMIX
Service & Diagnostics
Instrument Control
EMFs
System Report
Help
Context Help (F1)
Help Topics
What's New?
Spectral Scan - 1260 MWD VL [DEAAZ01095]
UV Lamp On
Sample Scan
from 200
to 300
step 1.0
Export Data
Spectral Scan - 1260 MWD VL [DEAAZ01095]
Absorbance [mAU]
2000
1500
1000
500
200
210
220
230
240
250
260
270
280
290
300
Wavelength [nm]
more...
Print Result
Rerun
Back
Connection Address: 192.168.254.11
Version B.02.04 [093] - Basic | Licenses 8/10
Iniciar
Analises
Microsoft Excel - PLA...
HPLC SALMIX (offline...
HPLC SALMIX - Agil...
PT
4:00 PM
6/25/2019

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0101.D
Sample Name: BR PCIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   1
Acq. Instrument : HPLC SALMIX                     Location :   51
Injection Date  : 6/26/2019 9:04:35 AM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

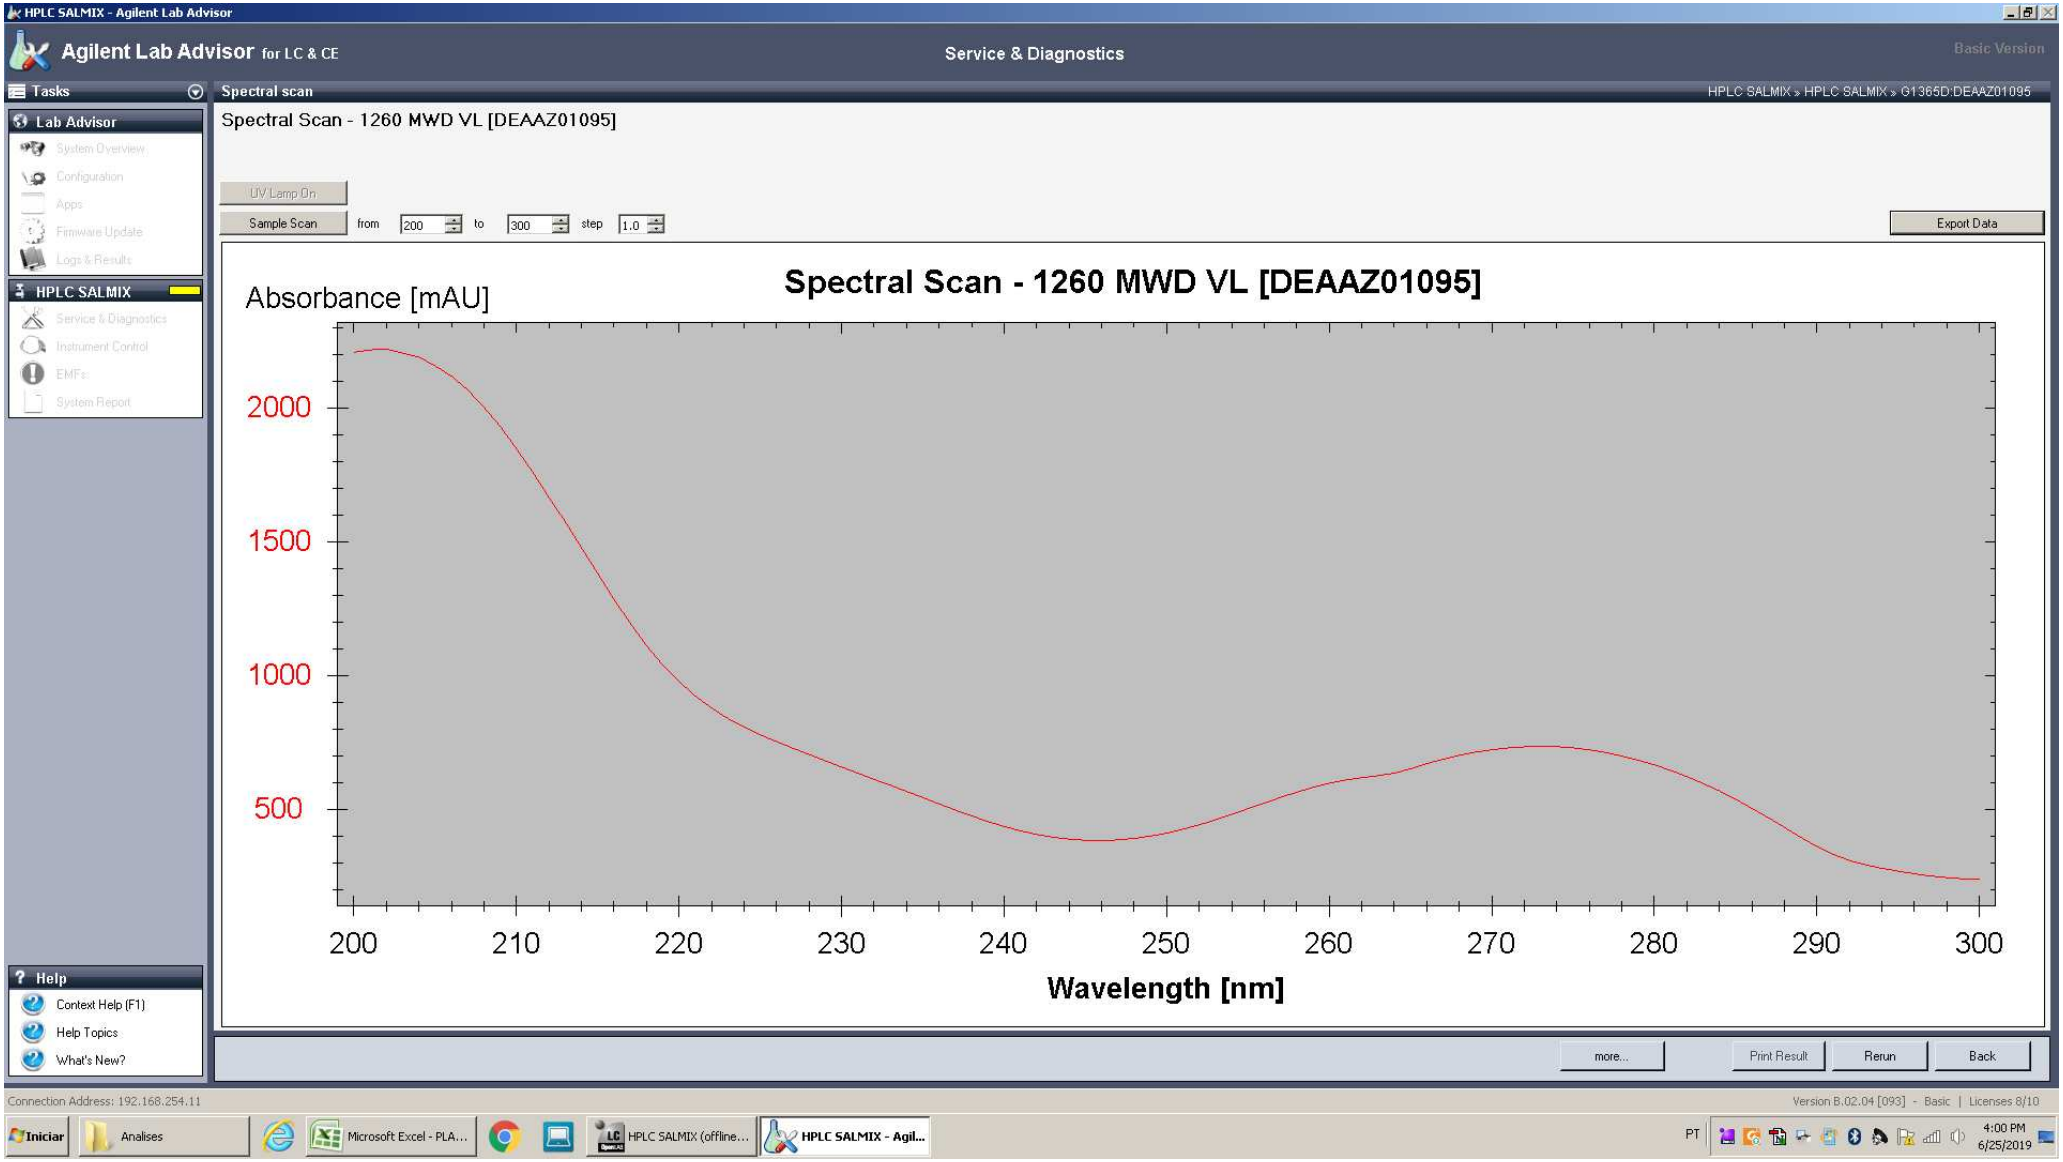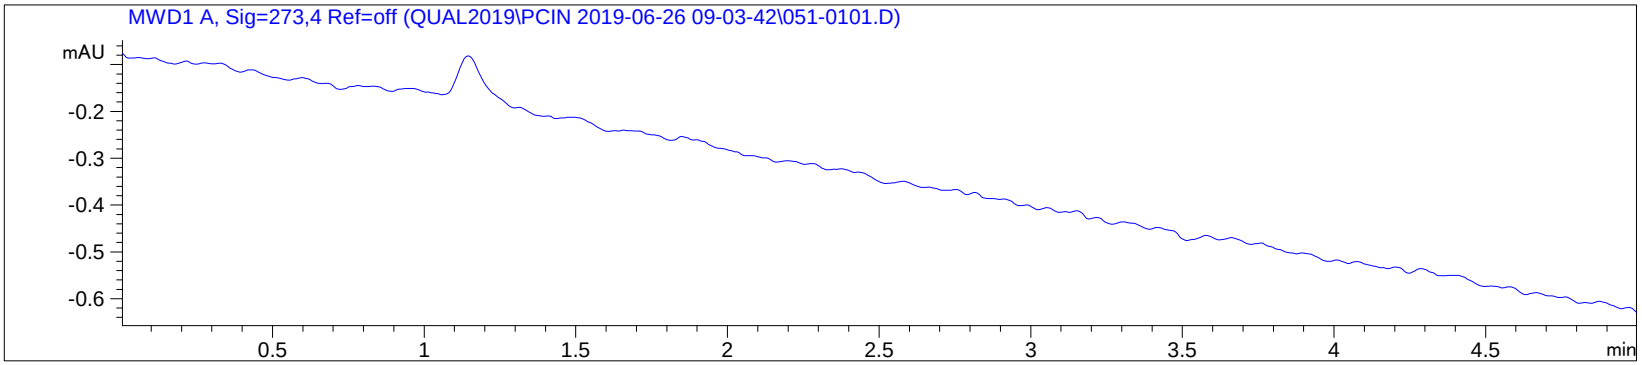


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.541            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0101.D
Sample Name: BR PCIN 001

Warning : Calibrated compound(s) not found

==========
==========
Area Percent Report
==========

Sorted By : Signal
Calib. Data Modified : Wednesday, June 26, 2019 9:39:28 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	2.541		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========
*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0201.D
Sample Name: PCIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   2
Acq. Instrument : HPLC SALMIX                     Location :   52
Injection Date  : 6/26/2019 9:10:34 AM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

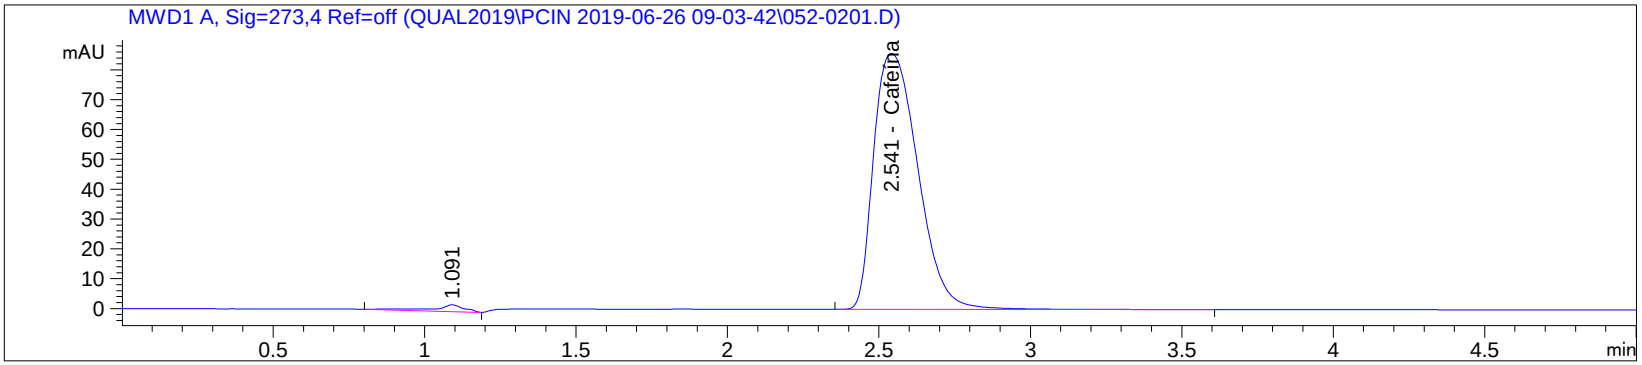


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.541 BB      870.51379 1.14875e-1  100.00000    Cafeína

Totals :                              100.00000


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0301.D
Sample Name: PCIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   3
Acq. Instrument : HPLC SALMIX                       Location :   52
Injection Date  : 6/26/2019 9:16:32 AM                   Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

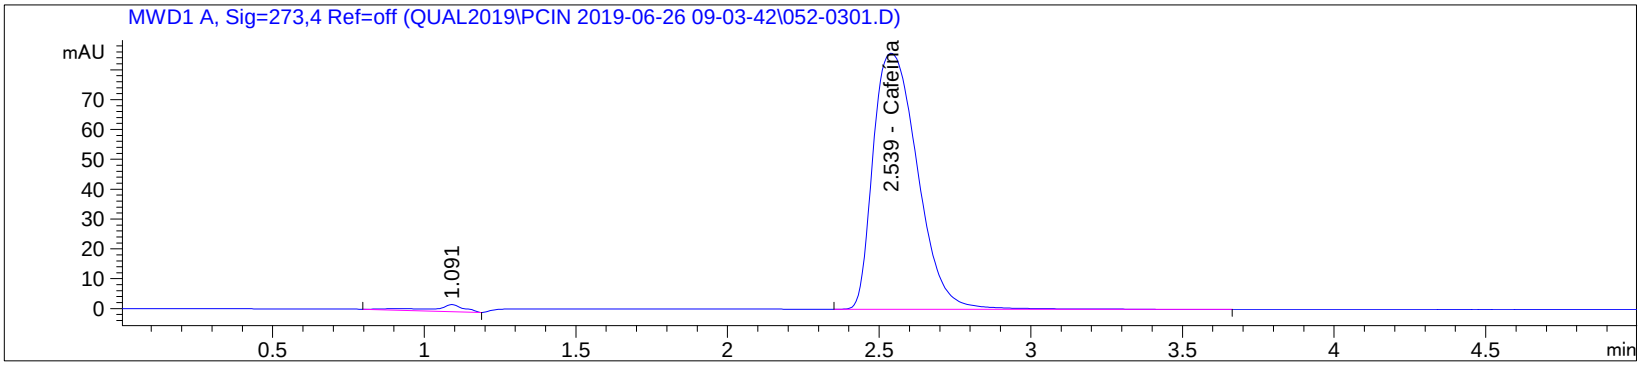


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.539 BB      871.51086 1.14875e-1  100.11454    Cafeína

Totals :                              100.11454


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0401.D
Sample Name: PCIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   4
Acq. Instrument : HPLC SALMIX                       Location :   52
Injection Date  : 6/26/2019 9:22:31 AM                   Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

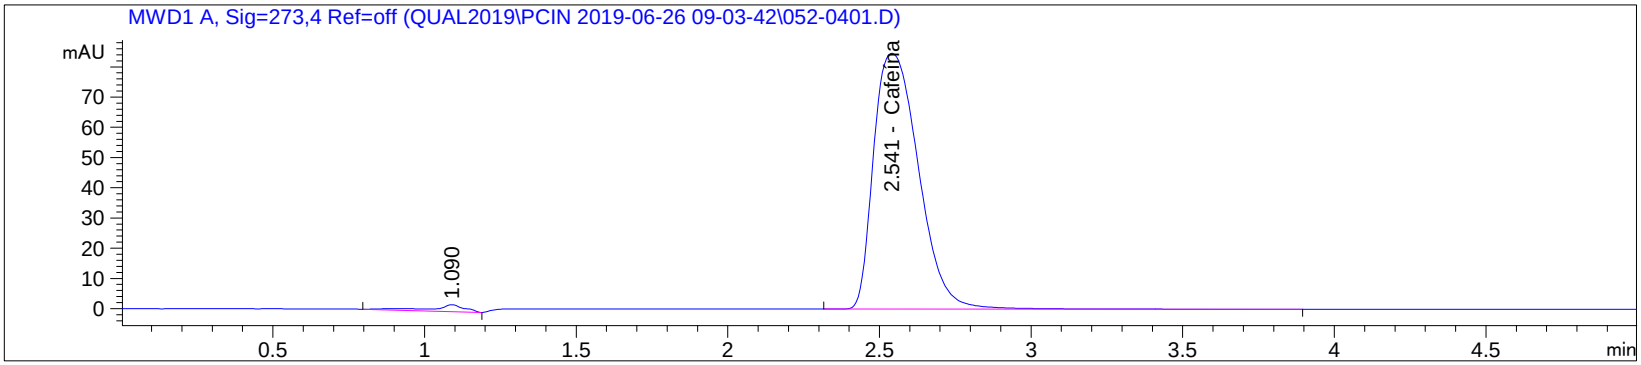


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.541 BB      872.28424 1.14875e-1  100.20338    Cafeína

Totals :                              100.20338


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0501.D
Sample Name: BR PCIN 002

```
================================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   5
Acq. Instrument : HPLC SALMIX                       Location :   51
Injection Date  : 6/26/2019 9:28:31 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

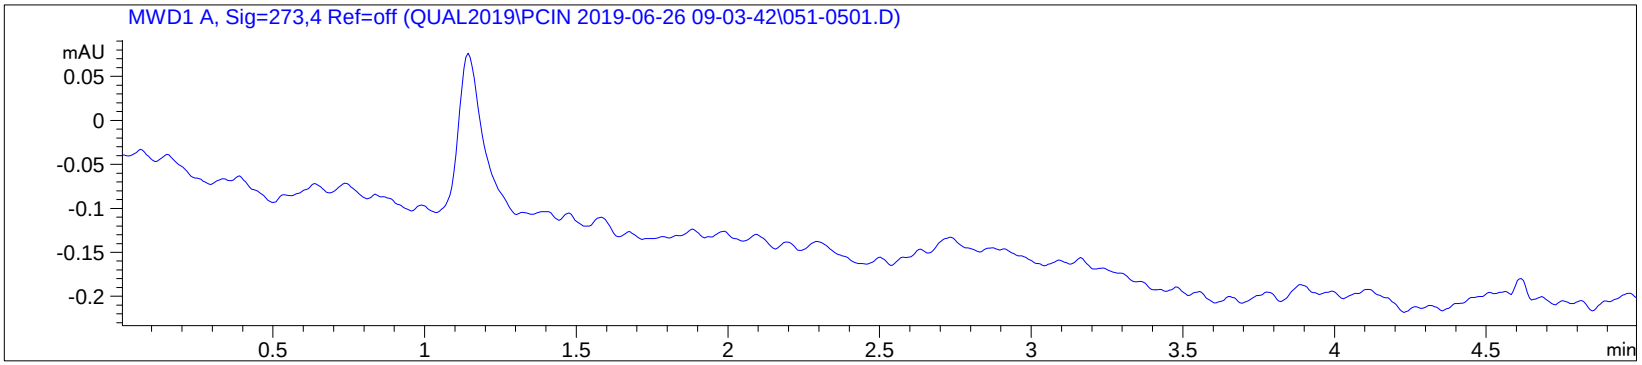


```
================================================================================
                       External Standard Report
================================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.541            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0501.D
Sample Name: BR PCIN 002

Warning : Calibrated compound(s) not found

==========
==========
Area Percent Report
==========

Sorted By : Signal
Calib. Data Modified : Wednesday, June 26, 2019 9:39:28 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	2.541		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========
*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0601.D
Sample Name: PCIN 004

```
==================================================================
Acq. Operator   : SISTEMA                       Seq. Line :   6
Acq. Instrument : HPLC SALMIX                    Location :   52
Injection Date  : 6/26/2019 9:34:31 AM                Inj :   1
                                               Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

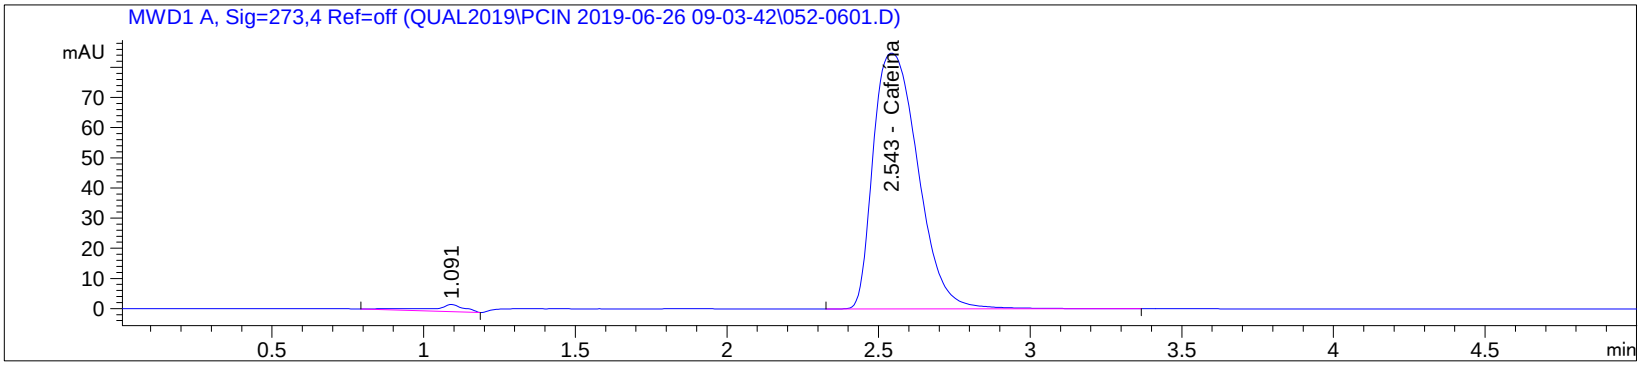


```
==================================================================
                      External Standard Report
==================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.543 BB      871.21173 1.14875e-1  100.08018    Cafeína

Totals :                              100.08018


==================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0701.D
Sample Name: PCIN 005

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   7
Acq. Instrument : HPLC SALMIX                     Location :   52
Injection Date  : 6/26/2019 9:40:30 AM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

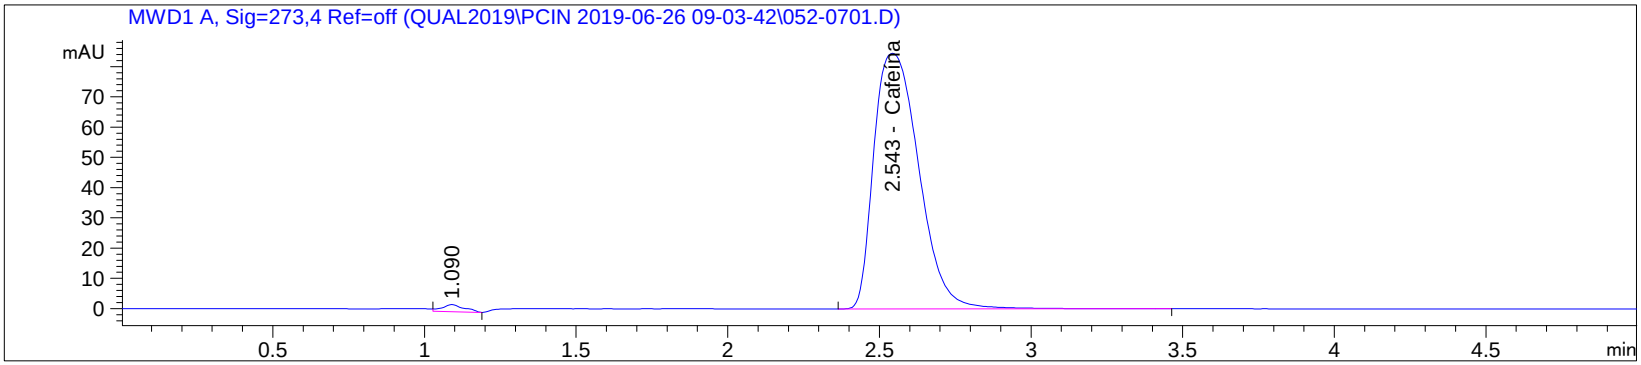


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.543 BB      872.40527 1.14875e-1  100.21728    Cafeína

Totals :                              100.21728


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\052-0801.D
Sample Name: PCIN 006

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   8
Acq. Instrument : HPLC SALMIX                       Location :   52
Injection Date  : 6/26/2019 9:46:28 AM                   Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

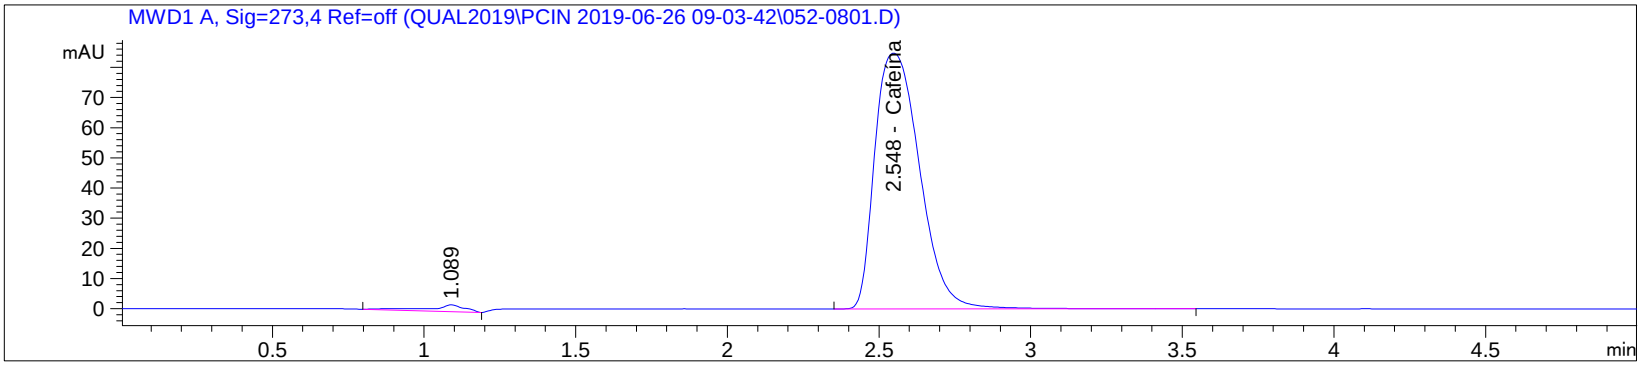


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  2.548 BB      871.96045 1.14875e-1  100.16618    Cafeína

Totals :                              100.16618


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0901.D
Sample Name: BR PCIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   9
Acq. Instrument : HPLC SALMIX                     Location :   51
Injection Date  : 6/26/2019 9:52:29 AM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M
Last changed    : 6/26/2019 9:03:42 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\QP_NOITE.M (Sequence Method)
Last changed    : 6/26/2019 10:10:49 AM by SISTEMA
                  (modified after loading)
```

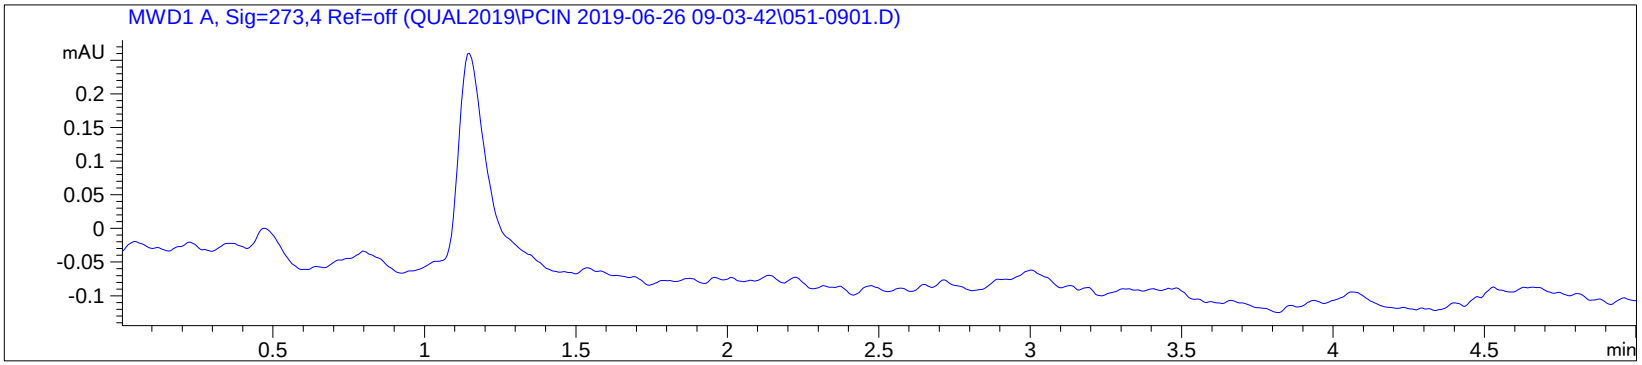


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 9:39:28 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.541            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :
```

Data File C:\Chem32\1\DATA\QUAL2019\PCIN 2019-06-26 09-03-42\051-0901.D
Sample Name: BR PCIN 003

Warning : Calibrated compound(s) not found

==========
==========
Area Percent Report
==========

Sorted By : Signal
Calib. Data Modified : Wednesday, June 26, 2019 9:39:28 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	2.541		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========
*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\053-0101.D
Sample Name: LDUV 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   1
Acq. Instrument : HPLC SALMIX                     Location :   53
Injection Date  : 6/26/2019 10:00:08 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M
Last changed    : 6/26/2019 9:59:11 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:14:53 AM by SISTEMA
                  (modified after loading)
```

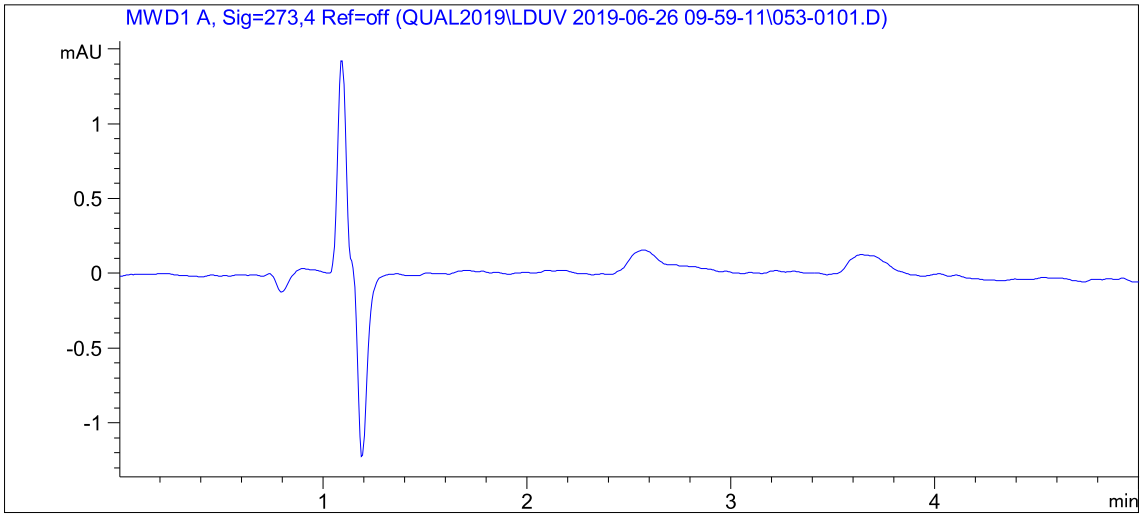


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      6/26/2019 10:14:32 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area      Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.556            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\053-0101.D
Sample Name: LDUV 001

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : 6/26/2019 10:14:32 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	2.556		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found


==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\054-0201.D
Sample Name: LDUV 002

==========

Acq. Operator : SISTEMA Seq. Line : 2
Acq. Instrument : HPLC SALMIX Location : 54
Injection Date : 6/26/2019 10:06:10 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M
Last changed : 6/26/2019 9:59:11 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M (Sequence Method)
Last changed : 6/26/2019 10:14:53 AM by SISTEMA
(modified after loading)

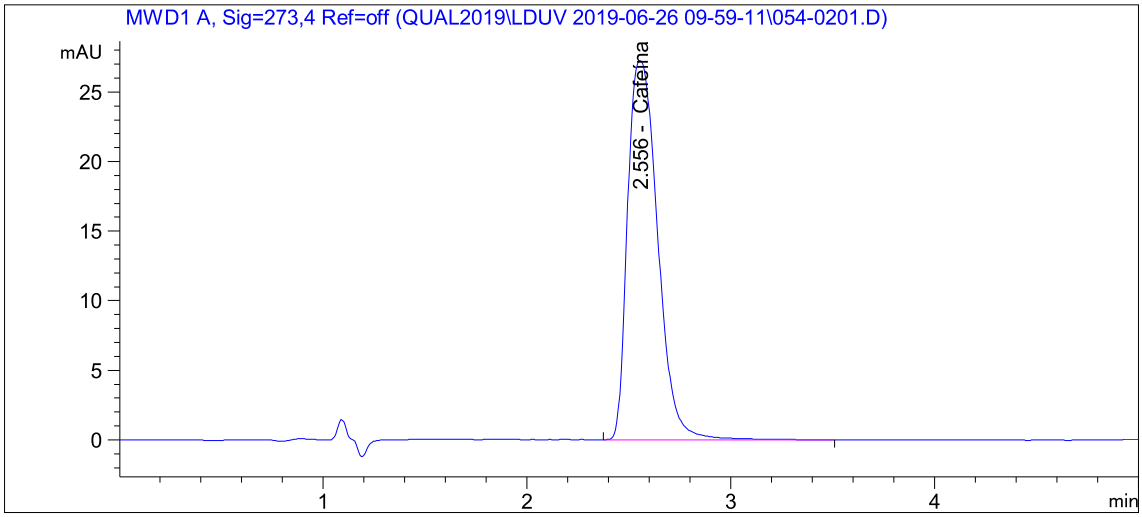

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : 6/26/2019 10:14:32 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.556	BB	279.15002	3.58230e-1	100.00000		Cafeína

Totals : 100.00000


==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\055-0301.D
Sample Name: LDUV 003

==========

Acq. Operator : SISTEMA Seq. Line : 3
Acq. Instrument : HPLC SALMIX Location : 55
Injection Date : 6/26/2019 10:12:15 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M
Last changed : 6/26/2019 9:59:11 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M (Sequence Method)
Last changed : 6/26/2019 10:14:53 AM by SISTEMA
(modified after loading)

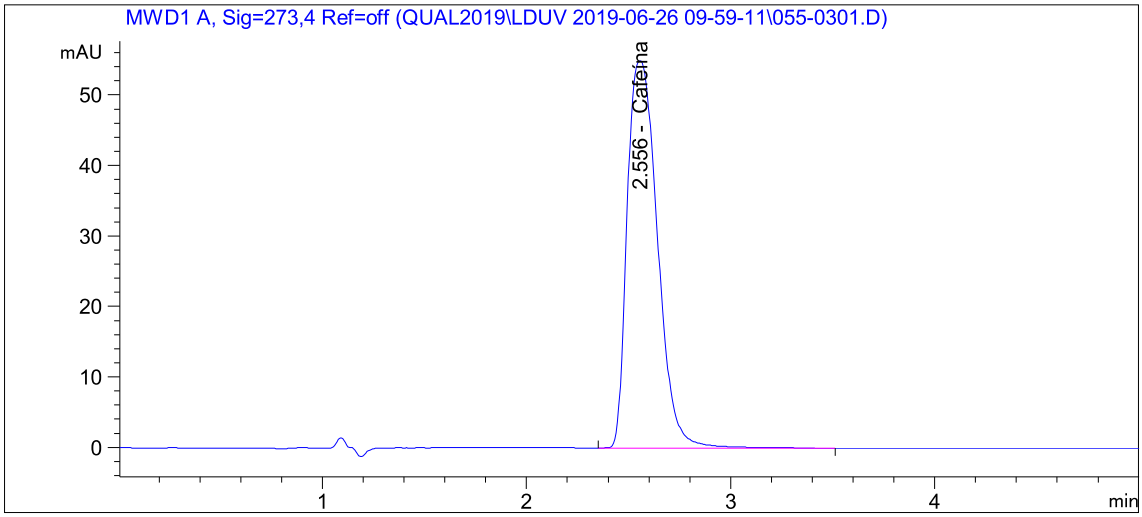

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : 6/26/2019 10:14:32 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.556	BB	564.83191	3.58230e-1	202.33991		Cafeína

Totals : 202.33991


==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\056-0401.D
Sample Name: LDUV 004

==========

Acq. Operator : SISTEMA Seq. Line : 4
Acq. Instrument : HPLC SALMIX Location : 56
Injection Date : 6/26/2019 10:18:17 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M
Last changed : 6/26/2019 9:59:11 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M (Sequence Method)
Last changed : 6/26/2019 10:14:53 AM by SISTEMA
(modified after loading)

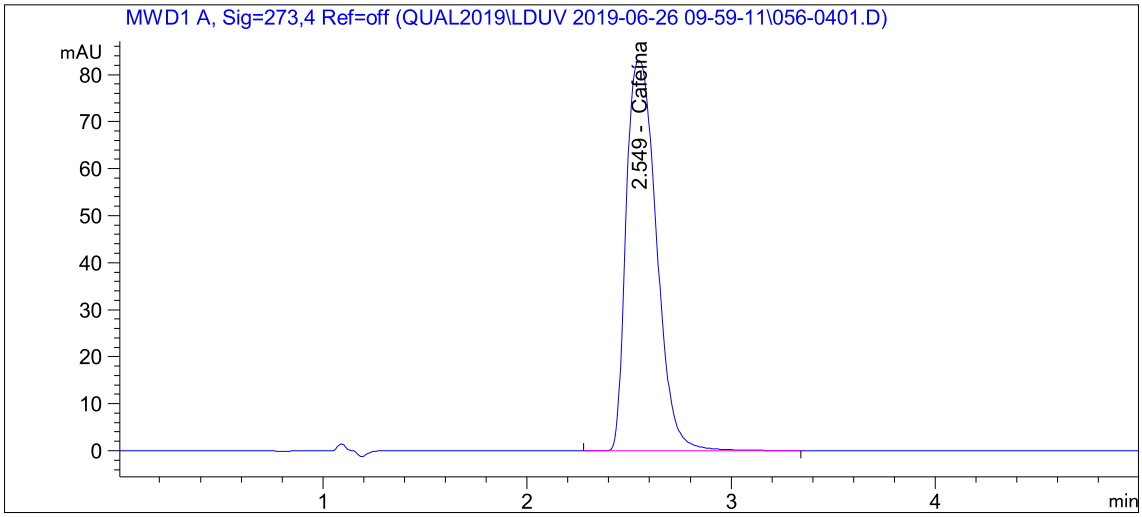

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : 6/26/2019 10:14:32 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.549	BB	852.83618	3.58230e-1	305.51177		Cafeína


Totals : 305.51177

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\057-0501.D
Sample Name: LDUV 005

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   5
Acq. Instrument : HPLC SALMIX                     Location :   57
Injection Date  : 6/26/2019 10:24:19 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M
Last changed    : 6/26/2019 9:59:11 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LDUV 2019-06-26 09-59-11\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:14:53 AM by SISTEMA
                  (modified after loading)
```

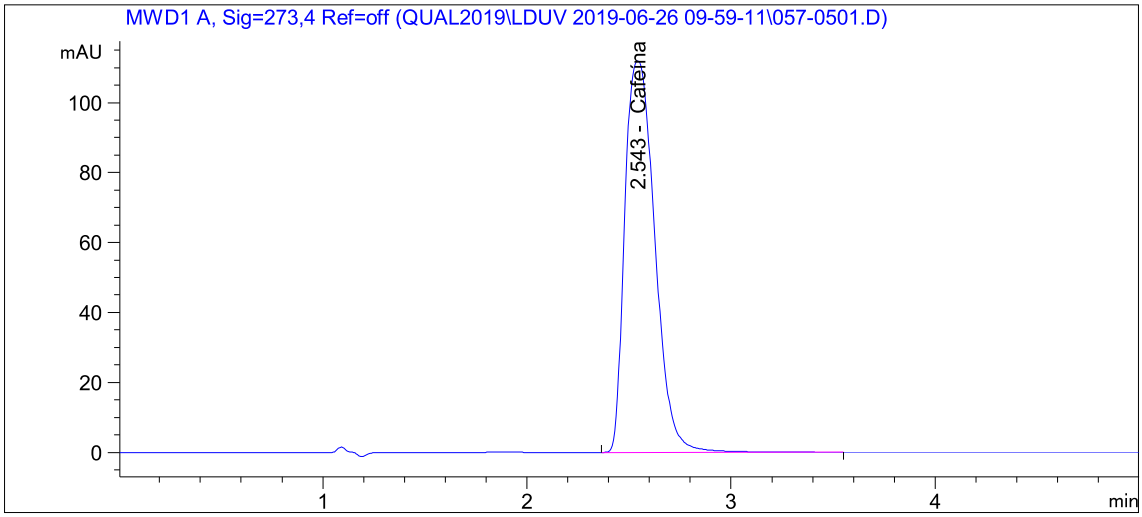


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      6/26/2019 10:14:32 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.543 BB     1141.35010 3.58230e-1  408.86620    Cafeína

Totals :                               408.86620


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0101.D
Sample Name: LIIN 001

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   1
Acq. Instrument : HPLC SALMIX                     Location :   58
Injection Date  : 6/26/2019 10:31:51 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M
Last changed    : 6/26/2019 10:31:35 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:43:51 AM by SISTEMA
                  (modified after loading)
```

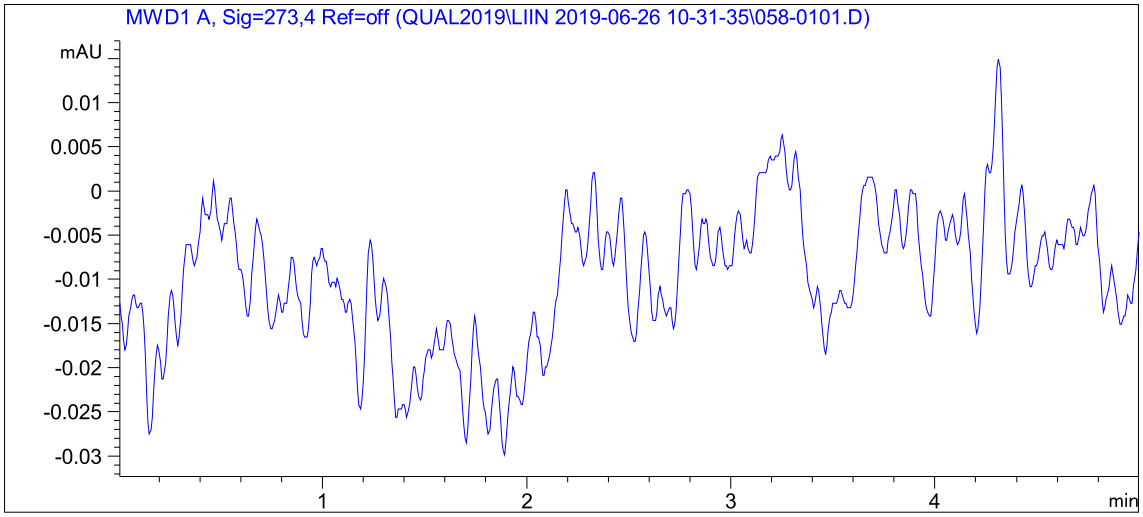


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 10:43:24 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.546            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0101.D
Sample Name: LIIN 001

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, June 26, 2019 10:43:24 AM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	2.546		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0201.D
Sample Name: LIIN 002

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   2
Acq. Instrument : HPLC SALMIX                     Location :   58
Injection Date  : 6/26/2019 10:37:51 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 5.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M
Last changed    : 6/26/2019 10:31:35 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:43:51 AM by SISTEMA
                  (modified after loading)
```

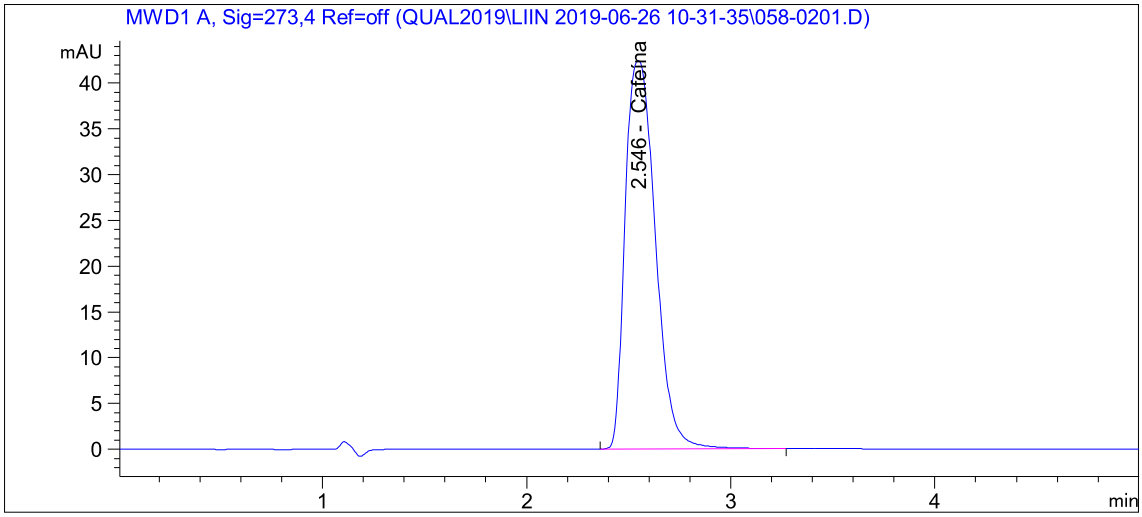


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 10:43:24 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.546 BB      435.24323 2.29757e-1  100.00000    Cafeína

Totals :                              100.00000


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0301.D
Sample Name: LIIN 003

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   3
Acq. Instrument : HPLC SALMIX                     Location :   58
Injection Date  : 6/26/2019 10:43:50 AM               Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M
Last changed    : 6/26/2019 10:31:35 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:43:51 AM by SISTEMA
                  (modified after loading)
```

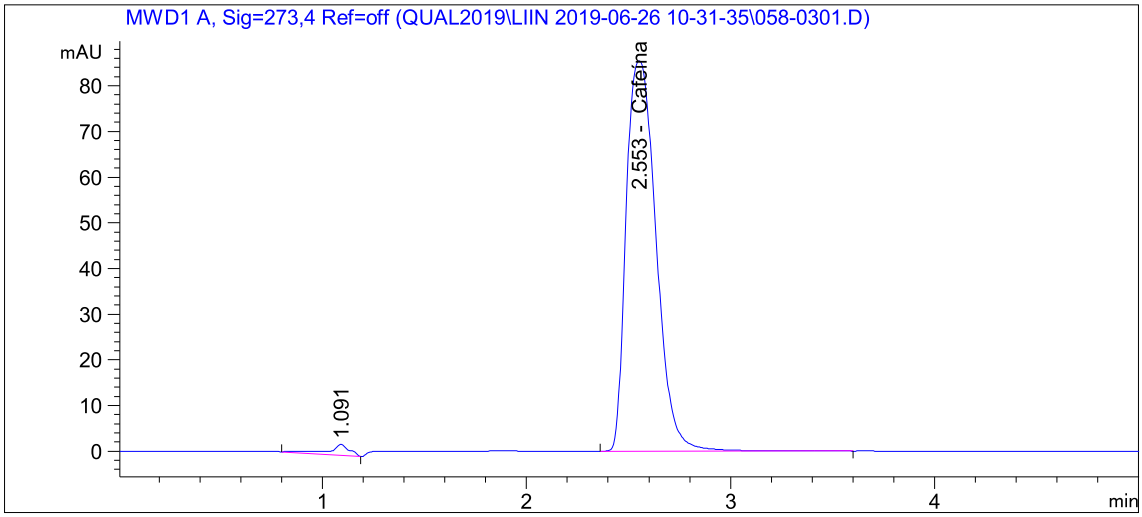


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 10:43:24 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area      Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]                [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.553 BB      868.71814 2.29757e-1  199.59372    Cafeína

Totals :                              199.59372


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0401.D
Sample Name: LIIN 004

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   4
Acq. Instrument : HPLC SALMIX                       Location :   58
Injection Date  : 6/26/2019 10:49:52 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M
Last changed    : 6/26/2019 10:31:35 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:43:51 AM by SISTEMA
                  (modified after loading)
```

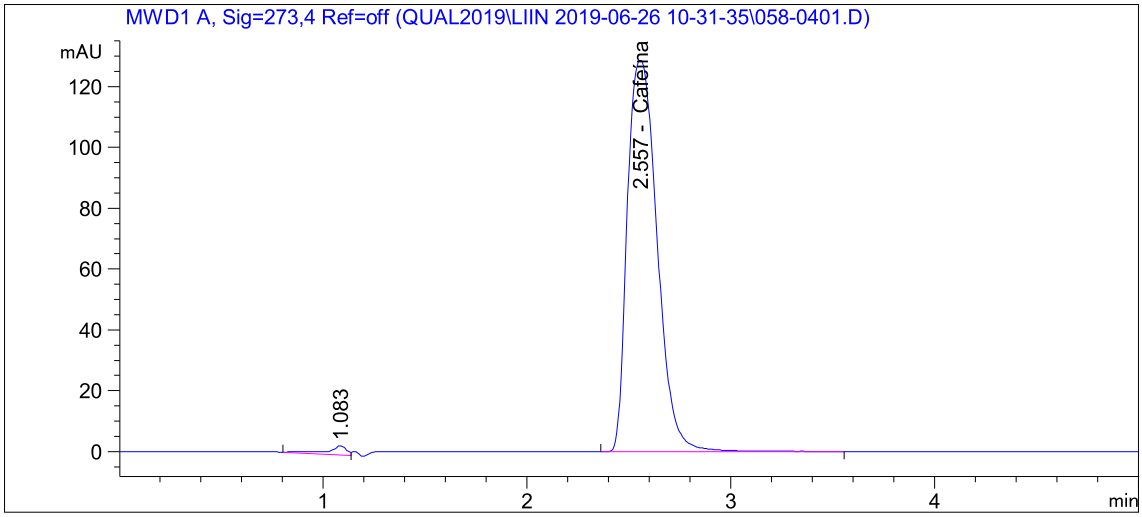


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 10:43:24 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.557 BB     1304.49719 2.29757e-1  299.71683    Cafeína

Totals :                              299.71683


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\058-0501.D
Sample Name: LIIN 005

```
==========================================================================
Acq. Operator   : SISTEMA                        Seq. Line :   5
Acq. Instrument : HPLC SALMIX                     Location :   58
Injection Date  : 6/26/2019 10:55:58 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Acq. Method     : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M
Last changed    : 6/26/2019 10:31:35 AM by SISTEMA
Analysis Method : C:\Chem32\1\DATA\QUAL2019\LIIN 2019-06-26 10-31-35\QP_NOITE.M (Sequence
                  Method)
Last changed    : 6/26/2019 10:43:51 AM by SISTEMA
                  (modified after loading)
```

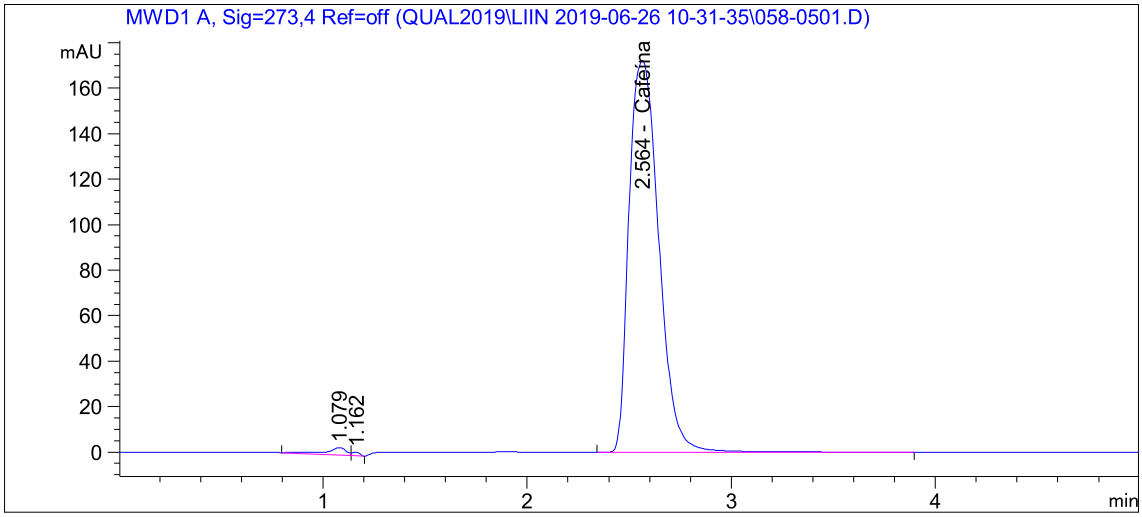


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, June 26, 2019 10:43:24 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=273,4 Ref=off


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  2.564 BB     1741.13464 2.29757e-1  400.03716    Cafeína

Totals :                              400.03716


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\DATA\QUAL2019\GRAD 2019-06-26 11-20-53\051-0101.D
Sample Name: GRAD AB

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   1
Acq. Instrument : HPLC SALMIX                       Location :   51
Injection Date  : 6/26/2019 11:21:10 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Method          : C:\Chem32\1\DATA\QUAL2019\GRAD 2019-06-26 11-20-53\GRAD AB.M (Sequence
                  Method)
Last changed    : 6/26/2019 11:20:53 AM by SISTEMA
Additional Info : Peak(s) manually integrated
```

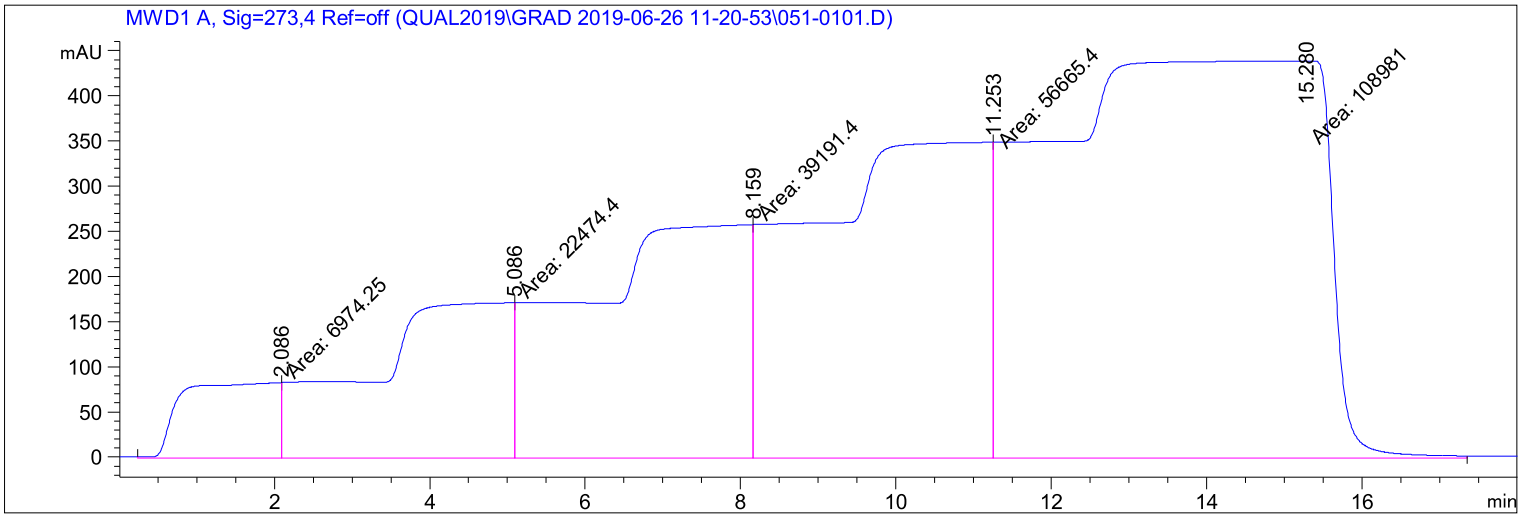


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   2.086 MF    1.3956 6974.24561   83.29090   2.9768
   2   5.086 FM    2.1814 2.24744e4   171.71463   9.5927
   3   8.159 FM    2.5291 3.91914e4   258.26678  16.7279
   4  11.253 FM    2.7032 5.66654e4   349.37079  24.1863
   5  15.280 FM    4.1327 1.08981e5   439.50754  46.5162


Totals :                 2.34287e5  1302.15064
```

==========

*** End of Report ***

Data File C:\Chem32\1\DATA\QUAL2019\GRAD 2019-06-26 11-20-53\051-0201.D
Sample Name: GRAD CD

```
==========================================================================
Acq. Operator   : SISTEMA                          Seq. Line :   2
Acq. Instrument : HPLC SALMIX                       Location :   51
Injection Date  : 6/26/2019 11:39:35 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Method          : C:\Chem32\1\DATA\QUAL2019\GRAD 2019-06-26 11-20-53\GRAD CD.M (Sequence
                  Method)
Last changed    : 6/26/2019 11:20:54 AM by SISTEMA
Additional Info : Peak(s) manually integrated
```

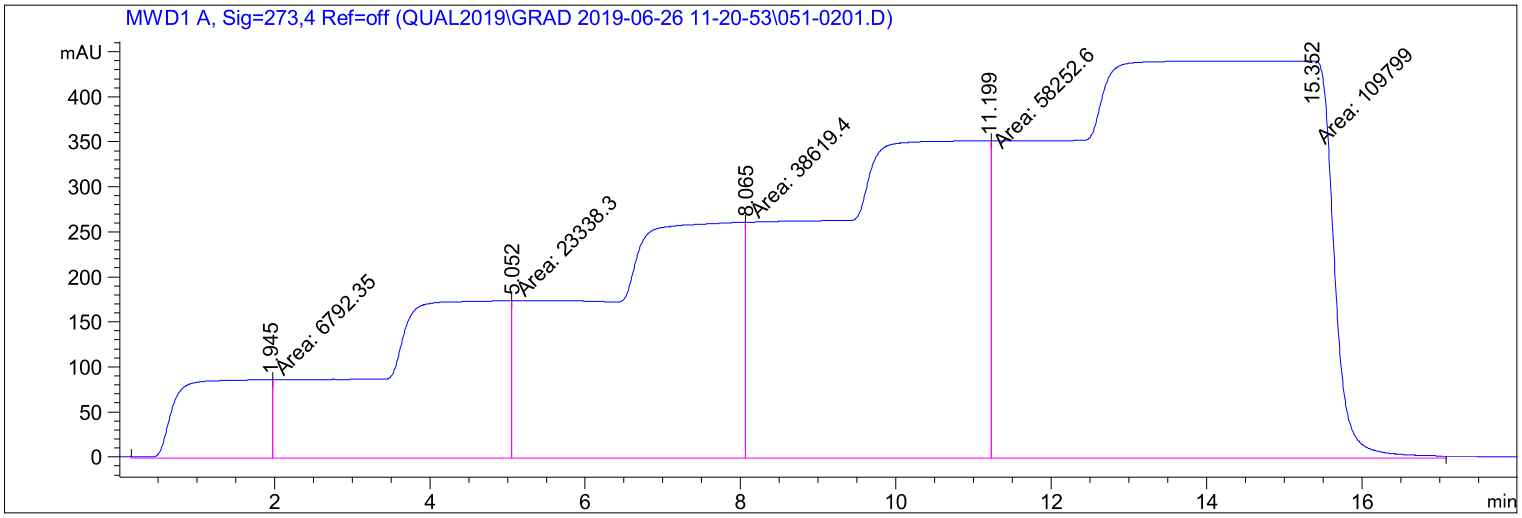


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: MWD1 A, Sig=273,4 Ref=off

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.945 MF    1.3046 6792.34766   86.77237   2.8684
   2   5.052 FM    2.2295 2.33383e4   174.46455   9.8556
   3   8.065 FM    2.4620 3.86194e4   261.44107  16.3088
   4  11.199 FM    2.7582 5.82526e4   351.99402  24.5998
   5  15.352 FM    4.1522 1.09799e5   440.72290  46.3674

Totals :                 2.36801e5  1315.39491
```

==========

*** End of Report ***