MicroLab

MicroLab

User: Vepakum\Insumos Farmaceuticos\Larissa

Status: Ready

Method: Teste Qualitativo2

21CFR11 Enabled

Current Instrument Type: **Cary 630**

Current Sampling Technology: **ATR 1-Bounce**

Instrument Status

Energy:	20694
Battery:	On AC power
Source:	1.896 / 2.702
Laser:	6415

Gain Adjust

Temperatures (°C)

Detector:	40.097
CPU:	31.875
IR board:	38.98
Power:	30.75
Block:	27.25

Version Information

Version:	5.2.1612.0
DLL Version:	5.2.76.0
Firmware Version:	1.96.00.0

Instrument Serial Number: MY16052005

Resetting the Clean validity will cause the next clean run to be stored as the new 'Good' Clean run.

Reset Clean Validity

For methods that do not require a new background on every sample, the 'Reset Background Validity' button will force a new background to be collected before the next sample collection occurs.

Reset Background Validity

Date Time format configuration (for generation of DateTime in files' names) :

Fixed: yyyy-MM-ddThh-mm-ss

Home

< Back

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 01 Exatidao ATR

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 01 Exatidao ATR_2023-04-05T09-15-59.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:15:59 AM

Instrument Model: Cary630

Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx


Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:18:15 AM
Report Generation GMT Date:04/05/2023 12:18:15 PM

Sample ID:01 Exatidao ATR
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:15:59 AM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\01 Exatidao ATR_2023-04-05T09-15-59.a2r

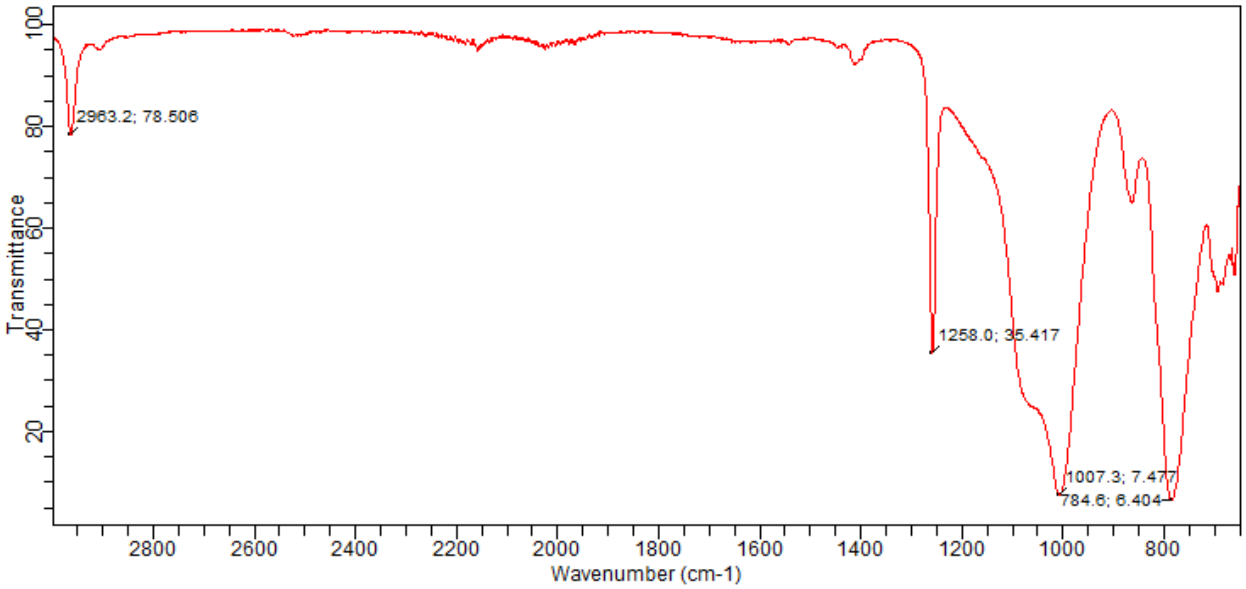

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 02 Resolucao

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 02 Resolucao_2023-04-05T09-20-29.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:20:29 AM

Instrument Model: Cary630


Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx

Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:23:26 AM
Report Generation GMT Date:04/05/2023 12:23:26 PM

Sample ID:02 Resolucao
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good
Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:20:29 AM
Range:3000 - 650
Apodization:Happ-Genzel
File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\02 Resolucao_2023-04-05T09-20-29.a2r

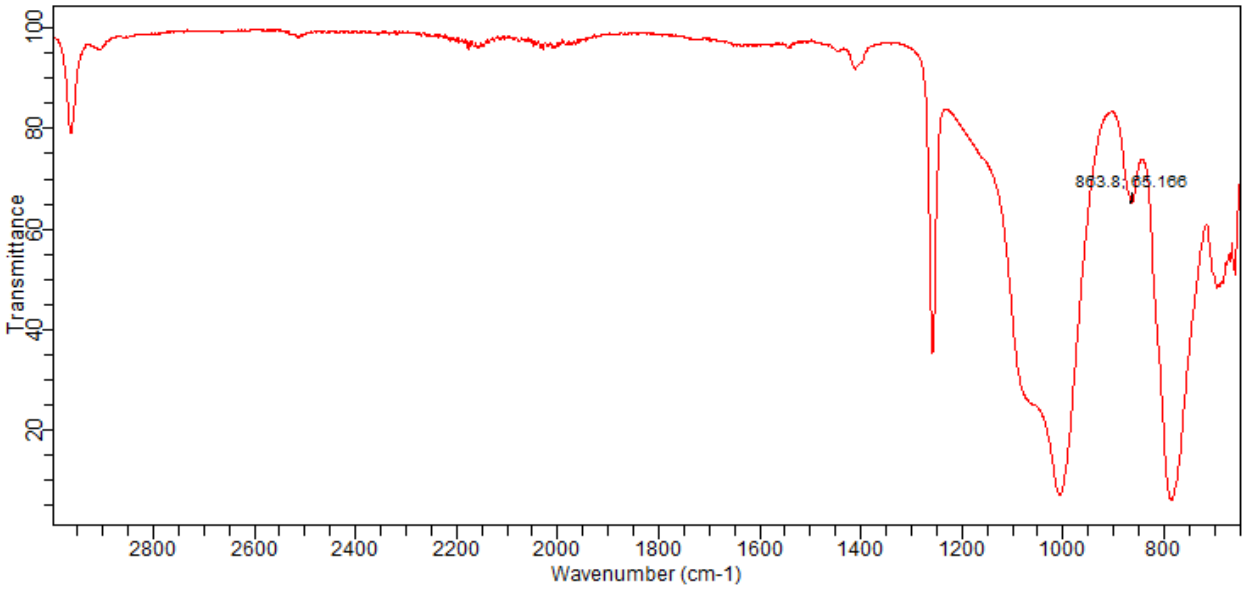

E-SIGNATURES

Signature

MicroLab

MicroLab

User: Vepakum\Insumos Farmaceuticos\Larissa


Status: Ready

Method: QUALIFICACAO

21CFR11 Enabled

Current Sample

Sample

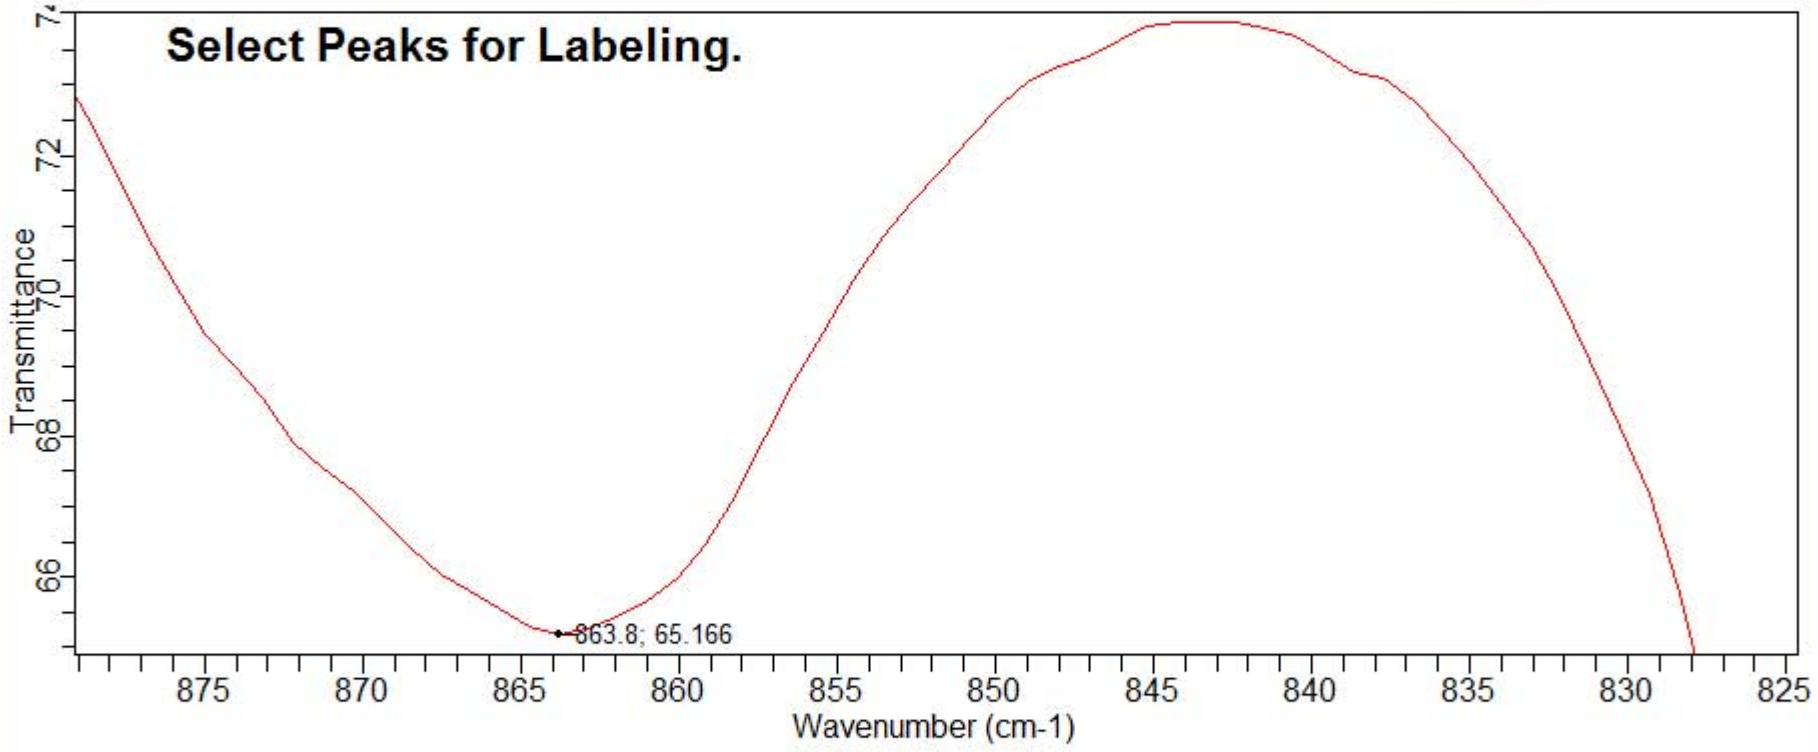

Home | Data Handling | E-Sign... | 21 CFR part 11 | Done

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 03 REP 01

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 03 REP 01_2023-04-05T09-25-14.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:25:14 AM

Instrument Model: Cary630

Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx


Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:26:23 AM
Report Generation GMT Date:04/05/2023 12:26:23 PM

Sample ID:03 REP 01
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:25:14 AM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\03 REP 01_2023-04-05T09-25-14.a2r

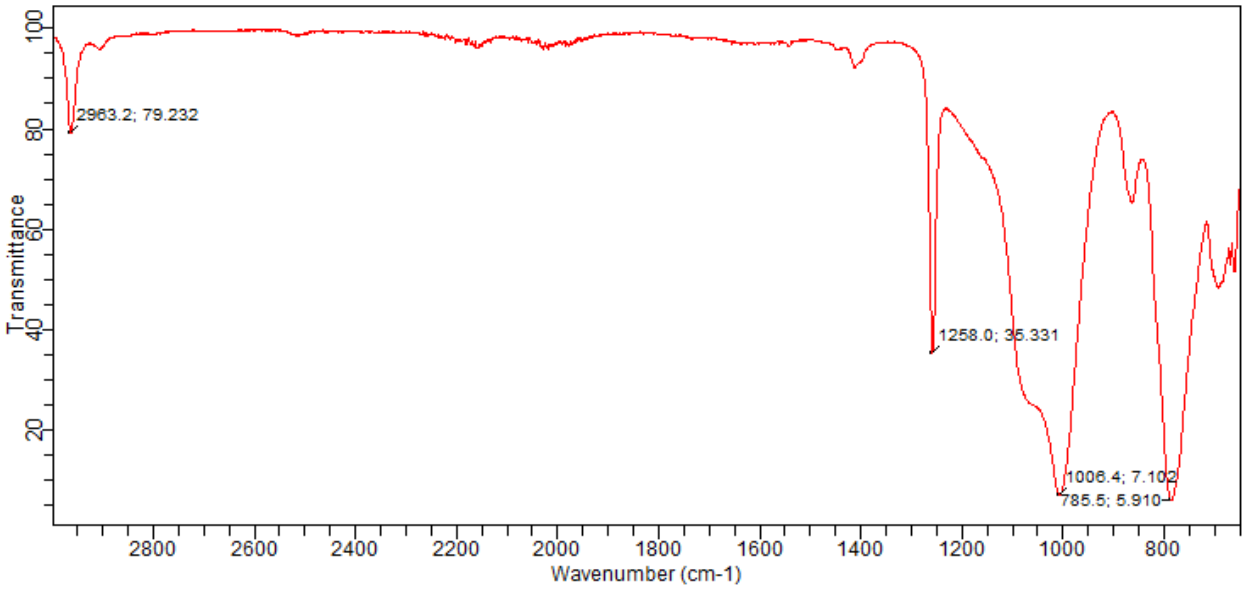

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 03 REP 02

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 03 REP 02_2023-04-05T09-27-38.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:27:38 AM

Instrument Model: Cary630

Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx


Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:28:39 AM
Report Generation GMT Date:04/05/2023 12:28:39 PM

Sample ID:03 REP 02
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:27:38 AM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\03 REP 02_2023-04-05T09-27-38.a2r

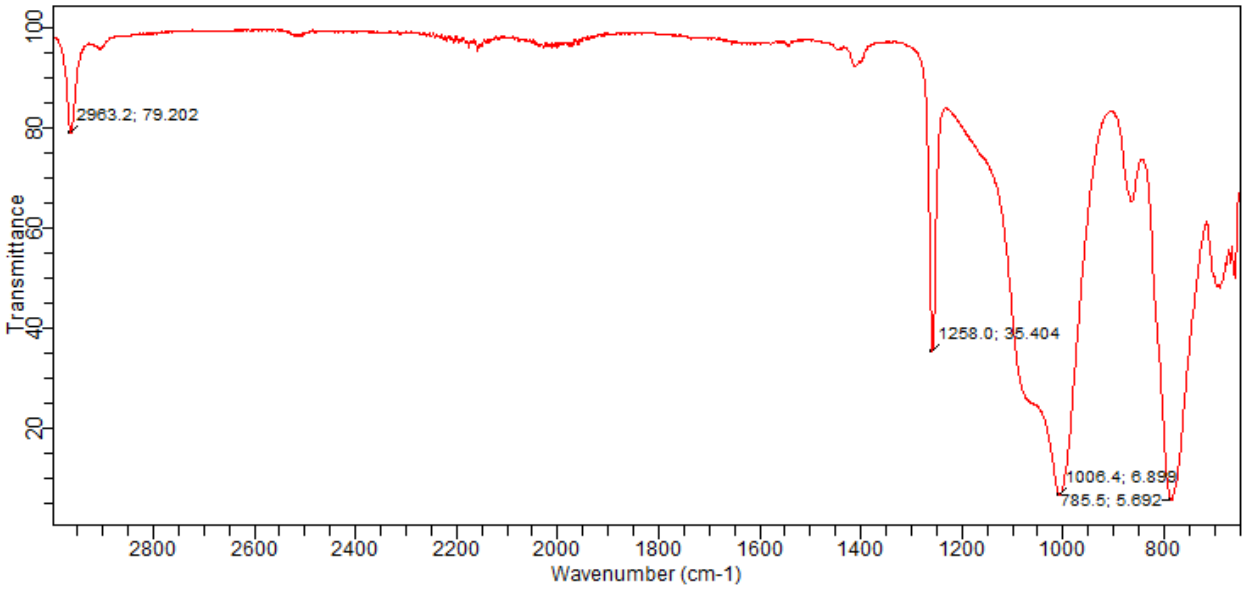

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 04 REP 01

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 04 REP 01_2023-04-05T09-30-10.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:30:10 AM

Instrument Model: Cary630

Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx


Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:31:03 AM
Report Generation GMT Date:04/05/2023 12:31:03 PM

Sample ID:04 REP 01
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:30:10 AM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\04 REP 01_2023-04-05T09-30-10.a2r

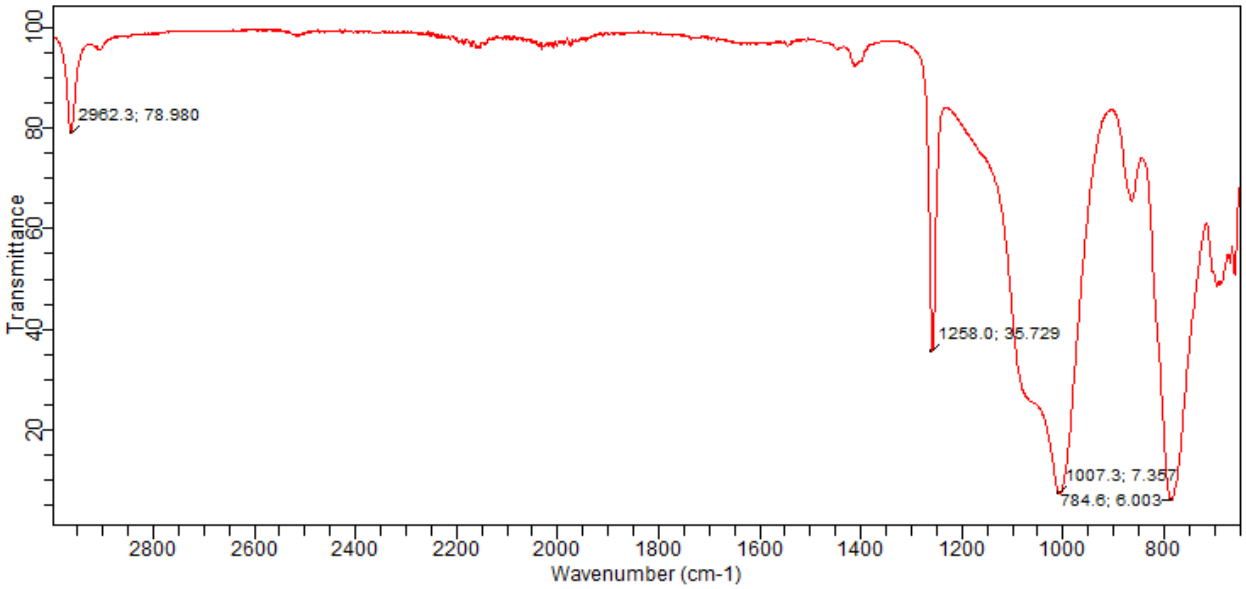

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 04 REP 02

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 04 REP 02_2023-04-05T09-36-02.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: QUALIFICACAO

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:36:02 AM

Instrument Model: Cary630


Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx

Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:37:07 AM
Report Generation GMT Date:04/05/2023 12:37:07 PM

Sample ID:04 REP 02
Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good
Method Name:QUALIFICACAO
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:36:02 AM
Range:3000 - 650
Apodization:Happ-Genzel
File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\04 REP 02_2023-04-05T09-36-02.a2r

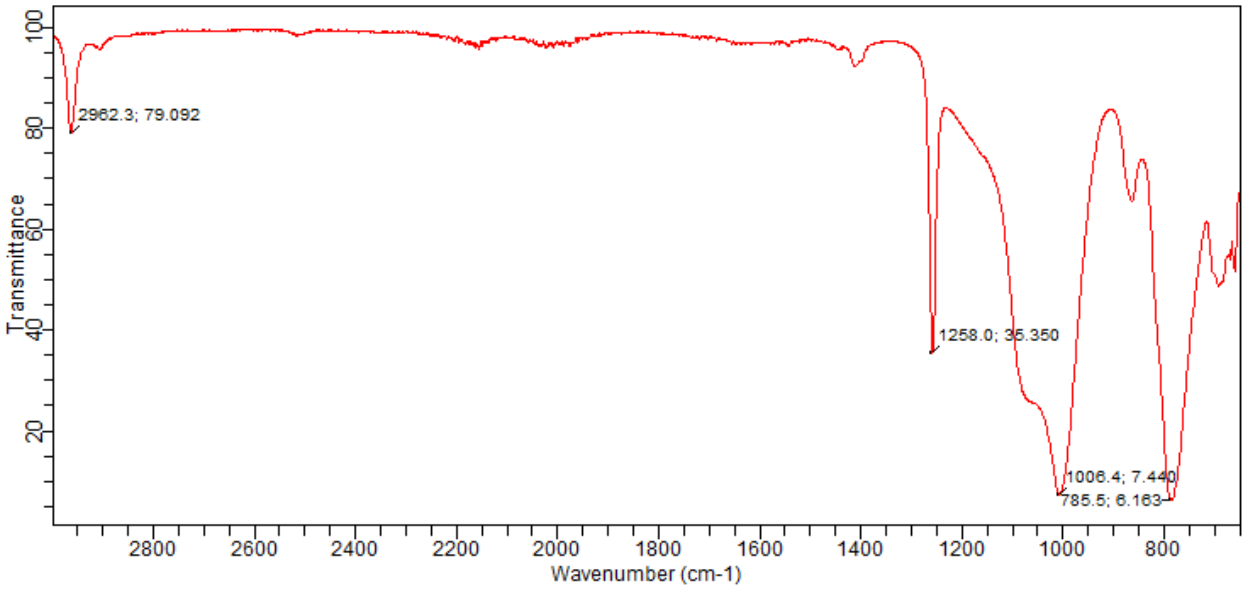

E-SIGNATURES

Signature

MicroLab

MicroLab

User: Vepakum\Insumos Farmaceuticos\Larissa

Status: Ready


Method: SENSIBILIDADE

21CFR part 11 SOFTWARE BY DLS SOLUTIONS

21CFR11 Enabled

Current Sample

Sample

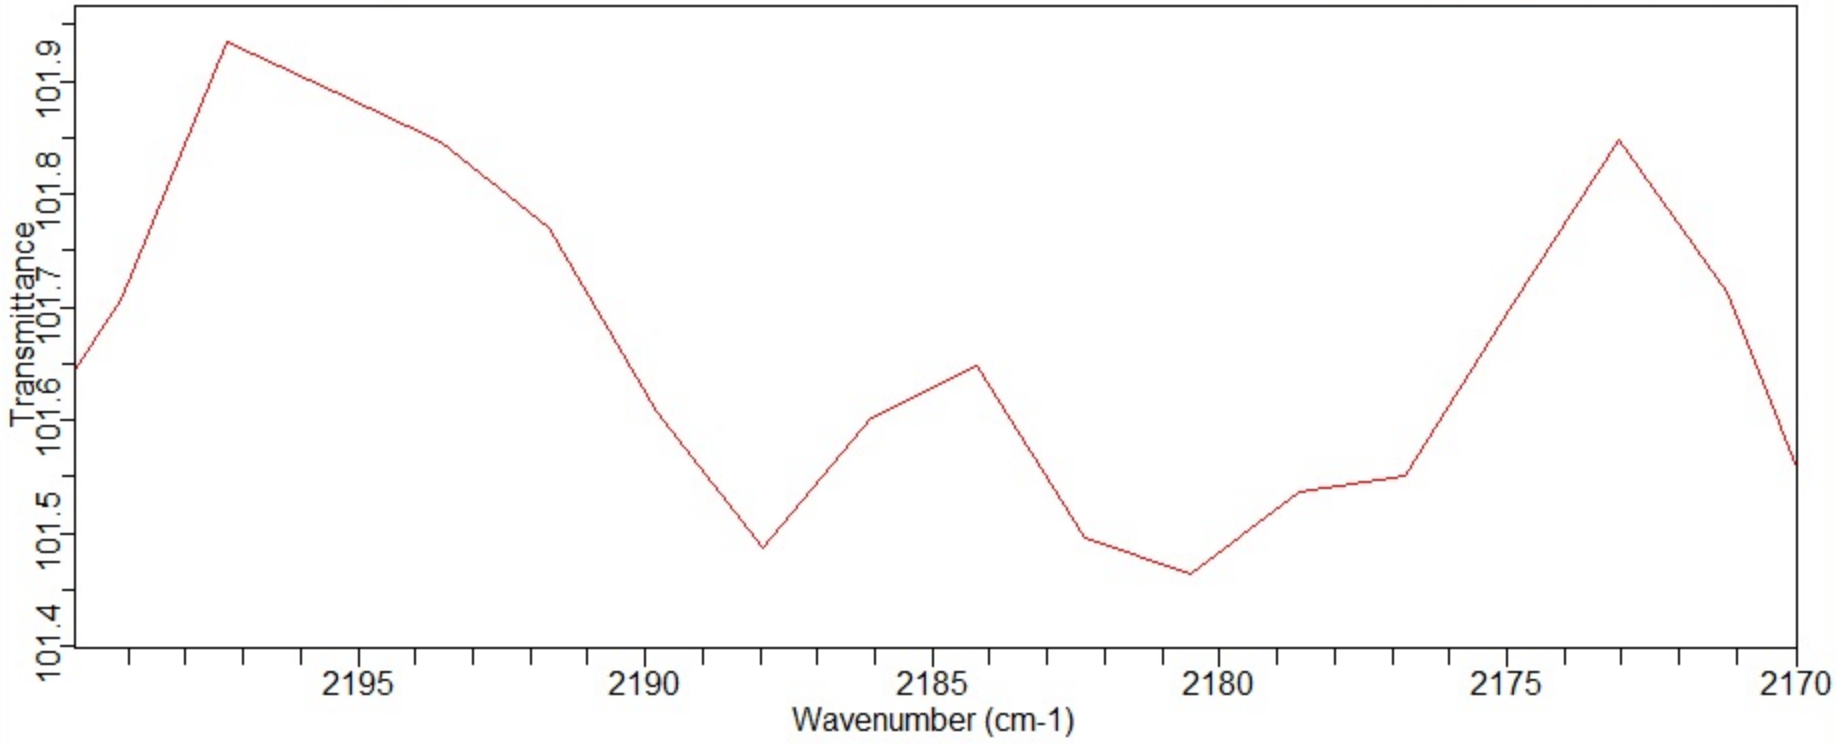

Home | Data Handling | E-Sign... | 21 CFR part 11 | Done

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 05 Sensibilidade

System Status: Good

File Location: CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 05 Sensibilidade_2023-04-05T09-41-28.a2r

PC/Workstation ID: CARY630-FTIR-HP

Software Version:MicroLab PC(21CFR11): 5.2.1612.0

FW Version:1.96.00.0

Data Information:
Method Name: SENSIBILIDADE

User: Vepakum\Insumos Farmaceuticos\Larissa

Date/Time: 04/05/2023 9:41:28 AM

Instrument Model: Cary630


Instrument S/N: MY16052005

Reporting Information:
Report Template: Spectrum.docx

Report Generated By: Vepakum\Insumos Farmaceuticos\Larissa

Report Generation Date: 04/05/2023 9:44:31 AM
Report Generation GMT Date:04/05/2023 12:44:31 PM

Sample ID:05 Sensibilidade
Sample Scans:48
Background Scans:48
Resolution:4
System Status:Good
Method Name:SENSIBILIDADE
User:Vepakum\Insumos Farmaceuticos\Larissa
Date/Time:04/05/2023 9:41:28 AM
Range:3000 - 650
Apodization:Happ-Genzel
File Location:CARY630-FTIR-HP\SQLEXPRESS|VAIMDB_Public(000)|Public Results\05 Sensibilidade_2023-04-05T09-41-28.a2r

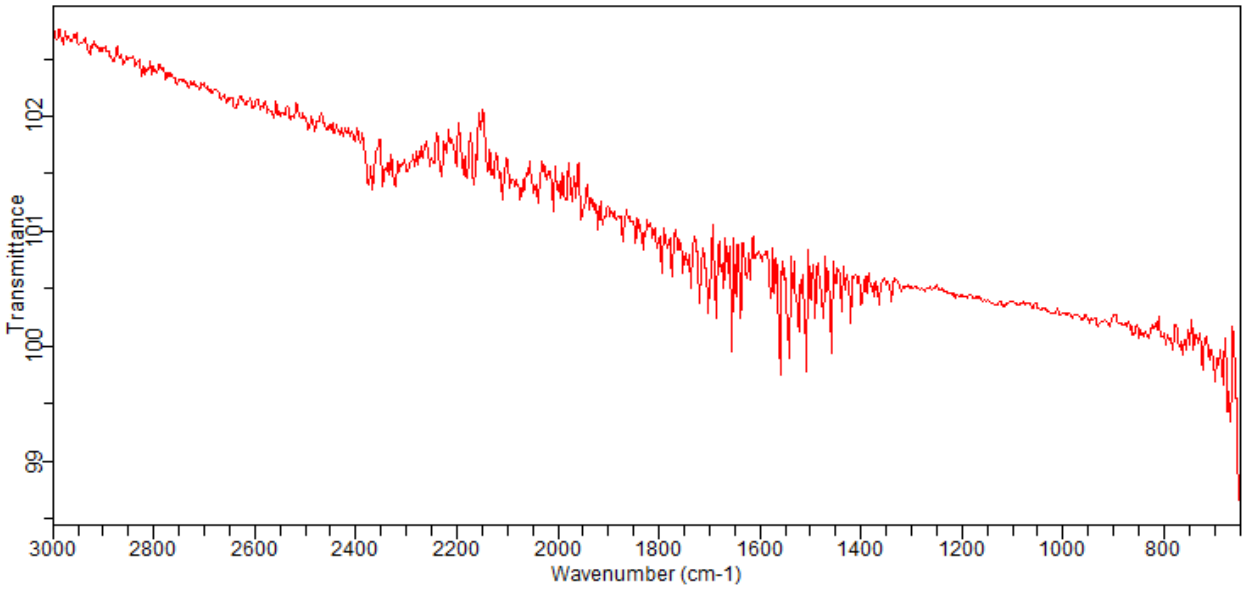

E-SIGNATURES

Signature