


DAD1, 1.650 (322 mAU, -) of 002-0101.D
DAD1, 1.650 (322 mAU, -) of 002-0101.D
mAU
EDUV => nm = 205 mAU = 325.071812
EDUV => nm = 273 mAU = 119.909286
EDUV => nm = 245 mAU = 32.281399
300
250
200
150
100
50
0
200
210
220
230
240
250
260
270
280
290
nm

Data File C:\CHEM32\1\DATA\PCIN\001-0101.D
Sample Name: Branco 1

Acq. Operator	: Michael	Seq. Line	: 1
Acq. Instrument	: Instrument 1	Location	: Vial 1
Injection Date	: 8/8/2018 3:12:04 PM	Inj	: 1
		Inj Volume	: 10 µl
Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 2:50:58 PM by Kelen		

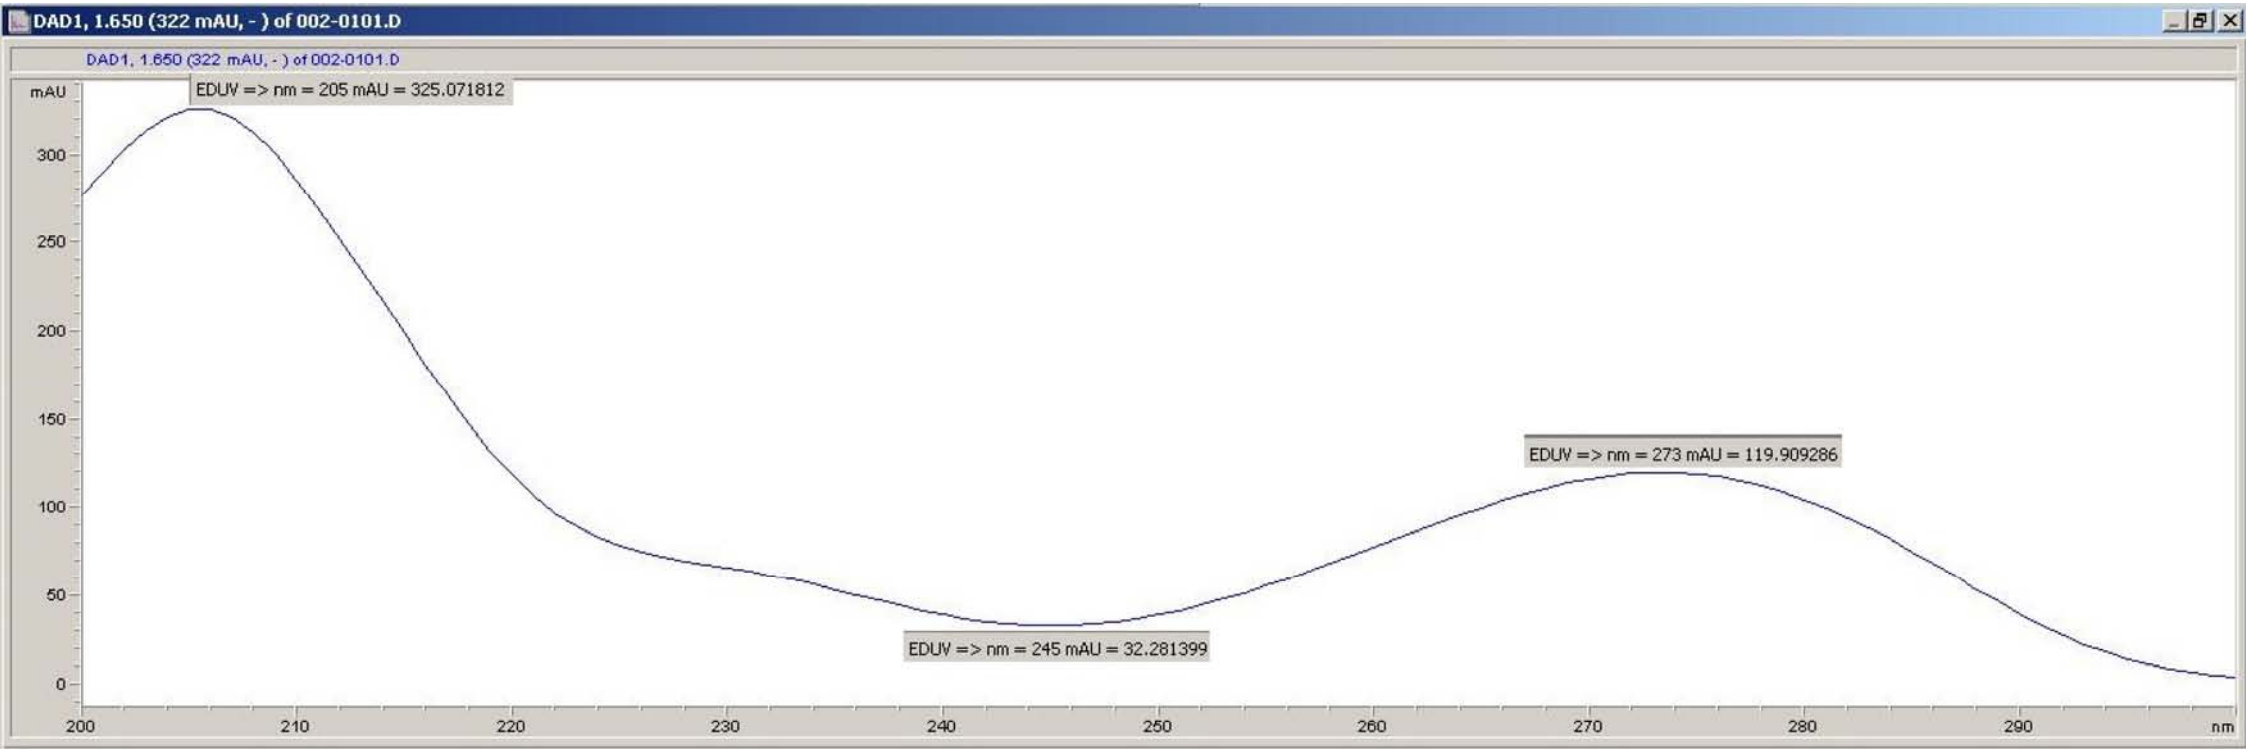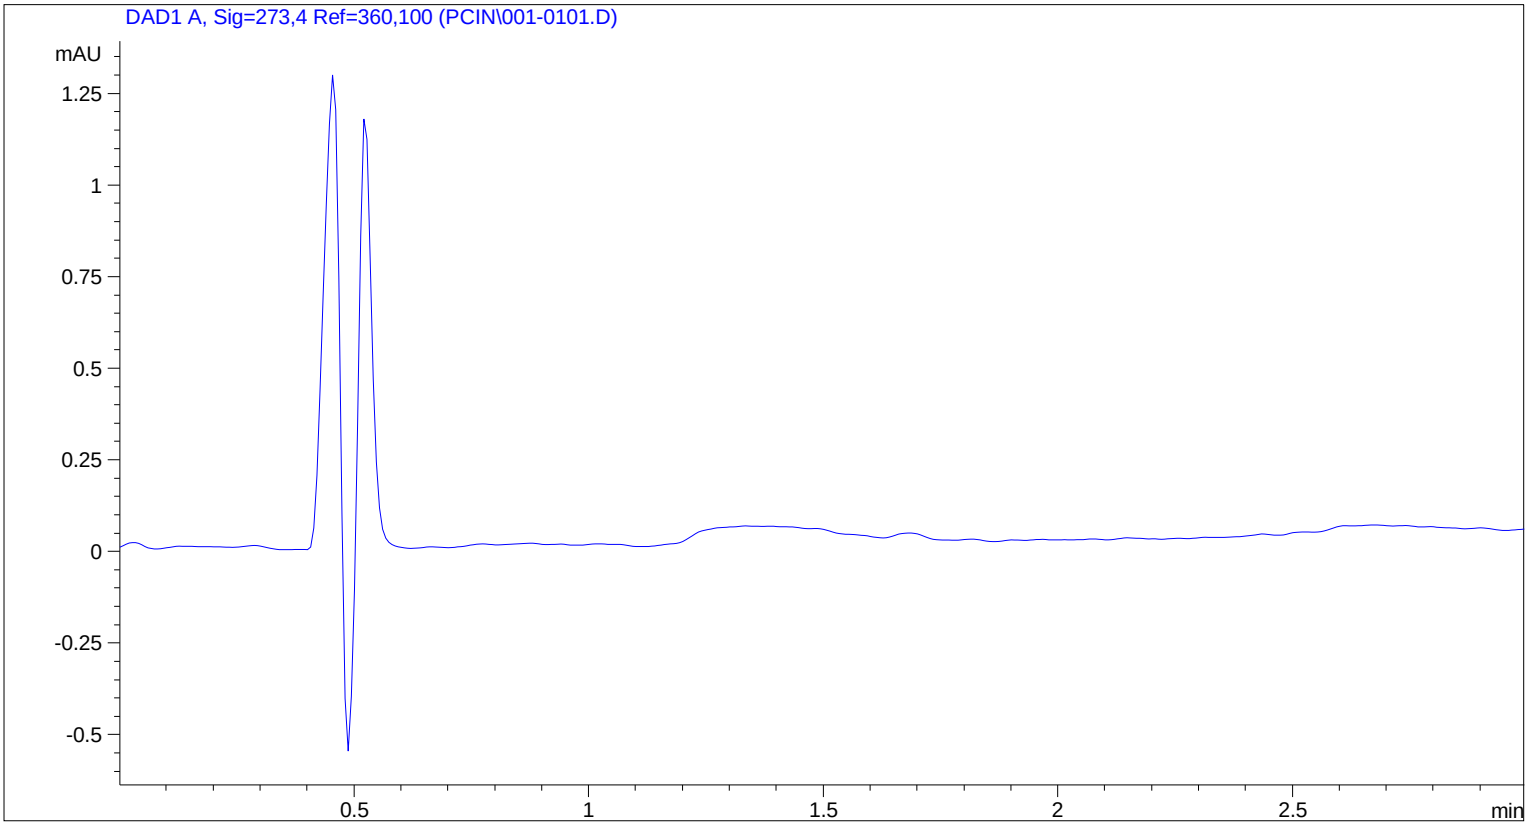

External Standard Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Area Percent Report


Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0201.D
Sample Name: PCIN 1

```
==================================================================
Acq. Operator   : Michael                       Seq. Line :   2
Acq. Instrument : Instrument 1                   Location : Vial 2
Injection Date  : 8/8/2018 3:16:44 PM                 Inj :   1
                                                Inj Volume : 10 µl
Method          : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
```

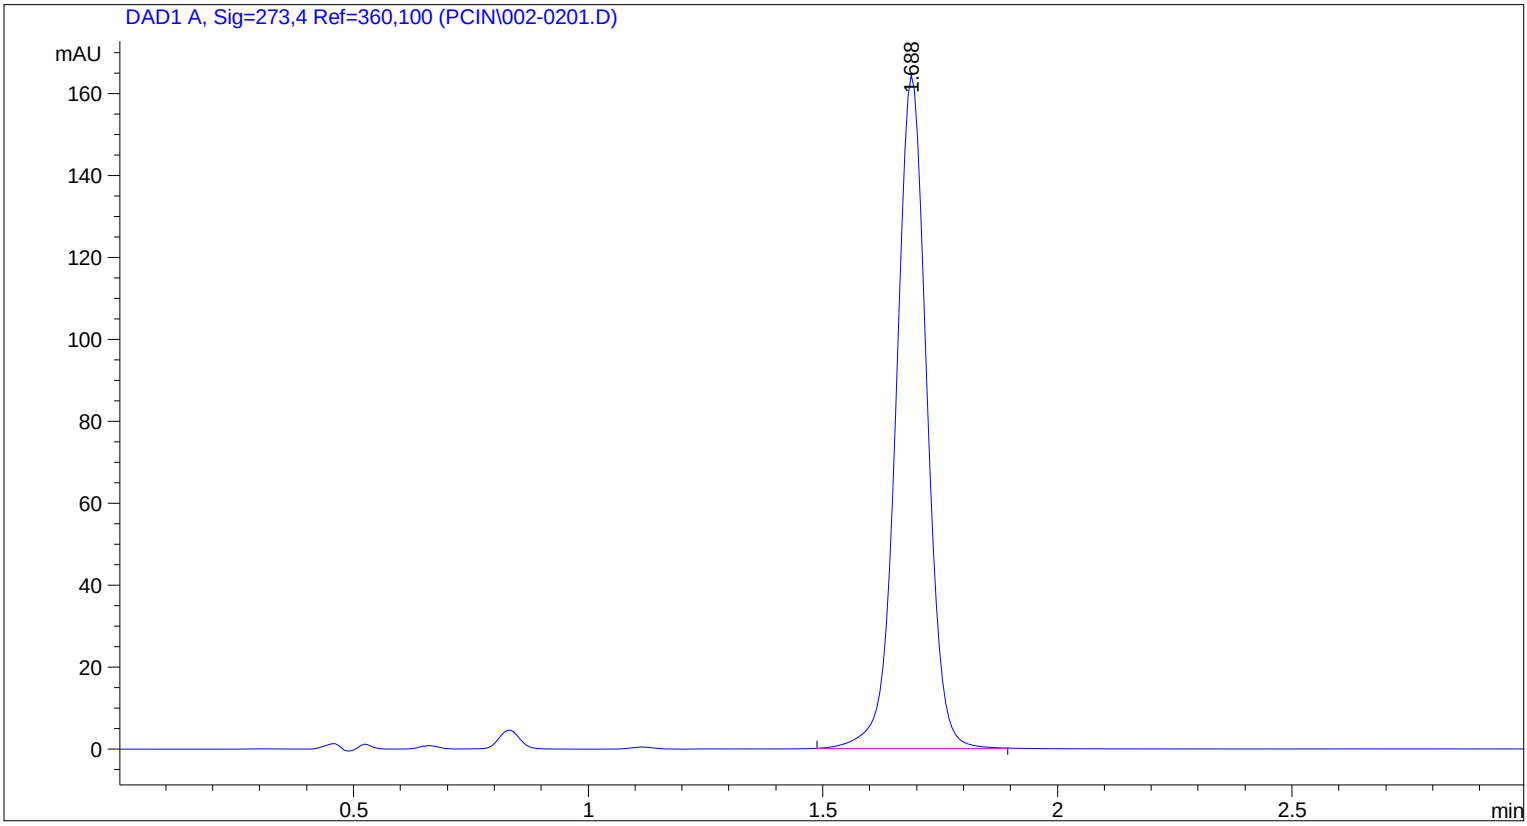


```
==================================================================
                    External Standard Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==================================================================
==================================================================
                       Area Percent Report
==================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.688 BB    0.0712  750.92114  164.53317 100.0000
```

Totals :	750.92114	164.53317


==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0301.D
Sample Name: PCIN 2

==========

Acq. Operator : Michael Seq. Line : 3
Acq. Instrument : Instrument 1 Location : Vial 2
Injection Date : 8/8/2018 3:21:23 PM Inj : 1
Inj Volume : 10 µl
Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed : 8/8/2018 2:50:58 PM by Kelen

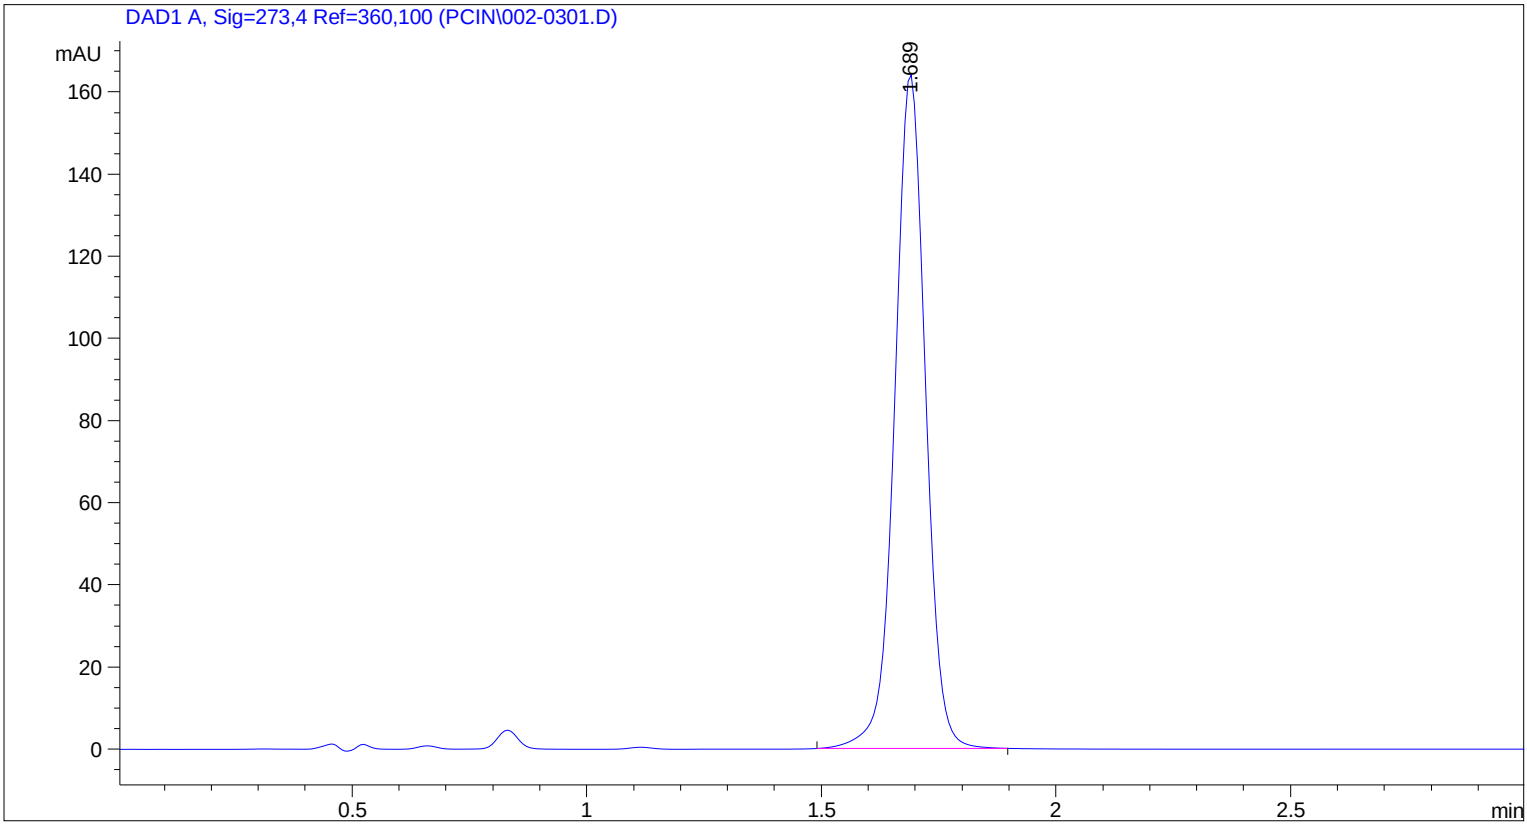

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.689	BB	0.0692	751.07001	164.57018	100.0000


Totals :	751.07001	164.57018

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0401.D
Sample Name: PCIN 3

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   4
Acq. Instrument : Instrument 1                    Location : Vial 2
Injection Date  : 8/8/2018 3:25:56 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Method          : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
```

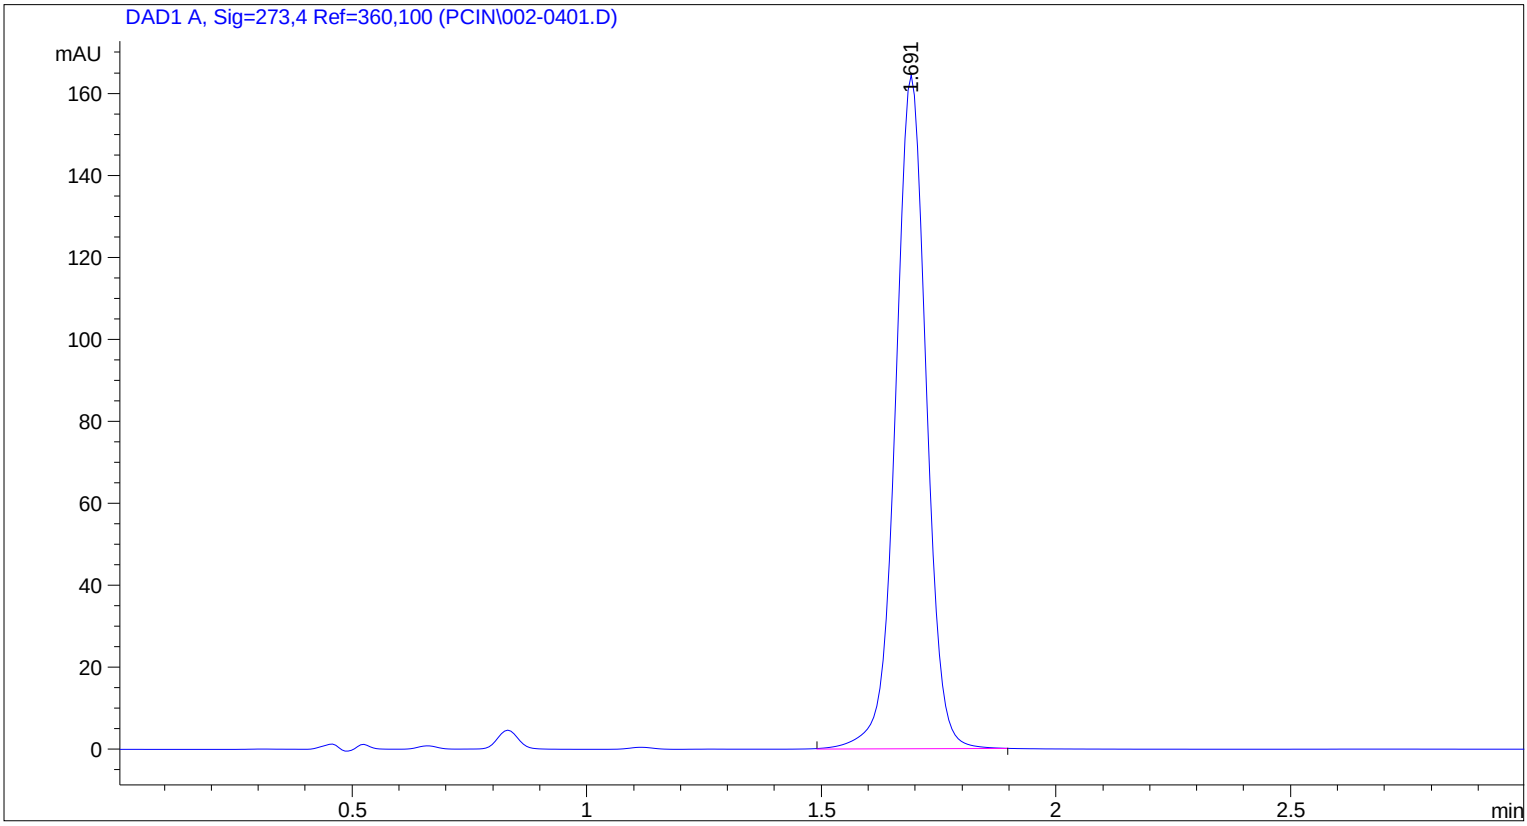


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.691 BB    0.0713  751.08636  164.49240 100.0000
```


Totals :	751.08636	164.49240

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\001-0501.D
Sample Name: Branco 2

Acq. Operator	: Michael	Seq. Line	: 5
Acq. Instrument	: Instrument 1	Location	: Vial 1
Injection Date	: 8/8/2018 3:30:40 PM	Inj	: 1
		Inj Volume	: 10 µl
Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 2:50:58 PM by Kelen		

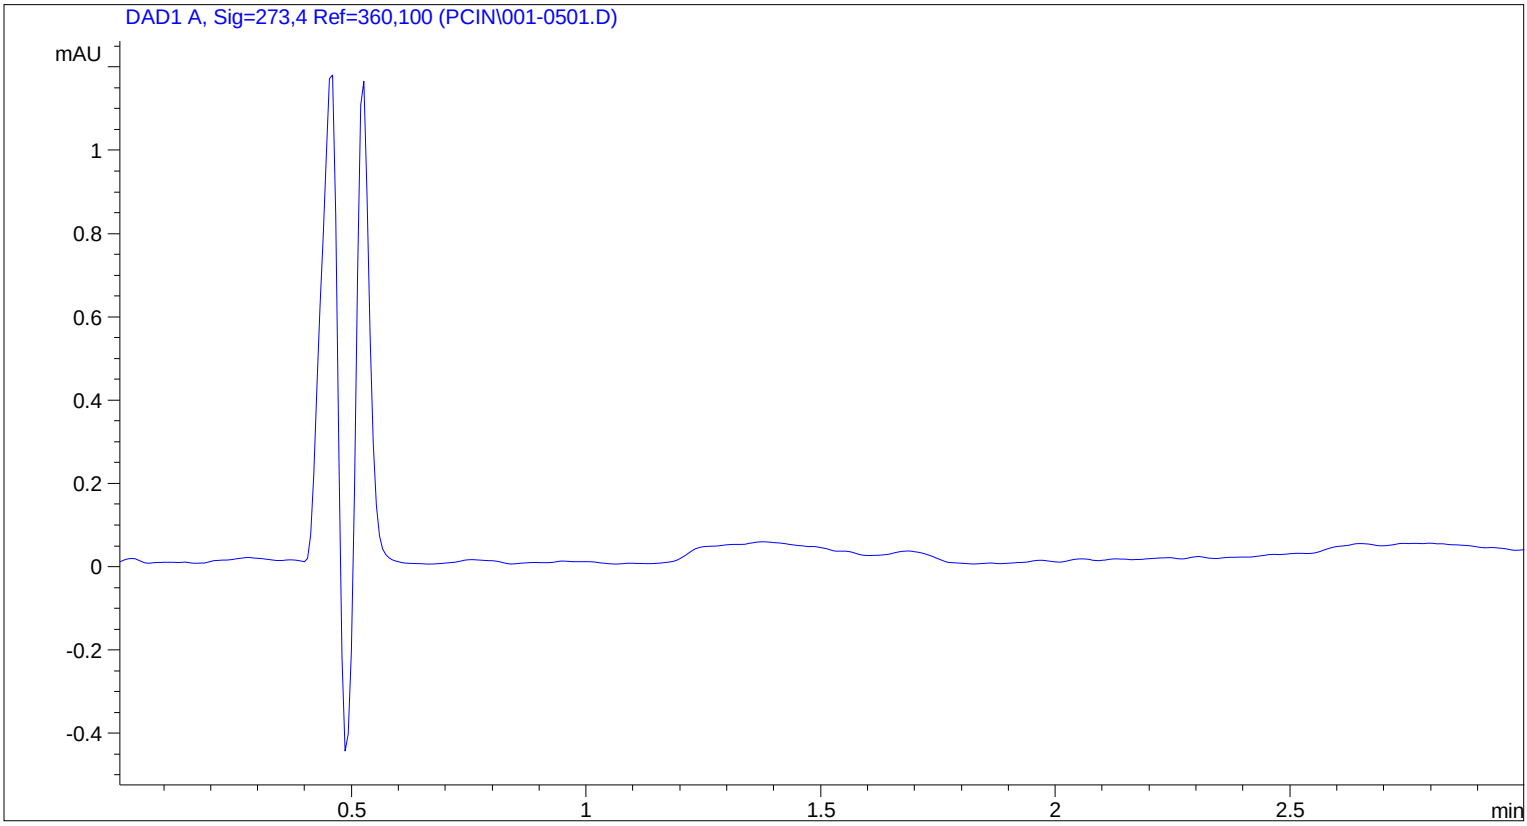

External Standard Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Area Percent Report


Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0601.D
Sample Name: PCIN 4

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   6
Acq. Instrument : Instrument 1                    Location : Vial 2
Injection Date  : 8/8/2018 3:35:15 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Method          : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
```

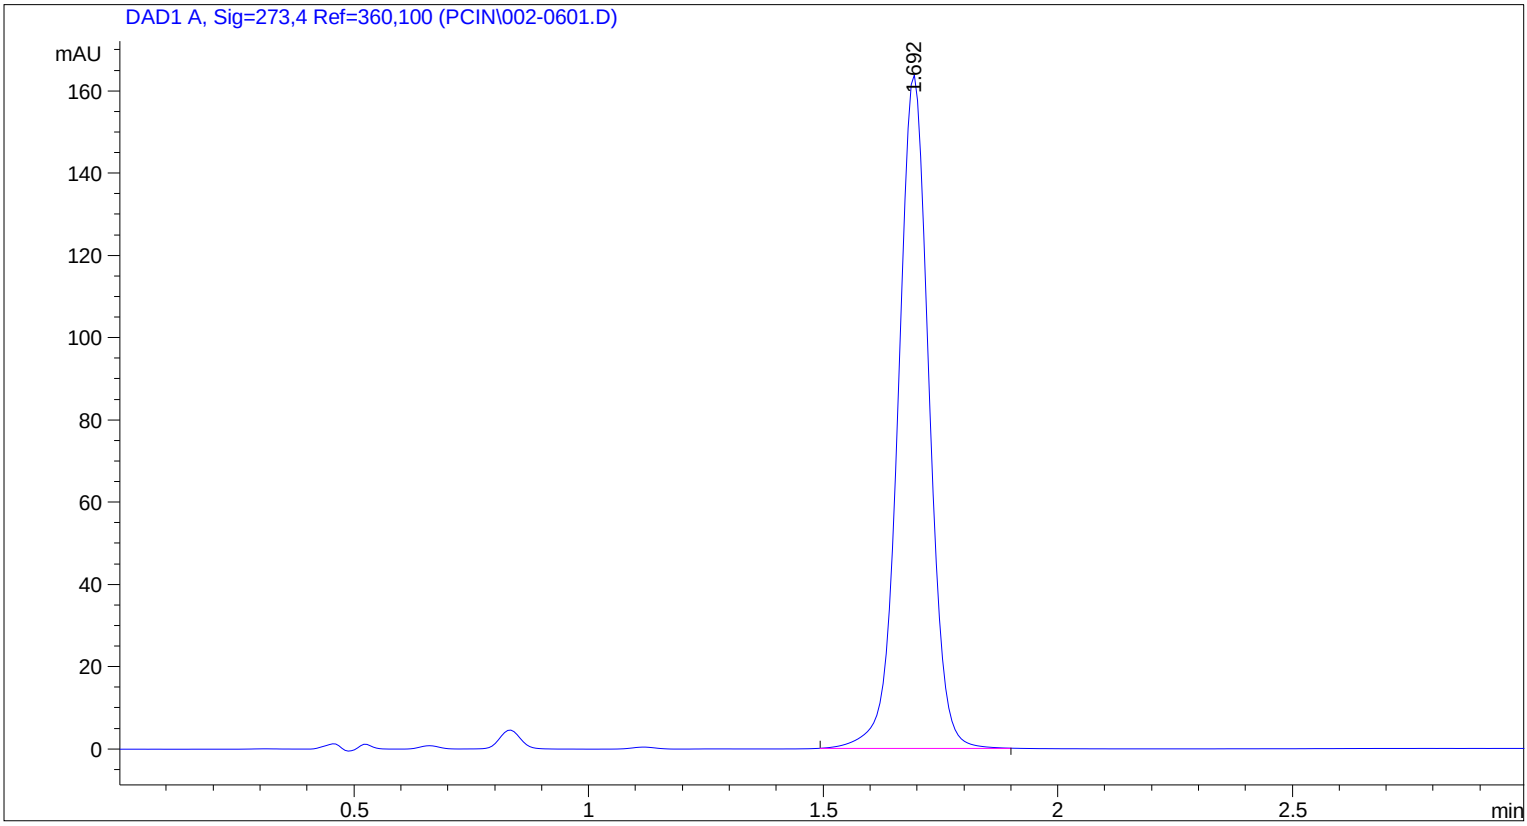


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.692 BB    0.0714  751.01025  164.07074 100.0000
```


Totals :	751.01025	164.07074

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0701.D
Sample Name: PCIN 5

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   7
Acq. Instrument : Instrument 1                    Location : Vial 2
Injection Date  : 8/8/2018 3:39:53 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Method          : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
```

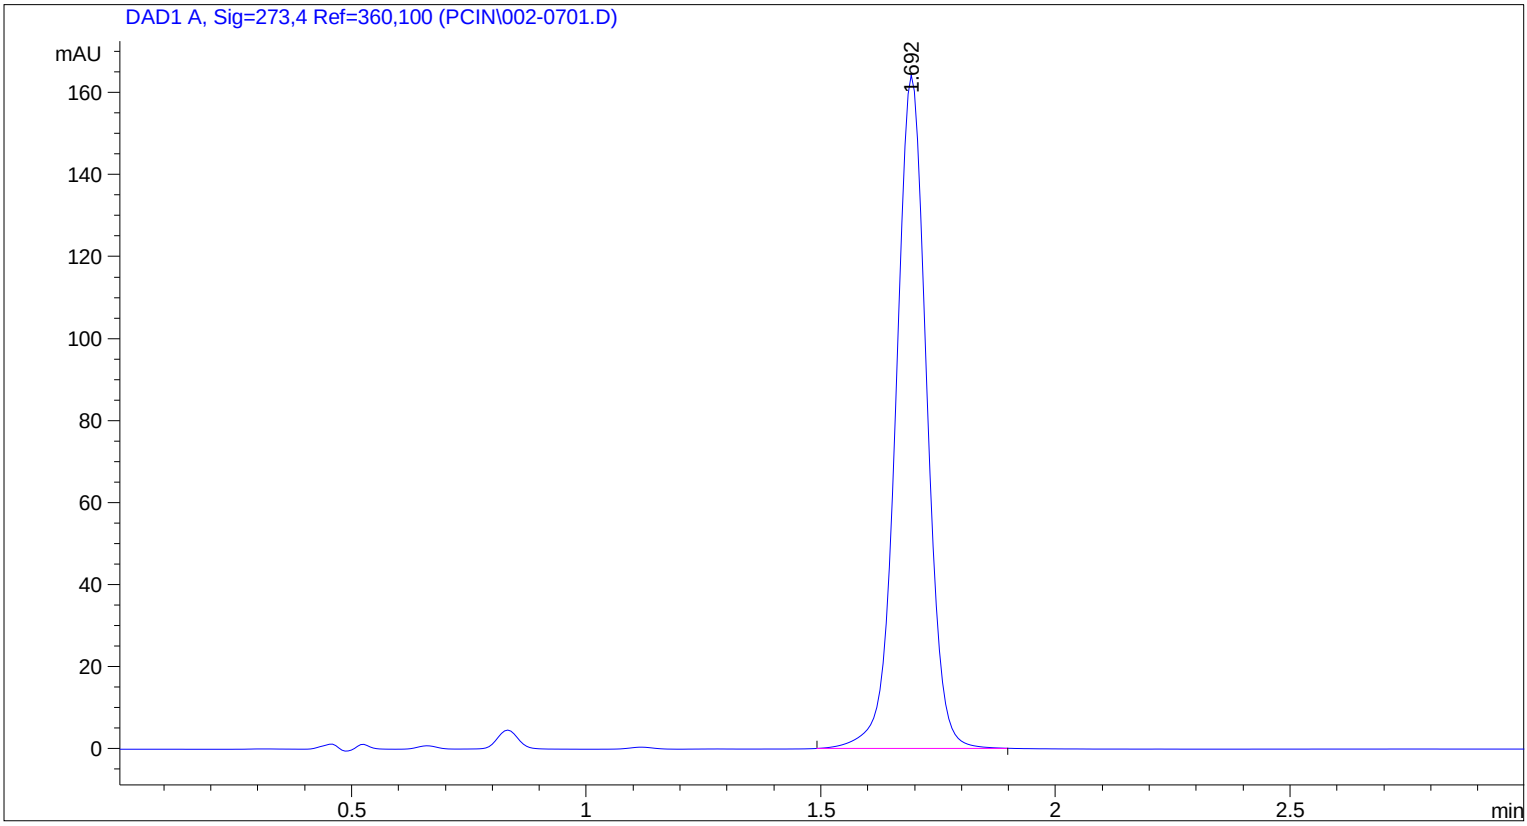


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.692 BB    0.0713  751.16760  164.34238 100.0000
```


Totals :	751.16760	164.34238

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\002-0801.D
Sample Name: PCIN 6

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   8
Acq. Instrument : Instrument 1                    Location : Vial 2
Injection Date  : 8/8/2018 3:44:27 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Method          : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
```

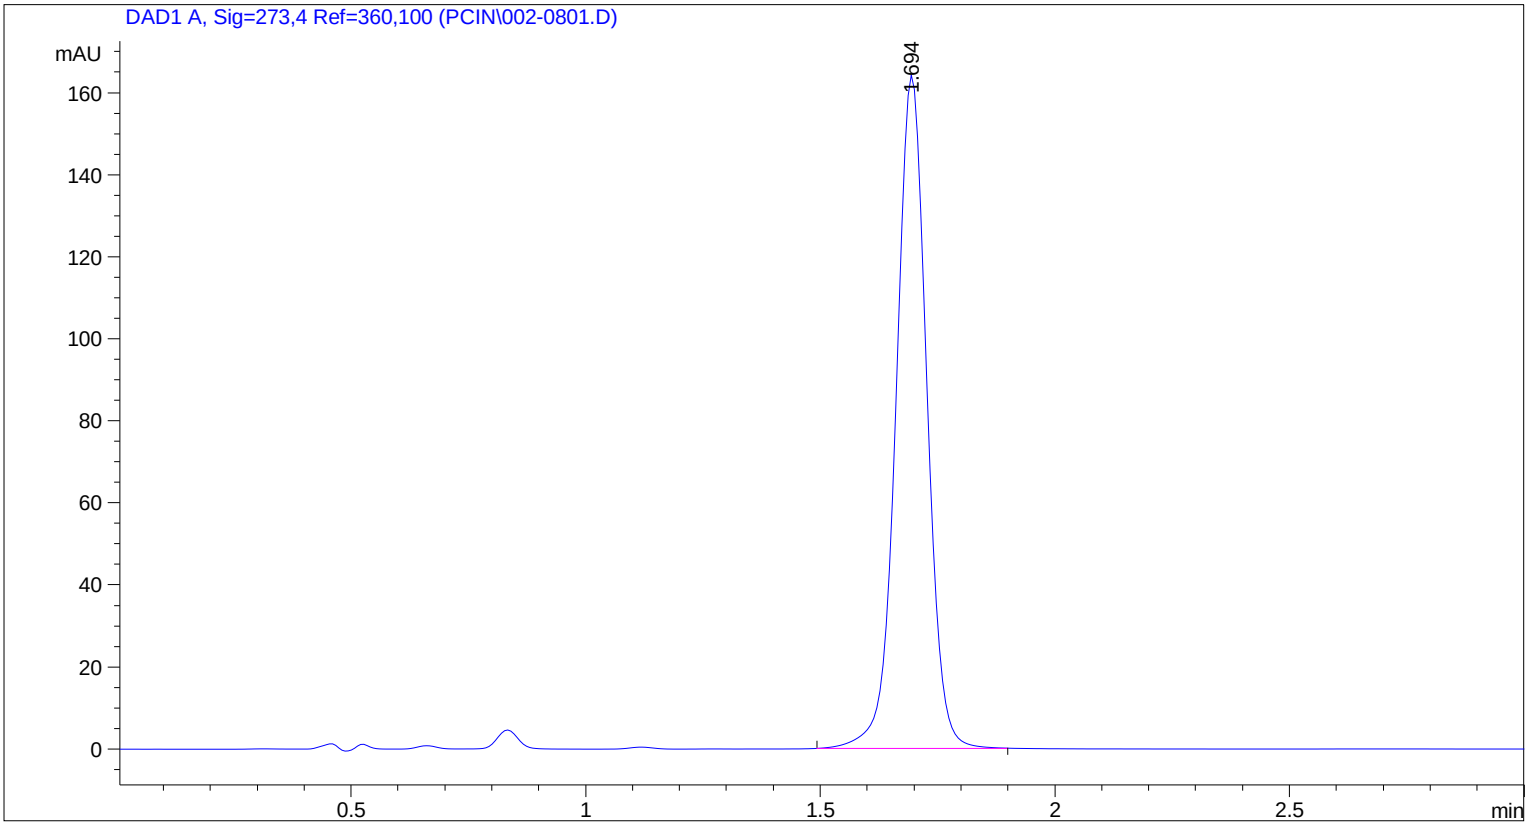


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.694 BB    0.0714  751.56390  164.32867 100.0000
```


Totals :	751.56390	164.32867

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\PCIN\001-0901.D
Sample Name: Branco 3

Acq. Operator	: Michael	Seq. Line	: 9
Acq. Instrument	: Instrument 1	Location	: Vial 1
Injection Date	: 8/8/2018 3:49:00 PM	Inj	: 1
		Inj Volume	: 10 µl
Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 2:50:58 PM by Kelen		

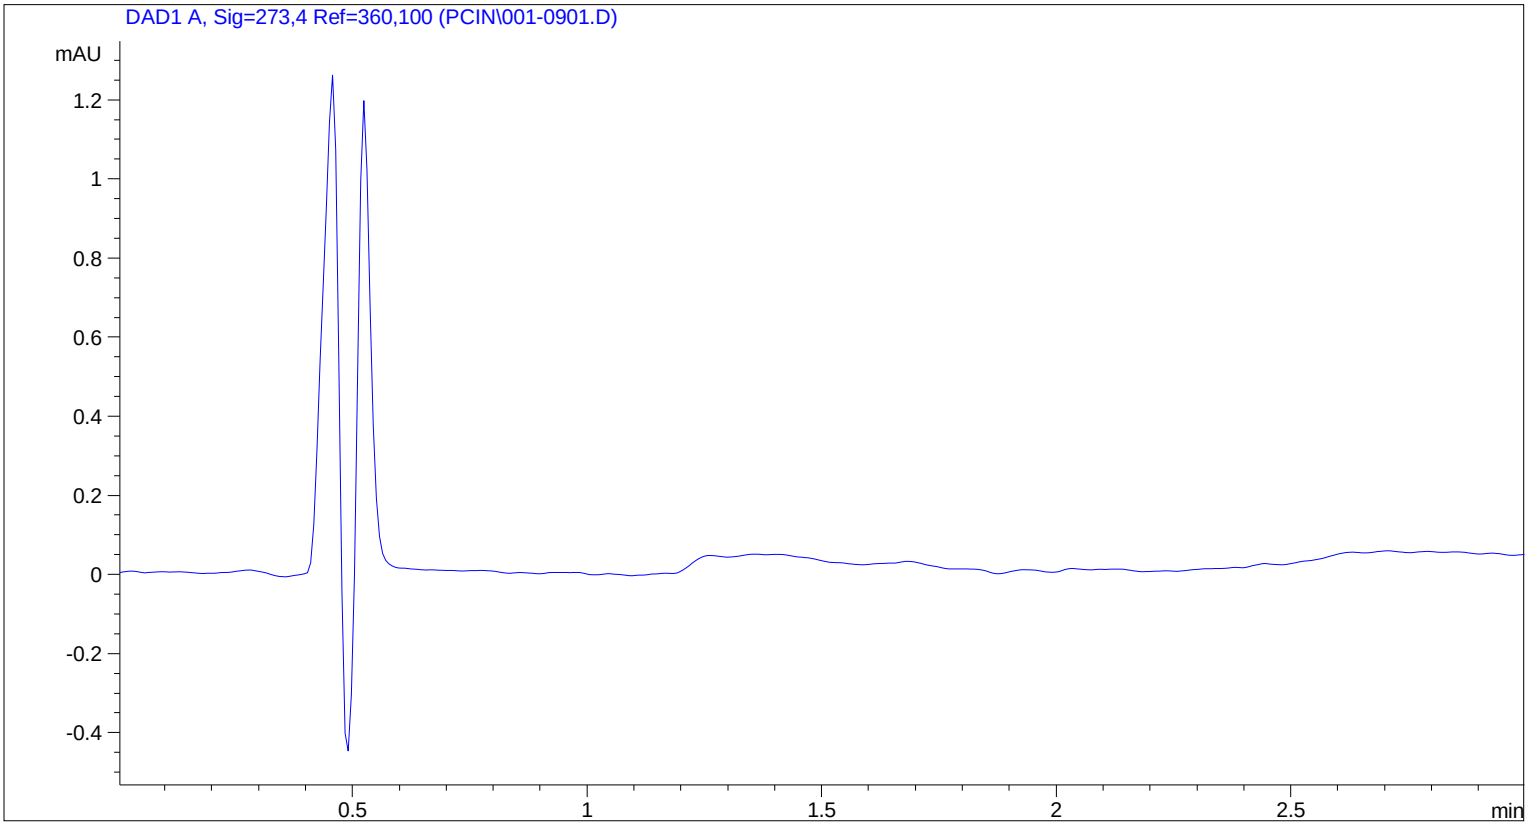

External Standard Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs


No peaks found

*** End of Report ***

Data File C:\CHEM32\1\DATA\LDUV\001-0101.D
Sample Name: LDUV 1

==========

Acq. Operator : Michael Seq. Line : 1
Acq. Instrument : Instrument 1 Location : Vial 1
Injection Date : 8/8/2018 3:56:51 PM Inj : 1
Inj Volume : 10 µl
Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed : 8/8/2018 2:50:58 PM by Kelen

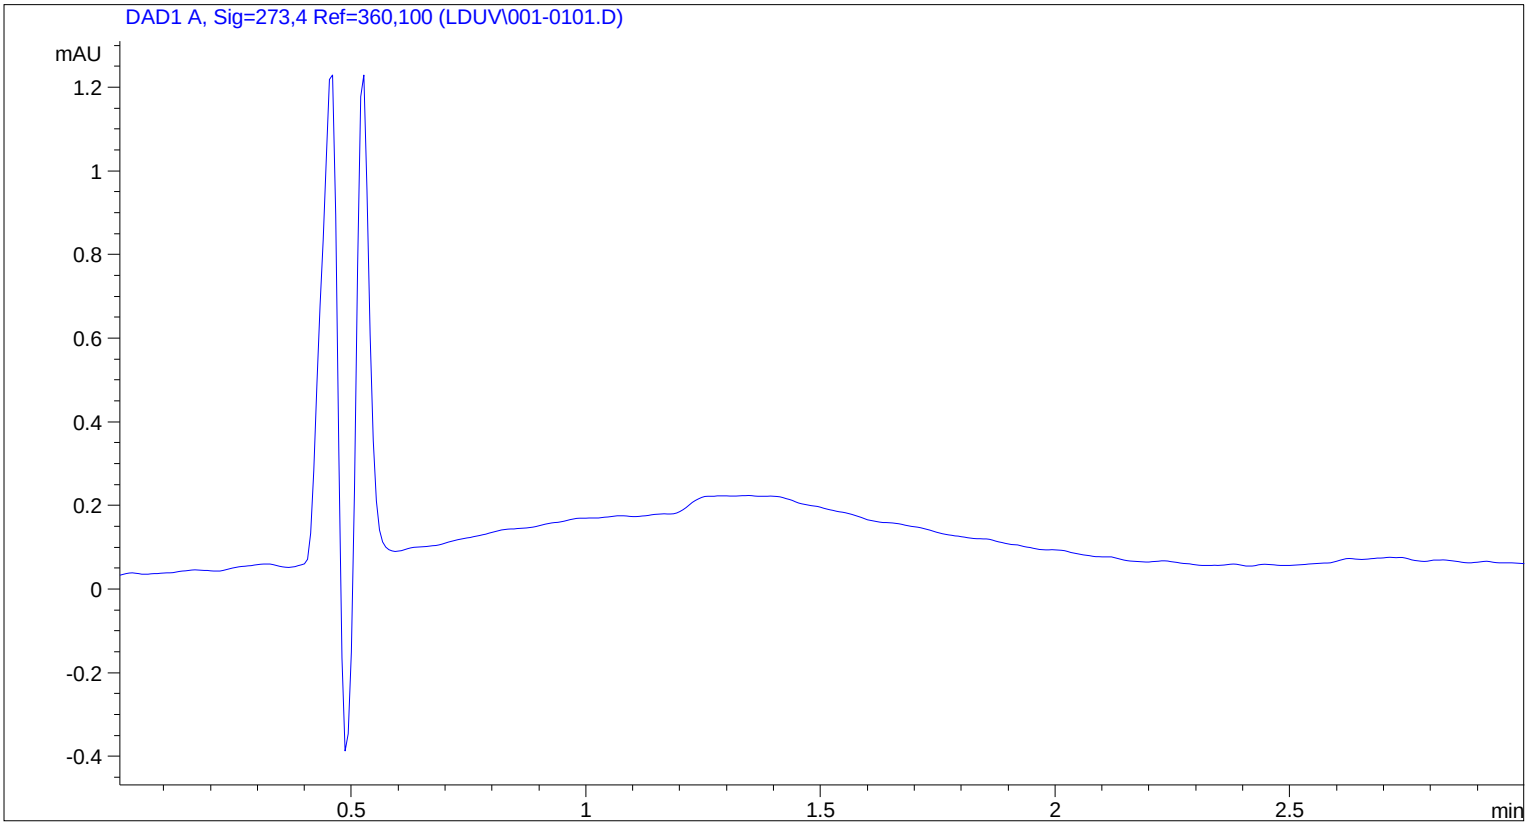

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\CHEM32\1\DATA\LDUV\002-0201.D
Sample Name: LDUV 2

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   2
Acq. Instrument : Instrument 1                    Location : Vial 2
Injection Date  : 8/8/2018 4:01:31 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

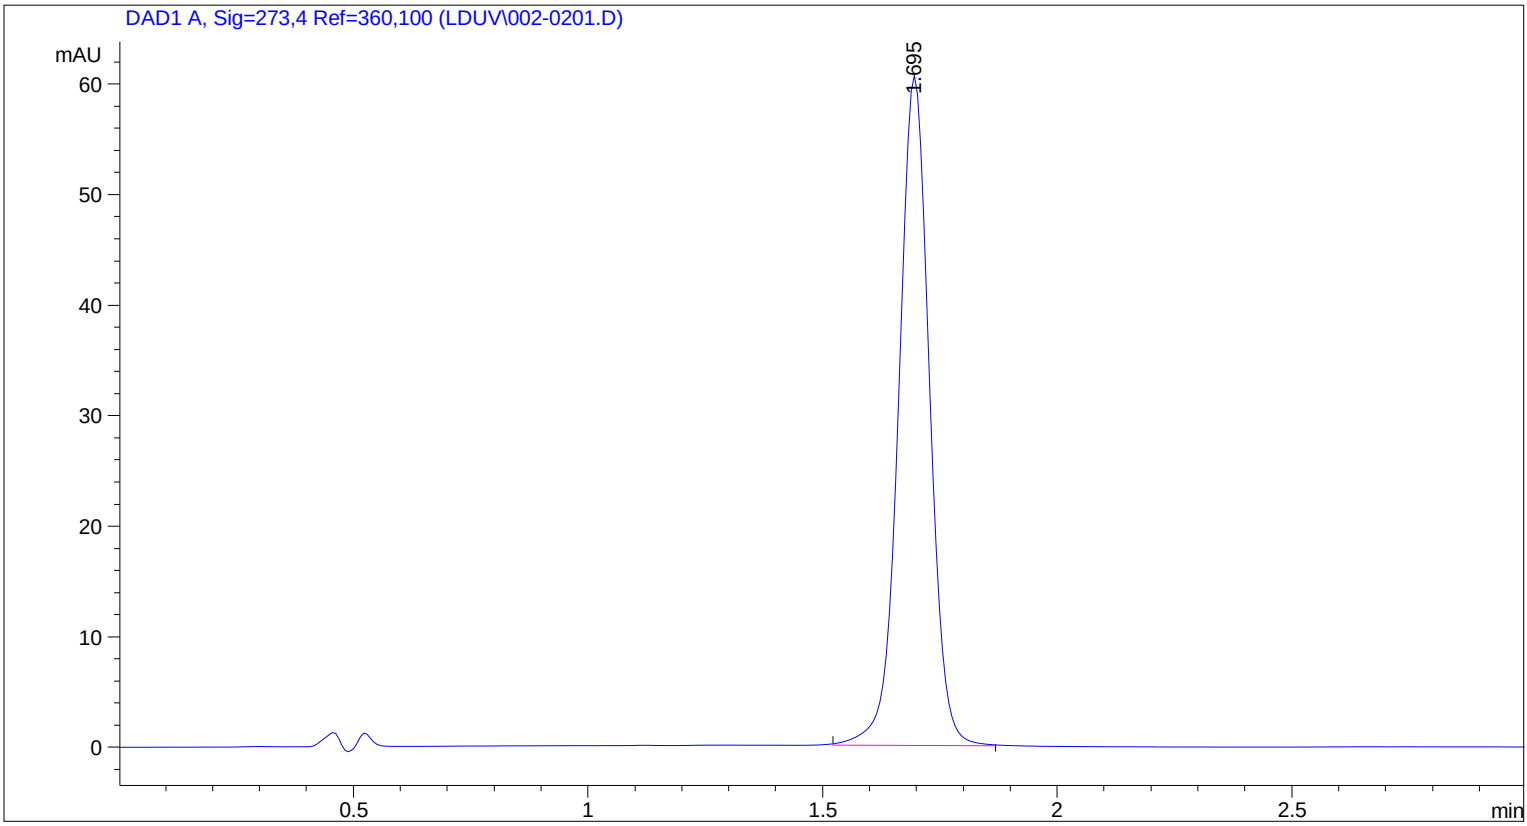


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LDUV\002-0201.D
Sample Name: LDUV 2


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.695	BB	0.0714	277.73029	60.62809	100.0000
Totals :				277.73029	60.62809	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LDUV\003-0301.D
Sample Name: LDUV 3

```
==========================================================================
Acq. Operator   : Michael                          Seq. Line :   3
Acq. Instrument : Instrument 1                      Location : Vial 3
Injection Date  : 8/8/2018 4:06:13 PM                    Inj :   1
                                                  Inj Volume : 10 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

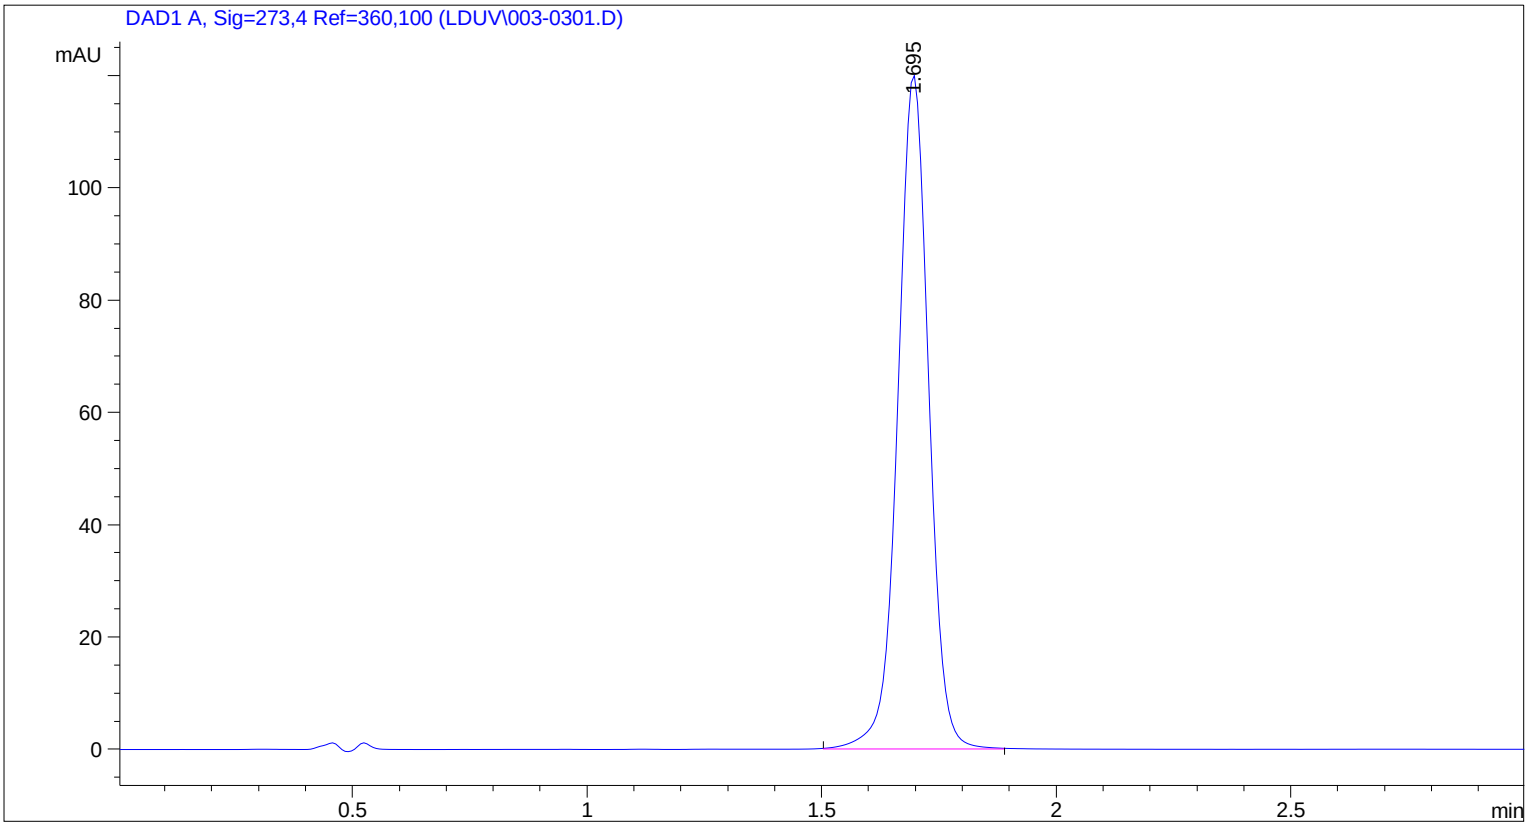


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LDUV\003-0301.D
Sample Name: LDUV 3

Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.695	BB	0.0714	550.27368	120.24940	100.0000
Totals :				550.27368	120.24940	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LDUV\004-0401.D
Sample Name: LDUV 4

==========

Acq. Operator	: Michael	Seq. Line	: 4
Acq. Instrument	: Instrument 1	Location	: Vial 4
Injection Date	: 8/8/2018 4:10:50 PM	Inj	: 1
		Inj Volume	: 10 µl
Acq. Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 2:50:58 PM by Kelen		
Analysis Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 4:07:50 PM by Kelen (modified after loading)		

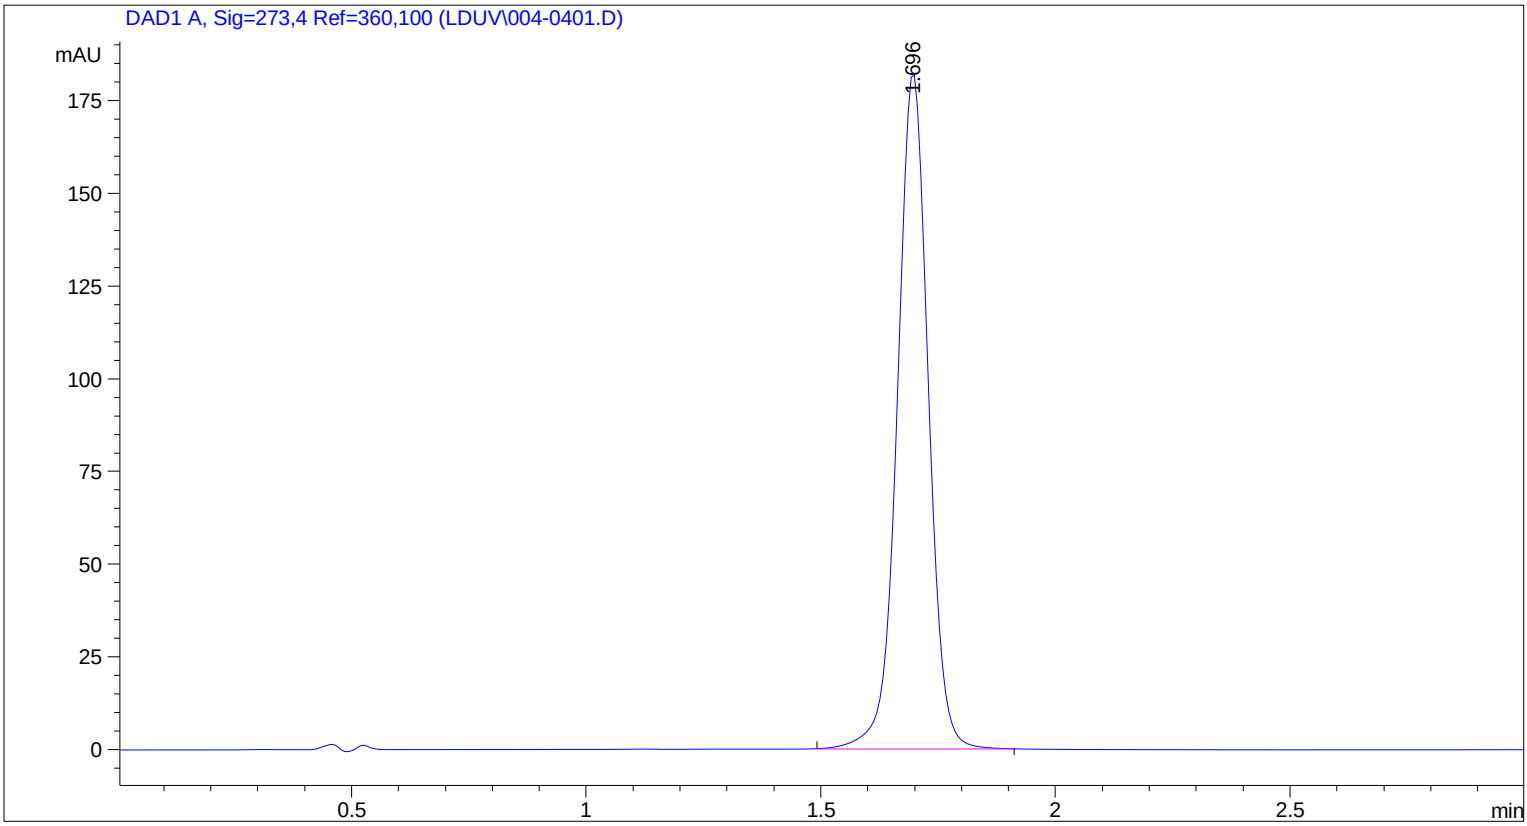

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Data File C:\CHEM32\1\DATA\LDUV\004-0401.D
Sample Name: LDUV 4


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.696	BB	0.0696	838.35669	182.59761	100.0000
Totals :				838.35669	182.59761	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LDUV\005-0501.D
Sample Name: LDUV 5

Acq. Operator	: Michael	Seq. Line	: 5
Acq. Instrument	: Instrument 1	Location	: Vial 5
Injection Date	: 8/8/2018 4:15:24 PM	Inj	: 1
		Inj Volume	: 10 µl
Acq. Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 2:50:58 PM by Kelen		
Analysis Method	: C:\CHEM32\1\METHODS\QUALIFICACAO2018.M		
Last changed	: 8/8/2018 4:07:50 PM by Kelen (modified after loading)		

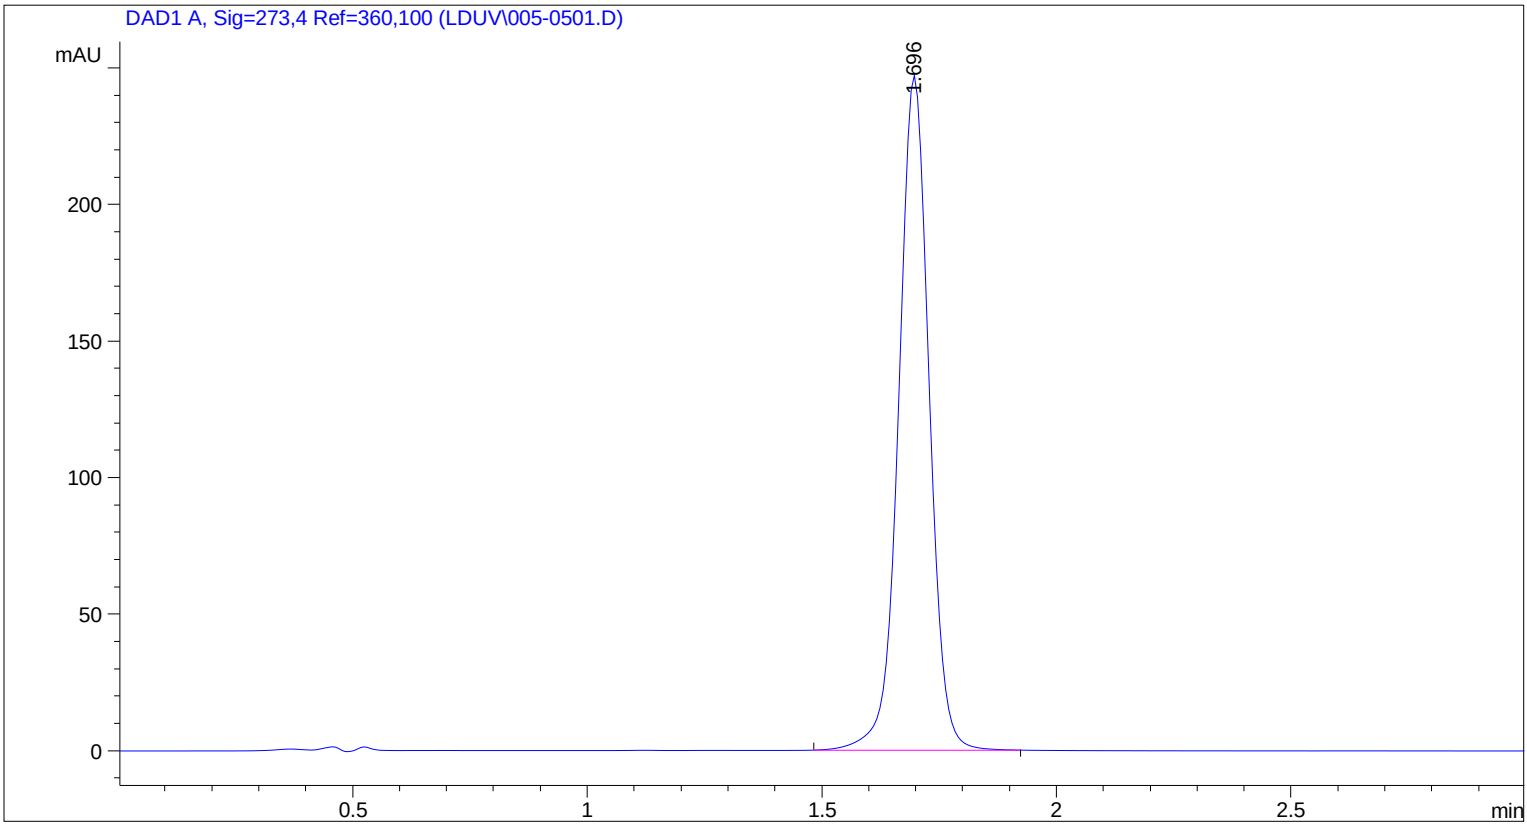

External Standard Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Data File C:\CHEM32\1\DATA\LDUV\005-0501.D
Sample Name: LDUV 5


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.696	BB	0.0708	1119.49707	247.20007	100.0000
Totals :				1119.49707	247.20007	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LIIN\001-0101.D
Sample Name: LIIN 1

```
==========================================================================
Acq. Operator   : Michael                          Seq. Line :   1
Acq. Instrument : Instrument 1                      Location : Vial 1
Injection Date  : 8/8/2018 4:26:42 PM                    Inj :   1
                                                  Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 0.1 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

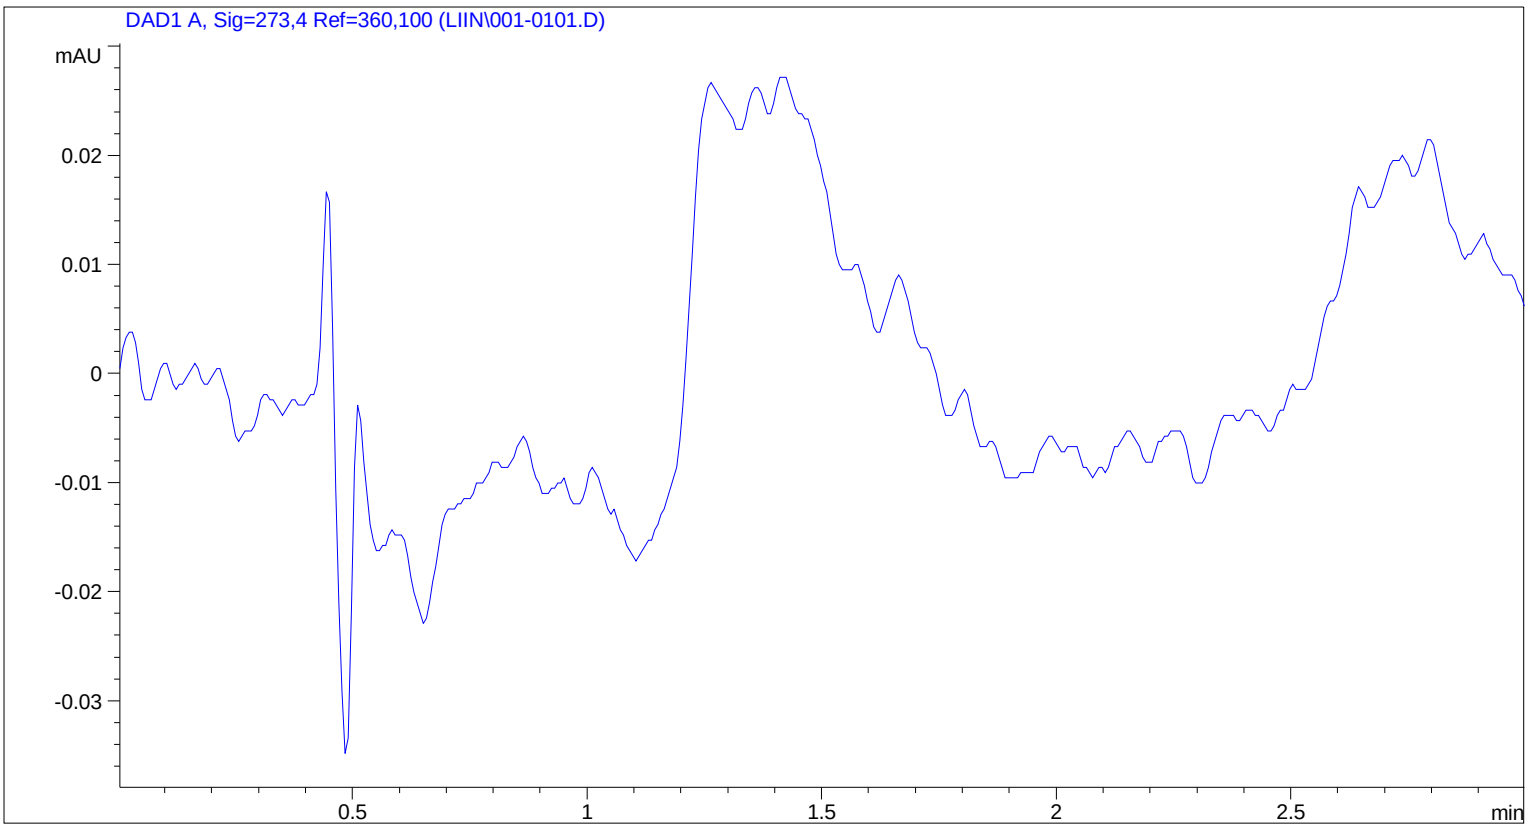


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\1\DATA\LIIN\001-0201.D
Sample Name: LIIN 2

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   2
Acq. Instrument : Instrument 1                    Location : Vial 1
Injection Date  : 8/8/2018 4:31:12 PM                 Inj :   1
                                                  Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 5 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

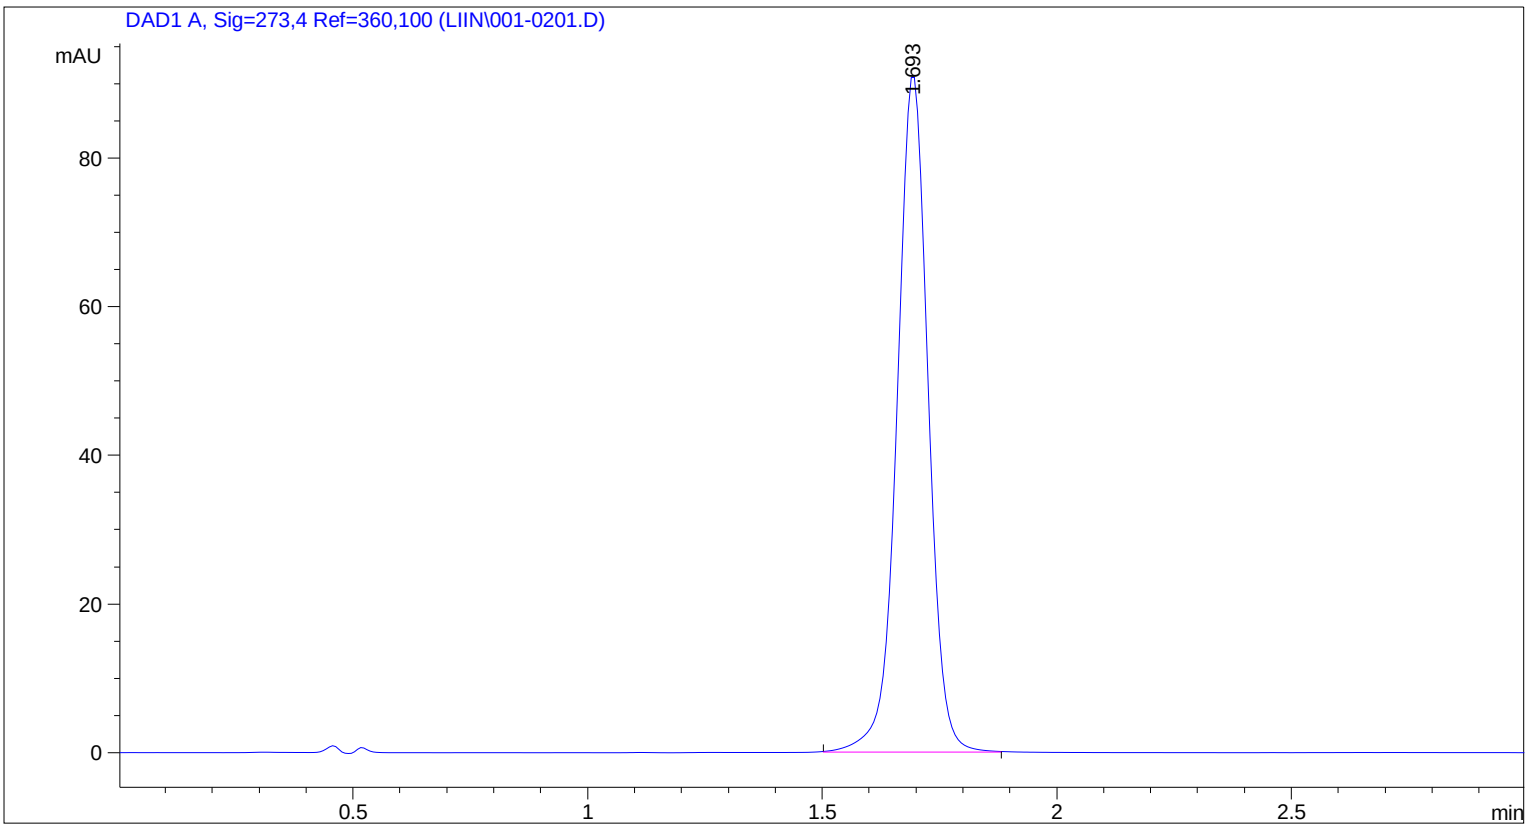


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LIIN\001-0201.D
Sample Name: LIIN 2


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.693	BB	0.0697	420.87579	91.47293	100.0000
Totals :				420.87579	91.47293	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LIIN\001-0301.D
Sample Name: LIIN 3

```
================================================================================
Acq. Operator   : Michael                          Seq. Line :   3
Acq. Instrument : Instrument 1                      Location : Vial 1
Injection Date  : 8/8/2018 4:35:46 PM                    Inj :   1
                                                  Inj Volume : 10 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

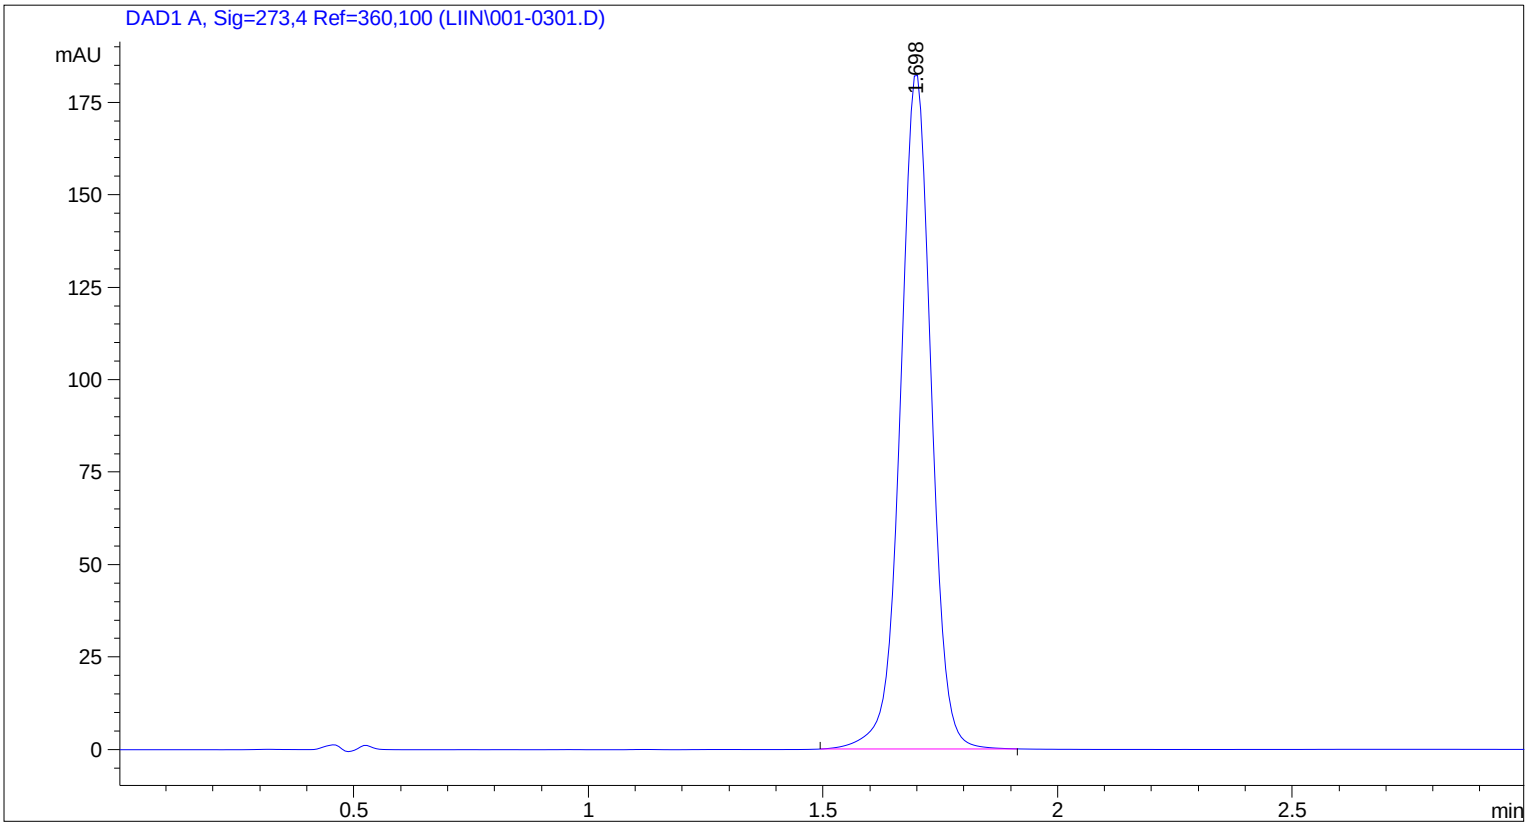


```
================================================================================
                      External Standard Report
================================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
================================================================================
================================================================================
                         Area Percent Report
================================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LIIN\001-0301.D
Sample Name: LIIN 3


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.698	BB	0.0694	839.53192	183.38367	100.0000
Totals :				839.53192	183.38367	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LIIN\001-0401.D
Sample Name: LIIN 4

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   4
Acq. Instrument : Instrument 1                    Location : Vial 1
Injection Date  : 8/8/2018 4:40:20 PM                 Inj :   1
                                                 Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 15 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

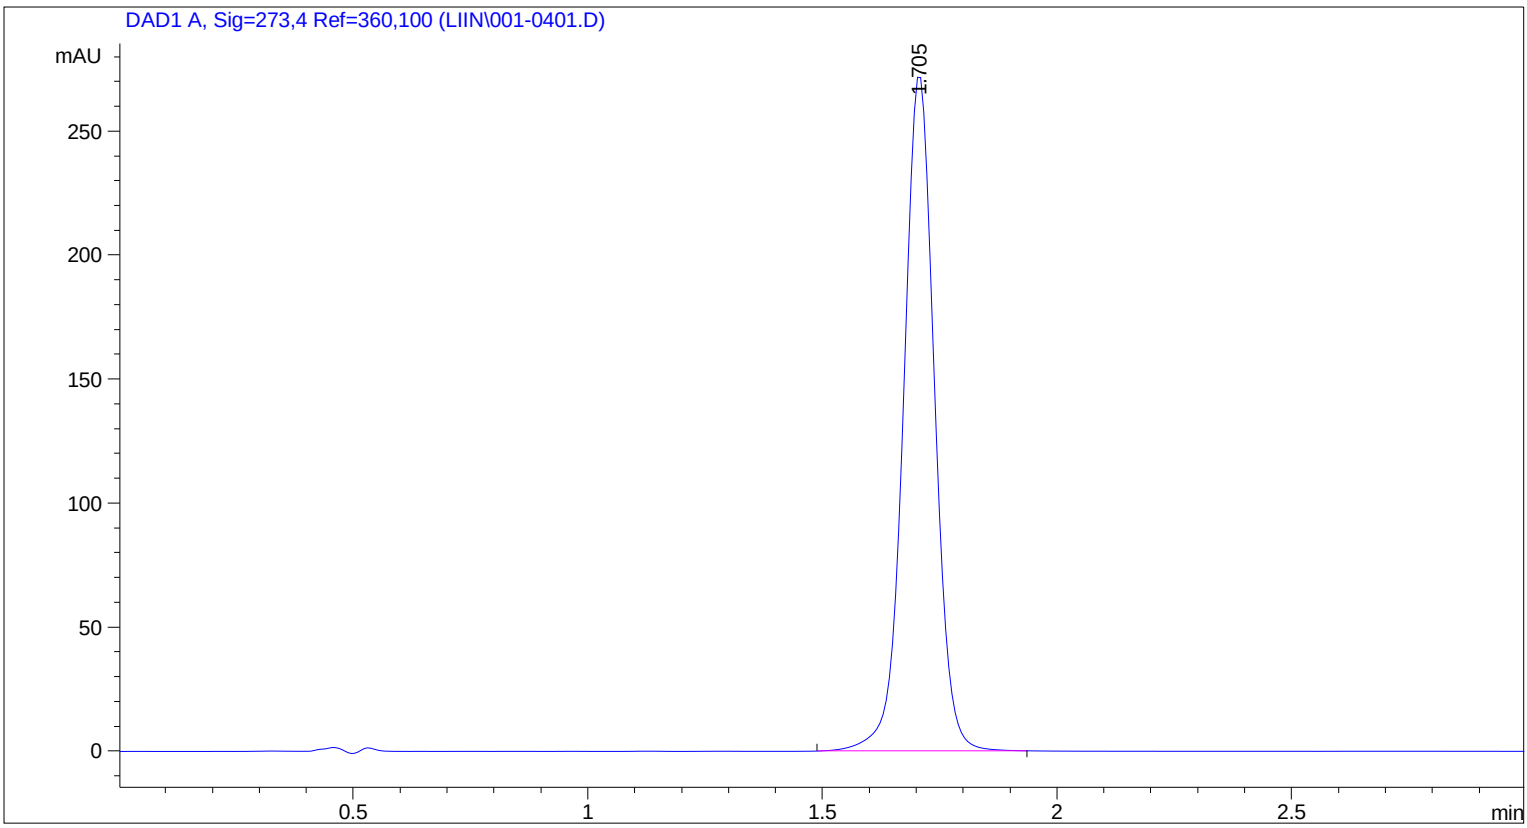


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LIIN\001-0401.D
Sample Name: LIIN 4


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.705	BB	0.0697	1258.19910	273.42767	100.0000
Totals :				1258.19910	273.42767	

*** End of Report ***

Data File C:\CHEM32\1\DATA\LIIN\001-0501.D
Sample Name: LIIN 5

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   5
Acq. Instrument : Instrument 1                    Location : Vial 1
Injection Date  : 8/8/2018 4:45:05 PM                  Inj :   1
                                                 Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 20 µl
Acq. Method     : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 2:50:58 PM by Kelen
Analysis Method : C:\CHEM32\1\METHODS\QUALIFICACAO2018.M
Last changed    : 8/8/2018 4:07:50 PM by Kelen
                  (modified after loading)
```

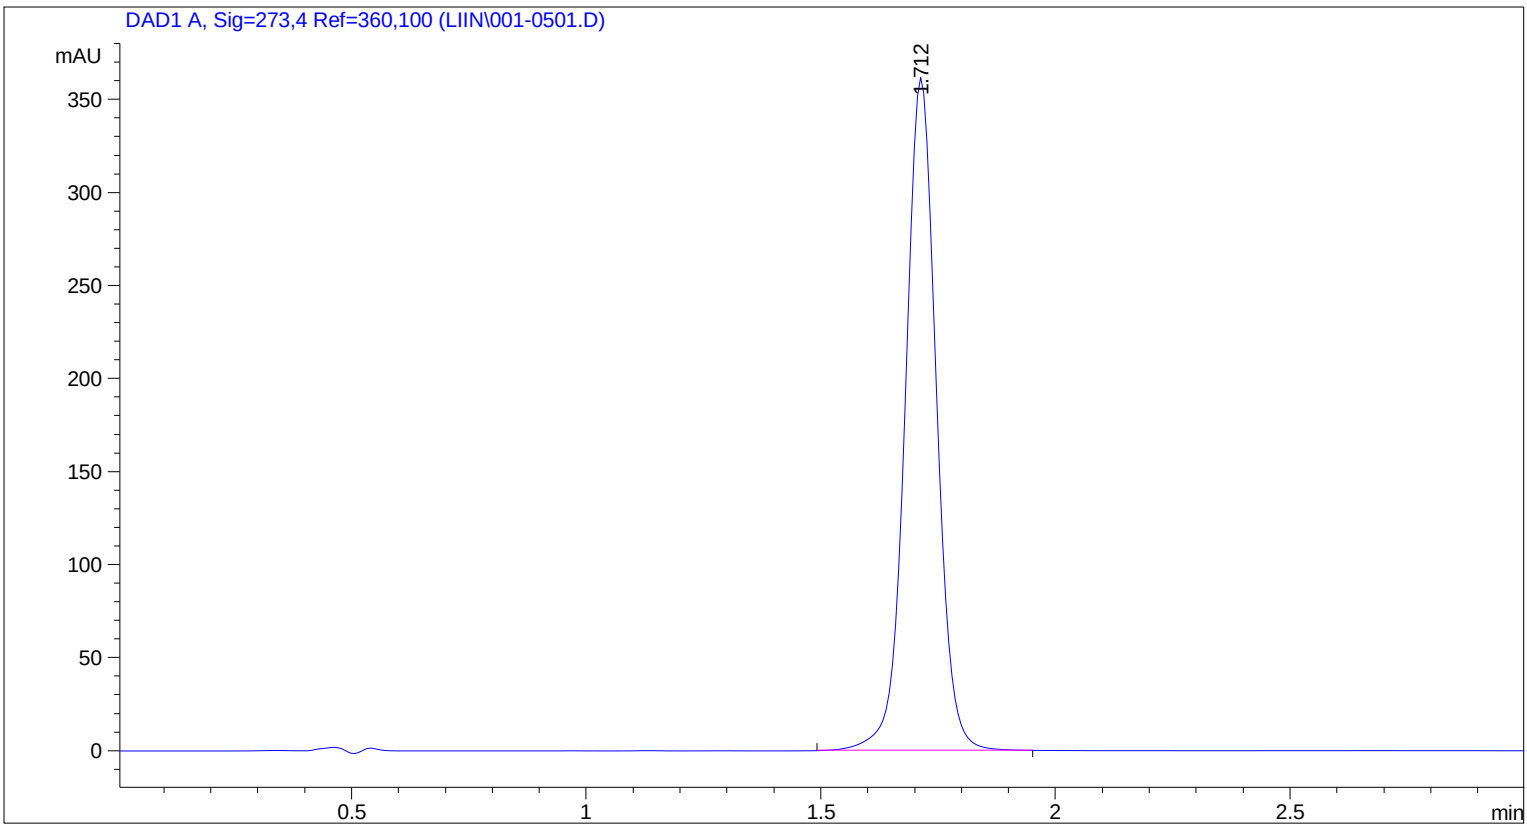


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Data File C:\CHEM32\1\DATA\LIIN\001-0501.D
Sample Name: LIIN 5


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.712	BB	0.0720	1676.14014	361.95792	100.0000
Totals :				1676.14014	361.95792	

*** End of Report ***

Data File C:\CHEM32\1\DATA\GRAD AB\001-0101.D
Sample Name: Grad AB

```
==========================================================================
Acq. Operator   : Michael                        Seq. Line :   1
Acq. Instrument : Instrument 1                    Location : Vial 1
Injection Date  : 8/9/2018 8:47:40 AM                  Inj :   1
                                                 Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 0.1 µl
Acq. Method     : C:\CHEM32\1\METHODS\GRAD AB2018.M
Last changed    : 8/8/2018 5:18:44 PM by Michael
Analysis Method : C:\CHEM32\1\METHODS\GRAD AB2018.M
Last changed    : 8/9/2018 9:12:08 AM by Michael
                  (modified after loading)
```

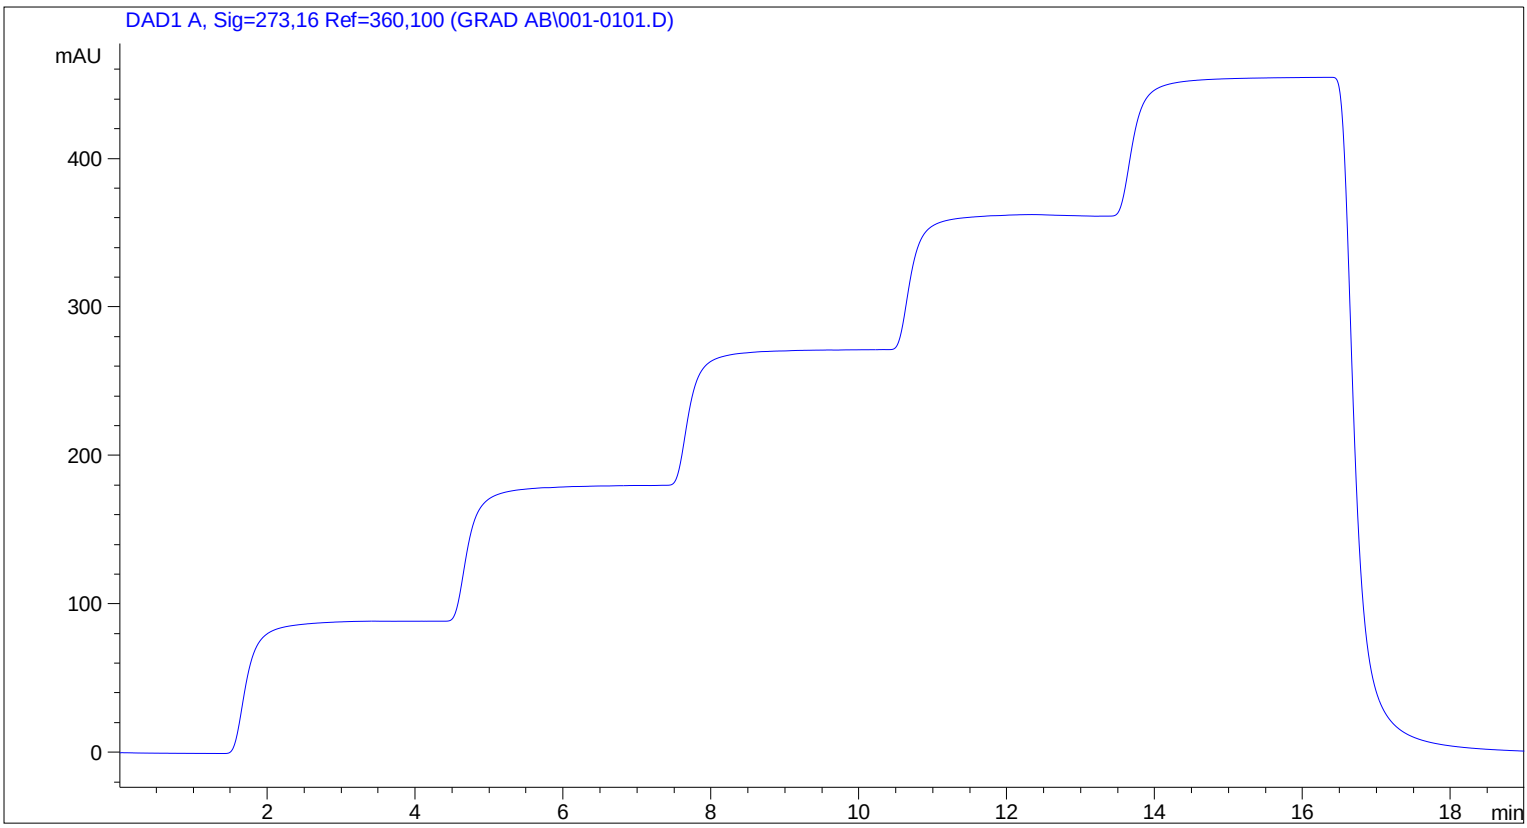


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\1\DATA\GRAD CD\001-0101.D
Sample Name: Grad CD

```
==========================================================================
Acq. Operator   : Michael                          Seq. Line :   1
Acq. Instrument : Instrument 1                      Location : Vial 1
Injection Date  : 8/9/2018 9:11:39 AM                    Inj :   1
                                                  Inj Volume : 10 µl
Different Inj Volume from Sequence !     Actual Inj Volume : 0.1 µl
Acq. Method     : C:\CHEM32\1\METHODS\GRAD CD2018.M
Last changed    : 8/8/2018 5:21:27 PM by Michael
Analysis Method : C:\CHEM32\1\METHODS\GRAD CD2018.M
Last changed    : 8/9/2018 9:32:45 AM by Michael
                  (modified after loading)
```

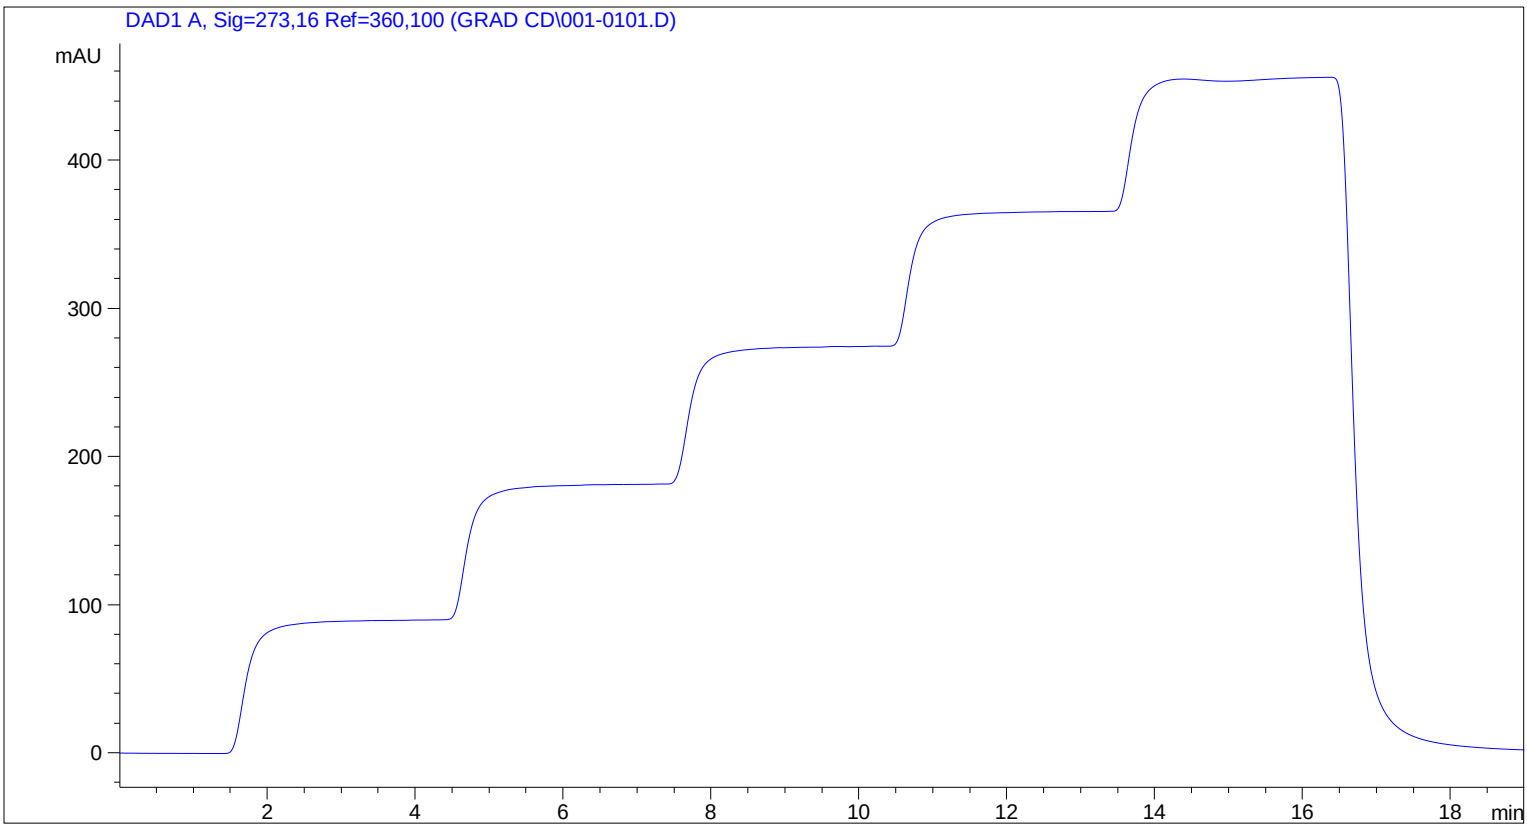


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```