
SAMPLE INFORMATION

Sample Name:	200	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	200
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:09:13 AMT		
Date Processed:	22/07/2021 09:08:48 AMT		

Auto-Scaled Chromatogram

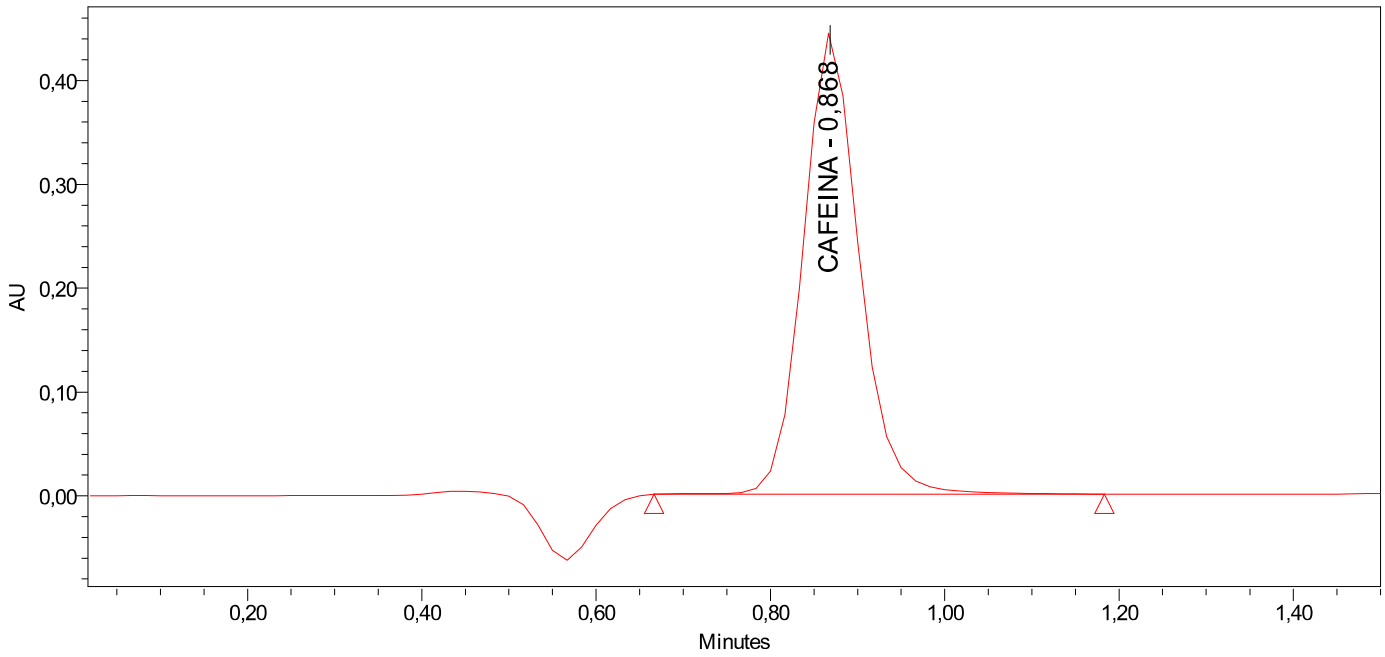


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	1972538	432629		

SAMPLE INFORMATION

Sample Name:	201	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	201
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:11:38 AMT		
Date Processed:	22/07/2021 09:08:56 AMT		

Auto-Scaled Chromatogram

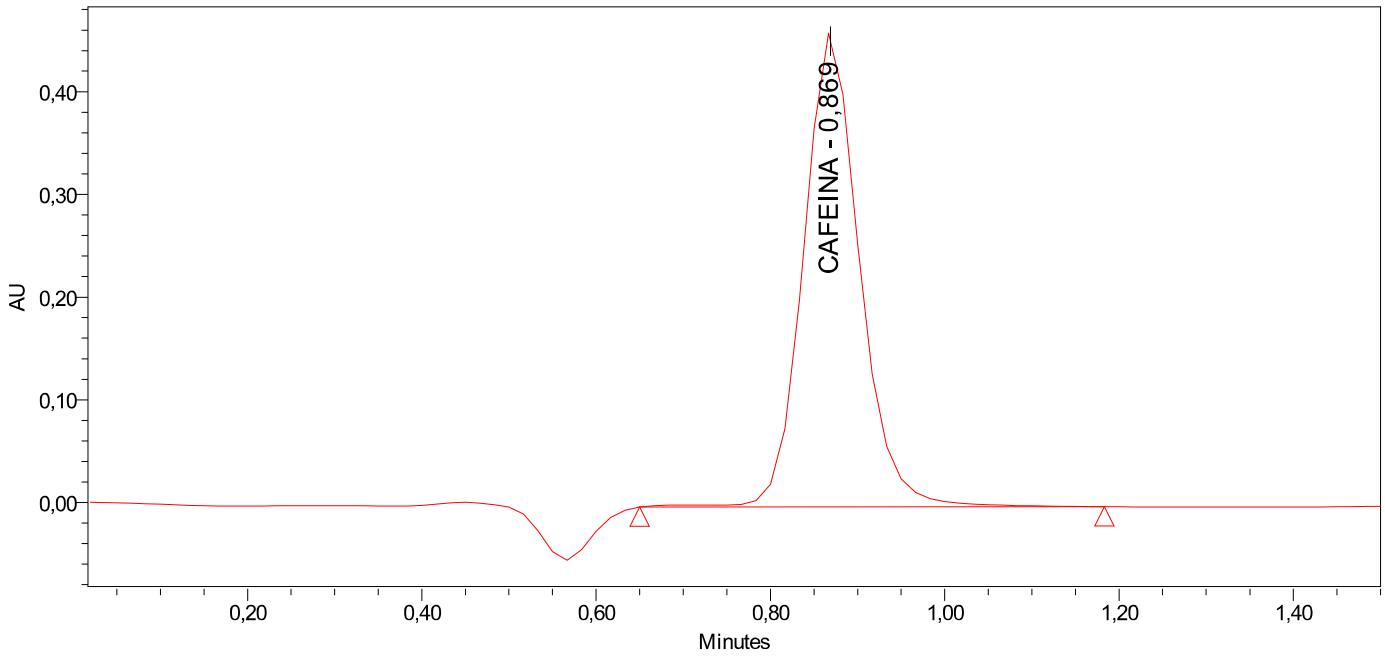


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	2057327	449584		

SAMPLE INFORMATION

Sample Name:	202	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	202
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:14:03 AMT		
Date Processed:	22/07/2021 09:09:03 AMT		

Auto-Scaled Chromatogram

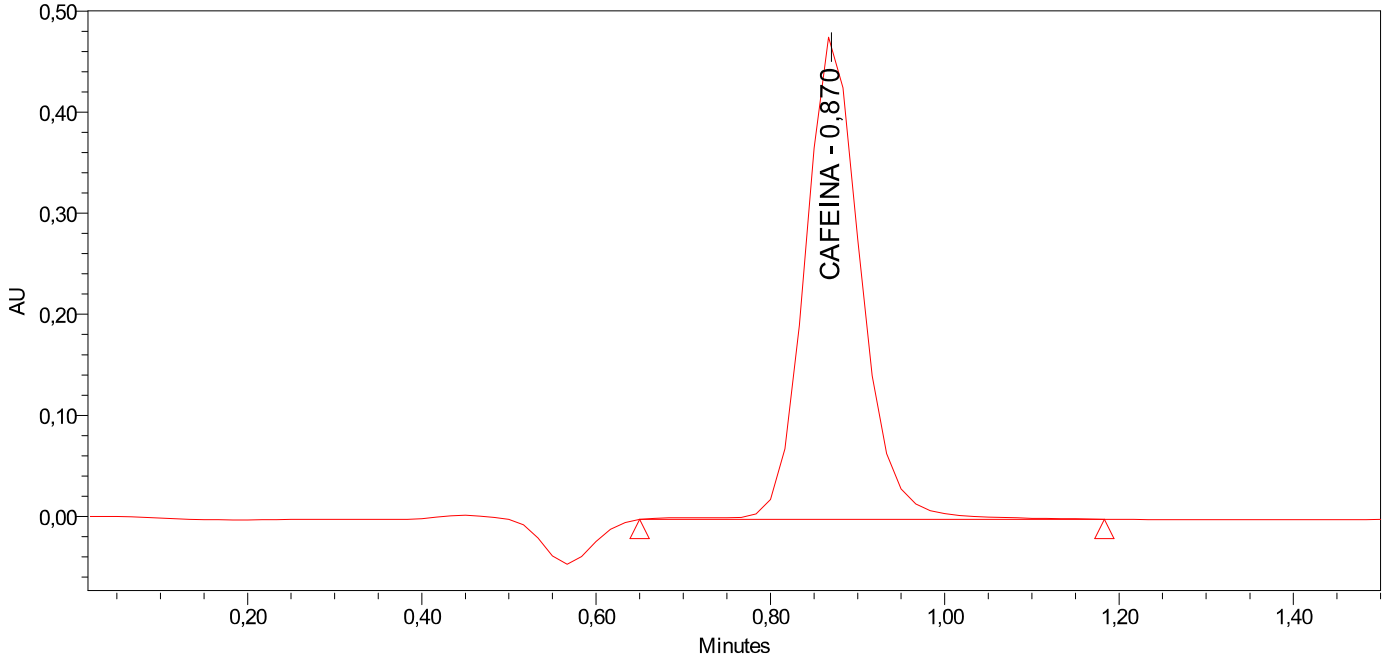


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,870	2128179	466040		

SAMPLE INFORMATION

Sample Name:	203	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	203
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:16:28 AMT		
Date Processed:	22/07/2021 09:09:10 AMT		

Auto-Scaled Chromatogram

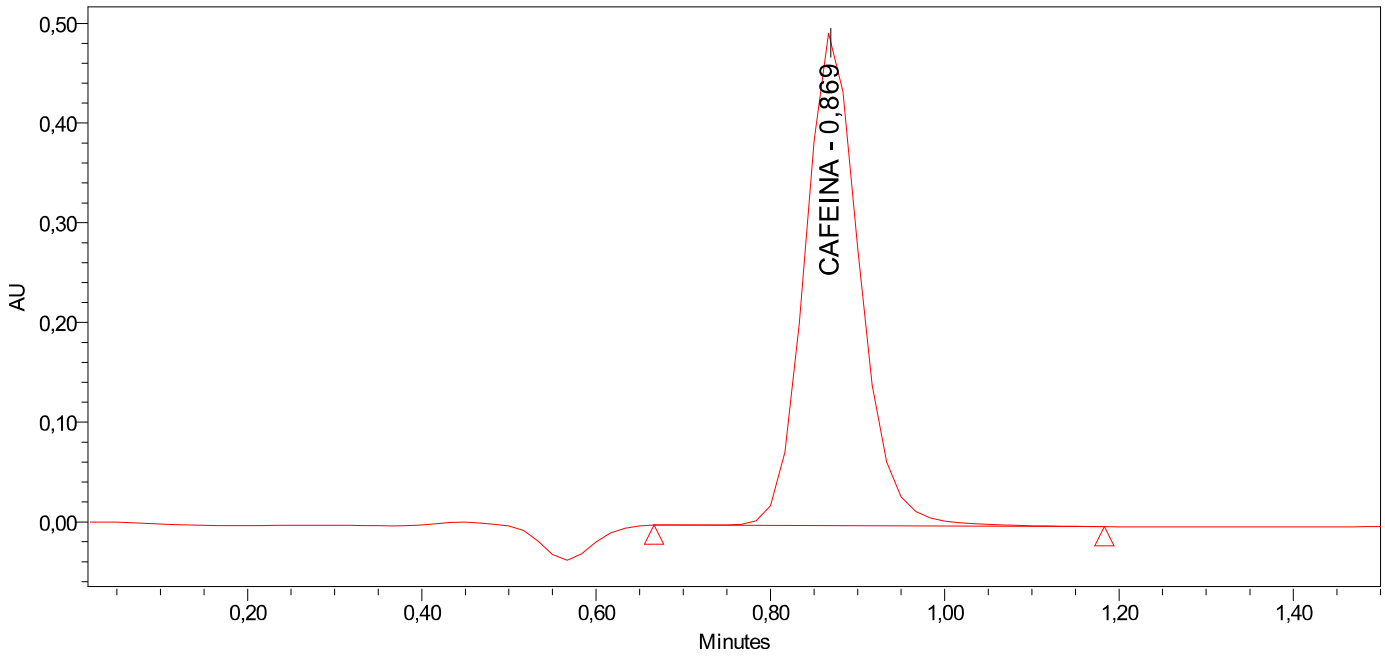


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	2170965	481713		

SAMPLE INFORMATION

Sample Name:	204	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	204
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:18:53 AMT		
Date Processed:	22/07/2021 09:09:19 AMT		

Auto-Scaled Chromatogram

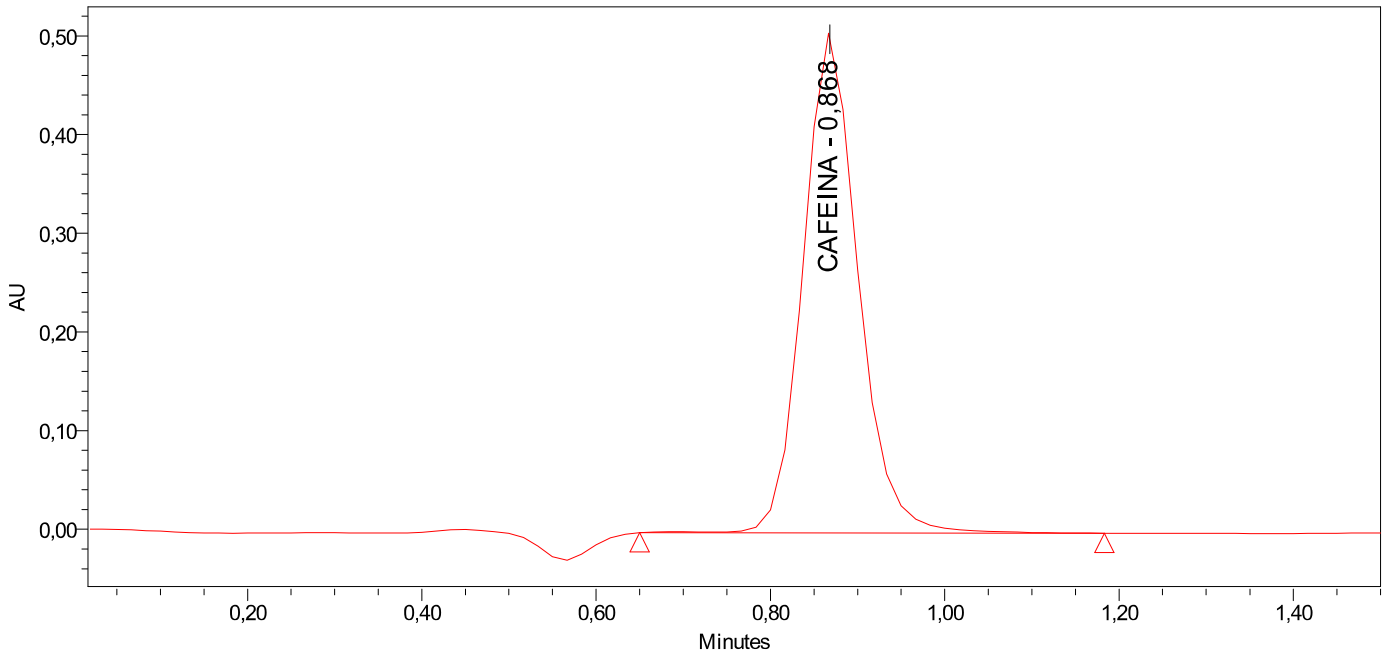


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	2215245	492566		

SAMPLE INFORMATION

Sample Name:	205	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	205
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:21:18 AMT		
Date Processed:	22/07/2021 09:09:27 AMT		

Auto-Scaled Chromatogram

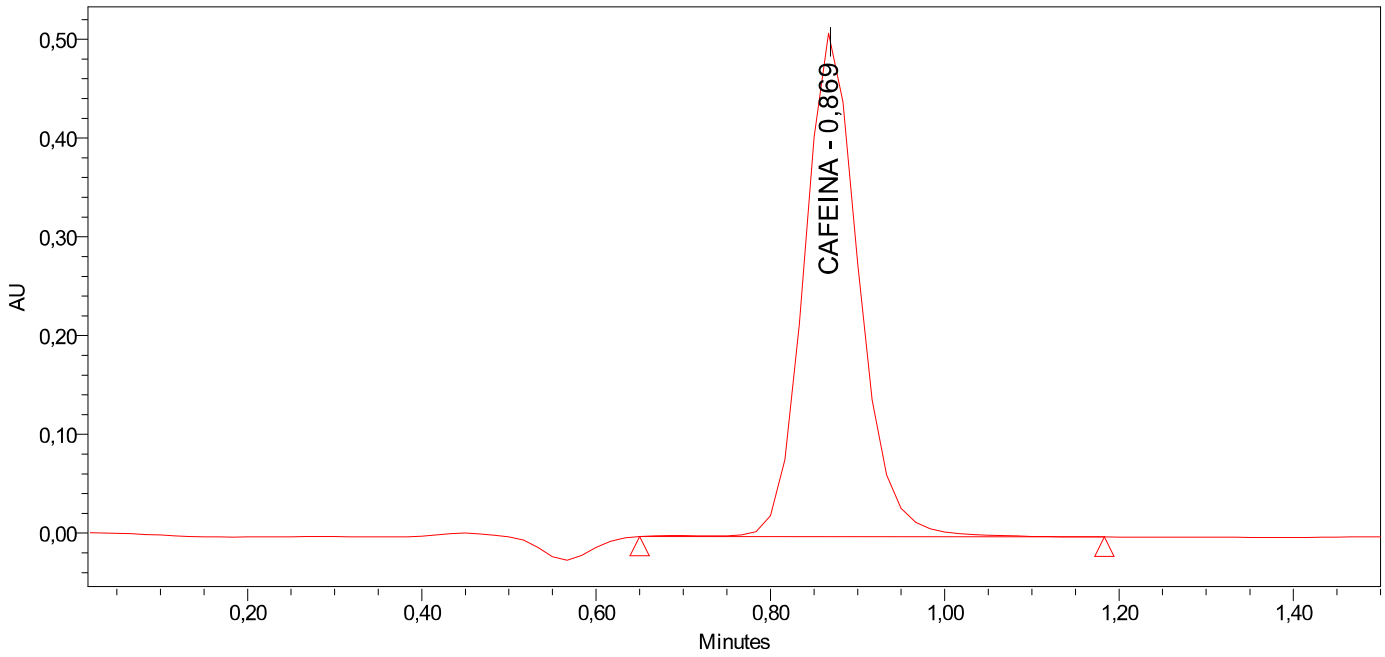


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	2225637	496330		

SAMPLE INFORMATION

Sample Name:	206	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	206
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:23:43 AMT		
Date Processed:	22/07/2021 09:09:41 AMT		

Auto-Scaled Chromatogram

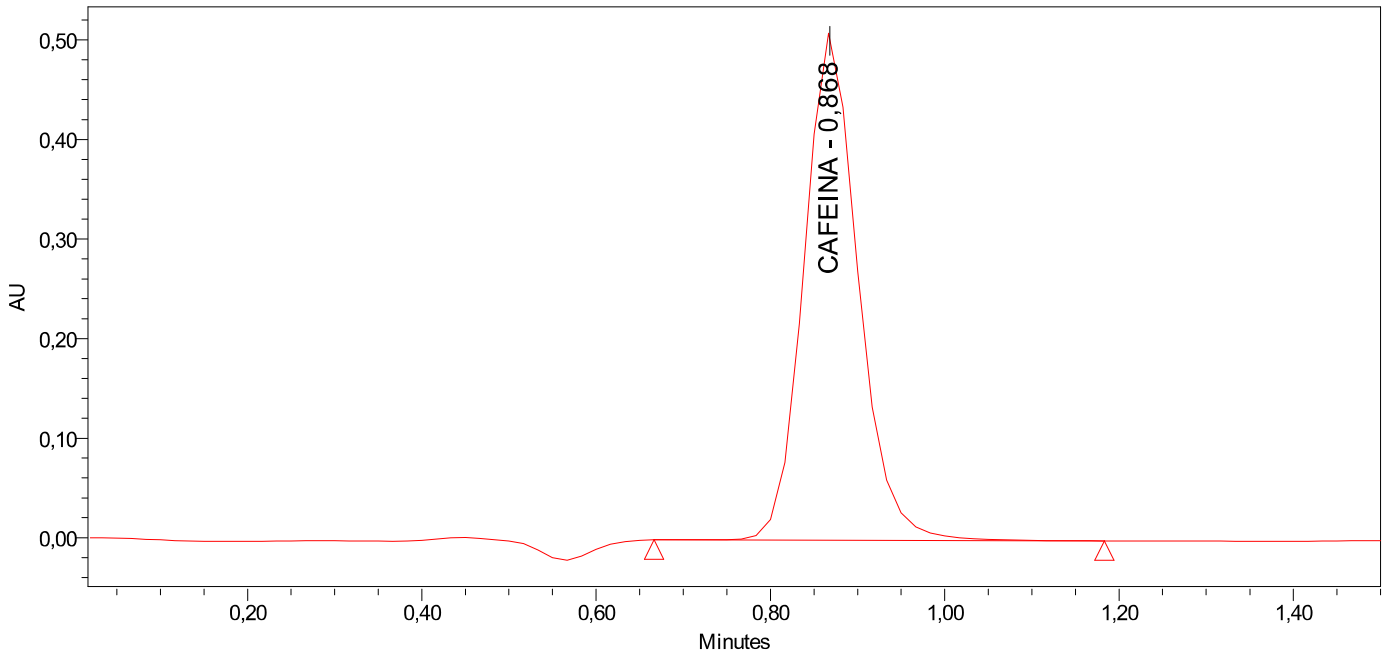


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	2201933	495187		

SAMPLE INFORMATION

Sample Name:	207	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	207
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:26:08 AMT		
Date Processed:	22/07/2021 09:09:50 AMT		

Auto-Scaled Chromatogram

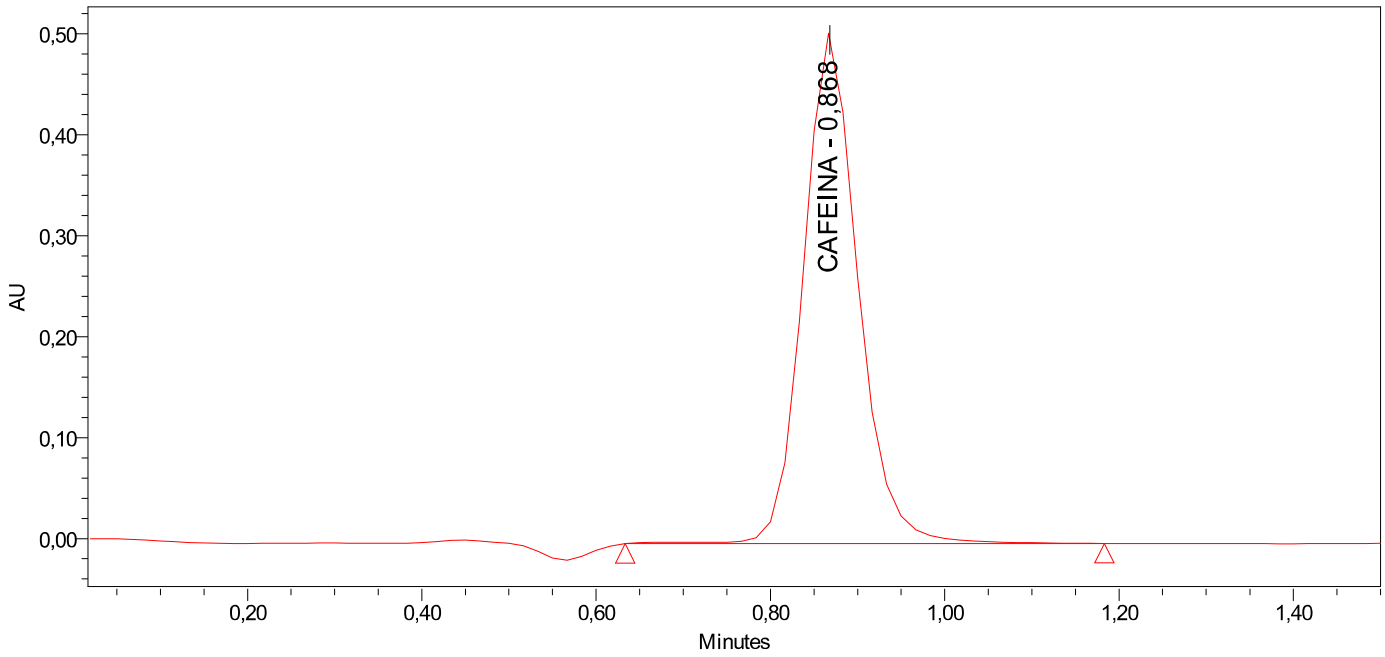


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	2196991	491140		

SAMPLE INFORMATION

Sample Name:	208	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	208
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:28:33 AMT		
Date Processed:	22/07/2021 09:10:00 AMT		

Auto-Scaled Chromatogram

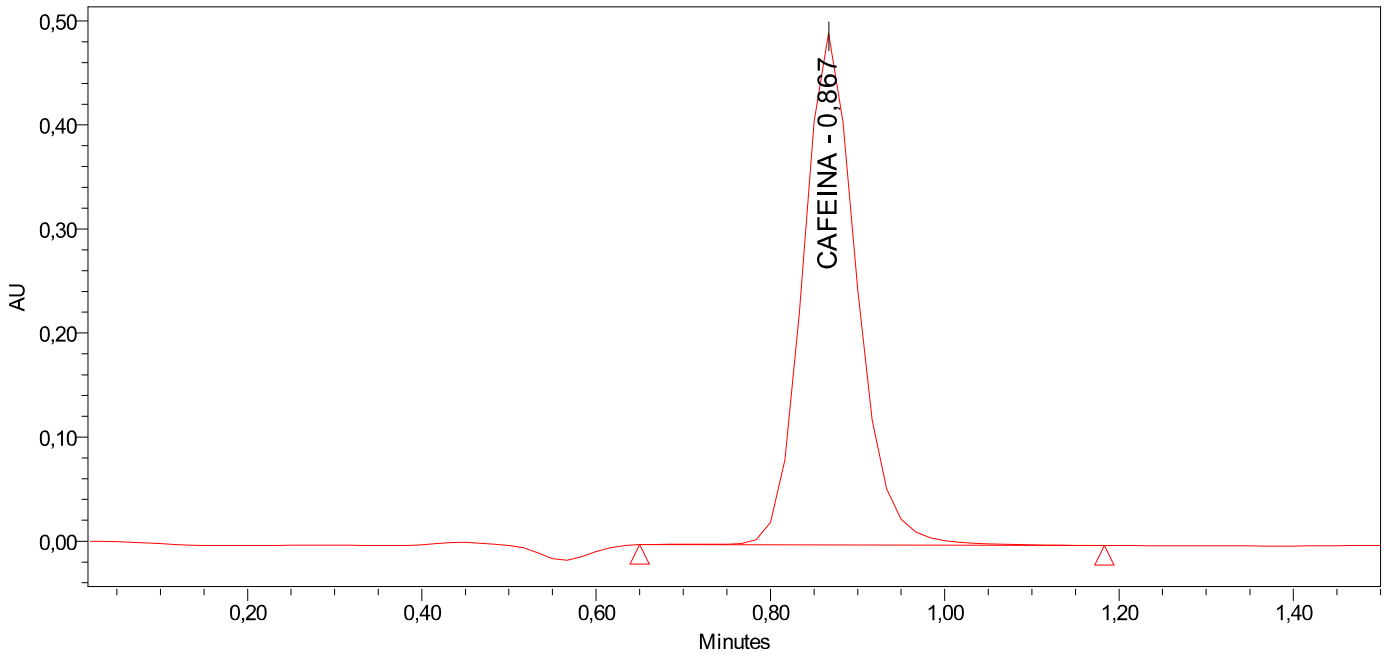


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,867	2120315	477877		

SAMPLE INFORMATION

Sample Name:	209	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	209
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:30:58 AMT		
Date Processed:	22/07/2021 09:10:08 AMT		

Auto-Scaled Chromatogram

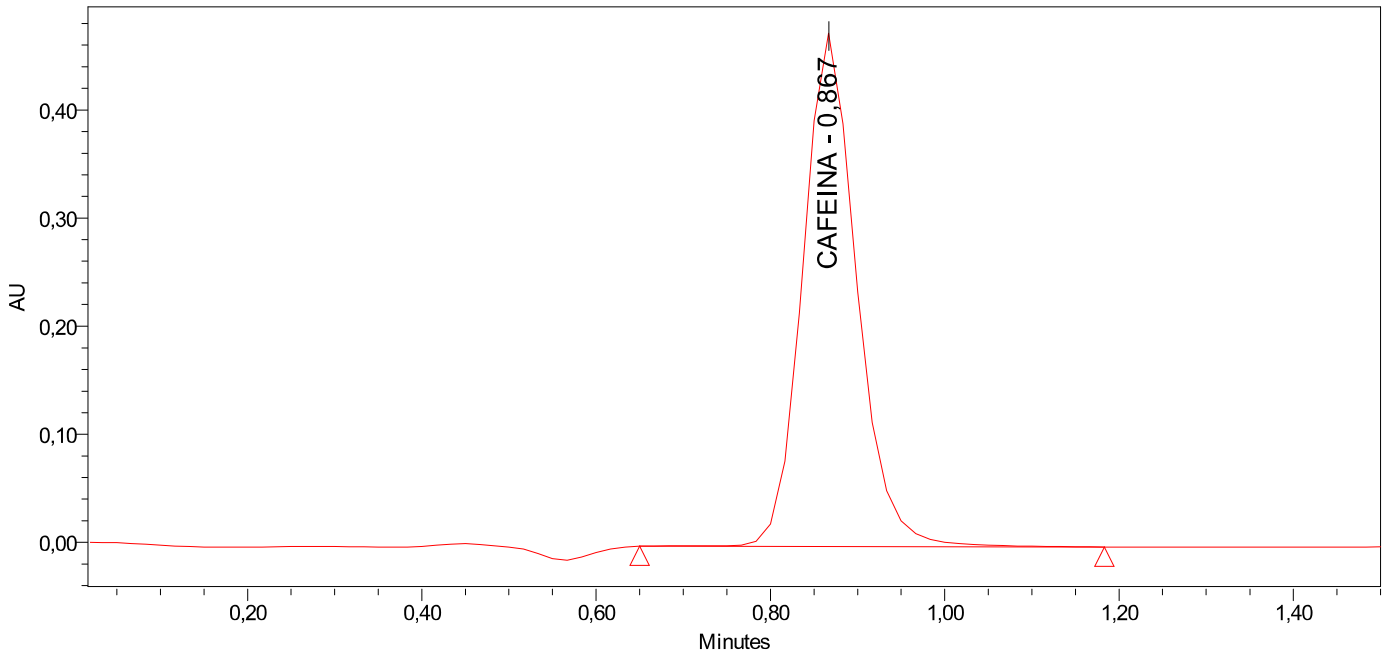


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,867	2041370	461013		

SAMPLE INFORMATION

Sample Name:	210	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	210
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:33:23 AMT		
Date Processed:	22/07/2021 09:10:15 AMT		

Auto-Scaled Chromatogram

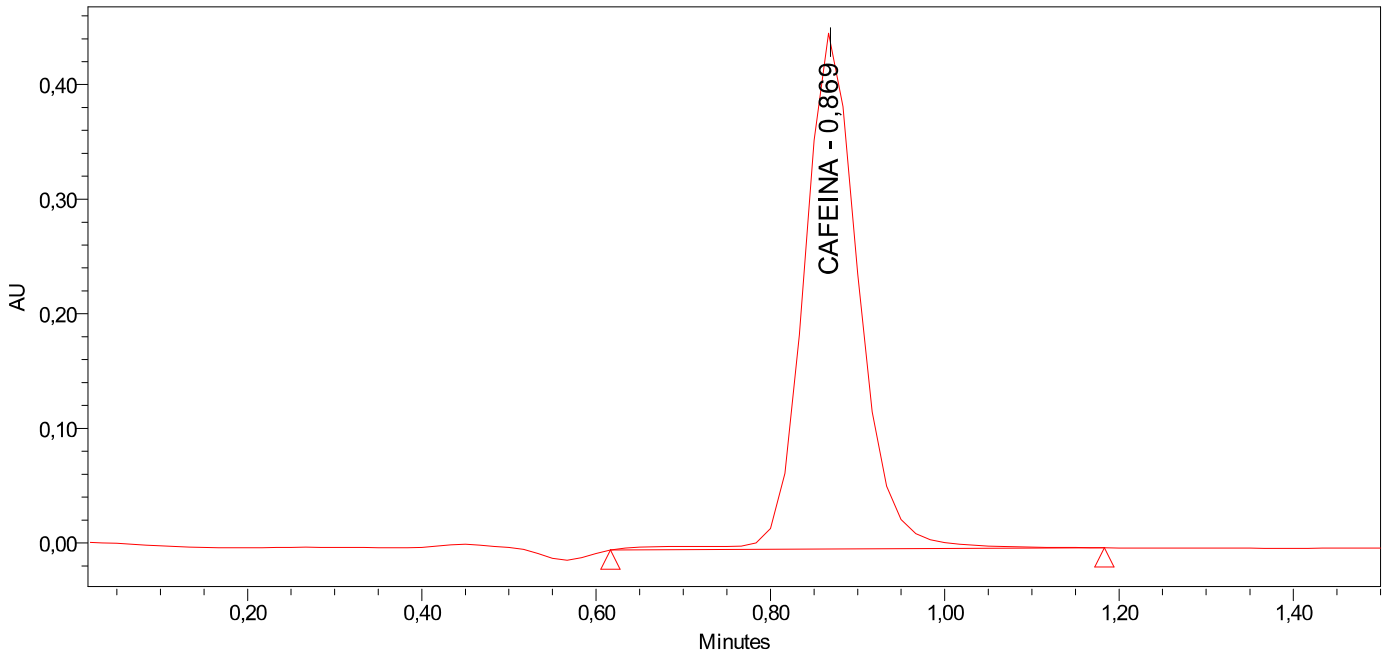


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	1970566	437434		

SAMPLE INFORMATION

Sample Name:	240	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	240
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:35:48 AMT		
Date Processed:	22/07/2021 09:13:52 AMT		

Auto-Scaled Chromatogram

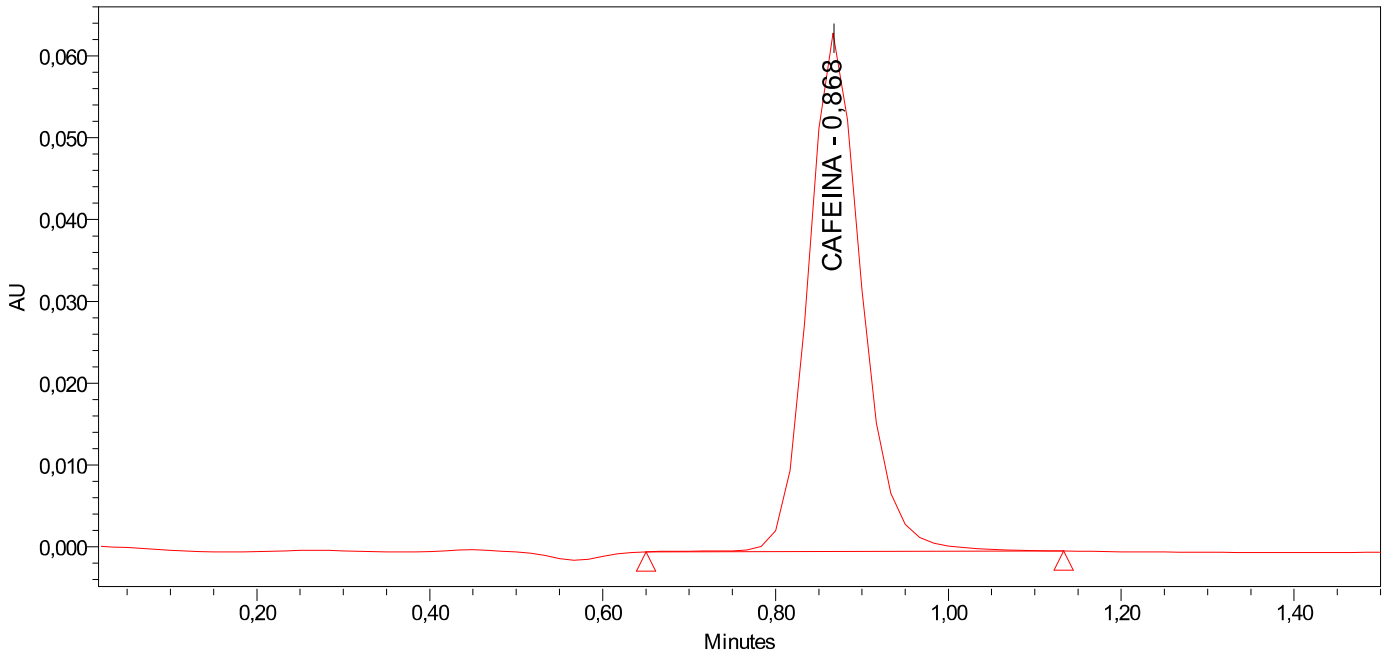


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	272047	61488		

SAMPLE INFORMATION

Sample Name:	241	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	241
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:38:13 AMT		
Date Processed:	22/07/2021 09:13:59 AMT		

Auto-Scaled Chromatogram

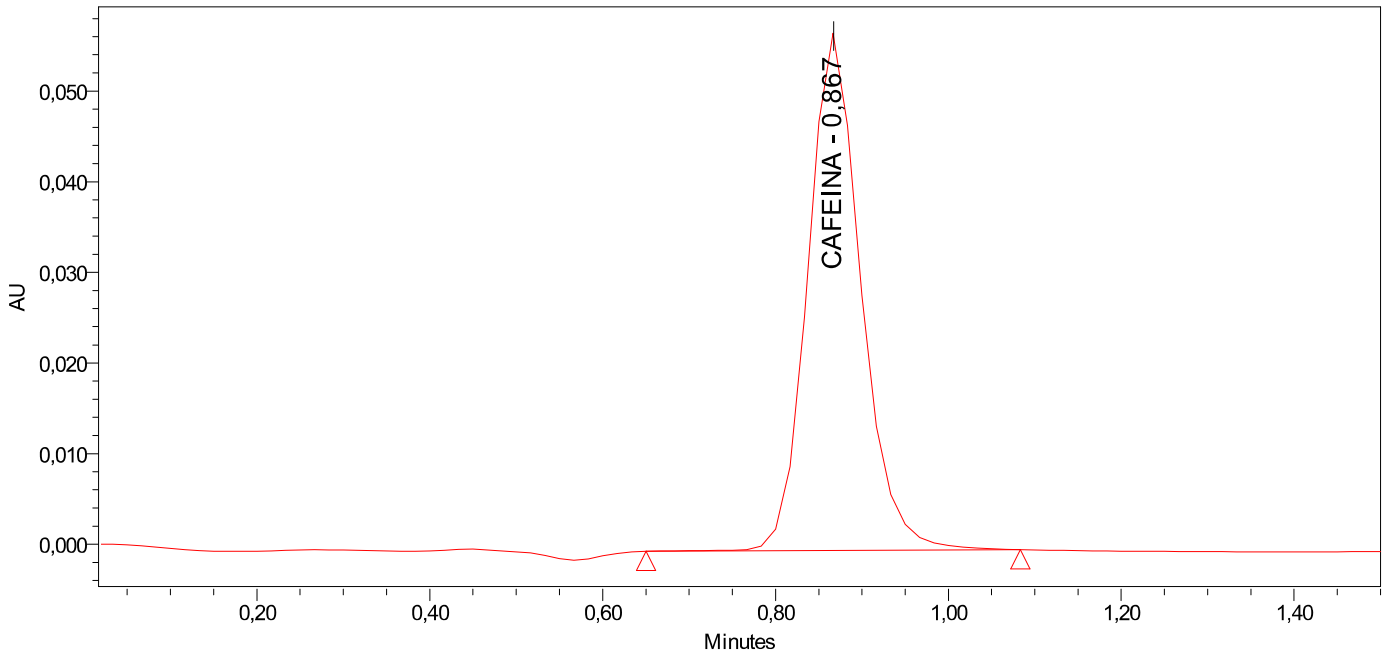


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,867	243811	55400		

SAMPLE INFORMATION

Sample Name:	242	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	242
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:40:38 AMT		
Date Processed:	22/07/2021 09:14:09 AMT		

Auto-Scaled Chromatogram

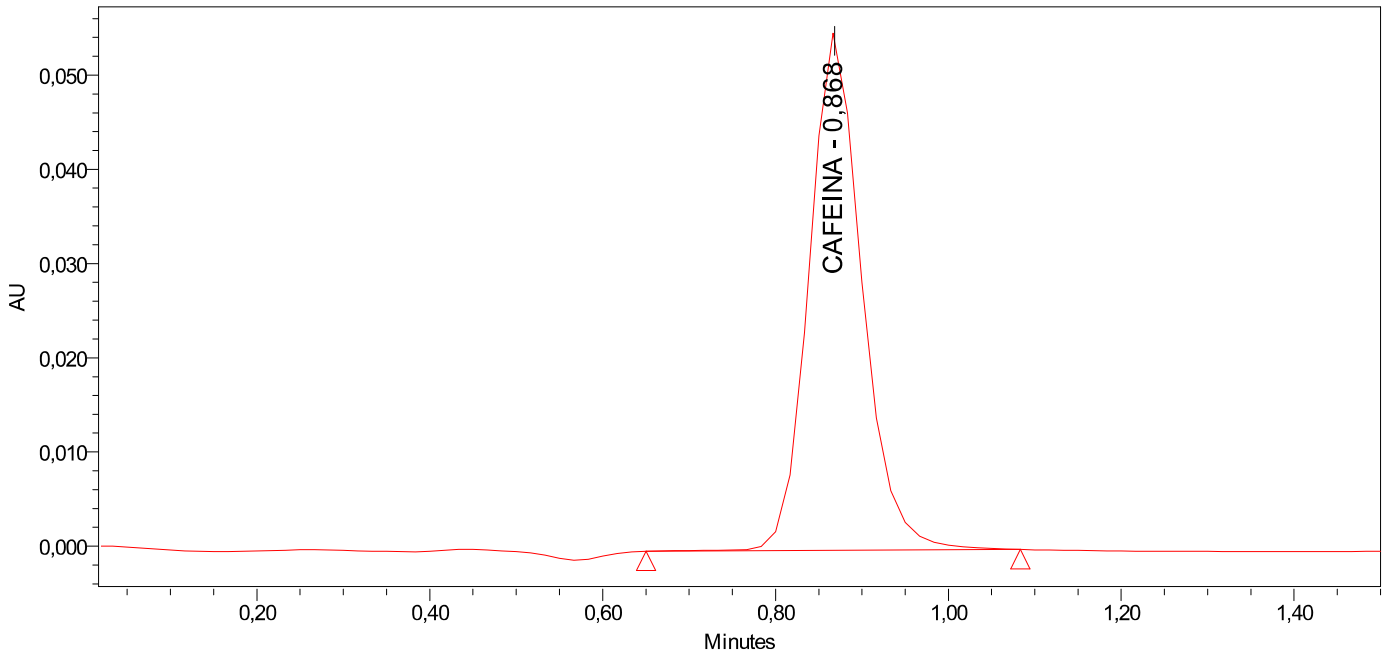


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,868	234484	53301		

SAMPLE INFORMATION

Sample Name:	243	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	243
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:43:03 AMT		
Date Processed:	22/07/2021 09:14:10 AMT		

Auto-Scaled Chromatogram

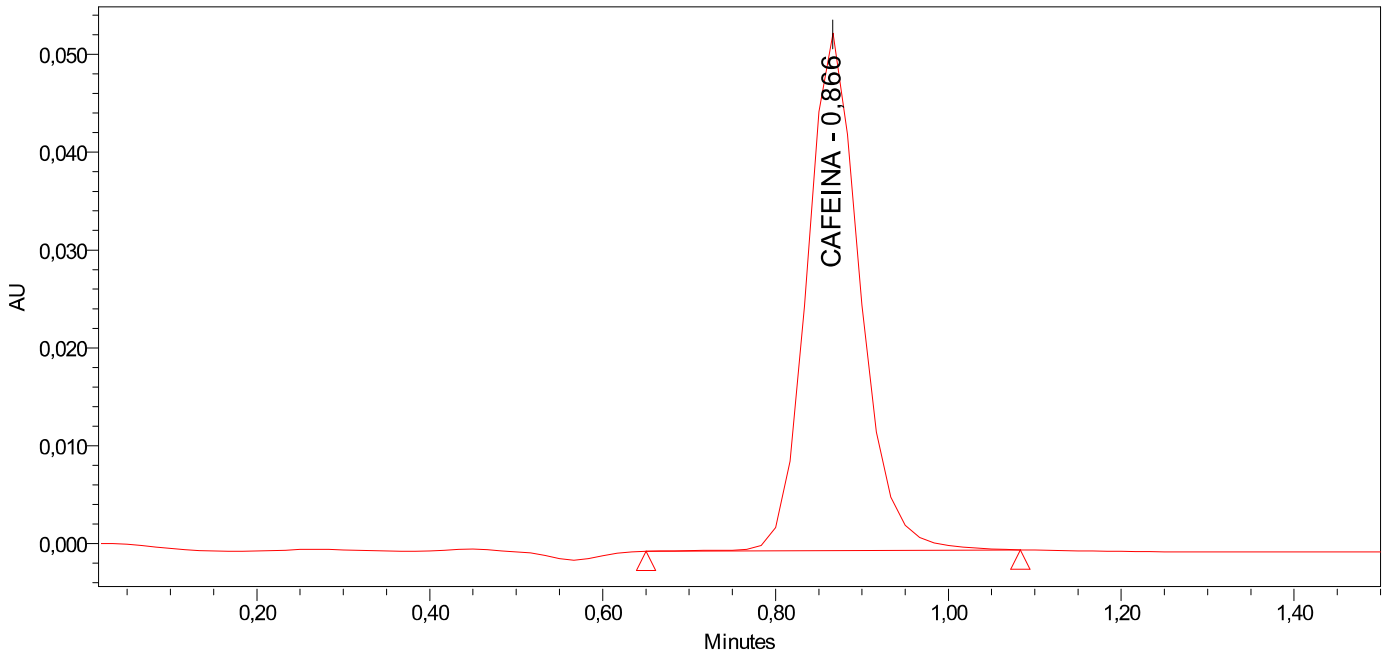


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,866	225870	51330		

SAMPLE INFORMATION

Sample Name:	244	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	244
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:45:28 AMT		
Date Processed:	22/07/2021 09:14:11 AMT		

Auto-Scaled Chromatogram

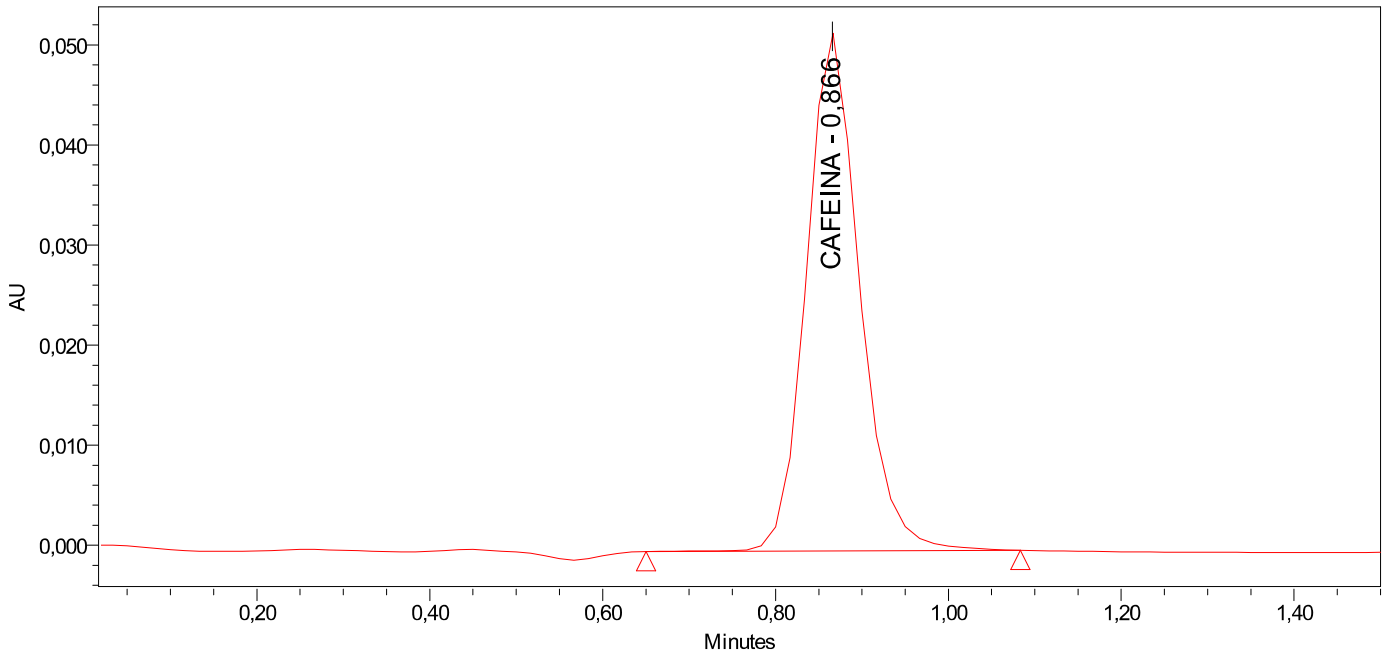


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,866	221217	50271		

SAMPLE INFORMATION

Sample Name:	245	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	245
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:47:53 AMT		
Date Processed:	22/07/2021 09:14:17 AMT		

Auto-Scaled Chromatogram

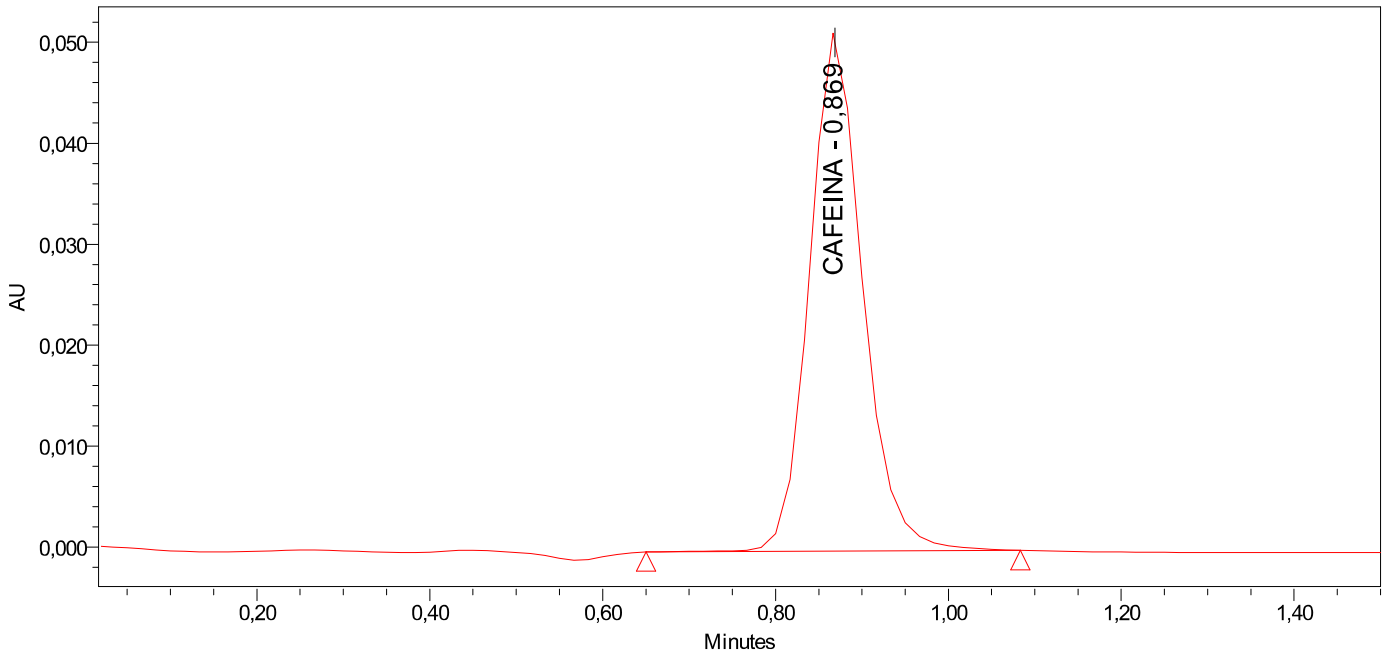


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	219125	49846		

SAMPLE INFORMATION

Sample Name:	246	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	246
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:50:18 AMT		
Date Processed:	22/07/2021 09:14:18 AMT		

Auto-Scaled Chromatogram

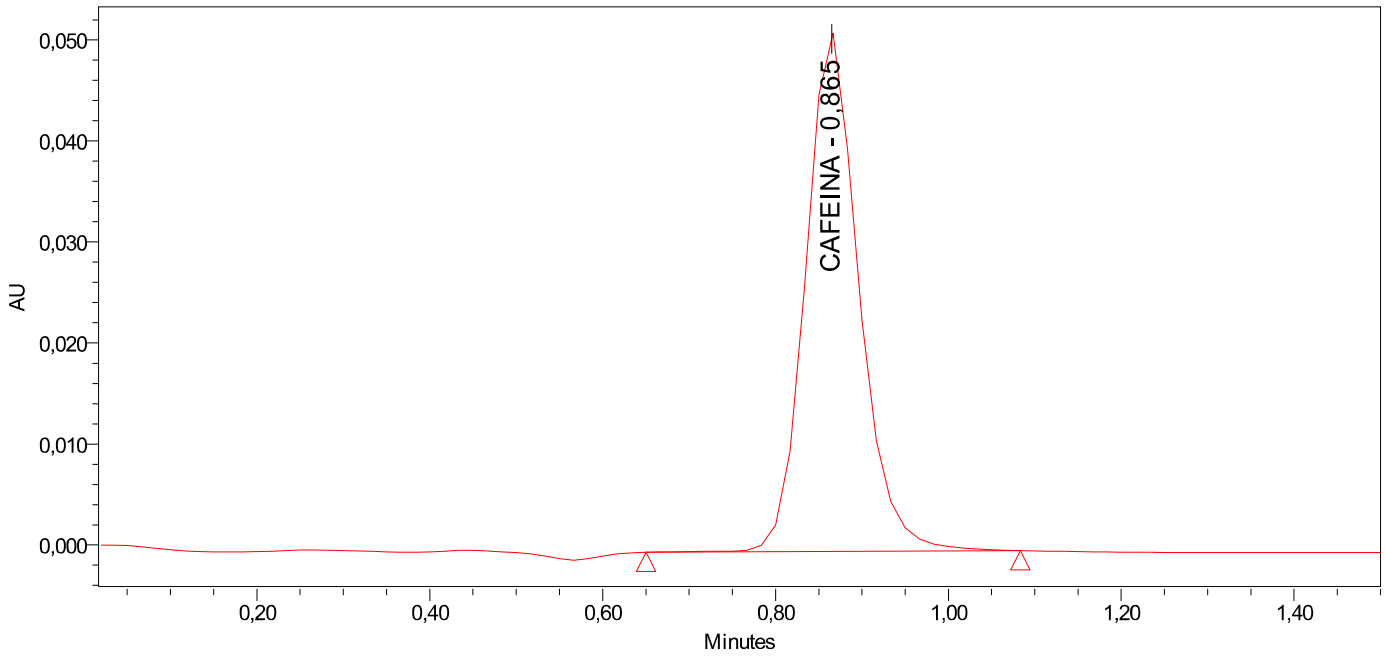


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	220159	49943		

SAMPLE INFORMATION

Sample Name:	247	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	247
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:52:43 AMT		
Date Processed:	22/07/2021 09:14:24 AMT		

Auto-Scaled Chromatogram

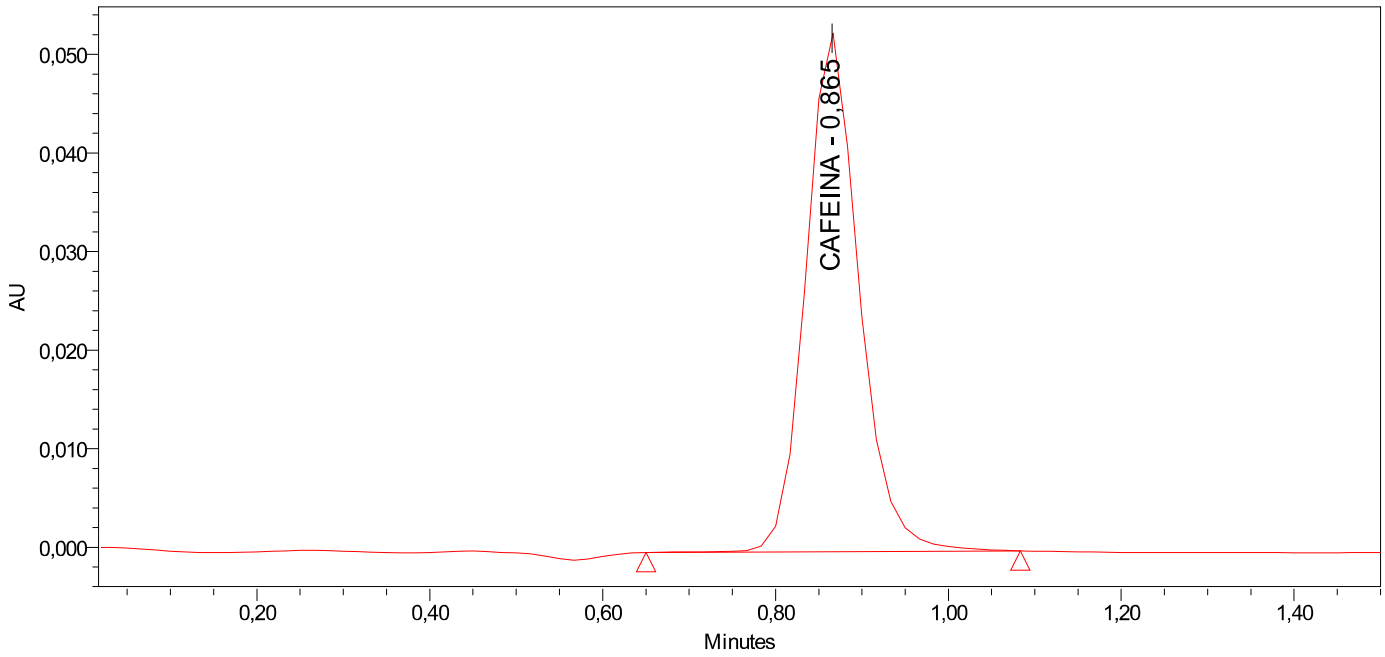


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	225211	51158		

SAMPLE INFORMATION

Sample Name:	248	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	248
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:55:08 AMT		
Date Processed:	22/07/2021 09:14:25 AMT		

Auto-Scaled Chromatogram

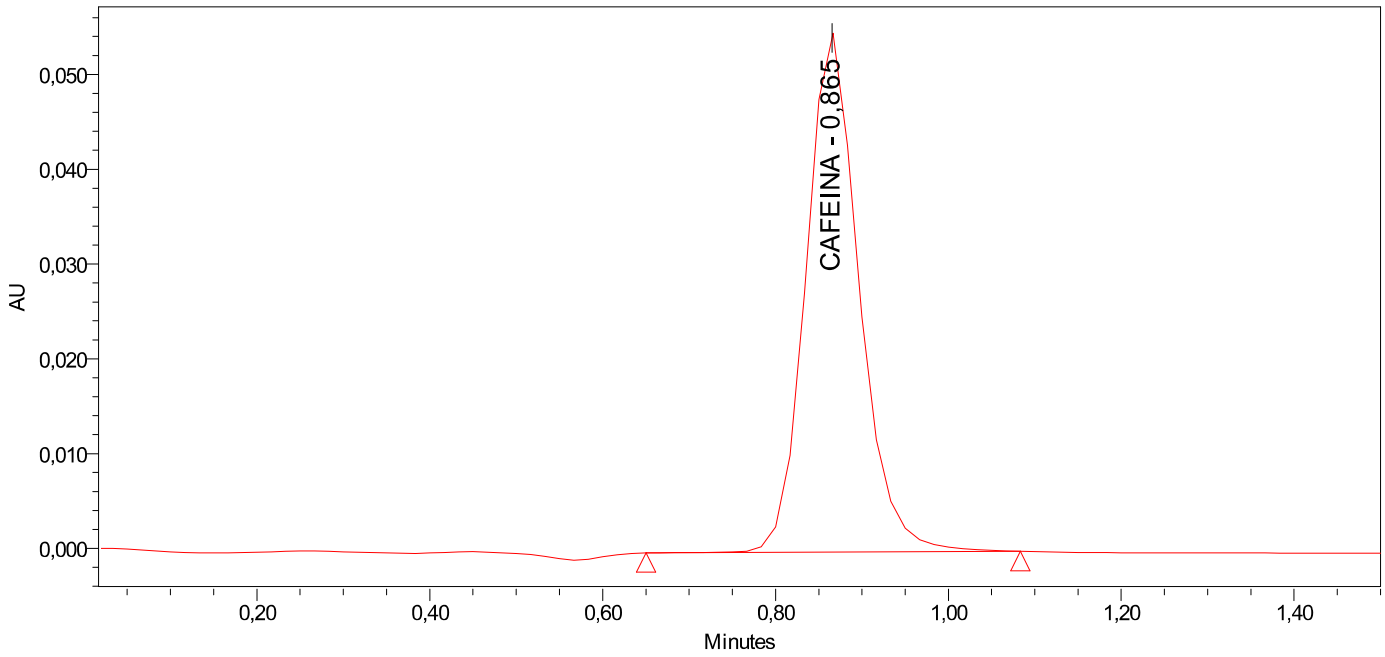


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	234253	53241		

SAMPLE INFORMATION

Sample Name:	249	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	249
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:57:33 AMT		
Date Processed:	22/07/2021 09:14:26 AMT		

Auto-Scaled Chromatogram

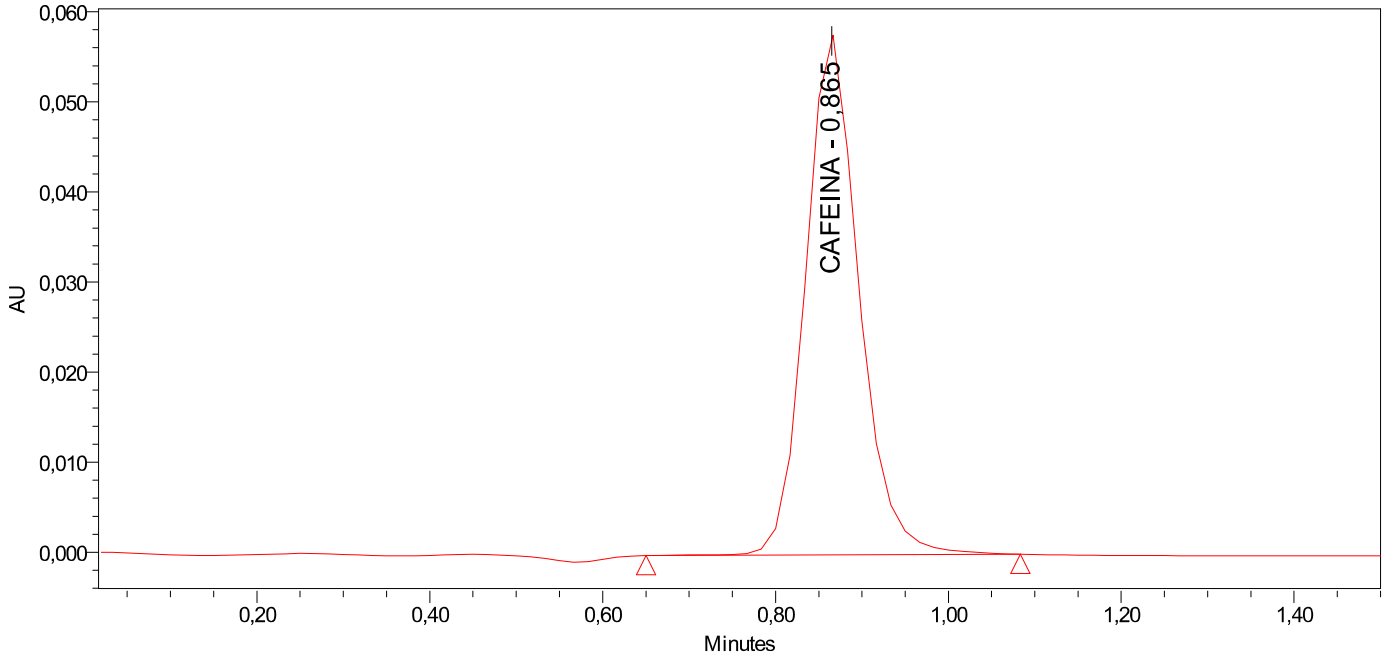


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	247291	56126		

SAMPLE INFORMATION

Sample Name:	250	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	250
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:59:57 AMT		
Date Processed:	22/07/2021 09:14:27 AMT		

Auto-Scaled Chromatogram

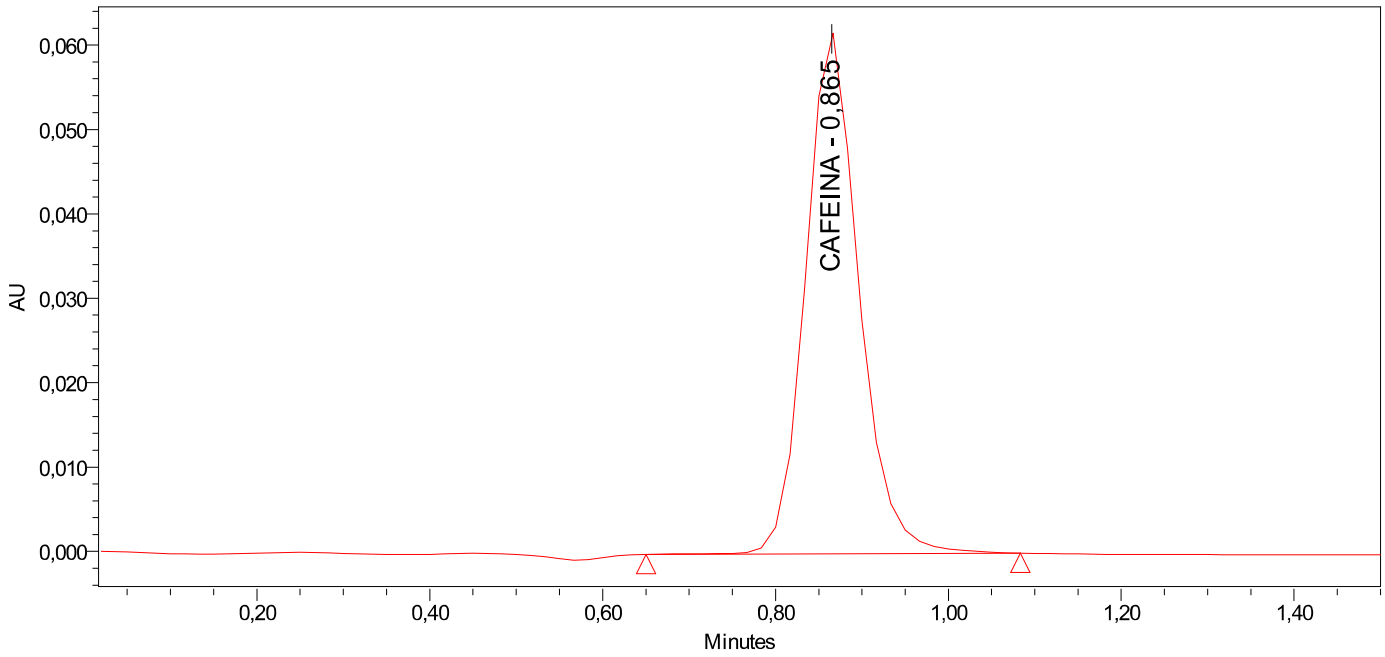


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	264372	60014		

SAMPLE INFORMATION

Sample Name:	268	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	268
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:02:20 AMT		
Date Processed:	22/07/2021 11:59:02 AMT		

Auto-Scaled Chromatogram

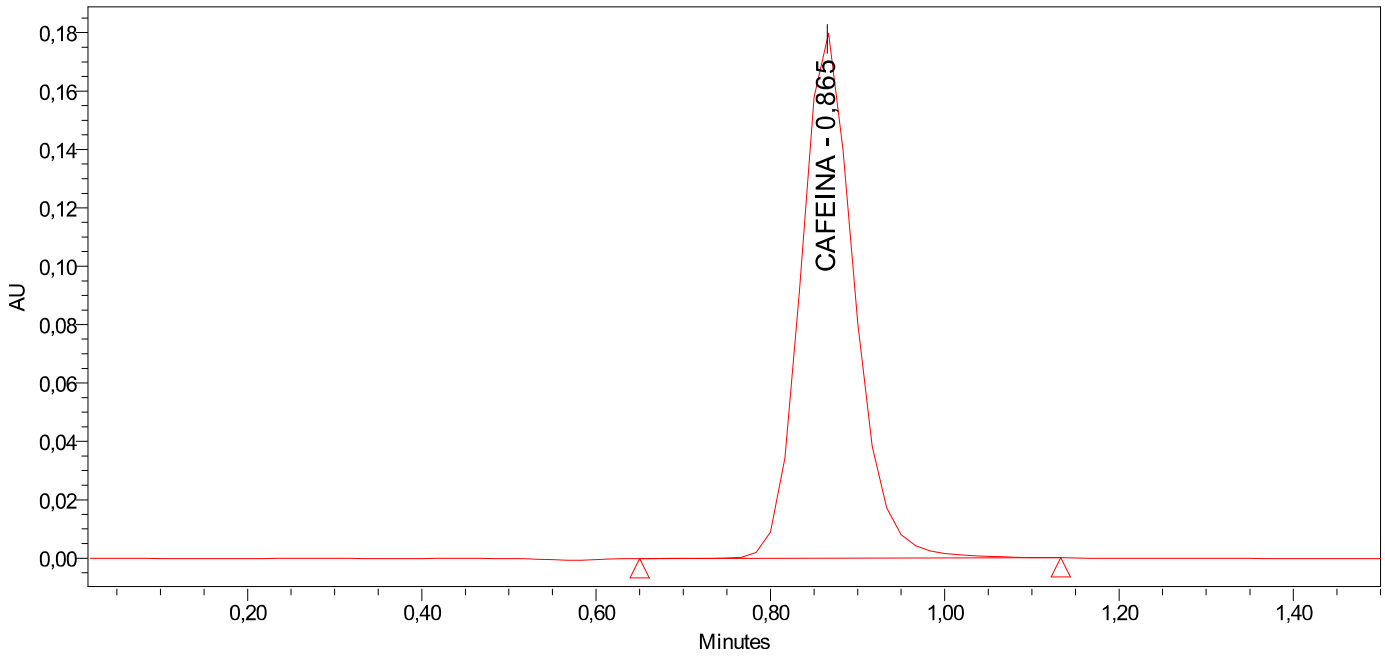


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,865	770928	175004		

SAMPLE INFORMATION

Sample Name:	269	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	269
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:04:43 AMT		
Date Processed:	22/07/2021 11:59:07 AMT		

Auto-Scaled Chromatogram

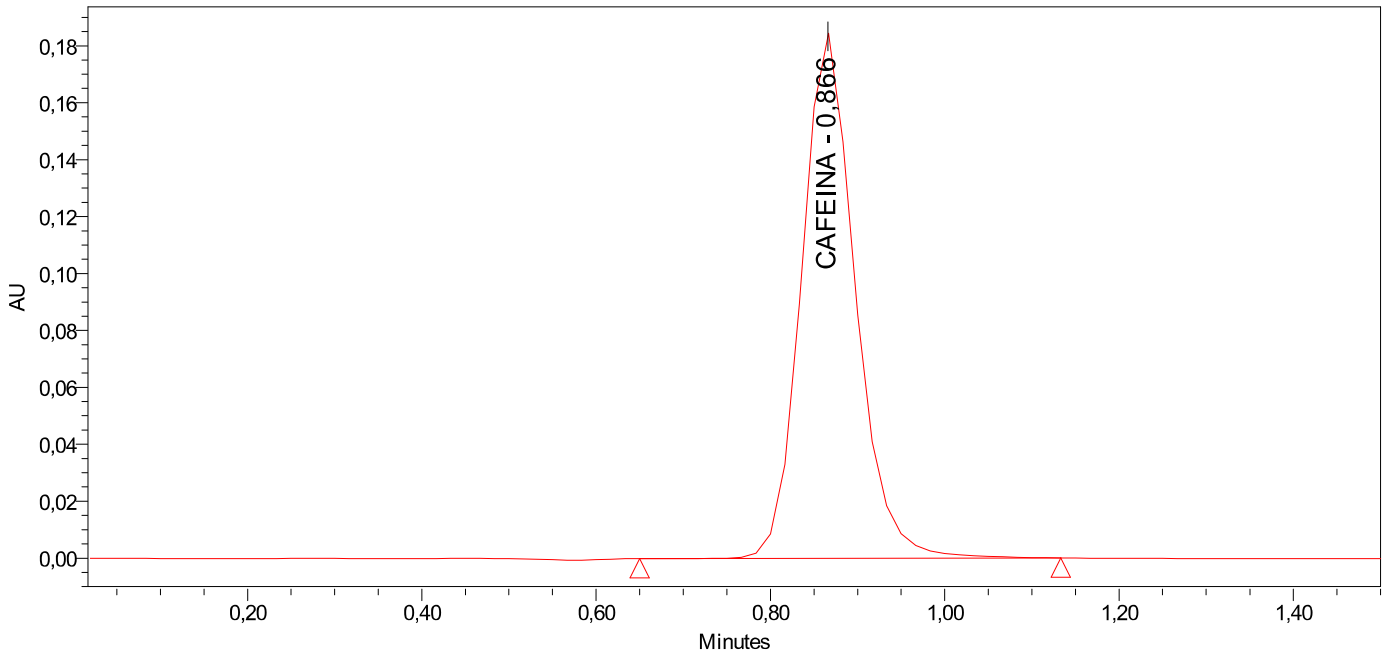


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,866	788003	179223		

SAMPLE INFORMATION

Sample Name:	270	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	270
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:07:08 AMT		
Date Processed:	22/07/2021 11:59:08 AMT		

Auto-Scaled Chromatogram

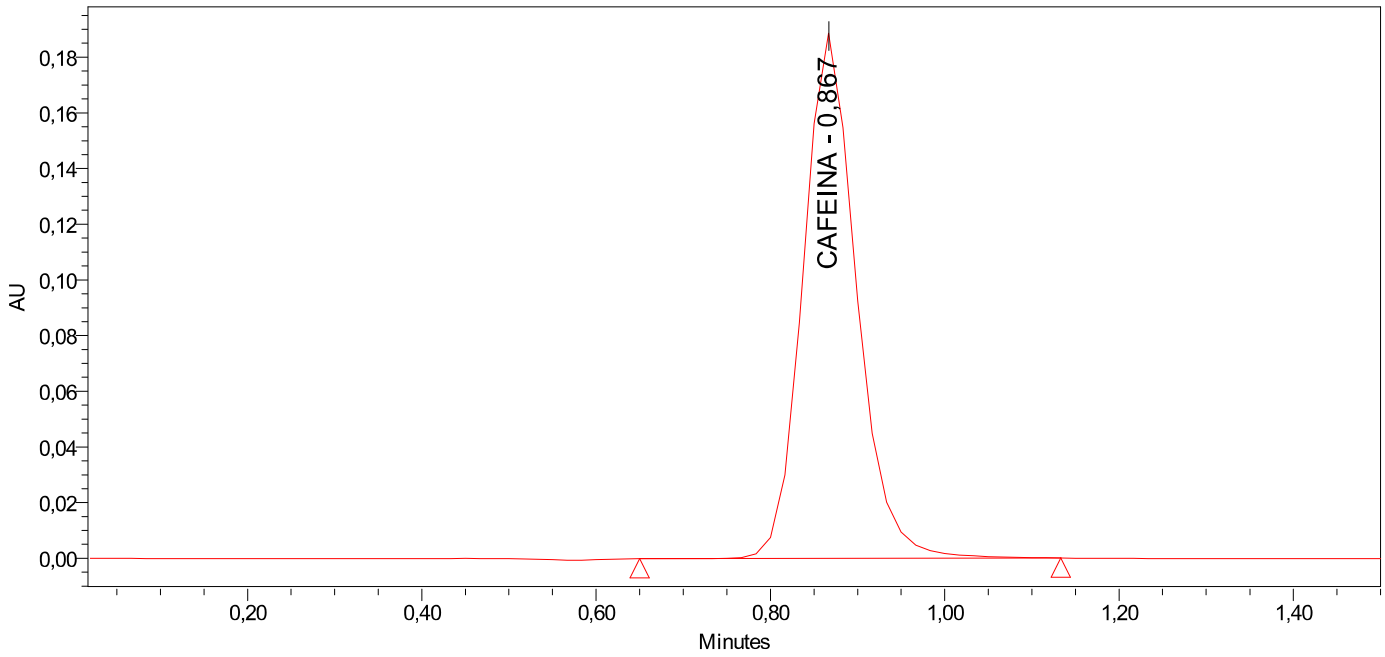


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,867	803258	183043		

SAMPLE INFORMATION

Sample Name:	271	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	271
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:09:32 AMT		
Date Processed:	22/07/2021 11:59:09 AMT		

Auto-Scaled Chromatogram

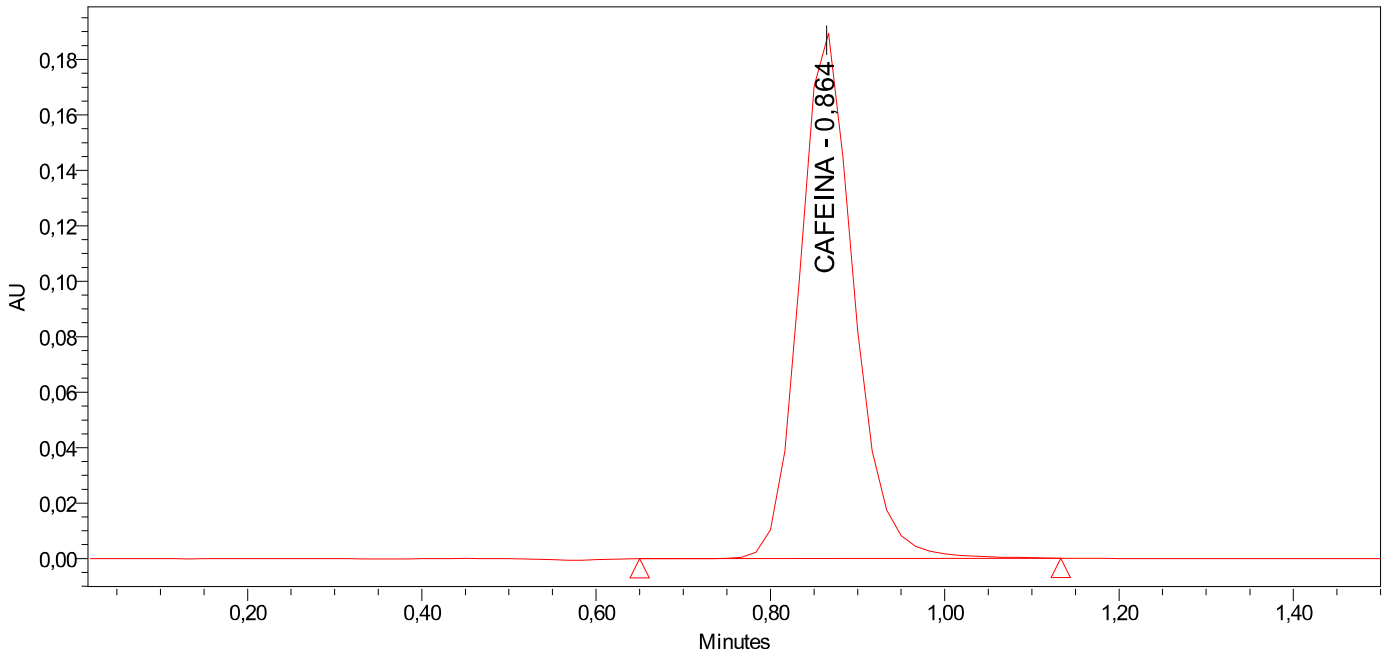


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,864	815210	184745		

SAMPLE INFORMATION

Sample Name:	272	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	272
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:11:55 AMT		
Date Processed:	22/07/2021 11:59:10 AMT		

Auto-Scaled Chromatogram

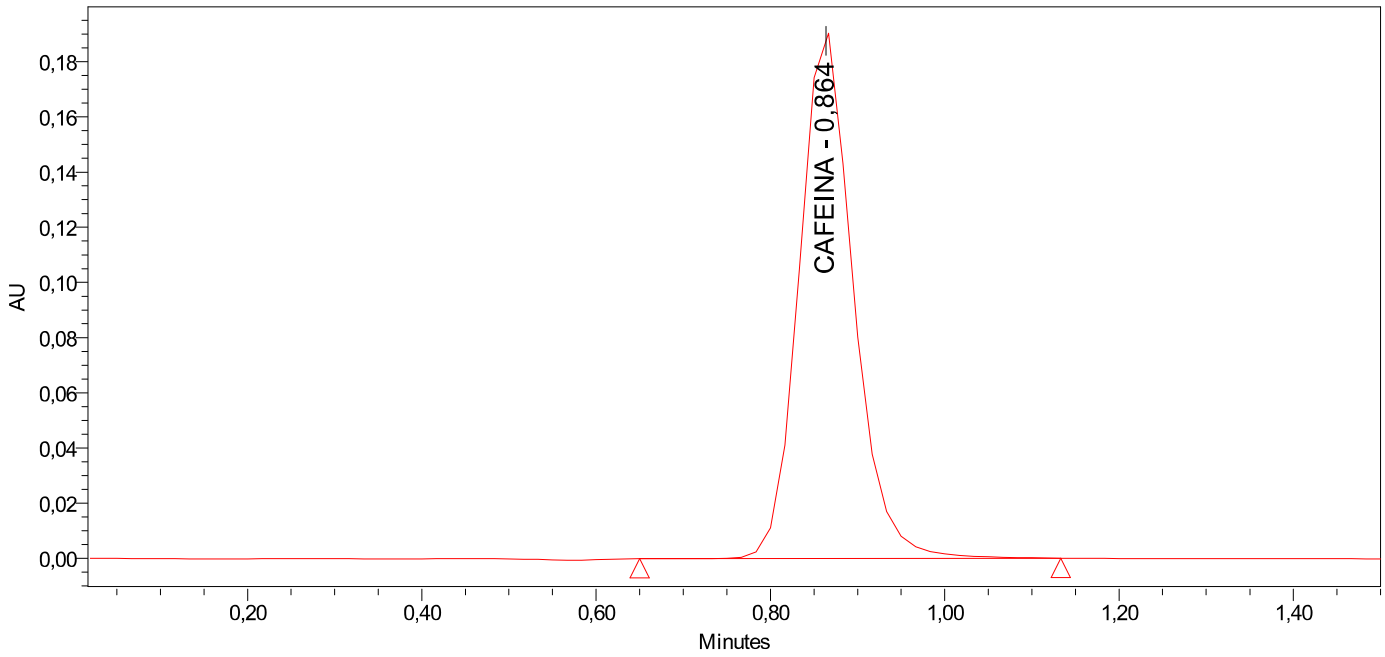


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,864	822768	186073		

SAMPLE INFORMATION

Sample Name:	273	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	273
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:14:18 AMT		
Date Processed:	22/07/2021 11:59:11 AMT		

Auto-Scaled Chromatogram

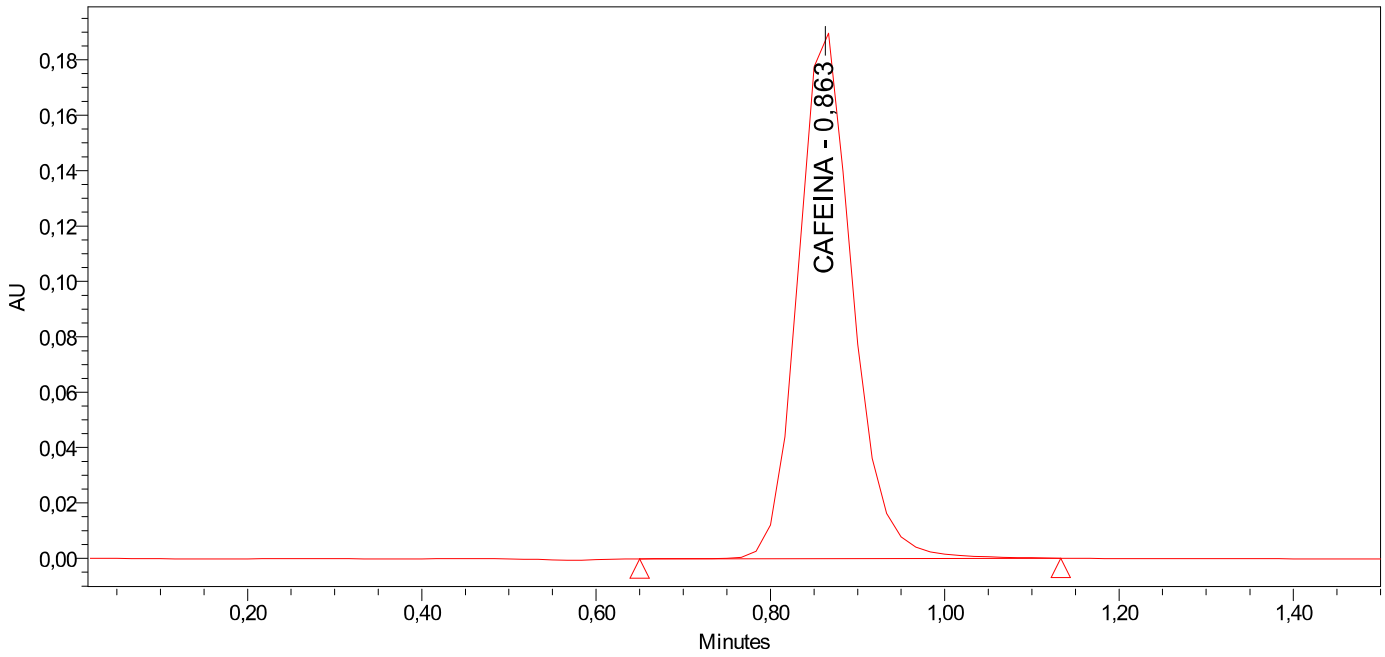


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,863	824861	186061		

SAMPLE INFORMATION

Sample Name:	274	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	274
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:16:41 AMT		
Date Processed:	22/07/2021 11:59:16 AMT		

Auto-Scaled Chromatogram

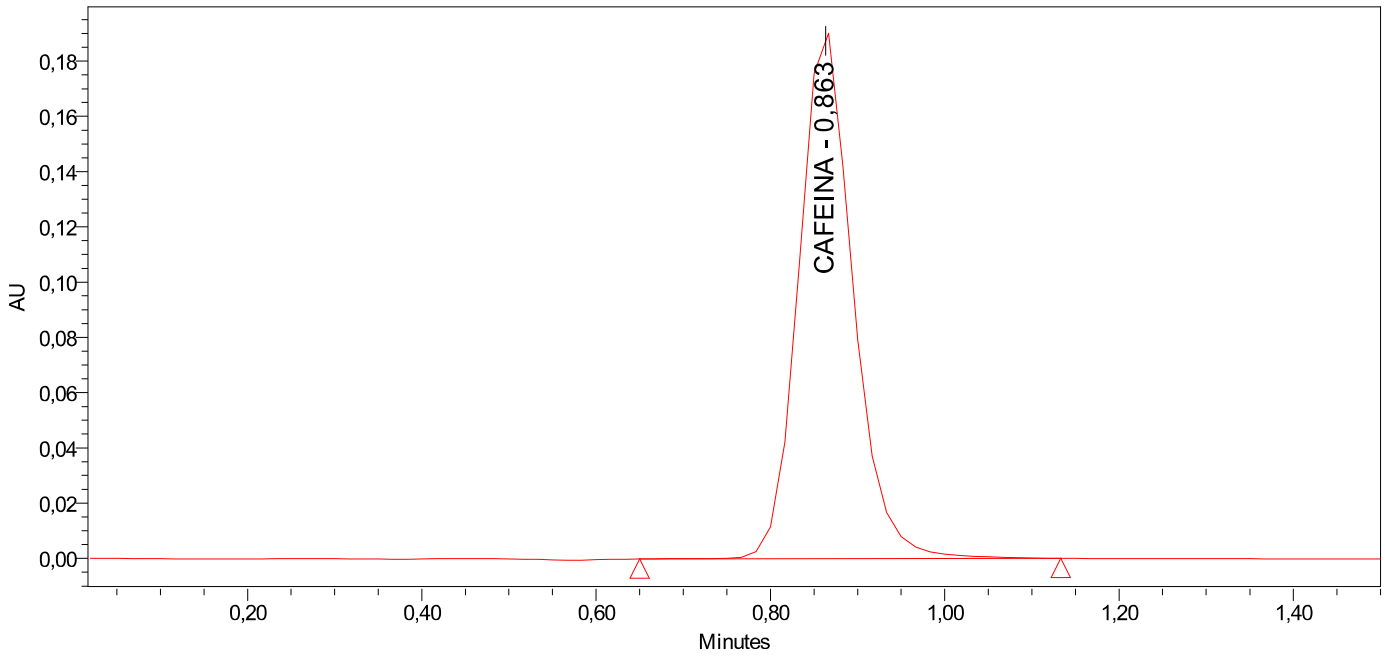


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,863	823621	186128		

SAMPLE INFORMATION

Sample Name:	275	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	275
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:19:04 AMT		
Date Processed:	22/07/2021 11:59:21 AMT		

Auto-Scaled Chromatogram

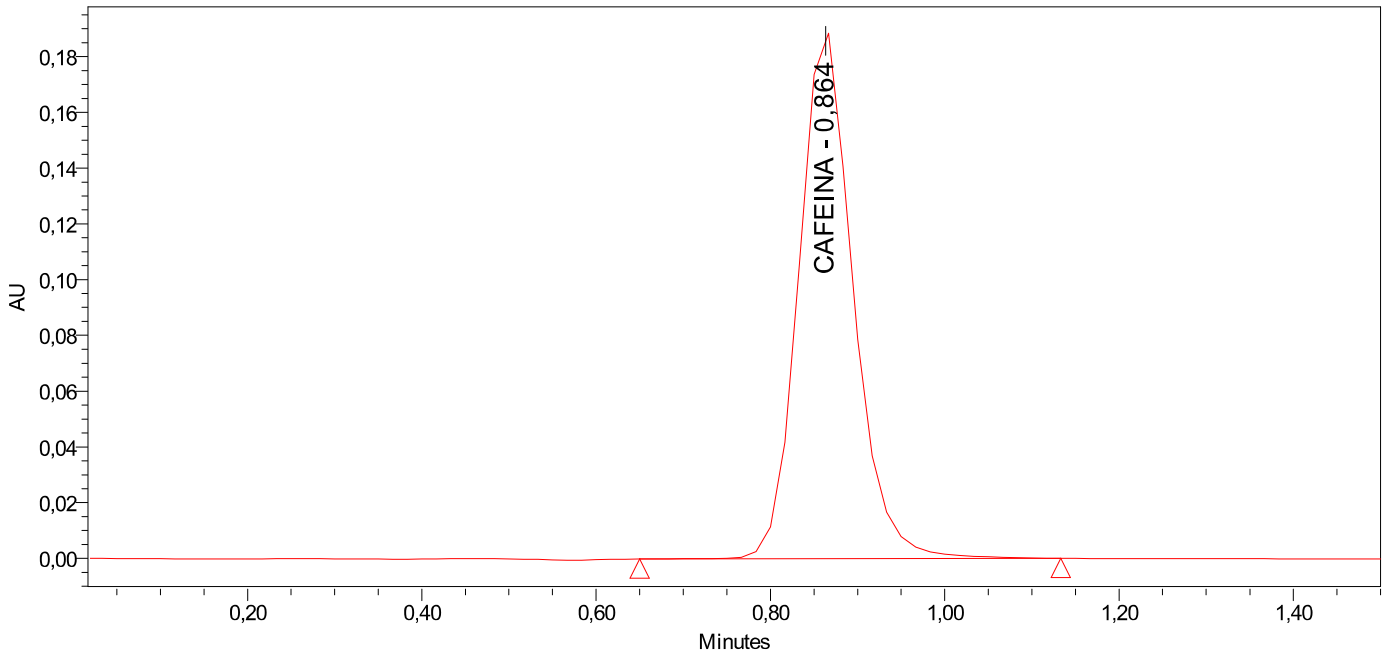


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,864	816319	184419		

SAMPLE INFORMATION

Sample Name:	276	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	276
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:21:27 AMT		
Date Processed:	22/07/2021 11:59:34 AMT		

Auto-Scaled Chromatogram

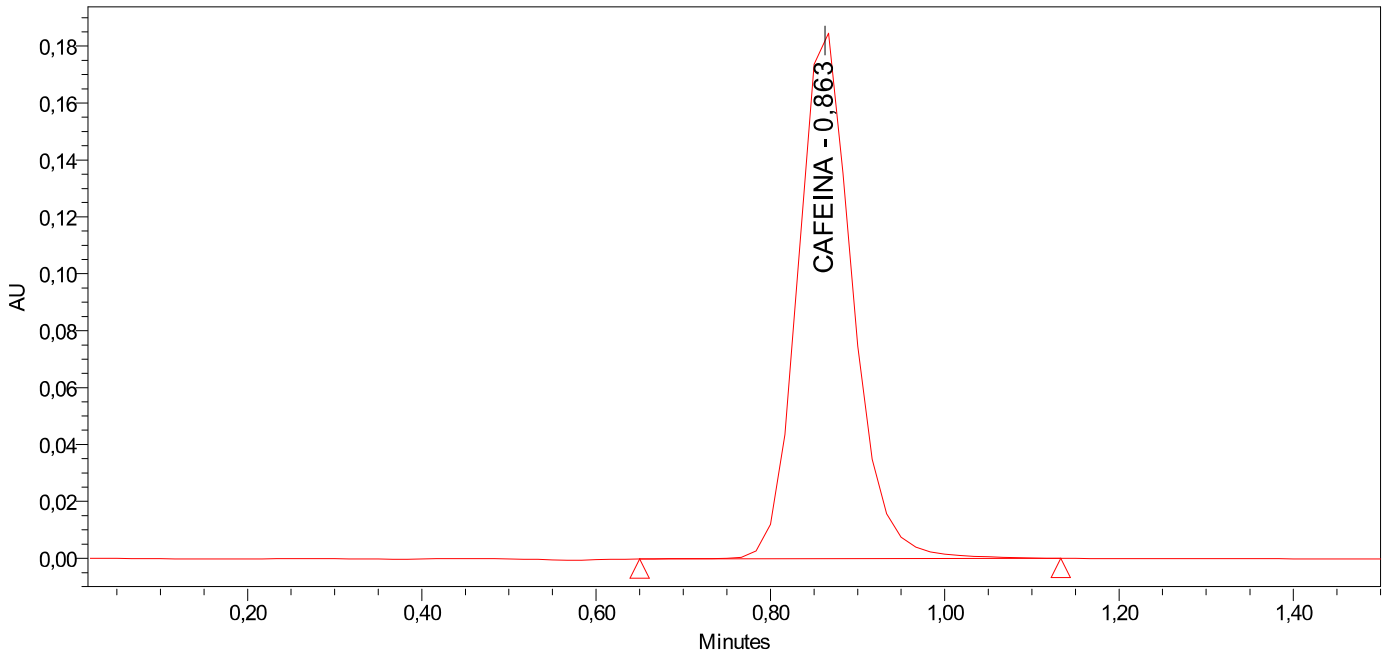


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,863	804720	181304		

SAMPLE INFORMATION

Sample Name:	277	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	277
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:23:50 AMT		
Date Processed:	22/07/2021 11:59:34 AMT		

Auto-Scaled Chromatogram

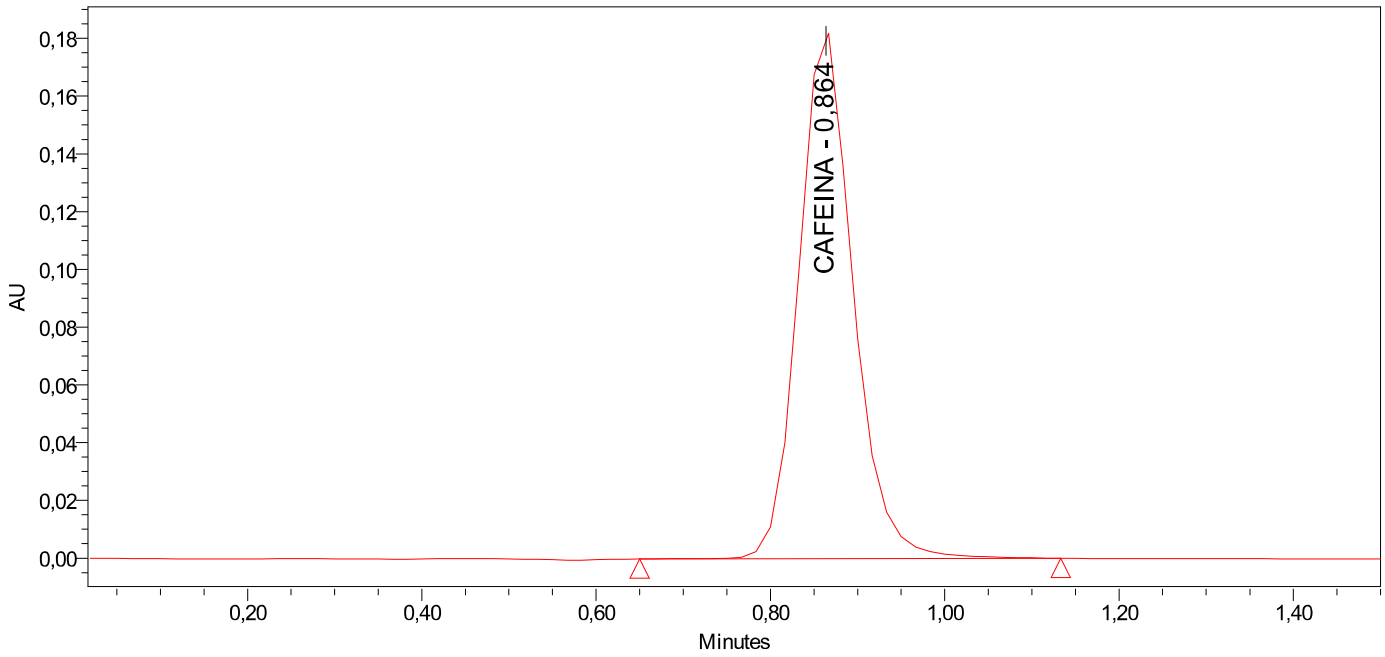


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,864	787248	177931		

SAMPLE INFORMATION

Sample Name:	278	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586
Vial:	24	Acq. Method Set:	278
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 09:26:13 AMT		
Date Processed:	22/07/2021 11:59:35 AMT		

Auto-Scaled Chromatogram

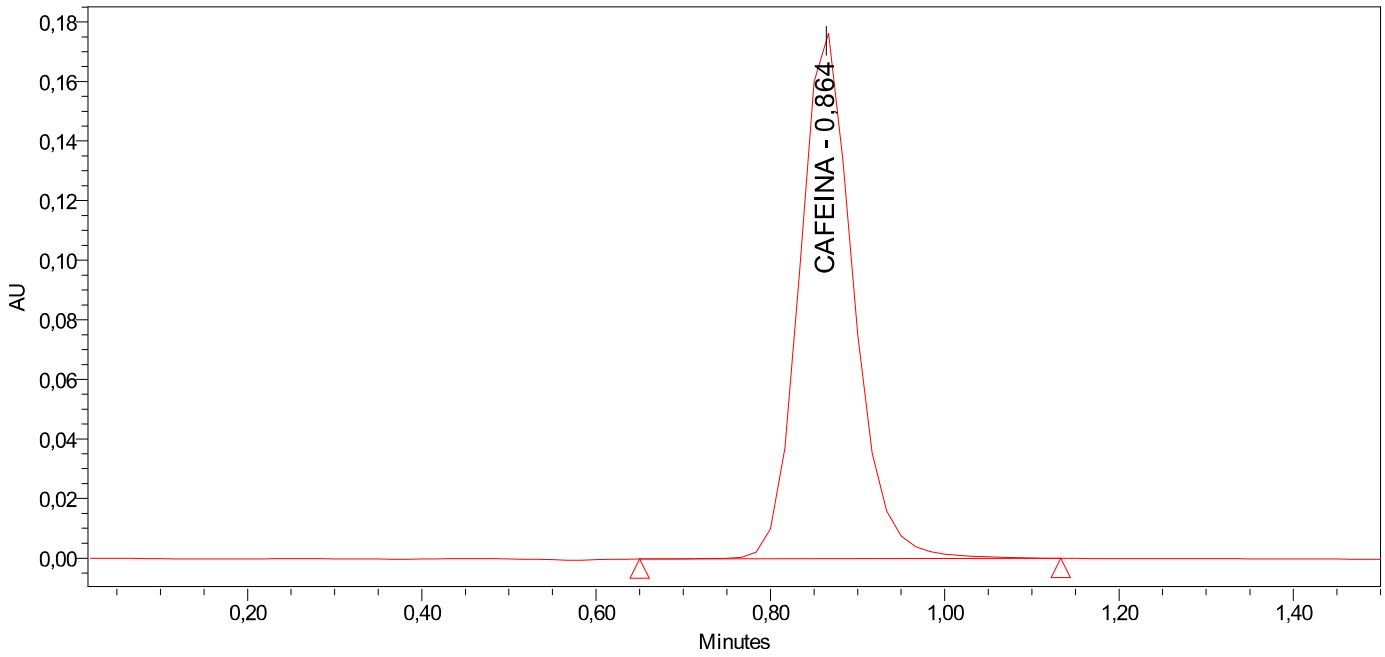


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,864	760394	172186		

SAMPLE INFORMATION

Sample Name:	BRANCO 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:11:36 AMT		
Date Processed:	21/07/2021 13:43:09 AMT		

Auto-Scaled Chromatogram

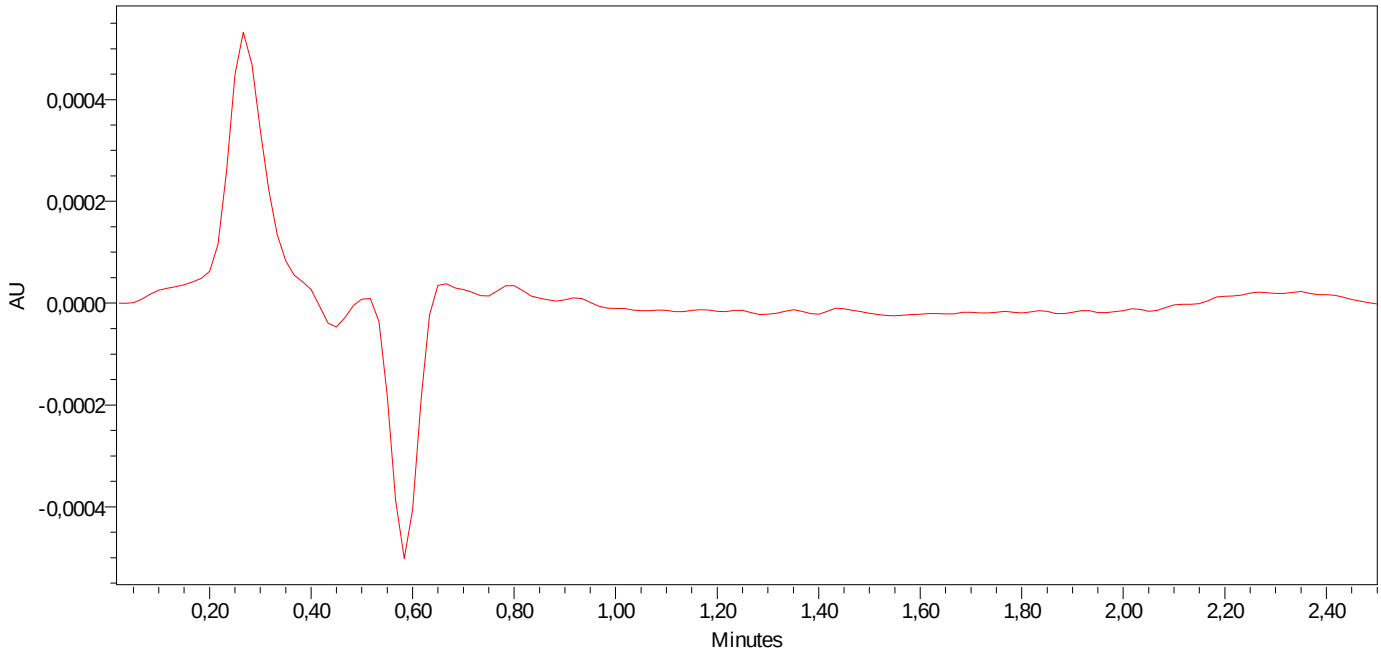


Peak Results

	Name	RT	Area	Height	Amount	Units
1						

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:28:24 AMT		
Date Processed:	21/07/2021 13:49:49 AMT		

Auto-Scaled Chromatogram

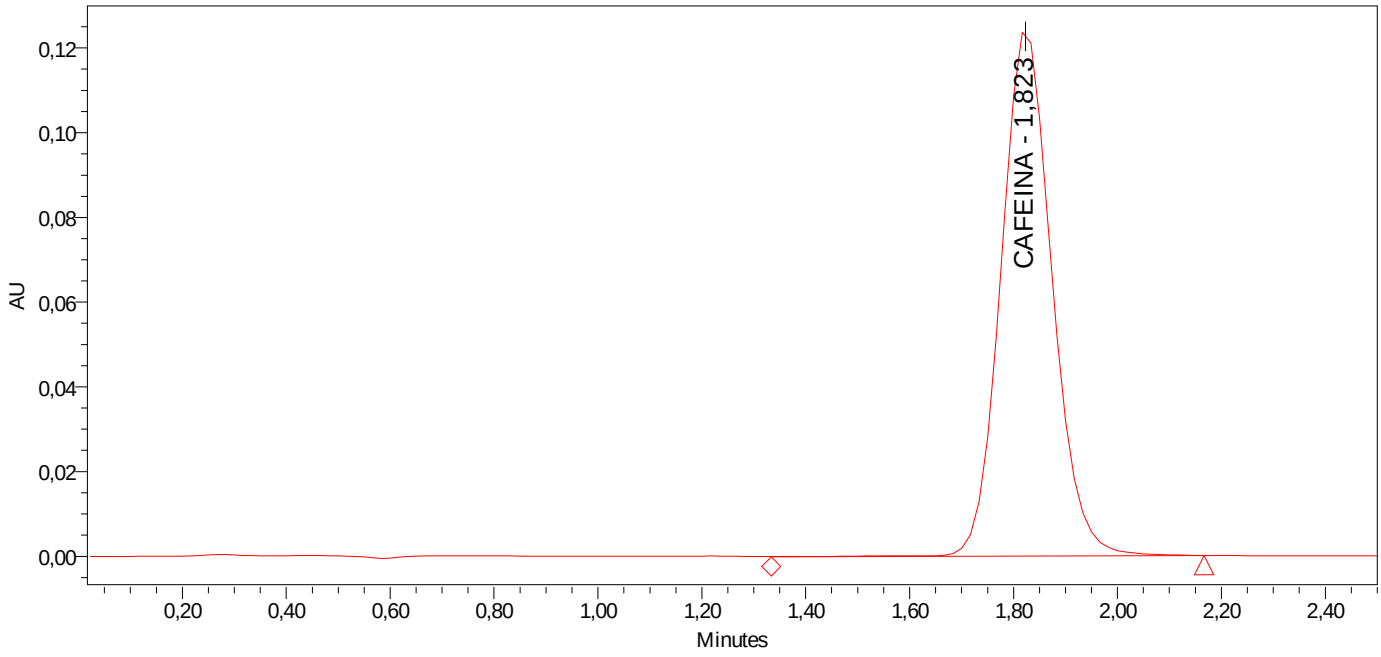


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,823	847436	124039		

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	2	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:18:17 AMT		
Date Processed:	21/07/2021 13:51:39 AMT		

Auto-Scaled Chromatogram

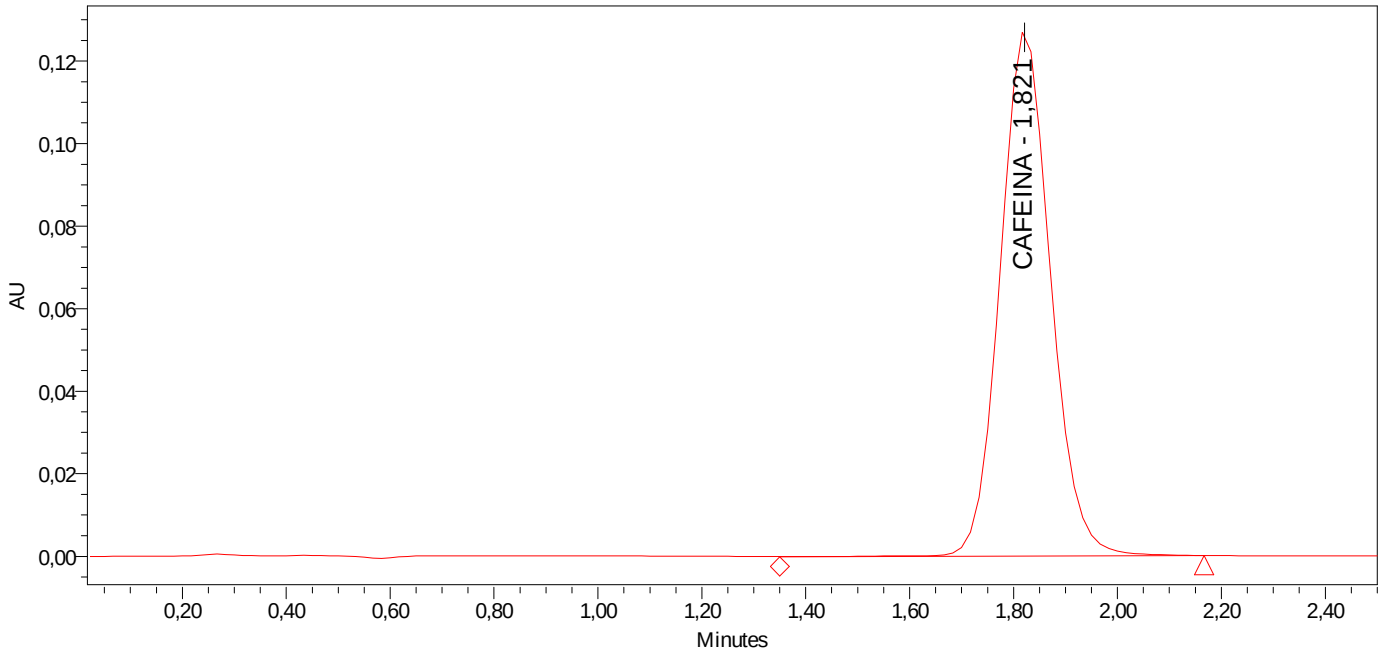


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,821	858006	126775		

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	3	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:21:32 AMT		
Date Processed:	21/07/2021 13:54:23 AMT		

Auto-Scaled Chromatogram

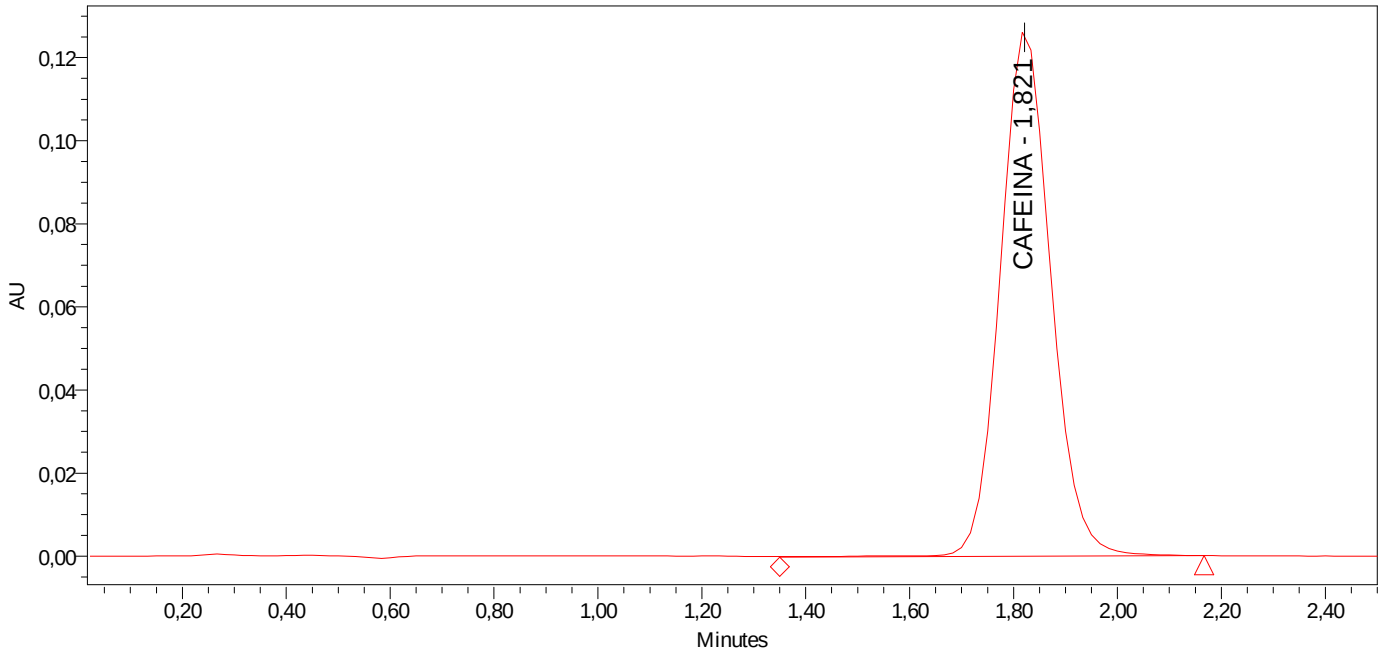


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,821	854832	126033		

SAMPLE INFORMATION

Sample Name:	BRANCO 2	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:24:59 AMT		
Date Processed:	21/07/2021 13:56:01 AMT		

Auto-Scaled Chromatogram

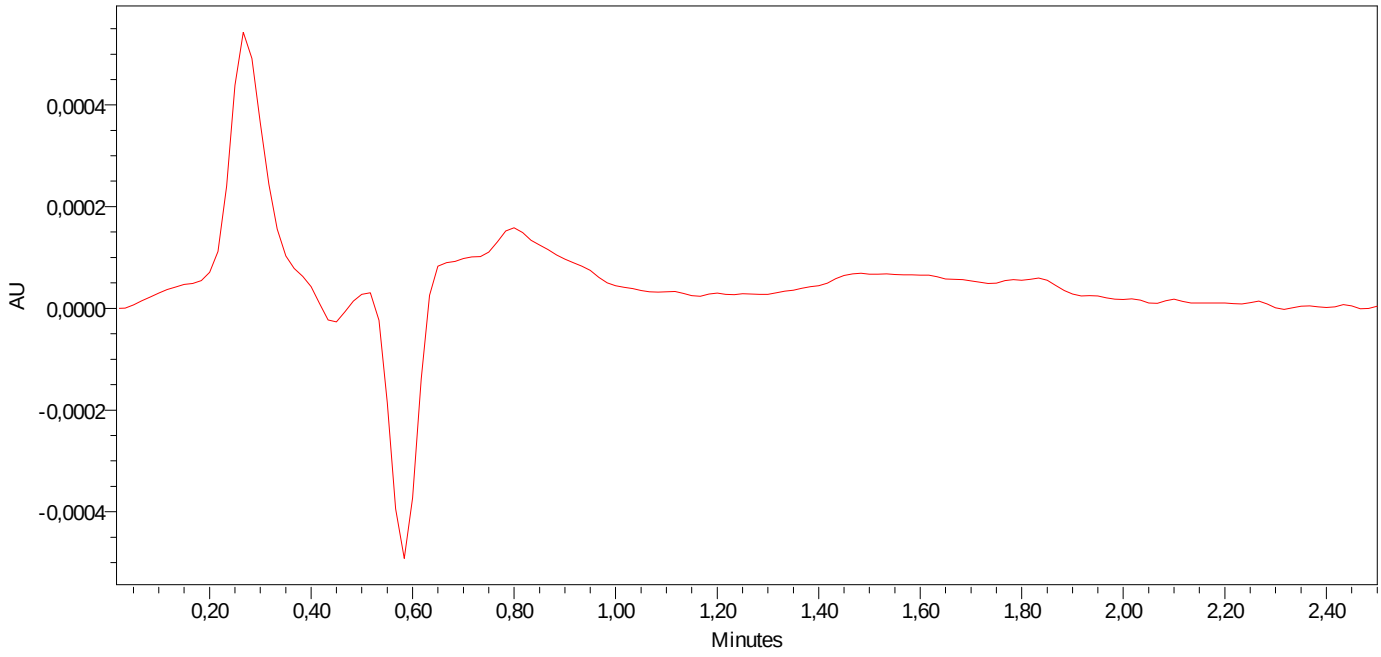


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:28:24 AMT		
Date Processed:	21/07/2021 13:56:51 AMT		

Auto-Scaled Chromatogram

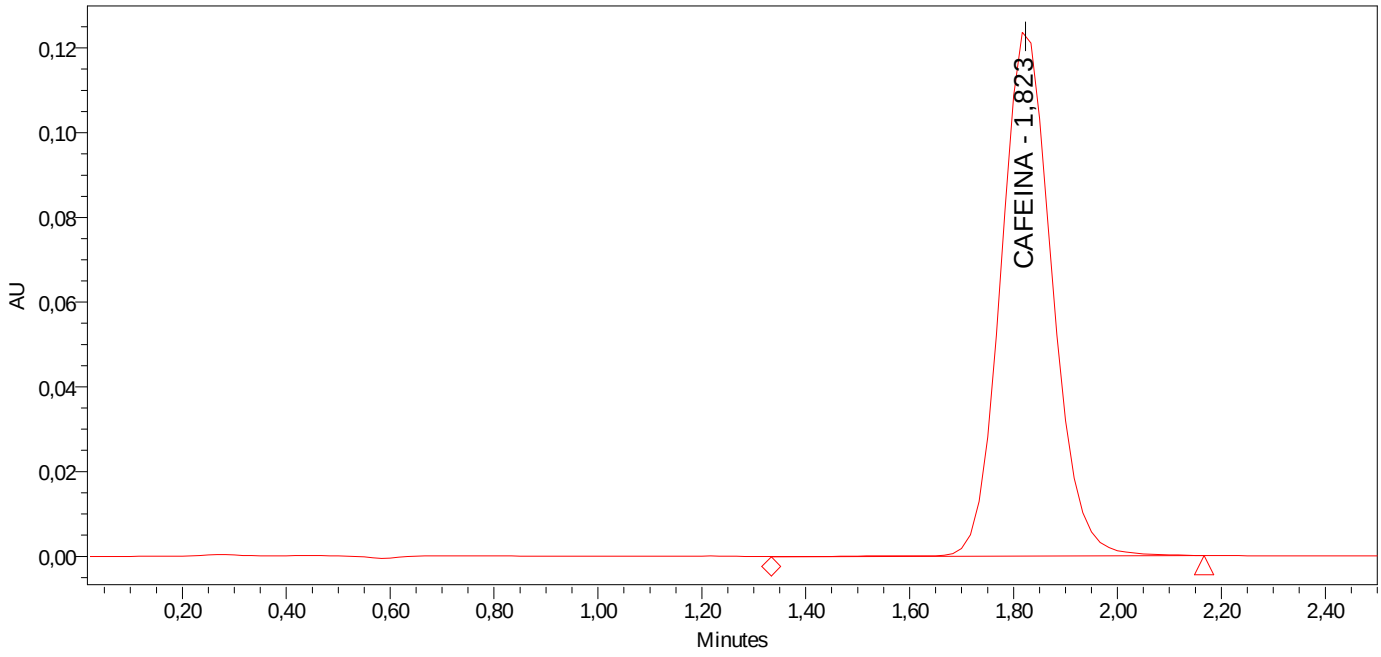


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,823	847436	124039		

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	2	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:31:41 AMT		
Date Processed:	21/07/2021 13:57:41 AMT		

Auto-Scaled Chromatogram

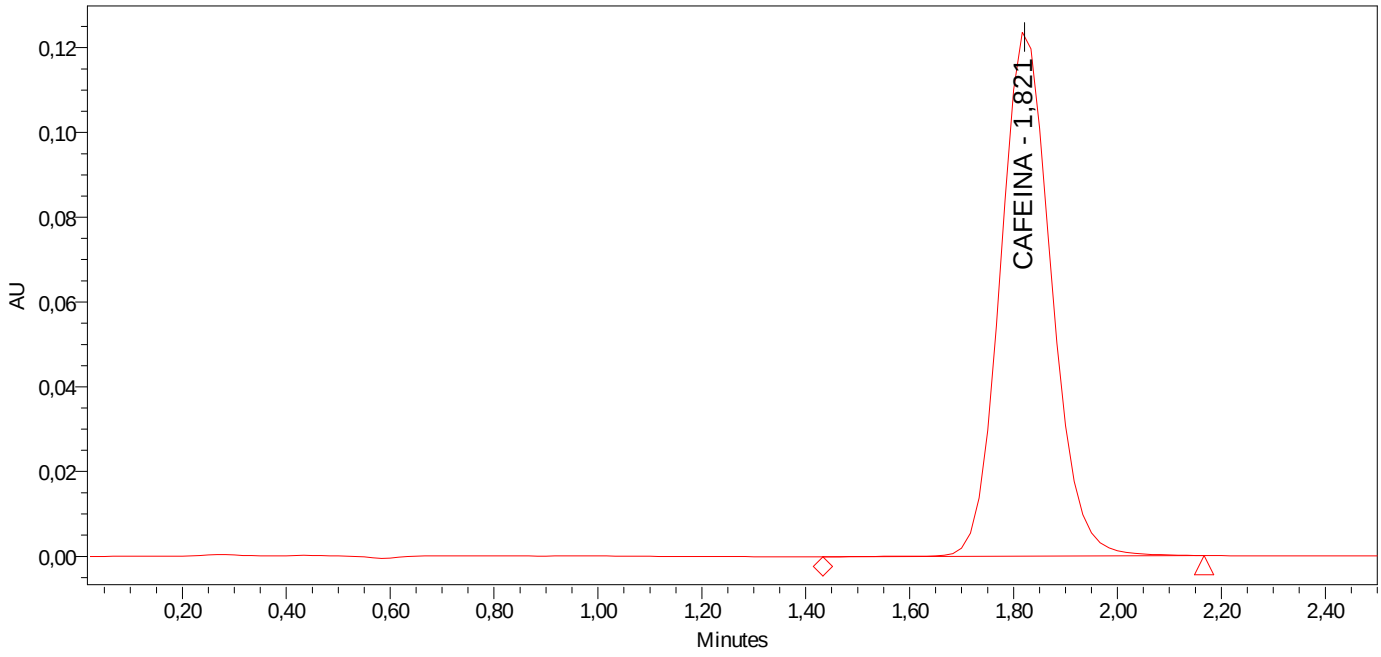


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,821	843261	123583		

SAMPLE INFORMATION

Sample Name:	PCIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	3	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:34:58 AMT		
Date Processed:	21/07/2021 13:58:49 AMT		

Auto-Scaled Chromatogram

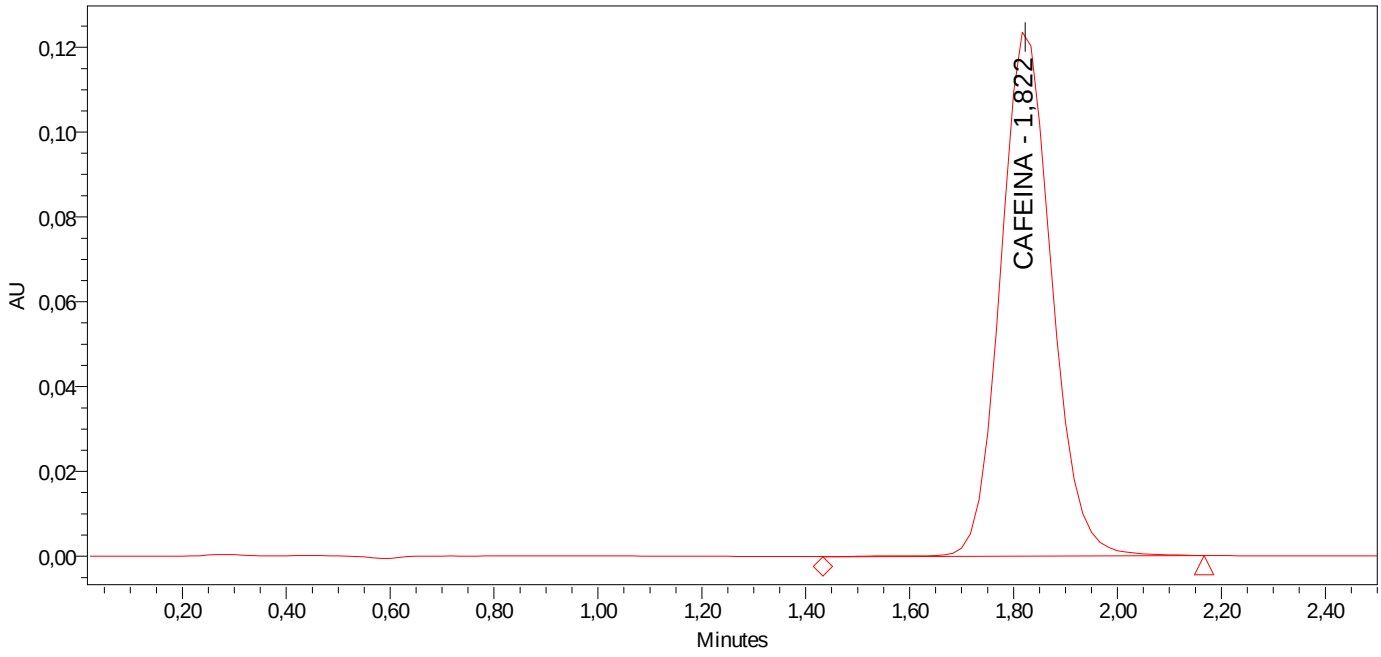


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,822	845154	123663		

SAMPLE INFORMATION

Sample Name:	BRANCO 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:40:47 AMT		
Date Processed:	21/07/2021 13:59:34 AMT		

Auto-Scaled Chromatogram

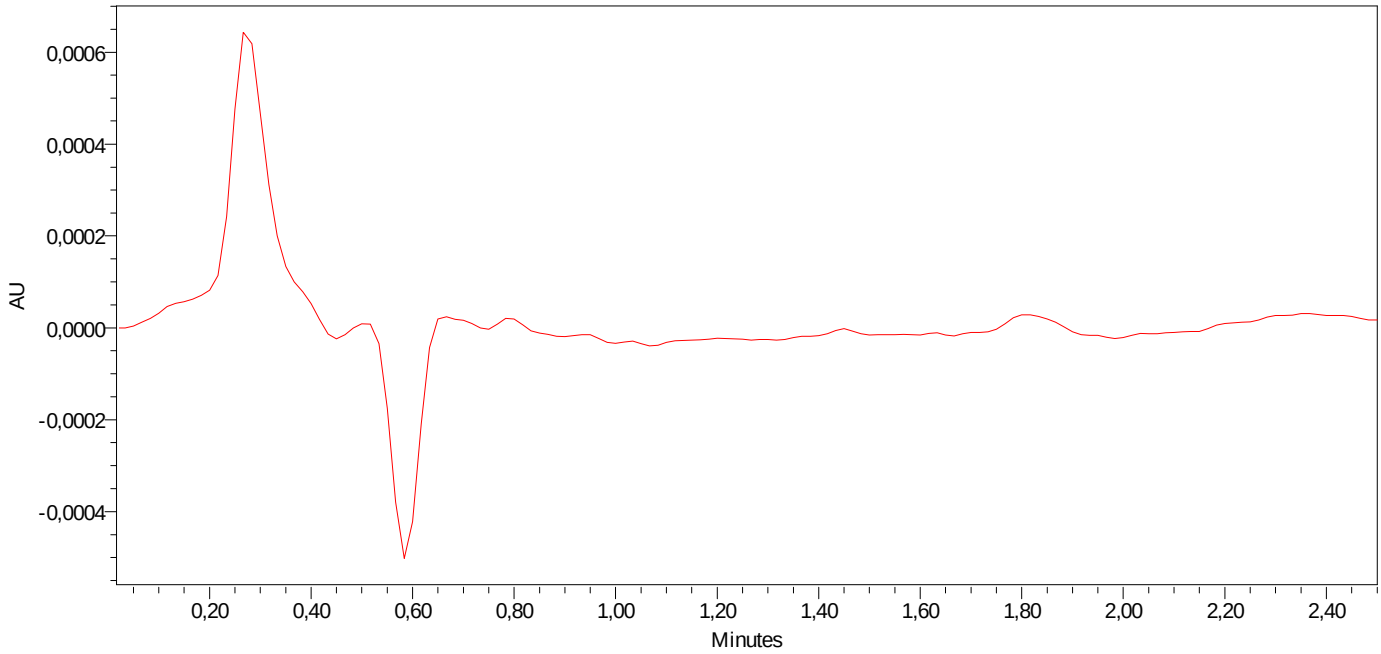


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	LDUV 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	4	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 14:01:09 AMT		
Date Processed:	21/07/2021 14:18:34 AMT		

Auto-Scaled Chromatogram

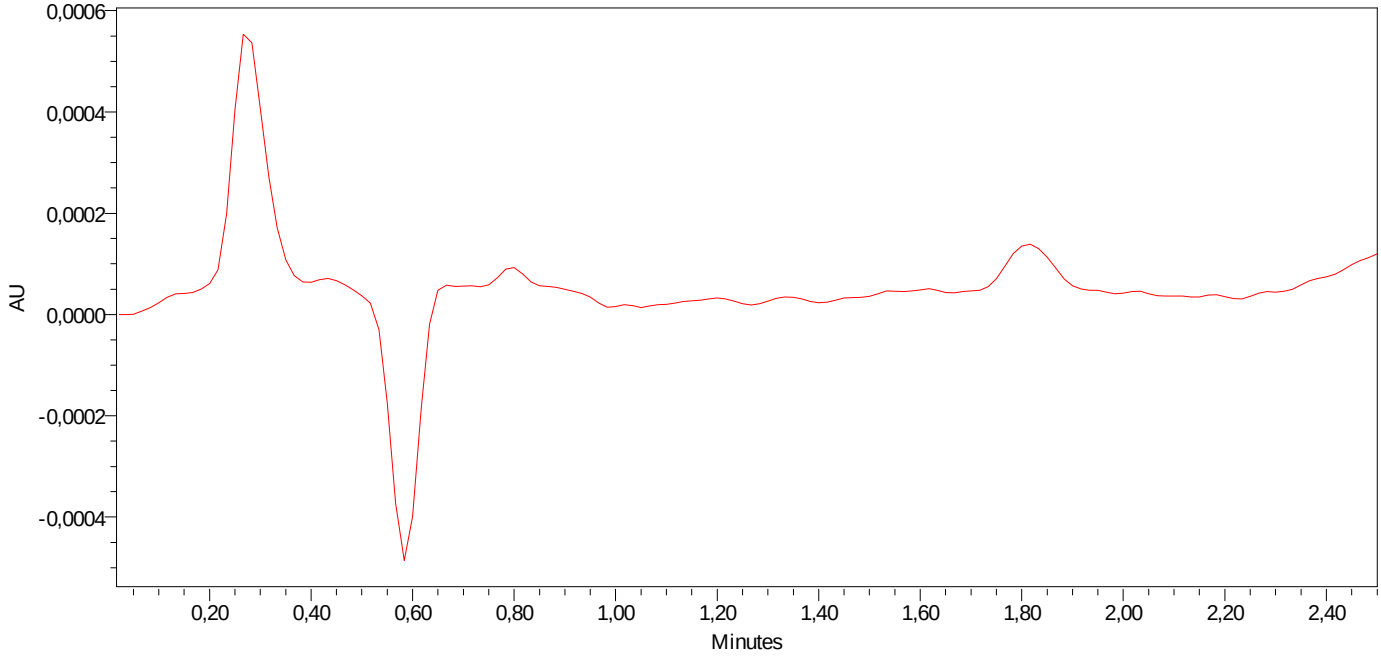


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	LDUV 2	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	5	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 14:04:34 AMT		
Date Processed:	21/07/2021 14:18:37 AMT		

Auto-Scaled Chromatogram

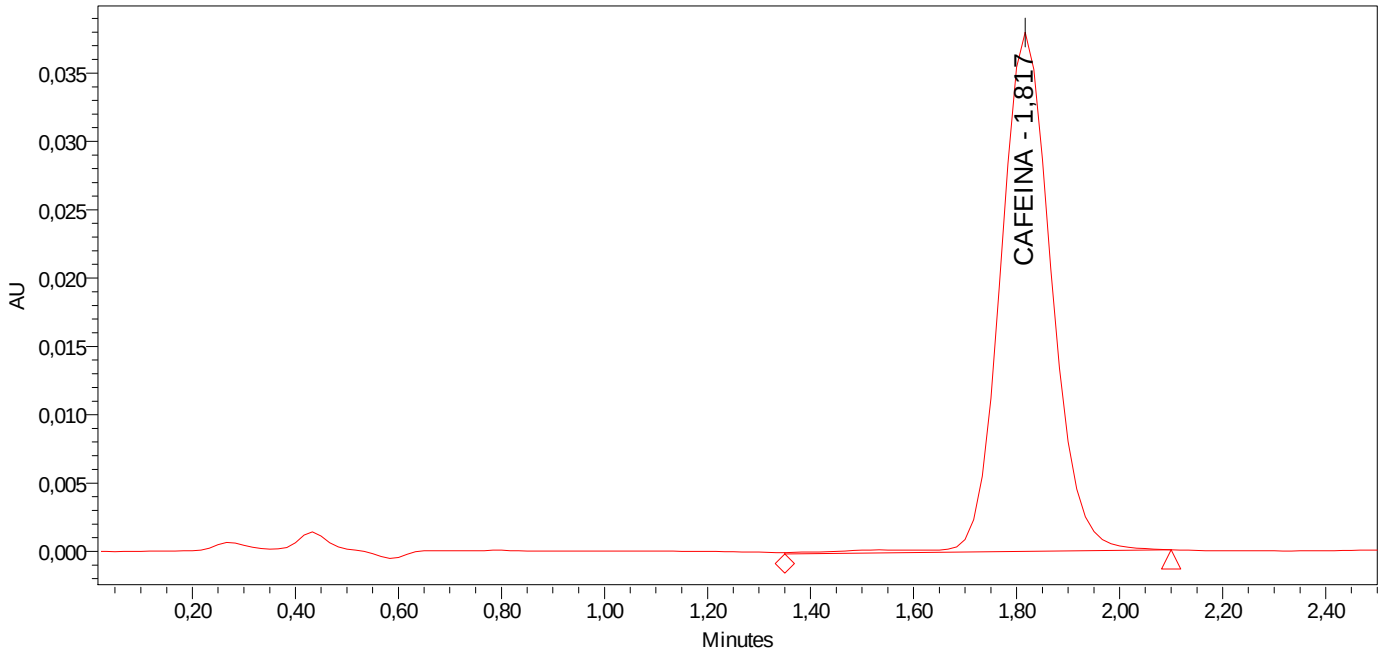


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,817	291418	37796		

SAMPLE INFORMATION

Sample Name:	LDUV 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	6	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 14:07:59 AMT		
Date Processed:	21/07/2021 14:18:41 AMT		

Auto-Scaled Chromatogram

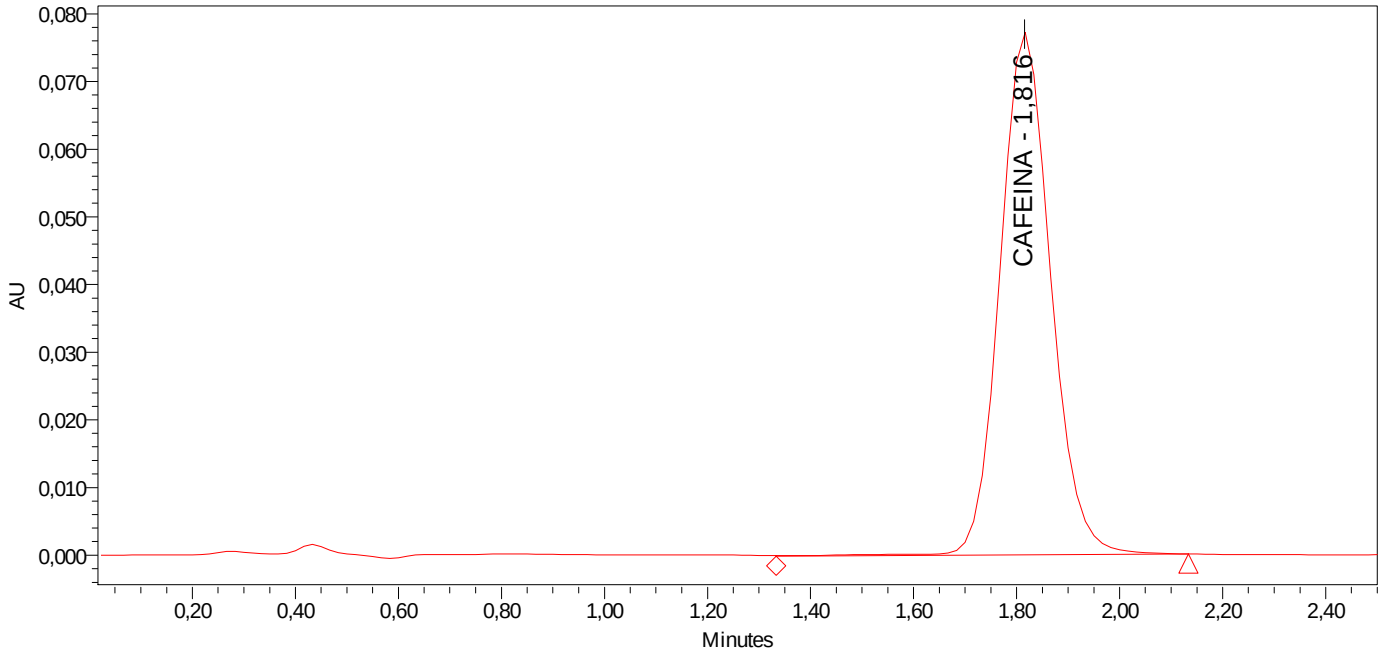


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,816	568505	76871		

SAMPLE INFORMATION

Sample Name:	LDUV 4	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	7	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 14:11:24 AMT		
Date Processed:	21/07/2021 14:18:44 AMT		

Auto-Scaled Chromatogram

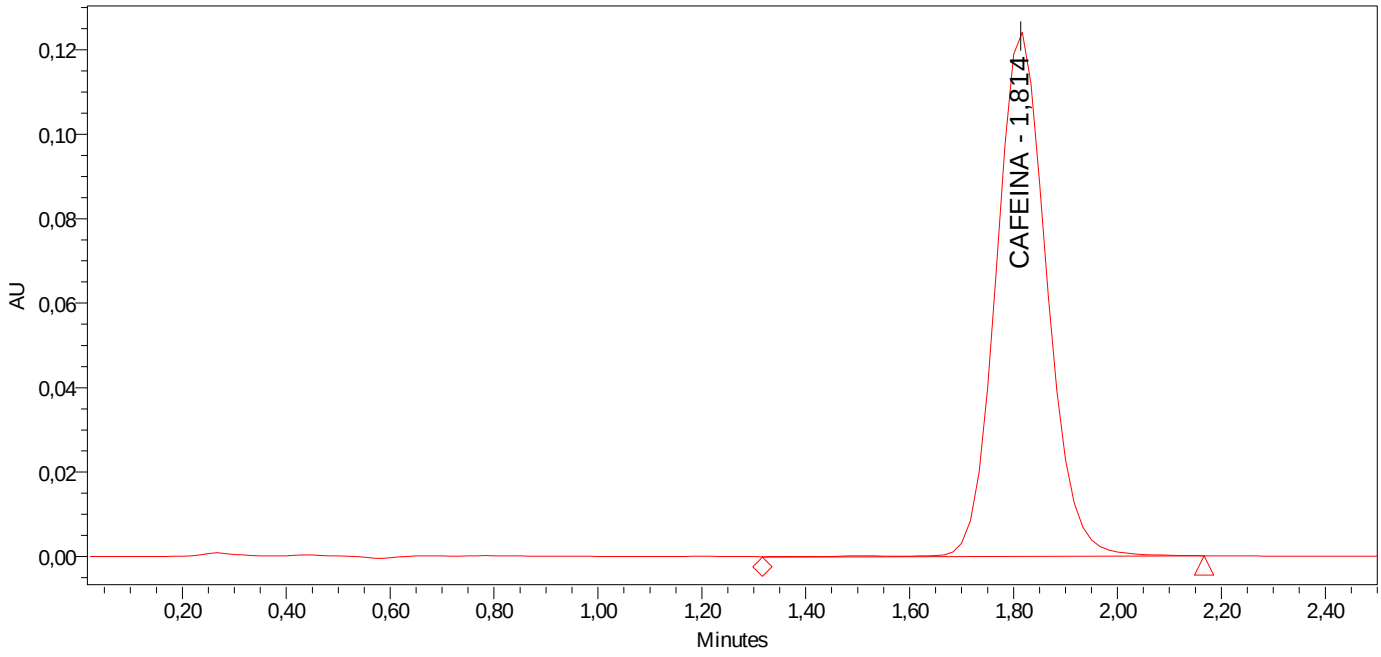


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,814	849517	123707		

SAMPLE INFORMATION

Sample Name:	LDUV 5	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	8	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 14:14:49 AMT		
Date Processed:	21/07/2021 14:18:47 AMT		

Auto-Scaled Chromatogram

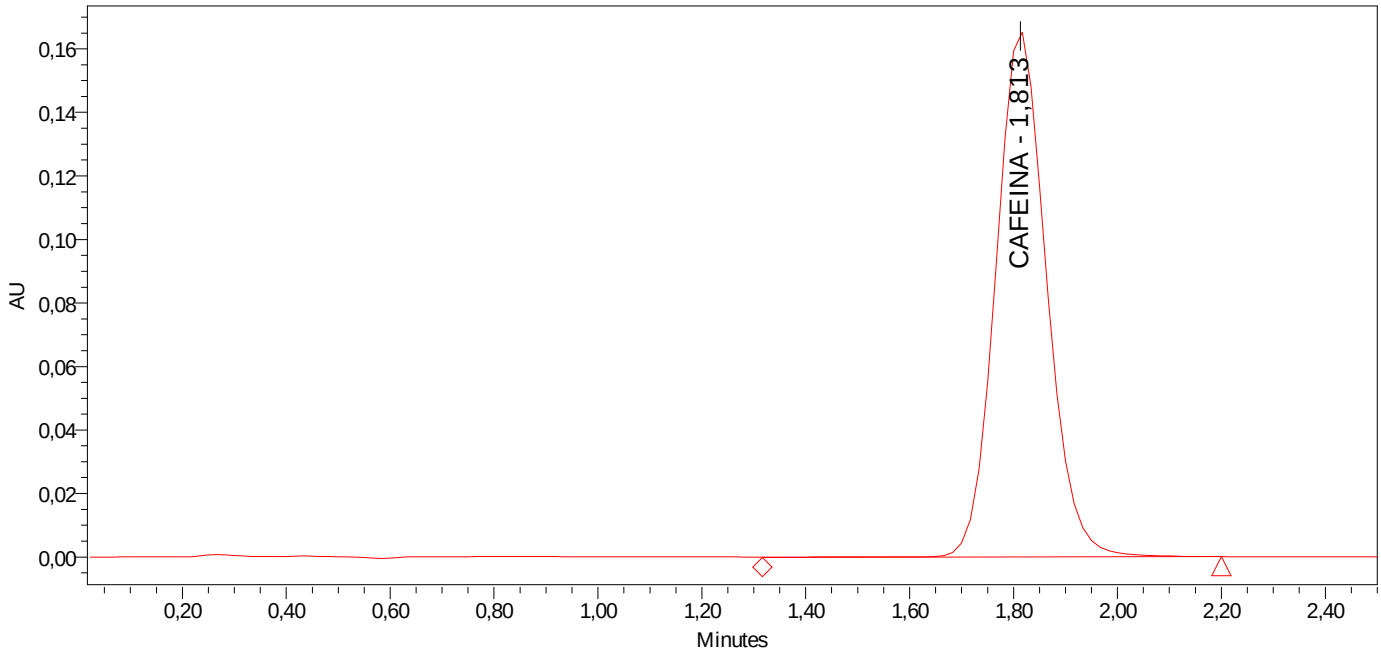

Peak Results


	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,813	1123255	164868		

SAMPLE INFORMATION

Sample Name:	LIIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1

Date Acquired:	21/07/2021 13:44:06 AMT
Date Processed:	21/07/2021 14:03:28 AMT

Auto-Scaled Chromatogram

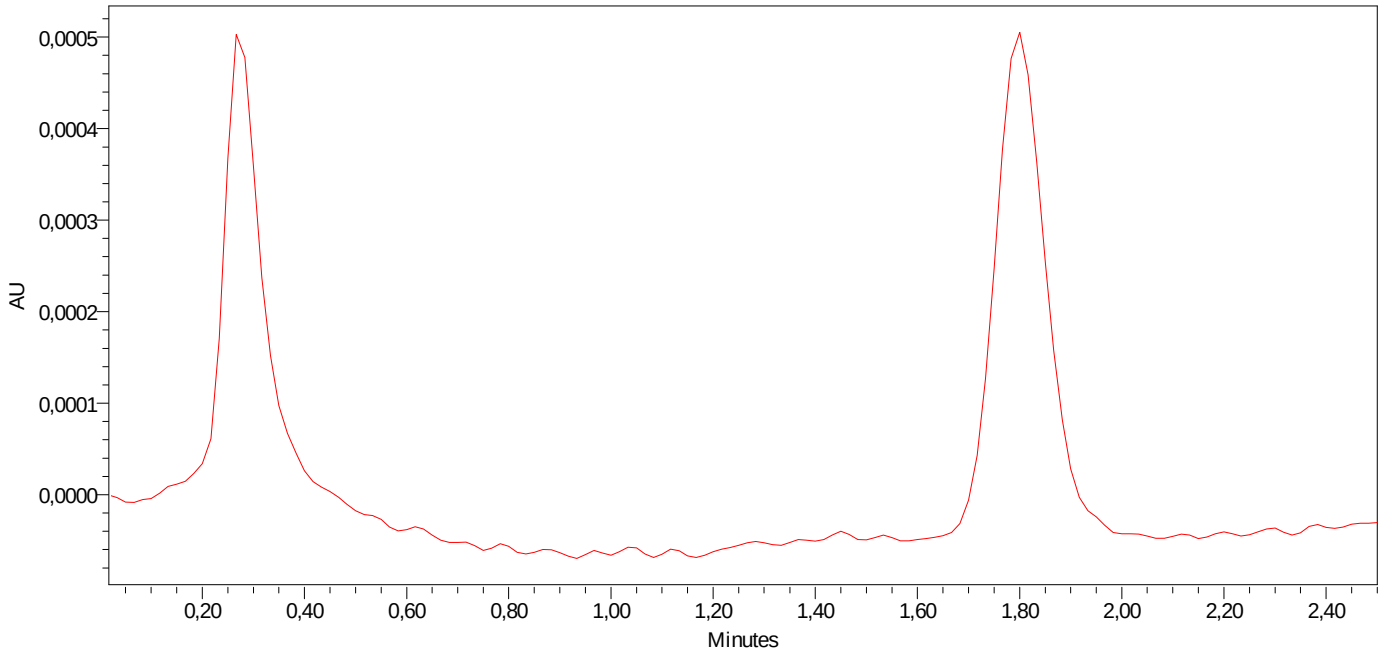


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	LIIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	5,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:47:27 AMT		
Date Processed:	21/07/2021 14:05:03 AMT		

Auto-Scaled Chromatogram

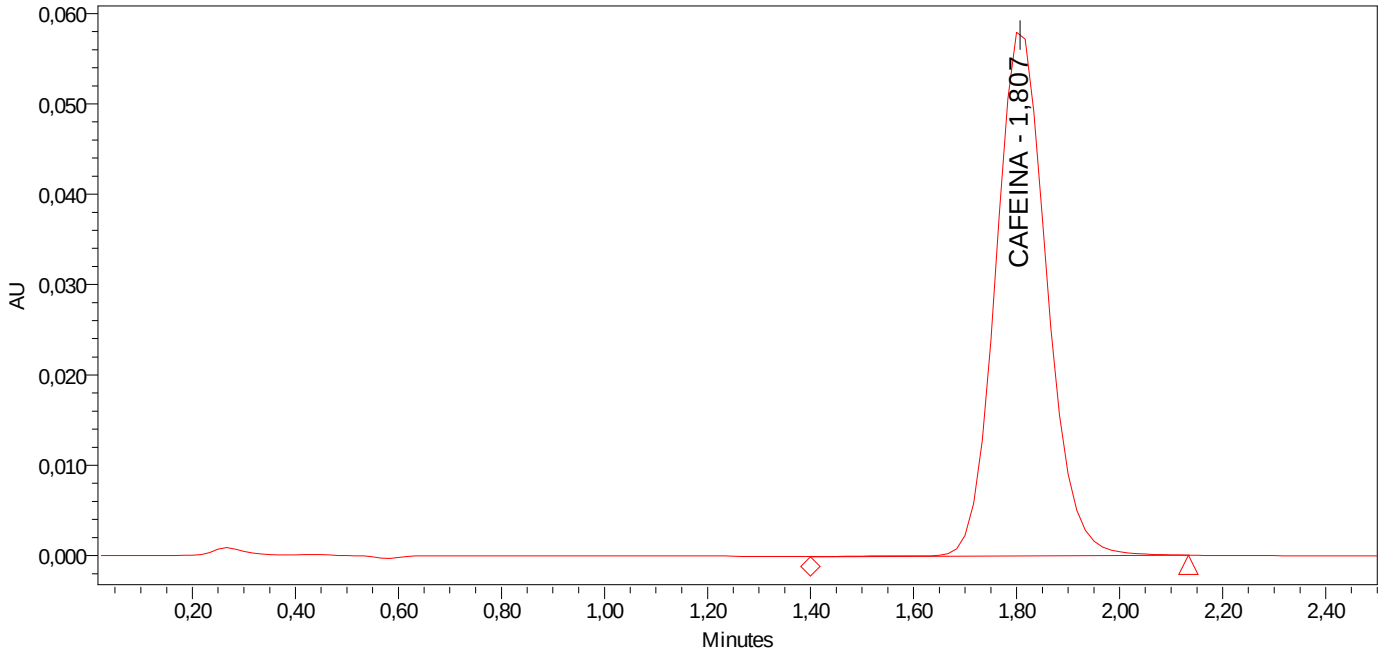


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,807	398658	58260		

SAMPLE INFORMATION

Sample Name:	LIIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:50:50 AMT		
Date Processed:	21/07/2021 14:05:07 AMT		

Auto-Scaled Chromatogram

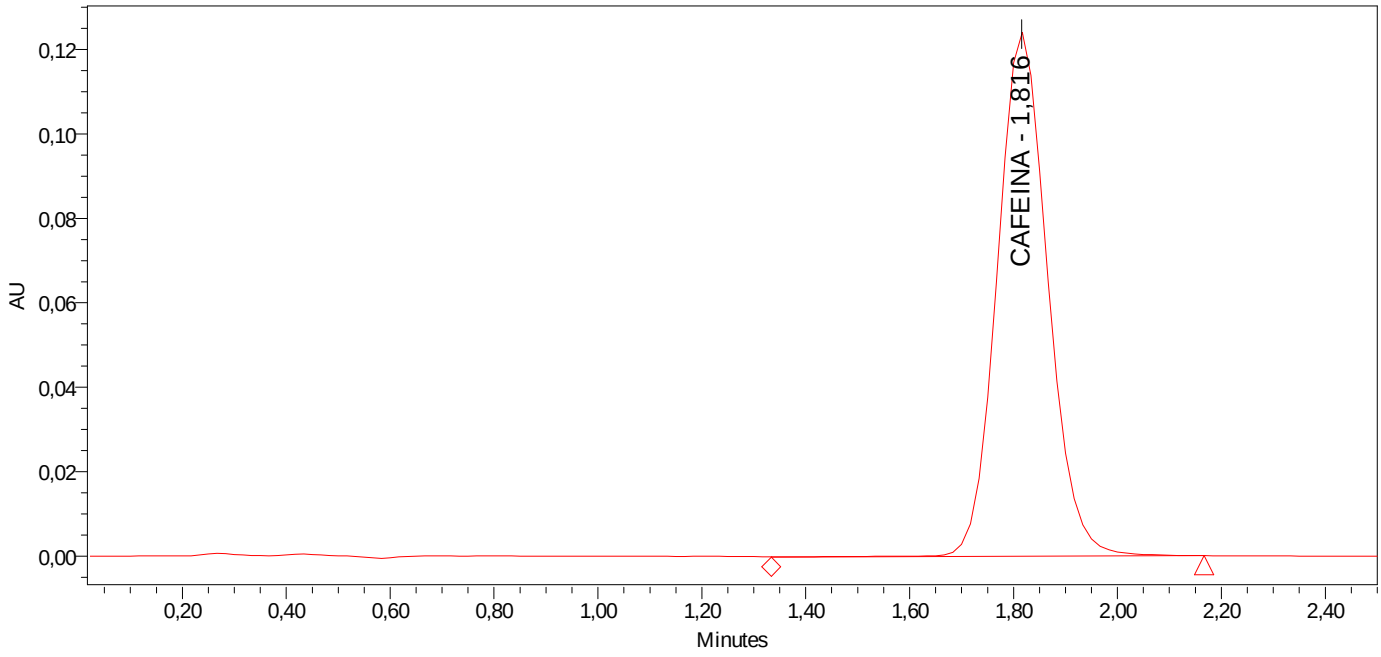


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,816	838671	123537		

SAMPLE INFORMATION

Sample Name:	LIIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	15,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:54:15 AMT		
Date Processed:	21/07/2021 14:05:08 AMT		

Auto-Scaled Chromatogram

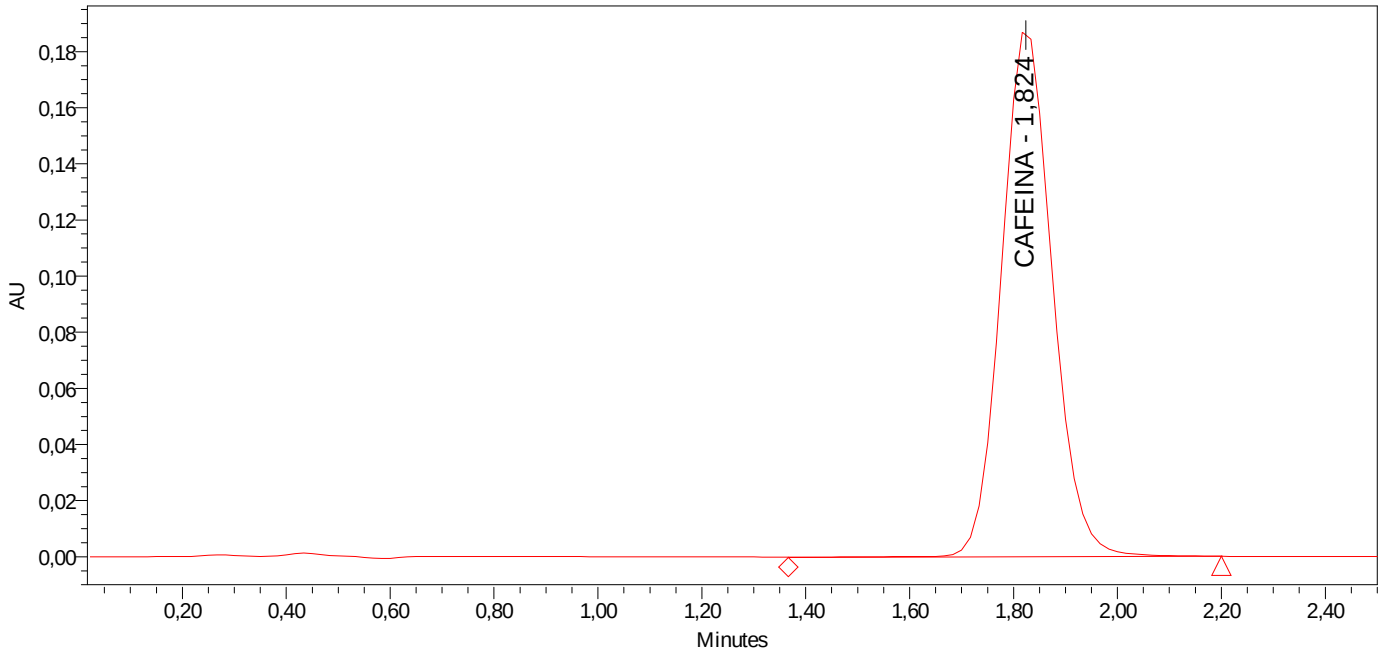


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,824	1274491	187897		

SAMPLE INFORMATION

Sample Name:	LIIN	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	20,00 ul	Channel Name:	2487Channel 1
Run Time:	2,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	21/07/2021 13:57:44 AMT		
Date Processed:	21/07/2021 14:05:20 AMT		

Auto-Scaled Chromatogram

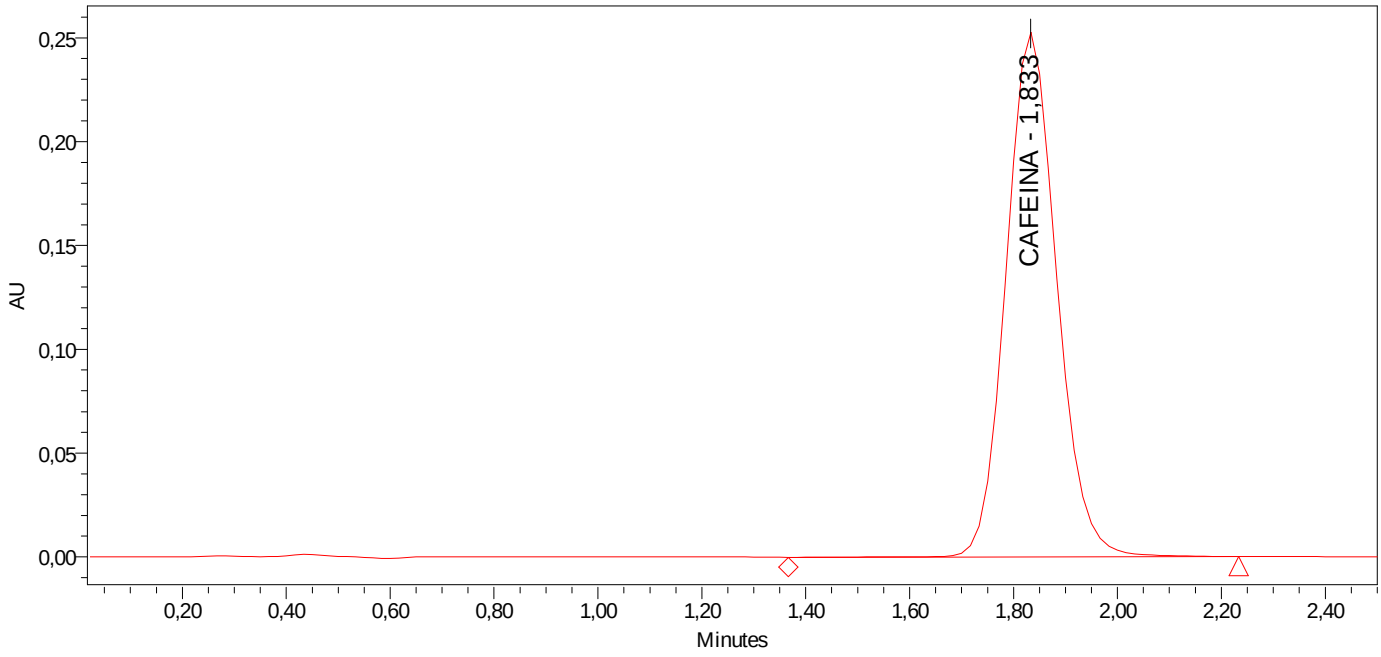


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,833	1709932	251403		

SAMPLE INFORMATION

Sample Name:	GRADIENTE AB	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586_1
Vial:	1	Acq. Method Set:	GRADIENTE AB_
Injection #:	2	Processing Method	GRADIENTE
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	14,0 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:23:41 AMT		
Date Processed:	22/07/2021 11:39:56 AMT		

Auto-Scaled Chromatogram

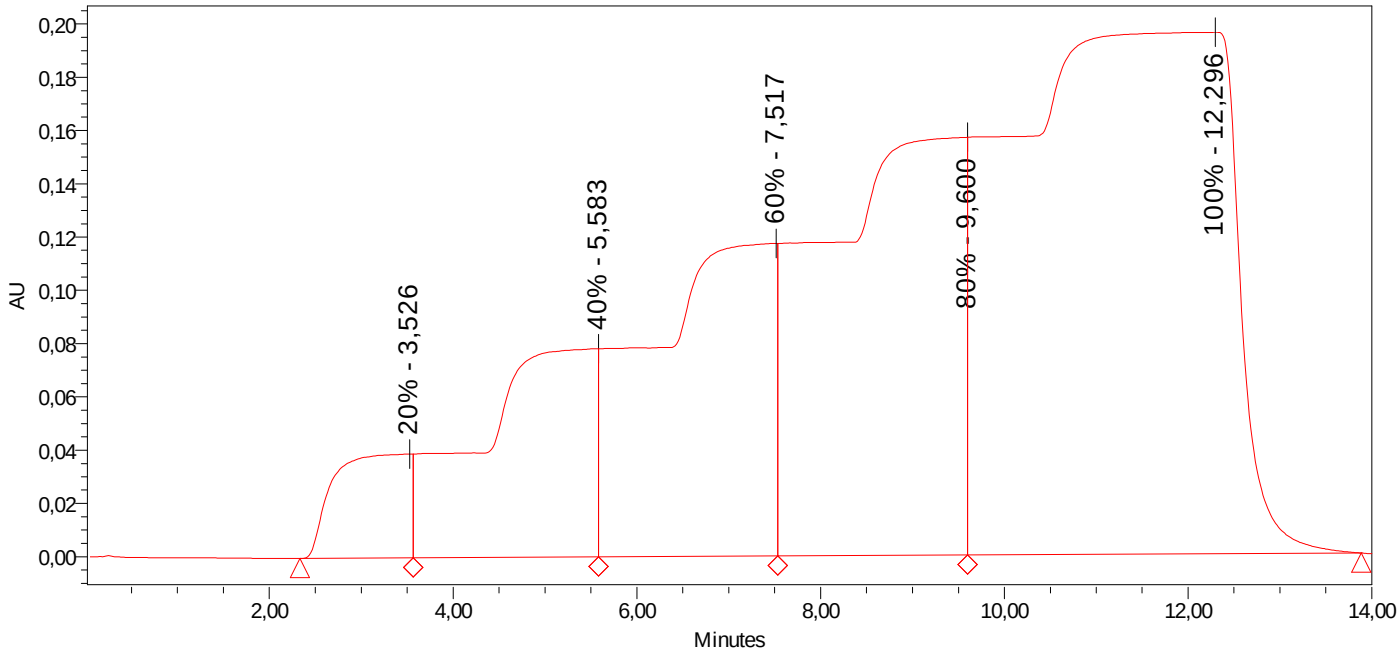


Peak Results

	Name	RT	Area	Height	Amount	Units
1	20%	3,526	2198635	38964		
2	40%	5,583	7001477	78168		
3	60%	7,517	11298572	117334		
4	80%	9,600	16899528	156858		
5	100%	12,296	33109384	195754		

SAMPLE INFORMATION

Sample Name:	GRADIENTE CD	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 586_1
Vial:	1	Acq. Method Set:	GRADIENTE CD_
Injection #:	1	Processing Method	GRADIENTE
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	14,0 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:38:37 AMT		
Date Processed:	22/07/2021 11:56:19 AMT		

Auto-Scaled Chromatogram

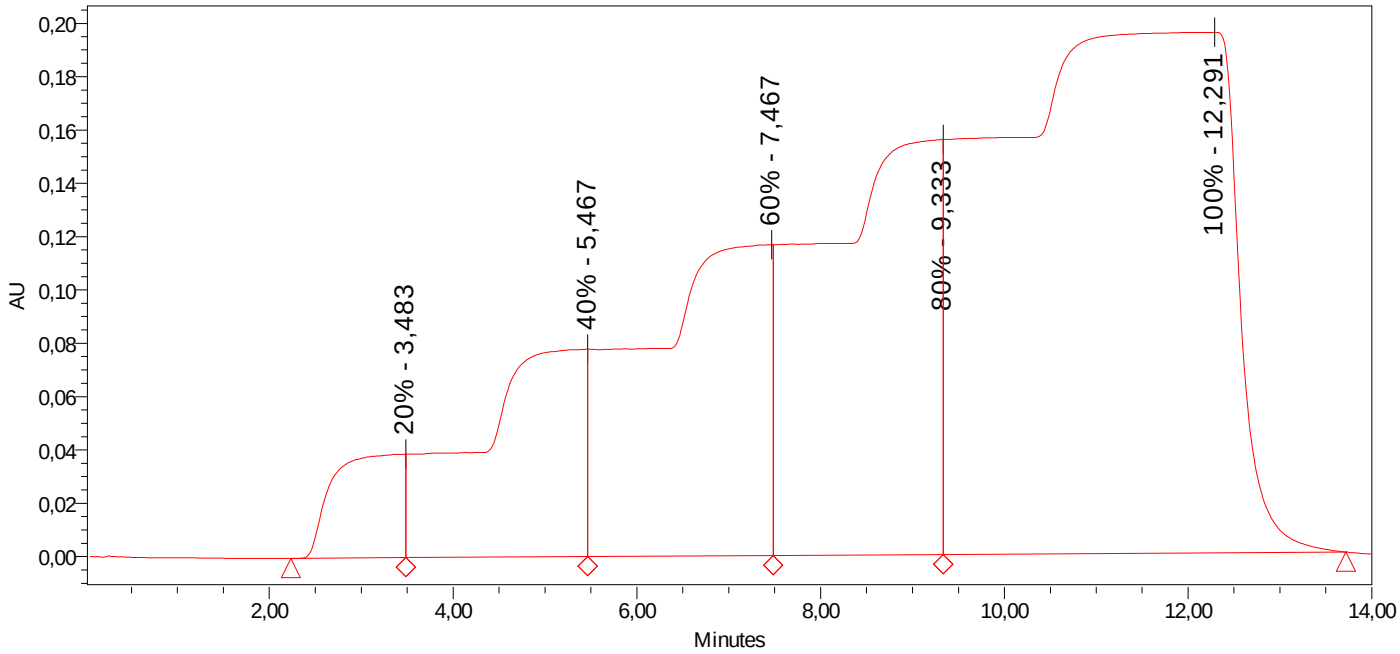

Peak Results

	Name	RT	Area	Height	Amount	Units
1	20%	3,483	2009302	38771		
2	40%	5,467	6662054	77801		
3	60%	7,467	11440609	116529		
4	80%	9,333	14678533	155663		
5	100%	12,291	35363526	195224		