
SAMPLE INFORMATION

Sample Name:	200	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	200
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:52:53 AMT		
Date Processed:	22/07/2021 11:50:14 AMT		

Auto-Scaled Chromatogram

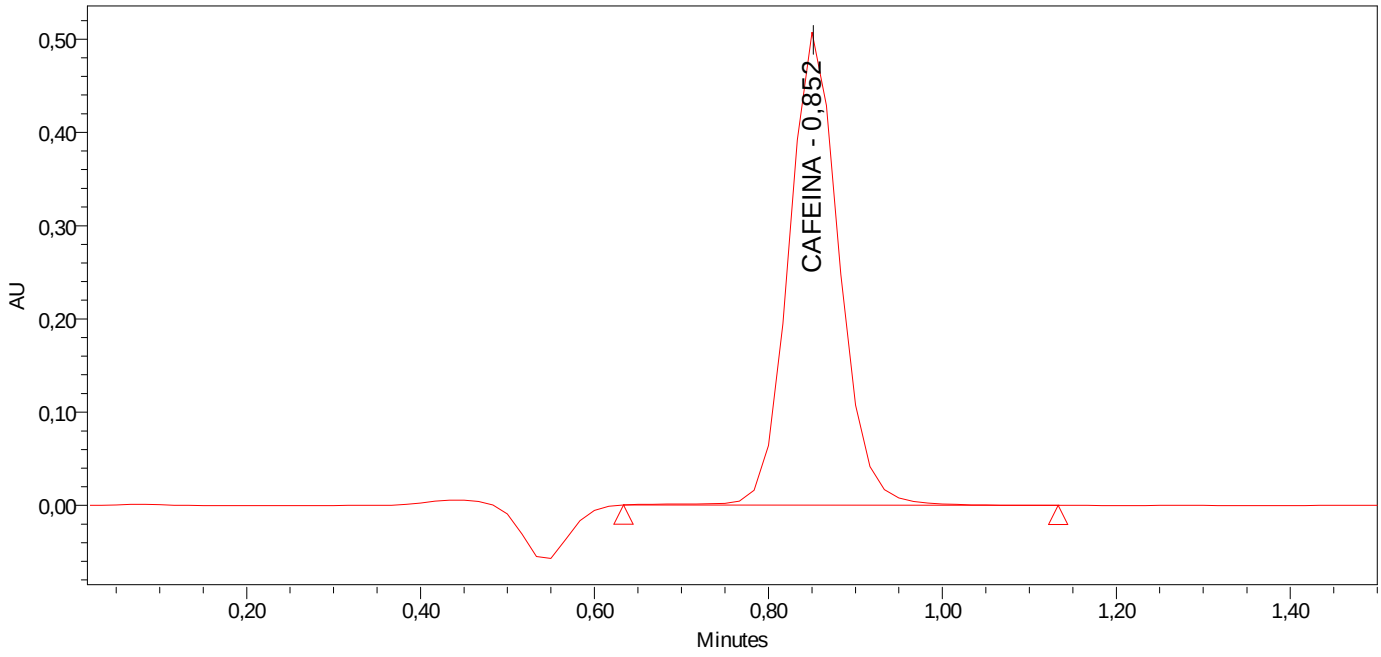


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	2044418	490331		

SAMPLE INFORMATION

Sample Name:	201	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	201
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:55:14 AMT		
Date Processed:	22/07/2021 11:50:26 AMT		

Auto-Scaled Chromatogram

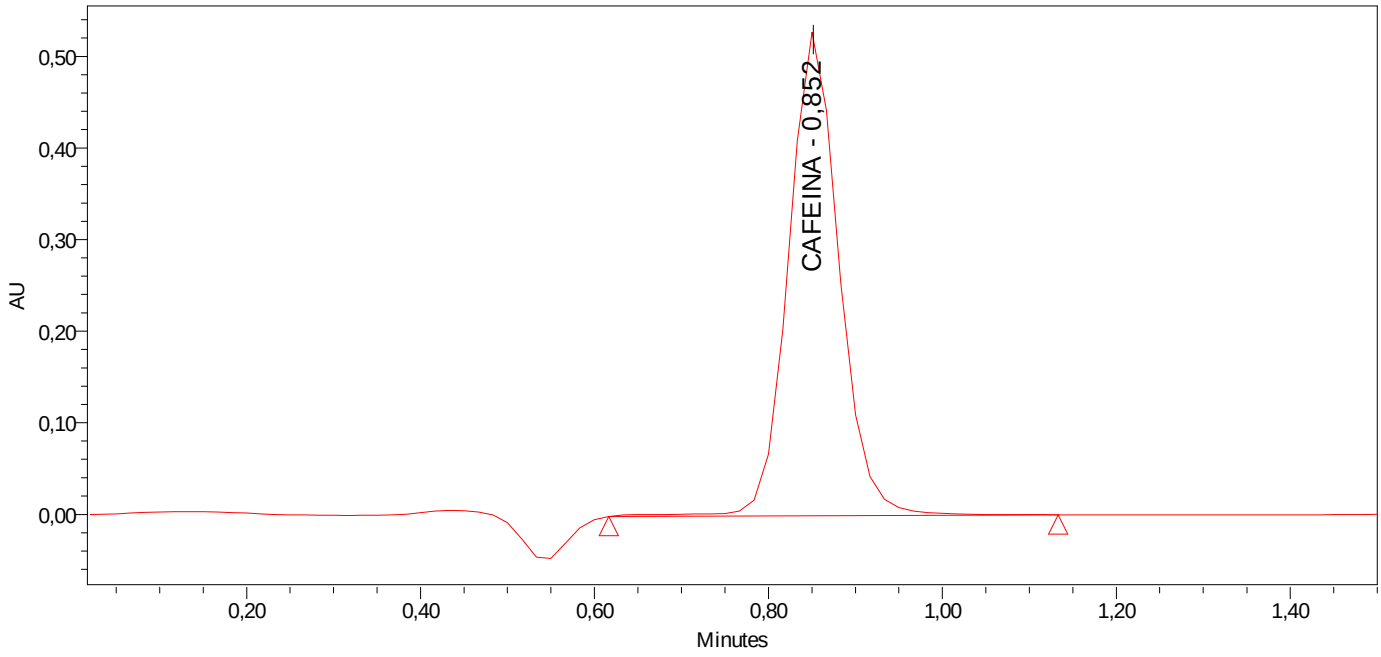


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	2133748	509806		

SAMPLE INFORMATION

Sample Name:	202	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	202
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:57:35 AMT		
Date Processed:	22/07/2021 11:50:35 AMT		

Auto-Scaled Chromatogram

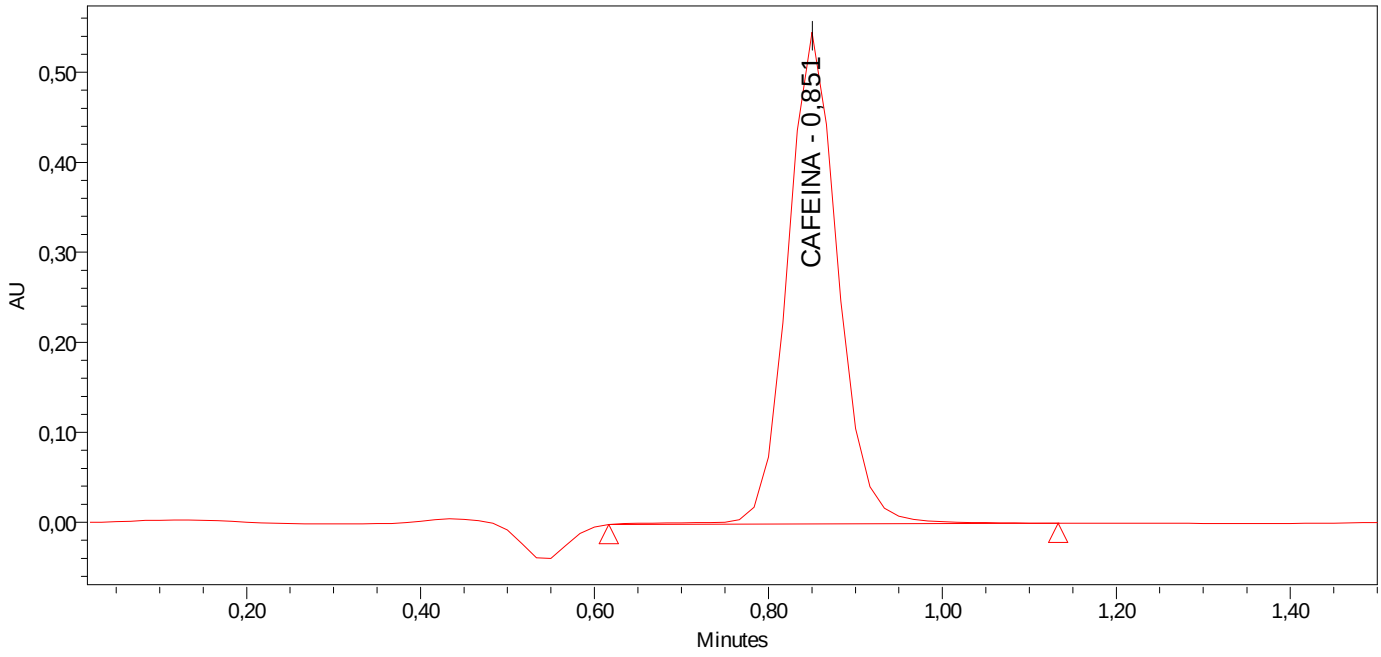


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	2193442	527012		

SAMPLE INFORMATION

Sample Name:	203	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	203
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:59:56 AMT		
Date Processed:	22/07/2021 11:50:42 AMT		

Auto-Scaled Chromatogram

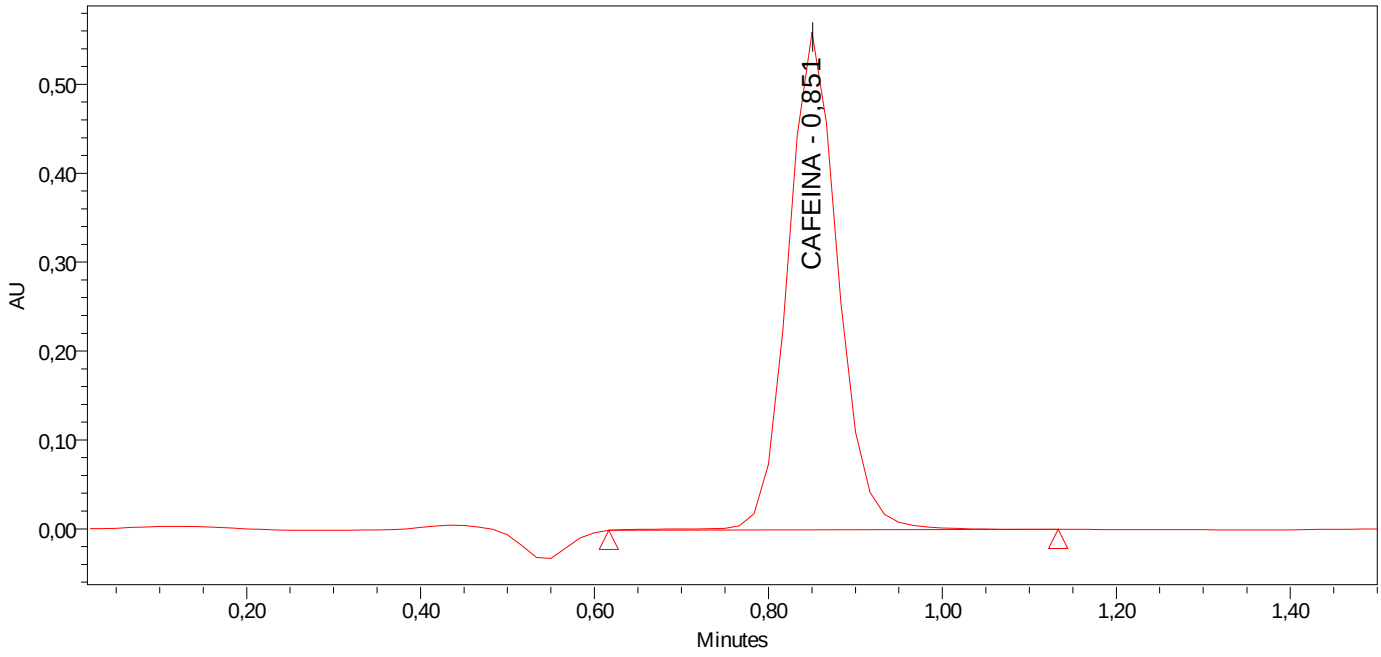


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	2242925	540104		

SAMPLE INFORMATION

Sample Name:	204	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	204
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:02:17 AMT		
Date Processed:	22/07/2021 11:50:51 AMT		

Auto-Scaled Chromatogram

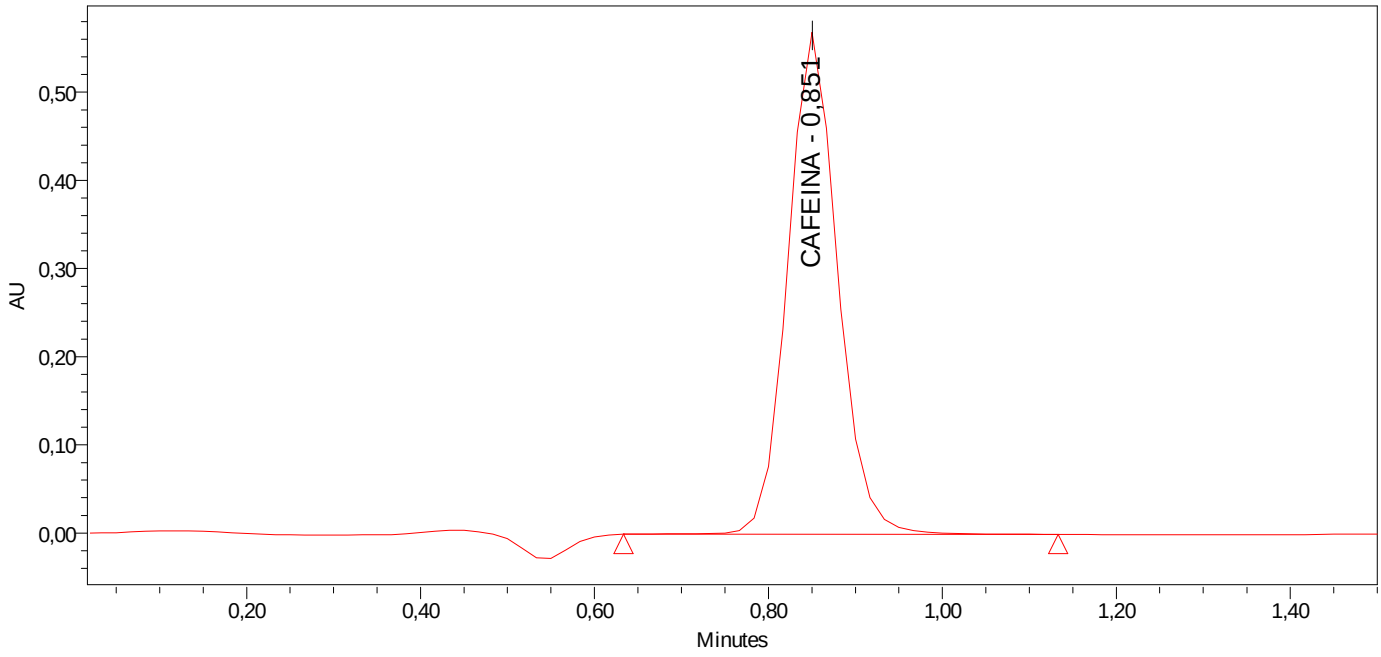


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	2263155	549125		

SAMPLE INFORMATION

Sample Name:	205	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	205
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:04:38 AMT		
Date Processed:	22/07/2021 11:50:59 AMT		

Auto-Scaled Chromatogram

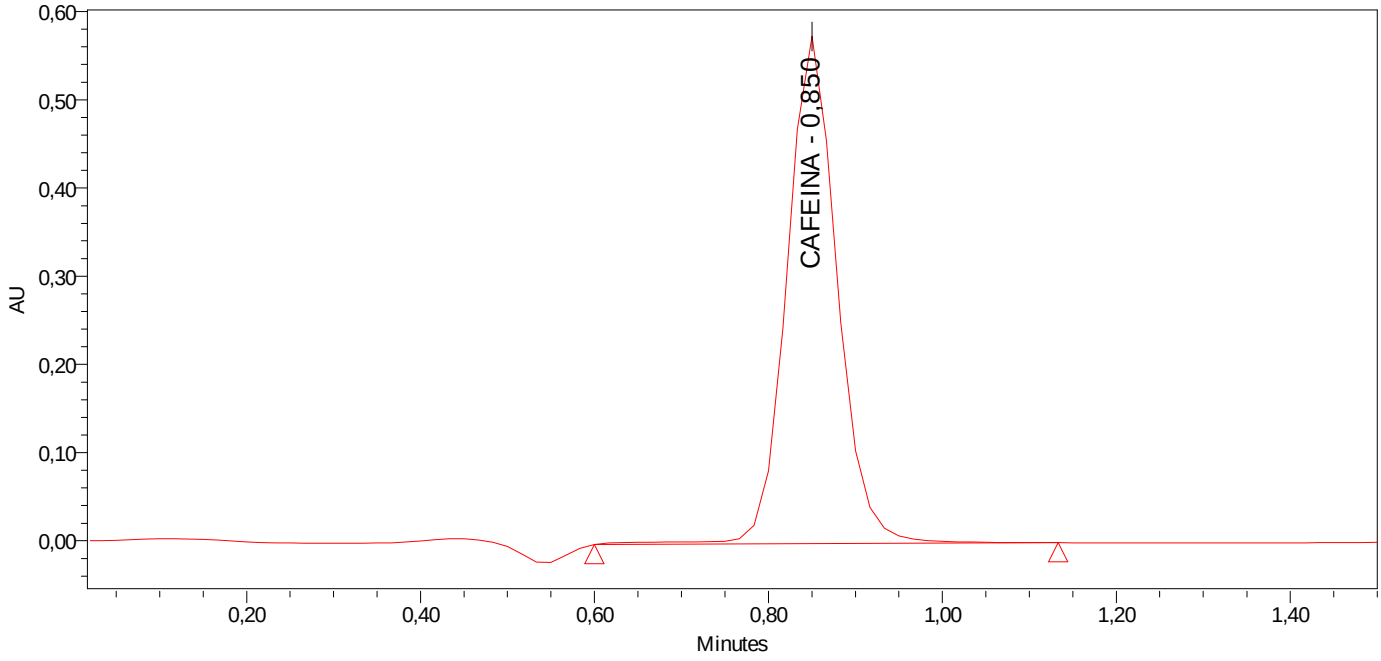


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	2316366	554880		

SAMPLE INFORMATION

Sample Name:	206	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	206
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:06:59 AMT		
Date Processed:	22/07/2021 11:51:06 AMT		

Auto-Scaled Chromatogram

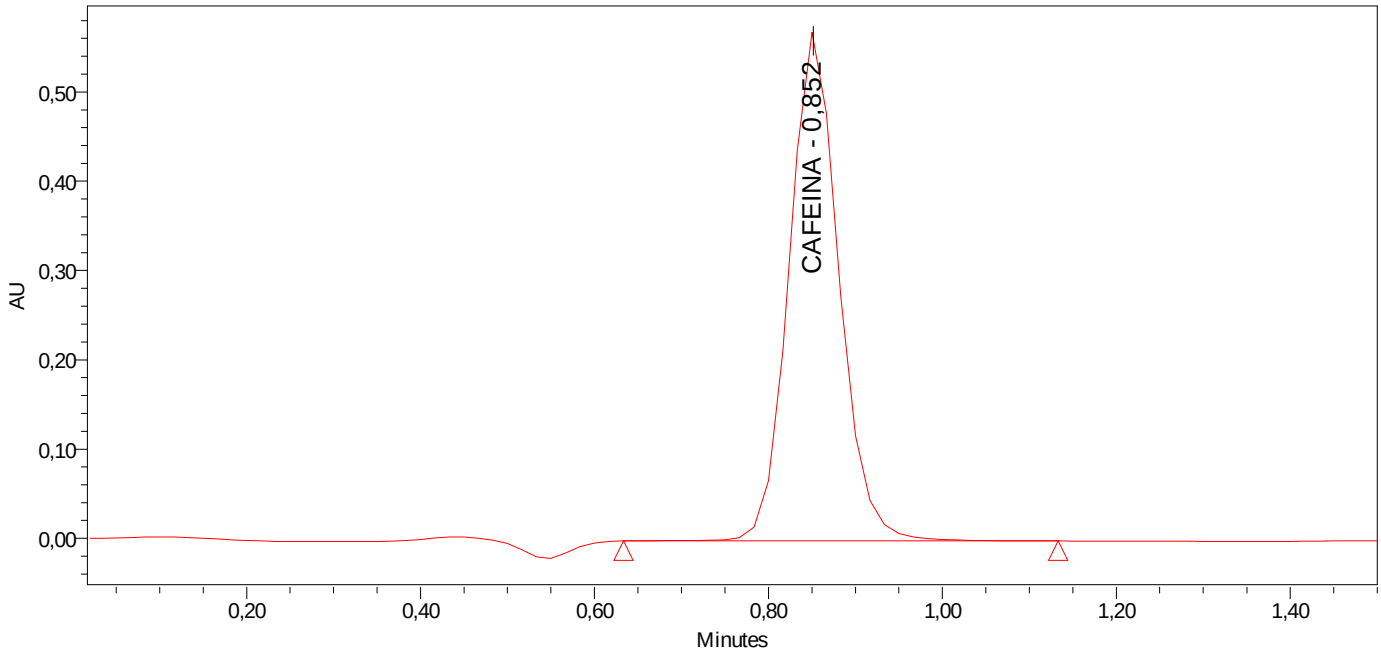


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	2265277	549978		

SAMPLE INFORMATION

Sample Name:	207	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	207
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:09:20 AMT		
Date Processed:	22/07/2021 11:51:14 AMT		

Auto-Scaled Chromatogram

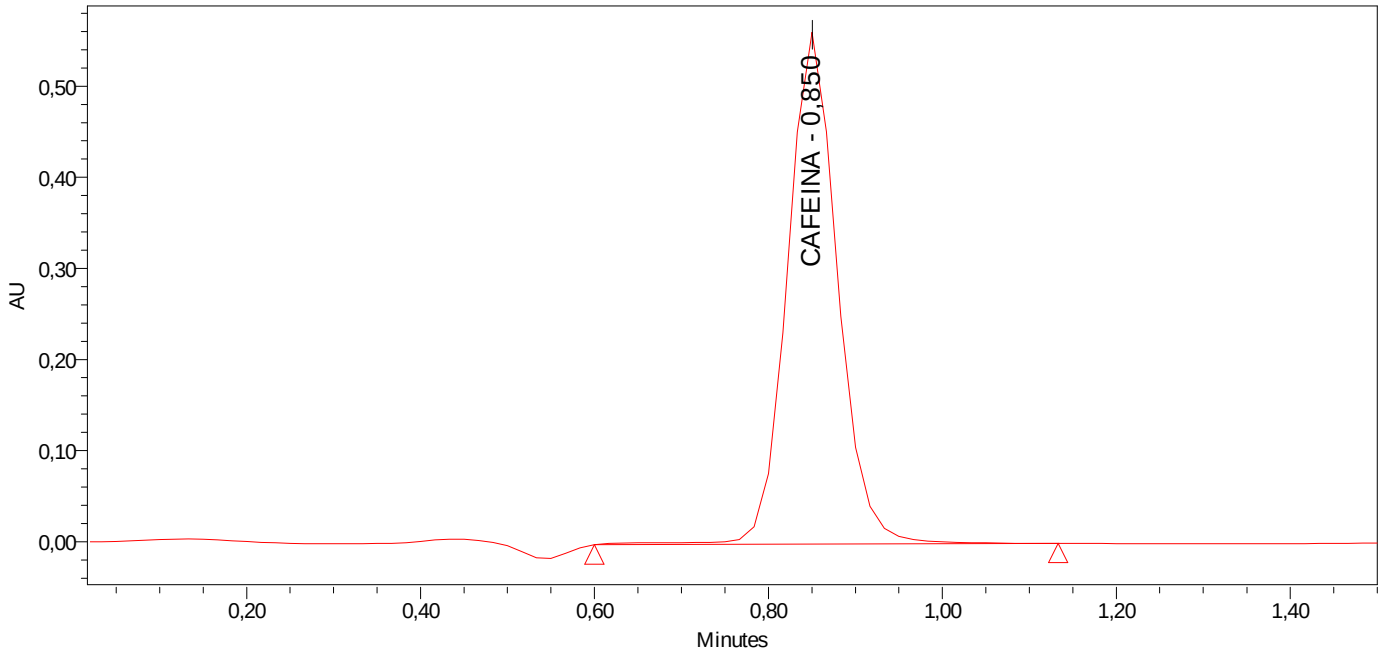


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	2255829	541834		

SAMPLE INFORMATION

Sample Name:	208	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	208
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:11:41 AMT		
Date Processed:	22/07/2021 11:51:20 AMT		

Auto-Scaled Chromatogram

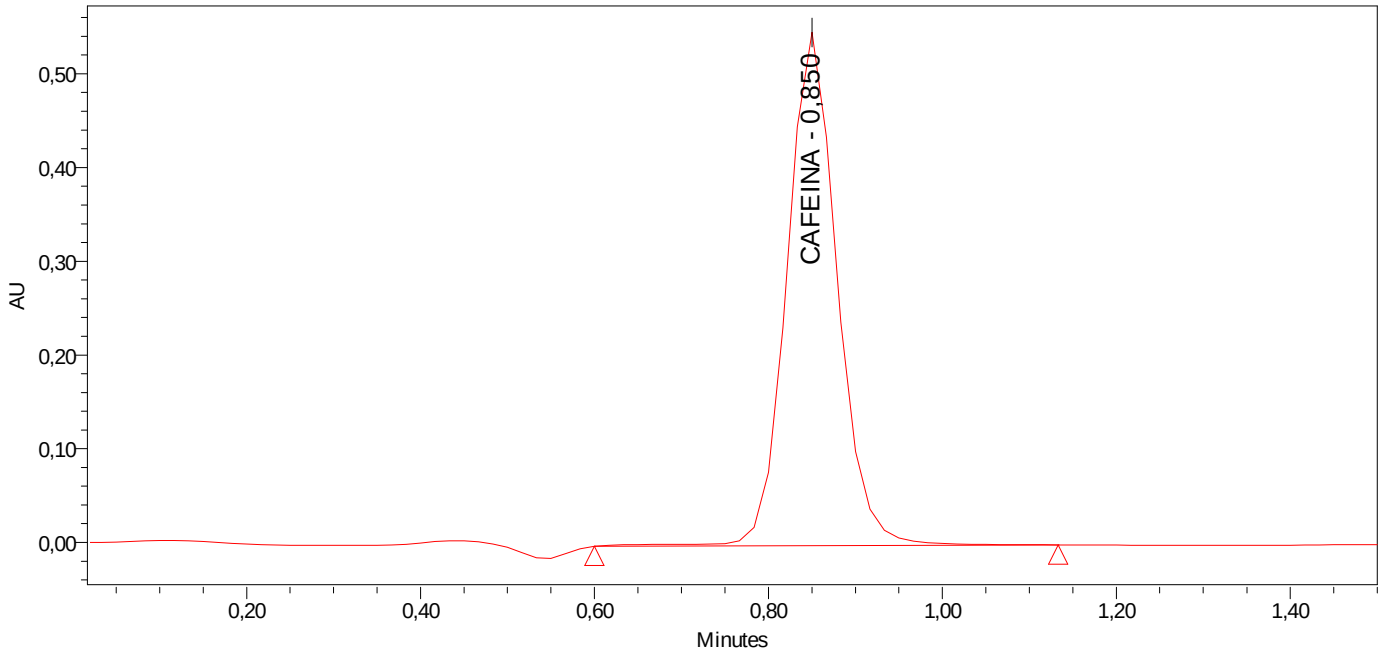


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	2194764	528145		

SAMPLE INFORMATION

Sample Name:	209	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	209
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:14:02 AMT		
Date Processed:	22/07/2021 11:51:29 AMT		

Auto-Scaled Chromatogram

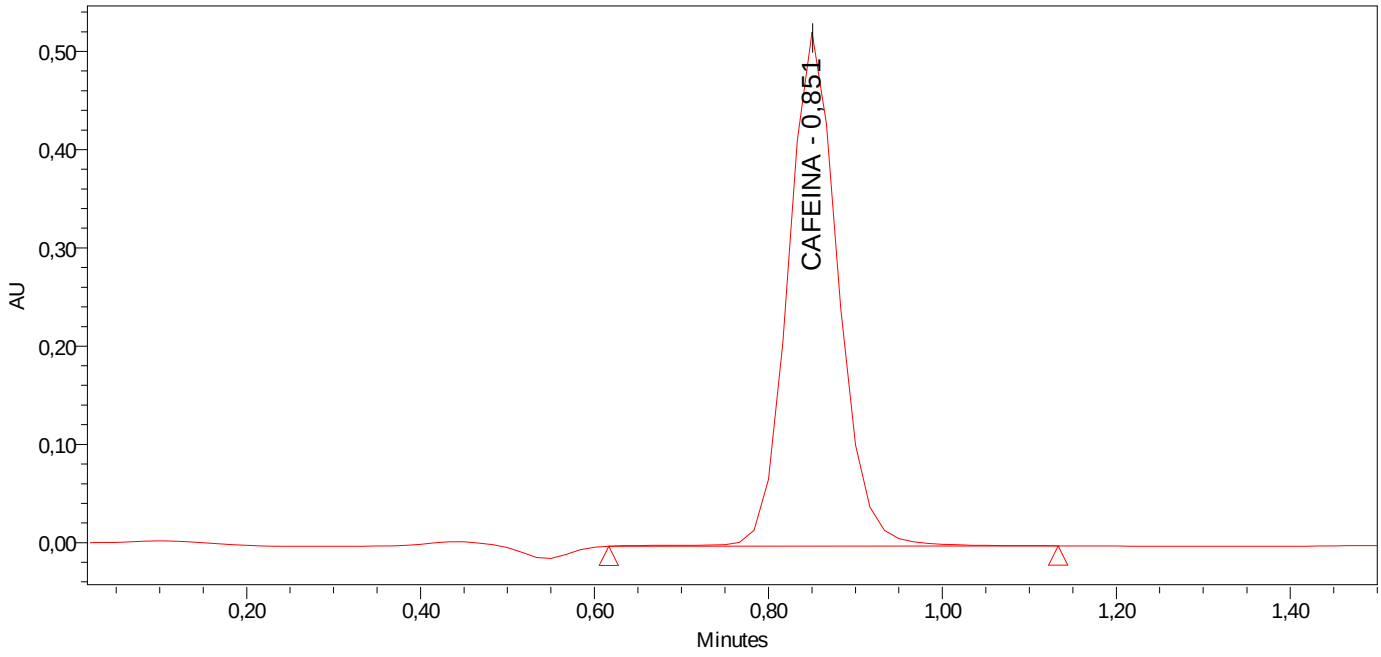


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	2085388	504683		

SAMPLE INFORMATION

Sample Name:	210	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	210
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:16:23 AMT		
Date Processed:	22/07/2021 11:51:36 AMT		

Auto-Scaled Chromatogram

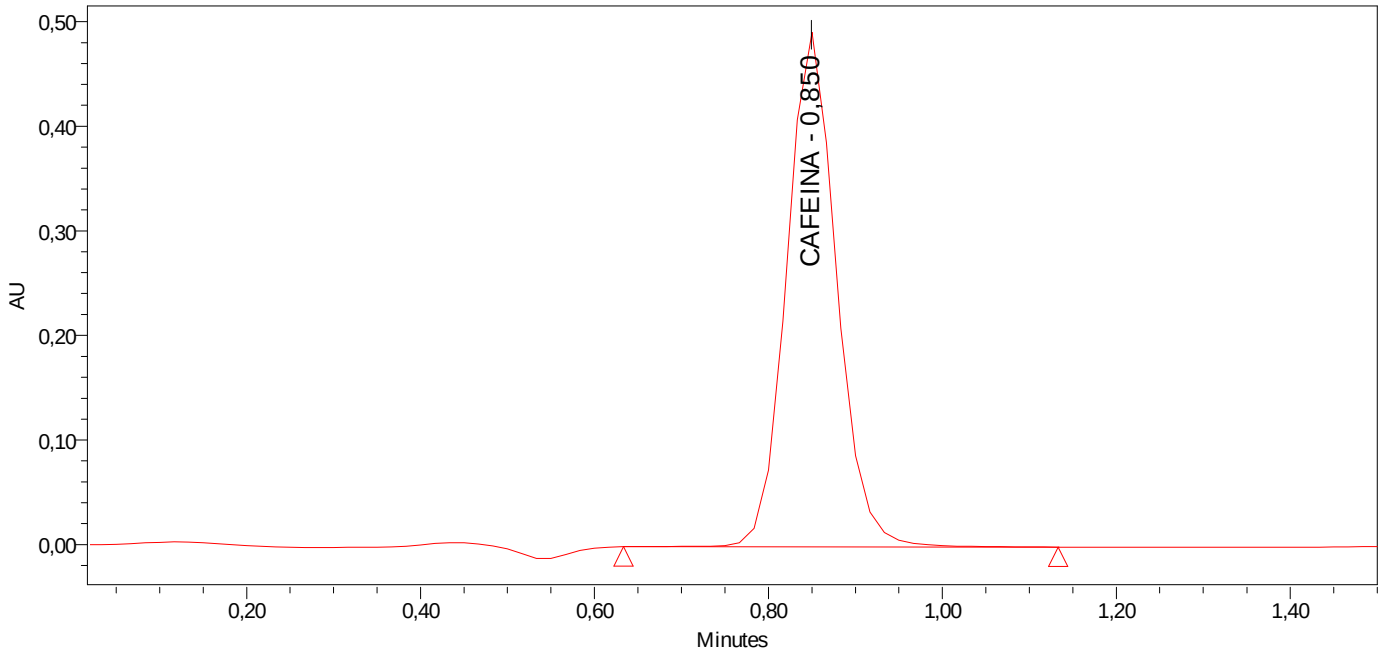


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	1959822	475050		

SAMPLE INFORMATION

Sample Name:	240	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	240
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:18:44 AMT		
Date Processed:	22/07/2021 11:44:33 AMT		

Auto-Scaled Chromatogram

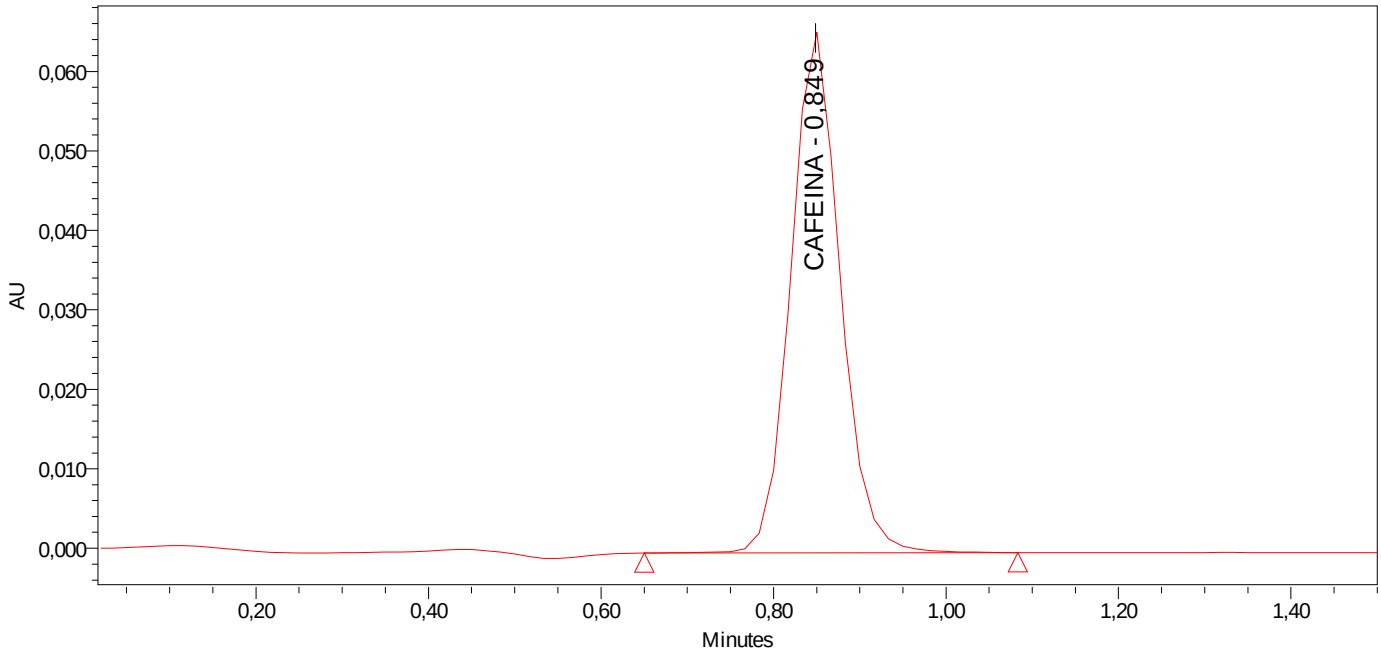


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	260447	63285		

SAMPLE INFORMATION

Sample Name:	241	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	241
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:21:05 AMT		
Date Processed:	22/07/2021 11:44:41 AMT		

Auto-Scaled Chromatogram

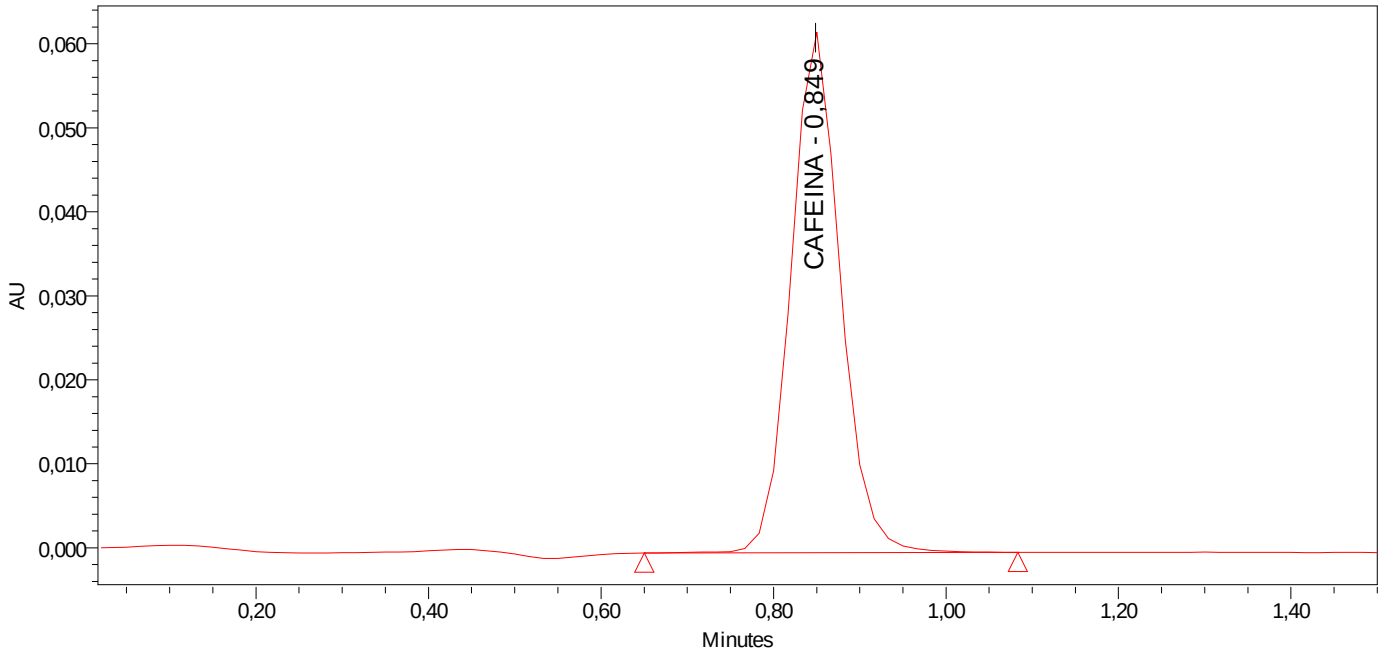


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	246810	59875		

SAMPLE INFORMATION

Sample Name:	242	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	242
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:23:26 AMT		
Date Processed:	22/07/2021 11:44:44 AMT		

Auto-Scaled Chromatogram

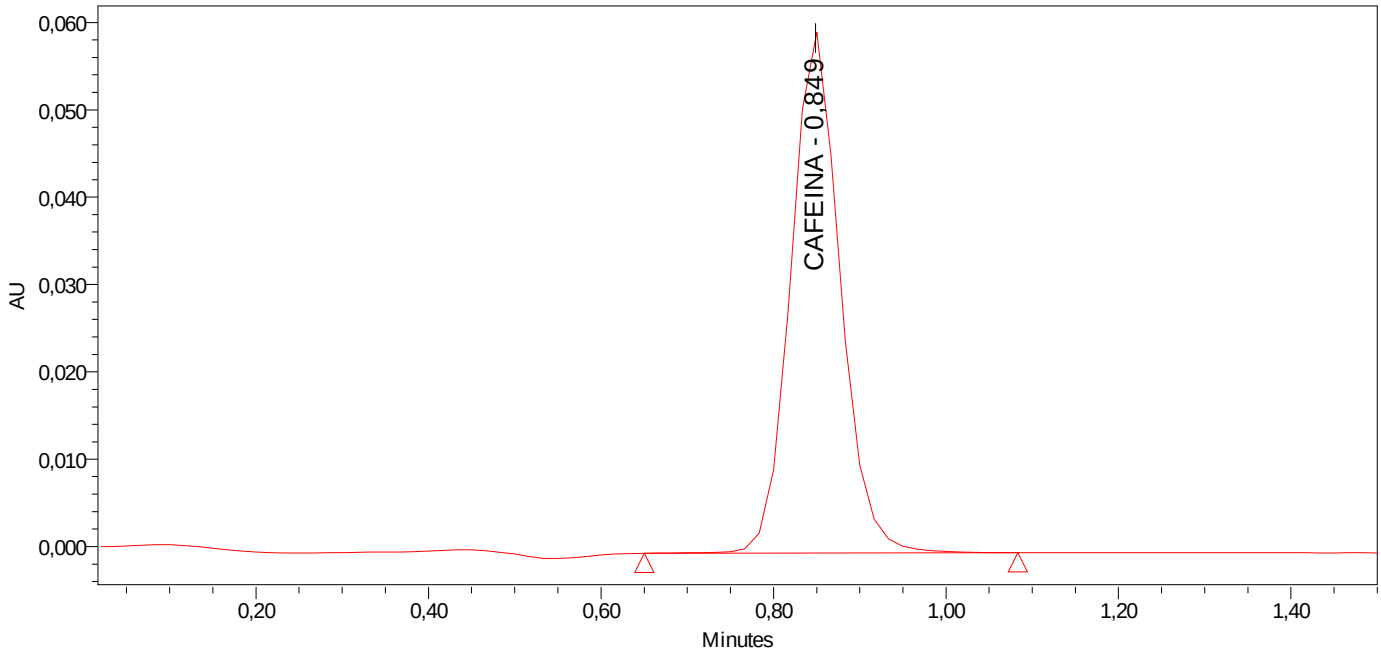


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	237963	57628		

SAMPLE INFORMATION

Sample Name:	243	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	243
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:25:47 AMT		
Date Processed:	22/07/2021 11:44:45 AMT		

Auto-Scaled Chromatogram

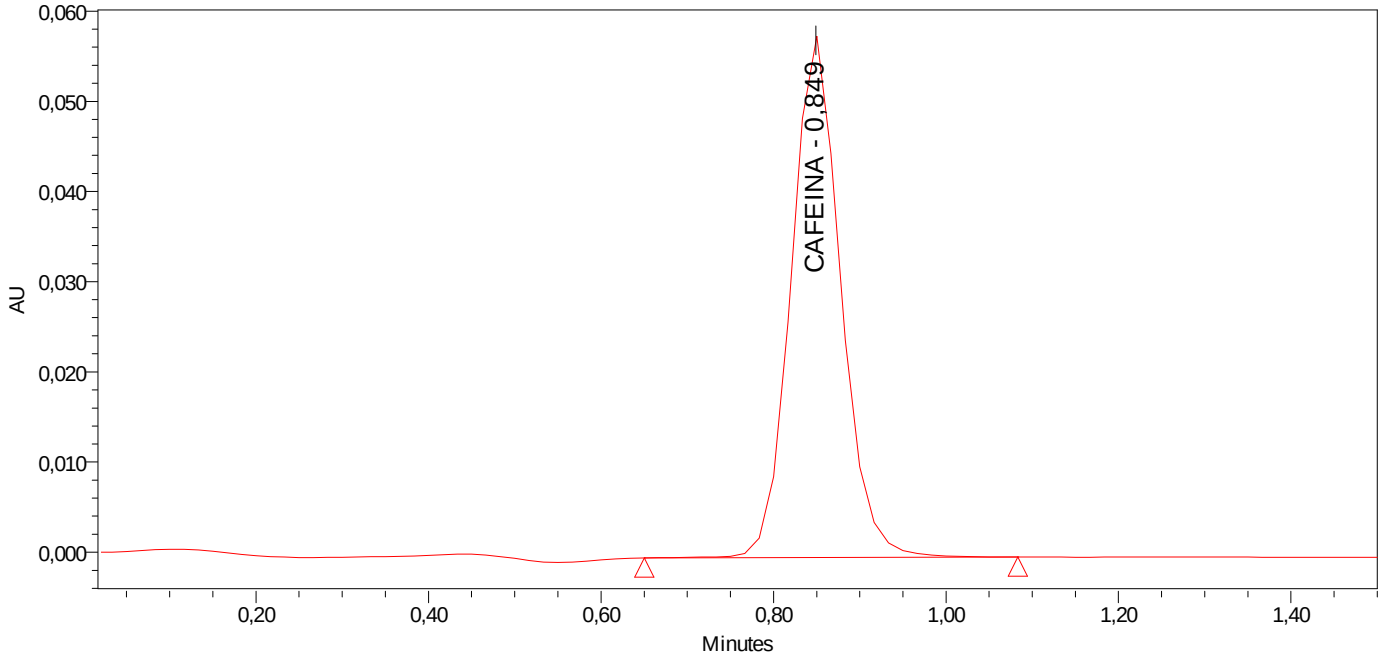


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	230774	55844		

SAMPLE INFORMATION

Sample Name:	244	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	244
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:28:08 AMT		
Date Processed:	22/07/2021 11:44:47 AMT		

Auto-Scaled Chromatogram

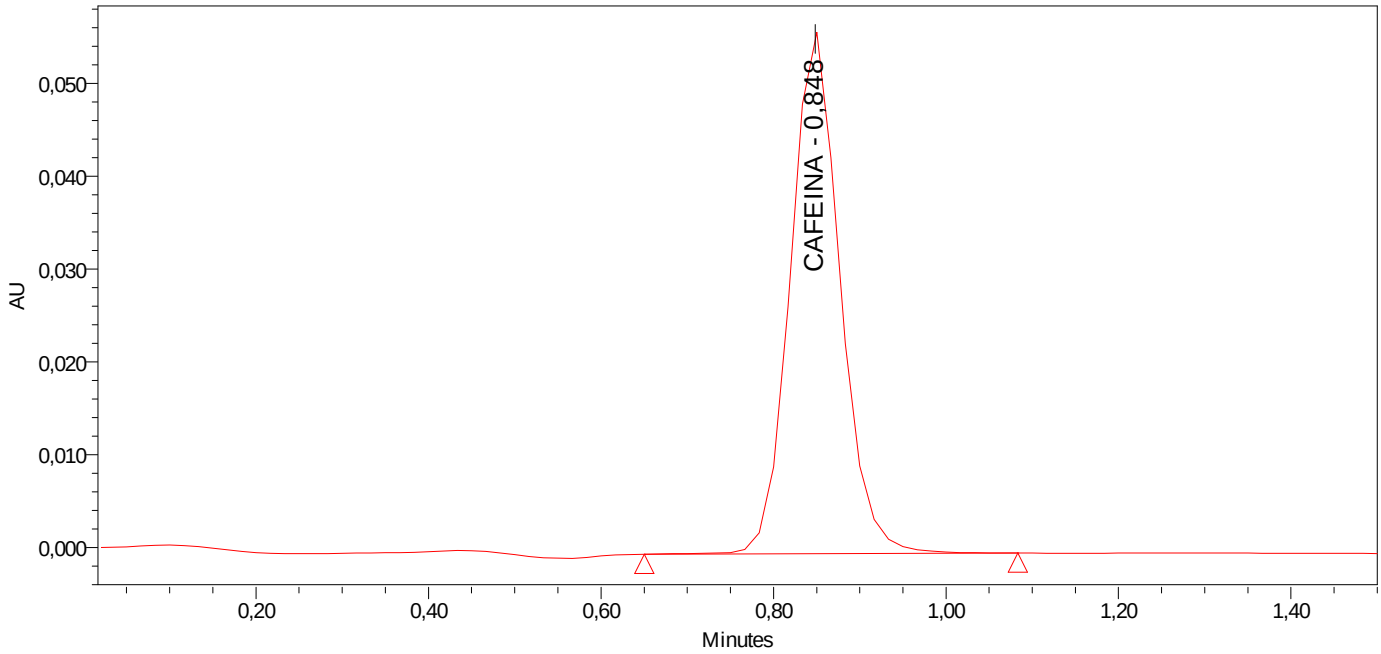


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	225424	54362		

SAMPLE INFORMATION

Sample Name:	245	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	245
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:30:29 AMT		
Date Processed:	22/07/2021 11:44:51 AMT		

Auto-Scaled Chromatogram

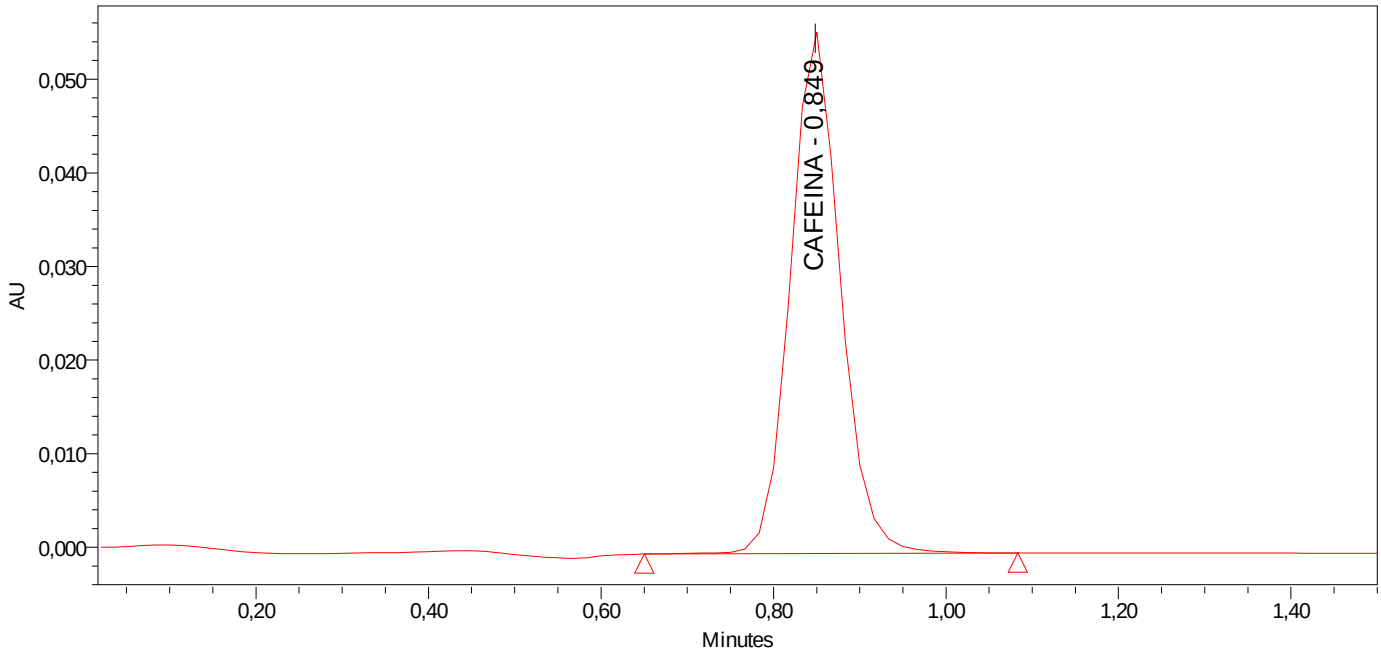


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	223645	53870		

SAMPLE INFORMATION

Sample Name:	246	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	246
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:32:50 AMT		
Date Processed:	22/07/2021 11:44:55 AMT		

Auto-Scaled Chromatogram

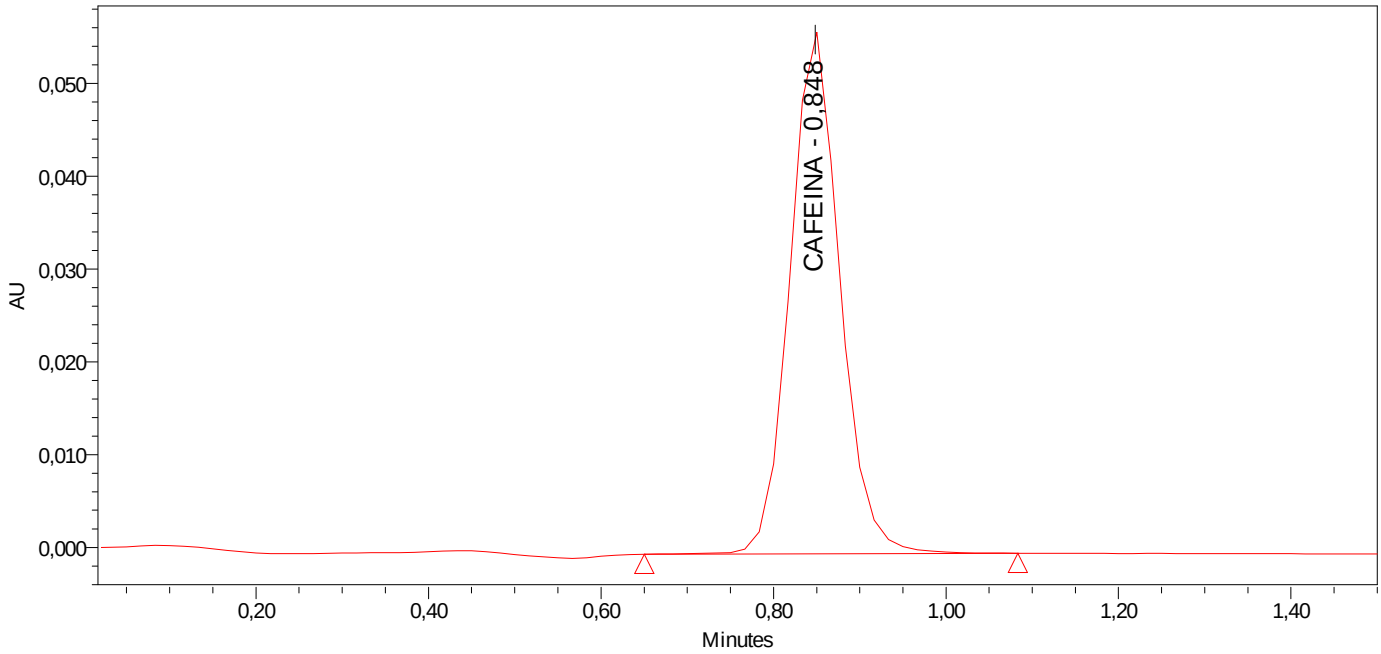


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	226197	54420		

SAMPLE INFORMATION

Sample Name:	247	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	247
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:35:11 AMT		
Date Processed:	22/07/2021 11:45:00 AMT		

Auto-Scaled Chromatogram

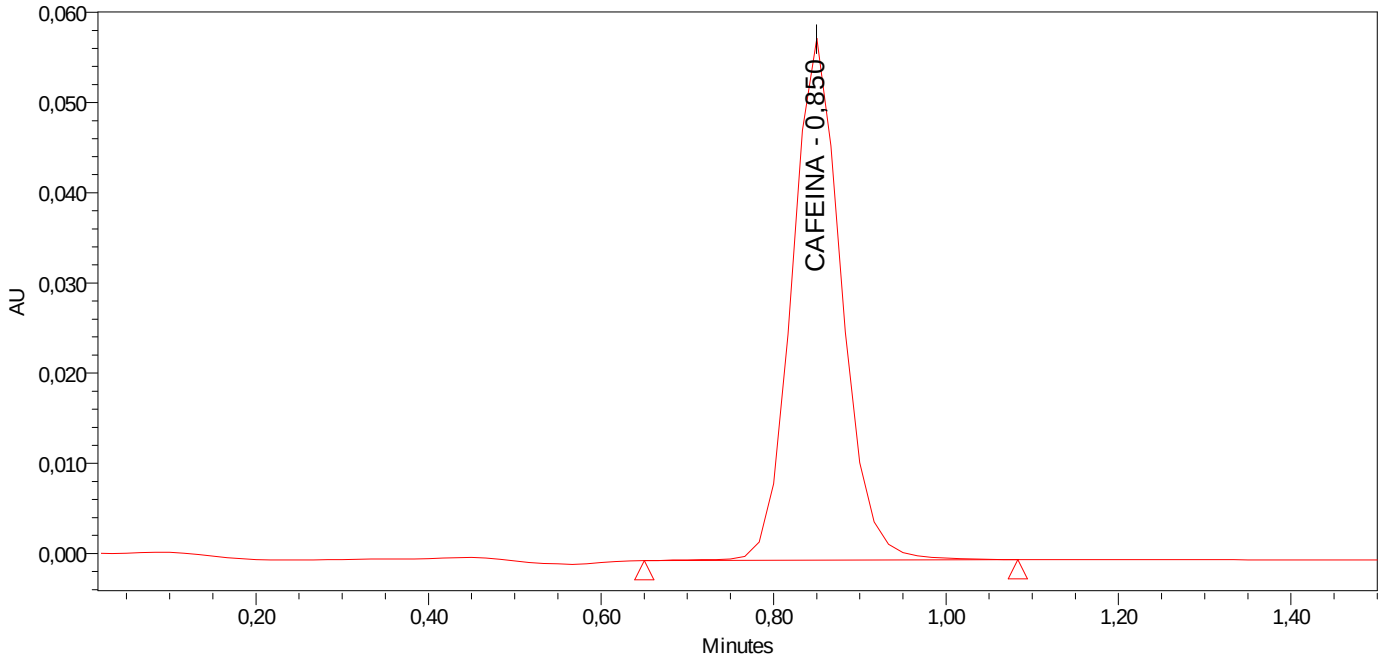


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	231704	55864		

SAMPLE INFORMATION

Sample Name:	248	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	248
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:37:32 AMT		
Date Processed:	22/07/2021 11:45:01 AMT		

Auto-Scaled Chromatogram

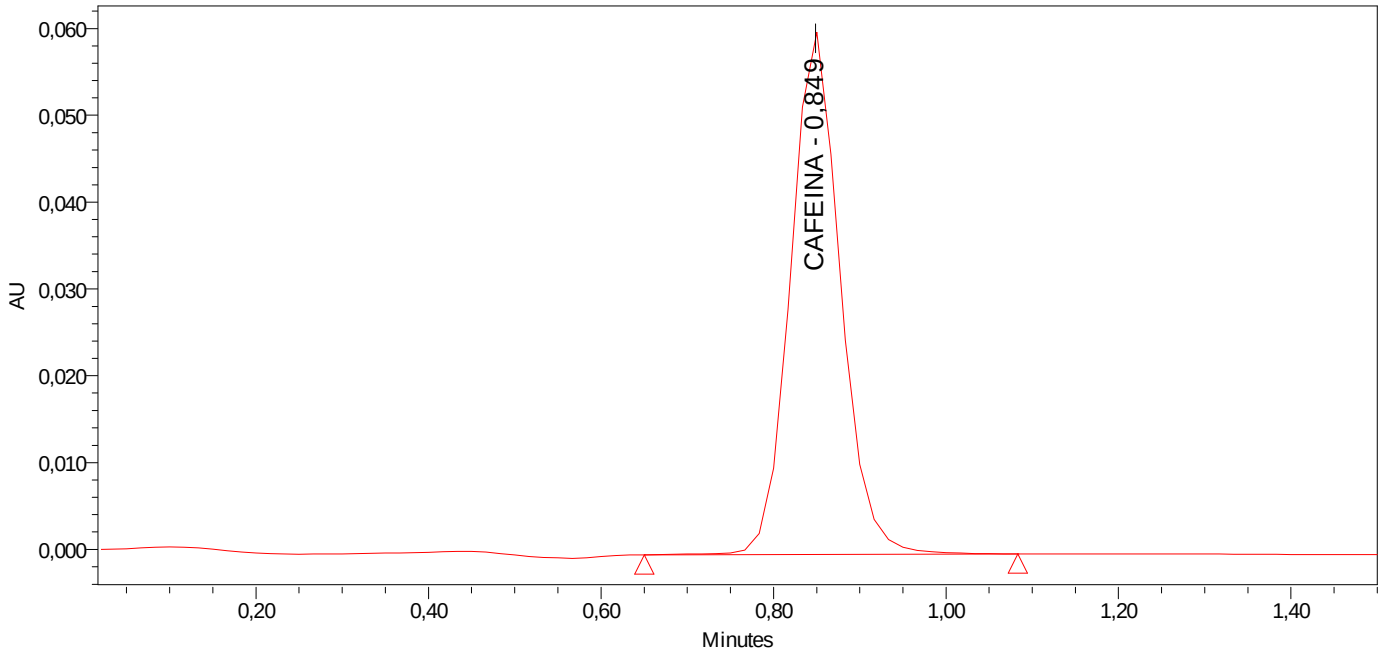


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,849	241873	58186		

SAMPLE INFORMATION

Sample Name:	249	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	249
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:39:53 AMT		
Date Processed:	22/07/2021 11:45:02 AMT		

Auto-Scaled Chromatogram

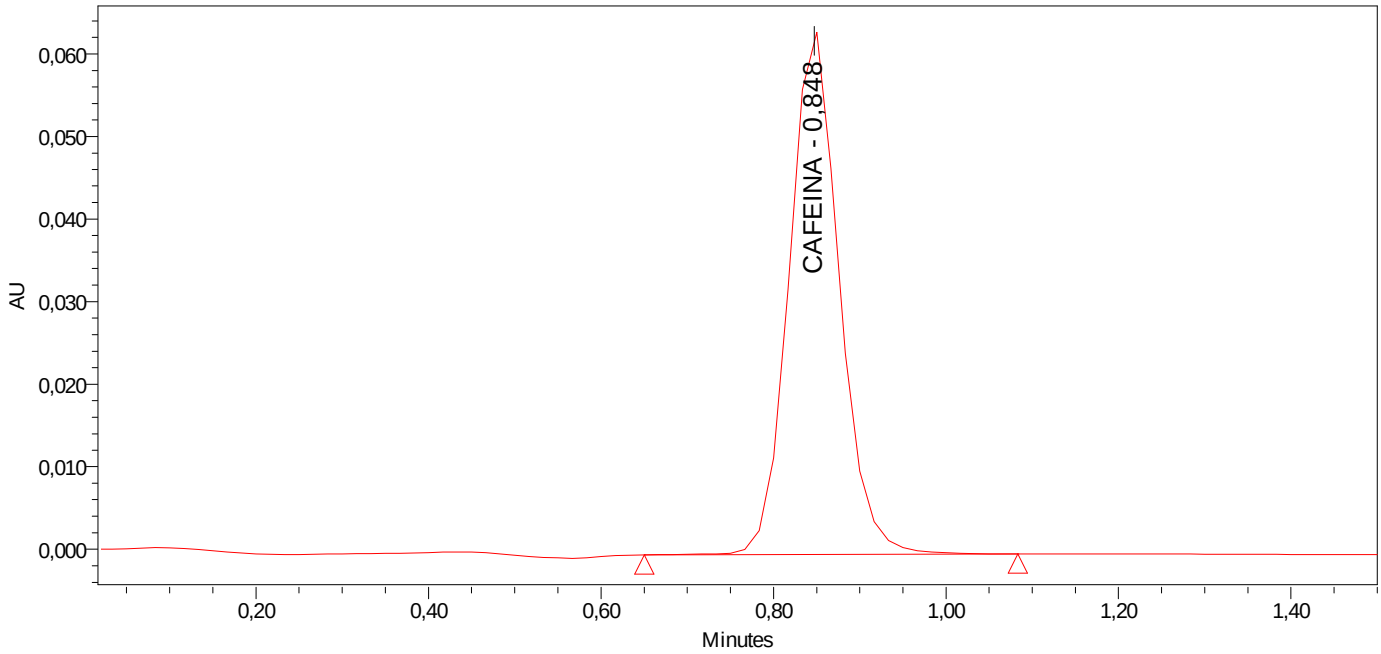


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	256166	61433		

SAMPLE INFORMATION

Sample Name:	250	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	250
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:42:14 AMT		
Date Processed:	22/07/2021 11:45:02 AMT		

Auto-Scaled Chromatogram

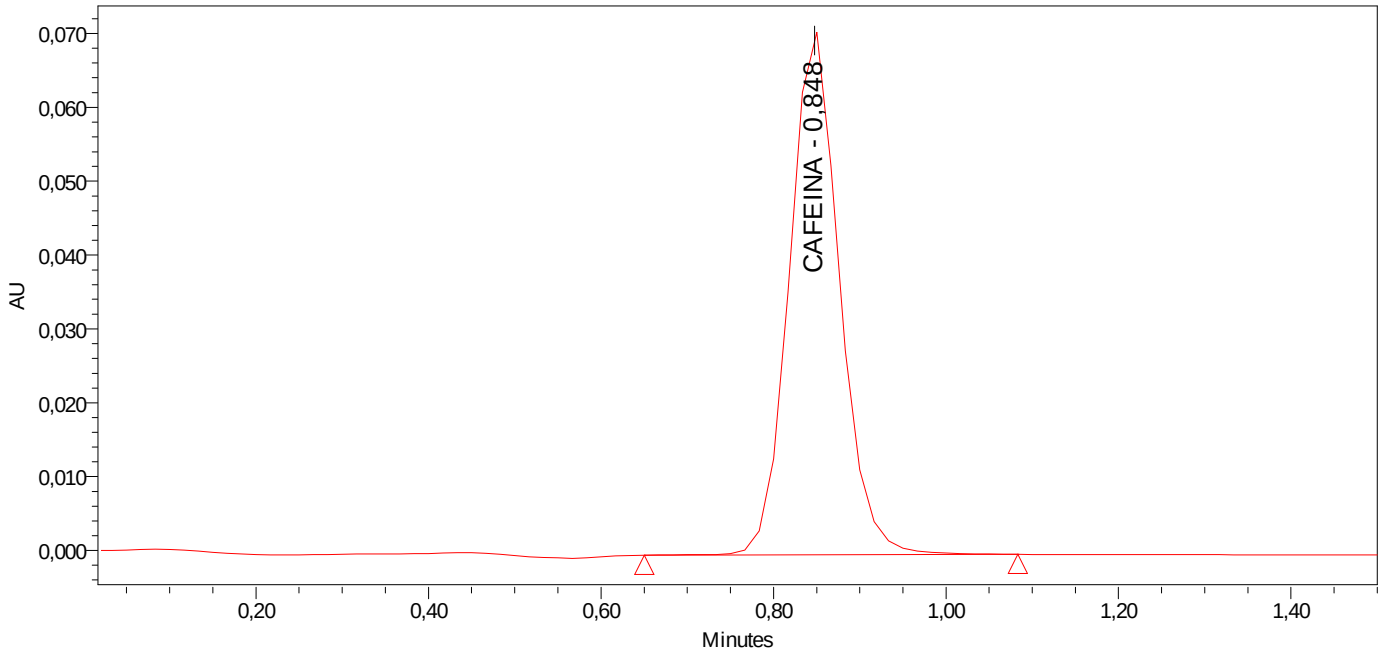


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	286663	68679		

SAMPLE INFORMATION

Sample Name:	268	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	268
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:44:35 AMT		
Date Processed:	22/07/2021 12:12:28 AMT		

Auto-Scaled Chromatogram

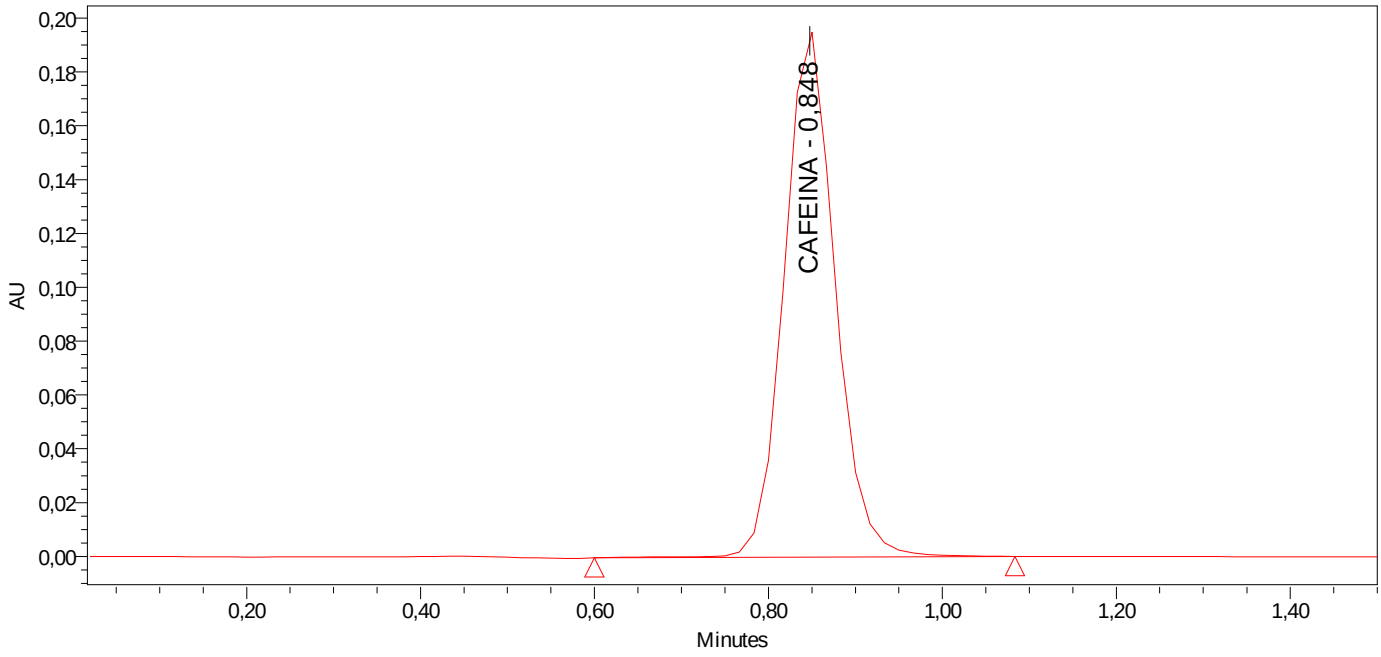


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	790554	189163		

SAMPLE INFORMATION

Sample Name:	269	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	269
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:46:56 AMT		
Date Processed:	22/07/2021 12:12:35 AMT		

Auto-Scaled Chromatogram

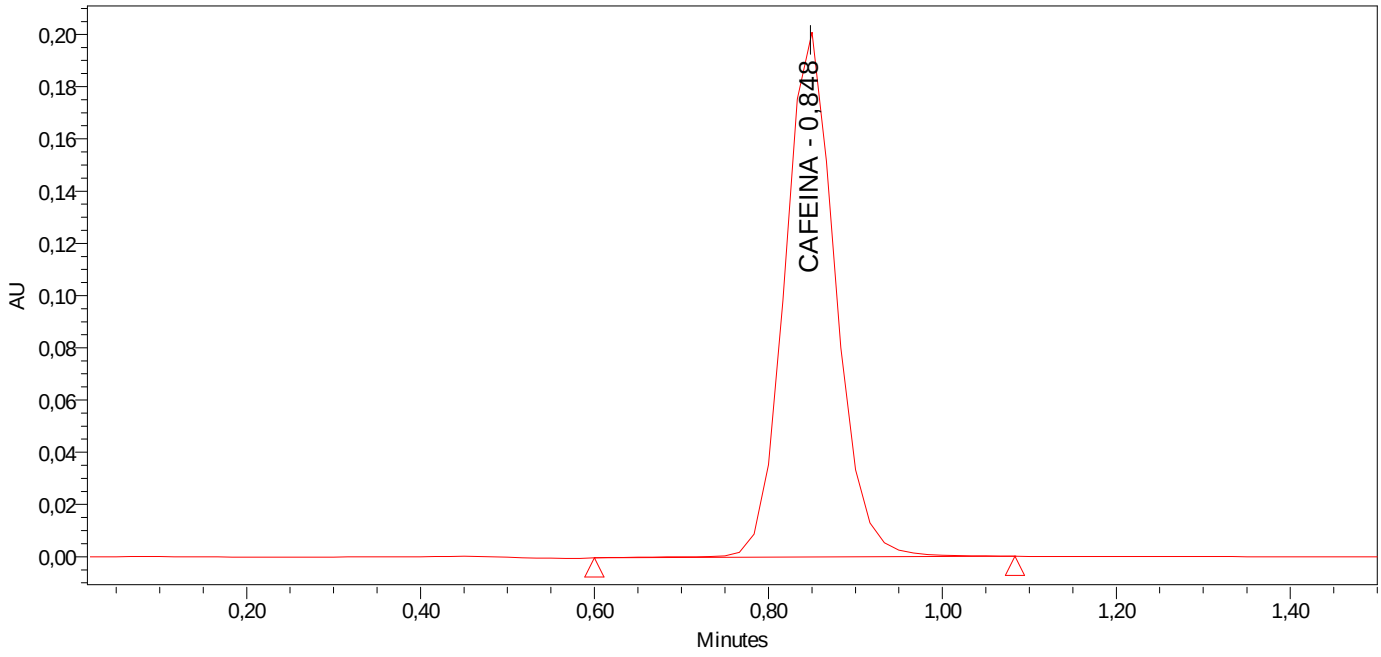


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	812147	194757		

SAMPLE INFORMATION

Sample Name:	270	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	270
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:49:17 AMT		
Date Processed:	22/07/2021 12:12:36 AMT		

Auto-Scaled Chromatogram

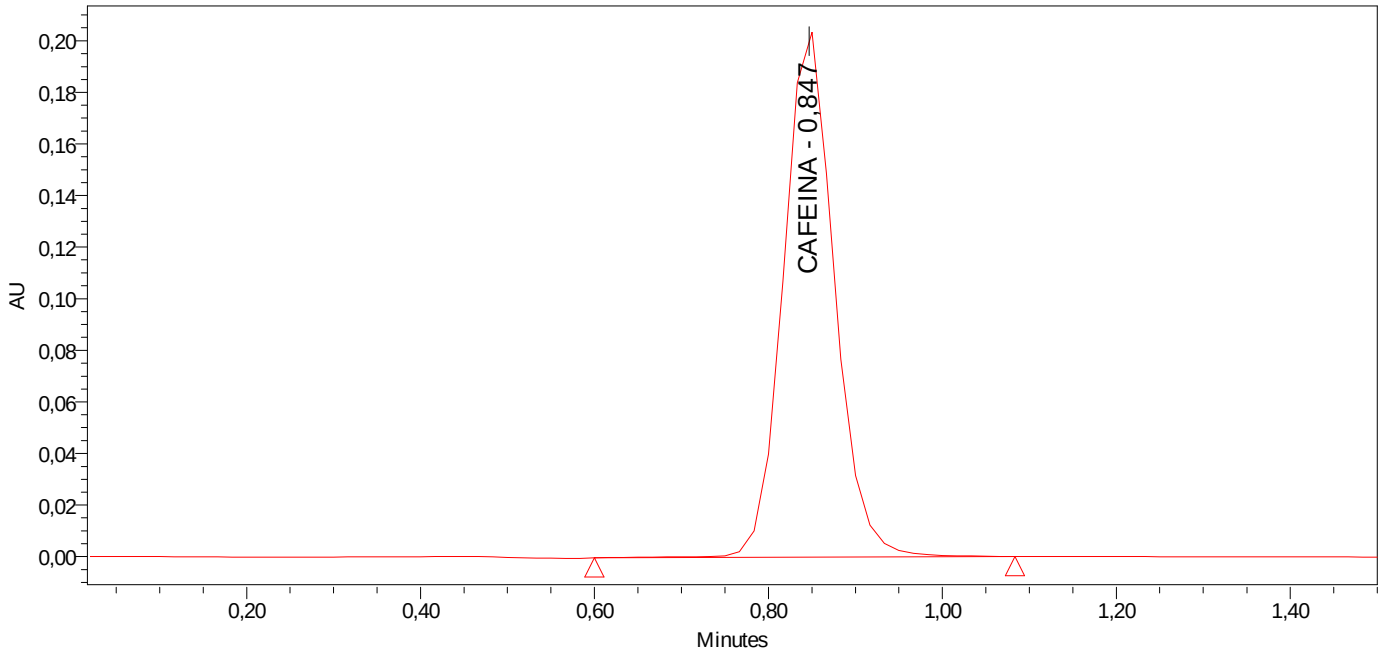


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	828807	197982		

SAMPLE INFORMATION

Sample Name:	271	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	271
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:51:38 AMT		
Date Processed:	22/07/2021 12:12:37 AMT		

Auto-Scaled Chromatogram

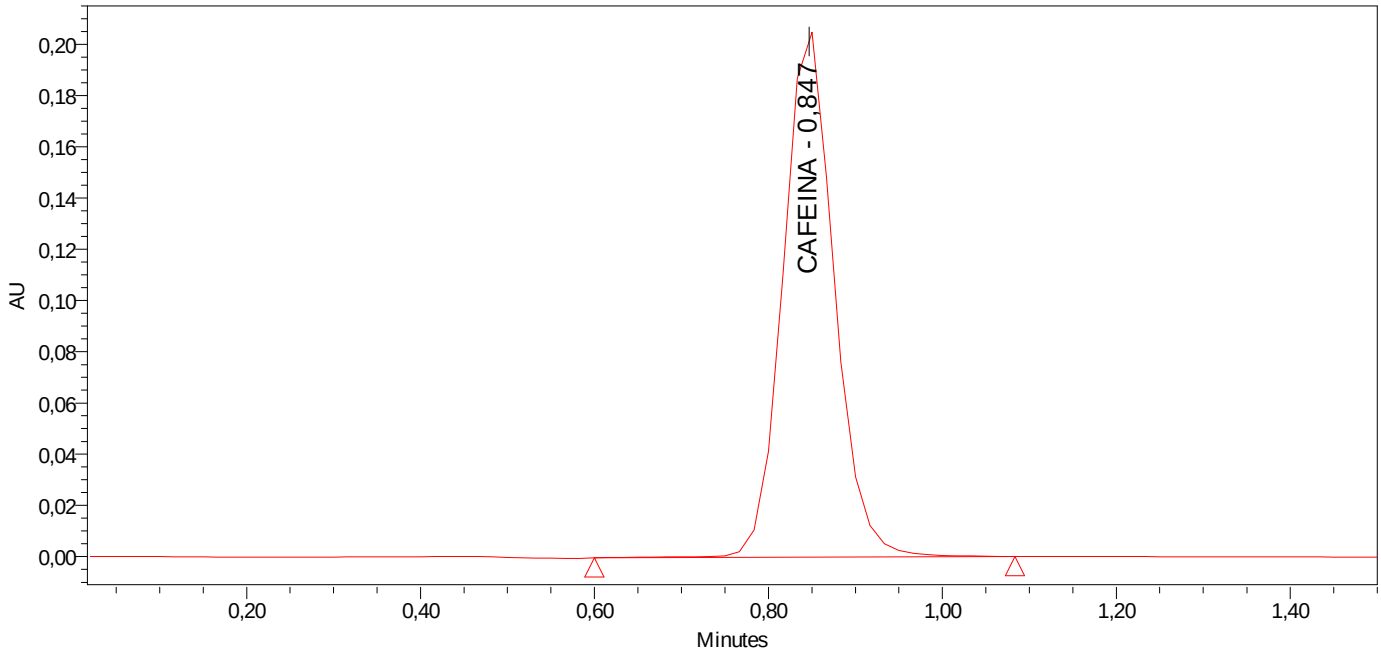


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	837482	199676		

SAMPLE INFORMATION

Sample Name:	272	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	272
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:53:59 AMT		
Date Processed:	22/07/2021 12:12:38 AMT		

Auto-Scaled Chromatogram

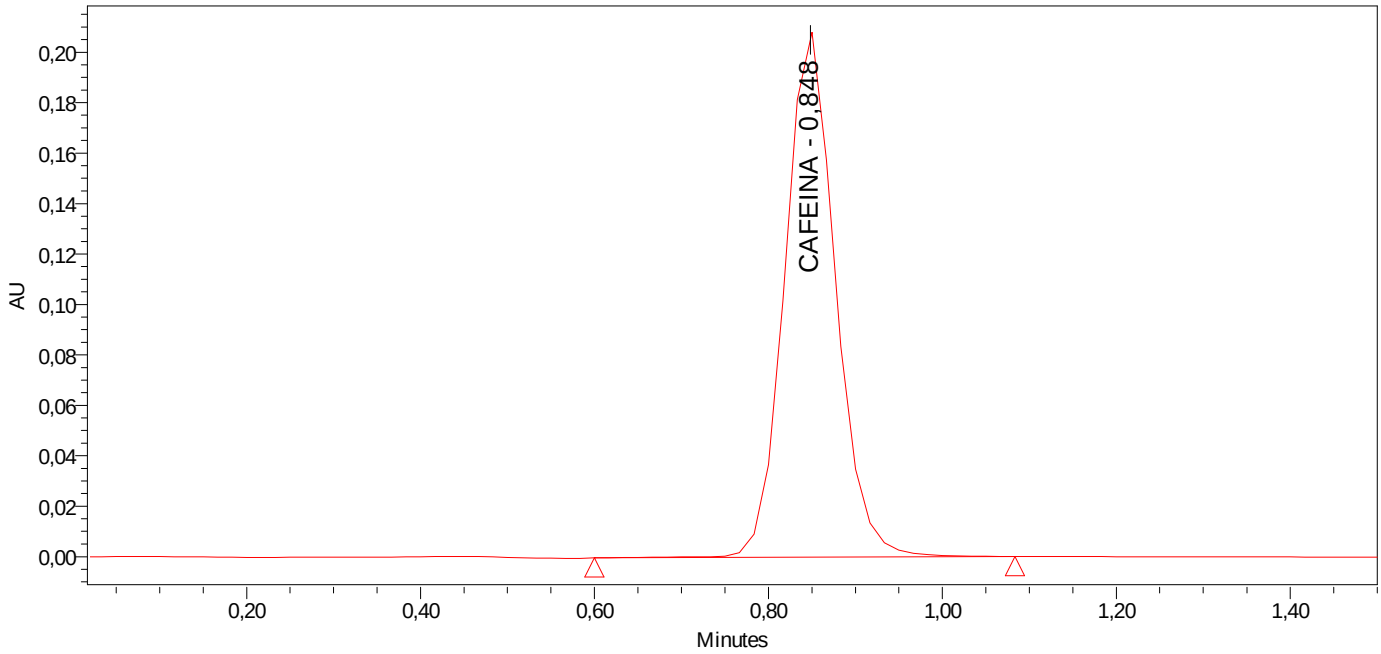


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	842117	201693		

SAMPLE INFORMATION

Sample Name:	273	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	273
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:56:20 AMT		
Date Processed:	22/07/2021 12:12:39 AMT		

Auto-Scaled Chromatogram

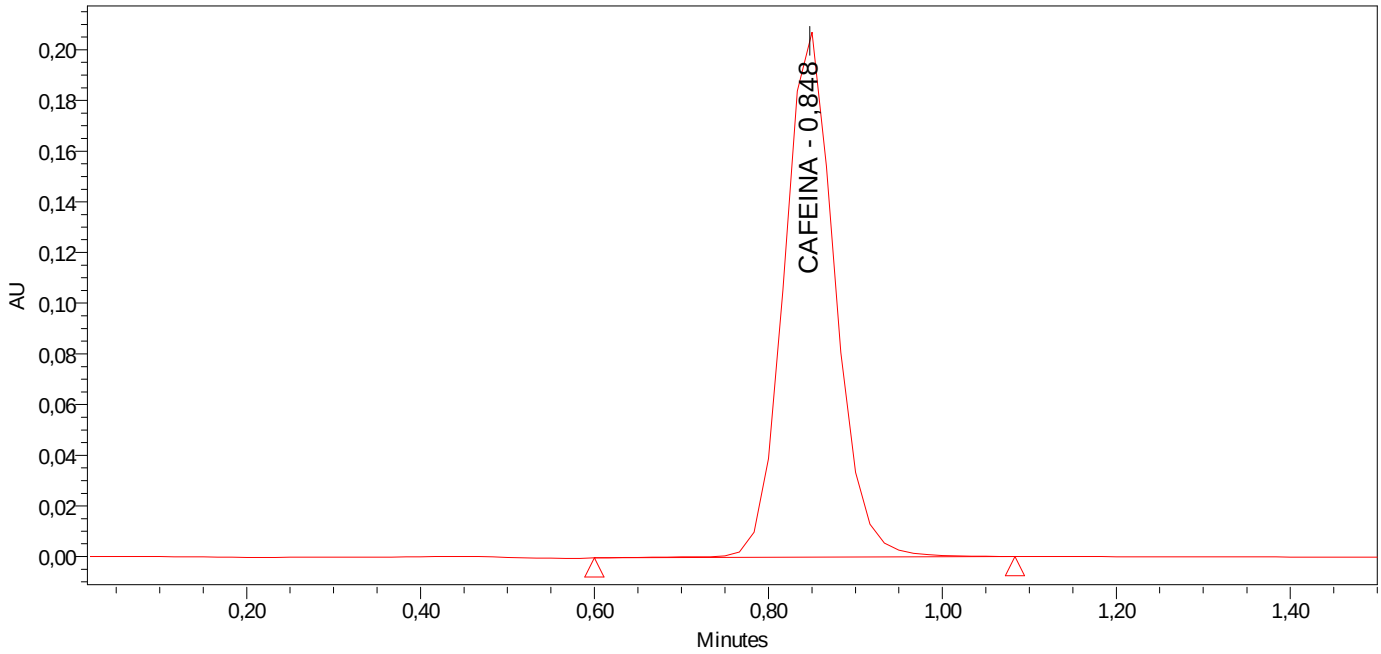


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	842514	201146		

SAMPLE INFORMATION

Sample Name:	274	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	274
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 11:58:41 AMT		
Date Processed:	22/07/2021 12:12:54 AMT		

Auto-Scaled Chromatogram

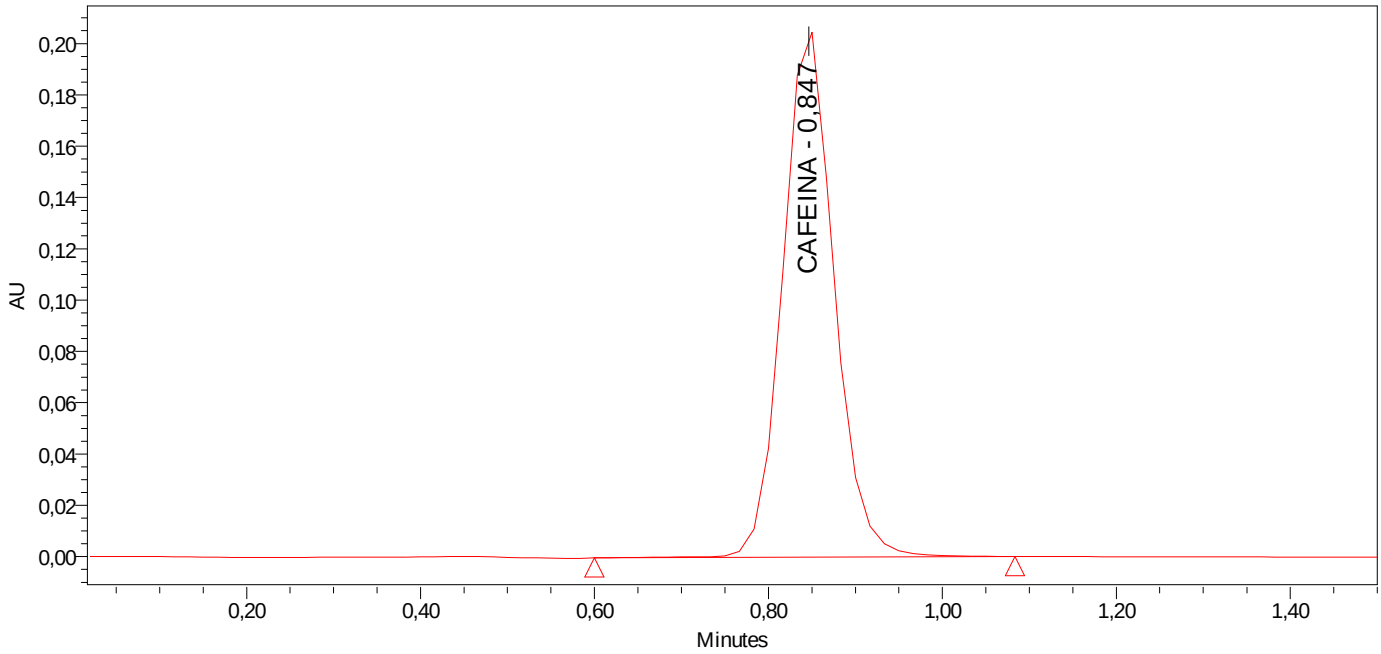


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	839519	199628		

SAMPLE INFORMATION

Sample Name:	275	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	275
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 12:01:02 AMT		
Date Processed:	22/07/2021 12:12:55 AMT		

Auto-Scaled Chromatogram

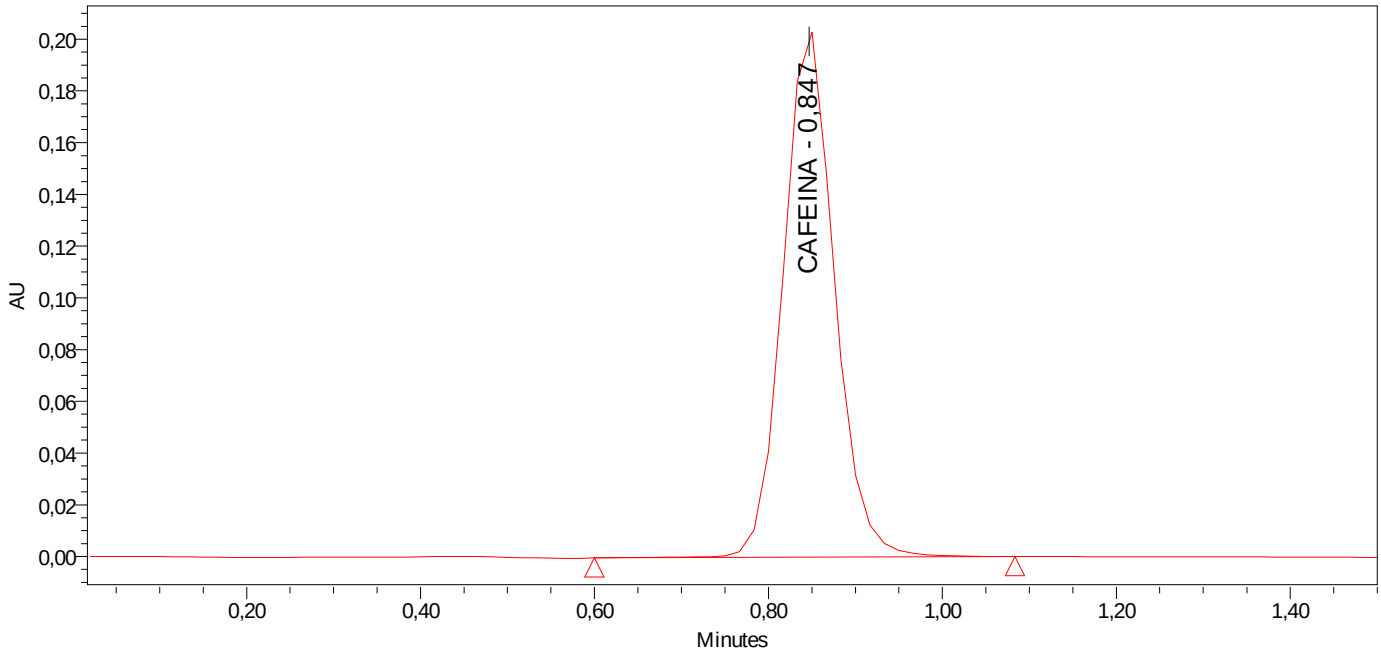


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	830850	197644		

SAMPLE INFORMATION

Sample Name:	276	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	276
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 12:03:23 AMT		
Date Processed:	22/07/2021 12:12:55 AMT		

Auto-Scaled Chromatogram

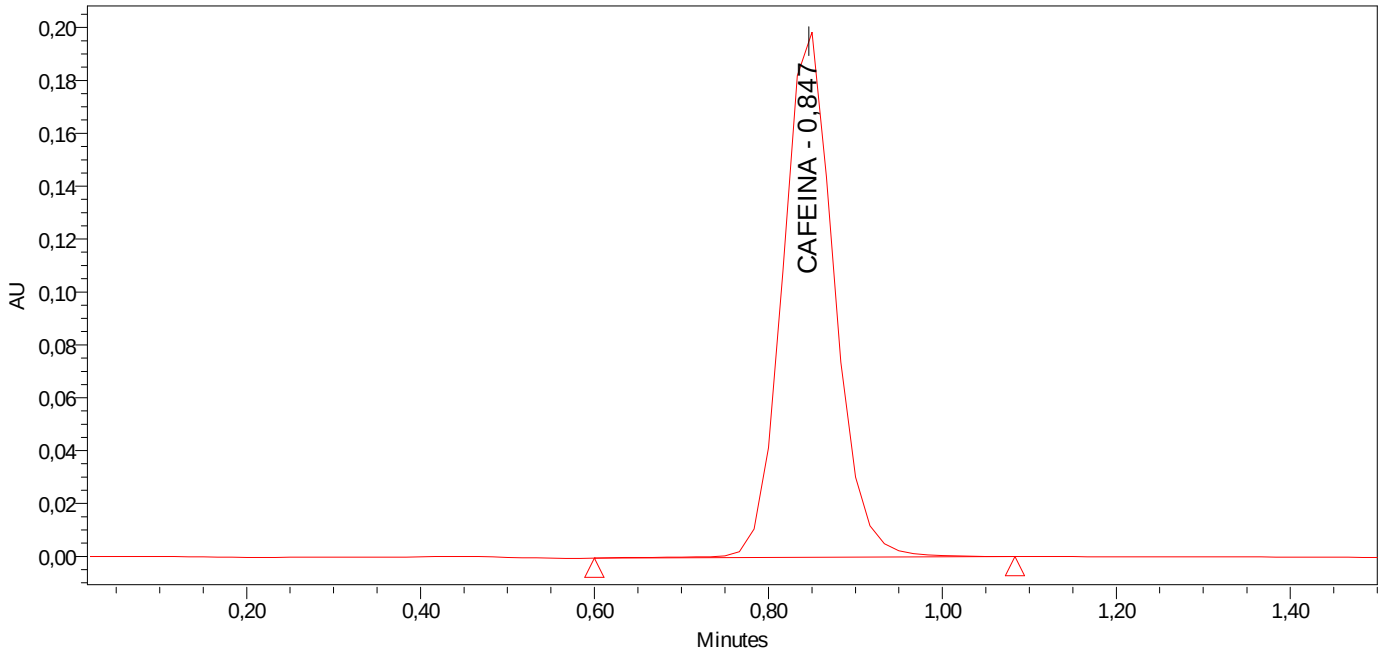


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	815232	193654		

SAMPLE INFORMATION

Sample Name:	277	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	277
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 12:05:44 AMT		
Date Processed:	22/07/2021 12:12:56 AMT		

Auto-Scaled Chromatogram

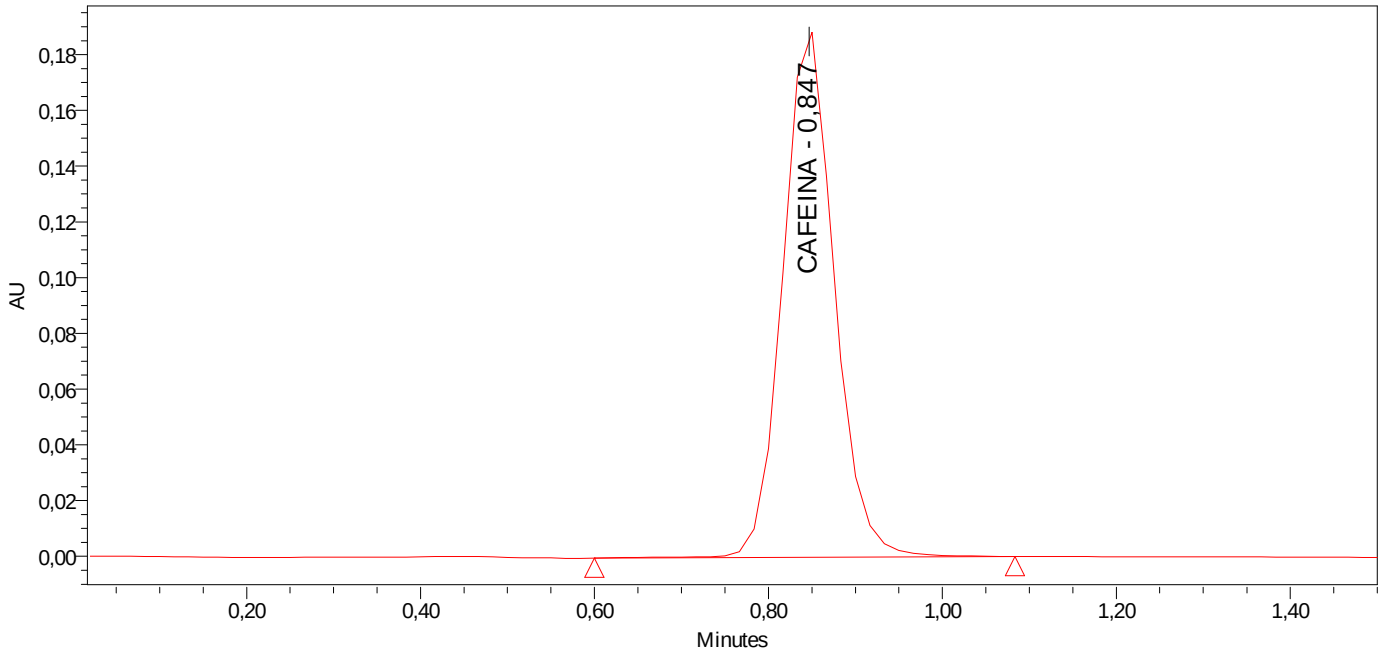


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,847	773232	183637		

SAMPLE INFORMATION

Sample Name:	278	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	9	Acq. Method Set:	278
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 12:08:05 AMT		
Date Processed:	22/07/2021 12:12:56 AMT		

Auto-Scaled Chromatogram

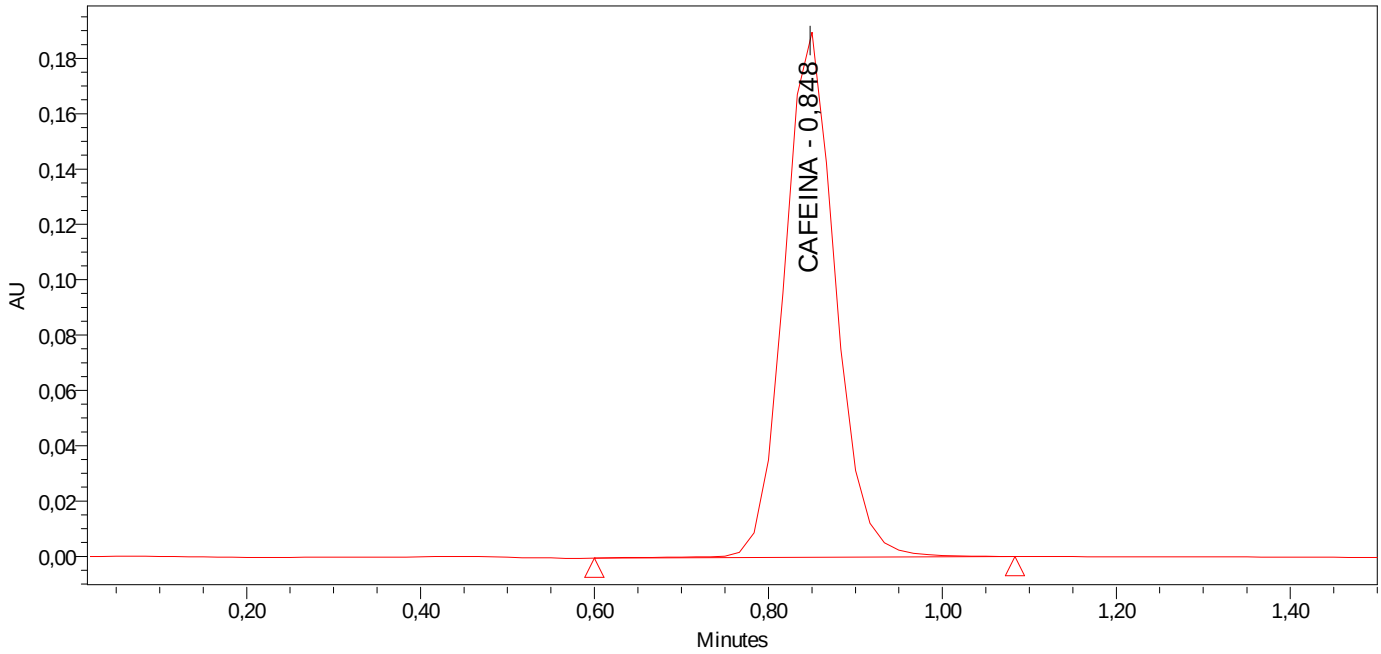


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,848	772751	184183		

SAMPLE INFORMATION

Sample Name:	BRANCO 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:08:12 AMT		
Date Processed:	22/07/2021 10:31:58 AMT		

Auto-Scaled Chromatogram

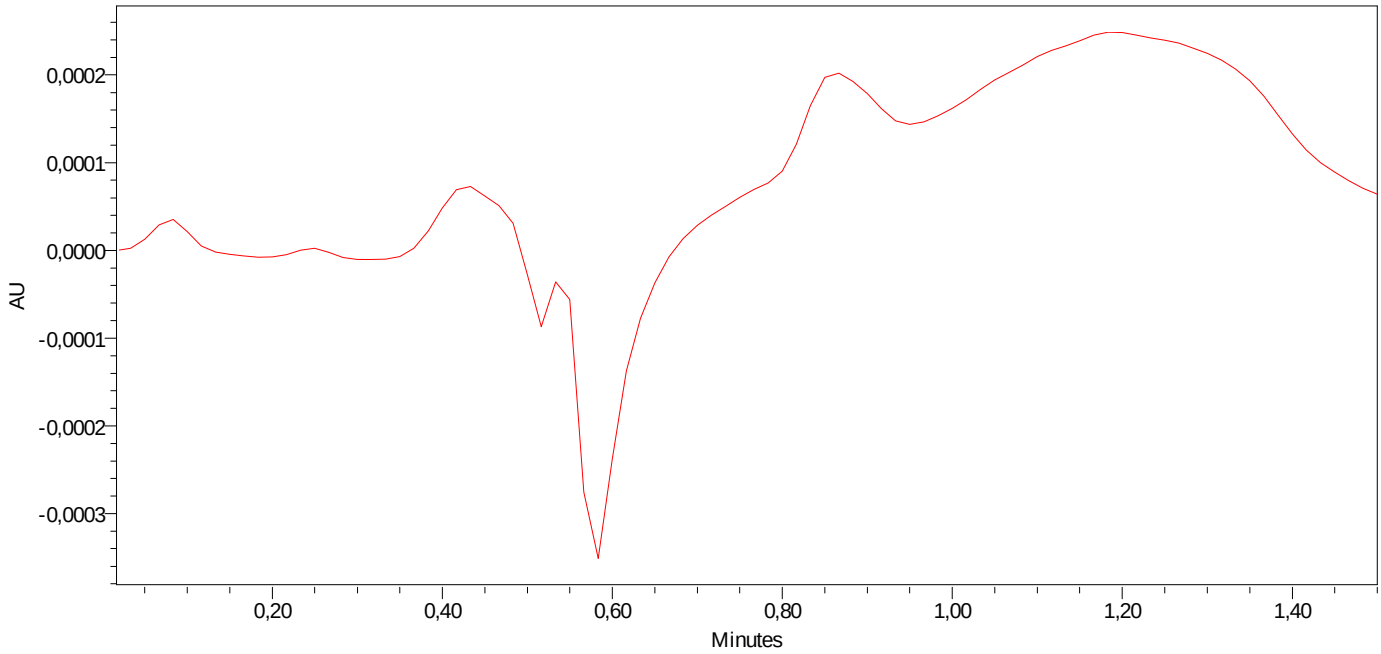


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	PCIN 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:10:33 AMT		
Date Processed:	22/07/2021 10:32:12 AMT		

Auto-Scaled Chromatogram

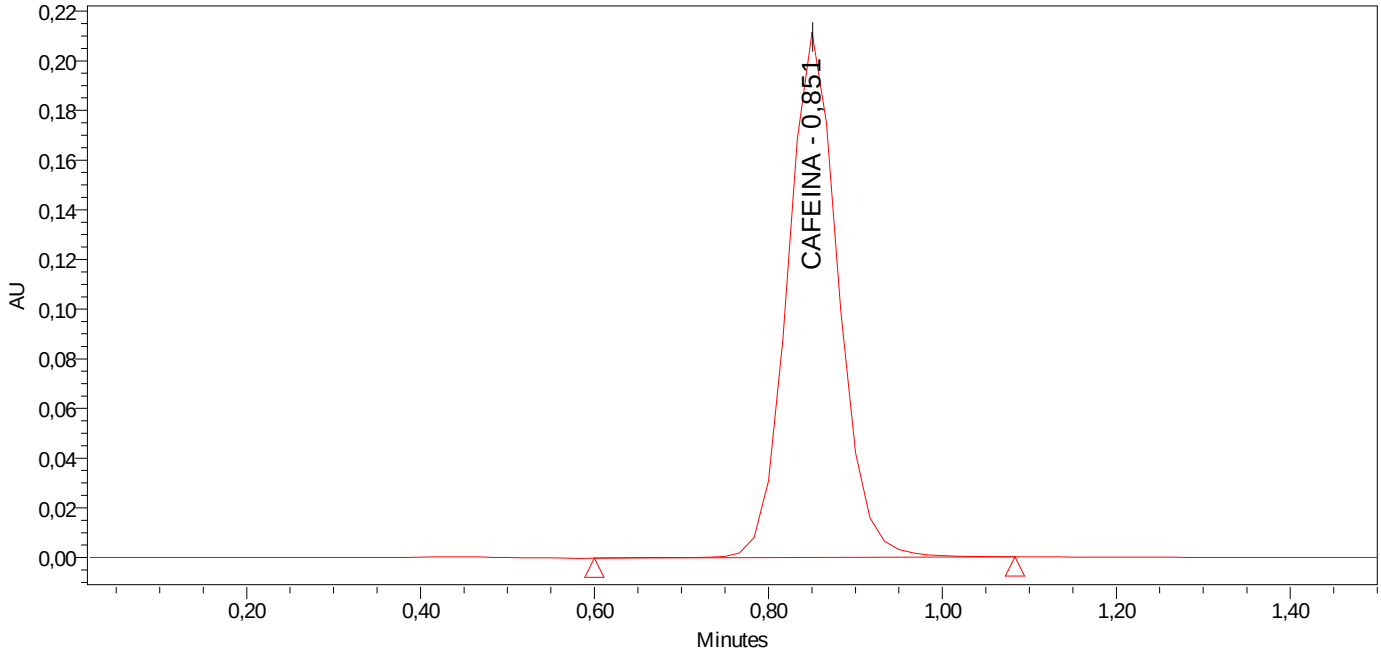


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	855937	204477		

SAMPLE INFORMATION

Sample Name:	PCIN 2	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:12:54 AMT		
Date Processed:	22/07/2021 10:32:20 AMT		

Auto-Scaled Chromatogram

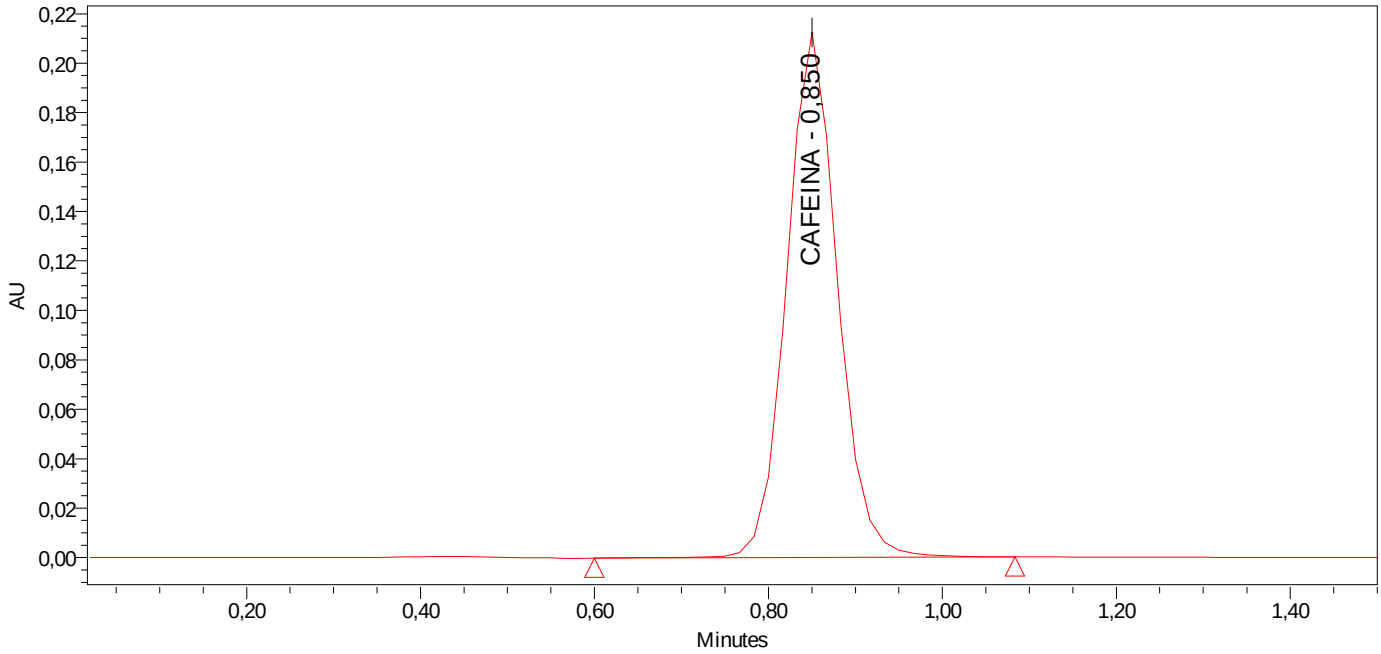


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,850	856253	205291		

SAMPLE INFORMATION

Sample Name:	PCIN 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:15:15 AMT		
Date Processed:	22/07/2021 10:32:21 AMT		

Auto-Scaled Chromatogram

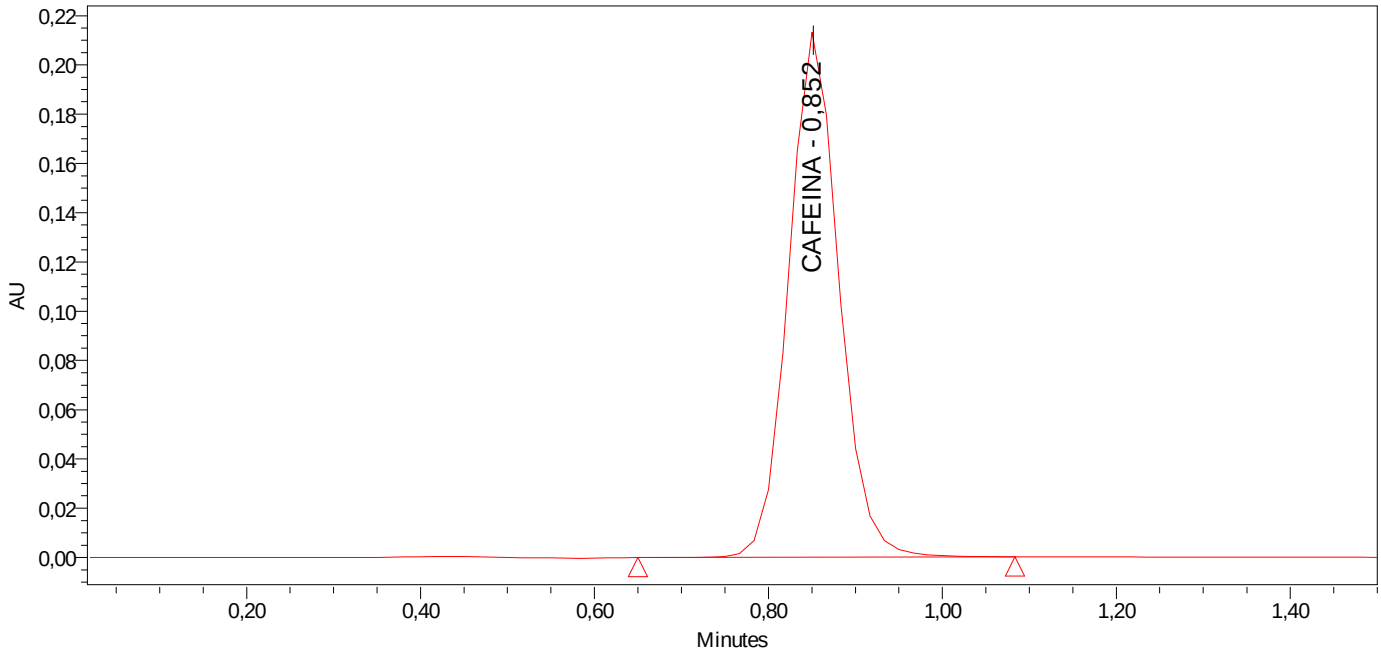


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	854328	206044		

SAMPLE INFORMATION

Sample Name:	BRANCO	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:17:38 AMT		
Date Processed:	22/07/2021 10:32:22 AMT		

Auto-Scaled Chromatogram

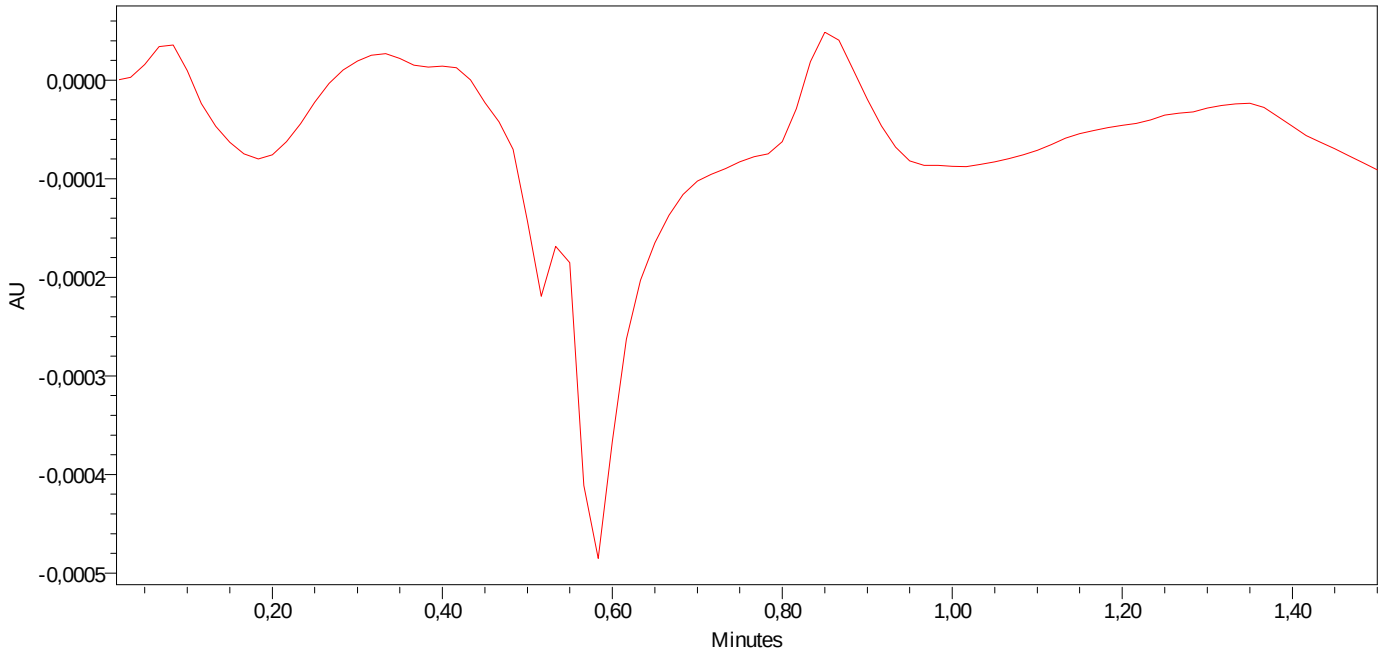


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	PCIN 4	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:19:59 AMT		
Date Processed:	22/07/2021 10:36:01 AMT		

Auto-Scaled Chromatogram

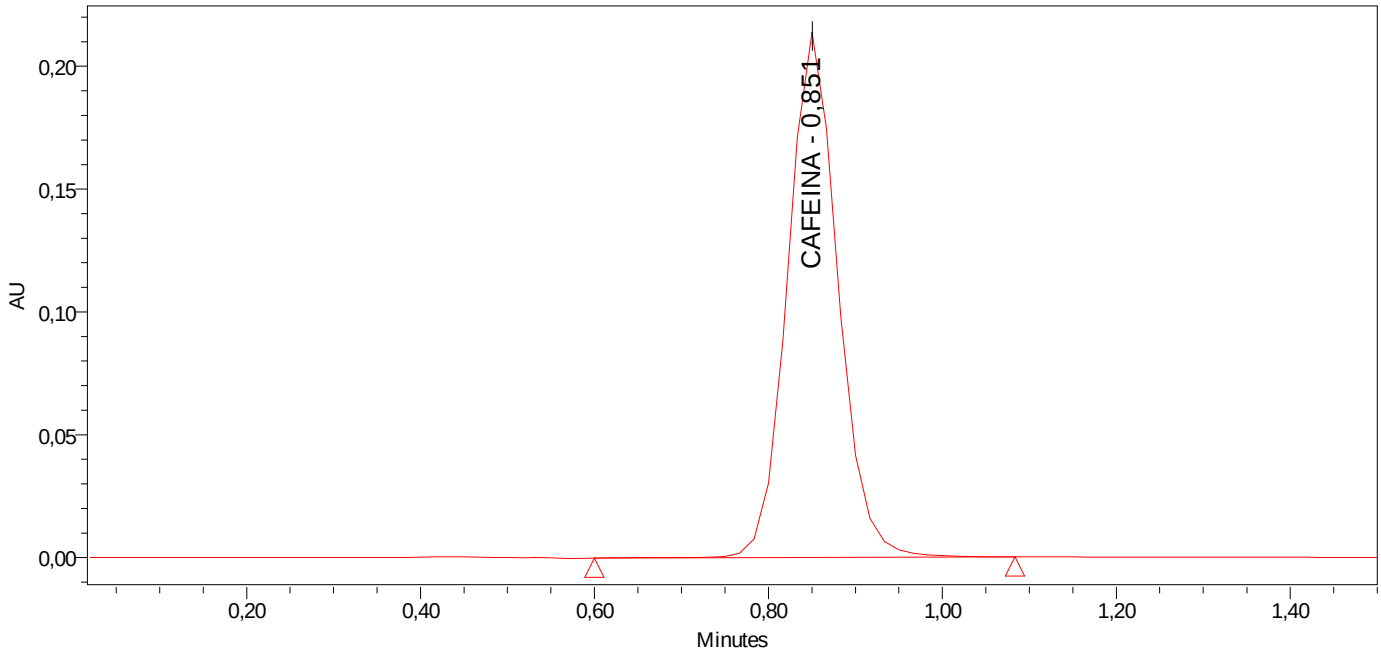


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	857643	206459		

SAMPLE INFORMATION

Sample Name:	PCIN 5	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:22:20 AMT		
Date Processed:	22/07/2021 10:36:02 AMT		

Auto-Scaled Chromatogram

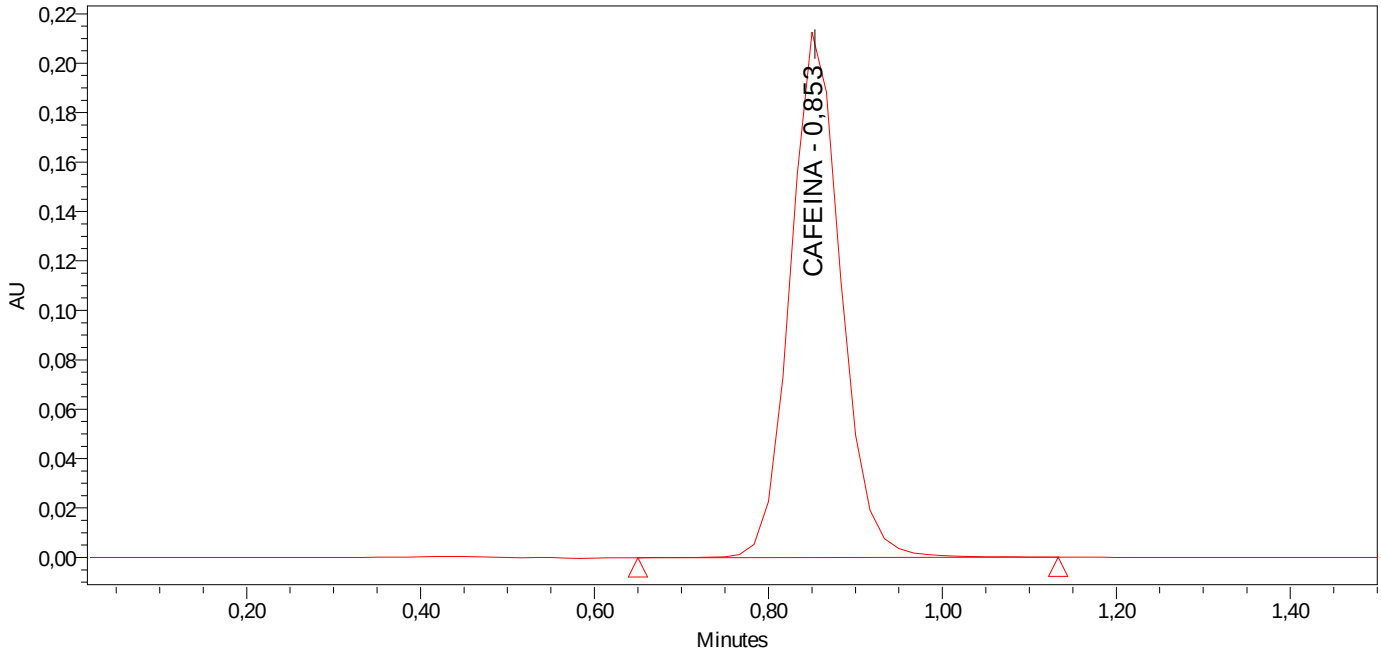


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,853	855398	206212		

SAMPLE INFORMATION

Sample Name:	PCIN 6	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	2	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:24:41 AMT		
Date Processed:	22/07/2021 10:36:02 AMT		

Auto-Scaled Chromatogram

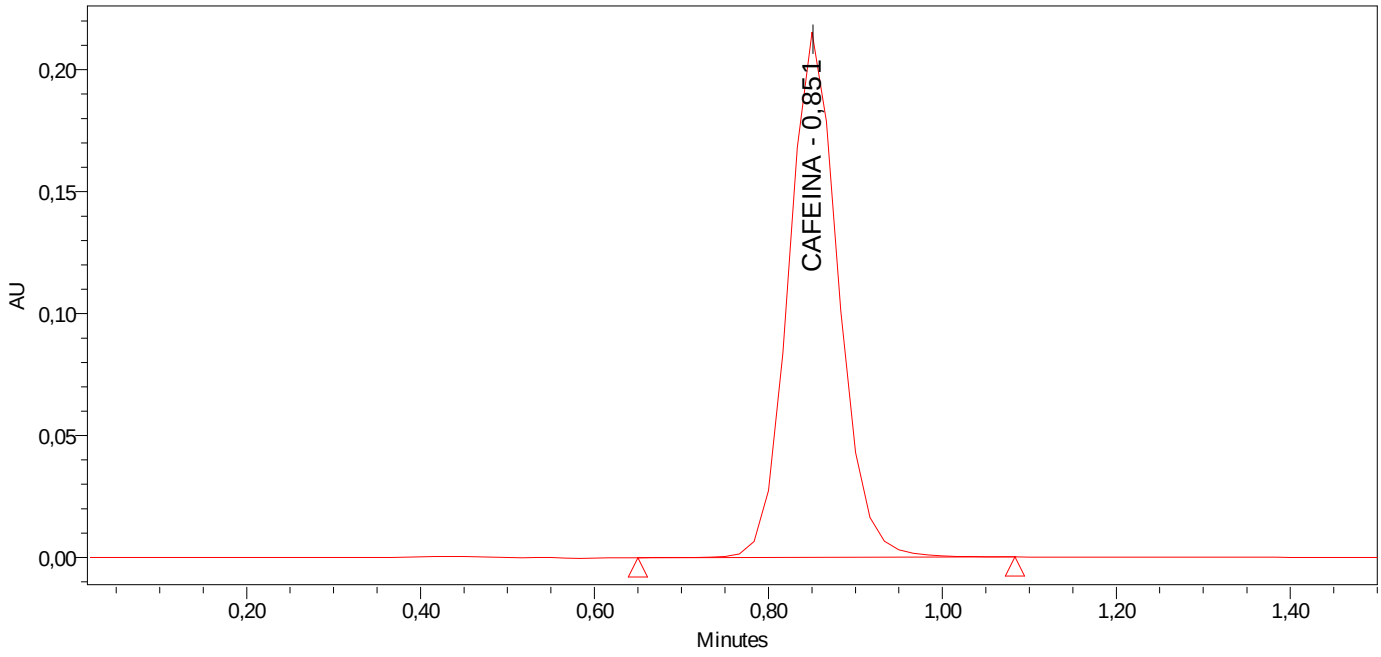


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	855448	207803		

SAMPLE INFORMATION

Sample Name:	BRANCO 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	1	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:27:04 AMT		
Date Processed:	22/07/2021 10:32:28 AMT		

Auto-Scaled Chromatogram

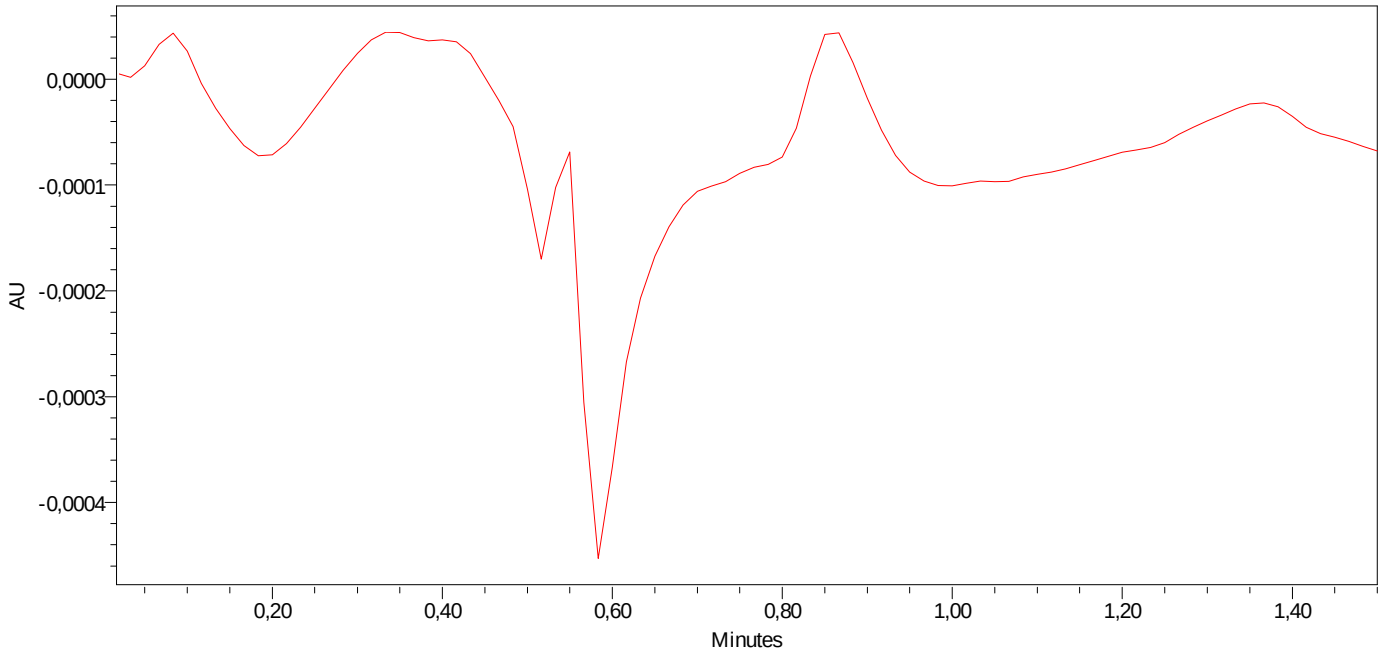


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	LDUV 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	4	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:41:08 AMT		
Date Processed:	22/07/2021 11:03:47 AMT		

Auto-Scaled Chromatogram

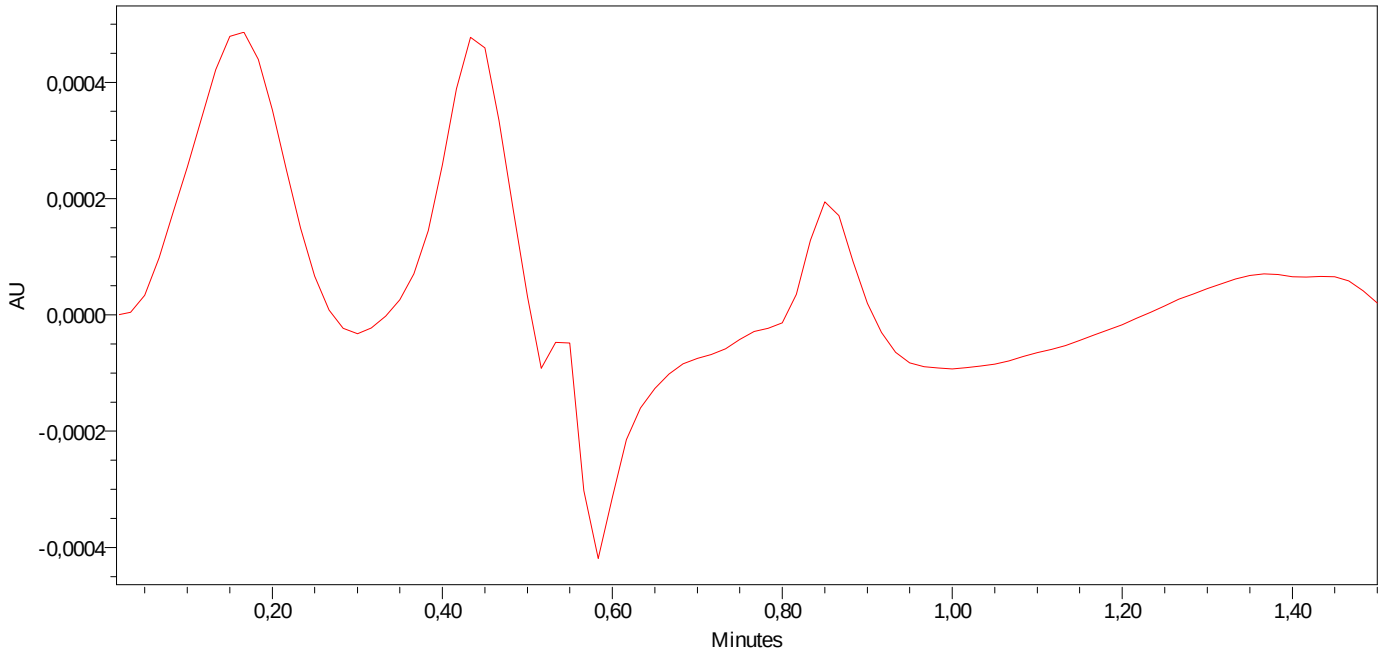


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	1,800				

SAMPLE INFORMATION

Sample Name:	LDUV 2	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	5	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:43:29 AMT		
Date Processed:	22/07/2021 11:03:50 AMT		

Auto-Scaled Chromatogram

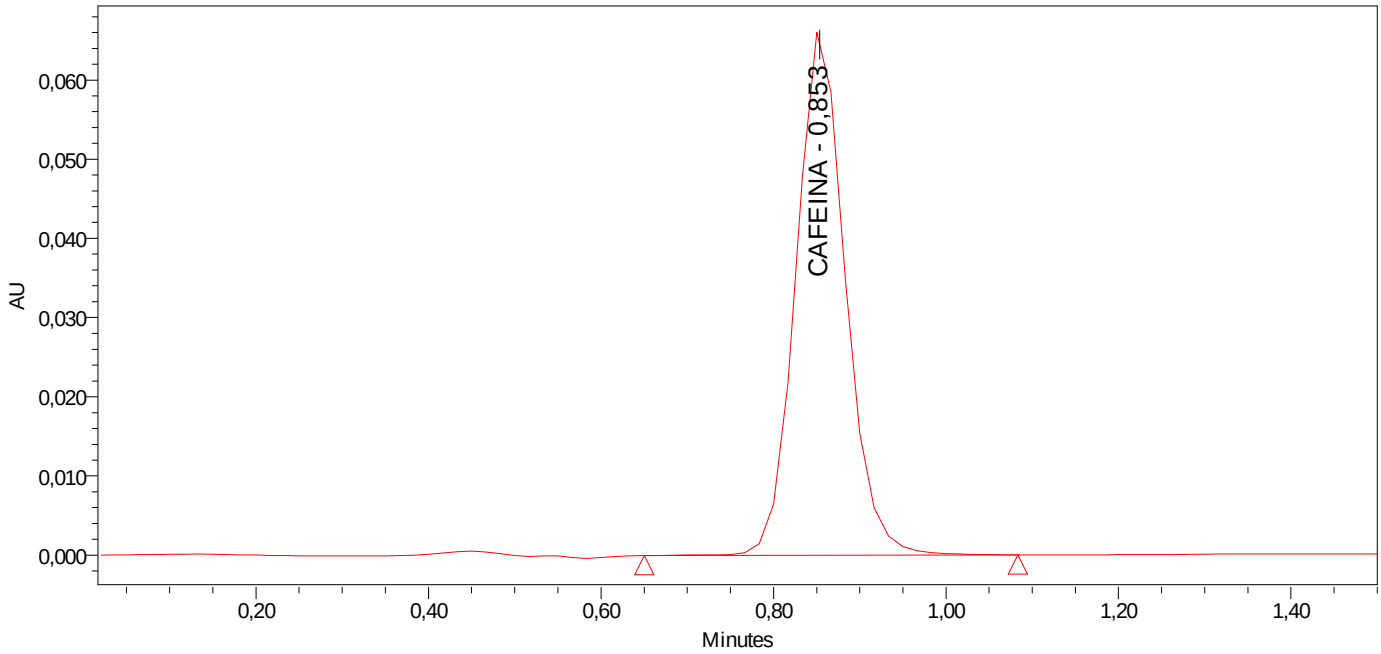


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,853	294038	64052		

SAMPLE INFORMATION

Sample Name:	LDUV 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	6	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:45:50 AMT		
Date Processed:	22/07/2021 11:03:56 AMT		

Auto-Scaled Chromatogram

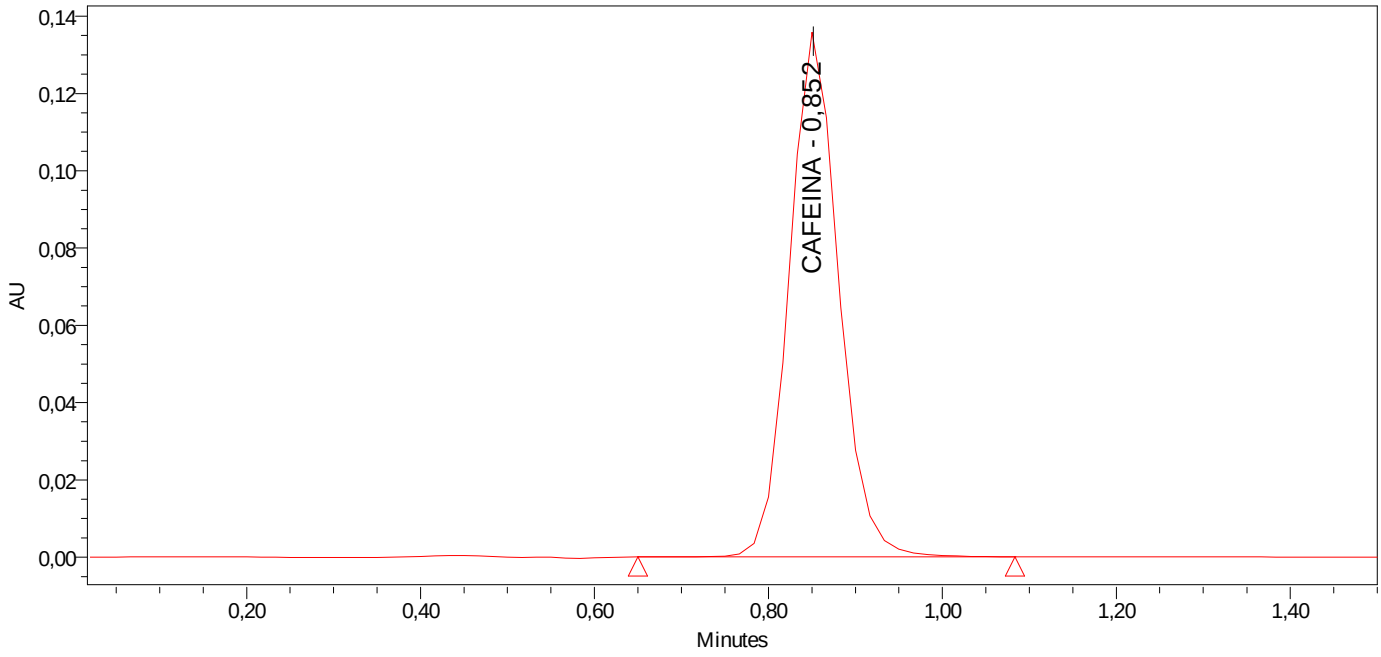


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	585410	130974		

SAMPLE INFORMATION

Sample Name:	LDUV 4	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	7	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:48:11 AMT		
Date Processed:	22/07/2021 11:03:57 AMT		

Auto-Scaled Chromatogram

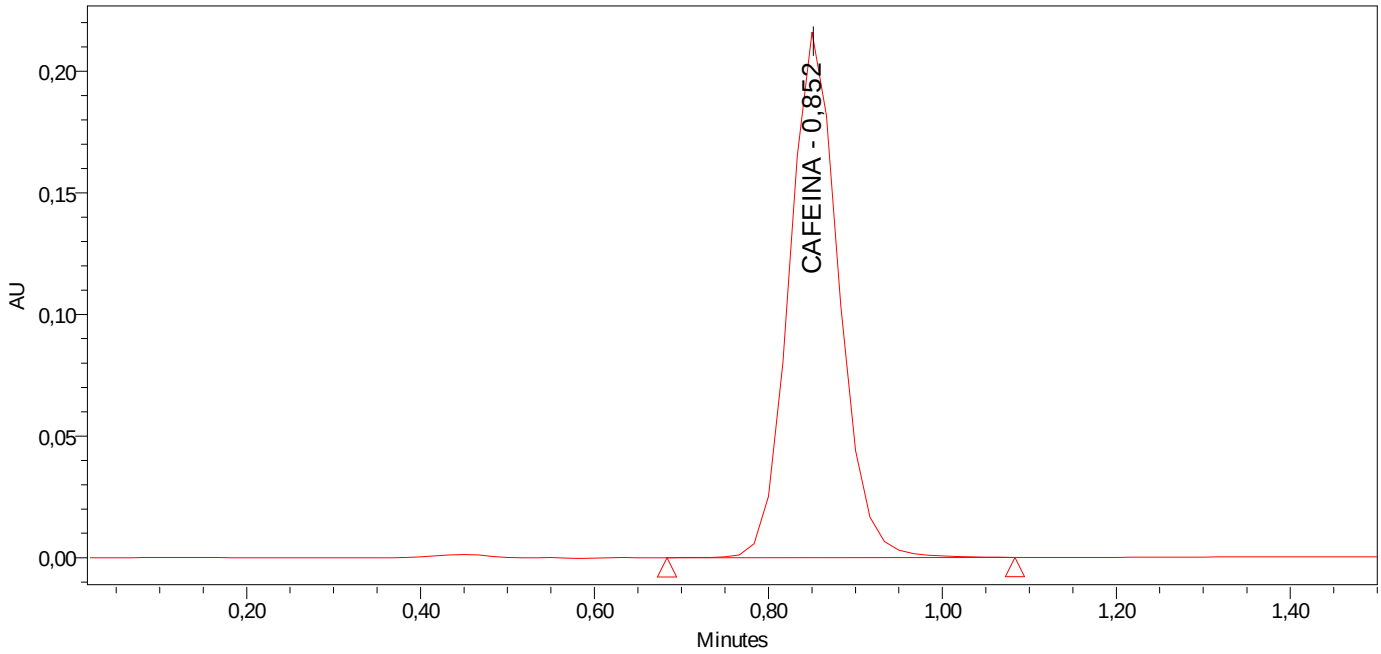


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,852	882163	208398		

SAMPLE INFORMATION

Sample Name:	LDUV 5	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	8	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:50:32 AMT		
Date Processed:	22/07/2021 11:03:59 AMT		

Auto-Scaled Chromatogram

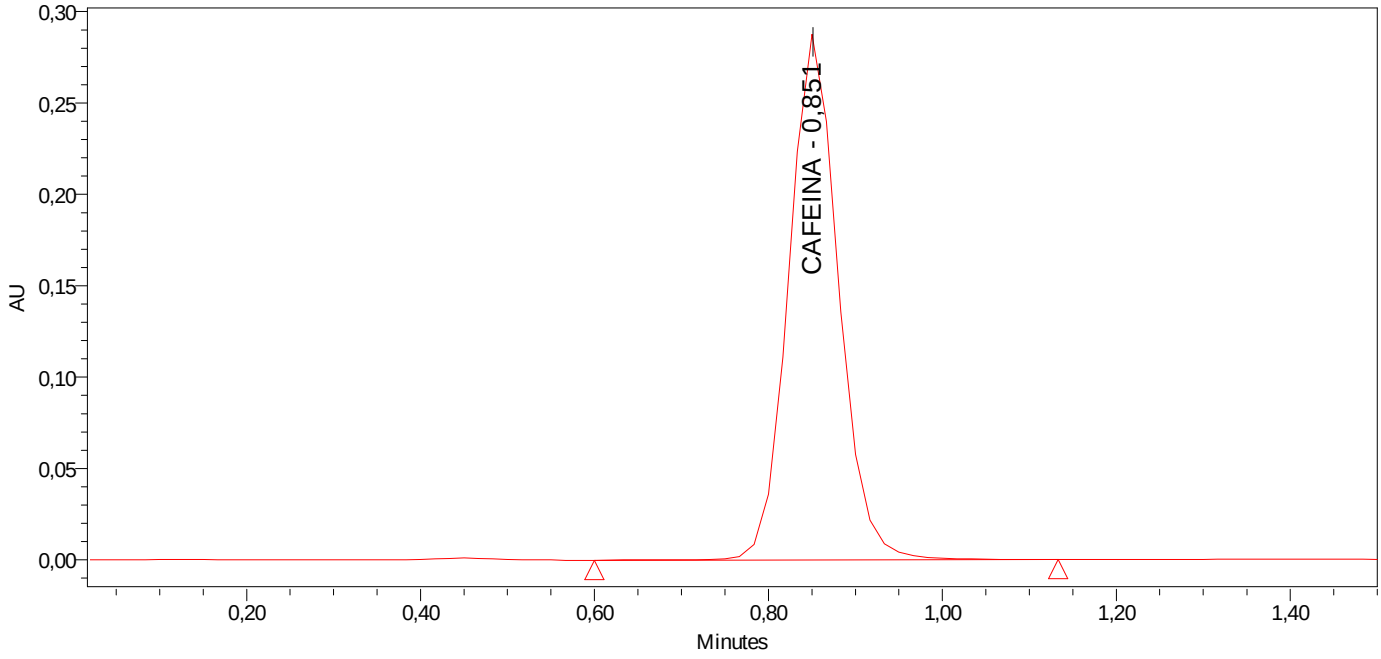


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,851	1143331	277712		

SAMPLE INFORMATION

Sample Name:	LIIN 1	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:29:19 AMT		
Date Processed:	22/07/2021 10:44:46 AMT		

Auto-Scaled Chromatogram

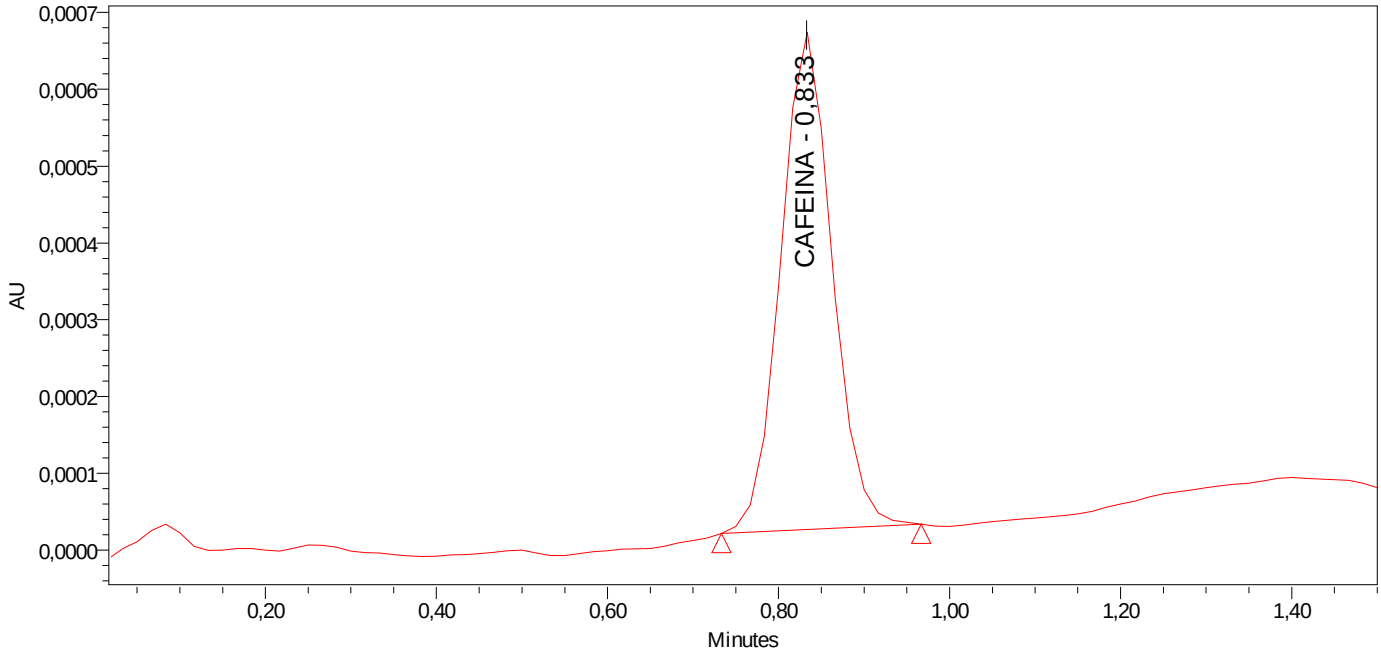


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,833	2704	629		

SAMPLE INFORMATION

Sample Name:	LIIN 2	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	5,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:31:38 AMT		
Date Processed:	22/07/2021 10:41:08 AMT		

Auto-Scaled Chromatogram

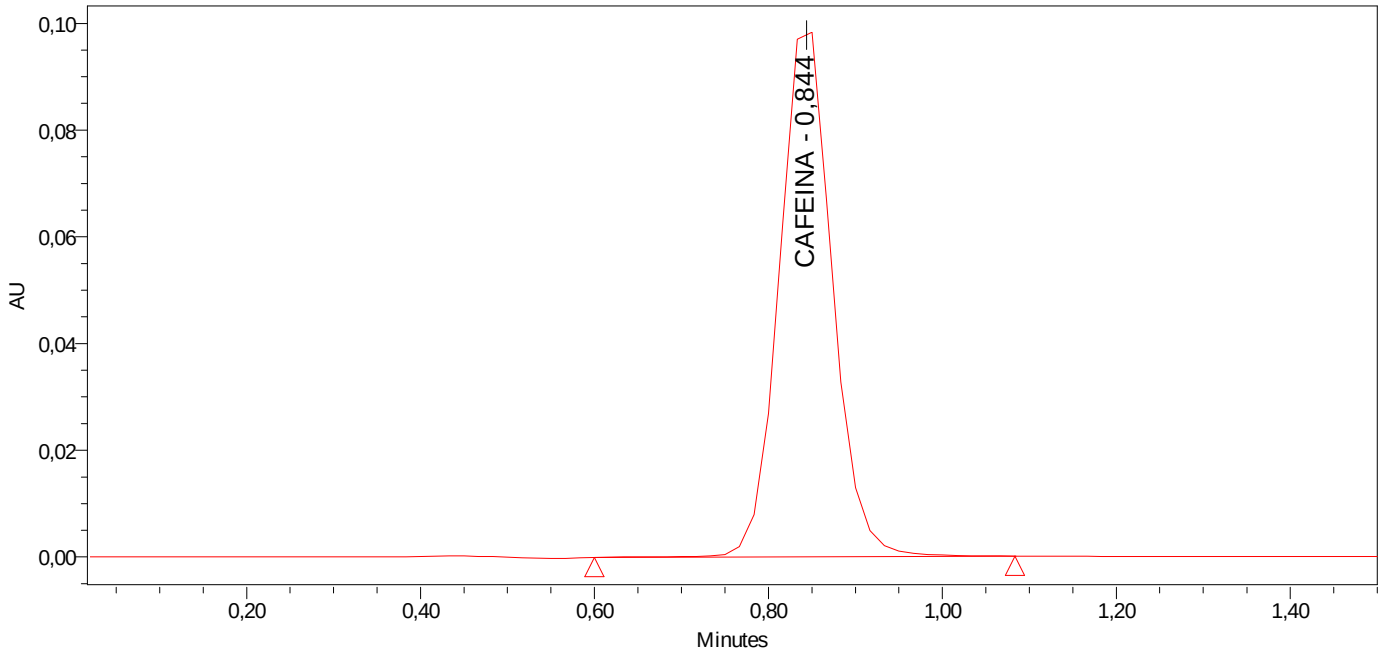


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,844	418203	97445		

SAMPLE INFORMATION

Sample Name:	LIIN 3	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	10,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:33:59 AMT		
Date Processed:	22/07/2021 10:41:15 AMT		

Auto-Scaled Chromatogram

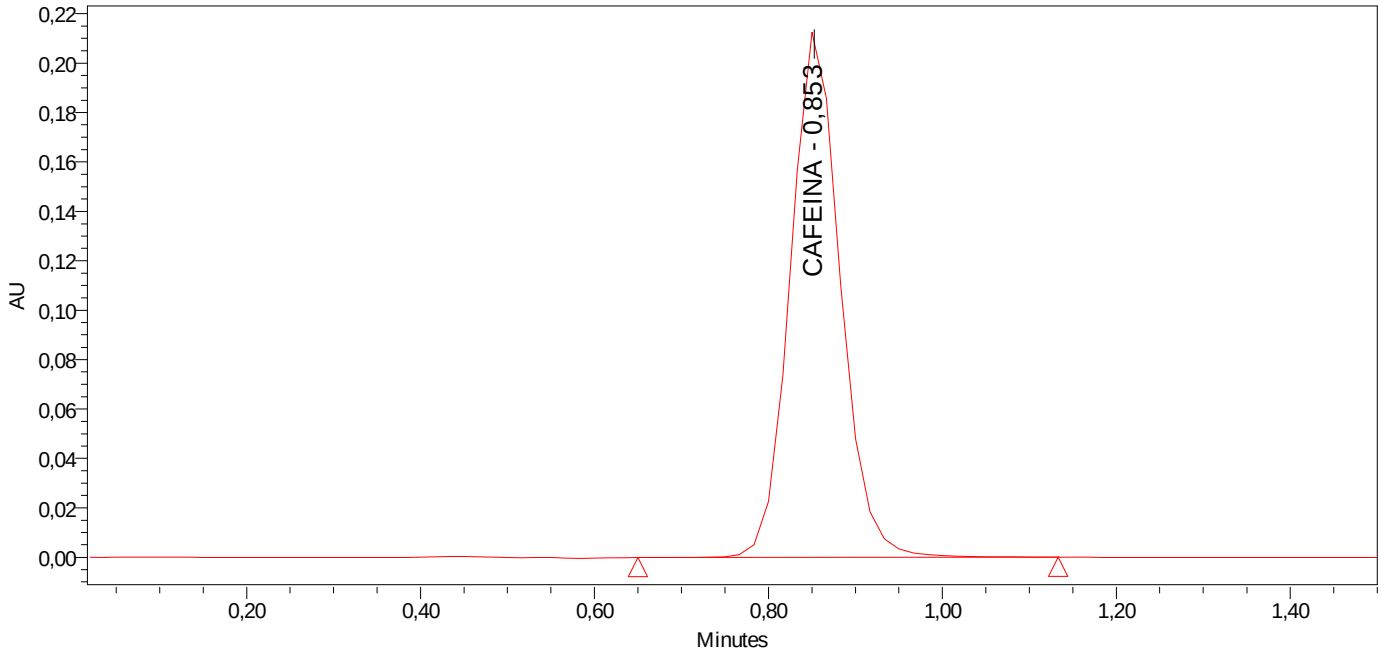


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,853	850203	205877		

SAMPLE INFORMATION

Sample Name:	LIIN 4	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	15,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:36:22 AMT		
Date Processed:	22/07/2021 10:41:17 AMT		

Auto-Scaled Chromatogram

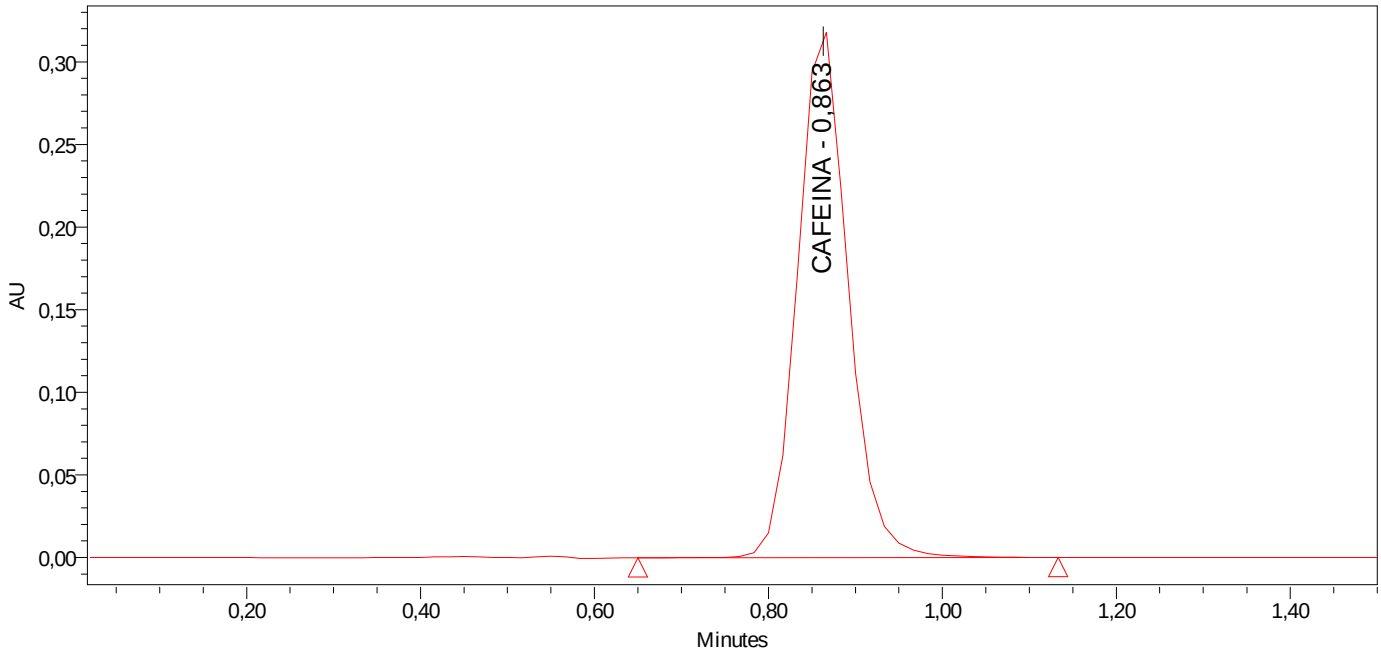


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,863	1283215	309830		

SAMPLE INFORMATION

Sample Name:	LIIN 5	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	3	Acq. Method Set:	QUALIFICAÇÃO
Injection #:	1	Processing Method	CAFEINA
Injection Volume:	20,00 ul	Channel Name:	2487Channel 1
Run Time:	1,5 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 10:38:47 AMT		
Date Processed:	22/07/2021 10:41:22 AMT		

Auto-Scaled Chromatogram

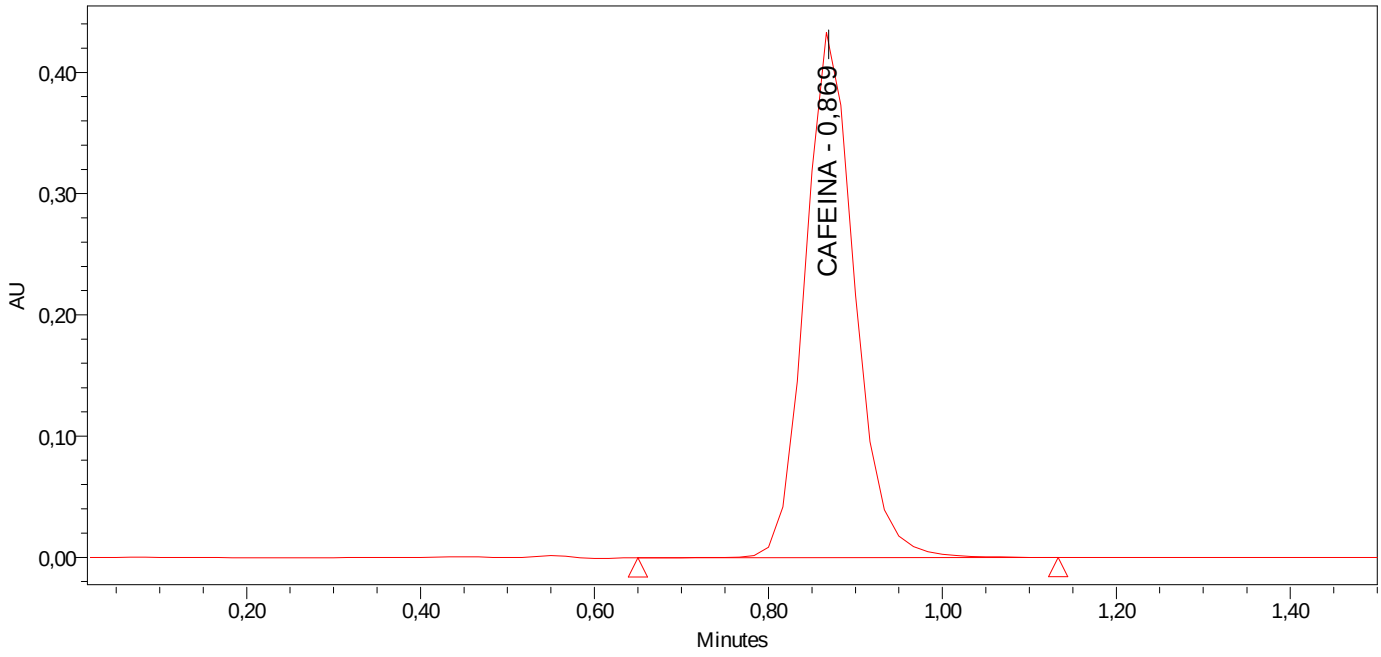


Peak Results

	Name	RT	Area	Height	Amount	Units
1	CAFEINA	0,869	1713932	418416		

SAMPLE INFORMATION

Sample Name:	GRADIENTE AB	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	1	Acq. Method Set:	GRADIENTE AB
Injection #:	3	Processing Method	GRADIENTE
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	14,0 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:04:58 AMT		
Date Processed:	22/07/2021 08:36:04 AMT		

Auto-Scaled Chromatogram

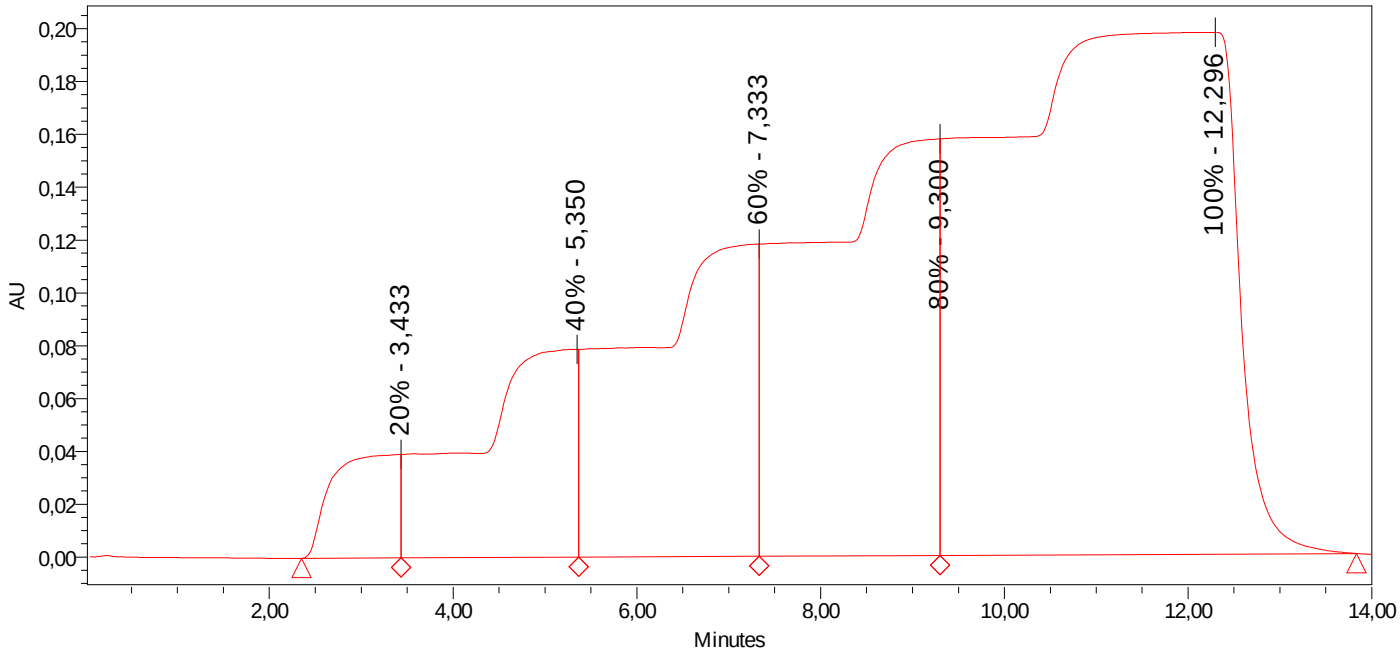


Peak Results

	Name	RT	Area	Height	Amount	Units
1	20%	3,433	1926224	39109		
2	40%	5,350	6386913	78610		
3	60%	7,333	11036452	118125		
4	80%	9,300	15665661	157672		
5	100%	12,296	36143853	197502		

SAMPLE INFORMATION

Sample Name:	GRADIENTE CD	Acquired By:	System
Sample Type:	Unknown	Sample Set Name	QUALIFICAÇÃO 587
Vial:	1	Acq. Method Set:	GRADIENTE CD
Injection #:	1	Processing Method	GRADIENTE
Injection Volume:	0,00 ul	Channel Name:	2487Channel 1
Run Time:	14,0 Minutes	Proc. Chnl. Descr.:	2487Channel 1
Date Acquired:	22/07/2021 08:19:50 AMT		
Date Processed:	22/07/2021 08:38:06 AMT		

Auto-Scaled Chromatogram

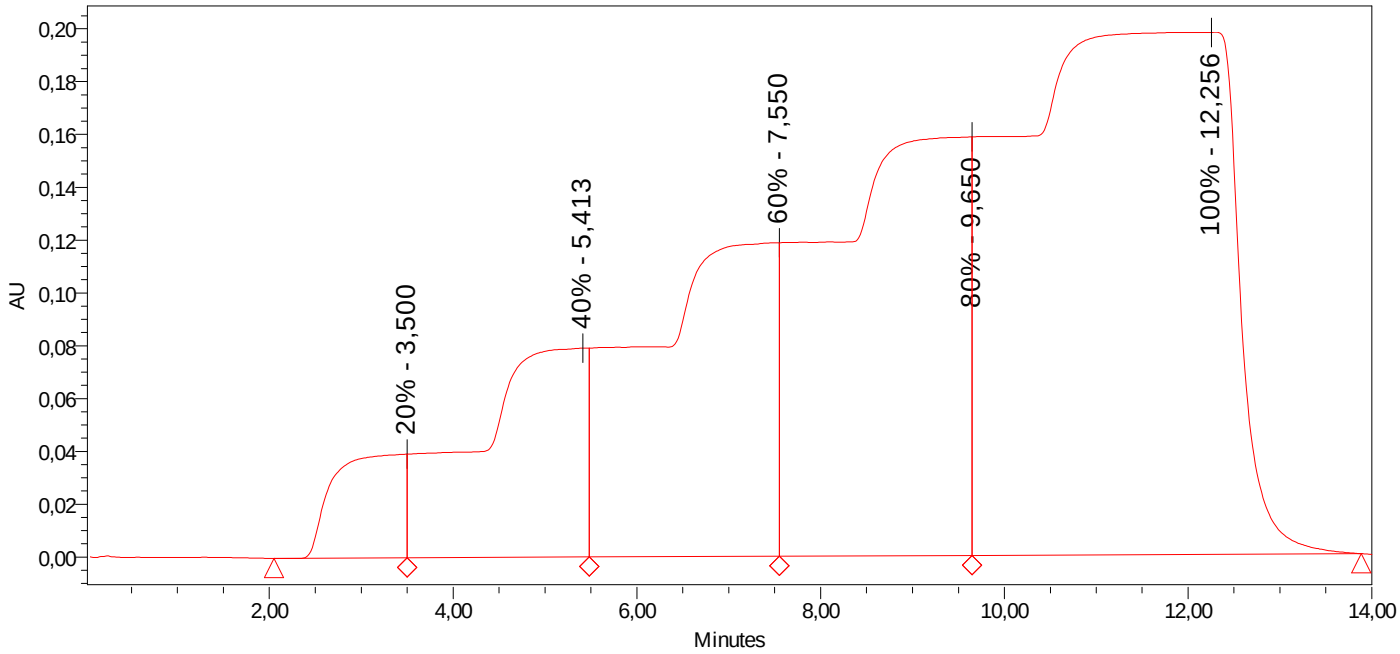

Peak Results

	Name	RT	Area	Height	Amount	Units
1	20%	3,500	2063256	39226		
2	40%	5,413	6825674	79113		
3	60%	7,550	12055782	118667		
4	80%	9,650	17460972	158455		
5	100%	12,256	32904917	197642		