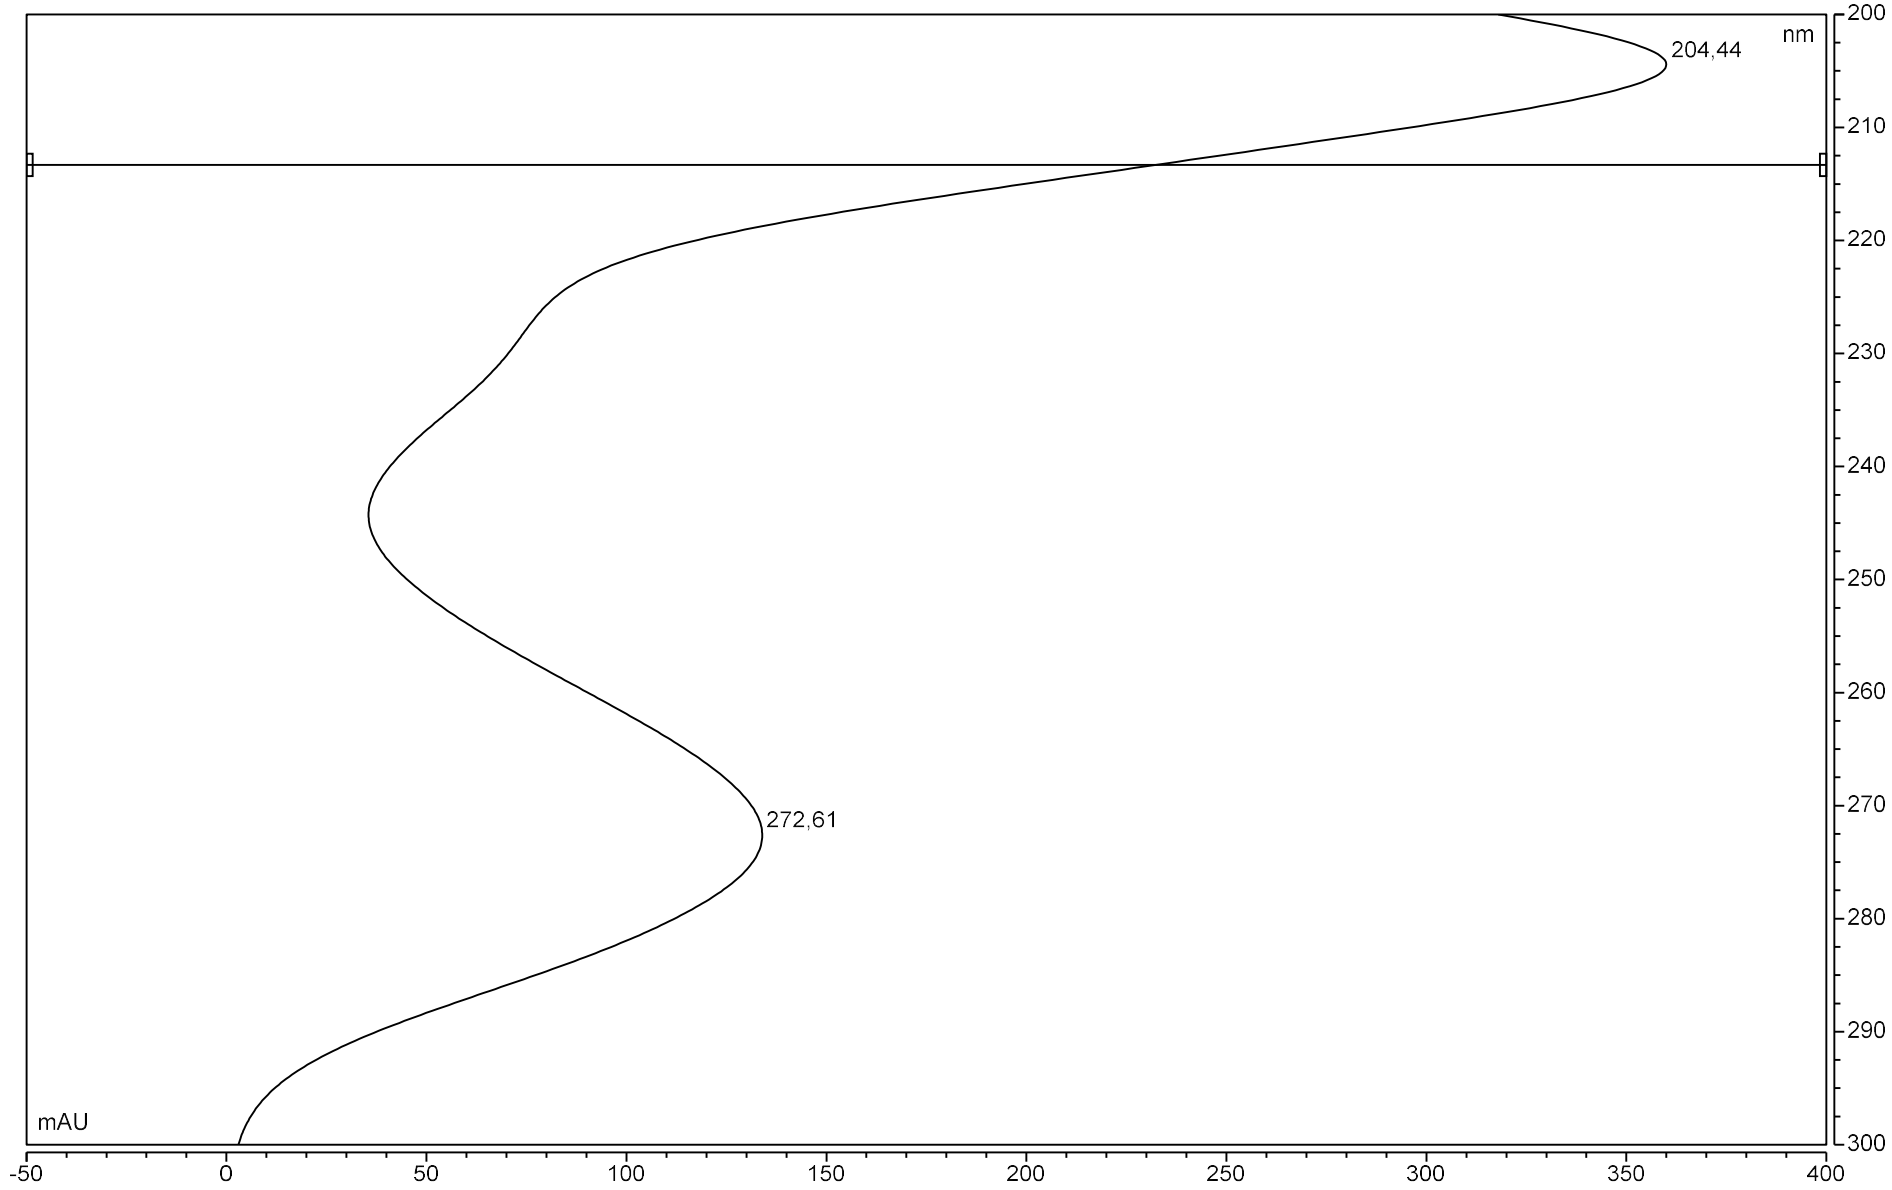
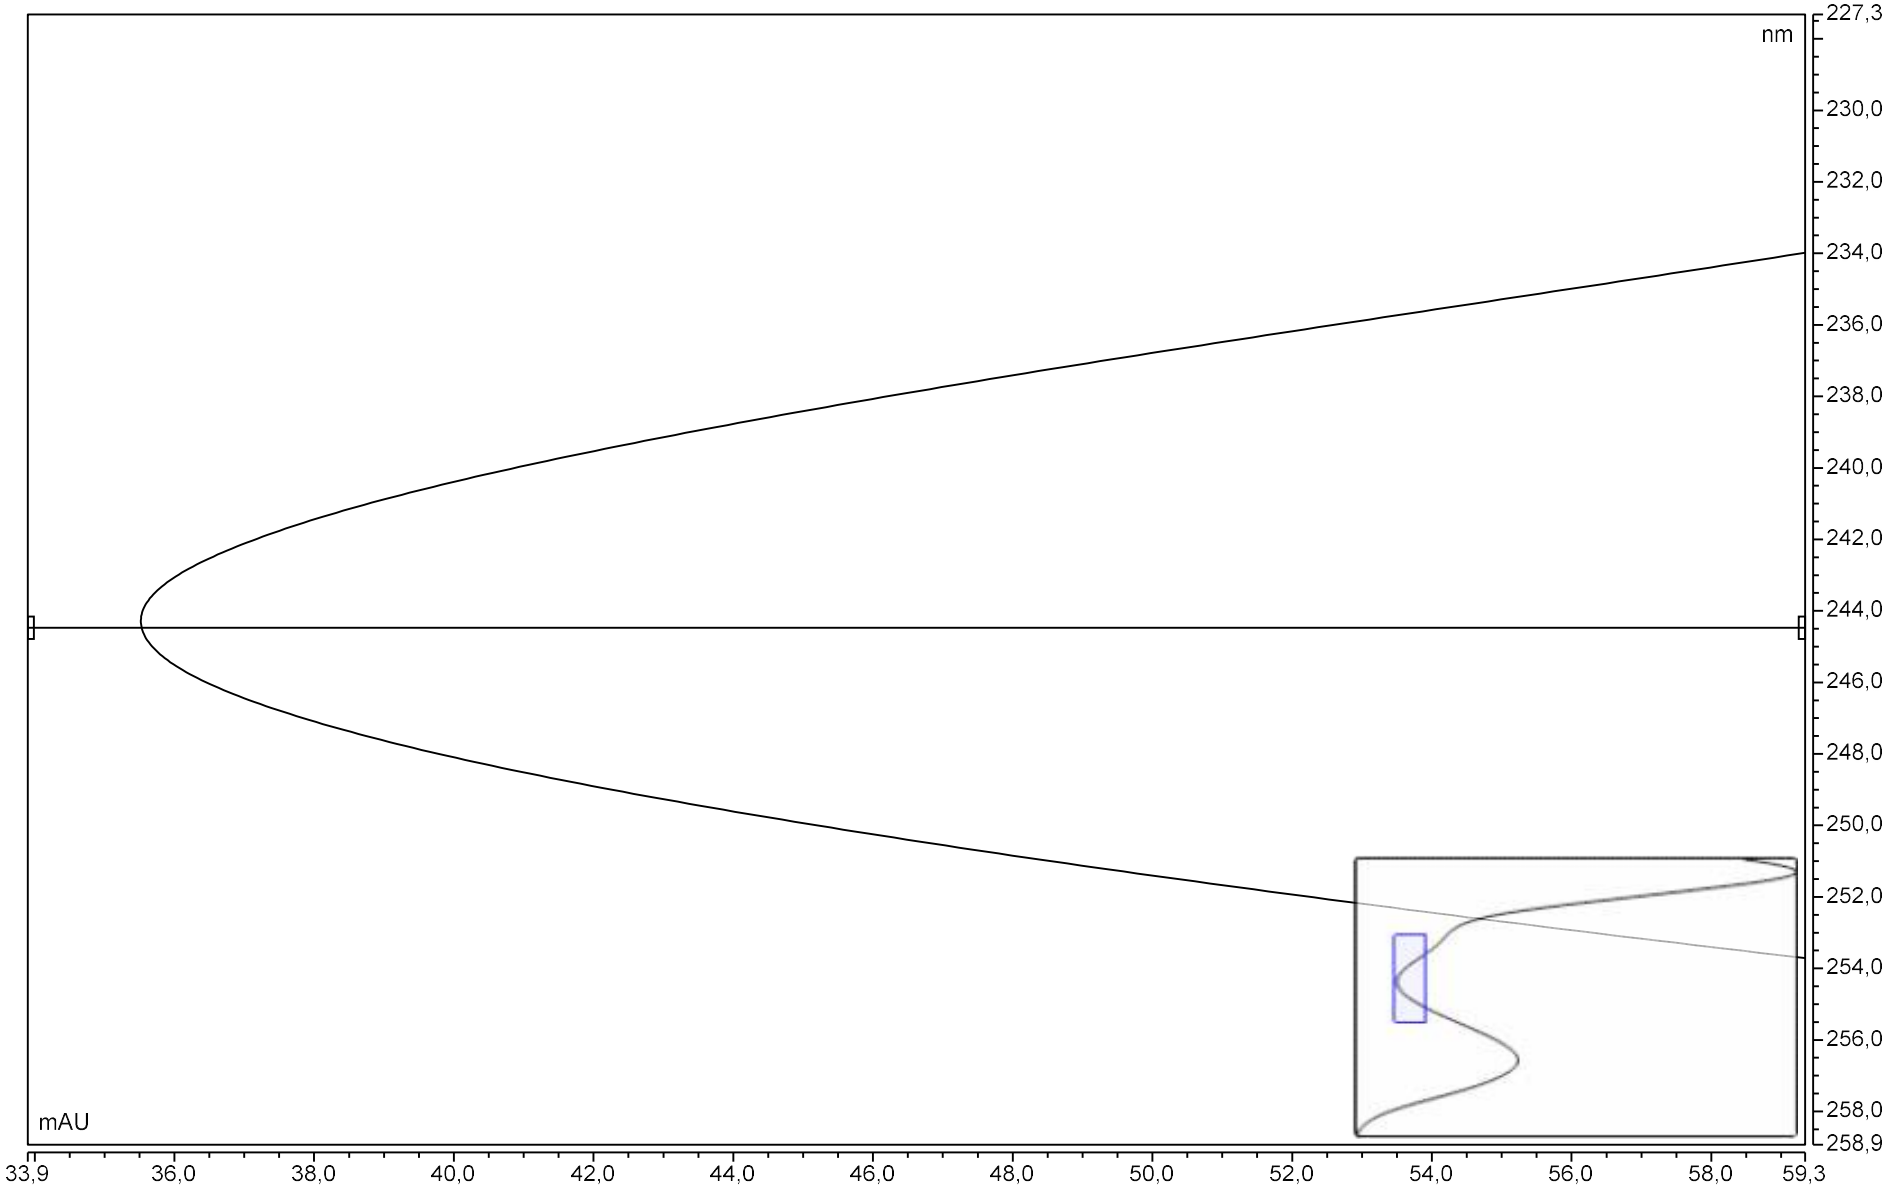

nm
204,44
272,61
mAU
200
210
220
230
240
250
260
270
280
290
300
-50
0
50
100
150
200
250
300
350
400



nm
227,3
230,0
232,0
234,0
236,0
238,0
240,0
242,0
244,0
246,0
248,0
250,0
252,0
254,0
256,0
258,0
258,9
mAU
33,9
36,0
38,0
40,0
42,0
44,0
46,0
48,0
50,0
52,0
54,0
56,0
58,0
59,3

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**B:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 12:06**	*Sample Weight:*	**1,0000**

Chromatogram

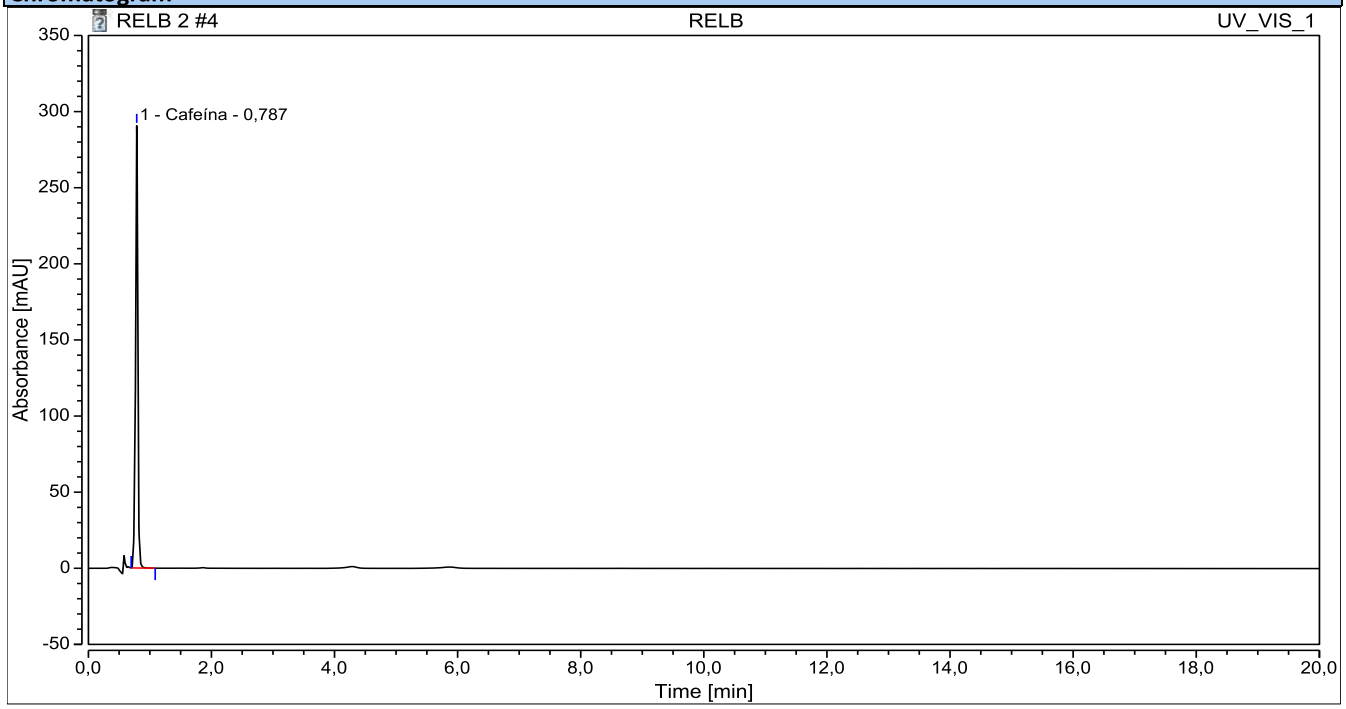

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,787	12,0128	290,490	100,00	100,00	n.a.
Total:			**12,013**	**290,490**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**B:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 12:06**	*Sample Weight:*	**1,0000**

Chromatogram

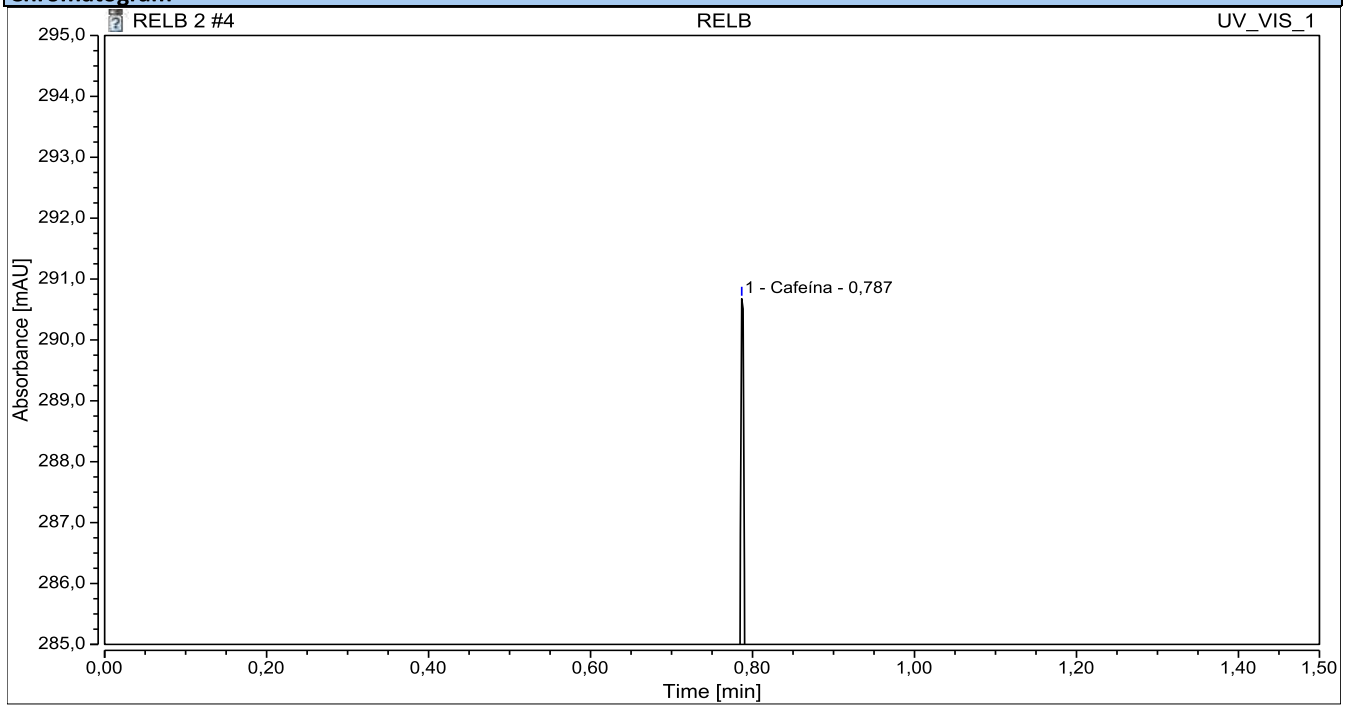

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,787	12,0128	290,490	100,00	100,00	n.a.
Total:			**12,013**	**290,490**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**B:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 12:06**	*Sample Weight:*	**1,0000**

Chromatogram

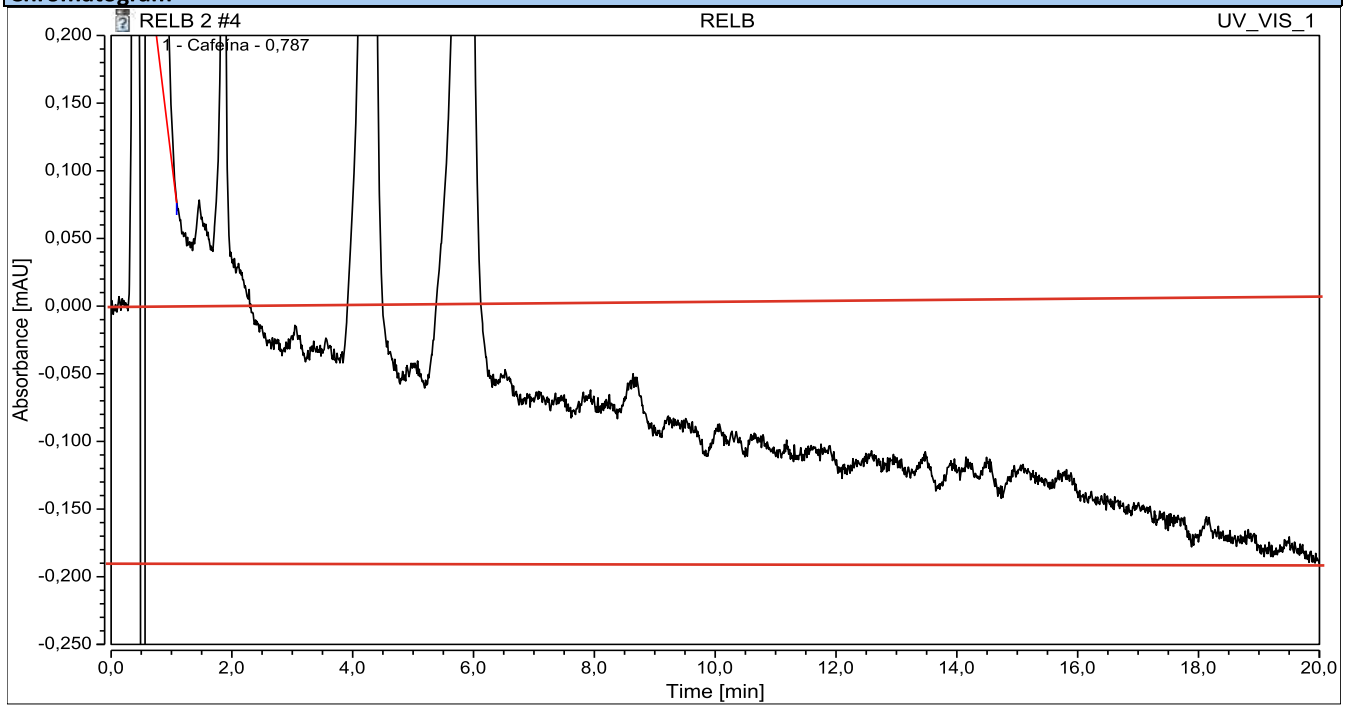

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,787	12,0128	290,490	100,00	100,00	n.a.
Total:			**12,013**	**290,490**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**B:B1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 12:06**	*Sample Weight:*	**1,0000**

Chromatogram

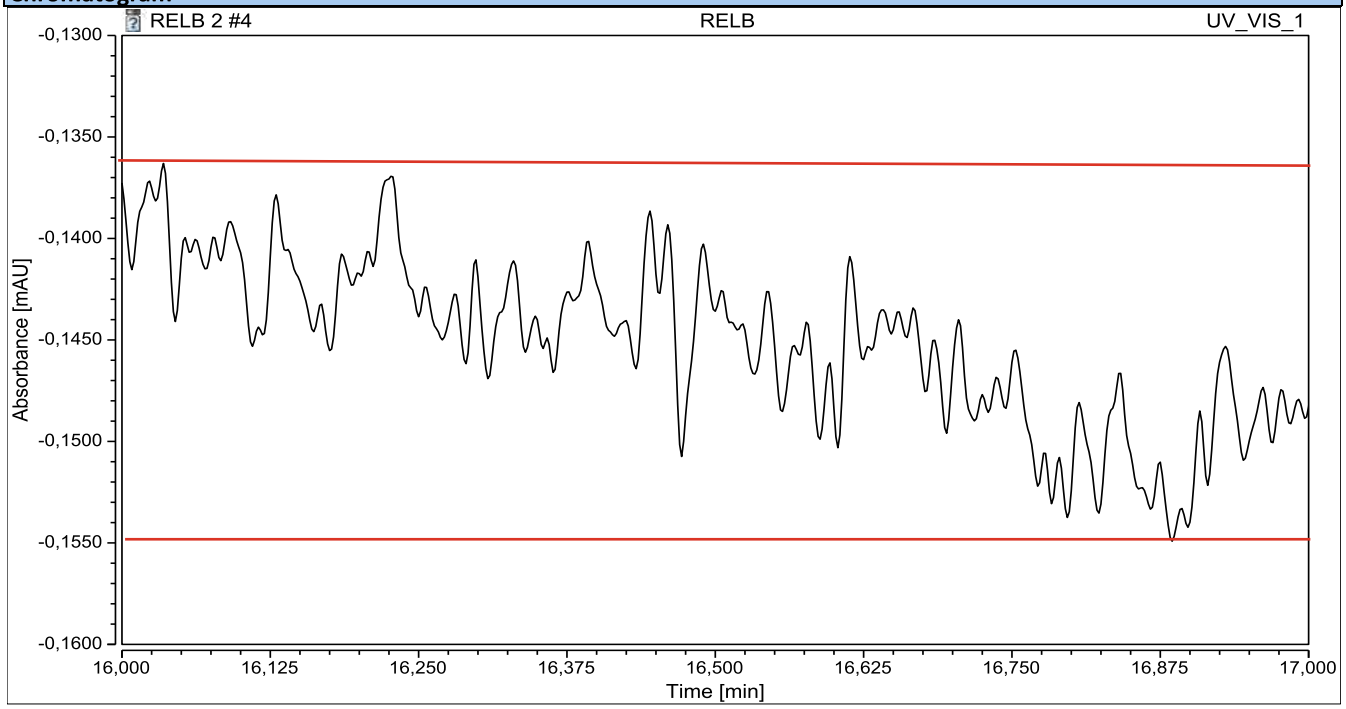

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,787	12,0128	290,490	100,00	100,00	n.a.
Total:			**12,013**	**290,490**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 01**	*Run Time (min):*	**2,00**
Vial Number:	**B:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 16:59**	*Sample Weight:*	**1,0000**

Chromatogram

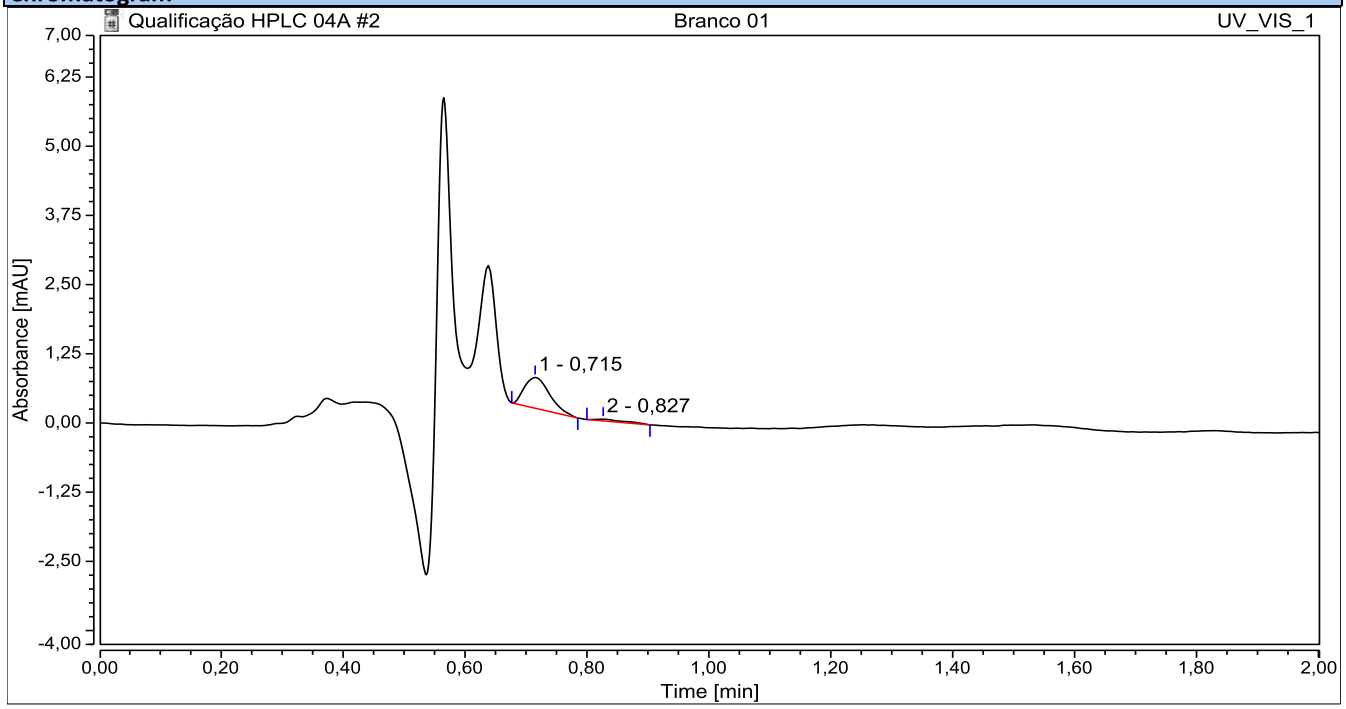

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:02**	*Sample Weight:*	**1,0000**

Chromatogram

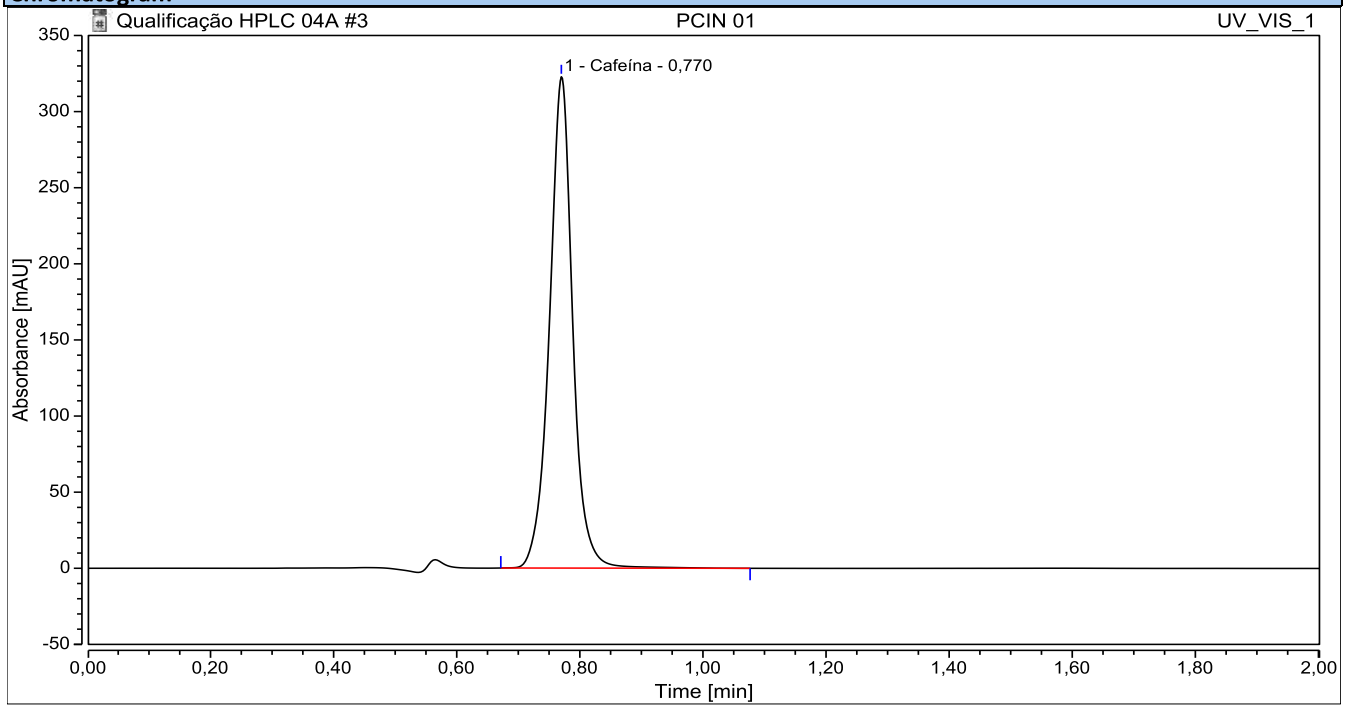

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	14,0736	322,767	100,00	100,00	n.a.
Total:			**14,074**	**322,767**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:05**	*Sample Weight:*	**1,0000**

Chromatogram

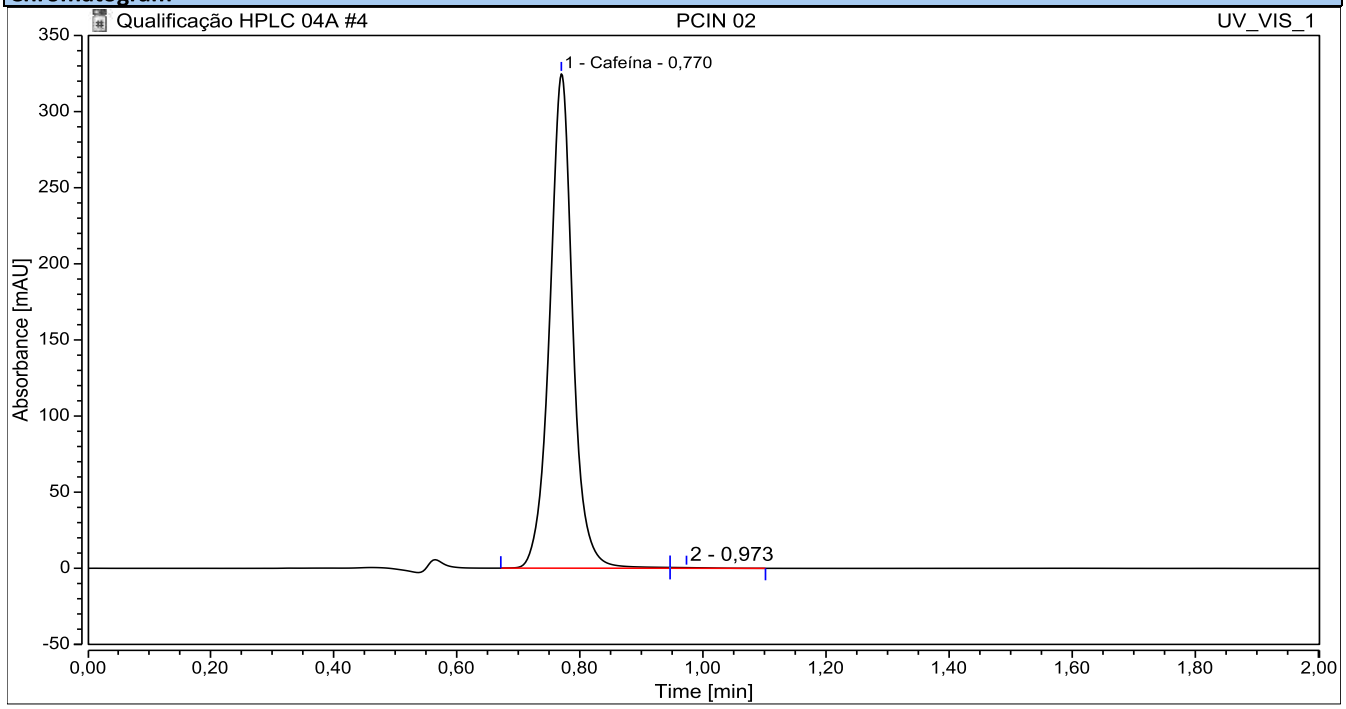

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	14,0757	324,720	99,79	99,87	n.a.
Total:			**14,076**	**324,720**	**99,786**	**99,870**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:07**	*Sample Weight:*	**1,0000**

Chromatogram

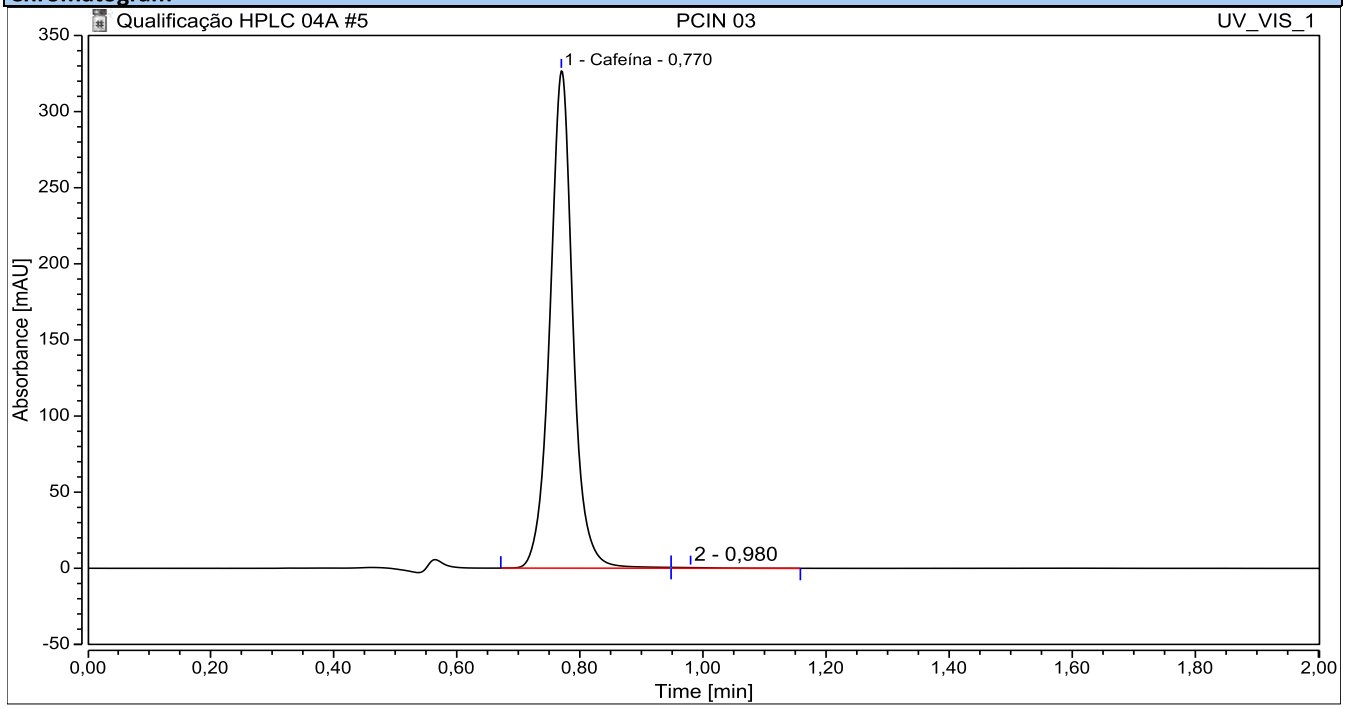

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	14,0770	326,686	99,76	99,87	n.a.
Total:			**14,077**	**326,686**	**99,759**	**99,871**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 02**	*Run Time (min):*	**2,00**
Vial Number:	**B:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:10**	*Sample Weight:*	**1,0000**

Chromatogram

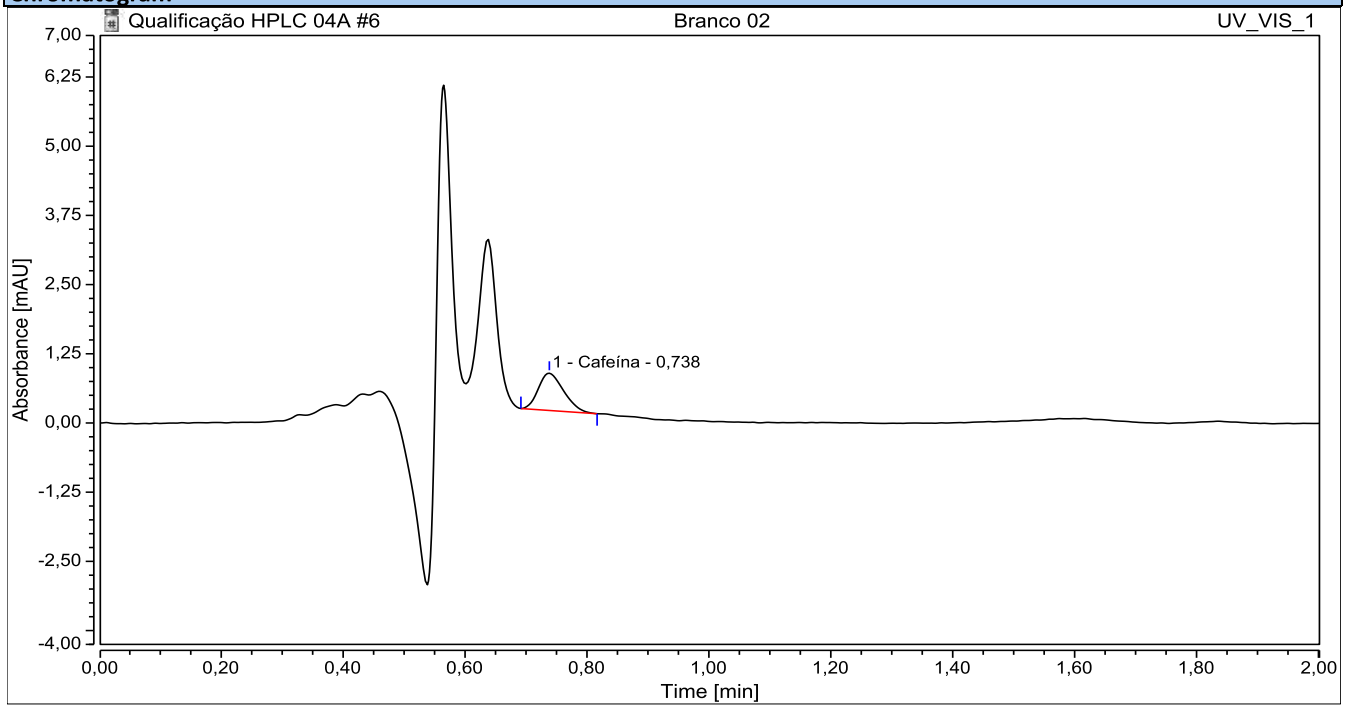

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,738	0,0325	0,673	100,00	100,00	n.a.
Total:			**0,033**	**0,673**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:13**	*Sample Weight:*	**1,0000**

Chromatogram

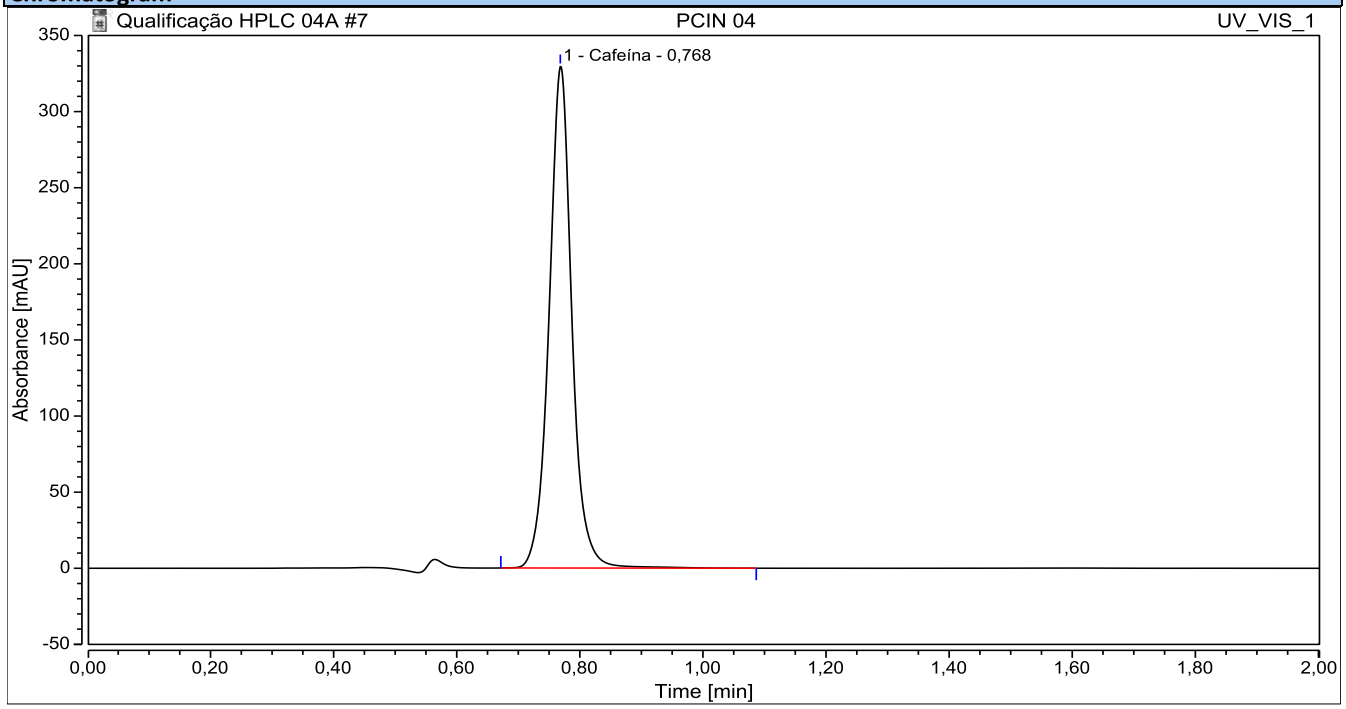

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,768	14,0981	329,490	100,00	100,00	n.a.
Total:			**14,098**	**329,490**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:15**	*Sample Weight:*	**1,0000**

Chromatogram

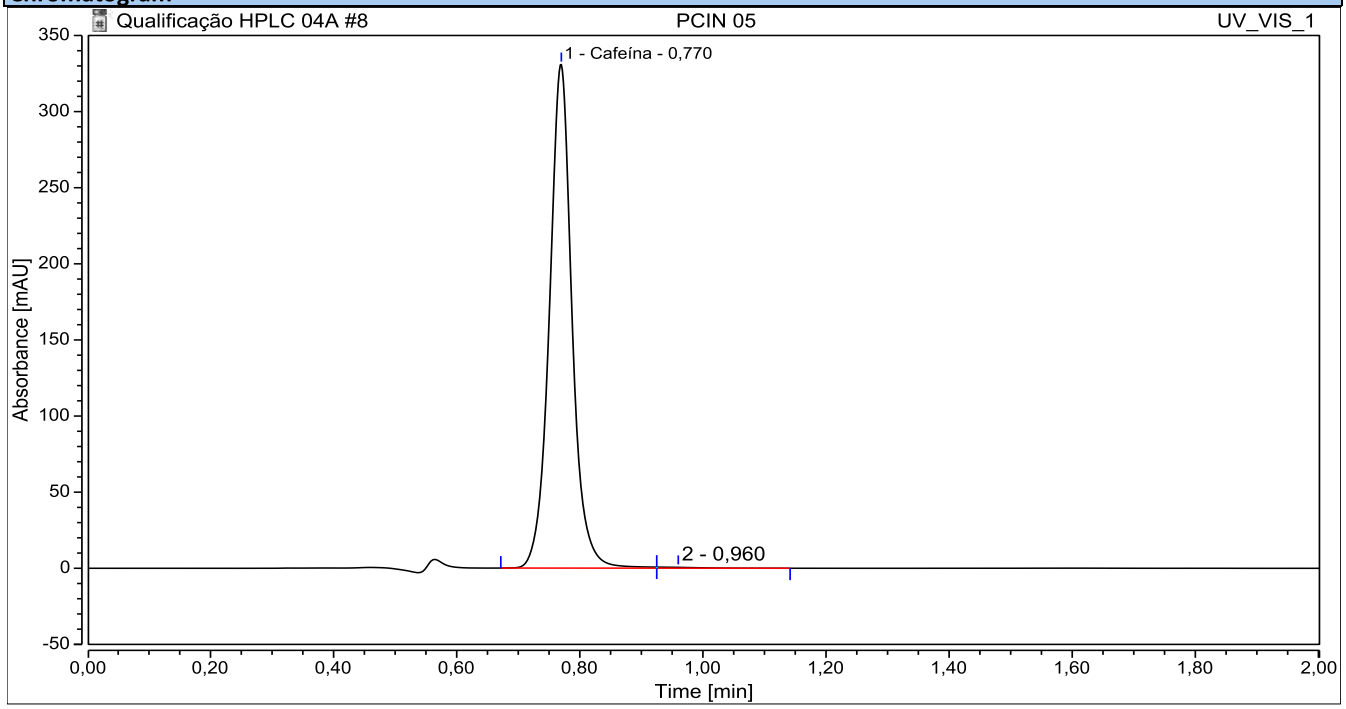

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	14,0637	330,803	99,68	99,84	n.a.
Total:			**14,064**	**330,803**	**99,684**	**99,837**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**2,00**
Vial Number:	**B:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:18**	*Sample Weight:*	**1,0000**

Chromatogram

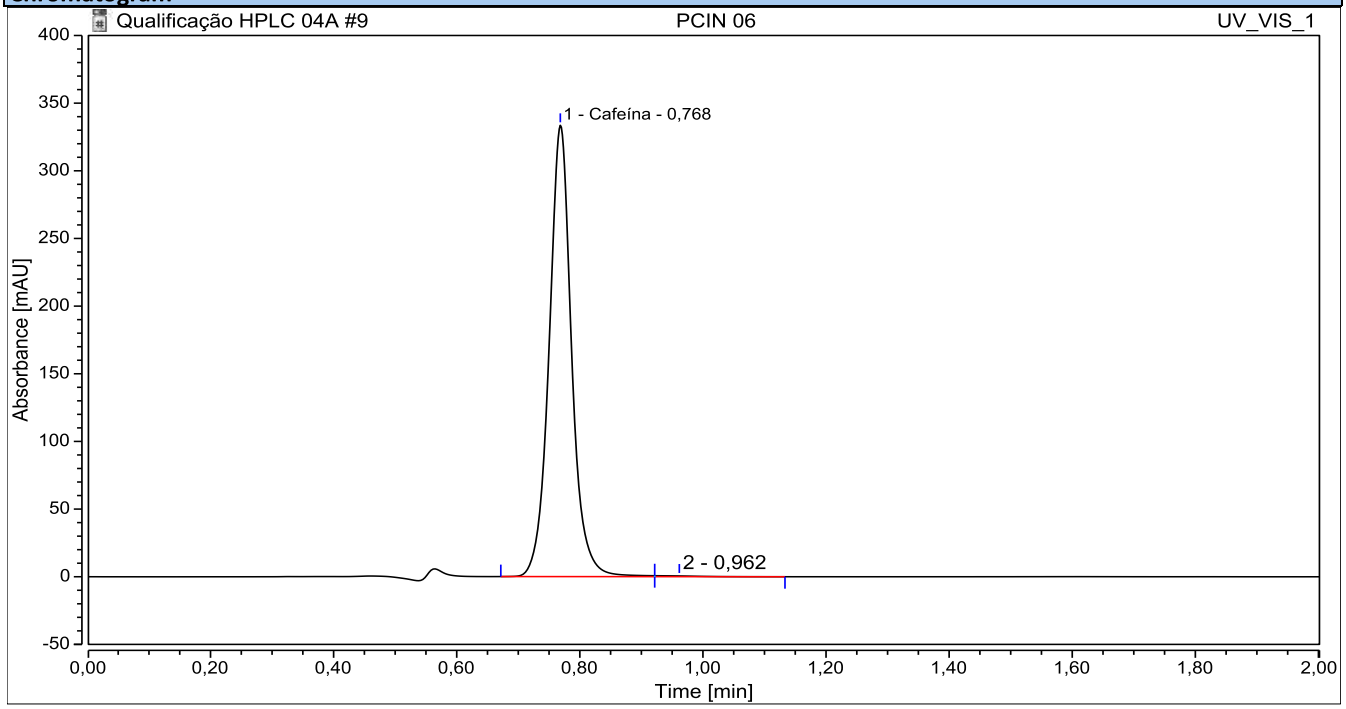

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,768	14,0809	333,527	99,67	99,84	n.a.
Total:			**14,081**	**333,527**	**99,672**	**99,841**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 03**	*Run Time (min):*	**2,00**
Vial Number:	**B:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:21**	*Sample Weight:*	**1,0000**

Chromatogram

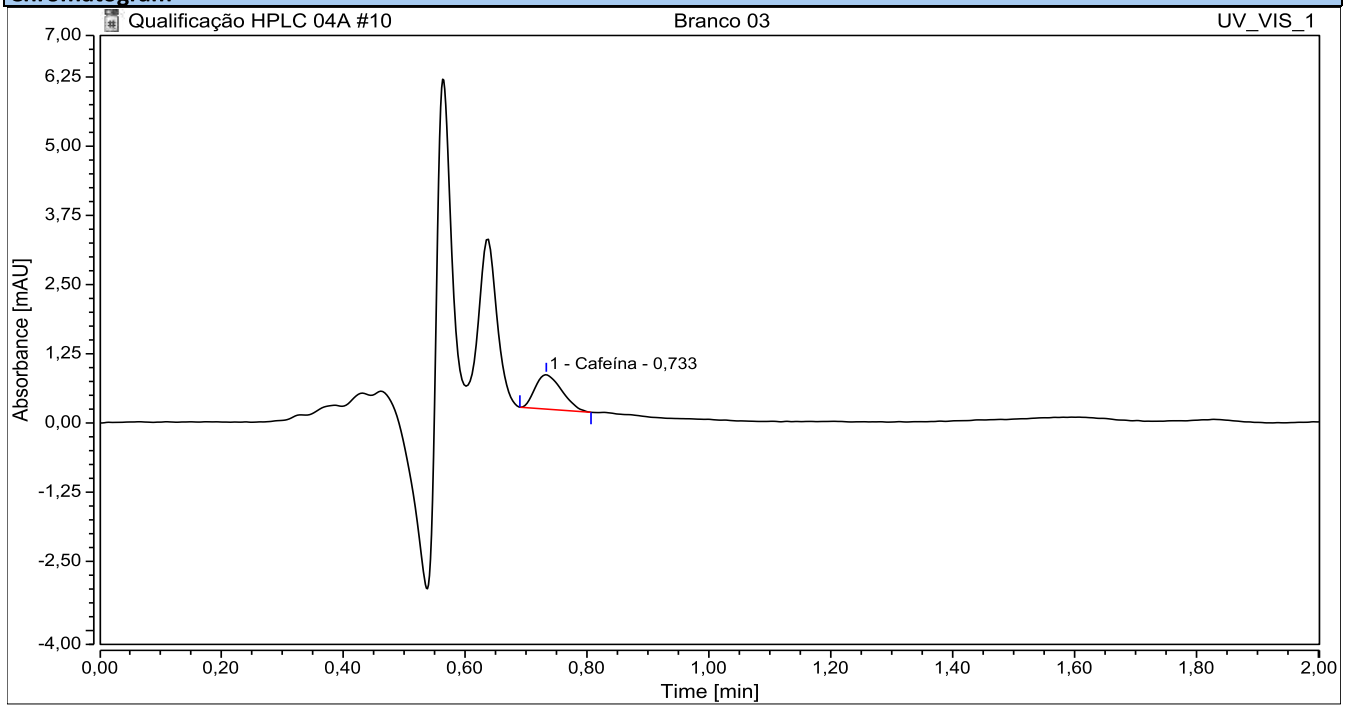

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,733	0,0316	0,621	100,00	100,00	n.a.
Total:			**0,032**	**0,621**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**2,00**
Vial Number:	**B:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:23**	*Sample Weight:*	**1,0000**

Chromatogram

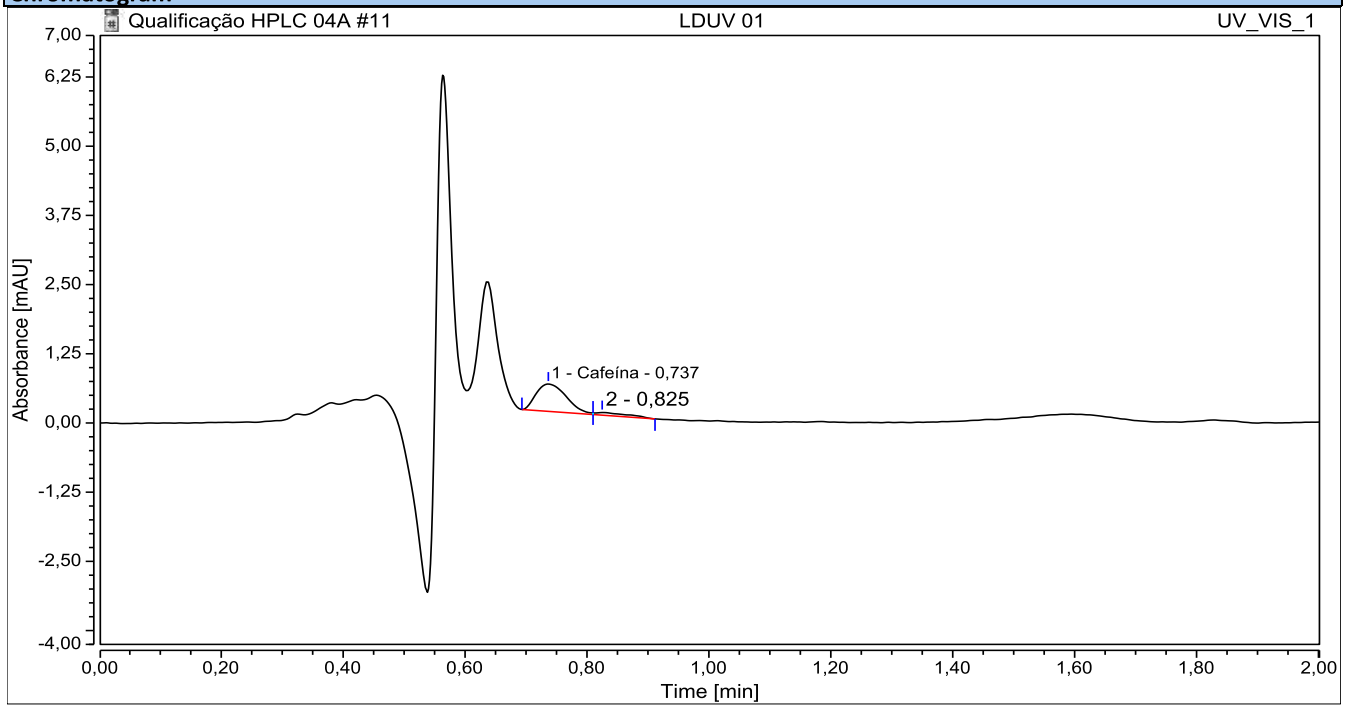

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,737	0,0285	0,494	89,44	91,21	n.a.
Total:			**0,028**	**0,494**	**89,442**	**91,209**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**2,00**
Vial Number:	**B:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:26**	*Sample Weight:*	**1,0000**

Chromatogram

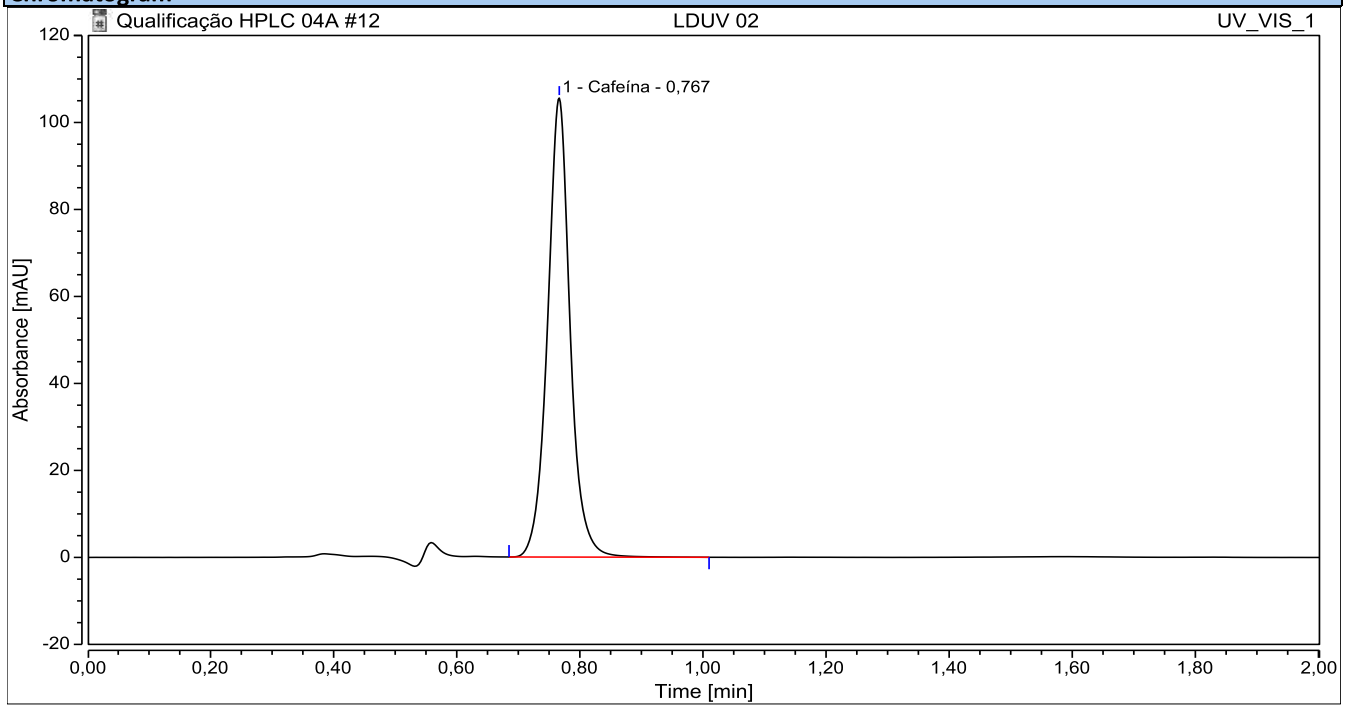

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,767	4,4734	105,536	100,00	100,00	n.a.
Total:			**4,473**	**105,536**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**2,00**
Vial Number:	**B:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:29**	*Sample Weight:*	**1,0000**

Chromatogram

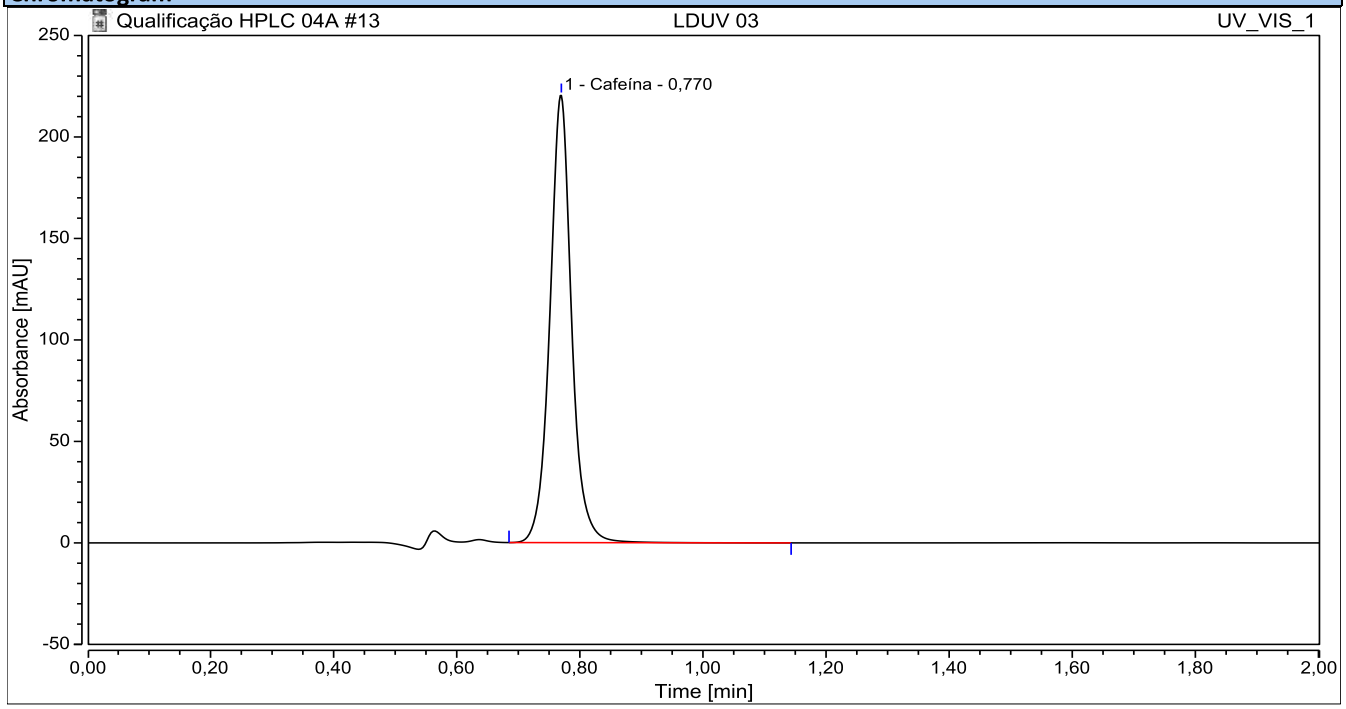

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	8,9990	220,299	100,00	100,00	n.a.
Total:			**8,999**	**220,299**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**2,00**
Vial Number:	**B:A7**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:31**	*Sample Weight:*	**1,0000**

Chromatogram

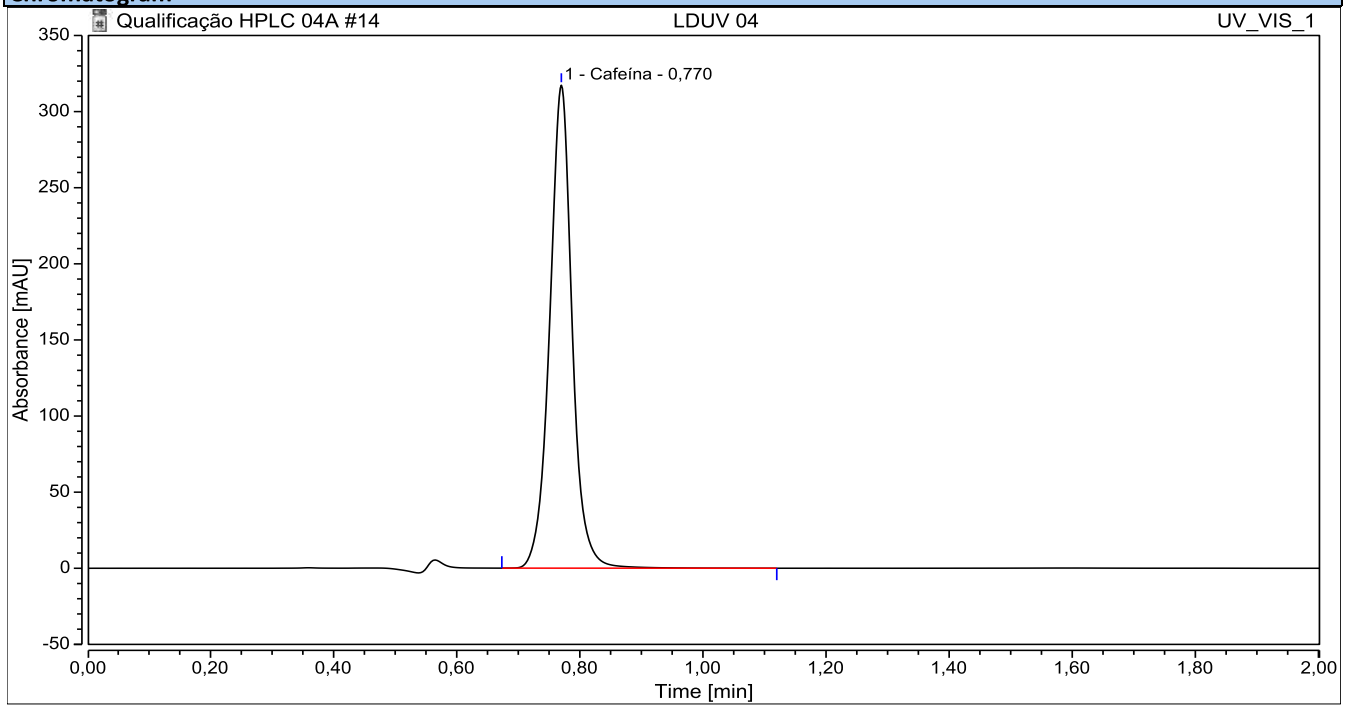

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	13,3727	317,247	100,00	100,00	n.a.
Total:			**13,373**	**317,247**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**2,00**
Vial Number:	**B:A8**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:34**	*Sample Weight:*	**1,0000**

Chromatogram

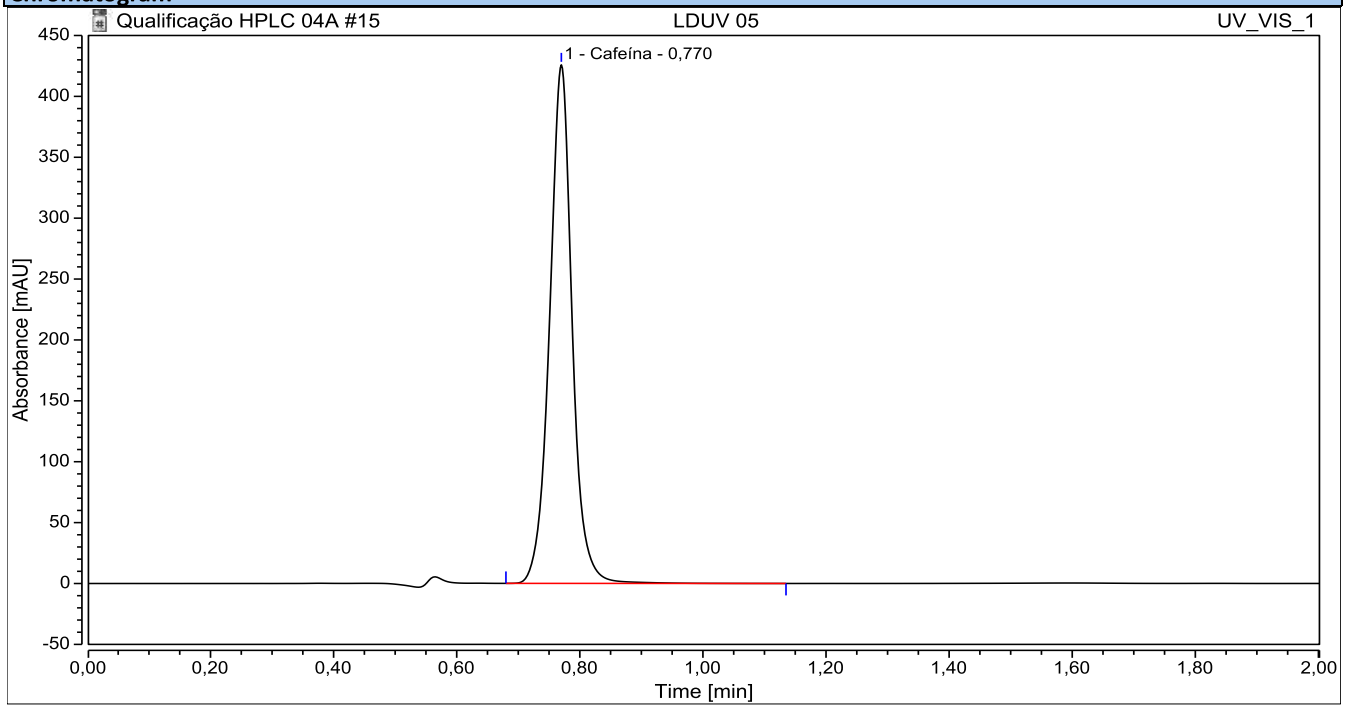

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	18,0090	425,825	100,00	100,00	n.a.
Total:			**18,009**	**425,825**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**2,00**
Vial Number:	**B:A9**	*Injection Volume:*	**0,10**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:50**	*Sample Weight:*	**1,0000**

Chromatogram

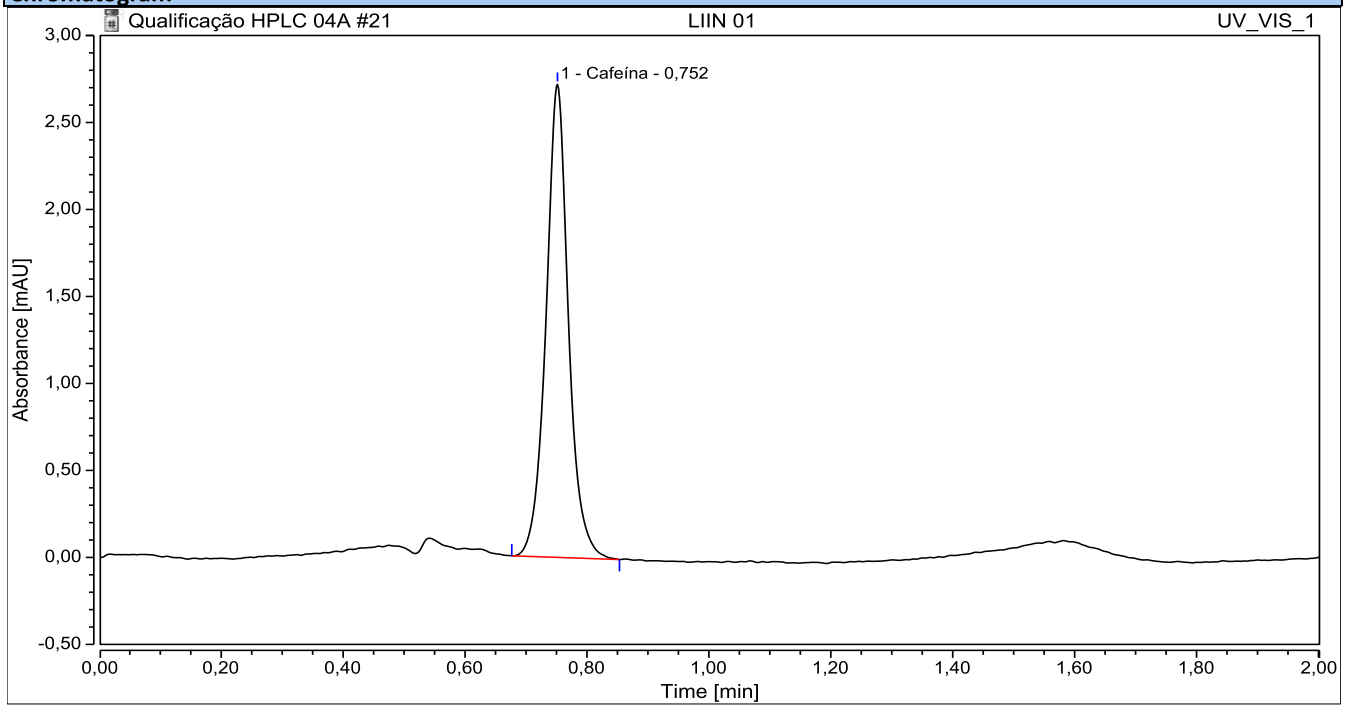

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,752	0,1159	2,719	100,00	100,00	n.a.
Total:			**0,116**	**2,719**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**2,00**
Vial Number:	**B:A9**	*Injection Volume:*	**5,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:53**	*Sample Weight:*	**1,0000**

Chromatogram

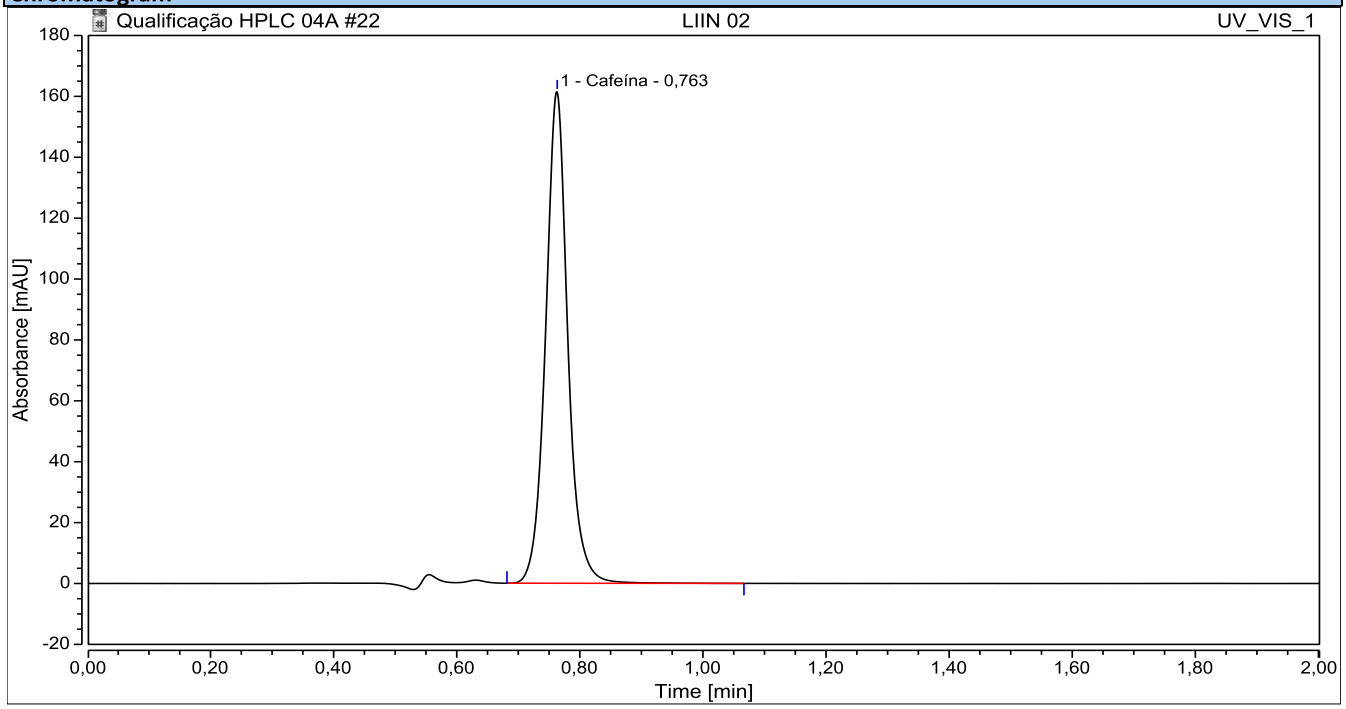

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,763	6,7217	161,396	100,00	100,00	n.a.
Total:			**6,722**	**161,396**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**2,00**
Vial Number:	**B:A9**	*Injection Volume:*	**10,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:55**	*Sample Weight:*	**1,0000**

Chromatogram

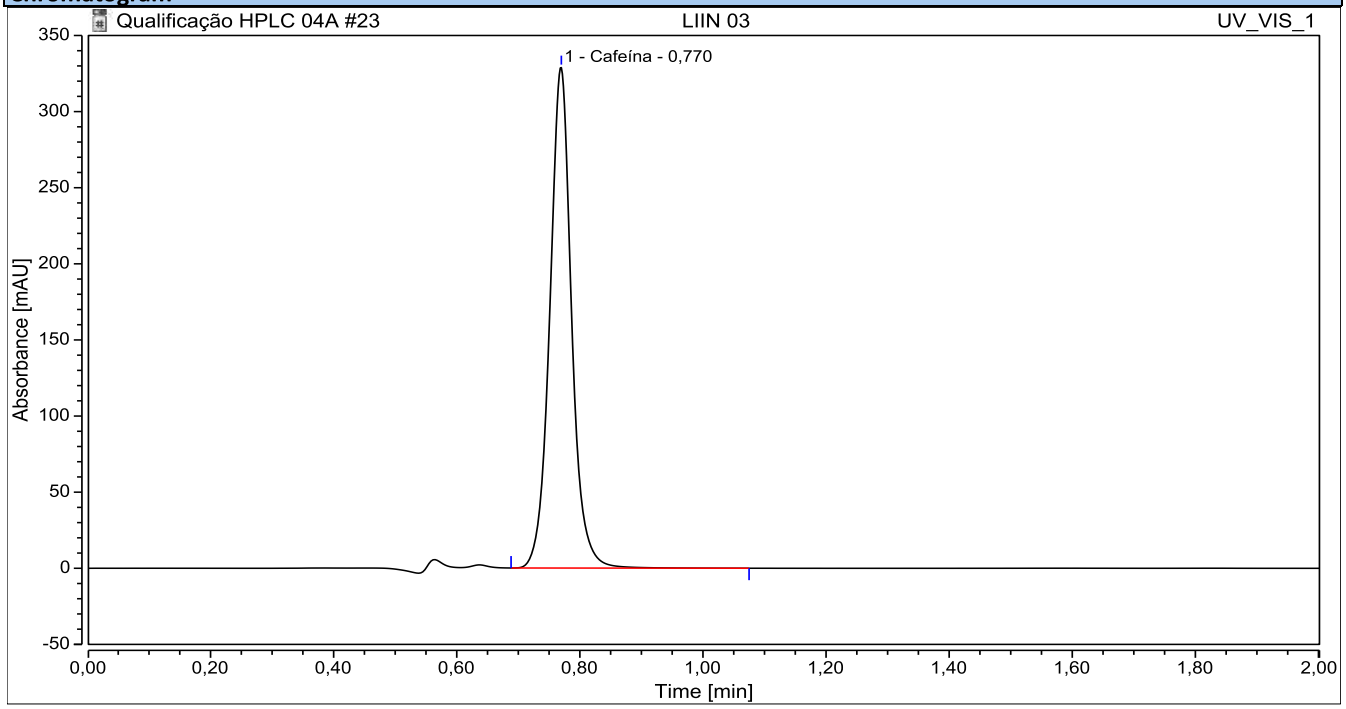

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,770	13,4419	328,757	100,00	100,00	n.a.
Total:			**13,442**	**328,757**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**2,00**
Vial Number:	**B:A9**	*Injection Volume:*	**15,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 17:58**	*Sample Weight:*	**1,0000**

Chromatogram

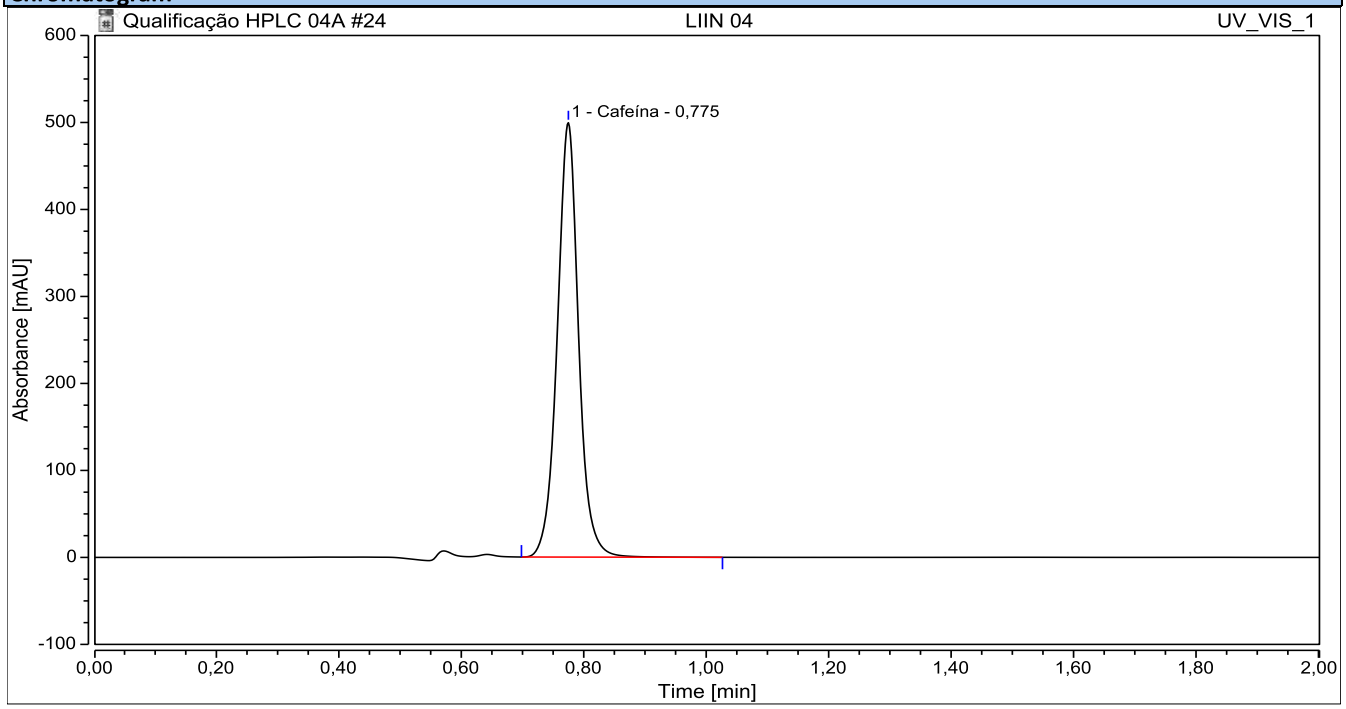

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,775	20,1054	499,354	100,00	100,00	n.a.
Total:			**20,105**	**499,354**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**2,00**
Vial Number:	**B:A9**	*Injection Volume:*	**20,00**
Injection Type:	**Matrix**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 04**	*Bandwidth:*	**4**
Processing Method:	**Integração Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/abr/25 18:01**	*Sample Weight:*	**1,0000**

Chromatogram

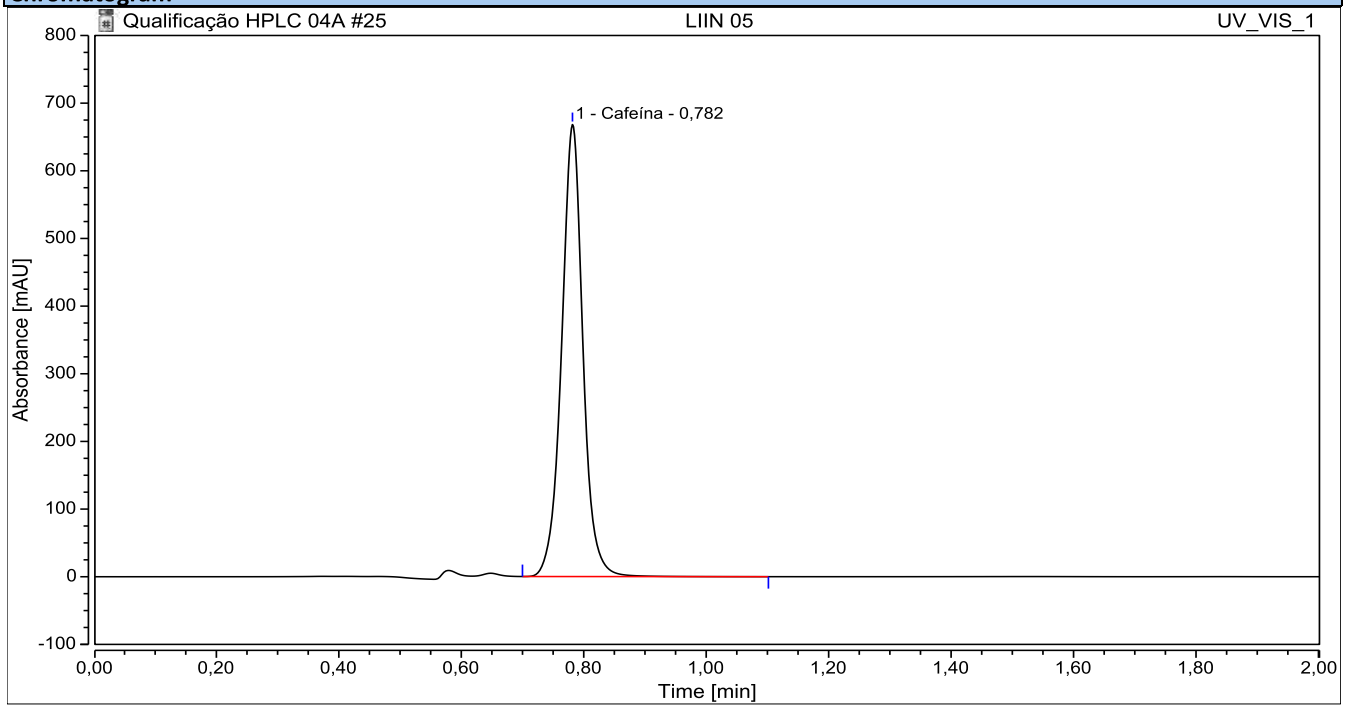

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,782	26,8385	668,137	100,00	100,00	n.a.
Total:			**26,839**	**668,137**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB**	*Run Time (min):*	**19,00**
Vial Number:	**B:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 14:55**	*Sample Weight:*	**1,0000**

Chromatogram

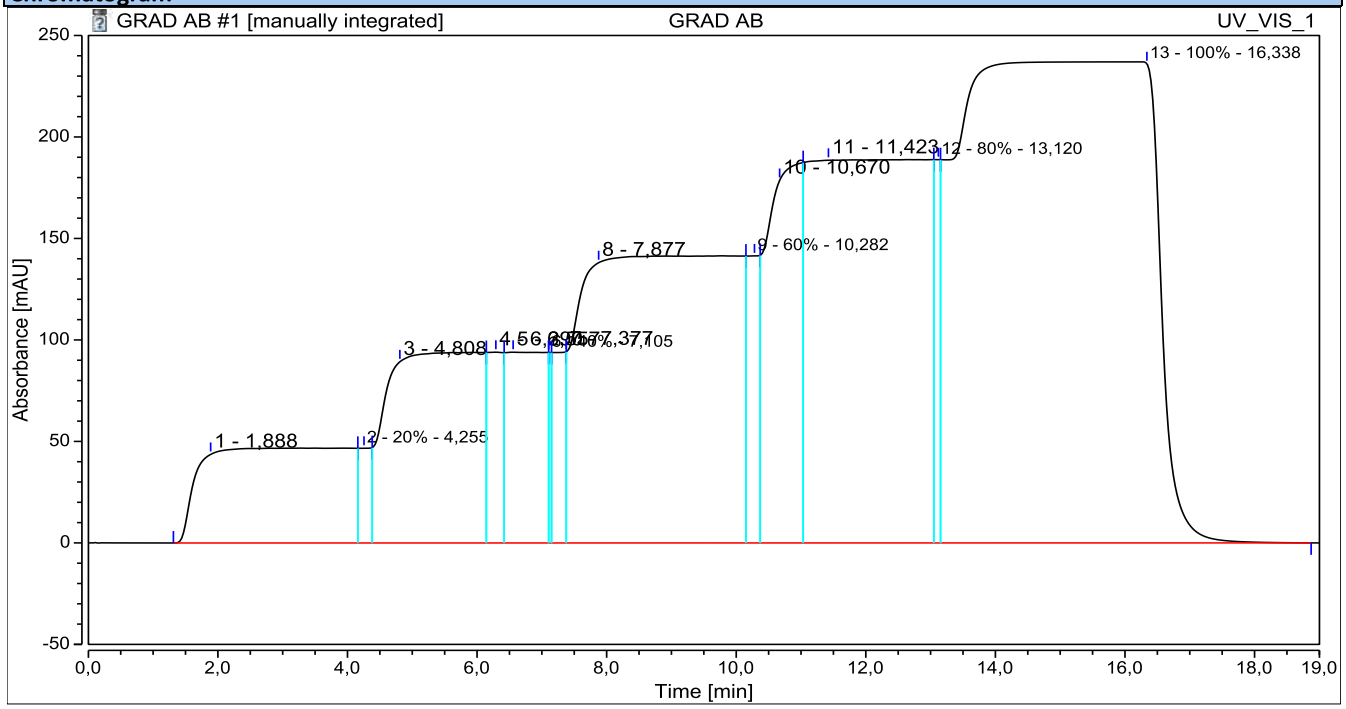

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,255	10,3489	46,669	0,49	2,87	n.a.
6	40%	7,105	4,2222	93,842	0,20	5,77	n.a.
9	60%	10,282	31,1112	141,438	1,47	8,69	n.a.
12	80%	13,120	19,5131	188,838	0,92	11,61	n.a.
13	100%	16,338	797,3129	236,083	37,55	14,51	n.a.
Total:			**862,508**	**706,869**	**40,620**	**43,441**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD CD**	*Run Time (min):*	**19,00**
Vial Number:	**B:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**08/abr/25 15:15**	*Sample Weight:*	**1,0000**

Chromatogram

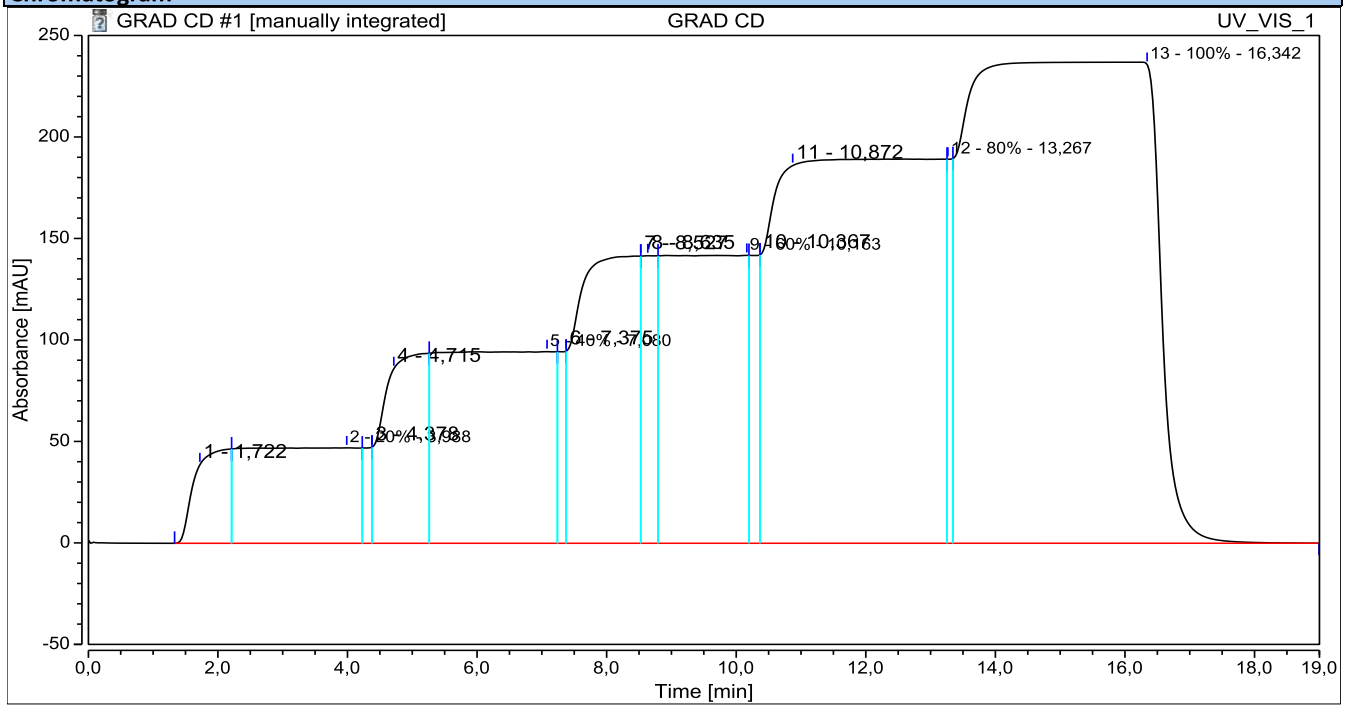

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	3,988	94,5487	47,009	4,44	2,96	n.a.
5	40%	7,080	186,3475	94,403	8,76	5,95	n.a.
9	60%	10,163	198,8888	141,831	9,35	8,94	n.a.
12	80%	13,267	17,3486	189,188	0,82	11,93	n.a.
13	100%	16,342	761,1968	235,899	35,77	14,87	n.a.
Total:			**1258,330**	**708,330**	**59,138**	**44,655**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.